
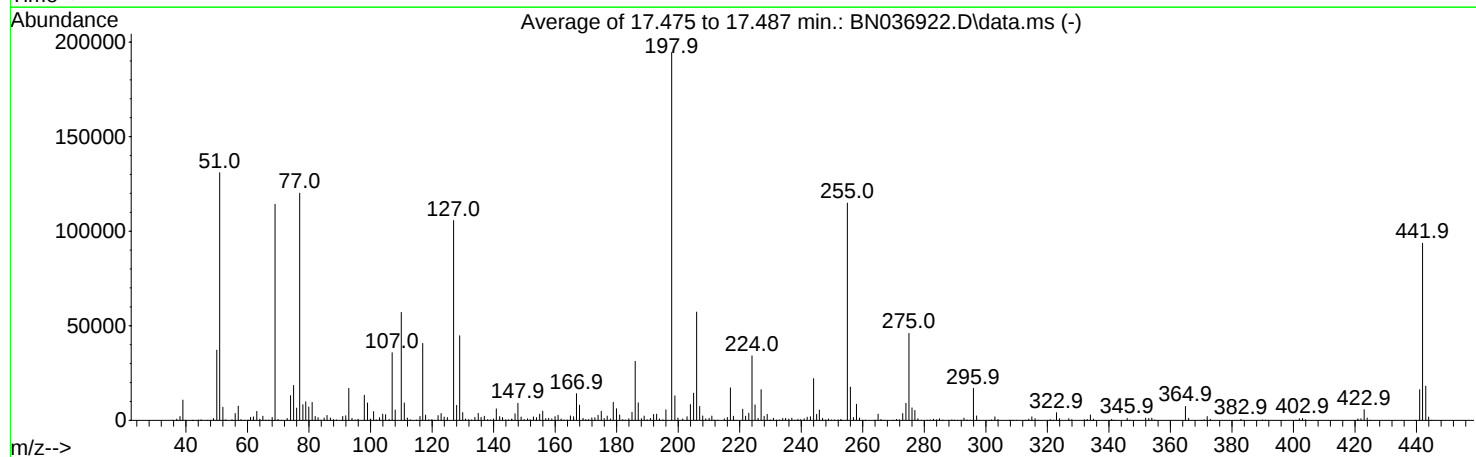


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042825\
Data File : BN036922.D
Acq On : 28 Apr 2025 10:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN042825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 28 15:35:03 2025

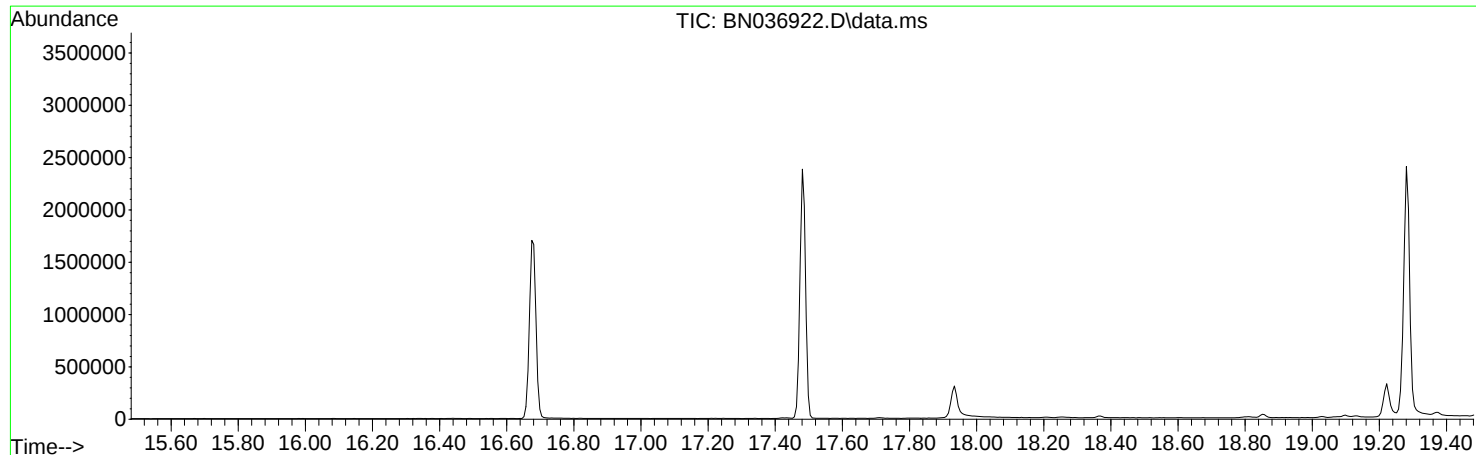

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	67.4	130988	PASS
68	69	0.00	2	1.4	1628	PASS
69	198	0.00	100	58.8	114280	PASS
70	69	0.00	2	0.4	478	PASS
127	198	10	80	54.3	105632	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	194475	PASS
199	198	5	9	6.7	12991	PASS
275	198	10	60	23.7	46040	PASS
365	198	1	100	3.8	7407	PASS
441	198	0.01	100	8.4	16253	PASS
442	442	50	100	100.0	93637	PASS
443	442	15	24	19.4	18149	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/28/2025	BNA_N	<u>BN036922.D</u>
Compound Name	Response	Retention Time
DDT	653394	20.522
DDD	6192	20.133
DDE	0	19.621
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6192	659586	0.94

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042825\
Data File : BN036922.D
Acq On : 28 Apr 2025 10:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 28 16:10:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

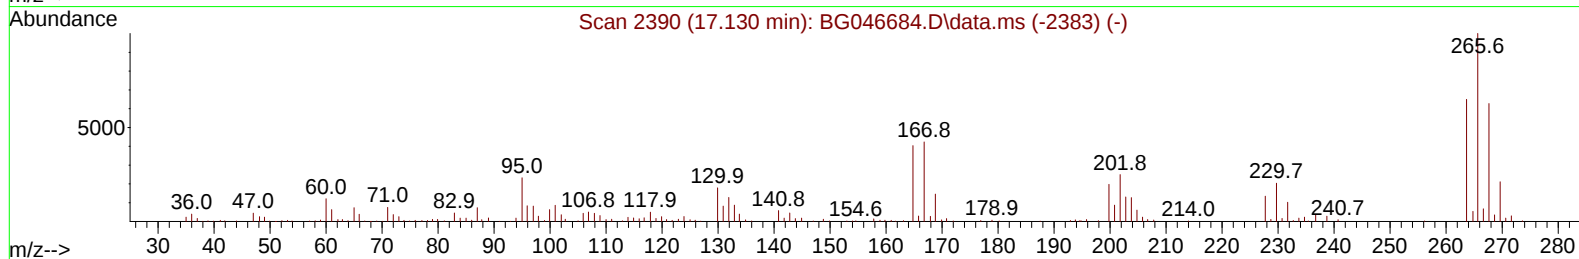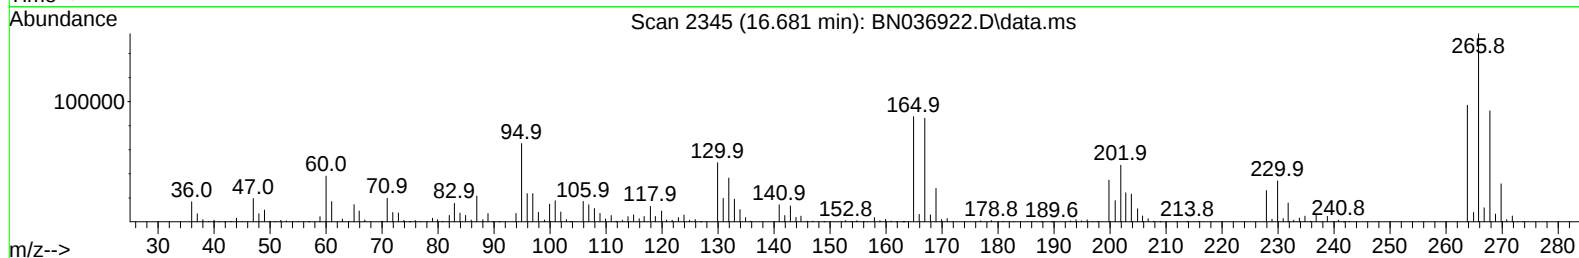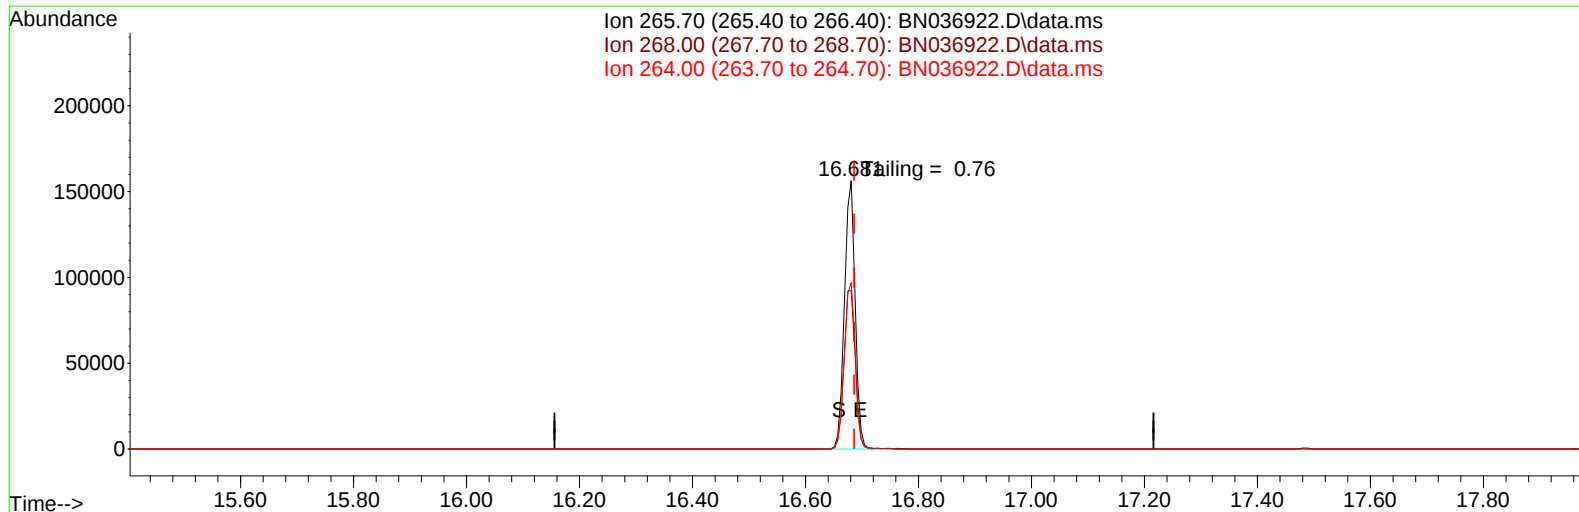

TIC: BN036922.D\data.ms

(70) Pentachlorophenol (C)

16.681min (-0.005) 20278.92 ng




response 204659

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.04
264.00	61.60	61.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042825\
Data File : BN036922.D
Acq On : 28 Apr 2025 10:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 28 16:10:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

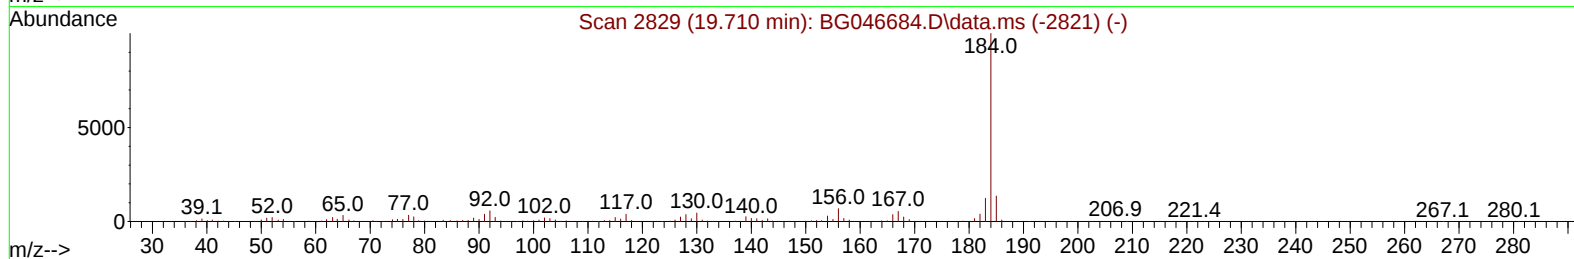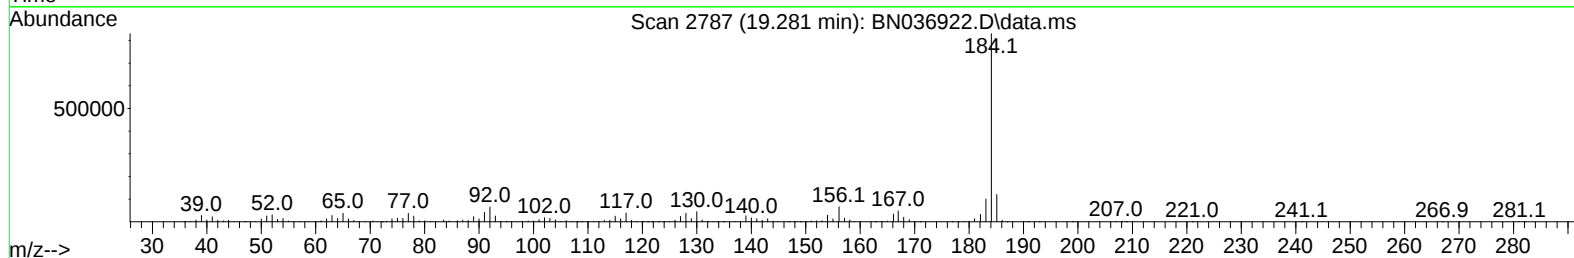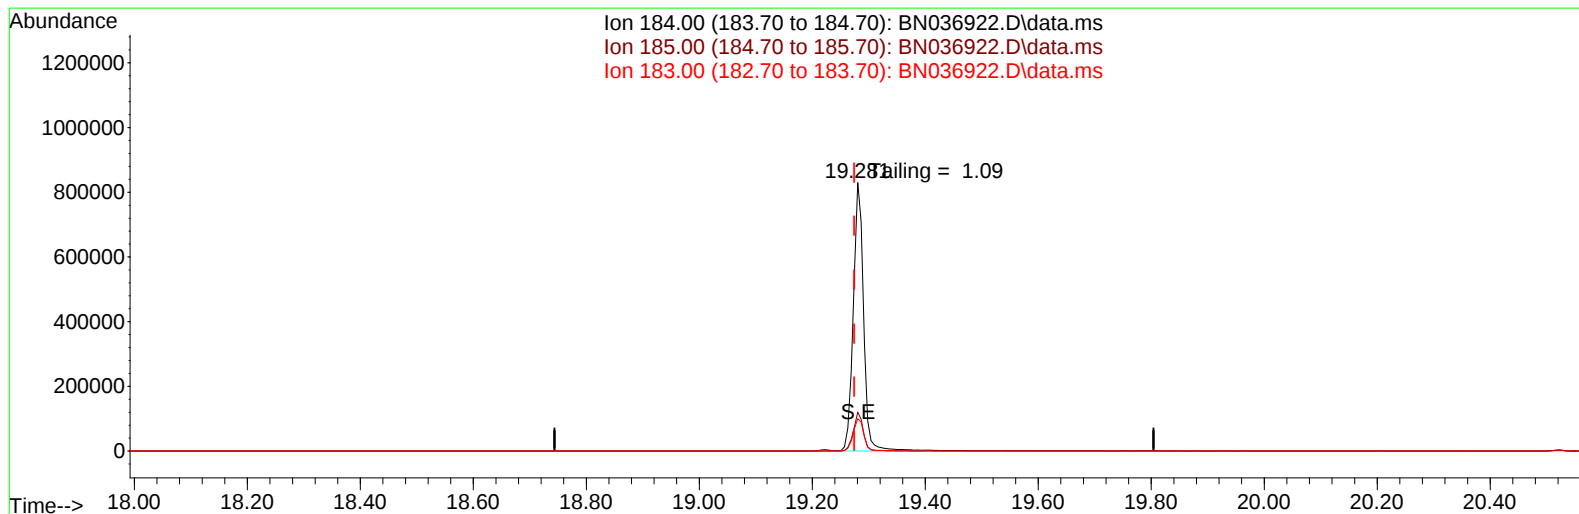

TIC: BN036922.D\data.ms

(77) Benzidine

19.281min (+ 0.006) 0.00 ng

response 1065531

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.51
183.00	13.20	12.08
0.00	0.00	0.00