
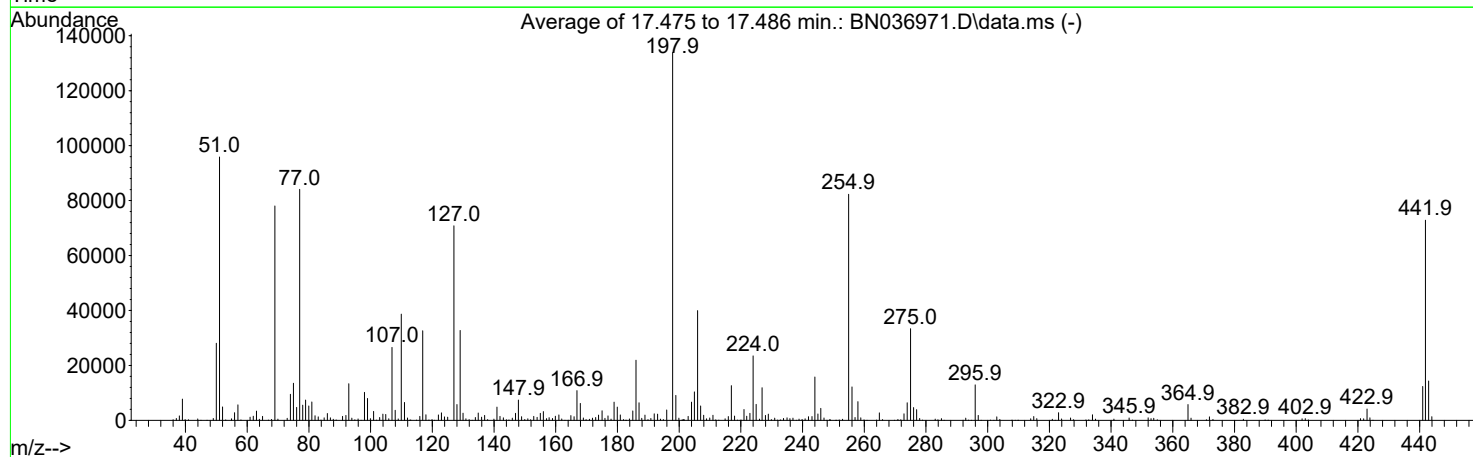


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050825\
Data File : BN036971.D
Acq On : 08 May 2025 13:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN042825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 28 15:35:03 2025

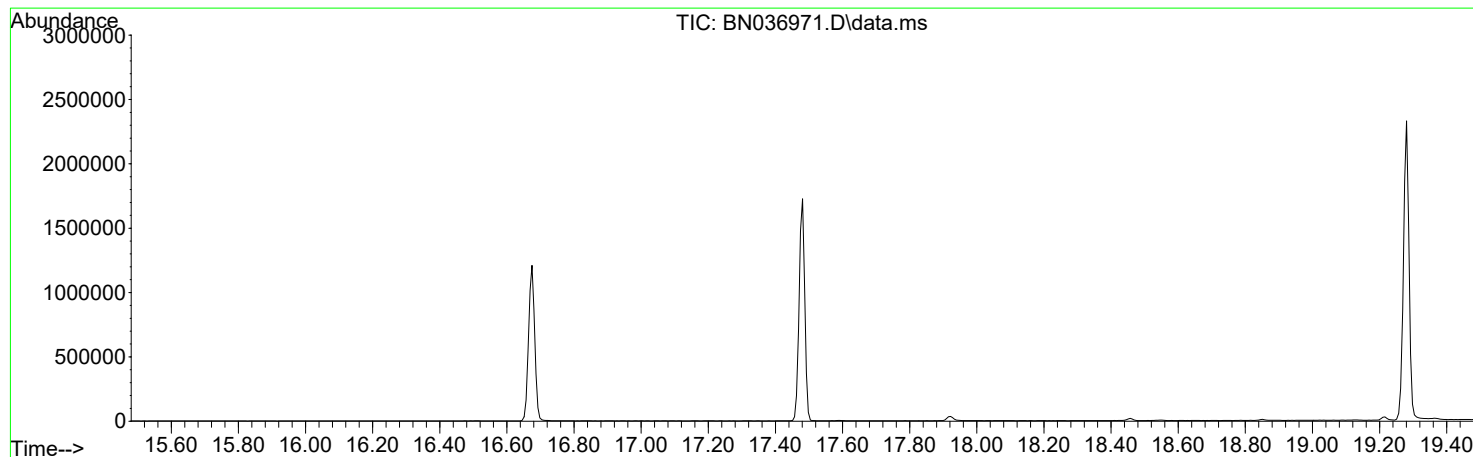

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	71.6	95861	PASS
68	69	0.00	2	0.4	347	PASS
69	198	0.00	100	58.3	78027	PASS
70	69	0.00	2	0.6	481	PASS
127	198	10	80	52.9	70819	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	133899	PASS
199	198	5	9	6.8	9104	PASS
275	198	10	60	24.9	33392	PASS
365	198	1	100	4.3	5794	PASS
441	198	0.01	100	9.2	12369	PASS
442	442	50	100	100.0	72864	PASS
443	442	15	24	19.7	14358	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/8/2025	BNA_N	<u>BN036971.D</u>
Compound Name	Response	Retention Time
DDT	487037	20.522
DDD	4120	20.133
DDE	63	19.569
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4183	491220	0.85

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050825\
Data File : BN036971.D
Acq On : 08 May 2025 13:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 08 17:01:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

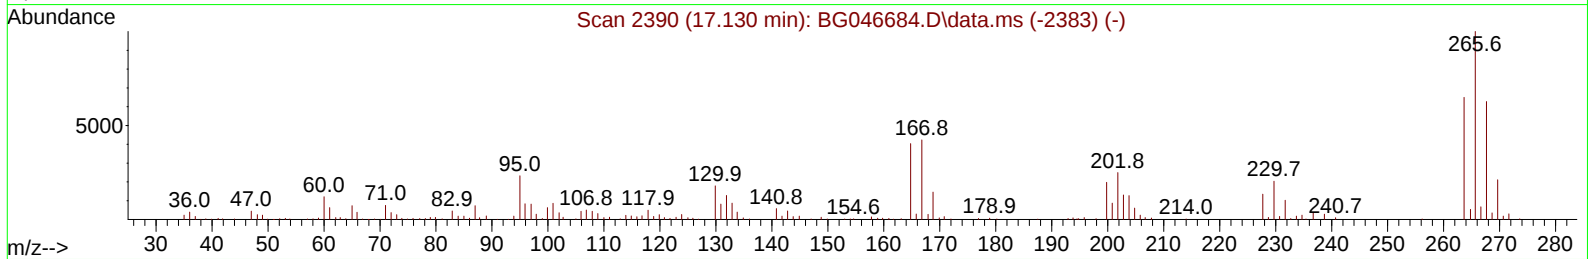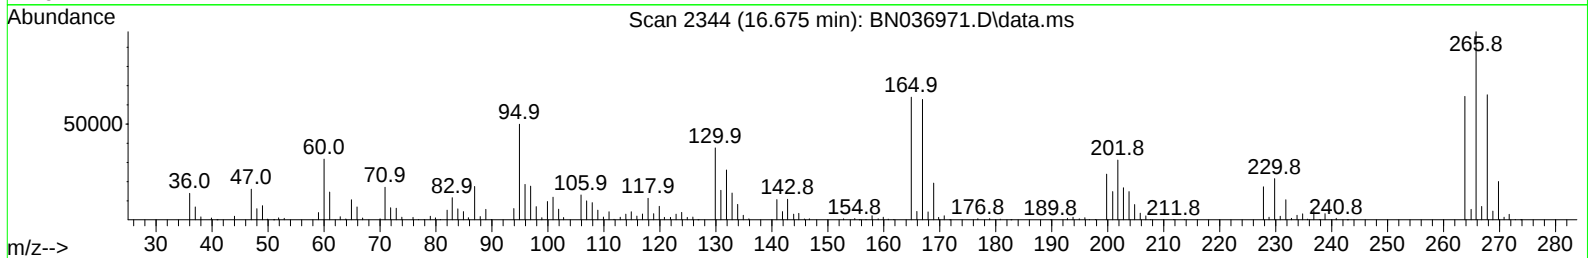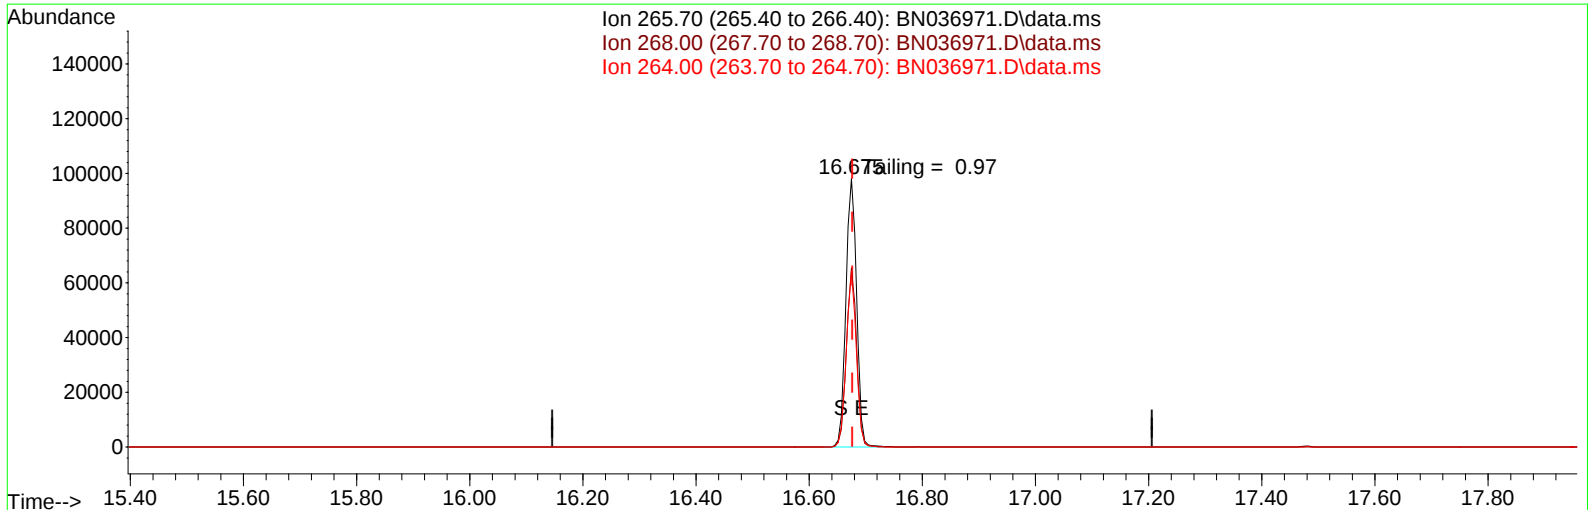

TIC: BN036971.D\data.ms

(70) Pentachlorophenol (C)

16.675min (-0.001) 17886.24 ng




response 128997

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.51
264.00	61.60	65.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050825\
Data File : BN036971.D
Acq On : 08 May 2025 13:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 08 17:01:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

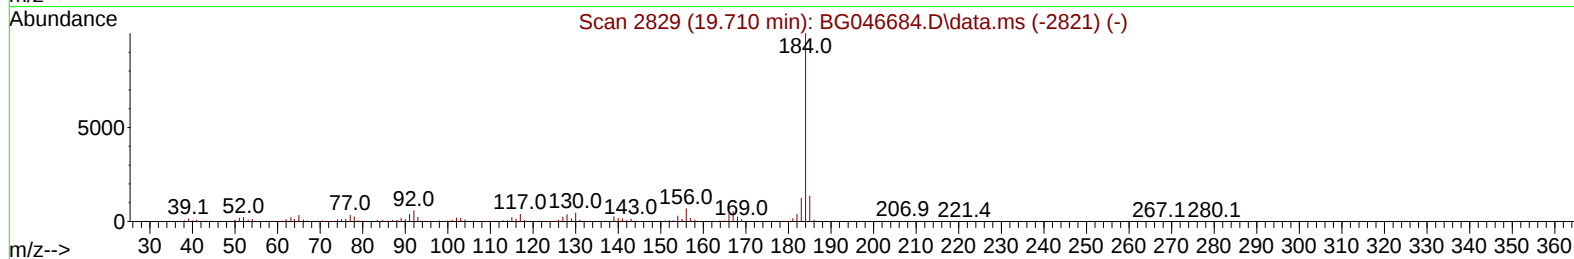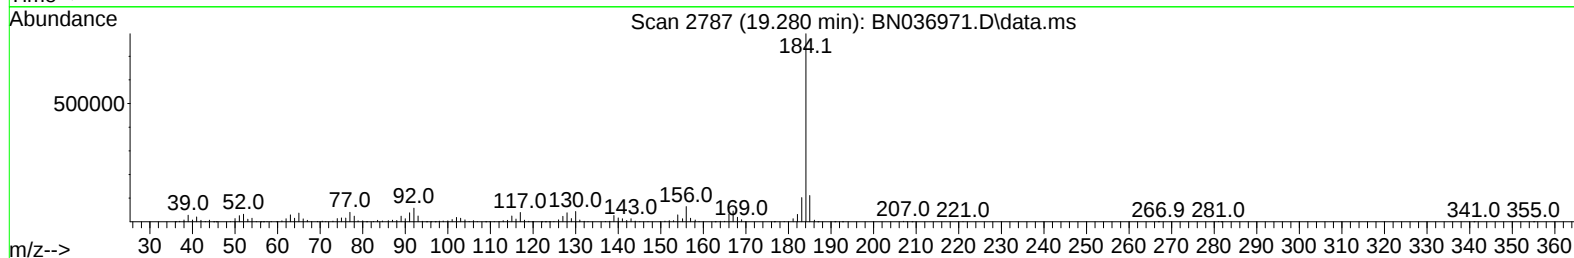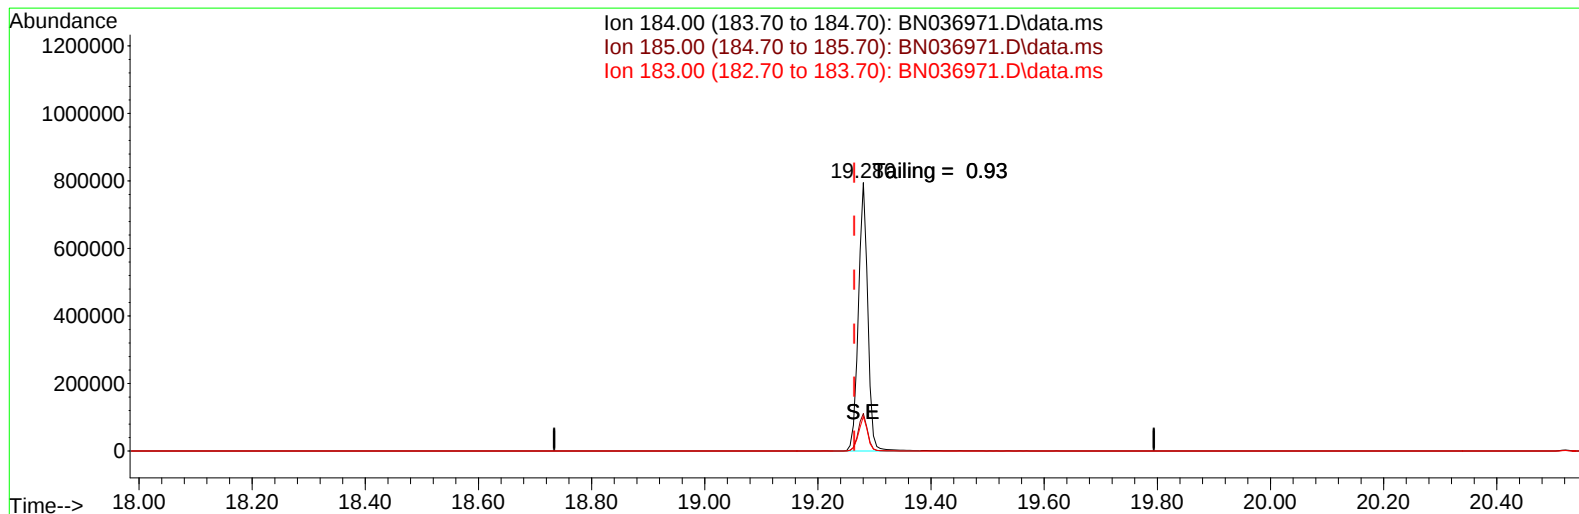

TIC: BN036971.D\data.ms

(77) Benzidine

19.280min (+ 0.016) 0.00 ng

response 917971

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.00
183.00	13.20	12.91
0.00	0.00	0.00