
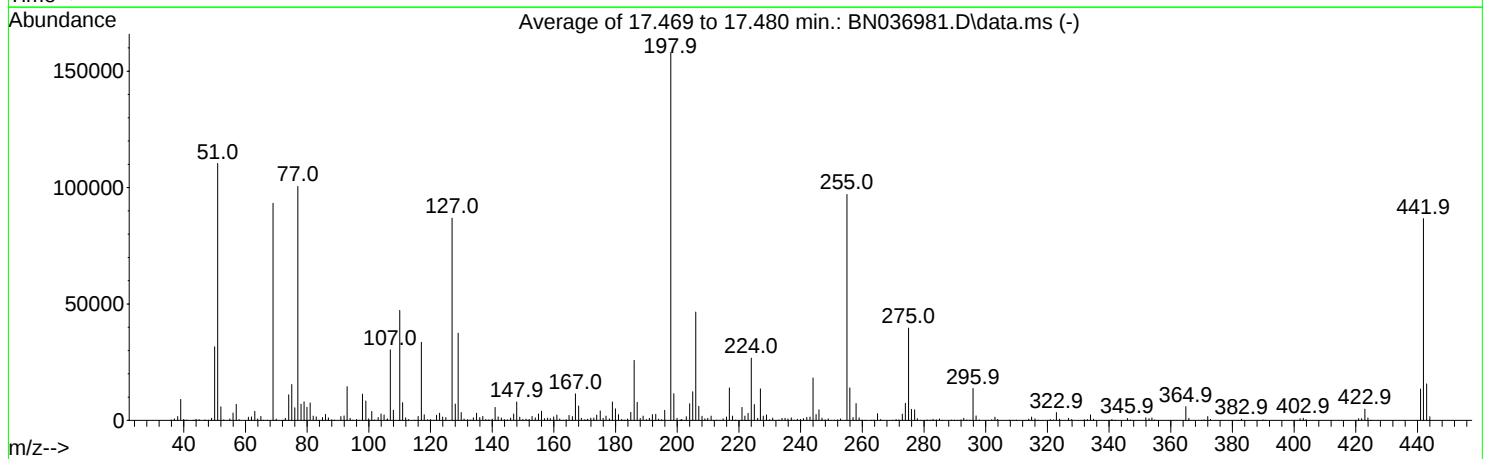


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051225\
Data File : BN036981.D
Acq On : 12 May 2025 13:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 12 18:05:36 2025

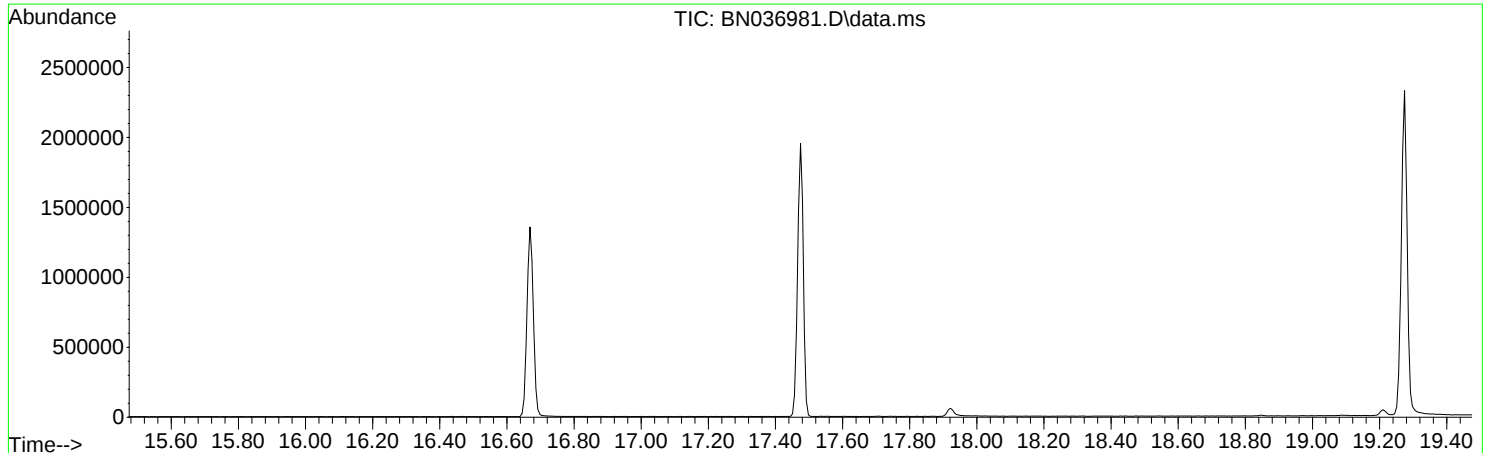

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	69.8	110372	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	59.0	93309	PASS
70	69	0.00	2	0.6	525	PASS
127	198	10	80	55.0	86912	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	158037	PASS
199	198	5	9	7.3	11485	PASS
275	198	10	60	25.1	39640	PASS
365	198	1	100	3.8	5930	PASS
441	198	0.01	100	8.5	13485	PASS
442	442	50	100	100.0	86653	PASS
443	442	15	24	18.1	15692	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/12/2025	BNA_N	<u>BN036981.D</u>
Compound Name	Response	Retention Time
DDT	504877	20.516
DDD	5050	20.121
DDE	0	19.569
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5050	509927	0.99

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051225\
Data File : BN036981.D
Acq On : 12 May 2025 13:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 12 18:21:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

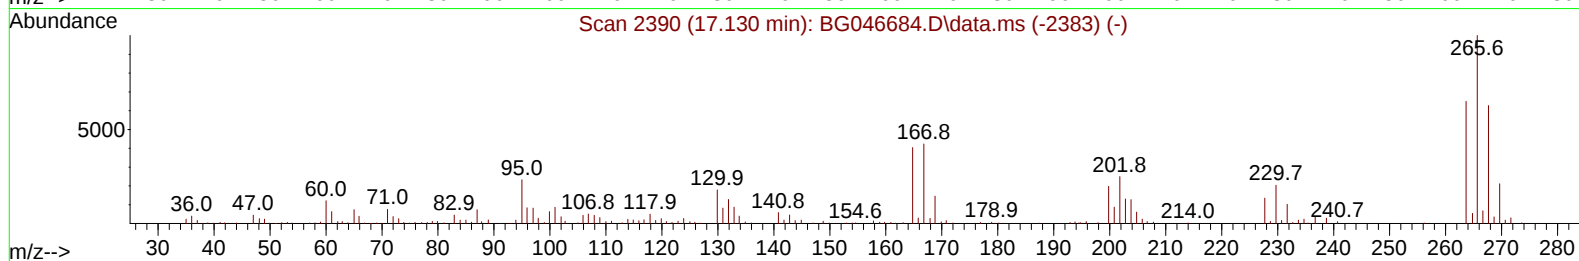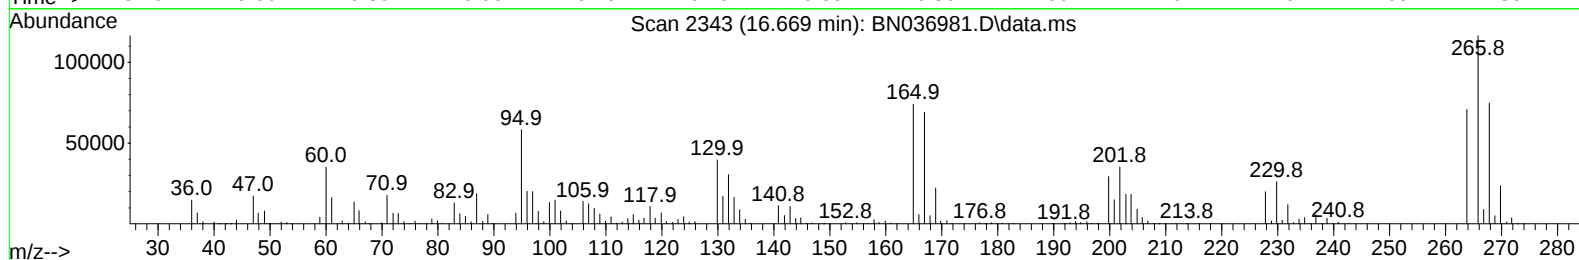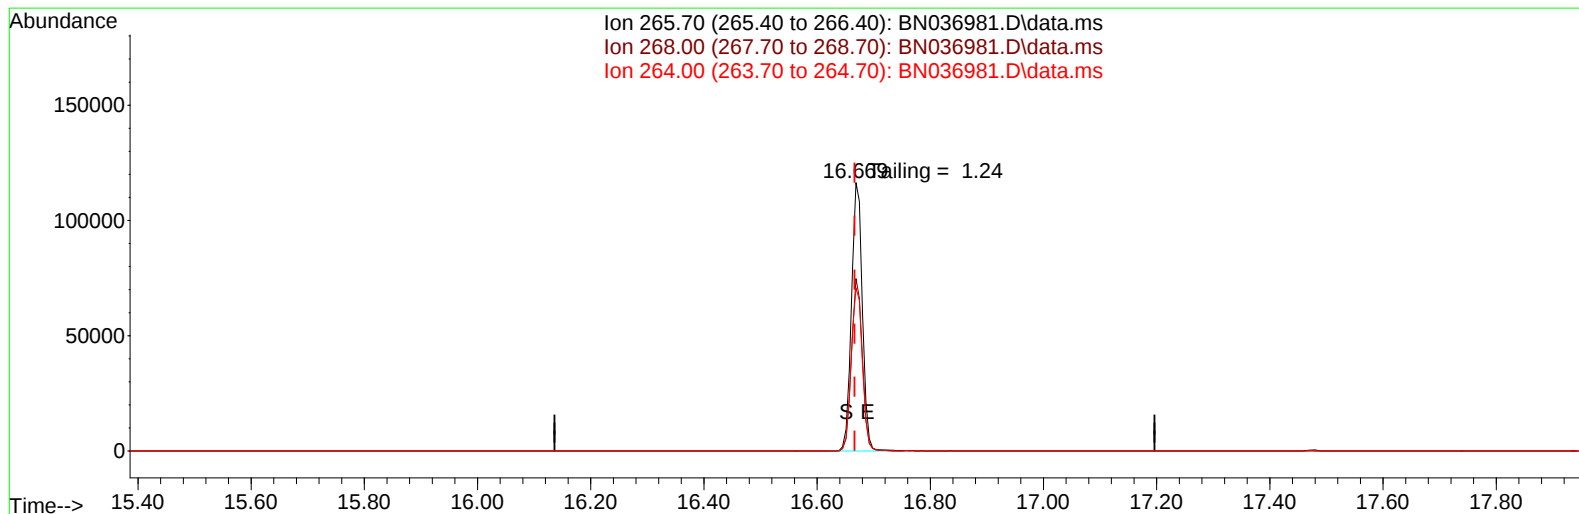

TIC: BN036981.D\data.ms

(70) Pentachlorophenol (C)

16.669min (+ 0.003) 17561.04 ng




response 156144

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.20
264.00	61.60	60.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051225\
Data File : BN036981.D
Acq On : 12 May 2025 13:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 12 18:21:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

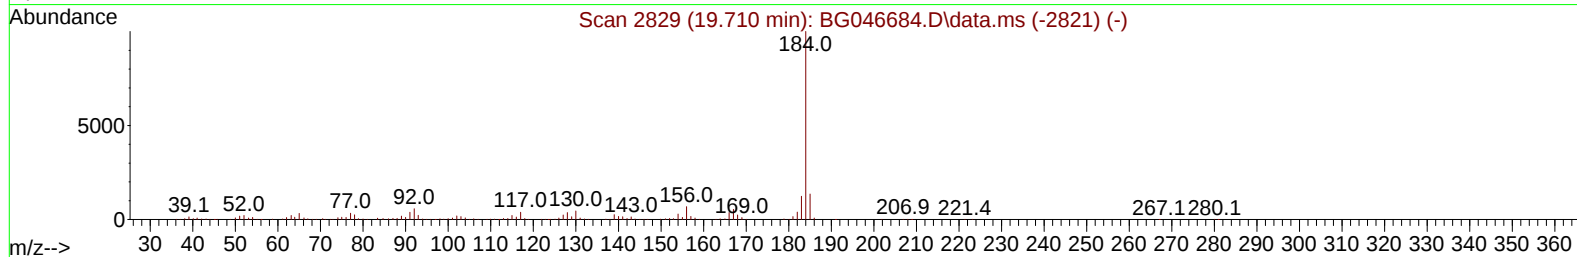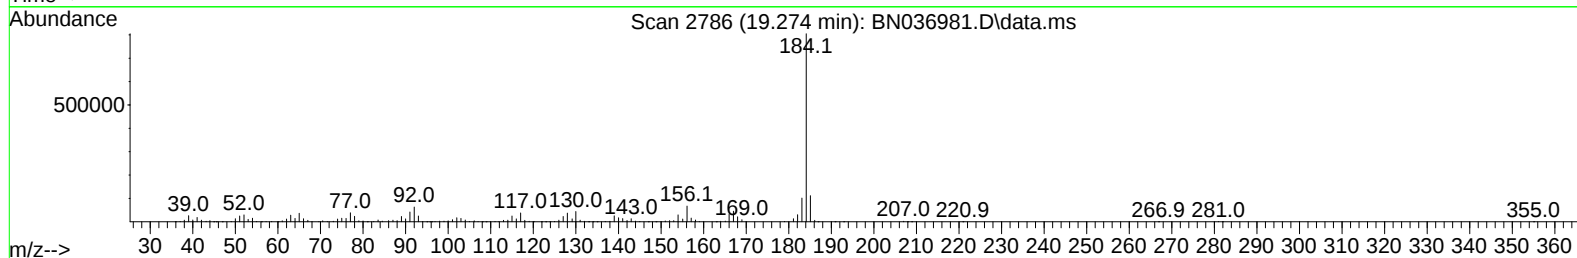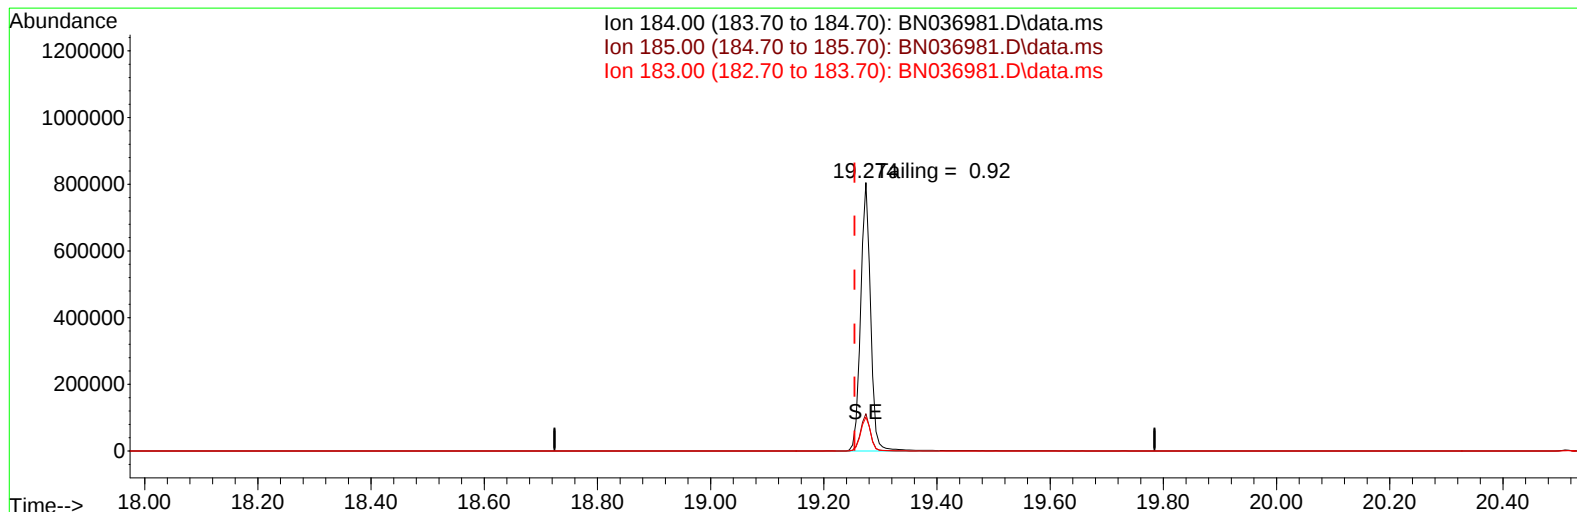

TIC: BN036981.D\data.ms

(77) Benzidine

19.274min (+ 0.020) 0.00 ng

response 985685

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.90
183.00	13.20	12.59
0.00	0.00	0.00