
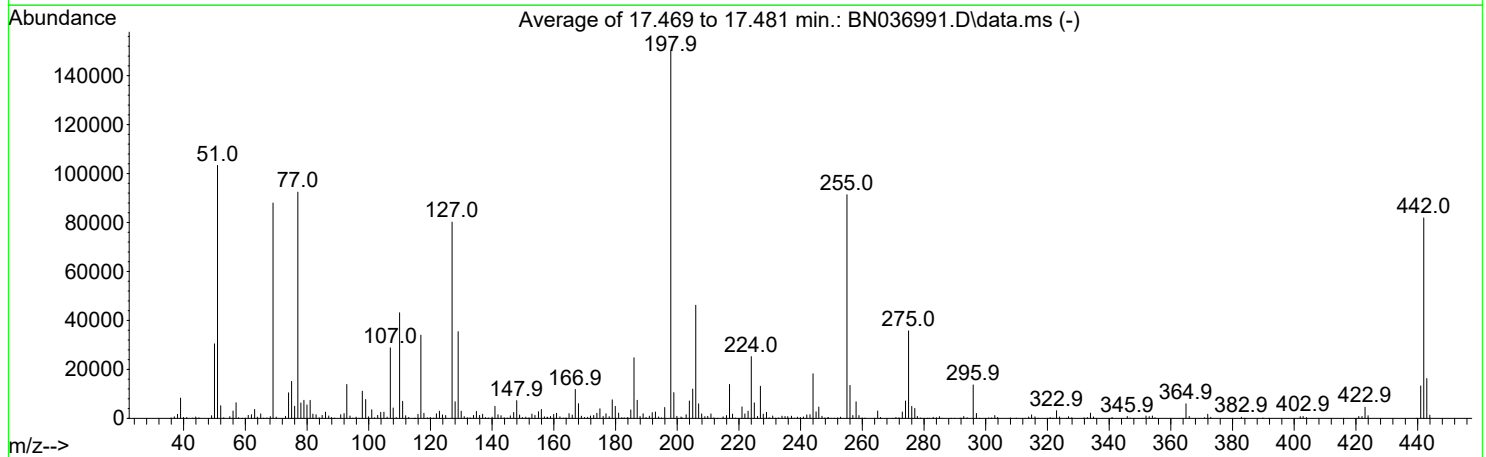


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051325\
Data File : BN036991.D
Acq On : 13 May 2025 09:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 12 18:05:36 2025

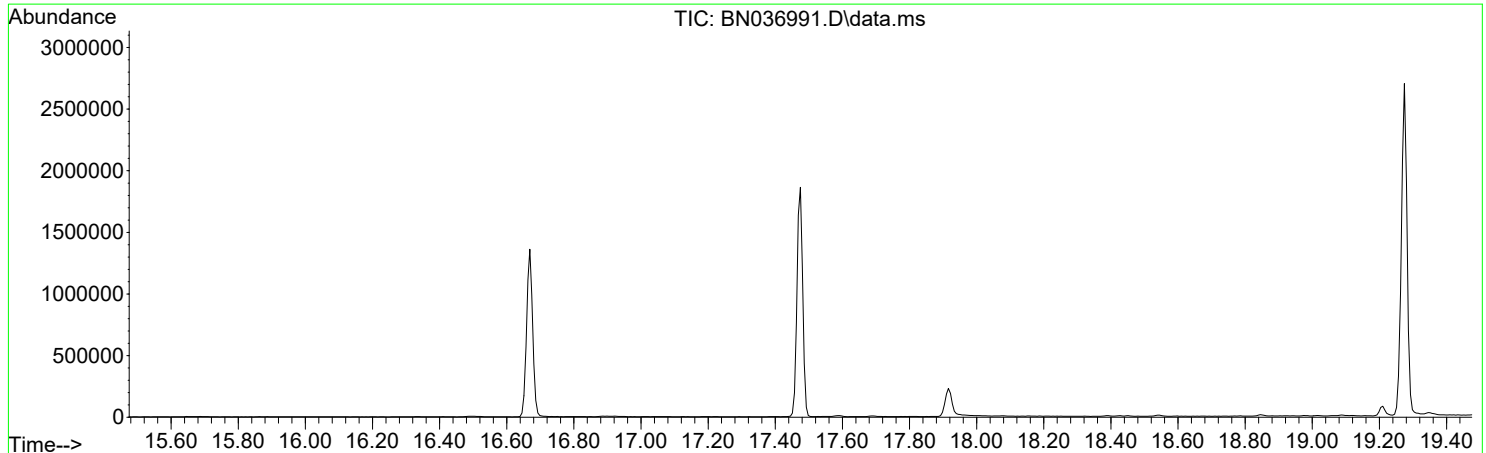

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	68.8	103320	PASS
68	69	0.00	2	0.8	711	PASS
69	198	0.00	100	58.5	87979	PASS
70	69	0.00	2	0.6	516	PASS
127	198	10	80	53.4	80205	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	150269	PASS
199	198	5	9	7.0	10508	PASS
275	198	10	60	23.8	35755	PASS
365	198	1	100	3.9	5927	PASS
441	198	0.01	100	8.8	13271	PASS
442	442	50	100	100.0	81907	PASS
443	442	15	24	19.8	16248	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/13/2025	BNA_N	<u>BN036991.D</u>
Compound Name	Response	Retention Time
DDT	537518	20.516
DDD	5973	20.122
DDE	151	19.569
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6124	543642	1.13

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051325\
Data File : BN036991.D
Acq On : 13 May 2025 09:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 13 15:42:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

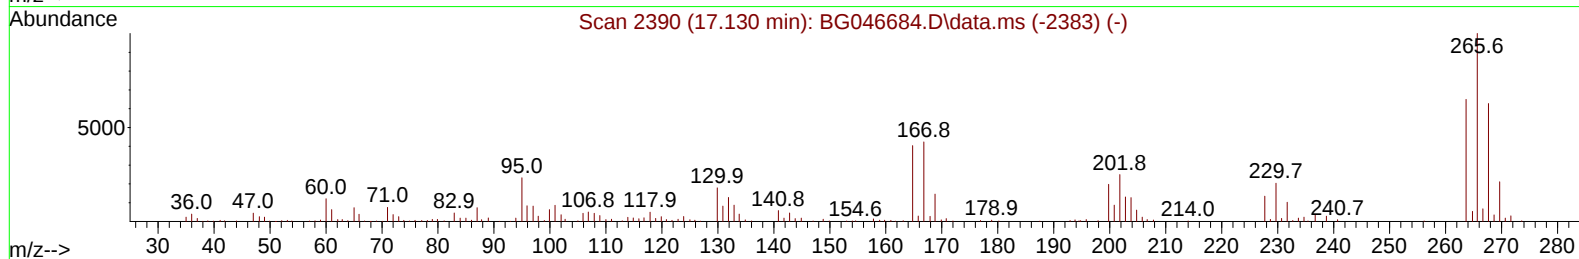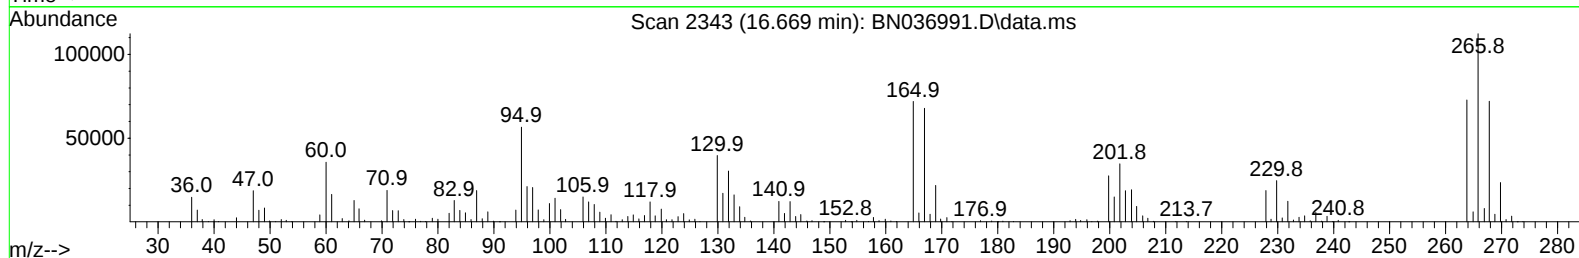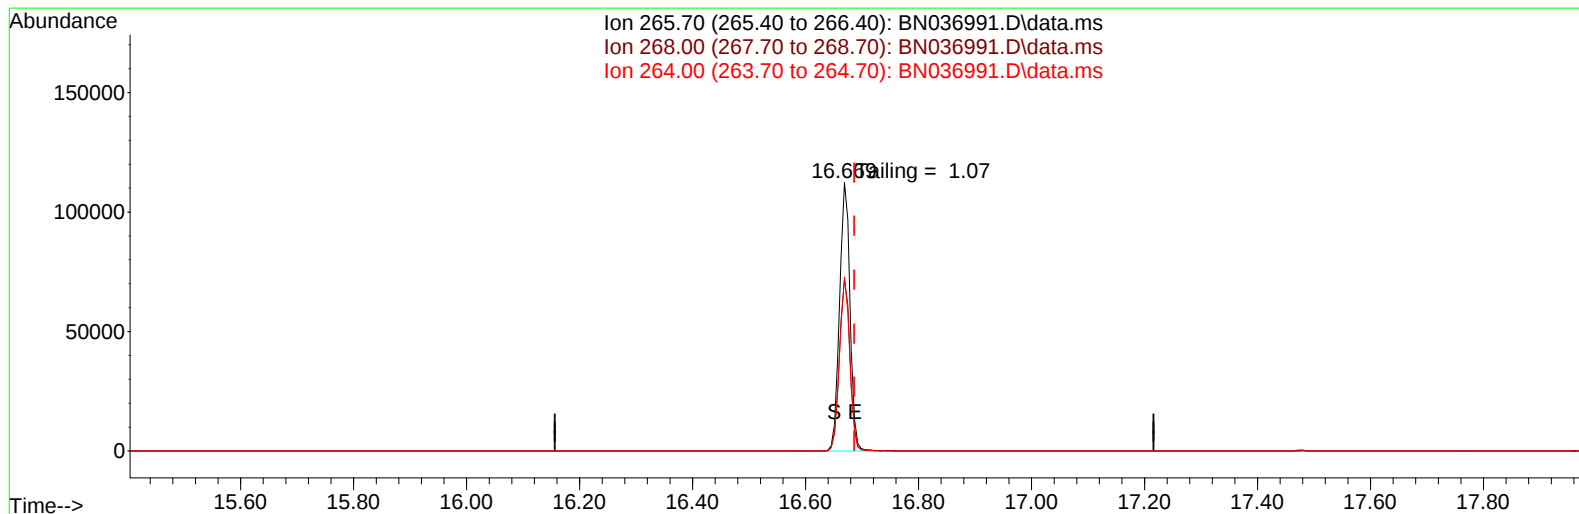

TIC: BN036991.D\data.ms

(70) Pentachlorophenol (C)

16.669min (-0.017) 16816.24 ng




response 143451

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.16
264.00	61.60	64.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051325\
Data File : BN036991.D
Acq On : 13 May 2025 09:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 13 15:42:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

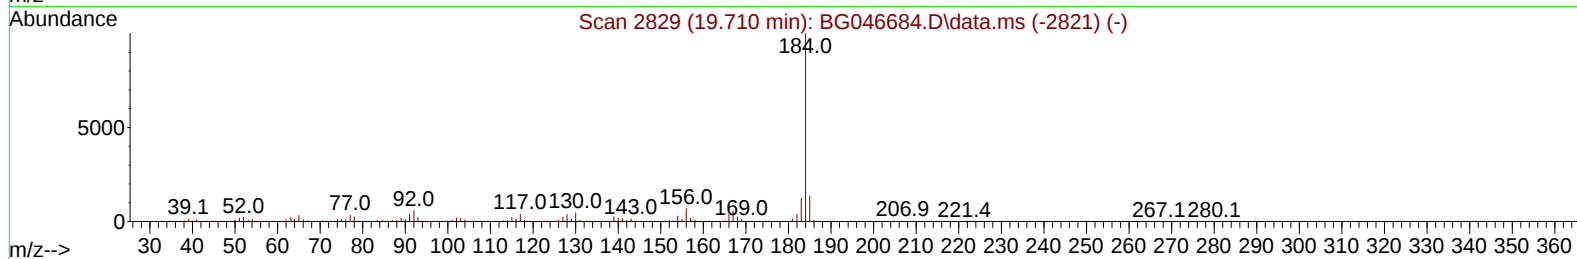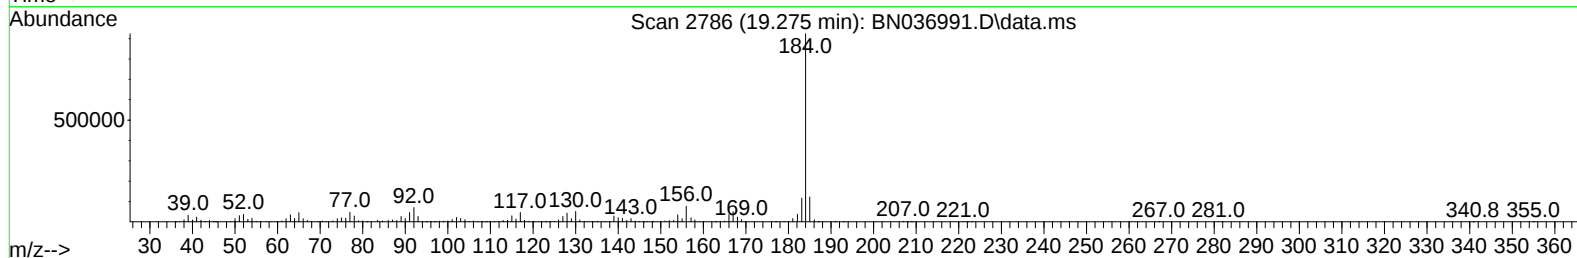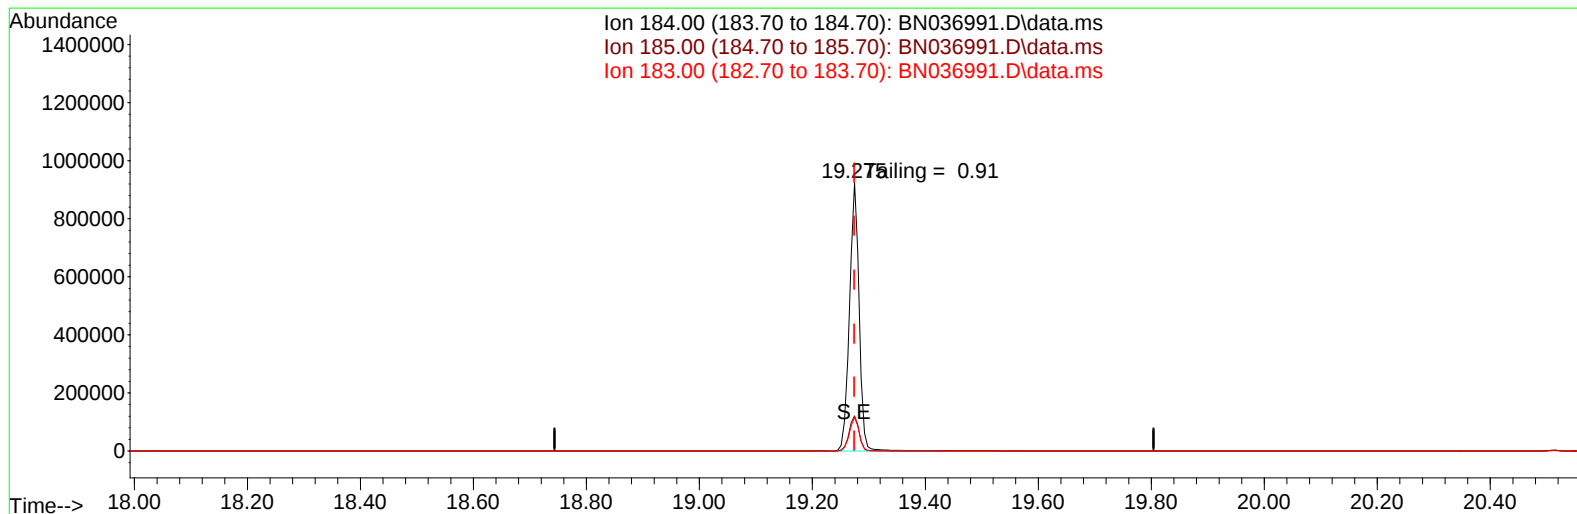

TIC: BN036991.D\data.ms

(77) Benzidine

19.275min (+ 0.000) 0.00 ng m

response 1098248

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.12
183.00	13.20	12.64
0.00	0.00	0.00