
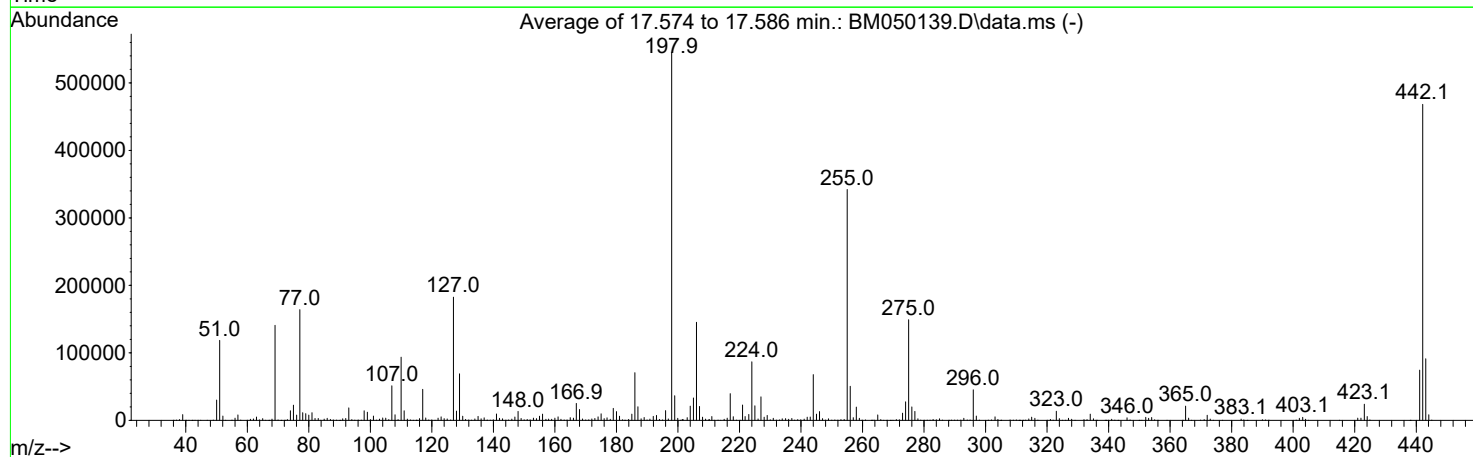


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050825\
 Data File : BM050139.D
 Acq On : 08 May 2025 09:59
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 08 12:03:21 2025

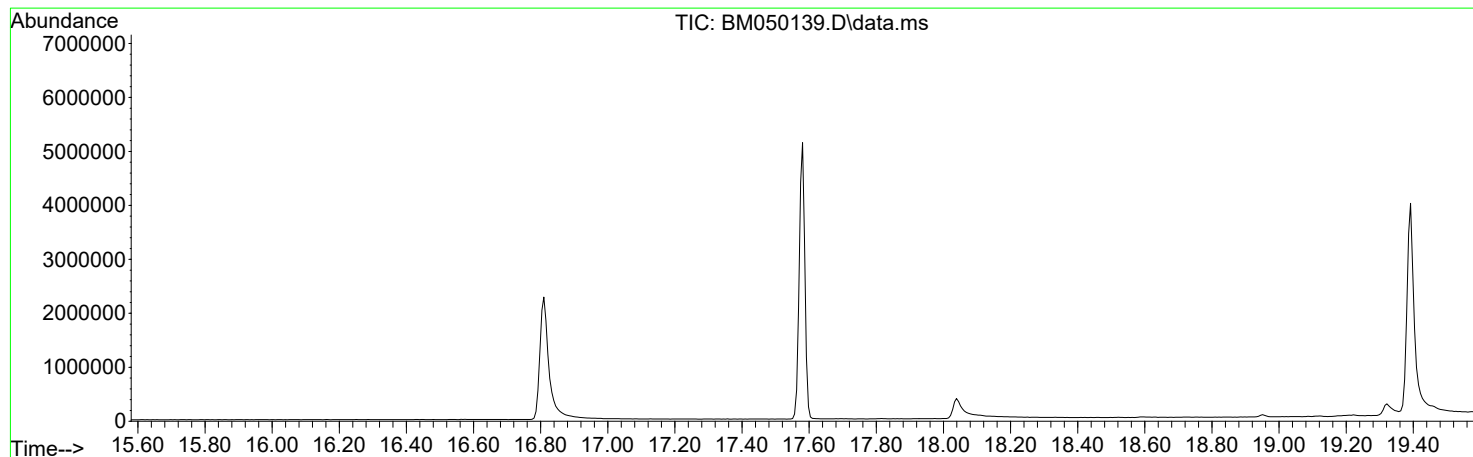

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.7	118511	PASS
68	69	0.00	2	1.4	2018	PASS
69	198	0.00	100	25.8	140810	PASS
70	69	0.00	2	0.4	628	PASS
127	198	10	80	33.5	182635	PASS
197	198	0.00	2	0.4	2160	PASS
198	198	100	100	100.0	545024	PASS
199	198	5	9	6.7	36635	PASS
275	198	10	60	27.3	149061	PASS
365	198	1	100	3.9	21040	PASS
441	198	0.01	100	13.6	74341	PASS
442	442	50	100	100.0	468224	PASS
443	442	15	24	19.5	91352	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/8/2025	BNA_M	<u>BM050139.D</u>
Compound Name	Response	Retention Time
DDT	1691185	20.621
DDD	32020	20.186
DDE	2862	19.674
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
34882	1726067	2.02

Instrument :
 BNA_M
 Client:Sampled :
 DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050825\
 Data File : BM050139.D
 Acq On : 08 May 2025 09:59
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: May 08 11:50:03 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 28 18:09:16 2025
 Response via : Initial Calibration

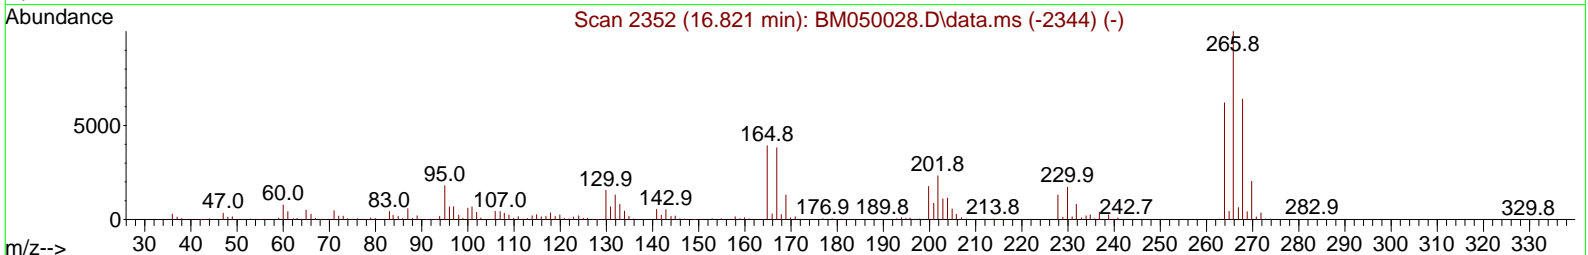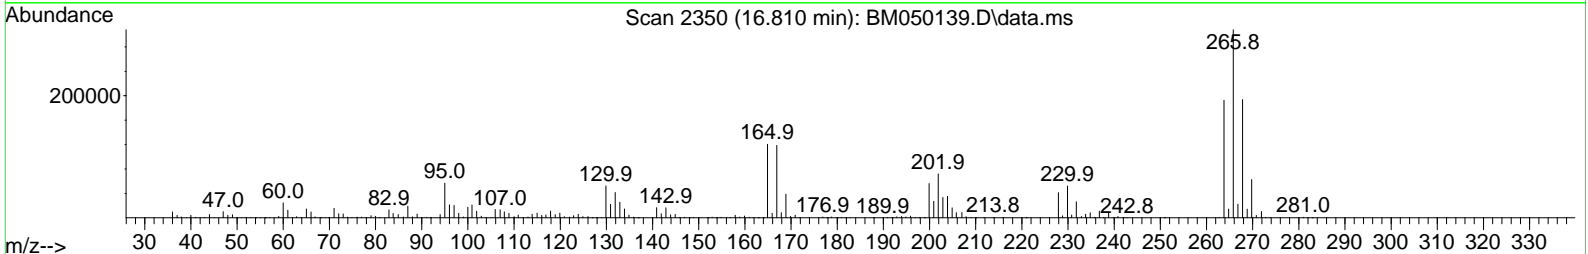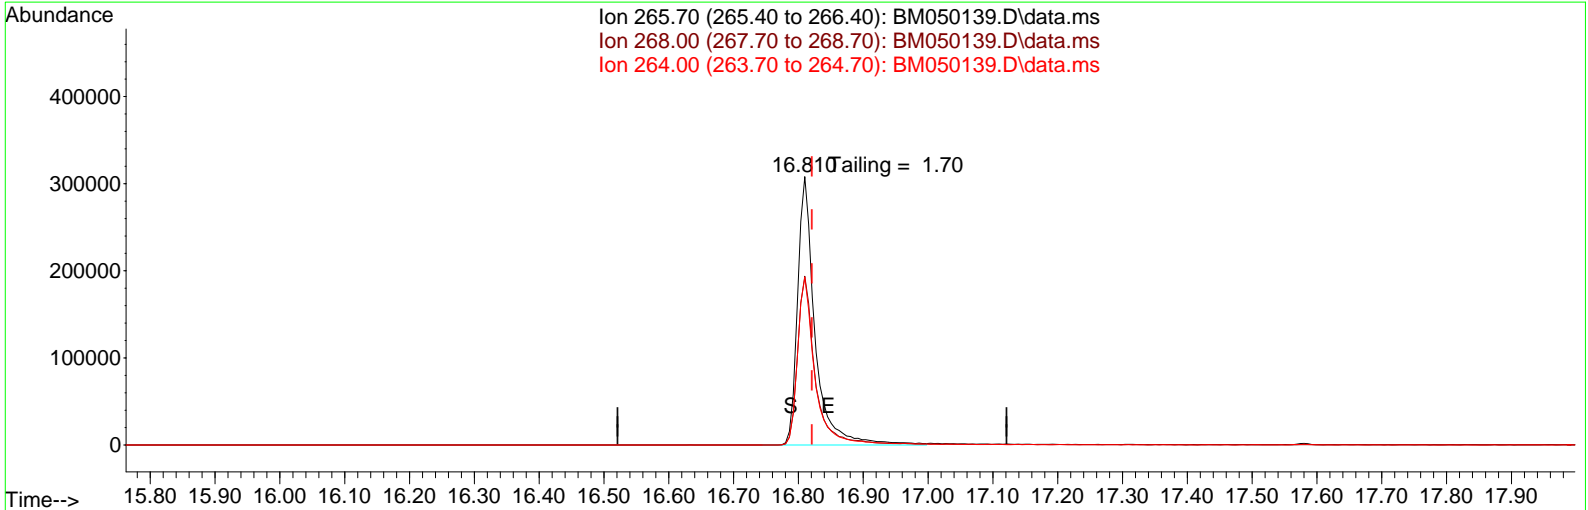

TIC: BM050139.D\data.ms

(70) Pentachlorophenol (C)

16.810min (-0.011) 902047.65 ng




response 580377

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	62.90
264.00	62.00	62.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050825\
 Data File : BM050139.D
 Acq On : 08 May 2025 09:59
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 DFTPP

Quant Time: May 08 11:50:03 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 28 18:09:16 2025
 Response via : Initial Calibration

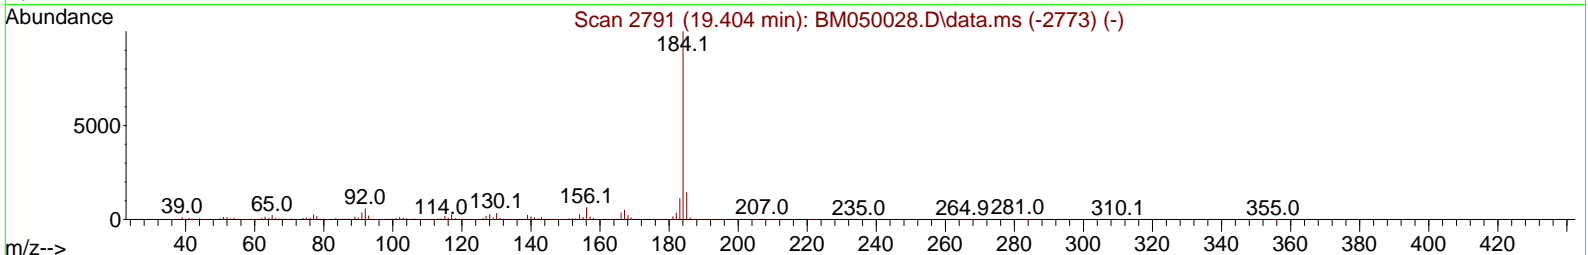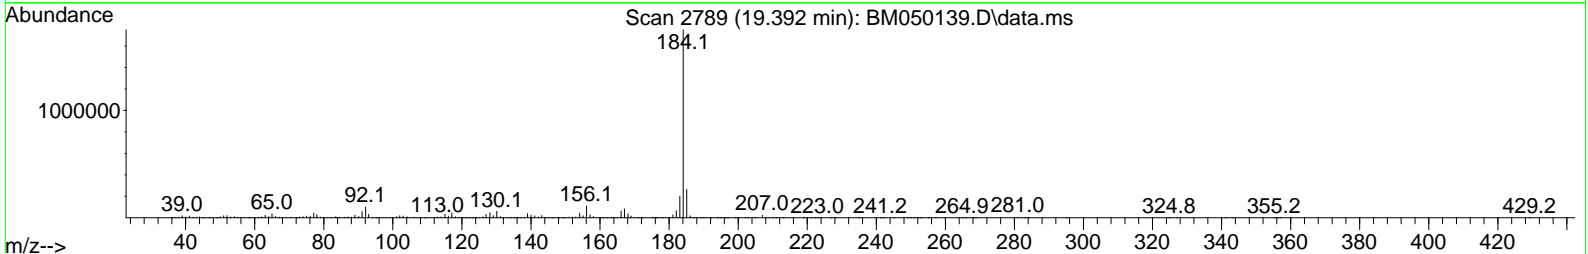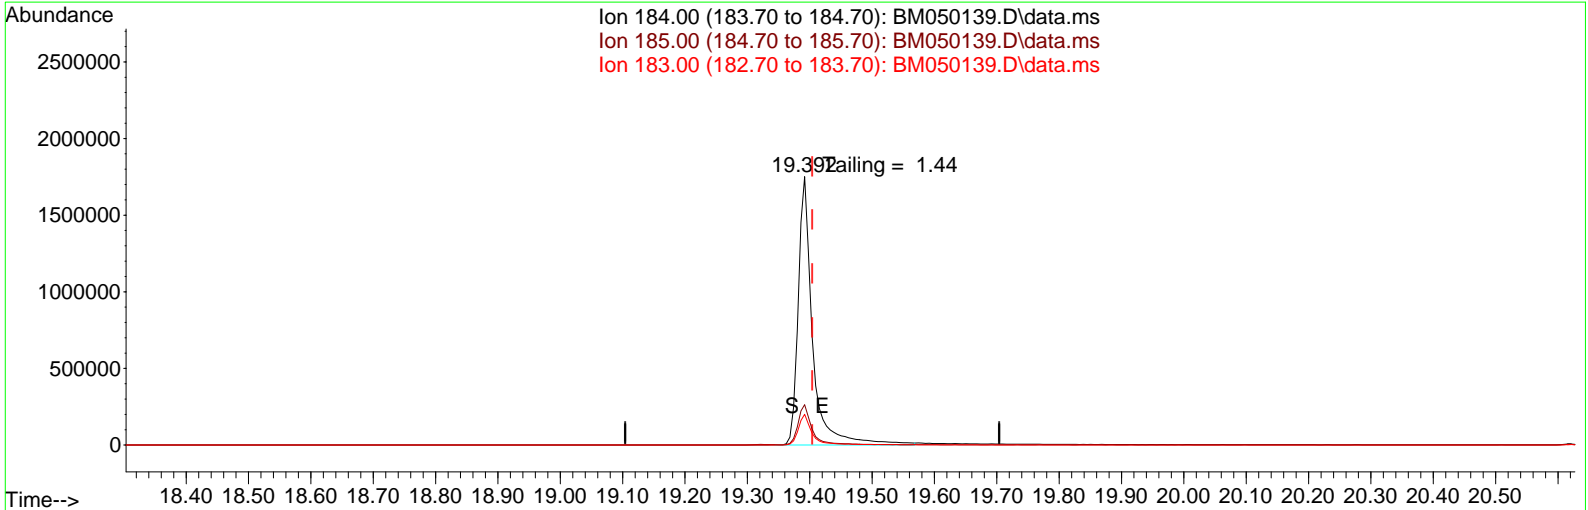

TIC: BM050139.D\data.ms

(77) Benzidine

19.392min (-0.012) 27949.85 ng

response 2854293

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.07
183.00	11.10	11.46
0.00	0.00	0.00