

Process Report

Order ID : Q1880

Date	Bottle ID	Lab Sample Number	InComing Vacuum	Canister ID	Can Size	Reg ID	Reg Size	Batch Code	Certification ID
04/25/2025	B2504018	Q1880-11	-1.4	10602	6 L	10203		C2504004	VL042307.D Seq :vl041025 TUNE : VL042299.D ICAL : VL042177.D CCAL : VL042300.D MB : VL042301.D
04/25/2025	B2504018	Q1880-10	-8.0	10326	6 L	10476		C2504004	VL042307.D Seq :vl041025 TUNE : VL042299.D ICAL : VL042177.D CCAL : VL042300.D MB : VL042301.D
04/25/2025	B2504018	Q1880-09	-7.1	10300	6 L	10110		C2504003	VL042219.D Seq :VL040425 TUNE : VL042214.D ICAL : VL042177.D CCAL : VL042215.D MB : VL042216.D
04/25/2025	B2504018	Q1880-08	-2.7	10282	6 L	10771		C2504005	VL042308.D Seq :vl041025 TUNE : VL042299.D ICAL : VL042177.D CCAL : VL042300.D MB : VL042301.D
04/25/2025	B2504018	Q1880-07	-6.3	10158	6 L	10785		C2504004	VL042307.D Seq :vl041025 TUNE : VL042299.D ICAL : VL042177.D CCAL : VL042300.D MB : VL042301.D
04/25/2025	B2504018	Q1880-06	-7.0	10024	6 L	10206		C2504005	VL042308.D Seq :vl041025 TUNE : VL042299.D ICAL : VL042177.D CCAL : VL042300.D MB : VL042301.D

Process Report

Order ID : Q1880

Date	Bottle ID	Lab Sample Number	InComing Vacuum	Canister ID	Can Size	Reg ID	Reg Size	Batch Code	Certification ID
04/25/2025	B2504019	Q1880-04	-5.9	10333	6 L	10222		C2504006	VL042316.D Seq :VL041125 TUNE : VL042311.D ICAL : VL042177.D CCAL : VL042312.D MB : VL042313.D
04/25/2025	B2504019	Q1880-05	-4.7	10401	6 L	10236		C2504007	VL042330.D Seq :VL041525 TUNE : VL042325.D ICAL : VL042177.D CCAL : VL042326.D MB : VL042327.D
04/25/2025	B2504019	Q1880-03	-5.9	10323	6 L	10537		C2504007	VL042330.D Seq :VL041525 TUNE : VL042325.D ICAL : VL042177.D CCAL : VL042326.D MB : VL042327.D
04/25/2025	B2504019	Q1880-02	-6.3	10268	6 L	10183		C2504007	VL042330.D Seq :VL041525 TUNE : VL042325.D ICAL : VL042177.D CCAL : VL042326.D MB : VL042327.D
04/25/2025	B2504019	Q1880-01	-6.7	10258	6 L	10567		C2504007	VL042330.D Seq :VL041525 TUNE : VL042325.D ICAL : VL042177.D CCAL : VL042326.D MB : VL042327.D



Canister Cleaning

284 Sheffield Street, Mountainside, New Jersey 07092 Phone : 908 789 8900 Fax : 908 789 8922

Canister Batch : C2504003

Type of Canister : 6 L

Cleaning Date : 04/03/2025

Analyst : SAM

Oven Temperature :

Canister	Vaccum After Cleaning ("Hg)	Vaccum After Cleaning Date	Analysis Date	VAC 24Hr ("Hg)	Vaccum After 24hr Date	New Sample Number	QC Canister	File
10300	-30	04/03/2025	04/04/2025	-30	04/04/2025	Q1880-09	10300	VL042219.D
10334	-30	04/03/2025	04/04/2025	-30	04/04/2025	Q1802-03	10300	VL042219.D



Canister Cleaning

284 Sheffield Street, Mountainside, New Jersey 07092 Phone : 908 789 8900 Fax : 908 789 8922

Canister Batch : C2504004

Type of Canister : 6 L

Cleaning Date : 04/09/2025

Analyst : SAM

Oven Temperature : 125.0 c

Canister	Vaccum After Cleaning ("Hg)	Vaccum After Cleaning Date	Analysis Date	VAC 24Hr ("Hg)	Vaccum After 24hr Date	New Sample Number	QC Canister	File
10602	-30	04/10/2025	04/10/2025	-30	04/11/2025	Q1880-11	10604	VL042307.D
10604	-30	04/10/2025	04/10/2025	-30	04/11/2025		10604	VL042307.D
10158	-30	04/10/2025	04/10/2025	-30	04/11/2025	Q1880-07	10604	VL042307.D
10326	-30	04/10/2025	04/10/2025	-30	04/11/2025	Q1880-10	10604	VL042307.D



Canister Cleaning

284 Sheffield Street, Mountainside, New Jersey 07092 Phone : 908 789 8900 Fax : 908 789 8922

Canister Batch : C2504005

Type of Canister : 6 L

Cleaning Date : 04/08/2025

Analyst : SAM

Oven Temperature : 125.0 c

Canister	Vaccum After Cleaning ("Hg)	Vaccum After Cleaning Date	Analysis Date	VAC 24Hr ("Hg)	Vaccum After 24hr Date	New Sample Number	QC Canister	File
10283	-30	04/09/2025	04/10/2025	-30	04/10/2025	Q1927-03	10445	VL042308.D
10445	-30	04/09/2025	04/10/2025	-30	04/10/2025	Q1927-05	10445	VL042308.D
10267	-30	04/09/2025	04/10/2025	-30	04/10/2025	Q1927-02	10445	VL042308.D
10282	-30	04/09/2025	04/10/2025	-30	04/10/2025	Q1880-08	10445	VL042308.D
10607	-30	04/09/2025	04/10/2025	-30	04/10/2025	Q1927-06	10607	VL042310.D
10320	-30	04/09/2025	04/10/2025	-30	04/10/2025	Q1927-04	10445	VL042308.D
10024	-30	04/09/2025	04/10/2025	-30	04/10/2025	Q1880-06	10445	VL042308.D
10197	-30	04/09/2025	04/10/2025	-30	04/10/2025	Q1927-01	10197	VL042309.D



Canister Cleaning

284 Sheffield Street, Mountainside, New Jersey 07092 Phone : 908 789 8900 Fax : 908 789 8922

Canister Batch : C2504006

Type of Canister : 6 L

Cleaning Date : 04/10/2025

Analyst : SAM

Oven Temperature : 125.0 c

Canister	Vaccum After Cleaning ("Hg)	Vaccum After Cleaning Date	Analysis Date	VAC 24Hr ("Hg)	Vaccum After 24hr Date	New Sample Number	QC Canister	File
10153	-30	04/11/2025	04/11/2025	-30	04/14/2025	Q1844-02	10596	VL042316.D
10596	-30	04/11/2025	04/11/2025	-30	04/14/2025	Q1881-01	10596	VL042316.D
10303	-30	04/11/2025	04/11/2025	-30	04/14/2025	Q1843-02	10596	VL042316.D
10296	-30	04/11/2025	04/11/2025	-30	04/14/2025		10596	VL042316.D
10321	-30	04/11/2025	04/11/2025	-30	04/14/2025	Q1844-01	10596	VL042316.D
10333	-30	04/11/2025	04/11/2025	-30	04/14/2025	Q1880-04	10596	VL042316.D
10279	-30	04/11/2025	04/11/2025	-30	04/14/2025		10596	VL042316.D
10605	-30	04/11/2025	04/11/2025	-30	04/14/2025	Q1843-01	10596	VL042316.D



Canister Cleaning

284 Sheffield Street, Mountainside, New Jersey 07092 Phone : 908 789 8900 Fax : 908 789 8922

Canister Batch : C2504007

Type of Canister : 6 L

Cleaning Date : 04/14/2025

Analyst : SAM

Oven Temperature : 125.0 c



Canister	Vaccum After Cleaning ("Hg)	Vaccum After Cleaning Date	Analysis Date	VAC 24Hr ("Hg)	Vaccum After 24hr Date	New Sample Number	QC Canister	File
10599	-30	04/15/2025	04/15/2025	-30	04/16/2025		10401	VL042330.D
10595	-30	04/15/2025	04/15/2025	-30	04/16/2025	Q1908-02	10401	VL042330.D
10268	-30	04/15/2025	04/15/2025	-30	04/16/2025	Q1880-02	10401	VL042330.D
10323	-30	04/15/2025	04/15/2025	-30	04/16/2025	Q1880-03	10401	VL042330.D
10258	-30	04/15/2025	04/15/2025	-30	04/16/2025	Q1880-01	10401	VL042330.D
10198	-30	04/15/2025	04/15/2025	-30	04/16/2025		10401	VL042330.D
10053	-30	04/15/2025	04/15/2025	-30	04/16/2025		10401	VL042330.D
10401	-30	04/15/2025	04/15/2025	-30	04/16/2025	Q1880-05	10401	VL042330.D

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
Data File : VL042171.D
Acq On : 27 Mar 2025 07:44
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Mar 28 02:00:52 2025



AutoFind: Scans 3177, 3178, 3179; Background Corrected with Scan 3150

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.0	87995	PASS
75	95	30	66	56.3	215296	PASS
95	95	100	100	100.0	382268	PASS
96	95	5	9	6.6	25383	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	63.8	243904	PASS
175	174	4	9	8.0	19539	PASS
176	174	93	101	95.7	233493	PASS
177	176	5	9	6.8	15877	PASS

Method Path : Z:\voasrv\HPCHEM1\MSVOA_L\methods\

Method File : VL032725AIR.M

Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022

Last Update : Fri Mar 28 02:00:52 2025

Response Via : Initial Calibration

Calibration Files

0.03=VL042177.D 0.1 =VL042176.D 0.5 =VL042175.D 1 =VL042174.D 2 =VL042173.D 10 =VL042172.D 15 =VL042178.D

Compound	0.03	0.1	0.5	1	2	10	15	Avg	%RSD

1) I Bromochloromethane	-----ISTD-----								
2) T Dichlorodifluo...			1.602	1.514	1.482	1.404	1.380	1.476	6.03
3) Chlorodifluoro...			1.622	1.541	1.514	1.457	1.408	1.508	5.41
4) Chloromethane			0.660	0.597	0.618	0.573	0.570	0.603	6.17
5) T Vinyl Chloride	0.882	0.705	0.635	0.576	0.584	0.549	0.546	0.639	18.84
6) T Bromomethane			0.327	0.268	0.266	0.256	0.250	0.273	11.20
7) Chloroethane			0.286	0.248	0.223	0.227	0.226	0.242	10.92
8) T Dichlorotetra...			1.306	1.283	1.274	1.214	1.211	1.257	3.40
9) T Propene			0.734	0.736	0.698	0.660	0.630	0.691	6.69
10) T Heptane			1.847	1.940	1.897	1.792	1.719	1.839	4.73
11) T Trichlorofluor...			1.562	1.457	1.480	1.339	1.346	1.437	6.59
12) T 1,1,2-Trichlor...			1.247	1.215	1.188	1.120	1.135	1.181	4.52
13) Ethanol			0.110	0.086	0.073	0.029	0.028	0.065	55.48
14) T Bromoethene			0.529	0.447	0.460	0.417	0.409	0.452	10.47
15) T Acetone			1.699	1.573	1.469	1.113	1.139	1.399	18.73
16) T 1,3-Butadiene			0.952	0.705	0.608	0.573	0.577	0.683	23.38
17) tert-Butyl alc...			1.935	1.799	1.756	1.618	1.601	1.742	7.91
18) T 1,1-Dichloroet...			0.624	0.565	0.560	0.504	0.507	0.552	8.99
19) T Isopropyl Alcohol			1.016	0.800	0.738	0.702	0.689	0.789	16.99
20) T Methylene Chlo...			0.624	0.563	0.545	0.438	0.435	0.521	15.85
21) T Allyl Chloride			1.067	1.022	1.020	0.902	0.921	0.986	7.25
22) T trans-1,2-Dich...			0.704	0.701	0.621	0.590	0.575	0.638	9.56
23) T Vinyl Acetate			0.754	0.692	0.550	0.498	0.532	0.605	18.40
24) T 1,1-Dichloroet...			1.247	1.208	1.187	1.122	1.149	1.183	4.17
25) T Ethyl Acetate			4.017	3.619	3.703	3.457	3.353	3.630	7.06
26) T Hexane			1.507	1.462	1.383	1.333	1.325	1.402	5.71
27) T Carbon Disulfide			1.608	1.512	1.538	1.436	1.423	1.503	5.07
28) T Methyl tert-Bu...			0.921	0.886	0.894	0.831	0.832	0.873	4.56
29) T Chloroform			2.233	2.068	2.071	1.932	1.956	2.052	5.81
30) T Cyclohexane			1.337	1.238	1.211	1.162	1.140	1.217	6.33
31) T cis-1,2-Dichlo...			1.507	1.460	1.426	1.371	1.353	1.423	4.44
32) T 1,1,1-Trichlor...	3.151	2.495	2.279	2.201	2.152	2.062	2.105	2.349	16.23

33) I 1,4-Difluorobenzene	-----ISTD-----								
34) T 2-Butanone			0.754	0.771	0.770	0.667	0.664	0.725	7.58
35) T Carbon Tetrach...	1.069	0.782	0.709	0.732	0.748	0.703	0.725	0.781	16.60
36) T Benzene			1.049	1.027	1.013	0.934	0.934	0.991	5.47
37) T 1,2-Dichloroet...			0.613	0.569	0.563	0.537	0.556	0.568	4.95
38) T Trichloroethene	0.463	0.437	0.438	0.408	0.398	0.374	0.378	0.414	8.00
39) T 1,2-Dichloropr...			0.386	0.373	0.365	0.337	0.344	0.361	5.68

Method Path : Z:\voasrv\HPCHEM1\MSVOA_L\methods\											
Method File : VL032725AIR.M											
40)	T	1,4-Dioxane			0.234	0.197	0.191	0.169	0.167	0.192	14.08
41)	T	Tetrahydrofuran			0.439	0.425	0.432	0.398	0.393	0.418	4.98
42)	T	Bromodichlorom...			0.778	0.779	0.802	0.769	0.785	0.782	1.58
43)		Methyl Methacr...			0.442	0.451	0.408	0.403	0.394	0.420	6.03
44)	T	2,2,4-Trimethy...			1.781	1.689	1.723	1.608	1.576	1.675	5.00
45)	T	t-1,3-Dichloro...			0.474	0.447	0.453	0.439	0.440	0.450	3.15
46)	T	cis-1,3-Dichlo...			0.549	0.560	0.566	0.550	0.535	0.552	2.12
47)	T	1,1,2-Trichlor...			0.419	0.382	0.379	0.364	0.365	0.382	5.88
48)	T	Dibromochlorom...			0.651	0.641	0.663	0.636	0.644	0.647	1.62
49)	T	Bromoform			0.566	0.588	0.597	0.582	0.570	0.581	2.18
50)	T	4-Methyl-2-Pen...			1.286	1.214	1.211	1.027	1.008	1.149	10.79
51)	T	2-Hexanone			0.999	1.018	1.031	0.844	0.827	0.944	10.56
52)	T	Tetrachloroethene	0.572	0.359	0.401	0.361	0.371	0.343	0.345	0.393	20.64
53)	T	Toluene			1.239	1.203	1.202	1.125	1.108	1.175	4.76
54)	T	1,2-Dibromoethane	0.574		0.543	0.538	0.520	0.508	0.510	0.532	4.74
-----ISTD-----											
55)	I	Chlorobenzene-d5									
56)		1,1,1,2-Tetrac...			0.576	0.575	0.576	0.510	0.515	0.550	6.30
57)	T	Chlorobenzene			1.024	0.979	0.994	0.875	0.871	0.949	7.46
58)	T	Ethyl Benzene			1.850	1.822	1.894	1.671	1.645	1.776	6.28
59)	T	m/p-Xylene			1.505	1.472	1.484	1.321	1.309	1.418	6.71
60)	T	o-Xylene			1.521	1.475	1.499	1.328	1.287	1.422	7.50
61)	T	Styrene			0.709	0.722	0.735	0.683	0.668	0.703	3.92
62)		Isopropylbenzene			2.290	2.199	2.261	1.962	1.920	2.126	8.14
63)	T	1,1,2,2-Tetrac...	0.986	0.800	0.907	0.889	0.893	0.796	0.777	0.864	8.78
64)		n-propylbenzene			0.578	0.581	0.576	0.499	0.502	0.547	7.81
65)		tert-Butylbenzene			2.190	2.071	2.144	1.736	1.691	1.966	11.96
66)	T	Benzyl Chloride			0.217	0.213	0.221	0.203	0.189	0.209	6.06
67)		sec-Butylbenzene			3.005	2.994	2.947	2.404	2.316	2.733	12.54
68)	S	1-Bromo-4-Fluo...	0.820	0.827	0.832	0.810	0.828	0.813	0.820	0.821	0.98
69)		p-Isopropyltol...			2.554	2.551	2.560	2.078	2.025	2.354	11.74
70)		n-Butylbenzene			2.536	2.598	2.682	2.137	2.082	2.407	11.51
71)		2-Chlorotoluene			1.717	1.728	1.759	1.538	1.510	1.650	7.07
72)	T	4-Ethyltoluene			1.834	1.859	1.929	1.629	1.601	1.770	8.26
73)	T	1,3,5-Trimethy...			1.616	1.671	1.677	1.387	1.381	1.546	9.71
74)	T	1,2,4-Trimethy...			1.994	1.958	1.966	1.510	1.478	1.781	14.74
75)	T	1,3-Dichlorobe...			1.036	1.022	1.063	0.882	0.882	0.977	8.99
76)	T	1,4-Dichlorobe...			1.030	1.017	1.040	0.888	0.886	0.972	8.05
77)	T	1,2-Dichlorobe...			1.012	1.031	1.014	0.850	0.850	0.951	9.78
78)	T	Hexachloro-1,3...			1.057	1.113	1.086	0.802	0.784	0.968	16.65
79)	T	Naphthalene	1.637		1.979	2.181	2.314	1.806	1.773	1.948	13.31
80)	T	Naphthalene,2-...			0.721	0.891	1.163	0.990	1.013	0.955	17.09
81)	T	1,2,4-Trichlor...			0.821	0.941	1.028	0.859	0.843	0.899	9.51

(#) = Out of Range

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
 Data File : VL042172.D
 Acq On : 27 Mar 2025 08:26
 Operator : SY/MD
 Sample : VSTDICCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICCC010

Manual Integrations
 APPROVED

Quant Time: Mar 28 01:31:57 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Mar 28 01:31:23 2025

Response via : Initial Calibration

Reviewed By : Semsettin Yesilyurt 03/31/2025
 Supervised By : Mahesh Dadoda 04/03/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.784	49	187002	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.952	114	545068	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.875	117	519536	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.371	95	422410	9.901	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.000%
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.496	85	262496	9.507	ppbv	100
3) Chlorodifluoromethane	1.473	51	272522	9.662	ppbv	100
4) Chloromethane	1.531	50	107099	9.491	ppbv	100
5) Vinyl Chloride	1.577	62	102699	8.925	ppbv	100
6) Bromomethane	1.664	94	47950	9.377	ppbv	100
7) Chloroethane	1.703	64	42516	9.387	ppbv	100
8) Dichlorotetrafluoroethane	1.551	85	227041	9.656	ppbv	100
9) Propene	1.483	41	123386	9.709	ppbv	100
10) Heptane	4.972	43	335086	9.744	ppbv	100
11) Trichlorofluoromethane	1.874	101	250349	9.318	ppbv	100
12) 1,1,2-Trichlorotrifluo...	2.137	101	209365	9.481	ppbv	100
13) Ethanol	1.719	45	5338	5.364	ppbv	100
14) Bromoethene	1.777	108	77999	9.220	ppbv	100
15) Acetone	1.832	43	208061	7.955	ppbv	100
16) 1,3-Butadiene	1.606	39	107104	9.105	ppbv	100
17) tert-Butyl alcohol	2.036	59	302616	9.290	ppbv	100
18) 1,1-Dichloroethene	2.030	96	94236	9.128	ppbv	100
19) Isopropyl Alcohol	1.884	45	131359	8.902	ppbv	100
20) Methylene Chloride	2.059	84	81828	8.401	ppbv	100
21) Allyl Chloride	2.091	41	168602	9.141	ppbv	100
22) trans-1,2-Dichloroethene	2.337	96	110371	9.149	ppbv	100
23) Vinyl Acetate	2.460	43	93080	8.563	ppbv	100
24) 1,1-Dichloroethane	2.405	63	209753	9.484	ppbv	100
25) Ethyl Acetate	2.833	43	646501	9.524	ppbv	100
26) Hexane	2.823	57	249331	9.510	ppbv	100
27) Carbon Disulfide	2.146	76	268507	9.550	ppbv	100
28) Methyl tert-Butyl Ether	2.438	73	155398	9.520	ppbv	100
29) Chloroform	2.845	83	361264	9.415	ppbv	100
30) Cyclohexane	3.852	84	217215	9.537	ppbv	100
31) cis-1,2-Dichloroethene	2.716	61	256425	9.634	ppbv	100
32) 1,1,1-Trichloroethane	3.363	97	385628	8.784	ppbv	100
34) 2-Butanone	2.554	43	363735	9.203	ppbv	100
35) Carbon Tetrachloride	3.758	117	382925	9.129	ppbv	100
36) Benzene	3.651	78	508860	9.417	ppbv	100
37) 1,2-Dichloroethane	3.214	62	292937	9.469	ppbv	100
38) Trichloroethene	4.545	130	204027	9.045	ppbv	100
39) 1,2-Dichloropropane	4.312	63	183439	9.321	ppbv	100
40) 1,4-Dioxane	4.577	88	92327	9.042	ppbv #	100
41) Tetrahydrofuran	3.049	42	216851	9.643	ppbv	100
42) Bromodichloromethane	4.483	83	418887	9.822	ppbv	100
43) Methyl Methacrylate	4.872	69	219399	9.618	ppbv	100
44) 2,2,4-Trimethylpentane	4.635	57	876649	9.600	ppbv	100
45) t-1,3-Dichloropropene	6.406	75	239180	9.746	ppbv	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
 Data File : VL042172.D
 Acq On : 27 Mar 2025 08:26
 Operator : SY/MD
 Sample : VSTDICCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICCC010

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 03/31/2025
 Supervised By : Mahesh Dadoda 04/03/2025

Quant Time: Mar 28 01:31:57 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2
 QLast Update : Fri Mar 28 01:31:23 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.593	75	300021	9.973	ppbv	100
47) 1,1,2-Trichloroethane	6.574	97	198176	9.526	ppbv	100
48) Dibromochloromethane	7.380	129	346499	9.828	ppbv	100
49) Bromoform	9.477	173	317189	10.021	ppbv	100
50) 4-Methyl-2-Pentanone	5.745	43	559800	8.934	ppbv	100
51) 2-Hexanone	7.432	43	460013	8.848	ppbv #	100
52) Tetrachloroethene	8.218	164	186912	8.722	ppbv	100
53) Toluene	6.927	91	613378	9.576	ppbv	100
54) 1,2-Dibromoethane	7.649	107	276797	9.536	ppbv	100
56) 1,1,1,2-Tetrachloroethane	8.917	131	265037	9.268	ppbv	100
57) Chlorobenzene	8.917	112	454511	9.223	ppbv	100
58) Ethyl Benzene	9.351	91	868003	9.406	ppbv	100
59) m/p-Xylene	9.549	91	1372806m	18.607	ppbv	
60) o-Xylene	9.960	91	689933	9.340	ppbv	100
61) Styrene	9.866	104	354697	9.706	ppbv	100
62) Isopropylbenzene	10.536	105	1019255	9.227	ppbv	100
63) 1,1,2,2-Tetrachloroethane	9.960	83	413392	9.210	ppbv	100
64) n-propylbenzene	10.986	120	259405	9.122	ppbv	100
65) tert-Butylbenzene	11.529	119	901951	8.828	ppbv	100
66) Benzyl Chloride	11.610	91	105411	9.724	ppbv	100
67) sec-Butylbenzene	11.766	105	1249106	8.796	ppbv	100
69) p-Isopropyltoluene	11.924	119	1079675	8.830	ppbv	100
70) n-Butylbenzene	12.277	91	1110351	8.879	ppbv	100
71) 2-Chlorotoluene	10.898	91	799102	9.320	ppbv	100
72) 4-Ethyltoluene	11.122	105	846232	9.200	ppbv	100
73) 1,3,5-Trimethylbenzene	11.199	105	720566	8.970	ppbv	100
74) 1,2,4-Trimethylbenzene	11.536	105	784745	8.480	ppbv	100
75) 1,3-Dichlorobenzene	11.604	146	458226	9.028	ppbv	100
76) 1,4-Dichlorobenzene	11.669	146	461371	9.134	ppbv	100
77) 1,2-Dichlorobenzene	11.944	146	441473	8.933	ppbv	100
78) Hexachloro-1,3-Butadiene	13.879	225	416735	8.284	ppbv	100
79) Naphthalene	13.510	128	938470	9.271	ppbv	100
80) Naphthalene,2-methyl-	14.455	142	514394	10.436	ppbv	100
81) 1,2,4-Trichlorobenzene	13.439	180	446420	9.561	ppbv	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
Data File : VL042172.D
Acq On : 27 Mar 2025 08:26
Operator : SY/MD
Sample : VSTDICCC010
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDICCC010

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 03/31/2025
Supervised By :Mahesh Dadoda 04/03/2025

Quant Time: Mar 28 01:31:57 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug
QLast Update : Fri Mar 28 01:31:23 2025
Response via : Initial Calibration



Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
 Data File : VL042173.D
 Acq On : 27 Mar 2025 08:59
 Operator : SY/MD
 Sample : VSTDICC002
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC002

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/31/2025
 Supervised By :Mahesh Dadoda 04/03/2025

Quant Time: Mar 28 01:32:52 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Mar 28 01:31:23 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.784	49	188395	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.952	114	546394	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.875	117	504538	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene 10.370 95 417532 10.077 ppbv 0.00
 Spiked Amount 10.000 Range 65 - 135 Recovery = 100.800%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.496	85	55859	2.008	ppbv	99
3) Chlorodifluoromethane	1.473	51	57045	2.007	ppbv	99
4) Chloromethane	1.531	50	23293	2.049	ppbv	94
5) Vinyl Chloride	1.576	62	21989	1.897	ppbv	99
6) Bromomethane	1.664	94	10027	1.946	ppbv	98
7) Chloroethane	1.703	64	8413	1.844	ppbv	92
8) Dichlorotetrafluoroethane	1.551	85	48008	2.027	ppbv	98
9) Propene	1.483	41	26295	2.054	ppbv	94
10) Heptane	4.972	43	71466	2.063	ppbv	99
11) Trichlorofluoromethane	1.874	101	55754	2.060	ppbv	99
12) 1,1,2-Trichlorotrifluo...	2.136	101	44761	2.012	ppbv	98
13) Ethanol	1.719	45	2748m	2.741	ppbv	
14) Bromoethene	1.780	108	17323	2.033	ppbv #	89
15) Acetone	1.832	43	55365	2.101	ppbv	95
16) 1,3-Butadiene	1.606	39	22894	1.932	ppbv	95
17) tert-Butyl alcohol	2.039	59	66174	2.016	ppbv	100
18) 1,1-Dichloroethene	2.030	96	21103	2.029	ppbv	95
19) Isopropyl Alcohol	1.884	45	27804	1.870	ppbv #	35
20) Methylene Chloride	2.059	84	20518	2.091	ppbv	96
21) Allyl Chloride	2.094	41	38425	2.068	ppbv	99
22) trans-1,2-Dichloroethene	2.337	96	23384	1.924	ppbv	92
23) Vinyl Acetate	2.460	43	20736	1.894	ppbv #	97
24) 1,1-Dichloroethane	2.405	63	44740	2.008	ppbv	99
25) Ethyl Acetate	2.832	43	139516	2.040	ppbv	99
26) Hexane	2.823	57	52095	1.972	ppbv	92
27) Carbon Disulfide	2.146	76	57969	2.047	ppbv #	76
28) Methyl tert-Butyl Ether	2.437	73	33703	2.049	ppbv	99
29) Chloroform	2.845	83	78043	2.019	ppbv	95
30) Cyclohexane	3.852	84	45641	1.989	ppbv	99
31) cis-1,2-Dichloroethene	2.719	61	53713	2.003	ppbv	96
32) 1,1,1-Trichloroethane	3.363	97	81070	1.833	ppbv	99
34) 2-Butanone	2.554	43	84157	2.124	ppbv	99
35) Carbon Tetrachloride	3.758	117	81735	1.944	ppbv	96
36) Benzene	3.651	78	110727	2.044	ppbv	97
37) 1,2-Dichloroethane	3.214	62	61476	1.982	ppbv	97
38) Trichloroethene	4.541	130	43501	1.924	ppbv	97
39) 1,2-Dichloropropane	4.308	63	39912	2.023	ppbv	93
40) 1,4-Dioxane	4.587	88	20884m	2.040	ppbv	
41) Tetrahydrofuran	3.056	42	47262	2.097	ppbv	99
42) Bromodichloromethane	4.483	83	87640	2.050	ppbv	99
43) Methyl Methacrylate	4.878	69	44624	1.952	ppbv	97
44) 2,2,4-Trimethylpentane	4.632	57	188282	2.057	ppbv	100
45) t-1,3-Dichloropropene	6.406	75	49461	2.011	ppbv	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
 Data File : VL042173.D
 Acq On : 27 Mar 2025 08:59
 Operator : SY/MD
 Sample : VSTDICC002
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC002

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 03/31/2025
 Supervised By : Mahesh Dadoda 04/03/2025

Quant Time: Mar 28 01:32:52 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2
 QLast Update : Fri Mar 28 01:31:23 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
46) cis-1,3-Dichloropropene	5.593	75	61829	2.050	ppbv	#	91
47) 1,1,2-Trichloroethane	6.577	97	41387	1.985	ppbv		95
48) Dibromochloromethane	7.383	129	72441	2.050	ppbv		100
49) Bromoform	9.477	173	65221	2.056	ppbv		98
50) 4-Methyl-2-Pentanone	5.752	43	132328	2.107	ppbv		99
51) 2-Hexanone	7.435	43	112681	2.162	ppbv	#	99
52) Tetrachloroethene	8.221	164	40558	1.888	ppbv		98
53) Toluene	6.923	91	131314	2.045	ppbv		99
54) 1,2-Dibromoethane	7.648	107	56799	1.952	ppbv		90
56) 1,1,1,2-Tetrachloroethane	8.920	131	58141	2.093	ppbv		97
57) Chlorobenzene	8.914	112	100308	2.096	ppbv	#	94
58) Ethyl Benzene	9.351	91	191114	2.132	ppbv		96
59) m/p-Xylene	9.548	91	299531m	4.181	ppbv		
60) o-Xylene	9.959	91	151292	2.109	ppbv		98
61) Styrene	9.865	104	74134	2.089	ppbv		98
62) Isopropylbenzene	10.535	105	228191	2.127	ppbv		99
63) 1,1,2,2-Tetrachloroethane	9.956	83	90114	2.067	ppbv		99
64) n-propylbenzene	10.985	120	58105	2.104	ppbv		92
65) tert-Butylbenzene	11.529	119	216336	2.180	ppbv		99
66) Benzyl Chloride	11.610	91	22272	2.116	ppbv		95
67) sec-Butylbenzene	11.762	105	297381	2.156	ppbv		99
69) p-Isopropyltoluene	11.921	119	258357	2.176	ppbv		100
70) n-Butylbenzene	12.277	91	270616	2.228	ppbv		99
71) 2-Chlorotoluene	10.898	91	177487	2.132	ppbv		100
72) 4-Ethyltoluene	11.121	105	194660	2.179	ppbv		99
73) 1,3,5-Trimethylbenzene	11.199	105	169221	2.169	ppbv		96
74) 1,2,4-Trimethylbenzene	11.532	105	198351	2.207	ppbv		96
75) 1,3-Dichlorobenzene	11.604	146	107217	2.175	ppbv		97
76) 1,4-Dichlorobenzene	11.668	146	104925	2.139	ppbv		99
77) 1,2-Dichlorobenzene	11.943	146	102310	2.132	ppbv		99
78) Hexachloro-1,3-Butadiene	13.879	225	109539	2.242	ppbv		99
79) Naphthalene	13.510	128	233451	2.375	ppbv		97
80) Naphthalene,2-methyl-	14.455	142	117313	2.451	ppbv		99
81) 1,2,4-Trichlorobenzene	13.435	180	103765	2.288	ppbv		97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
 Data File : VL042174.D
 Acq On : 27 Mar 2025 09:30
 Operator : SY/MD
 Sample : VSTDICC001
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC001

Manual Integrations
 APPROVED

Quant Time: Mar 28 01:33:49 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Mar 28 01:31:23 2025

Response via : Initial Calibration

Reviewed By : Semsettin Yesilyurt 03/31/2025
 Supervised By : Mahesh Dadoda 04/03/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.784	49	186244	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.952	114	537244	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.879	117	499830	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.371	95	404753	9.861	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	98.600%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.496	85	28203	1.026	ppbv	99
3) Chlorodifluoromethane	1.473	51	28693	1.021	ppbv	94
4) Chloromethane	1.531	50	11111	0.989	ppbv	99
5) Vinyl Chloride	1.577	62	10723	0.936	ppbv	98
6) Bromomethane	1.667	94	4984	0.979	ppbv	97
7) Chloroethane	1.703	64	4622	1.025	ppbv	100
8) Dichlorotetrafluoroethane	1.554	85	23886	1.020	ppbv	98
9) Propene	1.483	41	13699m	1.082	ppbv	
10) Heptane	4.975	43	36132	1.055	ppbv	100
11) Trichlorofluoromethane	1.875	101	27136	1.014	ppbv	96
12) 1,1,2-Trichlorotrifluo...	2.137	101	22629	1.029	ppbv	99
13) Ethanol	1.719	45	1610m	1.624	ppbv	
14) Bromoethene	1.781	108	8330	0.989	ppbv #	82
15) Acetone	1.836	43	29294	1.125	ppbv	95
16) 1,3-Butadiene	1.606	39	13133	1.121	ppbv	97
17) tert-Butyl alcohol	2.040	59	33500	1.033	ppbv	97
18) 1,1-Dichloroethene	2.033	96	10532	1.024	ppbv	89
19) Isopropyl Alcohol	1.884	45	14903	1.014	ppbv #	38
20) Methylene Chloride	2.059	84	10481	1.080	ppbv	93
21) Allyl Chloride	2.095	41	19039	1.036	ppbv	99
22) trans-1,2-Dichloroethene	2.341	96	13051m	1.086	ppbv	
23) Vinyl Acetate	2.464	43	12883m	1.190	ppbv	
24) 1,1-Dichloroethane	2.409	63	22505	1.022	ppbv	99
25) Ethyl Acetate	2.836	43	67402	0.997	ppbv #	96
26) Hexane	2.823	57	27223	1.043	ppbv	98
27) Carbon Disulfide	2.146	76	28167	1.006	ppbv #	47
28) Methyl tert-Butyl Ether	2.441	73	16501	1.015	ppbv	95
29) Chloroform	2.845	83	38516	1.008	ppbv	96
30) Cyclohexane	3.852	84	23052	1.016	ppbv	97
31) cis-1,2-Dichloroethene	2.716	61	27187	1.026	ppbv	89
32) 1,1,1-Trichloroethane	3.363	97	40993	0.938	ppbv	99
34) 2-Butanone	2.557	43	41423	1.063	ppbv	98
35) Carbon Tetrachloride	3.758	117	39345	0.952	ppbv	93
36) Benzene	3.651	78	55156	1.036	ppbv	94
37) 1,2-Dichloroethane	3.218	62	30543	1.002	ppbv	98
38) Trichloroethene	4.545	130	21906	0.985	ppbv	93
39) 1,2-Dichloropropane	4.312	63	20020	1.032	ppbv	99
40) 1,4-Dioxane	4.593	88	10592m	1.052	ppbv	
41) Tetrahydrofuran	3.056	42	22818	1.029	ppbv	97
42) Bromodichloromethane	4.483	83	41864	0.996	ppbv	90
43) Methyl Methacrylate	4.875	69	24233m	1.078	ppbv	
44) 2,2,4-Trimethylpentane	4.632	57	90727	1.008	ppbv	96
45) t-1,3-Dichloropropene	6.403	75	23993m	0.992	ppbv	

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
 Data File : VL042174.D
 Acq On : 27 Mar 2025 09:30
 Operator : SY/MD
 Sample : VSTDICC001
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC001

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 03/31/2025
 Supervised By : Mahesh Dadoda 04/03/2025

Quant Time: Mar 28 01:33:49 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Mar 28 01:31:23 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.593	75	30063	1.014	ppbv	93
47) 1,1,2-Trichloroethane	6.577	97	20546	1.002	ppbv	96
48) Dibromochloromethane	7.383	129	34425	0.991	ppbv	100
49) Bromoform	9.481	173	31610	1.013	ppbv	98
50) 4-Methyl-2-Pentanone	5.752	43	65226m	1.056	ppbv	
51) 2-Hexanone	7.438	43	54680	1.067	ppbv #	100
52) Tetrachloroethene	8.222	164	19415	0.919	ppbv	95
53) Toluene	6.927	91	64612	1.023	ppbv	99
54) 1,2-Dibromoethane	7.652	107	28879	1.009	ppbv	95
56) 1,1,1,2-Tetrachloroethane	8.924	131	28764	1.045	ppbv #	87
57) Chlorobenzene	8.917	112	48930	1.032	ppbv	93
58) Ethyl Benzene	9.348	91	91086	1.026	ppbv	97
59) m/p-Xylene	9.529	91	147162m	2.073	ppbv	
60) o-Xylene	9.960	91	73702	1.037	ppbv	96
61) Styrene	9.866	104	36110	1.027	ppbv	97
62) Isopropylbenzene	10.536	105	109897	1.034	ppbv	98
63) 1,1,2,2-Tetrachloroethane	9.960	83	44431	1.029	ppbv	99
64) n-propylbenzene	10.986	120	29054	1.062	ppbv	98
65) tert-Butylbenzene	11.526	119	103520	1.053	ppbv	96
66) Benzyl Chloride	11.614	91	10660	1.022	ppbv #	93
67) sec-Butylbenzene	11.762	105	149660	1.095	ppbv	97
69) p-Isopropyltoluene	11.921	119	127509	1.084	ppbv	99
70) n-Butylbenzene	12.280	91	129860	1.079	ppbv	99
71) 2-Chlorotoluene	10.898	91	86356	1.047	ppbv	100
72) 4-Ethyltoluene	11.122	105	92912	1.050	ppbv	99
73) 1,3,5-Trimethylbenzene	11.199	105	83497	1.080	ppbv	92
74) 1,2,4-Trimethylbenzene	11.533	105	97858	1.099	ppbv	94
75) 1,3-Dichlorobenzene	11.604	146	51096	1.046	ppbv	99
76) 1,4-Dichlorobenzene	11.669	146	50841	1.046	ppbv	99
77) 1,2-Dichlorobenzene	11.944	146	51523	1.084	ppbv	99
78) Hexachloro-1,3-Butadiene	13.879	225	55611	1.149	ppbv	97
79) Naphthalene	13.510	128	109031	1.120	ppbv	99
80) Naphthalene,2-methyl-	14.455	142	44518	0.939	ppbv	99
81) 1,2,4-Trichlorobenzene	13.436	180	47040	1.047	ppbv	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
Data File : VL042174.D
Acq On : 27 Mar 2025 09:30
Operator : SY/MD
Sample : VSTDICC001
Misc : 400mL/MSVOA_L
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 03/31/2025
Supervised By :Mahesh Dadoda 04/03/2025

Quant Time: Mar 28 01:33:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug
QLast Update : Fri Mar 28 01:31:23 2025
Response via : Initial Calibration



Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
 Data File : VL042175.D
 Acq On : 27 Mar 2025 10:01
 Operator : SY/MD
 Sample : VSTDICC0.5
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC0.5

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 03/31/2025
 Supervised By : Mahesh Dadoda 04/03/2025

Quant Time: Mar 28 01:34:42 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Mar 28 01:31:23 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.784	49	180502	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.952	114	523832	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.875	117	485078	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene 10.370 95 403513 10.130 ppbv 0.00
 Spiked Amount 10.000 Range 65 - 135 Recovery = 101.300%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.496	85	14455	0.542	ppbv	95
3) Chlorodifluoromethane	1.473	51	14637	0.538	ppbv #	89
4) Chloromethane	1.531	50	5956	0.547	ppbv	94
5) Vinyl Chloride	1.577	62	5732	0.516	ppbv	92
6) Bromomethane	1.664	94	2949	0.597	ppbv	95
7) Chloroethane	1.703	64	2582	0.591	ppbv #	87
8) Dichlorotetrafluoroethane	1.551	85	11783	0.519	ppbv	98
9) Propene	1.483	41	6622m	0.540	ppbv	
10) Heptane	4.972	43	16673	0.502	ppbv	89
11) Trichlorofluoromethane	1.874	101	14099	0.544	ppbv	92
12) 1,1,2-Trichlorotrifluo...	2.136	101	11252	0.528	ppbv	99
13) Ethanol	1.722	45	997	1.038	ppbv #	36
14) Bromoethene	1.780	108	4770	0.584	ppbv #	86
15) Acetone	1.835	43	15331	0.607	ppbv #	85
16) 1,3-Butadiene	1.606	39	8594	0.757	ppbv	82
17) tert-Butyl alcohol	2.039	59	17467	0.556	ppbv	97
18) 1,1-Dichloroethene	2.030	96	5634	0.565	ppbv #	92
19) Isopropyl Alcohol	1.884	45	9171	0.644	ppbv #	39
20) Methylene Chloride	2.059	84	5634	0.599	ppbv #	93
21) Allyl Chloride	2.091	41	9632	0.541	ppbv	89
22) trans-1,2-Dichloroethene	2.334	96	6353	0.546	ppbv	83
23) Vinyl Acetate	2.457	43	6809	0.649	ppbv #	91
24) 1,1-Dichloroethane	2.405	63	11258	0.527	ppbv	97
25) Ethyl Acetate	2.836	43	36258	0.553	ppbv	98
26) Hexane	2.823	57	13605	0.538	ppbv	92
27) Carbon Disulfide	2.146	76	14510	0.535	ppbv #	1
28) Methyl tert-Butyl Ether	2.437	73	8310	0.527	ppbv #	89
29) Chloroform	2.845	83	20149	0.544	ppbv	98
30) Cyclohexane	3.852	84	12063m	0.549	ppbv	
31) cis-1,2-Dichloroethene	2.719	61	13601	0.529	ppbv	92
32) 1,1,1-Trichloroethane	3.360	97	20567	0.485	ppbv	100
34) 2-Butanone	2.557	43	19739	0.520	ppbv	96
35) Carbon Tetrachloride	3.755	117	18558	0.460	ppbv	93
36) Benzene	3.651	78	27488	0.529	ppbv #	87
37) 1,2-Dichloroethane	3.214	62	16062	0.540	ppbv	100
38) Trichloroethene	4.538	130	11460m	0.529	ppbv	
39) 1,2-Dichloropropane	4.308	63	10123	0.535	ppbv	92
40) 1,4-Dioxane	4.593	88	6121m	0.624	ppbv	
41) Tetrahydrofuran	3.059	42	11509m	0.533	ppbv	
42) Bromodichloromethane	4.483	83	20374	0.497	ppbv #	98
43) Methyl Methacrylate	4.875	69	11583m	0.528	ppbv	
44) 2,2,4-Trimethylpentane	4.632	57	46646	0.532	ppbv	95
45) t-1,3-Dichloropropene	6.406	75	12404	0.526	ppbv #	79

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
 Data File : VL042175.D
 Acq On : 27 Mar 2025 10:01
 Operator : SY/MD
 Sample : VSTDICC0.5
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC0.5

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/31/2025
 Supervised By :Mahesh Dadoda 04/03/2025

Quant Time: Mar 28 01:34:42 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Mar 28 01:31:23 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.593	75	14374m	0.497	ppbv	
47) 1,1,2-Trichloroethane	6.574	97	10972m	0.549	ppbv	
48) Dibromochloromethane	7.380	129	17042	0.503	ppbv	99
49) Bromoform	9.480	173	14828	0.487	ppbv	98
50) 4-Methyl-2-Pentanone	5.758	43	33674	0.559	ppbv	97
51) 2-Hexanone	7.438	43	26154	0.523	ppbv #	100
52) Tetrachloroethene	8.218	164	10502	0.510	ppbv	94
53) Toluene	6.923	91	32444	0.527	ppbv	98
54) 1,2-Dibromoethane	7.648	107	14220	0.510	ppbv	99
56) 1,1,1,2-Tetrachloroethane	8.920	131	13959	0.523	ppbv #	1
57) Chlorobenzene	8.914	112	24826	0.540	ppbv #	91
58) Ethyl Benzene	9.348	91	44862	0.521	ppbv	96
59) m/p-Xylene	9.542	91	73028m	1.060	ppbv	
60) o-Xylene	9.959	91	36879	0.535	ppbv	98
61) Styrene	9.866	104	17198	0.504	ppbv	96
62) Isopropylbenzene	10.536	105	55531	0.538	ppbv	99
63) 1,1,2,2-Tetrachloroethane	9.959	83	21989	0.525	ppbv	96
64) n-propylbenzene	10.985	120	14030	0.528	ppbv	95
65) tert-Butylbenzene	11.526	119	53115	0.557	ppbv	100
66) Benzyl Chloride	11.613	91	5263	0.520	ppbv	97
67) sec-Butylbenzene	11.762	105	72879	0.550	ppbv	98
69) p-Isopropyltoluene	11.921	119	61933	0.542	ppbv	100
70) n-Butylbenzene	12.277	91	61507	0.527	ppbv	99
71) 2-Chlorotoluene	10.895	91	41637	0.520	ppbv	95
72) 4-Ethyltoluene	11.121	105	44473	0.518	ppbv #	94
73) 1,3,5-Trimethylbenzene	11.199	105	39190	0.523	ppbv	97
74) 1,2,4-Trimethylbenzene	11.532	105	48370	0.560	ppbv	97
75) 1,3-Dichlorobenzene	11.600	146	25122	0.530	ppbv	100
76) 1,4-Dichlorobenzene	11.668	146	24991	0.530	ppbv	97
77) 1,2-Dichlorobenzene	11.943	146	24548	0.532	ppbv	96
78) Hexachloro-1,3-Butadiene	13.879	225	25636	0.546	ppbv	99
79) Naphthalene	13.510	128	47990	0.508	ppbv	95
80) Naphthalene,2-methyl-	14.458	142	17486	0.380	ppbv	98
81) 1,2,4-Trichlorobenzene	13.436	180	19924	0.457	ppbv	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
Data File : VL042175.D
Acq On : 27 Mar 2025 10:01
Operator : SY/MD
Sample : VSTDICC0.5
Misc : 400mL/MSVOA_L
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDICC0.5

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 03/31/2025
Supervised By :Mahesh Dadoda 04/03/2025

Quant Time: Mar 28 01:34:42 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug
QLast Update : Fri Mar 28 01:31:23 2025
Response via : Initial Calibration



Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
 Data File : VL042176.D
 Acq On : 27 Mar 2025 10:32
 Operator : SY/MD
 Sample : VSTDICC0.1
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC0.1

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/31/2025
 Supervised By :Mahesh Dadoda 04/03/2025

Quant Time: Mar 28 01:35:34 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2
 QLast Update : Fri Mar 28 01:31:23 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.787	49	180740	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.955	114	528028	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.878	117	481506	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.374	95	398069	10.067	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	100.700%
Target Compounds						
5) Vinyl Chloride	1.580	62	1274	0.115	ppbv #	42
32) 1,1,1-Trichloroethane	3.366	97	4509m	0.106	ppbv	
35) Carbon Tetrachloride	3.768	117	4131m	0.102	ppbv	
38) Trichloroethene	4.551	130	2306m	0.106	ppbv	
52) Tetrachloroethene	8.225	164	1895m	0.091	ppbv	
54) 1,2-Dibromoethane	7.652	107	3033m	0.108	ppbv	
63) 1,1,2,2-Tetrachloroethane	9.966	83	3852m	0.093	ppbv	
79) Naphthalene	13.513	128	7882	0.084	ppbv #	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
Data File : VL042176.D
Acq On : 27 Mar 2025 10:32
Operator : SY/MD
Sample : VSTDICC0.1
Misc : 400mL/MSVOA_L
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDICC0.1

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 03/31/2025
Supervised By : Mahesh Dadoda 04/03/2025

Quant Time: Mar 28 01:35:34 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug
QLast Update : Fri Mar 28 01:31:23 2025
Response via : Initial Calibration



Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
 Data File : VL042177.D
 Acq On : 27 Mar 2025 11:03
 Operator : SY/MD
 Sample : VSTDICC0.03
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC0.03

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 03/31/2025
 Supervised By : Mahesh Dadoda 04/03/2025

Quant Time: Mar 28 01:36:24 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 2
 QLast Update : Fri Mar 28 01:31:23 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.787	49	178058	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.955	114	512915	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.878	117	475617	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.374	95	389935	9.983	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.800%
Target Compounds						
					Qvalue	
5) Vinyl Chloride	1.580	62	471m	0.043	ppbv	
32) 1,1,1-Trichloroethane	3.366	97	1683m	0.040	ppbv	
35) Carbon Tetrachloride	3.758	117	1645m	0.042	ppbv	
38) Trichloroethene	4.541	130	712m	0.034	ppbv	
52) Tetrachloroethene	8.208	164	880m	0.044	ppbv	
63) 1,1,2,2-Tetrachloroethane	9.963	83	1407m	0.034	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
Data File : VL042177.D
Acq On : 27 Mar 2025 11:03
Operator : SY/MD
Sample : VSTDICC0.03
Misc : 400mL/MSVOA_L
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDICC0.03

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 03/31/2025
Supervised By :Mahesh Dadoda 04/03/2025

Quant Time: Mar 28 01:36:24 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug
QLast Update : Fri Mar 28 01:31:23 2025
Response via : Initial Calibration



Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
 Data File : VL042178.D
 Acq On : 27 Mar 2025 11:36
 Operator : SY/MD
 Sample : VSTDICC015
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC015

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 03/31/2025
 Supervised By : Mahesh Dadoda 04/03/2025

Quant Time: Mar 28 01:37:01 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Mar 28 01:31:23 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.784	49	173372	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.952	114	499360	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.878	117	473077	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	10.374	95	387777	9.981	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.800%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.495	85	358962	14.023	ppbv	99
3) Chlorodifluoromethane	1.473	51	366164	14.002	ppbv	98
4) Chloromethane	1.531	50	148133	14.160	ppbv	98
5) Vinyl Chloride	1.576	62	141938	13.304	ppbv	97
6) Bromomethane	1.667	94	65113	13.734	ppbv	99
7) Chloroethane	1.703	64	58820	14.007	ppbv	99
8) Dichlorotetrafluoroethane	1.550	85	314834	14.442	ppbv	98
9) Propene	1.482	41	163799	13.902	ppbv	95
10) Heptane	4.972	43	446949	14.019	ppbv	99
11) Trichlorofluoromethane	1.874	101	349967	14.050	ppbv	98
12) 1,1,2-Trichlorotrifluo...	2.136	101	295217	14.419	ppbv	99
13) Ethanol	1.719	45	7382	8.001	ppbv	92
14) Bromoethene	1.780	108	106436	13.571	ppbv	98
15) Acetone	1.832	43	296254	12.218	ppbv	98
16) 1,3-Butadiene	1.605	39	150122	13.766	ppbv	100
17) tert-Butyl alcohol	2.039	59	416362	13.787	ppbv	99
18) 1,1-Dichloroethene	2.029	96	131720	13.762	ppbv	99
19) Isopropyl Alcohol	1.884	45	179117	13.093	ppbv	100
20) Methylene Chloride	2.059	84	113183	12.533	ppbv	95
21) Allyl Chloride	2.094	41	239440	14.002	ppbv	99
22) trans-1,2-Dichloroethene	2.337	96	149455	13.362	ppbv	98
23) Vinyl Acetate	2.460	43	138419	13.736	ppbv #	96
24) 1,1-Dichloroethane	2.405	63	298760	14.570	ppbv	99
25) Ethyl Acetate	2.832	43	871882	13.855	ppbv	100
26) Hexane	2.822	57	344636	14.178	ppbv	98
27) Carbon Disulfide	2.146	76	370022	14.196	ppbv	97
28) Methyl tert-Butyl Ether	2.437	73	216463	14.303	ppbv	95
29) Chloroform	2.845	83	508614	14.297	ppbv	100
30) Cyclohexane	3.852	84	296458	14.040	ppbv	99
31) cis-1,2-Dichloroethene	2.719	61	351945	14.262	ppbv	97
32) 1,1,1-Trichloroethane	3.363	97	547329	13.448	ppbv	99
34) 2-Butanone	2.554	43	497020	13.726	ppbv	99
35) Carbon Tetrachloride	3.758	117	543385	14.140	ppbv	100
36) Benzene	3.651	78	699549	14.131	ppbv	98
37) 1,2-Dichloroethane	3.214	62	416544	14.697	ppbv	99
38) Trichloroethene	4.541	130	283430	13.715	ppbv	98
39) 1,2-Dichloropropane	4.308	63	257891	14.304	ppbv	99
40) 1,4-Dioxane	4.577	88	124925	13.354	ppbv #	91
41) Tetrahydrofuran	3.049	42	294634	14.301	ppbv	100
42) Bromodichloromethane	4.483	83	587772	15.043	ppbv	99
43) Methyl Methacrylate	4.874	69	295300	14.130	ppbv	99
44) 2,2,4-Trimethylpentane	4.635	57	1180275	14.108	ppbv	99
45) t-1,3-Dichloropropene	6.405	75	329360	14.649	ppbv	96

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
 Data File : VL042178.D
 Acq On : 27 Mar 2025 11:36
 Operator : SY/MD
 Sample : VSTDICC015
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC015

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 03/31/2025
 Supervised By : Mahesh Dadoda 04/03/2025

Quant Time: Mar 28 01:37:01 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Mar 28 01:31:23 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.593	75	400813	14.542	ppbv	98
47) 1,1,2-Trichloroethane	6.577	97	273137	14.331	ppbv	98
48) Dibromochloromethane	7.383	129	482431	14.936	ppbv	100
49) Bromoform	9.480	173	427143	14.730	ppbv	99
50) 4-Methyl-2-Pentanone	5.745	43	755146	13.155	ppbv	99
51) 2-Hexanone	7.431	43	619419	13.005	ppbv #	99
52) Tetrachloroethene	8.221	164	258356	13.159	ppbv	95
53) Toluene	6.926	91	829648	14.137	ppbv	100
54) 1,2-Dibromoethane	7.645	107	381823	14.359	ppbv	97
56) 1,1,1,2-Tetrachloroethane	8.920	131	365410	14.032	ppbv	99
57) Chlorobenzene	8.917	112	618201	13.777	ppbv	100
58) Ethyl Benzene	9.351	91	1167096	13.889	ppbv	97
59) m/p-Xylene	9.548	91	1857561m	27.651	ppbv	
60) o-Xylene	9.962	91	913234	13.577	ppbv	99
61) Styrene	9.865	104	474195	14.250	ppbv	99
62) Isopropylbenzene	10.535	105	1362416	13.544	ppbv	99
63) 1,1,2,2-Tetrachloroethane	9.959	83	551386	13.491	ppbv	99
64) n-propylbenzene	10.985	120	356118	13.753	ppbv	94
65) tert-Butylbenzene	11.529	119	1200149	12.901	ppbv	98
66) Benzyl Chloride	11.613	91	134397	13.615	ppbv	100
67) sec-Butylbenzene	11.765	105	1643629	12.711	ppbv	99
69) p-Isopropyltoluene	11.924	119	1437016	12.906	ppbv	98
70) n-Butylbenzene	12.280	91	1477443	12.975	ppbv	99
71) 2-Chlorotoluene	10.898	91	1071432	13.724	ppbv	99
72) 4-Ethyltoluene	11.121	105	1136415	13.569	ppbv	99
73) 1,3,5-Trimethylbenzene	11.202	105	979783	13.395	ppbv	99
74) 1,2,4-Trimethylbenzene	11.535	105	1048874	12.447	ppbv	92
75) 1,3-Dichlorobenzene	11.607	146	626015	13.545	ppbv	99
76) 1,4-Dichlorobenzene	11.668	146	628694	13.668	ppbv	100
77) 1,2-Dichlorobenzene	11.947	146	602844	13.396	ppbv	100
78) Hexachloro-1,3-Butadiene	13.882	225	556392	12.147	ppbv	99
79) Naphthalene	13.513	128	1258479	13.653	ppbv	98
80) Naphthalene,2-methyl-	14.455	142	718900	16.018	ppbv	98
81) 1,2,4-Trichlorobenzene	13.439	180	598416	14.075	ppbv	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
Data File : VL042178.D
Acq On : 27 Mar 2025 11:36
Operator : SY/MD
Sample : VSTDIC015
Misc : 400mL/MSVOA_L
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDIC015

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 03/31/2025
Supervised By :Mahesh Dadoda 04/03/2025

Quant Time: Mar 28 01:37:01 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug
QLast Update : Fri Mar 28 01:31:23 2025
Response via : Initial Calibration



Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
 Data File : VL042179.D
 Acq On : 27 Mar 2025 12:23
 Operator : SY/MD
 Sample : VSTDICV010
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 ICVVL032725

Quant Time: Mar 28 02:05:15 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 03/31/2025
 Supervised By : Mahesh Dadoda 04/03/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.784	49	174350	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.952	114	498105	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.878	117	473357	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.374	95	379929	9.774	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	97.700%

Target Compounds	Qvalue					
2) Dichlorodifluoromethane	1.496	85	245714	9.545	ppbv	100
3) Chlorodifluoromethane	1.473	51	247046	9.394	ppbv	97
4) Chloromethane	1.531	50	98527	9.365	ppbv	98
5) Vinyl Chloride	1.577	62	95578	8.573	ppbv	97
6) Bromomethane	1.667	94	41950	8.799	ppbv	97
7) Chloroethane	1.703	64	37400	8.856	ppbv	94
8) Dichlorotetrafluoroethane	1.551	85	213819	9.753	ppbv	95
9) Propene	1.483	41	105338	8.739	ppbv	99
10) Heptane	4.972	43	298768	9.318	ppbv	100
11) Trichlorofluoromethane	1.874	101	236793	9.453	ppbv	97
12) 1,1,2-Trichlorotrifluo...	2.136	101	193965	9.421	ppbv	98
13) Ethanol	1.719	45	5773	5.066	ppbv	97
14) Bromoethene	1.780	108	73572	9.328	ppbv	97
15) Acetone	1.832	43	198300	8.132	ppbv	98
16) 1,3-Butadiene	1.606	39	97840	8.216	ppbv	99
17) tert-Butyl alcohol	2.039	59	276195	9.094	ppbv	99
18) 1,1-Dichloroethene	2.033	96	87137	9.053	ppbv	89
19) Isopropyl Alcohol	1.884	45	122768	8.923	ppbv	98
20) Methylene Chloride	2.059	84	72813	8.018	ppbv	97
21) Allyl Chloride	2.094	41	157418	9.154	ppbv	99
22) trans-1,2-Dichloroethene	2.337	96	101141	9.092	ppbv	93
23) Vinyl Acetate	2.460	43	90260	8.553	ppbv #	97
24) 1,1-Dichloroethane	2.405	63	197968	9.600	ppbv	99
25) Ethyl Acetate	2.832	43	592585	9.364	ppbv	99
26) Hexane	2.823	57	231125	9.455	ppbv	99
27) Carbon Disulfide	2.146	76	248834	9.493	ppbv	97
28) Methyl tert-Butyl Ether	2.437	73	146470	9.624	ppbv	95
29) Chloroform	2.845	83	344106	9.619	ppbv	100
30) Cyclohexane	3.852	84	197897	9.323	ppbv	98
31) cis-1,2-Dichloroethene	2.719	61	234487	9.449	ppbv	96
32) 1,1,1-Trichloroethane	3.363	97	365364	8.921	ppbv	99
34) 2-Butanone	2.554	43	331236	9.171	ppbv	99
35) Carbon Tetrachloride	3.758	117	363392	9.339	ppbv	98
36) Benzene	3.651	78	461261	9.341	ppbv	99
37) 1,2-Dichloroethane	3.217	62	273559	9.676	ppbv	99
38) Trichloroethene	4.541	130	191746	9.306	ppbv	97
39) 1,2-Dichloropropane	4.311	63	170839	9.500	ppbv	95
40) 1,4-Dioxane	4.577	88	80592	8.443	ppbv #	97
41) Tetrahydrofuran	3.052	42	196163	9.431	ppbv	99
42) Bromodichloromethane	4.486	83	384006	9.853	ppbv	100
43) Methyl Methacrylate	4.878	69	195339	9.344	ppbv	99
44) 2,2,4-Trimethylpentane	4.635	57	787400	9.436	ppbv	99
45) t-1,3-Dichloropropene	6.409	75	212335	9.467	ppbv	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
 Data File : VL042179.D
 Acq On : 27 Mar 2025 12:23
 Operator : SY/MD
 Sample : VSTDICV010
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 ICSVVL032725

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 03/31/2025
 Supervised By : Mahesh Dadoda 04/03/2025

Quant Time: Mar 28 02:05:15 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Mar 28 02:00:52 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.593	75	265101	9.643	ppbv	98
47) 1,1,2-Trichloroethane	6.577	97	183228	9.638	ppbv	98
48) Dibromochloromethane	7.383	129	322766	10.018	ppbv	100
49) Bromoform	9.480	173	285149	9.858	ppbv	99
50) 4-Methyl-2-Pentanone	5.749	43	500791	8.749	ppbv	99
51) 2-Hexanone	7.432	43	410889	8.741	ppbv #	99
52) Tetrachloroethene	8.221	164	173420	8.855	ppbv	93
53) Toluene	6.927	91	556897	9.514	ppbv	99
54) 1,2-Dibromoethane	7.645	107	256930	9.695	ppbv	98
56) 1,1,1,2-Tetrachloroethane	8.920	131	249270	9.567	ppbv	99
57) Chlorobenzene	8.917	112	422531	9.411	ppbv	98
58) Ethyl Benzene	9.351	91	791360	9.412	ppbv	98
59) m/p-Xylene	9.548	91	1260340m	18.772	ppbv	
60) o-Xylene	9.959	91	632918	9.404	ppbv	99
61) Styrene	9.866	104	315910	9.488	ppbv	99
62) Isopropylbenzene	10.539	105	944938	9.388	ppbv	100
63) 1,1,2,2-Tetrachloroethane	9.959	83	382635	9.357	ppbv	99
64) n-propylbenzene	10.985	120	244547	9.439	ppbv	98
65) tert-Butylbenzene	11.529	119	843828	9.065	ppbv	98
66) Benzyl Chloride	11.613	91	86804	8.789	ppbv	97
67) sec-Butylbenzene	11.765	105	1172636	9.063	ppbv	100
69) p-Isopropyltoluene	11.924	119	1019694	9.153	ppbv	100
70) n-Butylbenzene	12.280	91	1038548	9.115	ppbv	100
71) 2-Chlorotoluene	10.898	91	732874	9.382	ppbv	100
72) 4-Ethyltoluene	11.125	105	785185	9.370	ppbv	99
73) 1,3,5-Trimethylbenzene	11.202	105	673541	9.203	ppbv	98
74) 1,2,4-Trimethylbenzene	11.536	105	729155	8.648	ppbv	94
75) 1,3-Dichlorobenzene	11.607	146	426573	9.224	ppbv	99
76) 1,4-Dichlorobenzene	11.672	146	426318	9.263	ppbv	100
77) 1,2-Dichlorobenzene	11.947	146	412180	9.154	ppbv	99
78) Hexachloro-1,3-Butadiene	13.882	225	356386	7.776	ppbv	100
79) Naphthalene	13.513	128	773311	8.385	ppbv	99
80) Naphthalene,2-methyl-	14.455	142	323443	7.151	ppbv	99
81) 1,2,4-Trichlorobenzene	13.439	180	363863	8.553	ppbv	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
Data File : VL042179.D
Acq On : 27 Mar 2025 12:23
Operator : SY/MD
Sample : VSTDICV010
Misc : 400mL/MSVOA_L
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
ICVVL032725

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 03/31/2025
Supervised By : Mahesh Dadoda 04/03/2025

Quant Time: Mar 28 02:05:15 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug
QLast Update : Fri Mar 28 02:00:52 2025
Response via : Initial Calibration



Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
 Data File : VL042179.D
 Acq On : 27 Mar 2025 12:23
 Operator : SY/MD
 Sample : VSTDICV010
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 ICSVVL032725

Quant Time: Mar 28 02:05:15 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Min. RRF : 0.050 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	Bromochloromethane	1.000	1.000	0.0	93	0.00
2 T	Dichlorodifluoromethane	1.476	1.409	4.5	94	0.00
3	Chlorodifluoromethane	1.508	1.417	6.0	91	0.00
4	Chloromethane	0.603	0.565	6.3	92	0.00
5 T	Vinyl Chloride	0.639	0.548	14.2	93	0.00
6 T	Bromomethane	0.273	0.241	11.7	87	0.00
7	Chloroethane	0.242	0.215	11.2	88	0.00
8 T	Dichlorotetrafluoroethane	1.257	1.226	2.5	94	0.00
9 T	Propene	0.691	0.604	12.6	85	0.00
10 T	Heptane	1.839	1.714	6.8	89	0.00
11 T	Trichlorofluoromethane	1.437	1.358	5.5	95	0.00
12 T	1,1,2-Trichlorotrifluoroeth	1.181	1.113	5.8	93	0.00
13	Ethanol	0.065	0.033#	49.2#	108	0.00
14 T	Bromoethene	0.452	0.422	6.6	94	0.00
15 T	Acetone	1.399	1.137	18.7	95	0.00
16 T	1,3-Butadiene	0.683	0.561	17.9	91	0.00
17	tert-Butyl alcohol	1.742	1.584	9.1	91	0.00
18 T	1,1-Dichloroethene	0.552	0.500	9.4	92	0.00
19 T	Isopropyl Alcohol	0.789	0.704	10.8	93	0.00
20 T	Methylene Chloride	0.521	0.418	19.8	89	0.00
21 T	Allyl Chloride	0.986	0.903	8.4	93	0.00
22 T	trans-1,2-Dichloroethene	0.638	0.580	9.1	92	0.00
23 T	Vinyl Acetate	0.605	0.518	14.4	97	0.00
24 T	1,1-Dichloroethane	1.183	1.135	4.1	94	0.00
25 T	Ethyl Acetate	3.630	3.399	6.4	92	0.00
26 T	Hexane	1.402	1.326	5.4	93	0.00
27 T	Carbon Disulfide	1.503	1.427	5.1	93	0.00
28 T	Methyl tert-Butyl Ether	0.873	0.840	3.8	94	0.00
29 T	Chloroform	2.052	1.974	3.8	95	0.00
30 T	Cyclohexane	1.217	1.135	6.7	91	0.00
31 T	cis-1,2-Dichloroethene	1.423	1.345	5.5	91	0.00
32 T	1,1,1-Trichloroethane	2.349	2.096	10.8	95	0.00
33 I	1,4-Difluorobenzene	1.000	1.000	0.0	91	0.00
34 T	2-Butanone	0.725	0.665	8.3	91	0.00
35 T	Carbon Tetrachloride	0.781	0.730	6.5	95	0.00
36 T	Benzene	0.991	0.926	6.6	91	0.00
37 T	1,2-Dichloroethane	0.568	0.549	3.3	93	0.00
38 T	Trichloroethene	0.414	0.385	7.0	94	0.00
39 T	1,2-Dichloropropane	0.361	0.343	5.0	93	0.00
40 T	1,4-Dioxane	0.192	0.162	15.6	87	0.00
41 T	Tetrahydrofuran	0.418	0.394	5.7	90	0.00
42 T	Bromodichloromethane	0.782	0.771	1.4	92	0.00
43	Methyl Methacrylate	0.420	0.392	6.7	89	0.00
44 T	2,2,4-Trimethylpentane	1.675	1.581	5.6	90	0.00
45 T	t-1,3-Dichloropropene	0.450	0.426	5.3	89	0.00
46 T	cis-1,3-Dichloropropene	0.552	0.532	3.6	88	0.00
47 T	1,1,2-Trichloroethane	0.382	0.368	3.7	92	0.00
48 T	Dibromochloromethane	0.647	0.648	-0.2	93	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032725\
 Data File : VL042179.D
 Acq On : 27 Mar 2025 12:23
 Operator : SY/MD
 Sample : VSTDICV010
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 ICVVL032725

Quant Time: Mar 28 02:05:15 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Min. RRF : 0.050 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
49 T	Bromoform	0.581	0.572	1.5	90	0.00
50 T	4-Methyl-2-Pentanone	1.149	1.005	12.5	89	0.00
51 T	2-Hexanone	0.944	0.825	12.6	89	0.00
52 T	Tetrachloroethene	0.393	0.348	11.5	93	0.00
53 T	Toluene	1.175	1.118	4.9	91	0.00
54 T	1,2-Dibromoethane	0.532	0.516	3.0	93	0.00
55 I	Chlorobenzene-d5	1.000	1.000	0.0	91	0.00
56	1,1,1,2-Tetrachloroethane	0.550	0.527	4.2	94	0.00
57 T	Chlorobenzene	0.949	0.893	5.9	93	0.00
58 T	Ethyl Benzene	1.776	1.672	5.9	91	0.00
59 T	m/p-Xylene	1.418	1.331	6.1	92	0.00
60 T	o-Xylene	1.422	1.337	6.0	92	0.00
61 T	Styrene	0.703	0.667	5.1	89	0.00
62	Isopropylbenzene	2.126	1.996	6.1	93	0.00
63 T	1,1,2,2-Tetrachloroethane	0.864	0.808	6.5	93	0.00
64	n-propylbenzene	0.547	0.517	5.5	94	0.00
65	tert-Butylbenzene	1.966	1.783	9.3	94	0.00
66 T	Benzyl Chloride	0.209	0.183	12.4	82	0.00
67	sec-Butylbenzene	2.733	2.477	9.4	94	0.00
68 S	1-Bromo-4-Fluorobenzene	0.821	0.803	2.2	90	0.00
69	p-Isopropyltoluene	2.354	2.154	8.5	94	0.00
70	n-Butylbenzene	2.407	2.194	8.8	94	0.00
71	2-Chlorotoluene	1.650	1.548	6.2	92	0.00
72 T	4-Ethyltoluene	1.770	1.659	6.3	93	0.00
73 T	1,3,5-Trimethylbenzene	1.546	1.423	8.0	93	0.00
74 T	1,2,4-Trimethylbenzene	1.781	1.540	13.5	93	0.00
75 T	1,3-Dichlorobenzene	0.977	0.901	7.8	93	0.00
76 T	1,4-Dichlorobenzene	0.972	0.901	7.3	92	0.00
77 T	1,2-Dichlorobenzene	0.951	0.871	8.4	93	0.00
78 T	Hexachloro-1,3-Butadiene	0.968	0.753	22.2	86	0.00
79 T	Naphthalene	1.948	1.634	16.1	82	0.00
80 T	Naphthalene,2-methyl-	0.955	0.683	28.5	63	0.00
81 T	1,2,4-Trichlorobenzene	0.899	0.769	14.5	82	0.00

(#) = Out of Range


SPCC's out = 0 CCC's out = 0

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL040425\
Data File : VL042214.D
Acq On : 04 Apr 2025 08:05
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Mar 28 02:00:52 2025



AutoFind: Scans 3179, 3180, 3181; Background Corrected with Scan 3165

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.3	72739	PASS
75	95	30	66	57.9	166656	PASS
95	95	100	100	100.0	287979	PASS
96	95	5	9	6.5	18594	PASS
173	174	0.00	2	0.4	773	PASS
174	95	50	120	61.2	176384	PASS
175	174	4	9	7.3	12832	PASS
176	174	93	101	93.5	164907	PASS
177	176	5	9	6.4	10500	PASS

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL040425\
 Data File : VL042215.D
 Acq On : 04 Apr 2025 08:58
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDCCC010

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/07/2025
 Supervised By : Mahesh Dadoda 04/08/2025

Quant Time: Apr 05 01:58:44 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2025

QLast Update : Fri Mar 28 02:00:52 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.790	49	187369	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.962	114	519347	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.888	117	464975	10.000	ppbv	0.01

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene 10.380 95 383840 10.052 ppbv 0.00
 Spiked Amount 10.000 Range 65 - 135 Recovery = 100.500%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.499	85	263276	9.517	ppbv	99
3) Chlorodifluoromethane	1.476	51	264623	9.363	ppbv	96
4) Chloromethane	1.534	50	104117	9.209	ppbv	96
5) Vinyl Chloride	1.580	62	98352	8.209	ppbv	97
6) Bromomethane	1.667	94	44500	8.685	ppbv	97
7) Chloroethane	1.706	64	39804	8.771	ppbv	98
8) Dichlorotetrafluoroethane	1.554	85	227648	9.663	ppbv	93
9) Propene	1.486	41	101955	7.871	ppbv	99
10) Heptane	4.988	43	290775	8.439	ppbv	99
11) Trichlorofluoromethane	1.877	101	256266	9.520	ppbv	97
12) 1,1,2-Trichlorotrifluo...	2.140	101	195280	8.826	ppbv	97
13) Ethanol	1.722	45	5295	4.324	ppbv	99
14) Bromoethene	1.783	108	72355	8.536	ppbv	98
15) Acetone	1.835	43	219621	8.381	ppbv	96
16) 1,3-Butadiene	1.609	39	106868	8.351	ppbv	98
17) tert-Butyl alcohol	2.042	59	264585	8.107	ppbv	100
18) 1,1-Dichloroethene	2.036	96	87932	8.501	ppbv	95
19) Isopropyl Alcohol	1.887	45	123909	8.381	ppbv	98
20) Methylene Chloride	2.062	84	76274	7.815	ppbv	94
21) Allyl Chloride	2.097	41	158103	8.555	ppbv	98
22) trans-1,2-Dichloroethene	2.343	96	97729	8.175	ppbv	96
23) Vinyl Acetate	2.463	43	81872	7.219	ppbv	99
24) 1,1-Dichloroethane	2.411	63	199075	8.983	ppbv	99
25) Ethyl Acetate	2.839	43	602732	8.862	ppbv	99
26) Hexane	2.829	57	231730	8.821	ppbv	99
27) Carbon Disulfide	2.152	76	244246	8.670	ppbv	96
28) Methyl tert-Butyl Ether	2.444	73	131136	8.018	ppbv	97
29) Chloroform	2.852	83	378649	9.849	ppbv	99
30) Cyclohexane	3.861	84	196271	8.604	ppbv	96
31) cis-1,2-Dichloroethene	2.722	61	243455	9.129	ppbv	96
32) 1,1,1-Trichloroethane	3.373	97	401472	9.121	ppbv	98
34) 2-Butanone	2.560	43	347241	9.221	ppbv	100
35) Carbon Tetrachloride	3.764	117	412365	10.164	ppbv	97
36) Benzene	3.661	78	467443	9.079	ppbv	97
37) 1,2-Dichloroethane	3.221	62	307037	10.416	ppbv	97
38) Trichloroethene	4.554	130	199451	9.284	ppbv	98
39) 1,2-Dichloropropane	4.318	63	170450	9.090	ppbv	91
40) 1,4-Dioxane	4.590	88	81209	8.160	ppbv #	93
41) Tetrahydrofuran	3.059	42	189995	8.761	ppbv	98
42) Bromodichloromethane	4.496	83	416628	10.252	ppbv	98
43) Methyl Methacrylate	4.884	69	184838	8.480	ppbv	99
44) 2,2,4-Trimethylpentane	4.648	57	789050	9.069	ppbv	97
45) t-1,3-Dichloropropene	6.422	75	196583	8.407	ppbv	95

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL040425\
 Data File : VL042215.D
 Acq On : 04 Apr 2025 08:58
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDCCC010

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/07/2025
 Supervised By : Mahesh Dadoda 04/08/2025

Quant Time: Apr 05 01:58:44 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Mar 28 02:00:52 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.609	75	248725	8.677	ppbv	98
47) 1,1,2-Trichloroethane	6.590	97	188954	9.533	ppbv	96
48) Dibromochloromethane	7.396	129	338657	10.081	ppbv	100
49) Bromoform	9.490	173	291660	9.671	ppbv	100
50) 4-Methyl-2-Pentanone	5.761	43	485587	8.136	ppbv	98
51) 2-Hexanone	7.448	43	393233	8.024	ppbv #	96
52) Tetrachloroethene	8.231	164	170524	8.351	ppbv	94
53) Toluene	6.939	91	548226	8.982	ppbv	99
54) 1,2-Dibromoethane	7.661	107	262312	9.493	ppbv	95
56) 1,1,1,2-Tetrachloroethane	8.930	131	265488	10.373	ppbv	97
57) Chlorobenzene	8.927	112	435637	9.878	ppbv	97
58) Ethyl Benzene	9.360	91	787508	9.535	ppbv	100
59) m/p-Xylene	9.558	91	1320455m	20.022	ppbv	
60) o-Xylene	9.969	91	648429	9.808	ppbv	96
61) Styrene	9.875	104	307359	9.397	ppbv	99
62) Isopropylbenzene	10.545	105	991027	10.024	ppbv	100
63) 1,1,2,2-Tetrachloroethane	9.969	83	404850	10.079	ppbv	100
64) n-propylbenzene	10.995	120	263771	10.364	ppbv	96
65) tert-Butylbenzene	11.535	119	904984	9.898	ppbv	98
66) Benzyl Chloride	11.620	91	71677	7.388	ppbv	97
67) sec-Butylbenzene	11.772	105	1272047	10.009	ppbv	99
69) p-Isopropyltoluene	11.930	119	1096744	10.022	ppbv	99
70) n-Butylbenzene	12.283	91	1129301	10.090	ppbv	99
71) 2-Chlorotoluene	10.908	91	769367	10.027	ppbv	100
72) 4-Ethyltoluene	11.131	105	835598	10.151	ppbv	100
73) 1,3,5-Trimethylbenzene	11.209	105	724375	10.076	ppbv	98
74) 1,2,4-Trimethylbenzene	11.542	105	804419	9.712	ppbv	96
75) 1,3-Dichlorobenzene	11.613	146	469384	10.333	ppbv	99
76) 1,4-Dichlorobenzene	11.675	146	467820	10.348	ppbv	100
77) 1,2-Dichlorobenzene	11.950	146	460424	10.410	ppbv	99
78) Hexachloro-1,3-Butadiene	13.885	225	386022	8.574	ppbv	100
79) Naphthalene	13.516	128	931920	10.287	ppbv	99
80) Naphthalene,2-methyl-	14.461	142	470633	10.593	ppbv	99
81) 1,2,4-Trichlorobenzene	13.445	180	416845	9.975	ppbv	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL040425\
 Data File : VL042215.D
 Acq On : 04 Apr 2025 08:58
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 LabSampleId :
 VSTDCCC010

Quant Time: Apr 05 01:58:44 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Min. RRF : 0.050 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	Bromochloromethane	1.000	1.000	0.0	100	0.00
2 T	Dichlorodifluoromethane	1.476	1.405	4.8	100	0.00
3	Chlorodifluoromethane	1.508	1.412	6.4	97	0.00
4	Chloromethane	0.603	0.556	7.8	97	0.00
5 T	Vinyl Chloride	0.639	0.525	17.8	96	0.00
6 T	Bromomethane	0.273	0.237	13.2	93	0.00
7	Chloroethane	0.242	0.212	12.4	94	0.00
8 T	Dichlorotetrafluoroethane	1.257	1.215	3.3	100	0.00
9 T	Propene	0.691	0.544	21.3	83	0.00
10 T	Heptane	1.839	1.552	15.6	87	0.02
11 T	Trichlorofluoromethane	1.437	1.368	4.8	102	0.00
12 T	1,1,2-Trichlorotrifluoroeth	1.181	1.042	11.8	93	0.00
13	Ethanol	0.065	0.028#	56.9#	99	0.00
14 T	Bromoethene	0.452	0.386	14.6	93	0.00
15 T	Acetone	1.399	1.172	16.2	106	0.00
16 T	1,3-Butadiene	0.683	0.570	16.5	100	0.00
17	tert-Butyl alcohol	1.742	1.412	18.9	87	0.00
18 T	1,1-Dichloroethene	0.552	0.469	15.0	93	0.00
19 T	Isopropyl Alcohol	0.789	0.661	16.2	94	0.00
20 T	Methylene Chloride	0.521	0.407	21.9	93	0.00
21 T	Allyl Chloride	0.986	0.844	14.4	94	0.00
22 T	trans-1,2-Dichloroethene	0.638	0.522	18.2	89	0.00
23 T	Vinyl Acetate	0.605	0.437	27.8	88	0.00
24 T	1,1-Dichloroethane	1.183	1.062	10.2	95	0.00
25 T	Ethyl Acetate	3.630	3.217	11.4	93	0.00
26 T	Hexane	1.402	1.237	11.8	93	0.00
27 T	Carbon Disulfide	1.503	1.304	13.2	91	0.00
28 T	Methyl tert-Butyl Ether	0.873	0.700	19.8	84	0.00
29 T	Chloroform	2.052	2.021	1.5	105	0.00
30 T	Cyclohexane	1.217	1.048	13.9	90	0.00
31 T	cis-1,2-Dichloroethene	1.423	1.299	8.7	95	0.00
32 T	1,1,1-Trichloroethane	2.349	2.143	8.8	104	0.00
33 I	1,4-Difluorobenzene	1.000	1.000	0.0	95	0.00
34 T	2-Butanone	0.725	0.669	7.7	95	0.00
35 T	Carbon Tetrachloride	0.781	0.794	-1.7	108	0.00
36 T	Benzene	0.991	0.900	9.2	92	0.00
37 T	1,2-Dichloroethane	0.568	0.591	-4.0	105	0.00
38 T	Trichloroethene	0.414	0.384	7.2	98	0.00
39 T	1,2-Dichloropropane	0.361	0.328	9.1	93	0.00
40 T	1,4-Dioxane	0.192	0.156	18.8	88	0.01
41 T	Tetrahydrofuran	0.418	0.366	12.4	88	0.00
42 T	Bromodichloromethane	0.782	0.802	-2.6	99	0.01
43	Methyl Methacrylate	0.420	0.356	15.2	84	0.01
44 T	2,2,4-Trimethylpentane	1.675	1.519	9.3	90	0.01
45 T	t-1,3-Dichloropropene	0.450	0.379	15.8	82	0.02
46 T	cis-1,3-Dichloropropene	0.552	0.479	13.2	83	0.02
47 T	1,1,2-Trichloroethane	0.382	0.364	4.7	95	0.02
48 T	Dibromochloromethane	0.647	0.652	-0.8	98	0.02

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL040425\
 Data File : VL042215.D
 Acq On : 04 Apr 2025 08:58
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 LabSampleId :
 VSTDCCC010

Quant Time: Apr 05 01:58:44 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Min. RRF : 0.050 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
49 T	Bromoform	0.581	0.562	3.3	92	0.01
50 T	4-Methyl-2-Pentanone	1.149	0.935	18.6	87	0.02
51 T	2-Hexanone	0.944	0.757	19.8	85	0.02
52 T	Tetrachloroethene	0.393	0.328	16.5	91	0.01
53 T	Toluene	1.175	1.056	10.1	89	0.01
54 T	1,2-Dibromoethane	0.532	0.505	5.1	95	0.01
55 I	Chlorobenzene-d5	1.000	1.000	0.0	89	0.01
56	1,1,1,2-Tetrachloroethane	0.550	0.571	-3.8	100	0.01
57 T	Chlorobenzene	0.949	0.937	1.3	96	0.00
58 T	Ethyl Benzene	1.776	1.694	4.6	91	0.00
59 T	m/p-Xylene	1.418	1.420	-0.1	96	0.00
60 T	o-Xylene	1.422	1.395	1.9	94	0.00
61 T	Styrene	0.703	0.661	6.0	87	0.00
62	Isopropylbenzene	2.126	2.131	-0.2	97	0.00
63 T	1,1,2,2-Tetrachloroethane	0.864	0.871	-0.8	98	0.00
64	n-propylbenzene	0.547	0.567	-3.7	102	0.00
65	tert-Butylbenzene	1.966	1.946	1.0	100	0.00
66 T	Benzyl Chloride	0.209	0.154	26.3	68	0.00
67	sec-Butylbenzene	2.733	2.736	-0.1	102	0.00
68 S	1-Bromo-4-Fluorobenzene	0.821	0.826	-0.6	91	0.00
69	p-Isopropyltoluene	2.354	2.359	-0.2	102	0.00
70	n-Butylbenzene	2.407	2.429	-0.9	102	0.00
71	2-Chlorotoluene	1.650	1.655	-0.3	96	0.00
72 T	4-Ethyltoluene	1.770	1.797	-1.5	99	0.00
73 T	1,3,5-Trimethylbenzene	1.546	1.558	-0.8	101	0.00
74 T	1,2,4-Trimethylbenzene	1.781	1.730	2.9	103	0.00
75 T	1,3-Dichlorobenzene	0.977	1.009	-3.3	102	0.00
76 T	1,4-Dichlorobenzene	0.972	1.006	-3.5	101	0.00
77 T	1,2-Dichlorobenzene	0.951	0.990	-4.1	104	0.00
78 T	Hexachloro-1,3-Butadiene	0.968	0.830	14.3	93	0.00
79 T	Naphthalene	1.948	2.004	-2.9	99	0.00
80 T	Naphthalene,2-methyl-	0.955	1.012	-6.0	91	0.00
81 T	1,2,4-Trichlorobenzene	0.899	0.896	0.3	93	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL040425\
 Data File : VL042216.D
 Acq On : 04 Apr 2025 09:41
 Operator : SY/MD
 Sample : VL0404ABL01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0404ABL01

Quant Time: Apr 05 01:59:42 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.787	49	191004	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.962	114	523611	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.885	117	464191	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.380	95	364475	9.561	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	95.600%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL040425\
Data File : VL042216.D
Acq On : 04 Apr 2025 09:41
Operator : SY/MD
Sample : VL0404ABL01
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VL0404ABL01

Quant Time: Apr 05 01:59:42 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Fri Mar 28 02:00:52 2025
Response via : Initial Calibration



Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL040425\
 Data File : VL042219.D
 Acq On : 04 Apr 2025 11:16
 Operator : SY/MD
 Sample : QC040325 CAN 10300
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC040325 CAN 10300

Quant Time: Apr 05 02:00:53 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.784	49	181629	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.956	114	492050	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.882	117	439540	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.377	95	344682	9.549	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	95.500%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL040425\
Data File : VL042219.D
Acq On : 04 Apr 2025 11:16
Operator : SY/MD
Sample : QC040325 CAN 10300
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC040325 CAN 10300

Quant Time: Apr 05 02:00:53 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Fri Mar 28 02:00:52 2025
Response via : Initial Calibration

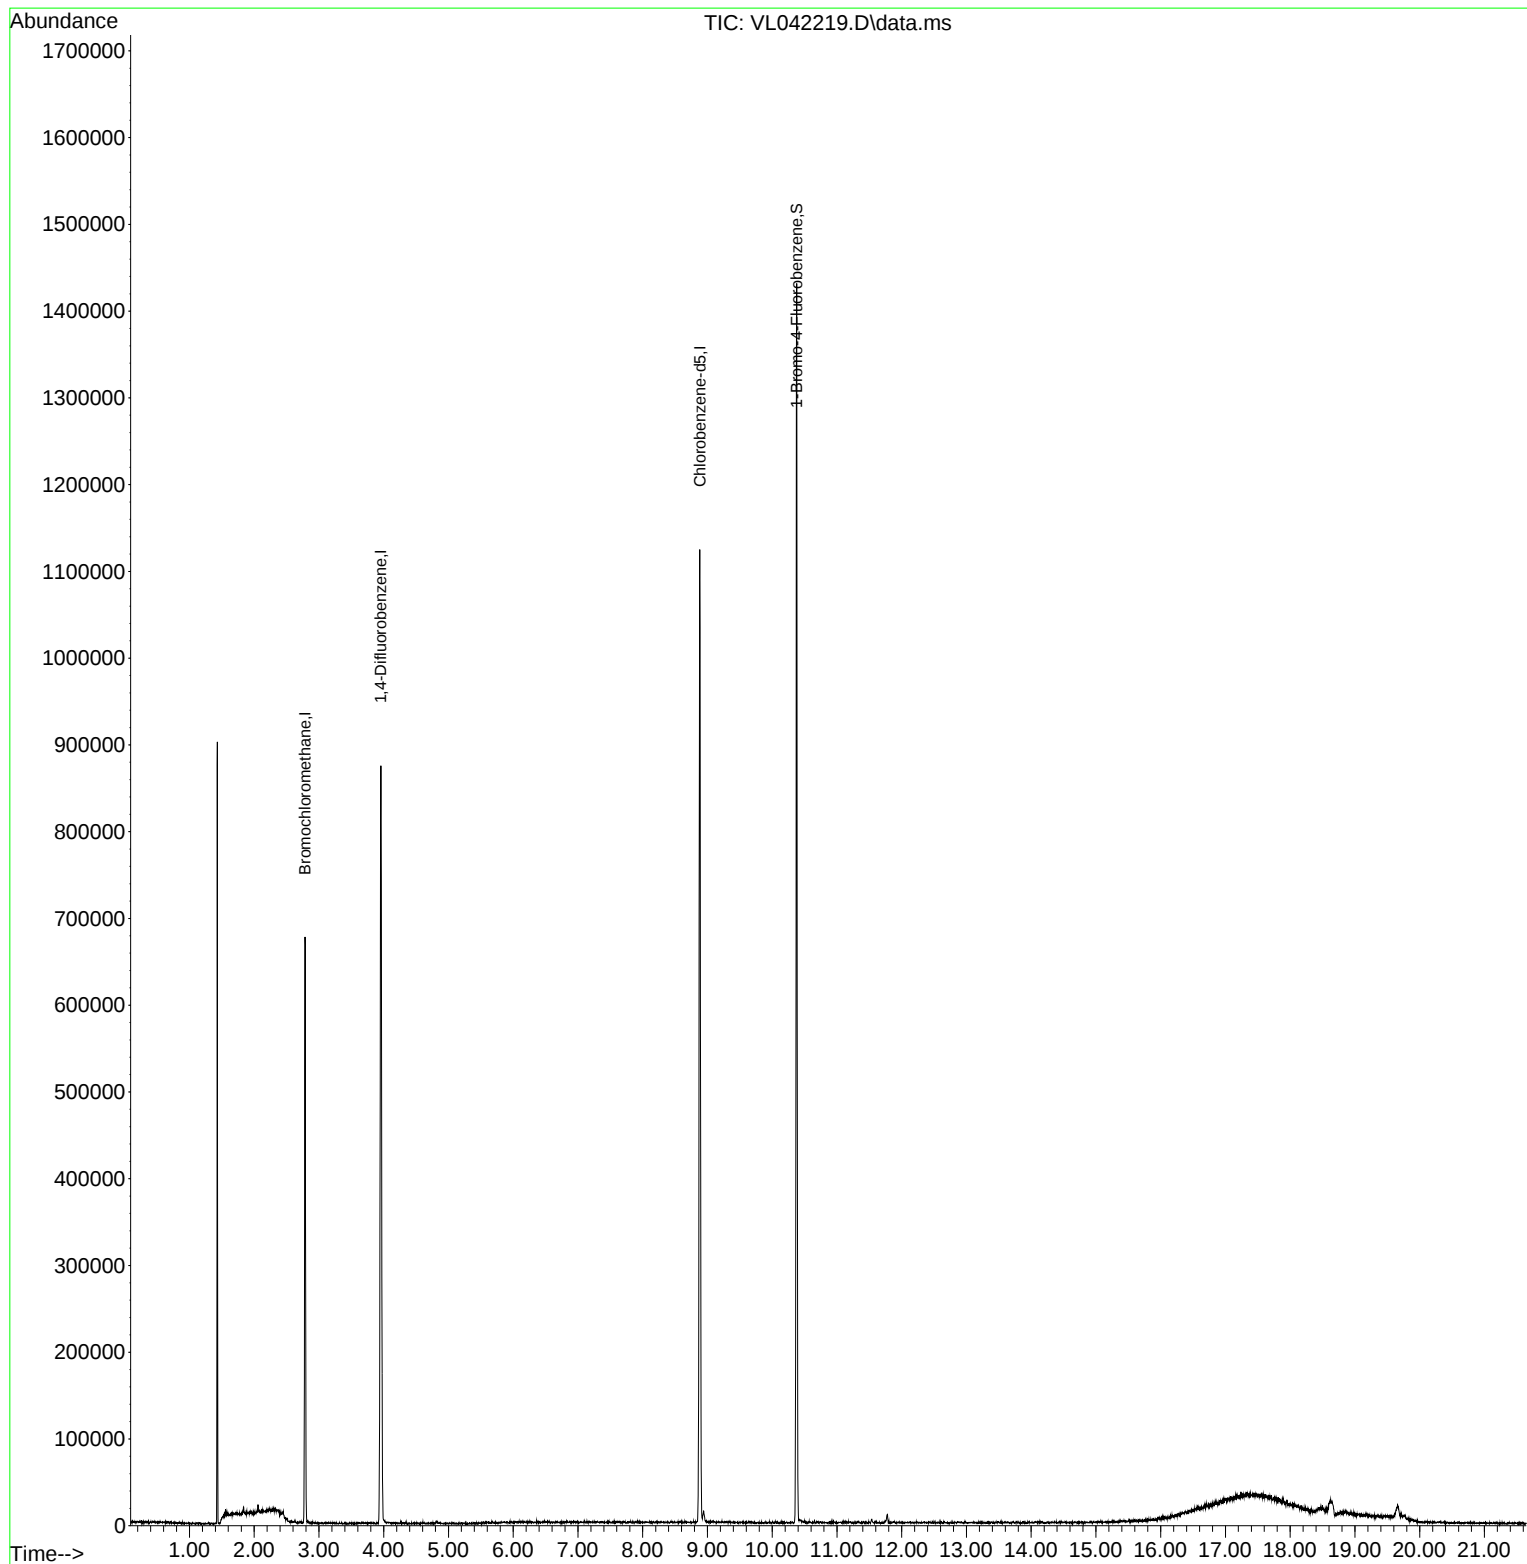

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL040425\
 Data File : VL042220.D
 Acq On : 04 Apr 2025 11:55
 Operator : SY/MD
 Sample : VL0404ABS01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0404ABS01

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/07/2025
 Supervised By :Mahesh Dadoda 04/08/2025

Quant Time: Apr 05 02:01:14 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug 2025

QLast Update : Fri Mar 28 02:00:52 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.790	49	185704	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.962	114	509064	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.888	117	456962	10.000	ppbv	0.01

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene 10.380 95 384044 10.234 ppbv 0.00
 Spiked Amount 10.000 Range 65 - 135 Recovery = 102.300%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.499	85	269944	9.845	ppbv	99
3) Chlorodifluoromethane	1.476	51	261247	9.327	ppbv	97
4) Chloromethane	1.535	50	100977	9.011	ppbv	97
5) Vinyl Chloride	1.580	62	97885	8.243	ppbv	97
6) Bromomethane	1.667	94	43311	8.529	ppbv	96
7) Chloroethane	1.706	64	38925	8.654	ppbv	98
8) Dichlorotetrafluoroethane	1.554	85	226404	9.696	ppbv	94
9) Propene	1.486	41	98481	7.671	ppbv	98
10) Heptane	4.982	43	290990	8.521	ppbv	99
11) Trichlorofluoromethane	1.878	101	258888	9.704	ppbv	100
12) 1,1,2-Trichlorotrifluo...	2.140	101	195978	8.937	ppbv	95
13) Ethanol	1.722	45	5793	4.773	ppbv	91
14) Bromoethene	1.784	108	72245	8.600	ppbv	98
15) Acetone	1.836	43	218906	8.429	ppbv	95
16) 1,3-Butadiene	1.609	39	109321	8.619	ppbv	96
17) tert-Butyl alcohol	2.043	59	268750	8.308	ppbv	99
18) 1,1-Dichloroethene	2.036	96	90266	8.805	ppbv	96
19) Isopropyl Alcohol	1.887	45	124365	8.487	ppbv	99
20) Methylene Chloride	2.062	84	75950	7.852	ppbv	96
21) Allyl Chloride	2.098	41	157041	8.574	ppbv	99
22) trans-1,2-Dichloroethene	2.344	96	103089	8.700	ppbv	98
23) Vinyl Acetate	2.464	43	85276	7.586	ppbv	97
24) 1,1-Dichloroethane	2.412	63	207336	9.440	ppbv	99
25) Ethyl Acetate	2.839	43	605091	8.977	ppbv	99
26) Hexane	2.829	57	230193	8.841	ppbv	98
27) Carbon Disulfide	2.153	76	237628	8.511	ppbv #	94
28) Methyl tert-Butyl Ether	2.444	73	137912	8.508	ppbv	95
29) Chloroform	2.852	83	384364	10.087	ppbv	99
30) Cyclohexane	3.862	84	192377	8.509	ppbv	96
31) cis-1,2-Dichloroethene	2.722	61	237721	8.993	ppbv	97
32) 1,1,1-Trichloroethane	3.370	97	396331	9.085	ppbv	99
34) 2-Butanone	2.561	43	339503	9.197	ppbv	98
35) Carbon Tetrachloride	3.768	117	410967	10.334	ppbv	96
36) Benzene	3.661	78	464642	9.207	ppbv	99
37) 1,2-Dichloroethane	3.221	62	306471	10.607	ppbv	98
38) Trichloroethene	4.554	130	190707	9.057	ppbv	96
39) 1,2-Dichloropropane	4.321	63	166615	9.065	ppbv	91
40) 1,4-Dioxane	4.587	88	85279	8.742	ppbv #	95
41) Tetrahydrofuran	3.059	42	186669	8.782	ppbv	99
42) Bromodichloromethane	4.496	83	417630	10.485	ppbv	96
43) Methyl Methacrylate	4.888	69	183270	8.578	ppbv	100
44) 2,2,4-Trimethylpentane	4.645	57	792460	9.292	ppbv	97
45) t-1,3-Dichloropropene	6.422	75	187871	8.196	ppbv	93

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL040425\
 Data File : VL042220.D
 Acq On : 04 Apr 2025 11:55
 Operator : SY/MD
 Sample : VL0404ABS01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0404ABS01

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/07/2025
 Supervised By :Mahesh Dadoda 04/08/2025

Quant Time: Apr 05 02:01:14 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Mar 28 02:00:52 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.610	75	235408	8.378	ppbv	95
47) 1,1,2-Trichloroethane	6.587	97	192846	9.926	ppbv	96
48) Dibromochloromethane	7.396	129	334902	10.171	ppbv	99
49) Bromoform	9.490	173	293331	9.923	ppbv	99
50) 4-Methyl-2-Pentanone	5.758	43	493794	8.441	ppbv	96
51) 2-Hexanone	7.445	43	393716	8.196	ppbv #	95
52) Tetrachloroethene	8.231	164	170397	8.514	ppbv	94
53) Toluene	6.940	91	540865	9.041	ppbv	99
54) 1,2-Dibromoethane	7.658	107	265033	9.786	ppbv	94
56) 1,1,1,2-Tetrachloroethane	8.930	131	269744	10.724	ppbv	99
57) Chlorobenzene	8.927	112	437108	10.085	ppbv	97
58) Ethyl Benzene	9.361	91	791626	9.753	ppbv	99
59) m/p-Xylene	9.539	91	1322210m	20.400	ppbv	
60) o-Xylene	9.969	91	665062	10.236	ppbv	98
61) Styrene	9.875	104	304392	9.470	ppbv	99
62) Isopropylbenzene	10.545	105	1008886	10.383	ppbv	100
63) 1,1,2,2-Tetrachloroethane	9.969	83	422180	10.694	ppbv	99
64) n-propylbenzene	10.995	120	263691	10.543	ppbv	99
65) tert-Butylbenzene	11.536	119	921281	10.252	ppbv	98
66) Benzyl Chloride	11.620	91	65520	6.872	ppbv	99
67) sec-Butylbenzene	11.772	105	1296409	10.379	ppbv	99
69) p-Isopropyltoluene	11.931	119	1119576	10.410	ppbv	100
70) n-Butylbenzene	12.287	91	1149751	10.453	ppbv	99
71) 2-Chlorotoluene	10.908	91	777635	10.312	ppbv	100
72) 4-Ethyltoluene	11.128	105	850373	10.511	ppbv	99
73) 1,3,5-Trimethylbenzene	11.209	105	737397	10.437	ppbv	98
74) 1,2,4-Trimethylbenzene	11.542	105	816996	10.037	ppbv	95
75) 1,3-Dichlorobenzene	11.613	146	475804	10.658	ppbv	99
76) 1,4-Dichlorobenzene	11.675	146	473366	10.654	ppbv	100
77) 1,2-Dichlorobenzene	11.950	146	470868	10.833	ppbv	99
78) Hexachloro-1,3-Butadiene	13.886	225	366515	8.284	ppbv	99
79) Naphthalene	13.517	128	842258	9.460	ppbv	99
80) Naphthalene,2-methyl-	14.462	142	310504	7.112	ppbv	98
81) 1,2,4-Trichlorobenzene	13.442	180	377618	9.195	ppbv	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Manual Integrations

Reviewed By :Semsettin Yesilyurt 04/07/2025
Supervised By :Mahesh Dadoda 04/08/2025



[illegible]

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041025\
Data File : VL042299.D
Acq On : 10 Apr 2025 08:46
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Mar 28 02:00:52 2025



AutoFind: Scans 3176, 3177, 3178; Background Corrected with Scan 3162

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.7	56629	PASS
75	95	30	66	57.1	131205	PASS
95	95	100	100	100.0	229611	PASS
96	95	5	9	6.9	15747	PASS
173	174	0.00	2	1.3	1863	PASS
174	95	50	120	62.9	144533	PASS
175	174	4	9	7.7	11082	PASS
176	174	93	101	95.7	138363	PASS
177	176	5	9	5.9	8219	PASS

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041025\
 Data File : VL042300.D
 Acq On : 10 Apr 2025 09:27
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDCCC010

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/11/2025
 Supervised By : Mahesh Dadoda 04/11/2025

Quant Time: Apr 11 01:54:45 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2025

QLast Update : Fri Mar 28 02:00:52 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.781	49	178247	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.952	114	448439	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.875	117	388079	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	10.370	95	315861	9.911	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.100%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.496	85	256858	9.760	ppbv	99
3) Chlorodifluoromethane	1.473	51	283366	10.540	ppbv	98
4) Chloromethane	1.531	50	106741	9.924	ppbv	98
5) Vinyl Chloride	1.576	62	95961	8.419	ppbv	96
6) Bromomethane	1.664	94	46181	9.475	ppbv	98
7) Chloroethane	1.699	64	40193	9.310	ppbv	95
8) Dichlorotetrafluoroethane	1.551	85	218294	9.740	ppbv	94
9) Propene	1.483	41	109223	8.863	ppbv	100
10) Heptane	4.972	43	324095	9.887	ppbv	98
11) Trichlorofluoromethane	1.874	101	247687	9.672	ppbv	99
12) 1,1,2-Trichlorotrifluo...	2.136	101	202744	9.632	ppbv	98
13) Ethanol	1.716	45	4951	4.250	ppbv	90
14) Bromoethene	1.777	108	71256	8.837	ppbv	97
15) Acetone	1.832	43	223555	8.968	ppbv	97
16) 1,3-Butadiene	1.606	39	109334	8.981	ppbv	96
17) tert-Butyl alcohol	2.036	59	251167	8.089	ppbv	99
18) 1,1-Dichloroethene	2.030	96	84843	8.622	ppbv	95
19) Isopropyl Alcohol	1.884	45	121282	8.623	ppbv	93
20) Methylene Chloride	2.056	84	78454	8.450	ppbv	96
21) Allyl Chloride	2.091	41	160287	9.117	ppbv	97
22) trans-1,2-Dichloroethene	2.337	96	100830	8.866	ppbv	97
23) Vinyl Acetate	2.457	43	87054	8.068	ppbv	98
24) 1,1-Dichloroethane	2.405	63	207493	9.842	ppbv	99
25) Ethyl Acetate	2.829	43	648989	10.031	ppbv	99
26) Hexane	2.819	57	242802	9.715	ppbv	95
27) Carbon Disulfide	2.146	76	246850	9.211	ppbv	97
28) Methyl tert-Butyl Ether	2.434	73	123776	7.955	ppbv	95
29) Chloroform	2.842	83	384275	10.507	ppbv	98
30) Cyclohexane	3.849	84	195121	8.992	ppbv	97
31) cis-1,2-Dichloroethene	2.716	61	230708	9.093	ppbv	98
32) 1,1,1-Trichloroethane	3.360	97	374626	8.947	ppbv	97
34) 2-Butanone	2.554	43	358677	11.030	ppbv	98
35) Carbon Tetrachloride	3.755	117	392632	11.208	ppbv	98
36) Benzene	3.648	78	478185	10.756	ppbv	98
37) 1,2-Dichloroethane	3.211	62	286987	11.276	ppbv	100
38) Trichloroethene	4.538	130	195692	10.550	ppbv	97
39) 1,2-Dichloropropane	4.305	63	177013	10.933	ppbv	93
40) 1,4-Dioxane	4.574	88	82234	9.570	ppbv #	96
41) Tetrahydrofuran	3.049	42	203688	10.878	ppbv	93
42) Bromodichloromethane	4.480	83	403381	11.496	ppbv	98
43) Methyl Methacrylate	4.871	69	174371	9.265	ppbv	97
44) 2,2,4-Trimethylpentane	4.629	57	854163	11.369	ppbv	97
45) t-1,3-Dichloropropene	6.406	75	165013	8.172	ppbv	94

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041025\
 Data File : VL042300.D
 Acq On : 10 Apr 2025 09:27
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDCCC010

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/11/2025
 Supervised By : Mahesh Dadoda 04/11/2025

Quant Time: Apr 11 01:54:45 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Mar 28 02:00:52 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.593	75	221829	8.962	ppbv	96
47) 1,1,2-Trichloroethane	6.571	97	195254	11.408	ppbv	98
48) Dibromochloromethane	7.377	129	318189	10.970	ppbv	100
49) Bromoform	9.477	173	285511	10.964	ppbv	99
50) 4-Methyl-2-Pentanone	5.742	43	507692	9.852	ppbv	94
51) 2-Hexanone	7.428	43	399883	9.449	ppbv #	94
52) Tetrachloroethene	8.215	164	162967	9.243	ppbv	97
53) Toluene	6.923	91	519861	9.865	ppbv	99
54) 1,2-Dibromoethane	7.642	107	258669	10.842	ppbv	99
56) 1,1,1,2-Tetrachloroethane	8.917	131	267799	12.536	ppbv	99
57) Chlorobenzene	8.914	112	449522	12.212	ppbv	94
58) Ethyl Benzene	9.348	91	745642	10.817	ppbv	100
59) m/p-Xylene	9.545	91	1300739m	23.631	ppbv	
60) o-Xylene	9.956	91	645311	11.695	ppbv	96
61) Styrene	9.866	104	277596	10.169	ppbv	99
62) Isopropylbenzene	10.532	105	963868	11.681	ppbv	99
63) 1,1,2,2-Tetrachloroethane	9.956	83	431966	12.884	ppbv	100
64) n-propylbenzene	10.985	120	255844	12.045	ppbv	99
65) tert-Butylbenzene	11.526	119	885906	11.609	ppbv	99
66) Benzyl Chloride	11.610	91	66712	8.239	ppbv	99
67) sec-Butylbenzene	11.762	105	1259760	11.876	ppbv	100
69) p-Isopropyltoluene	11.921	119	1081410	11.839	ppbv	99
70) n-Butylbenzene	12.277	91	1114385	11.930	ppbv	100
71) 2-Chlorotoluene	10.895	91	735700	11.488	ppbv	98
72) 4-Ethyltoluene	11.121	105	807663	11.756	ppbv	99
73) 1,3,5-Trimethylbenzene	11.199	105	697155	11.618	ppbv	100
74) 1,2,4-Trimethylbenzene	11.532	105	794178	11.489	ppbv	92
75) 1,3-Dichlorobenzene	11.604	146	483914	12.764	ppbv	98
76) 1,4-Dichlorobenzene	11.668	146	477802	12.663	ppbv	99
77) 1,2-Dichlorobenzene	11.943	146	479327	12.985	ppbv	98
78) Hexachloro-1,3-Butadiene	13.879	225	378178	10.064	ppbv	100
79) Naphthalene	13.510	128	909659	12.031	ppbv	100
80) Naphthalene,2-methyl-	14.455	142	421431	11.365	ppbv	99
81) 1,2,4-Trichlorobenzene	13.439	180	402576	11.543	ppbv	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041025\
 Data File : VL042300.D
 Acq On : 10 Apr 2025 09:27
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 LabSampleId :
 VSTDCCC010

Quant Time: Apr 11 01:54:45 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Min. RRF : 0.050 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	Bromochloromethane	1.000	1.000	0.0	95	0.00
2 T	Dichlorodifluoromethane	1.476	1.441	2.4	98	0.00
3	Chlorodifluoromethane	1.508	1.590	-5.4	104	0.00
4	Chloromethane	0.603	0.599	0.7	100	0.00
5 T	Vinyl Chloride	0.639	0.538	15.8	93	0.00
6 T	Bromomethane	0.273	0.259	5.1	96	0.00
7	Chloroethane	0.242	0.225	7.0	95	0.00
8 T	Dichlorotetrafluoroethane	1.257	1.225	2.5	96	0.00
9 T	Propene	0.691	0.613	11.3	89	0.00
10 T	Heptane	1.839	1.818	1.1	97	0.00
11 T	Trichlorofluoromethane	1.437	1.390	3.3	99	0.00
12 T	1,1,2-Trichlorotrifluoroeth	1.181	1.137	3.7	97	0.00
13	Ethanol	0.065	0.028#	56.9#	93	0.00
14 T	Bromoethene	0.452	0.400	11.5	91	0.00
15 T	Acetone	1.399	1.254	10.4	107	0.00
16 T	1,3-Butadiene	0.683	0.613	10.2	102	0.00
17	tert-Butyl alcohol	1.742	1.409	19.1	83	0.00
18 T	1,1-Dichloroethene	0.552	0.476	13.8	90	0.00
19 T	Isopropyl Alcohol	0.789	0.680	13.8	92	0.00
20 T	Methylene Chloride	0.521	0.440	15.5	96	0.00
21 T	Allyl Chloride	0.986	0.899	8.8	95	0.00
22 T	trans-1,2-Dichloroethene	0.638	0.566	11.3	91	0.00
23 T	Vinyl Acetate	0.605	0.488	19.3	94	0.00
24 T	1,1-Dichloroethane	1.183	1.164	1.6	99	0.00
25 T	Ethyl Acetate	3.630	3.641	-0.3	100	0.00
26 T	Hexane	1.402	1.362	2.9	97	0.00
27 T	Carbon Disulfide	1.503	1.385	7.9	92	0.00
28 T	Methyl tert-Butyl Ether	0.873	0.694	20.5	80	0.00
29 T	Chloroform	2.052	2.156	-5.1	106	0.00
30 T	Cyclohexane	1.217	1.095	10.0	90	0.00
31 T	cis-1,2-Dichloroethene	1.423	1.294	9.1	90	0.00
32 T	1,1,1-Trichloroethane	2.349	2.102	10.5	97	0.00
33 I	1,4-Difluorobenzene	1.000	1.000	0.0	82	0.00
34 T	2-Butanone	0.725	0.800	-10.3	99	0.00
35 T	Carbon Tetrachloride	0.781	0.876	-12.2	103	0.00
36 T	Benzene	0.991	1.066	-7.6	94	0.00
37 T	1,2-Dichloroethane	0.568	0.640	-12.7	98	0.00
38 T	Trichloroethene	0.414	0.436	-5.3	96	0.00
39 T	1,2-Dichloropropane	0.361	0.395	-9.4	96	0.00
40 T	1,4-Dioxane	0.192	0.183	4.7	89	0.00
41 T	Tetrahydrofuran	0.418	0.454	-8.6	94	0.00
42 T	Bromodichloromethane	0.782	0.900	-15.1	96	0.00
43	Methyl Methacrylate	0.420	0.389	7.4	79	0.00
44 T	2,2,4-Trimethylpentane	1.675	1.905	-13.7	97	0.00
45 T	t-1,3-Dichloropropene	0.450	0.368	18.2	69	0.00
46 T	cis-1,3-Dichloropropene	0.552	0.495	10.3	74	0.00
47 T	1,1,2-Trichloroethane	0.382	0.435	-13.9	99	0.00
48 T	Dibromochloromethane	0.647	0.710	-9.7	92	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041025\
 Data File : VL042300.D
 Acq On : 10 Apr 2025 09:27
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 LabSampleId :
 VSTDCCC010

Quant Time: Apr 11 01:54:45 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Min. RRF : 0.050 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
49 T	Bromoform	0.581	0.637	-9.6	90	0.00
50 T	4-Methyl-2-Pentanone	1.149	1.132	1.5	91	0.00
51 T	2-Hexanone	0.944	0.892	5.5	87	0.00
52 T	Tetrachloroethene	0.393	0.363	7.6	87	0.00
53 T	Toluene	1.175	1.159	1.4	85	0.00
54 T	1,2-Dibromoethane	0.532	0.577	-8.5	93	0.00
55 I	Chlorobenzene-d5	1.000	1.000	0.0	75	0.00
56	1,1,1,2-Tetrachloroethane	0.550	0.690	-25.5	101	0.00
57 T	Chlorobenzene	0.949	1.158	-22.0	99	0.00
58 T	Ethyl Benzene	1.776	1.921	-8.2	86	0.00
59 T	m/p-Xylene	1.418	1.676	-18.2	95	0.00
60 T	o-Xylene	1.422	1.663	-16.9	94	0.00
61 T	Styrene	0.703	0.715	-1.7	78	0.00
62	Isopropylbenzene	2.126	2.484	-16.8	95	0.00
63 T	1,1,2,2-Tetrachloroethane	0.864	1.113	-28.8	104	0.00
64	n-propylbenzene	0.547	0.659	-20.5	99	0.00
65	tert-Butylbenzene	1.966	2.283	-16.1	98	0.00
66 T	Benzyl Chloride	0.209	0.172	17.7	63	0.00
67	sec-Butylbenzene	2.733	3.246	-18.8	101	0.00
68 S	1-Bromo-4-Fluorobenzene	0.821	0.814	0.9	75	0.00
69	p-Isopropyltoluene	2.354	2.787	-18.4	100	0.00
70	n-Butylbenzene	2.407	2.872	-19.3	100	0.00
71	2-Chlorotoluene	1.650	1.896	-14.9	92	0.00
72 T	4-Ethyltoluene	1.770	2.081	-17.6	95	0.00
73 T	1,3,5-Trimethylbenzene	1.546	1.796	-16.2	97	0.00
74 T	1,2,4-Trimethylbenzene	1.781	2.046	-14.9	101	0.00
75 T	1,3-Dichlorobenzene	0.977	1.247	-27.6	106	0.00
76 T	1,4-Dichlorobenzene	0.972	1.231	-26.6	104	0.00
77 T	1,2-Dichlorobenzene	0.951	1.235	-29.9	109	0.00
78 T	Hexachloro-1,3-Butadiene	0.968	0.974	-0.6	91	0.00
79 T	Naphthalene	1.948	2.344	-20.3	97	0.00
80 T	Naphthalene,2-methyl-	0.955	1.086	-13.7	82	0.00
81 T	1,2,4-Trichlorobenzene	0.899	1.037	-15.4	90	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041025\
 Data File : VL042302.D
 Acq On : 10 Apr 2025 11:05
 Operator : SY/MD
 Sample : VL0410ABS01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0410ABS01

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/11/2025
 Supervised By : Mahesh Dadoda 04/11/2025

Quant Time: Apr 11 01:55:57 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2025

QLast Update : Fri Mar 28 02:00:52 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.780	49	181992	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.949	114	454728	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.872	117	404669	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene 10.370 95 327827 9.865 ppbv 0.00
 Spiked Amount 10.000 Range 65 - 135 Recovery = 98.600%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.495	85	251268	9.351	ppbv	100
3) Chlorodifluoromethane	1.473	51	281024	10.237	ppbv	100
4) Chloromethane	1.531	50	108261	9.858	ppbv	96
5) Vinyl Chloride	1.576	62	98639	8.476	ppbv	99
6) Bromomethane	1.664	94	45101	9.063	ppbv	98
7) Chloroethane	1.699	64	39048	8.858	ppbv	100
8) Dichlorotetrafluoroethane	1.550	85	217598	9.509	ppbv	96
9) Propene	1.479	41	109142	8.674	ppbv	98
10) Heptane	4.965	43	316659	9.462	ppbv	100
11) Trichlorofluoromethane	1.874	101	245155	9.376	ppbv	96
12) 1,1,2-Trichlorotrifluo...	2.133	101	188616	8.776	ppbv	98
13) Ethanol	1.719	45	6073	5.106	ppbv	83
14) Bromoethene	1.777	108	70885	8.610	ppbv	99
15) Acetone	1.832	43	224780	8.831	ppbv	97
16) 1,3-Butadiene	1.605	39	108045	8.692	ppbv	99
17) tert-Butyl alcohol	2.036	59	241572	7.620	ppbv	99
18) 1,1-Dichloroethene	2.029	96	84303	8.391	ppbv	99
19) Isopropyl Alcohol	1.881	45	121689	8.474	ppbv	93
20) Methylene Chloride	2.055	84	75086	7.921	ppbv	90
21) Allyl Chloride	2.091	41	159249	8.872	ppbv	97
22) trans-1,2-Dichloroethene	2.334	96	98486	8.482	ppbv	99
23) Vinyl Acetate	2.457	43	84988	7.715	ppbv	98
24) 1,1-Dichloroethane	2.402	63	202298	9.398	ppbv	99
25) Ethyl Acetate	2.829	43	654276	9.904	ppbv	99
26) Hexane	2.819	57	244625	9.587	ppbv	96
27) Carbon Disulfide	2.146	76	237591	8.683	ppbv #	95
28) Methyl tert-Butyl Ether	2.434	73	122255	7.696	ppbv	96
29) Chloroform	2.842	83	385486	10.323	ppbv	100
30) Cyclohexane	3.845	84	196837	8.884	ppbv	97
31) cis-1,2-Dichloroethene	2.716	61	233042	8.996	ppbv	96
32) 1,1,1-Trichloroethane	3.360	97	375253	8.777	ppbv	98
34) 2-Butanone	2.551	43	367560	11.147	ppbv	97
35) Carbon Tetrachloride	3.755	117	392214	11.041	ppbv	100
36) Benzene	3.648	78	484758	10.753	ppbv	98
37) 1,2-Dichloroethane	3.211	62	290241	11.246	ppbv	99
38) Trichloroethene	4.538	130	193516	10.288	ppbv	99
39) 1,2-Dichloropropane	4.305	63	178422	10.868	ppbv	92
40) 1,4-Dioxane	4.570	88	81717	9.378	ppbv #	96
41) Tetrahydrofuran	3.049	42	201299	10.601	ppbv	95
42) Bromodichloromethane	4.480	83	406194	11.416	ppbv	100
43) Methyl Methacrylate	4.871	69	177759	9.315	ppbv	99
44) 2,2,4-Trimethylpentane	4.628	57	844094	11.080	ppbv	97
45) t-1,3-Dichloropropene	6.402	75	168205	8.215	ppbv	93

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041025\
 Data File : VL042302.D
 Acq On : 10 Apr 2025 11:05
 Operator : SY/MD
 Sample : VL0410ABS01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0410ABS01

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/11/2025
 Supervised By : Mahesh Dadoda 04/11/2025

Quant Time: Apr 11 01:55:57 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Mar 28 02:00:52 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.587	75	226293	9.016	ppbv	98
47) 1,1,2-Trichloroethane	6.570	97	198266	11.424	ppbv	97
48) Dibromochloromethane	7.376	129	318857	10.841	ppbv	100
49) Bromoform	9.474	173	288223	10.915	ppbv	99
50) 4-Methyl-2-Pentanone	5.739	43	518035	9.913	ppbv	96
51) 2-Hexanone	7.428	43	414703	9.664	ppbv #	94
52) Tetrachloroethene	8.215	164	165334	9.248	ppbv	97
53) Toluene	6.923	91	527837	9.877	ppbv	100
54) 1,2-Dibromoethane	7.642	107	265105	10.958	ppbv	100
56) 1,1,1,2-Tetrachloroethane	8.917	131	269261	12.088	ppbv	99
57) Chlorobenzene	8.914	112	453135	11.805	ppbv	97
58) Ethyl Benzene	9.348	91	773516	10.761	ppbv	99
59) m/p-Xylene	9.542	91	1316027m	22.929	ppbv	
60) o-Xylene	9.956	91	656144	11.404	ppbv	96
61) Styrene	9.862	104	283752	9.968	ppbv	99
62) Isopropylbenzene	10.532	105	968339	11.254	ppbv	99
63) 1,1,2,2-Tetrachloroethane	9.956	83	437804	12.523	ppbv	99
64) n-propylbenzene	10.982	120	260101	11.743	ppbv	98
65) tert-Butylbenzene	11.526	119	891006	11.197	ppbv	99
66) Benzyl Chloride	11.610	91	67064	7.943	ppbv	98
67) sec-Butylbenzene	11.762	105	1266690	11.452	ppbv	99
69) p-Isopropyltoluene	11.921	119	1065111	11.183	ppbv	99
70) n-Butylbenzene	12.277	91	1117359	11.471	ppbv	99
71) 2-Chlorotoluene	10.895	91	738389	11.057	ppbv	98
72) 4-Ethyltoluene	11.118	105	818929	11.431	ppbv	99
73) 1,3,5-Trimethylbenzene	11.199	105	705360	11.273	ppbv	99
74) 1,2,4-Trimethylbenzene	11.532	105	800991	11.112	ppbv	97
75) 1,3-Dichlorobenzene	11.603	146	481728	12.185	ppbv	98
76) 1,4-Dichlorobenzene	11.668	146	479693	12.192	ppbv	99
77) 1,2-Dichlorobenzene	11.940	146	477721	12.411	ppbv	98
78) Hexachloro-1,3-Butadiene	13.879	225	380053	9.700	ppbv	99
79) Naphthalene	13.510	128	905270	11.482	ppbv	99
80) Naphthalene,2-methyl-	14.455	142	422199	10.919	ppbv	99
81) 1,2,4-Trichlorobenzene	13.435	180	402319	11.063	ppbv	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041025\
 Data File : VL042307.D
 Acq On : 10 Apr 2025 14:20
 Operator : SY/MD
 Sample : QC040925 CAN 10604
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC040925 CAN 10604

Quant Time: Apr 11 01:58:51 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.781	49	167662	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.952	114	409947	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.875	117	345392	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.370	95	261215	9.209	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	92.100%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041025\
Data File : VL042307.D
Acq On : 10 Apr 2025 14:20
Operator : SY/MD
Sample : QC040925 CAN 10604
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC040925 CAN 10604

Quant Time: Apr 11 01:58:51 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Fri Mar 28 02:00:52 2025
Response via : Initial Calibration



Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041025\
 Data File : VL042308.D
 Acq On : 10 Apr 2025 14:51
 Operator : SY/MD
 Sample : QC040825 CAN 10445
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC040825 CAN 10445

Quant Time: Apr 11 01:59:12 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.784	49	169533	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.955	114	400917	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.878	117	344890	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.374	95	257971	9.108	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	91.100%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041025\
Data File : VL042308.D
Acq On : 10 Apr 2025 14:51
Operator : SY/MD
Sample : QC040825 CAN 10445
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC040825 CAN 10445

Quant Time: Apr 11 01:59:12 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Fri Mar 28 02:00:52 2025
Response via : Initial Calibration





Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041125\
Data File : VL042311.D
Acq On : 11 Apr 2025 08:18
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Mar 28 02:00:52 2025



AutoFind: Scans 3178, 3179, 3180; Background Corrected with Scan 3165

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.4	51160	PASS
75	95	30	66	57.3	120195	PASS
95	95	100	100	100.0	209621	PASS
96	95	5	9	6.6	13755	PASS
173	174	0.00	2	0.5	631	PASS
174	95	50	120	61.1	128109	PASS
175	174	4	9	7.5	9591	PASS
176	174	93	101	94.7	121299	PASS
177	176	5	9	6.6	7977	PASS

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041125\
 Data File : VL042312.D
 Acq On : 11 Apr 2025 09:50
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDCCC010

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/16/2025
 Supervised By : Mahesh Dadoda 04/17/2025

Quant Time: Apr 11 22:56:21 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2025

QLast Update : Fri Mar 28 02:00:52 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.787	49	183700	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.959	114	463746	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.885	117	401340	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene 10.377 95 318204 9.655 ppbv 0.00
 Spiked Amount 10.000 Range 65 - 135 Recovery = 96.500%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.499	85	264775	9.762	ppbv	100
3) Chlorodifluoromethane	1.476	51	287991	10.394	ppbv	97
4) Chloromethane	1.531	50	111786	10.085	ppbv	98
5) Vinyl Chloride	1.580	62	102342	8.713	ppbv	95
6) Bromomethane	1.667	94	43054	8.571	ppbv	99
7) Chloroethane	1.703	64	41946	9.427	ppbv	98
8) Dichlorotetrafluoroethane	1.554	85	224489	9.719	ppbv	94
9) Propene	1.483	41	117677	9.266	ppbv	99
10) Heptane	4.981	43	334707	9.908	ppbv	100
11) Trichlorofluoromethane	1.877	101	250122	9.477	ppbv	99
12) 1,1,2-Trichlorotrifluo...	2.140	101	193510	8.920	ppbv	97
13) Ethanol	1.722	45	5849	4.872	ppbv	89
14) Bromoethene	1.780	108	73294	8.820	ppbv	100
15) Acetone	1.835	43	231724	9.019	ppbv	97
16) 1,3-Butadiene	1.609	39	112297	8.950	ppbv	97
17) tert-Butyl alcohol	2.039	59	255575	7.987	ppbv	99
18) 1,1-Dichloroethene	2.033	96	89512	8.827	ppbv	98
19) Isopropyl Alcohol	1.887	45	125233	8.639	ppbv	92
20) Methylene Chloride	2.062	84	76968	8.044	ppbv	93
21) Allyl Chloride	2.098	41	162998	8.996	ppbv	97
22) trans-1,2-Dichloroethene	2.340	96	101974	8.700	ppbv	95
23) Vinyl Acetate	2.463	43	95152	8.557	ppbv	99
24) 1,1-Dichloroethane	2.408	63	207862	9.567	ppbv	99
25) Ethyl Acetate	2.835	43	678920	10.182	ppbv	99
26) Hexane	2.826	57	256866	9.973	ppbv	98
27) Carbon Disulfide	2.149	76	243367	8.812	ppbv	98
28) Methyl tert-Butyl Ether	2.441	73	129141	8.053	ppbv	96
29) Chloroform	2.848	83	393638	10.443	ppbv	98
30) Cyclohexane	3.858	84	203526	9.100	ppbv	97
31) cis-1,2-Dichloroethene	2.722	61	247194	9.454	ppbv	97
32) 1,1,1-Trichloroethane	3.370	97	380312	8.813	ppbv	98
34) 2-Butanone	2.557	43	380682	11.321	ppbv	98
35) Carbon Tetrachloride	3.764	117	390140	10.769	ppbv	98
36) Benzene	3.658	78	506278	11.012	ppbv	97
37) 1,2-Dichloroethane	3.221	62	292183	11.101	ppbv	99
38) Trichloroethene	4.551	130	203156	10.591	ppbv	96
39) 1,2-Dichloropropane	4.315	63	185497	11.079	ppbv	97
40) 1,4-Dioxane	4.583	88	82376	9.270	ppbv #	98
41) Tetrahydrofuran	3.056	42	216646	11.188	ppbv	93
42) Bromodichloromethane	4.493	83	413250	11.389	ppbv	99
43) Methyl Methacrylate	4.884	69	184472	9.478	ppbv	96
44) 2,2,4-Trimethylpentane	4.642	57	872871	11.235	ppbv	98
45) t-1,3-Dichloropropene	6.422	75	176804	8.467	ppbv	97

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041125\
 Data File : VL042312.D
 Acq On : 11 Apr 2025 09:50
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDCCC010

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/16/2025
 Supervised By :Mahesh Dadoda 04/17/2025

Quant Time: Apr 11 22:56:21 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Mar 28 02:00:52 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.603	75	236039	9.222	ppbv	99
47) 1,1,2-Trichloroethane	6.583	97	202891	11.463	ppbv	98
48) Dibromochloromethane	7.389	129	333128	11.106	ppbv	99
49) Bromoform	9.484	173	294489	10.935	ppbv	100
50) 4-Methyl-2-Pentanone	5.755	43	531851	9.980	ppbv	95
51) 2-Hexanone	7.438	43	424035	9.689	ppbv #	94
52) Tetrachloroethene	8.224	164	170989	9.378	ppbv	97
53) Toluene	6.936	91	547579	10.048	ppbv	99
54) 1,2-Dibromoethane	7.655	107	267225	10.831	ppbv	99
56) 1,1,1,2-Tetrachloroethane	8.927	131	271350	12.283	ppbv	100
57) Chlorobenzene	8.924	112	460598	12.099	ppbv	98
58) Ethyl Benzene	9.357	91	779227	10.931	ppbv	98
59) m/p-Xylene	9.552	91	1323463m	23.249	ppbv	
60) o-Xylene	9.966	91	660065	11.567	ppbv	96
61) Styrene	9.872	104	291355	10.320	ppbv	99
62) Isopropylbenzene	10.542	105	988337	11.582	ppbv	98
63) 1,1,2,2-Tetrachloroethane	9.966	83	446341	12.873	ppbv	99
64) n-propylbenzene	10.992	120	268681	12.231	ppbv	97
65) tert-Butylbenzene	11.532	119	932850	11.820	ppbv	98
66) Benzyl Chloride	11.616	91	68675	8.201	ppbv	99
67) sec-Butylbenzene	11.769	105	1310042	11.942	ppbv	100
69) p-Isopropyltoluene	11.927	119	1107045	11.720	ppbv	99
70) n-Butylbenzene	12.283	91	1144571	11.848	ppbv	99
71) 2-Chlorotoluene	10.904	91	756562	11.423	ppbv	98
72) 4-Ethyltoluene	11.128	105	847821	11.932	ppbv	99
73) 1,3,5-Trimethylbenzene	11.205	105	729887	11.762	ppbv	99
74) 1,2,4-Trimethylbenzene	11.539	105	819490	11.463	ppbv	92
75) 1,3-Dichlorobenzene	11.610	146	492549	12.562	ppbv	99
76) 1,4-Dichlorobenzene	11.675	146	488636	12.522	ppbv	98
77) 1,2-Dichlorobenzene	11.950	146	494739	12.959	ppbv	98
78) Hexachloro-1,3-Butadiene	13.882	225	373025	9.599	ppbv	99
79) Naphthalene	13.516	128	824947	10.550	ppbv	100
80) Naphthalene,2-methyl-	14.458	142	276556	7.212	ppbv	98
81) 1,2,4-Trichlorobenzene	13.442	180	374714	10.389	ppbv	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041125\
 Data File : VL042312.D
 Acq On : 11 Apr 2025 09:50
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 LabSampleId :
 VSTDCCC010

Quant Time: Apr 11 22:56:21 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Min. RRF : 0.050 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	Bromochloromethane	1.000	1.000	0.0	98	0.00
2 T	Dichlorodifluoromethane	1.476	1.441	2.4	101	0.00
3	Chlorodifluoromethane	1.508	1.568	-4.0	106	0.00
4	Chloromethane	0.603	0.609	-1.0	104	0.00
5 T	Vinyl Chloride	0.639	0.557	12.8	100	0.00
6 T	Bromomethane	0.273	0.234	14.3	90	0.00
7	Chloroethane	0.242	0.228	5.8	99	0.00
8 T	Dichlorotetrafluoroethane	1.257	1.222	2.8	99	0.00
9 T	Propene	0.691	0.641	7.2	95	0.00
10 T	Heptane	1.839	1.822	0.9	100	0.00
11 T	Trichlorofluoromethane	1.437	1.362	5.2	100	0.00
12 T	1,1,2-Trichlorotrifluoroeth	1.181	1.053	10.8	92	0.00
13	Ethanol	0.065	0.032#	50.8#	110	0.00
14 T	Bromoethene	0.452	0.399	11.7	94	0.00
15 T	Acetone	1.399	1.261	9.9	111	0.00
16 T	1,3-Butadiene	0.683	0.611	10.5	105	0.00
17	tert-Butyl alcohol	1.742	1.391	20.1	84	0.00
18 T	1,1-Dichloroethene	0.552	0.487	11.8	95	0.00
19 T	Isopropyl Alcohol	0.789	0.682	13.6	95	0.00
20 T	Methylene Chloride	0.521	0.419	19.6	94	0.00
21 T	Allyl Chloride	0.986	0.887	10.0	97	0.00
22 T	trans-1,2-Dichloroethene	0.638	0.555	13.0	92	0.00
23 T	Vinyl Acetate	0.605	0.518	14.4	102	0.00
24 T	1,1-Dichloroethane	1.183	1.132	4.3	99	0.00
25 T	Ethyl Acetate	3.630	3.696	-1.8	105	0.00
26 T	Hexane	1.402	1.398	0.3	103	0.00
27 T	Carbon Disulfide	1.503	1.325	11.8	91	0.00
28 T	Methyl tert-Butyl Ether	0.873	0.703	19.5	83	0.00
29 T	Chloroform	2.052	2.143	-4.4	109	0.00
30 T	Cyclohexane	1.217	1.108	9.0	94	0.00
31 T	cis-1,2-Dichloroethene	1.423	1.346	5.4	96	0.00
32 T	1,1,1-Trichloroethane	2.349	2.070	11.9	99	0.00
33 I	1,4-Difluorobenzene	1.000	1.000	0.0	85	0.00
34 T	2-Butanone	0.725	0.821	-13.2	105	0.00
35 T	Carbon Tetrachloride	0.781	0.841	-7.7	102	0.00
36 T	Benzene	0.991	1.092	-10.2	99	0.00
37 T	1,2-Dichloroethane	0.568	0.630	-10.9	100	0.00
38 T	Trichloroethene	0.414	0.438	-5.8	100	0.00
39 T	1,2-Dichloropropane	0.361	0.400	-10.8	101	0.00
40 T	1,4-Dioxane	0.192	0.178	7.3	89	0.00
41 T	Tetrahydrofuran	0.418	0.467	-11.7	100	0.00
42 T	Bromodichloromethane	0.782	0.891	-13.9	99	0.00
43	Methyl Methacrylate	0.420	0.398	5.2	84	0.01
44 T	2,2,4-Trimethylpentane	1.675	1.882	-12.4	100	0.00
45 T	t-1,3-Dichloropropene	0.450	0.381	15.3	74	0.02
46 T	cis-1,3-Dichloropropene	0.552	0.509	7.8	79	0.00
47 T	1,1,2-Trichloroethane	0.382	0.438	-14.7	102	0.00
48 T	Dibromochloromethane	0.647	0.718	-11.0	96	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041125\
 Data File : VL042312.D
 Acq On : 11 Apr 2025 09:50
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 LabSampleId :
 VSTDCCC010

Quant Time: Apr 11 22:56:21 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Min. RRF : 0.050 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
49 T	Bromoform	0.581	0.635	-9.3	93	0.00
50 T	4-Methyl-2-Pentanone	1.149	1.147	0.2	95	0.00
51 T	2-Hexanone	0.944	0.914	3.2	92	0.00
52 T	Tetrachloroethene	0.393	0.369	6.1	91	0.00
53 T	Toluene	1.175	1.181	-0.5	89	0.00
54 T	1,2-Dibromoethane	0.532	0.576	-8.3	97	0.00
55 I	Chlorobenzene-d5	1.000	1.000	0.0	77	0.00
56	1,1,1,2-Tetrachloroethane	0.550	0.676	-22.9	102	0.00
57 T	Chlorobenzene	0.949	1.148	-21.0	101	0.00
58 T	Ethyl Benzene	1.776	1.942	-9.3	90	0.00
59 T	m/p-Xylene	1.418	1.649	-16.3	96	0.00
60 T	o-Xylene	1.422	1.645	-15.7	96	0.00
61 T	Styrene	0.703	0.726	-3.3	82	0.00
62	Isopropylbenzene	2.126	2.463	-15.9	97	0.00
63 T	1,1,2,2-Tetrachloroethane	0.864	1.112	-28.7	108	0.00
64	n-propylbenzene	0.547	0.669	-22.3	104	0.00
65	tert-Butylbenzene	1.966	2.324	-18.2	103	0.00
66 T	Benzyl Chloride	0.209	0.171	18.2	65	0.00
67	sec-Butylbenzene	2.733	3.264	-19.4	105	0.00
68 S	1-Bromo-4-Fluorobenzene	0.821	0.793	3.4	75	0.00
69	p-Isopropyltoluene	2.354	2.758	-17.2	103	0.00
70	n-Butylbenzene	2.407	2.852	-18.5	103	0.00
71	2-Chlorotoluene	1.650	1.885	-14.2	95	0.00
72 T	4-Ethyltoluene	1.770	2.112	-19.3	100	0.00
73 T	1,3,5-Trimethylbenzene	1.546	1.819	-17.7	101	0.00
74 T	1,2,4-Trimethylbenzene	1.781	2.042	-14.7	104	0.00
75 T	1,3-Dichlorobenzene	0.977	1.227	-25.6	107	0.00
76 T	1,4-Dichlorobenzene	0.972	1.218	-25.3	106	0.00
77 T	1,2-Dichlorobenzene	0.951	1.233	-29.7	112	0.00
78 T	Hexachloro-1,3-Butadiene	0.968	0.929	4.0	90	0.00
79 T	Naphthalene	1.948	2.055	-5.5	88	0.00
80 T	Naphthalene,2-methyl-	0.955	0.689	27.9	54	0.00
81 T	1,2,4-Trichlorobenzene	0.899	0.934	-3.9	84	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041125\
 Data File : VL042313.D
 Acq On : 11 Apr 2025 10:36
 Operator : SY/MD
 Sample : VL0411ABL01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0411ABL01

Quant Time: Apr 11 22:57:18 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.790	49	180225	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.962	114	445487	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.885	117	373548	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.380	95	277731	9.054	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	90.500%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041125\
Data File : VL042313.D
Acq On : 11 Apr 2025 10:36
Operator : SY/MD
Sample : VL0411ABL01
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VL0411ABL01

Quant Time: Apr 11 22:57:18 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Fri Mar 28 02:00:52 2025
Response via : Initial Calibration



Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041125\
 Data File : VL042314.D
 Acq On : 11 Apr 2025 11:23
 Operator : SY/MD
 Sample : VL0411ABS01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0411ABS01

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/16/2025
 Supervised By : Mahesh Dadoda 04/17/2025

Quant Time: Apr 11 22:57:41 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2025

QLast Update : Fri Mar 28 02:00:52 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.784	49	178456	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.955	114	444353	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.878	117	386060	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	10.374	95	314180	9.910	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.100%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.496	85	260154	9.873	ppbv	99
3) Chlorodifluoromethane	1.473	51	278310	10.339	ppbv	99
4) Chloromethane	1.531	50	109906	10.207	ppbv	97
5) Vinyl Chloride	1.577	62	99540	8.723	ppbv	96
6) Bromomethane	1.667	94	43354	8.884	ppbv	99
7) Chloroethane	1.703	64	40372	9.340	ppbv	100
8) Dichlorotetrafluoroethane	1.551	85	219210	9.769	ppbv	94
9) Propene	1.483	41	109077	8.841	ppbv	98
10) Heptane	4.975	43	325268	9.912	ppbv	98
11) Trichlorofluoromethane	1.874	101	247344	9.647	ppbv	98
12) 1,1,2-Trichlorotrifluo...	2.136	101	191456	9.085	ppbv	97
13) Ethanol	1.719	45	4928	4.225	ppbv	95
14) Bromoethene	1.780	108	70702	8.758	ppbv	99
15) Acetone	1.832	43	228988	9.175	ppbv	95
16) 1,3-Butadiene	1.606	39	110429	9.060	ppbv	97
17) tert-Butyl alcohol	2.039	59	243034	7.818	ppbv	100
18) 1,1-Dichloroethene	2.030	96	83233	8.449	ppbv	97
19) Isopropyl Alcohol	1.884	45	118345	8.404	ppbv #	34
20) Methylene Chloride	2.059	84	75264	8.097	ppbv	93
21) Allyl Chloride	2.094	41	157261	8.934	ppbv	98
22) trans-1,2-Dichloroethene	2.337	96	98769	8.674	ppbv	96
23) Vinyl Acetate	2.460	43	86563	8.014	ppbv	98
24) 1,1-Dichloroethane	2.405	63	206840	9.800	ppbv	99
25) Ethyl Acetate	2.836	43	656719	10.138	ppbv	99
26) Hexane	2.823	57	249860	9.986	ppbv	98
27) Carbon Disulfide	2.146	76	236998	8.833	ppbv	99
28) Methyl tert-Butyl Ether	2.438	73	122818	7.884	ppbv	97
29) Chloroform	2.845	83	384713	10.506	ppbv	100
30) Cyclohexane	3.852	84	196133	9.028	ppbv	97
31) cis-1,2-Dichloroethene	2.719	61	233371	9.187	ppbv	97
32) 1,1,1-Trichloroethane	3.363	97	370405	8.836	ppbv	98
34) 2-Butanone	2.554	43	362633	11.254	ppbv	98
35) Carbon Tetrachloride	3.758	117	389738	11.228	ppbv	99
36) Benzene	3.654	78	490339	11.131	ppbv	96
37) 1,2-Dichloroethane	3.214	62	290983	11.538	ppbv	100
38) Trichloroethene	4.545	130	195654	10.645	ppbv	99
39) 1,2-Dichloropropane	4.312	63	179954	11.217	ppbv	91
40) 1,4-Dioxane	4.580	88	80106	9.408	ppbv #	83
41) Tetrahydrofuran	3.052	42	202793	10.930	ppbv	94
42) Bromodichloromethane	4.486	83	405729	11.669	ppbv	97
43) Methyl Methacrylate	4.875	69	177423	9.514	ppbv	98
44) 2,2,4-Trimethylpentane	4.635	57	850971	11.431	ppbv	97
45) t-1,3-Dichloropropene	6.412	75	166246	8.309	ppbv	93

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041125\
 Data File : VL042314.D
 Acq On : 11 Apr 2025 11:23
 Operator : SY/MD
 Sample : VL0411ABS01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0411ABS01

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/16/2025
 Supervised By :Mahesh Dadoda 04/17/2025

Quant Time: Apr 11 22:57:41 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Mar 28 02:00:52 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.596	75	225952	9.213	ppbv	99
47) 1,1,2-Trichloroethane	6.580	97	198762	11.720	ppbv	97
48) Dibromochloromethane	7.383	129	321370	11.181	ppbv	100
49) Bromoform	9.480	173	291905	11.313	ppbv	99
50) 4-Methyl-2-Pentanone	5.749	43	514910	10.084	ppbv	95
51) 2-Hexanone	7.435	43	414681	9.889	ppbv #	94
52) Tetrachloroethene	8.221	164	165666	9.483	ppbv	96
53) Toluene	6.933	91	526341	10.079	ppbv	99
54) 1,2-Dibromoethane	7.649	107	264126	11.172	ppbv	97
56) 1,1,1,2-Tetrachloroethane	8.924	131	271061	12.755	ppbv	97
57) Chlorobenzene	8.921	112	457204	12.486	ppbv	96
58) Ethyl Benzene	9.354	91	761549	11.105	ppbv	98
59) m/p-Xylene	9.548	91	1323517m	24.171	ppbv	
60) o-Xylene	9.963	91	654791	11.929	ppbv	96
61) Styrene	9.869	104	284318	10.470	ppbv	98
62) Isopropylbenzene	10.539	105	975799	11.887	ppbv	98
63) 1,1,2,2-Tetrachloroethane	9.963	83	440972	13.222	ppbv	100
64) n-propylbenzene	10.989	120	264518	12.518	ppbv	96
65) tert-Butylbenzene	11.529	119	908946	11.973	ppbv	99
66) Benzyl Chloride	11.617	91	69548	8.634	ppbv	98
67) sec-Butylbenzene	11.765	105	1300090	12.320	ppbv	100
69) p-Isopropyltoluene	11.924	119	1095041	12.051	ppbv	98
70) n-Butylbenzene	12.280	91	1129853	12.159	ppbv	100
71) 2-Chlorotoluene	10.901	91	749737	11.768	ppbv	99
72) 4-Ethyltoluene	11.125	105	825037	12.071	ppbv	99
73) 1,3,5-Trimethylbenzene	11.202	105	711175	11.914	ppbv	99
74) 1,2,4-Trimethylbenzene	11.536	105	816505	11.873	ppbv	91
75) 1,3-Dichlorobenzene	11.607	146	484099	12.835	ppbv	98
76) 1,4-Dichlorobenzene	11.672	146	485460	12.933	ppbv	98
77) 1,2-Dichlorobenzene	11.947	146	485421	13.218	ppbv	98
78) Hexachloro-1,3-Butadiene	13.882	225	366850	9.814	ppbv	99
79) Naphthalene	13.513	128	820200	10.904	ppbv	100
80) Naphthalene,2-methyl-	14.455	142	274227	7.434	ppbv	98
81) 1,2,4-Trichlorobenzene	13.439	180	373404	10.762	ppbv	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041125\
Data File : VL042316.D
Acq On : 11 Apr 2025 12:40
Operator : SY/MD
Sample : QC041025CAN 10596
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC041025CAN 10596

Quant Time: Apr 11 22:59:00 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Fri Mar 28 02:00:52 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.787	49	170330	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.962	114	400070	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.885	117	341964	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	10.380	95	254170	9.051	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	90.500%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041125\
Data File : VL042316.D
Acq On : 11 Apr 2025 12:40
Operator : SY/MD
Sample : QC041025CAN 10596
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC041025CAN 10596

Quant Time: Apr 11 22:59:00 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Fri Mar 28 02:00:52 2025
Response via : Initial Calibration





Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
Data File : VL042325.D
Acq On : 15 Apr 2025 07:45
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Mar 28 02:00:52 2025



AutoFind: Scans 3185, 3186, 3187; Background Corrected with Scan 3171

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	24.0	62363	PASS
75	95	30	66	55.5	144299	PASS
95	95	100	100	100.0	260117	PASS
96	95	5	9	6.7	17331	PASS
173	174	0.00	2	1.3	2038	PASS
174	95	50	120	62.4	162261	PASS
175	174	4	9	6.8	11092	PASS
176	174	93	101	94.8	153792	PASS
177	176	5	9	6.2	9603	PASS

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
 Data File : VL042326.D
 Acq On : 15 Apr 2025 11:30
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDCCC010

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/16/2025
 Supervised By : Mahesh Dadoda 04/16/2025

Quant Time: Apr 16 01:29:10 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Mar 28 02:00:52 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.806	49	172263	10.000	ppbv	0.02
33) 1,4-Difluorobenzene	3.988	114	457227	10.000	ppbv	0.04
55) Chlorobenzene-d5	8.911	117	411493	10.000	ppbv	0.04

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene 10.403 95 325960 9.646 ppbv 0.03
 Spiked Amount 10.000 Range 65 - 135 Recovery = 96.500%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.505	85	214541	8.435	ppbv	99
3) Chlorodifluoromethane	1.483	51	235250	9.054	ppbv	98
4) Chloromethane	1.541	50	89653	8.625	ppbv	98
5) Vinyl Chloride	1.589	62	83204	7.554	ppbv	96
6) Bromomethane	1.677	94	36297	7.705	ppbv	99
7) Chloroethane	1.716	64	32145	7.704	ppbv	97
8) Dichlorotetrafluoroethane	1.564	85	182884	8.443	ppbv	94
9) Propene	1.492	41	101034	8.483	ppbv	98
10) Heptane	5.020	43	276748	8.736	ppbv	98
11) Trichlorofluoromethane	1.887	101	202387	8.178	ppbv	99
12) 1,1,2-Trichlorotrifluo...	2.153	101	157030	7.719	ppbv	98
13) Ethanol	1.732	45	4440	3.944	ppbv	93
14) Bromoethene	1.793	108	59588	7.646	ppbv	99
15) Acetone	1.845	43	183439	7.614	ppbv	96
16) 1,3-Butadiene	1.619	39	90954	7.731	ppbv	100
17) tert-Butyl alcohol	2.052	59	209737	6.990	ppbv	100
18) 1,1-Dichloroethene	2.046	96	72322	7.605	ppbv	96
19) Isopropyl Alcohol	1.897	45	104424	7.682	ppbv	98
20) Methylene Chloride	2.075	84	60337	6.725	ppbv	90
21) Allyl Chloride	2.111	41	132956	7.825	ppbv	98
22) trans-1,2-Dichloroethene	2.357	96	81572	7.422	ppbv	96
23) Vinyl Acetate	2.480	43	72160	6.920	ppbv	97
24) 1,1-Dichloroethane	2.425	63	169411	8.315	ppbv	100
25) Ethyl Acetate	2.855	43	564611	9.030	ppbv	99
26) Hexane	2.845	57	213782	8.851	ppbv	98
27) Carbon Disulfide	2.166	76	195452	7.547	ppbv	97
28) Methyl tert-Butyl Ether	2.457	73	116301	7.734	ppbv	96
29) Chloroform	2.868	83	314164	8.888	ppbv	100
30) Cyclohexane	3.884	84	173360	8.266	ppbv	98
31) cis-1,2-Dichloroethene	2.739	61	208160	8.490	ppbv	96
32) 1,1,1-Trichloroethane	3.392	97	311758	7.704	ppbv	98
34) 2-Butanone	2.577	43	317117	9.565	ppbv	97
35) Carbon Tetrachloride	3.790	117	317942	8.902	ppbv	99
36) Benzene	3.684	78	424254	9.360	ppbv	94
37) 1,2-Dichloroethane	3.243	62	239556	9.231	ppbv	100
38) Trichloroethene	4.583	130	172146	9.102	ppbv	96
39) 1,2-Dichloropropane	4.350	63	151707	9.190	ppbv	96
40) 1,4-Dioxane	4.622	88	72075	8.226	ppbv #	98
41) Tetrahydrofuran	3.075	42	181471	9.505	ppbv	95
42) Bromodichloromethane	4.525	83	333167	9.313	ppbv	97
43) Methyl Methacrylate	4.923	69	155399	8.098	ppbv	96
44) 2,2,4-Trimethylpentane	4.677	57	728571	9.511	ppbv	99
45) t-1,3-Dichloropropene	6.461	75	151063	7.338	ppbv	96

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
 Data File : VL042326.D
 Acq On : 15 Apr 2025 11:30
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDCCC010

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/16/2025
 Supervised By :Mahesh Dadoda 04/16/2025

Quant Time: Apr 16 01:29:10 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Mar 28 02:00:52 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.648	75	204339	8.097	ppbv	98
47) 1,1,2-Trichloroethane	6.626	97	163132	9.348	ppbv	97
48) Dibromochloromethane	7.425	129	272592	9.217	ppbv	99
49) Bromoform	9.513	173	238880	8.997	ppbv	100
50) 4-Methyl-2-Pentanone	5.800	43	442851	8.428	ppbv	97
51) 2-Hexanone	7.474	43	353471	8.192	ppbv #	97
52) Tetrachloroethene	8.260	164	144481	8.037	ppbv	98
53) Toluene	6.975	91	461854	8.595	ppbv	100
54) 1,2-Dibromoethane	7.687	107	220075	9.047	ppbv	97
56) 1,1,1,2-Tetrachloroethane	8.956	131	214175	9.455	ppbv	99
57) Chlorobenzene	8.953	112	375357	9.617	ppbv	97
58) Ethyl Benzene	9.383	91	639857	8.754	ppbv	99
59) m/p-Xylene	9.581	91	1063509m	18.222	ppbv	
60) o-Xylene	9.992	91	528896	9.040	ppbv	95
61) Styrene	9.898	104	245300	8.474	ppbv	97
62) Isopropylbenzene	10.565	105	794408	9.079	ppbv	98
63) 1,1,2,2-Tetrachloroethane	9.992	83	343786	9.671	ppbv	100
64) n-propylbenzene	11.015	120	212879	9.452	ppbv	95
65) tert-Butylbenzene	11.555	119	721078	8.911	ppbv	97
66) Benzyl Chloride	11.639	91	54427	6.339	ppbv	98
67) sec-Butylbenzene	11.791	105	1026079	9.123	ppbv	99
69) p-Isopropyltoluene	11.947	119	865385	8.935	ppbv	99
70) n-Butylbenzene	12.303	91	884265	8.928	ppbv	99
71) 2-Chlorotoluene	10.927	91	599592	8.830	ppbv	98
72) 4-Ethyltoluene	11.147	105	657765	9.029	ppbv	99
73) 1,3,5-Trimethylbenzene	11.228	105	557593	8.764	ppbv	99
74) 1,2,4-Trimethylbenzene	11.558	105	623563	8.507	ppbv #	86
75) 1,3-Dichlorobenzene	11.630	146	381572	9.492	ppbv	98
76) 1,4-Dichlorobenzene	11.694	146	380035	9.499	ppbv	98
77) 1,2-Dichlorobenzene	11.969	146	379896	9.706	ppbv	97
78) Hexachloro-1,3-Butadiene	13.902	225	311900	7.828	ppbv	99
79) Naphthalene	13.533	128	760876	9.490	ppbv	99
80) Naphthalene,2-methyl-	14.478	142	365398	9.294	ppbv	98
81) 1,2,4-Trichlorobenzene	13.461	180	337032	9.114	ppbv	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
 Data File : VL042326.D
 Acq On : 15 Apr 2025 11:30
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 LabSampleId :
 VSTDCCC010

Quant Time: Apr 16 01:29:10 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Min. RRF : 0.050 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	Bromochloromethane	1.000	1.000	0.0	92	0.02
2 T	Dichlorodifluoromethane	1.476	1.245	15.7	82	0.00
3	Chlorodifluoromethane	1.508	1.366	9.4	86	0.00
4	Chloromethane	0.603	0.520	13.8	84	0.00
5 T	Vinyl Chloride	0.639	0.483	24.4	81	0.01
6 T	Bromomethane	0.273	0.211	22.7	76	0.01
7	Chloroethane	0.242	0.187	22.7	76	0.01
8 T	Dichlorotetrafluoroethane	1.257	1.062	15.5	81	0.01
9 T	Propene	0.691	0.587	15.1	82	0.00
10 T	Heptane	1.839	1.607	12.6	83	0.05
11 T	Trichlorofluoromethane	1.437	1.175	18.2	81	0.01
12 T	1,1,2-Trichlorotrifluoroeth	1.181	0.912	22.8	75	0.02
13	Ethanol	0.065	0.026#	60.0#	83	0.01
14 T	Bromoethene	0.452	0.346	23.5	76	0.02
15 T	Acetone	1.399	1.065	23.9	88	0.01
16 T	1,3-Butadiene	0.683	0.528	22.7	85	0.01
17	tert-Butyl alcohol	1.742	1.218	30.1#	69	0.02
18 T	1,1-Dichloroethene	0.552	0.420	23.9	77	0.02
19 T	Isopropyl Alcohol	0.789	0.606	23.2	79	0.01
20 T	Methylene Chloride	0.521	0.350	32.8#	74	0.02
21 T	Allyl Chloride	0.986	0.772	21.7	79	0.02
22 T	trans-1,2-Dichloroethene	0.638	0.474	25.7	74	0.02
23 T	Vinyl Acetate	0.605	0.419	30.7#	78	0.02
24 T	1,1-Dichloroethane	1.183	0.983	16.9	81	0.02
25 T	Ethyl Acetate	3.630	3.278	9.7	87	0.02
26 T	Hexane	1.402	1.241	11.5	86	0.02
27 T	Carbon Disulfide	1.503	1.135	24.5	73	0.02
28 T	Methyl tert-Butyl Ether	0.873	0.675	22.7	75	0.02
29 T	Chloroform	2.052	1.824	11.1	87	0.02
30 T	Cyclohexane	1.217	1.006	17.3	80	0.03
31 T	cis-1,2-Dichloroethene	1.423	1.208	15.1	81	0.02
32 T	1,1,1-Trichloroethane	2.349	1.810	22.9	81	0.03
33 I	1,4-Difluorobenzene	1.000	1.000	0.0	84	0.04
34 T	2-Butanone	0.725	0.694	4.3	87	0.02
35 T	Carbon Tetrachloride	0.781	0.695	11.0	83	0.03
36 T	Benzene	0.991	0.928	6.4	83	0.03
37 T	1,2-Dichloroethane	0.568	0.524	7.7	82	0.03
38 T	Trichloroethene	0.414	0.377	8.9	84	0.04
39 T	1,2-Dichloropropane	0.361	0.332	8.0	83	0.04
40 T	1,4-Dioxane	0.192	0.158	17.7	78	0.05
41 T	Tetrahydrofuran	0.418	0.397	5.0	84	0.03
42 T	Bromodichloromethane	0.782	0.729	6.8	80	0.04
43	Methyl Methacrylate	0.420	0.340	19.0	71	0.05
44 T	2,2,4-Trimethylpentane	1.675	1.593	4.9	83	0.04
45 T	t-1,3-Dichloropropene	0.450	0.330	26.7	63	0.05
46 T	cis-1,3-Dichloropropene	0.552	0.447	19.0	68	0.05
47 T	1,1,2-Trichloroethane	0.382	0.357	6.5	82	0.05
48 T	Dibromochloromethane	0.647	0.596	7.9	79	0.05

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
 Data File : VL042326.D
 Acq On : 15 Apr 2025 11:30
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 LabSampleId :
 VSTDCCC010

Quant Time: Apr 16 01:29:10 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Min. RRF : 0.050 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
49 T	Bromoform	0.581	0.522	10.2	75	0.04
50 T	4-Methyl-2-Pentanone	1.149	0.969	15.7	79	0.05
51 T	2-Hexanone	0.944	0.773	18.1	77	0.04
52 T	Tetrachloroethene	0.393	0.316	19.6	77	0.04
53 T	Toluene	1.175	1.010	14.0	75	0.05
54 T	1,2-Dibromoethane	0.532	0.481	9.6	80	0.04
55 I	Chlorobenzene-d5	1.000	1.000	0.0	79	0.04
56	1,1,1,2-Tetrachloroethane	0.550	0.520	5.5	81	0.04
57 T	Chlorobenzene	0.949	0.912	3.9	83	0.04
58 T	Ethyl Benzene	1.776	1.555	12.4	74	0.03
59 T	m/p-Xylene	1.418	1.292	8.9	77	0.03
60 T	o-Xylene	1.422	1.285	9.6	77	0.03
61 T	Styrene	0.703	0.596	15.2	69	0.03
62	Isopropylbenzene	2.126	1.931	9.2	78	0.03
63 T	1,1,2,2-Tetrachloroethane	0.864	0.835	3.4	83	0.03
64	n-propylbenzene	0.547	0.517	5.5	82	0.03
65	tert-Butylbenzene	1.966	1.752	10.9	80	0.03
66 T	Benzyl Chloride	0.209	0.132	36.8#	52	0.03
67	sec-Butylbenzene	2.733	2.494	8.7	82	0.03
68 S	1-Bromo-4-Fluorobenzene	0.821	0.792	3.5	77	0.03
69	p-Isopropyltoluene	2.354	2.103	10.7	80	0.02
70	n-Butylbenzene	2.407	2.149	10.7	80	0.03
71	2-Chlorotoluene	1.650	1.457	11.7	75	0.03
72 T	4-Ethyltoluene	1.770	1.598	9.7	78	0.03
73 T	1,3,5-Trimethylbenzene	1.546	1.355	12.4	77	0.03
74 T	1,2,4-Trimethylbenzene	1.781	1.515	14.9	79	0.02
75 T	1,3-Dichlorobenzene	0.977	0.927	5.1	83	0.03
76 T	1,4-Dichlorobenzene	0.972	0.924	4.9	82	0.03
77 T	1,2-Dichlorobenzene	0.951	0.923	2.9	86	0.03
78 T	Hexachloro-1,3-Butadiene	0.968	0.758	21.7	75	0.02
79 T	Naphthalene	1.948	1.849	5.1	81	0.02
80 T	Naphthalene,2-methyl-	0.955	0.888	7.0	71	0.02
81 T	1,2,4-Trichlorobenzene	0.899	0.819	8.9	75	0.02

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
 Data File : VL042327.D
 Acq On : 15 Apr 2025 12:12
 Operator : SY/MD
 Sample : VL0415ABL01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0415ABL01

Quant Time: Apr 16 01:30:06 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.813	49	173729	10.000	ppbv	0.03
33) 1,4-Difluorobenzene	3.994	114	447320	10.000	ppbv	0.04
55) Chlorobenzene-d5	8.917	117	385318	10.000	ppbv	0.04

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.406	95	292759	9.252	ppbv	0.04
Spiked Amount	10.000	Range	65 - 135	Recovery	=	92.500%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
Data File : VL042327.D
Acq On : 15 Apr 2025 12:12
Operator : SY/MD
Sample : VL0415ABL01
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VL0415ABL01

Quant Time: Apr 16 01:30:06 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Fri Mar 28 02:00:52 2025
Response via : Initial Calibration



Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
 Data File : VL042328.D
 Acq On : 15 Apr 2025 12:54
 Operator : SY/MD
 Sample : VL0415ABS01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0415ABS01

Quant Time: Apr 16 01:30:27 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2025

QLast Update : Fri Mar 28 02:00:52 2025

Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 04/16/2025
 Supervised By : Mahesh Dadoda 04/16/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.810	49	171986	10.000	ppbv	0.03
33) 1,4-Difluorobenzene	3.994	114	444595	10.000	ppbv	0.04
55) Chlorobenzene-d5	8.917	117	399604	10.000	ppbv	0.04
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.406	95	318902	9.718	ppbv	0.04
Spiked Amount	10.000	Range	65 - 135	Recovery	=	97.200%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.509	85	214241	8.437	ppbv	99
3) Chlorodifluoromethane	1.486	51	234966	9.058	ppbv	97
4) Chloromethane	1.541	50	88230	8.502	ppbv	98
5) Vinyl Chloride	1.589	62	82221	7.476	ppbv	94
6) Bromomethane	1.680	94	36050	7.665	ppbv	100
7) Chloroethane	1.716	64	33039	7.931	ppbv	97
8) Dichlorotetrafluoroethane	1.564	85	178173	8.239	ppbv	95
9) Propene	1.492	41	94136	7.917	ppbv	99
10) Heptane	5.027	43	267288	8.451	ppbv	99
11) Trichlorofluoromethane	1.890	101	201665	8.162	ppbv	99
12) 1,1,2-Trichlorotrifluo...	2.156	101	154306	7.598	ppbv	98
13) Ethanol	1.732	45	4407	3.921	ppbv	97
14) Bromoethene	1.793	108	57635	7.408	ppbv	99
15) Acetone	1.848	43	178724	7.430	ppbv	96
16) 1,3-Butadiene	1.619	39	89479	7.617	ppbv	96
17) tert-Butyl alcohol	2.055	59	202421	6.757	ppbv	99
18) 1,1-Dichloroethene	2.049	96	69013	7.269	ppbv	97
19) Isopropyl Alcohol	1.900	45	100289	7.390	ppbv	97
20) Methylene Chloride	2.075	84	60054	6.704	ppbv	88
21) Allyl Chloride	2.111	41	127800	7.534	ppbv	98
22) trans-1,2-Dichloroethene	2.360	96	78991	7.198	ppbv	98
23) Vinyl Acetate	2.483	43	64777	6.222	ppbv	98
24) 1,1-Dichloroethane	2.428	63	168373	8.277	ppbv	99
25) Ethyl Acetate	2.861	43	545140	8.732	ppbv	99
26) Hexane	2.848	57	205629	8.528	ppbv	97
27) Carbon Disulfide	2.166	76	191388	7.402	ppbv	99
28) Methyl tert-Butyl Ether	2.460	73	107667	7.172	ppbv	96
29) Chloroform	2.874	83	309262	8.763	ppbv	100
30) Cyclohexane	3.891	84	165914	7.924	ppbv	98
31) cis-1,2-Dichloroethene	2.742	61	197651	8.074	ppbv	99
32) 1,1,1-Trichloroethane	3.395	97	304143	7.528	ppbv	97
34) 2-Butanone	2.580	43	300576	9.323	ppbv	98
35) Carbon Tetrachloride	3.797	117	314849	9.065	ppbv	99
36) Benzene	3.690	78	407959	9.256	ppbv	98
37) 1,2-Dichloroethane	3.247	62	235609	9.337	ppbv	99
38) Trichloroethene	4.590	130	164664	8.954	ppbv	96
39) 1,2-Dichloropropane	4.354	63	149260	9.299	ppbv	97
40) 1,4-Dioxane	4.625	88	68773	8.072	ppbv #	95
41) Tetrahydrofuran	3.082	42	173776	9.361	ppbv	95
42) Bromodichloromethane	4.532	83	327497	9.414	ppbv	99
43) Methyl Methacrylate	4.930	69	151531	8.121	ppbv	98
44) 2,2,4-Trimethylpentane	4.680	57	707832	9.503	ppbv	98
45) t-1,3-Dichloropropene	6.470	75	143714	7.179	ppbv	91

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
 Data File : VL042328.D
 Acq On : 15 Apr 2025 12:54
 Operator : SY/MD
 Sample : VL0415ABS01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0415ABS01

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/16/2025
 Supervised By :Mahesh Dadoda 04/16/2025

Quant Time: Apr 16 01:30:27 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Mar 28 02:00:52 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.658	75	192419	7.841	ppbv	96
47) 1,1,2-Trichloroethane	6.635	97	163251	9.621	ppbv	98
48) Dibromochloromethane	7.428	129	266192	9.256	ppbv	100
49) Bromoform	9.519	173	236686	9.168	ppbv	99
50) 4-Methyl-2-Pentanone	5.807	43	429988	8.416	ppbv	95
51) 2-Hexanone	7.480	43	344172	8.203	ppbv #	96
52) Tetrachloroethene	8.263	164	139845	8.000	ppbv	95
53) Toluene	6.978	91	447178	8.559	ppbv	99
54) 1,2-Dibromoethane	7.694	107	214982	9.089	ppbv	98
56) 1,1,1,2-Tetrachloroethane	8.959	131	216770	9.855	ppbv	98
57) Chlorobenzene	8.956	112	369132	9.739	ppbv	95
58) Ethyl Benzene	9.390	91	618669	8.716	ppbv	100
59) m/p-Xylene	9.584	91	1049238m	18.512	ppbv	
60) o-Xylene	9.995	91	517471	9.107	ppbv	96
61) Styrene	9.904	104	229601	8.168	ppbv	97
62) Isopropylbenzene	10.568	105	785673	9.247	ppbv	99
63) 1,1,2,2-Tetrachloroethane	9.995	83	351308	10.176	ppbv	99
64) n-propylbenzene	11.018	120	210294	9.615	ppbv	98
65) tert-Butylbenzene	11.558	119	718948	9.149	ppbv	97
66) Benzyl Chloride	11.642	91	55150	6.614	ppbv	99
67) sec-Butylbenzene	11.795	105	1018861	9.328	ppbv	100
69) p-Isopropyltoluene	11.950	119	863264	9.179	ppbv	99
70) n-Butylbenzene	12.306	91	891883	9.273	ppbv	99
71) 2-Chlorotoluene	10.930	91	590408	8.953	ppbv	99
72) 4-Ethyltoluene	11.150	105	652962	9.230	ppbv	98
73) 1,3,5-Trimethylbenzene	11.231	105	559451	9.055	ppbv	100
74) 1,2,4-Trimethylbenzene	11.565	105	632271	8.883	ppbv	97
75) 1,3-Dichlorobenzene	11.633	146	381882	9.782	ppbv	98
76) 1,4-Dichlorobenzene	11.697	146	383116	9.861	ppbv	98
77) 1,2-Dichlorobenzene	11.973	146	386768	10.175	ppbv	98
78) Hexachloro-1,3-Butadiene	13.905	225	314860	8.138	ppbv	100
79) Naphthalene	13.539	128	777722	9.989	ppbv	99
80) Naphthalene,2-methyl-	14.481	142	375541	9.836	ppbv	98
81) 1,2,4-Trichlorobenzene	13.465	180	343011	9.551	ppbv	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
 Data File : VL042330.D
 Acq On : 15 Apr 2025 13:57
 Operator : SY/MD
 Sample : QC041425 CAN 10401
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC041425 CAN 10401

Quant Time: Apr 16 01:31:42 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.813	49	162884	10.000	ppbv	0.03
33) 1,4-Difluorobenzene	3.997	114	405181	10.000	ppbv	0.05
55) Chlorobenzene-d5	8.917	117	353699	10.000	ppbv	0.04

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.406	95	273327	9.410	ppbv	0.04
Spiked Amount	10.000	Range	65 - 135	Recovery	=	94.100%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
Data File : VL042330.D
Acq On : 15 Apr 2025 13:57
Operator : SY/MD
Sample : QC041425 CAN 10401
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC041425 CAN 10401

Quant Time: Apr 16 01:31:42 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Fri Mar 28 02:00:52 2025
Response via : Initial Calibration



Instrument ID: **MSVOA_L**

Daily Analysis Runlog For Sequence/QC Batch ID # VL032725

Review By	Maresh Dadoda	Review On	4/3/2025 8:14:07 AM		
Supervise By	Semsettin Yesilyurt	Supervise On	4/3/2025 8:45:16 AM		
SubDirectory	VL032725	HP Acquire Method	TO15AIR.M	HP Processing Method	VL032725AIR.M
STD. NAME		STD REF.#			
Tune/Reschk		AP2589			
Initial Calibration Stds		AP2593,AP2595,AP2596			
CCC		AP2593			
Internal Standard/PEM		AP2589			
ICV/I.BLK		AP2594			
Surrogate Standard					
MS/MSD Standard					
LCS Standard					

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VL042171.D	27 Mar 2025 07:44	SY/MD	Ok
2	VSTDICCC010	VL042172.D	27 Mar 2025 08:26	SY/MD	Ok,M
3	VSTDICCC002	VL042173.D	27 Mar 2025 08:59	SY/MD	Ok,M
4	VSTDICCC001	VL042174.D	27 Mar 2025 09:30	SY/MD	Ok,M
5	VSTDICCC0.5	VL042175.D	27 Mar 2025 10:01	SY/MD	Ok,M
6	VSTDICCC0.1	VL042176.D	27 Mar 2025 10:32	SY/MD	Ok,M
7	VSTDICCC0.03	VL042177.D	27 Mar 2025 11:03	SY/MD	Ok,M
8	VSTDICCC015	VL042178.D	27 Mar 2025 11:36	SY/MD	Ok,M
9	VSTDICV010	VL042179.D	27 Mar 2025 12:23	SY/MD	Ok,M
10	VL0327ABL01	VL042180.D	27 Mar 2025 13:50	SY/MD	Ok
11	VL0327ABS01	VL042181.D	27 Mar 2025 14:39	SY/MD	Ok,M
12	QC032625 CAN 10448	VL042182.D	27 Mar 2025 16:41	SY/MD	Ok
13	Q1649-01	VL042183.D	27 Mar 2025 17:13	SY/MD	Not Ok
14	Q1649-02	VL042184.D	27 Mar 2025 17:45	SY/MD	Not Ok
15	Q1669-01	VL042185.D	27 Mar 2025 18:22	SY/MD	Dilution
16	Q1669-02	VL042186.D	27 Mar 2025 18:59	SY/MD	Ok,M
17	Q1669-03	VL042187.D	27 Mar 2025 19:36	SY/MD	Ok,M
18	Q1669-04	VL042188.D	27 Mar 2025 20:12	SY/MD	Ok,M
19	Q1669-09	VL042189.D	27 Mar 2025 20:48	SY/MD	Ok,M
20	Q1669-09DUP	VL042190.D	27 Mar 2025 21:24	SY/MD	Ok,M
21	Q1669-05	VL042191.D	27 Mar 2025 21:57	SY/MD	Not Ok

Instrument ID: **MSVOA_L**

Daily Analysis Runlog For Sequence/QC Batch ID # VL032725

Review By	Maresh Dadoda	Review On	4/3/2025 8:14:07 AM		
Supervise By	Semsettin Yesilyurt	Supervise On	4/3/2025 8:45:16 AM		
SubDirectory	VL032725	HP Acquire Method	TO15AIR.M	HP Processing Method	VL032725AIR.M
STD. NAME		STD REF.#			
Tune/Reschk		AP2589			
Initial Calibration Stds		AP2593,AP2595,AP2596			
CCC		AP2593			
Internal Standard/PEM		AP2589			
ICV/I.BLK		AP2594			
Surrogate Standard					
MS/MSD Standard					
LCS Standard					

22	Q1669-07DL	VL042192.D	27 Mar 2025 22:29	SY/MD	Ok,M
23	Q1669-08	VL042193.D	27 Mar 2025 23:01	SY/MD	Not Ok
24	VIBLK	VL042194.D	27 Mar 2025 23:34	SY/MD	Ok
25	Q1669-01DL	VL042195.D	28 Mar 2025 00:06	SY/MD	Ok,M
26	Q1669-01DUP	VL042196.D	28 Mar 2025 00:44	SY/MD	Ok,M
27	Q1669-05	VL042197.D	28 Mar 2025 01:20	SY/MD	Ok,M
28	Q1669-07	VL042198.D	28 Mar 2025 01:57	SY/MD	Dilution
29	Q1669-08	VL042199.D	28 Mar 2025 02:33	SY/MD	Ok,M

M : Manual Integration

Instrument ID: **MSVOA_L**

Daily Analysis Runlog For Sequence/QC Batch ID # VL040425

Review By	Semsettin Yesilyurt	Review On	4/7/2025 1:45:32 PM		
Supervise By	Maresh Dadoda	Supervise On	4/8/2025 1:55:16 AM		
SubDirectory	VL040425	HP Acquire Method	TO15AIR.M	HP Processing Method	VL032725AIR.M
STD. NAME		STD REF.#			
Tune/Reschk		AP2591			
Initial Calibration Stds		AP2593,AP2595,AP2596			
CCC		AP2593			
Internal Standard/PEM		AP2591			
ICV/I.BLK		AP2594			
Surrogate Standard					
MS/MSD Standard					
LCS Standard					

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VL042214.D	04 Apr 2025 08:05	SY/MD	Ok
2	VSTDCCC010	VL042215.D	04 Apr 2025 08:58	SY/MD	Ok,M
3	VL0404ABL01	VL042216.D	04 Apr 2025 09:41	SY/MD	Ok
4	QC040125 CAN 10258	VL042217.D	04 Apr 2025 10:13	SY/MD	Ok
5	QC040325 CAN 10401	VL042218.D	04 Apr 2025 10:44	SY/MD	Ok
6	QC040325 CAN 10300	VL042219.D	04 Apr 2025 11:16	SY/MD	Ok
7	VL0404ABS01	VL042220.D	04 Apr 2025 11:55	SY/MD	Ok,M
8	Q1691-01	VL042221.D	04 Apr 2025 12:46	SY/MD	Ok,M
9	Q1691-01DUP	VL042222.D	04 Apr 2025 13:20	SY/MD	Ok,M
10	Q1691-01DL	VL042223.D	04 Apr 2025 13:51	SY/MD	Not Ok
11	Q1691-02	VL042224.D	04 Apr 2025 14:26	SY/MD	Ok,M
12	Q1691-03	VL042225.D	04 Apr 2025 15:50	SY/MD	Ok,M
13	Q1691-04	VL042226.D	04 Apr 2025 16:24	SY/MD	Ok,M

M : Manual Integration

Instrument ID: **MSVOA_L**

Daily Analysis Runlog For Sequence/QC Batch ID # VL041025

Review By	Semsettin Yesilyurt	Review On	4/11/2025 8:15:54 AM		
Supervise By	Mahesh Dadoda	Supervise On	4/11/2025 2:00:08 PM		
SubDirectory	VL041025	HP Acquire Method	TO15AIR.M	HP Processing Method	VL032725AIR.M
STD. NAME		STD REF.#			
Tune/Reschk		AP2591			
Initial Calibration Stds		AP2593,AP2595,AP2596			
CCC		AP2593			
Internal Standard/PEM		AP2591			
ICV/I.BLK		AP2594			
Surrogate Standard					
MS/MSD Standard					
LCS Standard					

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VL042299.D	10 Apr 2025 08:46	SY/MD	Ok
2	VSTDCCC010	VL042300.D	10 Apr 2025 09:27	SY/MD	Ok,M
3	VL0410ABL01	VL042301.D	10 Apr 2025 10:11	SY/MD	Ok
4	VL0410ABS01	VL042302.D	10 Apr 2025 11:05	SY/MD	Ok,M
5	Q1772-02	VL042303.D	10 Apr 2025 11:56	SY/MD	Ok,M
6	Q1772-02DUP	VL042304.D	10 Apr 2025 12:30	SY/MD	Ok,M
7	Q1772-01	VL042305.D	10 Apr 2025 13:01	SY/MD	Ok,M
8	QC040925 CAN 10604	VL042306.D	10 Apr 2025 13:49	SY/MD	Not Ok
9	QC040925 CAN 10604	VL042307.D	10 Apr 2025 14:20	SY/MD	Ok
10	QC040825 CAN 10445	VL042308.D	10 Apr 2025 14:51	SY/MD	Ok
11	CAN10197	VL042309.D	10 Apr 2025 15:23	SY/MD	Ok
12	CAN10607	VL042310.D	10 Apr 2025 15:54	SY/MD	Ok

M : Manual Integration

Instrument ID: **MSVOA_L**

Daily Analysis Runlog For Sequence/QC Batch ID # VL041125

Review By	Semsettin Yesilyurt	Review On	4/16/2025 9:18:47 PM		
Supervise By	Maresh Dadoda	Supervise On	4/17/2025 1:40:37 PM		
SubDirectory	VL041125	HP Acquire Method	TO15AIR.M	HP Processing Method	VL032725AIR.M
STD. NAME		STD REF.#			
Tune/Reschk	AP2591				
Initial Calibration Stds	AP2593,AP2595,AP2596				
CCC	AP2593				
Internal Standard/PEM	AP2591				
ICV/I.BLK	AP2594				
Surrogate Standard					
MS/MSD Standard					
LCS Standard					

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VL042311.D	11 Apr 2025 08:18	SY/MD	Ok
2	VSTDCCC010	VL042312.D	11 Apr 2025 09:50	SY/MD	Ok,M
3	VL0411ABL01	VL042313.D	11 Apr 2025 10:36	SY/MD	Ok
4	VL0411ABS01	VL042314.D	11 Apr 2025 11:23	SY/MD	Ok,M
5	QC041025CAN 10596	VL042315.D	11 Apr 2025 12:08	SY/MD	Not Ok
6	QC041025CAN 10596	VL042316.D	11 Apr 2025 12:40	SY/MD	Ok
7	Q1665-03	VL042317.D	11 Apr 2025 13:15	SY/MD	Dilution
8	Q1665-03DUP	VL042318.D	11 Apr 2025 13:52	SY/MD	Ok,M
9	Q1665-10	VL042319.D	11 Apr 2025 14:27	SY/MD	Dilution
10	Q1665-11	VL042320.D	11 Apr 2025 15:01	SY/MD	Dilution
11	Q1665-18	VL042321.D	11 Apr 2025 15:36	SY/MD	Dilution
12	Q1665-03DL	VL042322.D	11 Apr 2025 16:08	SY/MD	Ok
13	Q1665-10DL	VL042323.D	11 Apr 2025 16:39	SY/MD	Dilution
14	Q1665-11DL	VL042324.D	11 Apr 2025 17:10	SY/MD	Ok,M

M : Manual Integration

Instrument ID: **MSVOA_L**

Daily Analysis Runlog For Sequence/QC Batch ID # VL041525

Review By	Semsettin Yesilyurt	Review On	4/16/2025 2:19:24 PM		
Supervise By	Maresh Dadoda	Supervise On	4/16/2025 3:47:46 PM		
SubDirectory	VL041525	HP Acquire Method	TO15AIR.M	HP Processing Method	VL032725AIR.M
STD. NAME		STD REF.#			
Tune/Reschk		AP2591			
Initial Calibration Stds		AP2593,AP2595,AP2596			
CCC		AP2593			
Internal Standard/PEM		AP2591			
ICV/I.BLK		AP2594			
Surrogate Standard					
MS/MSD Standard					
LCS Standard					

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VL042325.D	15 Apr 2025 07:45	SY/MD	Ok
2	VSTDCCC010	VL042326.D	15 Apr 2025 11:30	SY/MD	Ok,M
3	VL0415ABL01	VL042327.D	15 Apr 2025 12:12	SY/MD	Ok
4	VL0415ABS01	VL042328.D	15 Apr 2025 12:54	SY/MD	Ok,M
5	QC041425 CAN 10401	VL042329.D	15 Apr 2025 13:26	SY/MD	Not Ok
6	QC041425 CAN 10401	VL042330.D	15 Apr 2025 13:57	SY/MD	Ok
7	Q1665-18DL	VL042331.D	15 Apr 2025 14:29	SY/MD	Ok
8	Q1665-10DL2	VL042332.D	15 Apr 2025 15:01	SY/MD	Ok,M
9	Q1802-02	VL042333.D	15 Apr 2025 15:35	SY/MD	Ok,M
10	Q1802-02DUP	VL042334.D	15 Apr 2025 16:08	SY/MD	Ok,M
11	Q1802-03	VL042335.D	15 Apr 2025 16:42	SY/MD	Ok,M
12	Q1802-01	VL042336.D	15 Apr 2025 17:14	SY/MD	Dilution
13	Q1802-01DL	VL042337.D	15 Apr 2025 17:46	SY/MD	Not Ok
14	Q1802-01DL	VL042338.D	15 Apr 2025 18:21	SY/MD	Ok,M

M : Manual Integration