

Instrument ID: **MSVOA_L**

Daily Analysis Runlog For Sequence/QC Batch ID # VL041525

Review By	Semsettin Yesilyurt	Review On	4/16/2025 2:19:24 PM		
Supervise By	Maresh Dadoda	Supervise On	4/16/2025 3:47:46 PM		
SubDirectory	VL041525	HP Acquire Method	TO15AIR.M	HP Processing Method	VL032725AIR.M
STD. NAME		STD REF.#			
Tune/Reschk		AP2591			
Initial Calibration Stds		AP2593,AP2595,AP2596			
CCC		AP2593			
Internal Standard/PEM		AP2591			
ICV/I.BLK		AP2594			
Surrogate Standard					
MS/MSD Standard					
LCS Standard					

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VL042325.D	15 Apr 2025 07:45	SY/MD	Ok
2	VSTDCCC010	VL042326.D	15 Apr 2025 11:30	SY/MD	Ok,M
3	VL0415ABL01	VL042327.D	15 Apr 2025 12:12	SY/MD	Ok
4	VL0415ABS01	VL042328.D	15 Apr 2025 12:54	SY/MD	Ok,M
5	QC041425 CAN 10401	VL042329.D	15 Apr 2025 13:26	SY/MD	Not Ok
6	QC041425 CAN 10401	VL042330.D	15 Apr 2025 13:57	SY/MD	Ok
7	Q1665-18DL	VL042331.D	15 Apr 2025 14:29	SY/MD	Ok
8	Q1665-10DL2	VL042332.D	15 Apr 2025 15:01	SY/MD	Ok,M
9	Q1802-02	VL042333.D	15 Apr 2025 15:35	SY/MD	Ok,M
10	Q1802-02DUP	VL042334.D	15 Apr 2025 16:08	SY/MD	Ok,M
11	Q1802-03	VL042335.D	15 Apr 2025 16:42	SY/MD	Ok,M
12	Q1802-01	VL042336.D	15 Apr 2025 17:14	SY/MD	Dilution
13	Q1802-01DL	VL042337.D	15 Apr 2025 17:46	SY/MD	Not Ok
14	Q1802-01DL	VL042338.D	15 Apr 2025 18:21	SY/MD	Ok,M

M : Manual Integration

Instrument ID: MSVOA_L

Daily Analysis Runlog For Sequence/QC Batch ID # VL042925

Review By	Semsettin Yesilyurt	Review On	4/30/2025 2:23:53 PM		
Supervise By	Mahesh Dadoda	Supervise On	4/30/2025 2:28:33 PM		
SubDirectory	VL042925	HP Acquire Method	TO15AIR.M	HP Processing Method	VL041725AIR.M
STD. NAME	STD REF.#				
Tune/Reschk	AP2602				
Initial Calibration Stds	AP2598,AP2599,AP2600				
CCC	AP2598				
Internal Standard/PEM	AP2602				
ICV/I.BLK	AP2601				
Surrogate Standard					
MS/MSD Standard					
LCS Standard					

22	Q1908-02	VL042456.D	29 Apr 2025 21:58	SY/MD	Ok,M
----	----------	------------	-------------------	-------	------

M : Manual Integration

Process Report

Order ID : Q1880

Date	Bottle ID	Lab Sample Number	InComing Vacuum	Canister ID	Can Size	Reg ID	Reg Size	Batch Code	Certification ID
04/25/2025	B2504018	Q1880-11	-1.4	10602	6 L	10203		C2504004	VL042307.D Seq :vl041025 TUNE : VL042299.D ICAL : VL042177.D CCAL : VL042300.D MB : VL042301.D
04/25/2025	B2504018	Q1880-10	-8.0	10326	6 L	10476		C2504004	VL042307.D Seq :vl041025 TUNE : VL042299.D ICAL : VL042177.D CCAL : VL042300.D MB : VL042301.D
04/25/2025	B2504018	Q1880-09	-7.1	10300	6 L	10110		C2504003	VL042219.D Seq :VL040425 TUNE : VL042214.D ICAL : VL042177.D CCAL : VL042215.D MB : VL042216.D
04/25/2025	B2504018	Q1880-08	-2.7	10282	6 L	10771		C2504005	VL042308.D Seq :vl041025 TUNE : VL042299.D ICAL : VL042177.D CCAL : VL042300.D MB : VL042301.D
04/25/2025	B2504018	Q1880-07	-6.3	10158	6 L	10785		C2504004	VL042307.D Seq :vl041025 TUNE : VL042299.D ICAL : VL042177.D CCAL : VL042300.D MB : VL042301.D
04/25/2025	B2504018	Q1880-06	-7.0	10024	6 L	10206		C2504005	VL042308.D Seq :vl041025 TUNE : VL042299.D ICAL : VL042177.D CCAL : VL042300.D MB : VL042301.D

Process Report

Order ID : Q1880



Date	Bottle ID	Lab Sample Number	InComing Vacuum	Canister ID	Can Size	Reg ID	Reg Size	Batch Code	Certification ID
04/25/2025	B2504019	Q1880-04	-5.9	10333	6 L	10222		C2504006	VL042316.D Seq :VL041125 TUNE : VL042311.D ICAL : VL042177.D CCAL : VL042312.D MB : VL042313.D
04/25/2025	B2504019	Q1880-05	-4.7	10401	6 L	10236		C2504007	VL042330.D Seq :VL041525 TUNE : VL042325.D ICAL : VL042177.D CCAL : VL042326.D MB : VL042327.D
04/25/2025	B2504019	Q1880-03	-5.9	10323	6 L	10537		C2504007	VL042330.D Seq :VL041525 TUNE : VL042325.D ICAL : VL042177.D CCAL : VL042326.D MB : VL042327.D
04/25/2025	B2504019	Q1880-02	-6.3	10268	6 L	10183		C2504007	VL042330.D Seq :VL041525 TUNE : VL042325.D ICAL : VL042177.D CCAL : VL042326.D MB : VL042327.D
04/25/2025	B2504019	Q1880-01	-6.7	10258	6 L	10567		C2504007	VL042330.D Seq :VL041525 TUNE : VL042325.D ICAL : VL042177.D CCAL : VL042326.D MB : VL042327.D

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
Data File : VL042325.D
Acq On : 15 Apr 2025 07:45
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Mar 28 02:00:52 2025

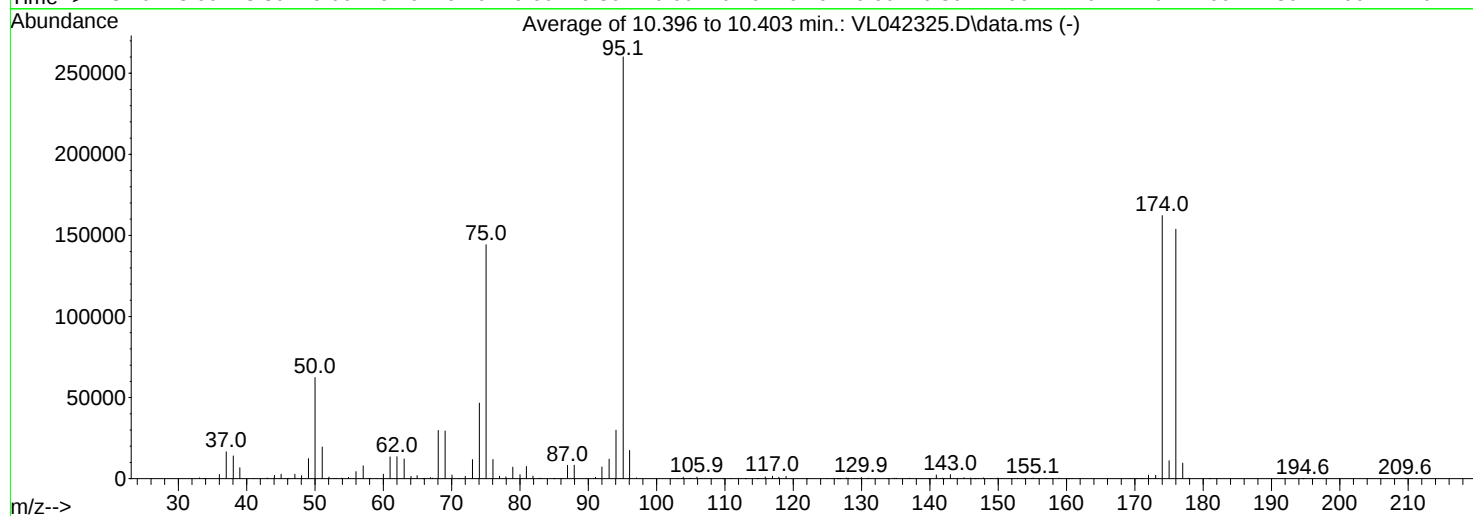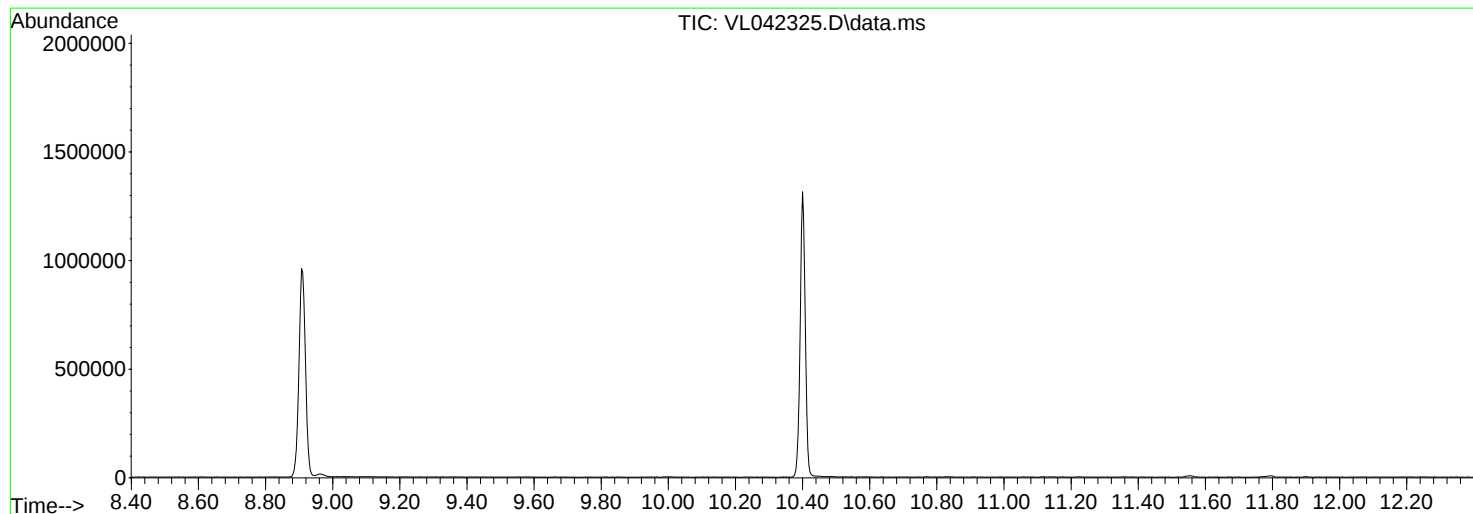

AutoFind: Scans 3185, 3186, 3187; Background Corrected with Scan 3171

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	24.0	62363	PASS
75	95	30	66	55.5	144299	PASS
95	95	100	100	100.0	260117	PASS
96	95	5	9	6.7	17331	PASS
173	174	0.00	2	1.3	2038	PASS
174	95	50	120	62.4	162261	PASS
175	174	4	9	6.8	11092	PASS
176	174	93	101	94.8	153792	PASS
177	176	5	9	6.2	9603	PASS

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
 Data File : VL042326.D
 Acq On : 15 Apr 2025 11:30
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDCCC010

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/16/2025
 Supervised By : Mahesh Dadoda 04/16/2025

Quant Time: Apr 16 01:29:10 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Mar 28 02:00:52 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.806	49	172263	10.000	ppbv	0.02
33) 1,4-Difluorobenzene	3.988	114	457227	10.000	ppbv	0.04
55) Chlorobenzene-d5	8.911	117	411493	10.000	ppbv	0.04

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene 10.403 95 325960 9.646 ppbv 0.03
 Spiked Amount 10.000 Range 65 - 135 Recovery = 96.500%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.505	85	214541	8.435	ppbv	99
3) Chlorodifluoromethane	1.483	51	235250	9.054	ppbv	98
4) Chloromethane	1.541	50	89653	8.625	ppbv	98
5) Vinyl Chloride	1.589	62	83204	7.554	ppbv	96
6) Bromomethane	1.677	94	36297	7.705	ppbv	99
7) Chloroethane	1.716	64	32145	7.704	ppbv	97
8) Dichlorotetrafluoroethane	1.564	85	182884	8.443	ppbv	94
9) Propene	1.492	41	101034	8.483	ppbv	98
10) Heptane	5.020	43	276748	8.736	ppbv	98
11) Trichlorofluoromethane	1.887	101	202387	8.178	ppbv	99
12) 1,1,2-Trichlorotrifluo...	2.153	101	157030	7.719	ppbv	98
13) Ethanol	1.732	45	4440	3.944	ppbv	93
14) Bromoethene	1.793	108	59588	7.646	ppbv	99
15) Acetone	1.845	43	183439	7.614	ppbv	96
16) 1,3-Butadiene	1.619	39	90954	7.731	ppbv	100
17) tert-Butyl alcohol	2.052	59	209737	6.990	ppbv	100
18) 1,1-Dichloroethene	2.046	96	72322	7.605	ppbv	96
19) Isopropyl Alcohol	1.897	45	104424	7.682	ppbv	98
20) Methylene Chloride	2.075	84	60337	6.725	ppbv	90
21) Allyl Chloride	2.111	41	132956	7.825	ppbv	98
22) trans-1,2-Dichloroethene	2.357	96	81572	7.422	ppbv	96
23) Vinyl Acetate	2.480	43	72160	6.920	ppbv	97
24) 1,1-Dichloroethane	2.425	63	169411	8.315	ppbv	100
25) Ethyl Acetate	2.855	43	564611	9.030	ppbv	99
26) Hexane	2.845	57	213782	8.851	ppbv	98
27) Carbon Disulfide	2.166	76	195452	7.547	ppbv	97
28) Methyl tert-Butyl Ether	2.457	73	116301	7.734	ppbv	96
29) Chloroform	2.868	83	314164	8.888	ppbv	100
30) Cyclohexane	3.884	84	173360	8.266	ppbv	98
31) cis-1,2-Dichloroethene	2.739	61	208160	8.490	ppbv	96
32) 1,1,1-Trichloroethane	3.392	97	311758	7.704	ppbv	98
34) 2-Butanone	2.577	43	317117	9.565	ppbv	97
35) Carbon Tetrachloride	3.790	117	317942	8.902	ppbv	99
36) Benzene	3.684	78	424254	9.360	ppbv	94
37) 1,2-Dichloroethane	3.243	62	239556	9.231	ppbv	100
38) Trichloroethene	4.583	130	172146	9.102	ppbv	96
39) 1,2-Dichloropropane	4.350	63	151707	9.190	ppbv	96
40) 1,4-Dioxane	4.622	88	72075	8.226	ppbv #	98
41) Tetrahydrofuran	3.075	42	181471	9.505	ppbv	95
42) Bromodichloromethane	4.525	83	333167	9.313	ppbv	97
43) Methyl Methacrylate	4.923	69	155399	8.098	ppbv	96
44) 2,2,4-Trimethylpentane	4.677	57	728571	9.511	ppbv	99
45) t-1,3-Dichloropropene	6.461	75	151063	7.338	ppbv	96

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
 Data File : VL042326.D
 Acq On : 15 Apr 2025 11:30
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDCCC010

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/16/2025
 Supervised By : Mahesh Dadoda 04/16/2025

Quant Time: Apr 16 01:29:10 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Mar 28 02:00:52 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.648	75	204339	8.097	ppbv	98
47) 1,1,2-Trichloroethane	6.626	97	163132	9.348	ppbv	97
48) Dibromochloromethane	7.425	129	272592	9.217	ppbv	99
49) Bromoform	9.513	173	238880	8.997	ppbv	100
50) 4-Methyl-2-Pentanone	5.800	43	442851	8.428	ppbv	97
51) 2-Hexanone	7.474	43	353471	8.192	ppbv #	97
52) Tetrachloroethene	8.260	164	144481	8.037	ppbv	98
53) Toluene	6.975	91	461854	8.595	ppbv	100
54) 1,2-Dibromoethane	7.687	107	220075	9.047	ppbv	97
56) 1,1,1,2-Tetrachloroethane	8.956	131	214175	9.455	ppbv	99
57) Chlorobenzene	8.953	112	375357	9.617	ppbv	97
58) Ethyl Benzene	9.383	91	639857	8.754	ppbv	99
59) m/p-Xylene	9.581	91	1063509m	18.222	ppbv	
60) o-Xylene	9.992	91	528896	9.040	ppbv	95
61) Styrene	9.898	104	245300	8.474	ppbv	97
62) Isopropylbenzene	10.565	105	794408	9.079	ppbv	98
63) 1,1,2,2-Tetrachloroethane	9.992	83	343786	9.671	ppbv	100
64) n-propylbenzene	11.015	120	212879	9.452	ppbv	95
65) tert-Butylbenzene	11.555	119	721078	8.911	ppbv	97
66) Benzyl Chloride	11.639	91	54427	6.339	ppbv	98
67) sec-Butylbenzene	11.791	105	1026079	9.123	ppbv	99
69) p-Isopropyltoluene	11.947	119	865385	8.935	ppbv	99
70) n-Butylbenzene	12.303	91	884265	8.928	ppbv	99
71) 2-Chlorotoluene	10.927	91	599592	8.830	ppbv	98
72) 4-Ethyltoluene	11.147	105	657765	9.029	ppbv	99
73) 1,3,5-Trimethylbenzene	11.228	105	557593	8.764	ppbv	99
74) 1,2,4-Trimethylbenzene	11.558	105	623563	8.507	ppbv #	86
75) 1,3-Dichlorobenzene	11.630	146	381572	9.492	ppbv	98
76) 1,4-Dichlorobenzene	11.694	146	380035	9.499	ppbv	98
77) 1,2-Dichlorobenzene	11.969	146	379896	9.706	ppbv	97
78) Hexachloro-1,3-Butadiene	13.902	225	311900	7.828	ppbv	99
79) Naphthalene	13.533	128	760876	9.490	ppbv	99
80) Naphthalene,2-methyl-	14.478	142	365398	9.294	ppbv	98
81) 1,2,4-Trichlorobenzene	13.461	180	337032	9.114	ppbv	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
Data File : VL042326.D
Acq On : 15 Apr 2025 11:30
Operator : SY/MD
Sample : VSTDCCC010
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDCCC010

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 04/16/2025
Supervised By : Mahesh Dadoda 04/16/2025


Quant Time: Apr 16 01:29:10 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug

QLast Update : Fri Mar 28 02:00:52 2025

Response via : Initial Calibration

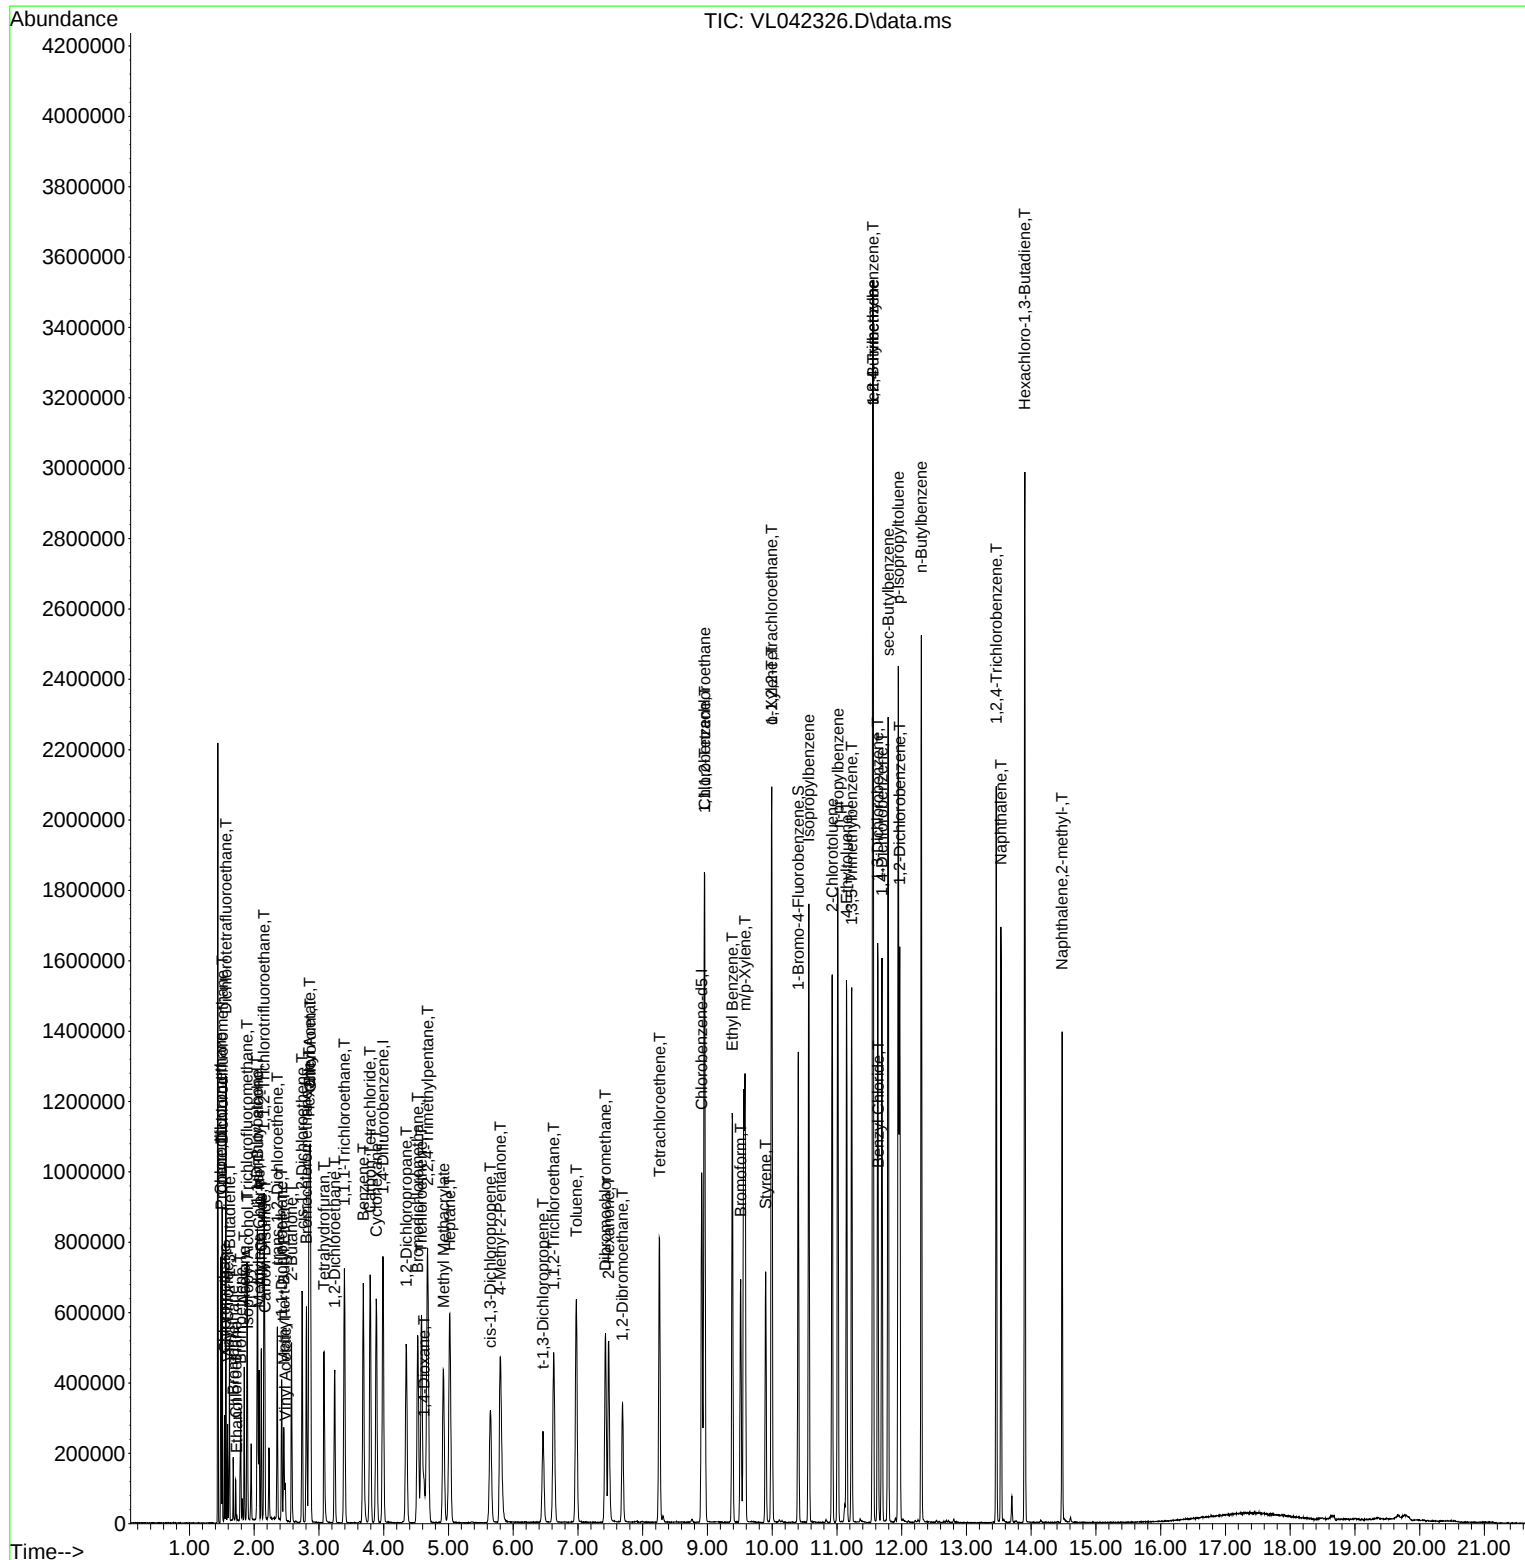

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
 Data File : VL042326.D
 Acq On : 15 Apr 2025 11:30
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 LabSampleId :
 VSTDCCC010

Quant Time: Apr 16 01:29:10 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Min. RRF : 0.050 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	Bromochloromethane	1.000	1.000	0.0	92	0.02
2 T	Dichlorodifluoromethane	1.476	1.245	15.7	82	0.00
3	Chlorodifluoromethane	1.508	1.366	9.4	86	0.00
4	Chloromethane	0.603	0.520	13.8	84	0.00
5 T	Vinyl Chloride	0.639	0.483	24.4	81	0.01
6 T	Bromomethane	0.273	0.211	22.7	76	0.01
7	Chloroethane	0.242	0.187	22.7	76	0.01
8 T	Dichlorotetrafluoroethane	1.257	1.062	15.5	81	0.01
9 T	Propene	0.691	0.587	15.1	82	0.00
10 T	Heptane	1.839	1.607	12.6	83	0.05
11 T	Trichlorofluoromethane	1.437	1.175	18.2	81	0.01
12 T	1,1,2-Trichlorotrifluoroeth	1.181	0.912	22.8	75	0.02
13	Ethanol	0.065	0.026#	60.0#	83	0.01
14 T	Bromoethene	0.452	0.346	23.5	76	0.02
15 T	Acetone	1.399	1.065	23.9	88	0.01
16 T	1,3-Butadiene	0.683	0.528	22.7	85	0.01
17	tert-Butyl alcohol	1.742	1.218	30.1#	69	0.02
18 T	1,1-Dichloroethene	0.552	0.420	23.9	77	0.02
19 T	Isopropyl Alcohol	0.789	0.606	23.2	79	0.01
20 T	Methylene Chloride	0.521	0.350	32.8#	74	0.02
21 T	Allyl Chloride	0.986	0.772	21.7	79	0.02
22 T	trans-1,2-Dichloroethene	0.638	0.474	25.7	74	0.02
23 T	Vinyl Acetate	0.605	0.419	30.7#	78	0.02
24 T	1,1-Dichloroethane	1.183	0.983	16.9	81	0.02
25 T	Ethyl Acetate	3.630	3.278	9.7	87	0.02
26 T	Hexane	1.402	1.241	11.5	86	0.02
27 T	Carbon Disulfide	1.503	1.135	24.5	73	0.02
28 T	Methyl tert-Butyl Ether	0.873	0.675	22.7	75	0.02
29 T	Chloroform	2.052	1.824	11.1	87	0.02
30 T	Cyclohexane	1.217	1.006	17.3	80	0.03
31 T	cis-1,2-Dichloroethene	1.423	1.208	15.1	81	0.02
32 T	1,1,1-Trichloroethane	2.349	1.810	22.9	81	0.03
33 I	1,4-Difluorobenzene	1.000	1.000	0.0	84	0.04
34 T	2-Butanone	0.725	0.694	4.3	87	0.02
35 T	Carbon Tetrachloride	0.781	0.695	11.0	83	0.03
36 T	Benzene	0.991	0.928	6.4	83	0.03
37 T	1,2-Dichloroethane	0.568	0.524	7.7	82	0.03
38 T	Trichloroethene	0.414	0.377	8.9	84	0.04
39 T	1,2-Dichloropropane	0.361	0.332	8.0	83	0.04
40 T	1,4-Dioxane	0.192	0.158	17.7	78	0.05
41 T	Tetrahydrofuran	0.418	0.397	5.0	84	0.03
42 T	Bromodichloromethane	0.782	0.729	6.8	80	0.04
43	Methyl Methacrylate	0.420	0.340	19.0	71	0.05
44 T	2,2,4-Trimethylpentane	1.675	1.593	4.9	83	0.04
45 T	t-1,3-Dichloropropene	0.450	0.330	26.7	63	0.05
46 T	cis-1,3-Dichloropropene	0.552	0.447	19.0	68	0.05
47 T	1,1,2-Trichloroethane	0.382	0.357	6.5	82	0.05
48 T	Dibromochloromethane	0.647	0.596	7.9	79	0.05

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
 Data File : VL042326.D
 Acq On : 15 Apr 2025 11:30
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 LabSampleId :
 VSTDCCC010

Quant Time: Apr 16 01:29:10 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Min. RRF : 0.050 Min. Rel. Area : 20% Max. R.T. Dev 0.50min
 Max. RRF Dev : 30% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
49 T	Bromoform	0.581	0.522	10.2	75	0.04
50 T	4-Methyl-2-Pentanone	1.149	0.969	15.7	79	0.05
51 T	2-Hexanone	0.944	0.773	18.1	77	0.04
52 T	Tetrachloroethene	0.393	0.316	19.6	77	0.04
53 T	Toluene	1.175	1.010	14.0	75	0.05
54 T	1,2-Dibromoethane	0.532	0.481	9.6	80	0.04
55 I	Chlorobenzene-d5	1.000	1.000	0.0	79	0.04
56	1,1,1,2-Tetrachloroethane	0.550	0.520	5.5	81	0.04
57 T	Chlorobenzene	0.949	0.912	3.9	83	0.04
58 T	Ethyl Benzene	1.776	1.555	12.4	74	0.03
59 T	m/p-Xylene	1.418	1.292	8.9	77	0.03
60 T	o-Xylene	1.422	1.285	9.6	77	0.03
61 T	Styrene	0.703	0.596	15.2	69	0.03
62	Isopropylbenzene	2.126	1.931	9.2	78	0.03
63 T	1,1,2,2-Tetrachloroethane	0.864	0.835	3.4	83	0.03
64	n-propylbenzene	0.547	0.517	5.5	82	0.03
65	tert-Butylbenzene	1.966	1.752	10.9	80	0.03
66 T	Benzyl Chloride	0.209	0.132	36.8#	52	0.03
67	sec-Butylbenzene	2.733	2.494	8.7	82	0.03
68 S	1-Bromo-4-Fluorobenzene	0.821	0.792	3.5	77	0.03
69	p-Isopropyltoluene	2.354	2.103	10.7	80	0.02
70	n-Butylbenzene	2.407	2.149	10.7	80	0.03
71	2-Chlorotoluene	1.650	1.457	11.7	75	0.03
72 T	4-Ethyltoluene	1.770	1.598	9.7	78	0.03
73 T	1,3,5-Trimethylbenzene	1.546	1.355	12.4	77	0.03
74 T	1,2,4-Trimethylbenzene	1.781	1.515	14.9	79	0.02
75 T	1,3-Dichlorobenzene	0.977	0.927	5.1	83	0.03
76 T	1,4-Dichlorobenzene	0.972	0.924	4.9	82	0.03
77 T	1,2-Dichlorobenzene	0.951	0.923	2.9	86	0.03
78 T	Hexachloro-1,3-Butadiene	0.968	0.758	21.7	75	0.02
79 T	Naphthalene	1.948	1.849	5.1	81	0.02
80 T	Naphthalene,2-methyl-	0.955	0.888	7.0	71	0.02
81 T	1,2,4-Trichlorobenzene	0.899	0.819	8.9	75	0.02

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
 Data File : VL042327.D
 Acq On : 15 Apr 2025 12:12
 Operator : SY/MD
 Sample : VL0415ABL01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0415ABL01

Quant Time: Apr 16 01:30:06 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.813	49	173729	10.000	ppbv	0.03
33) 1,4-Difluorobenzene	3.994	114	447320	10.000	ppbv	0.04
55) Chlorobenzene-d5	8.917	117	385318	10.000	ppbv	0.04

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.406	95	292759	9.252	ppbv	0.04
Spiked Amount	10.000	Range	65 - 135	Recovery	=	92.500%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
Data File : VL042327.D
Acq On : 15 Apr 2025 12:12
Operator : SY/MD
Sample : VL0415ABL01
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VL0415ABL01

Quant Time: Apr 16 01:30:06 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Fri Mar 28 02:00:52 2025
Response via : Initial Calibration

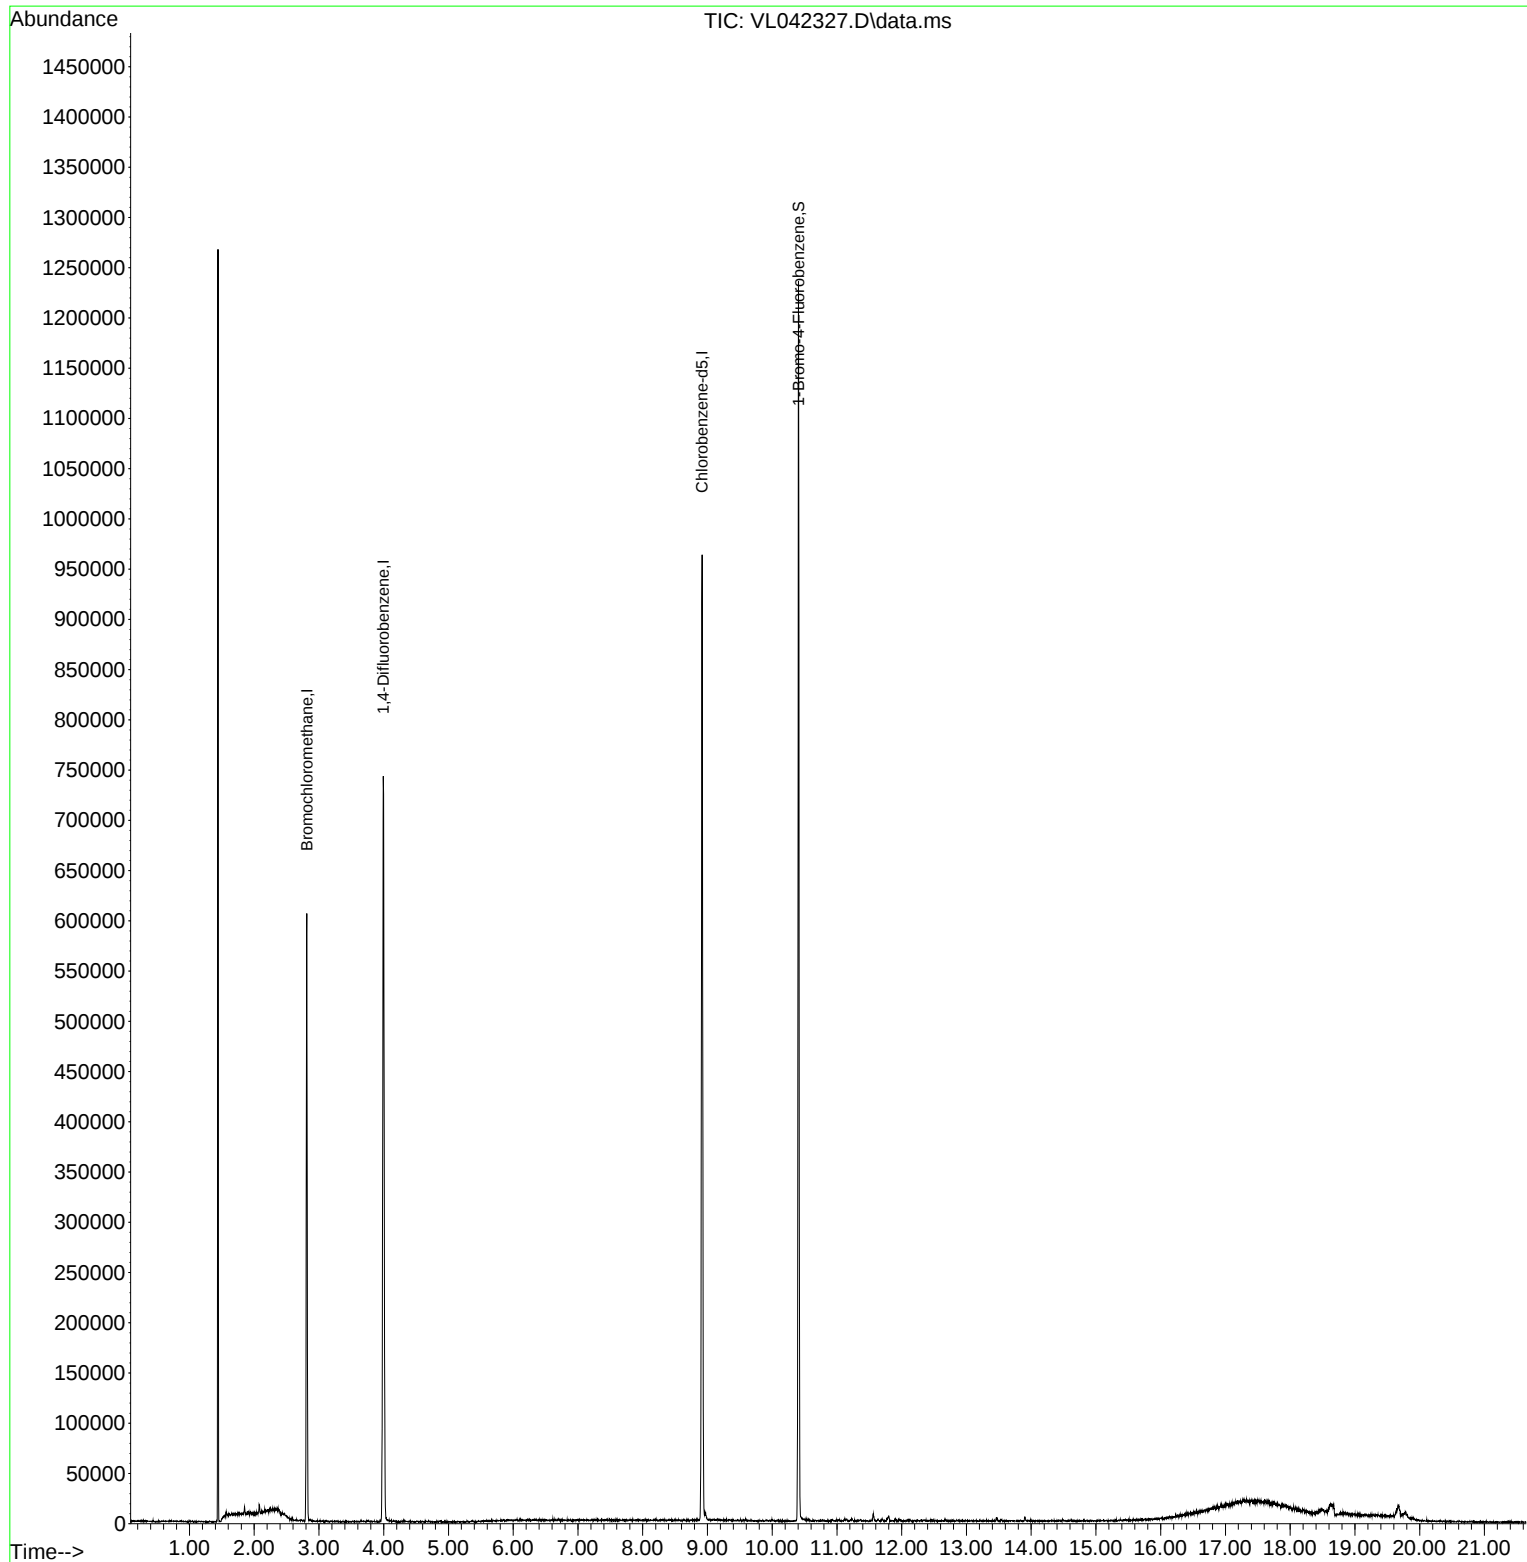

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
 Data File : VL042328.D
 Acq On : 15 Apr 2025 12:54
 Operator : SY/MD
 Sample : VL0415ABS01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0415ABS01

Quant Time: Apr 16 01:30:27 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 04/16/2025
 Supervised By : Mahesh Dadoda 04/16/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.810	49	171986	10.000	ppbv	0.03
33) 1,4-Difluorobenzene	3.994	114	444595	10.000	ppbv	0.04
55) Chlorobenzene-d5	8.917	117	399604	10.000	ppbv	0.04
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.406	95	318902	9.718	ppbv	0.04
Spiked Amount	10.000	Range	65 - 135	Recovery	=	97.200%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.509	85	214241	8.437	ppbv	99
3) Chlorodifluoromethane	1.486	51	234966	9.058	ppbv	97
4) Chloromethane	1.541	50	88230	8.502	ppbv	98
5) Vinyl Chloride	1.589	62	82221	7.476	ppbv	94
6) Bromomethane	1.680	94	36050	7.665	ppbv	100
7) Chloroethane	1.716	64	33039	7.931	ppbv	97
8) Dichlorotetrafluoroethane	1.564	85	178173	8.239	ppbv	95
9) Propene	1.492	41	94136	7.917	ppbv	99
10) Heptane	5.027	43	267288	8.451	ppbv	99
11) Trichlorofluoromethane	1.890	101	201665	8.162	ppbv	99
12) 1,1,2-Trichlorotrifluo...	2.156	101	154306	7.598	ppbv	98
13) Ethanol	1.732	45	4407	3.921	ppbv	97
14) Bromoethene	1.793	108	57635	7.408	ppbv	99
15) Acetone	1.848	43	178724	7.430	ppbv	96
16) 1,3-Butadiene	1.619	39	89479	7.617	ppbv	96
17) tert-Butyl alcohol	2.055	59	202421	6.757	ppbv	99
18) 1,1-Dichloroethene	2.049	96	69013	7.269	ppbv	97
19) Isopropyl Alcohol	1.900	45	100289	7.390	ppbv	97
20) Methylene Chloride	2.075	84	60054	6.704	ppbv	88
21) Allyl Chloride	2.111	41	127800	7.534	ppbv	98
22) trans-1,2-Dichloroethene	2.360	96	78991	7.198	ppbv	98
23) Vinyl Acetate	2.483	43	64777	6.222	ppbv	98
24) 1,1-Dichloroethane	2.428	63	168373	8.277	ppbv	99
25) Ethyl Acetate	2.861	43	545140	8.732	ppbv	99
26) Hexane	2.848	57	205629	8.528	ppbv	97
27) Carbon Disulfide	2.166	76	191388	7.402	ppbv	99
28) Methyl tert-Butyl Ether	2.460	73	107667	7.172	ppbv	96
29) Chloroform	2.874	83	309262	8.763	ppbv	100
30) Cyclohexane	3.891	84	165914	7.924	ppbv	98
31) cis-1,2-Dichloroethene	2.742	61	197651	8.074	ppbv	99
32) 1,1,1-Trichloroethane	3.395	97	304143	7.528	ppbv	97
34) 2-Butanone	2.580	43	300576	9.323	ppbv	98
35) Carbon Tetrachloride	3.797	117	314849	9.065	ppbv	99
36) Benzene	3.690	78	407959	9.256	ppbv	98
37) 1,2-Dichloroethane	3.247	62	235609	9.337	ppbv	99
38) Trichloroethene	4.590	130	164664	8.954	ppbv	96
39) 1,2-Dichloropropane	4.354	63	149260	9.299	ppbv	97
40) 1,4-Dioxane	4.625	88	68773	8.072	ppbv #	95
41) Tetrahydrofuran	3.082	42	173776	9.361	ppbv	95
42) Bromodichloromethane	4.532	83	327497	9.414	ppbv	99
43) Methyl Methacrylate	4.930	69	151531	8.121	ppbv	98
44) 2,2,4-Trimethylpentane	4.680	57	707832	9.503	ppbv	98
45) t-1,3-Dichloropropene	6.470	75	143714	7.179	ppbv	91

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
 Data File : VL042328.D
 Acq On : 15 Apr 2025 12:54
 Operator : SY/MD
 Sample : VL0415ABS01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0415ABS01

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/16/2025
 Supervised By :Mahesh Dadoda 04/16/2025

Quant Time: Apr 16 01:30:27 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Mar 28 02:00:52 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.658	75	192419	7.841	ppbv	96
47) 1,1,2-Trichloroethane	6.635	97	163251	9.621	ppbv	98
48) Dibromochloromethane	7.428	129	266192	9.256	ppbv	100
49) Bromoform	9.519	173	236686	9.168	ppbv	99
50) 4-Methyl-2-Pentanone	5.807	43	429988	8.416	ppbv	95
51) 2-Hexanone	7.480	43	344172	8.203	ppbv #	96
52) Tetrachloroethene	8.263	164	139845	8.000	ppbv	95
53) Toluene	6.978	91	447178	8.559	ppbv	99
54) 1,2-Dibromoethane	7.694	107	214982	9.089	ppbv	98
56) 1,1,1,2-Tetrachloroethane	8.959	131	216770	9.855	ppbv	98
57) Chlorobenzene	8.956	112	369132	9.739	ppbv	95
58) Ethyl Benzene	9.390	91	618669	8.716	ppbv	100
59) m/p-Xylene	9.584	91	1049238m	18.512	ppbv	
60) o-Xylene	9.995	91	517471	9.107	ppbv	96
61) Styrene	9.904	104	229601	8.168	ppbv	97
62) Isopropylbenzene	10.568	105	785673	9.247	ppbv	99
63) 1,1,2,2-Tetrachloroethane	9.995	83	351308	10.176	ppbv	99
64) n-propylbenzene	11.018	120	210294	9.615	ppbv	98
65) tert-Butylbenzene	11.558	119	718948	9.149	ppbv	97
66) Benzyl Chloride	11.642	91	55150	6.614	ppbv	99
67) sec-Butylbenzene	11.795	105	1018861	9.328	ppbv	100
69) p-Isopropyltoluene	11.950	119	863264	9.179	ppbv	99
70) n-Butylbenzene	12.306	91	891883	9.273	ppbv	99
71) 2-Chlorotoluene	10.930	91	590408	8.953	ppbv	99
72) 4-Ethyltoluene	11.150	105	652962	9.230	ppbv	98
73) 1,3,5-Trimethylbenzene	11.231	105	559451	9.055	ppbv	100
74) 1,2,4-Trimethylbenzene	11.565	105	632271	8.883	ppbv	97
75) 1,3-Dichlorobenzene	11.633	146	381882	9.782	ppbv	98
76) 1,4-Dichlorobenzene	11.697	146	383116	9.861	ppbv	98
77) 1,2-Dichlorobenzene	11.973	146	386768	10.175	ppbv	98
78) Hexachloro-1,3-Butadiene	13.905	225	314860	8.138	ppbv	100
79) Naphthalene	13.539	128	777722	9.989	ppbv	99
80) Naphthalene,2-methyl-	14.481	142	375541	9.836	ppbv	98
81) 1,2,4-Trichlorobenzene	13.465	180	343011	9.551	ppbv	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Manual Integrations APPROVED

Quant Time: Apr 16 01:30:27 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug
QLast Update : Fri Mar 28 02:00:52 2025
Response via : Initial Calibration



Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
 Data File : VL042330.D
 Acq On : 15 Apr 2025 13:57
 Operator : SY/MD
 Sample : QC041425 CAN 10401
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC041425 CAN 10401

Quant Time: Apr 16 01:31:42 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Mar 28 02:00:52 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.813	49	162884	10.000	ppbv	0.03
33) 1,4-Difluorobenzene	3.997	114	405181	10.000	ppbv	0.05
55) Chlorobenzene-d5	8.917	117	353699	10.000	ppbv	0.04

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.406	95	273327	9.410	ppbv	0.04
Spiked Amount	10.000	Range	65 - 135	Recovery	=	94.100%

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
Data File : VL042330.D
Acq On : 15 Apr 2025 13:57
Operator : SY/MD
Sample : QC041425 CAN 10401
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC041425 CAN 10401

Quant Time: Apr 16 01:31:42 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Fri Mar 28 02:00:52 2025
Response via : Initial Calibration

