

**DATA PACKAGE  
GC SEMI-VOLATILES**

**PROJECT NAME : RAYMARK SUPERFUND SITE**

**NOBIS GROUP**

**585 Middlesex Street**

**Lowell, MA - 01851**

**Phone No: 978-683-0891**

**ORDER ID : Q1883**

**ATTENTION : Adam Roy**



**Laboratory Certification ID # 20012**

Q1883-Herbicide Group1



**1 of 574**

1) HERBICIDE GROUP1 Data	2	
2) Signature Page	4	
3) Case Narrative	5	
4) Qualifier Page	7	
5) Conformance/Non Conformance	8	
6) QA Checklist	10	
7) Chronicle	11	
8) Hit Summary	13	
9) QC Data Summary For Herbicide Group1	14	
9.1) Deuterated Monitoring Compound Summary	15	
9.2) MS/MSD Summary	16	
9.3) LCS/LCSD Summary	18	
9.4) Method Blank Summary	19	
10) Sample Data	20	
10.1) OU4-PCS-TC-27-042325	21	
10.2) OU4-PCS-TC-28-042325	25	
10.3) OU4-PCS-TC-29-042325	29	
10.4) OU4-PCS-TC-30-042325	33	
10.5) OU4-PCS-TC-31-042325	37	
10.6) OU4-PCS-TC-32-042325	41	
10.7) OU4-VSL-18-042325	45	
10.8) OU4-VSL-19-042325	49	
11) Calibration Data Summary	53	
11.1) Initial Calibration Data	54	
11.1.1) PS042325	54	
11.2) Continued Calibration Data	118	
11.2.1) PS029991.D	118	
11.2.2) PS030002.D	132	
11.2.3) PS030013.D	146	
11.2.4) PS030016.D	160	
11.2.5) PS030026.D	174	
11.2.6) PS030029.D	188	
11.2.7) PS030041.D	202	
11.3) Analytical Seq	216	
12) Compound Detection Summary	218	



## Table Of Contents for Q1883

13) QC Sample Data	221
13.1) Method Blank Data	222
13.2) PIBLK Data	226
13.3) LCS Data	258
13.4) MS Data	269
13.5) MSD Data	280
14) Manual Integration	291
15) Analytical Runlogs	298
16) Percent Solid	313
17) Extraction Logs	319
17.1) PB167796.pdf	319
17.2) PB167796IC.pdf	321
18) Standard Prep Logs	322
19) Shipping Document	370
19.1) Chain Of Custody	371
19.2) Lab Certificate	372
19.3) Internal COC	373
20) Not Reviewed Data	375

## Cover Page

**Order ID :** Q1883

**Project ID :** Raymark Superfund Site

**Client :** Nobis Group

### Lab Sample Number

Q1883-01  
Q1883-02  
Q1883-03  
Q1883-04  
Q1883-05  
Q1883-06  
Q1883-07  
Q1883-08  
Q1883-09  
Q1883-10  
Q1883-11  
Q1883-12  
Q1883-13  
Q1883-14  
Q1883-15  
Q1883-16  
Q1883-17

### Client Sample Number

OU4-PCS-TC-27-042325  
OU4-PCS-TC-27-042325  
OU4-PCS-TC-28-042325  
OU4-PCS-TC-28-042325  
OU4-PCS-TC-29-042325  
OU4-PCS-TC-29-042325  
OU4-PCS-TC-30-042325  
OU4-PCS-TC-30-042325  
OU4-PCS-TC-31-042325  
OU4-PCS-TC-31-042325  
OU4-PCS-TC-32-042325  
OU4-PCS-TC-32-042325  
OU4-VSL-18-042325  
OU4-VSL-18-042325  
OU4-VSL-19-042325  
OU4-VSL-19-042325  
SO-TB-01-042325

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hard copy data package has been authorized by the laboratory manager or his designee, as verified by the following signature.

**APPROVED**

Signature :

*By Nimisha Pandya, QA/QC Supervisor at 9:33 am, May 09, 2025*

Date: 5/7/2025

NYDOH CERTIFICATION NO - 11376

NJDEP CERTIFICATION NO - 20012

## CASE NARRATIVE

**Nobis Group**

**Project Name:** Raymark Superfund Site

**Project # N/A**

**Order ID # Q1883**

**Test Name:** Herbicide Group1

### **A. Number of Samples and Date of Receipt:**

17 Solid samples were received on 04/25/2025.

### **B. Parameters**

According to the Chain of Custody document, the following analyses were requested: Cyanide, Herbicide Group1, Mercury, Metals ICP-TAL, METALS-TAL, PCB, Pesticide-TCL, SPLP Extraction, SPLP Mercury, SPLP MetalGroup3, SVOCMS Group3, VOCMS Group1 and VOCMS Group3. This data package contains results for Herbicide Group1.

### **C. Analytical Techniques:**

The analysis was performed on instrument ECD\_S. The front column is RTX-CLPesticides which is 30 meters, 0.32 mm ID, 0.5 um df,: Catalog #: 11139. The rear column is RTX-CLPesticides2 which is 30 meters, 0.32 mm ID, 0.25 um df, Catalog #: 11324The analysis of Herbicide Group1s was based on method 8151A and extraction was done based on method 3541.

### **D. QA/ QC Samples:**

The Holding Times were met for all analysis.

The Surrogate recoveries met the acceptable criteria except for WC-5MS [2,4-DCAA(1) - 191%, 2,4-DCAA(2) - 303%], WC-5MSD [2,4-DCAA(1) - 194%, 2 and4-DCAA(2) - 308%]MS and MSD surrogate failure confirmed with parent sample.

The Retention Times were acceptable for all samples.

The MS {Q1906-05MS} with File ID: PS029999.D recoveries met the requirements for all compounds except for Dalapon[196%], Dinoseb[0%] Due to matrix interference..

The MSD {Q1906-05MSD} with File ID: PS030000.D recoveries met the acceptable requirements except for Dalapon[193%], Dinoseb[0%] Due to matrix interference.

The RPD met criteria .

The Blank Spike met requirements for all samples .

The Blank analysis did not indicate the presence of lab contamination.

The Initial Calibration met the requirements .

The Continuous Calibration met the requirements .



284 Sheffield Street, Mountainside, NJ 07092  
Phone: 908 789 8900 Fax: 908 789 8922

#### **E. Additional Comments:**

As per special requirement for this project form-1 are reported in mg/kg.  
The not QT review data is reported in the Miscellaneous.  
The soil samples results are based on a dry weight basis.

#### **F. Manual Integration Comments:**

Please refer to the Manual integration Report included with the Run Logs for information on the manual integrations performed.

---

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. The laboratory manager or his designee, as verified by the following signature has authorized release of the data contained in this hard copy data package.

**APPROVED**

Signature \_\_\_\_\_

*By Nimisha Pandya, QA/QC Supervisor at 9:34 am, May 09, 2025*

**DATA REPORTING QUALIFIERS- ORGANIC**

For reporting results, the following "Results Qualifiers" are used:

- Value If the result is a value greater than or equal to the detection limit, report the value
- U** Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. "10 U". This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
- ND** Indicates the analyte was analyzed for, but not detected
- J** Indicates an estimated value. This flag is used:  
(1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.)  
(2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
- B** Indicates the analyte was found in the blank as well as the sample report as "12 B".
- E** Indicates the analyte's concentration exceeds the calibrated range of the instrument for that specific analysis.
- D** This flag identifies all compounds identified in an analysis at a secondary dilution factor.
- P** This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a "P".
- N** This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
- A** This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
- Q** Indicates the LCS did not meet the control limits requirements



284 Sheffield Street, Mountainside, NJ 07092 Phone: 908 789 8900 Fax: 908 789 8922

**GC ANALYSIS CONFORMANCE/NON-CONFORMANCE SUMMARY**

ORDER ID: Q1883

MATRIX: Solid

METHOD: 8151A/3541

	NA	NO	YES
1. Chromatograms Labeled/Compounds Identified.			✓
2. Standard Summary Submitted.			✓
3. Calibration - Initial Calibration performed within 30 days before sample analysis and continuing calibration performed within 24 hours of sample analysis, 12 HOURS IF 8000 SERIES METHOD.			✓
The Initial Calibration met the requirements . The Continuous Calibration met the requirements .			
4. Blank Contamination - If yes, list compounds and concentrations in each blank:			✓
5. Surrogate Recoveries Meet Criteria			✓
If not met, list those compounds and their recoveries which fall outside the acceptable ranges.			
The Surrogate recoveries met the acceptable criteria except for WC-5MS [2,4-DCAA(1) - 191%, 2,4-DCAA(2) - 303%], WC-5MSD [2,4-DCAA(1) - 194%, 2 and 4-DCAA(2) - 308%]MS and MSD surrogate failure confirmed with parent sample.			
6. Matrix Spike/Matrix Spike Duplicate Recoveries Meet Criteria			✓
If not met, list those compounds and their recoveries which fall outside the acceptable range.			
The MS {Q1906-05MS} with File ID: PS029999.D recoveries met the requirements for all compounds except for Dalapon[196%], Dinoseb[0%] Due to matrix interference..			
The MSD {Q1906-05MSD} with File ID: PS030000.D recoveries met the acceptable requirements except for Dalapon[193%], Dinoseb[0%] Due to matrix interference.			
The Blank Spike met requirements for all samples . The RPD met criteria .			
7. Retention Time Shift Meet Criteria (if applicable)			✓
Comments:			
8. Extraction Holding Time Met			✓
If not met, list number of days exceeded for each sample:			



284 Sheffield Street, Mountainside, NJ 07092 Phone: 908 789 8900 Fax: 908 789 8922

**GC ANALYSIS CONFORMANCE/NON-CONFORMANCE SUMMARY (CONTINUED)**

NA      NO      YES

9. Analysis Holding Time Met ✓

If not met, list those compounds and their recoveries which fall outside the acceptable range.

**ADDITIONAL COMMENTS:**

As per special requirement for this project form-1 are reported in mg/kg.

The not QT review data is reported in the Miscellaneous.

The soil samples results are based on a dry weight basis.

**REVIEWED**

QA REVIEW

*By Sohil Jodhani, QA/QC Director at 9:00 am, May 09, 2025*

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

## APPENDIX A

### QA REVIEW GENERAL DOCUMENTATION

Project #: Q1883

Completed

For thorough review, the report must have the following:

#### GENERAL:

Are all original paperwork present (chain of custody, record of communication, airbill, sample management lab chronicle, login page)

✓

Check chain-of-custody for proper relinquish/return of samples

✓

Is the chain of custody signed and complete

✓

Check internal chain-of-custody for proper relinquish/return of samples /sample extracts

✓

Collect information for each project id from server. Were all requirements followed

✓

#### COVER PAGE:

Do numbers of samples correspond to the number of samples in the Chain of Custody on login page

✓

Do lab numbers and client Ids on cover page agree with the Chain of Custody

✓

#### CHAIN OF CUSTODY:

Do requested analyses on Chain of Custody agree with form I results

✓

Do requested analyses on Chain of Custody agree with the log-in page

✓

Were the correct method log-in for analysis according to the Analytical Request and Chain of Castody

✓

Were the samples received within hold time

✓

Were any problems found with the samples at arrival recorded in the Sample Management Laboratory Chronicle

✓

#### ANALYTICAL:

Was method requirement followed?

✓

Was client requirement followed?

✓

Does the case narrative summarize all QC failure?

✓

All runlogs and manual integration are reviewed for requirements

✓

All manual calculations and /or hand notations verified

✓

QA Review Signature: SOHIL JODHANI

Date: 05/07/2025

## LAB CHRONICLE

<b>OrderID:</b>	Q1883	<b>OrderDate:</b>	4/25/2025 10:10:00 AM					
<b>Client:</b>	Nobis Group	<b>Project:</b>	Raymark Superfund Site					
<b>Contact:</b>	Adam Roy	<b>Location:</b>	L41,L51,VOA Ref. #2 Soil, VOA Ref. #3 Water					
LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
<b>Q1883-01</b>	<b>OU4-PCS-TC-27-0423 25</b>	<b>SOIL</b>			<b>04/23/25</b>			<b>04/25/25</b>
			Herbicide Group1	8151A		04/30/25	05/01/25	
			PCB	8082A		04/29/25	04/29/25	
			Pesticide-TCL	8081B		04/28/25	04/29/25	
<b>Q1883-03</b>	<b>OU4-PCS-TC-28-0423 25</b>	<b>SOIL</b>			<b>04/23/25</b>			<b>04/25/25</b>
			Herbicide Group1	8151A		04/30/25	05/01/25	
			PCB	8082A		04/29/25	04/29/25	
			Pesticide-TCL	8081B		04/28/25	04/29/25	
<b>Q1883-05</b>	<b>OU4-PCS-TC-29-0423 25</b>	<b>SOIL</b>			<b>04/23/25</b>			<b>04/25/25</b>
			Herbicide Group1	8151A		04/30/25	05/01/25	
			PCB	8082A		04/29/25	04/29/25	
			Pesticide-TCL	8081B		04/28/25	04/29/25	
<b>Q1883-07</b>	<b>OU4-PCS-TC-30-0423 25</b>	<b>SOIL</b>			<b>04/23/25</b>			<b>04/25/25</b>
			Herbicide Group1	8151A		04/30/25	05/01/25	
			PCB	8082A		04/29/25	04/29/25	
			Pesticide-TCL	8081B		04/28/25	04/29/25	
<b>Q1883-09</b>	<b>OU4-PCS-TC-31-0423 25</b>	<b>SOIL</b>			<b>04/23/25</b>			<b>04/25/25</b>
			Herbicide Group1	8151A		04/30/25	05/01/25	
			PCB	8082A		04/29/25	04/29/25	
			Pesticide-TCL	8081B		04/28/25	04/29/25	
<b>Q1883-11</b>	<b>OU4-PCS-TC-32-0423 25</b>	<b>SOIL</b>			<b>04/23/25</b>			<b>04/25/25</b>
			Herbicide Group1	8151A		04/30/25	05/01/25	

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

## LAB CHRONICLE

<b>Q1883-13</b>	<b>OU4-VSL-18-042325</b>	<b>SOIL</b>	PCB	8082A	04/29/25	04/29/25
			Pesticide-TCL	8081B	04/28/25	04/29/25
					<b>04/23/25</b>	<b>04/25/25</b>
			Herbicide Group1	8151A	04/30/25	05/01/25
<b>Q1883-15</b>	<b>OU4-VSL-19-042325</b>	<b>SOIL</b>	PCB	8082A	04/29/25	04/29/25
			Pesticide-TCL	8081B	04/28/25	04/29/25
					<b>04/23/25</b>	<b>04/25/25</b>
			Herbicide Group1	8151A	04/30/25	05/01/25
			PCB	8082A	04/29/25	04/29/25
			Pesticide-TCL	8081B	04/28/25	04/29/25

### Hit Summary Sheet SW-846

SDG No.: Q1883

Order ID: Q1883

Client: Nobis Group

Project ID: Raymark Superfund Site

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	LOD	RDL	Units
-----------	-----------	--------	-----------	---------------	---	-----	-----	-----	-------

Client ID :

Total Concentration: 0.000

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20



# QC SUMMARY

### Surrogate Summary

**SDG No.:** Q1883

**Client:** Nobis Group

**Analytical Method:** 8151A

Lab Sample ID	Client ID	Parameter	Limits						
			Column	Spike	Result	Rec	Qual	Low	High
I.BLK-PS029918.D	PIBLK-PS029918.D	2,4-DCAA	1	500	433	87	*	32	138
		2,4-DCAA	2	500	433	87	*	32	138
I.BLK-PS029990.D	PIBLK-PS029990.D	2,4-DCAA	1	500	525	105	*	32	138
		2,4-DCAA	2	500	558	112	*	32	138
Q1906-05MS	WC-5MS	2,4-DCAA	1	500	956	191	*	27	122
		2,4-DCAA	2	500	1520	303	*	27	122
Q1906-05MSD	WC-5MSD	2,4-DCAA	1	500	969	194	*	27	122
		2,4-DCAA	2	500	1540	308	*	27	122
I.BLK-PS030001.D	PIBLK-PS030001.D	2,4-DCAA	1	500	518	104	*	32	138
		2,4-DCAA	2	500	565	113	*	32	138
PB167796BL	PB167796BL	2,4-DCAA	1	500	433	87	*	27	122
		2,4-DCAA	2	500	413	83	*	27	122
I.BLK-PS030012.D	PIBLK-PS030012.D	2,4-DCAA	1	500	551	110	*	32	138
		2,4-DCAA	2	500	588	118	*	32	138
I.BLK-PS030015.D	PIBLK-PS030015.D	2,4-DCAA	1	500	534	107	*	32	138
		2,4-DCAA	2	500	567	113	*	32	138
Q1883-01	OU4-PCS-TC-27-042325	2,4-DCAA	1	500	412	82	*	27	122
		2,4-DCAA	2	500	400	80	*	27	122
Q1883-03	OU4-PCS-TC-28-042325	2,4-DCAA	1	500	338	68	*	27	122
		2,4-DCAA	2	500	337	67	*	27	122
Q1883-05	OU4-PCS-TC-29-042325	2,4-DCAA	1	500	138	28	*	27	122
		2,4-DCAA	2	500	135	27	*	27	122
Q1883-07	OU4-PCS-TC-30-042325	2,4-DCAA	1	500	371	74	*	27	122
		2,4-DCAA	2	500	350	70	*	27	122
Q1883-09	OU4-PCS-TC-31-042325	2,4-DCAA	1	500	390	78	*	27	122
		2,4-DCAA	2	500	380	76	*	27	122
Q1883-11	OU4-PCS-TC-32-042325	2,4-DCAA	1	500	327	65	*	27	122
		2,4-DCAA	2	500	318	64	*	27	122
Q1883-13	OU4-VSL-18-042325	2,4-DCAA	1	500	365	73	*	27	122
		2,4-DCAA	2	500	345	69	*	27	122
Q1883-15	OU4-VSL-19-042325	2,4-DCAA	1	500	401	80	*	27	122
		2,4-DCAA	2	500	409	82	*	27	122
I.BLK-PS030025.D	PIBLK-PS030025.D	2,4-DCAA	1	500	562	112	*	32	138
		2,4-DCAA	2	500	598	120	*	32	138
I.BLK-PS030028.D	PIBLK-PS030028.D	2,4-DCAA	1	500	530	106	*	32	138
		2,4-DCAA	2	500	553	111	*	32	138
PB167796BS	PB167796BS	2,4-DCAA	1	500	530	106	*	27	122
		2,4-DCAA	2	500	540	108	*	27	122
I.BLK-PS030040.D	PIBLK-PS030040.D	2,4-DCAA	1	500	529	106	*	32	138
		2,4-DCAA	2	500	552	110	*	32	138

### Matrix Spike/Matrix Spike Duplicate Summary

**SW-846**

**SDG No.:** Q1883

**Client:** Nobis Group

**Analytical Method:** 8151A

**DataFile :** PS029999.D

<b>Lab Sample ID:</b>	<b>Parameter</b>	<b>Spike</b>	<b>Sample</b>			<b>Rec</b>	<b>Rec Qual</b>	<b>RPD</b>	<b>RPD Qual</b>	<b>Limits</b>		
			<b>Result</b>	<b>Result</b>	<b>Units</b>					<b>Low</b>	<b>High</b>	<b>RPD</b>
<b>Client Sample ID:</b> WC-5MS												
Q1906-05MS	DICAMBA	199.2	0	131	ug/Kg	66				38	132	
	Dalapon	199.2	0	391	ug/Kg	196	*			70	130	
	DICHLORPROP	199.2	0	135	ug/Kg	68				28	155	
	2,4-D	199.2	0	165	ug/Kg	83				28	144	
	2,4,5-TP(Silvex)	199.2	0	96.8	ug/Kg	49				43	129	
	2,4,5-T	199.2	0	111	ug/Kg	56				31	138	
	2,4-DB	199.2	0	81.8	ug/Kg	41				34	142	
	Dinoseb	199.2	0	0	ug/Kg	0	*			57	152	

### Matrix Spike/Matrix Spike Duplicate Summary

**SW-846**

**SDG No.:** Q1883

**Client:** Nobis Group

**Analytical Method:** 8151A

**DataFile :** PS030000.D

<b>Lab Sample ID:</b>	<b>Parameter</b>	Sample			<b>Rec</b>	<b>RPD</b>	<b>Limits</b>	
		<b>Spike</b>	<b>Result</b>	<b>Units</b>			<b>Low</b>	<b>High</b>
<b>Client Sample ID:</b> WC-5MSD	<b>WC-5MSD</b>							
Q1906-05MSD	DICAMBA	199.3	0	133	ug/Kg	67	2	38
	Dalapon	199.3	0	384	ug/Kg	193	*	70
	DICHLORPROP	199.3	0	137	ug/Kg	69	1	28
	2,4-D	199.3	0	168	ug/Kg	84	1	28
	2,4,5-TP(Silvex)	199.3	0	100	ug/Kg	50	2	43
	2,4,5-T	199.3	0	113	ug/Kg	57	2	31
	2,4-DB	199.3	0	84.5	ug/Kg	42	2	34
	Dinoseb	199.3	0	0	ug/Kg	0	*	57
						0		152
								20

### Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: Q1883

Client: Nobis Group

Analytical Method: 8151A

Datafile : PS030038.D

Lab Sample ID	Parameter	Spike	Result	Units	Rec	RPD	Qual	RPD	Low	High	RPD
PB167796BS	DICAMBA	166.6	172	ug/Kg	103				38	132	
	Dalapon	166.6	165	ug/Kg	99				70	130	
	DICHLORPROP	166.6	172	ug/Kg	103				28	155	
	2,4-D	166.6	170	ug/Kg	102				28	144	
	2,4,5-TP(Silvex)	166.6	175	ug/Kg	105				43	129	
	2,4,5-T	166.6	173	ug/Kg	104				31	138	
	2,4-DB	166.6	172	ug/Kg	103				34	142	
	Dinoseb	166.6	170	ug/Kg	102				57	152	

4C

PESTICIDE METHOD BLANK SUMMARY

EPA SAMPLE NO.

PB167796BL

Lab Name: CHEMTECH

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883

SAS No.: Q1883 SDG NO.: Q1883

Lab Sample ID: PB167796BL

Lab File ID: PS030011.D

Matrix: (soil/water) Solid

Extraction: (Type) SOXH

Sulfur Cleanup: (Y/N) N

Date Extracted: 04/30/2025

Date Analyzed (1): 05/01/2025

Date Analyzed (2): 05/01/2025

Time Analyzed (1): 11:24

Time Analyzed (2): 11:24

Instrument ID (1): ECD\_S

Instrument ID (2): ECD\_S

GC Column (1): RTX-CLP

ID: 0.32 (mm)

GC Column (2): RTX-CLP2

ID: 0.32 (mm)

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED 1	DATE ANALYZED 2
WC-5MS	Q1906-05MS	PS029999.D	05/01/2025	05/01/2025
WC-5MSD	Q1906-05MSD	PS030000.D	05/01/2025	05/01/2025
OU4-PCS-TC-27-042325	Q1883-01	PS030017.D	05/01/2025	05/01/2025
OU4-PCS-TC-28-042325	Q1883-03	PS030018.D	05/01/2025	05/01/2025
OU4-PCS-TC-29-042325	Q1883-05	PS030019.D	05/01/2025	05/01/2025
OU4-PCS-TC-30-042325	Q1883-07	PS030020.D	05/01/2025	05/01/2025
OU4-PCS-TC-31-042325	Q1883-09	PS030021.D	05/01/2025	05/01/2025
OU4-PCS-TC-32-042325	Q1883-11	PS030022.D	05/01/2025	05/01/2025
OU4-VSL-18-042325	Q1883-13	PS030023.D	05/01/2025	05/01/2025
OU4-VSL-19-042325	Q1883-15	PS030024.D	05/01/2025	05/01/2025
PB167796BS	PB167796BS	PS030038.D	05/05/2025	05/05/2025

COMMENTS:



# SAMPLE

# DATA



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/23/25	
Project:	Raymark Superfund Site			Date Received:	04/25/25	
Client Sample ID:	OU4-PCS-TC-27-042325			SDG No.:	Q1883	
Lab Sample ID:	Q1883-01			Matrix:	SOIL	
Analytical Method:	SW8151A			% Solid:	94.5	Decanted:
Sample Wt/Vol:	30.01	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	Herbicide Group1	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	8151A					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PS030017.D	1	04/30/25 08:50	05/01/25 13:51	PB167796

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
1918-00-9	DICAMBA	0.035	U	0.0082	0.035	0.071	mg/Kg
75-99-0	DALAPON	0.053	U	0.019	0.053	0.071	mg/Kg
120-36-5	DICHLORPROP	0.035	U	0.014	0.035	0.071	mg/Kg
94-75-7	2,4-D	0.035	U	0.0096	0.035	0.071	mg/Kg
93-72-1	2,4,5-TP (Silvex)	0.035	U	0.0096	0.035	0.071	mg/Kg
93-76-5	2,4,5-T	0.035	U	0.0092	0.035	0.071	mg/Kg
94-82-6	2,4-DB	0.035	U	0.026	0.035	0.071	mg/Kg
88-85-7	DINOSEB	0.035	U	0.011	0.035	0.071	mg/Kg
<b>SURROGATES</b>							
19719-28-9	2,4-DCAA	412		27 - 122		82%	SPK: 500

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030017.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 13:51  
 Operator : AR\AJ  
 Sample : Q1883-01  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

**Instrument :**  
 ECD\_S  
**ClientSampleId :**  
 OU4-PCS-TC-27-042325

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:28:26 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.937 7.461 1013.4E6 281.8E6 411.762m 399.933m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030017.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 13:51  
 Operator : AR\AJ  
 Sample : Q1883-01  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1


Instrument :  
 ECD\_S  
 ClientSampleId :  
 OU4-PCS-TC-27-042325


**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:28:26 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

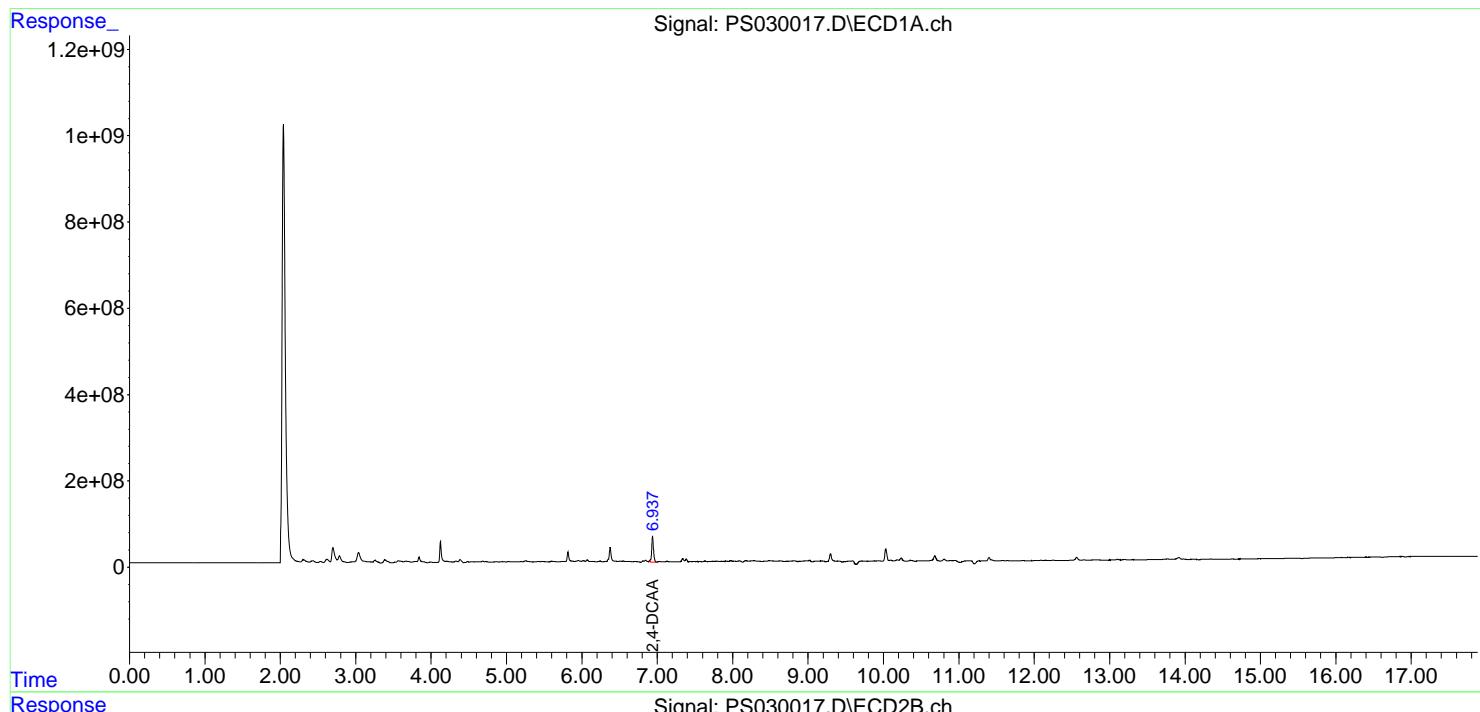

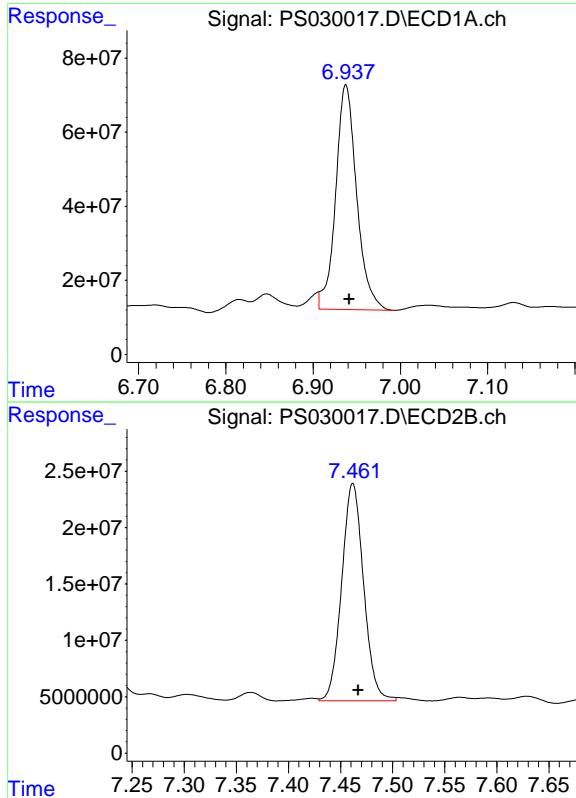

#4 2,4-DCAA

R.T.: 6.937 min  
 Delta R.T.: -0.004 min  
 Response: 1013379759 ECD\_S  
 Conc: 411.76 ng/ml ClientSampleId : OU4-PCS-TC-27-042325

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

#4 2,4-DCAA

R.T.: 7.461 min  
 Delta R.T.: -0.006 min  
 Response: 281759390  
 Conc: 399.93 ng/ml

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14
- 15
- 16
- 17
- 18
- 19
- 20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/23/25	
Project:	Raymark Superfund Site			Date Received:	04/25/25	
Client Sample ID:	OU4-PCS-TC-28-042325			SDG No.:	Q1883	
Lab Sample ID:	Q1883-03			Matrix:	SOIL	
Analytical Method:	SW8151A			% Solid:	94.5	Decanted:
Sample Wt/Vol:	30.06	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	Herbicide Group1	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	8151A					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PS030018.D	1	04/30/25 08:50	05/01/25 14:15	PB167796

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
1918-00-9	DICAMBA	0.035	U	0.0082	0.035	0.071	mg/Kg
75-99-0	DALAPON	0.053	U	0.019	0.053	0.071	mg/Kg
120-36-5	DICHLORPROP	0.035	U	0.014	0.035	0.071	mg/Kg
94-75-7	2,4-D	0.035	U	0.0095	0.035	0.071	mg/Kg
93-72-1	2,4,5-TP (Silvex)	0.035	U	0.0096	0.035	0.071	mg/Kg
93-76-5	2,4,5-T	0.035	U	0.0092	0.035	0.071	mg/Kg
94-82-6	2,4-DB	0.035	U	0.026	0.035	0.071	mg/Kg
88-85-7	DINOSEB	0.035	U	0.011	0.035	0.071	mg/Kg
<b>SURROGATES</b>							
19719-28-9	2,4-DCAA	338		27 - 122		68%	SPK: 500

Comments:

U = Not Detected  
 LOQ = Limit of Quantitation  
 MDL = Method Detection Limit  
 LOD = Limit of Detection  
 E = Value Exceeds Calibration Range  
 P = Indicates >25% difference for detected concentrations between the two GC columns  
 Q = indicates LCS control criteria did not meet requirements  
 M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value  
 B = Analyte Found in Associated Method Blank  
 N = Presumptive Evidence of a Compound  
 \* = Values outside of QC limits  
 D = Dilution  
 S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.  
 () = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030018.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 14:15  
 Operator : AR\AJ  
 Sample : Q1883-03  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

**Instrument :**  
 ECD\_S  
**ClientSampleId :**  
 OU4-PCS-TC-28-042325

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:28:39 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.937 7.461 831.9E6 237.4E6 338.028m 337.021m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030018.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 14:15  
 Operator : AR\AJ  
 Sample : Q1883-03  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1


Instrument :  
 ECD\_S  
 ClientSampleId :  
 OU4-PCS-TC-28-042325


**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:28:39 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

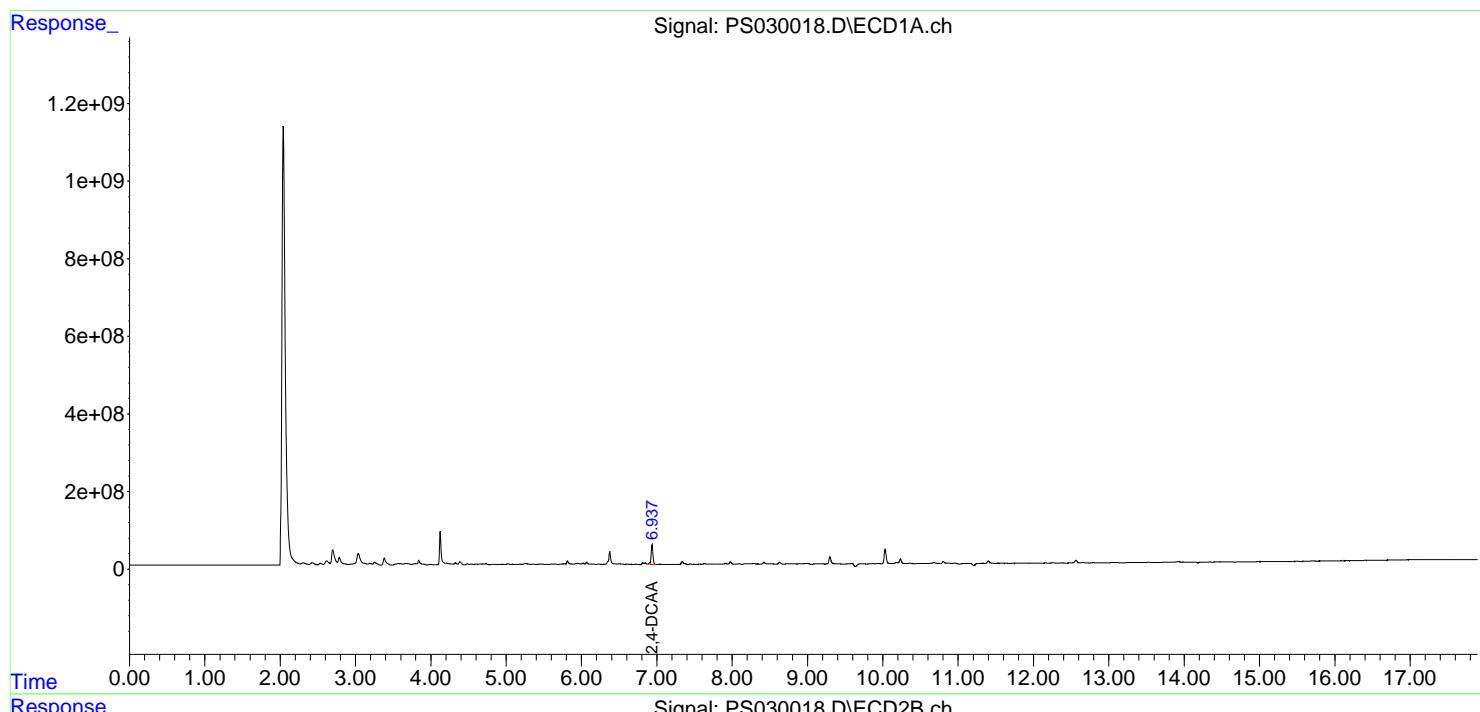

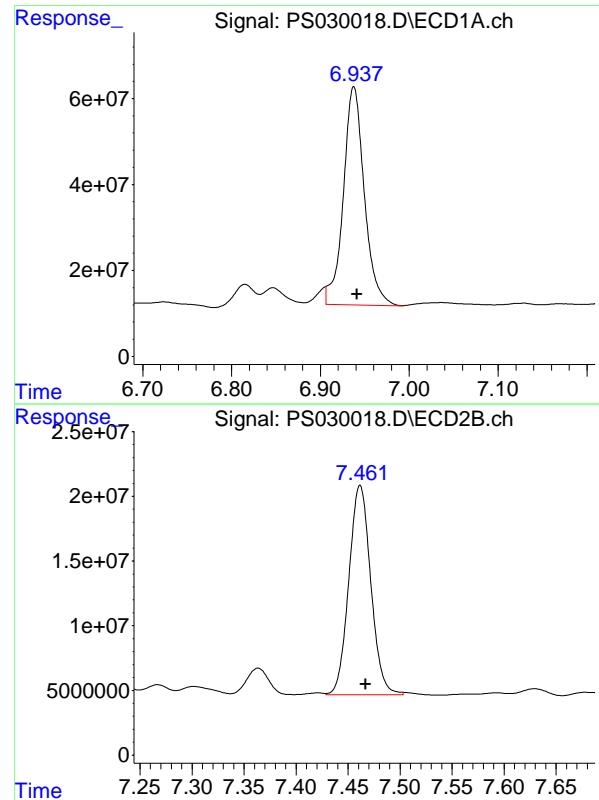

#4 2,4-DCAA

R.T.: 6.937 min  
 Delta R.T.: -0.004 min  
 Response: 831913853 ECD\_S  
 Conc: 338.03 ng/ml ClientSampleId : OU4-PCS-TC-28-042325

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

#4 2,4-DCAA

R.T.: 7.461 min  
 Delta R.T.: -0.006 min  
 Response: 237436771  
 Conc: 337.02 ng/ml

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14
- 15
- 16
- 17
- 18
- 19
- 20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/23/25	
Project:	Raymark Superfund Site			Date Received:	04/25/25	
Client Sample ID:	OU4-PCS-TC-29-042325			SDG No.:	Q1883	
Lab Sample ID:	Q1883-05			Matrix:	SOIL	
Analytical Method:	SW8151A			% Solid:	95.7	Decanted:
Sample Wt/Vol:	30.05	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	Herbicide Group1	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	8151A					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PS030019.D	1	04/30/25 08:50	05/01/25 14:39	PB167796

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
1918-00-9	DICAMBA	0.034	U	0.0081	0.034	0.070	mg/Kg
75-99-0	DALAPON	0.052	U	0.018	0.052	0.070	mg/Kg
120-36-5	DICHLORPROP	0.034	U	0.013	0.034	0.070	mg/Kg
94-75-7	2,4-D	0.034	U	0.0094	0.034	0.070	mg/Kg
93-72-1	2,4,5-TP (Silvex)	0.034	U	0.0095	0.034	0.070	mg/Kg
93-76-5	2,4,5-T	0.034	U	0.0091	0.034	0.070	mg/Kg
94-82-6	2,4-DB	0.034	U	0.025	0.034	0.070	mg/Kg
88-85-7	DINOSEB	0.034	U	0.011	0.034	0.070	mg/Kg
<b>SURROGATES</b>							
19719-28-9	2,4-DCAA	138		27 - 122		28%	SPK: 500

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030019.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 14:39  
 Operator : AR\AJ  
 Sample : Q1883-05  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**OU4-PCS-TC-29-042325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:28:53 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

---

System Monitoring Compounds

4) S	2,4-DCAA	6.938	7.461	340.5E6	95257086	138.335	135.209
------	----------	-------	-------	---------	----------	---------	---------

---

Target Compounds

---


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030019.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 14:39  
 Operator : AR\AJ  
 Sample : Q1883-05  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**OU4-PCS-TC-29-042325**


Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:28:53 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

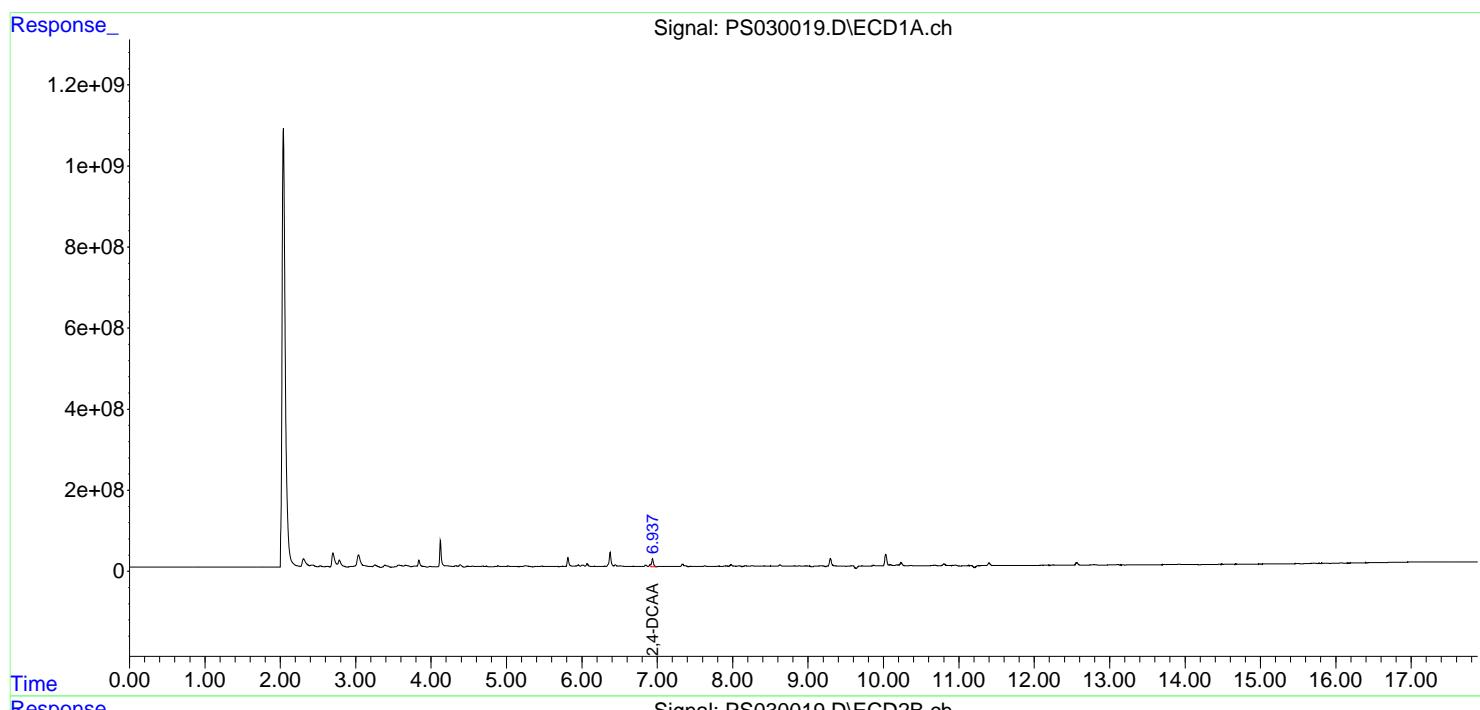


#4 2,4-DCAA

R.T.: 6.938 min  
Delta R.T.: -0.004 min  
Response: 340454069 ECD\_S  
Conc: 138.34 ng/ml ClientSampleId : OU4-PCS-TC-29-042325

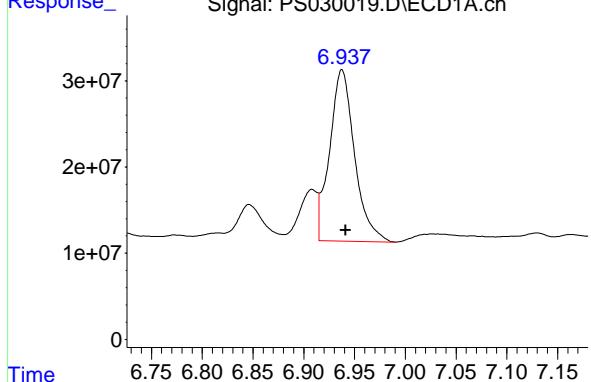

#4 2,4-DCAA

R.T.: 7.461 min  
Delta R.T.: -0.006 min  
Response: 95257086  
Conc: 135.21 ng/ml

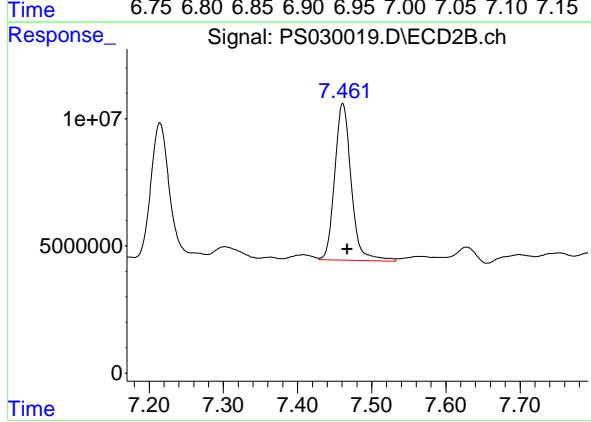



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/23/25	
Project:	Raymark Superfund Site			Date Received:	04/25/25	
Client Sample ID:	OU4-PCS-TC-30-042325			SDG No.:	Q1883	
Lab Sample ID:	Q1883-07			Matrix:	SOIL	
Analytical Method:	SW8151A			% Solid:	96.5	Decanted:
Sample Wt/Vol:	30.03	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	Herbicide Group1	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	8151A					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PS030020.D	1	04/30/25 08:50	05/01/25 15:04	PB167796

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
1918-00-9	DICAMBA	0.034	U	0.0080	0.034	0.069	mg/Kg
75-99-0	DALAPON	0.052	U	0.018	0.052	0.069	mg/Kg
120-36-5	DICHLORPROP	0.034	U	0.013	0.034	0.069	mg/Kg
94-75-7	2,4-D	0.034	U	0.0094	0.034	0.069	mg/Kg
93-72-1	2,4,5-TP (Silvex)	0.034	U	0.0094	0.034	0.069	mg/Kg
93-76-5	2,4,5-T	0.034	U	0.0090	0.034	0.069	mg/Kg
94-82-6	2,4-DB	0.034	U	0.025	0.034	0.069	mg/Kg
88-85-7	DINOSEB	0.034	U	0.011	0.034	0.069	mg/Kg
<b>SURROGATES</b>							
19719-28-9	2,4-DCAA	371		27 - 122		74%	SPK: 500

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030020.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 15:04  
 Operator : AR\AJ  
 Sample : Q1883-07  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

**Instrument :**  
 ECD\_S  
**ClientSampleId :**  
 OU4-PCS-TC-30-042325

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:29:04 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.937 7.461 912.0E6 246.3E6 370.553m 349.662m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030020.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 15:04  
 Operator : AR\AJ  
 Sample : Q1883-07  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1


Instrument :  
 ECD\_S  
 ClientSampleId :  
 OU4-PCS-TC-30-042325


**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:29:04 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

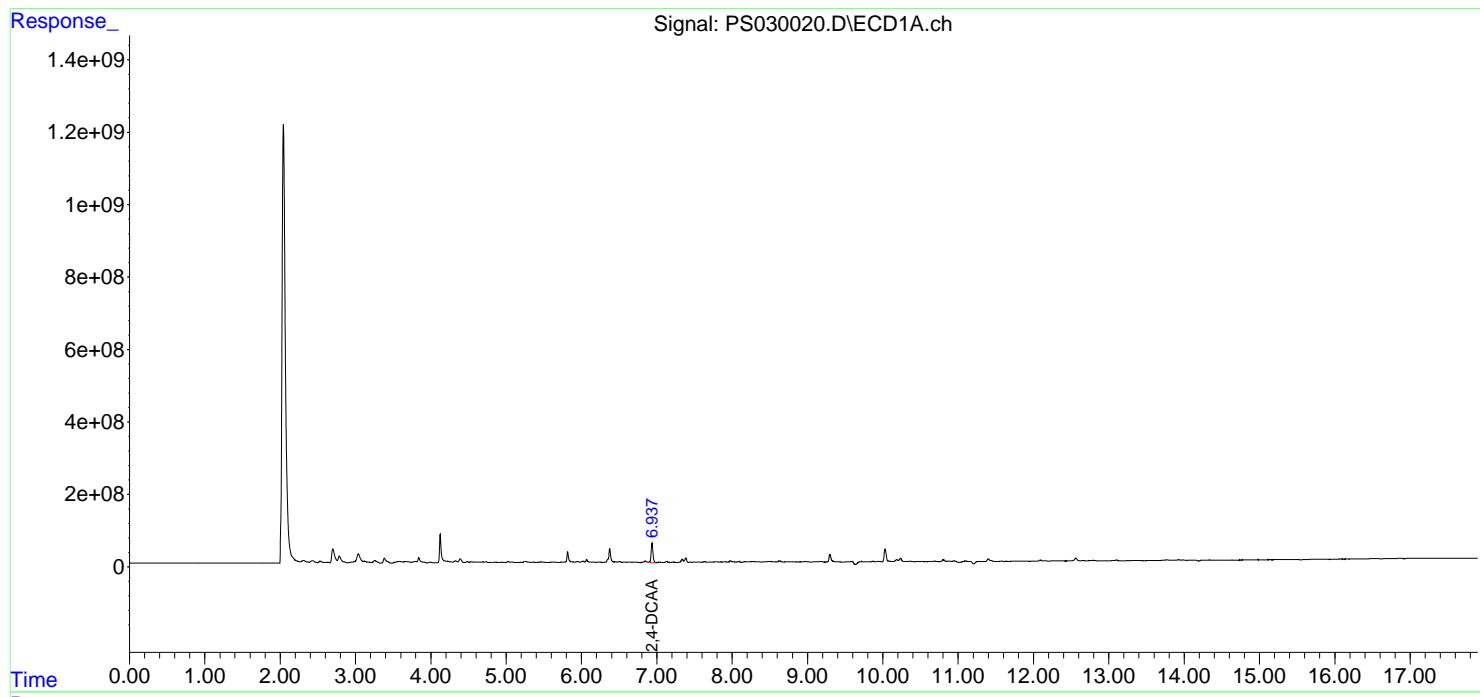

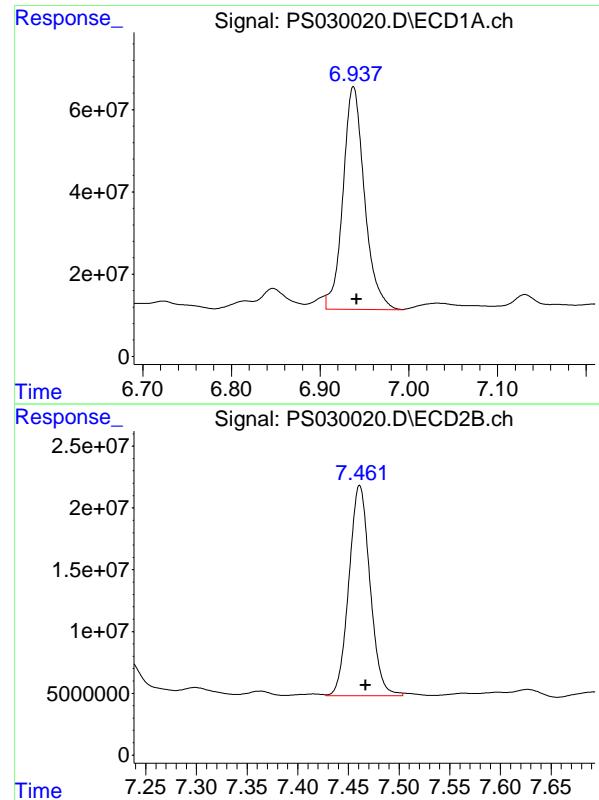

#4 2,4-DCAA

R.T.: 6.937 min  
 Delta R.T.: -0.004 min  
 Response: 911959187 ECD\_S  
 Conc: 370.55 ng/ml ClientSampleId : OU4-PCS-TC-30-042325

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

#4 2,4-DCAA

R.T.: 7.461 min  
 Delta R.T.: -0.006 min  
 Response: 246342602  
 Conc: 349.66 ng/ml

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group		Date Collected:	04/23/25	
Project:	Raymark Superfund Site		Date Received:	04/25/25	
Client Sample ID:	OU4-PCS-TC-31-042325		SDG No.:	Q1883	
Lab Sample ID:	Q1883-09		Matrix:	SOIL	
Analytical Method:	SW8151A		% Solid:	96.9	Decanted:
Sample Wt/Vol:	30.04	Units: g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL		Test:	Herbicide Group1	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	8151A				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PS030021.D	1	04/30/25 08:50	05/01/25 15:28	PB167796

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
1918-00-9	DICAMBA	0.034	U	0.0080	0.034	0.069	mg/Kg
75-99-0	DALAPON	0.052	U	0.018	0.052	0.069	mg/Kg
120-36-5	DICHLORPROP	0.034	U	0.013	0.034	0.069	mg/Kg
94-75-7	2,4-D	0.034	U	0.0093	0.034	0.069	mg/Kg
93-72-1	2,4,5-TP (Silvex)	0.034	U	0.0093	0.034	0.069	mg/Kg
93-76-5	2,4,5-T	0.034	U	0.0090	0.034	0.069	mg/Kg
94-82-6	2,4-DB	0.034	U	0.025	0.034	0.069	mg/Kg
88-85-7	DINOSEB	0.034	U	0.011	0.034	0.069	mg/Kg
<b>SURROGATES</b>							
19719-28-9	2,4-DCAA	390		27 - 122		78%	SPK: 500

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030021.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 15:28  
 Operator : AR\AJ  
 Sample : Q1883-09  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

**Instrument :**  
 ECD\_S  
**ClientSampleId :**  
 OU4-PCS-TC-31-042325

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:29:18 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.937 7.461 960.5E6 267.8E6 390.265m 380.058

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030021.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 15:28  
 Operator : AR\AJ  
 Sample : Q1883-09  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1



Instrument :  
 ECD\_S  
 ClientSampleId :  
 OU4-PCS-TC-31-042325


**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:29:18 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

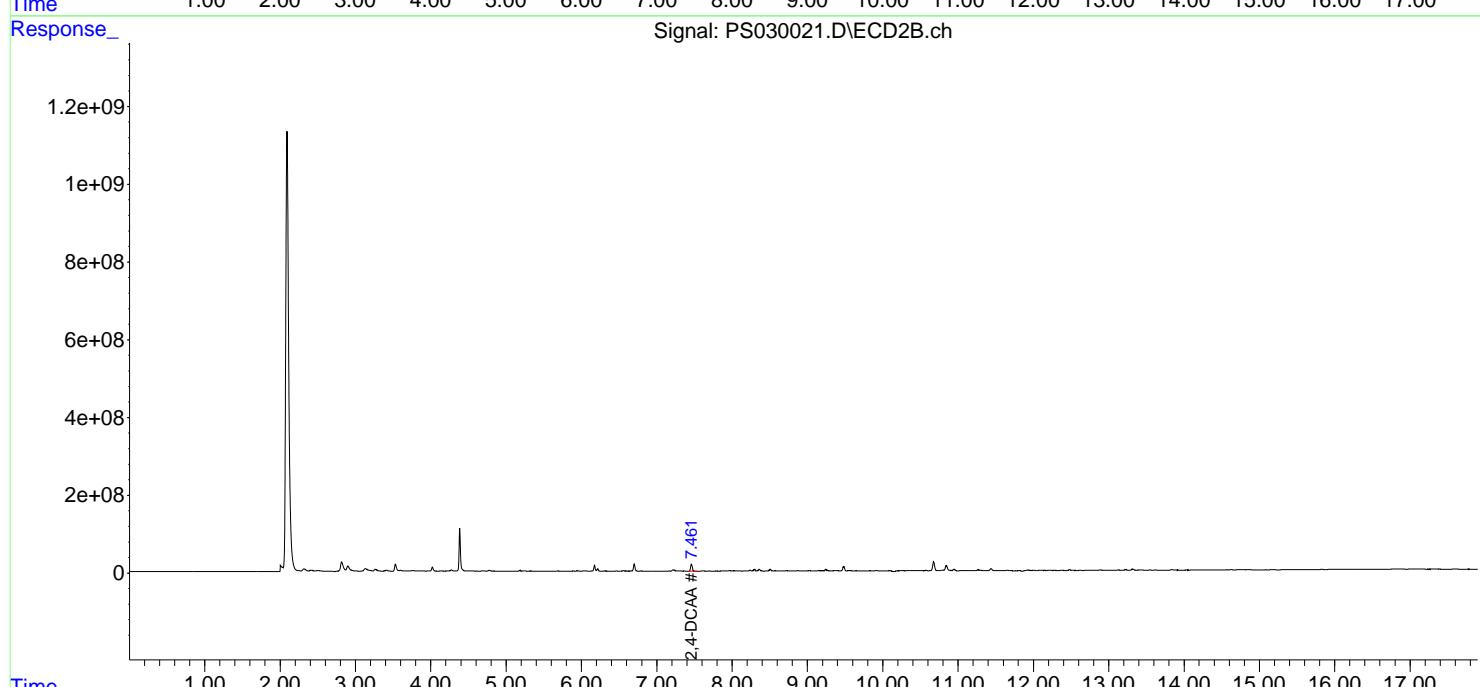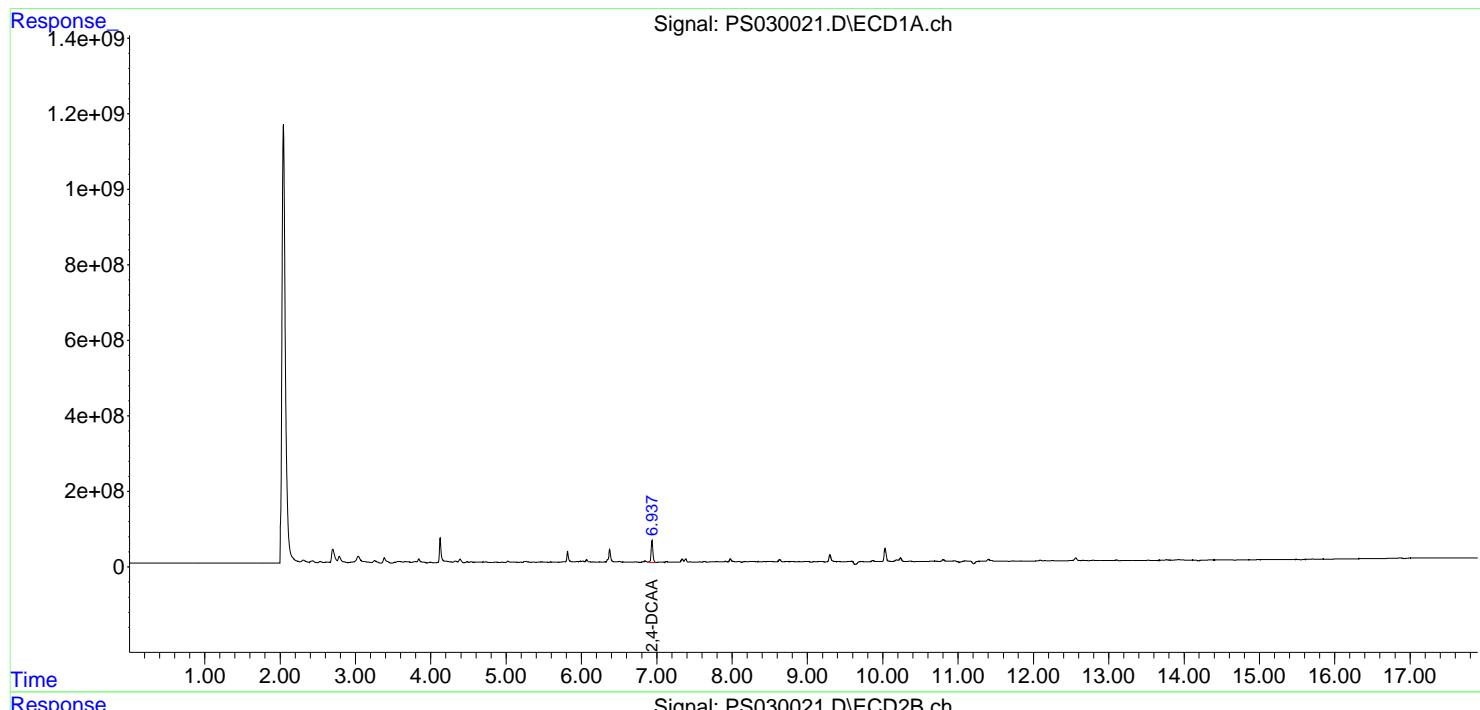

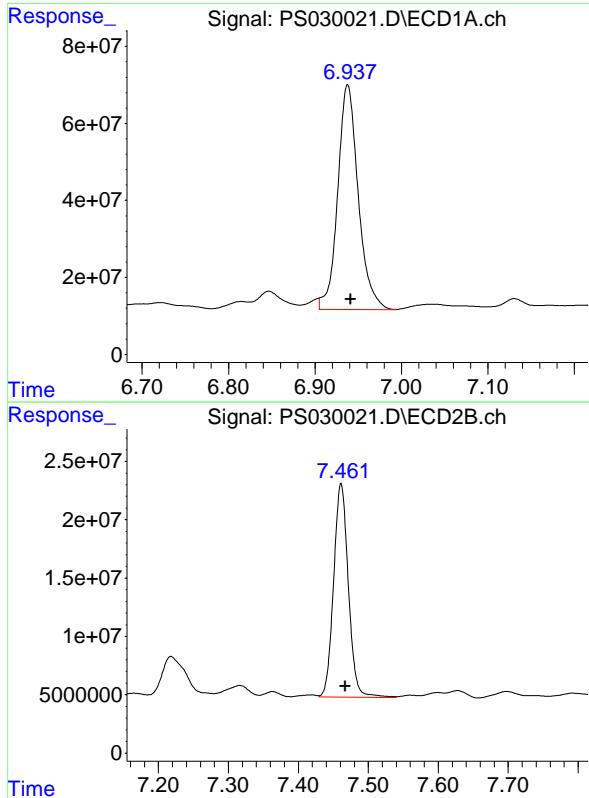

#4 2,4-DCAA

R.T.: 6.937 min  
Delta R.T.: -0.004 min  
Response: 960472157  
Conc: 390.26 ng/ml

Instrument: ECD\_S  
ClientSampleId: OU4-PCS-TC-31-042325

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
Supervised By :mohammad ahmed 05/05/2025

#4 2,4-DCAA

R.T.: 7.461 min  
Delta R.T.: -0.006 min  
Response: 267757330  
Conc: 380.06 ng/ml

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/23/25	
Project:	Raymark Superfund Site			Date Received:	04/25/25	
Client Sample ID:	OU4-PCS-TC-32-042325			SDG No.:	Q1883	
Lab Sample ID:	Q1883-11			Matrix:	SOIL	
Analytical Method:	SW8151A			% Solid:	97.3	Decanted:
Sample Wt/Vol:	30.02	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	Herbicide Group1	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	8151A					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PS030022.D	1	04/30/25 08:50	05/01/25 15:52	PB167796

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
1918-00-9	DICAMBA	0.034	U	0.0080	0.034	0.069	mg/Kg
75-99-0	DALAPON	0.051	U	0.018	0.051	0.069	mg/Kg
120-36-5	DICHLORPROP	0.034	U	0.013	0.034	0.069	mg/Kg
94-75-7	2,4-D	0.034	U	0.0093	0.034	0.069	mg/Kg
93-72-1	2,4,5-TP (Silvex)	0.034	U	0.0093	0.034	0.069	mg/Kg
93-76-5	2,4,5-T	0.034	U	0.0089	0.034	0.069	mg/Kg
94-82-6	2,4-DB	0.034	U	0.025	0.034	0.069	mg/Kg
88-85-7	DINOSEB	0.034	U	0.011	0.034	0.069	mg/Kg
<b>SURROGATES</b>							
19719-28-9	2,4-DCAA	327		27 - 122		65%	SPK: 500

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
Data File : PS030022.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 01 May 2025 15:52  
Operator : AR\AJ  
Sample : Q1883-11  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
OU4-PCS-TC-32-042325

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: May 02 01:29:35 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
Quant Title : 8080.M  
QLast Update : Wed Apr 23 12:57:40 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

---

System Monitoring Compounds

4) S	2,4-DCAA	6.938	7.461	804.3E6	223.7E6	326.812	317.536
------	----------	-------	-------	---------	---------	---------	---------

Target Compounds

---



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030022.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 15:52  
 Operator : AR\AJ  
 Sample : Q1883-11  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**OU4-PCS-TC-32-042325**


Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:29:35 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

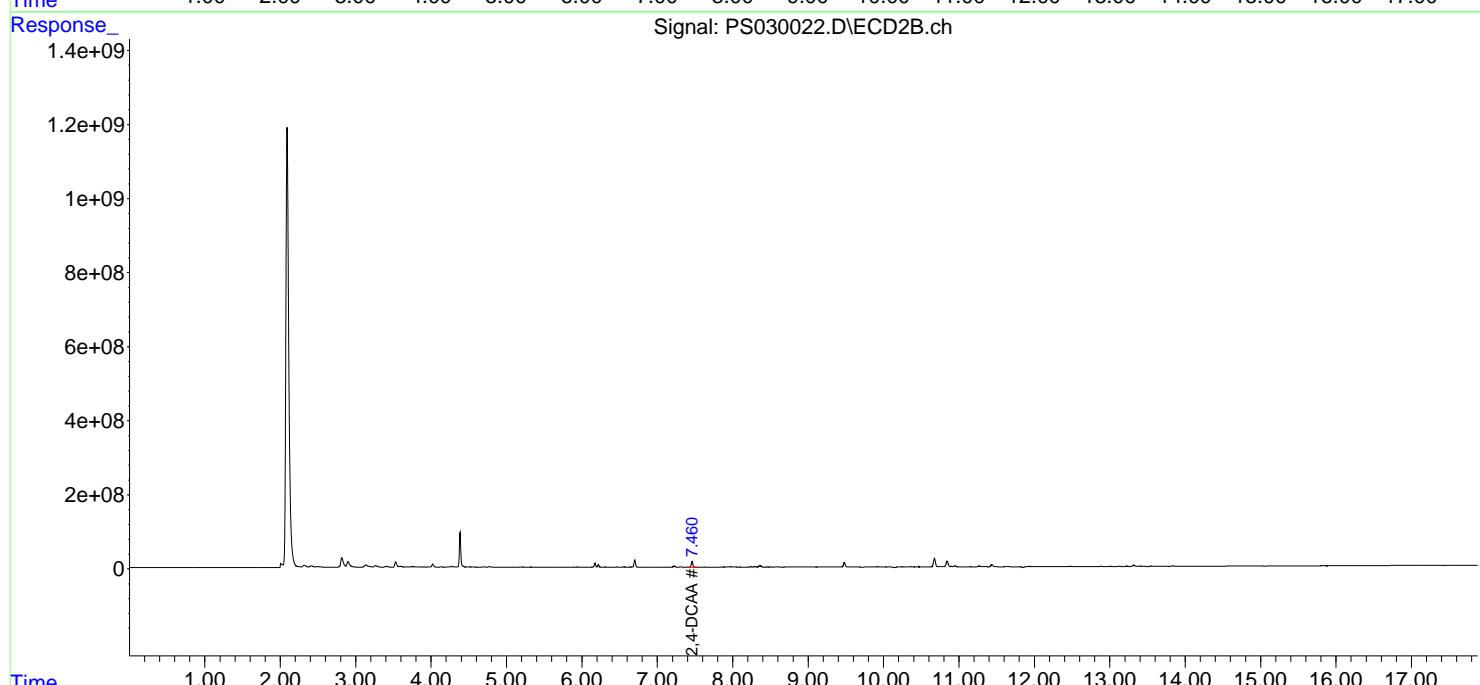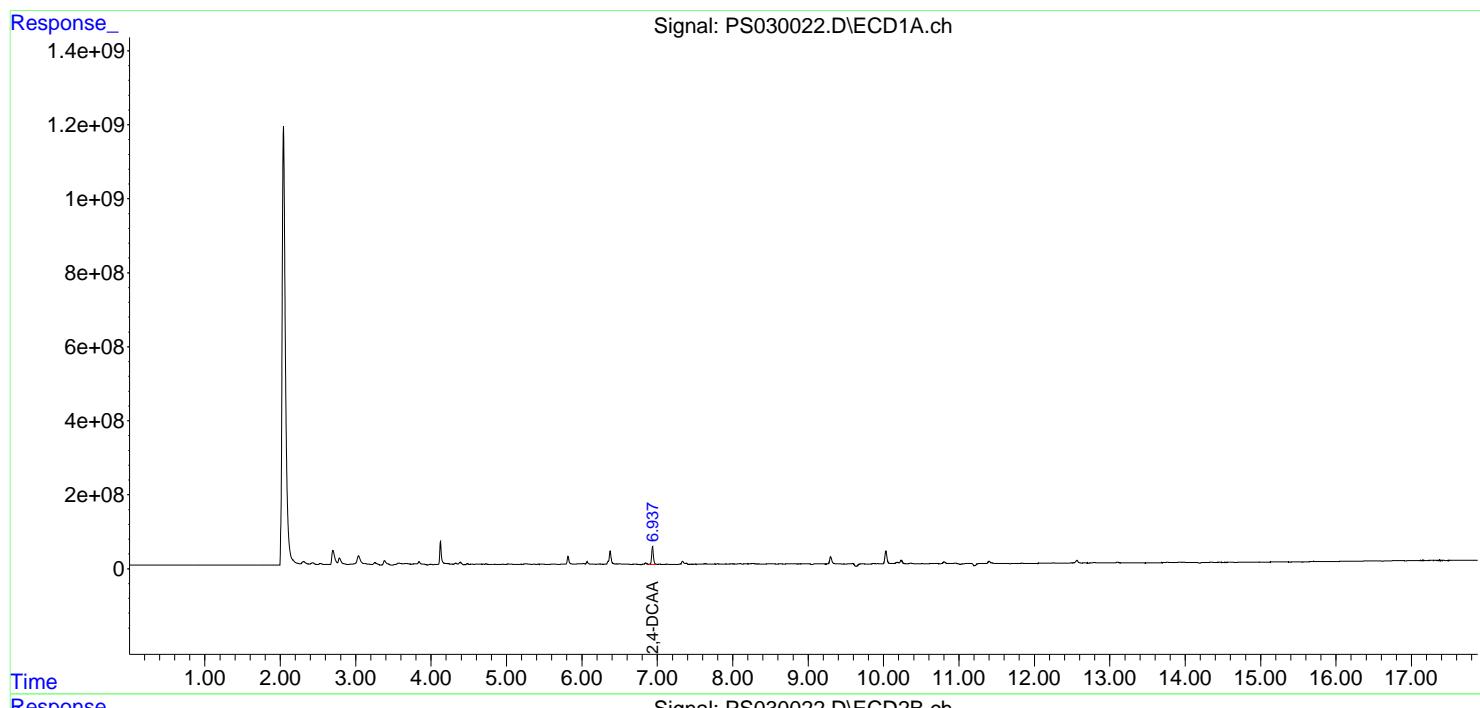


#4 2,4-DCAA

R.T.: 6.938 min  
Delta R.T.: -0.004 min  
Response: 804310408 ECD\_S  
Conc: 326.81 ng/ml ClientSampleId : OU4-PCS-TC-32-042325

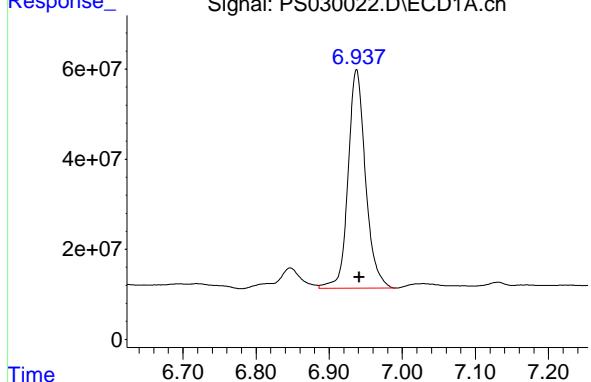

#4 2,4-DCAA

R.T.: 7.461 min  
Delta R.T.: -0.006 min  
Response: 223709231  
Conc: 317.54 ng/ml

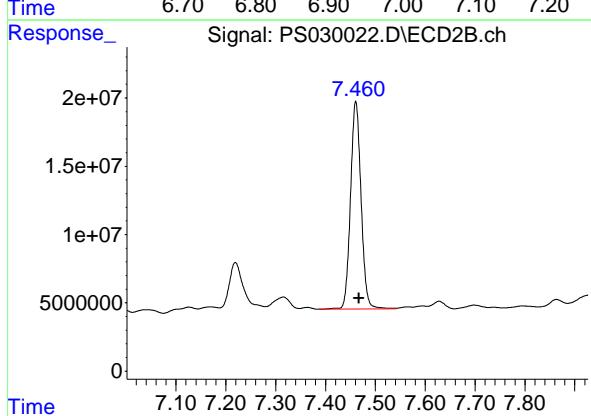



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group		Date Collected:	04/23/25	
Project:	Raymark Superfund Site		Date Received:	04/25/25	
Client Sample ID:	OU4-VSL-18-042325		SDG No.:	Q1883	
Lab Sample ID:	Q1883-13		Matrix:	SOIL	
Analytical Method:	SW8151A		% Solid:	94.7	Decanted:
Sample Wt/Vol:	30.04	Units: g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL		Test:	Herbicide Group1	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	8151A				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PS030023.D	1	04/30/25 08:50	05/01/25 16:16	PB167796

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
1918-00-9	DICAMBA	0.035	U	0.0082	0.035	0.071	mg/Kg
75-99-0	DALAPON	0.053	U	0.019	0.053	0.071	mg/Kg
120-36-5	DICHLORPROP	0.035	U	0.014	0.035	0.071	mg/Kg
94-75-7	2,4-D	0.035	U	0.0095	0.035	0.071	mg/Kg
93-72-1	2,4,5-TP (Silvex)	0.035	U	0.0096	0.035	0.071	mg/Kg
93-76-5	2,4,5-T	0.035	U	0.0092	0.035	0.071	mg/Kg
94-82-6	2,4-DB	0.035	U	0.026	0.035	0.071	mg/Kg
88-85-7	DINOSEB	0.035	U	0.011	0.035	0.071	mg/Kg
<b>SURROGATES</b>							
19719-28-9	2,4-DCAA	365		27 - 122		73%	SPK: 500

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030023.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 16:16  
 Operator : AR\AJ  
 Sample : Q1883-13  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**OU4-VSL-18-042325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:29:58 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

---

System Monitoring Compounds

4) S	2,4-DCAA	6.937	7.461	899.3E6	243.3E6	365.401	345.280
------	----------	-------	-------	---------	---------	---------	---------

---

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030023.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 16:16  
 Operator : AR\AJ  
 Sample : Q1883-13  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**OU4-VSL-18-042325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:29:58 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

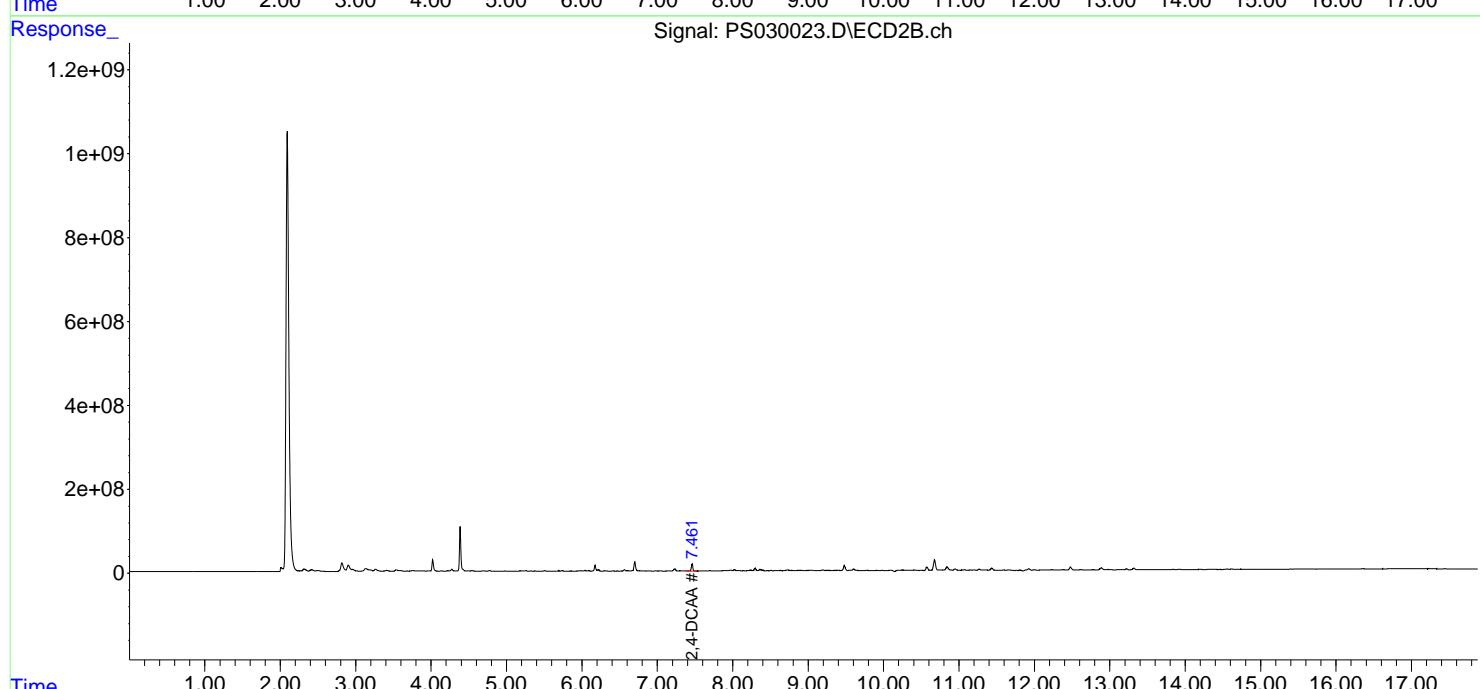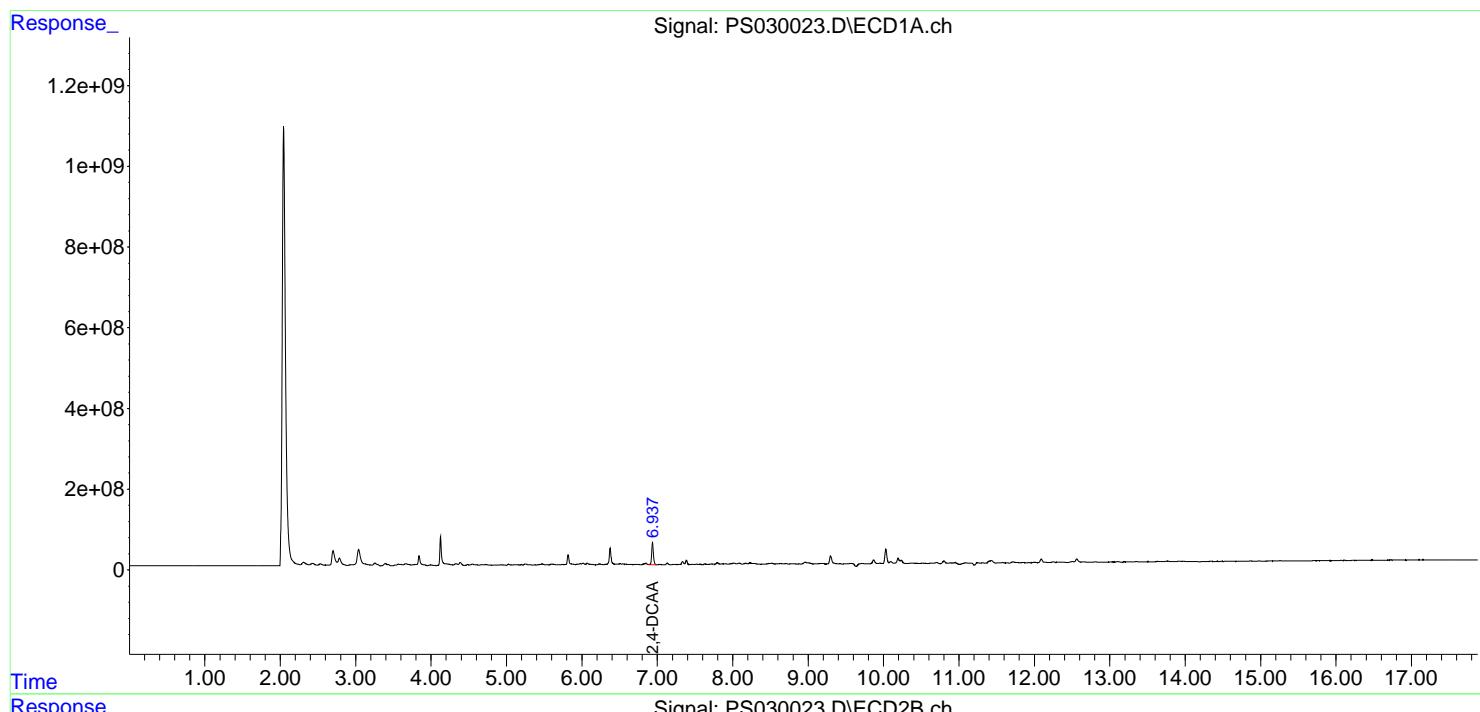

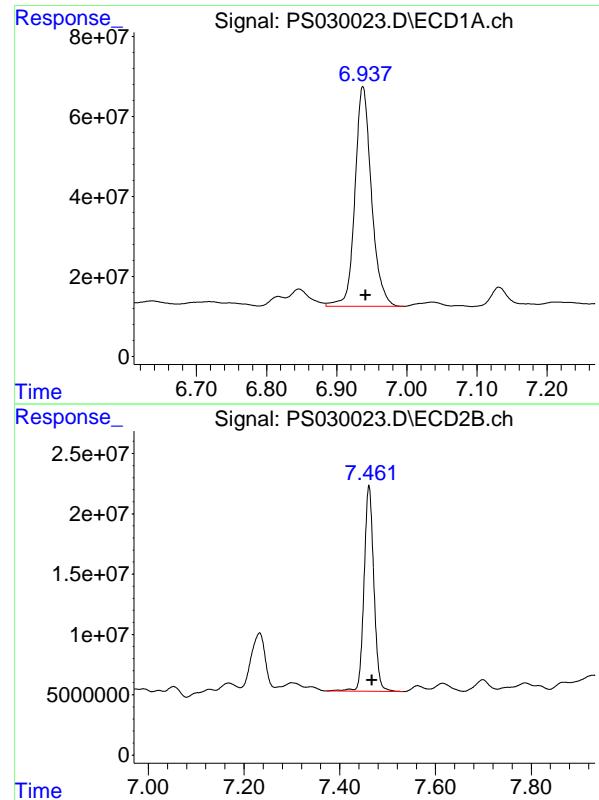

#4 2,4-DCAA

R.T.: 6.937 min  
Delta R.T.: -0.004 min  
Response: 899281602 ECD\_S  
Conc: 365.40 ng/ml ClientSampleId : OU4-VSL-18-042325

#4 2,4-DCAA

R.T.: 7.461 min  
Delta R.T.: -0.006 min  
Response: 243255379 Conc: 345.28 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group		Date Collected:	04/23/25	
Project:	Raymark Superfund Site		Date Received:	04/25/25	
Client Sample ID:	OU4-VSL-19-042325		SDG No.:	Q1883	
Lab Sample ID:	Q1883-15		Matrix:	SOIL	
Analytical Method:	SW8151A		% Solid:	95.8	Decanted:
Sample Wt/Vol:	30.07	Units: g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL		Test:	Herbicide Group1	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	8151A				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PS030024.D	1	04/30/25 08:50	05/01/25 16:40	PB167796

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
1918-00-9	DICAMBA	0.034	U	0.0081	0.034	0.070	mg/Kg
75-99-0	DALAPON	0.052	U	0.018	0.052	0.070	mg/Kg
120-36-5	DICHLORPROP	0.034	U	0.013	0.034	0.070	mg/Kg
94-75-7	2,4-D	0.034	U	0.0094	0.034	0.070	mg/Kg
93-72-1	2,4,5-TP (Silvex)	0.034	U	0.0094	0.034	0.070	mg/Kg
93-76-5	2,4,5-T	0.034	U	0.0091	0.034	0.070	mg/Kg
94-82-6	2,4-DB	0.034	U	0.025	0.034	0.070	mg/Kg
88-85-7	DINOSEB	0.034	U	0.011	0.034	0.070	mg/Kg
<b>SURROGATES</b>							
19719-28-9	2,4-DCAA	409		27 - 122		82%	SPK: 500

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
Data File : PS030024.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 01 May 2025 16:40  
Operator : AR\AJ  
Sample : Q1883-15  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
OU4-VSL-19-042325

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: May 02 01:30:16 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
Quant Title : 8080.M  
QLast Update : Wed Apr 23 12:57:40 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

---

System Monitoring Compounds

4) S	2,4-DCAA	6.938	7.461	987.0E6	288.1E6	401.029	408.938
------	----------	-------	-------	---------	---------	---------	---------

Target Compounds

---



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030024.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 16:40  
 Operator : AR\AJ  
 Sample : Q1883-15  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**OU4-VSL-19-042325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:30:16 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

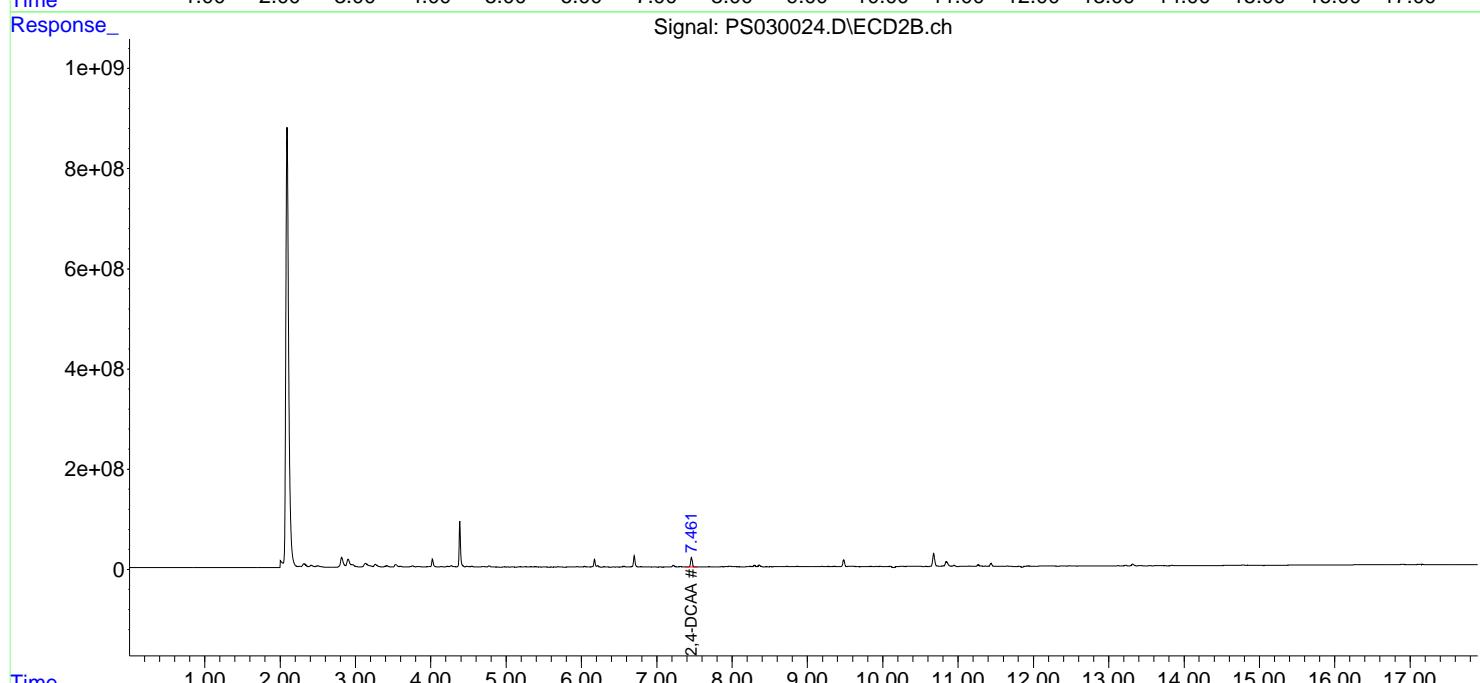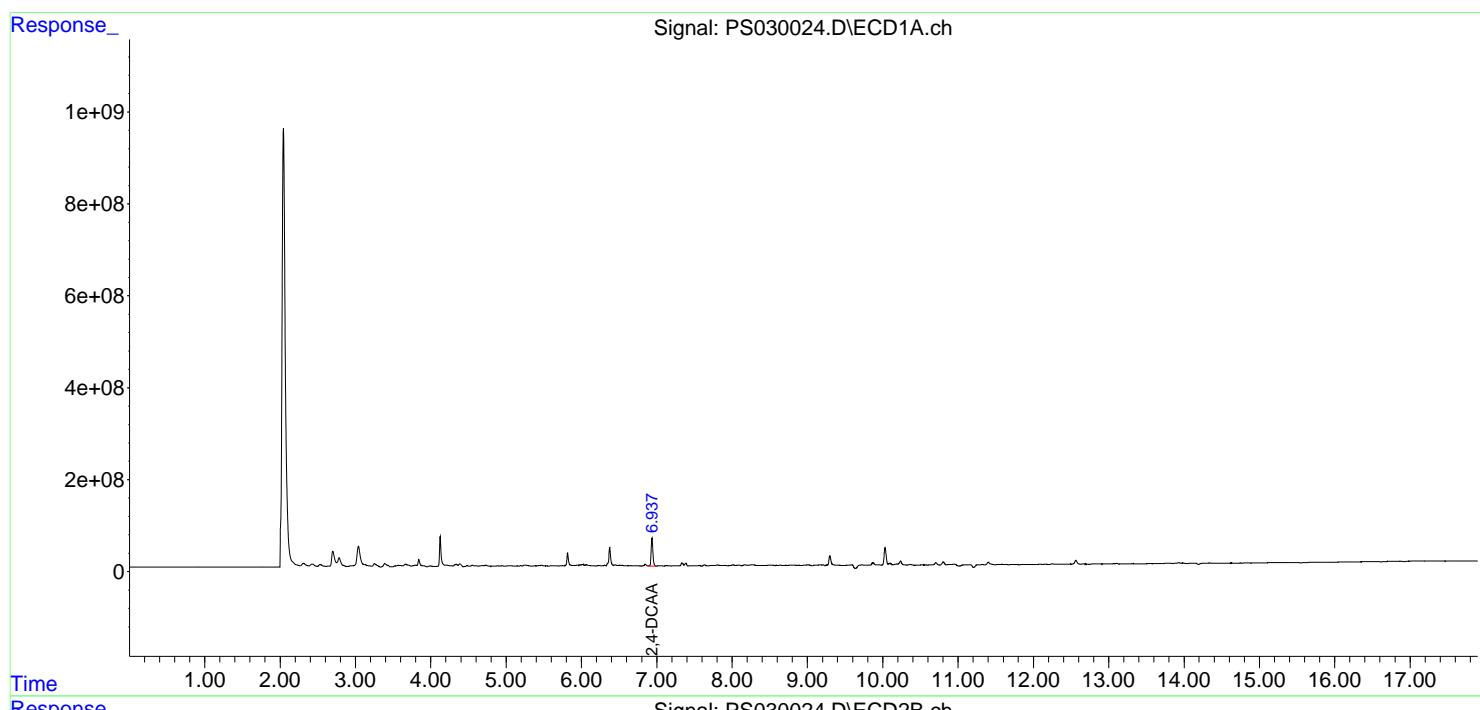

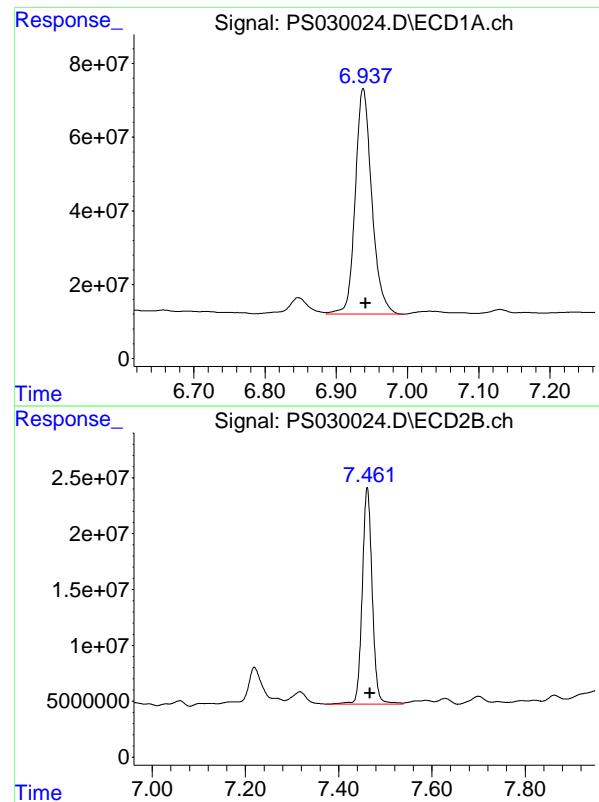

#4 2,4-DCAA

R.T.: 6.938 min  
Delta R.T.: -0.004 min  
Response: 986963633 ECD\_S  
Conc: 401.03 ng/ml ClientSampleId : OU4-VSL-19-042325

#4 2,4-DCAA

R.T.: 7.461 min  
Delta R.T.: -0.006 min  
Response: 288103690  
Conc: 408.94 ng/ml



# CALIBRATION

# SUMMARY



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### RETENTION TIMES OF INITIAL CALIBRATION

<b>Contract:</b>	<u>NOBI03</u>							
<b>Lab Code:</b>	<u>CHEM</u>		<b>Case No.:</b>	<u>Q1883</u>	<b>SAS No.:</b>	<u>Q1883</u>	<b>SDG NO.:</b>	<u>Q1883</u>
<b>Instrument ID:</b>	<u>ECD_S</u>		<b>Calibration Date(s):</b>		<u>04/23/2025</u>		<u>04/23/2025</u>	
			<b>Calibration Times:</b>		<u>11:01</u>		<u>12:37</u>	

GC Column: RTX-CLP ID: 0.32 (mm)

<b>LAB FILE ID:</b>	RT 200 =	<u>PS029919.D</u>	RT 500 =	<u>PS029920.D</u>
	RT 750 =	<u>PS029921.D</u>	RT 1000 =	<u>PS029922.D</u>
			RT 1500 =	<u>PS029923.D</u>

COMPOUND	RT 200	RT 500	RT 750	RT 1000	RT 1500	MEAN RT	RT WINDOW	FROM	TO
2,4,5-T	9.15	9.15	9.14	9.14	9.14	9.14	9.04	9.24	
2,4,5-TP(Silvex)	8.86	8.86	8.86	8.86	8.86	8.86	8.76	8.96	
2,4-D	8.02	8.02	8.02	8.02	8.02	8.02	7.92	8.12	
2,4-DB	9.70	9.70	9.70	9.70	9.70	9.70	9.60	9.80	
2,4-DCAA	6.94	6.94	6.94	6.94	6.94	6.94	6.84	7.04	
Dalapon	2.45	2.45	2.45	2.45	2.45	2.45	2.35	2.55	
DICAMBA	7.12	7.12	7.12	7.12	7.12	7.12	7.02	7.22	
DICHLORPROP	7.80	7.80	7.80	7.80	7.80	7.80	7.70	7.90	
Dinoseb	10.87	10.87	10.87	10.87	10.87	10.87	10.77	10.97	



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### RETENTION TIMES OF INITIAL CALIBRATION

<b>Contract:</b>	<u>NOBI03</u>						
<b>Lab Code:</b>	<u>CHEM</u>	<b>Case No.:</b>	<u>Q1883</u>	<b>SAS No.:</b>	<u>Q1883</u>	<b>SDG NO.:</b>	<u>Q1883</u>
<b>Instrument ID:</b>	<u>ECD_S</u>	<b>Calibration Date(s):</b>		<u>04/23/2025</u>		<u>04/23/2025</u>	
		<b>Calibration Times:</b>		<u>11:01</u>		<u>12:37</u>	

GC Column: RTX-CLP2 ID: 0.32 (mm)

<b>LAB FILE ID:</b>	RT 200 =	<u>PS029919.D</u>	RT 500 =	<u>PS029920.D</u>
	RT 750 =	<u>PS029921.D</u>	RT 1000 =	<u>PS029922.D</u>
			RT 1500 =	<u>PS029923.D</u>

COMPOUND	RT 200	RT 500	RT 750	RT 1000	RT 1500	MEAN RT	RT WINDOW	
							FROM	TO
2,4,5-T	9.95	9.95	9.95	9.95	9.95	9.95	9.85	10.05
2,4,5-TP(Silvex)	9.54	9.54	9.54	9.54	9.54	9.54	9.44	9.64
2,4-D	8.66	8.66	8.66	8.66	8.66	8.66	8.56	8.76
2,4-DB	10.51	10.51	10.51	10.51	10.51	10.51	10.41	10.61
2,4-DCAA	7.47	7.47	7.47	7.47	7.47	7.47	7.37	7.57
Dalapon	2.53	2.53	2.53	2.52	2.52	2.52	2.42	2.62
DICAMBA	7.65	7.65	7.65	7.65	7.65	7.65	7.55	7.75
DICHLORPROP	8.35	8.35	8.35	8.35	8.35	8.35	8.25	8.45
Dinoseb	10.88	10.88	10.88	10.88	10.88	10.88	10.78	10.98



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: NOBI03  
 Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883  
 Instrument ID: ECD\_S Calibration Date(s): 04/23/2025 04/23/2025  
 Calibration Times: 11:01 12:37  
 GC Column: RTX-CLP ID: 0.32 (mm)

LAB FILE ID:	CF 200 =	<u>PS029919.D</u>	CF 500 =	<u>PS029920.D</u>
	CF 750 =	<u>PS029921.D</u>	CF 1000 =	<u>PS029922.D</u>

COMPOUND	CF 200	CF 500	CF 750	CF 1000	CF 1500	CF	% RSD
2,4,5-T	16505300000	14051400000	13586300000	13082600000	13039900000	14053100000	10
2,4,5-TP(Silvex)	16213200000	13862200000	13431300000	12910500000	12897000000	13862800000	10
2,4-D	3379530000	2797950000	2695740000	2590800000	2600340000	2812870000	12
2,4-DB	2544360000	2254920000	2220820000	2167640000	2239040000	2285360000	7
2,4-DCAA	3038250000	2463560000	2343090000	2233670000	2226830000	2461080000	14
Dalapon	4639950000	4240730000	4001870000	3801310000	3792430000	4095260000	9
DICAMBA	11438400000	9878540000	9619200000	9265370000	9312840000	9902870000	9
DICHLOLORPROP	3106740000	2525040000	2414030000	2305320000	2319400000	2534110000	13
Dinoseb	12057500000	10136700000	9900160000	9369950000	9402820000	10173400000	11



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: NOBI03  
 Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883  
 Instrument ID: ECD\_S Calibration Date(s): 04/23/2025 04/23/2025  
 Calibration Times: 11:01 12:37  
 GC Column: RTX-CLP2 ID: 0.32 (mm)

LAB FILE ID:	CF 200 =	<u>PS029919.D</u>	CF 500 =	<u>PS029920.D</u>
	CF 750 =	<u>PS029921.D</u>	CF 1000 =	<u>PS029922.D</u>

COMPOUND	CF 200	CF 500	CF 750	CF 1000	CF 1500	CF	% RSD
2,4,5-T	8525110000	7667180000	7627750000	7425390000	7567570000	7762600000	6
2,4,5-TP(Silvex)	8841790000	8081200000	8077540000	7871670000	8036560000	8181750000	5
2,4-D	1299090000	1113240000	1091000000	1054800000	1077400000	1127110000	9
2,4-DB	882651000	763494000	795790000	776318000	805960000	804842000	6
2,4-DCAA	807639000	692361000	682858000	661991000	677736000	704517000	8
Dalapon	2089590000	1714890000	1661930000	1593710000	1620600000	1736140000	12
DICAMBA	4120140000	3813580000	3900860000	3853240000	4062500000	3950060000	3
DICHLOLORPROP	1163430000	987784000	972110000	937504000	958998000	1003960000	9
Dinoseb	6538160000	5743240000	5708570000	5526360000	5638570000	5830980000	7

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029919.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 11:01  
 Operator : AR\AJ  
 Sample : HSTDICC200  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**HSTDICC200**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 12:21:29 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:13:04 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

#### System Monitoring Compounds

4) S 2,4-DCAA 6.942 7.467 607.6E6 161.5E6 232.374 221.995

#### Target Compounds

1) T	Dalapon	2.449	2.525	844.5E6	380.3E6	193.384m	208.714
2) T	3,5-DICHL...	6.146	6.463	802.7E6	206.9E6	212.813	205.094
3) T	4-Nitroph...	6.733	7.001	383.7E6	162.2E6	206.288	204.354
5) T	DICAMBA	7.118	7.653	2150.4E6	774.6E6	208.534	196.353
6) T	MCPP	7.295	7.758	112.8E6	31299306	18.132	18.050
7) T	MCPA	7.437	7.988	169.4E6	48918025	19.260	20.374
8) T	DICHLORPROP	7.799	8.348	584.1E6	218.7E6	217.778	210.088
9) T	2,4-D	8.021	8.661	635.4E6	244.2E6	214.810	209.141
10) T	Pentachlo...	8.298	9.163	7828.1E6	4208.5E6	211.528	201.368
11) T	2,4,5-TP ...	8.862	9.542	3080.5E6	1679.9E6	212.416	201.589
12) T	2,4,5-T	9.145	9.947	3136.0E6	1619.8E6	213.126	204.001
13) T	2,4-DB	9.704	10.507	483.4E6	167.7E6	206.590	206.030
14) T	DINOSEB	10.866	10.881	2266.8E6	1229.2E6	211.888	204.977
15) T	Picloram	10.686	11.918	3927.9E6	2710.5E6	208.185	221.777m
16) T	DCPA	11.167	11.918	3823.9E6	2388.5E6	214.204	203.950m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029919.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 11:01  
 Operator : AR\AJ  
 Sample : HSTDICC200  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1



Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 12:21:29 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:13:04 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation





Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

**Instrument :**  
 ECD\_S  
**ClientSampleId :**  
 HSTDICC200

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

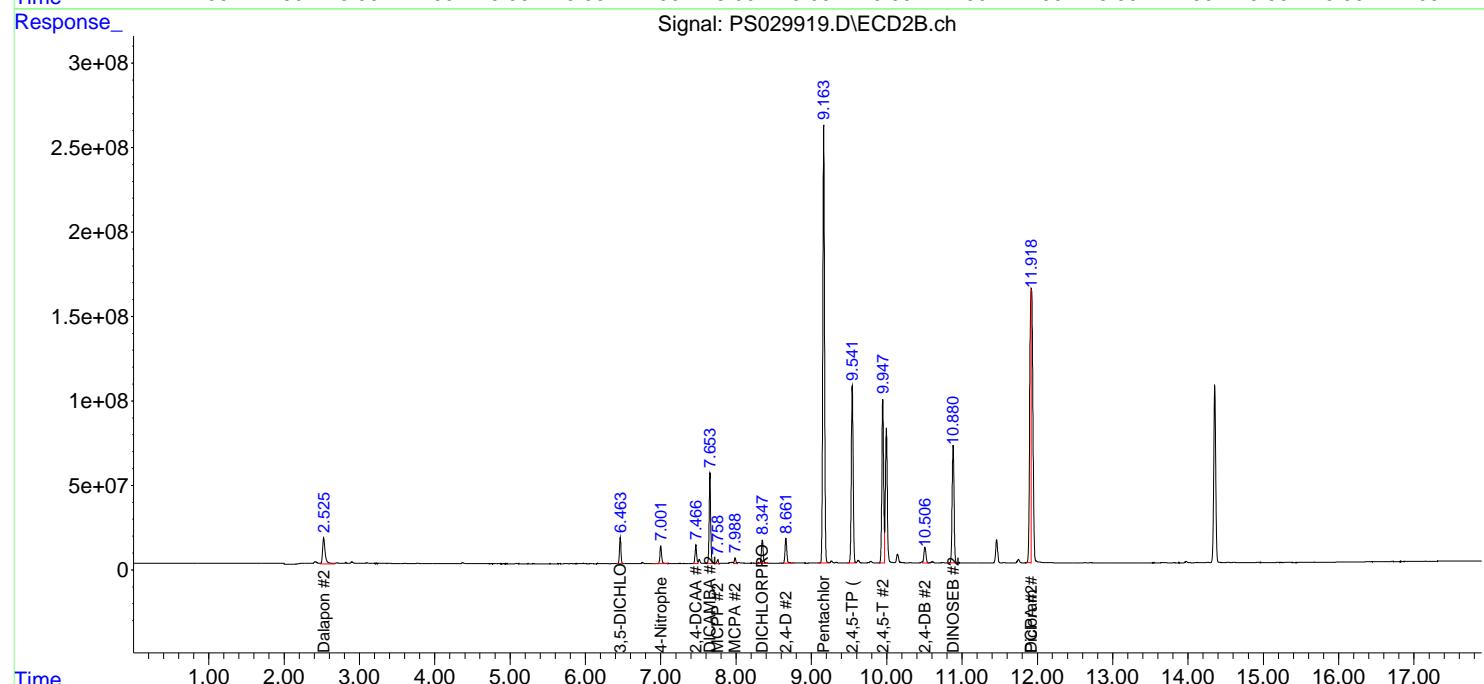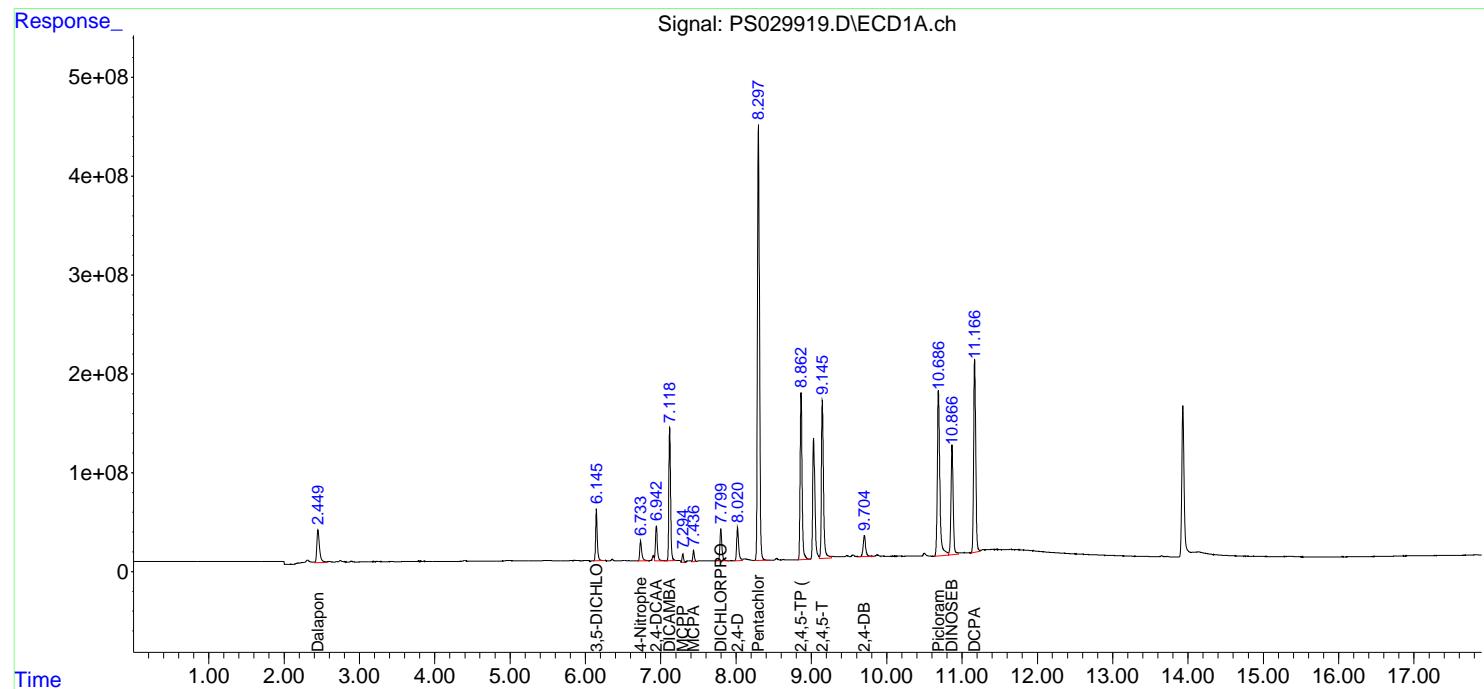

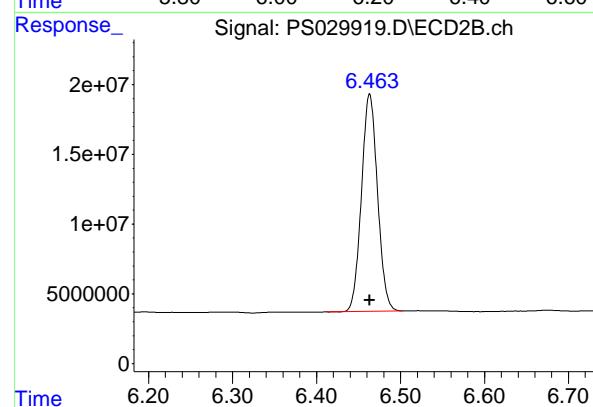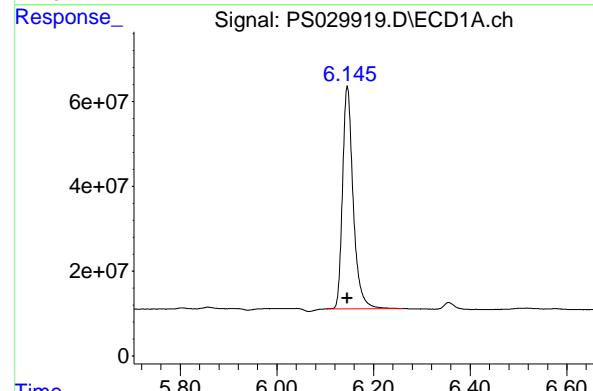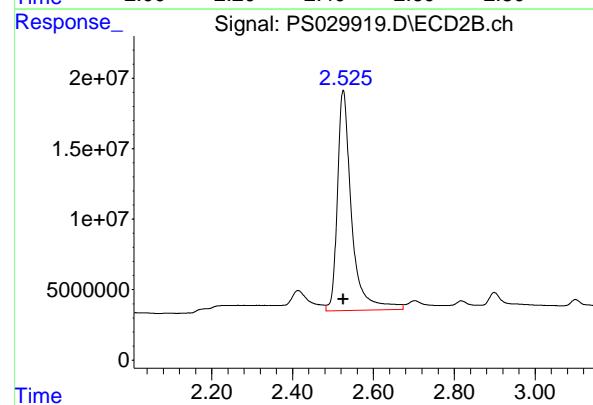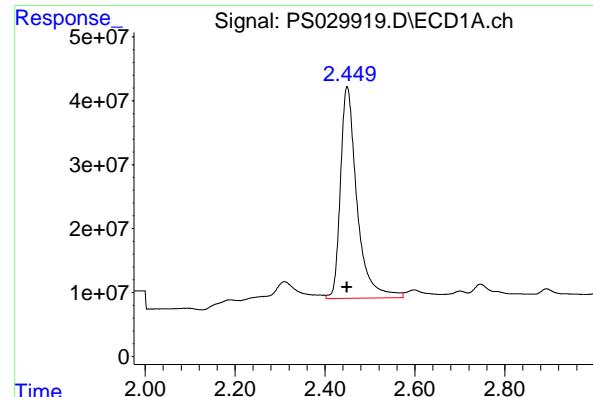

#1 Dalapon

R.T.: 2.449 min  
 Delta R.T.: 0.000 min  
 Response: 844471314 ECD\_S  
 Conc: 193.38 ng/ml ClientSampleId : HSTDICC200

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

#1 Dalapon

R.T.: 2.525 min  
 Delta R.T.: 0.000 min  
 Response: 380305456  
 Conc: 208.71 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.146 min  
 Delta R.T.: 0.000 min  
 Response: 802682173  
 Conc: 212.81 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.463 min  
 Delta R.T.: 0.000 min  
 Response: 206925954  
 Conc: 205.09 ng/ml

## #3 4-Nitrophenol

R.T.: 6.733 min  
 Delta R.T.: 0.000 min  
 Response: 383695461  
 Conc: 206.29 ng/ml  
 Instrument: ECD\_S  
 ClientSampleId : HSTDICC200

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

## #3 4-Nitrophenol





R.T.: 7.001 min  
 Delta R.T.: 0.000 min  
 Response: 162220636  
 Conc: 204.35 ng/ml

## #4 2,4-DCAA

R.T.: 6.942 min  
 Delta R.T.: 0.000 min  
 Response: 607649568  
 Conc: 232.37 ng/ml

## #4 2,4-DCAA

R.T.: 7.467 min  
 Delta R.T.: 0.000 min  
 Response: 161527736  
 Conc: 221.99 ng/ml

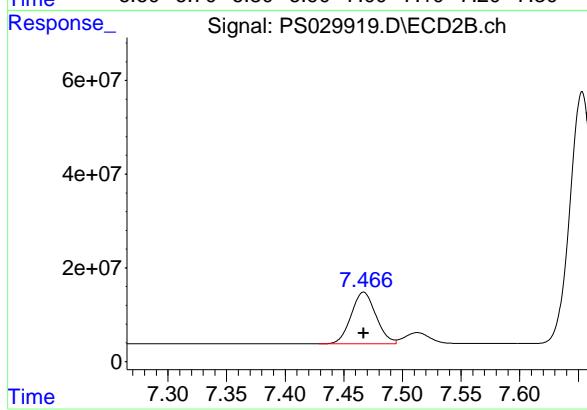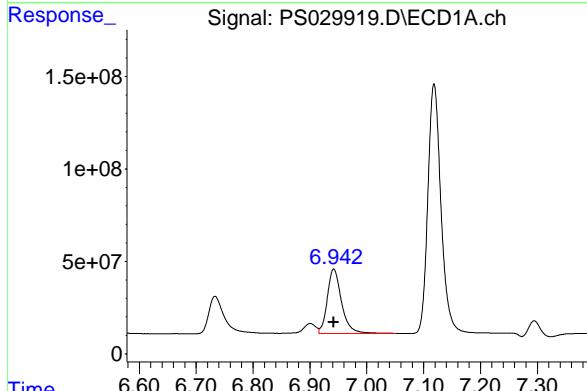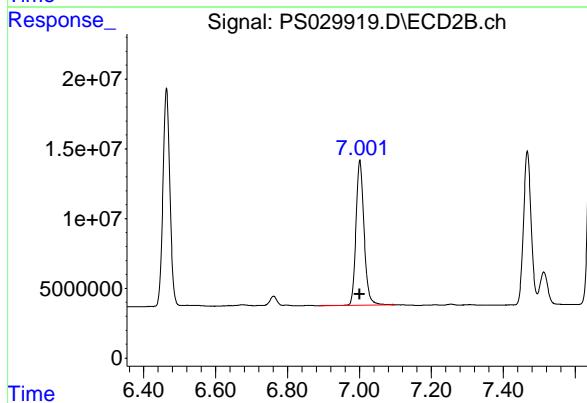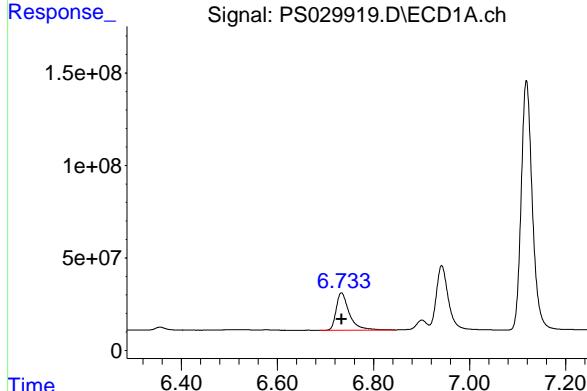

## #5 DICAMBA

R.T.: 7.118 min  
 Delta R.T.: 0.000 min  
 Response: 2150414141 ECD\_S  
 Conc: 208.53 ng/ml ClientSampleId : HSTDICC200

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

## #5 DICAMBA





R.T.: 7.653 min  
 Delta R.T.: 0.000 min  
 Response: 774585769  
 Conc: 196.35 ng/ml





## #6 MCPP

R.T.: 7.295 min  
 Delta R.T.: 0.000 min  
 Response: 112779199  
 Conc: 18.13 ug/ml

## #6 MCPP

R.T.: 7.758 min  
 Delta R.T.: 0.000 min  
 Response: 31299306  
 Conc: 18.05 ug/ml

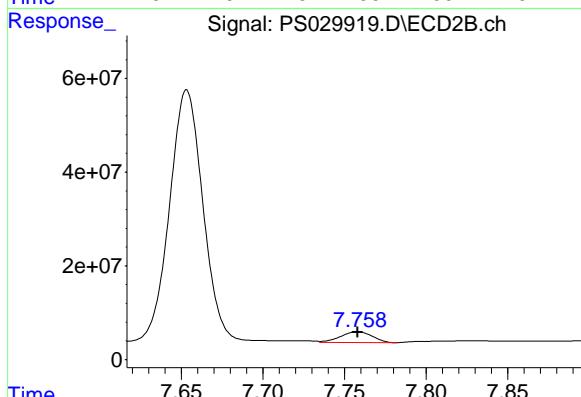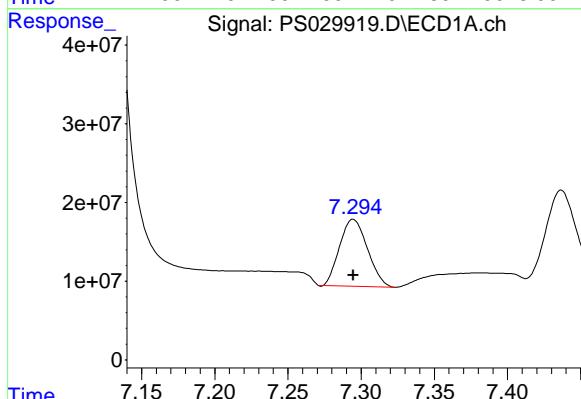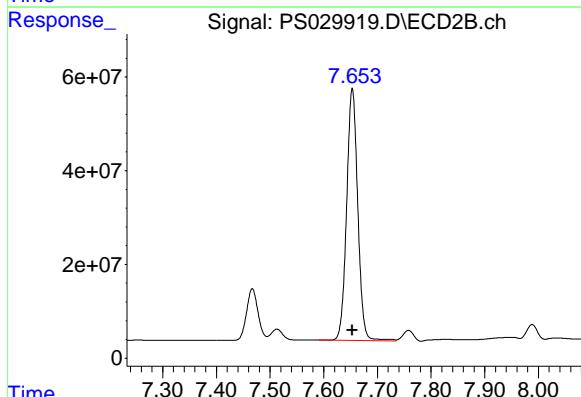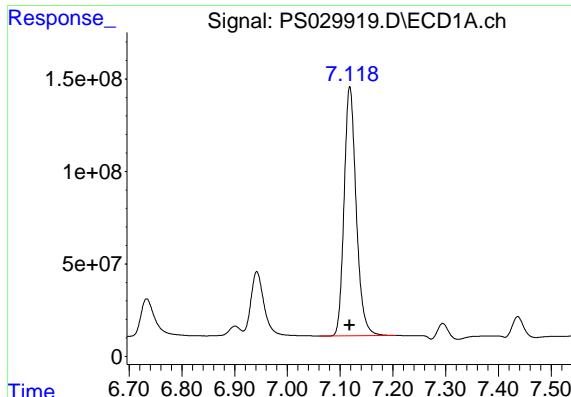

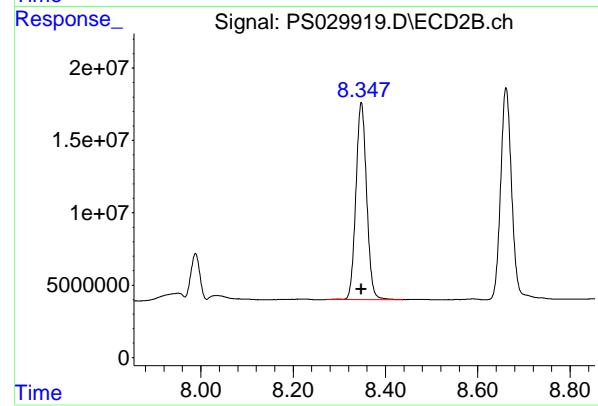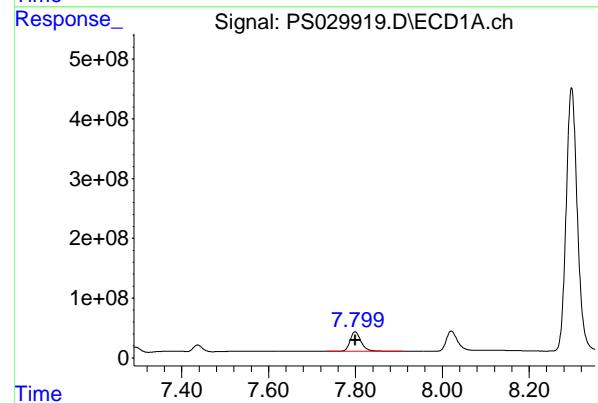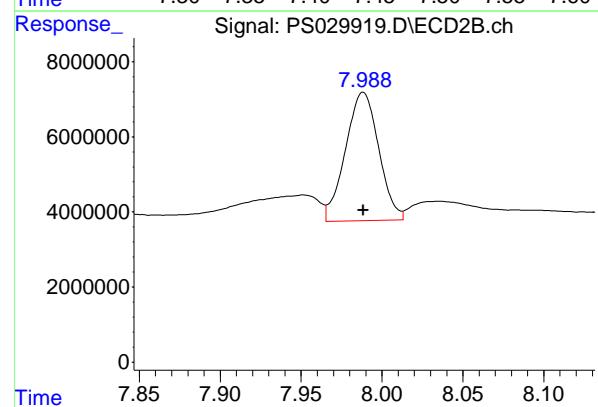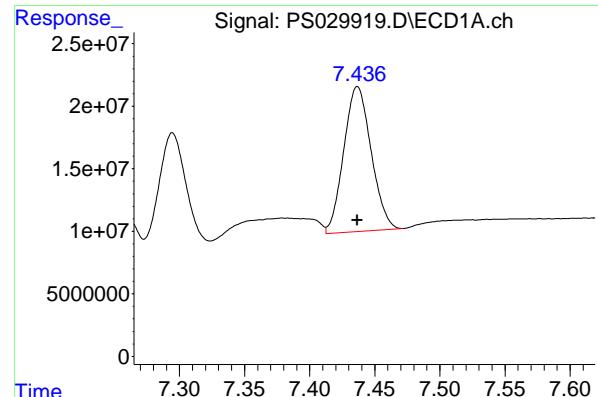

## #7 MCPA

R.T.: 7.437 min  
 Delta R.T.: 0.000 min  
 Instrument: ECD\_S  
 Response: 169402932  
 Conc: 19.26 ug/ml  
 ClientSampleId: HSTDICC200

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

## #7 MCPA

R.T.: 7.988 min  
 Delta R.T.: 0.000 min  
 Response: 48918025  
 Conc: 20.37 ug/ml

## #8 DICHLORPROP

R.T.: 7.799 min  
 Delta R.T.: 0.000 min  
 Response: 584067087  
 Conc: 217.78 ng/ml

## #8 DICHLORPROP

R.T.: 8.348 min  
 Delta R.T.: 0.000 min  
 Response: 218723918  
 Conc: 210.09 ng/ml

#9 2,4-D

R.T.: 8.021 min  
 Delta R.T.: 0.000 min  
 Response: 635351443 Instrument: ECD\_S  
 Conc: 214.81 ng/ml ClientSampleId : HSTDICC200

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

#9 2,4-D





R.T.: 8.661 min  
 Delta R.T.: 0.000 min  
 Response: 244229801  
 Conc: 209.14 ng/ml


#10 Pentachlorophenol

R.T.: 8.298 min  
 Delta R.T.: 0.000 min  
 Response: 7828106091  
 Conc: 211.53 ng/ml

#10 Pentachlorophenol

R.T.: 9.163 min  
 Delta R.T.: 0.000 min  
 Response: 4208465177  
 Conc: 201.37 ng/ml

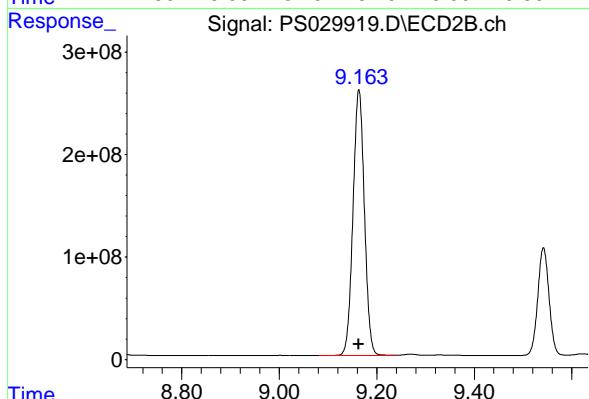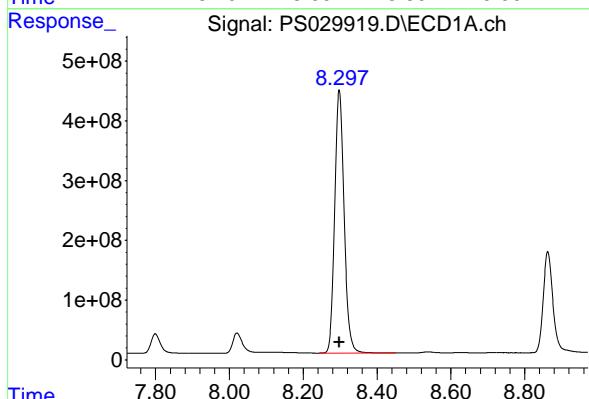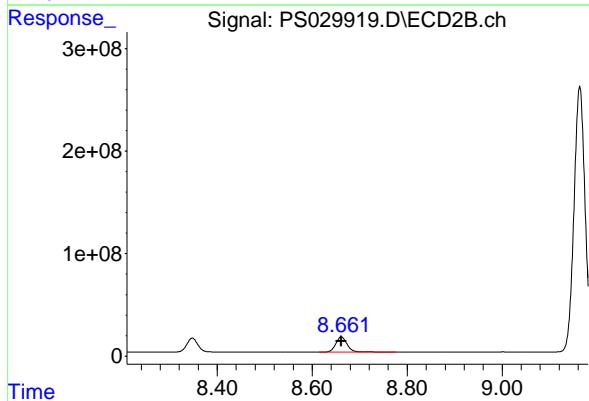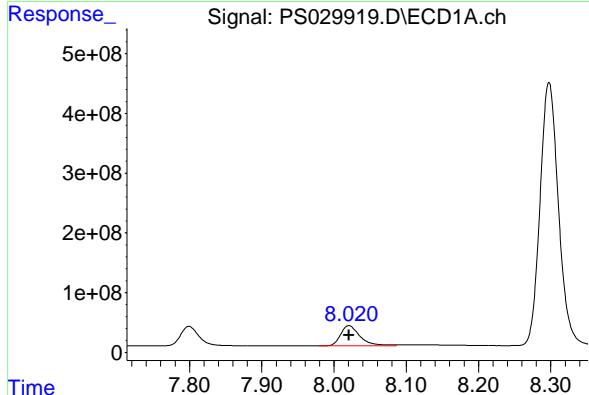

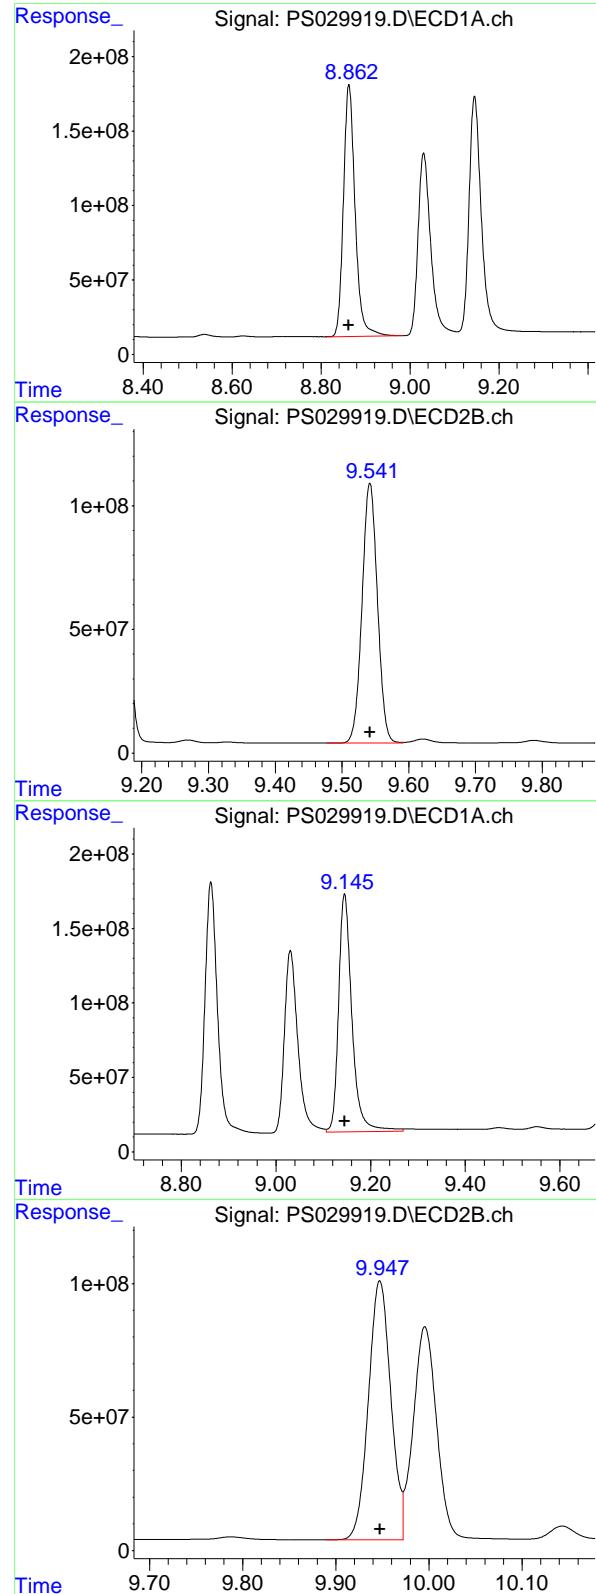

#11 2,4,5-TP (SILVEX)

R.T.: 8.862 min

Delta R.T.: 0.000 min

Instrument: ECD\_S

Response: 3080510531 ClientSampleId :

Conc: 212.42 ng/ml HSTDICC200

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025

Supervised By :mohammad ahmed 04/26/2025

#11 2,4,5-TP (SILVEX)

R.T.: 9.542 min

Delta R.T.: 0.000 min

Response: 1679940962

Conc: 201.59 ng/ml

#12 2,4,5-T

R.T.: 9.145 min

Delta R.T.: 0.000 min

Response: 3136007230

Conc: 213.13 ng/ml

#12 2,4,5-T

R.T.: 9.947 min

Delta R.T.: 0.000 min

Response: 1619770655

Conc: 204.00 ng/ml

#13 2,4-DB

R.T.: 9.704 min  
 Delta R.T.: 0.000 min  
 Response: 483428317  
 Conc: 206.59 ng/ml  
 Instrument: ECD\_S  
 ClientSampleId : HSTDICC200

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

#13 2,4-DB





R.T.: 10.507 min  
 Delta R.T.: 0.000 min  
 Response: 167703688  
 Conc: 206.03 ng/ml


#14 DINOSEB

R.T.: 10.866 min  
 Delta R.T.: 0.000 min  
 Response: 2266806582  
 Conc: 211.89 ng/ml

#14 DINOSEB

R.T.: 10.881 min  
 Delta R.T.: 0.000 min  
 Response: 1229173921  
 Conc: 204.98 ng/ml

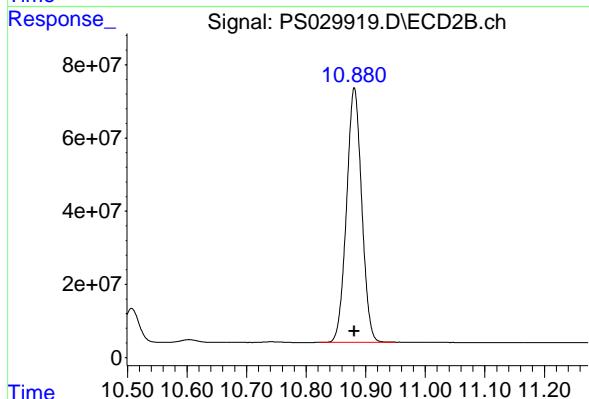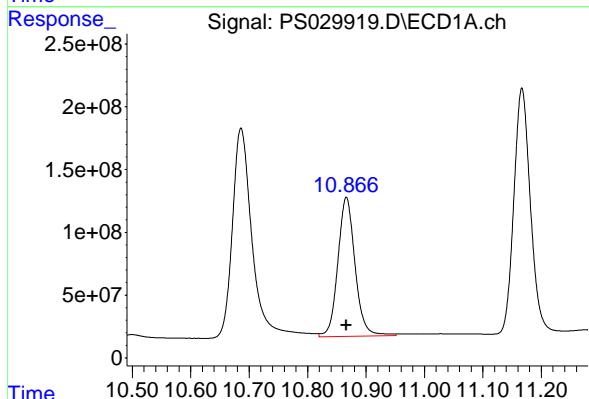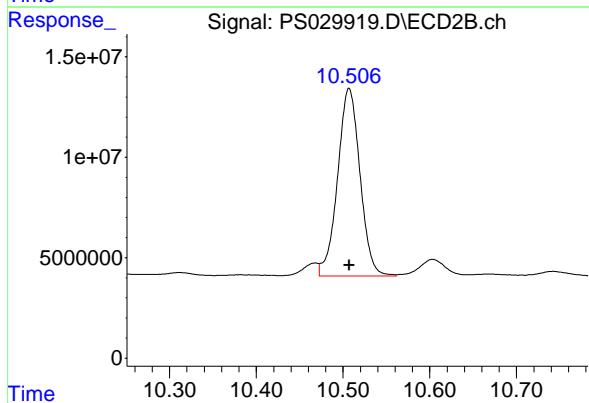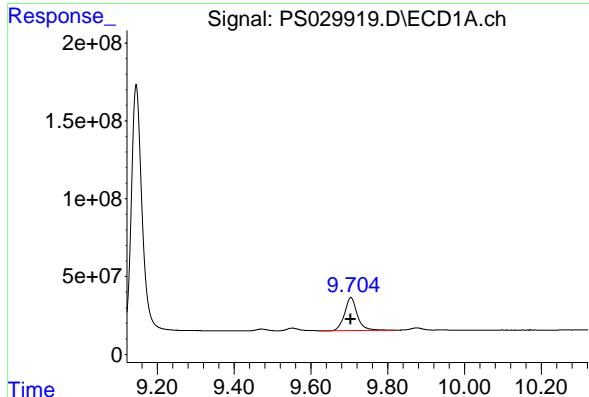

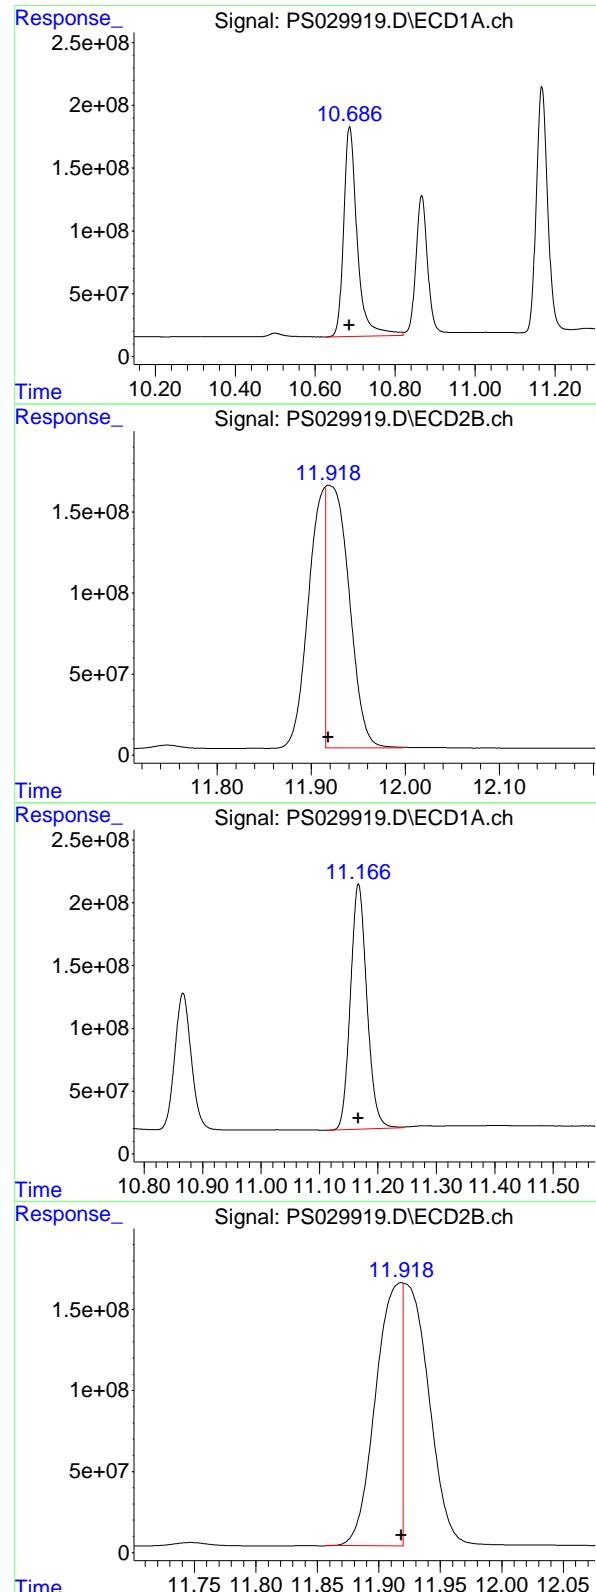

## #15 Picloram

R.T.: 10.686 min  
 Delta R.T.: 0.000 min  
 Response: 3927930714 ECD\_S  
 Conc: 208.18 ng/ml ClientSampleId : HSTDICC200

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

## #15 Picloram

R.T.: 11.918 min  
 Delta R.T.: 0.000 min  
 Response: 2710469284  
 Conc: 221.78 ng/ml

## #16 DCPA

R.T.: 11.167 min  
 Delta R.T.: 0.000 min  
 Response: 3823873526  
 Conc: 214.20 ng/ml

## #16 DCPA

R.T.: 11.918 min  
 Delta R.T.: 0.000 min  
 Response: 2388549576  
 Conc: 203.95 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029920.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 11:25  
 Operator : AR\AJ  
 Sample : HSTDICC500  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**HSTDICC500**

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 12:18:02 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:13:04 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

4) S 2,4-DCAA 6.942 7.467 1231.8E6 346.2E6 512.532 503.455

**Target Compounds**

1) T	Dalapon	2.449	2.525	1929.5E6	780.3E6	468.186	462.137
2) T	3,5-DICHL...	6.146	6.463	1662.7E6	449.2E6	475.061	469.317
3) T	4-Nitroph...	6.733	7.001	802.3E6	342.6E6	462.200	459.862
5) T	DICAMBA	7.118	7.653	4642.9E6	1792.4E6	476.252	464.683
6) T	MCPP	7.296	7.759	290.7E6	82241844	45.918	46.500
7) T	MCPA	7.438	7.990	399.1E6	105.5E6	46.188	46.156
8) T	DICHLORPROP	7.799	8.347	1186.8E6	464.3E6	480.564	473.759
9) T	2,4-D	8.020	8.661	1315.0E6	523.2E6	478.744	474.742
10) T	Pentachlo...	8.297	9.164	16887.6E6	9661.5E6	483.734	476.543
11) T	2,4,5-TP ...	8.862	9.542	6584.5E6	3838.6E6	482.498	475.108
12) T	2,4,5-T	9.145	9.948	6674.4E6	3641.9E6	482.992	476.224
13) T	2,4-DB	9.703	10.507	1071.1E6	362.7E6	478.618	465.162
14) T	DINOSEB	10.866	10.881	4764.3E6	2699.3E6	475.549	471.423
15) T	Picloram	10.685	11.923	8585.2E6	5454.2E6	477.895	452.164m
16) T	DCPA	11.167	11.919	8208.3E6	5573.5E6	488.029	495.898m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029920.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 11:25  
 Operator : AR\AJ  
 Sample : HSTDICC500  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1



Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDICC500





**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 12:18:02 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:13:04 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

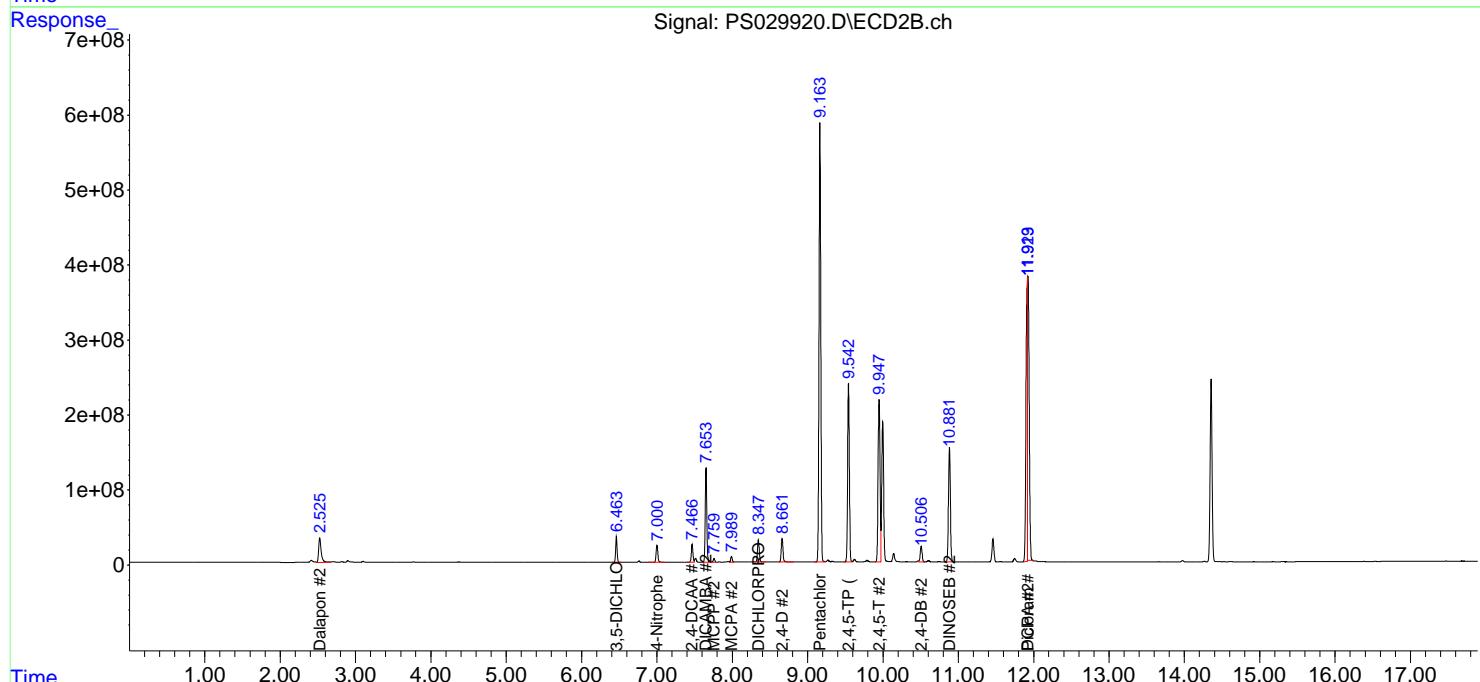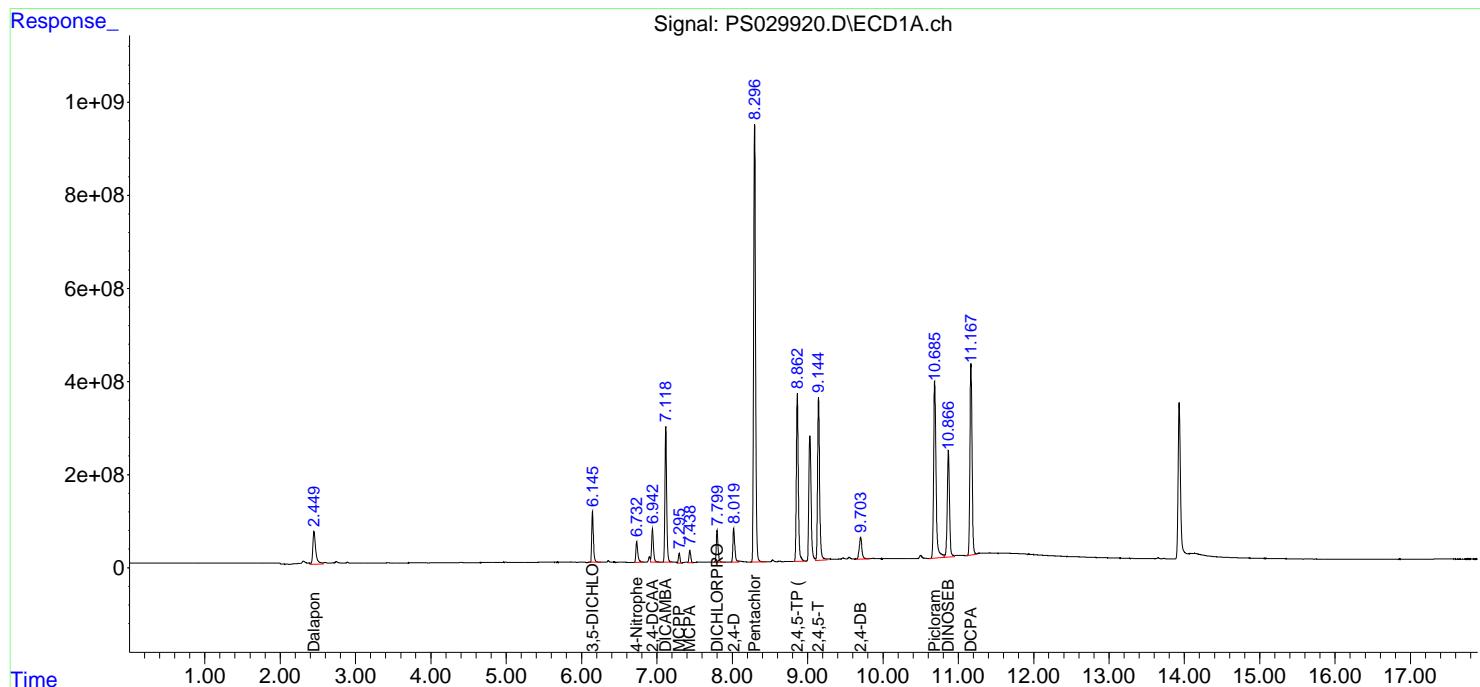

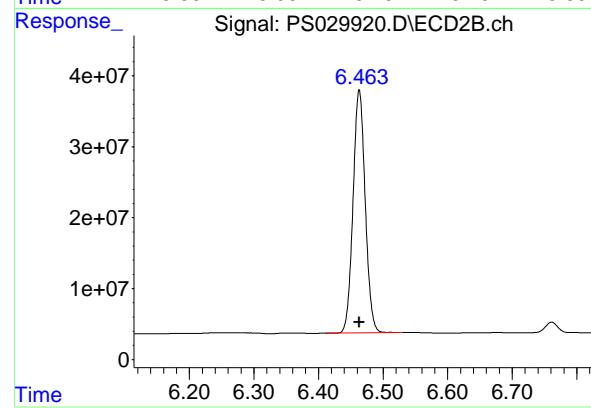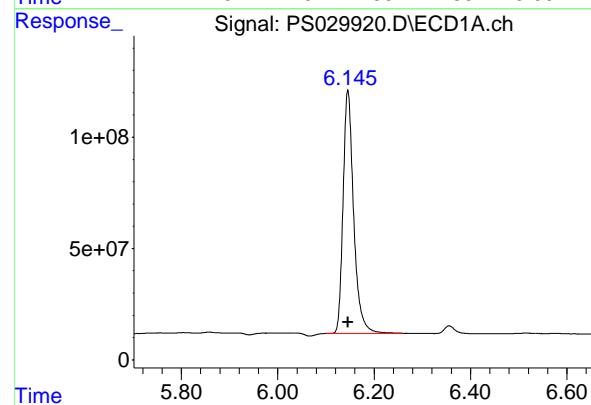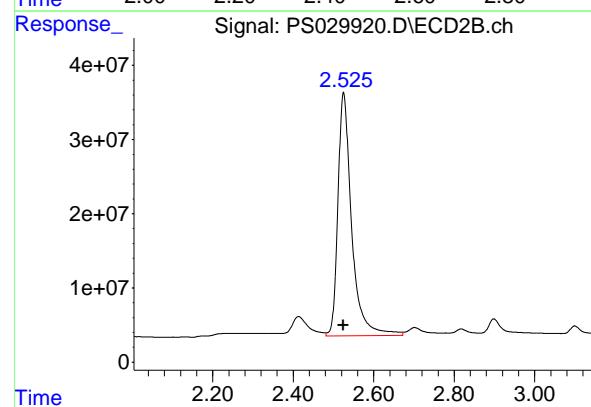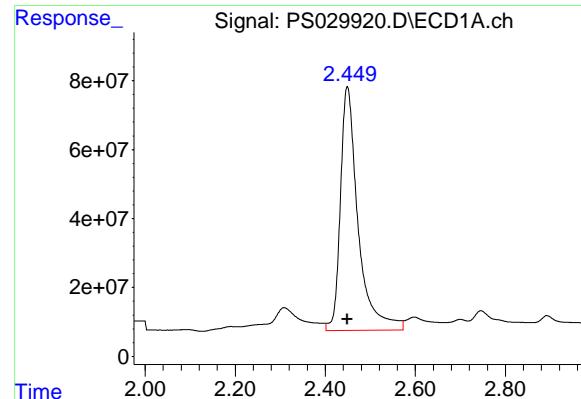

## #1 Dalapon

R.T.: 2.449 min  
 Delta R.T.: 0.000 min  
 Response: 1929533765  
 Conc: 468.19 ng/ml  
 Instrument: ECD\_S  
 ClientSampleId : HSTDICC500

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

## #1 Dalapon

R.T.: 2.525 min  
 Delta R.T.: 0.000 min  
 Response: 780277133  
 Conc: 462.14 ng/ml

## #2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.146 min  
 Delta R.T.: 0.000 min  
 Response: 1662675840  
 Conc: 475.06 ng/ml

## #2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.463 min  
 Delta R.T.: 0.000 min  
 Response: 449204324  
 Conc: 469.32 ng/ml

## #3 4-Nitrophenol

R.T.: 6.733 min  
 Delta R.T.: 0.000 min  
 Response: 802328512  
 Conc: 462.20 ng/ml  
**Instrument:** ECD\_S  
**ClientSampleId :** HSTDICC500

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

## #3 4-Nitrophenol





R.T.: 7.001 min  
 Delta R.T.: 0.000 min  
 Response: 342629938  
 Conc: 459.86 ng/ml

## #4 2,4-DCAA

R.T.: 6.942 min  
 Delta R.T.: 0.000 min  
 Response: 1231780921  
 Conc: 512.53 ng/ml

## #4 2,4-DCAA

R.T.: 7.467 min  
 Delta R.T.: 0.000 min  
 Response: 346180636  
 Conc: 503.46 ng/ml

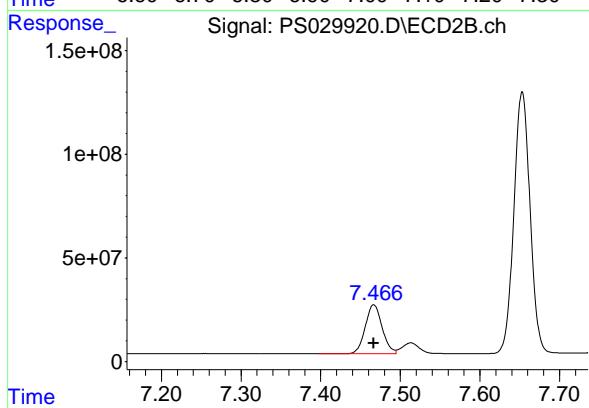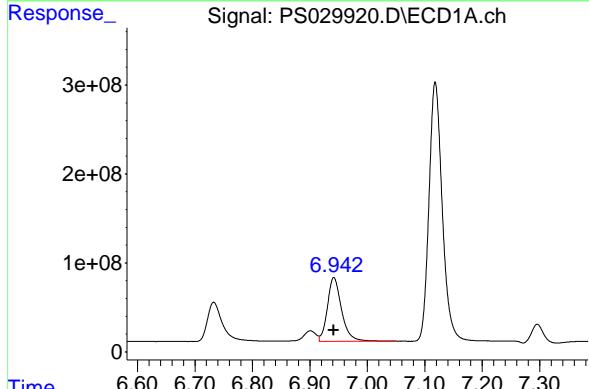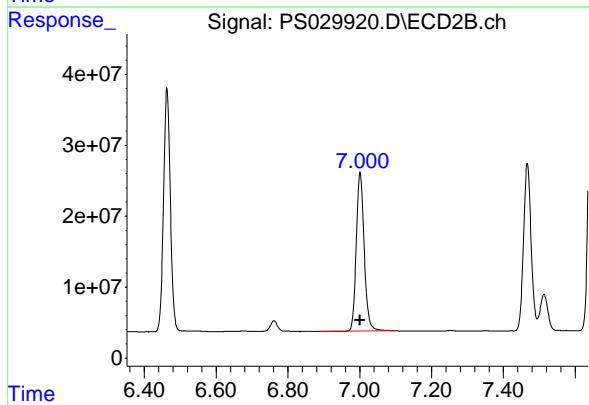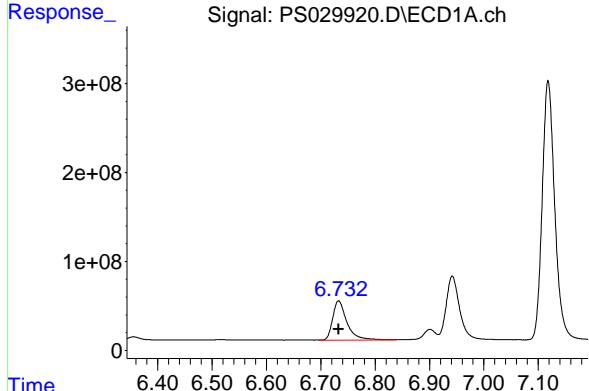

## #5 DICAMBA

R.T.: 7.118 min  
 Delta R.T.: 0.000 min  
 Response: 4642915948  
 Conc: 476.25 ng/ml  
 Instrument: ECD\_S  
 ClientSampleId : HSTDICC500

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

## #5 DICAMBA





R.T.: 7.653 min  
 Delta R.T.: 0.000 min  
 Response: 1792383950  
 Conc: 464.68 ng/ml

## #6 MCPP

R.T.: 7.296 min  
 Delta R.T.: 0.000 min  
 Response: 290670931  
 Conc: 45.92 ug/ml

## #6 MCPP

R.T.: 7.759 min  
 Delta R.T.: 0.000 min  
 Response: 82241844  
 Conc: 46.50 ug/ml

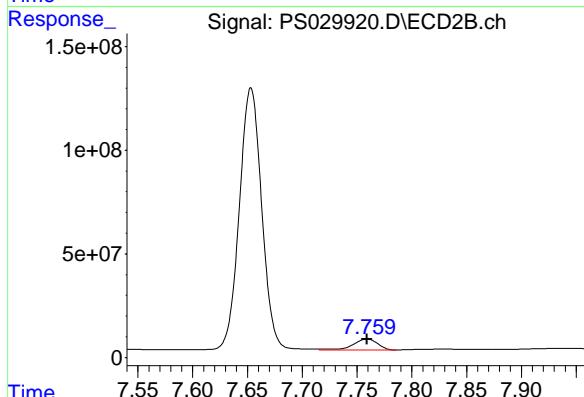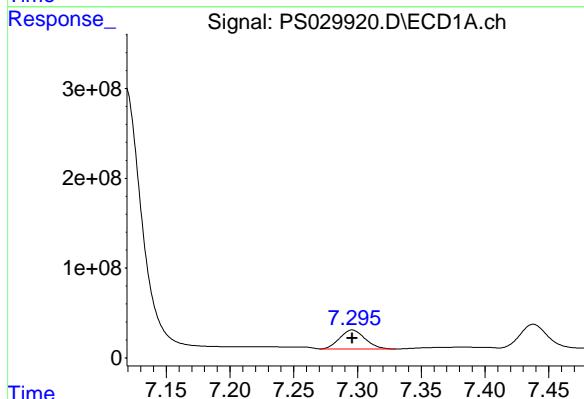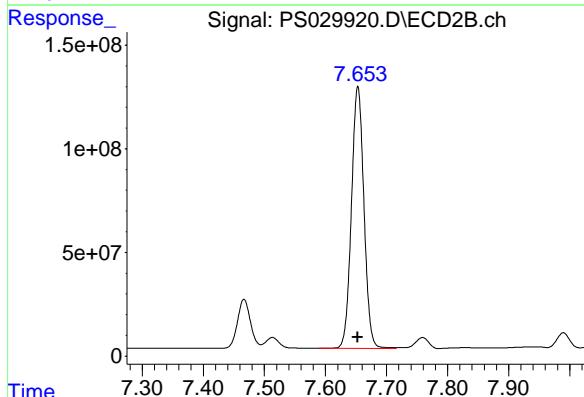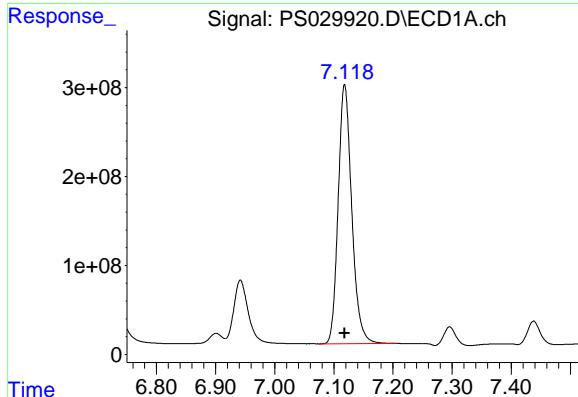

#7 MCPA

R.T.: 7.438 min  
 Delta R.T.: 0.000 min  
 Response: 399051123  
 Conc: 46.19 ug/ml  
 Instrument: ECD\_S  
 ClientSampleId : HSTDICC500

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

#7 MCPA





R.T.: 7.990 min  
 Delta R.T.: 0.000 min  
 Response: 105534297  
 Conc: 46.16 ug/ml

#8 DICHLORPROP

R.T.: 7.799 min  
 Delta R.T.: 0.000 min  
 Response: 1186769618  
 Conc: 480.56 ng/ml

#8 DICHLORPROP

R.T.: 8.347 min  
 Delta R.T.: 0.000 min  
 Response: 464258436  
 Conc: 473.76 ng/ml

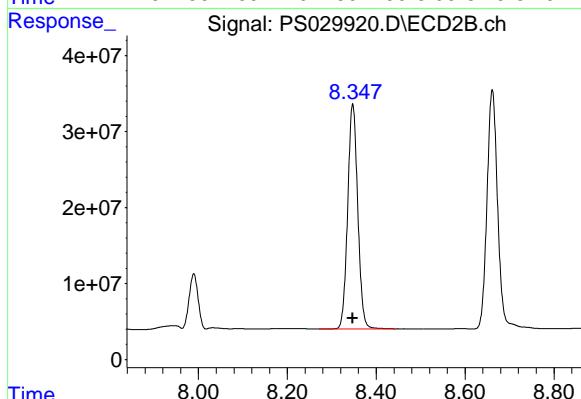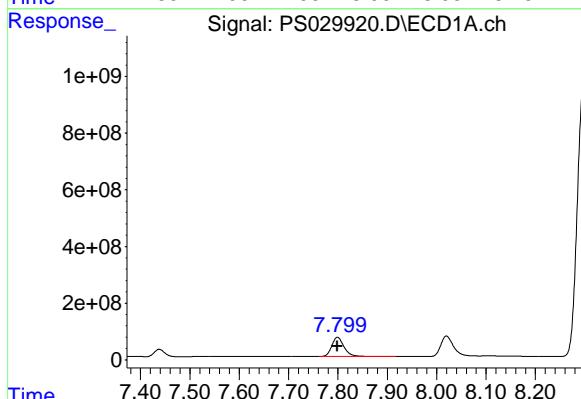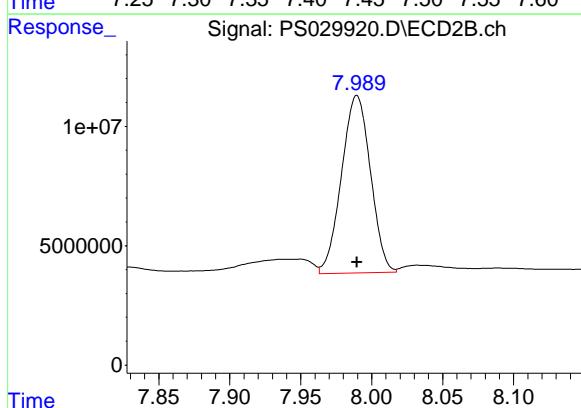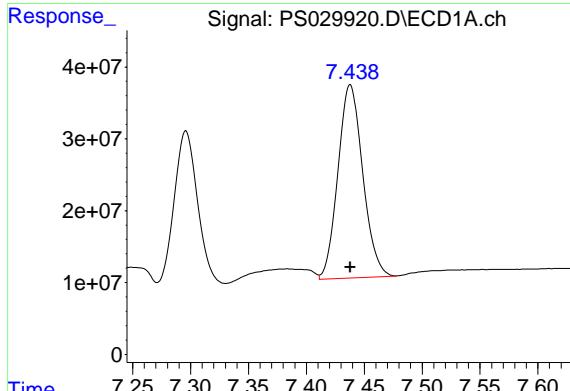

#9 2,4-D

R.T.: 8.020 min  
 Delta R.T.: 0.000 min  
 Response: 1315035111 Instrument:  
 Conc: 478.74 ng/ml ClientSampleId :  
 HSTDICC500

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

#9 2,4-D





R.T.: 8.661 min  
 Delta R.T.: 0.000 min  
 Response: 523223015  
 Conc: 474.74 ng/ml

#10 Pentachlorophenol

R.T.: 8.297 min  
 Delta R.T.: 0.000 min  
 Response: 16887638820  
 Conc: 483.73 ng/ml

#10 Pentachlorophenol

R.T.: 9.164 min  
 Delta R.T.: 0.000 min  
 Response: 9661508840  
 Conc: 476.54 ng/ml

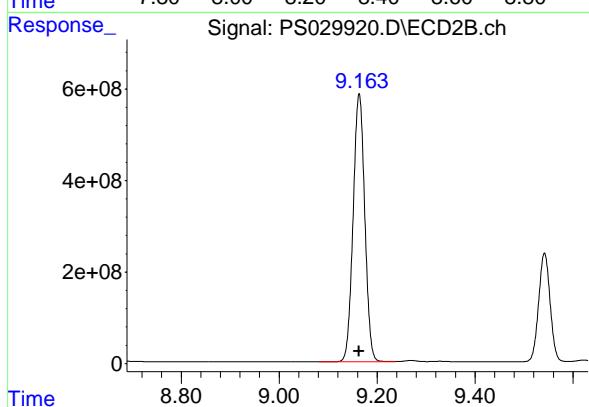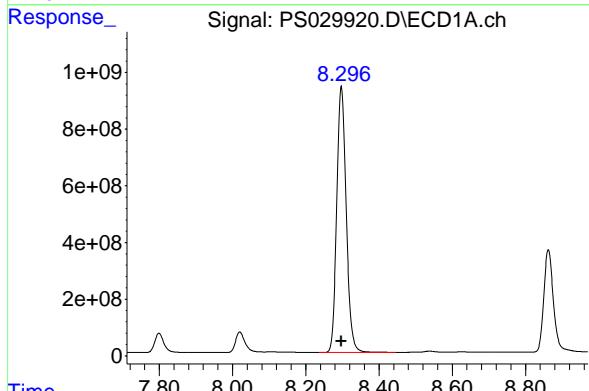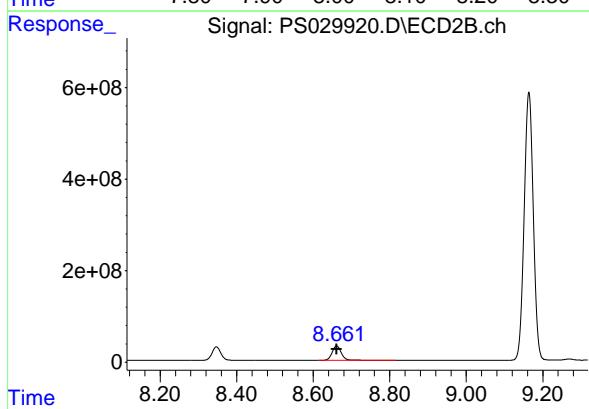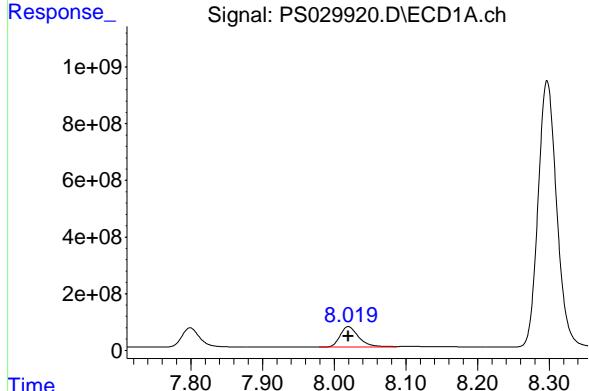

#11 2,4,5-TP (SILVEX)

R.T.: 8.862 min

Delta R.T.: 0.000 min

Instrument: ECD\_S


Response: 6584545232 ClientSampleId :

Conc: 482.50 ng/ml HSTDICC500

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025

Supervised By :mohammad ahmed 04/26/2025

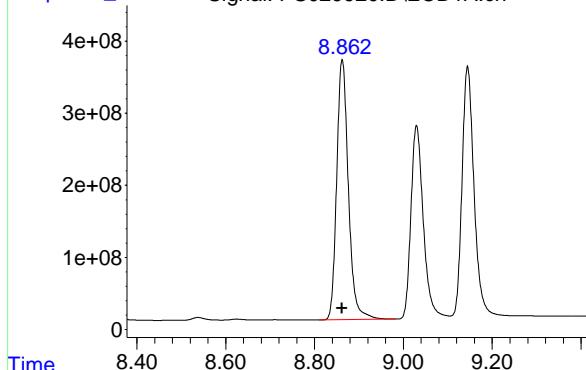


#11 2,4,5-TP (SILVEX)

R.T.: 9.542 min

Delta R.T.: 0.000 min

Response: 3838568800

Conc: 475.11 ng/ml

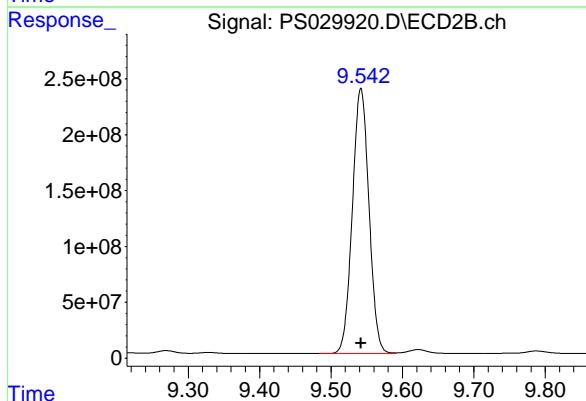


#12 2,4,5-T

R.T.: 9.145 min

Delta R.T.: 0.000 min

Response: 6674392581

Conc: 482.99 ng/ml

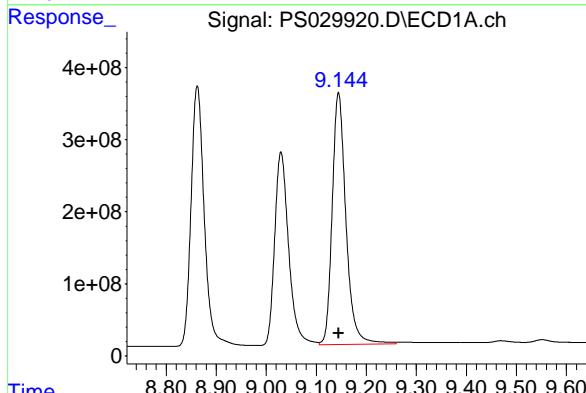


#12 2,4,5-T

R.T.: 9.948 min

Delta R.T.: 0.000 min

Response: 3641908671

Conc: 476.22 ng/ml

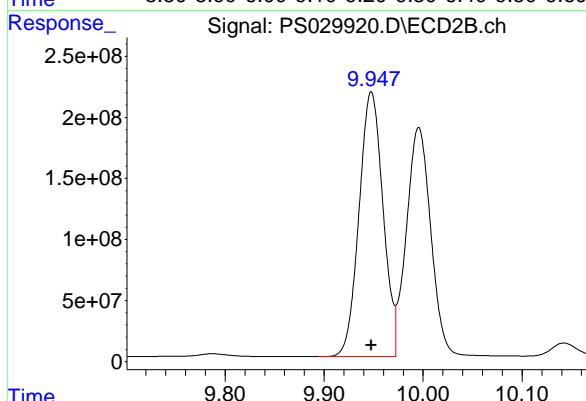

#13 2,4-DB

R.T.: 9.703 min  
 Delta R.T.: 0.000 min  
 Response: 1071085603  
 Conc: 478.62 ng/ml  
 Instrument: ECD\_S  
 ClientSampleId : HSTDICC500

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

#13 2,4-DB





R.T.: 10.507 min  
 Delta R.T.: 0.000 min  
 Response: 362659677  
 Conc: 465.16 ng/ml

#14 DINOSEB


R.T.: 10.866 min  
 Delta R.T.: 0.000 min  
 Response: 4764255395  
 Conc: 475.55 ng/ml

#14 DINOSEB

R.T.: 10.881 min  
 Delta R.T.: 0.000 min  
 Response: 2699322247  
 Conc: 471.42 ng/ml

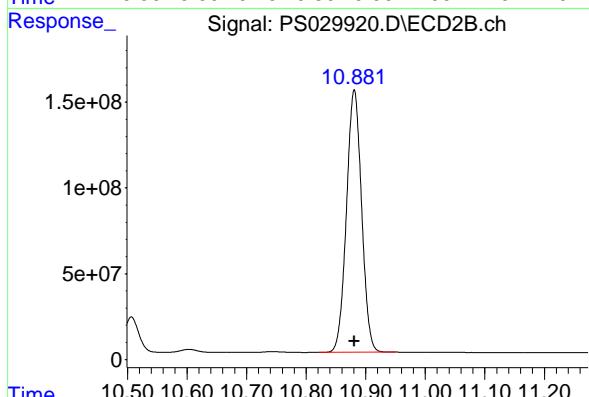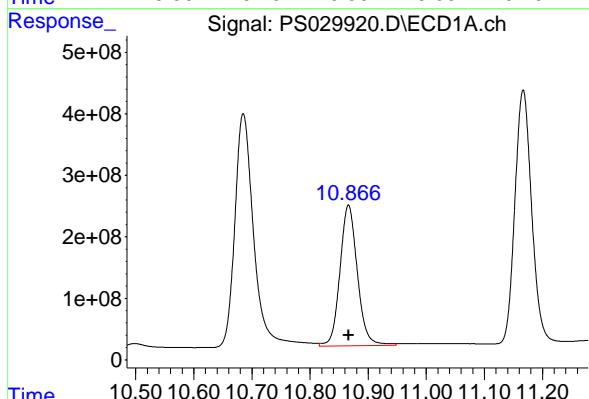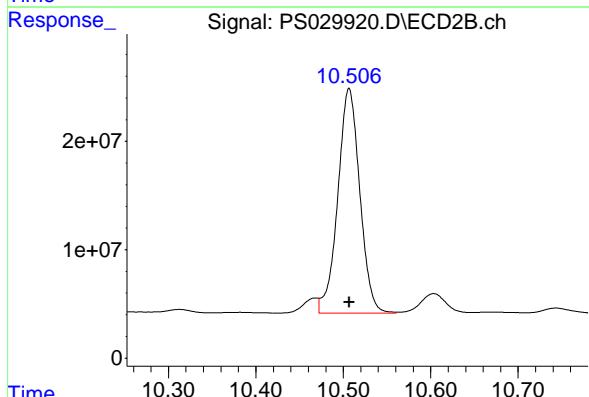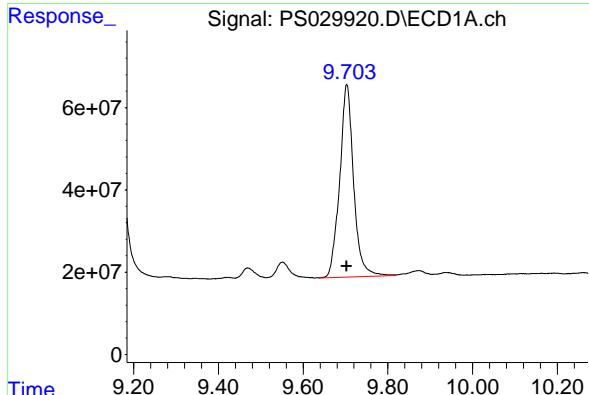

#15 Picloram

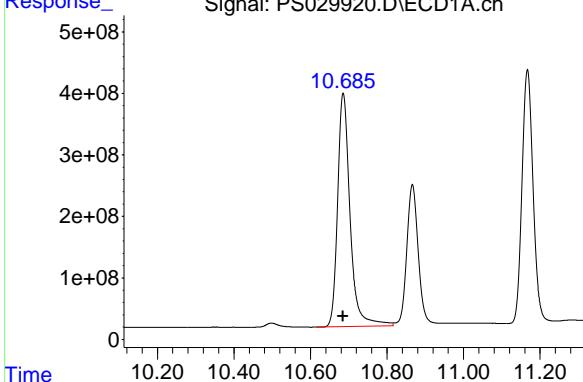

R.T.: 10.685 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_S  
Response: 8585191140  
Conc: 477.89 ng/ml  
ClientSampleId: HSTDICC500

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 04/24/2025  
Supervised By :mohammad ahmed 04/26/2025

#15 Picloram



R.T.: 11.923 min  
Delta R.T.: 0.000 min  
Response: 5454177256  
Conc: 452.16 ng/ml

#16 DCPA

R.T.: 11.167 min  
Delta R.T.: 0.000 min  
Response: 8208335626  
Conc: 488.03 ng/ml

#16 DCPA

R.T.: 11.919 min  
Delta R.T.: 0.000 min  
Response: 5573532100  
Conc: 495.90 ng/ml

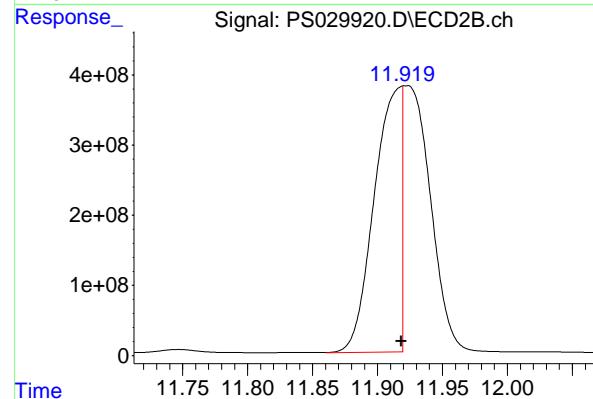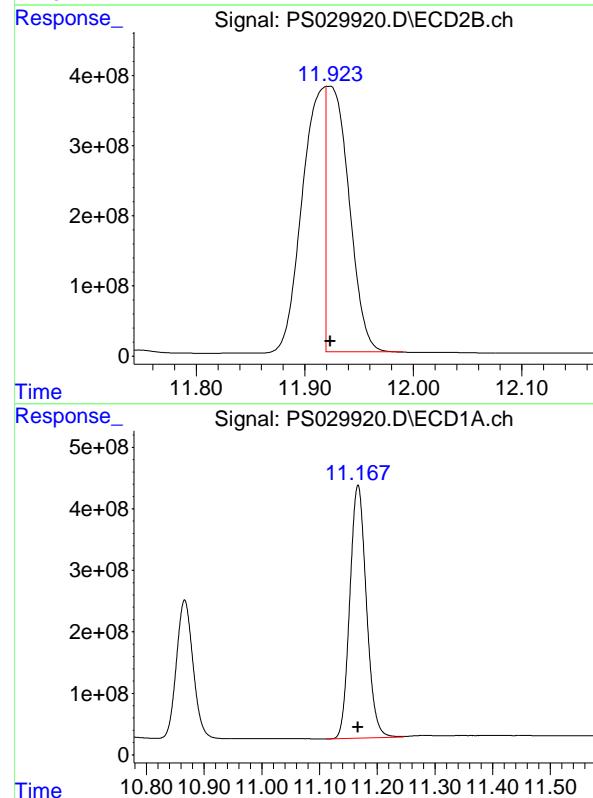

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029921.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 11:49  
 Operator : AR\AJ  
 Sample : HSTDICC750  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**HSTDICC750**

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 12:13:23 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:13:04 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

4) S 2,4-DCAA 6.942 7.467 1757.3E6 512.1E6 750.000 750.000

**Target Compounds**

1) T	Dalapon	2.449	2.525	2731.3E6	1134.3E6	682.500	682.500
2) T	3,5-DICHL...	6.146	6.463	2388.4E6	661.4E6	697.500	697.500
3) T	4-Nitroph...	6.732	7.001	1166.0E6	503.1E6	682.500	682.500
5) T	DICAMBA	7.118	7.653	6781.5E6	2750.1E6	705.000	705.000
6) T	MCPP	7.297	7.761	456.6E6	126.0E6	70.500	70.500
7) T	MCPA	7.440	7.991	606.7E6	160.7E6	69.750	69.750
8) T	DICHLORPROP	7.799	8.348	1701.9E6	685.3E6	705.000	705.000
9) T	2,4-D	8.019	8.661	1900.5E6	769.2E6	705.000	705.000
10) T	Pentachlo...	8.297	9.163	24416.7E6	14398.4E6	712.500	712.500
11) T	2,4,5-TP ...	8.862	9.542	9569.8E6	5755.2E6	712.500	712.500
12) T	2,4,5-T	9.144	9.947	9680.3E6	5434.8E6	712.500	712.500
13) T	2,4-DB	9.703	10.507	1582.3E6	567.0E6	712.500	712.500
14) T	DINOSEB	10.866	10.881	6979.6E6	4024.5E6	705.000	705.000
15) T	Picloram	10.685	11.920	12721.8E6	8674.9E6	712.500	724.031m
16) T	DCPA	11.166	11.918	11907.4E6	8089.3E6	720.000	728.090m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029921.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 11:49  
 Operator : AR\AJ  
 Sample : HSTDICC750  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1



Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDICC750





**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 12:13:23 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:13:04 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

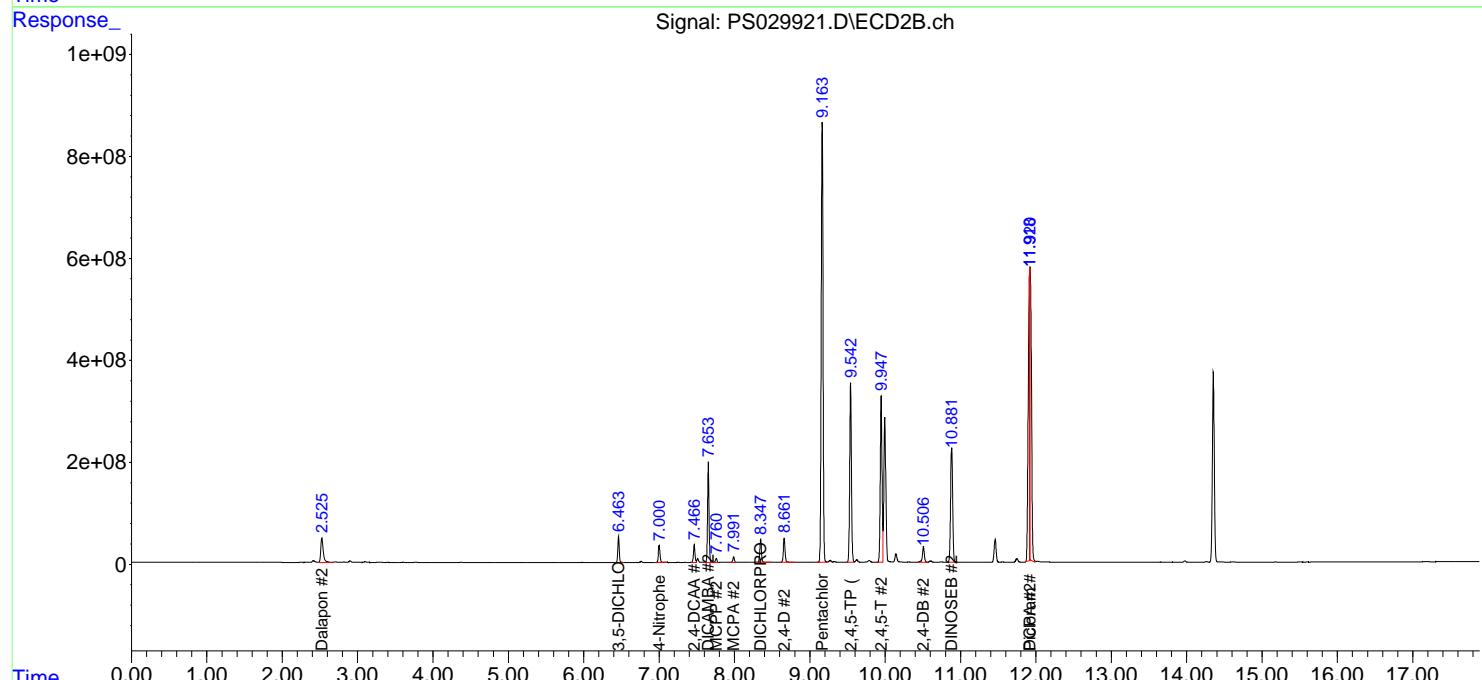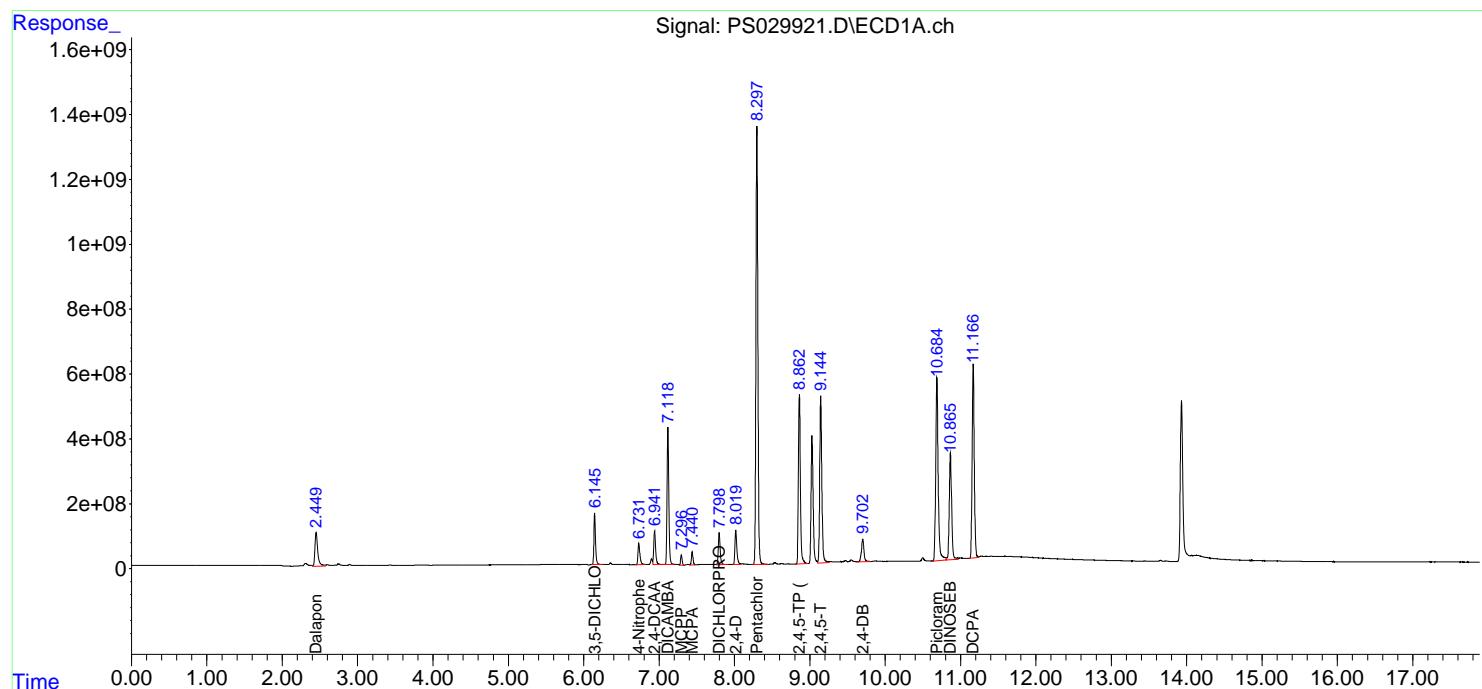

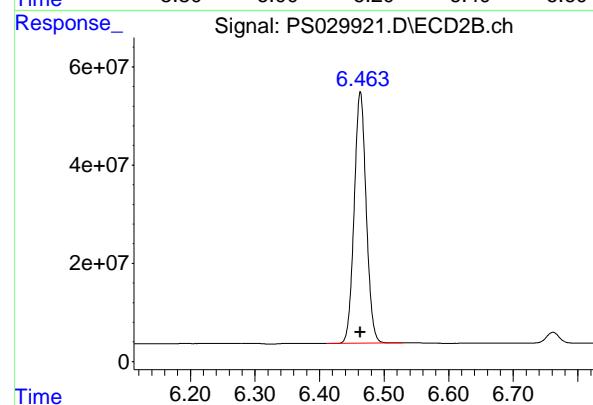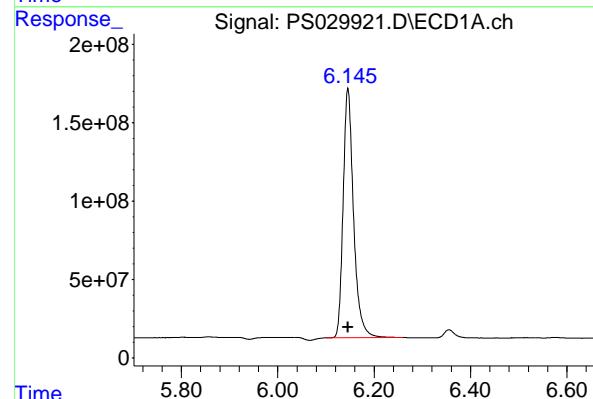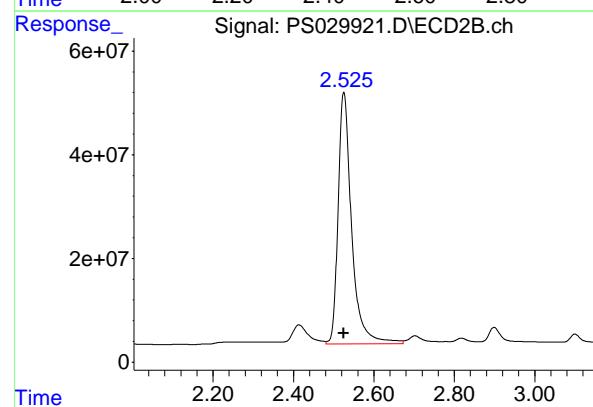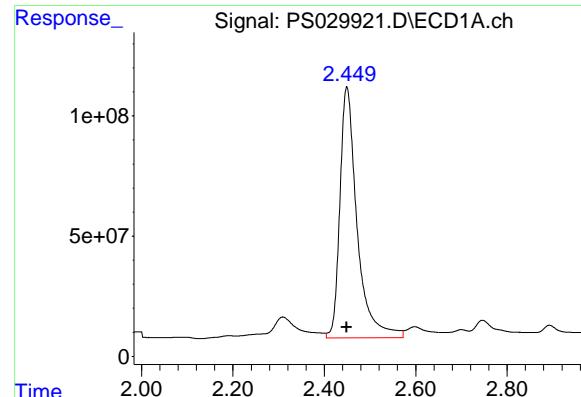

#1 Dalapon

R.T.: 2.449 min  
 Delta R.T.: 0.000 min  
 Response: 2731274284 ECD\_S  
 Conc: 682.50 ng/ml ClientSampleId : HSTDICC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

#1 Dalapon

R.T.: 2.525 min  
 Delta R.T.: 0.000 min  
 Response: 1134264471  
 Conc: 682.50 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.146 min  
 Delta R.T.: 0.000 min  
 Response: 2388375809  
 Conc: 697.50 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.463 min  
 Delta R.T.: 0.000 min  
 Response: 661411771  
 Conc: 697.50 ng/ml

## #3 4-Nitrophenol

R.T.: 6.732 min  
 Delta R.T.: 0.000 min  
 Response: 1165994997  
 Conc: 682.50 ng/ml  
 Instrument: ECD\_S  
 ClientSampleId : HSTDICC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

## #3 4-Nitrophenol





R.T.: 7.001 min  
 Delta R.T.: 0.000 min  
 Response: 503078374  
 Conc: 682.50 ng/ml





## #4 2,4-DCAA

R.T.: 6.942 min  
 Delta R.T.: 0.000 min  
 Response: 1757314349  
 Conc: 750.00 ng/ml

## #4 2,4-DCAA

R.T.: 7.467 min  
 Delta R.T.: 0.000 min  
 Response: 512143835  
 Conc: 750.00 ng/ml

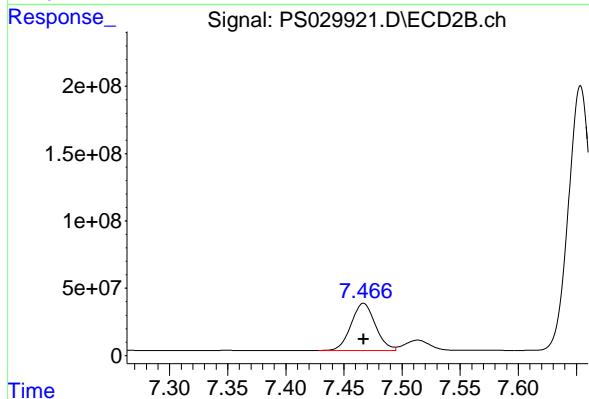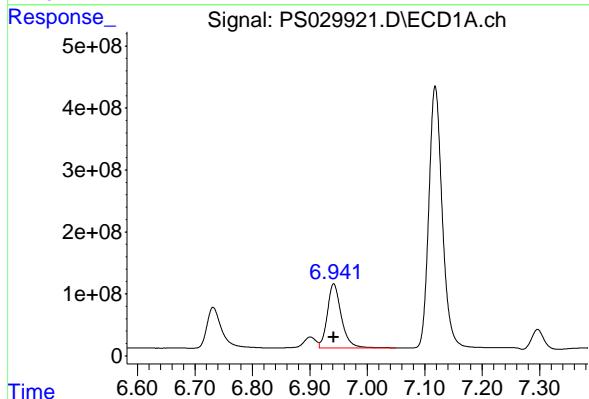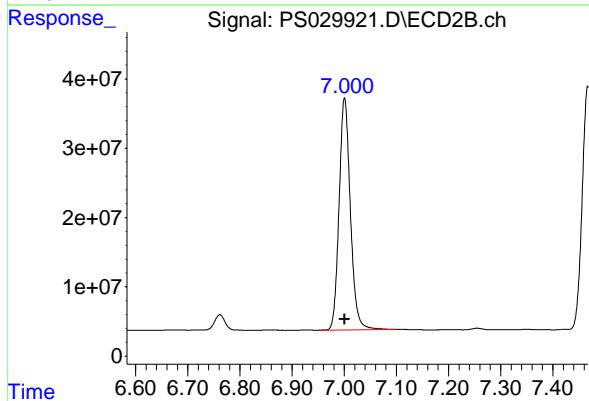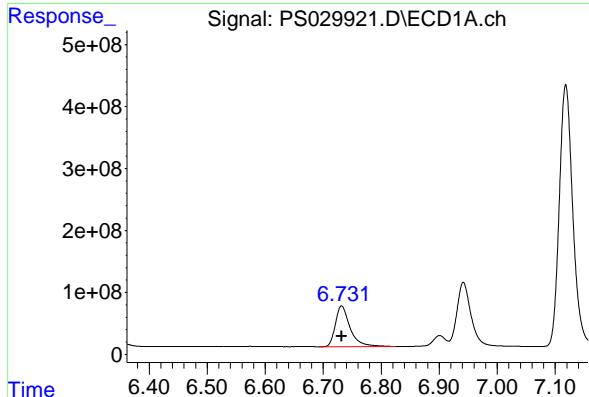

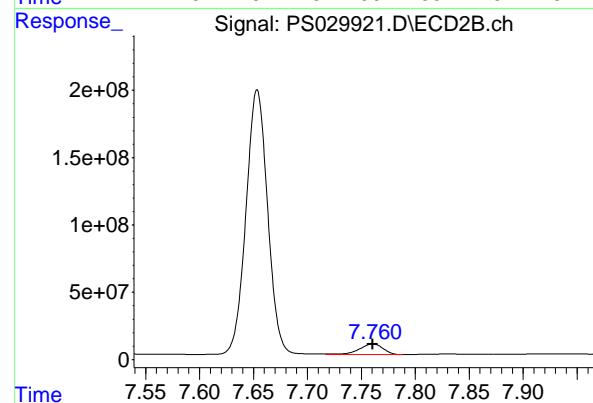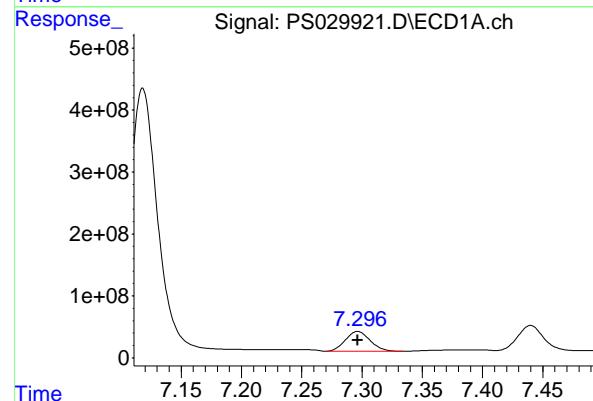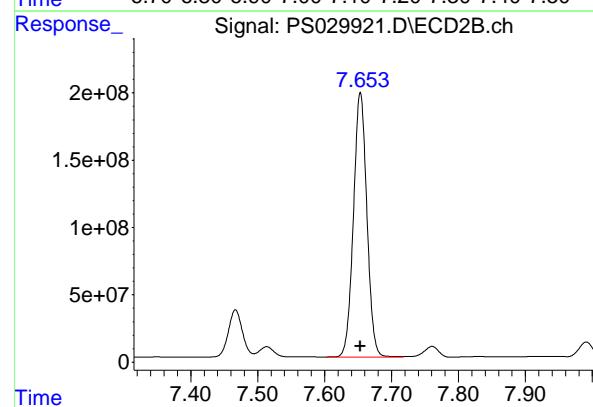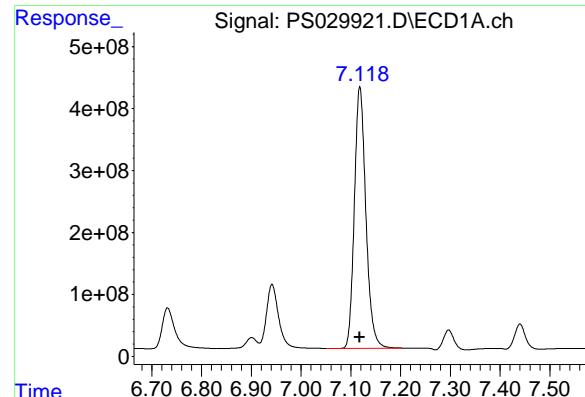

## #5 DICAMBA

R.T.: 7.118 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_S  
Response: 6781538346  
Conc: 705.00 ng/ml  
ClientSampleId: HSTDICC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 04/24/2025  
Supervised By :mohammad ahmed 04/26/2025

## #5 DICAMBA

R.T.: 7.653 min  
Delta R.T.: 0.000 min  
Response: 2750105949  
Conc: 705.00 ng/ml

## #6 MCPP

R.T.: 7.297 min  
Delta R.T.: 0.000 min  
Response: 456554341  
Conc: 70.50 ug/ml

## #6 MCPP

R.T.: 7.761 min  
Delta R.T.: 0.000 min  
Response: 126016285  
Conc: 70.50 ug/ml

#7 MCPA

R.T.: 7.440 min  
 Delta R.T.: 0.000 min  
 Response: 606675377  
 Conc: 69.75 ug/ml  
 Instrument: ECD\_S  
 ClientSampleId : HSTDICC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

#7 MCPA





R.T.: 7.991 min  
 Delta R.T.: 0.000 min  
 Response: 160659432  
 Conc: 69.75 ug/ml

#8 DICHLORPROP

R.T.: 7.799 min  
 Delta R.T.: 0.000 min  
 Response: 1701892611  
 Conc: 705.00 ng/ml

#8 DICHLORPROP

R.T.: 8.348 min  
 Delta R.T.: 0.000 min  
 Response: 685337493  
 Conc: 705.00 ng/ml

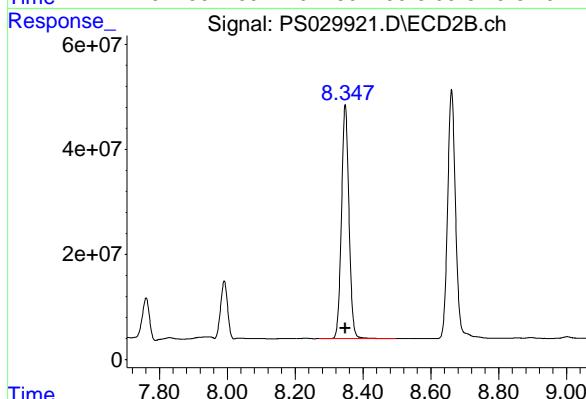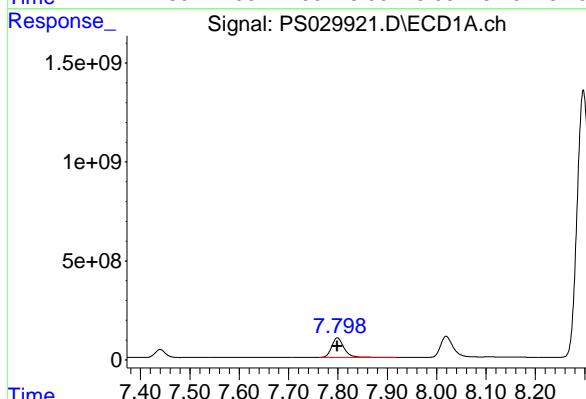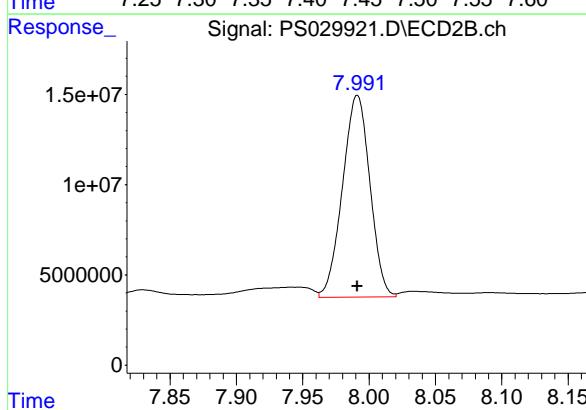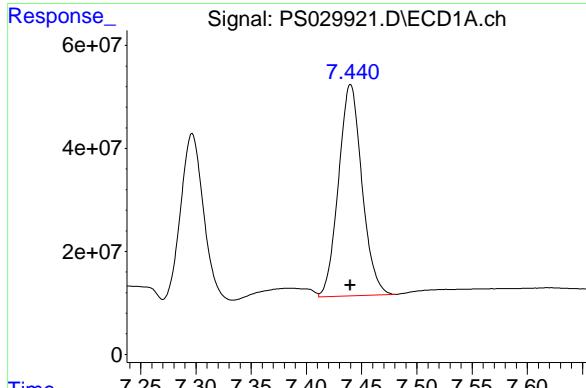

#9 2,4-D

R.T.: 8.019 min  
 Delta R.T.: 0.000 min  
 Response: 1900496204 ECD\_S  
 Conc: 705.00 ng/ml Client SampleId : HSTDICC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

#9 2,4-D





R.T.: 8.661 min  
 Delta R.T.: 0.000 min  
 Response: 769155125  
 Conc: 705.00 ng/ml

#10 Pentachlorophenol

R.T.: 8.297 min  
 Delta R.T.: 0.000 min  
 Response: 24416691751  
 Conc: 712.50 ng/ml

#10 Pentachlorophenol

R.T.: 9.163 min  
 Delta R.T.: 0.000 min  
 Response: 14398444463  
 Conc: 712.50 ng/ml

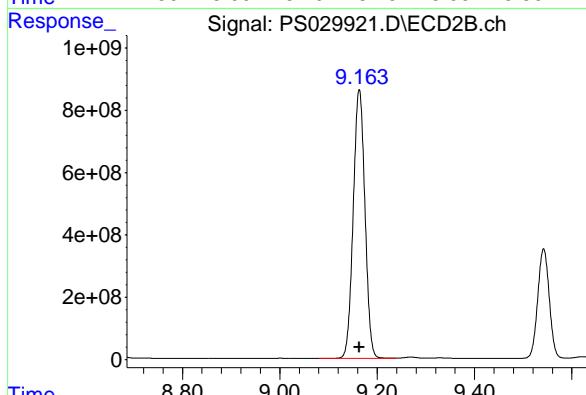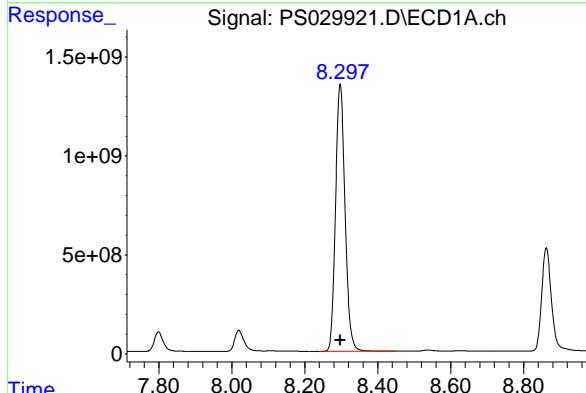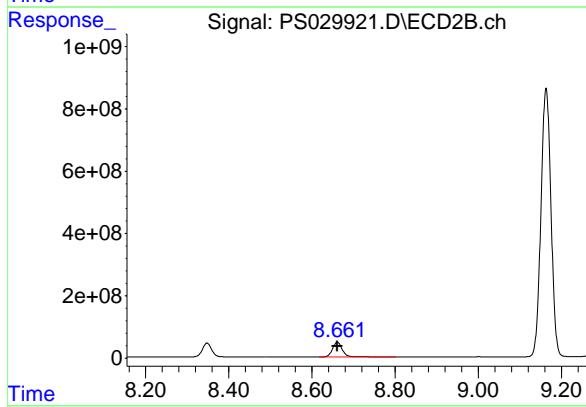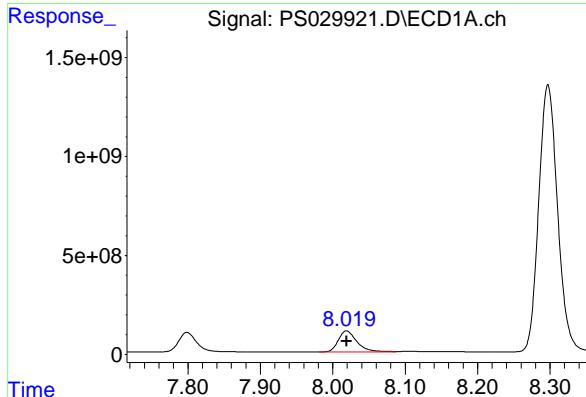

#11 2,4,5-TP (SILVEX)

R.T.: 8.862 min

Delta R.T.: 0.000 min

Instrument: ECD\_S


Response: 9569830576 ClientSampleId :

Conc: 712.50 ng/ml HSTDICC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025

Supervised By :mohammad ahmed 04/26/2025

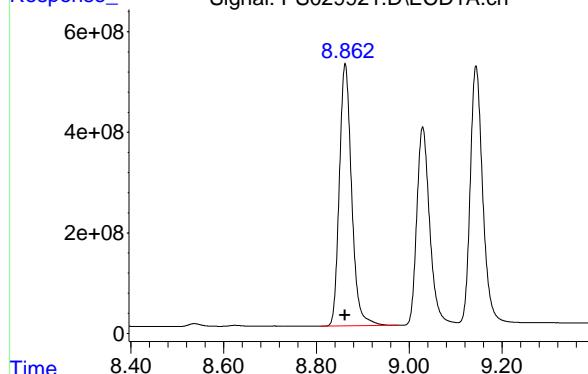


#11 2,4,5-TP (SILVEX)

R.T.: 9.542 min

Delta R.T.: 0.000 min

Response: 5755245929

Conc: 712.50 ng/ml

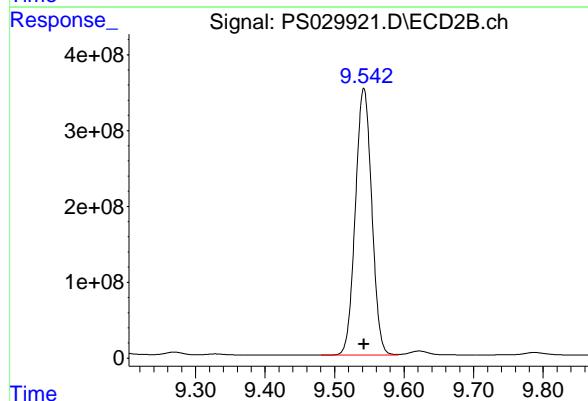


#12 2,4,5-T

R.T.: 9.144 min

Delta R.T.: 0.000 min

Response: 9680261593

Conc: 712.50 ng/ml

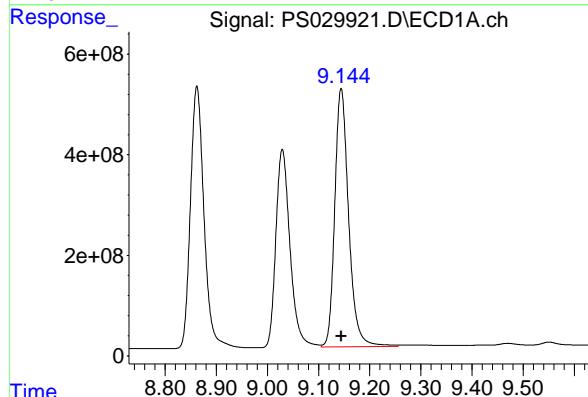


#12 2,4,5-T

R.T.: 9.947 min

Delta R.T.: 0.000 min

Response: 5434774786

Conc: 712.50 ng/ml

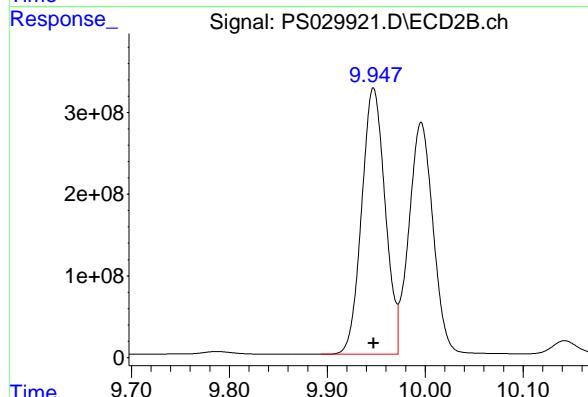

#13 2,4-DB

R.T.: 9.703 min  
 Delta R.T.: 0.000 min  
 Response: 1582337187 ECD\_S  
 Conc: 712.50 ng/ml ClientSampleId : HSTDICC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

#13 2,4-DB





R.T.: 10.507 min  
 Delta R.T.: 0.000 min  
 Response: 567000464  
 Conc: 712.50 ng/ml

#14 DINOSEB

R.T.: 10.866 min  
 Delta R.T.: 0.000 min  
 Response: 6979616298  
 Conc: 705.00 ng/ml

#14 DINOSEB

R.T.: 10.881 min  
 Delta R.T.: 0.000 min  
 Response: 4024544896  
 Conc: 705.00 ng/ml

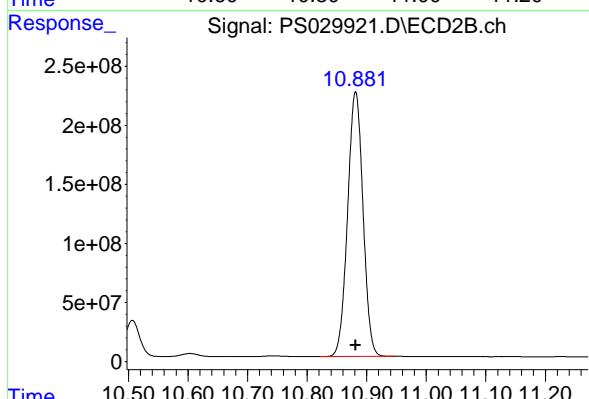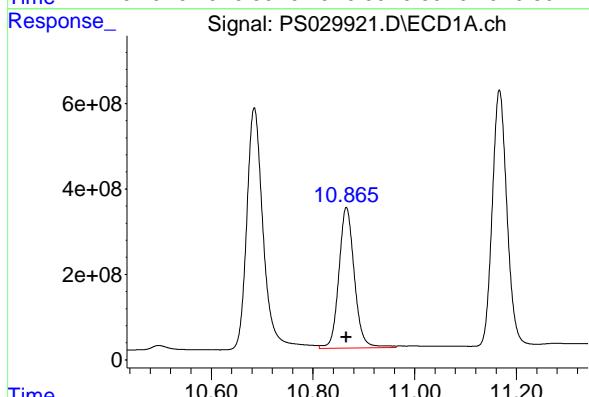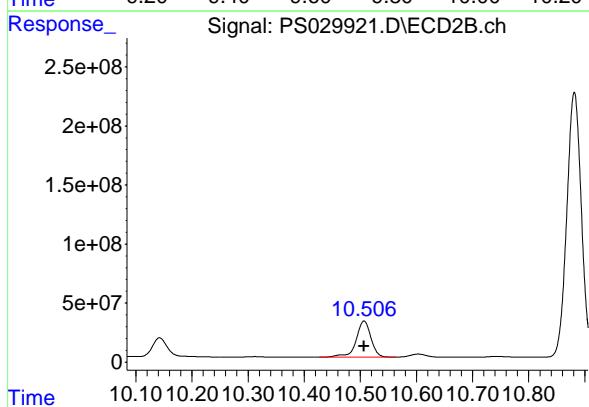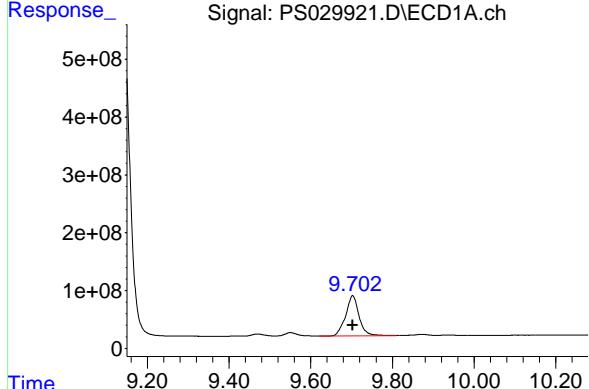

## #15 Picloram

R.T.: 10.685 min  
 Delta R.T.: 0.000 min  
 Response: 12721770760  
 Instrument: ECD\_S  
 Conc: 712.50 ng/ml  
 ClientSampleId : HSTDICC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

## #15 Picloram





R.T.: 11.920 min  
 Delta R.T.: 0.000 min  
 Response: 8674908222  
 Conc: 724.03 ng/ml

## #16 DCPA

R.T.: 11.166 min  
 Delta R.T.: 0.000 min  
 Response: 11907371025  
 Conc: 720.00 ng/ml

## #16 DCPA

R.T.: 11.918 min  
 Delta R.T.: 0.000 min  
 Response: 8089285607  
 Conc: 728.09 ng/ml

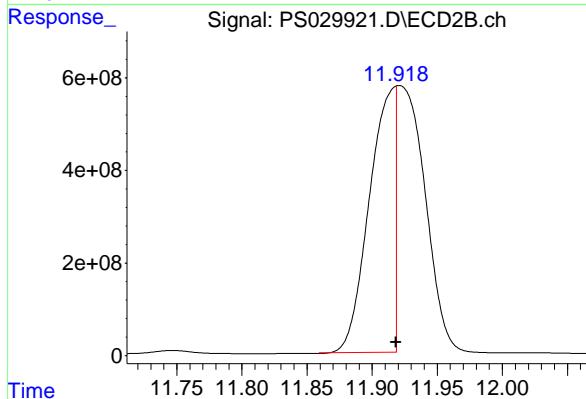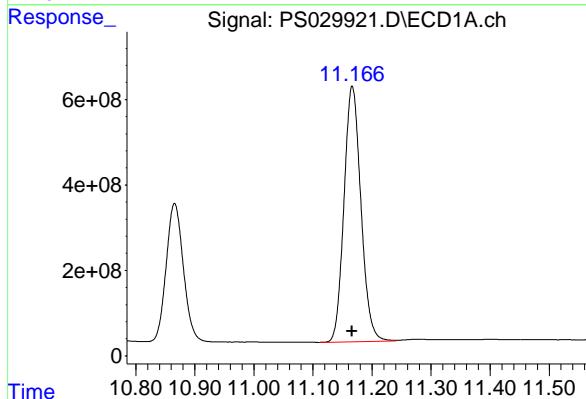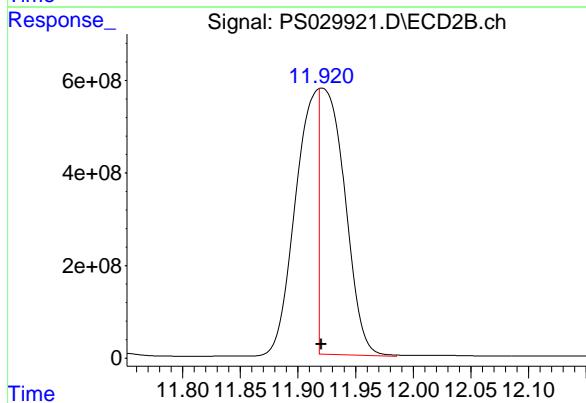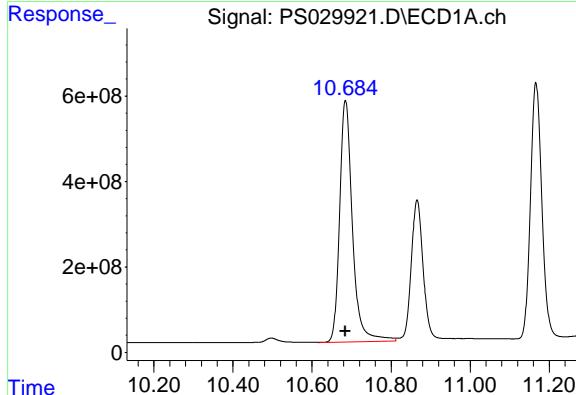

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029922.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 12:13  
 Operator : AR\AJ  
 Sample : HSTDICC1000  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**HSTDICC1000**

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 12:41:26 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:41:18 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

4) S 2,4-DCAA 6.941 7.466 2233.7E6 662.0E6 886.503 930.792

**Target Compounds**

1) T	Dalapon	2.448	2.524	3459.2E6	1450.3E6	829.350	821.672
2) T	3,5-DICHL...	6.145	6.463	3047.9E6	855.5E6	835.452	867.026
3) T	4-Nitroph...	6.731	7.000	1500.3E6	650.1E6	830.199	840.006
5) T	DICAMBA	7.118	7.652	8709.4E6	3622.0E6	866.580	923.531
6) T	MCPP	7.297	7.761	613.1E6	163.4E6	97.394	94.159
7) T	MCPA	7.440	7.992	802.4E6	212.9E6	91.664	89.703
8) T	DICHLORPROP	7.798	8.347	2167.0E6	881.3E6	837.398	868.054
9) T	2,4-D	8.018	8.661	2435.4E6	991.5E6	849.738	870.102
10) T	Pentachlo...	8.297	9.163	31038.8E6	18517.9E6	864.019	901.215
11) T	2,4,5-TP ...	8.862	9.542	12264.9E6	7478.1E6	869.588	909.959
12) T	2,4,5-T	9.144	9.947	12428.5E6	7054.1E6	868.738	903.059
13) T	2,4-DB	9.702	10.506	2059.3E6	737.5E6	896.524	916.649
14) T	DINOSEB	10.866	10.881	8807.7E6	5194.8E6	849.671	883.604
15) T	Picloram	10.685	11.920	16510.1E6	11094.8E6	892.660	889.281m
16) T	DCPA	11.166	11.918	15201.9E6	10311.4E6	876.317	906.507m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029922.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 12:13  
 Operator : AR\AJ  
 Sample : HSTDICC1000  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1



Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDICC1000

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 12:41:26 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:41:18 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

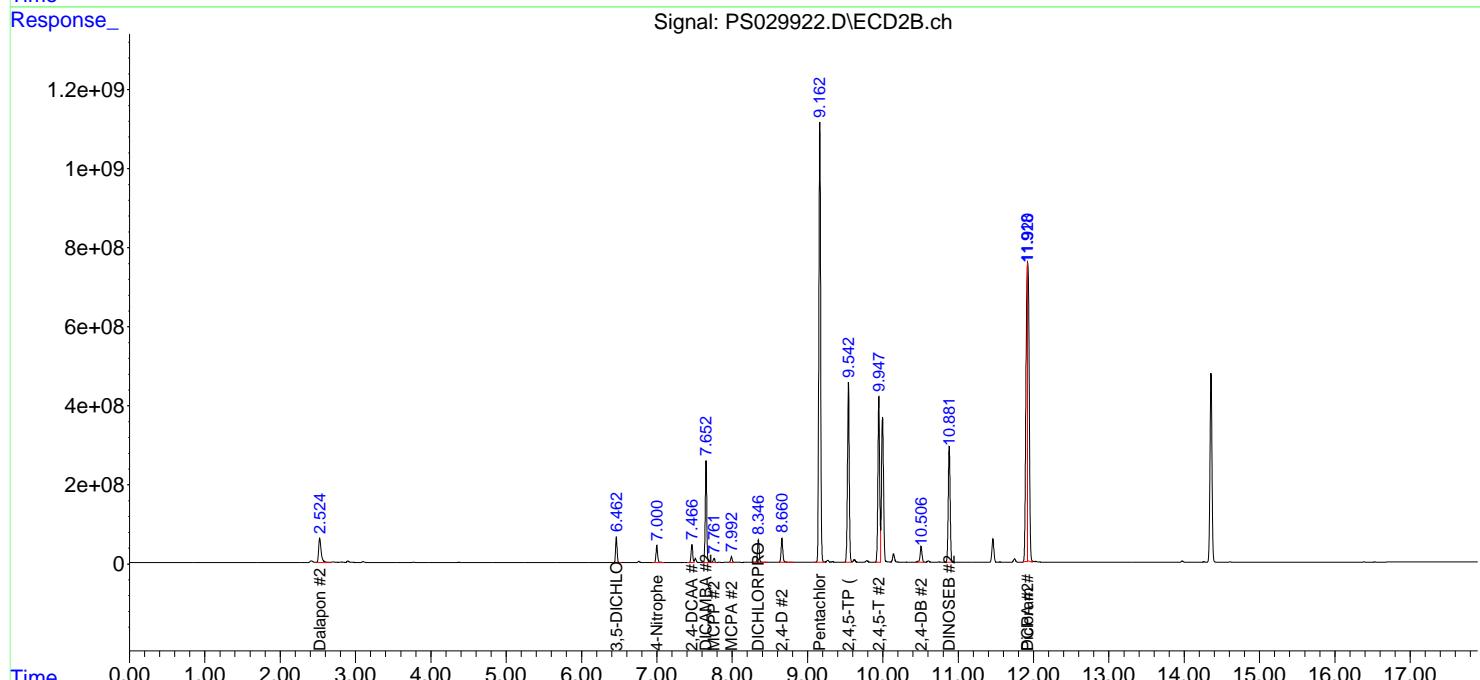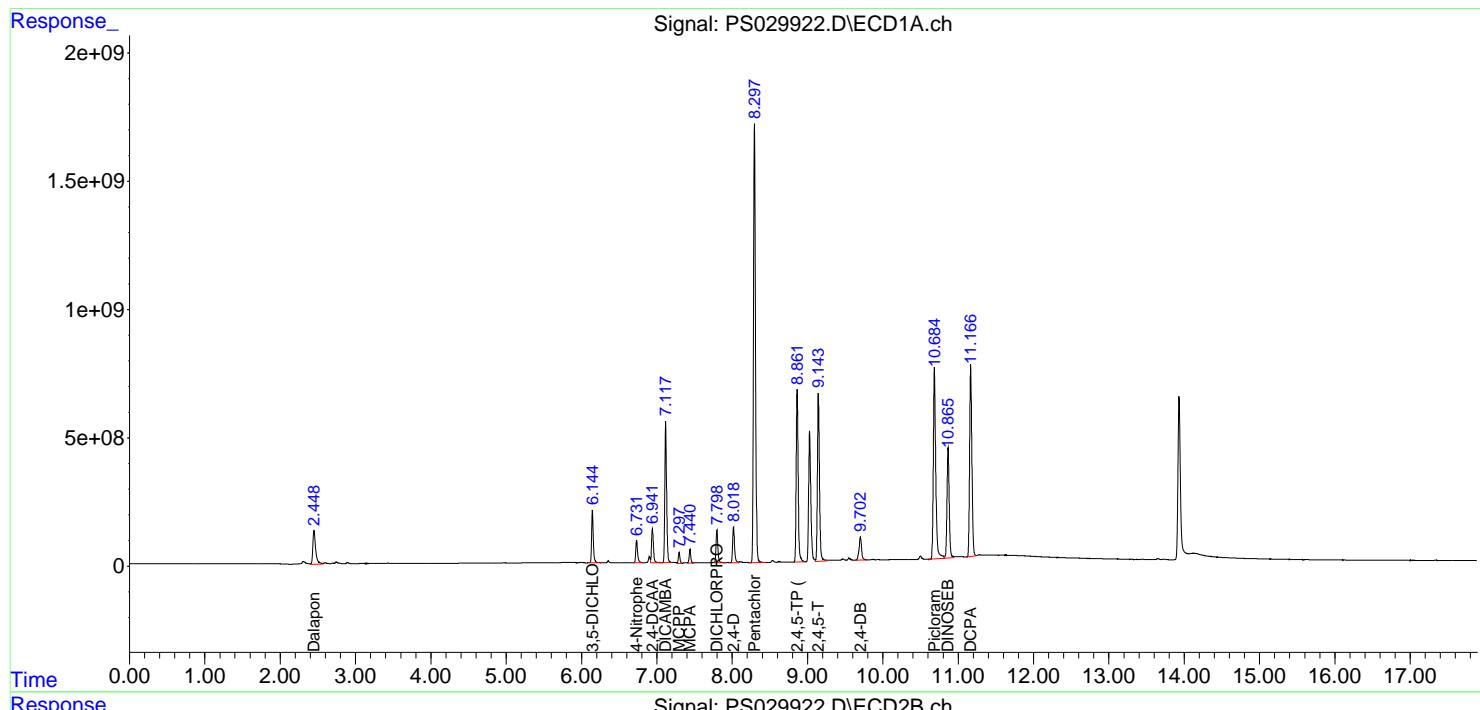

## #1 Dalapon

R.T.: 2.448 min  
 Delta R.T.: 0.000 min  
 Response: 3459192542  
 Conc: 829.35 ng/ml  
 Instrument: ECD\_S  
 ClientSampleId : HSTDICC1000

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

## #1 Dalapon





R.T.: 2.524 min  
 Delta R.T.: 0.000 min  
 Response: 1450275646  
 Conc: 821.67 ng/ml

## #2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.145 min  
 Delta R.T.: 0.000 min  
 Response: 3047853600  
 Conc: 835.45 ng/ml

## #2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.463 min  
 Delta R.T.: 0.000 min  
 Response: 855462143  
 Conc: 867.03 ng/ml

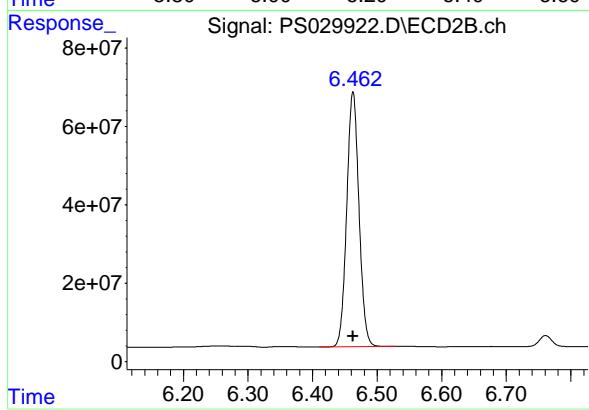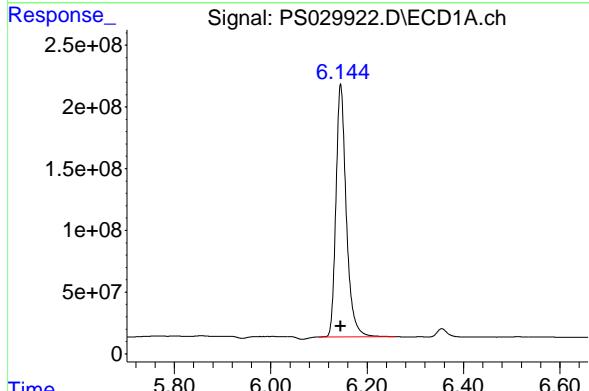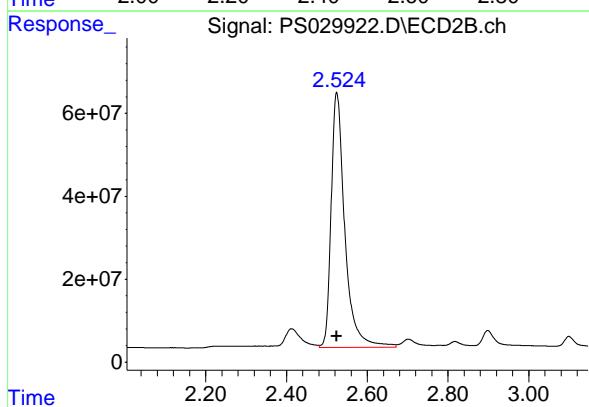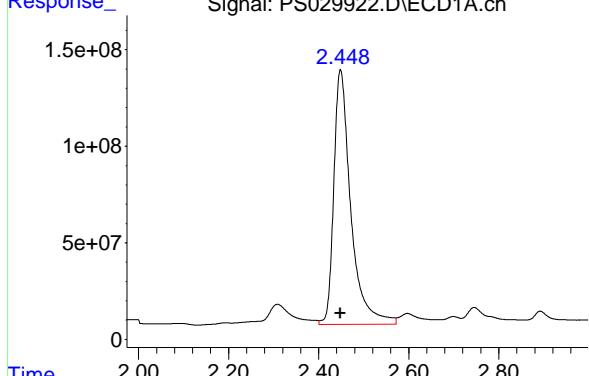

## #3 4-Nitrophenol

R.T.: 6.731 min  
 Delta R.T.: 0.000 min  
 Response: 1500313179 ECD\_S  
 Conc: 830.20 ng/ml ClientSampleId : HSTDICC1000

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

## #3 4-Nitrophenol





R.T.: 7.000 min  
 Delta R.T.: 0.000 min  
 Response: 650145921  
 Conc: 840.01 ng/ml

## #4 2,4-DCAA

R.T.: 6.941 min  
 Delta R.T.: 0.000 min  
 Response: 2233667943  
 Conc: 886.50 ng/ml

## #4 2,4-DCAA

R.T.: 7.466 min  
 Delta R.T.: 0.000 min  
 Response: 661990920  
 Conc: 930.79 ng/ml

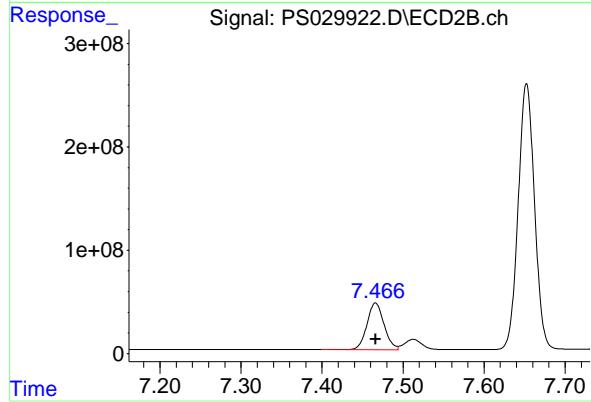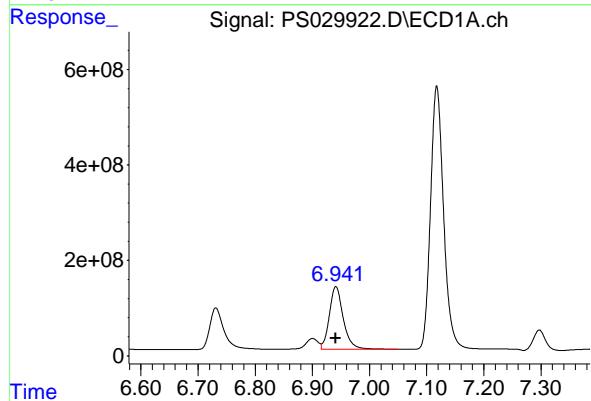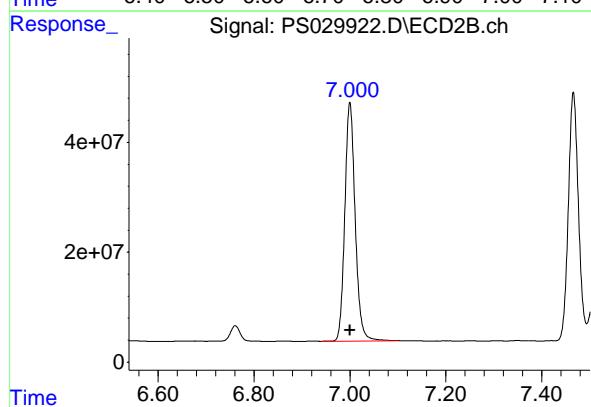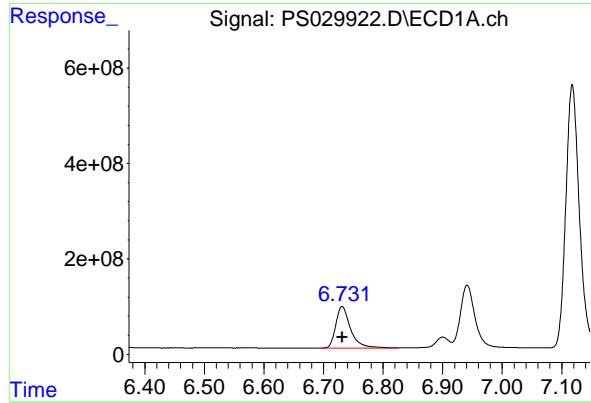

## #5 DICAMBA

R.T.: 7.118 min  
 Delta R.T.: 0.000 min  
 Response: 8709449271 ECD\_S  
 Conc: 866.58 ng/ml ClientSampleId : HSTDICC1000

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

## #5 DICAMBA





R.T.: 7.652 min  
 Delta R.T.: 0.000 min  
 Response: 3622048735  
 Conc: 923.53 ng/ml

## #6 MCPP

R.T.: 7.297 min  
 Delta R.T.: 0.000 min  
 Response: 613146849  
 Conc: 97.39 ug/ml

## #6 MCPP

R.T.: 7.761 min  
 Delta R.T.: 0.000 min  
 Response: 163368164  
 Conc: 94.16 ug/ml

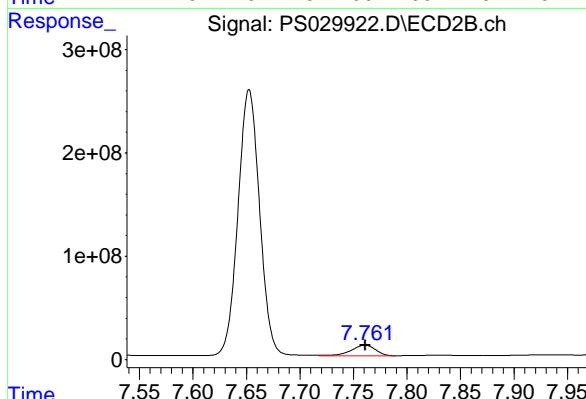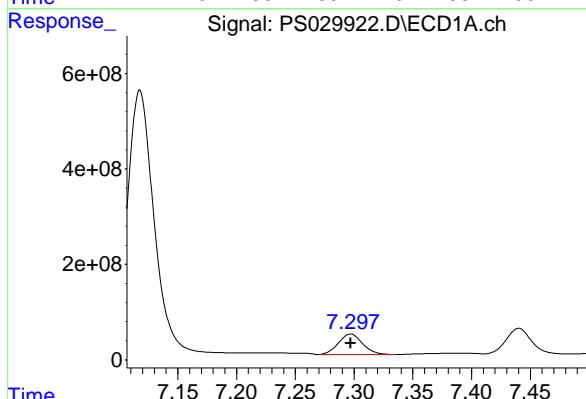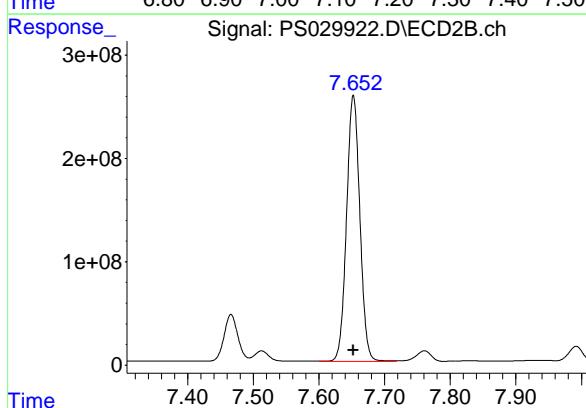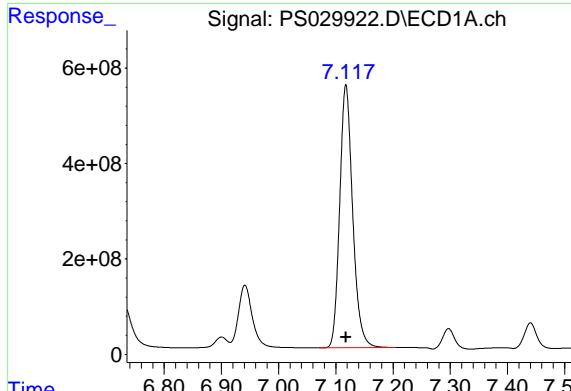

#7 MCPA

R.T.: 7.440 min  
 Delta R.T.: 0.000 min  
 Response: 802417459  
 Conc: 91.66 ug/ml  
 Instrument: ECD\_S  
 ClientSampleId : HSTDICC1000

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

#7 MCPA



R.T.: 7.992 min  
 Delta R.T.: 0.000 min  
 Response: 212857828  
 Conc: 89.70 ug/ml

#8 DICHLORPROP

R.T.: 7.798 min  
 Delta R.T.: 0.000 min  
 Response: 2167004704  
 Conc: 837.40 ng/ml

#8 DICHLORPROP

R.T.: 8.347 min  
 Delta R.T.: 0.000 min  
 Response: 881253779  
 Conc: 868.05 ng/ml

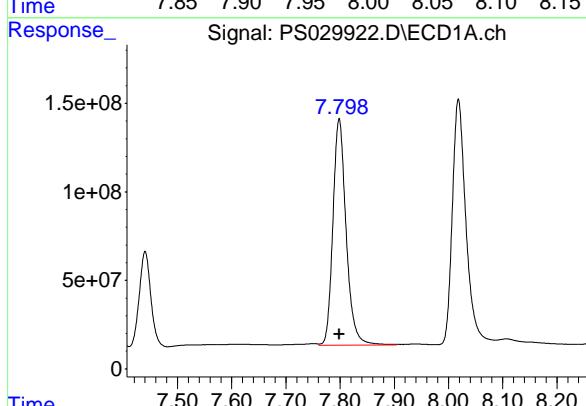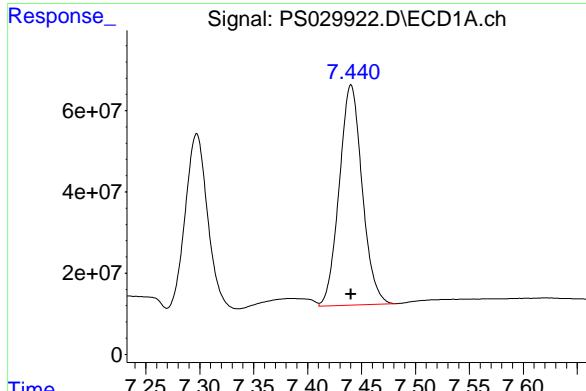

#9 2,4-D

R.T.: 8.018 min  
 Delta R.T.: 0.000 min  
 Response: 2435353652 ECD\_S  
 Conc: 849.74 ng/ml ClientSampleId : HSTDICC1000

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

#9 2,4-D





R.T.: 8.661 min  
 Delta R.T.: 0.000 min  
 Response: 991509756  
 Conc: 870.10 ng/ml

#10 Pentachlorophenol

R.T.: 8.297 min  
 Delta R.T.: 0.000 min  
 Response: 31038781576  
 Conc: 864.02 ng/ml

#10 Pentachlorophenol

R.T.: 9.163 min  
 Delta R.T.: 0.000 min  
 Response: 18517872387  
 Conc: 901.22 ng/ml

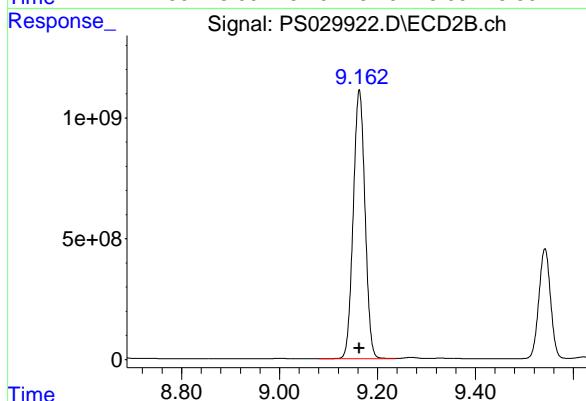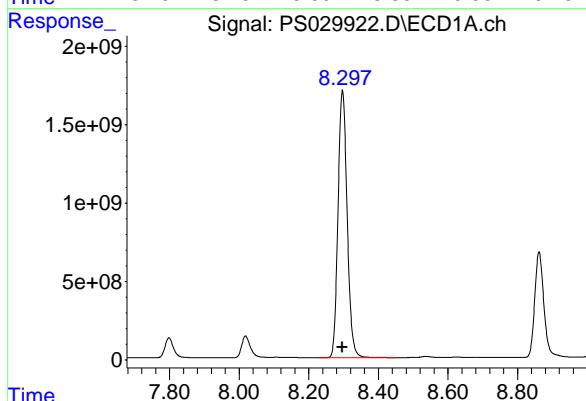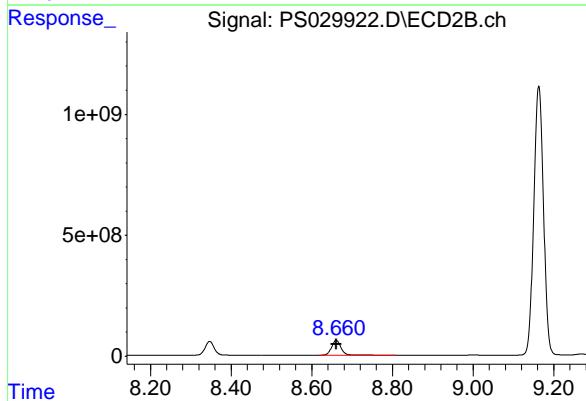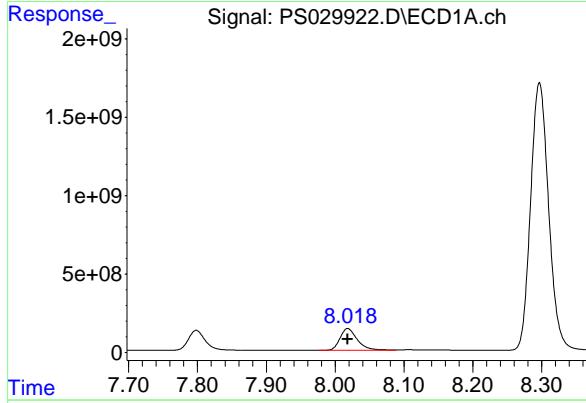

#11 2,4,5-TP (SILVEX)

R.T.: 8.862 min

Delta R.T.: 0.000 min

Instrument: ECD\_S


Response: 12264939701 ClientSampleId :

Conc: 869.59 ng/ml HSTDICC1000

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025

Supervised By :mohammad ahmed 04/26/2025

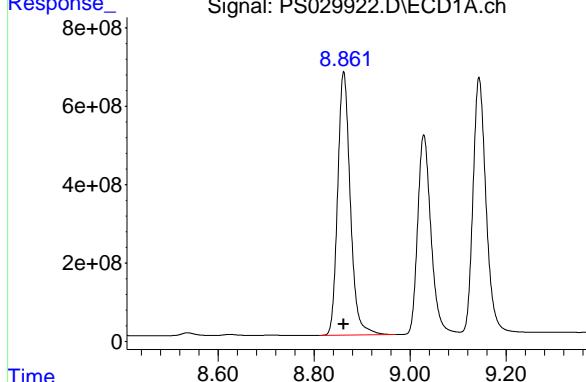


#11 2,4,5-TP (SILVEX)

R.T.: 9.542 min

Delta R.T.: 0.000 min

Response: 7478086402

Conc: 909.96 ng/ml

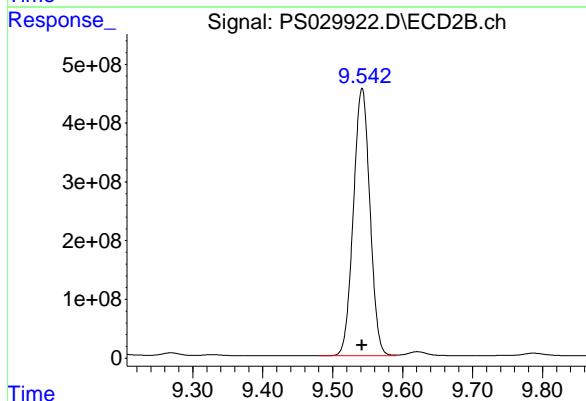


#12 2,4,5-T

R.T.: 9.144 min

Delta R.T.: 0.000 min

Response: 12428516949

Conc: 868.74 ng/ml

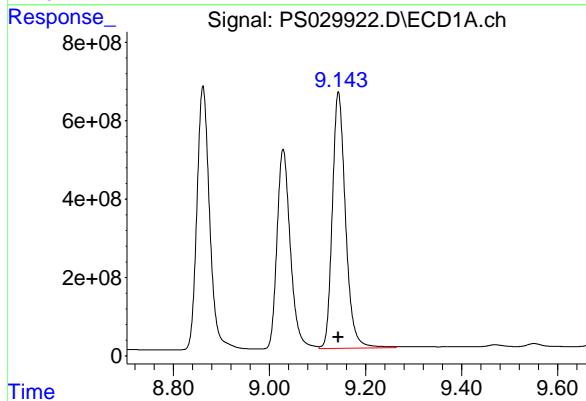


#12 2,4,5-T

R.T.: 9.947 min


Delta R.T.: 0.000 min

Response: 7054117355

Conc: 903.06 ng/ml

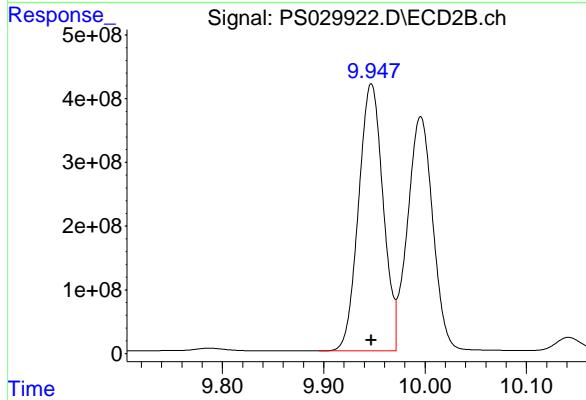

#13 2,4-DB

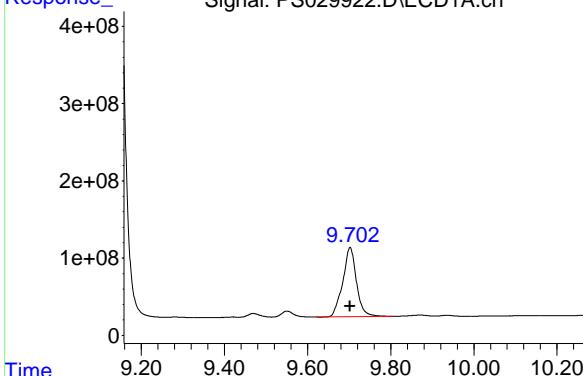

R.T.: 9.702 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_S  
Response: 2059257414  
Conc: 896.52 ng/ml  
ClientSampleId: HSTDICC1000

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 04/24/2025  
Supervised By :mohammad ahmed 04/26/2025

#13 2,4-DB



R.T.: 10.506 min  
Delta R.T.: 0.000 min  
Response: 737501651  
Conc: 916.65 ng/ml

#14 DINOSEB

R.T.: 10.866 min  
Delta R.T.: 0.000 min  
Response: 8807749773  
Conc: 849.67 ng/ml

#14 DINOSEB

R.T.: 10.881 min  
Delta R.T.: 0.000 min  
Response: 5194780641  
Conc: 883.60 ng/ml

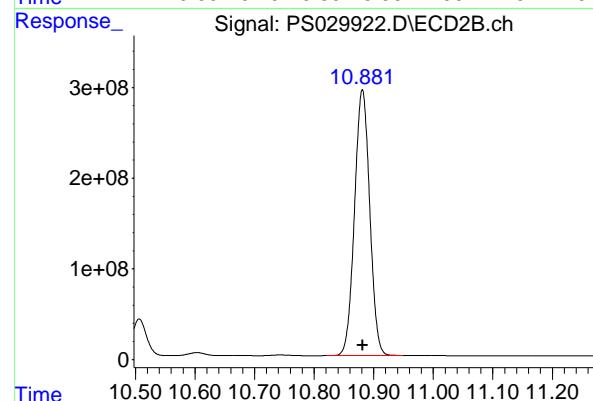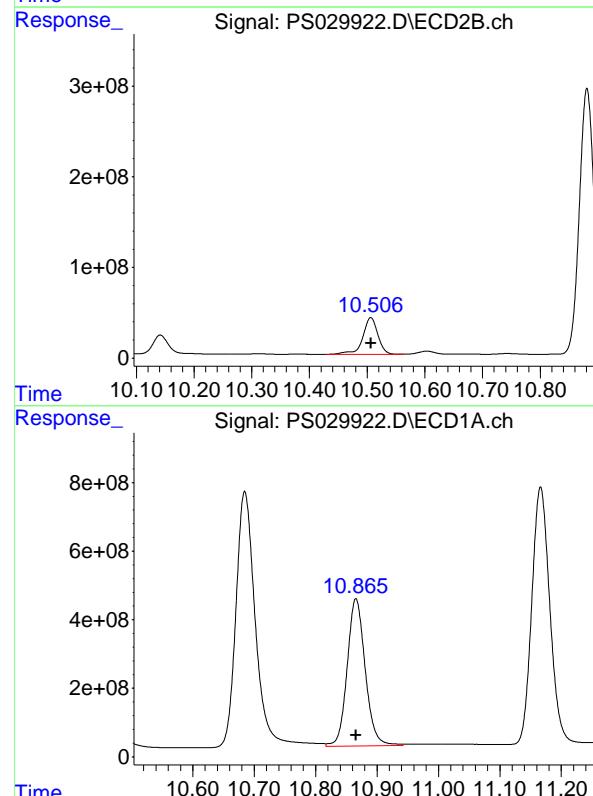

## #15 Picloram

R.T.: 10.685 min  
 Delta R.T.: 0.000 min  
 Instrument: ECD\_S  
 Response: 16510101945  
 Conc: 892.66 ng/ml  
 ClientSampleId: HSTDICC1000

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

## #15 Picloram





R.T.: 11.920 min  
 Delta R.T.: 0.000 min  
 Response: 11094799278  
 Conc: 889.28 ng/ml

## #16 DCPA

R.T.: 11.166 min  
 Delta R.T.: 0.000 min  
 Response: 15201932980  
 Conc: 876.32 ng/ml

## #16 DCPA

R.T.: 11.918 min  
 Delta R.T.: 0.000 min  
 Response: 10311432555  
 Conc: 906.51 ng/ml

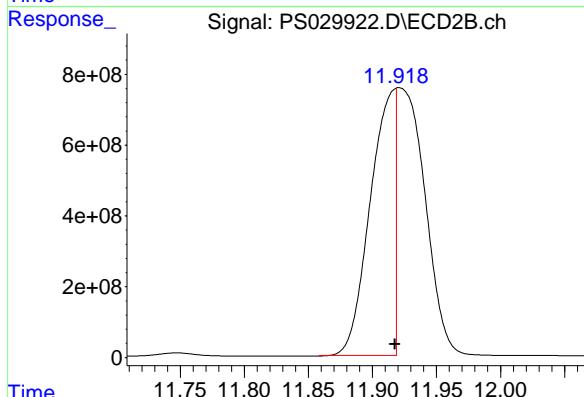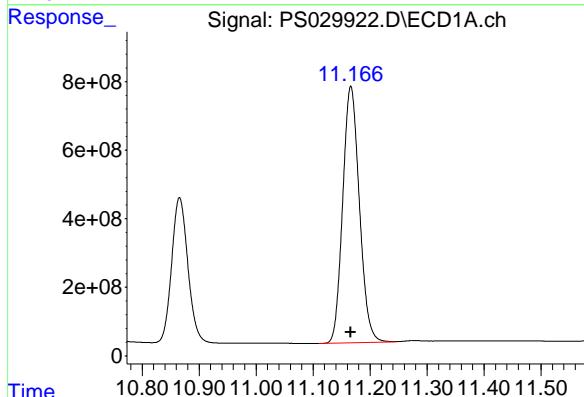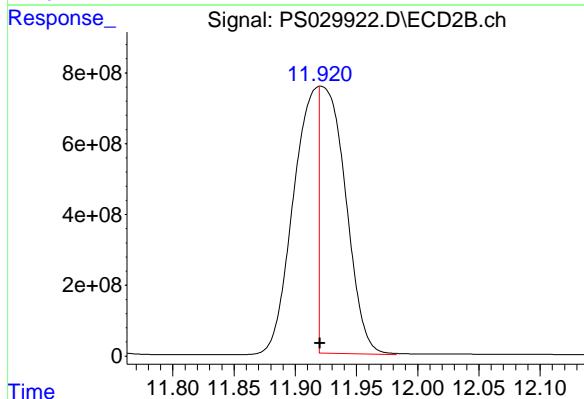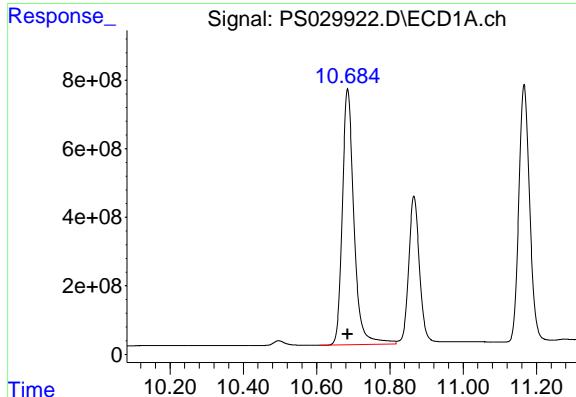

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029923.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 12:37  
 Operator : AR\AJ  
 Sample : HSTDICC1500  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**HSTDICC1500**

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 12:55:49 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:55:41 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

4) S 2,4-DCAA 6.941 7.467 3340.2E6 1016.6E6 1357.229 1442.979

**Target Compounds**

1) T	Dalapon	2.448	2.524	5176.7E6	2212.1E6	1264.064	1274.156
2) T	3,5-DICHL...	6.145	6.463	4570.5E6	1313.0E6	1278.892	1343.156
3) T	4-Nitroph...	6.731	7.001	2304.0E6	1001.5E6	1291.971	1307.566
5) T	DICAMBA	7.118	7.654	13131.1E6	5728.1E6	1325.990	1450.134
6) T	MCPP	7.300	7.765	992.1E6	254.5E6	153.962	145.490
7) T	MCPA	7.444	7.996	1275.2E6	326.1E6	144.397	137.819
8) T	DICHLORPROP	7.799	8.348	3270.4E6	1352.2E6	1290.535	1346.848
9) T	2,4-D	8.019	8.661	3666.5E6	1519.1E6	1303.464	1347.820
10) T	Pentachlo...	8.300	9.164	43790.4E6	27835.1E6	1255.279	1368.166
11) T	2,4,5-TP ...	8.862	9.543	18378.2E6	11452.1E6	1325.717	1399.712
12) T	2,4,5-T	9.144	9.947	18581.8E6	10783.8E6	1322.259	1389.199
13) T	2,4-DB	9.702	10.507	3190.6E6	1148.5E6	1396.120	1426.978
14) T	DINOSEB	10.866	10.881	13258.0E6	7950.4E6	1303.197	1363.473
15) T	Picloram	10.684	11.923	25181.9E6	16837.9E6	1373.763	1364.679m
16) T	DCPA	11.166	11.918	22629.5E6	14875.5E6	1329.504	1311.664m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029923.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 12:37  
 Operator : AR\AJ  
 Sample : HSTDICC1500  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1



Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDICC1500

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 12:55:49 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:55:41 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

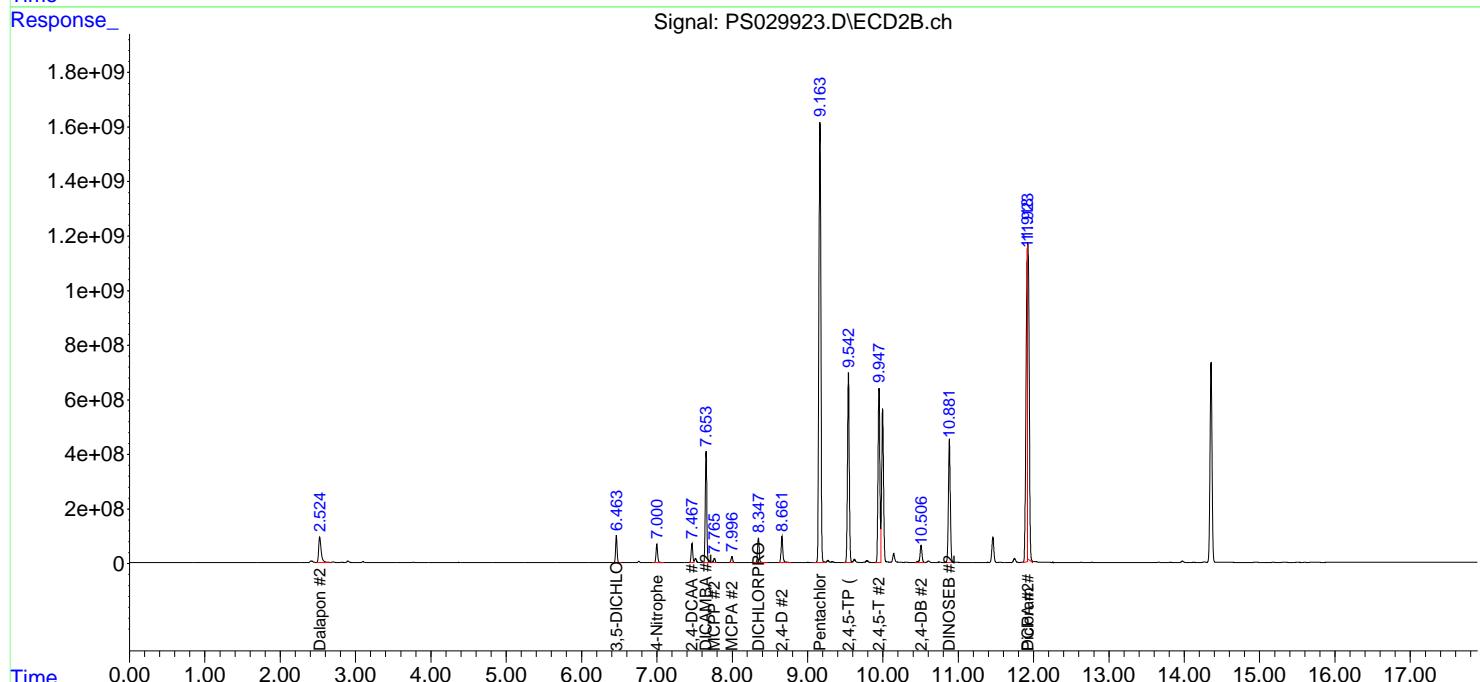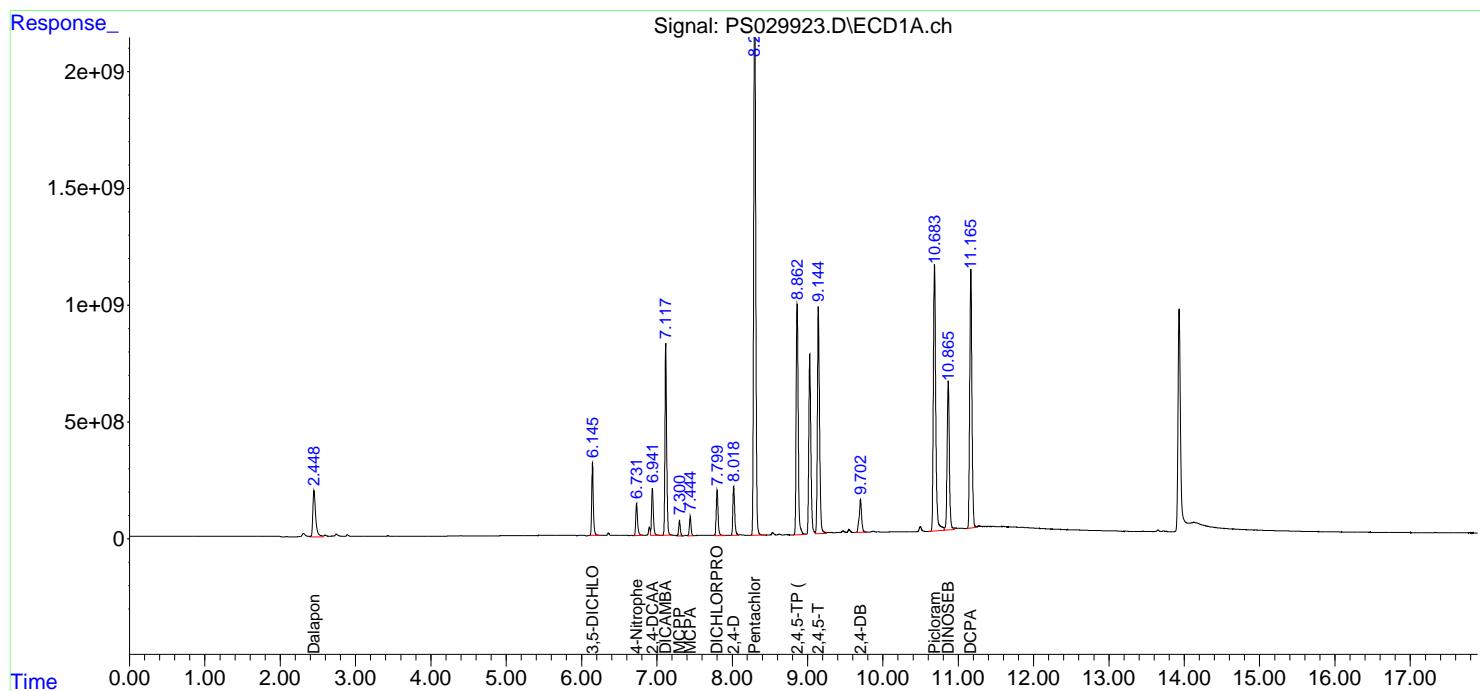

## #1 Dalapon

R.T.: 2.448 min  
 Delta R.T.: 0.000 min  
 Response: 5176670282 ECD\_S  
 Conc: 1264.06 ng/ml  
 ClientSampleId : HSTDICC1500

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

## #1 Dalapon





R.T.: 2.524 min  
 Delta R.T.: 0.000 min  
 Response: 2212117489  
 Conc: 1274.16 ng/ml





## #2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.145 min  
 Delta R.T.: 0.000 min  
 Response: 4570485622  
 Conc: 1278.89 ng/ml

## #2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.463 min  
 Delta R.T.: 0.000 min  
 Response: 1313041128  
 Conc: 1343.16 ng/ml

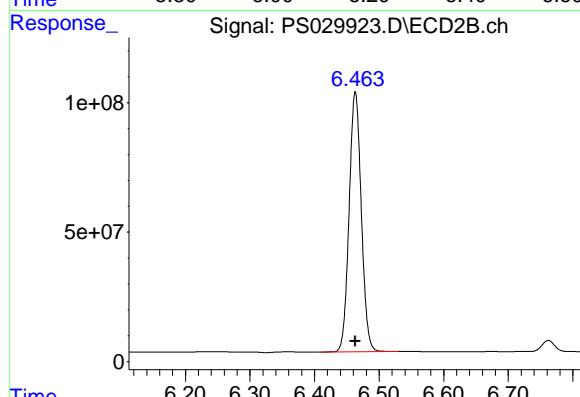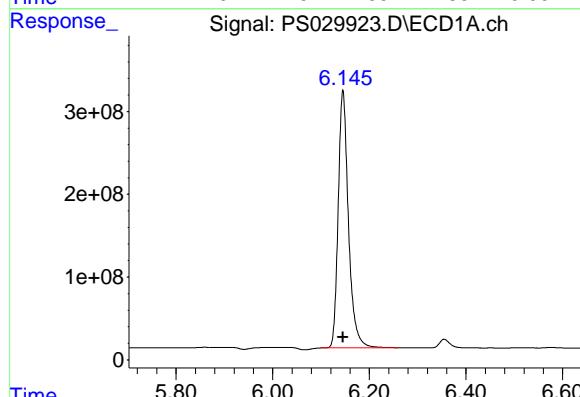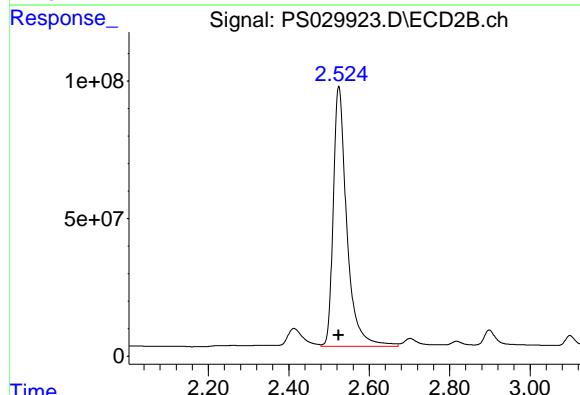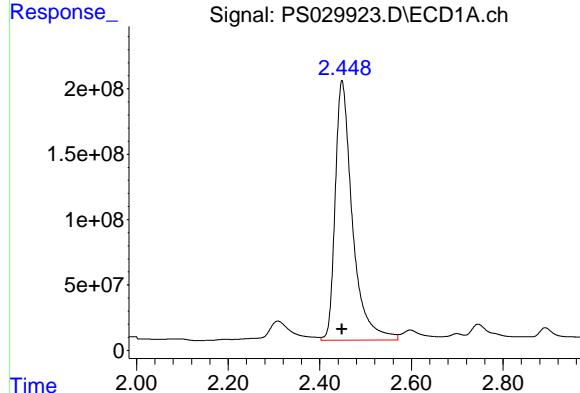

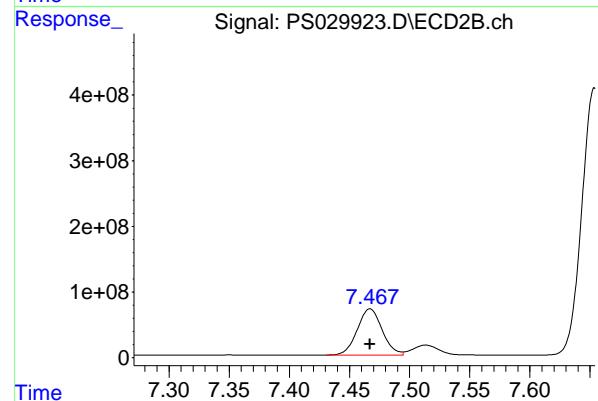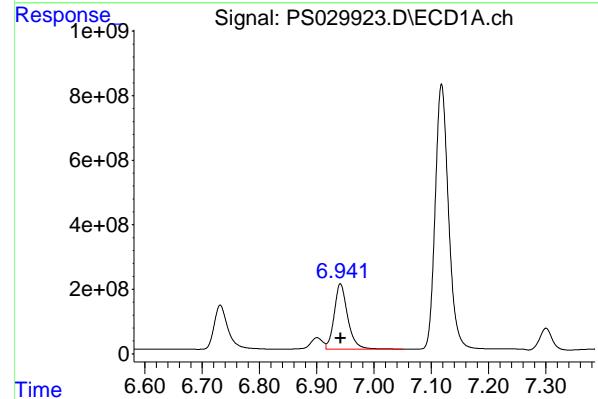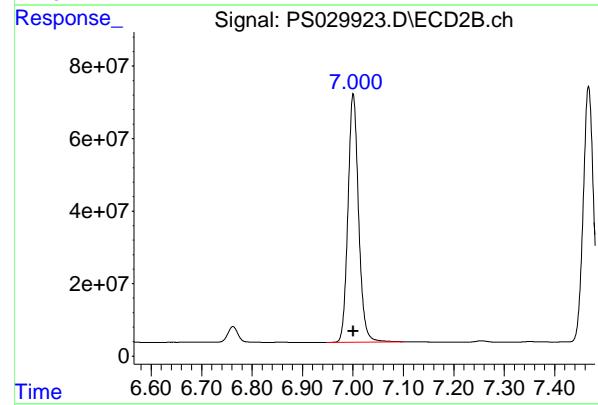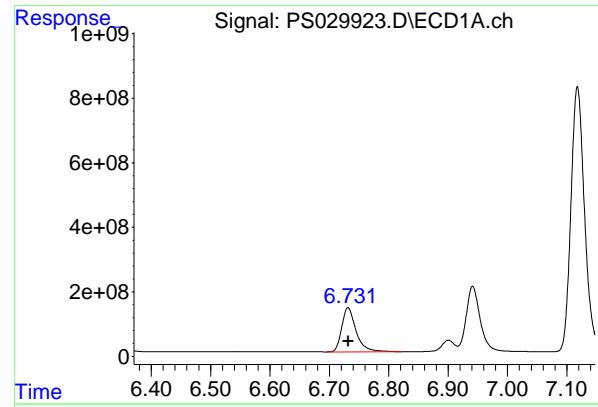

## #3 4-Nitrophenol

R.T.: 6.731 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_S  
Response: 2303997056  
Conc: 1291.97 ng/ml  
ClientSampleId : HSTDICC1500

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
Supervised By :mohammad ahmed 04/26/2025

## #3 4-Nitrophenol


R.T.: 7.001 min  
Delta R.T.: 0.000 min  
Response: 1001492635  
Conc: 1307.57 ng/ml

## #4 2,4-DCAA

R.T.: 6.941 min  
Delta R.T.: 0.000 min  
Response: 3340247176  
Conc: 1357.23 ng/ml

## #4 2,4-DCAA

R.T.: 7.467 min  
Delta R.T.: 0.000 min  
Response: 1016603254  
Conc: 1442.98 ng/ml

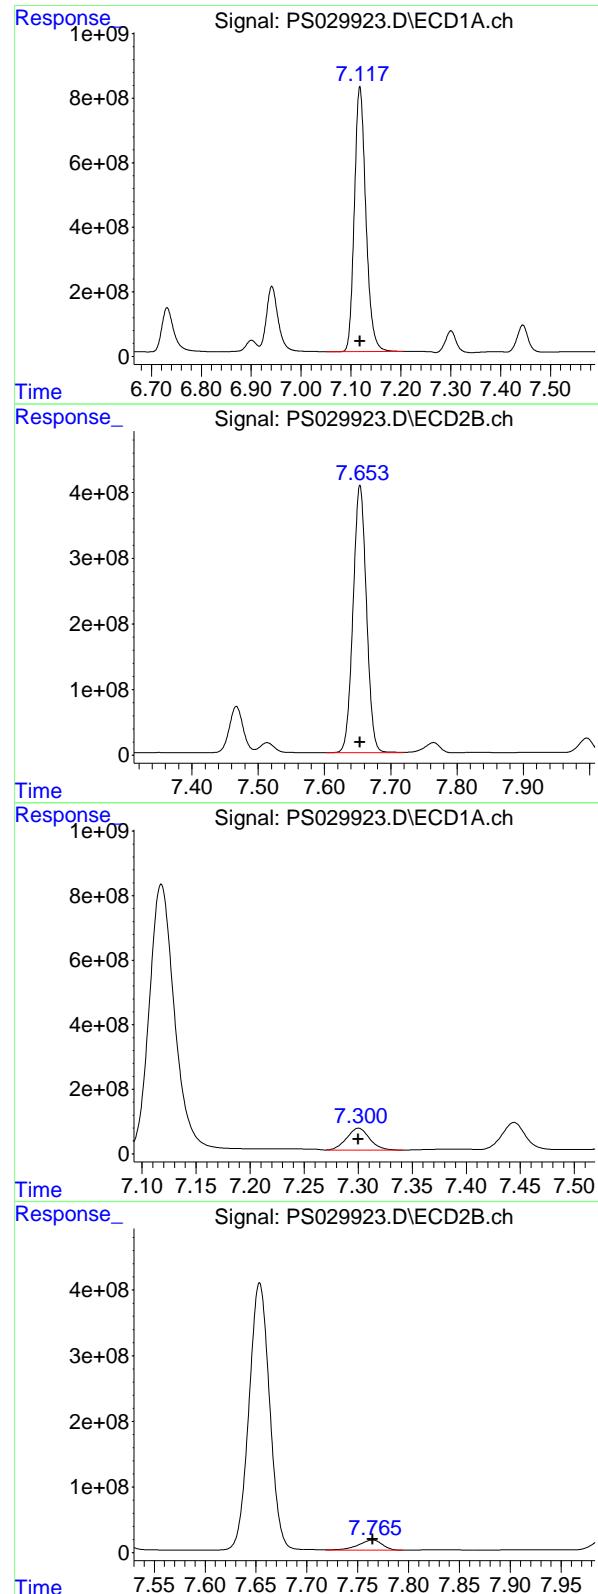

## #5 DICAMBA

R.T.: 7.118 min  
 Delta R.T.: 0.000 min  
 Instrument: ECD\_S  
 Response: 13131098945  
 Conc: 1325.99 ng/ml  
 ClientSampleId : HSTDICC1500

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

## #5 DICAMBA

R.T.: 7.654 min  
 Delta R.T.: 0.000 min  
 Response: 5728123349  
 Conc: 1450.13 ng/ml

## #6 MCPP

R.T.: 7.300 min  
 Delta R.T.: 0.000 min  
 Response: 992077341  
 Conc: 153.96 ug/ml

## #6 MCPP

R.T.: 7.765 min  
 Delta R.T.: 0.000 min  
 Response: 254454768  
 Conc: 145.49 ug/ml

#7 MCPA

R.T.: 7.444 min  
 Delta R.T.: 0.000 min  
 Response: 1275219029  
 Conc: 144.40 ug/ml  
 Instrument: ECD\_S  
 ClientSampleId : HSTDICC1500

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

#7 MCPA





R.T.: 7.996 min  
 Delta R.T.: 0.000 min  
 Response: 326053003  
 Conc: 137.82 ug/ml

#8 DICHLORPROP

R.T.: 7.799 min  
 Delta R.T.: 0.000 min  
 Response: 3270356058  
 Conc: 1290.54 ng/ml

#8 DICHLORPROP

R.T.: 8.348 min  
 Delta R.T.: 0.000 min  
 Response: 1352187583  
 Conc: 1346.85 ng/ml

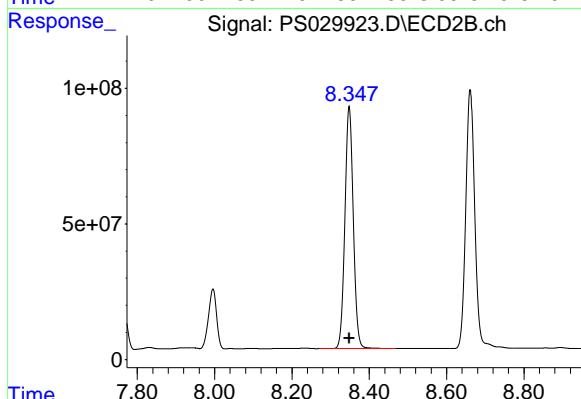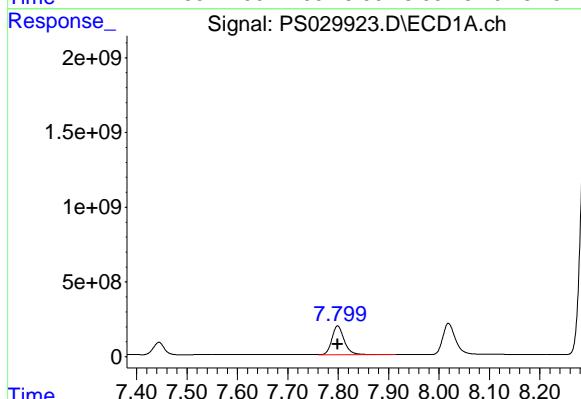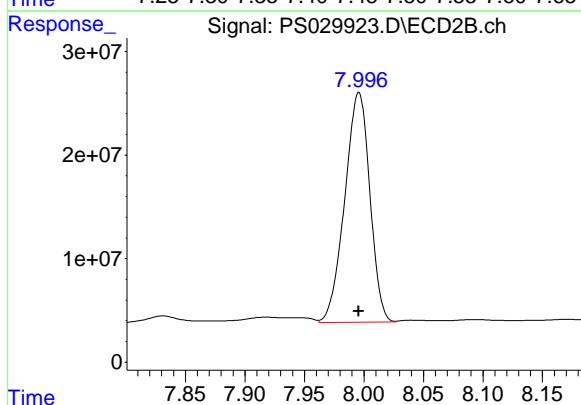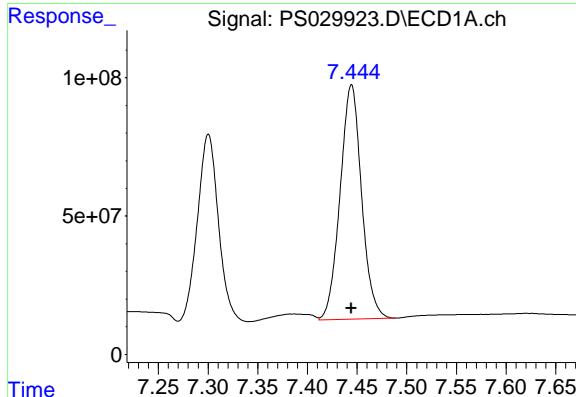

#9 2,4-D

R.T.: 8.019 min  
 Delta R.T.: 0.000 min  
 Response: 3666476235 ECD\_S  
 Conc: 1303.46 ng/ml ClientSampleId : HSTDICC1500

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

#9 2,4-D


R.T.: 8.661 min  
 Delta R.T.: 0.000 min  
 Response: 1519137434  
 Conc: 1347.82 ng/ml

#10 Pentachlorophenol

R.T.: 8.300 min  
 Delta R.T.: 0.000 min  
 Response: 43790422023  
 Conc: 1255.28 ng/ml


#10 Pentachlorophenol

R.T.: 9.164 min  
 Delta R.T.: 0.000 min  
 Response: 27835080663  
 Conc: 1368.17 ng/ml

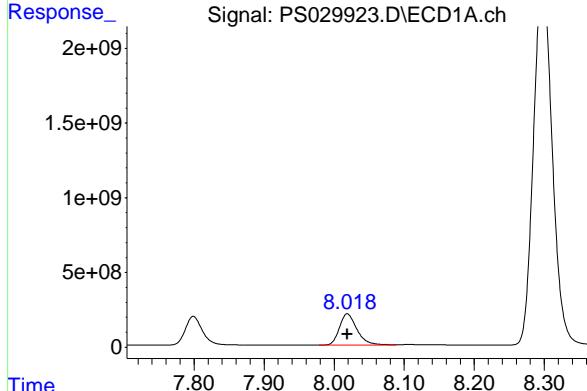


#9 2,4-D

R.T.: 8.661 min  
 Delta R.T.: 0.000 min  
 Response: 1519137434  
 Conc: 1347.82 ng/ml

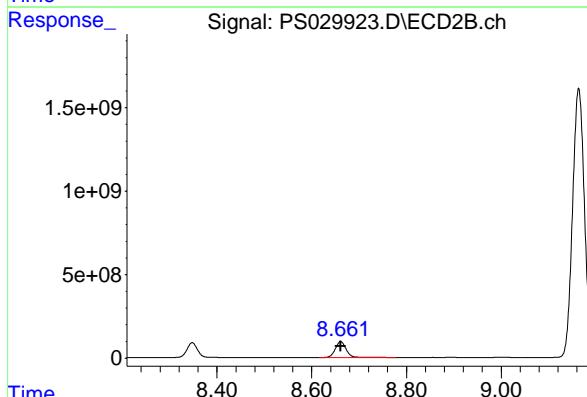


#10 Pentachlorophenol

R.T.: 8.300 min  
 Delta R.T.: 0.000 min  
 Response: 43790422023  
 Conc: 1255.28 ng/ml

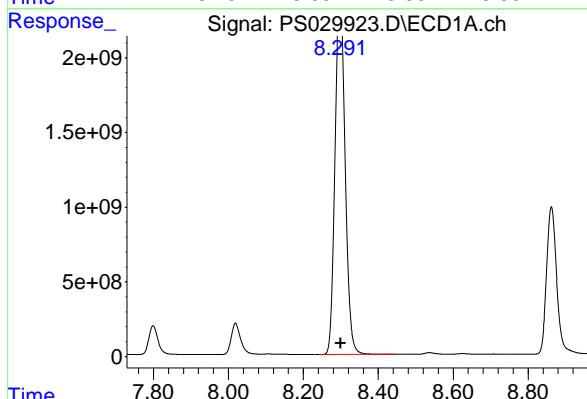


#10 Pentachlorophenol

R.T.: 9.164 min  
 Delta R.T.: 0.000 min  
 Response: 27835080663  
 Conc: 1368.17 ng/ml

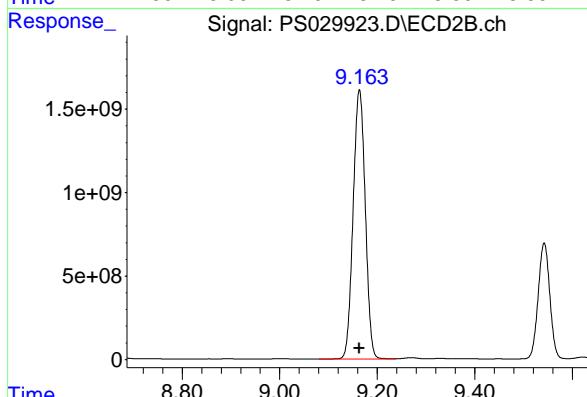

#11 2,4,5-TP (SILVEX)

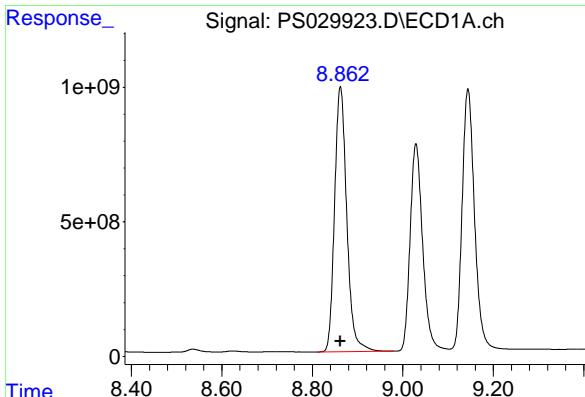

R.T.: 8.862 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_S  
Response: 18378203400  
Conc: 1325.72 ng/ml  
ClientSampleId: HSTDICC1500

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
Supervised By :mohammad ahmed 04/26/2025

#11 2,4,5-TP (SILVEX)



R.T.: 9.543 min  
Delta R.T.: 0.000 min  
Response: 11452091600  
Conc: 1399.71 ng/ml


#12 2,4,5-T

R.T.: 9.144 min  
Delta R.T.: 0.000 min  
Response: 18581844789  
Conc: 1322.26 ng/ml

#12 2,4,5-T

R.T.: 9.947 min  
Delta R.T.: 0.000 min  
Response: 10783792004  
Conc: 1389.20 ng/ml

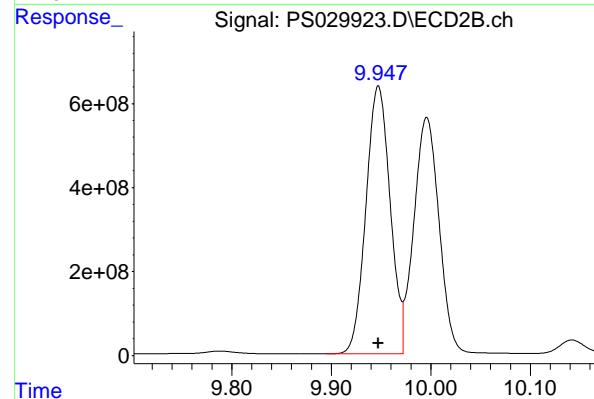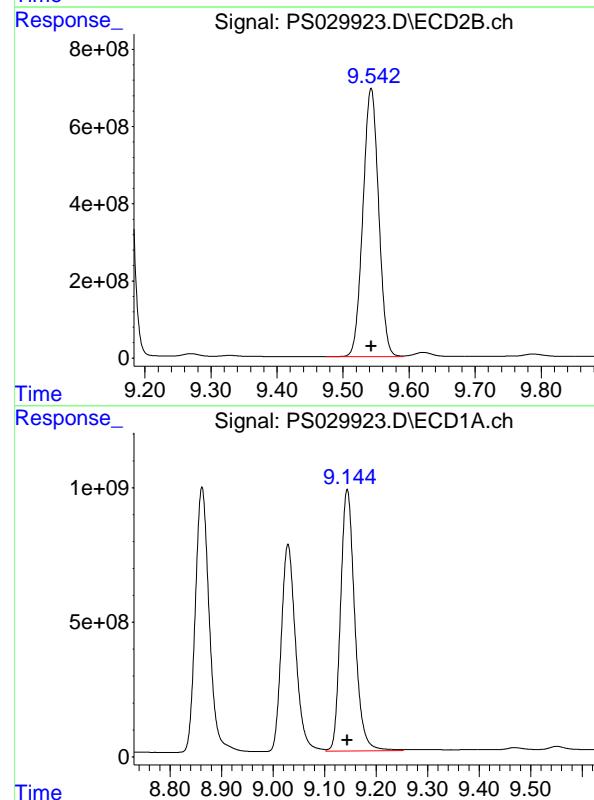

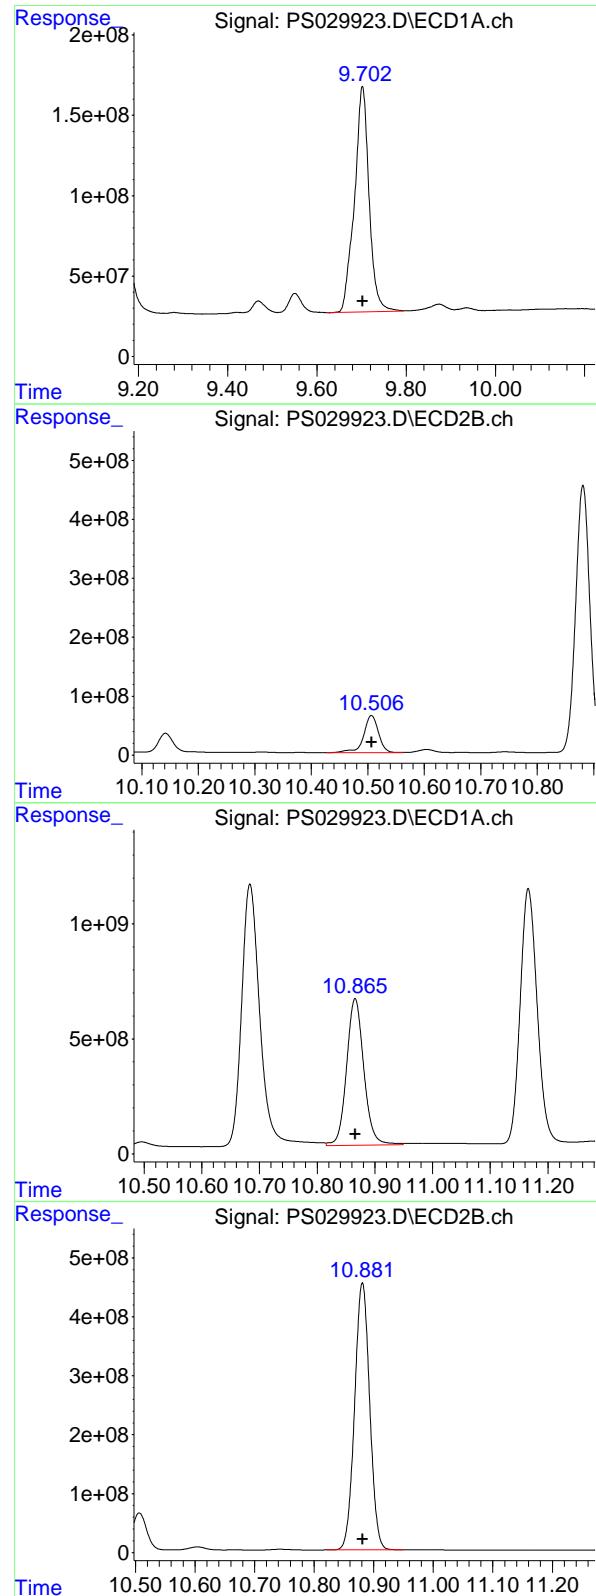

#13 2,4-DB

R.T.: 9.702 min  
 Delta R.T.: 0.000 min  
 Response: 3190632076 ECD\_S  
 Conc: 1396.12 ng/ml  
 ClientSampleId : HSTDICC1500

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

#13 2,4-DB

R.T.: 10.507 min  
 Delta R.T.: 0.000 min  
 Response: 1148492462  
 Conc: 1426.98 ng/ml

#14 DINOSEB

R.T.: 10.866 min  
 Delta R.T.: 0.000 min  
 Response: 13257982778  
 Conc: 1303.20 ng/ml

#14 DINOSEB

R.T.: 10.881 min  
 Delta R.T.: 0.000 min  
 Response: 7950383575  
 Conc: 1363.47 ng/ml

## #15 Picloram

R.T.: 10.684 min  
 Delta R.T.: 0.000 min  
 Instrument: ECD\_S  
 Response: 25181937899  
 Conc: 1373.76 ng/ml  
 ClientSampleId: HSTDICC1500

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

## #15 Picloram





R.T.: 11.923 min  
 Delta R.T.: 0.000 min  
 Response: 16837876459  
 Conc: 1364.68 ng/ml

## #16 DCPA

R.T.: 11.166 min  
 Delta R.T.: 0.000 min  
 Response: 22629488258  
 Conc: 1329.50 ng/ml

## #16 DCPA

R.T.: 11.918 min  
 Delta R.T.: 0.000 min  
 Response: 14875468261  
 Conc: 1311.66 ng/ml

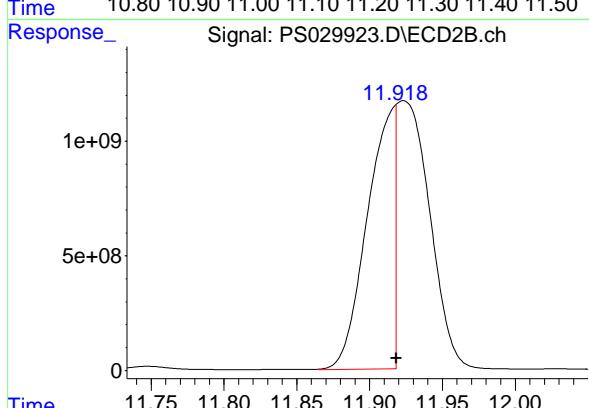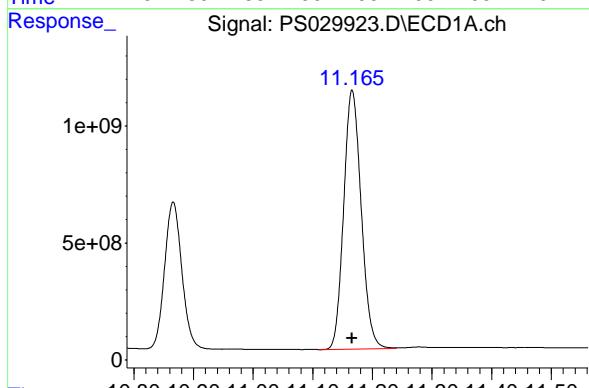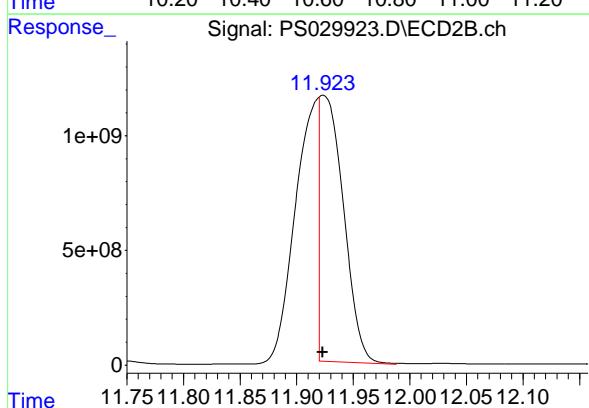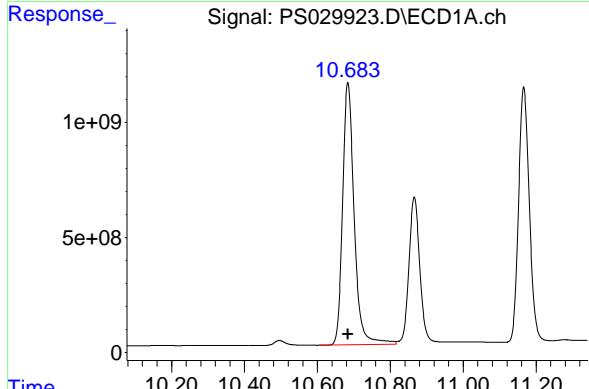

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029924.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 13:01  
 Operator : AR\AJ  
 Sample : HSTDICV750  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**ICVPS042325**

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 13:20:38 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

4) S 2,4-DCAA 6.941 7.467 1785.1E6 522.8E6 725.315 742.096

**Target Compounds**

1) T	Dalapon	2.449	2.525	2793.7E6	1167.7E6	682.183	672.600
2) T	3,5-DICHL...	6.145	6.463	2447.4E6	679.4E6	684.816	695.005
3) T	4-Nitroph...	6.732	7.000	1167.8E6	514.6E6	654.846	671.850
5) T	DICAMBA	7.118	7.653	6990.7E6	2822.8E6	705.926	714.619
6) T	MCPP	7.297	7.760	467.2E6	127.4E6	72.508	72.837
7) T	MCPA	7.439	7.991	617.1E6	165.5E6	69.876	69.959
8) T	DICHLORPROP	7.798	8.347	1751.5E6	702.7E6	691.189	699.969
9) T	2,4-D	8.018	8.661	1976.8E6	789.4E6	702.764	700.374
10) T	Pentachlo...	8.297	9.163	25231.5E6	14767.7E6	723.277	725.871
11) T	2,4,5-TP ...	8.862	9.542	9894.0E6	5913.4E6	713.706	722.753
12) T	2,4,5-T	9.144	9.947	9990.5E6	5588.6E6	710.908	719.944
13) T	2,4-DB	9.702	10.506	1649.4E6	582.7E6	721.719	724.013
14) T	DINOSEB	10.866	10.881	7070.7E6	4118.9E6	695.014	706.382
15) T	Picloram	10.685	11.923	13255.1E6	9024.0E6	723.112	734.636m
16) T	DCPA	11.167	11.918	12285.5E6	8142.3E6	721.785	722.370m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029924.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 13:01  
 Operator : AR\AJ  
 Sample : HSTDICV750  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1



Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 13:20:38 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

**Instrument :**  
 ECD\_S  
**ClientSampleId :**  
 ICPVPS042325

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

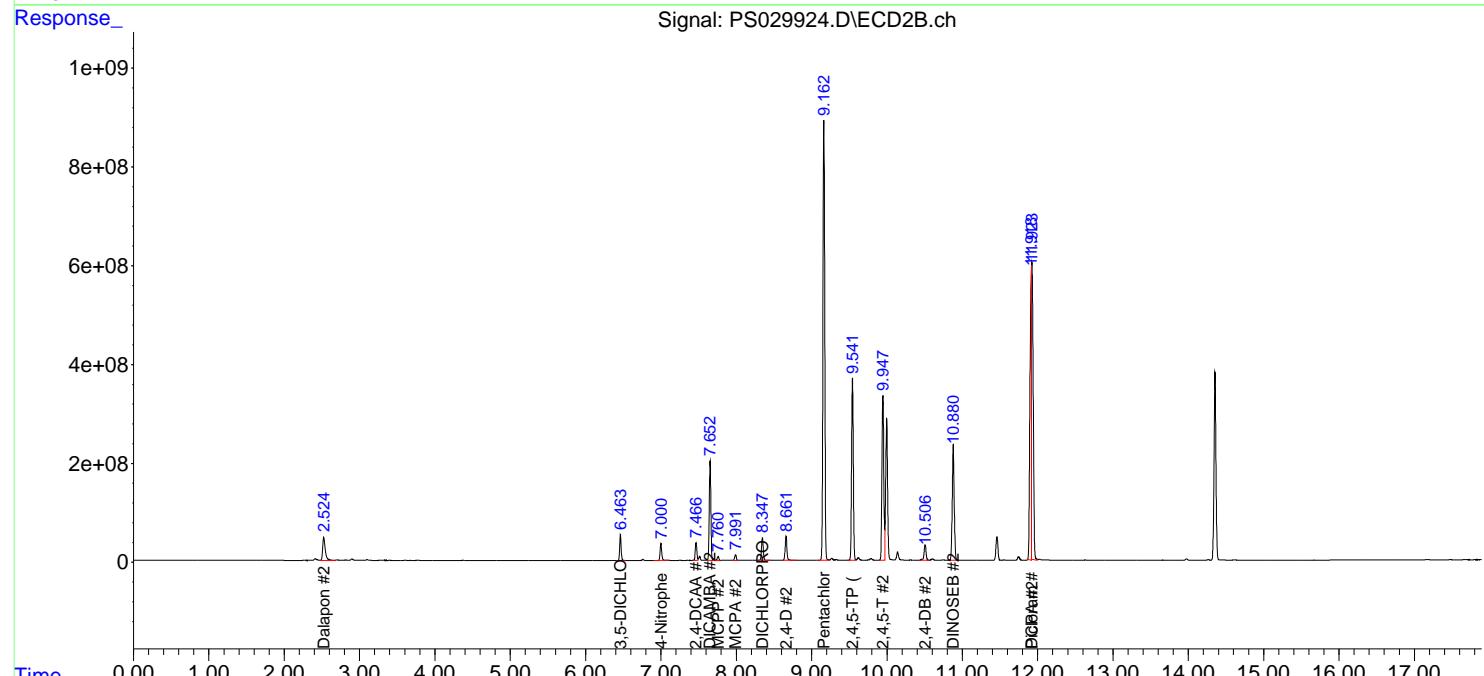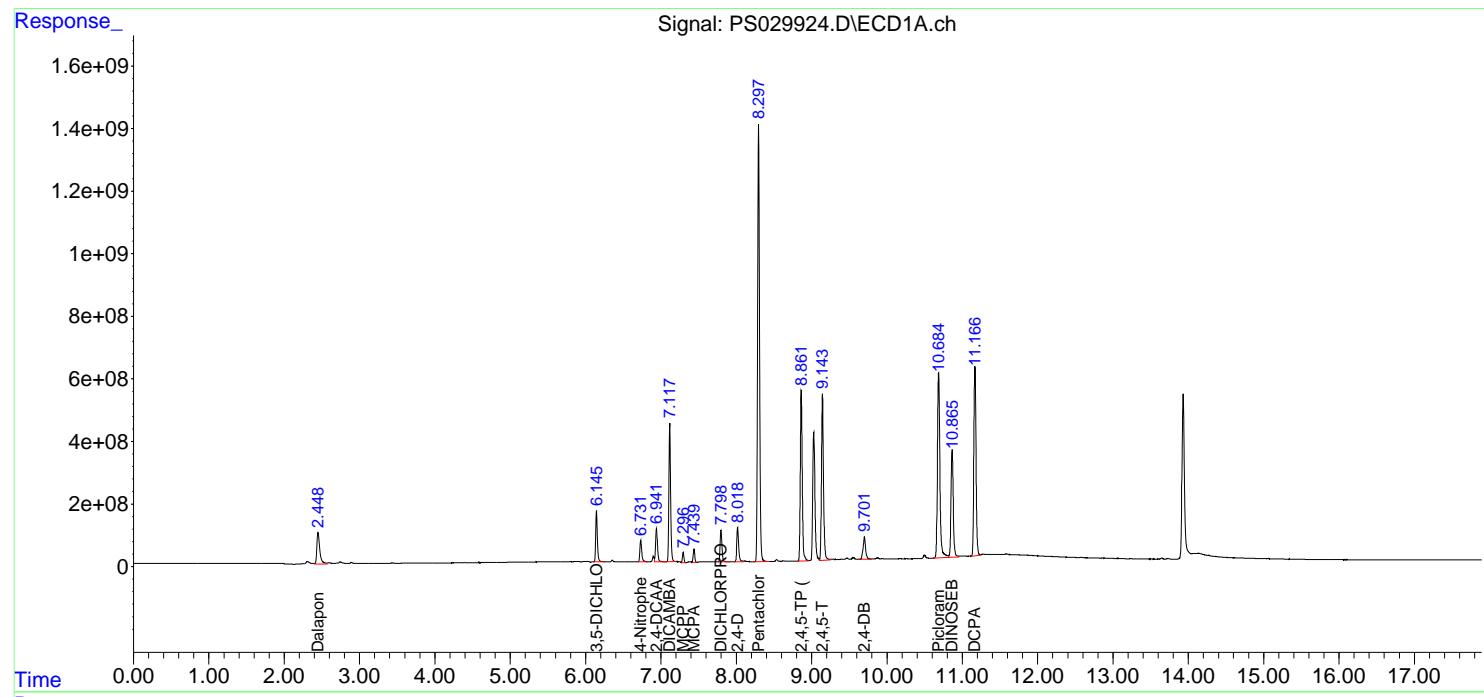

## #1 Dalapon

R.T.: 2.449 min  
 Delta R.T.: 0.000 min  
 Response: 2793715347  
 Conc: 682.18 ng/ml  
 Instrument: ECD\_S  
 ClientSampleId : ICVPS042325

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

## #1 Dalapon





R.T.: 2.525 min  
 Delta R.T.: 0.000 min  
 Response: 1167729659  
 Conc: 672.60 ng/ml





## #2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.145 min  
 Delta R.T.: 0.000 min  
 Response: 2447386587  
 Conc: 684.82 ng/ml

## #2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.463 min  
 Delta R.T.: 0.000 min  
 Response: 679422841  
 Conc: 695.01 ng/ml

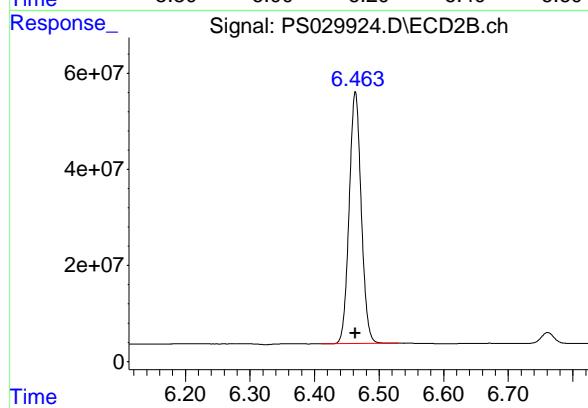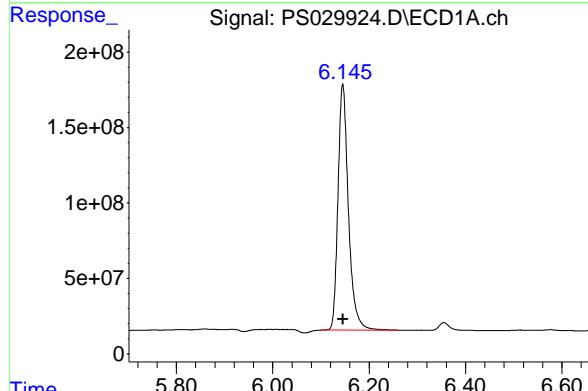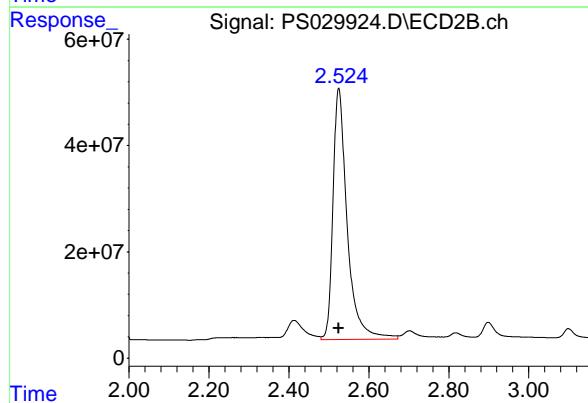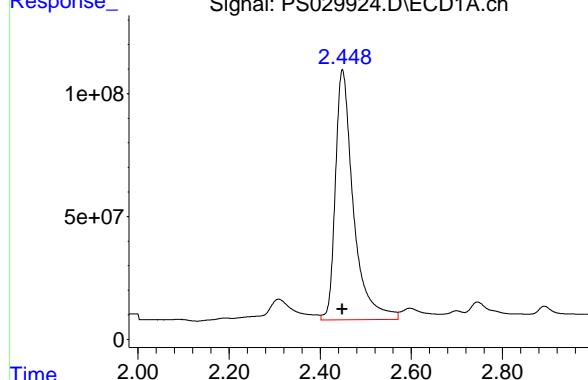

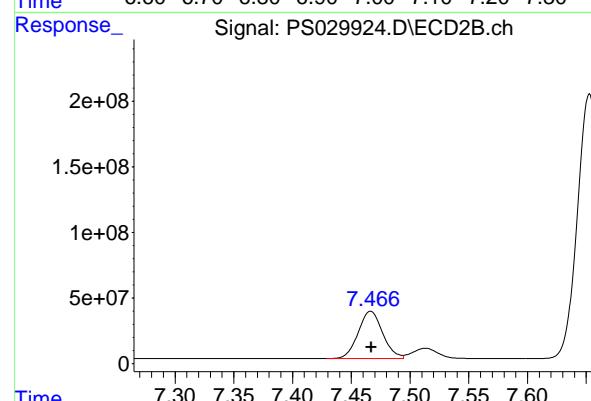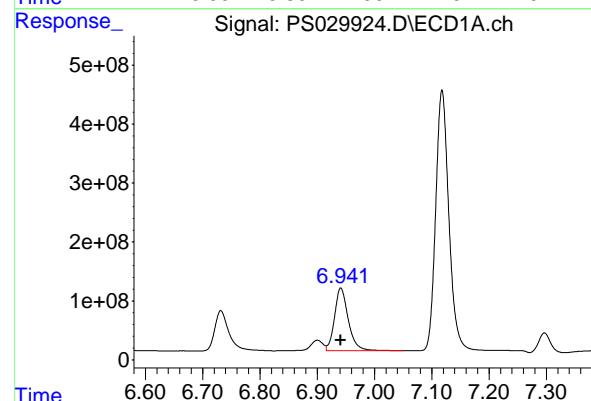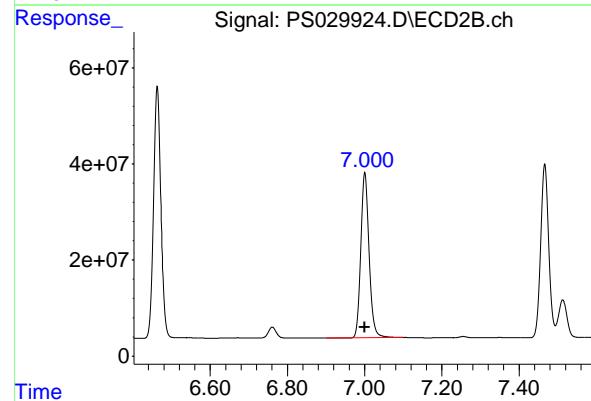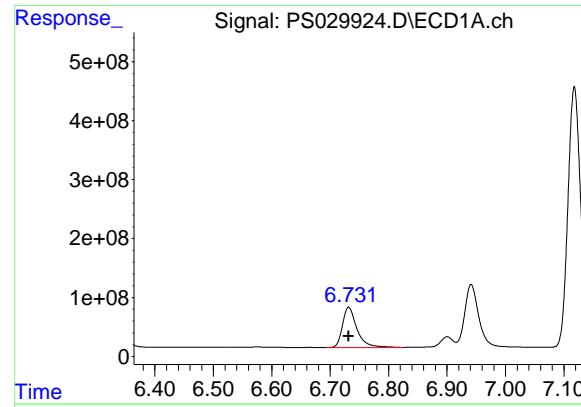

## #3 4-Nitrophenol

R.T.: 6.732 min  
 Delta R.T.: 0.000 min  
 Response: 1167800121 ECD\_S  
 Conc: 654.85 ng/ml ClientSampleId : ICVPS042325

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

## #3 4-Nitrophenol

R.T.: 7.000 min  
 Delta R.T.: 0.000 min  
 Response: 514583941  
 Conc: 671.85 ng/ml

## #4 2,4-DCAA

R.T.: 6.941 min  
 Delta R.T.: 0.000 min  
 Response: 1785057977  
 Conc: 725.32 ng/ml

## #4 2,4-DCAA

R.T.: 7.467 min  
 Delta R.T.: 0.000 min  
 Response: 522819399  
 Conc: 742.10 ng/ml

## #5 DICAMBA

R.T.: 7.118 min  
 Delta R.T.: 0.000 min  
 Response: 6990688242 ECD\_S  
 Conc: 705.93 ng/ml ClientSampleId :  
 ICPVPS042325

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

## #5 DICAMBA





R.T.: 7.653 min  
 Delta R.T.: 0.000 min  
 Response: 2822792480  
 Conc: 714.62 ng/ml



## #6 MCPP

R.T.: 7.297 min  
 Delta R.T.: -0.004 min  
 Response: 467215325  
 Conc: 72.51 ug/ml

## #6 MCPP

R.T.: 7.760 min  
 Delta R.T.: -0.004 min  
 Response: 127389122  
 Conc: 72.84 ug/ml

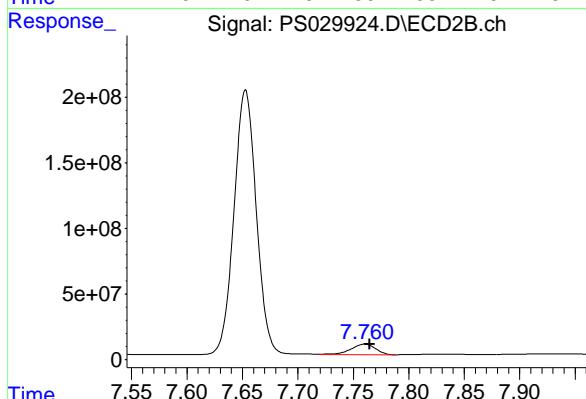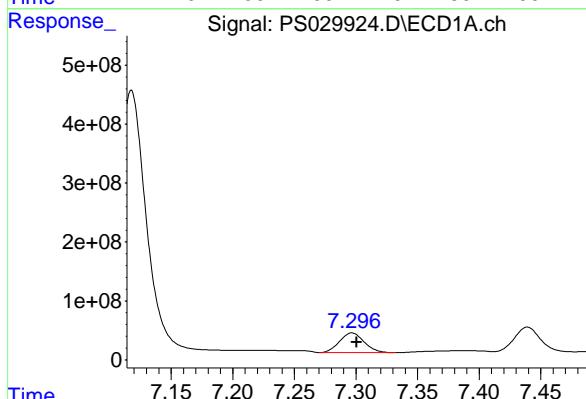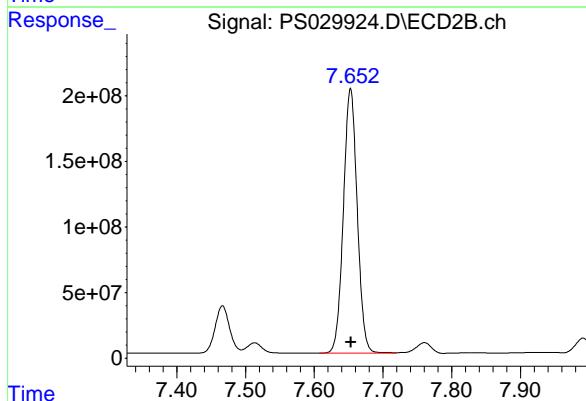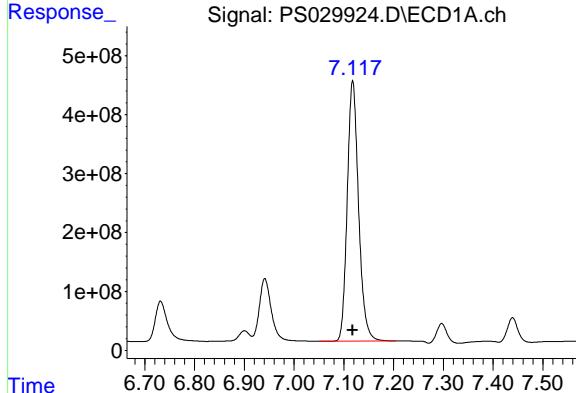

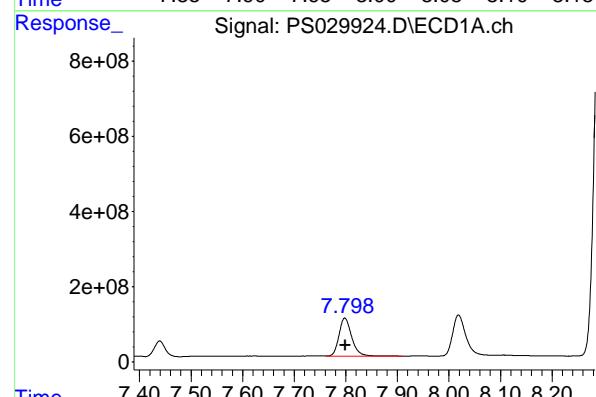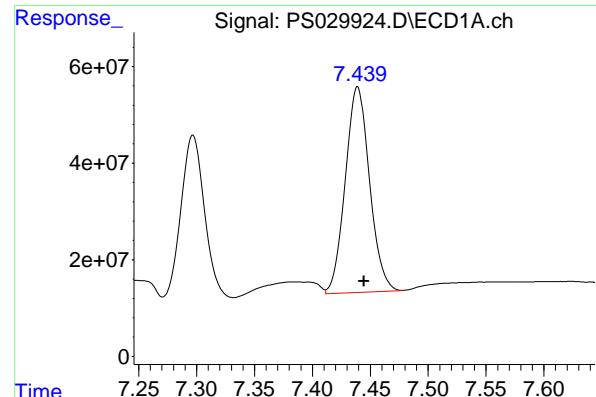

#7 MCPA

R.T.: 7.439 min  
 Delta R.T.: -0.005 min  
 Response: 617101386  
 Conc: 69.88 ug/ml

Instrument: ECD\_S  
 ClientSampleId : ICVPS042325

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

#7 MCPA

R.T.: 7.991 min  
 Delta R.T.: -0.005 min  
 Response: 165509058  
 Conc: 69.96 ug/ml

#8 DICHLORPROP

R.T.: 7.798 min  
 Delta R.T.: 0.000 min  
 Response: 1751547333  
 Conc: 691.19 ng/ml

#8 DICHLORPROP

R.T.: 8.347 min  
 Delta R.T.: 0.000 min  
 Response: 702743426  
 Conc: 699.97 ng/ml

#9 2,4-D

R.T.: 8.018 min  
 Delta R.T.: 0.000 min  
 Response: 1976784235  
 Conc: 702.76 ng/ml  
 Instrument: ECD\_S  
 ClientSampleId : ICVPS042325

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

#9 2,4-D


R.T.: 8.661 min  
 Delta R.T.: 0.000 min  
 Response: 789396429  
 Conc: 700.37 ng/ml

#10 Pentachlorophenol

R.T.: 8.297 min  
 Delta R.T.: -0.002 min  
 Response: 25231541630  
 Conc: 723.28 ng/ml


#10 Pentachlorophenol

R.T.: 9.163 min  
 Delta R.T.: 0.000 min  
 Response: 14767707242  
 Conc: 725.87 ng/ml

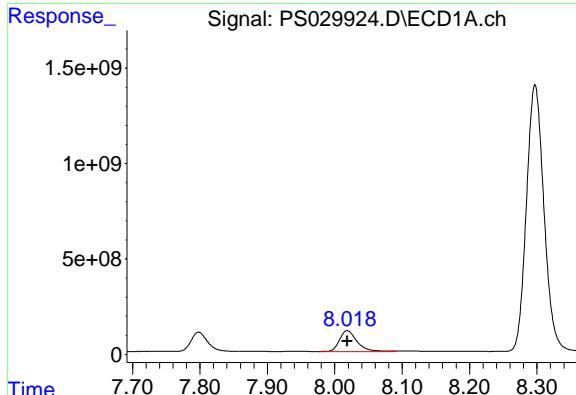


#9 2,4-D

R.T.: 8.661 min  
 Delta R.T.: 0.000 min  
 Response: 789396429  
 Conc: 700.37 ng/ml

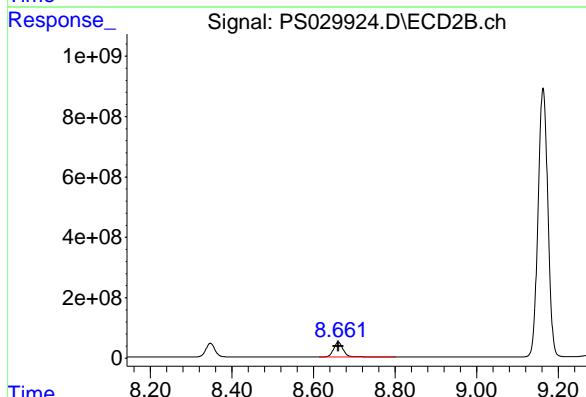


#10 Pentachlorophenol

R.T.: 8.297 min  
 Delta R.T.: -0.002 min  
 Response: 25231541630  
 Conc: 723.28 ng/ml

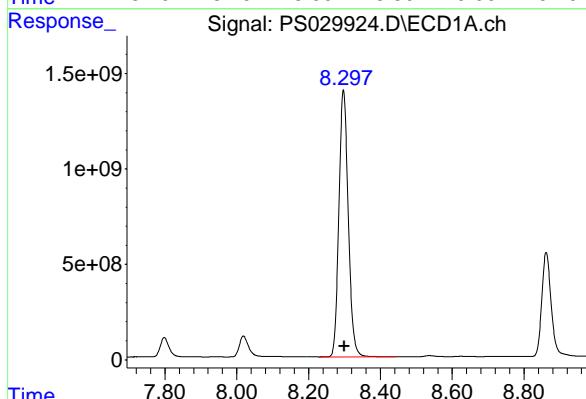

#10 Pentachlorophenol

R.T.: 9.163 min  
 Delta R.T.: 0.000 min  
 Response: 14767707242  
 Conc: 725.87 ng/ml

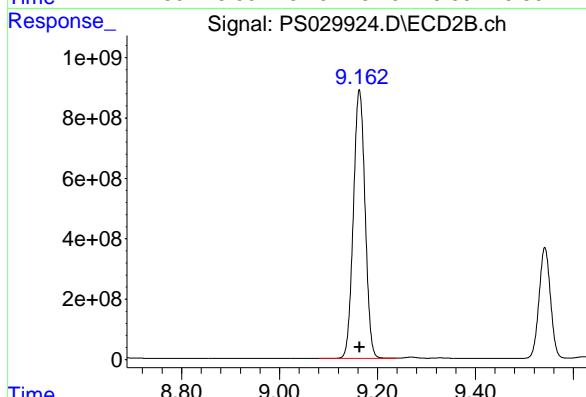

#11 2,4,5-TP (SILVEX)

R.T.: 8.862 min

Delta R.T.: 0.000 min

Instrument: ECD\_S

Response: 9893987718 ClientSampleId :

Conc: 713.71 ng/ml ICVPS042325

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
Supervised By :mohammad ahmed 04/26/2025

#11 2,4,5-TP (SILVEX)

R.T.: 9.542 min

Delta R.T.: 0.000 min

Response: 5913388172

Conc: 722.75 ng/ml

#12 2,4,5-T

R.T.: 9.144 min

Delta R.T.: 0.000 min

Response: 9990461422

Conc: 710.91 ng/ml


#12 2,4,5-T

R.T.: 9.947 min

Delta R.T.: 0.000 min

Response: 5588639706

Conc: 719.94 ng/ml

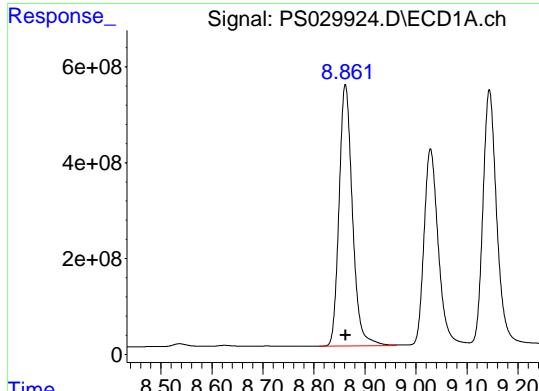


#11 2,4,5-TP (SILVEX)

R.T.: 9.542 min

Delta R.T.: 0.000 min

Response: 5913388172

Conc: 722.75 ng/ml

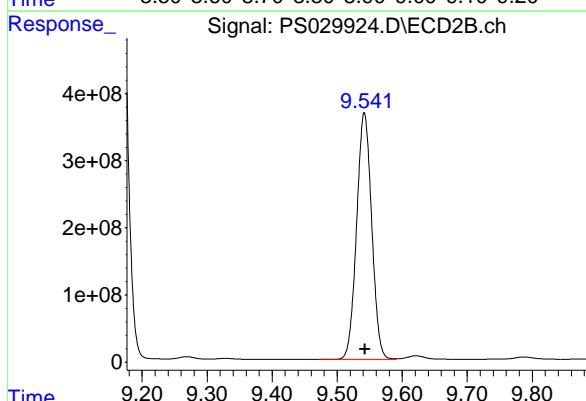


#12 2,4,5-T

R.T.: 9.144 min

Delta R.T.: 0.000 min

Response: 9990461422

Conc: 710.91 ng/ml

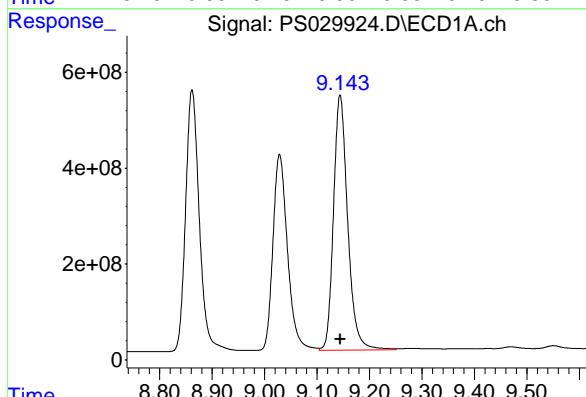


#12 2,4,5-T


R.T.: 9.947 min

Delta R.T.: 0.000 min

Response: 5588639706

Conc: 719.94 ng/ml

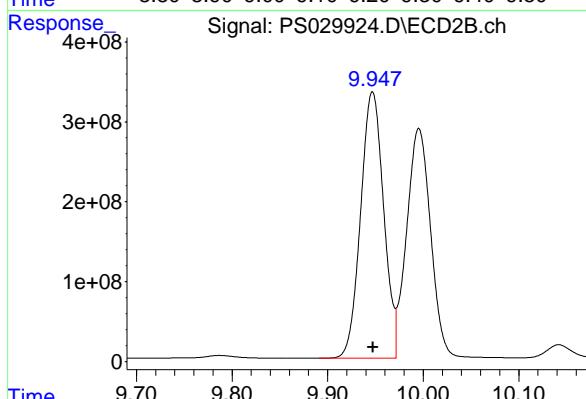

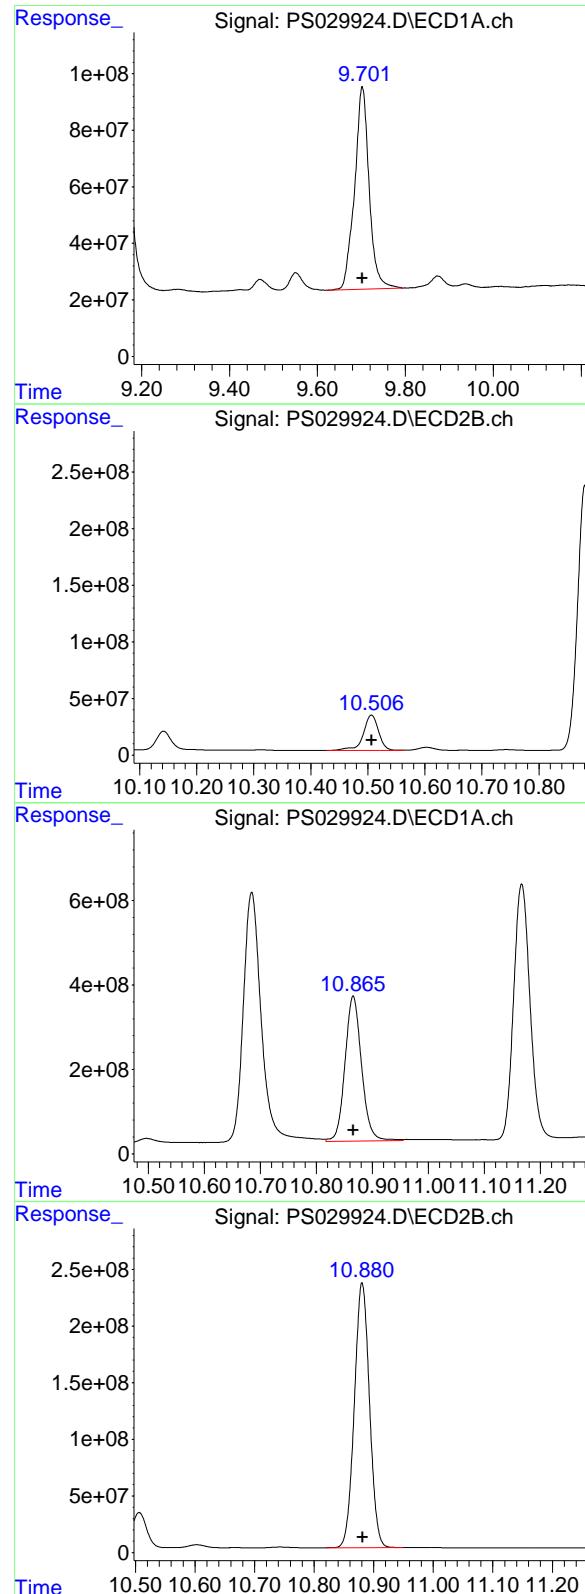

#13 2,4-DB

R.T.: 9.702 min  
 Delta R.T.: 0.000 min  
 Response: 1649385436 ECD\_S  
 Conc: 721.72 ng/ml ClientSampleId :  
 ICPVPS042325

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

#13 2,4-DB

R.T.: 10.506 min  
 Delta R.T.: 0.000 min  
 Response: 582716222  
 Conc: 724.01 ng/ml

#14 DINOSEB

R.T.: 10.866 min  
 Delta R.T.: 0.000 min  
 Response: 7070677904  
 Conc: 695.01 ng/ml

#14 DINOSEB

R.T.: 10.881 min  
 Delta R.T.: 0.000 min  
 Response: 4118901701  
 Conc: 706.38 ng/ml

## #15 Picloram

R.T.: 10.685 min  
 Delta R.T.: 0.000 min  
 Response: 13255096434 ECD\_S  
 Conc: 723.11 ng/ml ClientSampleId :  
 ICVPS042325

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 04/24/2025  
 Supervised By :mohammad ahmed 04/26/2025

## #15 Picloram





R.T.: 11.923 min  
 Delta R.T.: 0.000 min  
 Response: 9024004077  
 Conc: 734.64 ng/ml

## #16 DCPA

R.T.: 11.167 min  
 Delta R.T.: 0.000 min  
 Response: 12285496361  
 Conc: 721.78 ng/ml

## #16 DCPA

R.T.: 11.918 min  
 Delta R.T.: 0.000 min  
 Response: 8142309135  
 Conc: 722.37 ng/ml

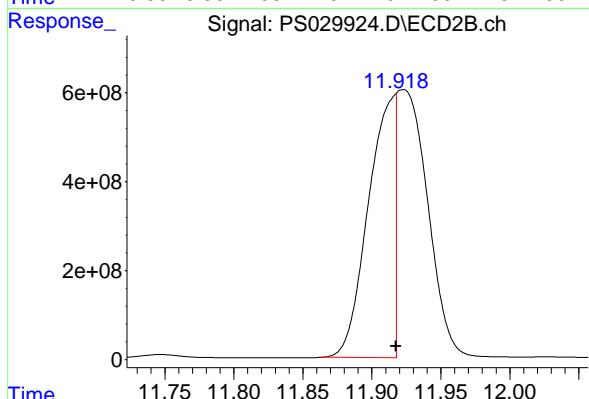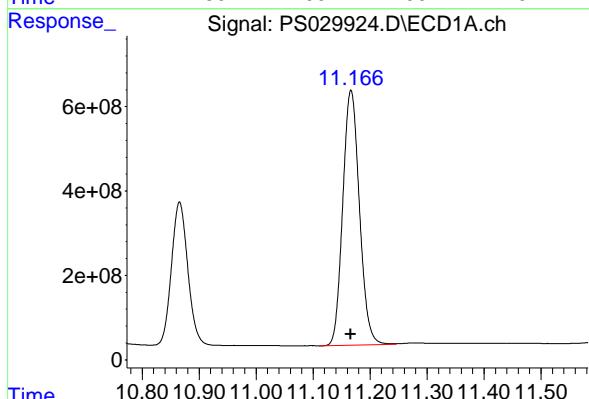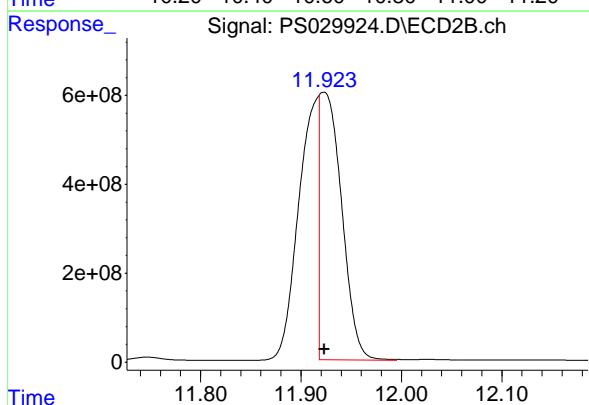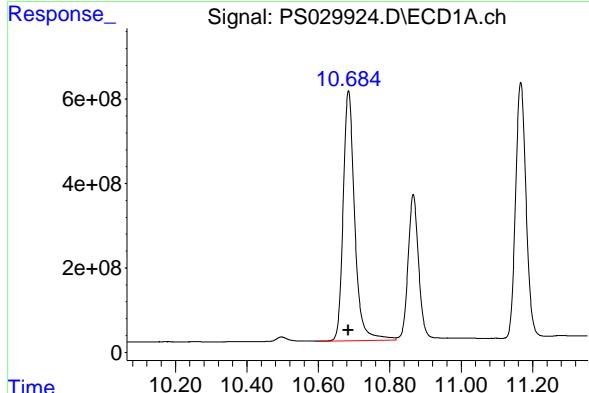



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

Continuing Calib Date: 05/01/2025 Initial Calibration Date(s): 04/23/2025 04/23/2025

Continuing Calib Time: 01:22 Initial Calibration Time(s): 11:01 12:37

GC Column: RTX-CLP ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
DICAMBA	7.12	7.12	7.02	7.22	0.00
2,4-DCAA	6.94	6.94	6.84	7.04	0.00
Dalapon	2.45	2.45	2.35	2.55	0.00
DICHLORPROP	7.80	7.80	7.70	7.90	0.00
2,4-D	8.02	8.02	7.92	8.12	0.00
2,4,5-TP(Silvex)	8.86	8.86	8.76	8.96	0.00
2,4,5-T	9.14	9.14	9.04	9.24	0.00
2,4-DB	9.70	9.70	9.60	9.80	0.00
Dinoseb	10.86	10.87	10.77	10.97	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

Continuing Calib Date: 05/01/2025 Initial Calibration Date(s): 04/23/2025 04/23/2025

Continuing Calib Time: 01:22 Initial Calibration Time(s): 11:01 12:37

GC Column: RTX-CLP2 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
DICAMBA	7.65	7.65	7.55	7.75	0.00
2,4-DCAA	7.46	7.47	7.37	7.57	0.01
Dalapon	2.52	2.53	2.43	2.63	0.01
DICHLORPROP	8.34	8.35	8.25	8.45	0.01
2,4-D	8.66	8.66	8.56	8.76	0.01
2,4,5-TP(Silvex)	9.53	9.54	9.44	9.64	0.01
2,4,5-T	9.94	9.95	9.85	10.05	0.01
2,4-DB	10.50	10.51	10.41	10.61	0.01
Dinoseb	10.87	10.88	10.78	10.98	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

GC Column: RTX-CLP ID: 0.32 (mm) Initi. Calib. Date(s): 04/23/2025 04/23/2025

Client Sample No.: CCAL01 Date Analyzed: 05/01/2025

Lab Sample No.: HSTDCCC750 Data File : PS029991.D Time Analyzed: 01:22

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
2,4,5-T	9.141	9.044	9.244	736.550	712.500	3.4
2,4,5-TP(Silvex)	8.858	8.762	8.962	730.550	712.500	2.5
2,4-D	8.016	7.919	8.119	715.650	705.000	1.5
2,4-DB	9.699	9.603	9.803	764.140	712.500	7.2
2,4-DCAA	6.939	6.842	7.042	758.550	750.000	1.1
Dalapon	2.449	2.349	2.549	706.400	682.500	3.5
DICAMBA	7.116	7.018	7.218	723.860	705.000	2.7
DICHLORPROP	7.796	7.699	7.899	704.420	705.000	-0.1
Dinoseb	10.861	10.766	10.966	714.800	705.000	1.4



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

GC Column: RTX-CLP2 ID: 0.32 (mm) Initi. Calib. Date(s): 04/23/2025 04/23/2025

Client Sample No.: CCAL01 Date Analyzed: 05/01/2025

Lab Sample No.: HSTDCCC750 Data File : PS029991.D Time Analyzed: 01:22

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
2,4,5-T	9.938	9.847	10.047	776.840	712.500	9.0
2,4,5-TP(Silvex)	9.534	9.442	9.642	786.260	712.500	10.4
2,4-D	8.655	8.561	8.761	748.240	705.000	6.1
2,4-DB	10.497	10.407	10.607	729.270	712.500	2.4
2,4-DCAA	7.463	7.367	7.567	801.050	750.000	6.8
Dalapon	2.523	2.425	2.625	711.230	682.500	4.2
DICAMBA	7.649	7.553	7.753	781.610	705.000	10.9
DICHLORPROP	8.342	8.248	8.448	757.570	705.000	7.5
Dinoseb	10.870	10.781	10.981	758.310	705.000	7.6

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS029991.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 01:22  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDCCC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 01 01:46:42 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

4) S 2,4-DCAA 6.939 7.463 1866.9E6 564.4E6 758.552 801.051

**Target Compounds**

1) T	Dalapon	2.449	2.523	2892.9E6	1234.8E6	706.400	711.228
2) T	3,5-DICHL...	6.143	6.460	2518.3E6	726.1E6	704.648	742.792
3) T	4-Nitroph...	6.729	6.996	1243.4E6	555.8E6	697.248	725.719
5) T	DICAMBA	7.116	7.649	7168.2E6	3087.4E6	723.855	781.611
6) T	MCPP	7.294	7.756	466.6E6	129.0E6	72.412	73.739
7) T	MCPA	7.437	7.986	642.6E6	171.6E6	72.763	72.534
8) T	DICHLORPROP	7.796	8.342	1785.1E6	760.6E6	704.424	757.567
9) T	2,4-D	8.016	8.655	2013.0E6	843.4E6	715.648	748.243
10) T	Pentachlo...	8.294	9.156	25792.5E6	16172.6E6	739.359	794.924
11) T	2,4,5-TP ...	8.858	9.534	10127.5E6	6432.9E6	730.547	786.255
12) T	2,4,5-T	9.141	9.938	10350.9E6	6030.3E6	736.554	776.838
13) T	2,4-DB	9.699	10.497	1746.3E6	586.9E6	764.144	729.270
14) T	DINOSEB	10.861	10.870	7271.9E6	4421.7E6	714.798	758.306
15) T	Picloram	10.680	11.908	13551.6E6	9856.9E6	739.289	802.440m
16) T	DCPA	11.163	11.903	12619.6E6	8081.5E6	741.412	716.977m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS029991.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 01:22  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1



Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 01 01:46:42 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation





Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDCCC750

### Manual Integrations APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

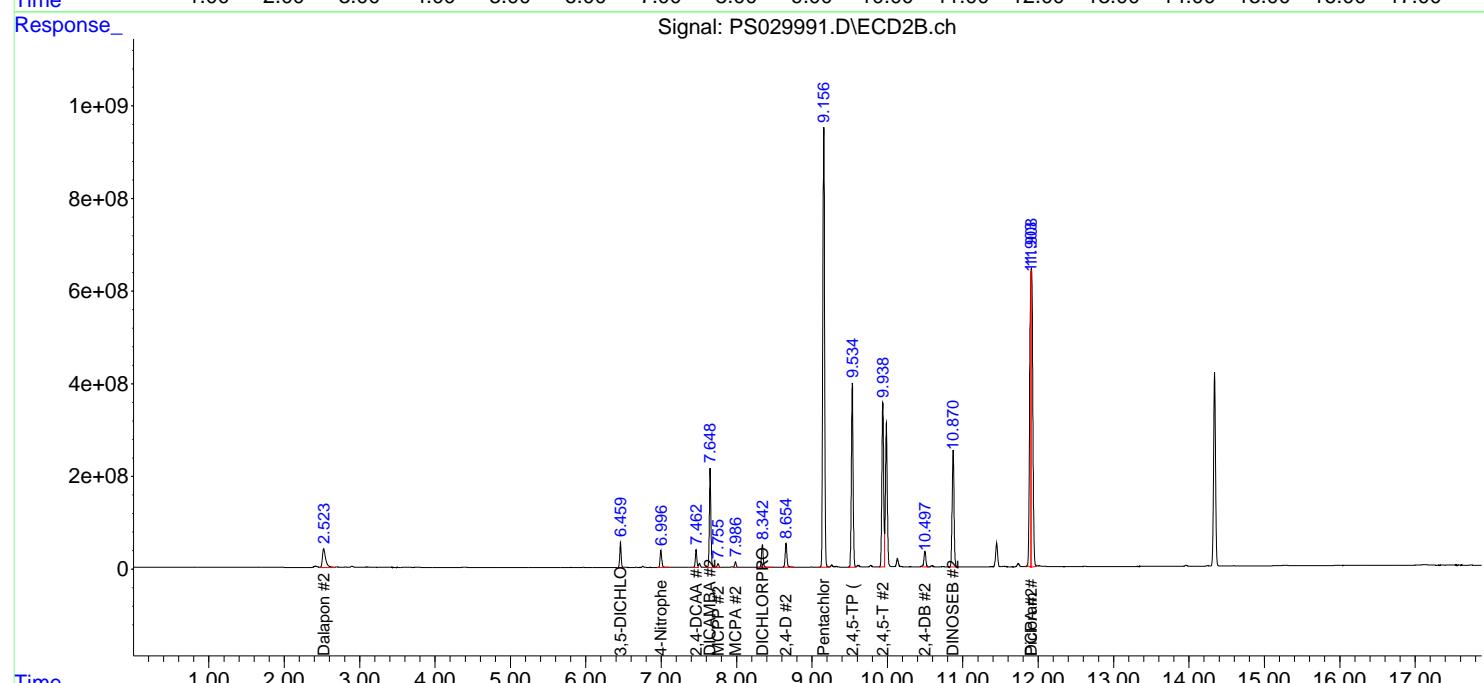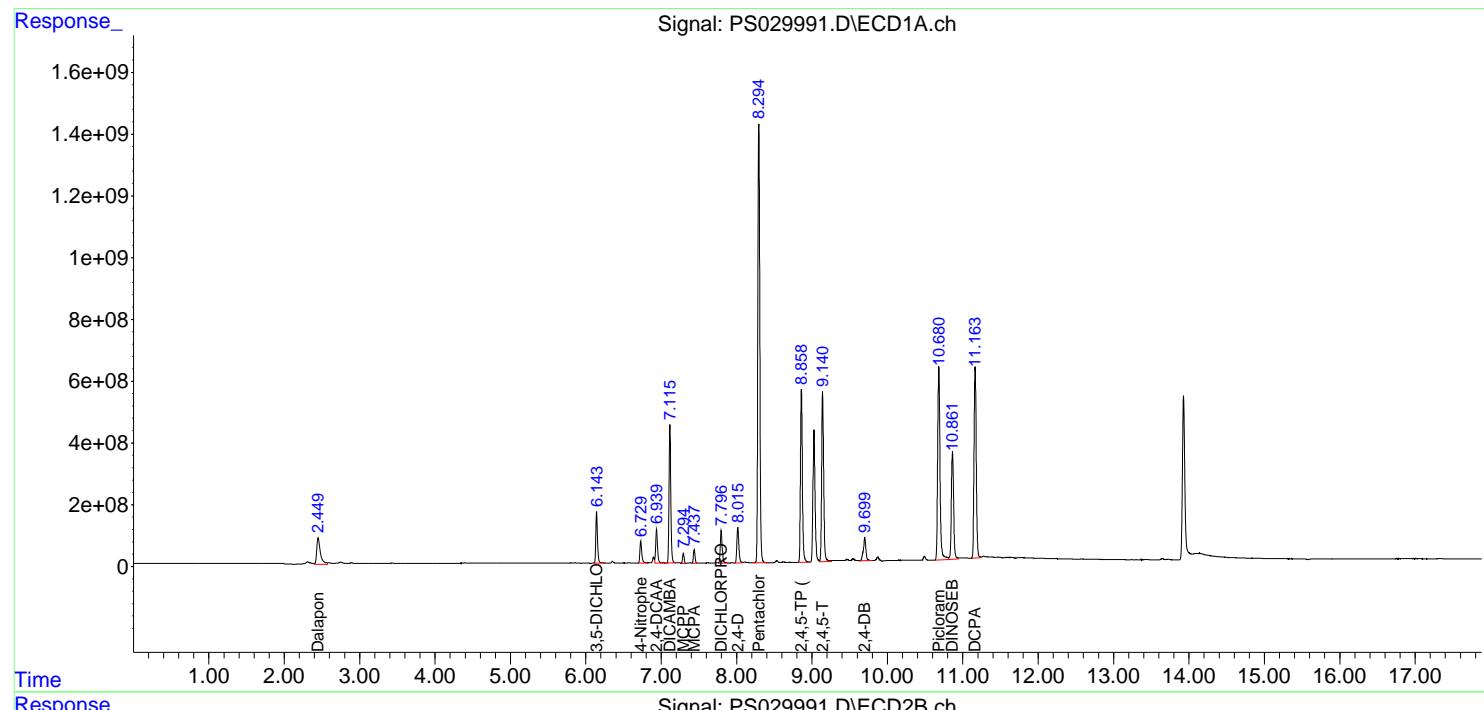

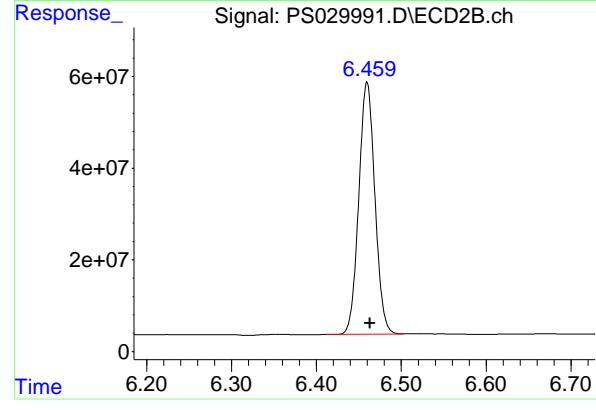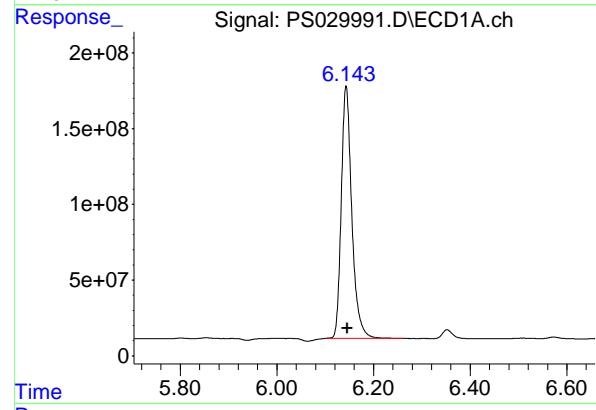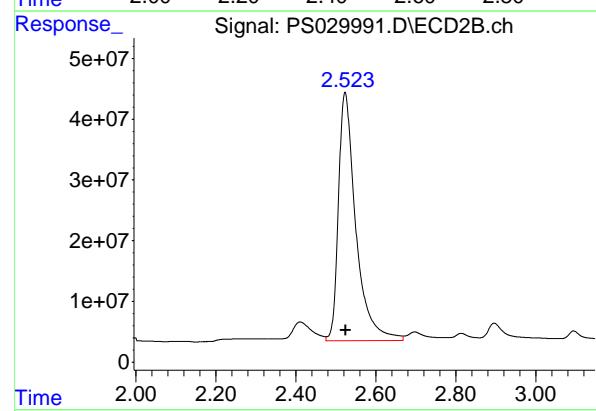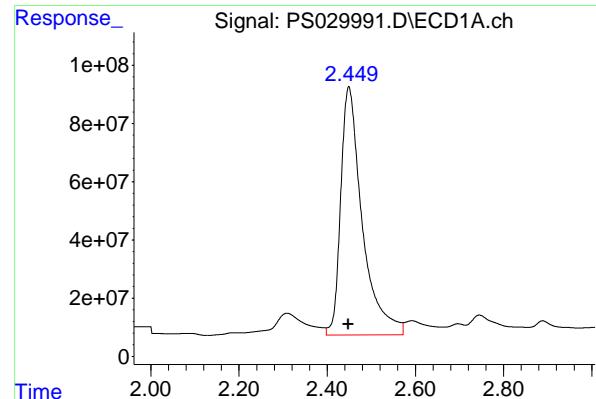

#1 Dalapon

R.T.: 2.449 min  
 Delta R.T.: 0.001 min  
 Response: 2892891563  
 Conc: 706.40 ng/ml  
 Instrument: ECD\_S  
 ClientSampleId : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

#1 Dalapon





R.T.: 2.523 min  
 Delta R.T.: -0.001 min  
 Response: 1234794085  
 Conc: 711.23 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.143 min  
 Delta R.T.: -0.002 min  
 Response: 2518260122  
 Conc: 704.65 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.460 min  
 Delta R.T.: -0.003 min  
 Response: 726137732  
 Conc: 742.79 ng/ml

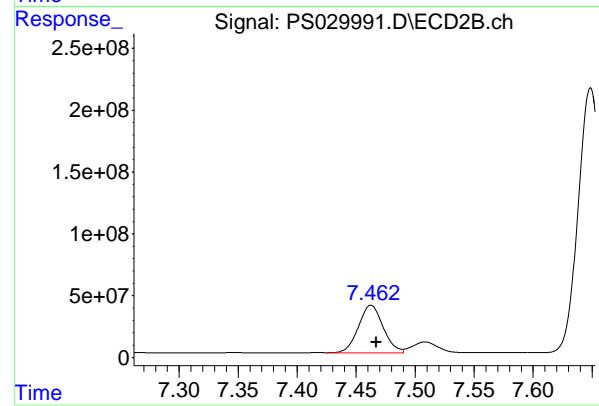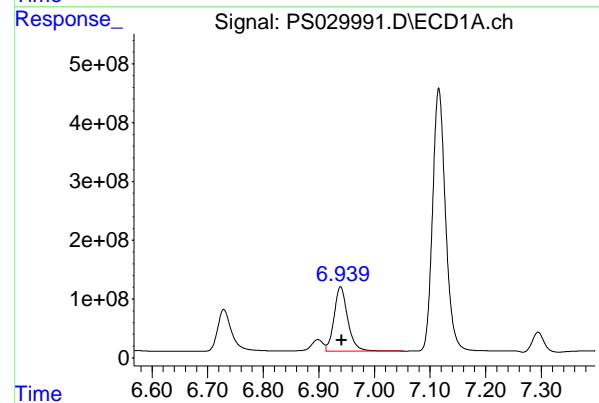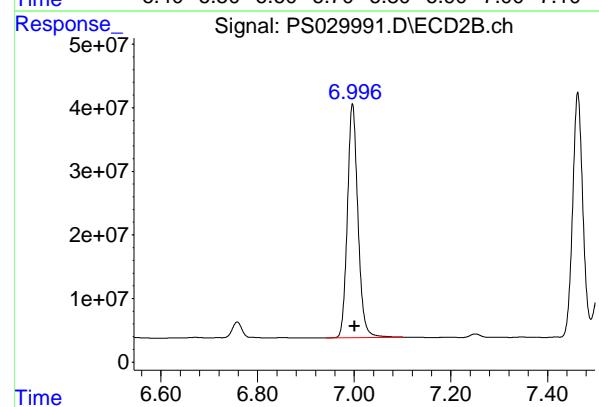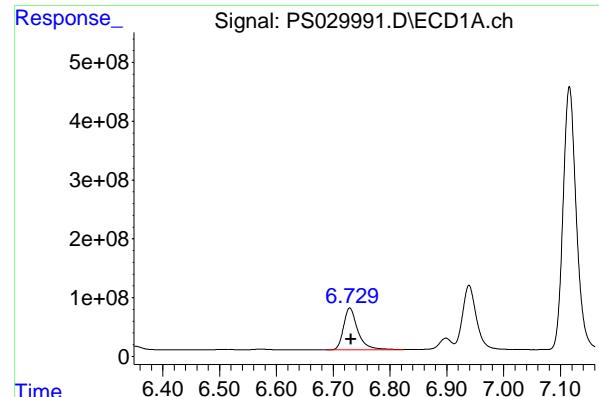

## #3 4-Nitrophenol

R.T.: 6.729 min  
Delta R.T.: -0.002 min  
Instrument: ECD\_S  
Response: 1243415669  
Conc: 697.25 ng/ml  
ClientSampleId: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
Supervised By :mohammad ahmed 05/02/2025

## #3 4-Nitrophenol


R.T.: 6.996 min  
Delta R.T.: -0.004 min  
Response: 555843920  
Conc: 725.72 ng/ml

## #4 2,4-DCAA

R.T.: 6.939 min  
Delta R.T.: -0.002 min  
Response: 1866856353  
Conc: 758.55 ng/ml

## #4 2,4-DCAA

R.T.: 7.463 min  
Delta R.T.: -0.004 min  
Response: 564353935  
Conc: 801.05 ng/ml

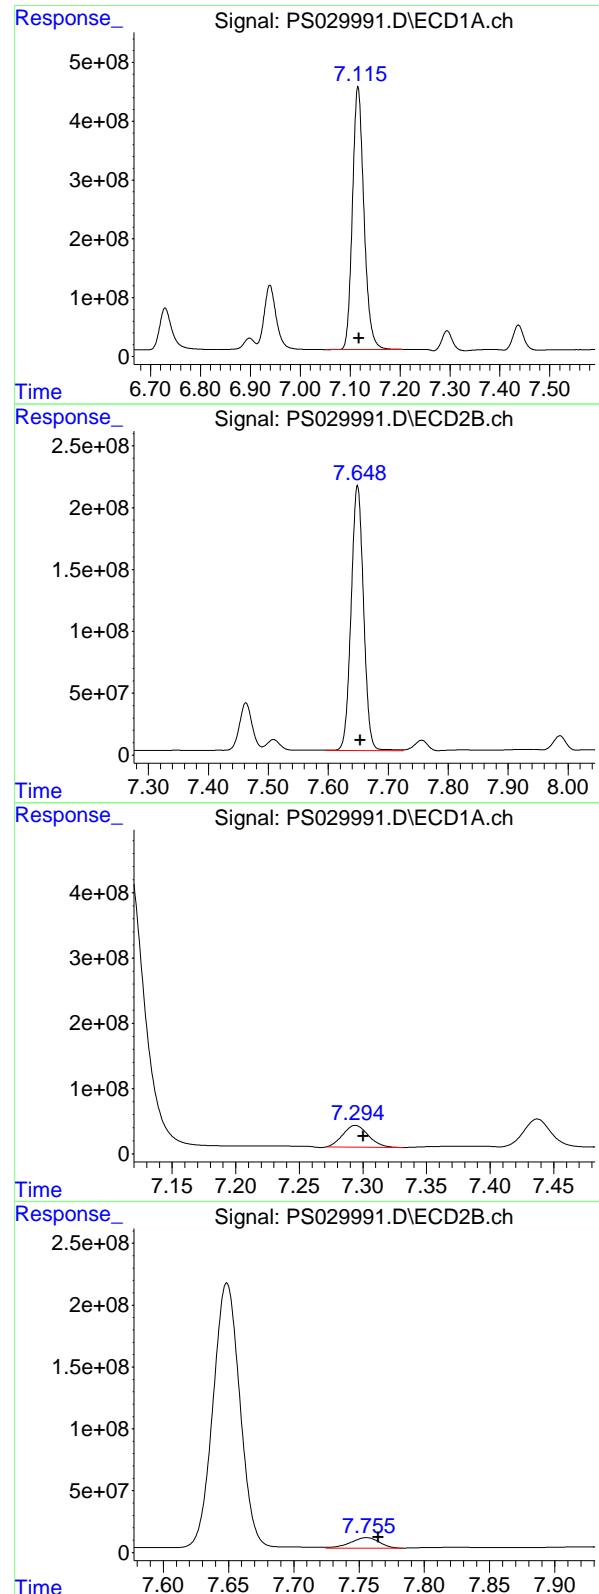

## #5 DICAMBA

R.T.: 7.116 min  
 Delta R.T.: -0.002 min  
 Response: 7168239889  
 Conc: 723.86 ng/ml  
 Instrument: ECD\_S  
 ClientSampleId : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

## #5 DICAMBA





R.T.: 7.649 min  
 Delta R.T.: -0.005 min  
 Response: 3087414925  
 Conc: 781.61 ng/ml

## #6 MCPP

R.T.: 7.294 min  
 Delta R.T.: -0.006 min  
 Response: 466598554  
 Conc: 72.41 ug/ml

## #6 MCPP

R.T.: 7.756 min  
 Delta R.T.: -0.009 min  
 Response: 128965896  
 Conc: 73.74 ug/ml

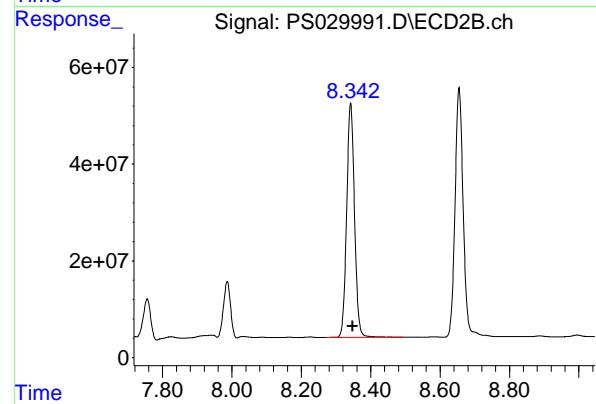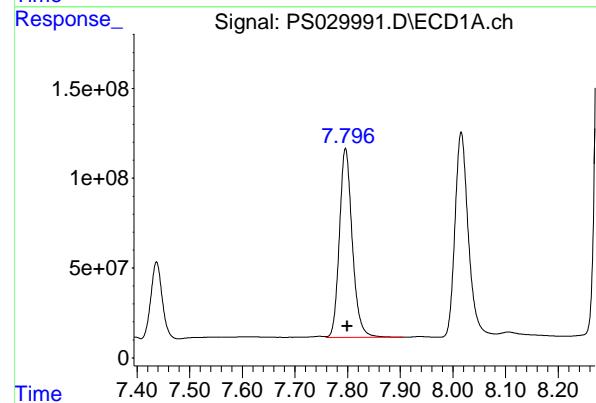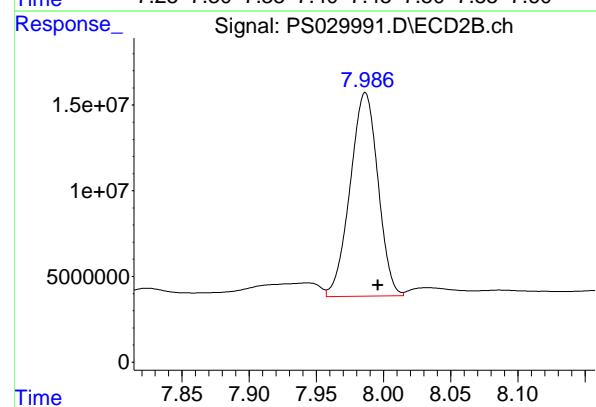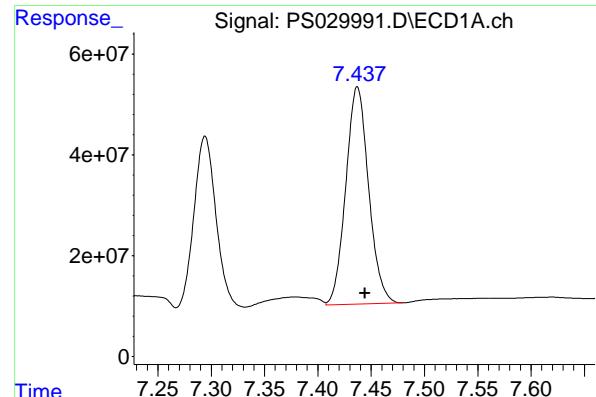

#7 MCPA

R.T.: 7.437 min  
 Delta R.T.: -0.007 min  
 Response: 642595119  
 Conc: 72.76 ug/ml

Instrument: ECD\_S  
 Client Sample Id: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

#7 MCPA





R.T.: 7.986 min  
 Delta R.T.: -0.009 min  
 Response: 171601600  
 Conc: 72.53 ug/ml

#8 DICHLORPROP

R.T.: 7.796 min  
 Delta R.T.: -0.003 min  
 Response: 1785086910  
 Conc: 704.42 ng/ml

#8 DICHLORPROP

R.T.: 8.342 min  
 Delta R.T.: -0.006 min  
 Response: 760570474  
 Conc: 757.57 ng/ml

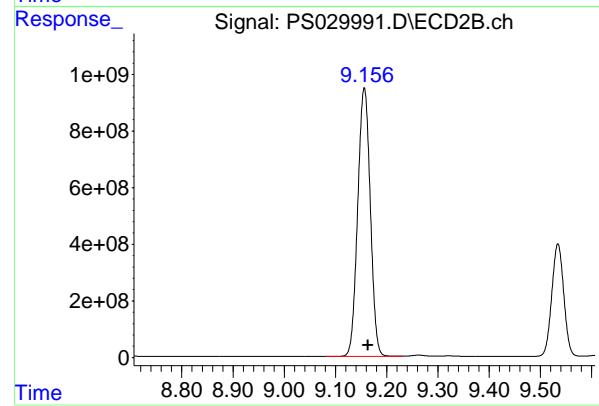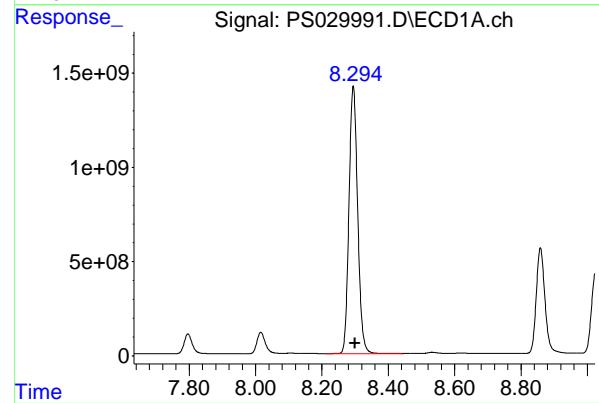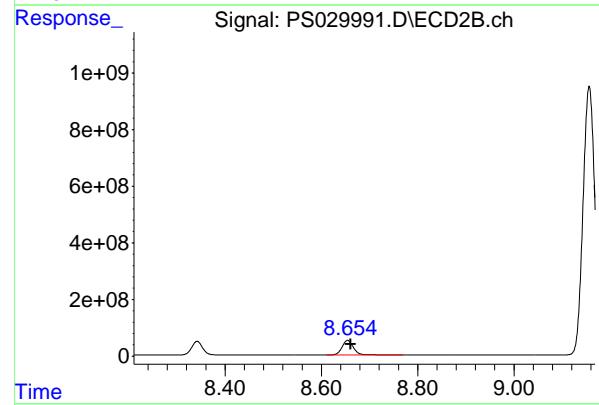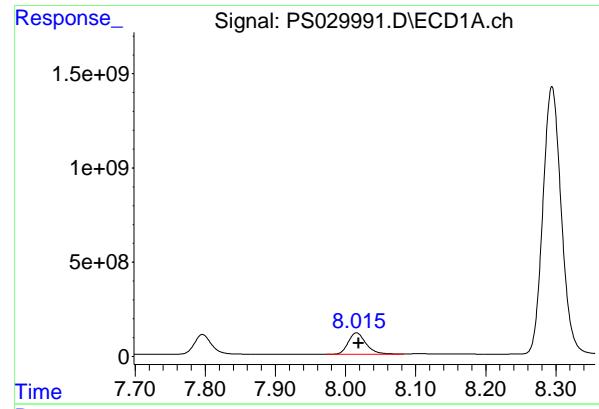

#9 2,4-D

R.T.: 8.016 min  
 Delta R.T.: -0.003 min  
 Response: 2013024091 ECD\_S  
 Conc: 715.65 ng/ml Client SampleId : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

#9 2,4-D





R.T.: 8.655 min  
 Delta R.T.: -0.007 min  
 Response: 843350175  
 Conc: 748.24 ng/ml

#10 Pentachlorophenol

R.T.: 8.294 min  
 Delta R.T.: -0.005 min  
 Response: 25792542501  
 Conc: 739.36 ng/ml

#10 Pentachlorophenol

R.T.: 9.156 min  
 Delta R.T.: -0.007 min  
 Response: 16172585032  
 Conc: 794.92 ng/ml

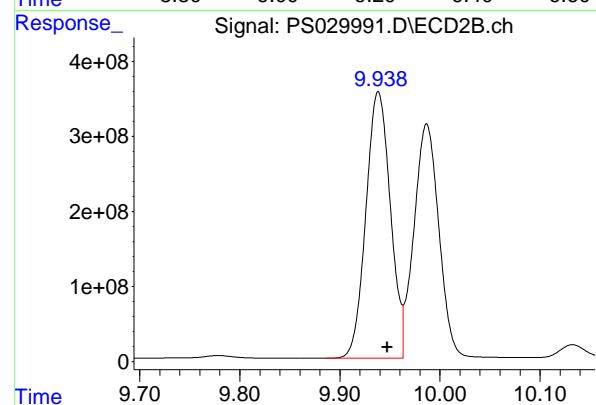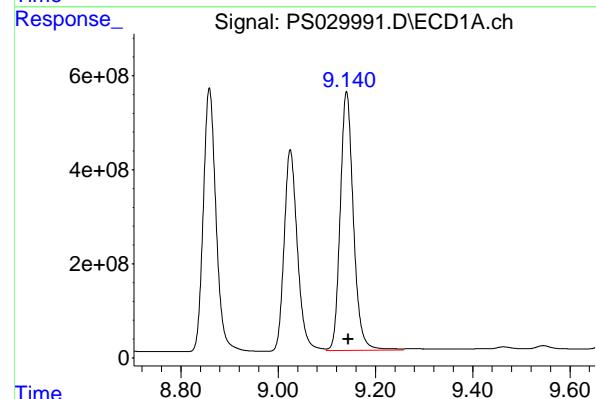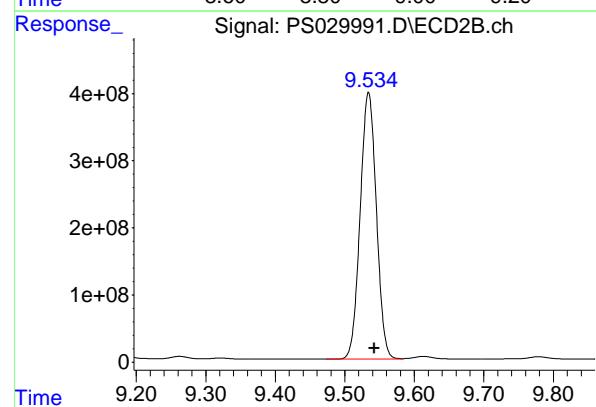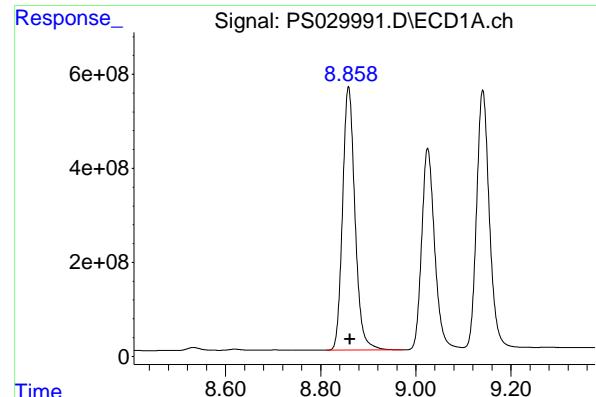

#11 2,4,5-TP (SILVEX)

R.T.: 8.858 min

Delta R.T.: -0.004 min

Instrument: ECD\_S

Response: 10127462888

Conc: 730.55 ng/ml

ClientSampleId:

HSTDCCC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/01/2025

Supervised By :mohammad ahmed 05/02/2025

#11 2,4,5-TP (SILVEX)

R.T.: 9.534 min

Delta R.T.: -0.008 min

Response: 6432945338

Conc: 786.26 ng/ml

#12 2,4,5-T

R.T.: 9.141 min

Delta R.T.: -0.003 min

Response: 10350875514

Conc: 736.55 ng/ml





#12 2,4,5-T

R.T.: 9.938 min

Delta R.T.: -0.009 min

Response: 6030280570

Conc: 776.84 ng/ml

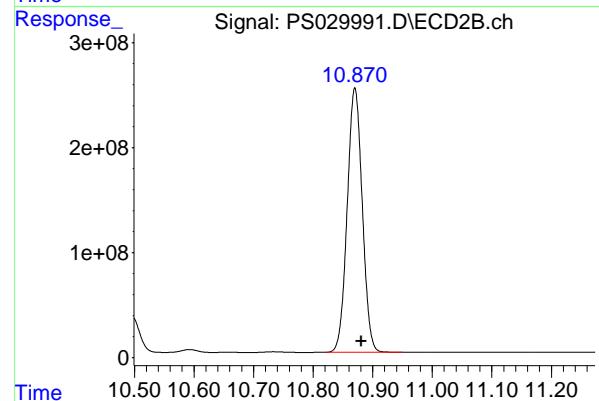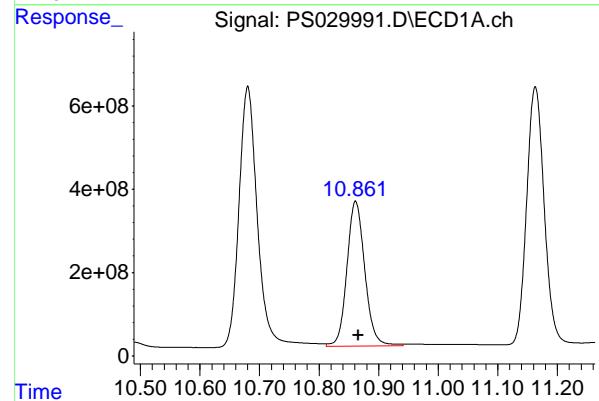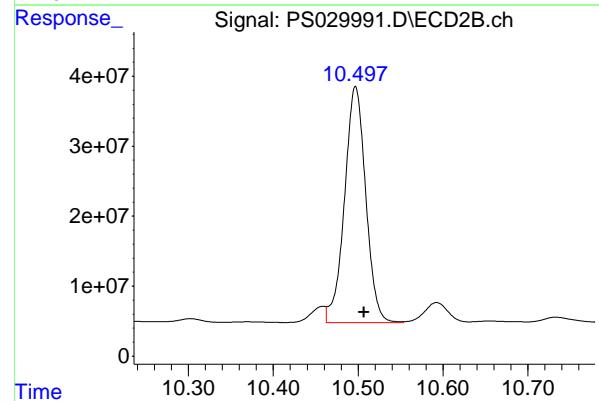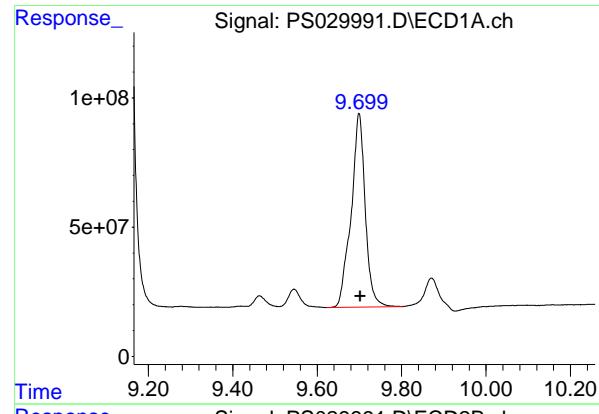

#13 2,4-DB

R.T.: 9.699 min  
Delta R.T.: -0.003 min  
Instrument: ECD\_S  
Response: 1746342018  
Conc: 764.14 ng/ml  
ClientSampleId: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
Supervised By :mohammad ahmed 05/02/2025

#13 2,4-DB


R.T.: 10.497 min  
Delta R.T.: -0.010 min  
Response: 586947234  
Conc: 729.27 ng/ml

#14 DINOSEB

R.T.: 10.861 min  
Delta R.T.: -0.005 min  
Response: 7271944355  
Conc: 714.80 ng/ml

#14 DINOSEB

R.T.: 10.870 min  
Delta R.T.: -0.011 min  
Response: 4421665636  
Conc: 758.31 ng/ml

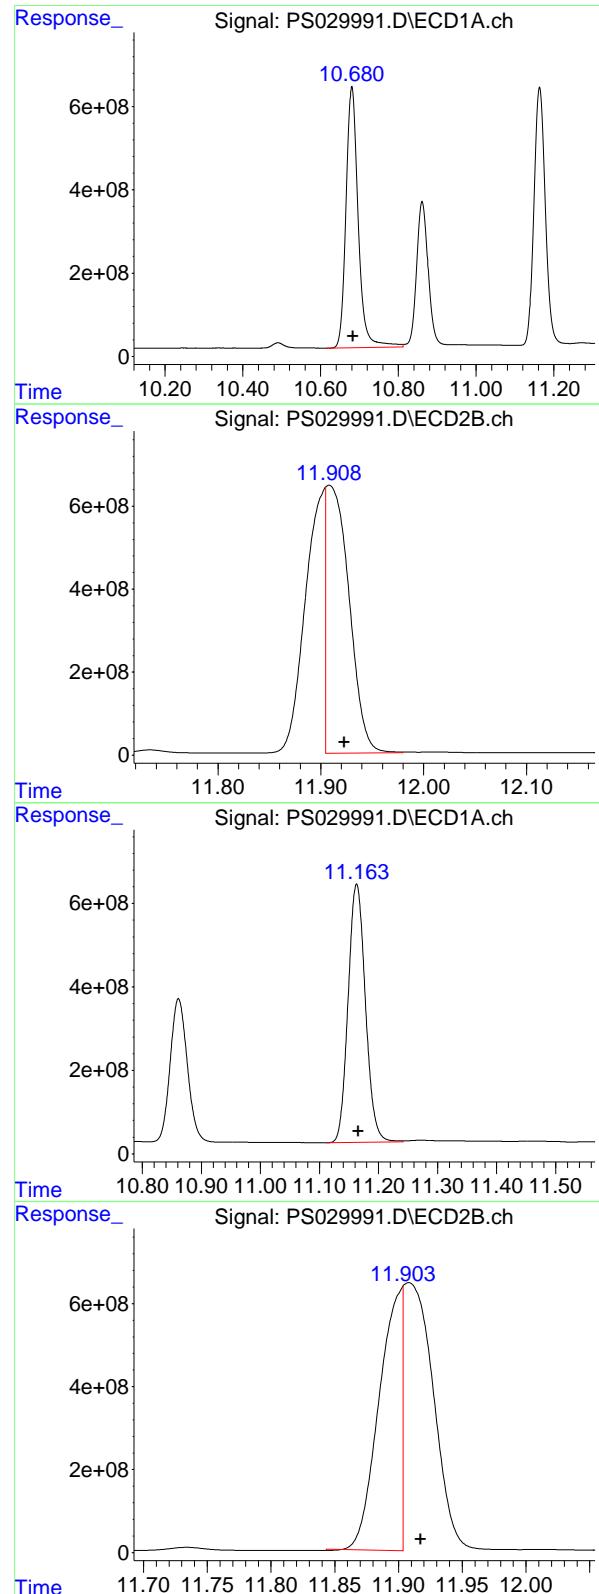

## #15 Picloram

R.T.: 10.680 min  
 Delta R.T.: -0.003 min  
 Response: 13551620682 ECD\_S  
 Conc: 739.29 ng/ml Client Sample ID : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

## #15 Picloram

R.T.: 11.908 min  
 Delta R.T.: -0.015 min  
 Response: 9856886671  
 Conc: 802.44 ng/ml

## #16 DCPA

R.T.: 11.163 min  
 Delta R.T.: -0.003 min  
 Response: 12619577763  
 Conc: 741.41 ng/ml

## #16 DCPA

R.T.: 11.903 min  
 Delta R.T.: -0.014 min  
 Response: 8081518817  
 Conc: 716.98 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

Continuing Calib Date: 05/01/2025 Initial Calibration Date(s): 04/23/2025 04/23/2025

Continuing Calib Time: 06:59 Initial Calibration Time(s): 11:01 12:37

GC Column: RTX-CLP ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
DICAMBA	7.12	7.12	7.02	7.22	0.01
2,4-DCAA	6.94	6.94	6.84	7.04	0.00
Dalapon	2.45	2.45	2.35	2.55	0.00
DICHLORPROP	7.80	7.80	7.70	7.90	0.00
2,4-D	8.02	8.02	7.92	8.12	0.00
2,4,5-TP(Silvex)	8.86	8.86	8.76	8.96	0.00
2,4,5-T	9.14	9.14	9.04	9.24	0.00
2,4-DB	9.70	9.70	9.60	9.80	0.00
Dinoseb	10.86	10.87	10.77	10.97	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

Continuing Calib Date: 05/01/2025 Initial Calibration Date(s): 04/23/2025 04/23/2025

Continuing Calib Time: 06:59 Initial Calibration Time(s): 11:01 12:37

GC Column: RTX-CLP2 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
DICAMBA	7.65	7.65	7.55	7.75	0.00
2,4-DCAA	7.46	7.47	7.37	7.57	0.01
Dalapon	2.52	2.53	2.43	2.63	0.01
DICHLORPROP	8.34	8.35	8.25	8.45	0.01
2,4-D	8.66	8.66	8.56	8.76	0.01
2,4,5-TP(Silvex)	9.53	9.54	9.44	9.64	0.01
2,4,5-T	9.94	9.95	9.85	10.05	0.01
2,4-DB	10.50	10.51	10.41	10.61	0.01
Dinoseb	10.87	10.88	10.78	10.98	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

GC Column: RTX-CLP ID: 0.32 (mm) Initi. Calib. Date(s): 04/23/2025 04/23/2025

Client Sample No.: CCAL02 Date Analyzed: 05/01/2025

Lab Sample No.: HSTDCCC750 Data File : PS030002.D Time Analyzed: 06:59

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
2,4,5-T	9.140	9.044	9.244	722.200	712.500	1.4
2,4,5-TP(Silvex)	8.858	8.762	8.962	720.000	712.500	1.1
2,4-D	8.015	7.919	8.119	700.150	705.000	-0.7
2,4-DB	9.698	9.603	9.803	748.260	712.500	5.0
2,4-DCAA	6.939	6.842	7.042	735.570	750.000	-1.9
Dalapon	2.449	2.349	2.549	677.710	682.500	-0.7
DICAMBA	7.115	7.018	7.218	705.880	705.000	0.1
DICHLORPROP	7.796	7.699	7.899	687.850	705.000	-2.4
Dinoseb	10.860	10.766	10.966	690.110	705.000	-2.1



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

GC Column: RTX-CLP2 ID: 0.32 (mm) Initi. Calib. Date(s): 04/23/2025 04/23/2025

Client Sample No.: CCAL02 Date Analyzed: 05/01/2025

Lab Sample No.: HSTDCCC750 Data File : PS030002.D Time Analyzed: 06:59

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
2,4,5-T	9.938	9.847	10.047	770.350	712.500	8.1
2,4,5-TP(Silvex)	9.534	9.442	9.642	779.550	712.500	9.4
2,4-D	8.655	8.561	8.761	741.780	705.000	5.2
2,4-DB	10.496	10.407	10.607	739.380	712.500	3.8
2,4-DCAA	7.462	7.367	7.567	794.140	750.000	5.9
Dalapon	2.523	2.425	2.625	696.160	682.500	2.0
DICAMBA	7.648	7.553	7.753	780.920	705.000	10.8
DICHLORPROP	8.342	8.248	8.448	760.750	705.000	7.9
Dinoseb	10.870	10.781	10.981	739.550	705.000	4.9

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS030002.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 06:59  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDCCC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 01 07:14:45 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

4) S 2,4-DCAA 6.939 7.462 1810.3E6 559.5E6 735.571 794.137

**Target Compounds**

1) T	Dalapon	2.449	2.523	2775.4E6	1208.6E6	677.707	696.158
2) T	3,5-DICHL...	6.143	6.459	2465.8E6	721.5E6	689.978	738.090
3) T	4-Nitroph...	6.729	6.996	1209.4E6	555.7E6	678.175	725.560
5) T	DICAMBA	7.115	7.648	6990.3E6	3084.7E6	705.883	780.916
6) T	MCPP	7.294	7.756	452.6E6	123.1E6	70.239	70.364
7) T	MCPA	7.437	7.986	612.8E6	164.2E6	69.392	69.420
8) T	DICHLORPROP	7.796	8.342	1743.1E6	763.8E6	687.852	760.753
9) T	2,4-D	8.015	8.655	1969.4E6	836.1E6	700.153	741.775
10) T	Pentachlo...	8.294	9.155	25274.2E6	16072.4E6	724.501	790.000
11) T	2,4,5-TP ...	8.858	9.534	9981.3E6	6378.1E6	720.003	779.555
12) T	2,4,5-T	9.140	9.938	10149.2E6	5979.9E6	722.205	770.353
13) T	2,4-DB	9.698	10.496	1710.1E6	595.1E6	748.265	739.381
14) T	DINOSEB	10.860	10.870	7020.8E6	4312.3E6	690.113	739.552
15) T	Picloram	10.679	11.907	13213.8E6	9663.9E6	720.858	786.730m
16) T	DCPA	11.162	11.904	12337.1E6	8644.1E6	724.817	766.893m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS030002.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 06:59  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1



Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 01 07:14:45 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation





Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDCCC750

### Manual Integrations APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

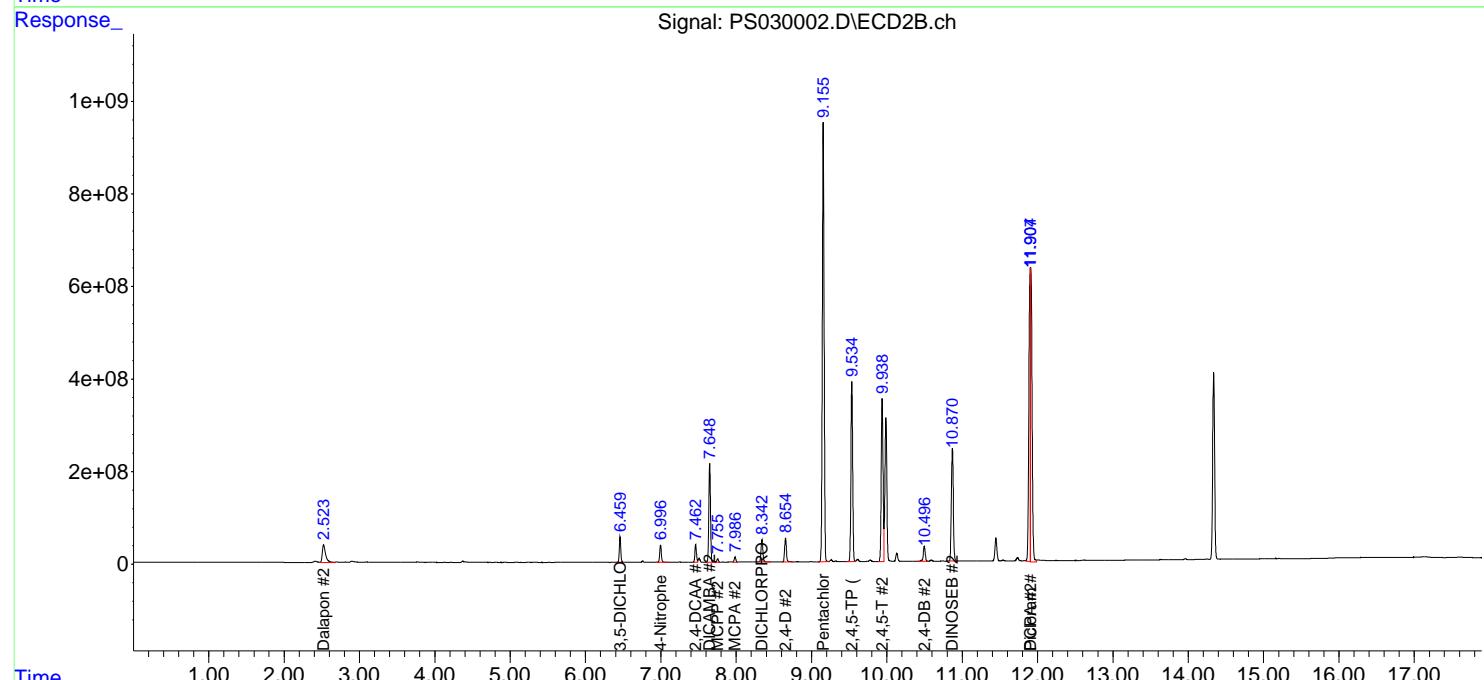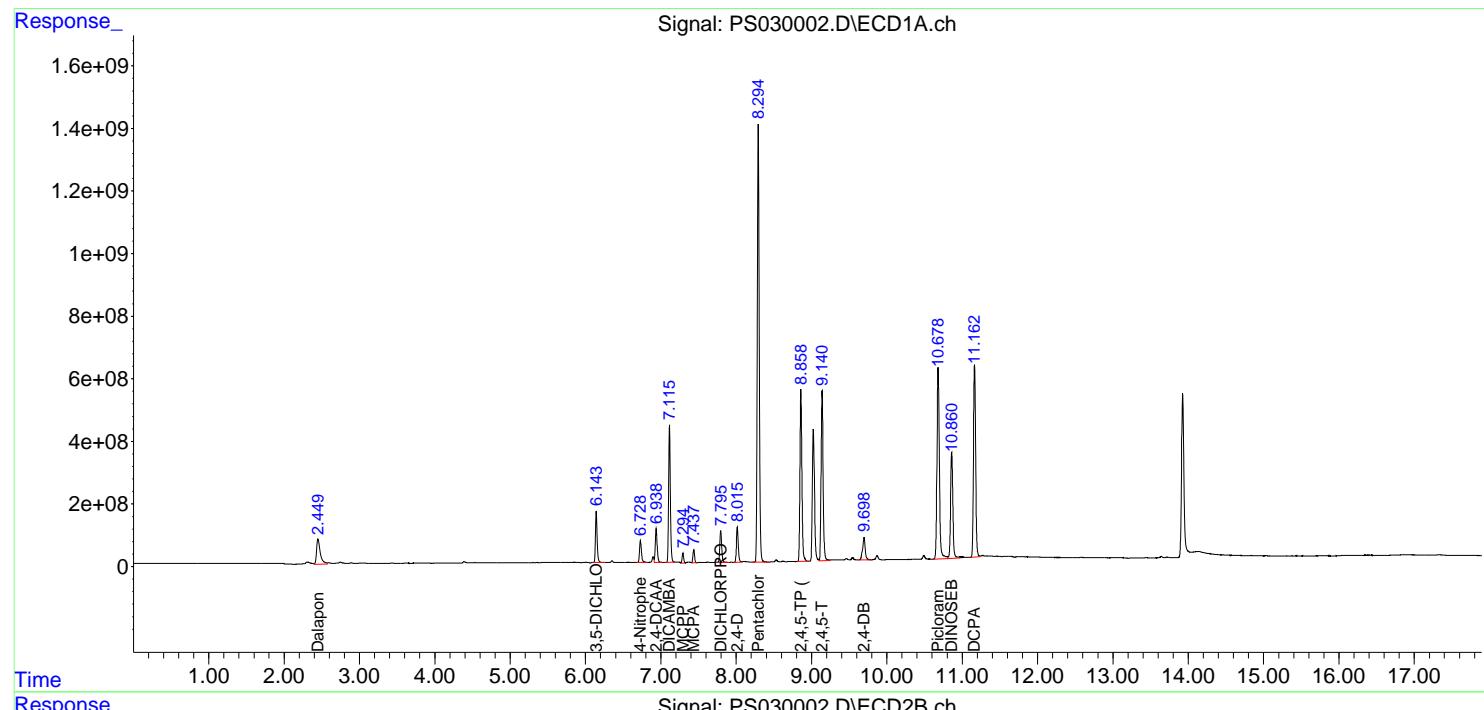

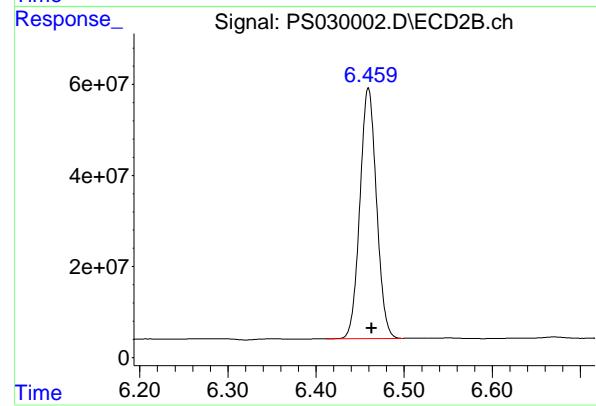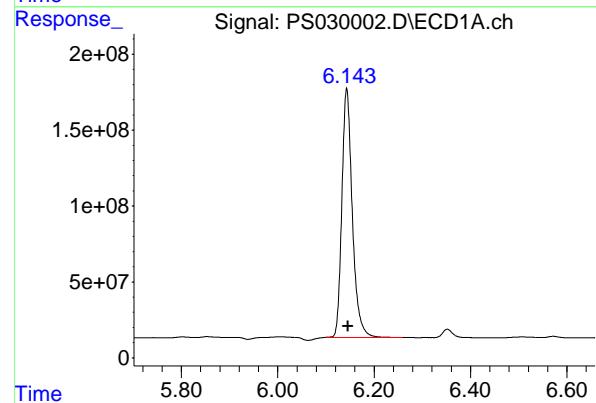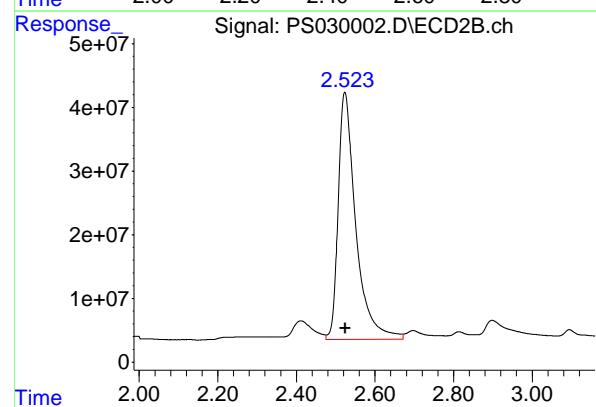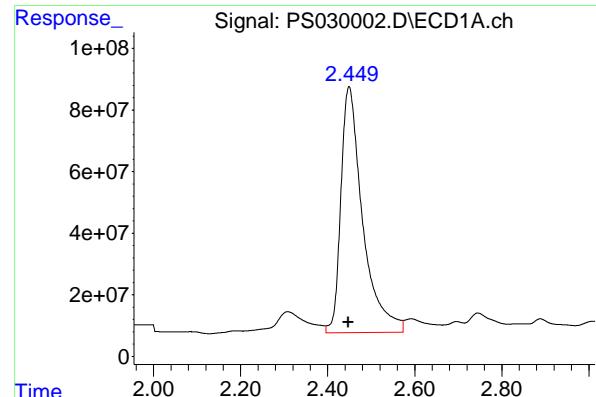

#1 Dalapon

R.T.: 2.449 min  
 Delta R.T.: 0.001 min  
 Response: 2775385295  
 Conc: 677.71 ng/ml

Instrument: ECD\_S  
 Client Sample Id: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

#1 Dalapon





R.T.: 2.523 min  
 Delta R.T.: 0.000 min  
 Response: 1208630888  
 Conc: 696.16 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.143 min  
 Delta R.T.: -0.002 min  
 Response: 2465834422  
 Conc: 689.98 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.459 min  
 Delta R.T.: -0.004 min  
 Response: 721541539  
 Conc: 738.09 ng/ml

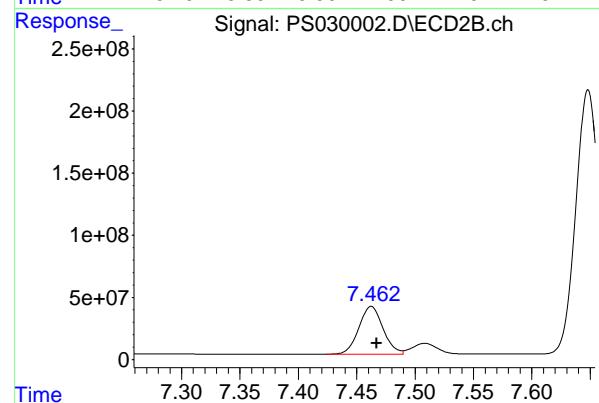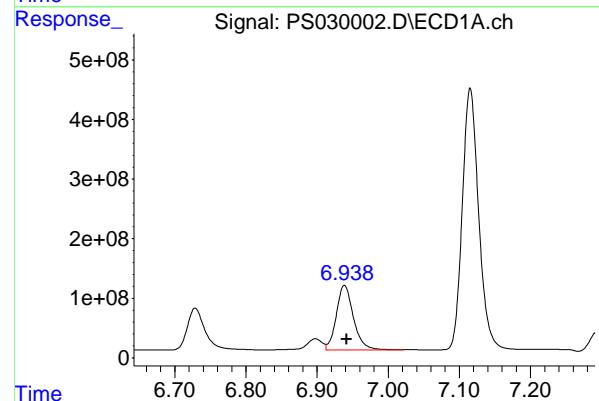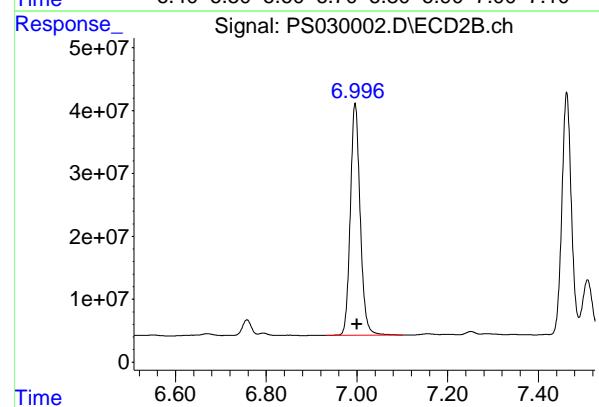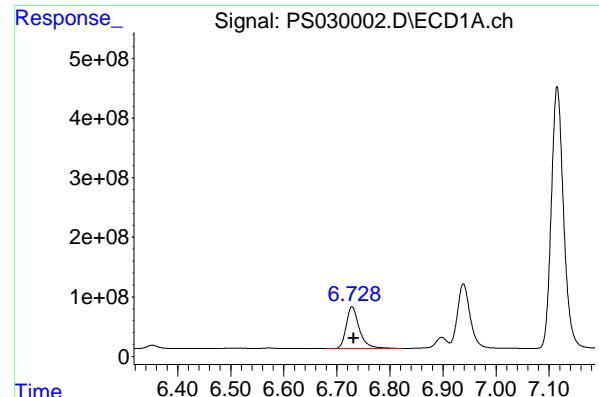

## #3 4-Nitrophenol

R.T.: 6.729 min  
Delta R.T.: -0.003 min  
Instrument: ECD\_S  
Response: 1209402202  
Conc: 678.17 ng/ml  
ClientSampleId: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
Supervised By :mohammad ahmed 05/02/2025

## #3 4-Nitrophenol





R.T.: 6.996 min  
Delta R.T.: -0.005 min  
Response: 555722167  
Conc: 725.56 ng/ml

## #4 2,4-DCAA

R.T.: 6.939 min  
Delta R.T.: -0.003 min  
Response: 1810298034  
Conc: 735.57 ng/ml

## #4 2,4-DCAA

R.T.: 7.462 min  
Delta R.T.: -0.005 min  
Response: 559483066  
Conc: 794.14 ng/ml

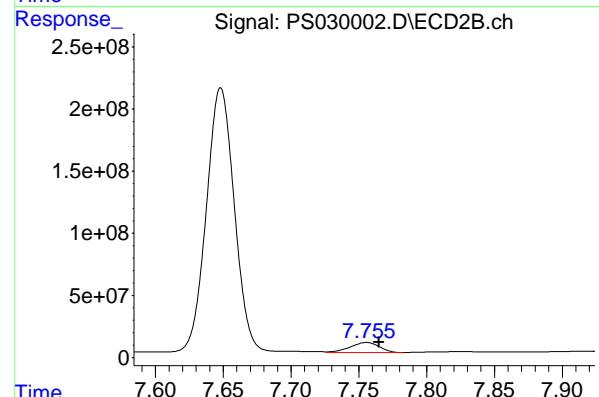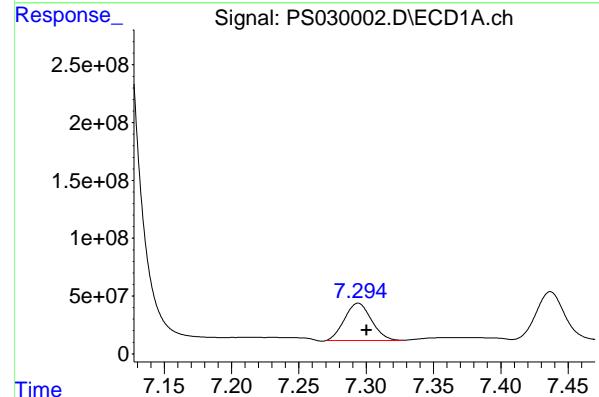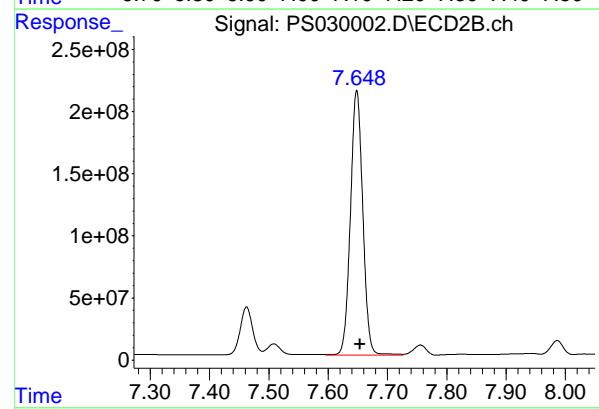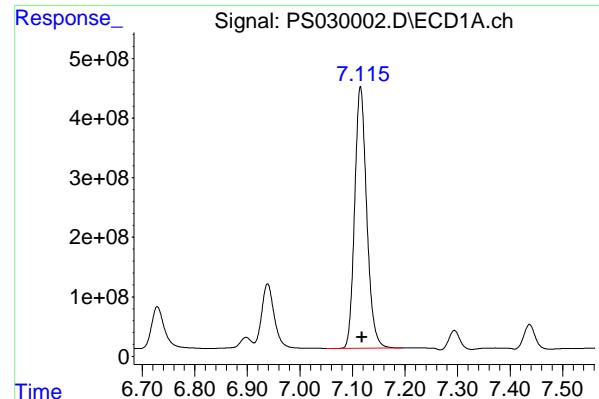

## #5 DICAMBA

R.T.: 7.115 min  
Delta R.T.: -0.003 min  
Instrument: ECD\_S  
Response: 6990261354  
Conc: 705.88 ng/ml  
ClientSampleId: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
Supervised By :mohammad ahmed 05/02/2025

## #5 DICAMBA





R.T.: 7.648 min  
Delta R.T.: -0.005 min  
Response: 3084666816  
Conc: 780.92 ng/ml

## #6 MCPP

R.T.: 7.294 min  
Delta R.T.: -0.006 min  
Response: 452596677  
Conc: 70.24 ug/ml

## #6 MCPP

R.T.: 7.756 min  
Delta R.T.: -0.009 min  
Response: 123062529  
Conc: 70.36 ug/ml

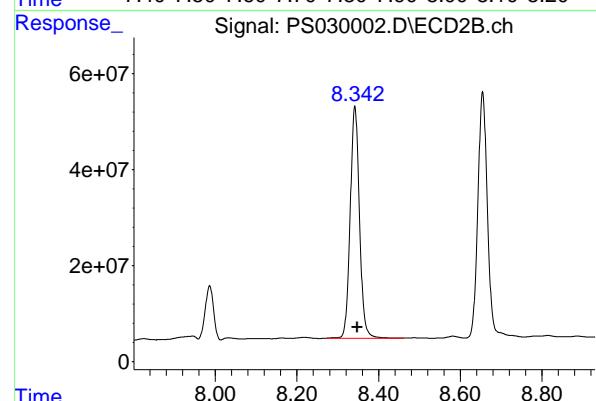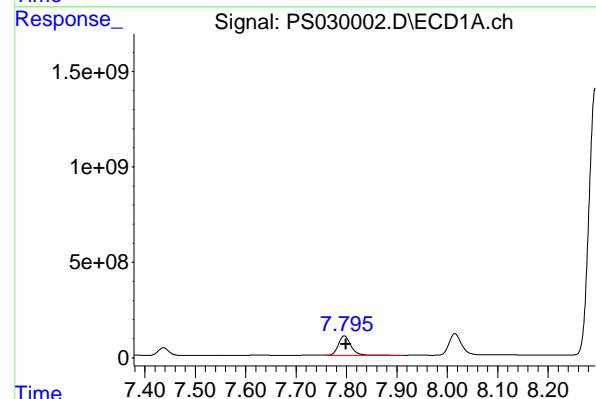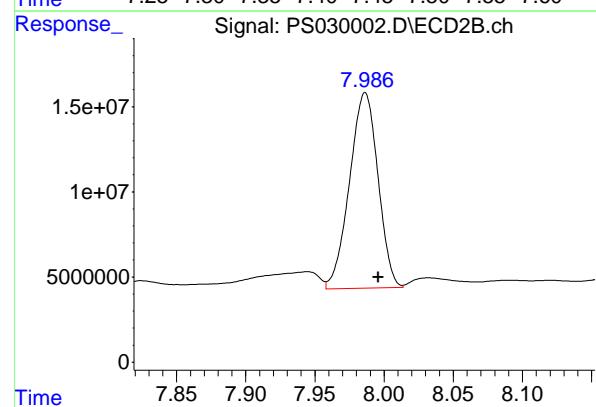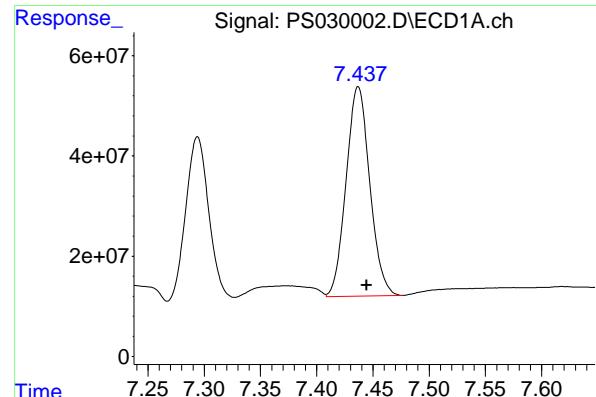

#7 MCPA

R.T.: 7.437 min  
 Delta R.T.: -0.008 min  
 Response: 612821796 ECD\_S  
 Conc: 69.39 ug/ml ClientSampleId : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

#7 MCPA





R.T.: 7.986 min  
 Delta R.T.: -0.009 min  
 Response: 164234366  
 Conc: 69.42 ug/ml

#8 DICHLORPROP

R.T.: 7.796 min  
 Delta R.T.: -0.003 min  
 Response: 1743091262  
 Conc: 687.85 ng/ml

#8 DICHLORPROP

R.T.: 8.342 min  
 Delta R.T.: -0.006 min  
 Response: 763768910  
 Conc: 760.75 ng/ml

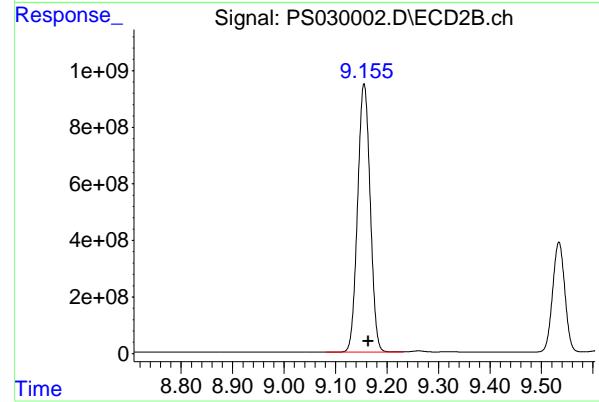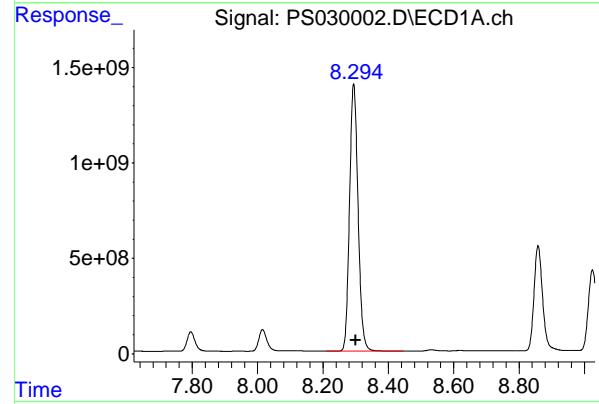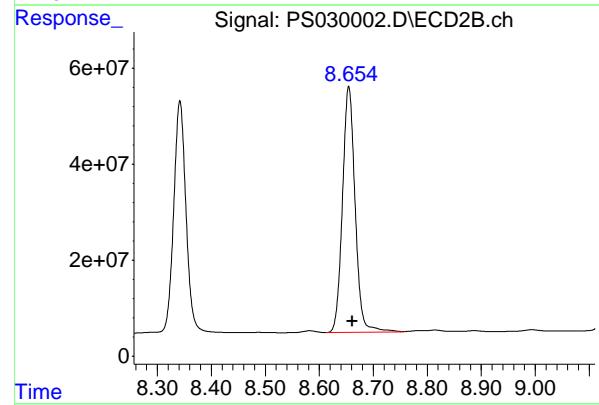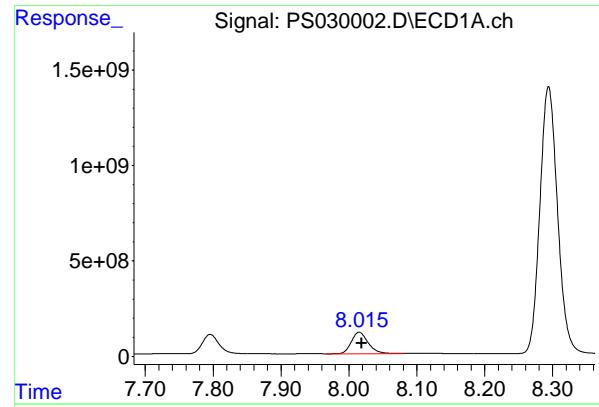

#9 2,4-D

R.T.: 8.015 min  
 Delta R.T.: -0.004 min  
 Response: 1969440235  
 Conc: 700.15 ng/ml

Instrument: ECD\_S  
 Client Sample Id: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

#9 2,4-D


R.T.: 8.655 min  
 Delta R.T.: -0.006 min  
 Response: 836059988  
 Conc: 741.78 ng/ml

#10 Pentachlorophenol

R.T.: 8.294 min  
 Delta R.T.: -0.006 min  
 Response: 25274216279  
 Conc: 724.50 ng/ml

#10 Pentachlorophenol

R.T.: 9.155 min  
 Delta R.T.: -0.008 min  
 Response: 16072410428  
 Conc: 790.00 ng/ml

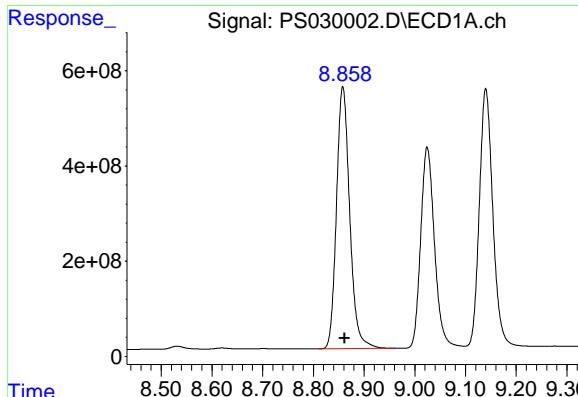


#11 2,4,5-TP (SILVEX)

R.T.: 8.858 min  
Delta R.T.: -0.004 min  
Instrument: ECD\_S  
Response: 9981291001  
Conc: 720.00 ng/ml  
ClientSampleId: HSTDCCC750


Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
Supervised By :mohammad ahmed 05/02/2025

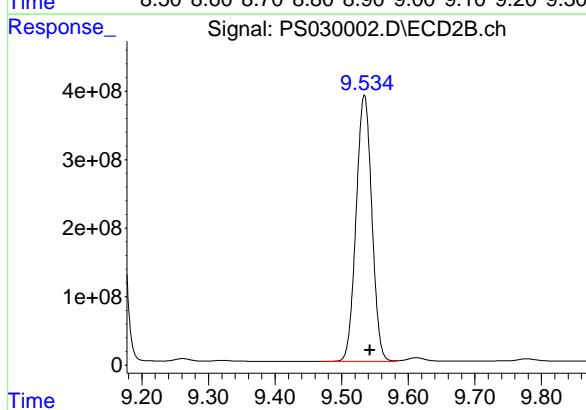


#11 2,4,5-TP (SILVEX)

R.T.: 9.534 min  
Delta R.T.: -0.009 min  
Response: 6378120993  
Conc: 779.55 ng/ml

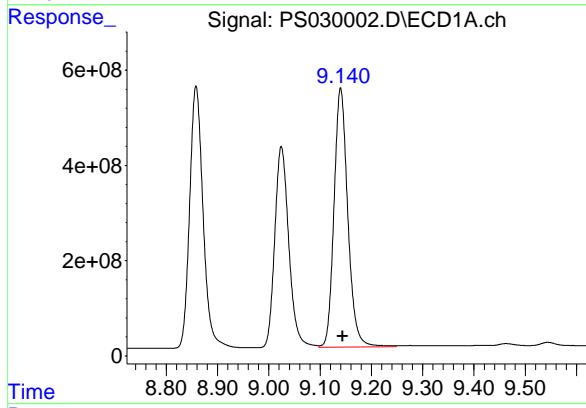


#12 2,4,5-T

R.T.: 9.140 min  
Delta R.T.: -0.004 min  
Response: 10149222516  
Conc: 722.20 ng/ml

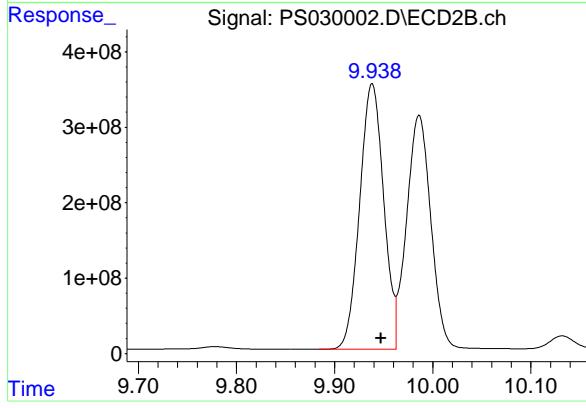

#12 2,4,5-T

R.T.: 9.938 min  
Delta R.T.: -0.009 min  
Response: 5979942577  
Conc: 770.35 ng/ml

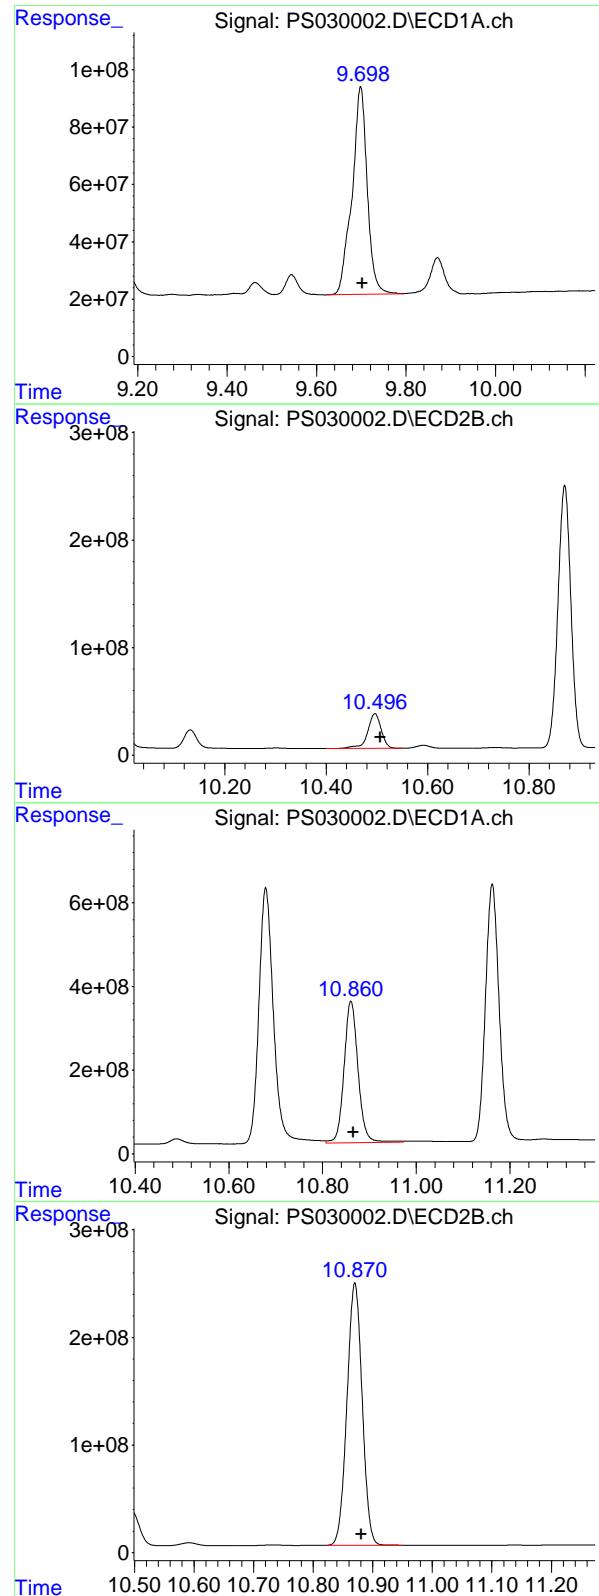

#13 2,4-DB

R.T.: 9.698 min  
 Delta R.T.: -0.004 min  
 Response: 1710051124 ECD\_S  
 Conc: 748.26 ng/ml Client SampleId : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

#13 2,4-DB


R.T.: 10.496 min  
 Delta R.T.: -0.010 min  
 Response: 595085100  
 Conc: 739.38 ng/ml

#14 DINOSEB

R.T.: 10.860 min  
 Delta R.T.: -0.005 min  
 Response: 7020810578  
 Conc: 690.11 ng/ml

#14 DINOSEB

R.T.: 10.870 min  
 Delta R.T.: -0.011 min  
 Response: 4312313988  
 Conc: 739.55 ng/ml

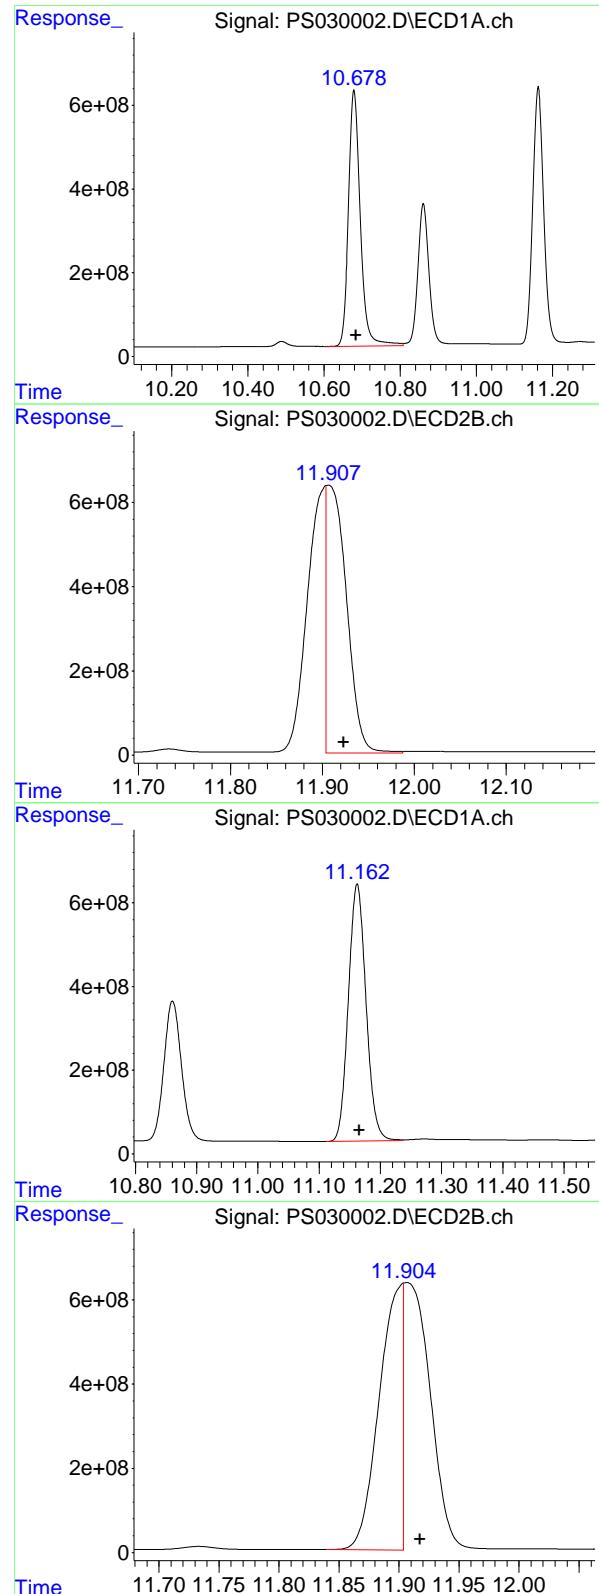

## #15 Picloram

R.T.: 10.679 min  
 Delta R.T.: -0.005 min  
 Instrument: ECD\_S  
 Response: 13213782052  
 Conc: 720.86 ng/ml  
 ClientSampleId: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

## #15 Picloram

R.T.: 11.907 min  
 Delta R.T.: -0.016 min  
 Response: 9663913283  
 Conc: 786.73 ng/ml

## #16 DCPA

R.T.: 11.162 min  
 Delta R.T.: -0.004 min  
 Response: 12337113007  
 Conc: 724.82 ng/ml

## #16 DCPA

R.T.: 11.904 min  
 Delta R.T.: -0.014 min  
 Response: 8644146772  
 Conc: 766.89 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

Continuing Calib Date: 05/01/2025 Initial Calibration Date(s): 04/23/2025 04/23/2025

Continuing Calib Time: 12:12 Initial Calibration Time(s): 11:01 12:37

GC Column: RTX-CLP ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
DICAMBA	7.12	7.12	7.02	7.22	0.00
2,4-DCAA	6.94	6.94	6.84	7.04	0.00
Dalapon	2.45	2.45	2.35	2.55	0.00
DICHLORPROP	7.80	7.80	7.70	7.90	0.00
2,4-D	8.02	8.02	7.92	8.12	0.00
2,4,5-TP(Silvex)	8.86	8.86	8.76	8.96	0.00
2,4,5-T	9.14	9.14	9.04	9.24	0.00
2,4-DB	9.70	9.70	9.60	9.80	0.00
Dinoseb	10.86	10.87	10.77	10.97	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

Continuing Calib Date: 05/01/2025 Initial Calibration Date(s): 04/23/2025 04/23/2025

Continuing Calib Time: 12:12 Initial Calibration Time(s): 11:01 12:37

GC Column: RTX-CLP2 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
DICAMBA	7.65	7.65	7.55	7.75	0.00
2,4-DCAA	7.46	7.47	7.37	7.57	0.01
Dalapon	2.52	2.53	2.43	2.63	0.01
DICHLORPROP	8.34	8.35	8.25	8.45	0.01
2,4-D	8.65	8.66	8.56	8.76	0.01
2,4,5-TP(Silvex)	9.53	9.54	9.44	9.64	0.01
2,4,5-T	9.94	9.95	9.85	10.05	0.01
2,4-DB	10.50	10.51	10.41	10.61	0.02
Dinoseb	10.87	10.88	10.78	10.98	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

GC Column: RTX-CLP ID: 0.32 (mm) Initi. Calib. Date(s): 04/23/2025 04/23/2025

Client Sample No.: CCAL03 Date Analyzed: 05/01/2025

Lab Sample No.: HSTDCCC750 Data File : PS030013.D Time Analyzed: 12:12

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
2,4,5-T	9.140	9.044	9.244	745.600	712.500	4.6
2,4,5-TP(Silvex)	8.858	8.762	8.962	742.010	712.500	4.1
2,4-D	8.015	7.919	8.119	720.060	705.000	2.1
2,4-DB	9.698	9.603	9.803	763.740	712.500	7.2
2,4-DCAA	6.939	6.842	7.042	760.450	750.000	1.4
Dalapon	2.450	2.349	2.549	694.070	682.500	1.7
DICAMBA	7.116	7.018	7.218	728.740	705.000	3.4
DICHLORPROP	7.796	7.699	7.899	708.330	705.000	0.5
Dinoseb	10.861	10.766	10.966	719.310	705.000	2.0



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

GC Column: RTX-CLP2 ID: 0.32 (mm) Initi. Calib. Date(s): 04/23/2025 04/23/2025

Client Sample No.: CCAL03 Date Analyzed: 05/01/2025

Lab Sample No.: HSTDCCC750 Data File : PS030013.D Time Analyzed: 12:12

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
2,4,5-T	9.937	9.847	10.047	784.080	712.500	10.0
2,4,5-TP(Silvex)	9.533	9.442	9.642	796.690	712.500	11.8
2,4-D	8.654	8.561	8.761	757.120	705.000	7.4
2,4-DB	10.495	10.407	10.607	757.220	712.500	6.3
2,4-DCAA	7.462	7.367	7.567	820.590	750.000	9.4
Dalapon	2.523	2.425	2.625	705.560	682.500	3.4
DICAMBA	7.648	7.553	7.753	800.730	705.000	13.6
DICHLORPROP	8.341	8.248	8.448	768.250	705.000	9.0
Dinoseb	10.869	10.781	10.981	755.960	705.000	7.2

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS030013.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 12:12  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**HSTDCCC750**

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 04:57:06 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

4) S 2,4-DCAA 6.939 7.462 1871.5E6 578.1E6 760.455 820.588

**Target Compounds**

1) T	Dalapon	2.450	2.523	2842.4E6	1225.0E6	694.072	705.564
2) T	3,5-DICHL...	6.143	6.459	2534.7E6	733.0E6	709.256	749.766
3) T	4-Nitroph...	6.729	6.996	1248.9E6	553.9E6	700.337	723.117
5) T	DICAMBA	7.116	7.648	7216.6E6	3162.9E6	728.740	800.727
6) T	MCPP	7.294	7.755	476.8E6	127.0E6	73.990	72.588
7) T	MCPA	7.437	7.986	642.0E6	173.5E6	72.694	73.321
8) T	DICHLORPROP	7.796	8.341	1795.0E6	771.3E6	708.332	768.253
9) T	2,4-D	8.015	8.654	2025.4E6	853.4E6	720.064	757.125
10) T	Pentachlo...	8.294	9.155	25966.6E6	16440.0E6	744.350	808.069
11) T	2,4,5-TP ...	8.858	9.533	10286.3E6	6518.3E6	742.007	796.691
12) T	2,4,5-T	9.140	9.937	10478.0E6	6086.5E6	745.600	784.085
13) T	2,4-DB	9.698	10.495	1745.4E6	609.4E6	763.742	757.220
14) T	DINOSEB	10.861	10.869	7317.8E6	4408.0E6	719.308	755.957
15) T	Picloram	10.680	11.905	13288.4E6	8972.7E6	724.926	730.458m
16) T	DCPA	11.162	11.901	12725.4E6	7783.9E6	747.629	690.569m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS030013.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 12:12  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1


Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 04:57:06 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation





Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDCCC750

### Manual Integrations APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

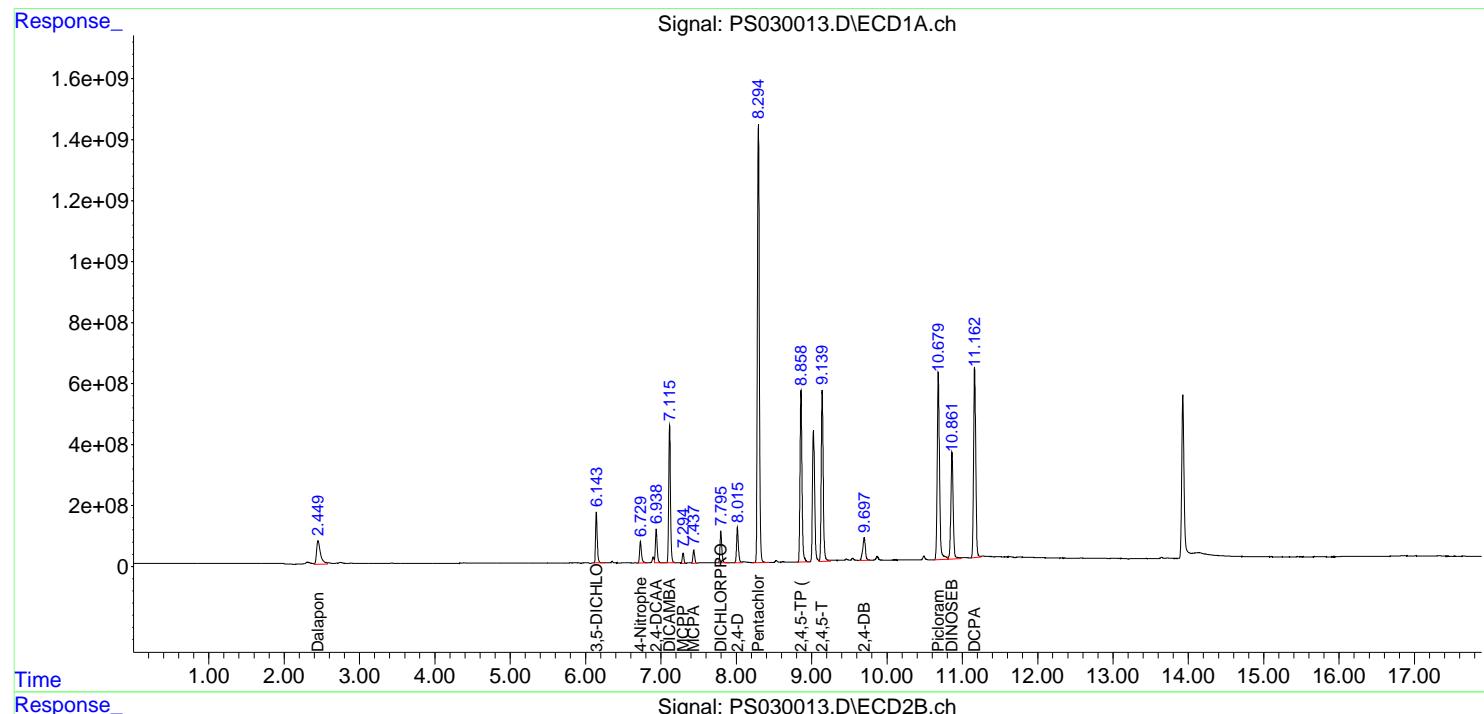

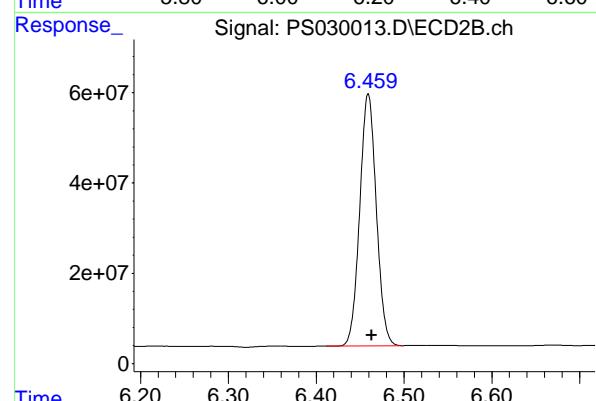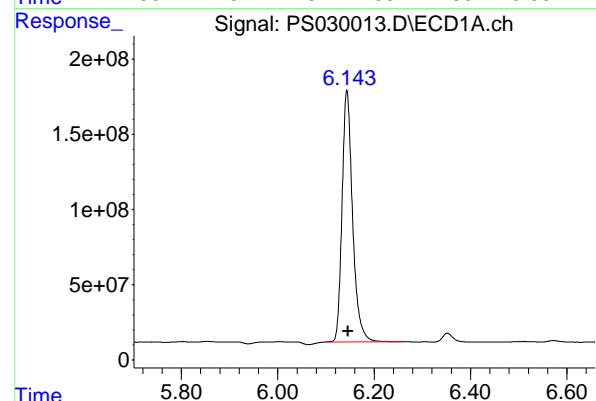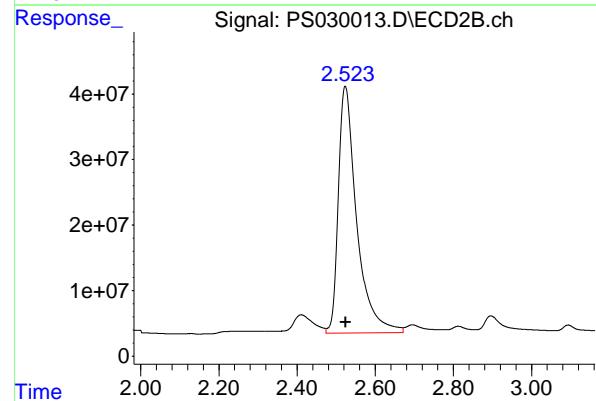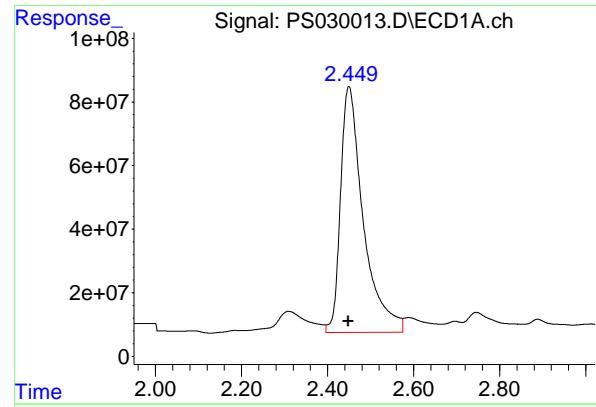

#1 Dalapon

R.T.: 2.450 min  
 Delta R.T.: 0.002 min  
 Response: 2842405390  
 Conc: 694.07 ng/ml

Instrument: ECD\_S  
 Client Sample Id: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

#1 Dalapon





R.T.: 2.523 min  
 Delta R.T.: -0.001 min  
 Response: 1224960796  
 Conc: 705.56 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.143 min  
 Delta R.T.: -0.002 min  
 Response: 2534729517  
 Conc: 709.26 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.459 min  
 Delta R.T.: -0.004 min  
 Response: 732955479  
 Conc: 749.77 ng/ml

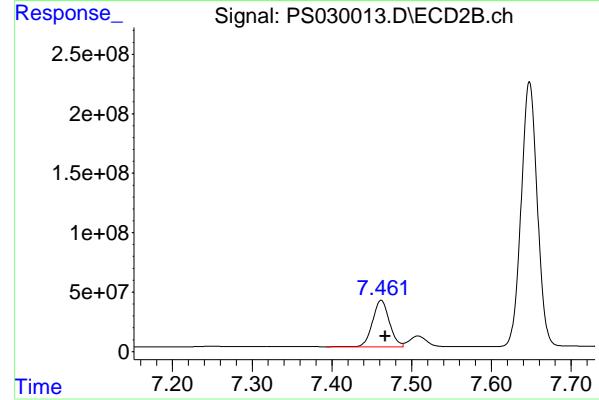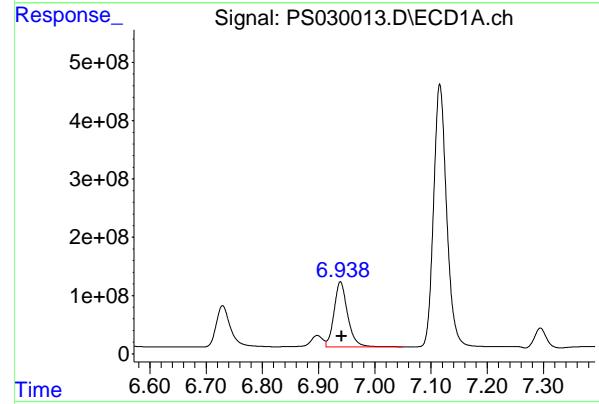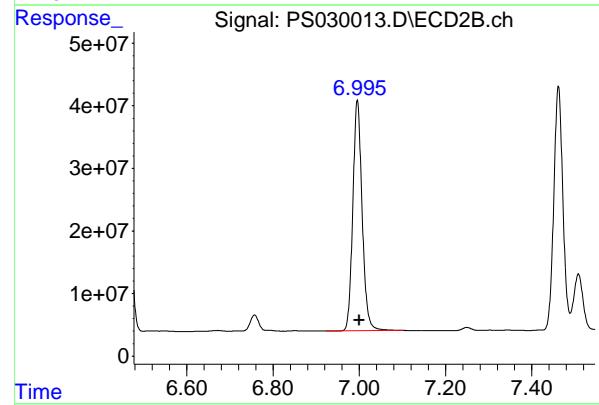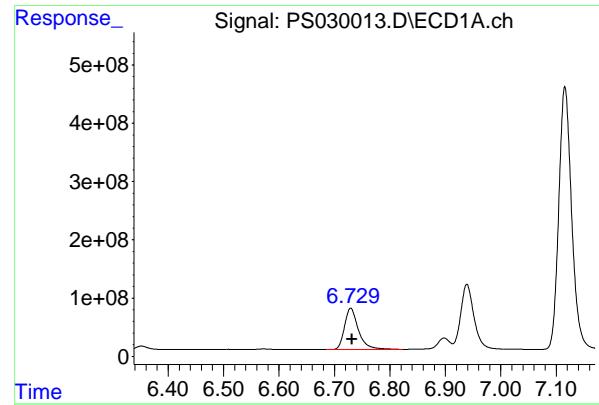

## #3 4-Nitrophenol

R.T.: 6.729 min  
Delta R.T.: -0.002 min  
Instrument: ECD\_S  
Response: 1248924020  
Conc: 700.34 ng/ml  
ClientSampleId: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
Supervised By :mohammad ahmed 05/05/2025

## #3 4-Nitrophenol





R.T.: 6.996 min  
Delta R.T.: -0.005 min  
Response: 553850837  
Conc: 723.12 ng/ml

## #4 2,4-DCAA

R.T.: 6.939 min  
Delta R.T.: -0.003 min  
Response: 1871539269  
Conc: 760.45 ng/ml

## #4 2,4-DCAA

R.T.: 7.462 min  
Delta R.T.: -0.005 min  
Response: 578117969  
Conc: 820.59 ng/ml

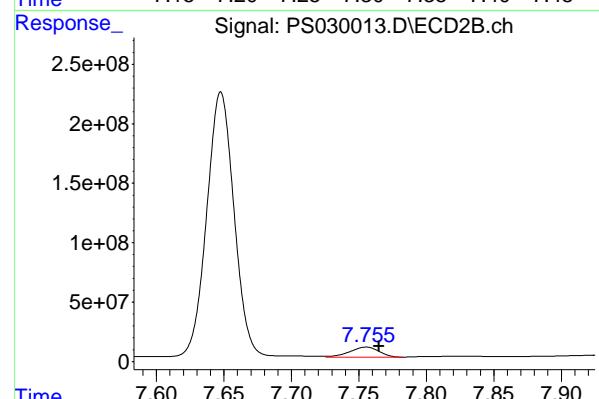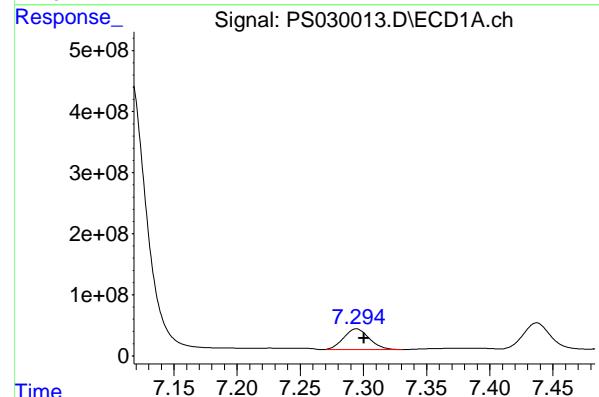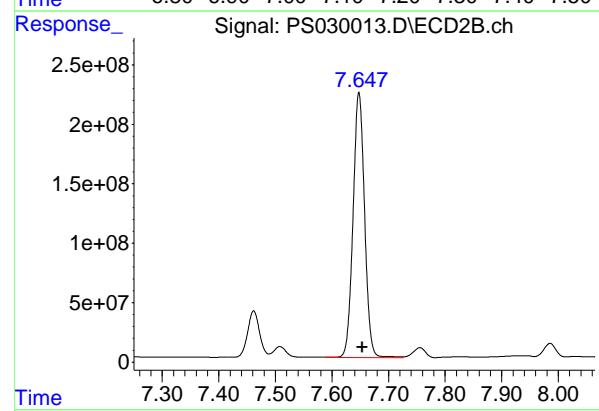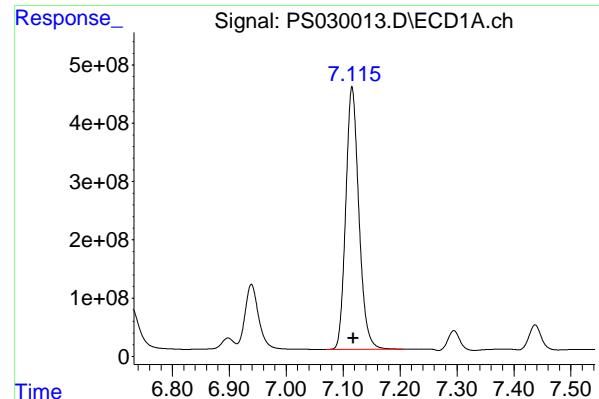

## #5 DICAMBA

R.T.: 7.116 min  
 Delta R.T.: -0.002 min  
 Response: 7216610889  
 Conc: 728.74 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

## #5 DICAMBA





R.T.: 7.648 min  
 Delta R.T.: -0.006 min  
 Response: 3162921794  
 Conc: 800.73 ng/ml

## #6 MCPP

R.T.: 7.294 min  
 Delta R.T.: -0.006 min  
 Response: 476765864  
 Conc: 73.99 ug/ml

## #6 MCPP

R.T.: 7.755 min  
 Delta R.T.: -0.009 min  
 Response: 126951961  
 Conc: 72.59 ug/ml

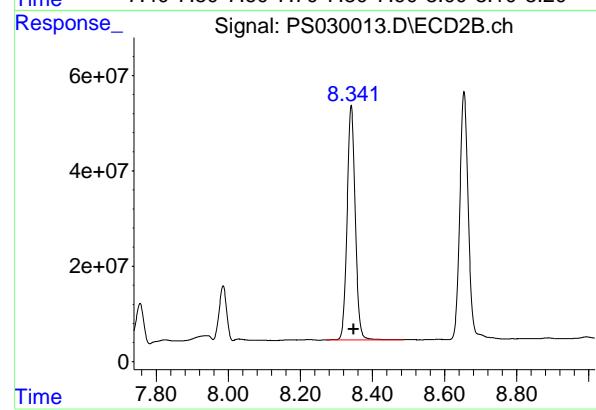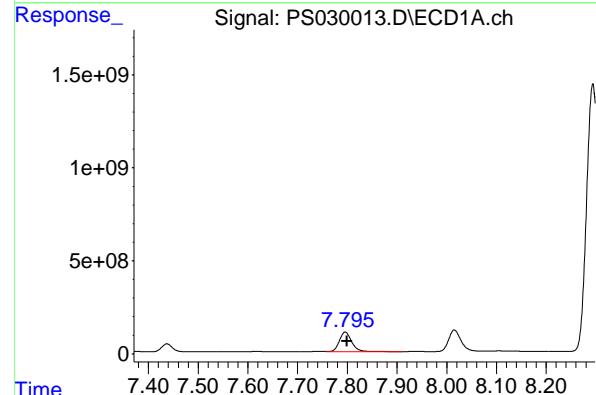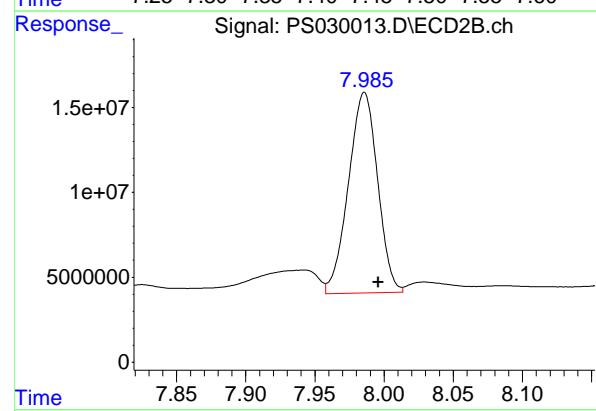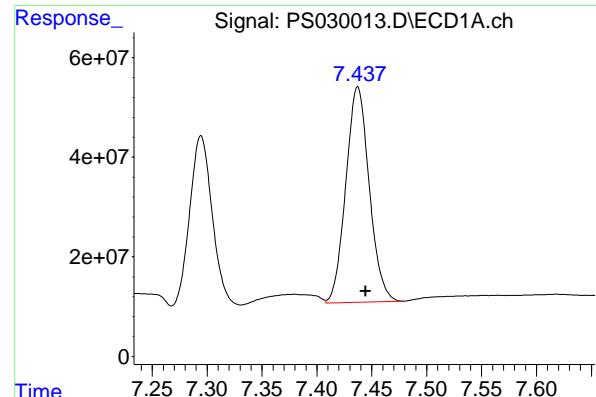

#7 MCPA

R.T.: 7.437 min  
 Delta R.T.: -0.007 min  
 Response: 641986097  
 Conc: 72.69 ug/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

#7 MCPA





R.T.: 7.986 min  
 Delta R.T.: -0.010 min  
 Response: 173462992  
 Conc: 73.32 ug/ml

#8 DICHLORPROP

R.T.: 7.796 min  
 Delta R.T.: -0.003 min  
 Response: 1794988816  
 Conc: 708.33 ng/ml

#8 DICHLORPROP

R.T.: 8.341 min  
 Delta R.T.: -0.007 min  
 Response: 771298752  
 Conc: 768.25 ng/ml

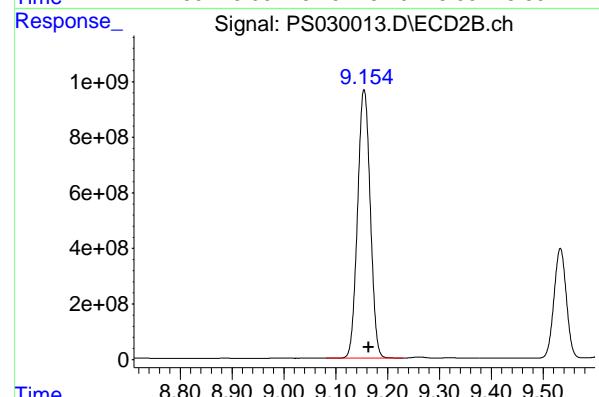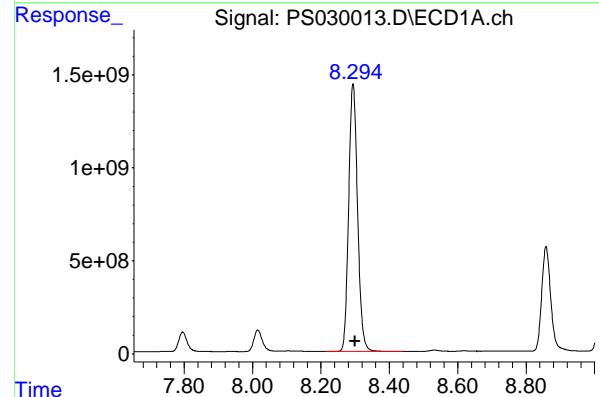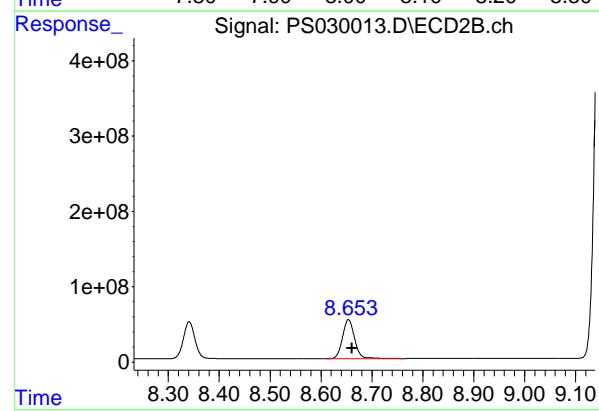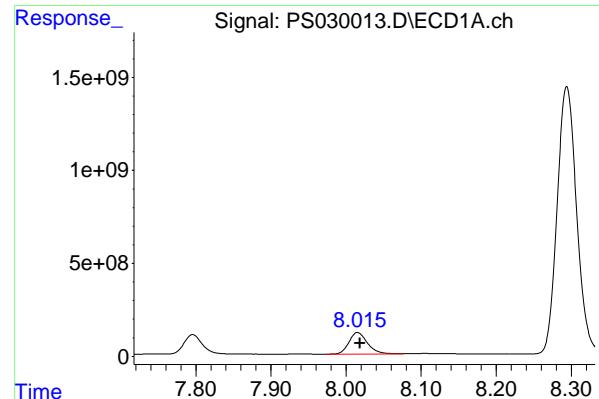

#9 2,4-D

R.T.: 8.015 min  
Delta R.T.: -0.003 min  
Instrument: ECD\_S  
Response: 2025447050  
Conc: 720.06 ng/ml  
ClientSampleId: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
Supervised By :mohammad ahmed 05/05/2025

#9 2,4-D





R.T.: 8.654 min  
Delta R.T.: -0.007 min  
Response: 853360684  
Conc: 757.12 ng/ml

#10 Pentachlorophenol

R.T.: 8.294 min  
Delta R.T.: -0.006 min  
Response: 25966648022  
Conc: 744.35 ng/ml

#10 Pentachlorophenol

R.T.: 9.155 min  
Delta R.T.: -0.009 min  
Response: 16440020170  
Conc: 808.07 ng/ml

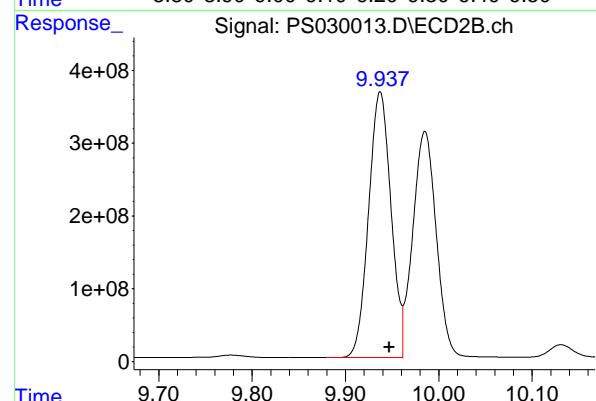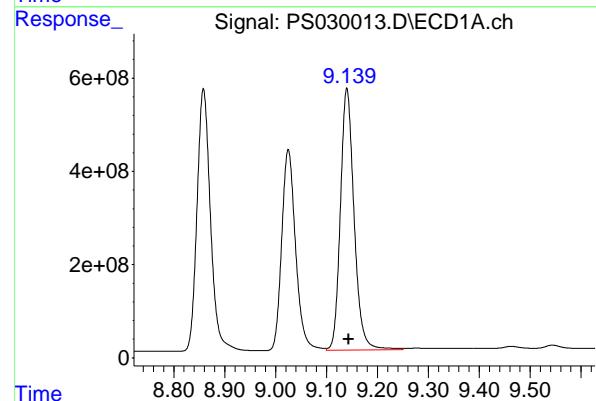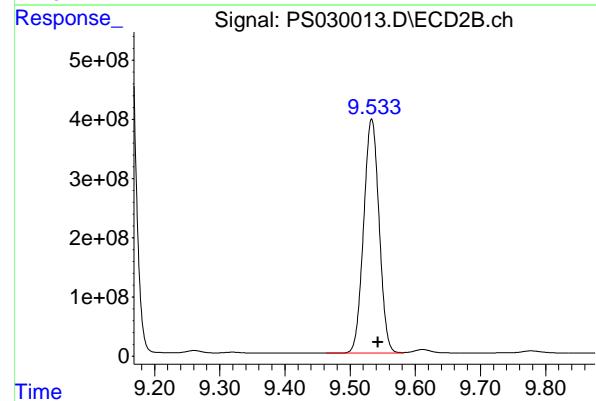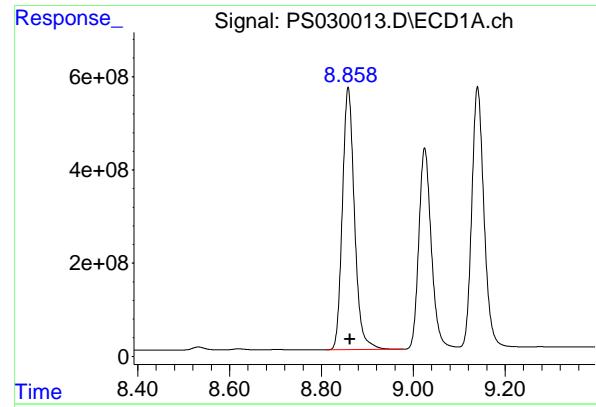

#11 2,4,5-TP (SILVEX)

R.T.: 8.858 min  
 Delta R.T.: -0.004 min  
 Response: 10286319183 ECD\_S  
 Conc: 742.01 ng/ml Client Sample Id : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

#11 2,4,5-TP (SILVEX)


R.T.: 9.533 min  
 Delta R.T.: -0.010 min  
 Response: 6518329316  
 Conc: 796.69 ng/ml

#12 2,4,5-T

R.T.: 9.140 min  
 Delta R.T.: -0.004 min  
 Response: 10478000956  
 Conc: 745.60 ng/ml

#12 2,4,5-T

R.T.: 9.937 min  
 Delta R.T.: -0.010 min  
 Response: 6086536736  
 Conc: 784.08 ng/ml

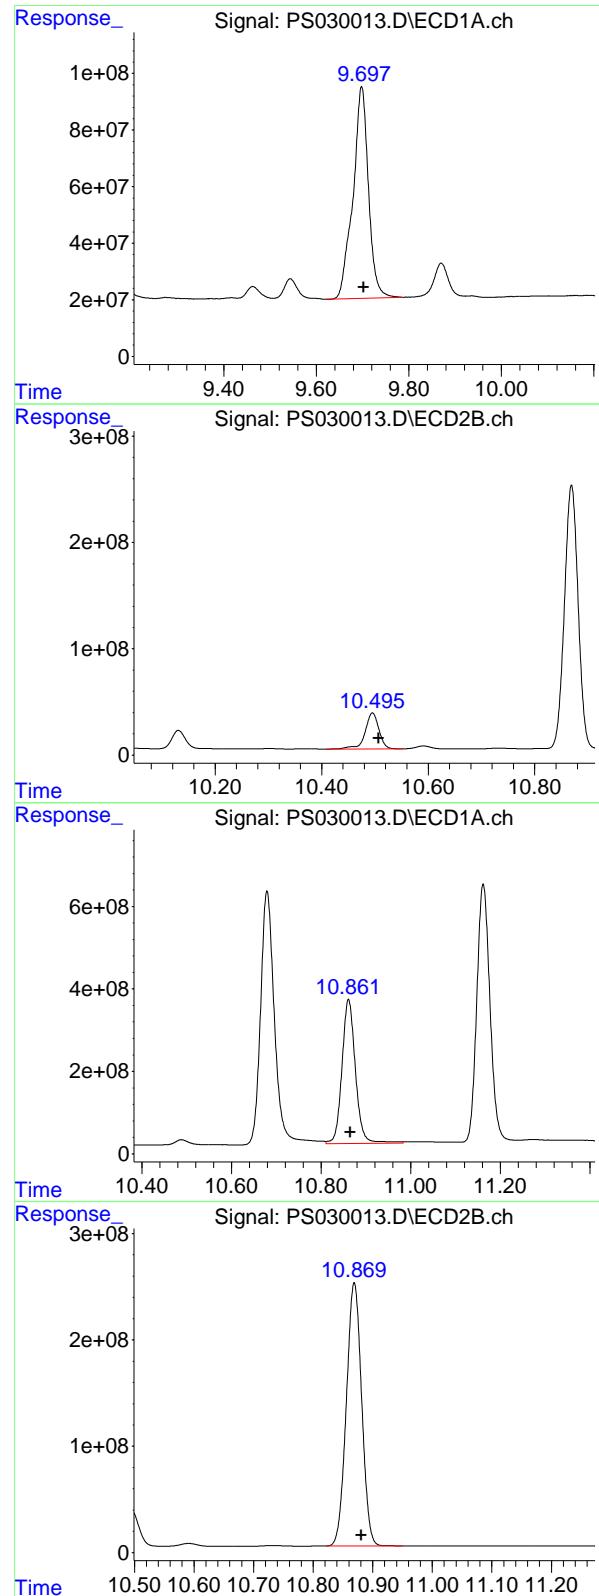

#13 2,4-DB

R.T.: 9.698 min  
 Delta R.T.: -0.004 min  
 Response: 1745423457  
 Conc: 763.74 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

#13 2,4-DB


R.T.: 10.495 min  
 Delta R.T.: -0.011 min  
 Response: 609442670  
 Conc: 757.22 ng/ml

#14 DINOSEB

R.T.: 10.861 min  
 Delta R.T.: -0.005 min  
 Response: 7317825824  
 Conc: 719.31 ng/ml

#14 DINOSEB

R.T.: 10.869 min  
 Delta R.T.: -0.012 min  
 Response: 4407971468  
 Conc: 755.96 ng/ml

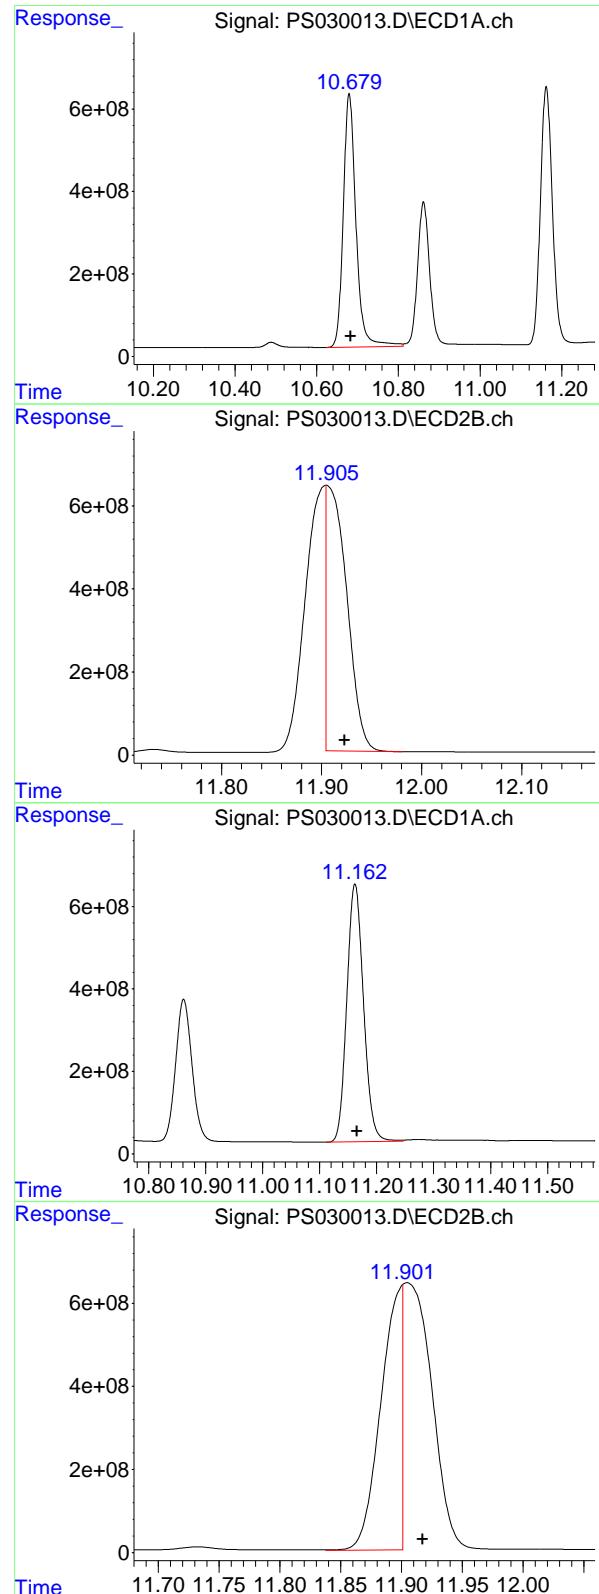

## #15 Picloram

R.T.: 10.680 min  
 Delta R.T.: -0.004 min  
 Response: 13288353705  
 Conc: 724.93 ng/ml  
 Instrument: ECD\_S  
 ClientSampleId : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

## #15 Picloram

R.T.: 11.905 min  
 Delta R.T.: -0.018 min  
 Response: 8972685377  
 Conc: 730.46 ng/ml

## #16 DCPA

R.T.: 11.162 min  
 Delta R.T.: -0.004 min  
 Response: 12725385376  
 Conc: 747.63 ng/ml

## #16 DCPA

R.T.: 11.901 min  
 Delta R.T.: -0.017 min  
 Response: 7783857280  
 Conc: 690.57 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

Continuing Calib Date: 05/01/2025 Initial Calibration Date(s): 04/23/2025 04/23/2025

Continuing Calib Time: 13:27 Initial Calibration Time(s): 11:01 12:37

GC Column: RTX-CLP ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
DICAMBA	7.12	7.12	7.02	7.22	0.01
2,4-DCAA	6.94	6.94	6.84	7.04	0.00
Dalapon	2.45	2.45	2.35	2.55	0.00
DICHLORPROP	7.80	7.80	7.70	7.90	0.00
2,4-D	8.01	8.02	7.92	8.12	0.01
2,4,5-TP(Silvex)	8.86	8.86	8.76	8.96	0.00
2,4,5-T	9.14	9.14	9.04	9.24	0.00
2,4-DB	9.70	9.70	9.60	9.80	0.00
Dinoseb	10.86	10.87	10.77	10.97	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

Continuing Calib Date: 05/01/2025 Initial Calibration Date(s): 04/23/2025 04/23/2025

Continuing Calib Time: 13:27 Initial Calibration Time(s): 11:01 12:37

GC Column: RTX-CLP2 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
DICAMBA	7.65	7.65	7.55	7.75	0.00
2,4-DCAA	7.46	7.47	7.37	7.57	0.01
Dalapon	2.52	2.53	2.43	2.63	0.01
DICHLORPROP	8.34	8.35	8.25	8.45	0.01
2,4-D	8.65	8.66	8.56	8.76	0.01
2,4,5-TP(Silvex)	9.53	9.54	9.44	9.64	0.01
2,4,5-T	9.94	9.95	9.85	10.05	0.01
2,4-DB	10.50	10.51	10.41	10.61	0.02
Dinoseb	10.87	10.88	10.78	10.98	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

GC Column: RTX-CLP ID: 0.32 (mm) Initi. Calib. Date(s): 04/23/2025 04/23/2025

Client Sample No.: CCAL04 Date Analyzed: 05/01/2025

Lab Sample No.: HSTDCCC750 Data File : PS030016.D Time Analyzed: 13:27

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
2,4,5-T	9.139	9.044	9.244	754.230	712.500	5.9
2,4,5-TP(Silvex)	8.858	8.762	8.962	749.690	712.500	5.2
2,4-D	8.014	7.919	8.119	725.960	705.000	3.0
2,4-DB	9.698	9.603	9.803	768.520	712.500	7.9
2,4-DCAA	6.938	6.842	7.042	765.770	750.000	2.1
Dalapon	2.449	2.349	2.549	683.250	682.500	0.1
DICAMBA	7.115	7.018	7.218	731.570	705.000	3.8
DICHLORPROP	7.795	7.699	7.899	714.120	705.000	1.3
Dinoseb	10.860	10.766	10.966	724.710	705.000	2.8



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

GC Column: RTX-CLP2 ID: 0.32 (mm) Initi. Calib. Date(s): 04/23/2025 04/23/2025

Client Sample No.: CCAL04 Date Analyzed: 05/01/2025

Lab Sample No.: HSTDCCC750 Data File : PS030016.D Time Analyzed: 13:27

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
2,4,5-T	9.937	9.847	10.047	784.510	712.500	10.1
2,4,5-TP(Silvex)	9.533	9.442	9.642	796.150	712.500	11.7
2,4-D	8.654	8.561	8.761	757.870	705.000	7.5
2,4-DB	10.495	10.407	10.607	769.370	712.500	8.0
2,4-DCAA	7.462	7.367	7.567	816.790	750.000	8.9
Dalapon	2.523	2.425	2.625	696.660	682.500	2.1
DICAMBA	7.648	7.553	7.753	796.150	705.000	12.9
DICHLORPROP	8.341	8.248	8.448	771.490	705.000	9.4
Dinoseb	10.869	10.781	10.981	758.940	705.000	7.7

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030016.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 13:27  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDCCC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:28:08 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

4) S 2,4-DCAA 6.938 7.462 1884.6E6 575.4E6 765.767 816.786

**Target Compounds**

1) T	Dalapon	2.449	2.523	2798.1E6	1209.5E6	683.247	696.662
2) T	3,5-DICHL...	6.143	6.459	2544.7E6	733.9E6	712.034	750.706
3) T	4-Nitroph...	6.728	6.996	1257.5E6	552.2E6	705.169	720.931
5) T	DICAMBA	7.115	7.648	7244.6E6	3144.8E6	731.569	796.146
6) T	MCPP	7.294	7.755	469.8E6	129.0E6	72.914	73.740
7) T	MCPA	7.436	7.986	645.8E6	171.6E6	73.130	72.542
8) T	DICHLORPROP	7.795	8.341	1809.7E6	774.5E6	714.123	771.491
9) T	2,4-D	8.014	8.654	2042.0E6	854.2E6	725.956	757.867
10) T	Pentachlo...	8.293	9.155	26148.2E6	16409.8E6	749.553	806.585
11) T	2,4,5-TP ...	8.858	9.533	10392.9E6	6513.9E6	749.693	796.152
12) T	2,4,5-T	9.139	9.937	10599.2E6	6089.9E6	754.227	784.513
13) T	2,4-DB	9.698	10.495	1756.3E6	619.2E6	768.523	769.370
14) T	DINOSEB	10.860	10.869	7372.8E6	4425.3E6	724.708	758.937
15) T	Picloram	10.679	11.905	13694.5E6	8880.4E6	747.085	722.943m
16) T	DCPA	11.161	11.900	12916.6E6	7671.9E6	758.863	680.636m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030016.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 13:27  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1



Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:28:08 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation





Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDCCC750

### Manual Integrations APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

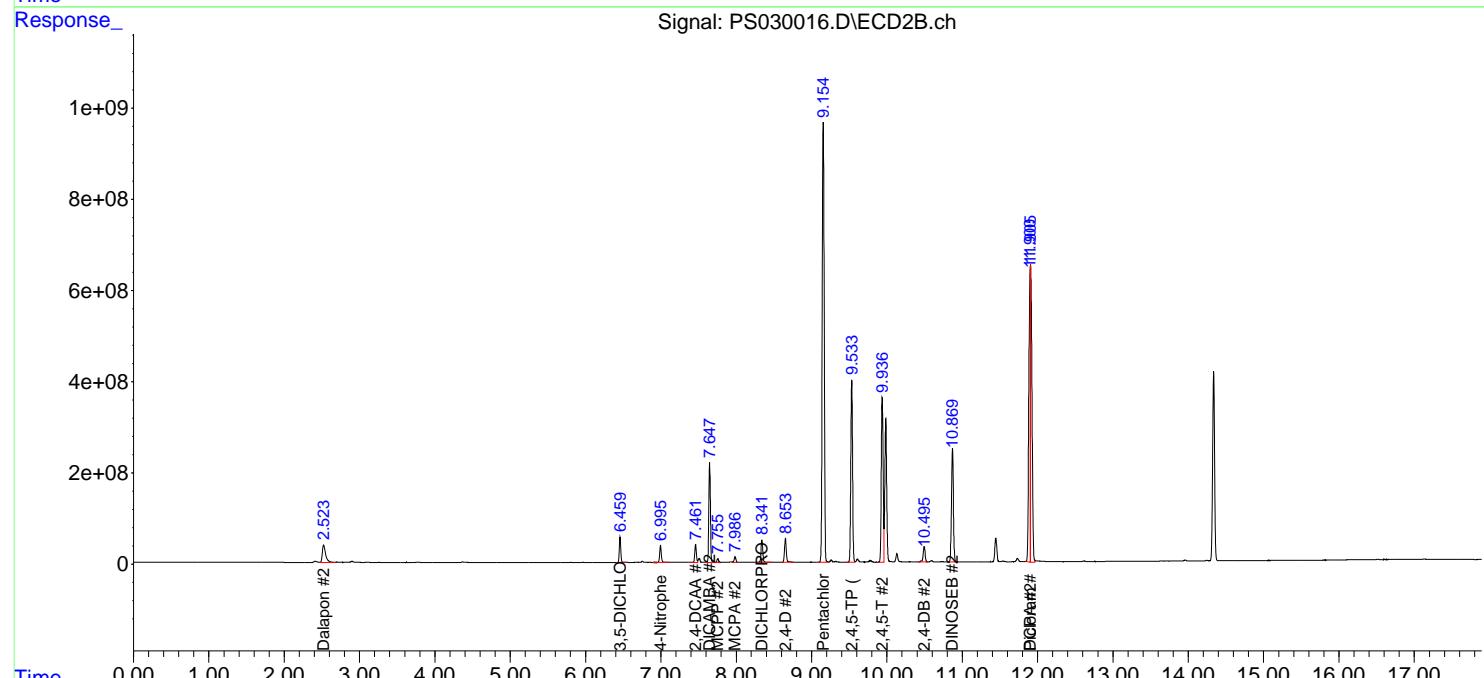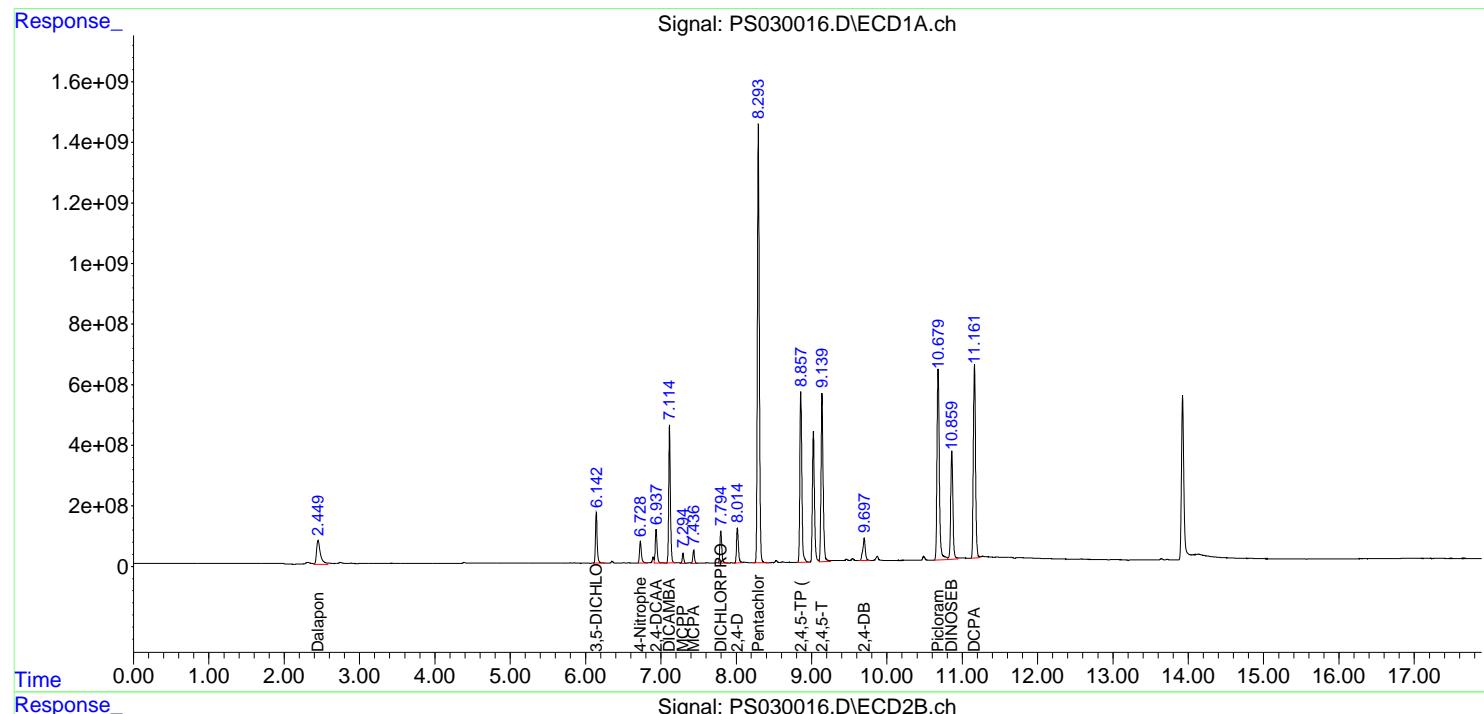

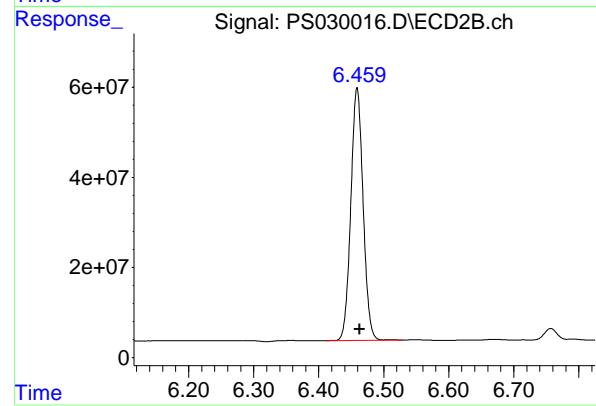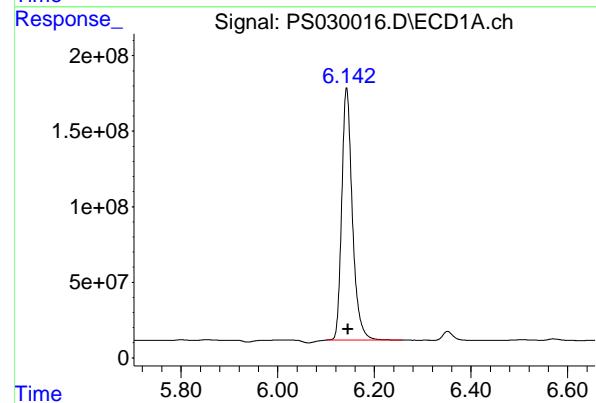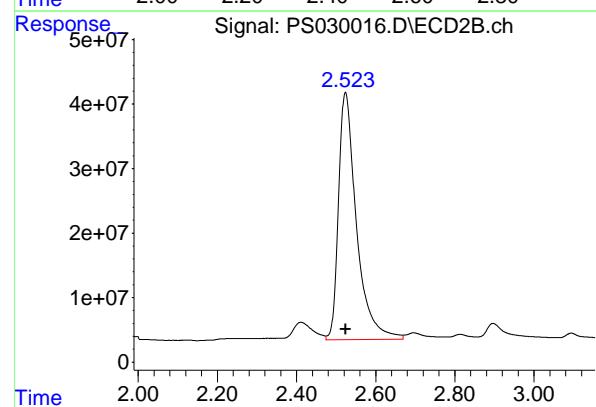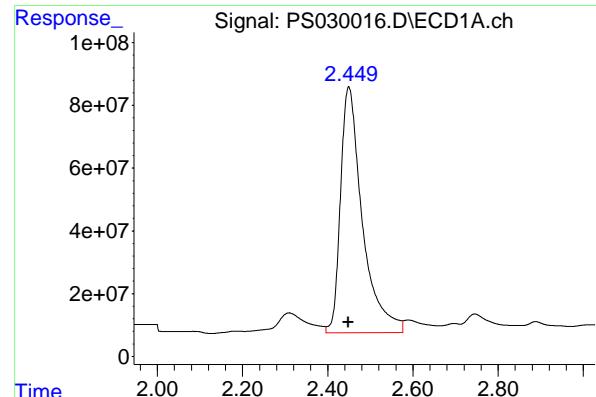

#1 Dalapon

R.T.: 2.449 min  
 Delta R.T.: 0.001 min  
 Response: 2798074434 ECD\_S  
 Conc: 683.25 ng/ml Client SampleId : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

#1 Dalapon





R.T.: 2.523 min  
 Delta R.T.: 0.000 min  
 Response: 1209506191  
 Conc: 696.66 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.143 min  
 Delta R.T.: -0.003 min  
 Response: 2544656484  
 Conc: 712.03 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.459 min  
 Delta R.T.: -0.004 min  
 Response: 733875039  
 Conc: 750.71 ng/ml

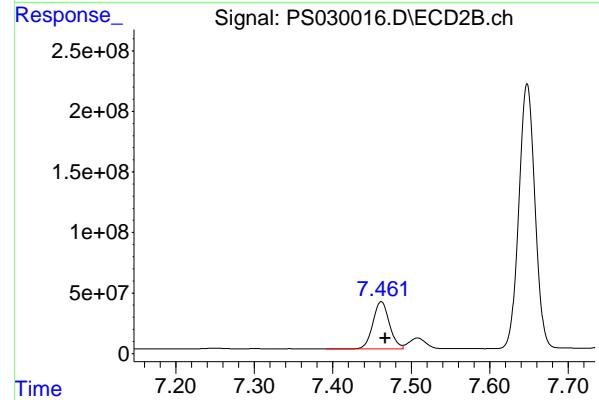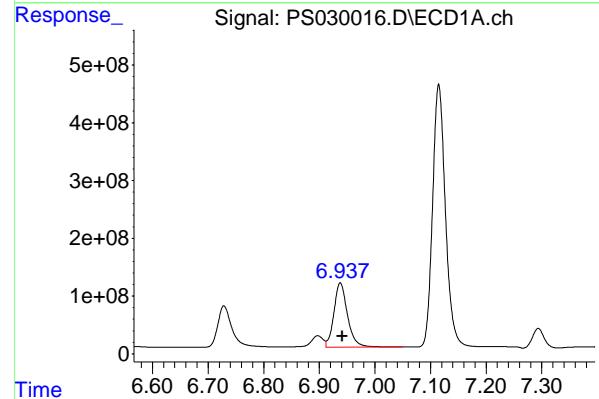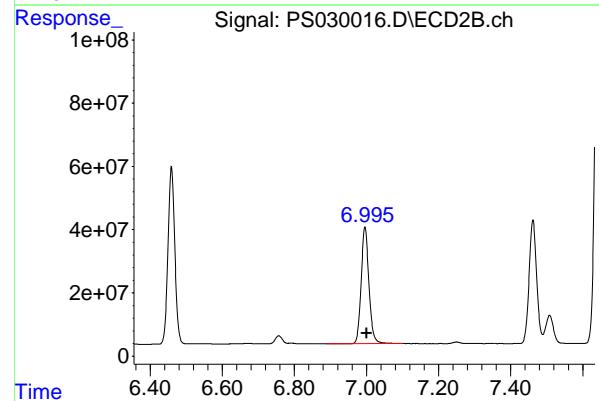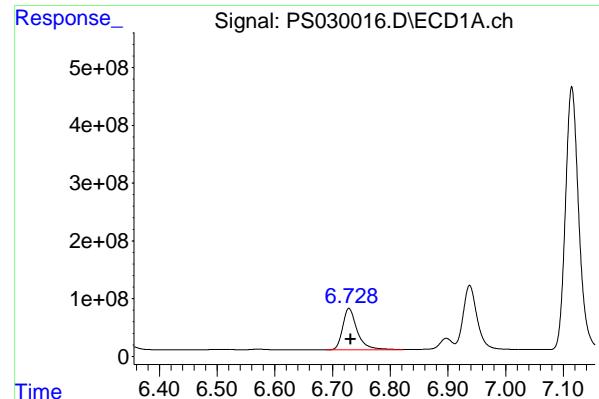

## #3 4-Nitrophenol

R.T.: 6.728 min  
Delta R.T.: -0.003 min  
Instrument: ECD\_S  
Response: 1257541620  
Conc: 705.17 ng/ml  
ClientSampleId: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
Supervised By :mohammad ahmed 05/05/2025

## #3 4-Nitrophenol


R.T.: 6.996 min  
Delta R.T.: -0.005 min  
Response: 552176387  
Conc: 720.93 ng/ml

## #4 2,4-DCAA

R.T.: 6.938 min  
Delta R.T.: -0.004 min  
Response: 1884613932  
Conc: 765.77 ng/ml

## #4 2,4-DCAA

R.T.: 7.462 min  
Delta R.T.: -0.005 min  
Response: 575439313  
Conc: 816.79 ng/ml

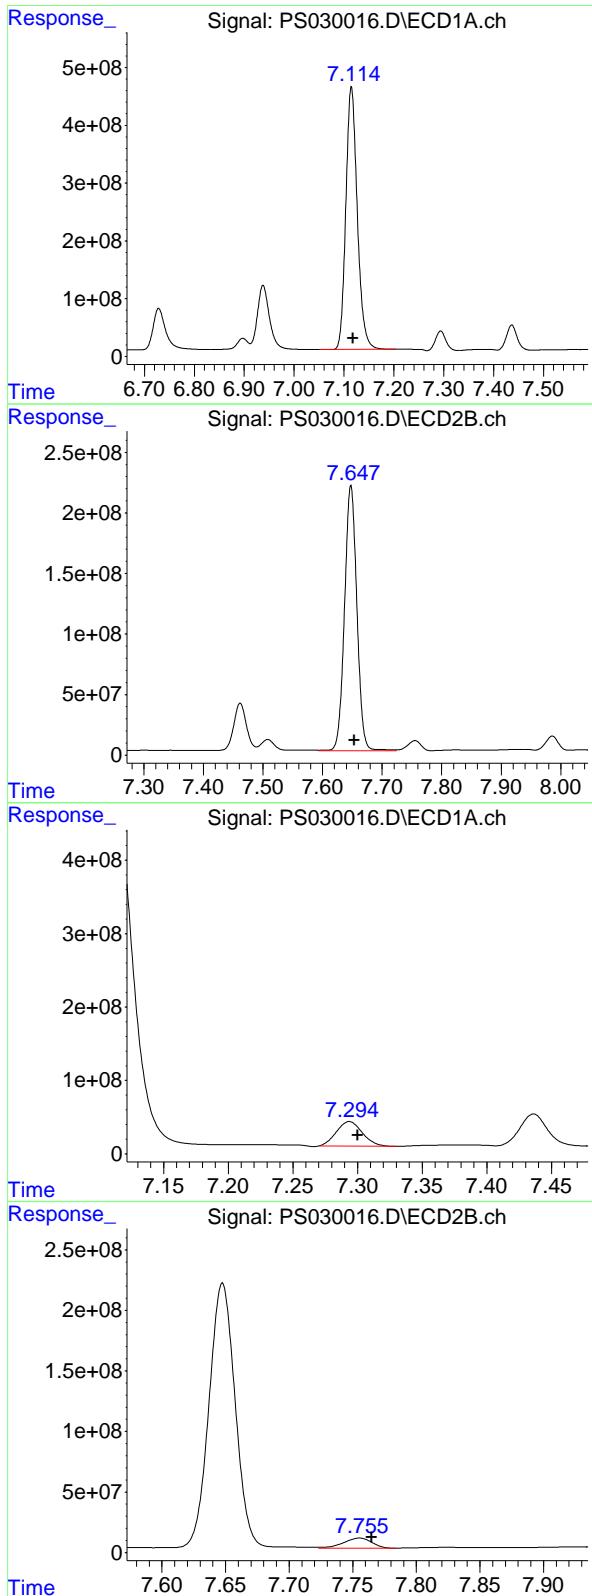

## #5 DICAMBA

R.T.: 7.115 min  
 Delta R.T.: -0.003 min  
 Response: 7244628718 ECD\_S  
 Conc: 731.57 ng/ml Client SampleId : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

## #5 DICAMBA





R.T.: 7.648 min  
 Delta R.T.: -0.006 min  
 Response: 3144828216  
 Conc: 796.15 ng/ml

## #6 MCPP

R.T.: 7.294 min  
 Delta R.T.: -0.006 min  
 Response: 469831489  
 Conc: 72.91 ug/ml

## #6 MCPP

R.T.: 7.755 min  
 Delta R.T.: -0.010 min  
 Response: 128968282  
 Conc: 73.74 ug/ml

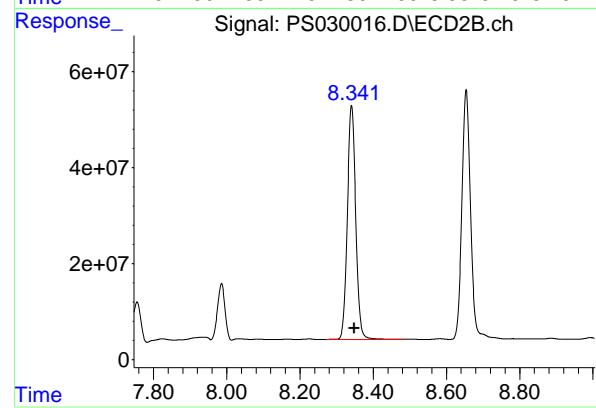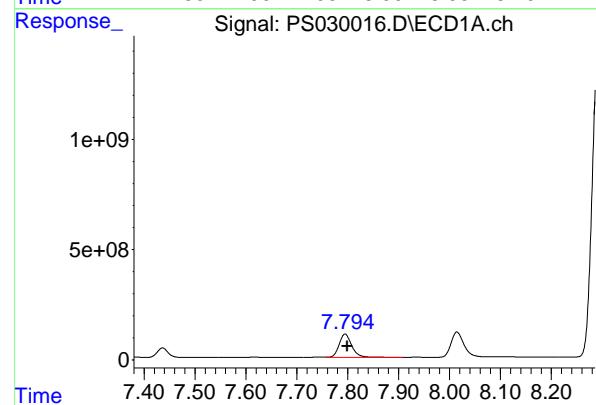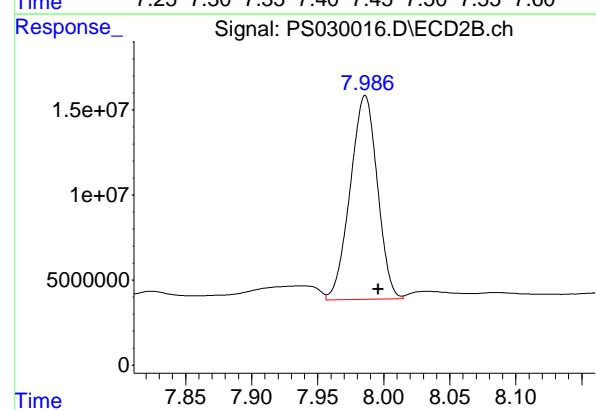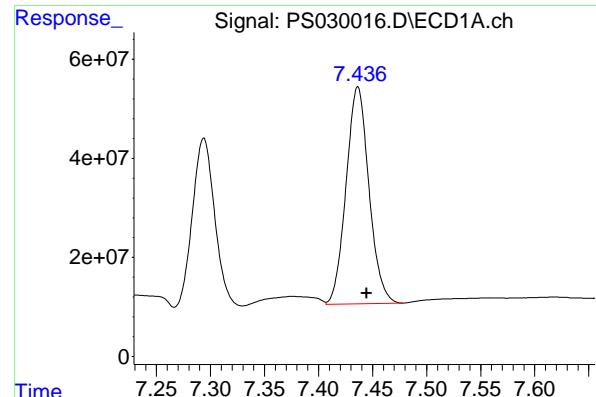

#7 MCPA

R.T.: 7.436 min  
 Delta R.T.: -0.008 min  
 Response: 645840618  
 Conc: 73.13 ug/ml

Instrument: ECD\_S  
 ClientSampleId : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

#7 MCPA





R.T.: 7.986 min  
 Delta R.T.: -0.010 min  
 Response: 171619066  
 Conc: 72.54 ug/ml

#8 DICHLORPROP

R.T.: 7.795 min  
 Delta R.T.: -0.004 min  
 Response: 1809664833  
 Conc: 714.12 ng/ml

#8 DICHLORPROP

R.T.: 8.341 min  
 Delta R.T.: -0.007 min  
 Response: 774549366  
 Conc: 771.49 ng/ml

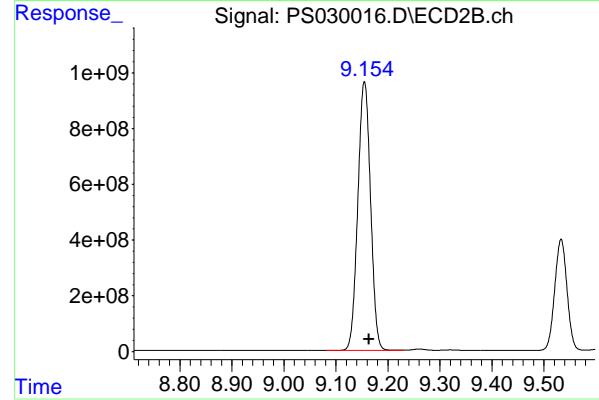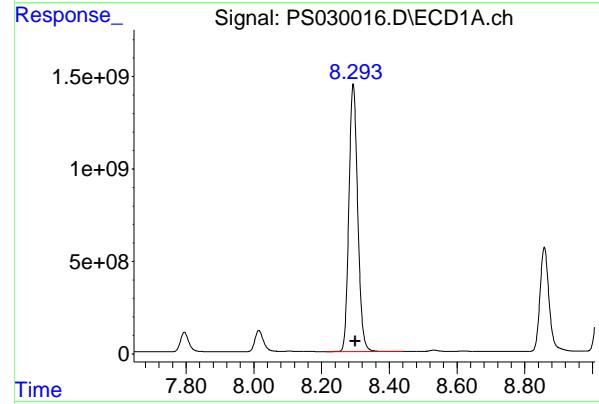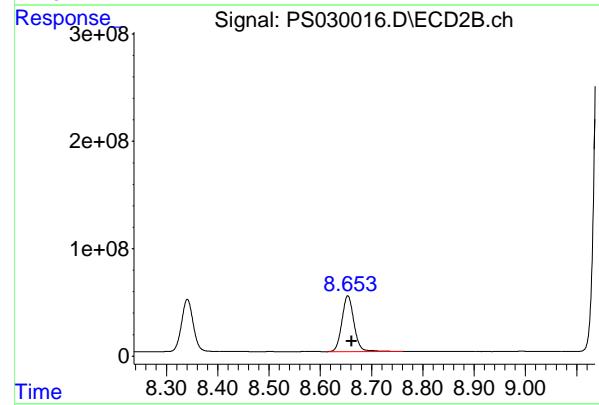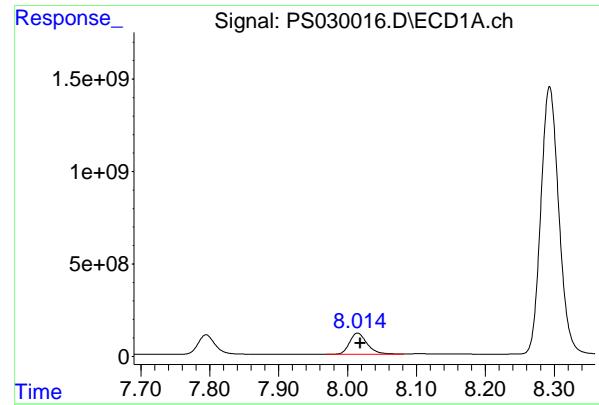

#9 2,4-D

R.T.: 8.014 min  
Delta R.T.: -0.004 min  
Instrument: ECD\_S  
Response: 2042021191  
Conc: 725.96 ng/ml  
ClientSampleId: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
Supervised By :mohammad ahmed 05/05/2025

#9 2,4-D





R.T.: 8.654 min  
Delta R.T.: -0.007 min  
Response: 854197073  
Conc: 757.87 ng/ml

#10 Pentachlorophenol

R.T.: 8.293 min  
Delta R.T.: -0.006 min  
Response: 26148171863  
Conc: 749.55 ng/ml

#10 Pentachlorophenol

R.T.: 9.155 min  
Delta R.T.: -0.009 min  
Response: 16409812223  
Conc: 806.58 ng/ml

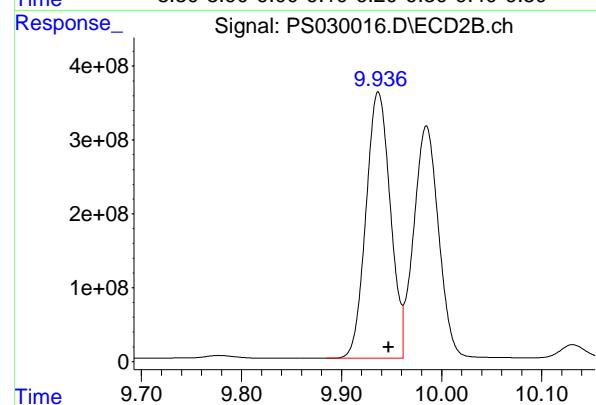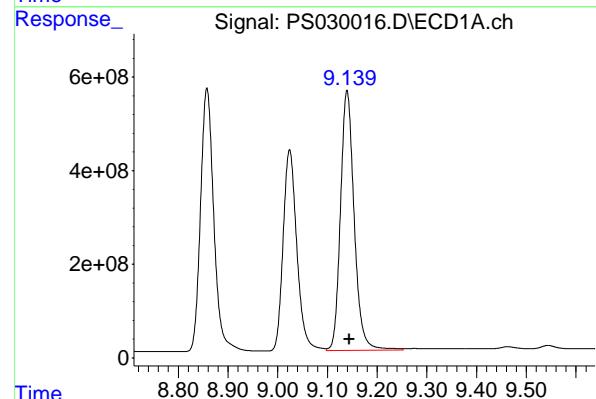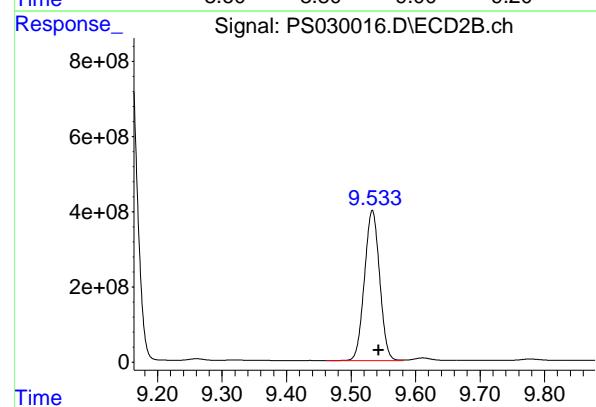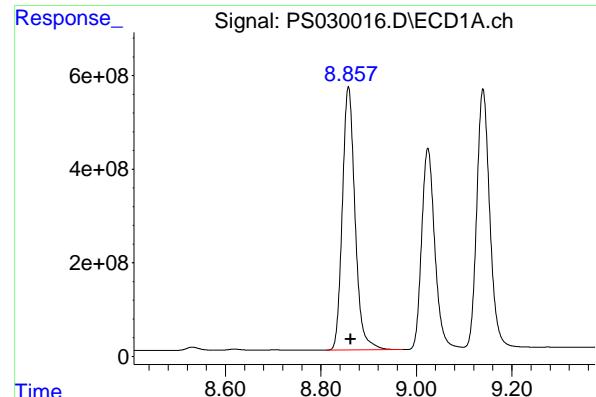

#11 2,4,5-TP (SILVEX)

R.T.: 8.858 min  
Delta R.T.: -0.004 min  
Instrument: ECD\_S  
Response: 10392876642  
Conc: 749.69 ng/ml  
ClientSampleId: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
Supervised By :mohammad ahmed 05/05/2025

#11 2,4,5-TP (SILVEX)


R.T.: 9.533 min  
Delta R.T.: -0.010 min  
Response: 6513919285  
Conc: 796.15 ng/ml

#12 2,4,5-T

R.T.: 9.139 min  
Delta R.T.: -0.005 min  
Response: 10599227676  
Conc: 754.23 ng/ml

#12 2,4,5-T

R.T.: 9.937 min  
Delta R.T.: -0.010 min  
Response: 6089857207  
Conc: 784.51 ng/ml

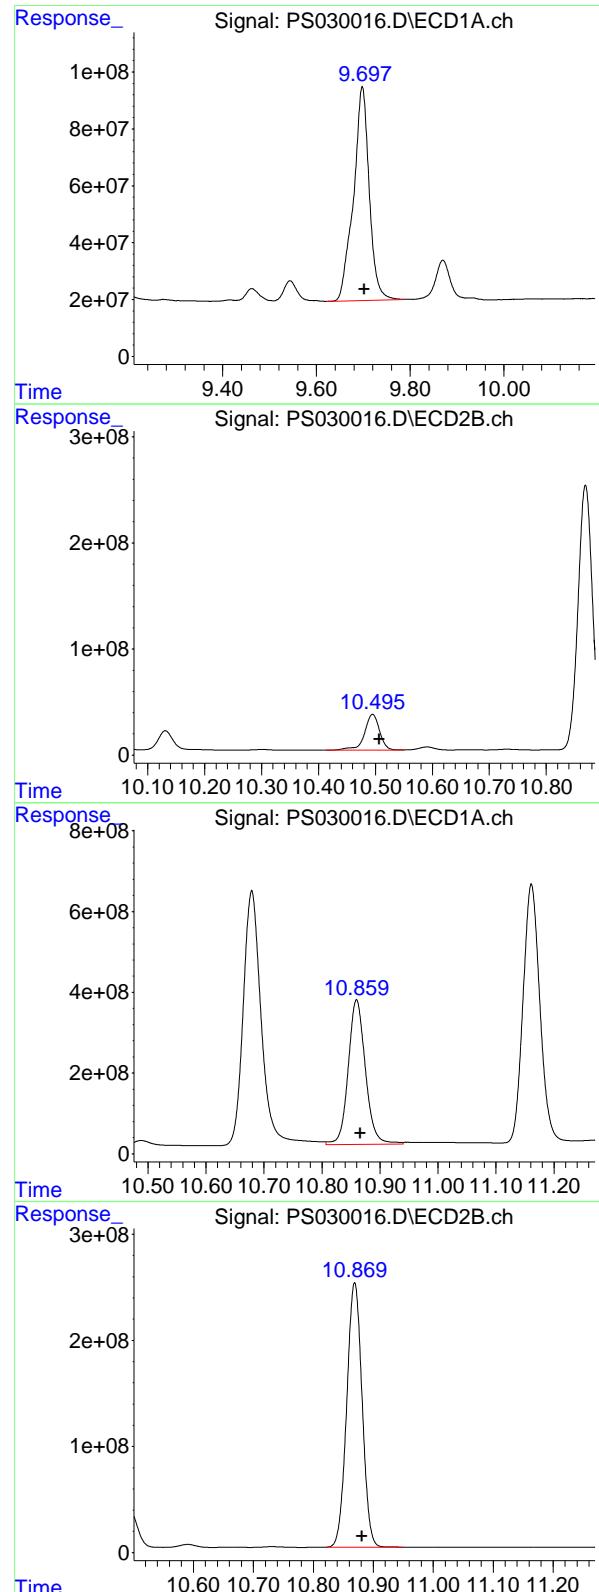

#13 2,4-DB

R.T.: 9.698 min  
 Delta R.T.: -0.004 min  
 Response: 1756348858 ECD\_S  
 Conc: 768.52 ng/ml ClientSampleId : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

#13 2,4-DB


R.T.: 10.495 min  
 Delta R.T.: -0.011 min  
 Response: 619221462  
 Conc: 769.37 ng/ml

#14 DINOSEB

R.T.: 10.860 min  
 Delta R.T.: -0.006 min  
 Response: 7372763225  
 Conc: 724.71 ng/ml

#14 DINOSEB

R.T.: 10.869 min  
 Delta R.T.: -0.012 min  
 Response: 4425346841  
 Conc: 758.94 ng/ml

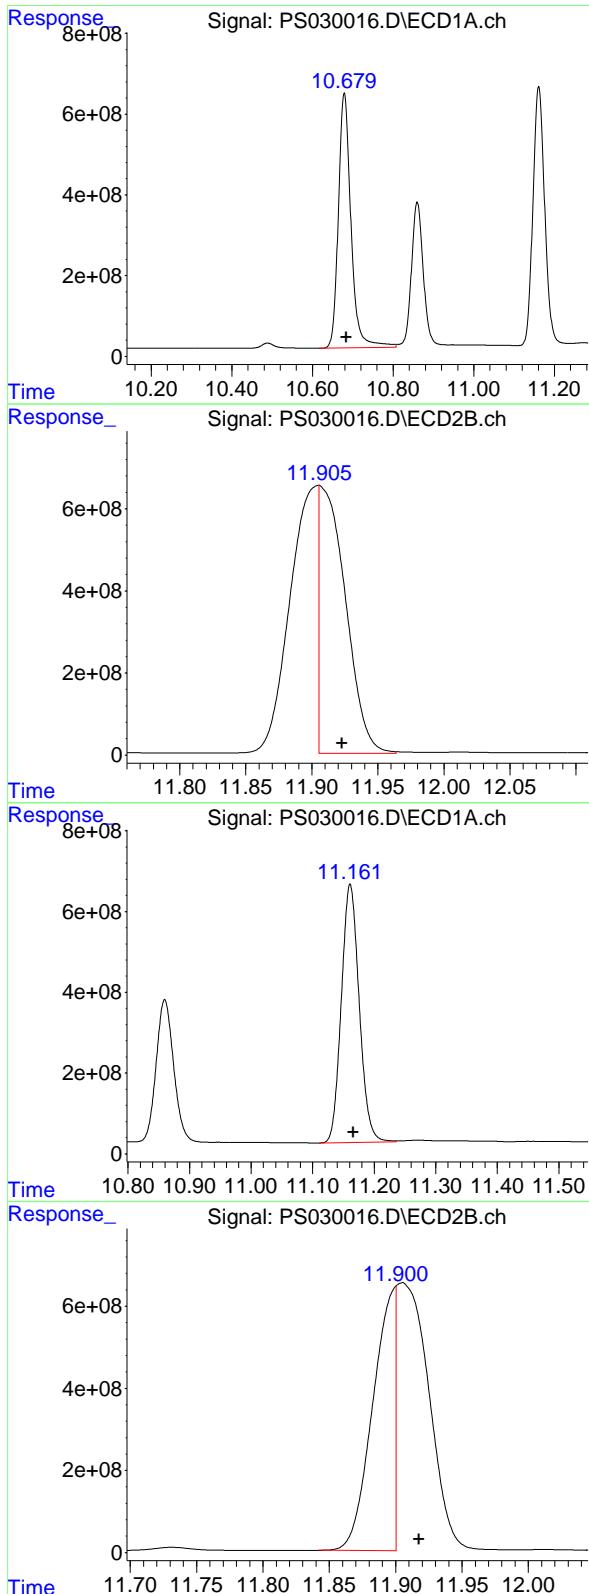

## #15 Picloram

R.T.: 10.679 min  
 Delta R.T.: -0.005 min  
 Response: 13694525497  
 Conc: 747.08 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

## #15 Picloram

R.T.: 11.905 min  
 Delta R.T.: -0.018 min  
 Response: 8880378028  
 Conc: 722.94 ng/ml

## #16 DCPA

R.T.: 11.161 min  
 Delta R.T.: -0.005 min  
 Response: 12916607287  
 Conc: 758.86 ng/ml

## #16 DCPA

R.T.: 11.900 min  
 Delta R.T.: -0.018 min  
 Response: 7671890624  
 Conc: 680.64 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

Continuing Calib Date: 05/01/2025 Initial Calibration Date(s): 04/23/2025 04/23/2025

Continuing Calib Time: 17:28 Initial Calibration Time(s): 11:01 12:37

GC Column: RTX-CLP ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW		DIFF RT
			FROM	TO	
DICAMBA	7.11	7.12	7.02	7.22	0.01
2,4-DCAA	6.94	6.94	6.84	7.04	0.00
Dalapon	2.45	2.45	2.35	2.55	0.00
DICHLORPROP	7.80	7.80	7.70	7.90	0.00
2,4-D	8.02	8.02	7.92	8.12	0.00
2,4,5-TP(Silvex)	8.86	8.86	8.76	8.96	0.00
2,4,5-T	9.14	9.14	9.04	9.24	0.00
2,4-DB	9.70	9.70	9.60	9.80	0.00
Dinoseb	10.86	10.87	10.77	10.97	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

Continuing Calib Date: 05/01/2025 Initial Calibration Date(s): 04/23/2025 04/23/2025

Continuing Calib Time: 17:28 Initial Calibration Time(s): 11:01 12:37

GC Column: RTX-CLP2 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
DICAMBA	7.65	7.65	7.55	7.75	0.00
2,4-DCAA	7.46	7.47	7.37	7.57	0.01
Dalapon	2.52	2.53	2.43	2.63	0.01
DICHLORPROP	8.34	8.35	8.25	8.45	0.01
2,4-D	8.65	8.66	8.56	8.76	0.01
2,4,5-TP(Silvex)	9.53	9.54	9.44	9.64	0.01
2,4,5-T	9.94	9.95	9.85	10.05	0.01
2,4-DB	10.50	10.51	10.41	10.61	0.02
Dinoseb	10.87	10.88	10.78	10.98	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

GC Column: RTX-CLP ID: 0.32 (mm) Initi. Calib. Date(s): 04/23/2025 04/23/2025

Client Sample No.: CCAL05 Date Analyzed: 05/01/2025

Lab Sample No.: HSTDCCC750 Data File : PS030026.D Time Analyzed: 17:28

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
2,4,5-T	9.139	9.044	9.244	757.220	712.500	6.3
2,4,5-TP(Silvex)	8.857	8.762	8.962	751.430	712.500	5.5
2,4-D	8.015	7.919	8.119	727.280	705.000	3.2
2,4-DB	9.698	9.603	9.803	769.080	712.500	7.9
2,4-DCAA	6.938	6.842	7.042	767.300	750.000	2.3
Dalapon	2.448	2.349	2.549	682.430	682.500	0.0
DICAMBA	7.114	7.018	7.218	731.810	705.000	3.8
DICHLORPROP	7.795	7.699	7.899	717.350	705.000	1.8
Dinoseb	10.860	10.766	10.966	739.100	705.000	4.8



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

GC Column: RTX-CLP2 ID: 0.32 (mm) Initi. Calib. Date(s): 04/23/2025 04/23/2025

Client Sample No.: CCAL05 Date Analyzed: 05/01/2025

Lab Sample No.: HSTDCCC750 Data File : PS030026.D Time Analyzed: 17:28

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
2,4,5-T	9.937	9.847	10.047	790.510	712.500	10.9
2,4,5-TP(Silvex)	9.533	9.442	9.642	801.340	712.500	12.5
2,4-D	8.653	8.561	8.761	765.270	705.000	8.5
2,4-DB	10.495	10.407	10.607	767.700	712.500	7.7
2,4-DCAA	7.462	7.367	7.567	808.570	750.000	7.8
Dalapon	2.523	2.425	2.625	682.630	682.500	0.0
DICAMBA	7.648	7.553	7.753	797.610	705.000	13.1
DICHLORPROP	8.341	8.248	8.448	798.240	705.000	13.2
Dinoseb	10.869	10.781	10.981	761.200	705.000	8.0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030026.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 17:28  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDCCC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:30:46 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

4) S 2,4-DCAA 6.938 7.462 1888.4E6 569.7E6 767.297 808.568

**Target Compounds**

1) T	Dalapon	2.448	2.523	2794.7E6	1185.1E6	682.429	682.626
2) T	3,5-DICHL...	6.142	6.459	2569.7E6	738.2E6	719.036	755.171
3) T	4-Nitroph...	6.728	6.995	1269.3E6	560.2E6	711.772	731.395
5) T	DICAMBA	7.114	7.648	7247.0E6	3150.6E6	731.806	797.615
6) T	MCPP	7.293	7.755	448.3E6	125.9E6	69.578	72.009
7) T	MCPA	7.436	7.985	641.0E6	170.3E6	72.586	71.966
8) T	DICHLORPROP	7.795	8.341	1817.9E6	801.4E6	717.354	798.239
9) T	2,4-D	8.015	8.653	2045.8E6	862.5E6	727.283	765.272
10) T	Pentachlo...	8.293	9.154	26237.5E6	16512.9E6	752.115	811.653
11) T	2,4,5-TP ...	8.857	9.533	10417.0E6	6556.3E6	751.434	801.336
12) T	2,4,5-T	9.139	9.937	10641.3E6	6136.4E6	757.218	790.511
13) T	2,4-DB	9.698	10.495	1757.6E6	617.9E6	769.084	767.700
14) T	DINOSEB	10.860	10.869	7519.2E6	4438.6E6	739.099	761.205
15) T	Picloram	10.678	11.905	13425.7E6	8937.7E6	732.418	727.610m
16) T	DCPA	11.161	11.901	12986.2E6	8028.3E6	762.952	712.257m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030026.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 17:28  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1



Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:30:46 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation





Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDCCC750

### Manual Integrations APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

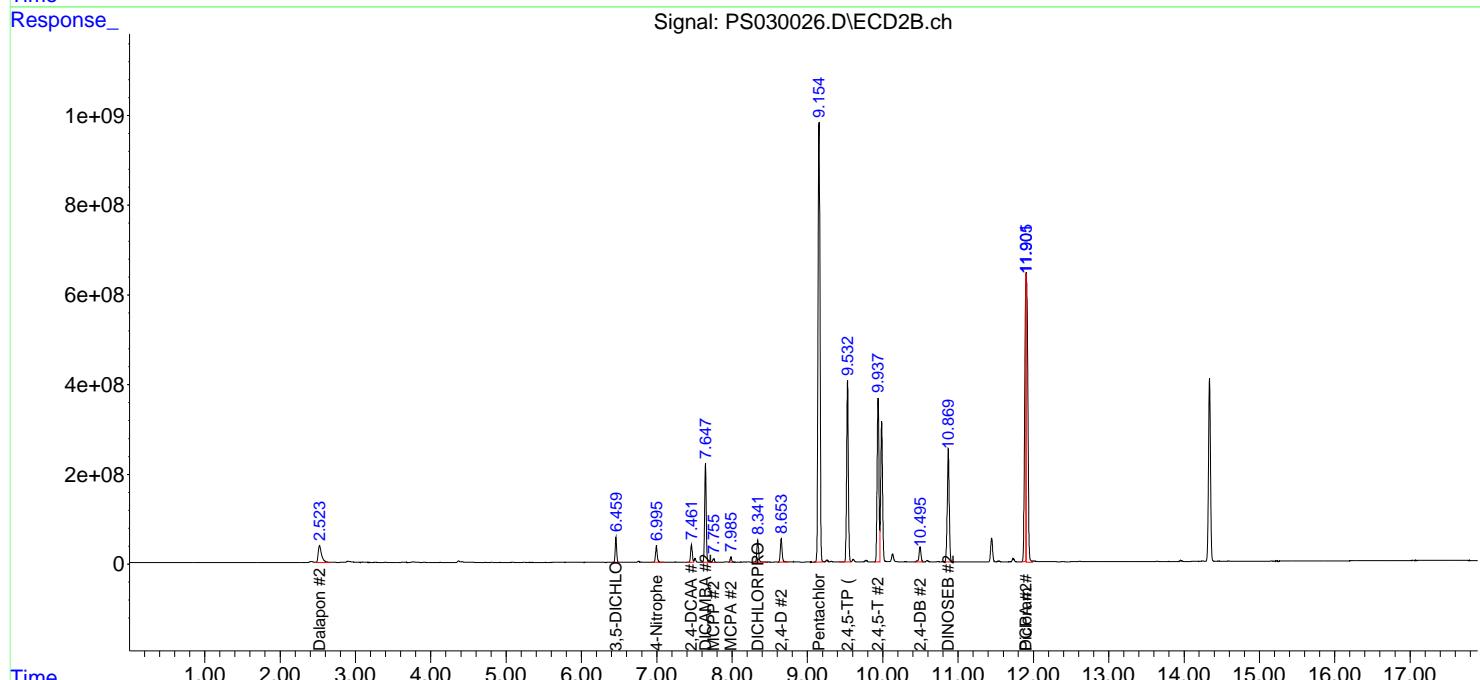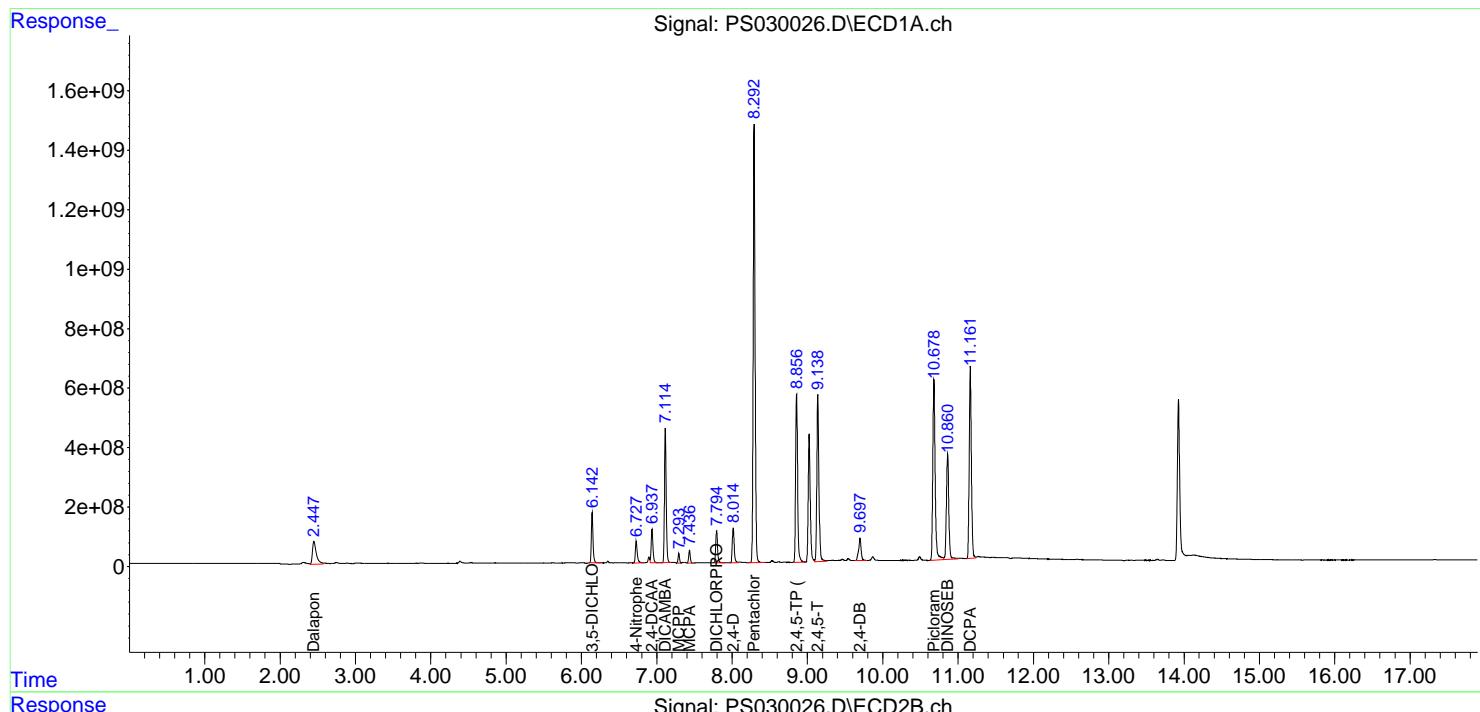

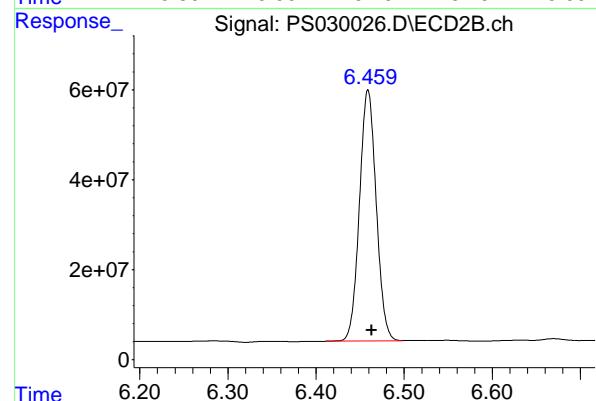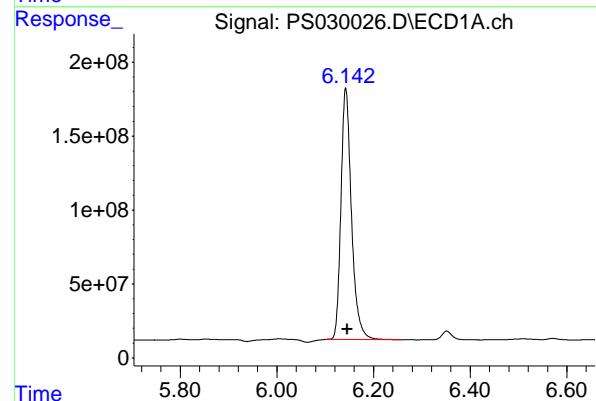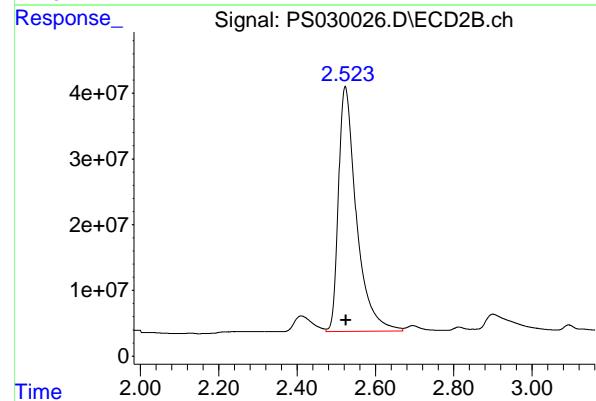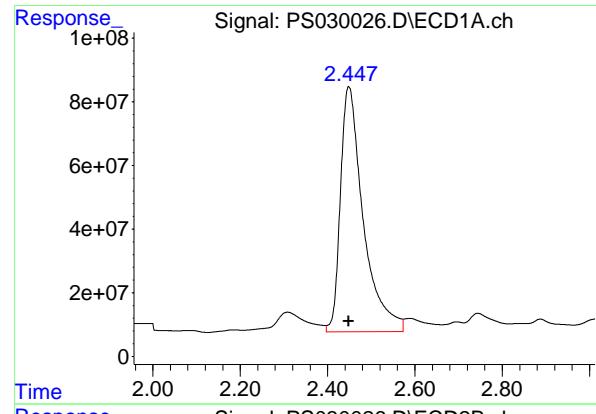

#1 Dalapon

R.T.: 2.448 min  
 Delta R.T.: 0.000 min  
 Response: 2794723971 ECD\_S  
 Conc: 682.43 ng/ml ClientSampleId : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

#1 Dalapon





R.T.: 2.523 min  
 Delta R.T.: -0.002 min  
 Response: 1185136689  
 Conc: 682.63 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.142 min  
 Delta R.T.: -0.003 min  
 Response: 2569680983  
 Conc: 719.04 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.459 min  
 Delta R.T.: -0.004 min  
 Response: 738239496  
 Conc: 755.17 ng/ml

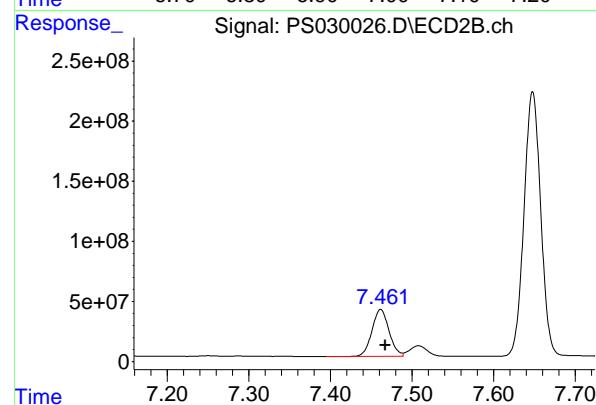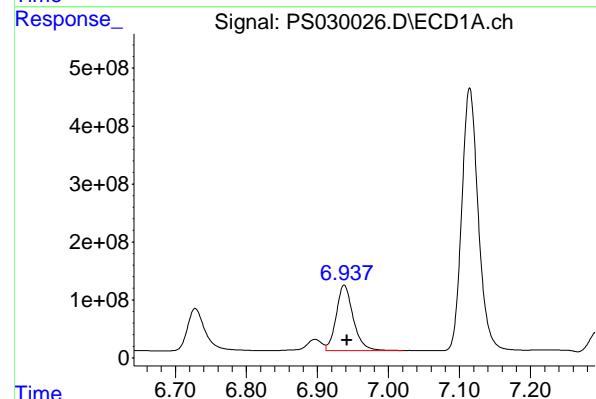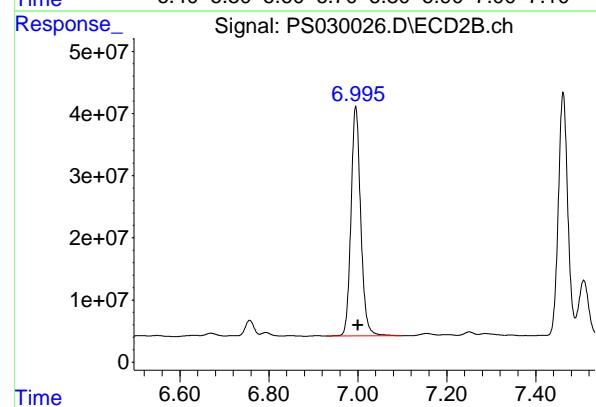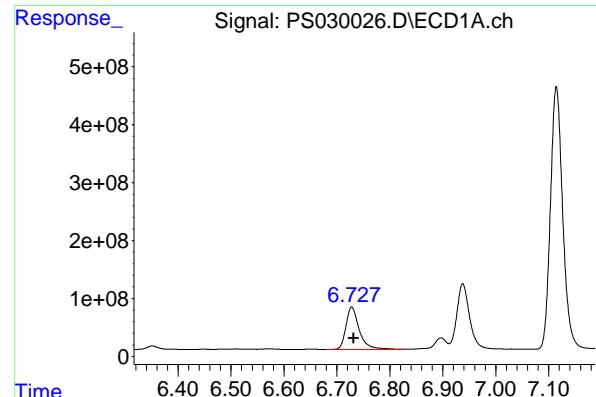

## #3 4-Nitrophenol

R.T.: 6.728 min  
 Delta R.T.: -0.003 min  
 Response: 1269317960  
 Conc: 711.77 ng/ml

Instrument: ECD\_S  
 Client Sample Id: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

## #3 4-Nitrophenol


R.T.: 6.995 min  
 Delta R.T.: -0.005 min  
 Response: 560191374  
 Conc: 731.40 ng/ml

## #4 2,4-DCAA

R.T.: 6.938 min  
 Delta R.T.: -0.004 min  
 Response: 1888378898  
 Conc: 767.30 ng/ml

## #4 2,4-DCAA

R.T.: 7.462 min  
 Delta R.T.: -0.006 min  
 Response: 569650088  
 Conc: 808.57 ng/ml

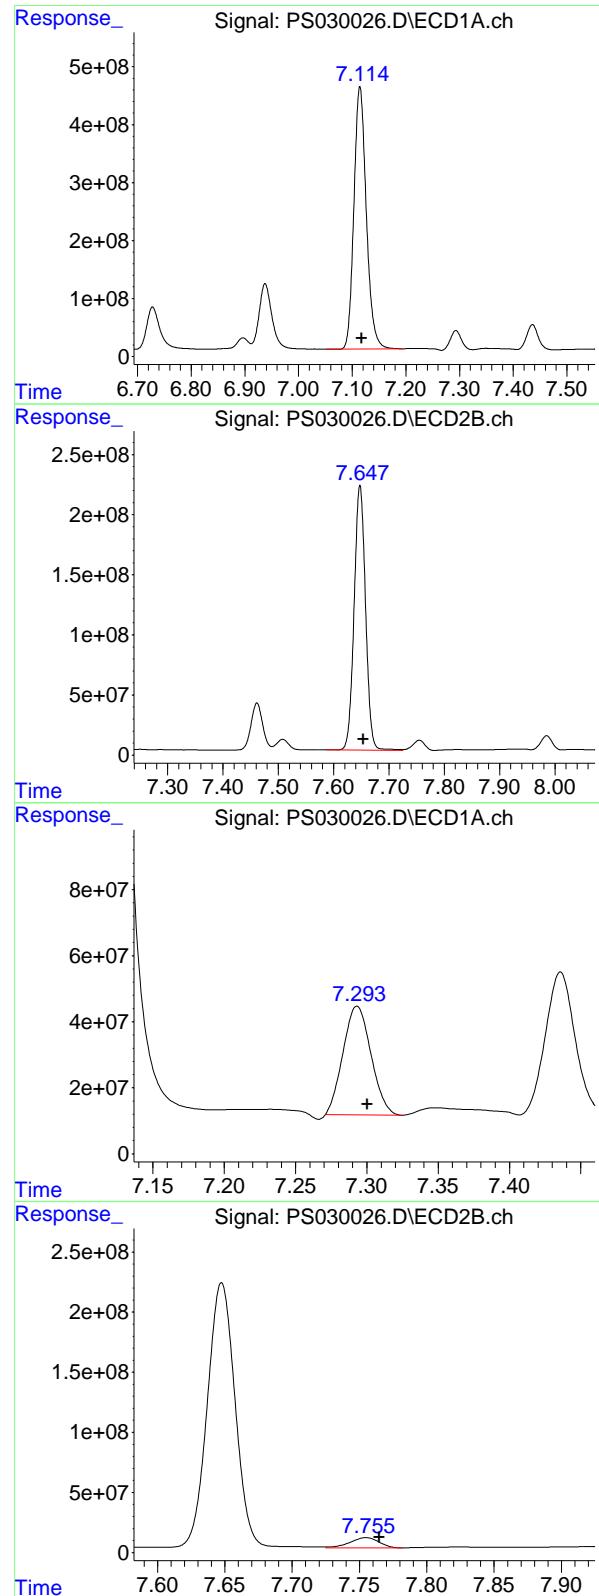

## #5 DICAMBA

R.T.: 7.114 min  
 Delta R.T.: -0.003 min  
 Response: 7246972846  
 Conc: 731.81 ng/ml  
 Instrument: ECD\_S  
 ClientSampleId : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

## #5 DICAMBA





R.T.: 7.648 min  
 Delta R.T.: -0.006 min  
 Response: 3150630491  
 Conc: 797.61 ng/ml

## #6 MCPP

R.T.: 7.293 min  
 Delta R.T.: -0.007 min  
 Response: 448334279  
 Conc: 69.58 ug/ml

## #6 MCPP

R.T.: 7.755 min  
 Delta R.T.: -0.010 min  
 Response: 125940998  
 Conc: 72.01 ug/ml

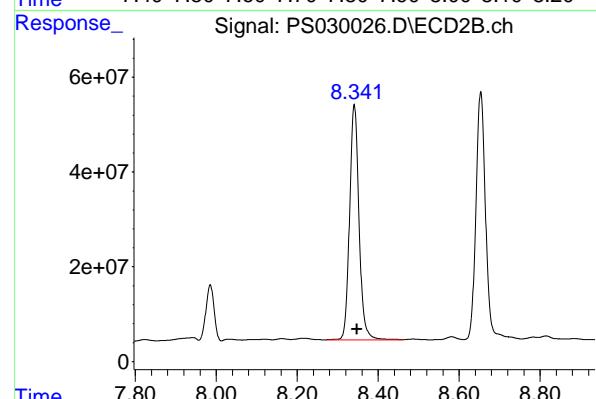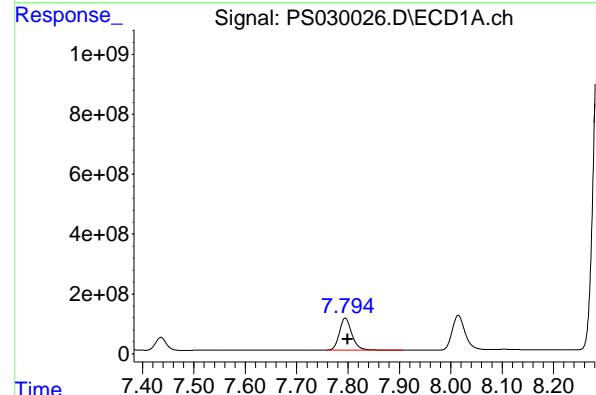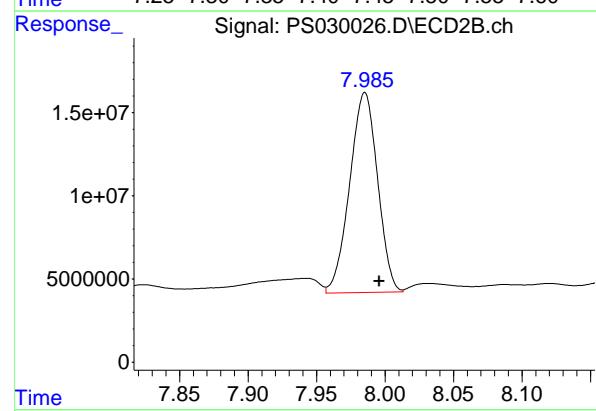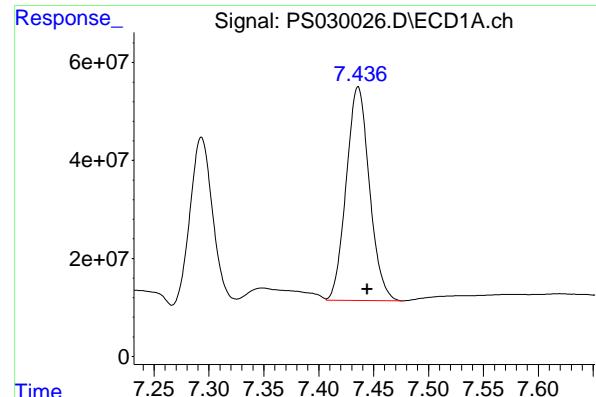

## #7 MCPA

R.T.: 7.436 min  
 Delta R.T.: -0.009 min  
 Response: 641028979  
 Conc: 72.59 ug/ml

Instrument: ECD\_S  
 Client SampleId : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

## #7 MCPA





R.T.: 7.985 min  
 Delta R.T.: -0.010 min  
 Response: 170258090  
 Conc: 71.97 ug/ml

## #8 DICHLORPROP

R.T.: 7.795 min  
 Delta R.T.: -0.004 min  
 Response: 1817853046  
 Conc: 717.35 ng/ml

## #8 DICHLORPROP

R.T.: 8.341 min  
 Delta R.T.: -0.007 min  
 Response: 801403222  
 Conc: 798.24 ng/ml

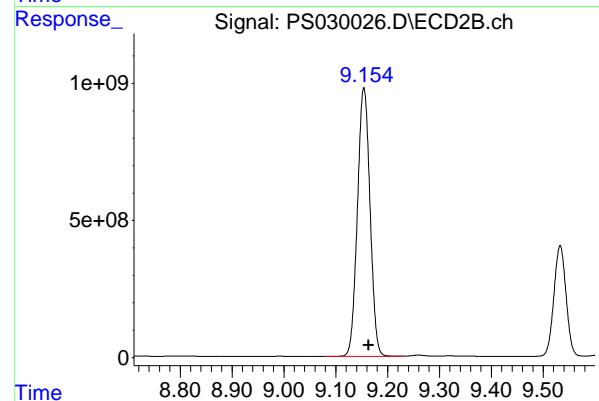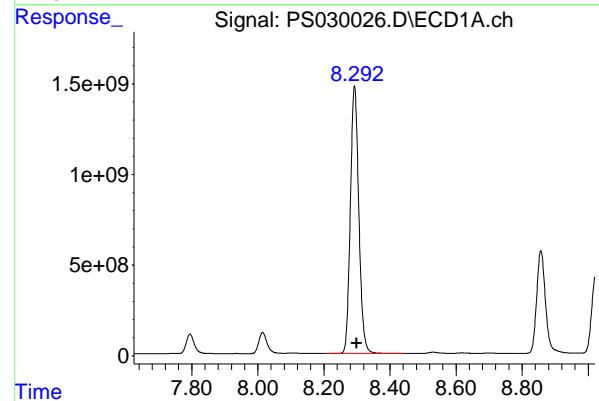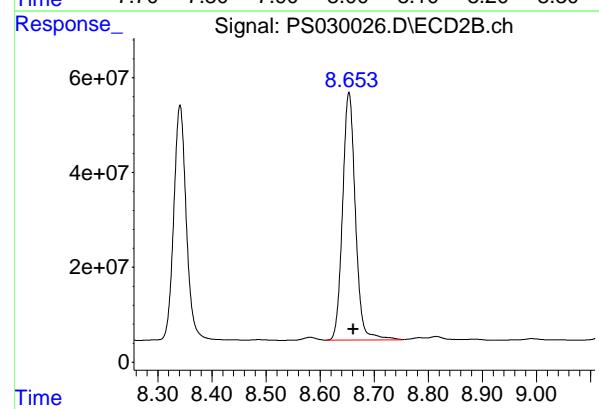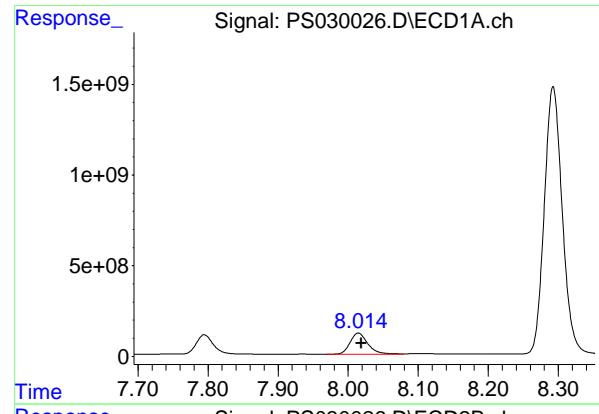

#9 2,4-D

R.T.: 8.015 min  
 Delta R.T.: -0.004 min  
 Response: 2045753582 ECD\_S  
 Conc: 727.28 ng/ml ClientSampleId : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

#9 2,4-D





R.T.: 8.653 min  
 Delta R.T.: -0.008 min  
 Response: 862543014  
 Conc: 765.27 ng/ml

#10 Pentachlorophenol

R.T.: 8.293 min  
 Delta R.T.: -0.007 min  
 Response: 26237549087  
 Conc: 752.12 ng/ml

#10 Pentachlorophenol

R.T.: 9.154 min  
 Delta R.T.: -0.009 min  
 Response: 16512921319  
 Conc: 811.65 ng/ml

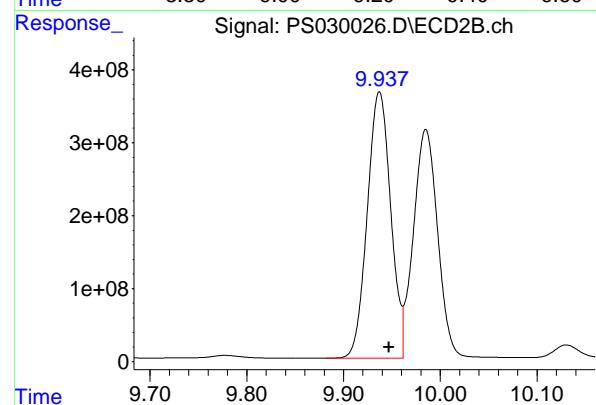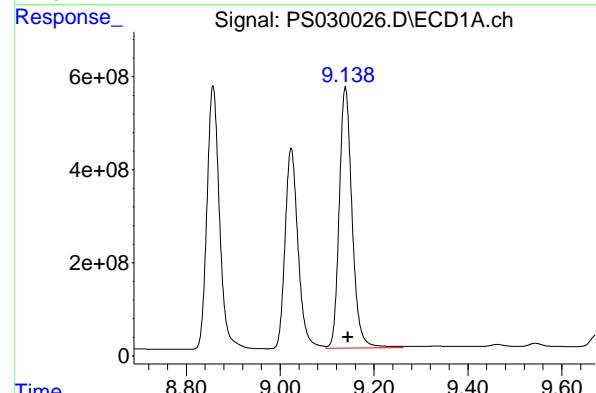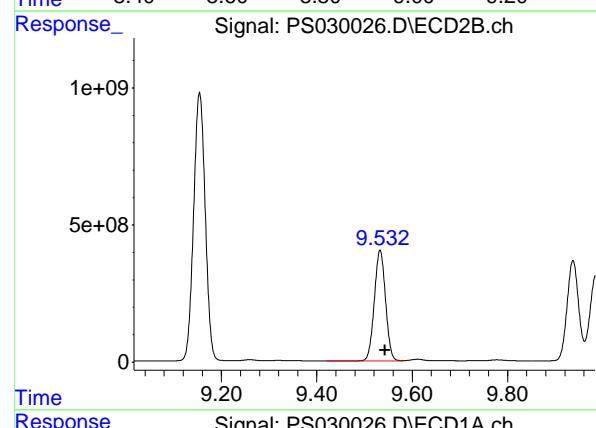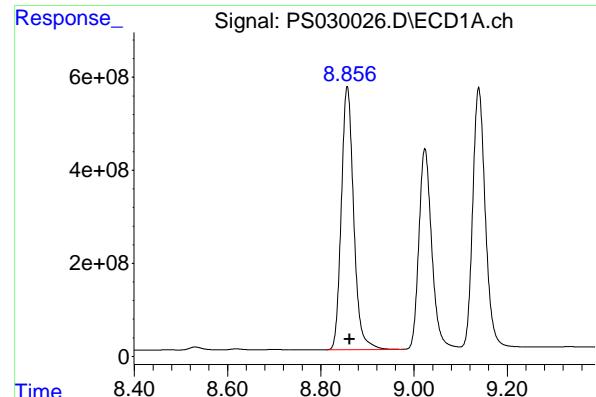

#11 2,4,5-TP (SILVEX)

R.T.: 8.857 min  
 Delta R.T.: -0.005 min  
 Response: 10417003423 ECD\_S  
 Conc: 751.43 ng/ml ClientSampleId : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

#11 2,4,5-TP (SILVEX)


R.T.: 9.533 min  
 Delta R.T.: -0.010 min  
 Response: 6556330082  
 Conc: 801.34 ng/ml

#12 2,4,5-T

R.T.: 9.139 min  
 Delta R.T.: -0.005 min  
 Response: 10641265427  
 Conc: 757.22 ng/ml

#12 2,4,5-T

R.T.: 9.937 min  
 Delta R.T.: -0.010 min  
 Response: 6136416767  
 Conc: 790.51 ng/ml

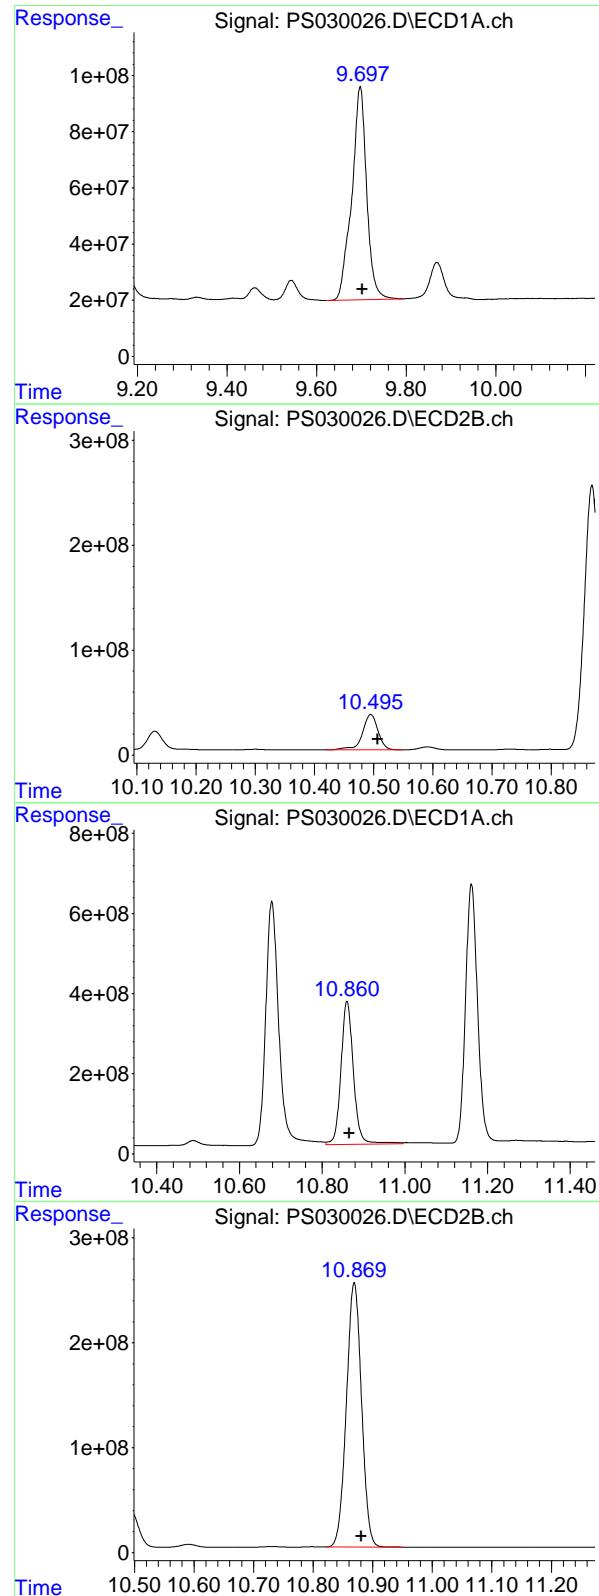

#13 2,4-DB

R.T.: 9.698 min  
 Delta R.T.: -0.004 min  
 Response: 1757631293 ECD\_S  
 Conc: 769.08 ng/ml Client SampleId : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

#13 2,4-DB


R.T.: 10.495 min  
 Delta R.T.: -0.011 min  
 Response: 617877165  
 Conc: 767.70 ng/ml

#14 DINOSEB

R.T.: 10.860 min  
 Delta R.T.: -0.006 min  
 Response: 7519170257  
 Conc: 739.10 ng/ml

#14 DINOSEB

R.T.: 10.869 min  
 Delta R.T.: -0.012 min  
 Response: 4438570711  
 Conc: 761.20 ng/ml

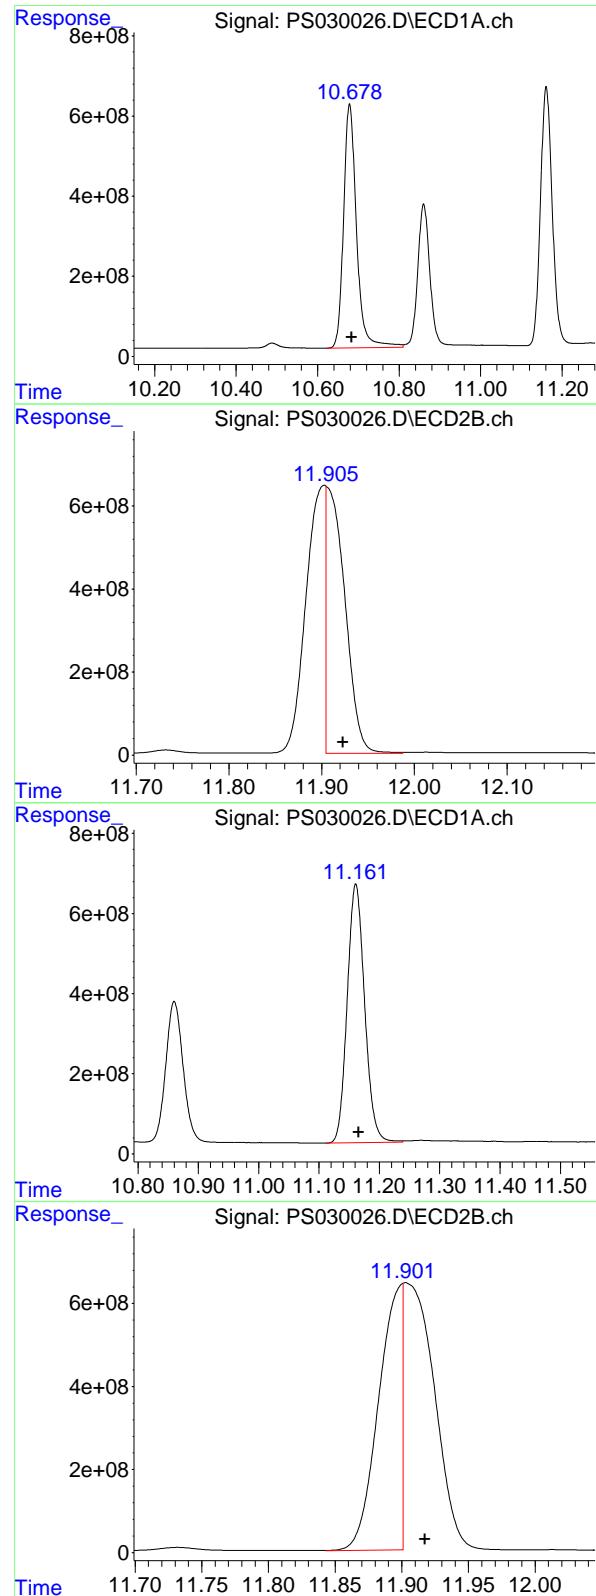

#15 Picloram

R.T.: 10.678 min  
 Delta R.T.: -0.005 min  
 Response: 13425673369 ECD\_S  
 Conc: 732.42 ng/ml Client Sample Id : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/02/2025  
 Supervised By :mohammad ahmed 05/05/2025

#15 Picloram

R.T.: 11.905 min  
 Delta R.T.: -0.018 min  
 Response: 8937696368  
 Conc: 727.61 ng/ml

#16 DCPA

R.T.: 11.161 min  
 Delta R.T.: -0.005 min  
 Response: 12986203927  
 Conc: 762.95 ng/ml

#16 DCPA

R.T.: 11.901 min  
 Delta R.T.: -0.017 min  
 Response: 8028317306  
 Conc: 712.26 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

Continuing Calib Date: 05/05/2025 Initial Calibration Date(s): 04/23/2025 04/23/2025

Continuing Calib Time: 09:55 Initial Calibration Time(s): 11:01 12:37

GC Column: RTX-CLP ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW		DIFF RT
			FROM	TO	
DICAMBA	7.11	7.12	7.02	7.22	0.01
2,4-DCAA	6.94	6.94	6.84	7.04	0.00
Dalapon	2.45	2.45	2.35	2.55	0.00
DICHLORPROP	7.80	7.80	7.70	7.90	0.00
2,4-D	8.02	8.02	7.92	8.12	0.00
2,4,5-TP(Silvex)	8.86	8.86	8.76	8.96	0.00
2,4,5-T	9.14	9.14	9.04	9.24	0.00
2,4-DB	9.70	9.70	9.60	9.80	0.00
Dinoseb	10.86	10.87	10.77	10.97	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

Continuing Calib Date: 05/05/2025 Initial Calibration Date(s): 04/23/2025 04/23/2025

Continuing Calib Time: 09:55 Initial Calibration Time(s): 11:01 12:37

GC Column: RTX-CLP2 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
DICAMBA	7.64	7.65	7.55	7.75	0.01
2,4-DCAA	7.46	7.47	7.37	7.57	0.01
Dalapon	2.52	2.53	2.43	2.63	0.01
DICHLORPROP	8.34	8.35	8.25	8.45	0.01
2,4-D	8.65	8.66	8.56	8.76	0.01
2,4,5-TP(Silvex)	9.53	9.54	9.44	9.64	0.01
2,4,5-T	9.93	9.95	9.85	10.05	0.02
2,4-DB	10.49	10.51	10.41	10.61	0.02
Dinoseb	10.87	10.88	10.78	10.98	0.02



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

GC Column: RTX-CLP ID: 0.32 (mm) Initi. Calib. Date(s): 04/23/2025 04/23/2025

Client Sample No.: CCAL06 Date Analyzed: 05/05/2025

Lab Sample No.: HSTDCCC750 Data File : PS030029.D Time Analyzed: 09:55

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
2,4,5-T	9.140	9.044	9.244	757.080	712.500	6.3
2,4,5-TP(Silvex)	8.857	8.762	8.962	758.140	712.500	6.4
2,4-D	8.015	7.919	8.119	776.810	705.000	10.2
2,4-DB	9.698	9.603	9.803	770.300	712.500	8.1
2,4-DCAA	6.938	6.842	7.042	772.860	750.000	3.0
Dalapon	2.446	2.349	2.549	769.750	682.500	12.8
DICAMBA	7.114	7.018	7.218	745.680	705.000	5.8
DICHLORPROP	7.795	7.699	7.899	758.480	705.000	7.6
Dinoseb	10.861	10.766	10.966	741.300	705.000	5.1



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

GC Column: RTX-CLP2 ID: 0.32 (mm) Initi. Calib. Date(s): 04/23/2025 04/23/2025

Client Sample No.: CCAL06 Date Analyzed: 05/05/2025

Lab Sample No.: HSTDCCC750 Data File : PS030029.D Time Analyzed: 09:55

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
2,4,5-T	9.933	9.847	10.047	770.140	712.500	8.1
2,4,5-TP(Silvex)	9.528	9.442	9.642	784.120	712.500	10.1
2,4-D	8.649	8.561	8.761	745.960	705.000	5.8
2,4-DB	10.491	10.407	10.607	757.060	712.500	6.3
2,4-DCAA	7.456	7.367	7.567	788.400	750.000	5.1
Dalapon	2.517	2.425	2.625	730.340	682.500	7.0
DICAMBA	7.642	7.553	7.753	789.280	705.000	12.0
DICHLORPROP	8.336	8.248	8.448	749.950	705.000	6.4
Dinoseb	10.865	10.781	10.981	753.620	705.000	6.9

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050525\  
 Data File : PS030029.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 05 May 2025 09:55  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDCCC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/06/2025  
 Supervised By :mohammad ahmed 05/07/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 05 12:29:05 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

4) S 2,4-DCAA 6.938 7.456 1902.1E6 555.4E6 772.860 788.396

**Target Compounds**

1) T	Dalapon	2.446	2.517	3152.3E6	1268.0E6	769.749	730.345
2) T	3,5-DICHL...	6.142	6.454	2580.1E6	718.9E6	721.950	735.376
3) T	4-Nitroph...	6.728	6.990	1270.3E6	554.2E6	712.324	723.635
5) T	DICAMBA	7.114	7.642	7384.3E6	3117.7E6	745.677	789.285
6) T	MCPP	7.293	7.750	474.5E6	139.3E6	73.642	79.630
7) T	MCPA	7.436	7.981	643.1E6	166.0E6	72.816	70.169
8) T	DICHLORPROP	7.795	8.336	1922.1E6	752.9E6	758.477	749.952
9) T	2,4-D	8.015	8.649	2185.1E6	840.8E6	776.807	745.962
10) T	Pentachlo...	8.293	9.150	26374.8E6	16140.6E6	756.051	793.353
11) T	2,4,5-TP ...	8.857	9.528	10510.0E6	6415.5E6	758.140	784.122
12) T	2,4,5-T	9.140	9.933	10639.4E6	5978.3E6	757.082	770.140
13) T	2,4-DB	9.698	10.491	1760.4E6	609.3E6	770.297	757.064
14) T	DINOSEB	10.861	10.865	7541.6E6	4394.3E6	741.305	753.615
15) T	Picloram	10.679	11.902	13895.4E6	8583.7E6	758.042	698.789m
16) T	DCPA	11.162	11.900	12980.1E6	8855.1E6	762.591	785.607m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050525\  
 Data File : PS030029.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 05 May 2025 09:55  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1



Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 05 12:29:05 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation





Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDCCC750

### Manual Integrations APPROVED

Reviewed By :Abdul Mirza 05/06/2025  
 Supervised By :mohammad ahmed 05/07/2025

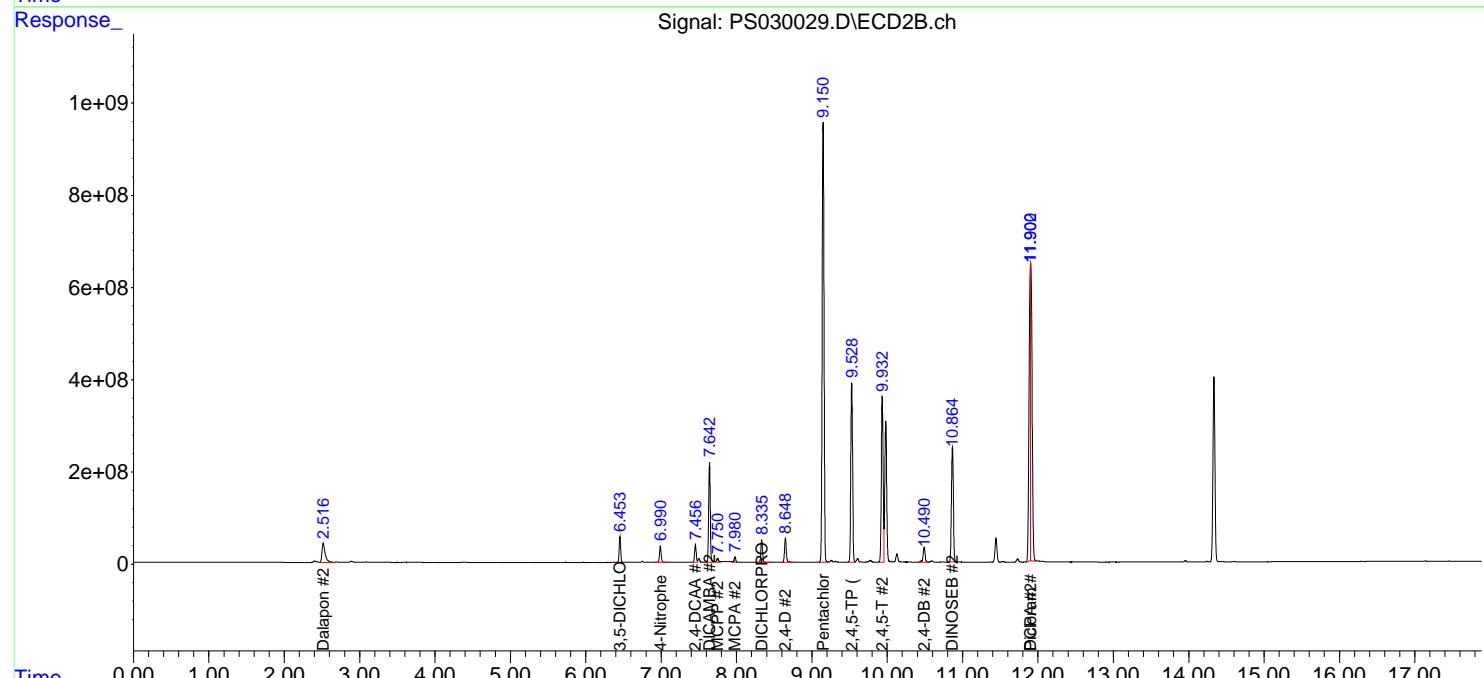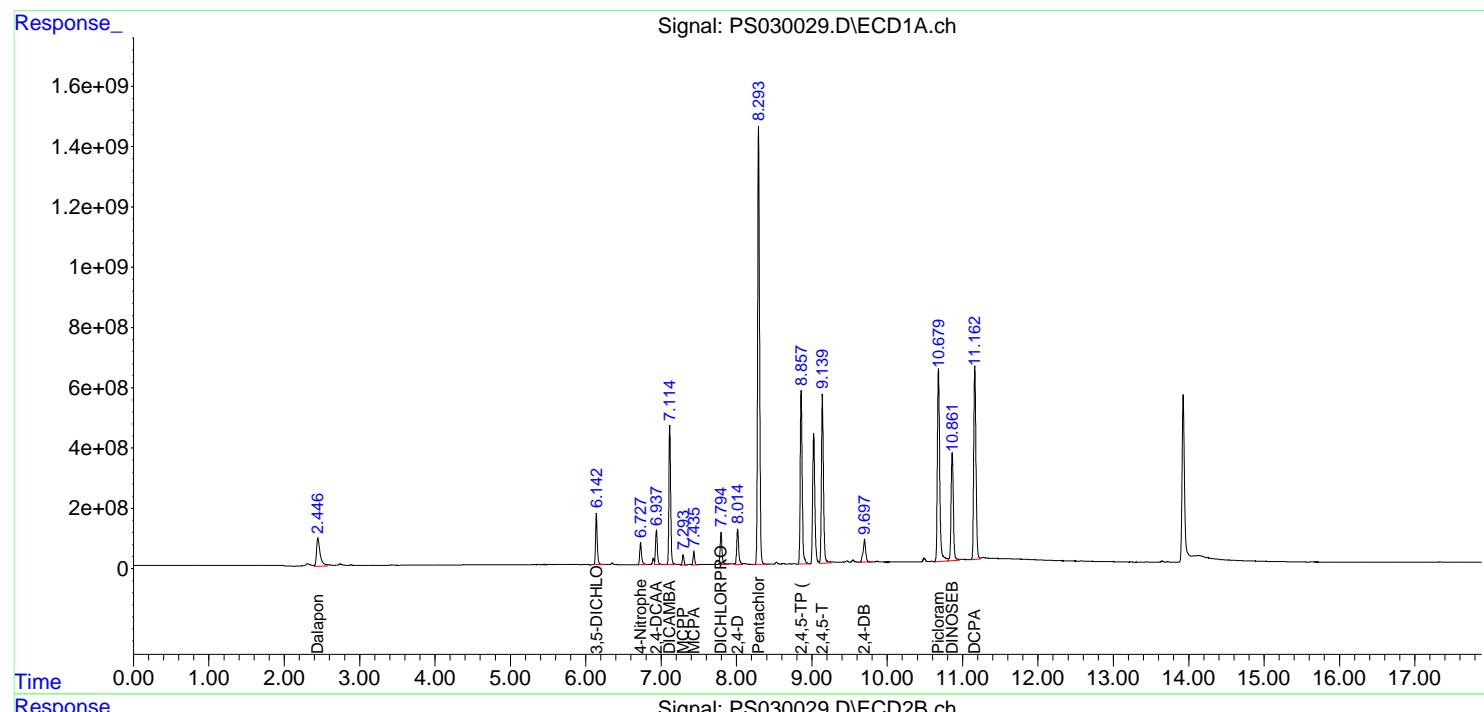

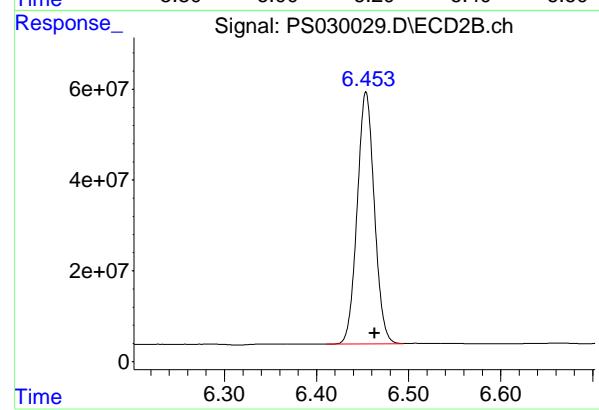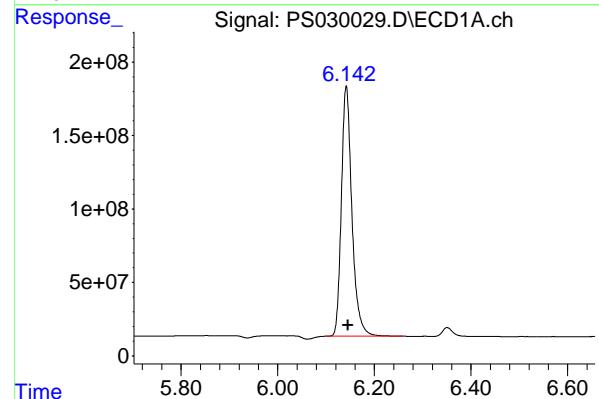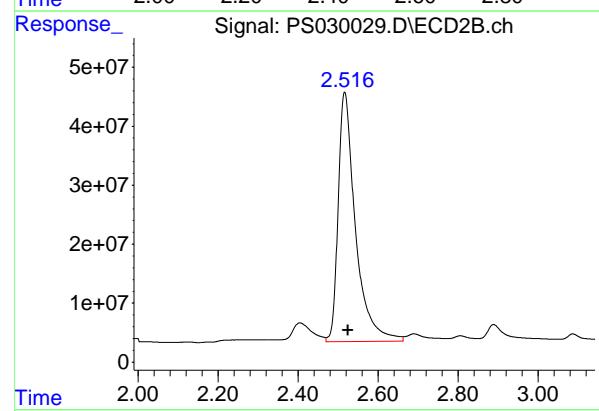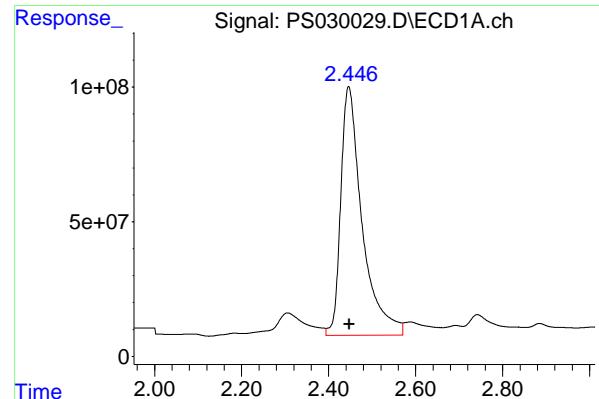

#1 Dalapon

R.T.: 2.446 min  
 Delta R.T.: -0.002 min  
 Response: 3152321923 ECD\_S  
 Conc: 769.75 ng/ml ClientSampleId : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/06/2025  
 Supervised By :mohammad ahmed 05/07/2025

#1 Dalapon





R.T.: 2.517 min  
 Delta R.T.: -0.008 min  
 Response: 1267983437  
 Conc: 730.34 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.142 min  
 Delta R.T.: -0.003 min  
 Response: 2580095757  
 Conc: 721.95 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.454 min  
 Delta R.T.: -0.009 min  
 Response: 718888293  
 Conc: 735.38 ng/ml

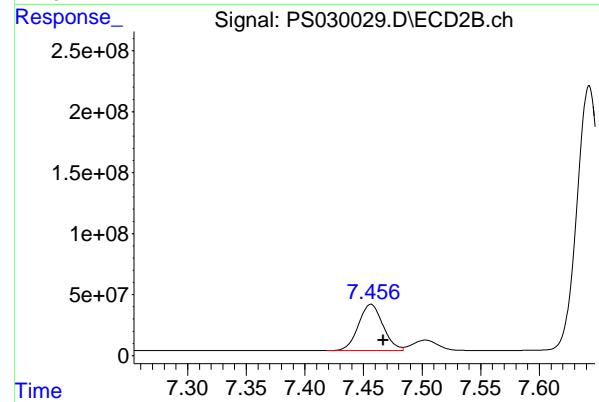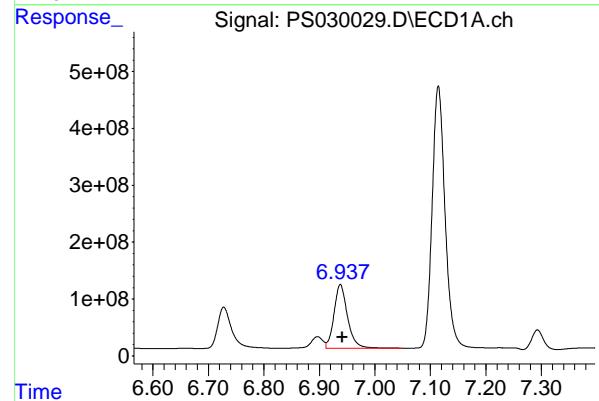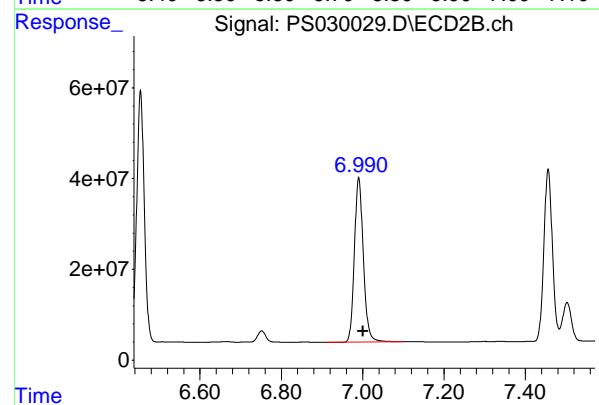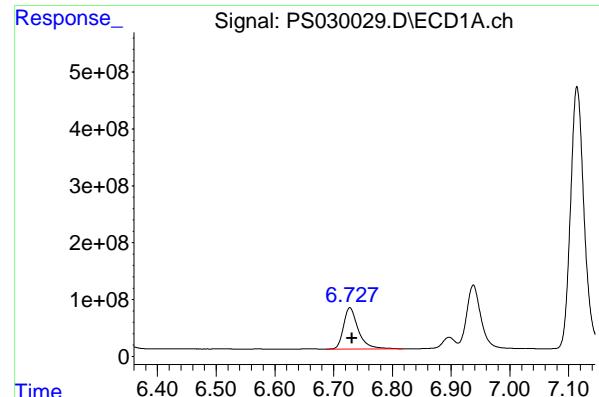

## #3 4-Nitrophenol

R.T.: 6.728 min  
Delta R.T.: -0.004 min  
Instrument: ECD\_S  
Response: 1270301802  
Conc: 712.32 ng/ml  
ClientSampleId: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/06/2025  
Supervised By :mohammad ahmed 05/07/2025

## #3 4-Nitrophenol


R.T.: 6.990 min  
Delta R.T.: -0.010 min  
Response: 554247176  
Conc: 723.63 ng/ml

## #4 2,4-DCAA

R.T.: 6.938 min  
Delta R.T.: -0.004 min  
Response: 1902069709  
Conc: 772.86 ng/ml

## #4 2,4-DCAA

R.T.: 7.456 min  
Delta R.T.: -0.011 min  
Response: 555438378  
Conc: 788.40 ng/ml

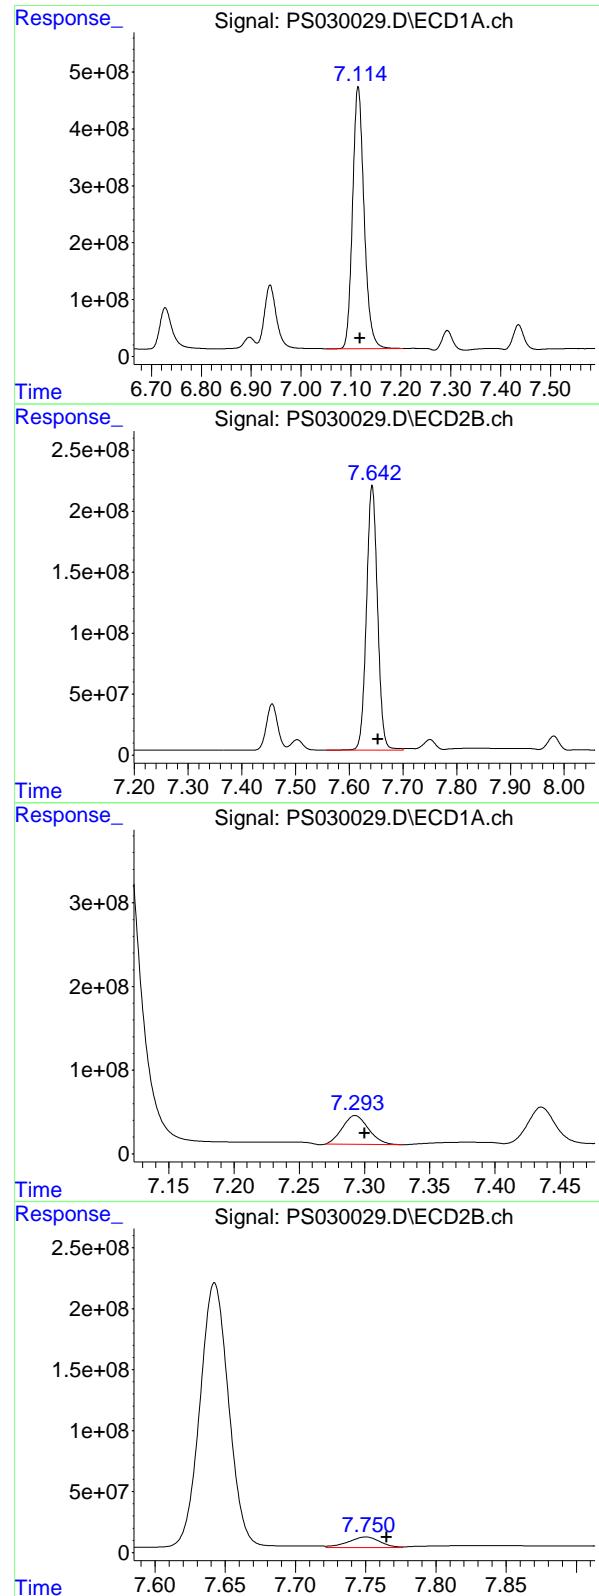

## #5 DICAMBA

R.T.: 7.114 min  
 Delta R.T.: -0.004 min  
 Response: 7384334899  
 Conc: 745.68 ng/ml  
 Instrument: ECD\_S  
 ClientSampleId : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/06/2025  
 Supervised By :mohammad ahmed 05/07/2025

## #5 DICAMBA





R.T.: 7.642 min  
 Delta R.T.: -0.011 min  
 Response: 3117725389  
 Conc: 789.28 ng/ml

## #6 MCPP

R.T.: 7.293 min  
 Delta R.T.: -0.007 min  
 Response: 474519993  
 Conc: 73.64 ug/ml

## #6 MCPP

R.T.: 7.750 min  
 Delta R.T.: -0.014 min  
 Response: 139269003  
 Conc: 79.63 ug/ml

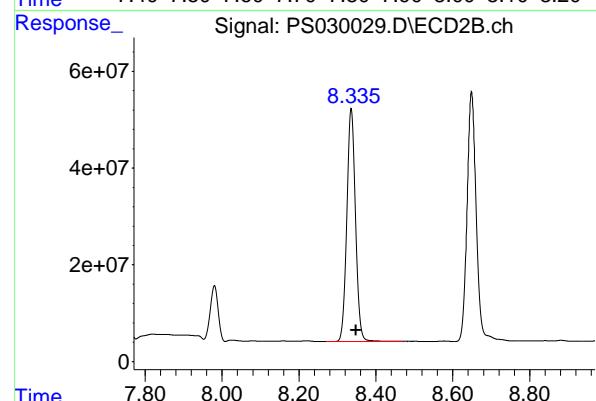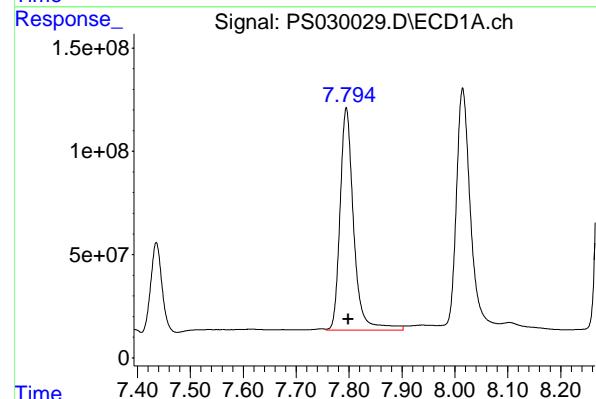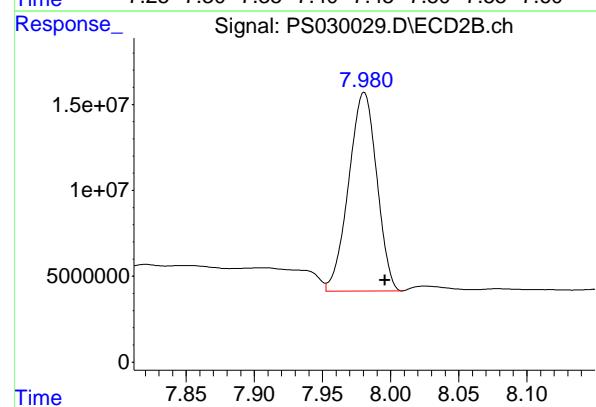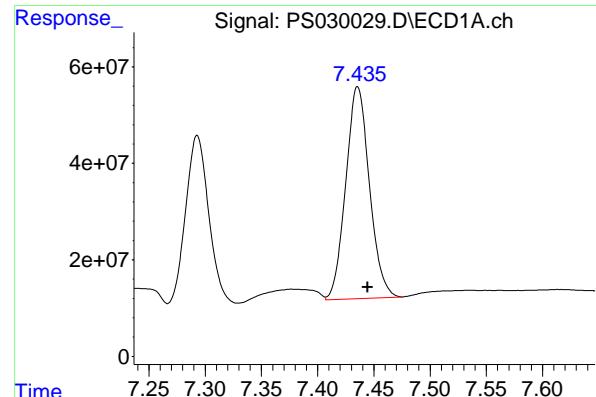

## #7 MCPA

R.T.: 7.436 min  
Delta R.T.: -0.009 min  
Instrument: ECD\_S  
Response: 643063428  
Conc: 72.82 ug/ml  
ClientSampleId: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/06/2025  
Supervised By :mohammad ahmed 05/07/2025

## #7 MCPA





R.T.: 7.981 min  
Delta R.T.: -0.015 min  
Response: 166006369  
Conc: 70.17 ug/ml

## #8 DICHLORPROP

R.T.: 7.795 min  
Delta R.T.: -0.004 min  
Response: 1922063526  
Conc: 758.48 ng/ml

## #8 DICHLORPROP

R.T.: 8.336 min  
Delta R.T.: -0.012 min  
Response: 752925374  
Conc: 749.95 ng/ml

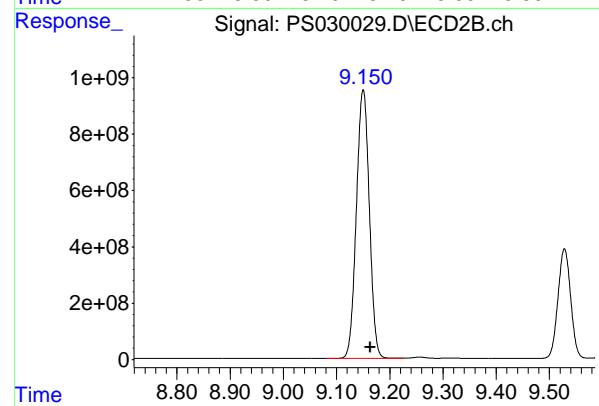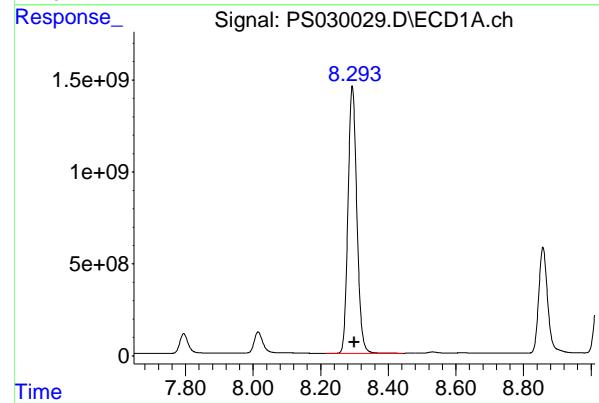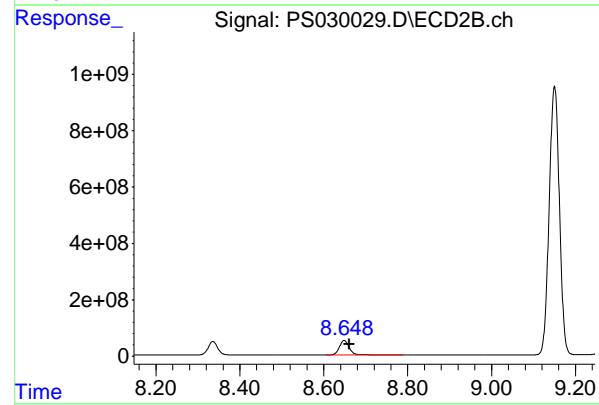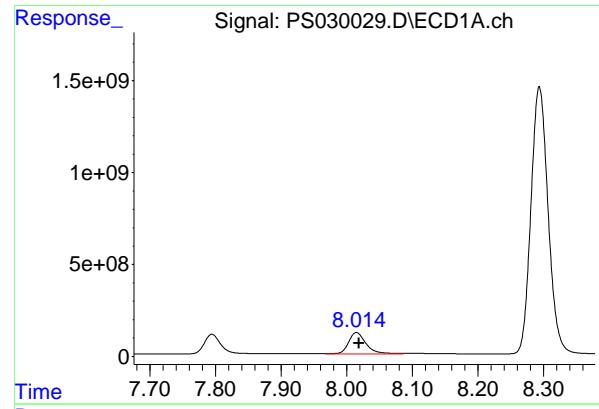

#9 2,4-D

R.T.: 8.015 min  
 Delta R.T.: -0.004 min  
 Response: 2185058539  
 Conc: 776.81 ng/ml

Instrument: ECD\_S  
 Client Sample ID: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/06/2025  
 Supervised By :mohammad ahmed 05/07/2025

#9 2,4-D





R.T.: 8.649 min  
 Delta R.T.: -0.012 min  
 Response: 840778929  
 Conc: 745.96 ng/ml

#10 Pentachlorophenol

R.T.: 8.293 min  
 Delta R.T.: -0.006 min  
 Response: 26374849284  
 Conc: 756.05 ng/ml

#10 Pentachlorophenol

R.T.: 9.150 min  
 Delta R.T.: -0.013 min  
 Response: 16140623302  
 Conc: 793.35 ng/ml

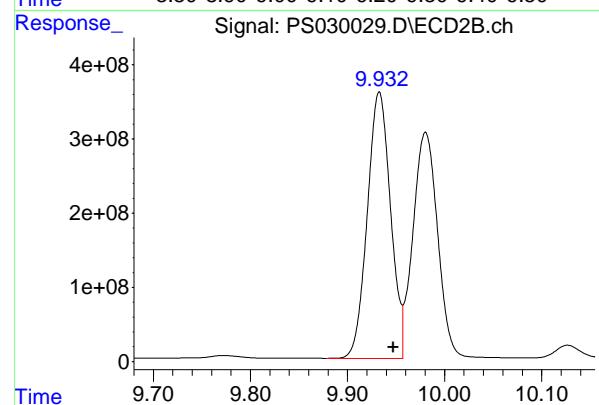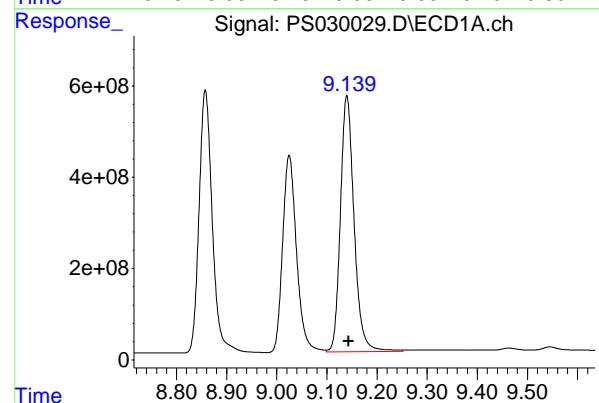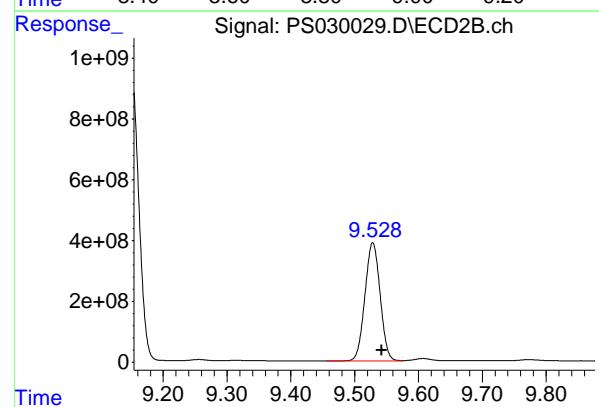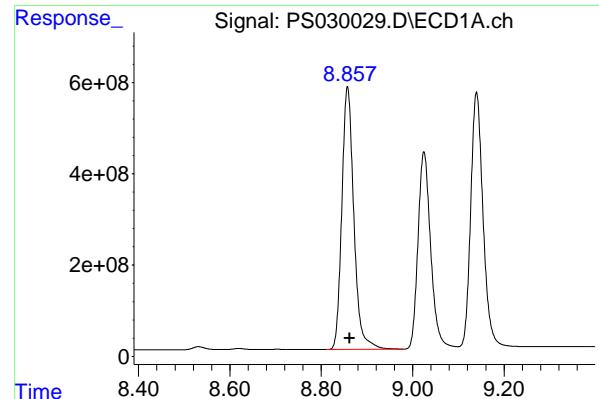

#11 2,4,5-TP (SILVEX)

R.T.: 8.857 min

Delta R.T.: -0.005 min

Instrument: ECD\_S

Response: 10509968082

Conc: 758.14 ng/ml

ClientSampleId: HSTDCCC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/06/2025

Supervised By :mohammad ahmed 05/07/2025

#11 2,4,5-TP (SILVEX)

R.T.: 9.528 min

Delta R.T.: -0.014 min

Response: 6415490809

Conc: 784.12 ng/ml

#12 2,4,5-T

R.T.: 9.140 min

Delta R.T.: -0.004 min

Response: 10639353854

Conc: 757.08 ng/ml


#12 2,4,5-T

R.T.: 9.933 min

Delta R.T.: -0.015 min

Response: 5978287108

Conc: 770.14 ng/ml

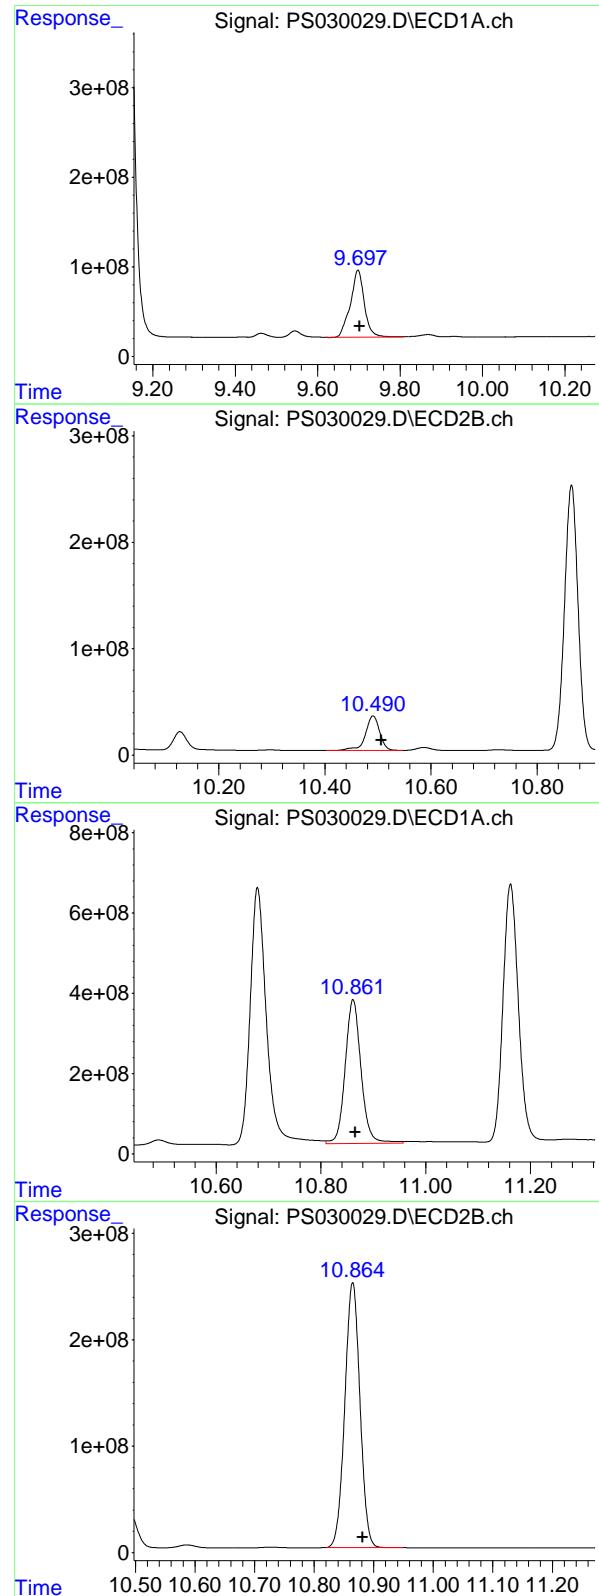

#13 2,4-DB

R.T.: 9.698 min  
 Delta R.T.: -0.004 min  
 Response: 1760403680 ECD\_S  
 Conc: 770.30 ng/ml Client Sample Id : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/06/2025  
 Supervised By :mohammad ahmed 05/07/2025

#13 2,4-DB


R.T.: 10.491 min  
 Delta R.T.: -0.016 min  
 Response: 609316861  
 Conc: 757.06 ng/ml

#14 DINOSEB

R.T.: 10.861 min  
 Delta R.T.: -0.004 min  
 Response: 7541611717  
 Conc: 741.30 ng/ml

#14 DINOSEB

R.T.: 10.865 min  
 Delta R.T.: -0.016 min  
 Response: 4394315725  
 Conc: 753.62 ng/ml

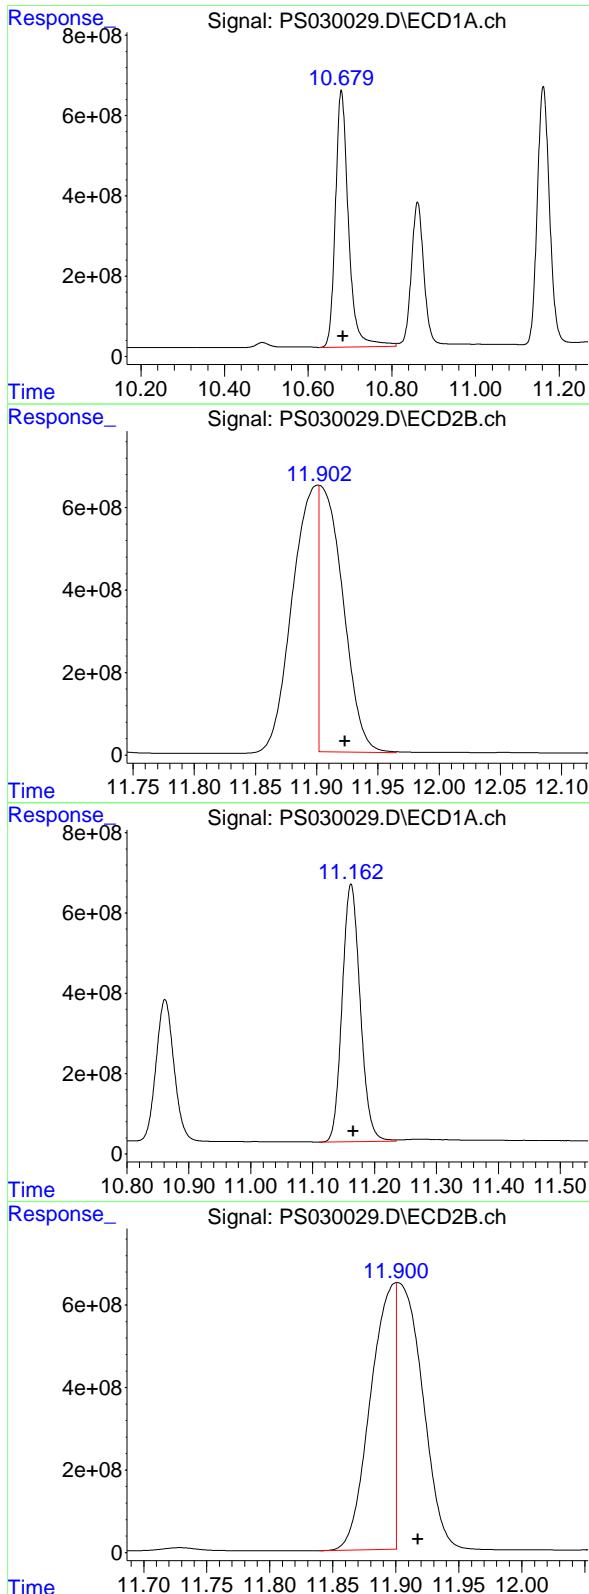

## #15 Picloram

R.T.: 10.679 min  
 Delta R.T.: -0.004 min  
 Response: 13895378925  
 Conc: 758.04 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/06/2025  
 Supervised By :mohammad ahmed 05/07/2025

## #15 Picloram

R.T.: 11.902 min  
 Delta R.T.: -0.021 min  
 Response: 8583671437  
 Conc: 698.79 ng/ml

## #16 DCPA

R.T.: 11.162 min  
 Delta R.T.: -0.004 min  
 Response: 12980066848  
 Conc: 762.59 ng/ml

## #16 DCPA

R.T.: 11.900 min  
 Delta R.T.: -0.018 min  
 Response: 8855092205  
 Conc: 785.61 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

Continuing Calib Date: 05/05/2025 Initial Calibration Date(s): 04/23/2025 04/23/2025

Continuing Calib Time: 16:41 Initial Calibration Time(s): 11:01 12:37

GC Column: RTX-CLP ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW		DIFF RT
			FROM	TO	
DICAMBA	7.11	7.12	7.02	7.22	0.01
2,4-DCAA	6.94	6.94	6.84	7.04	0.00
Dalapon	2.45	2.45	2.35	2.55	0.01
DICHLORPROP	7.79	7.80	7.70	7.90	0.01
2,4-D	8.01	8.02	7.92	8.12	0.01
2,4,5-TP(Silvex)	8.86	8.86	8.76	8.96	0.00
2,4,5-T	9.14	9.14	9.04	9.24	0.00
2,4-DB	9.70	9.70	9.60	9.80	0.00
Dinoseb	10.86	10.87	10.77	10.97	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

Continuing Calib Date: 05/05/2025 Initial Calibration Date(s): 04/23/2025 04/23/2025

Continuing Calib Time: 16:41 Initial Calibration Time(s): 11:01 12:37

GC Column: RTX-CLP2 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM	TO	DIFF RT
DICAMBA	7.64	7.65	7.55	7.75	0.01
2,4-DCAA	7.46	7.47	7.37	7.57	0.02
Dalapon	2.52	2.53	2.43	2.63	0.01
DICHLORPROP	8.34	8.35	8.25	8.45	0.01
2,4-D	8.65	8.66	8.56	8.76	0.01
2,4,5-TP(Silvex)	9.53	9.54	9.44	9.64	0.01
2,4,5-T	9.93	9.95	9.85	10.05	0.02
2,4-DB	10.49	10.51	10.41	10.61	0.02
Dinoseb	10.86	10.88	10.78	10.98	0.02



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

GC Column: RTX-CLP ID: 0.32 (mm) Initi. Calib. Date(s): 04/23/2025 04/23/2025

Client Sample No.: CCAL07 Date Analyzed: 05/05/2025

Lab Sample No.: HSTDCCC750 Data File : PS030041.D Time Analyzed: 16:41

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
2,4,5-T	9.139	9.044	9.244	707.160	712.500	-0.7
2,4,5-TP(Silvex)	8.857	8.762	8.962	704.000	712.500	-1.2
2,4-D	8.014	7.919	8.119	687.970	705.000	-2.4
2,4-DB	9.699	9.603	9.803	717.320	712.500	0.7
2,4-DCAA	6.936	6.842	7.042	721.190	750.000	-3.8
Dalapon	2.445	2.349	2.549	720.930	682.500	5.6
DICAMBA	7.114	7.018	7.218	688.440	705.000	-2.3
DICHLORPROP	7.794	7.699	7.899	674.770	705.000	-4.3
Dinoseb	10.861	10.766	10.966	699.240	705.000	-0.8



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

### CALIBRATION VERIFICATION SUMMARY

Contract: NOBI03

Lab Code: CHEM Case No.: Q1883 SAS No.: Q1883 SDG NO.: Q1883

GC Column: RTX-CLP2 ID: 0.32 (mm) Initi. Calib. Date(s): 04/23/2025 04/23/2025

Client Sample No.: CCAL07 Date Analyzed: 05/05/2025

Lab Sample No.: HSTDCCC750 Data File : PS030041.D Time Analyzed: 16:41

COMPOUND	RT	RT WINDOW FROM	TO	CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
2,4,5-T	9.932	9.847	10.047	719.530	712.500	1.0
2,4,5-TP(Silvex)	9.527	9.442	9.642	729.410	712.500	2.4
2,4-D	8.648	8.561	8.761	696.650	705.000	-1.2
2,4-DB	10.490	10.407	10.607	693.040	712.500	-2.7
2,4-DCAA	7.455	7.367	7.567	737.500	750.000	-1.7
Dalapon	2.516	2.425	2.625	674.830	682.500	-1.1
DICAMBA	7.642	7.553	7.753	730.790	705.000	3.7
DICHLORPROP	8.335	8.248	8.448	708.150	705.000	0.4
Dinoseb	10.864	10.781	10.981	696.840	705.000	-1.2

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050525\  
 Data File : PS030041.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 05 May 2025 16:41  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDCCC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/06/2025  
 Supervised By :mohammad ahmed 05/07/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 06 01:40:04 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

4) S 2,4-DCAA 6.936 7.455 1774.9E6 519.6E6 721.191 737.501

**Target Compounds**

1) T	Dalapon	2.445	2.516	2952.4E6	1171.6E6	720.926	674.830
2) T	3,5-DICHL...	6.141	6.453	2409.7E6	672.1E6	674.261	687.519
3) T	4-Nitroph...	6.727	6.988	1181.1E6	512.8E6	662.301	669.462m
5) T	DICAMBA	7.114	7.642	6817.6E6	2886.7E6	688.443	730.789
6) T	MCPP	7.292	7.748	422.5E6	110.6E6	65.574	63.223
7) T	MCPA	7.435	7.979	581.0E6	149.4E6	65.784	63.137
8) T	DICHLORPROP	7.794	8.335	1709.9E6	711.0E6	674.770	708.151
9) T	2,4-D	8.014	8.648	1935.2E6	785.2E6	687.965	696.646
10) T	Pentachlo...	8.292	9.149	24554.7E6	15042.3E6	703.874	739.367
11) T	2,4,5-TP ...	8.857	9.527	9759.5E6	5967.9E6	704.004	729.413
12) T	2,4,5-T	9.139	9.932	9937.7E6	5585.4E6	707.156	719.532
13) T	2,4-DB	9.699	10.490	1639.3E6	557.8E6	717.316	693.045
14) T	DINOSEB	10.861	10.864	7113.6E6	4063.2E6	699.237	696.838
15) T	Picloram	10.680	11.903	13035.9E6	7955.5E6	711.154	647.647m
16) T	DCPA	11.162	11.900	12175.4E6	8586.9E6	715.318	761.813m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050525\  
 Data File : PS030041.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 05 May 2025 16:41  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1



Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDCCC750





**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/06/2025  
 Supervised By :mohammad ahmed 05/07/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 06 01:40:04 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

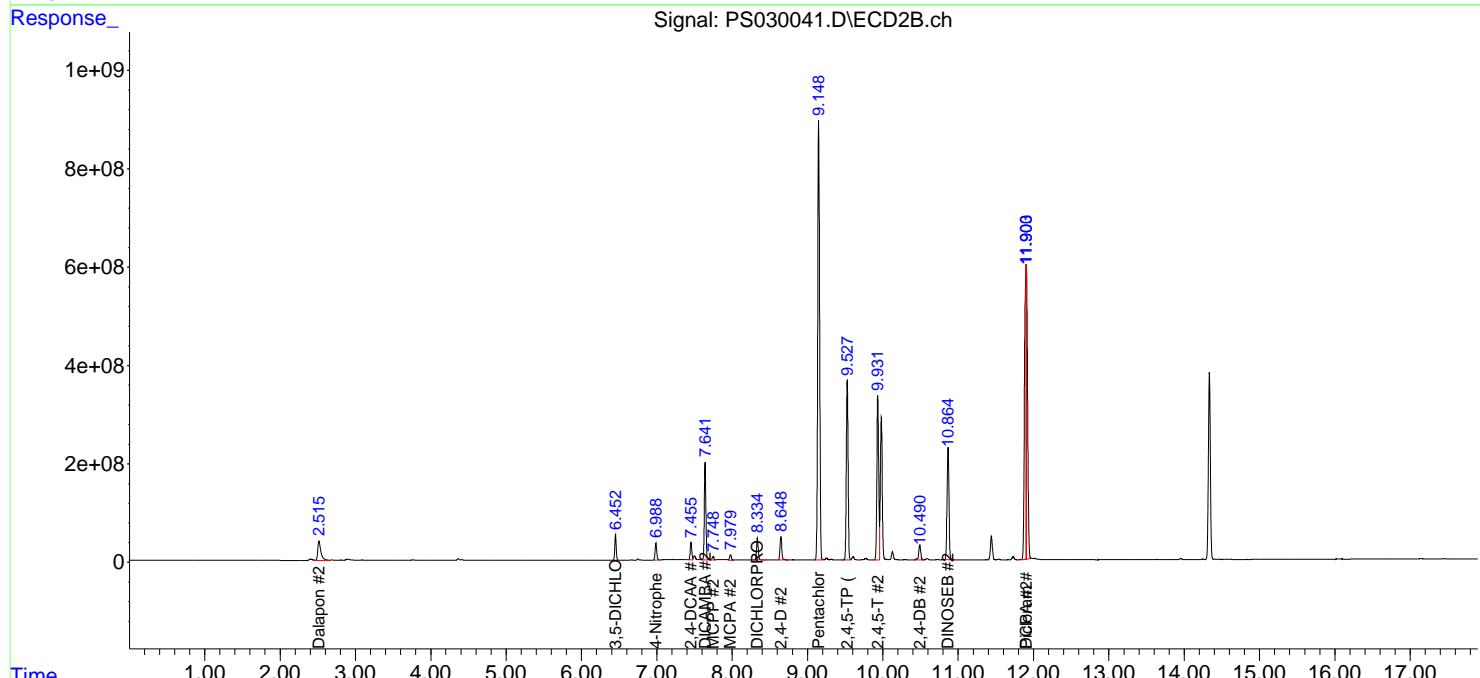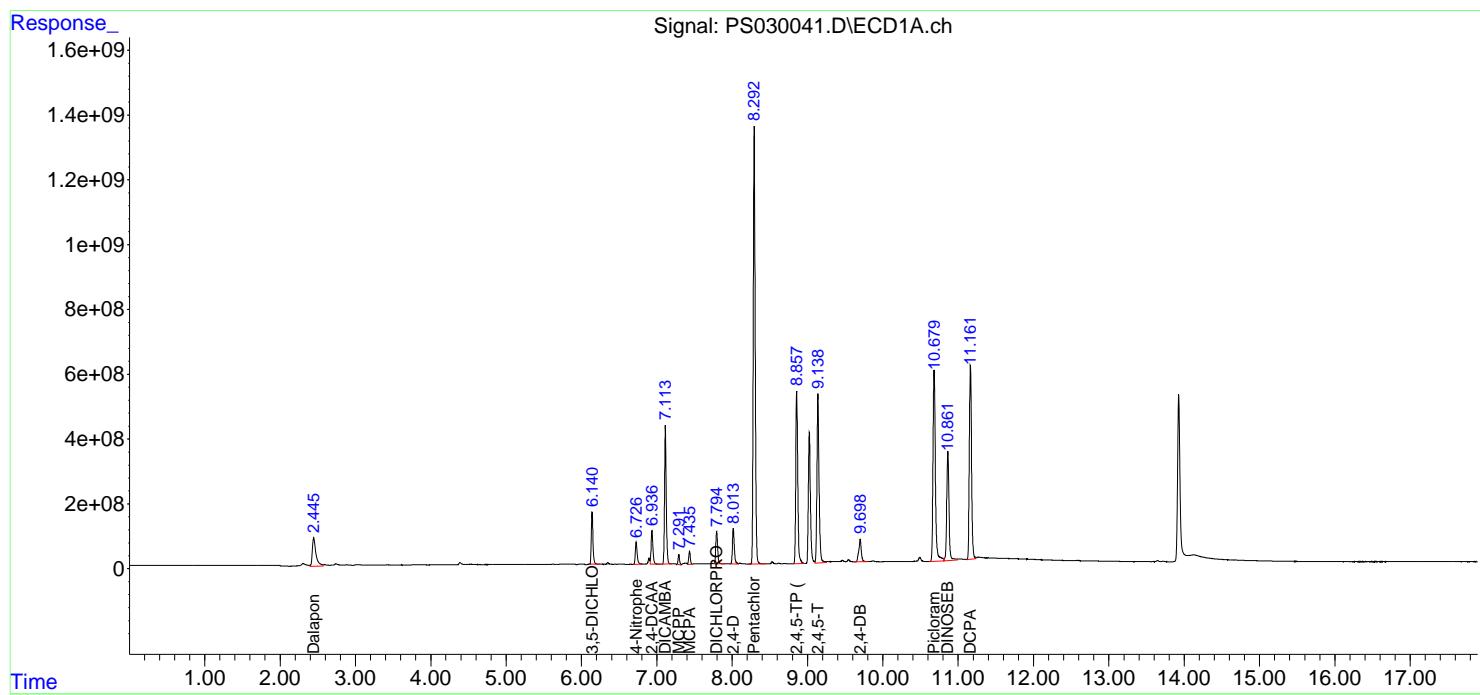

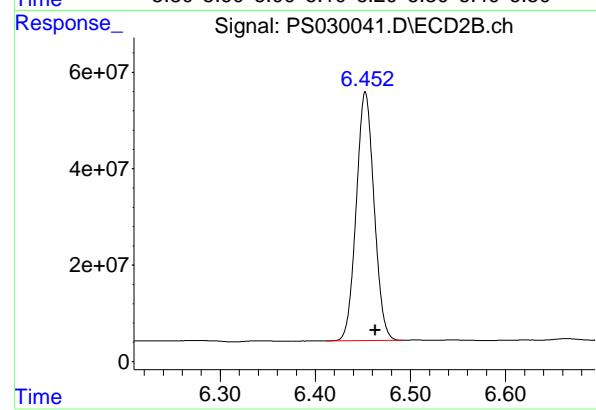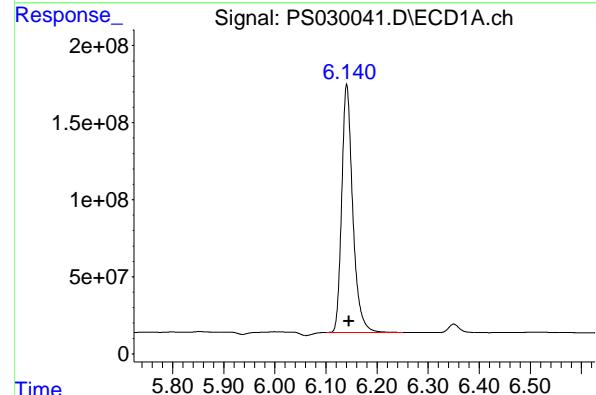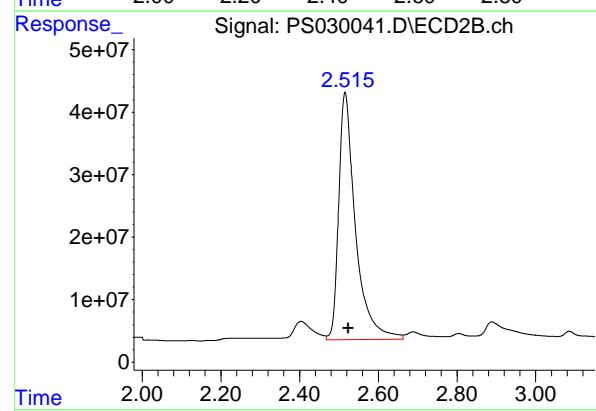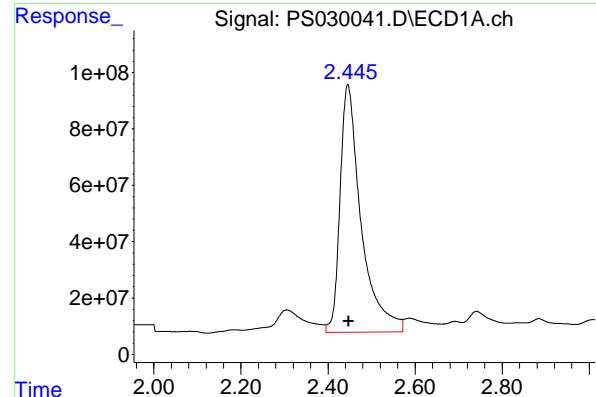

## #1 Dalapon

R.T.: 2.445 min  
Delta R.T.: -0.003 min  
Instrument: ECD\_S  
Response: 2952377655  
Conc: 720.93 ng/ml ClientSampleId : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/06/2025  
Supervised By :mohammad ahmed 05/07/2025

## #1 Dalapon





R.T.: 2.516 min  
Delta R.T.: -0.009 min  
Response: 1171602771  
Conc: 674.83 ng/ml

## #2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.141 min  
Delta R.T.: -0.005 min  
Response: 2409663155  
Conc: 674.26 ng/ml

## #2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.453 min  
Delta R.T.: -0.010 min  
Response: 672104770  
Conc: 687.52 ng/ml

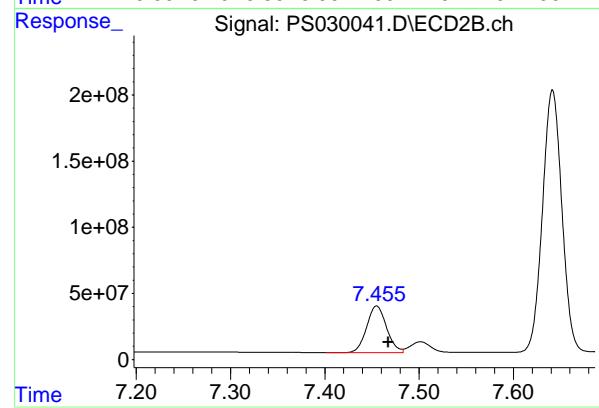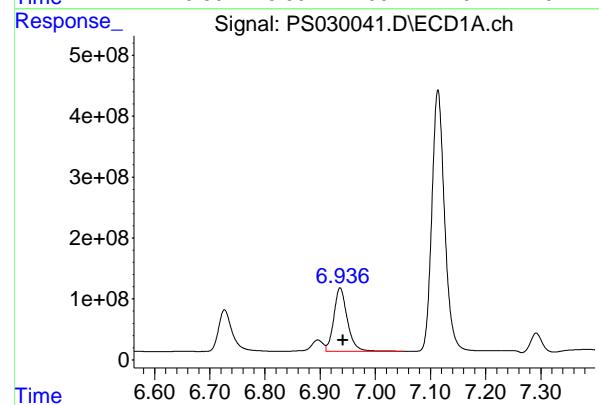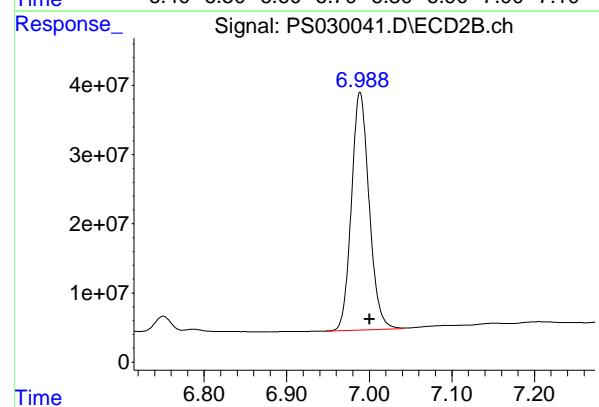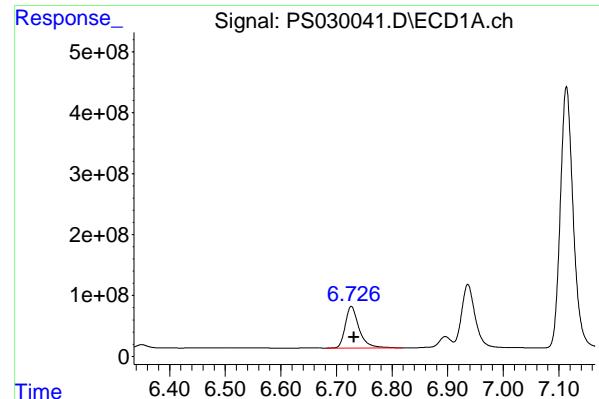

## #3 4-Nitrophenol

R.T.: 6.727 min  
 Delta R.T.: -0.005 min  
 Response: 1181094054 ECD\_S  
 Conc: 662.30 ng/ml ClientSampleId : HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/06/2025  
 Supervised By :mohammad ahmed 05/07/2025

## #3 4-Nitrophenol





R.T.: 6.988 min  
 Delta R.T.: -0.012 min  
 Response: 512755332  
 Conc: 669.46 ng/ml

## #4 2,4-DCAA

R.T.: 6.936 min  
 Delta R.T.: -0.005 min  
 Response: 1774908871  
 Conc: 721.19 ng/ml

## #4 2,4-DCAA

R.T.: 7.455 min  
 Delta R.T.: -0.012 min  
 Response: 519581780  
 Conc: 737.50 ng/ml

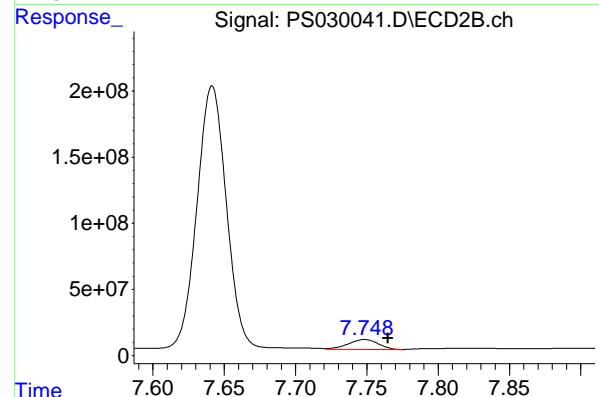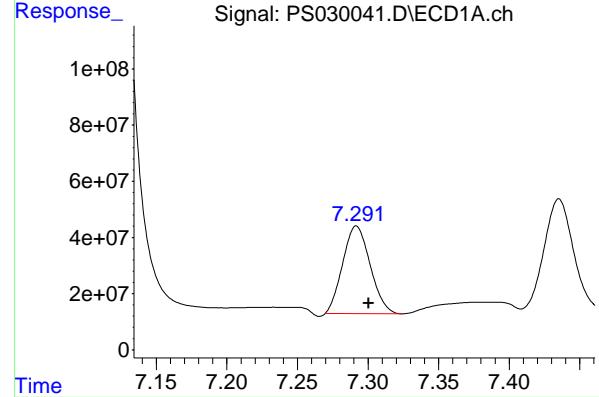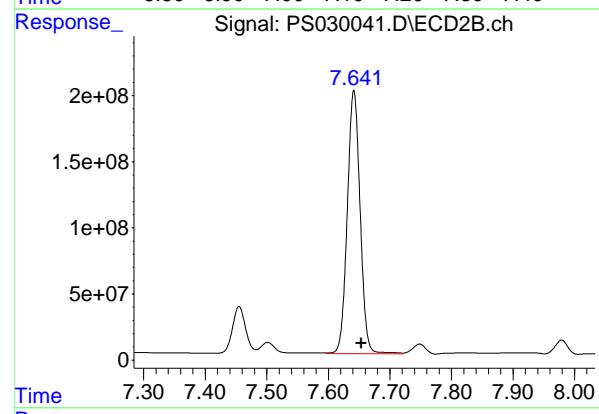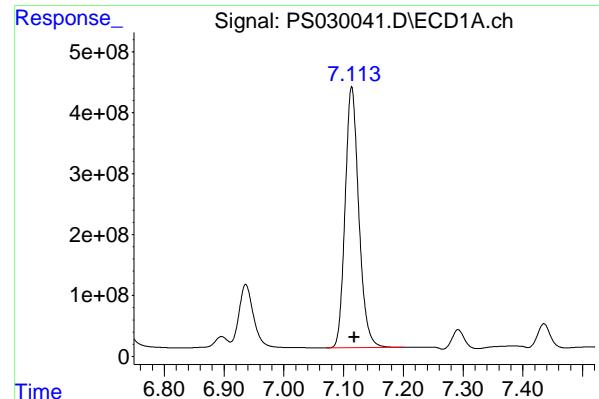

## #5 DICAMBA

R.T.: 7.114 min  
 Delta R.T.: -0.004 min  
 Response: 6817562025  
 Conc: 688.44 ng/ml

Instrument: ECD\_S  
 Client Sample Id: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/06/2025  
 Supervised By :mohammad ahmed 05/07/2025

## #5 DICAMBA





R.T.: 7.642 min  
 Delta R.T.: -0.012 min  
 Response: 2886665237  
 Conc: 730.79 ng/ml

## #6 MCPP

R.T.: 7.292 min  
 Delta R.T.: -0.009 min  
 Response: 422534047  
 Conc: 65.57 ug/ml

## #6 MCPP

R.T.: 7.748 min  
 Delta R.T.: -0.016 min  
 Response: 110573744  
 Conc: 63.22 ug/ml

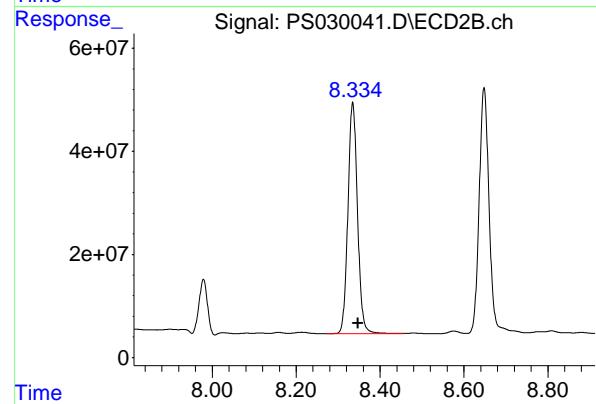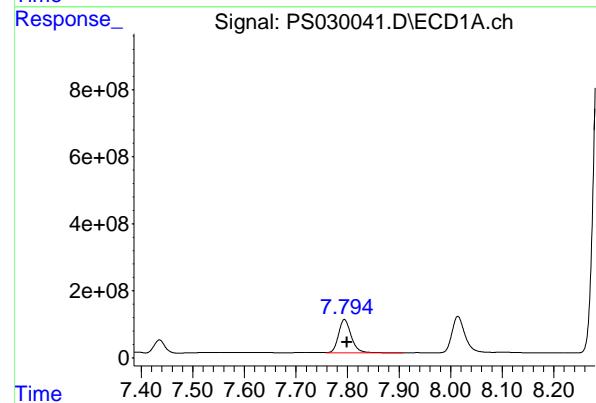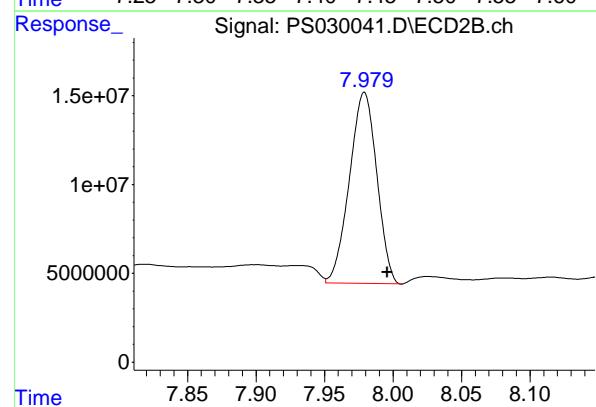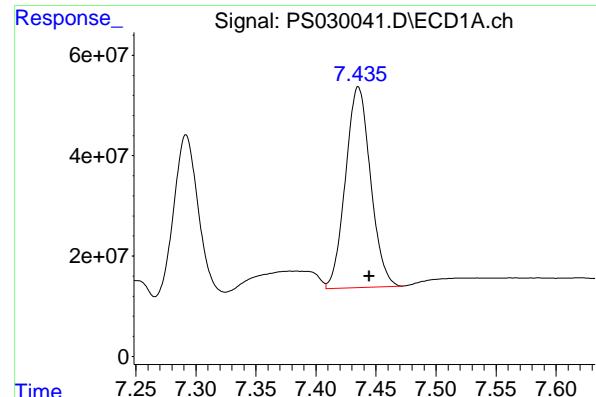

#7 MCPA

R.T.: 7.435 min  
 Delta R.T.: -0.009 min  
 Response: 580958132  
 Conc: 65.78 ug/ml

Instrument: ECD\_S  
 Client Sample ID: HSTDCCC750

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/06/2025  
 Supervised By :mohammad ahmed 05/07/2025

#7 MCPA


R.T.: 7.979 min  
 Delta R.T.: -0.017 min  
 Response: 149368796  
 Conc: 63.14 ug/ml

#8 DICHLORPROP

R.T.: 7.794 min  
 Delta R.T.: -0.005 min  
 Response: 1709939199  
 Conc: 674.77 ng/ml

#8 DICHLORPROP

R.T.: 8.335 min  
 Delta R.T.: -0.013 min  
 Response: 710958723  
 Conc: 708.15 ng/ml

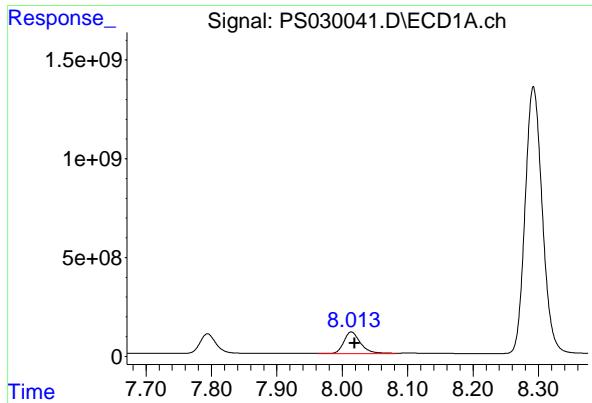


#9 2,4-D

R.T.: 8.014 min  
 Delta R.T.: -0.005 min  
 Response: 1935157953  
 Conc: 687.97 ng/ml  
 Instrument: ECD\_S  
 ClientSampleId : HSTDCCC750


Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/06/2025  
 Supervised By :mohammad ahmed 05/07/2025

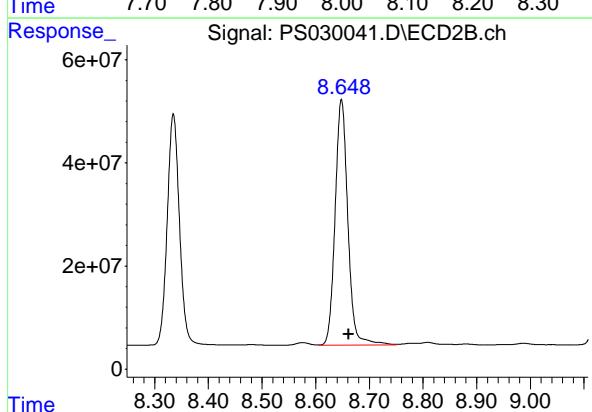


#9 2,4-D

R.T.: 8.648 min  
 Delta R.T.: -0.013 min  
 Response: 785195057  
 Conc: 696.65 ng/ml

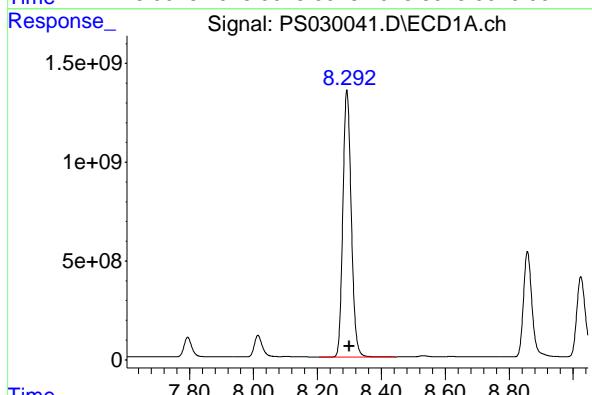


#10 Pentachlorophenol

R.T.: 8.292 min  
 Delta R.T.: -0.007 min  
 Response: 24554651193  
 Conc: 703.87 ng/ml

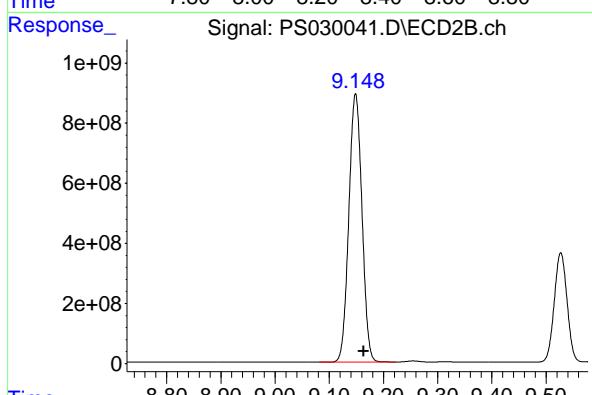

#10 Pentachlorophenol

R.T.: 9.149 min  
 Delta R.T.: -0.015 min  
 Response: 15042285138  
 Conc: 739.37 ng/ml

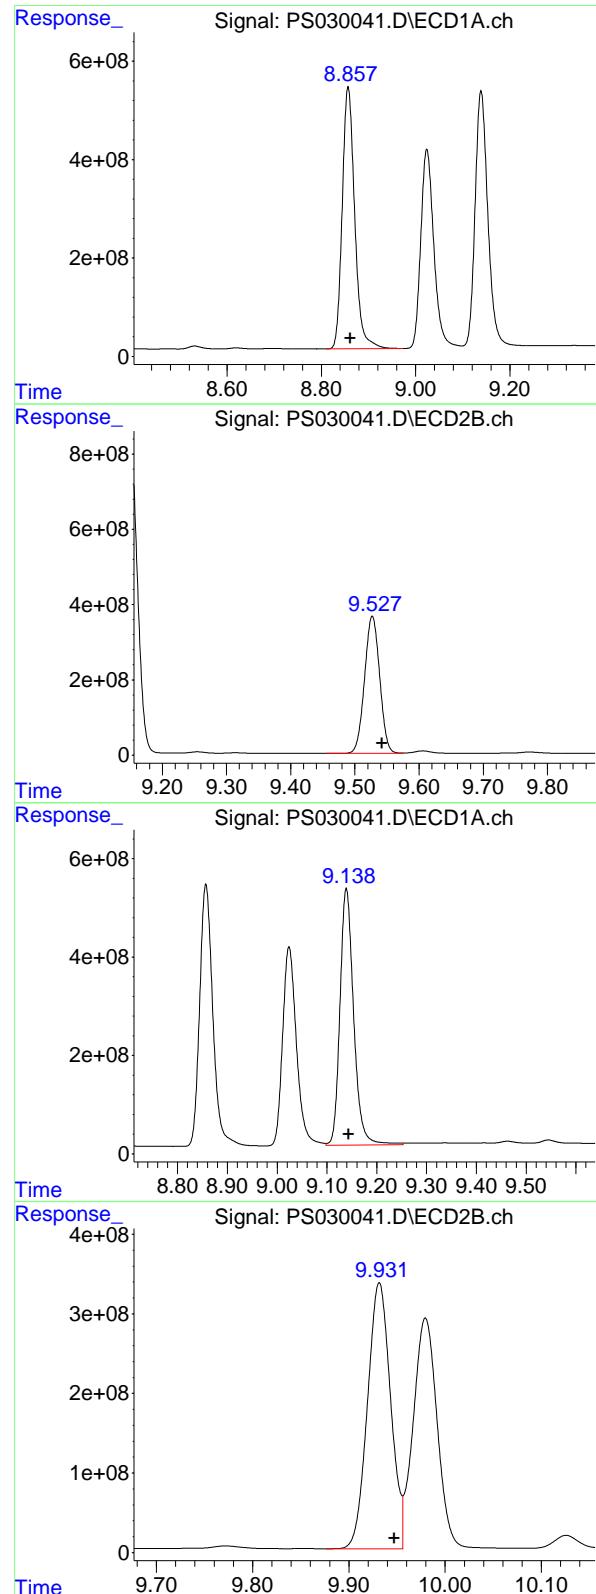

#11 2,4,5-TP (SILVEX)

R.T.: 8.857 min

Delta R.T.: -0.005 min

Instrument: ECD\_S

Response: 9759498519 ClientSampleId :

Conc: 704.00 ng/ml HSTDCCC750

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/06/2025  
Supervised By :mohammad ahmed 05/07/2025

#11 2,4,5-TP (SILVEX)

R.T.: 9.527 min

Delta R.T.: -0.015 min

Response: 5967877580

Conc: 729.41 ng/ml

#12 2,4,5-T

R.T.: 9.139 min

Delta R.T.: -0.005 min

Response: 9937744206

Conc: 707.16 ng/ml


#12 2,4,5-T

R.T.: 9.932 min

Delta R.T.: -0.015 min

Response: 5585441010

Conc: 719.53 ng/ml

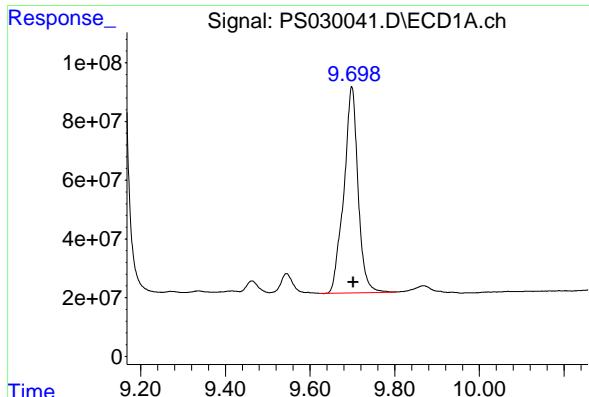


#13 2,4-DB

R.T.: 9.699 min  
Delta R.T.: -0.003 min  
Instrument: ECD\_S  
Response: 1639322217  
Conc: 717.32 ng/ml  
ClientSampleId: HSTDCCC750


Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/06/2025  
Supervised By :mohammad ahmed 05/07/2025

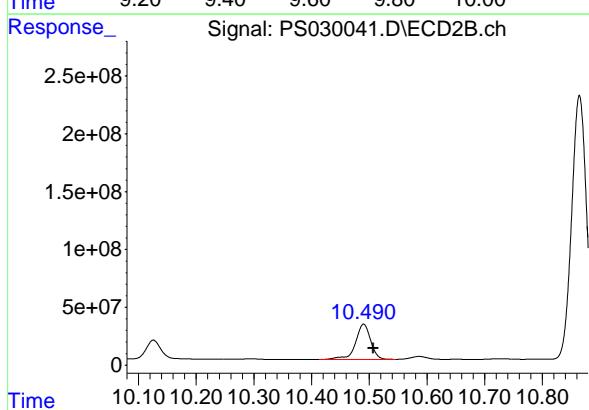


#13 2,4-DB

R.T.: 10.490 min  
Delta R.T.: -0.016 min  
Response: 557791820  
Conc: 693.04 ng/ml

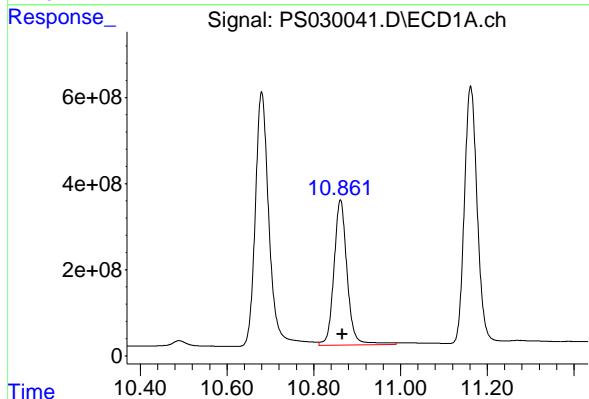


#14 DINOSEB

R.T.: 10.861 min  
Delta R.T.: -0.004 min  
Response: 7113634891  
Conc: 699.24 ng/ml

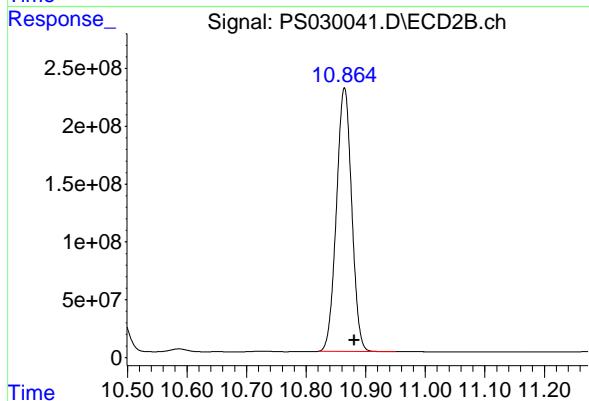

#14 DINOSEB

R.T.: 10.864 min  
Delta R.T.: -0.017 min  
Response: 4063249852  
Conc: 696.84 ng/ml

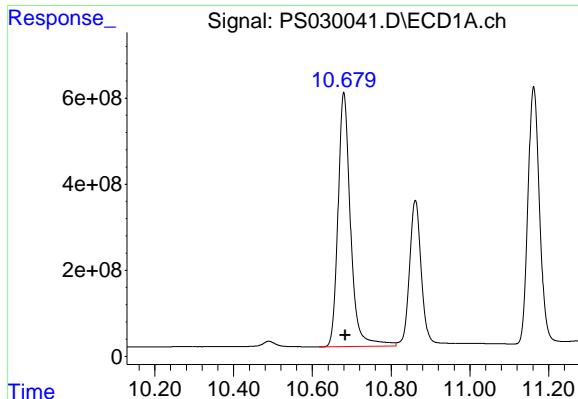


#15 Picloram

R.T.: 10.680 min  
Delta R.T.: -0.004 min  
Instrument: ECD\_S  
Response: 13035887532  
Conc: 711.15 ng/ml  
ClientSampleId: HSTDCCC750


Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/06/2025  
Supervised By :mohammad ahmed 05/07/2025

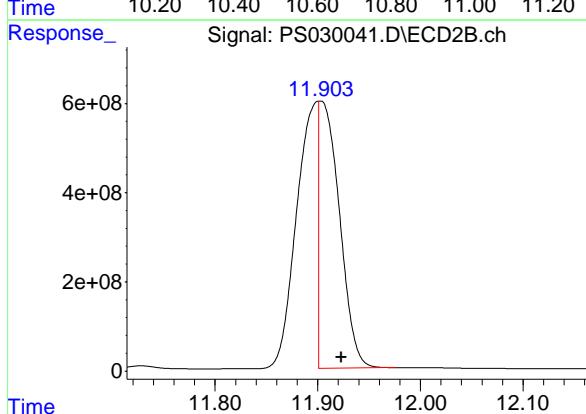


#15 Picloram

R.T.: 11.903 min  
Delta R.T.: -0.020 min  
Response: 7955463020  
Conc: 647.65 ng/ml

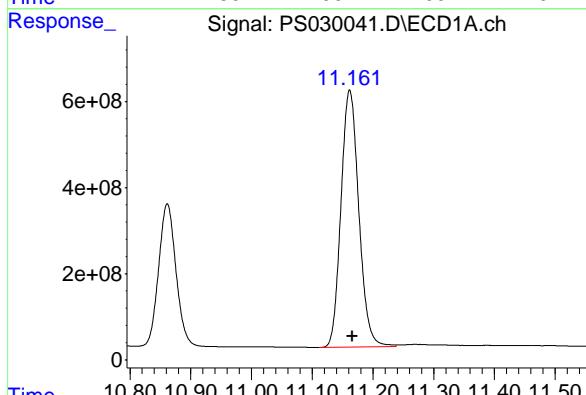

#16 DCPA

R.T.: 11.162 min  
Delta R.T.: -0.004 min  
Response: 12175434673  
Conc: 715.32 ng/ml

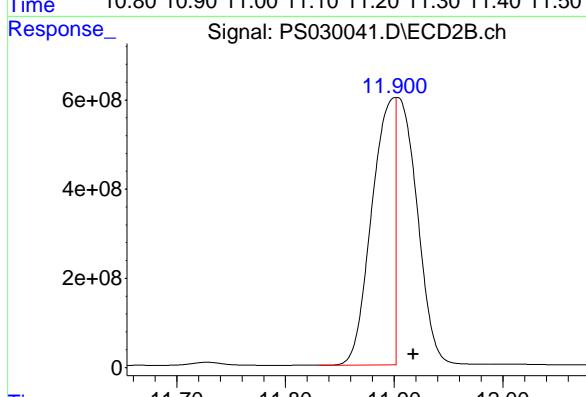

#16 DCPA

R.T.: 11.900 min  
Delta R.T.: -0.017 min  
Response: 8586896527  
Conc: 761.81 ng/ml

## Analytical Sequence

Client: Nobis Group	SDG No.: Q1883		
Project: Raymark Superfund Site	Instrument ID: ECD_S		
GC Column: RTX-CLP	ID: 0.32 (mm)	Inst. Calib. Date(s): 04/23/2025	04/23/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES, AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCAA RT #	RT #
I.BLK	LBLK	04/23/2025	10:37	PS029918.D	6.94	0.00
HSTDICC200	HSTDICC200	04/23/2025	11:01	PS029919.D	6.94	0.00
HSTDICC500	HSTDICC500	04/23/2025	11:25	PS029920.D	6.94	0.00
HSTDICC750	HSTDICC750	04/23/2025	11:49	PS029921.D	6.94	0.00
HSTDICC1000	HSTDICC1000	04/23/2025	12:13	PS029922.D	6.94	0.00
HSTDICC1500	HSTDICC1500	04/23/2025	12:37	PS029923.D	6.94	0.00
I.BLK	LBLK	05/01/2025	00:58	PS029990.D	6.94	0.00
HSTDCCC750	HSTDCCC750	05/01/2025	01:22	PS029991.D	6.94	0.00
WC-5MS	Q1906-05MS	05/01/2025	04:34	PS029999.D	6.92	0.00
WC-5MSD	Q1906-05MSD	05/01/2025	04:58	PS030000.D	6.92	0.00
I.BLK	LBLK	05/01/2025	06:10	PS030001.D	6.94	0.00
HSTDCCC750	HSTDCCC750	05/01/2025	06:59	PS030002.D	6.94	0.00
PB167796BL	PB167796BL	05/01/2025	11:24	PS030011.D	6.94	0.00
I.BLK	LBLK	05/01/2025	11:48	PS030012.D	6.94	0.00
HSTDCCC750	HSTDCCC750	05/01/2025	12:12	PS030013.D	6.94	0.00
I.BLK	LBLK	05/01/2025	13:03	PS030015.D	6.94	0.00
HSTDCCC750	HSTDCCC750	05/01/2025	13:27	PS030016.D	6.94	0.00
OU4-PCS-TC-27-042325	Q1883-01	05/01/2025	13:51	PS030017.D	6.94	0.00
OU4-PCS-TC-28-042325	Q1883-03	05/01/2025	14:15	PS030018.D	6.94	0.00
OU4-PCS-TC-29-042325	Q1883-05	05/01/2025	14:39	PS030019.D	6.94	0.00
OU4-PCS-TC-30-042325	Q1883-07	05/01/2025	15:04	PS030020.D	6.94	0.00
OU4-PCS-TC-31-042325	Q1883-09	05/01/2025	15:28	PS030021.D	6.94	0.00
OU4-PCS-TC-32-042325	Q1883-11	05/01/2025	15:52	PS030022.D	6.94	0.00
OU4-VSL-18-042325	Q1883-13	05/01/2025	16:16	PS030023.D	6.94	0.00
OU4-VSL-19-042325	Q1883-15	05/01/2025	16:40	PS030024.D	6.94	0.00
I.BLK	LBLK	05/01/2025	17:04	PS030025.D	6.94	0.00
HSTDCCC750	HSTDCCC750	05/01/2025	17:28	PS030026.D	6.94	0.00
I.BLK	LBLK	05/05/2025	08:38	PS030028.D	6.94	0.00
HSTDCCC750	HSTDCCC750	05/05/2025	09:55	PS030029.D	6.94	0.00
PB167796BS	PB167796BS	05/05/2025	13:47	PS030038.D	6.94	0.00
I.BLK	LBLK	05/05/2025	14:35	PS030040.D	6.94	0.00
HSTDCCC750	HSTDCCC750	05/05/2025	16:41	PS030041.D	6.94	0.00

## Analytical Sequence

Client: Nobis Group	SDG No.: Q1883		
Project: Raymark Superfund Site	Instrument ID: ECD_S		
GC Column: RTX-CLP2	ID: 0.32 (mm)	Inst. Calib. Date(s): 04/23/2025	04/23/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES, AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCAA RT #	RT #
I.BLK	LBLK	04/23/2025	10:37	PS029918.D	7.47	0.00
HSTDICC200	HSTDICC200	04/23/2025	11:01	PS029919.D	7.47	0.00
HSTDICC500	HSTDICC500	04/23/2025	11:25	PS029920.D	7.47	0.00
HSTDICC750	HSTDICC750	04/23/2025	11:49	PS029921.D	7.47	0.00
HSTDICC1000	HSTDICC1000	04/23/2025	12:13	PS029922.D	7.47	0.00
HSTDICC1500	HSTDICC1500	04/23/2025	12:37	PS029923.D	7.47	0.00
I.BLK	LBLK	05/01/2025	00:58	PS029990.D	7.46	0.00
HSTDCCC750	HSTDCCC750	05/01/2025	01:22	PS029991.D	7.46	0.00
WC-5MS	Q1906-05MS	05/01/2025	04:34	PS029999.D	7.46	0.00
WC-5MSD	Q1906-05MSD	05/01/2025	04:58	PS030000.D	7.46	0.00
I.BLK	LBLK	05/01/2025	06:10	PS030001.D	7.46	0.00
HSTDCCC750	HSTDCCC750	05/01/2025	06:59	PS030002.D	7.46	0.00
PB167796BL	PB167796BL	05/01/2025	11:24	PS030011.D	7.46	0.00
I.BLK	LBLK	05/01/2025	11:48	PS030012.D	7.46	0.00
HSTDCCC750	HSTDCCC750	05/01/2025	12:12	PS030013.D	7.46	0.00
I.BLK	LBLK	05/01/2025	13:03	PS030015.D	7.46	0.00
HSTDCCC750	HSTDCCC750	05/01/2025	13:27	PS030016.D	7.46	0.00
OU4-PCS-TC-27-042325	Q1883-01	05/01/2025	13:51	PS030017.D	7.46	0.00
OU4-PCS-TC-28-042325	Q1883-03	05/01/2025	14:15	PS030018.D	7.46	0.00
OU4-PCS-TC-29-042325	Q1883-05	05/01/2025	14:39	PS030019.D	7.46	0.00
OU4-PCS-TC-30-042325	Q1883-07	05/01/2025	15:04	PS030020.D	7.46	0.00
OU4-PCS-TC-31-042325	Q1883-09	05/01/2025	15:28	PS030021.D	7.46	0.00
OU4-PCS-TC-32-042325	Q1883-11	05/01/2025	15:52	PS030022.D	7.46	0.00
OU4-VSL-18-042325	Q1883-13	05/01/2025	16:16	PS030023.D	7.46	0.00
OU4-VSL-19-042325	Q1883-15	05/01/2025	16:40	PS030024.D	7.46	0.00
I.BLK	LBLK	05/01/2025	17:04	PS030025.D	7.46	0.00
HSTDCCC750	HSTDCCC750	05/01/2025	17:28	PS030026.D	7.46	0.00
I.BLK	LBLK	05/05/2025	08:38	PS030028.D	7.46	0.00
HSTDCCC750	HSTDCCC750	05/05/2025	09:55	PS030029.D	7.46	0.00
PB167796BS	PB167796BS	05/05/2025	13:47	PS030038.D	7.46	0.00
I.BLK	LBLK	05/05/2025	14:35	PS030040.D	7.46	0.00
HSTDCCC750	HSTDCCC750	05/05/2025	16:41	PS030041.D	7.46	0.00

### COMPOUND DETECTION SUMMARY

**CLIENT SAMPLE NO.**

**PB167796BS**

<b>Contract:</b>	<b>NOBI03</b>						
<b>Lab Code:</b>	<b>CHEM</b>	<b>Case No.:</b>	<b>Q1883</b>	<b>SAS No.:</b>	<b>Q1883</b>	<b>SDG NO.:</b>	<b>Q1883</b>
<b>Lab Sample ID:</b>	<b>PB167796BS</b>			<b>Date(s) Analyzed:</b>	<b>05/05/2025</b>	<b>05/05/2025</b>	
<b>Instrument ID (1):</b>	<b>ECD_S</b>			<b>Instrument ID (2):</b>	<b>ECD_S</b>		
<b>GC Column: (1):</b>	<b>RTX-CLP</b>	<b>ID:</b>	<b>0.32 (mm)</b>	<b>GC Column:(2):</b>	<b>RTX-CLP2</b>	<b>ID:</b>	<b>0.32 (mm)</b>

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	%RPD
			FROM	TO		
2,4,5-T	1	9.14	9.09	9.19	171	1.2
	2	9.94	9.89	9.99	173	
2,4,5-TP(Silvex)	1	8.86	8.81	8.91	170	2.9
	2	9.53	9.48	9.58	175	
2,4-D	1	8.01	7.96	8.06	167	1.8
	2	8.65	8.60	8.70	170	
2,4-DB	1	9.70	9.65	9.75	172	2.9
	2	10.50	10.45	10.55	167	
Dalapon	1	2.45	2.40	2.50	165	3.1
	2	2.52	2.47	2.57	160	
DICHLOPROP	1	7.79	7.74	7.84	164	4.8
	2	8.34	8.29	8.39	172	
Dinoseb	1	10.86	10.81	10.91	168	1.2
	2	10.87	10.82	10.92	170	
DICAMBA	1	7.11	7.06	7.16	166	3.6
	2	7.65	7.60	7.70	172	

### COMPOUND DETECTION SUMMARY

**CLIENT SAMPLE NO.**

WC-5MS

<b>Contract:</b>	<u>NOBI03</u>						
<b>Lab Code:</b>	<u>CHEM</u>	<b>Case No.:</b>	<u>Q1883</u>	<b>SAS No.:</b>	<u>Q1883</u>	<b>SDG NO.:</b>	<u>Q1883</u>
<b>Lab Sample ID:</b>	<u>Q1906-05MS</u>			<b>Date(s) Analyzed:</b>	<u>05/01/2025</u>	<b>05/01/2025</b>	
<b>Instrument ID (1):</b>	<u>ECD_S</u>			<b>Instrument ID (2):</b>	<u>ECD_S</u>		
<b>GC Column: (1):</b>	<u>RTX-CLP</u>	<b>ID:</b>	<u>0.32 (mm)</u>	<b>GC Column:(2):</b>	<u>RTX-CLP2</u>	<b>ID:</b>	<u>0.32 (mm)</u>

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	%RPD
			FROM	TO		
Dalapon	1	2.44	2.39	2.49	270	36.6
	2	2.52	2.47	2.57	391	
DICHLORPROP	1	7.80	7.75	7.85	102	27.8
	2	8.34	8.29	8.39	135	
2,4-D	1	8.02	7.97	8.07	165	3.1
	2	8.65	8.60	8.70	160	
2,4,5-TP(Silvex)	1	8.86	8.81	8.91	80.7	18.1
	2	9.53	9.48	9.58	96.8	
2,4,5-T	1	9.14	9.09	9.19	103	7.5
	2	9.94	9.89	9.99	111	
2,4-DB	1	9.70	9.65	9.75	81.8	1
	2	10.49	10.44	10.54	81.0	
DICAMBA	1	7.12	7.07	7.17	125	4.7
	2	7.65	7.60	7.70	131	

### COMPOUND DETECTION SUMMARY

**CLIENT SAMPLE NO.**

**WC-5MSD**

<b>Contract:</b>	<b>NOBI03</b>						
<b>Lab Code:</b>	<b>CHEM</b>	<b>Case No.:</b>	<b>Q1883</b>	<b>SAS No.:</b>	<b>Q1883</b>	<b>SDG NO.:</b>	<b>Q1883</b>
<b>Lab Sample ID:</b>	<b>Q1906-05MSD</b>			<b>Date(s) Analyzed:</b>	<b>05/01/2025</b>	<b>05/01/2025</b>	
<b>Instrument ID (1):</b>	<b>ECD_S</b>			<b>Instrument ID (2):</b>	<b>ECD_S</b>		
<b>GC Column: (1):</b>	<b>RTX-CLP</b>	<b>ID:</b>	<b>0.32 (mm)</b>	<b>GC Column:(2):</b>	<b>RTX-CLP2</b>	<b>ID:</b>	<b>0.32 (mm)</b>

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	%RPD
			FROM	TO		
2,4,5-T	1	9.14	9.09	9.19	104	8.3
	2	9.94	9.89	9.99	113	
Dalapon	1	2.44	2.39	2.49	261	38.1
	2	2.52	2.47	2.57	384	
DICHLORPROP	1	7.80	7.75	7.85	100	31.2
	2	8.34	8.29	8.39	137	
2,4-D	1	8.02	7.97	8.07	168	3
	2	8.65	8.60	8.70	163	
2,4,5-TP(Silvex)	1	8.86	8.81	8.91	82.9	18.7
	2	9.53	9.48	9.58	100	
2,4-DB	1	9.70	9.65	9.75	72.2	15.7
	2	10.49	10.44	10.54	84.5	
DICAMBA	1	7.11	7.06	7.16	126	5.4
	2	7.65	7.60	7.70	133	



# QC SAMPLE

# DATA



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	
Project:	Raymark Superfund Site			Date Received:	
Client Sample ID:	PB167796BL			SDG No.:	Q1883
Lab Sample ID:	PB167796BL			Matrix:	SOIL
Analytical Method:	SW8151A			% Solid:	100 Decanted:
Sample Wt/Vol:	30.01	Units:	g	Final Vol:	10000 uL
Soil Aliquot Vol:			uL	Test:	Herbicide Group1
Extraction Type:				Injection Volume :	
GPC Factor :	1.0	PH :			
Prep Method :	8151A				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PS030011.D	1	04/30/25 08:50	05/01/25 11:24	PB167796

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
1918-00-9	DICAMBA	0.033	U	0.0077	0.033	0.067	mg/Kg
75-99-0	DALAPON	0.050	U	0.018	0.050	0.067	mg/Kg
120-36-5	DICHLORPROP	0.033	U	0.013	0.033	0.067	mg/Kg
94-75-7	2,4-D	0.033	U	0.0090	0.033	0.067	mg/Kg
93-72-1	2,4,5-TP (Silvex)	0.033	U	0.0091	0.033	0.067	mg/Kg
93-76-5	2,4,5-T	0.033	U	0.0087	0.033	0.067	mg/Kg
94-82-6	2,4-DB	0.033	U	0.024	0.033	0.067	mg/Kg
88-85-7	DINOSEB	0.033	U	0.011	0.033	0.067	mg/Kg
<b>SURROGATES</b>							
19719-28-9	2,4-DCAA	433		27 - 122		87%	SPK: 500

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
Data File : PS030011.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 01 May 2025 11:24  
Operator : AR\AJ  
Sample : PB167796BL  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
PB167796BL

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: May 02 04:56:09 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
Quant Title : 8080.M  
QLast Update : Wed Apr 23 12:57:40 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

---

System Monitoring Compounds

4) S	2,4-DCAA	6.937	7.461	1065.7E6	291.0E6	433.015	413.084
------	----------	-------	-------	----------	---------	---------	---------

Target Compounds

---



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS030011.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 11:24  
 Operator : AR\AJ  
 Sample : PB167796BL  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 PB167796BL

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 04:56:09 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

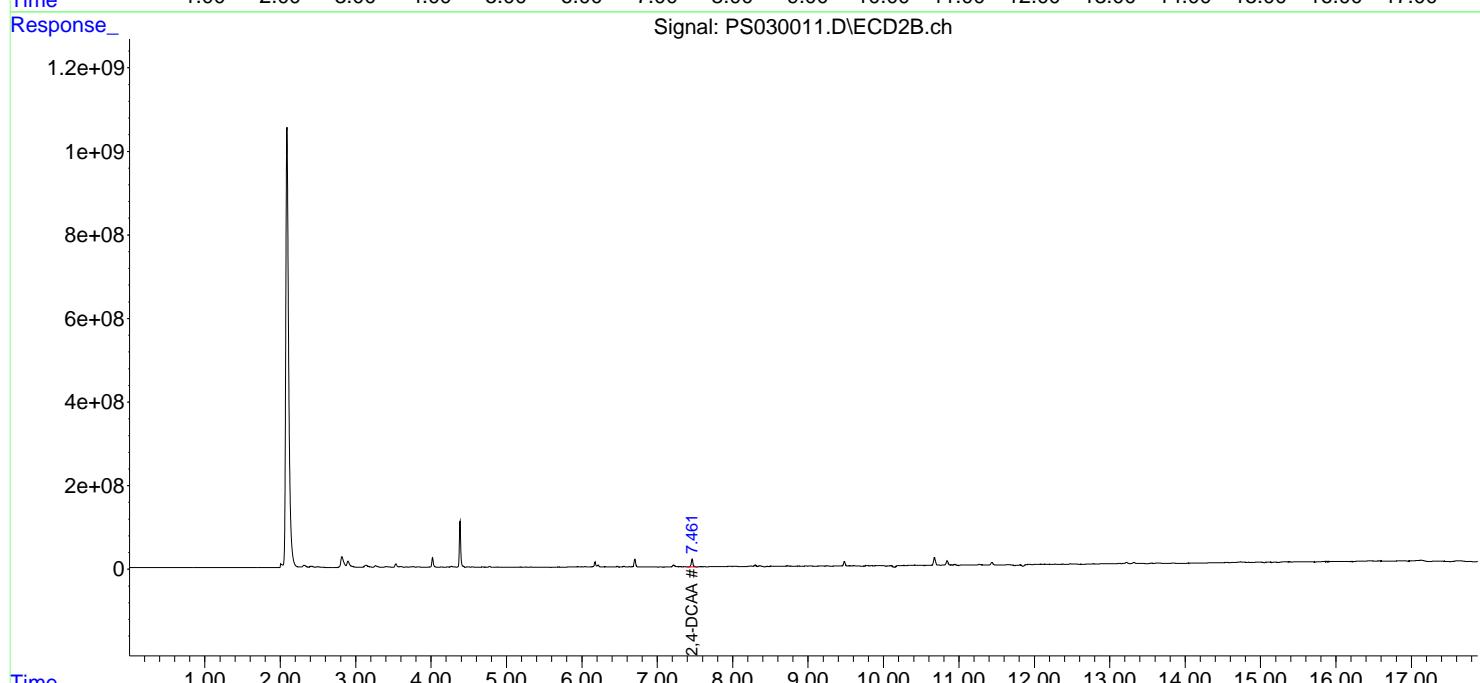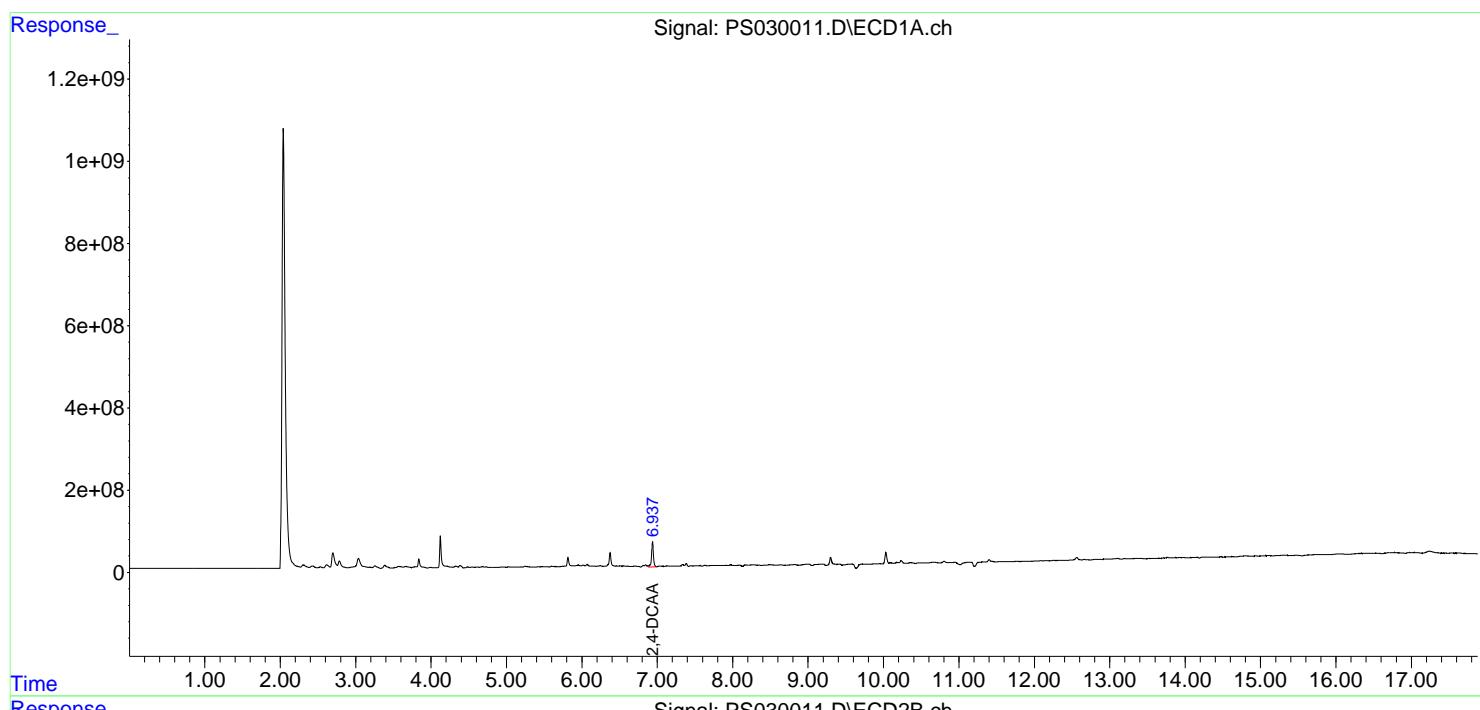

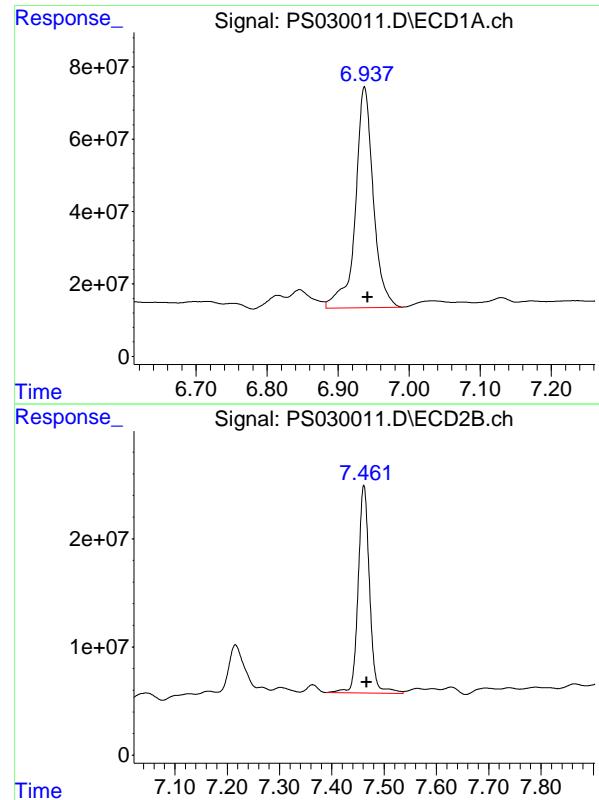

#4 2,4-DCAA

R.T.: 6.937 min  
Delta R.T.: -0.004 min  
Instrument: ECD\_S  
Response: 1065684673  
Conc: 433.02 ng/ml  
ClientSampleId: PB167796BL

#4 2,4-DCAA

R.T.: 7.461 min  
Delta R.T.: -0.006 min  
Instrument: ECD\_S  
Response: 291024810  
Conc: 413.08 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group		Date Collected:	04/23/25	
Project:	Raymark Superfund Site		Date Received:	04/23/25	
Client Sample ID:	PIBLK-PS029918.D		SDG No.:	Q1883	
Lab Sample ID:	I.BLK-PS029918.D		Matrix:	WATER	
Analytical Method:	SW8151A		% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units: mL	Final Vol:	10000	uL
Soil Aliquot Vol:	uL		Test:	Herbicide Group1	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	SW3510C				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PS029918.D	1		04/23/25	PS042325

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
<b>TARGETS</b>							
1918-00-9	DICAMBA	0.0015	U	0.00065	0.0015	0.0020	mg/L
75-99-0	DALAPON	0.0015	U	0.00098	0.0015	0.0020	mg/L
120-36-5	DICHLORPROP	0.0015	U	0.00076	0.0015	0.0020	mg/L
94-75-7	2,4-D	0.0015	U	0.00092	0.0015	0.0020	mg/L
93-72-1	2,4,5-TP (Silvex)	0.0015	U	0.00078	0.0015	0.0020	mg/L
93-76-5	2,4,5-T	0.0015	U	0.00071	0.0015	0.0020	mg/L
94-82-6	2,4-DB	0.0015	U	0.00065	0.0015	0.0020	mg/L
88-85-7	DINOSEB	0.0015	U	0.00089	0.0015	0.0020	mg/L
<b>SURROGATES</b>							
19719-28-9	2,4-DCAA	433		32 - 138		87%	SPK: 500

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029918.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 10:37  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

**Instrument :**  
 ECD\_S  
**ClientSampleId :**  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 12:58:18 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	6.942	7.467	1065.1E6	304.8E6	432.760	432.665
------	----------	-------	-------	----------	---------	---------	---------

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029918.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 10:37  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 12:58:18 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

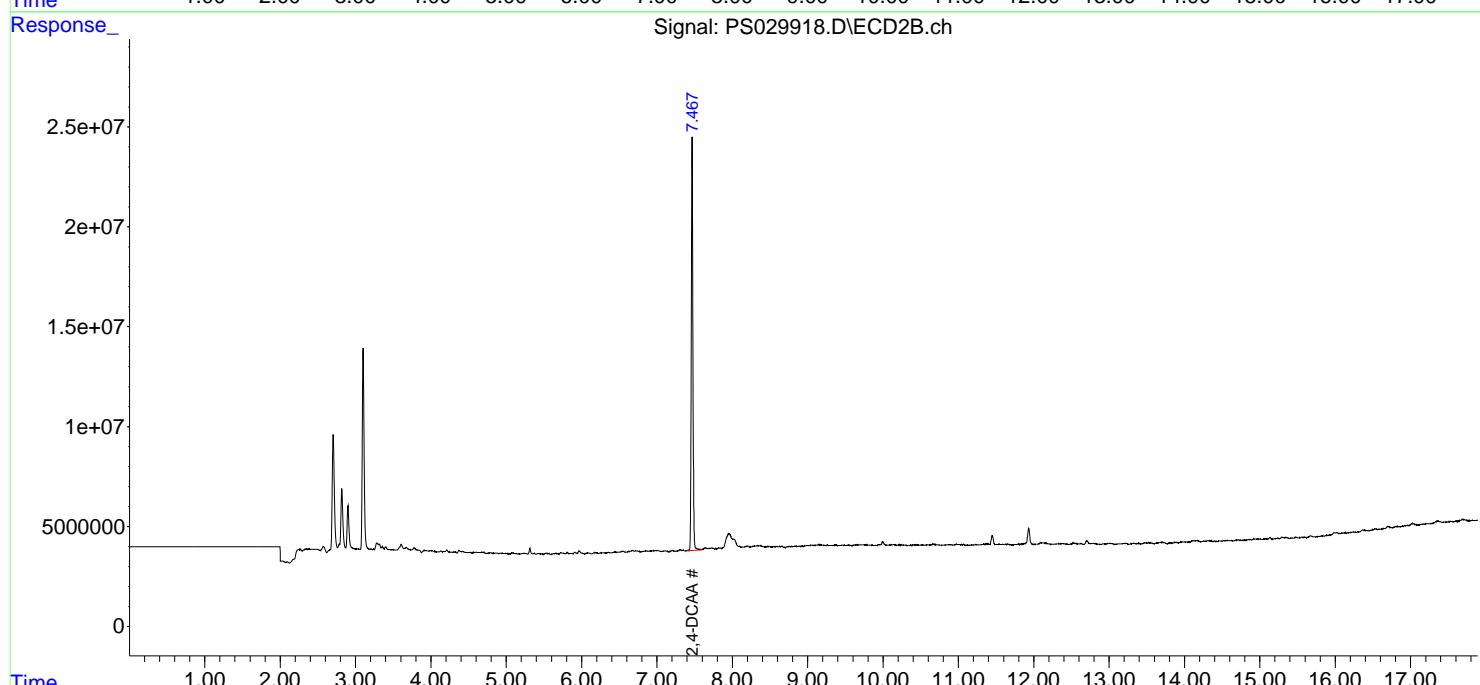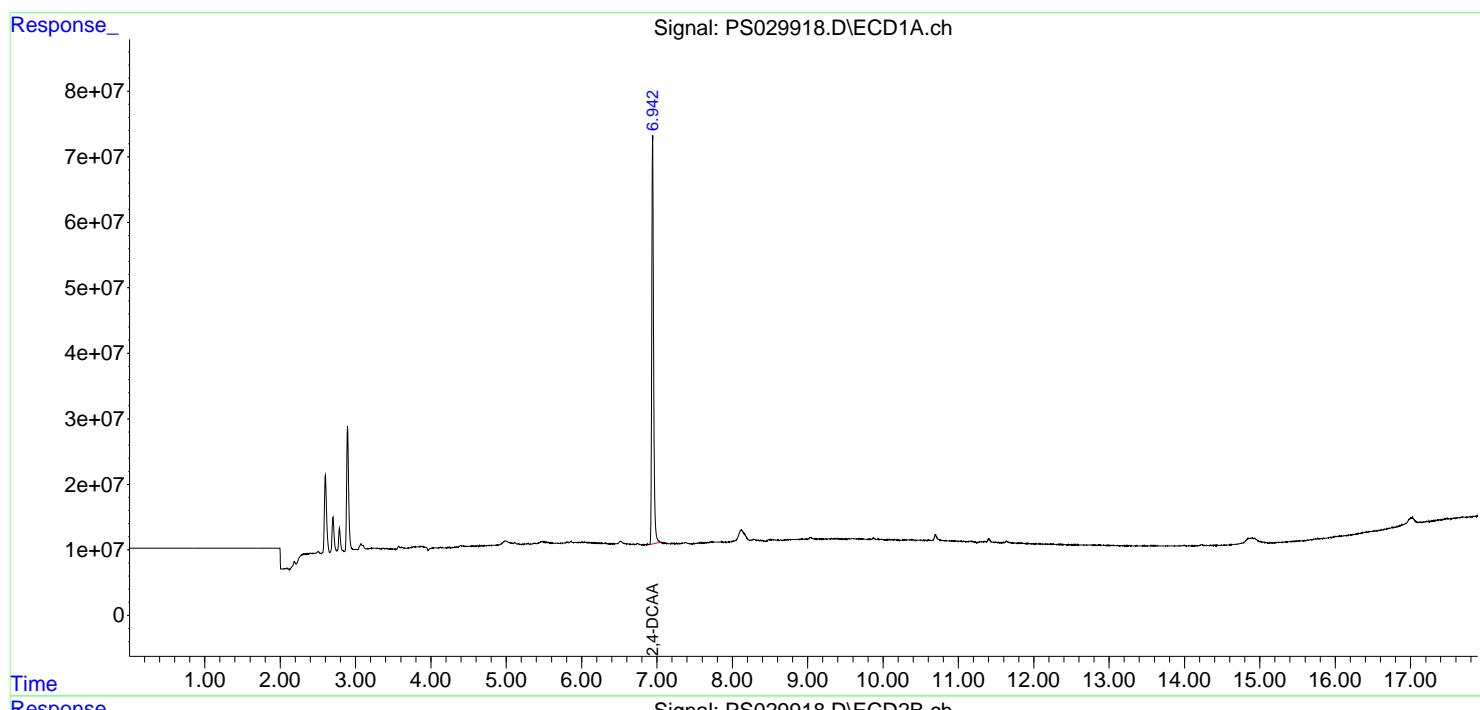

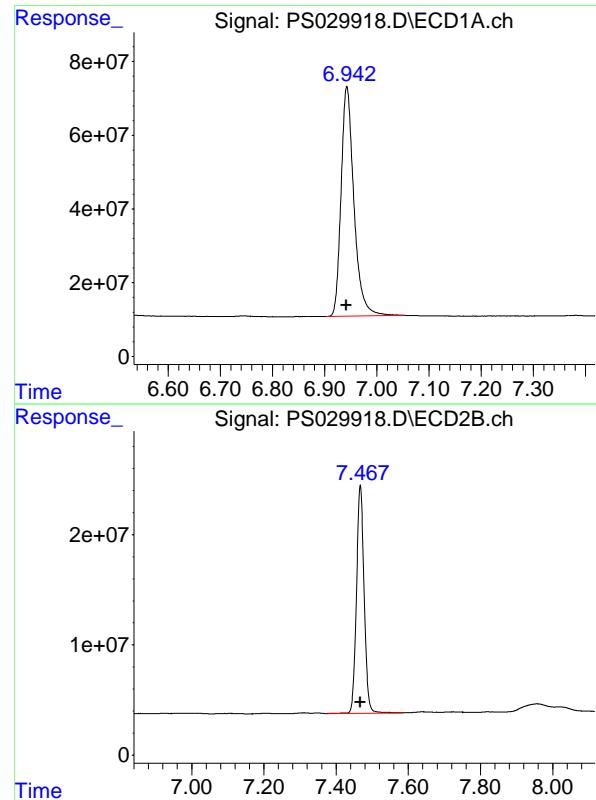

#4 2,4-DCAA

R.T.: 6.942 min  
Delta R.T.: 0.001 min  
Instrument: ECD\_S  
Response: 1065056072  
Conc: 432.76 ng/ml  
ClientSampleId: I.BLK

#4 2,4-DCAA

R.T.: 7.467 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_S  
Response: 304820126  
Conc: 432.67 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group		Date Collected:	05/01/25	
Project:	Raymark Superfund Site		Date Received:	05/01/25	
Client Sample ID:	PIBLK-PS029990.D		SDG No.:	Q1883	
Lab Sample ID:	I.BLK-PS029990.D		Matrix:	WATER	
Analytical Method:	SW8151A		% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units: mL	Final Vol:	10000	uL
Soil Aliquot Vol:	uL		Test:	Herbicide Group1	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	SW3510C				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PS029990.D	1		05/01/25	ps043025

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
<b>TARGETS</b>							
1918-00-9	DICAMBA	0.0015	U	0.00065	0.0015	0.0020	mg/L
75-99-0	DALAPON	0.0015	U	0.00098	0.0015	0.0020	mg/L
120-36-5	DICHLORPROP	0.0015	U	0.00076	0.0015	0.0020	mg/L
94-75-7	2,4-D	0.0015	U	0.00092	0.0015	0.0020	mg/L
93-72-1	2,4,5-TP (Silvex)	0.0015	U	0.00078	0.0015	0.0020	mg/L
93-76-5	2,4,5-T	0.0015	U	0.00071	0.0015	0.0020	mg/L
94-82-6	2,4-DB	0.0015	U	0.00065	0.0015	0.0020	mg/L
88-85-7	DINOSEB	0.0015	U	0.00089	0.0015	0.0020	mg/L
<b>SURROGATES</b>							
19719-28-9	2,4-DCAA	558		32 - 138		112%	SPK: 500

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS029990.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 00:58  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

**Instrument :**  
ECD\_S  
**ClientSampleId :**  
I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 01 01:46:12 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	6.939	7.463	1292.7E6	393.2E6	525.261	558.137
------	----------	-------	-------	----------	---------	---------	---------

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS029990.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 00:58  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 01 01:46:12 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

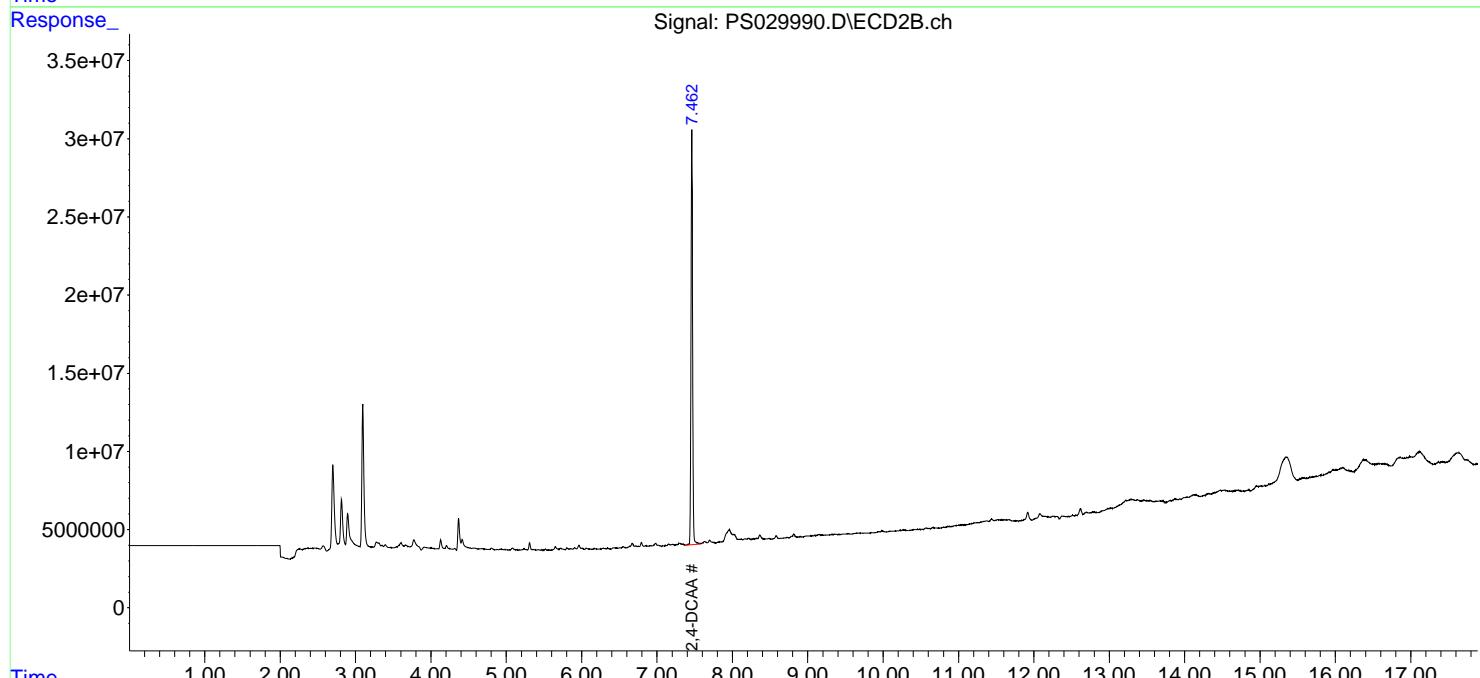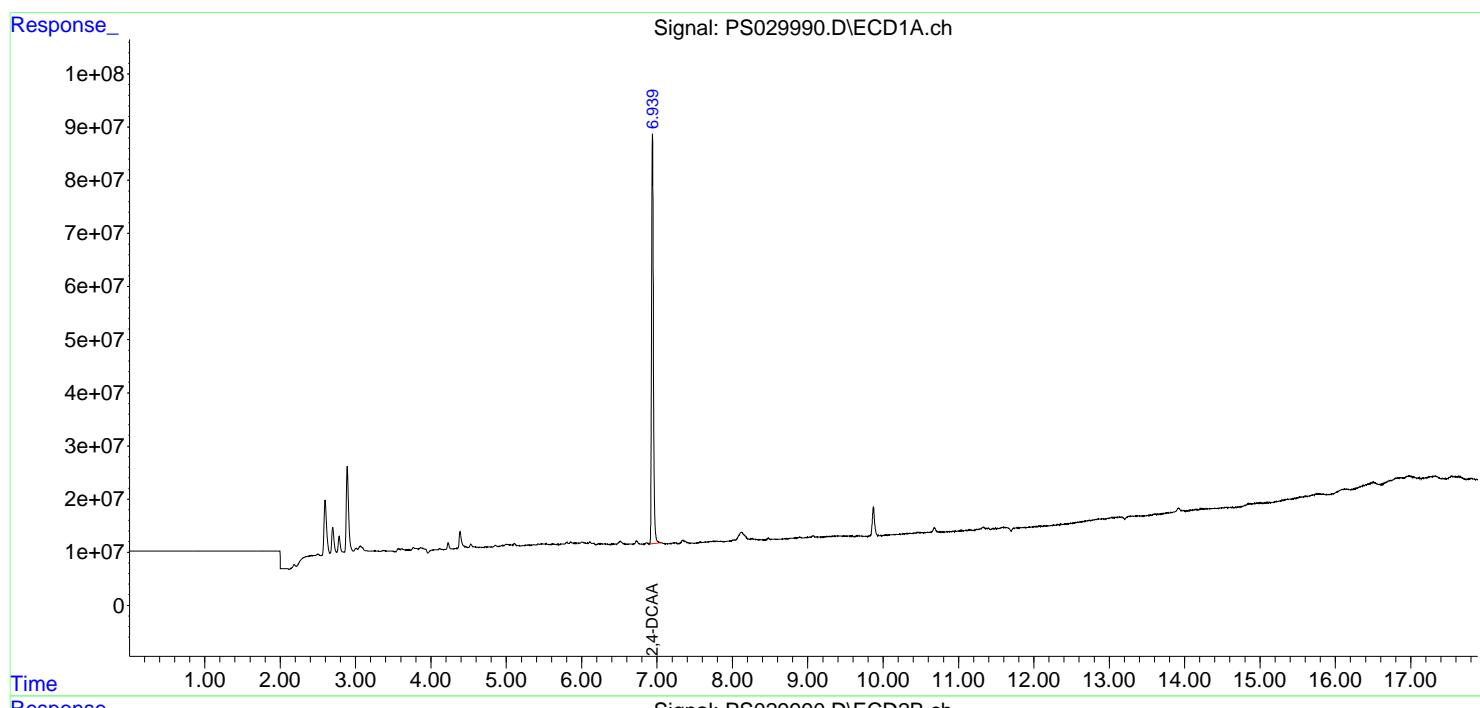

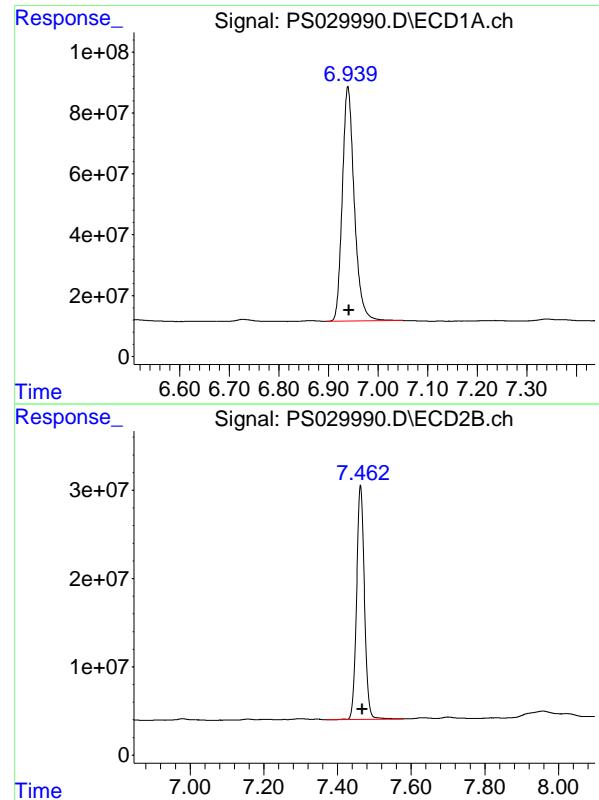

#4 2,4-DCAA

R.T.: 6.939 min  
Delta R.T.: -0.002 min  
Instrument: ECD\_S  
Response: 1292708429  
Conc: 525.26 ng/ml  
ClientSampleId: I.BLK

#4 2,4-DCAA

R.T.: 7.463 min  
Delta R.T.: -0.005 min  
Instrument: ECD\_S  
Response: 393217170  
Conc: 558.14 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group		Date Collected:	05/01/25	
Project:	Raymark Superfund Site		Date Received:	05/01/25	
Client Sample ID:	PIBLK-PS030001.D		SDG No.:	Q1883	
Lab Sample ID:	I.BLK-PS030001.D		Matrix:	WATER	
Analytical Method:	SW8151A		% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units: mL	Final Vol:	10000	uL
Soil Aliquot Vol:	uL		Test:	Herbicide Group1	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	SW3510C				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PS030001.D	1		05/01/25	ps043025

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
<b>TARGETS</b>							
1918-00-9	DICAMBA	0.0015	U	0.00065	0.0015	0.0020	mg/L
75-99-0	DALAPON	0.0015	U	0.00098	0.0015	0.0020	mg/L
120-36-5	DICHLORPROP	0.0015	U	0.00076	0.0015	0.0020	mg/L
94-75-7	2,4-D	0.0015	U	0.00092	0.0015	0.0020	mg/L
93-72-1	2,4,5-TP (Silvex)	0.0015	U	0.00078	0.0015	0.0020	mg/L
93-76-5	2,4,5-T	0.0015	U	0.00071	0.0015	0.0020	mg/L
94-82-6	2,4-DB	0.0015	U	0.00065	0.0015	0.0020	mg/L
88-85-7	DINOSEB	0.0015	U	0.00089	0.0015	0.0020	mg/L
<b>SURROGATES</b>							
19719-28-9	2,4-DCAA	565		32 - 138		113%	SPK: 500

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS030001.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 06:10  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

**Instrument :**  
ECD\_S  
**ClientSampleId :**  
I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 01 06:43:36 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	6.938	7.462	1273.6E6	398.3E6	517.514	565.310
------	----------	-------	-------	----------	---------	---------	---------

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS030001.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 06:10  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 01 06:43:36 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

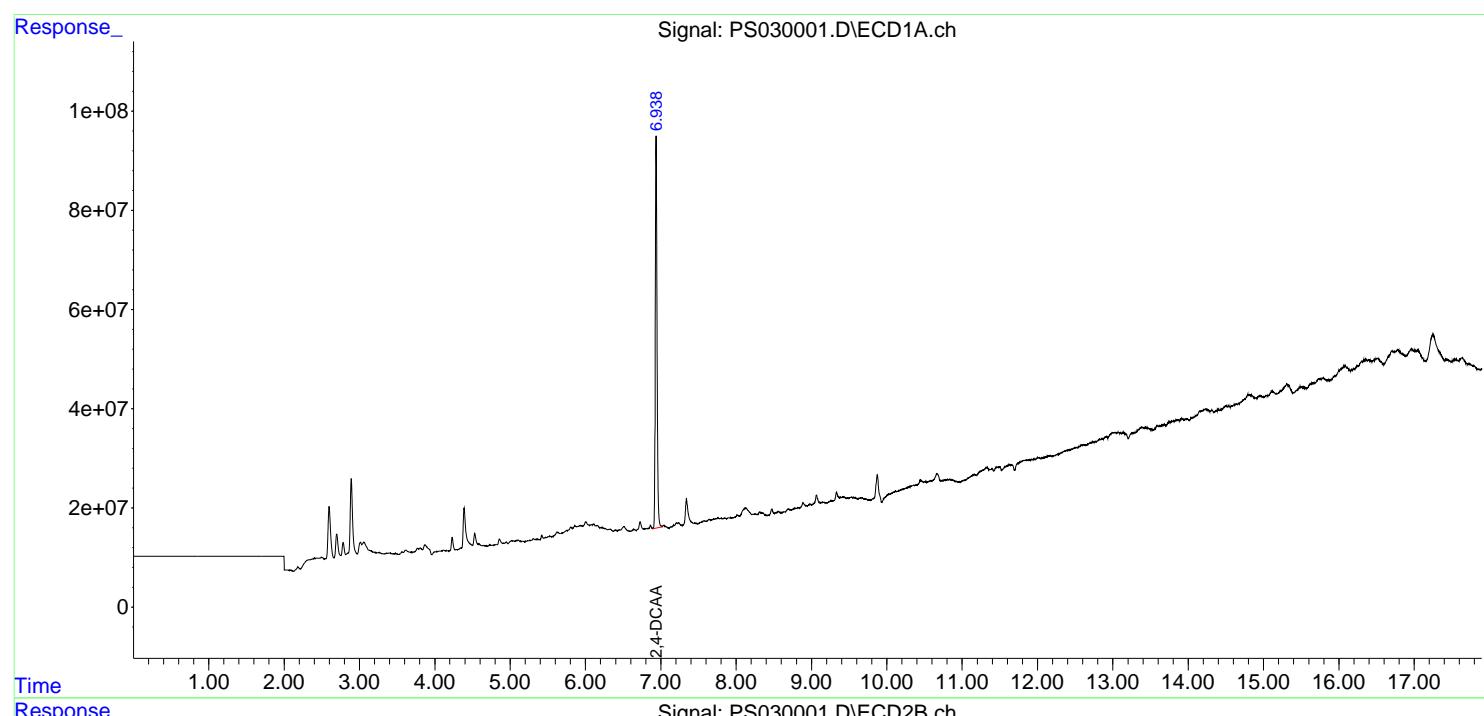

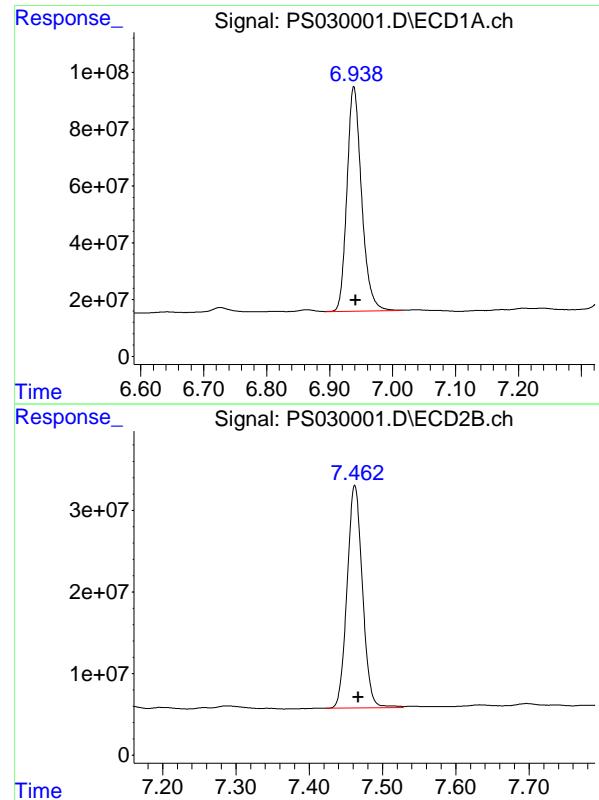

#4 2,4-DCAA

R.T.: 6.938 min  
Delta R.T.: -0.003 min  
Instrument: ECD\_S  
Response: 1273643413  
Conc: 517.51 ng/ml  
ClientSampleId: I.BLK

#4 2,4-DCAA

R.T.: 7.462 min  
Delta R.T.: -0.005 min  
Instrument: ECD\_S  
Response: 398270175  
Conc: 565.31 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group		Date Collected:	05/01/25	
Project:	Raymark Superfund Site		Date Received:	05/01/25	
Client Sample ID:	PIBLK-PS030012.D		SDG No.:	Q1883	
Lab Sample ID:	I.BLK-PS030012.D		Matrix:	WATER	
Analytical Method:	SW8151A		% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units: mL	Final Vol:	10000	uL
Soil Aliquot Vol:	uL		Test:	Herbicide Group1	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	SW3510C				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PS030012.D	1		05/01/25	ps043025

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
<b>TARGETS</b>							
1918-00-9	DICAMBA	0.0015	U	0.00065	0.0015	0.0020	mg/L
75-99-0	DALAPON	0.0015	U	0.00098	0.0015	0.0020	mg/L
120-36-5	DICHLORPROP	0.0015	U	0.00076	0.0015	0.0020	mg/L
94-75-7	2,4-D	0.0015	U	0.00092	0.0015	0.0020	mg/L
93-72-1	2,4,5-TP (Silvex)	0.0015	U	0.00078	0.0015	0.0020	mg/L
93-76-5	2,4,5-T	0.0015	U	0.00071	0.0015	0.0020	mg/L
94-82-6	2,4-DB	0.0015	U	0.00065	0.0015	0.0020	mg/L
88-85-7	DINOSEB	0.0015	U	0.00089	0.0015	0.0020	mg/L
<b>SURROGATES</b>							
19719-28-9	2,4-DCAA	588		32 - 138		118%	SPK: 500

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS030012.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 11:48  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

**Instrument :**  
 ECD\_S  
**ClientSampleId :**  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 04:56:40 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

#### System Monitoring Compounds

4) S	2,4-DCAA	6.938	7.462	1355.2E6	414.2E6	550.671	587.866
------	----------	-------	-------	----------	---------	---------	---------

#### Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS030012.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 11:48  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 04:56:40 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

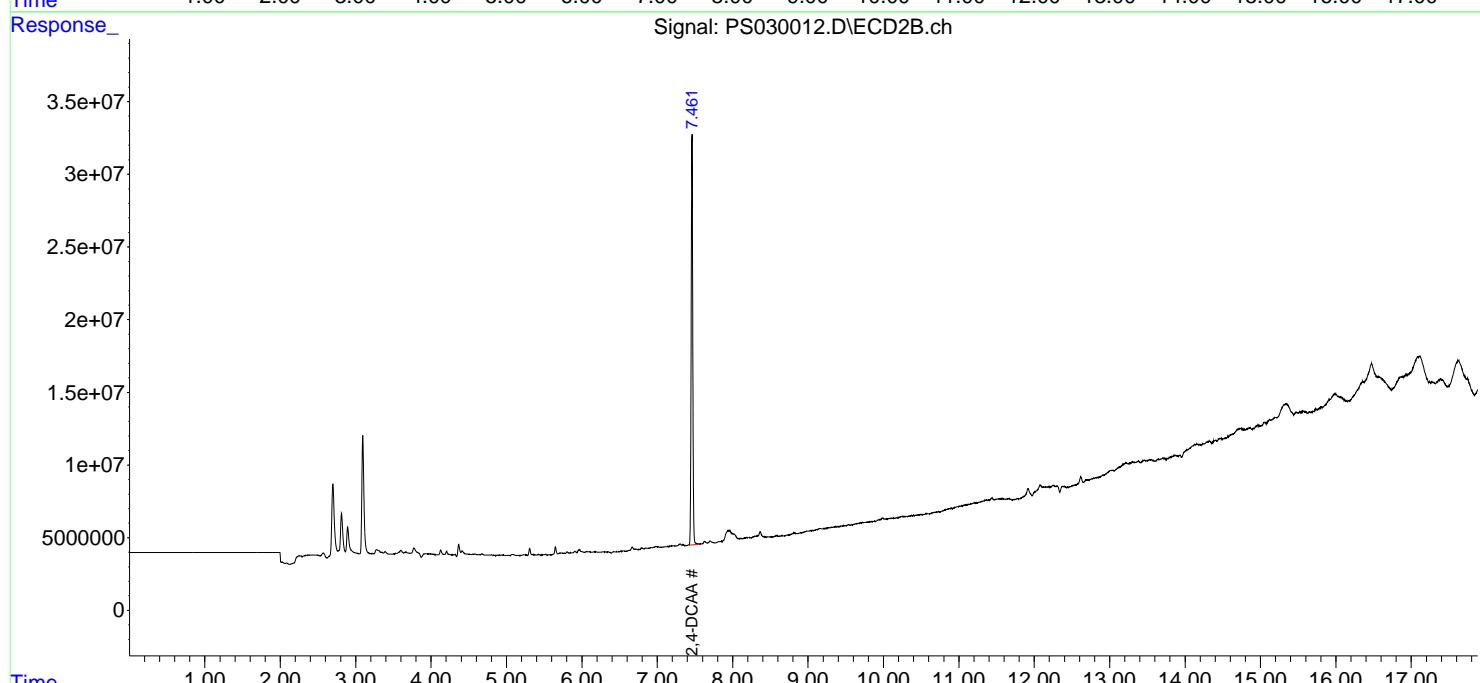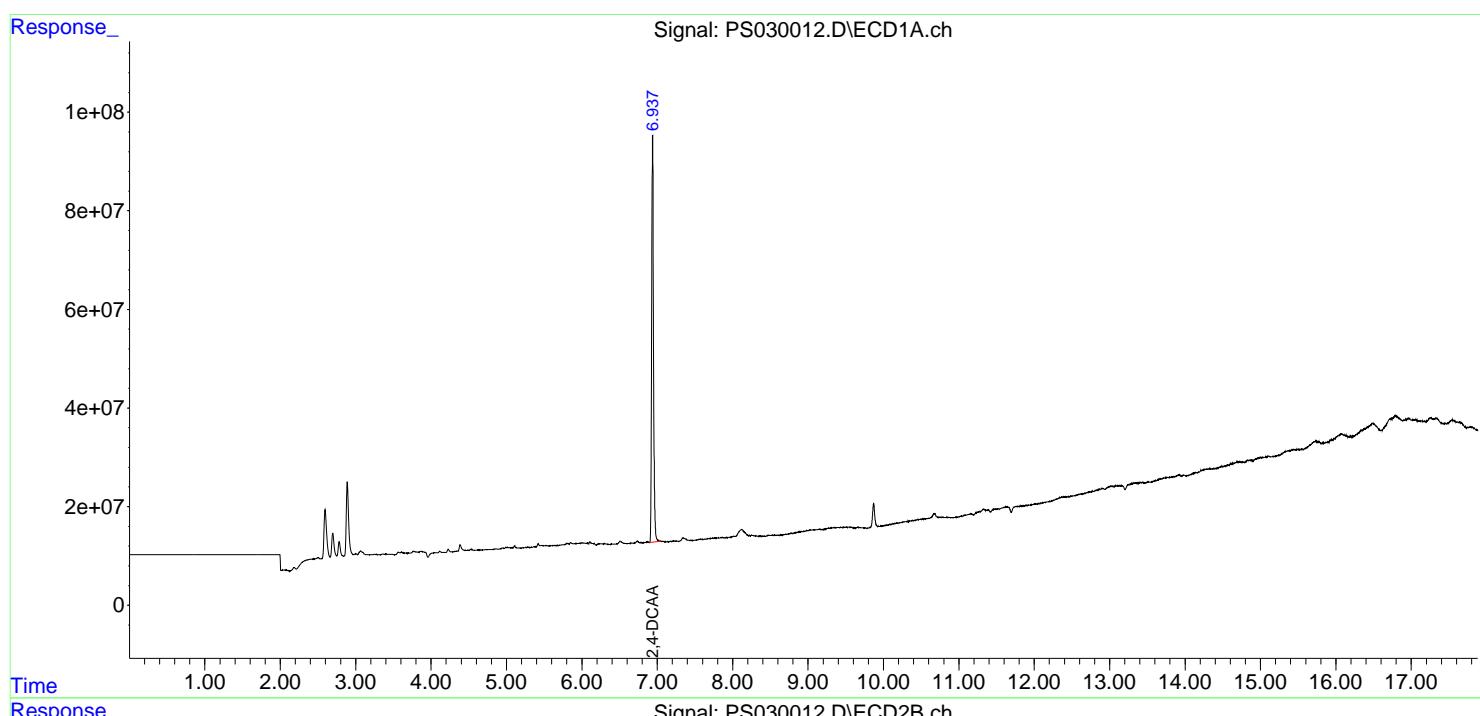

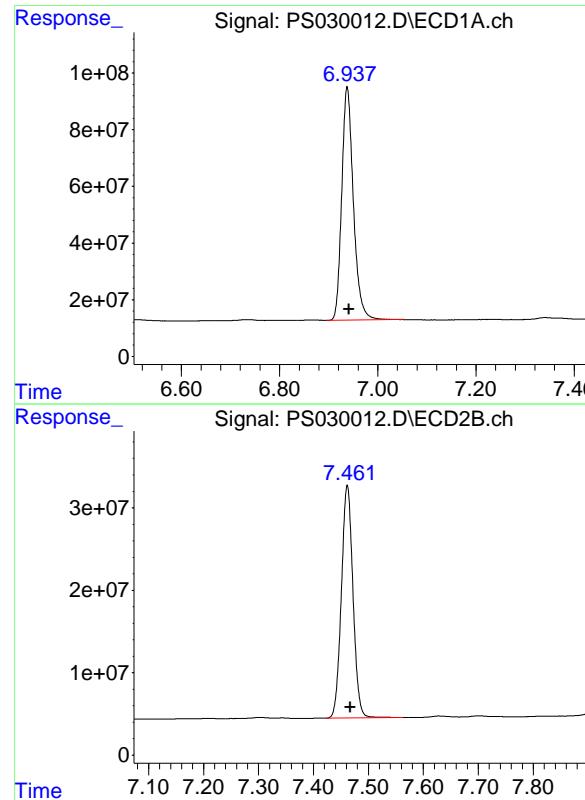

#4 2,4-DCAA

R.T.: 6.938 min  
Delta R.T.: -0.004 min  
Instrument: ECD\_S  
Response: 1355245620  
Conc: 550.67 ng/ml  
ClientSampleId: I.BLK

#4 2,4-DCAA

R.T.: 7.462 min  
Delta R.T.: -0.005 min  
Instrument: ECD\_S  
Response: 414161543  
Conc: 587.87 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group		Date Collected:	05/01/25	
Project:	Raymark Superfund Site		Date Received:	05/01/25	
Client Sample ID:	PIBLK-PS030015.D		SDG No.:	Q1883	
Lab Sample ID:	I.BLK-PS030015.D		Matrix:	WATER	
Analytical Method:	SW8151A		% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units: mL	Final Vol:	10000	uL
Soil Aliquot Vol:	uL		Test:	Herbicide Group1	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	SW3510C				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PS030015.D	1		05/01/25	PS050125

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
<b>TARGETS</b>							
1918-00-9	DICAMBA	0.0015	U	0.00065	0.0015	0.0020	mg/L
75-99-0	DALAPON	0.0015	U	0.00098	0.0015	0.0020	mg/L
120-36-5	DICHLORPROP	0.0015	U	0.00076	0.0015	0.0020	mg/L
94-75-7	2,4-D	0.0015	U	0.00092	0.0015	0.0020	mg/L
93-72-1	2,4,5-TP (Silvex)	0.0015	U	0.00078	0.0015	0.0020	mg/L
93-76-5	2,4,5-T	0.0015	U	0.00071	0.0015	0.0020	mg/L
94-82-6	2,4-DB	0.0015	U	0.00065	0.0015	0.0020	mg/L
88-85-7	DINOSEB	0.0015	U	0.00089	0.0015	0.0020	mg/L
<b>SURROGATES</b>							
19719-28-9	2,4-DCAA	567		32 - 138		113%	SPK: 500

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030015.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 13:03  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

**Instrument :**  
 ECD\_S  
**ClientSampleId :**  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:27:58 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

#### System Monitoring Compounds

4) S	2,4-DCAA	6.938	7.461	1314.8E6	399.5E6	534.222	567.062
------	----------	-------	-------	----------	---------	---------	---------

#### Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030015.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 13:03  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:27:58 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

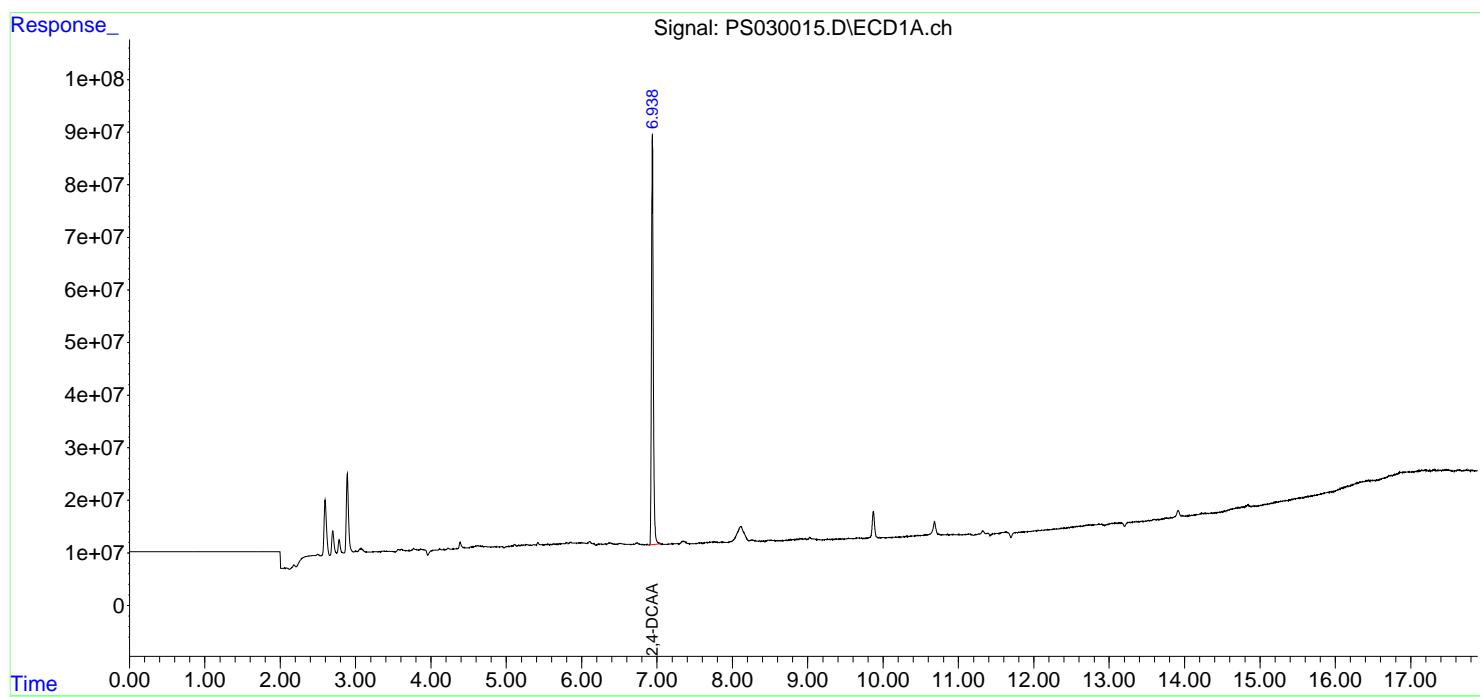

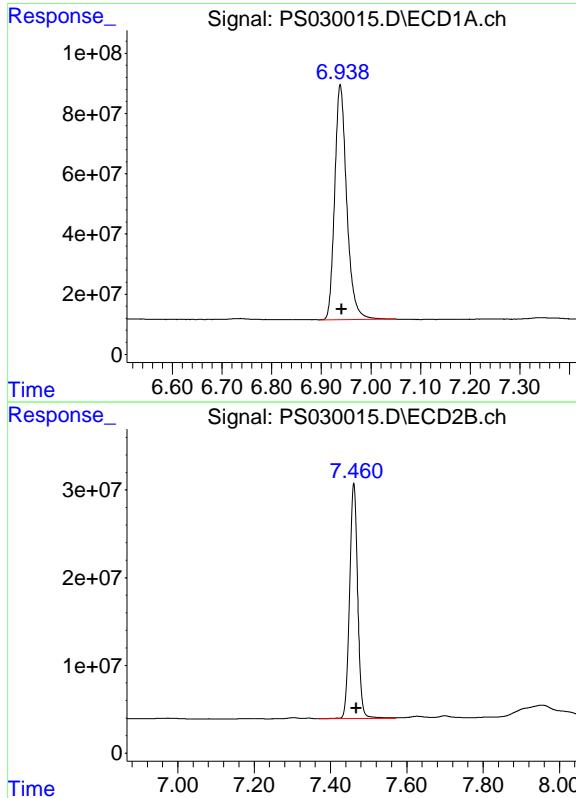

#4 2,4-DCAA

R.T.: 6.938 min  
Delta R.T.: -0.003 min  
Instrument: ECD\_S  
Response: 1314762398  
Conc: 534.22 ng/ml  
ClientSampleId: I.BLK

#4 2,4-DCAA

R.T.: 7.461 min  
Delta R.T.: -0.006 min  
Instrument: ECD\_S  
Response: 399504566  
Conc: 567.06 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group		Date Collected:	05/01/25	
Project:	Raymark Superfund Site		Date Received:	05/01/25	
Client Sample ID:	PIBLK-PS030025.D		SDG No.:	Q1883	
Lab Sample ID:	I.BLK-PS030025.D		Matrix:	WATER	
Analytical Method:	SW8151A		% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units: mL	Final Vol:	10000	uL
Soil Aliquot Vol:	uL		Test:	Herbicide Group1	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	SW3510C				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PS030025.D	1		05/01/25	PS050125

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
<b>TARGETS</b>							
1918-00-9	DICAMBA	0.0015	U	0.00065	0.0015	0.0020	mg/L
75-99-0	DALAPON	0.0015	U	0.00098	0.0015	0.0020	mg/L
120-36-5	DICHLORPROP	0.0015	U	0.00076	0.0015	0.0020	mg/L
94-75-7	2,4-D	0.0015	U	0.00092	0.0015	0.0020	mg/L
93-72-1	2,4,5-TP (Silvex)	0.0015	U	0.00078	0.0015	0.0020	mg/L
93-76-5	2,4,5-T	0.0015	U	0.00071	0.0015	0.0020	mg/L
94-82-6	2,4-DB	0.0015	U	0.00065	0.0015	0.0020	mg/L
88-85-7	DINOSEB	0.0015	U	0.00089	0.0015	0.0020	mg/L
<b>SURROGATES</b>							
19719-28-9	2,4-DCAA	598		32 - 138		120%	SPK: 500

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030025.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 17:04  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

**Instrument :**  
 ECD\_S  
**ClientSampleId :**  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:30:32 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

---

System Monitoring Compounds

4) S	2,4-DCAA	6.937	7.461	1382.9E6	421.1E6	561.916	597.779
------	----------	-------	-------	----------	---------	---------	---------

---

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030025.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 17:04  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:30:32 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

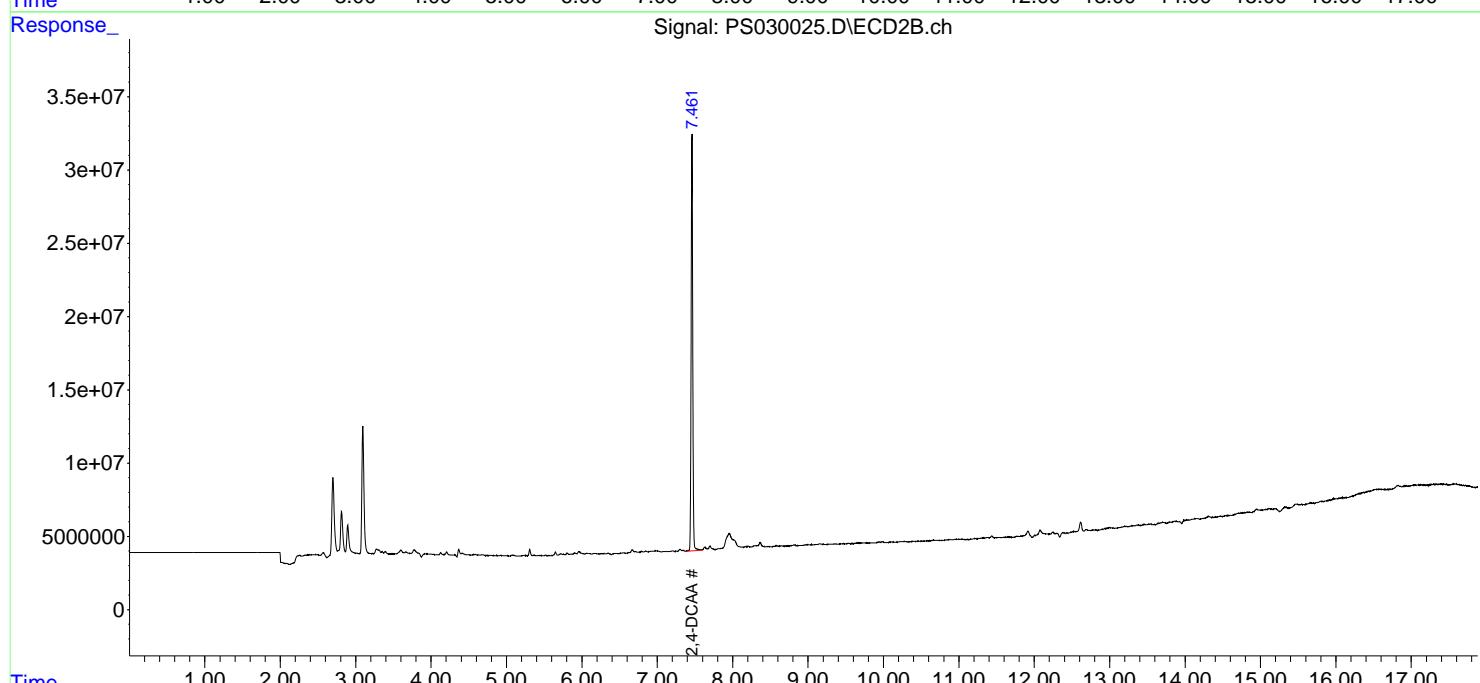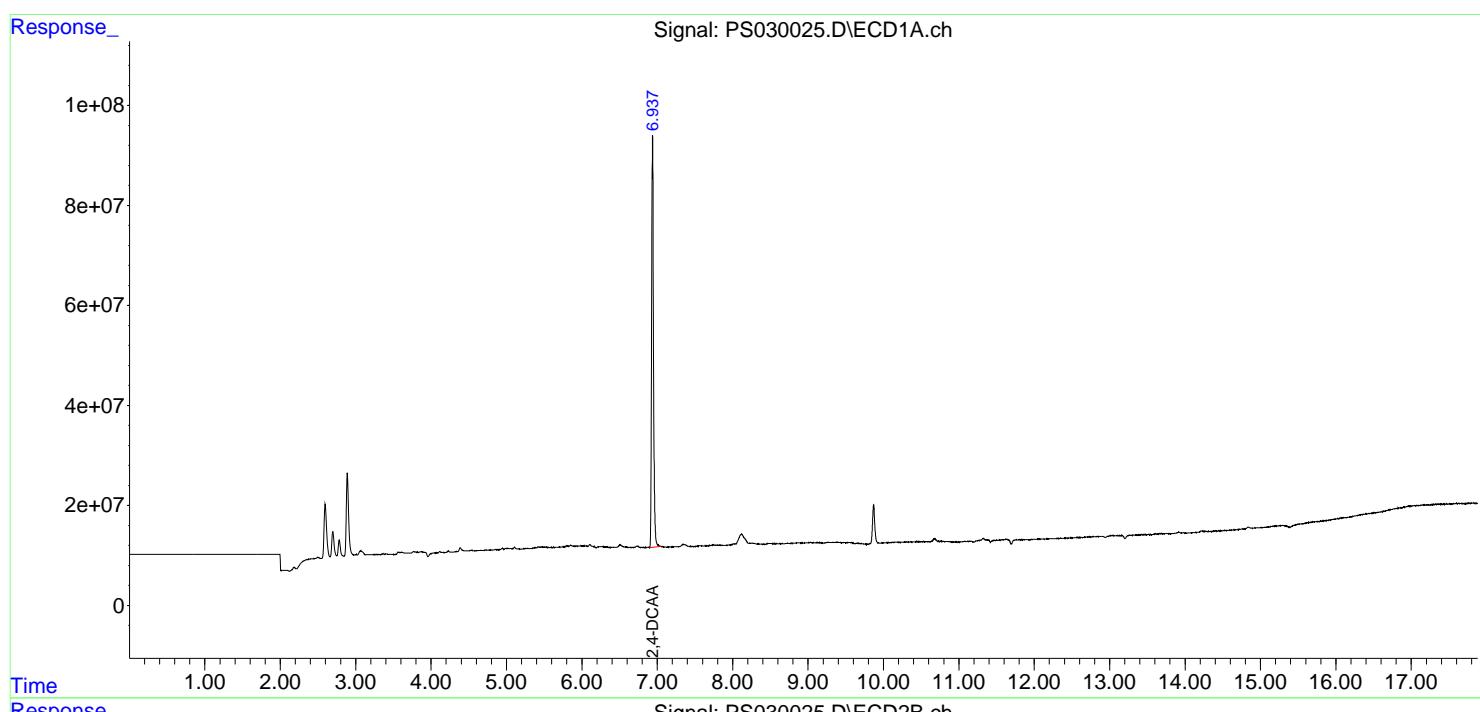

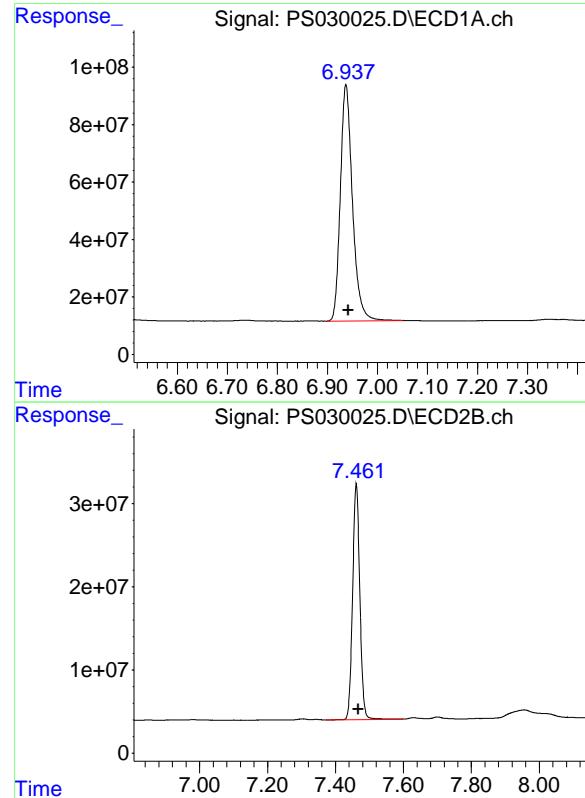

#4 2,4-DCAA

R.T.: 6.937 min  
Delta R.T.: -0.004 min  
Instrument: ECD\_S  
Response: 1382919654  
Conc: 561.92 ng/ml  
ClientSampleId: I.BLK

#4 2,4-DCAA

R.T.: 7.461 min  
Delta R.T.: -0.006 min  
Instrument: ECD\_S  
Response: 421145565  
Conc: 597.78 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	05/05/25			
Project:	Raymark Superfund Site			Date Received:	05/05/25			
Client Sample ID:	PIBLK-PS030028.D			SDG No.:	Q1883			
Lab Sample ID:	I.BLK-PS030028.D			Matrix:	WATER			
Analytical Method:	SW8151A			% Solid:	0	Decanted:		
Sample Wt/Vol:	1000	Units:	mL	Final Vol:	10000	uL		
Soil Aliquot Vol:	uL			Test:	Herbicide Group1			
Extraction Type:				Injection Volume :				
GPC Factor :	1.0	PH :						
Prep Method :	SW3510C							

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PS030028.D	1		05/05/25	ps050525

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
<b>TARGETS</b>							
1918-00-9	DICAMBA	0.0015	U	0.00065	0.0015	0.0020	mg/L
75-99-0	DALAPON	0.0015	U	0.00098	0.0015	0.0020	mg/L
120-36-5	DICHLORPROP	0.0015	U	0.00076	0.0015	0.0020	mg/L
94-75-7	2,4-D	0.0015	U	0.00092	0.0015	0.0020	mg/L
93-72-1	2,4,5-TP (Silvex)	0.0015	U	0.00078	0.0015	0.0020	mg/L
93-76-5	2,4,5-T	0.0015	U	0.00071	0.0015	0.0020	mg/L
94-82-6	2,4-DB	0.0015	U	0.00065	0.0015	0.0020	mg/L
88-85-7	DINOSEB	0.0015	U	0.00089	0.0015	0.0020	mg/L
<b>SURROGATES</b>							
19719-28-9	2,4-DCAA	553		32 - 138		111%	SPK: 500

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050525\  
 Data File : PS030028.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 05 May 2025 08:38  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

**Instrument :**  
 ECD\_S  
**ClientSampleId :**  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 05 12:28:41 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	6.938	7.461	1305.4E6	389.9E6	530.428	553.396
------	----------	-------	-------	----------	---------	---------	---------

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050525\  
 Data File : PS030028.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 05 May 2025 08:38  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 05 12:28:41 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

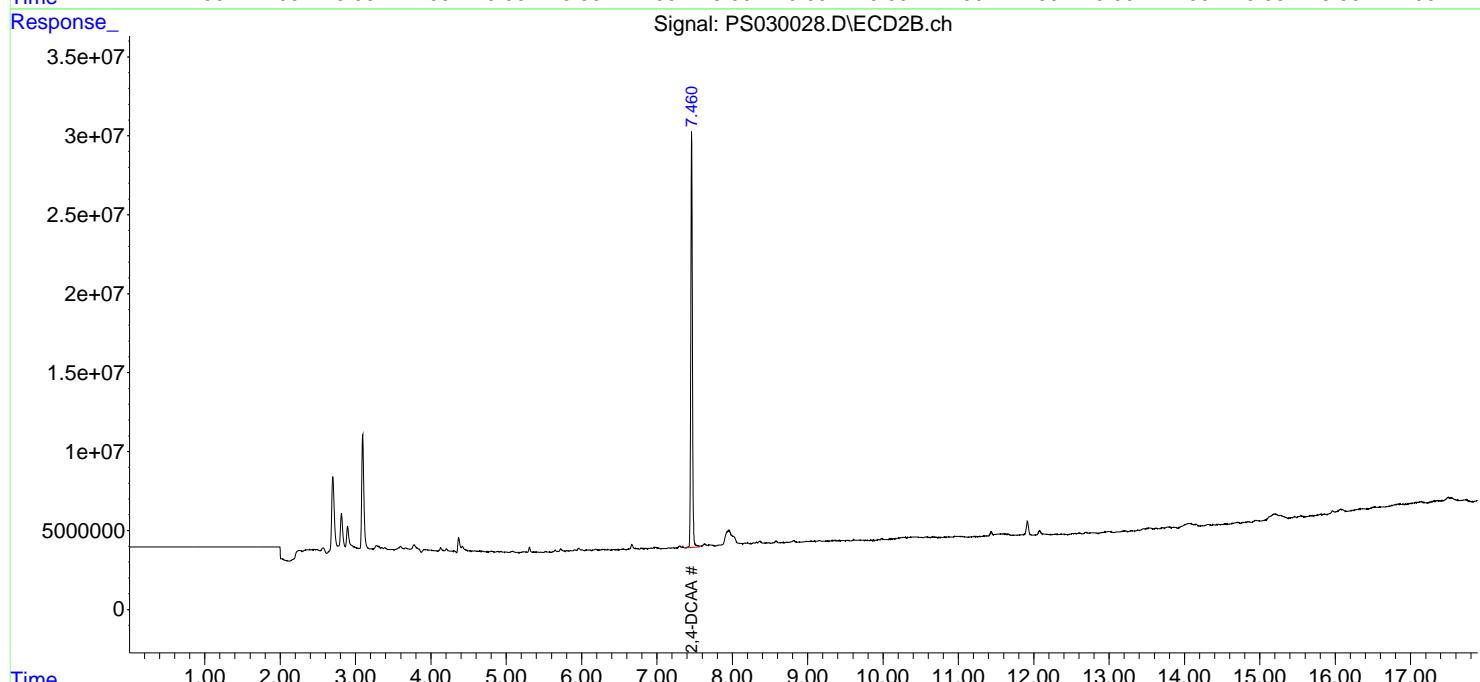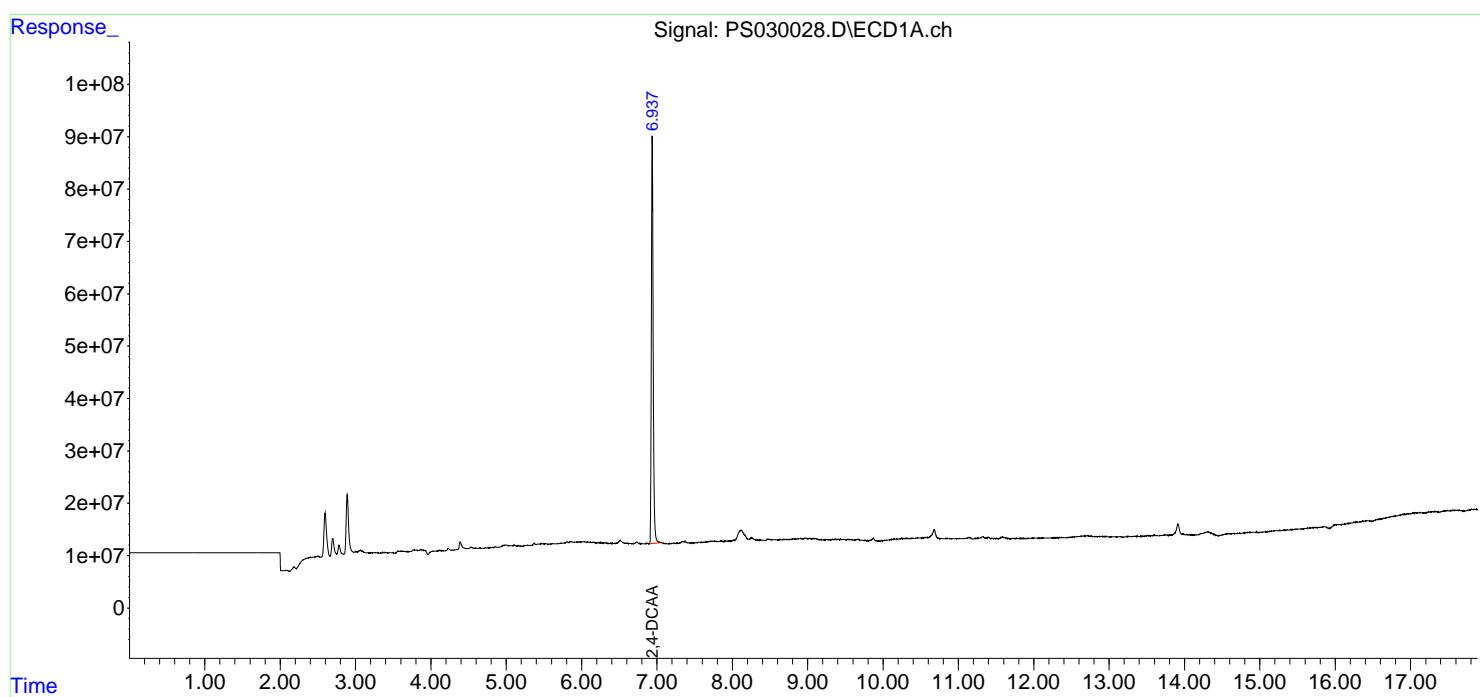

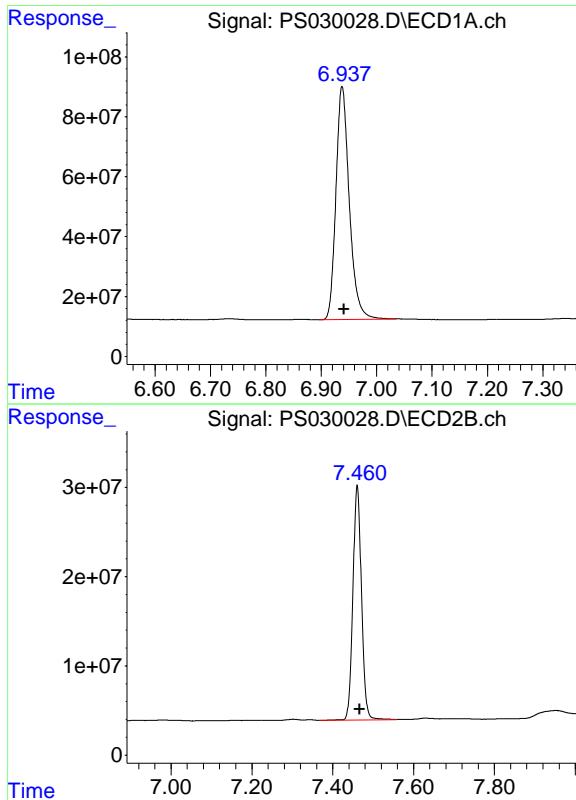

#4 2,4-DCAA

R.T.: 6.938 min  
Delta R.T.: -0.004 min  
Instrument: ECD\_S  
Response: 1305426093  
Conc: 530.43 ng/ml  
ClientSampleId: I.BLK

#4 2,4-DCAA

R.T.: 7.461 min  
Delta R.T.: -0.006 min  
Instrument: ECD\_S  
Response: 389876808  
Conc: 553.40 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	05/05/25			
Project:	Raymark Superfund Site			Date Received:	05/05/25			
Client Sample ID:	PIBLK-PS030040.D			SDG No.:	Q1883			
Lab Sample ID:	I.BLK-PS030040.D			Matrix:	WATER			
Analytical Method:	SW8151A			% Solid:	0	Decanted:		
Sample Wt/Vol:	1000	Units:	mL	Final Vol:	10000	uL		
Soil Aliquot Vol:	uL			Test:	Herbicide Group1			
Extraction Type:				Injection Volume :				
GPC Factor :	1.0	PH :						
Prep Method :	SW3510C							

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PS030040.D	1		05/05/25	ps050525

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
<b>TARGETS</b>							
1918-00-9	DICAMBA	0.0015	U	0.00065	0.0015	0.0020	mg/L
75-99-0	DALAPON	0.0015	U	0.00098	0.0015	0.0020	mg/L
120-36-5	DICHLORPROP	0.0015	U	0.00076	0.0015	0.0020	mg/L
94-75-7	2,4-D	0.0015	U	0.00092	0.0015	0.0020	mg/L
93-72-1	2,4,5-TP (Silvex)	0.0015	U	0.00078	0.0015	0.0020	mg/L
93-76-5	2,4,5-T	0.0015	U	0.00071	0.0015	0.0020	mg/L
94-82-6	2,4-DB	0.0015	U	0.00065	0.0015	0.0020	mg/L
88-85-7	DINOSEB	0.0015	U	0.00089	0.0015	0.0020	mg/L
<b>SURROGATES</b>							
19719-28-9	2,4-DCAA	552		32 - 138		110%	SPK: 500

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050525\  
 Data File : PS030040.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 05 May 2025 14:35  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

**Instrument :**  
 ECD\_S  
**ClientSampleId :**  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 06 01:39:41 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

#### System Monitoring Compounds

4) S	2,4-DCAA	6.938	7.461	1302.1E6	389.2E6	529.085	552.472
------	----------	-------	-------	----------	---------	---------	---------

#### Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050525\  
 Data File : PS030040.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 05 May 2025 14:35  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 06 01:39:41 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

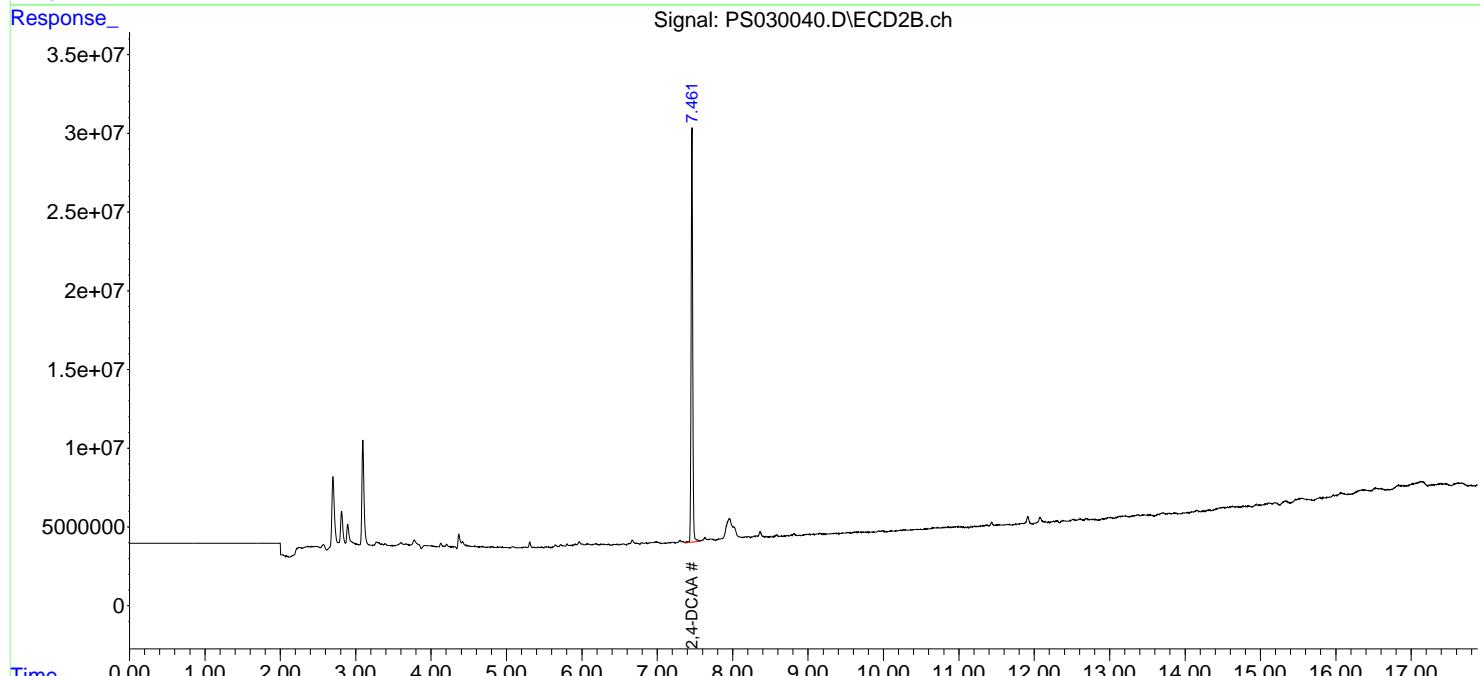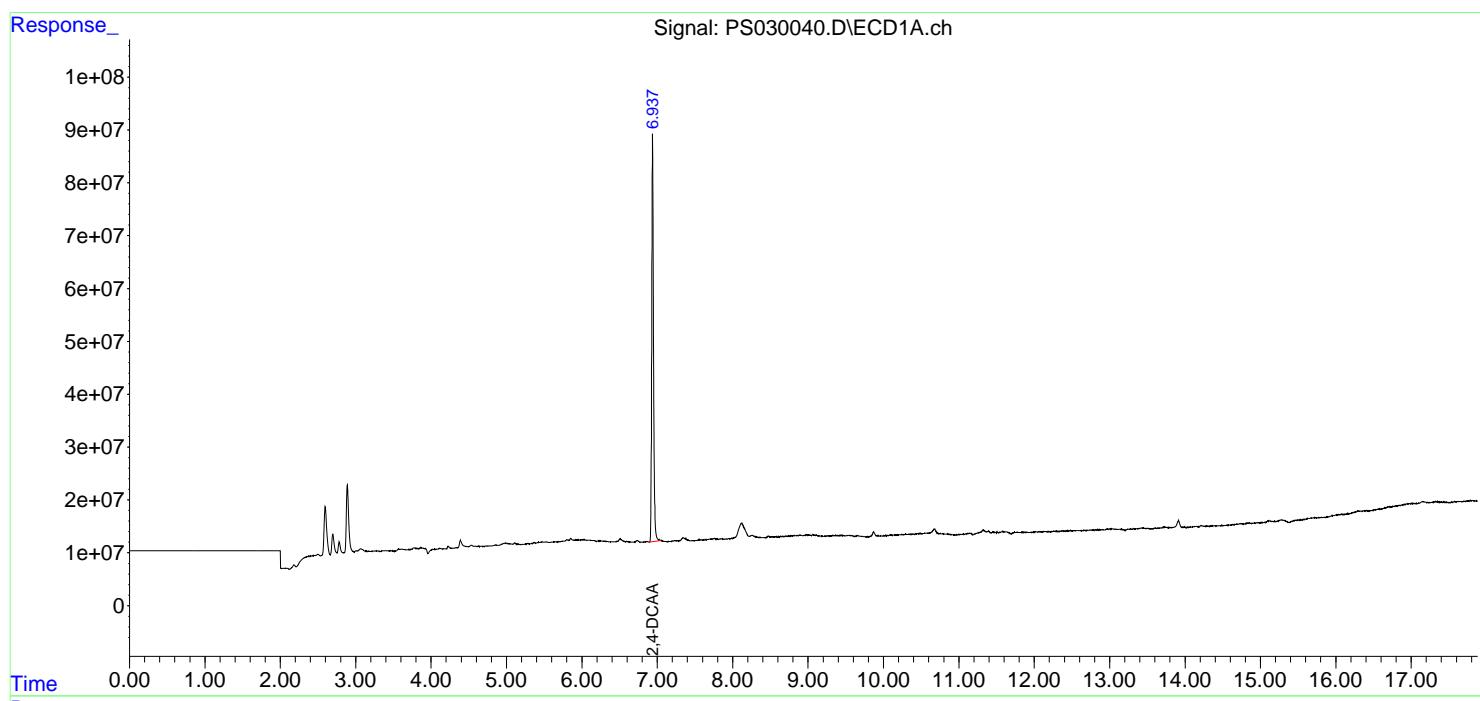

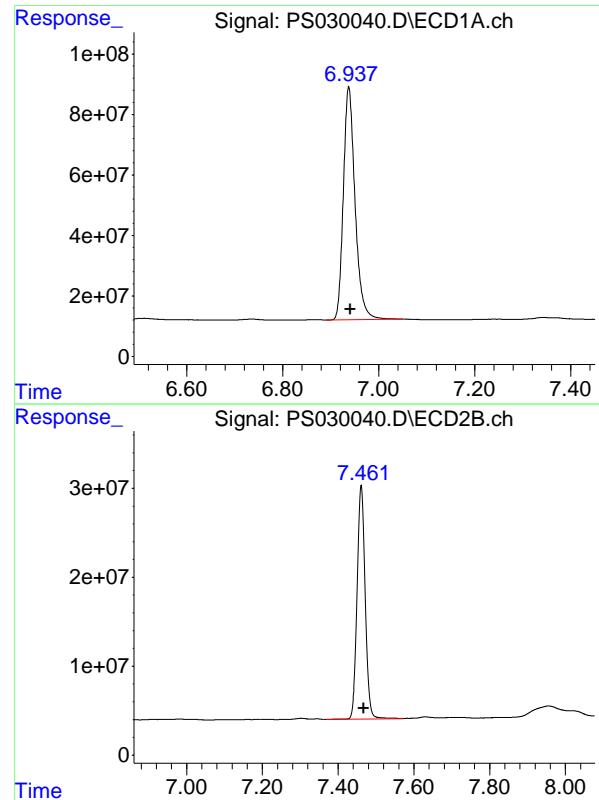

#4 2,4-DCAA

R.T.: 6.938 min  
Delta R.T.: -0.004 min  
Instrument: ECD\_S  
Response: 1302120132  
Conc: 529.09 ng/ml  
ClientSampleId: I.BLK

#4 2,4-DCAA

R.T.: 7.461 min  
Delta R.T.: -0.006 min  
Instrument: ECD\_S  
Response: 389225615  
Conc: 552.47 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group		Date Collected:	
Project:	Raymark Superfund Site		Date Received:	
Client Sample ID:	PB167796BS		SDG No.:	Q1883
Lab Sample ID:	PB167796BS		Matrix:	SOIL
Analytical Method:	SW8151A		% Solid:	100 Decanted:
Sample Wt/Vol:	30.02	Units: g	Final Vol:	10000 uL
Soil Aliquot Vol:	uL		Test:	Herbicide Group1
Extraction Type:			Injection Volume :	
GPC Factor :	1.0	PH :		
Prep Method :	8151A			

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PS030038.D	1	04/30/25 08:50	05/05/25 13:47	PB167796

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
1918-00-9	DICAMBA	0.17		0.0077	0.033	0.067	mg/Kg
75-99-0	DALAPON	0.17		0.018	0.050	0.067	mg/Kg
120-36-5	DICHLORPROP	0.17		0.013	0.033	0.067	mg/Kg
94-75-7	2,4-D	0.17		0.0090	0.033	0.067	mg/Kg
93-72-1	2,4,5-TP (Silvex)	0.18		0.0091	0.033	0.067	mg/Kg
93-76-5	2,4,5-T	0.17		0.0087	0.033	0.067	mg/Kg
94-82-6	2,4-DB	0.17		0.024	0.033	0.067	mg/Kg
88-85-7	DINOSEB	0.17		0.011	0.033	0.067	mg/Kg
<b>SURROGATES</b>							
19719-28-9	2,4-DCAA	540		27 - 122		108%	SPK: 500

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050525\  
 Data File : PS030038.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 05 May 2025 13:47  
 Operator : AR\AJ  
 Sample : PB167796BS  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 PB167796BS

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/06/2025  
 Supervised By :mohammad ahmed 05/07/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 06 01:38:53 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

4) S 2,4-DCAA 6.937 7.461 1303.7E6 380.1E6 529.742 539.538

**Target Compounds**

1) T	Dalapon	2.449	2.523	2026.9E6	836.0E6	494.933	481.542
2) T	3,5-DICHL...	6.142	6.459	1748.8E6	487.0E6	489.353	498.167
3) T	4-Nitroph...	6.728	6.996	852.1E6	376.7E6	477.797	491.891
5) T	DICAMBA	7.114	7.647	4939.4E6	2039.7E6	498.784	516.364
6) T	MCPP	7.292	7.753	295.3E6	80604259	45.824	46.087
7) T	MCPA	7.434	7.983	412.6E6	112.5E6	46.719	47.564
8) T	DICHLORPROP	7.794	8.340	1243.9E6	517.9E6	490.874	515.829
9) T	2,4-D	8.014	8.653	1407.4E6	573.8E6	500.356	509.096
10) T	Pentachlo...	8.292	9.154	18046.0E6	10930.7E6	517.300	537.274
11) T	2,4,5-TP ...	8.856	9.532	7064.9E6	4305.5E6	509.626	526.230
12) T	2,4,5-T	9.138	9.936	7219.0E6	4034.3E6	513.694	519.714
13) T	2,4-DB	9.697	10.495	1180.4E6	404.5E6	516.485	502.607
14) T	DINOSEB	10.859	10.868	5116.9E6	2968.0E6	502.969	509.004
15) T	Picloram	10.678	11.903	9032.0E6	6199.1E6	492.728	504.661m
16) T	DCPA	11.160	11.902	8804.0E6	5502.2E6	517.242	488.145m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050525\  
 Data File : PS030038.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 05 May 2025 13:47  
 Operator : AR\AJ  
 Sample : PB167796BS  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1



Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 06 01:38:53 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation





Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Instrument :  
 ECD\_S  
 ClientSampleId :  
 PB167796BS

### Manual Integrations APPROVED

Reviewed By :Abdul Mirza 05/06/2025  
 Supervised By :mohammad ahmed 05/07/2025

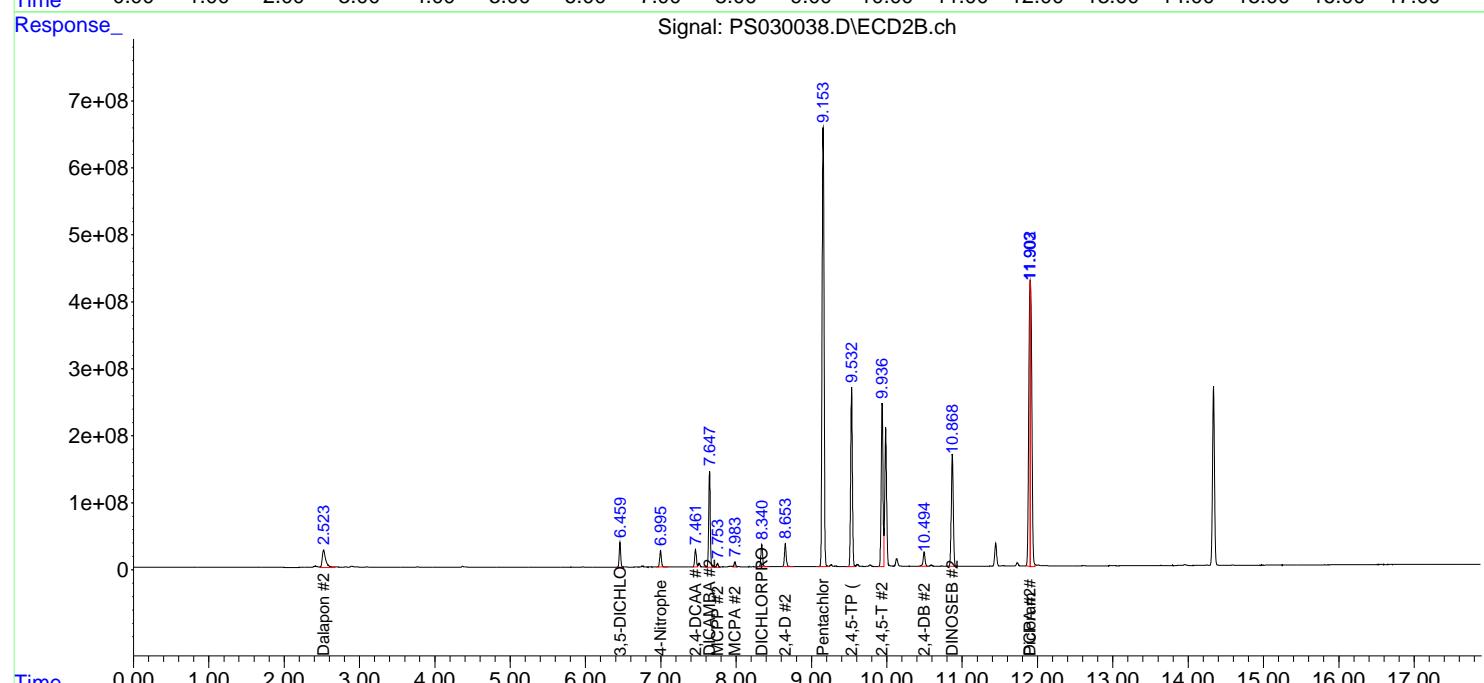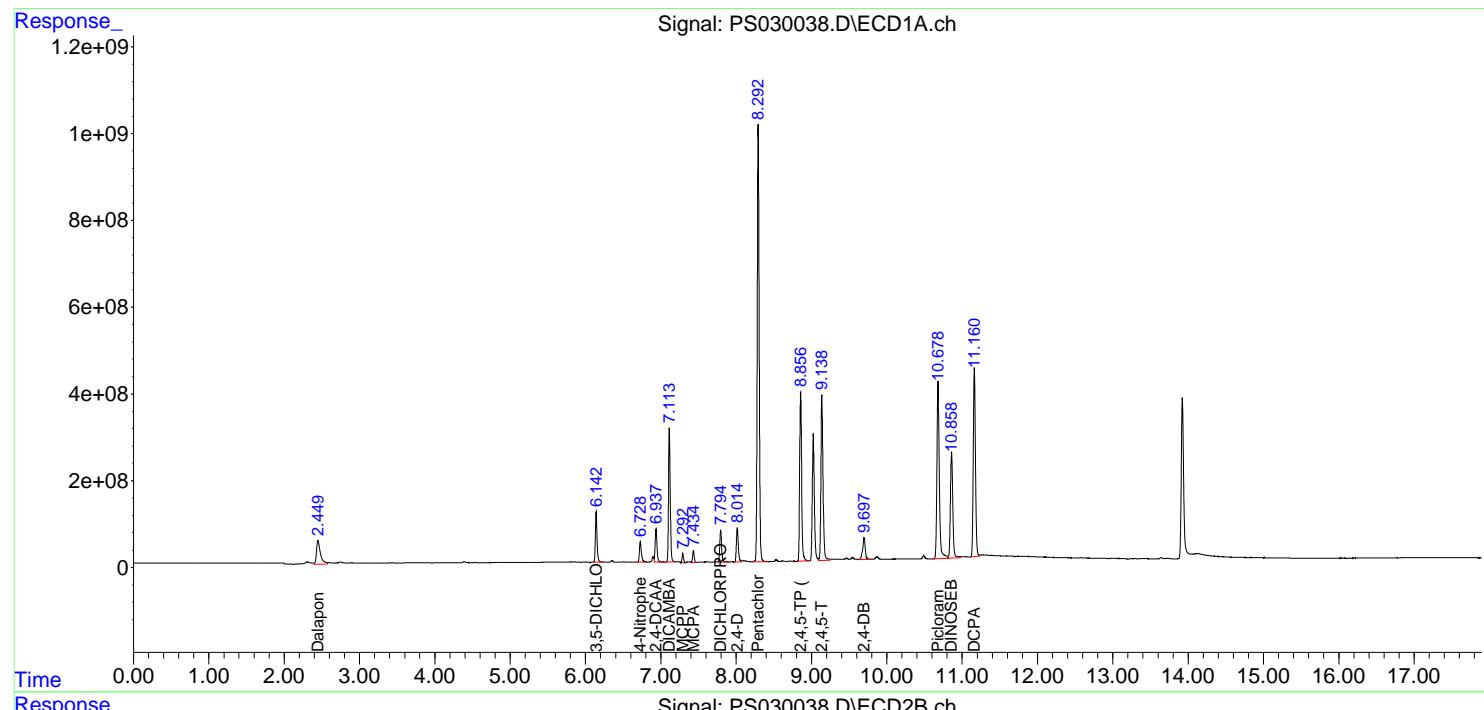

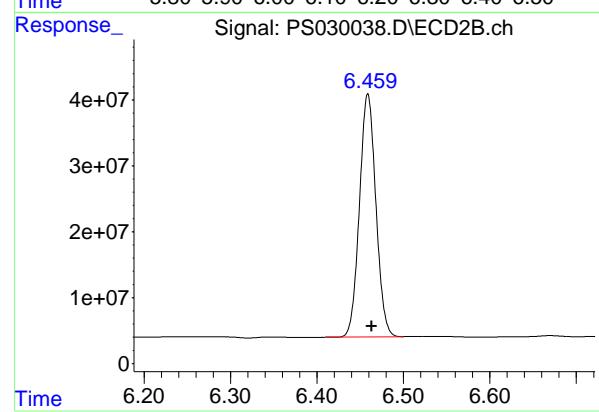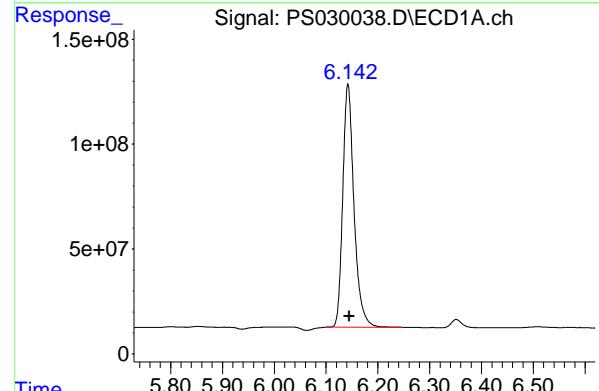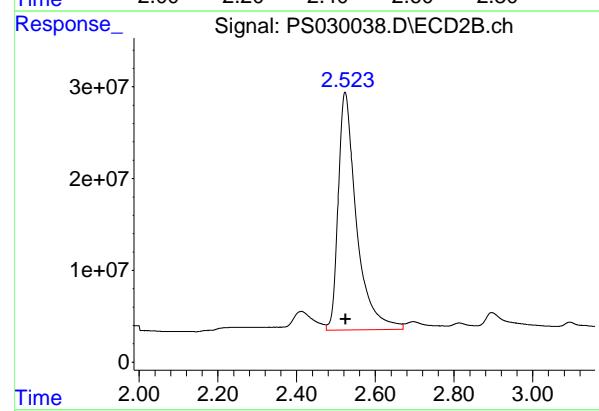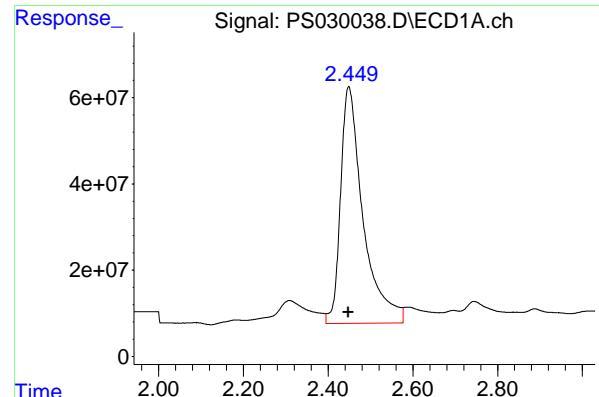

#1 Dalapon

R.T.: 2.449 min  
 Delta R.T.: 0.000 min  
 Response: 2026876943 ECD\_S  
 Conc: 494.93 ng/ml Client Sample Id : PB167796BS

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/06/2025  
 Supervised By :mohammad ahmed 05/07/2025

#1 Dalapon





R.T.: 2.523 min  
 Delta R.T.: -0.001 min  
 Response: 836026719  
 Conc: 481.54 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.142 min  
 Delta R.T.: -0.003 min  
 Response: 1748841469  
 Conc: 489.35 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.459 min  
 Delta R.T.: -0.004 min  
 Response: 486997904  
 Conc: 498.17 ng/ml

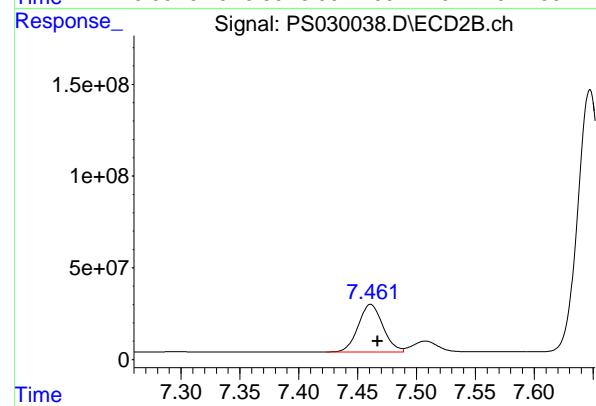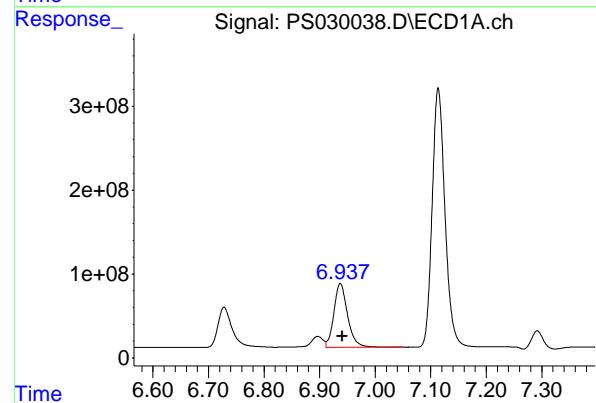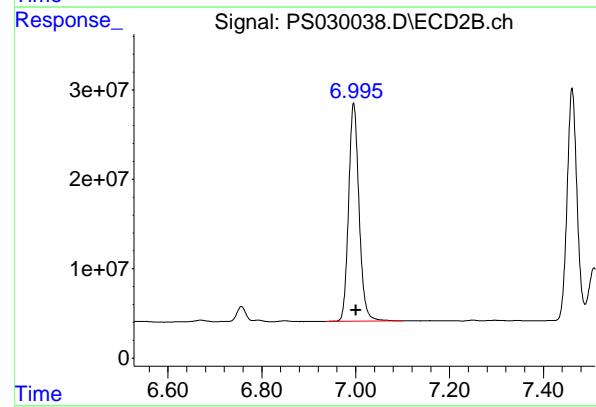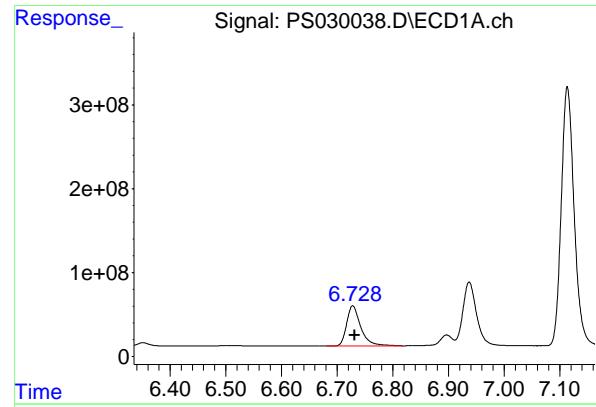

## #3 4-Nitrophenol

R.T.: 6.728 min  
Delta R.T.: -0.003 min  
Instrument: ECD\_S  
Response: 852065133  
Conc: 477.80 ng/ml  
ClientSampleId: PB167796BS

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/06/2025  
Supervised By :mohammad ahmed 05/07/2025

## #3 4-Nitrophenol





R.T.: 6.996 min  
Delta R.T.: -0.005 min  
Response: 376749767  
Conc: 491.89 ng/ml

## #4 2,4-DCAA

R.T.: 6.937 min  
Delta R.T.: -0.004 min  
Response: 1303737946  
Conc: 529.74 ng/ml

## #4 2,4-DCAA

R.T.: 7.461 min  
Delta R.T.: -0.006 min  
Response: 380113891  
Conc: 539.54 ng/ml

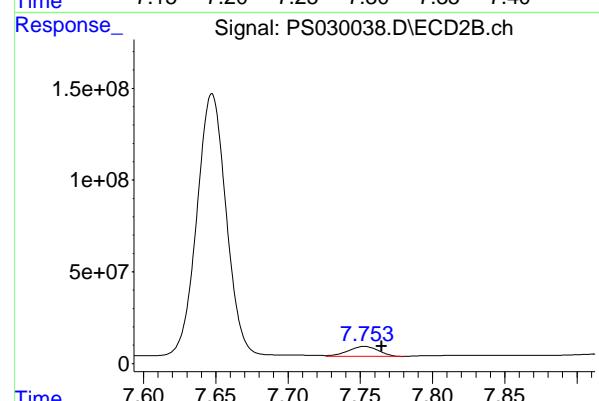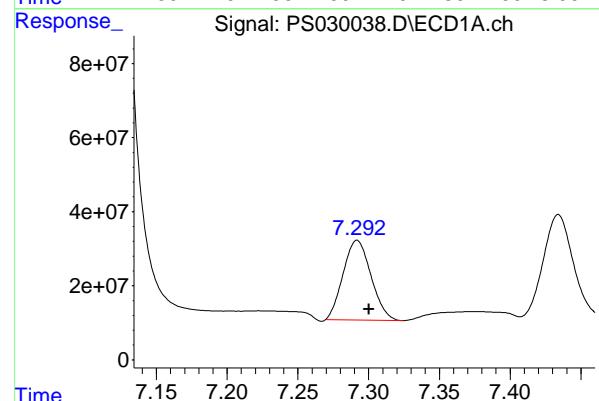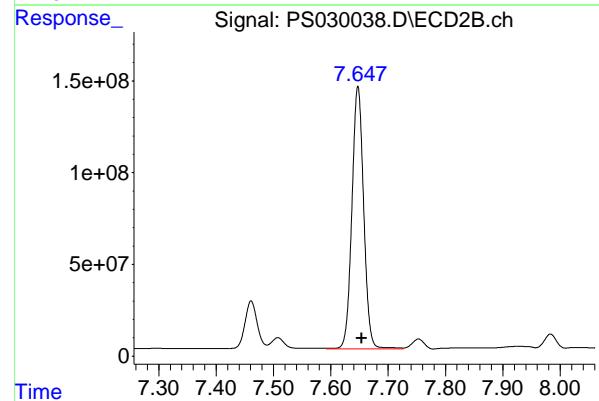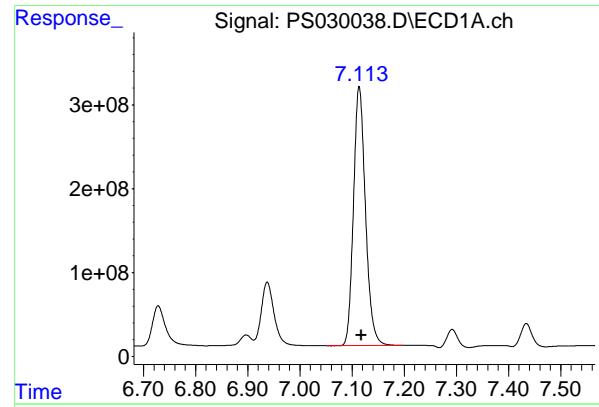

## #5 DICAMBA

R.T.: 7.114 min  
 Delta R.T.: -0.004 min  
 Response: 4939392609 ECD\_S  
 Conc: 498.78 ng/ml Client SampleId : PB167796BS

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/06/2025  
 Supervised By :mohammad ahmed 05/07/2025

## #5 DICAMBA



R.T.: 7.647 min  
 Delta R.T.: -0.006 min  
 Response: 2039671767  
 Conc: 516.36 ng/ml

## #6 MCPP

R.T.: 7.292 min  
 Delta R.T.: -0.008 min  
 Response: 295272711  
 Conc: 45.82 ug/ml

## #6 MCPP

R.T.: 7.753 min  
 Delta R.T.: -0.012 min  
 Response: 80604259  
 Conc: 46.09 ug/ml

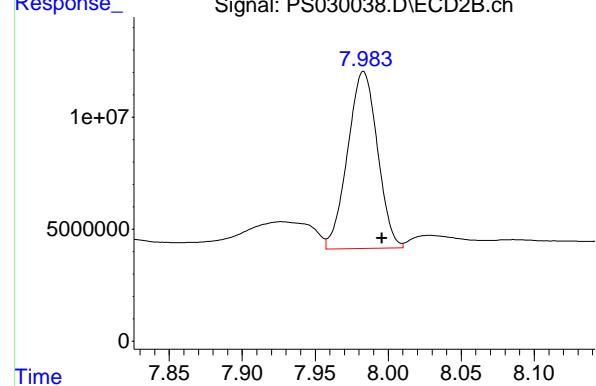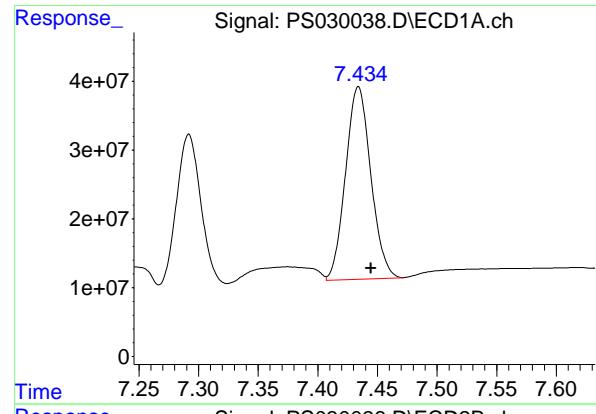

## #7 MCPA

R.T.: 7.434 min  
 Delta R.T.: -0.010 min  
 Response: 412595382  
 Conc: 46.72 ug/ml

Instrument: ECD\_S  
 Client Sample Id: PB167796BS

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/06/2025  
 Supervised By :mohammad ahmed 05/07/2025

## #7 MCPA





R.T.: 7.983 min  
 Delta R.T.: -0.013 min  
 Response: 112526574  
 Conc: 47.56 ug/ml

## #8 DICHLORPROP

R.T.: 7.794 min  
 Delta R.T.: -0.005 min  
 Response: 1243928182  
 Conc: 490.87 ng/ml

## #8 DICHLORPROP

R.T.: 8.340 min  
 Delta R.T.: -0.007 min  
 Response: 517874081  
 Conc: 515.83 ng/ml

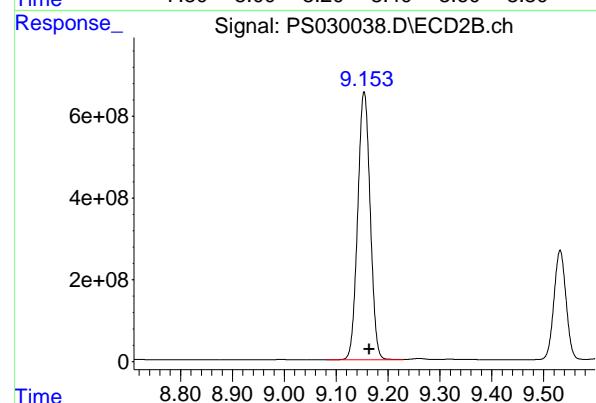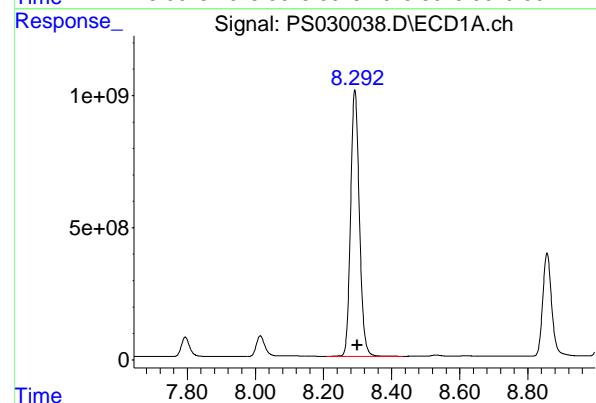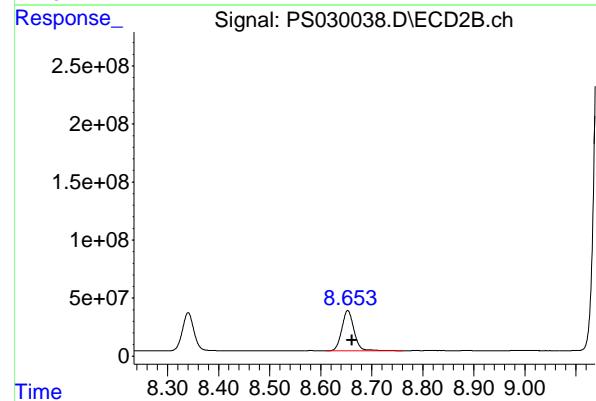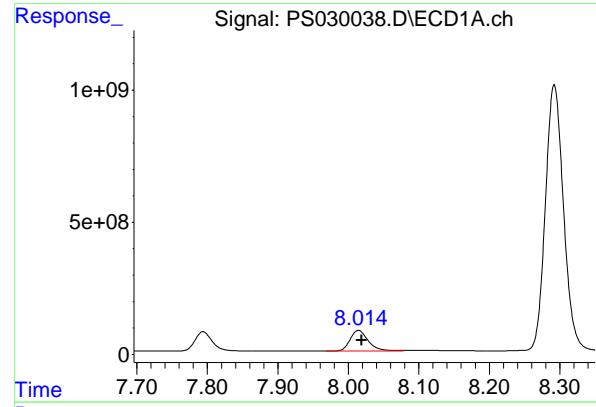

#9 2,4-D

R.T.: 8.014 min  
Delta R.T.: -0.004 min  
Instrument: ECD\_S  
Response: 1407438073  
Conc: 500.36 ng/ml  
ClientSampleId: PB167796BS

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/06/2025  
Supervised By :mohammad ahmed 05/07/2025

#9 2,4-D





R.T.: 8.653 min  
Delta R.T.: -0.008 min  
Response: 573806176  
Conc: 509.10 ng/ml

#10 Pentachlorophenol

R.T.: 8.292 min  
Delta R.T.: -0.008 min  
Response: 18046010957  
Conc: 517.30 ng/ml

#10 Pentachlorophenol

R.T.: 9.154 min  
Delta R.T.: -0.010 min  
Response: 10930731101  
Conc: 537.27 ng/ml

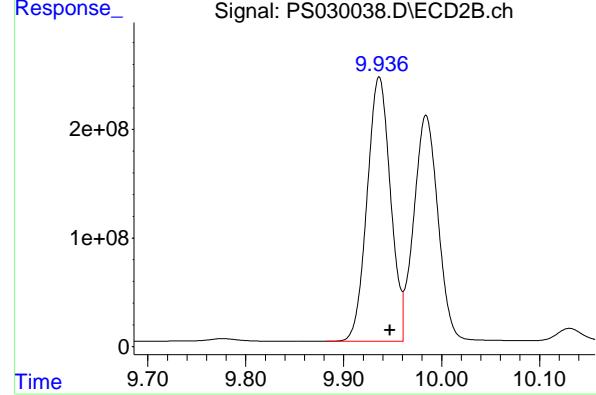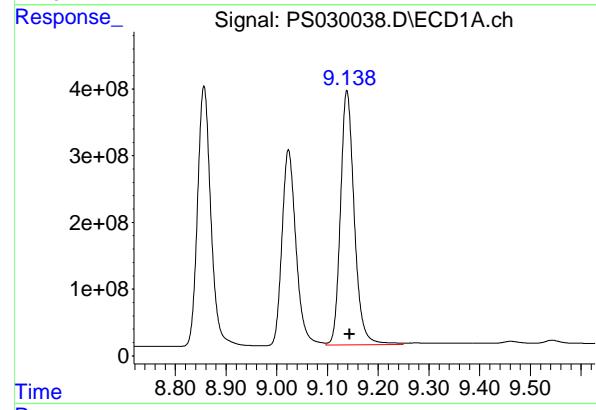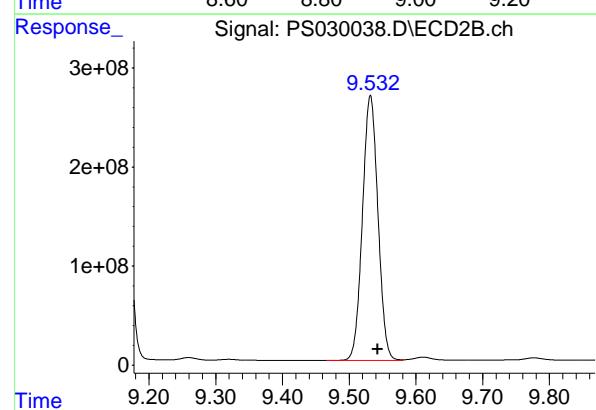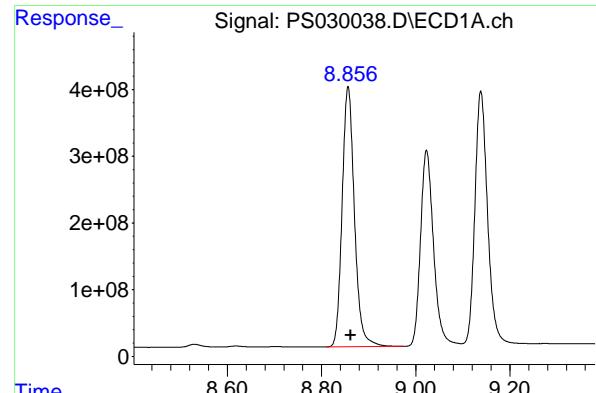

#11 2,4,5-TP (SILVEX)

R.T.: 8.856 min

Delta R.T.: -0.006 min

Instrument: ECD\_S

Response: 7064866109 ClientSampleId :

Conc: 509.63 ng/ml PB167796BS

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/06/2025

Supervised By :mohammad ahmed 05/07/2025

#11 2,4,5-TP (SILVEX)

R.T.: 9.532 min

Delta R.T.: -0.011 min

Response: 4305484681

Conc: 526.23 ng/ml

#12 2,4,5-T

R.T.: 9.138 min

Delta R.T.: -0.006 min

Response: 7218996712

Conc: 513.69 ng/ml





#12 2,4,5-T

R.T.: 9.936 min

Delta R.T.: -0.011 min

Response: 4034329145

Conc: 519.71 ng/ml

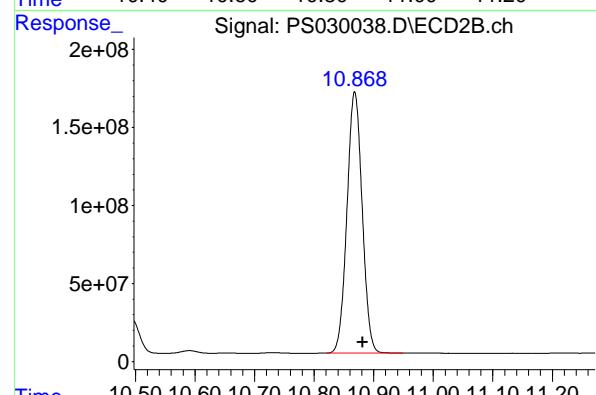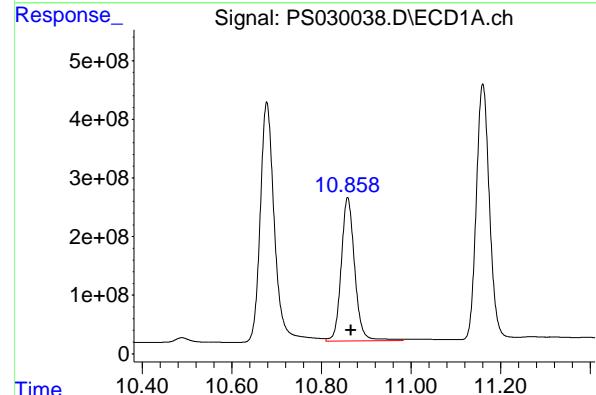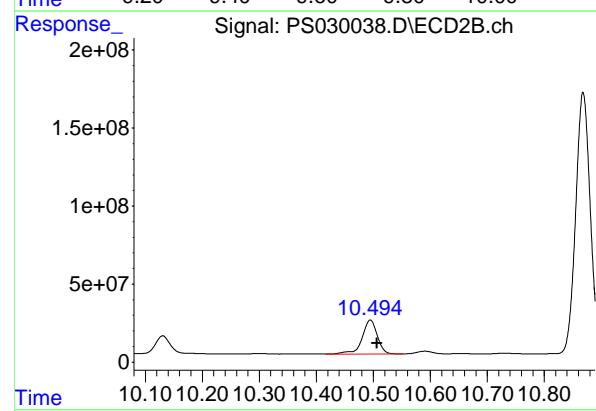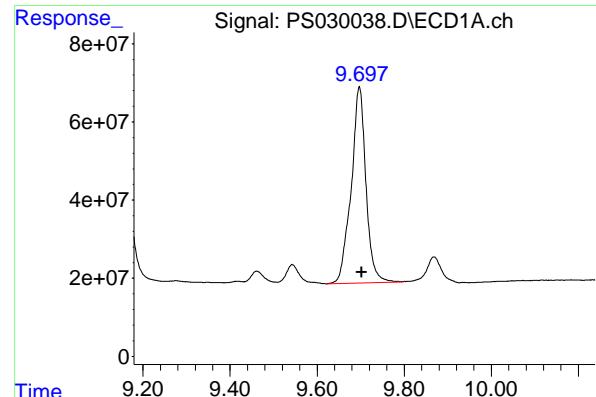

#13 2,4-DB

R.T.: 9.697 min  
 Delta R.T.: -0.005 min  
 Response: 1180351095 ECD\_S  
 Conc: 516.48 ng/ml Client Sample ID : PB167796BS

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/06/2025  
 Supervised By :mohammad ahmed 05/07/2025

#13 2,4-DB


R.T.: 10.495 min  
 Delta R.T.: -0.012 min  
 Response: 404519772  
 Conc: 502.61 ng/ml

#14 DINOSEB

R.T.: 10.859 min  
 Delta R.T.: -0.007 min  
 Response: 5116917707  
 Conc: 502.97 ng/ml

#14 DINOSEB

R.T.: 10.868 min  
 Delta R.T.: -0.013 min  
 Response: 2967993353  
 Conc: 509.00 ng/ml

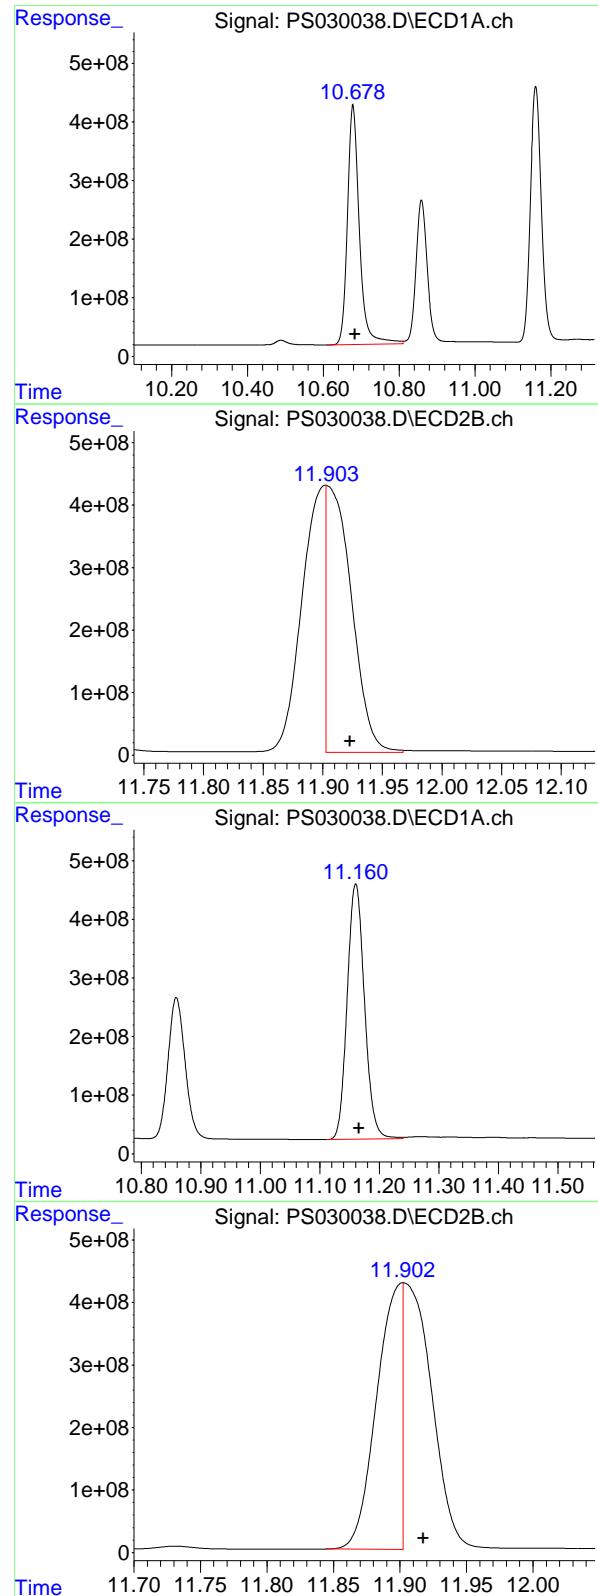

## #15 Picloram

R.T.: 10.678 min  
 Delta R.T.: -0.005 min  
 Response: 9032014243 ECD\_S  
 Conc: 492.73 ng/ml Client Sample ID: PB167796BS

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/06/2025  
 Supervised By :mohammad ahmed 05/07/2025

## #15 Picloram

R.T.: 11.903 min  
 Delta R.T.: -0.020 min  
 Response: 6199068847  
 Conc: 504.66 ng/ml

## #16 DCPA

R.T.: 11.160 min  
 Delta R.T.: -0.006 min  
 Response: 8803982200  
 Conc: 517.24 ng/ml

## #16 DCPA

R.T.: 11.902 min  
 Delta R.T.: -0.016 min  
 Response: 5502196952  
 Conc: 488.14 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/28/25	
Project:	Raymark Superfund Site			Date Received:	04/28/25	
Client Sample ID:	WC-5MS			SDG No.:	Q1883	
Lab Sample ID:	Q1906-05MS			Matrix:	SOIL	
Analytical Method:	SW8151A			% Solid:	83.5	Decanted:
Sample Wt/Vol:	30.06	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	Herbicide Group1	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	8151A					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PS029999.D	1	04/30/25 08:50	05/01/25 04:34	PB167796

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
1918-00-9	DICAMBA	0.13		0.0093	0.039	0.080	mg/Kg
75-99-0	DALAPON	0.39	P	0.021	0.060	0.080	mg/Kg
120-36-5	DICHLORPROP	0.14	P	0.015	0.039	0.080	mg/Kg
94-75-7	2,4-D	0.17		0.011	0.039	0.080	mg/Kg
93-72-1	2,4,5-TP (Silvex)	0.097		0.011	0.039	0.080	mg/Kg
93-76-5	2,4,5-T	0.11		0.010	0.039	0.080	mg/Kg
94-82-6	2,4-DB	0.082		0.029	0.039	0.080	mg/Kg
88-85-7	DINOSEB	0.039	U	0.013	0.039	0.080	mg/Kg
<b>SURROGATES</b>							
19719-28-9	2,4-DCAA	1520	*	27 - 122		303%	SPK: 500

Comments:

U = Not Detected  
 LOQ = Limit of Quantitation  
 MDL = Method Detection Limit  
 LOD = Limit of Detection  
 E = Value Exceeds Calibration Range  
 P = Indicates >25% difference for detected concentrations between the two GC columns  
 Q = indicates LCS control criteria did not meet requirements  
 M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value  
 B = Analyte Found in Associated Method Blank  
 N = Presumptive Evidence of a Compound  
 \* = Values outside of QC limits  
 D = Dilution  
 S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.  
 () = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS029999.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 04:34  
 Operator : AR\AJ  
 Sample : Q1906-05MS  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 WC-5MS

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 01 04:56:31 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

4) S 2,4-DCAA 6.919 7.462 2352.7E6 1067.4E6 955.960 1515.125 #

**Target Compounds**

1) T	Dalapon	2.442	2.515	2778.7E6	1703.5E6	678.528	981.208	#
2) T	3,5-DICHL...	6.142	6.459	1089.2E6	276.7E6	304.768m	283.063	
3) T	4-Nitroph...	6.705	6.964	108.8E6	80838331	60.990	105.544m#	
5) T	DICAMBA	7.115	7.647	3104.5E6	1301.2E6	313.498m	329.411	
6) T	MCPP	7.292	7.739	169.1E6	167.6E6	26.245	95.838	#
7) T	MCPA	7.434	7.981	275.9E6	85484678	31.237	36.133	
8) T	DICHLORPROP	7.796	8.341	648.1E6	340.2E6	255.749m	338.858	#
9) T	2,4-D	8.015	8.654	1168.3E6	453.2E6	415.356	402.054	
10) T	Pentachlo...	8.293	9.155	5741.5E6	3568.2E6	164.582m	175.388	
11) T	2,4,5-TP ...	8.857	9.533	2807.2E6	1987.5E6	202.496m	242.916m	
12) T	2,4,5-T	9.140	9.938	3632.2E6	2158.8E6	258.462	278.109	
13) T	2,4-DB	9.700	10.494	469.1E6	163.6E6	205.243m	203.327m	
15) T	Picloram	10.680	11.903	5787.6E6	4817.9E6	315.734	392.218m	
16) T	DCPA	11.162	11.901	6627.9E6	4674.0E6	389.398m	414.671m	

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS029999.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 04:34  
 Operator : AR\AJ  
 Sample : Q1906-05MS  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1



Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 01 04:56:31 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation





Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Instrument :  
 ECD\_S  
 ClientSampleId :  
 WC-5MS

### Manual Integrations APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

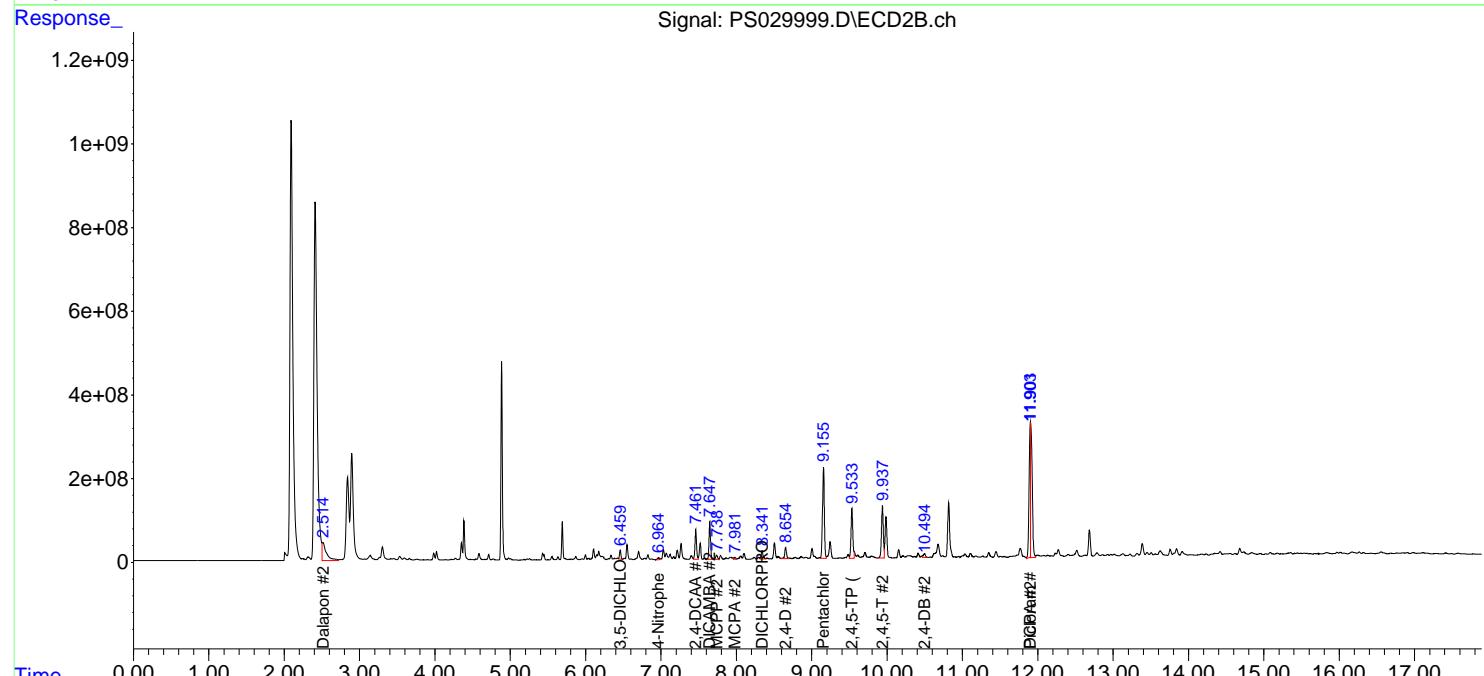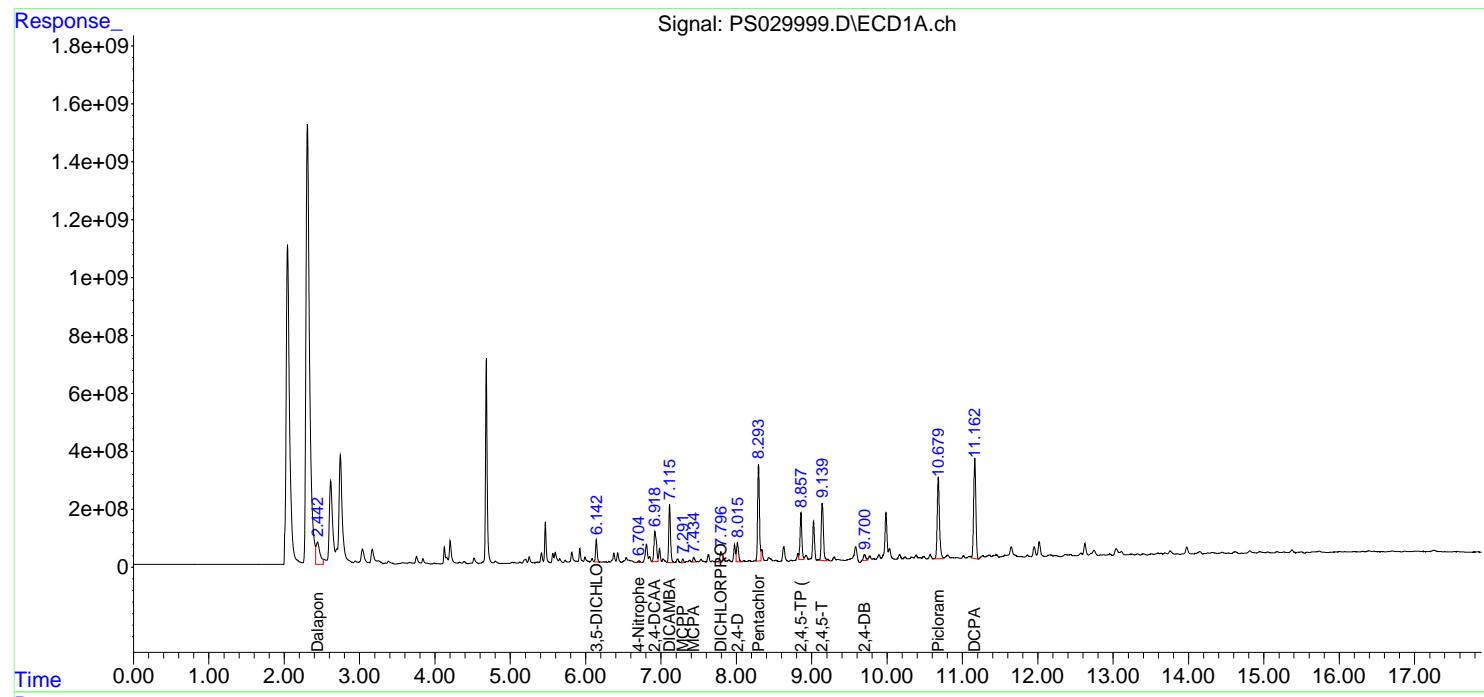

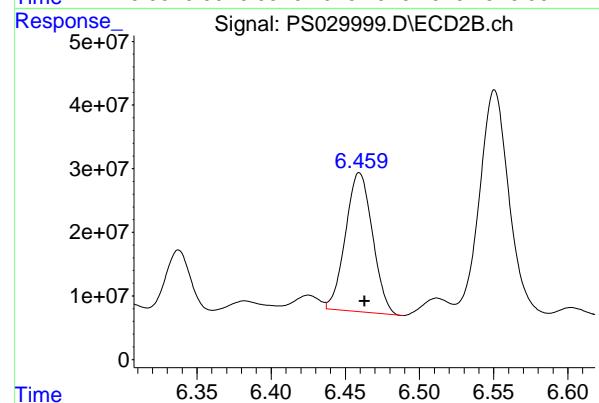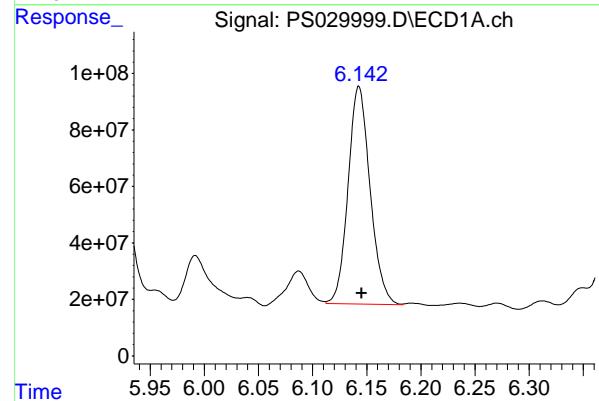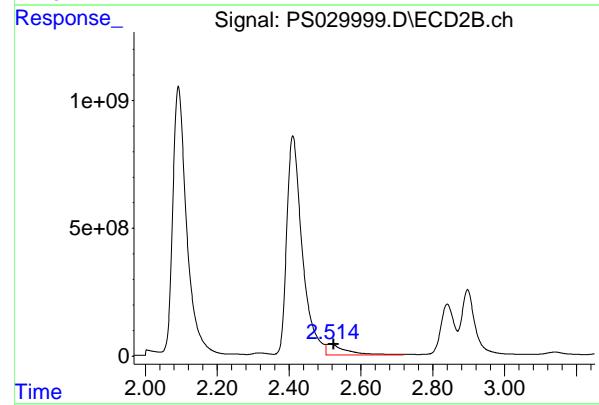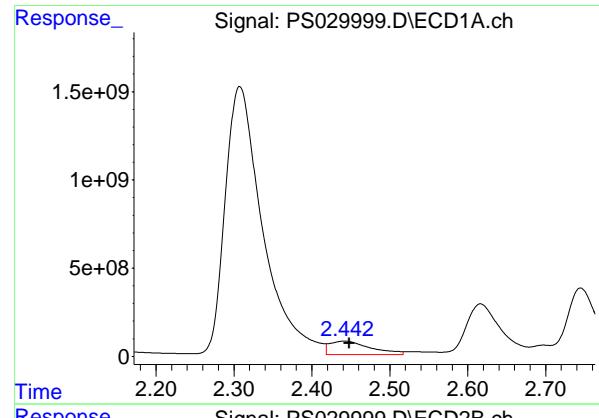

#1 Dalapon

R.T.: 2.442 min  
Delta R.T.: -0.006 min  
Instrument: ECD\_S  
Response: 2778749021  
Conc: 678.53 ng/ml  
Client Sample Id: WC-5MS

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
Supervised By :mohammad ahmed 05/02/2025

#1 Dalapon





R.T.: 2.515 min  
Delta R.T.: -0.010 min  
Response: 1703518196  
Conc: 981.21 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.142 min  
Delta R.T.: -0.003 min  
Response: 1089175555  
Conc: 304.77 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.459 min  
Delta R.T.: -0.004 min  
Response: 276716083  
Conc: 283.06 ng/ml

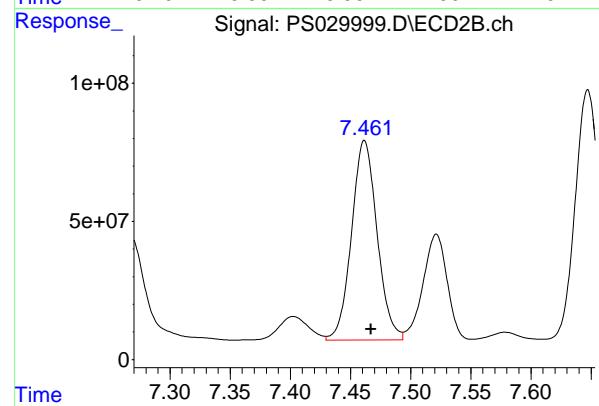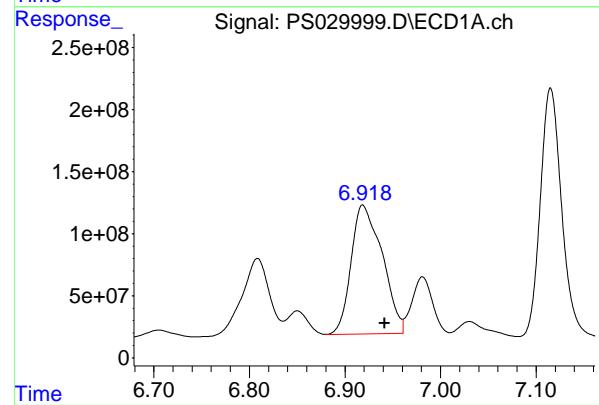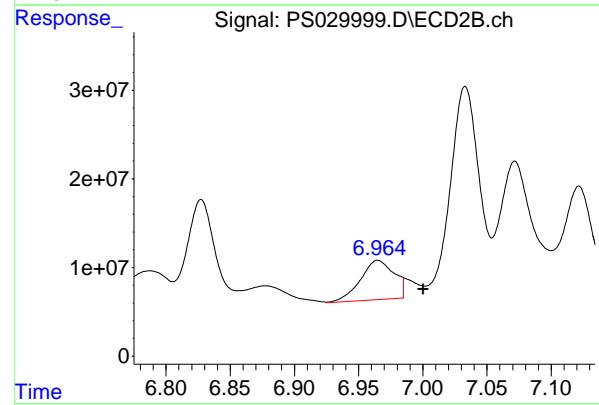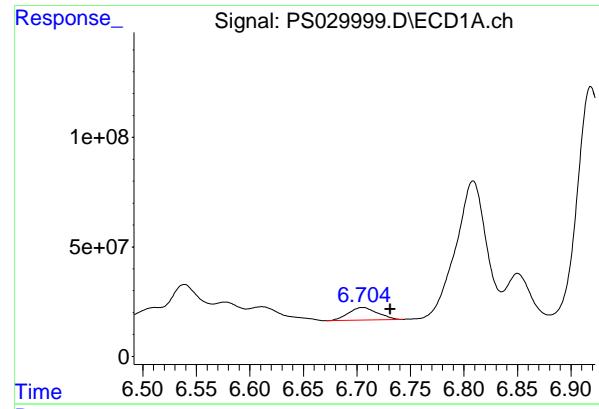

## #3 4-Nitrophenol

R.T.: 6.705 min  
Delta R.T.: -0.026 min  
Response: 108765273  
Conc: 60.99 ng/ml

Instrument: ECD\_S  
ClientSampleId: WC-5MS

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
Supervised By :mohammad ahmed 05/02/2025

## #3 4-Nitrophenol




R.T.: 6.964 min  
Delta R.T.: -0.036 min  
Response: 80838331  
Conc: 105.54 ng/ml

## #4 2,4-DCAA

R.T.: 6.919 min  
Delta R.T.: -0.022 min  
Response: 2352694270  
Conc: 955.96 ng/ml

## #4 2,4-DCAA

R.T.: 7.462 min  
Delta R.T.: -0.005 min  
Response: 1067430949  
Conc: 1515.12 ng/ml

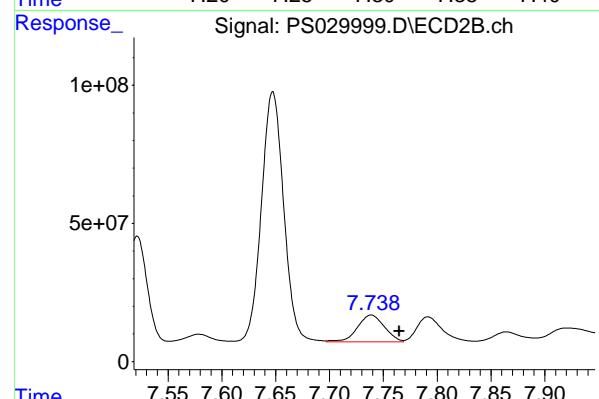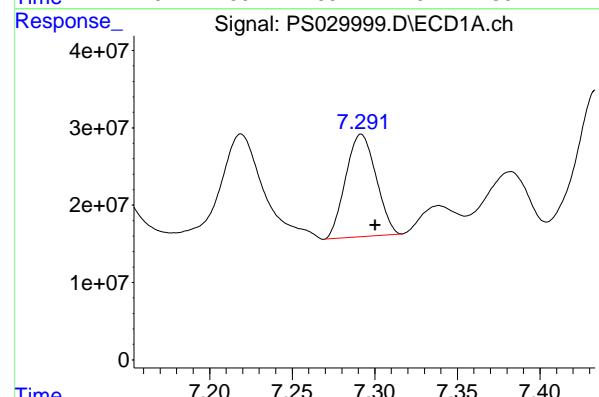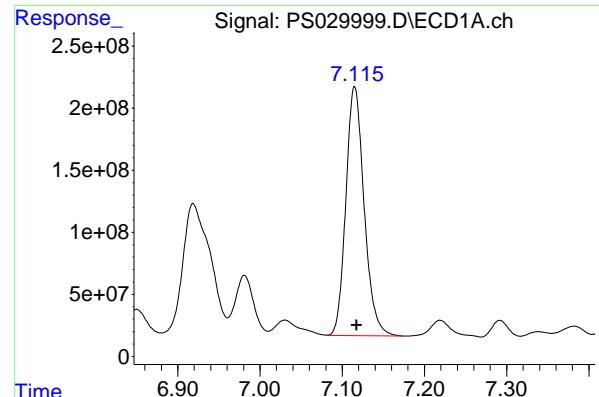

## #5 DICAMBA

R.T.: 7.115 min  
Delta R.T.: -0.003 min  
Instrument: ECD\_S  
Response: 3104526552  
Conc: 313.50 ng/ml  
ClientSampleId: WC-5MS

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
Supervised By :mohammad ahmed 05/02/2025

## #5 DICAMBA





R.T.: 7.647 min  
Delta R.T.: -0.006 min  
Response: 1301192862  
Conc: 329.41 ng/ml

## #6 MCPP

R.T.: 7.292 min  
Delta R.T.: -0.009 min  
Response: 169114247  
Conc: 26.25 ug/ml

## #6 MCPP

R.T.: 7.739 min  
Delta R.T.: -0.026 min  
Response: 167616033  
Conc: 95.84 ug/ml

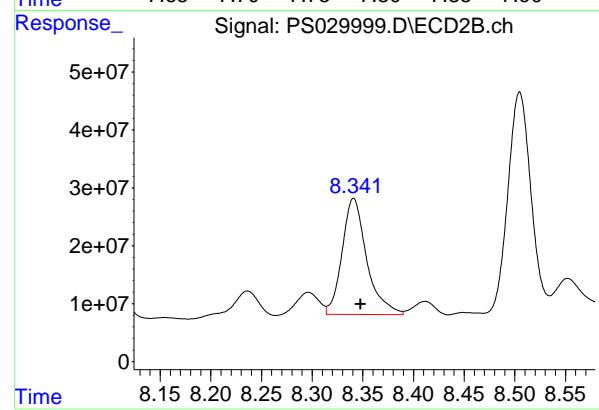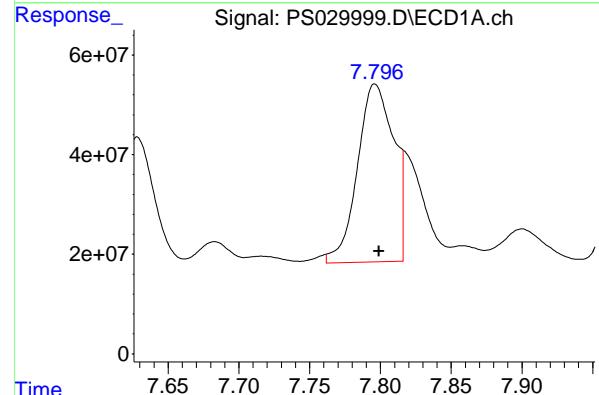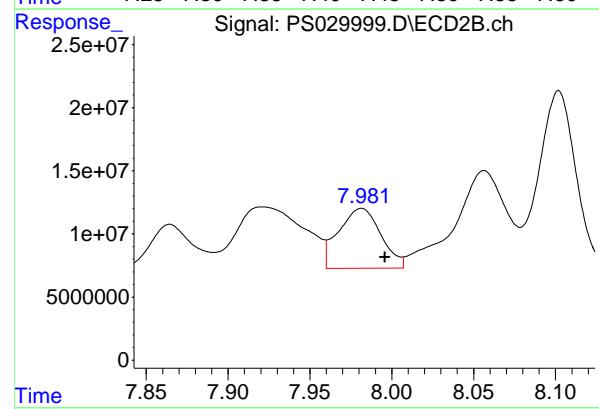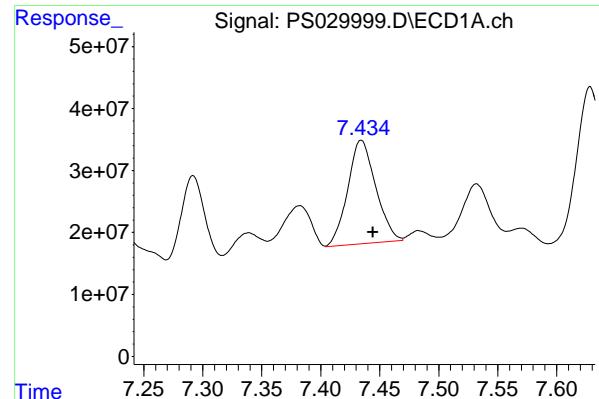

#7 MCPA

R.T.: 7.434 min  
 Delta R.T.: -0.010 min  
 Response: 275866896  
 Conc: 31.24 ug/ml

Instrument: ECD\_S  
 ClientSampleId: WC-5MS

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

#7 MCPA





R.T.: 7.981 min  
 Delta R.T.: -0.014 min  
 Response: 85484678  
 Conc: 36.13 ug/ml

#8 DICHLORPROP

R.T.: 7.796 min  
 Delta R.T.: -0.003 min  
 Response: 648094351  
 Conc: 255.75 ng/ml

#8 DICHLORPROP

R.T.: 8.341 min  
 Delta R.T.: -0.007 min  
 Response: 340201612  
 Conc: 338.86 ng/ml

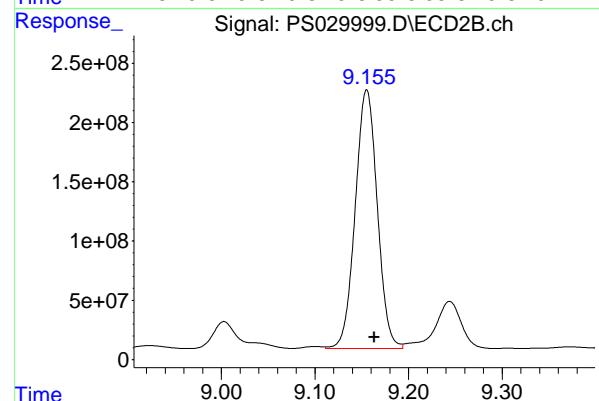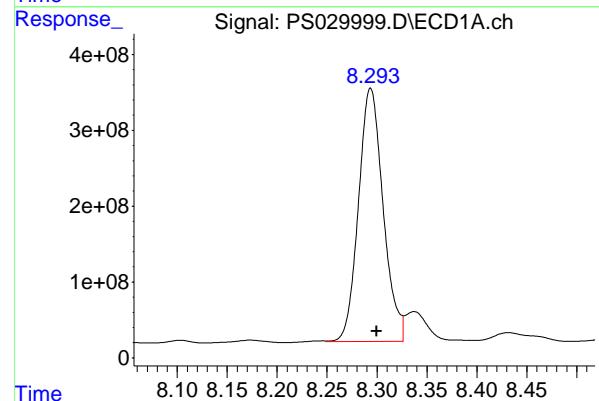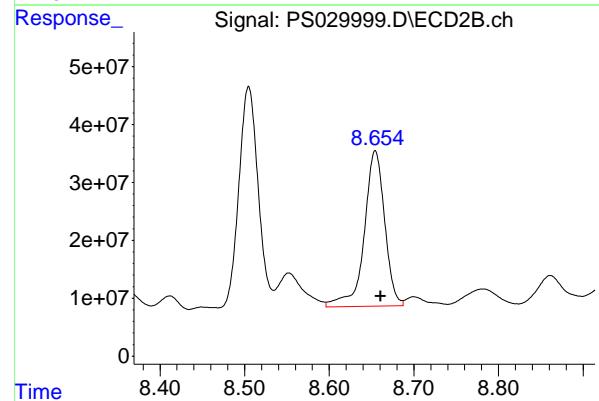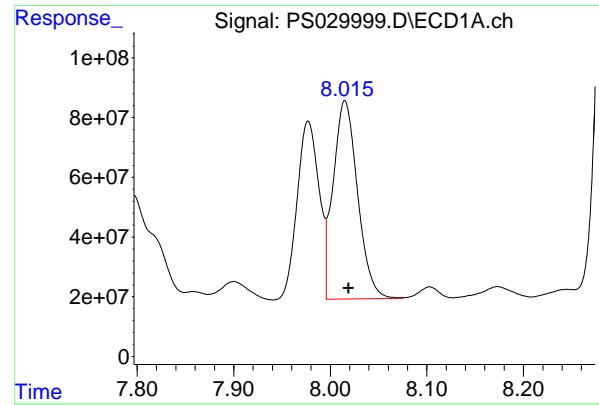

#9 2,4-D

R.T.: 8.015 min  
 Delta R.T.: -0.004 min  
 Response: 1168343085 ECD\_S  
 Conc: 415.36 ng/ml Client Sample ID : WC-5MS

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

#9 2,4-D





R.T.: 8.654 min  
 Delta R.T.: -0.007 min  
 Response: 453157976  
 Conc: 402.05 ng/ml

#10 Pentachlorophenol

R.T.: 8.293 min  
 Delta R.T.: -0.006 min  
 Response: 5741459866  
 Conc: 164.58 ng/ml

#10 Pentachlorophenol

R.T.: 9.155 min  
 Delta R.T.: -0.008 min  
 Response: 3568229586  
 Conc: 175.39 ng/ml

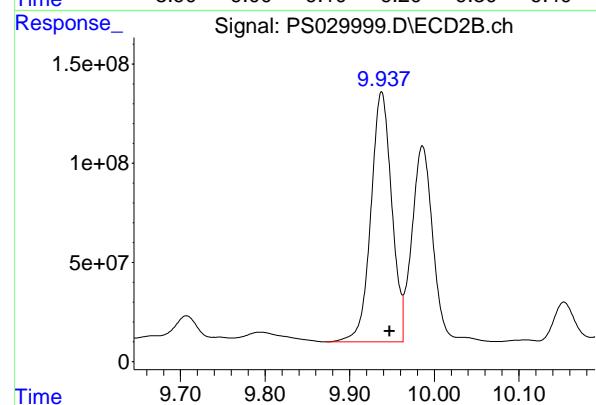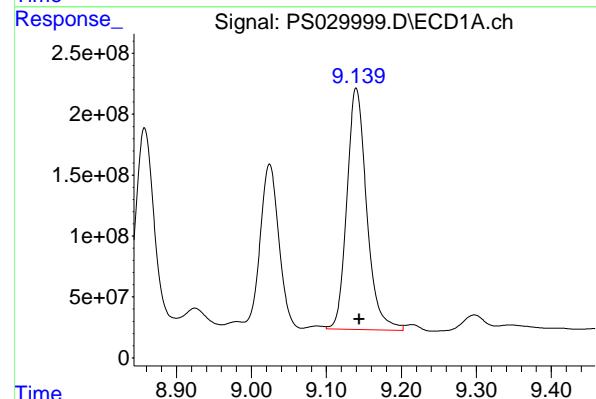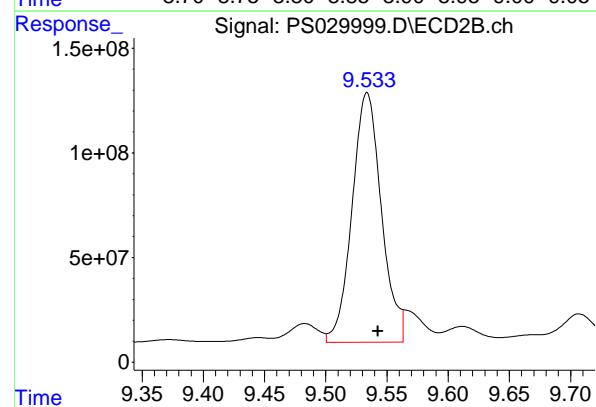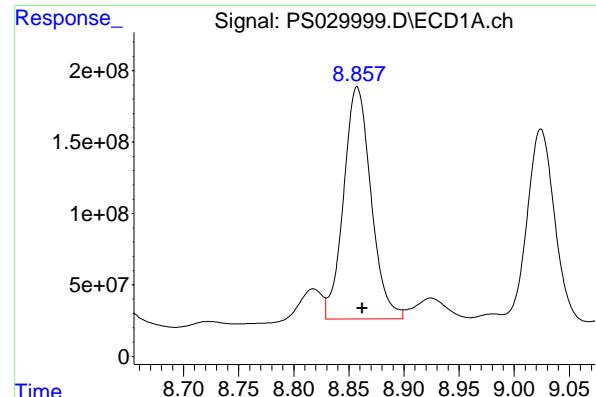

#11 2,4,5-TP (SILVEX)

R.T.: 8.857 min

Delta R.T.: -0.005 min

Instrument: ECD\_S

Response: 2807170683

Conc: 202.50 ng/ml

ClientSampleId: WC-5MS

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
Supervised By :mohammad ahmed 05/02/2025

#11 2,4,5-TP (SILVEX)

R.T.: 9.533 min

Delta R.T.: -0.009 min

Response: 1987477002

Conc: 242.92 ng/ml

#12 2,4,5-T

R.T.: 9.140 min

Delta R.T.: -0.004 min

Response: 3632188453

Conc: 258.46 ng/ml


#12 2,4,5-T

R.T.: 9.938 min

Delta R.T.: -0.010 min

Response: 2158849749

Conc: 278.11 ng/ml

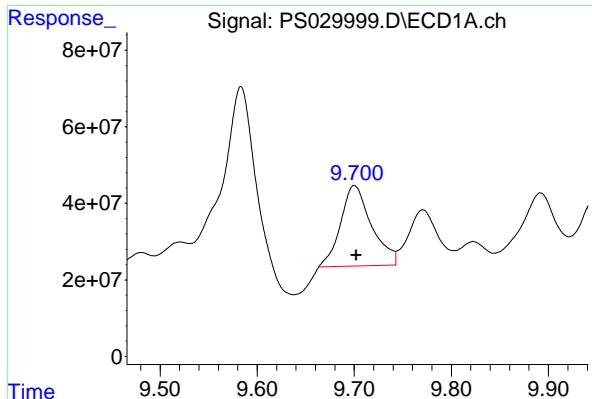


#13 2,4-DB

R.T.: 9.700 min  
 Delta R.T.: -0.002 min  
 Response: 469054192 ECD\_S  
 Conc: 205.24 ng/ml ClientSampleId : WC-5MS


Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

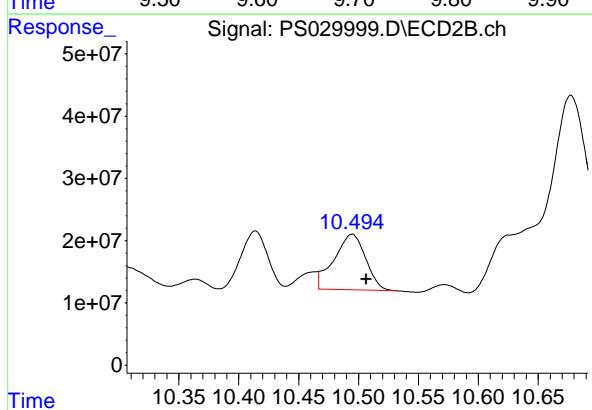


#13 2,4-DB

R.T.: 10.494 min  
 Delta R.T.: -0.012 min  
 Response: 163646510  
 Conc: 203.33 ng/ml

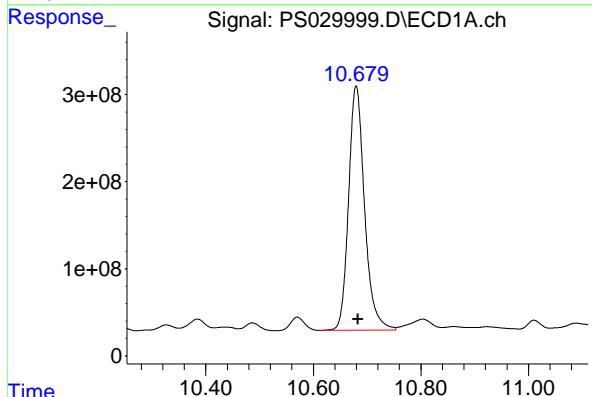


#15 Picloram

R.T.: 10.680 min  
 Delta R.T.: -0.004 min  
 Response: 5787594197  
 Conc: 315.73 ng/ml

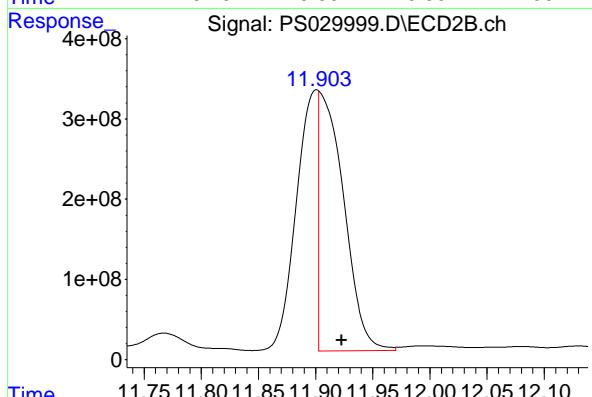

#15 Picloram

R.T.: 11.903 min  
 Delta R.T.: -0.020 min  
 Response: 4817867384  
 Conc: 392.22 ng/ml

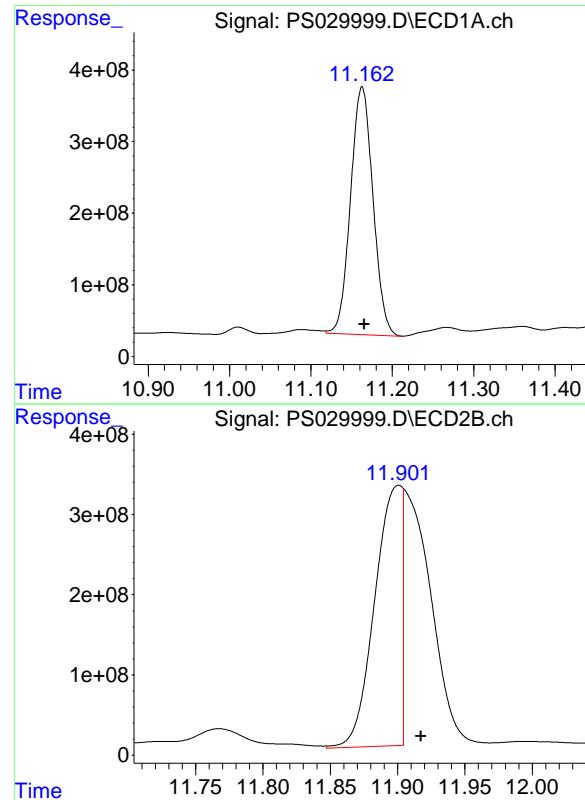

#16 DCPA

R.T.: 11.162 min  
 Delta R.T.: -0.004 min  
 Response: 6627935599 ECD\_S  
 Conc: 389.40 ng/ml Client Sample ID : WC-5MS

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14
- 15
- 16
- 17
- 18
- 19
- 20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Nobis Group			Date Collected:	04/28/25	
Project:	Raymark Superfund Site			Date Received:	04/28/25	
Client Sample ID:	WC-5MSD			SDG No.:	Q1883	
Lab Sample ID:	Q1906-05MSD			Matrix:	SOIL	
Analytical Method:	SW8151A			% Solid:	83.5	Decanted:
Sample Wt/Vol:	30.04	Units:	g	Final Vol:	10000	uL
Soil Aliquot Vol:	uL			Test:	Herbicide Group1	
Extraction Type:				Injection Volume :		
GPC Factor :	1.0	PH :				
Prep Method :	8151A					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PS030000.D	1	04/30/25 08:50	05/01/25 04:58	PB167796

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units(Dry Weight)
<b>TARGETS</b>							
1918-00-9	DICAMBA	0.13		0.0093	0.040	0.080	mg/Kg
75-99-0	DALAPON	0.38	P	0.021	0.060	0.080	mg/Kg
120-36-5	DICHLORPROP	0.14	P	0.015	0.040	0.080	mg/Kg
94-75-7	2,4-D	0.17		0.011	0.040	0.080	mg/Kg
93-72-1	2,4,5-TP (Silvex)	0.10		0.011	0.040	0.080	mg/Kg
93-76-5	2,4,5-T	0.11		0.010	0.040	0.080	mg/Kg
94-82-6	2,4-DB	0.085		0.029	0.040	0.080	mg/Kg
88-85-7	DINOSEB	0.040	U	0.013	0.040	0.080	mg/Kg
<b>SURROGATES</b>							
19719-28-9	2,4-DCAA	1540	*	27 - 122		308%	SPK: 500

Comments:

U = Not Detected  
 LOQ = Limit of Quantitation  
 MDL = Method Detection Limit  
 LOD = Limit of Detection  
 E = Value Exceeds Calibration Range  
 P = Indicates >25% difference for detected concentrations between the two GC columns  
 Q = indicates LCS control criteria did not meet requirements  
 M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value  
 B = Analyte Found in Associated Method Blank  
 N = Presumptive Evidence of a Compound  
 \* = Values outside of QC limits  
 D = Dilution  
 S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.  
 () = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS030000.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 04:58  
 Operator : AR\AJ  
 Sample : Q1906-05MSD  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 WC-5MSD

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 01 05:15:48 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

**System Monitoring Compounds**

4) S 2,4-DCAA 6.919 7.462 2383.8E6 1086.7E6 968.580 1542.476 #

**Target Compounds**

1) T	Dalapon	2.443	2.516	2684.7E6	1670.2E6	655.570	962.008	#
2) T	3,5-DICHL...	6.142	6.459	1091.5E6	282.0E6	305.432m	288.501	
3) T	4-Nitroph...	6.705	6.965	111.4E6	93163381	62.467	121.636m#	
5) T	DICAMBA	7.114	7.648	3137.2E6	1321.2E6	316.802m	334.474	
6) T	MCPP	7.292	7.738	166.7E6	168.2E6	25.863	96.144	#
7) T	MCPA	7.434	7.982	275.0E6	84049137	31.136	35.527	
8) T	DICHLORPROP	7.795	8.341	637.3E6	345.5E6	251.505m	344.094	#
9) T	2,4-D	8.015	8.654	1183.7E6	461.4E6	420.814	409.339	
10) T	Pentachlo...	8.293	9.155	5829.4E6	3626.2E6	167.103	178.239	
11) T	2,4,5-TP ...	8.857	9.533	2881.3E6	2060.0E6	207.846m	251.776m	
12) T	2,4,5-T	9.140	9.937	3680.4E6	2208.5E6	261.892	284.499	
13) T	2,4-DB	9.700	10.493	414.0E6	170.6E6	181.138m	212.019m	
15) T	Picloram	10.679	11.904	5832.1E6	4481.7E6	318.161	364.849m	
16) T	DCPA	11.162	11.900	6578.7E6	3900.7E6	386.502	346.066m	

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS030000.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 04:58  
 Operator : AR\AJ  
 Sample : Q1906-05MSD  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1



Instrument :  
 ECD\_S  
 ClientSampleId :  
 WC-5MSD



**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 01 05:15:48 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

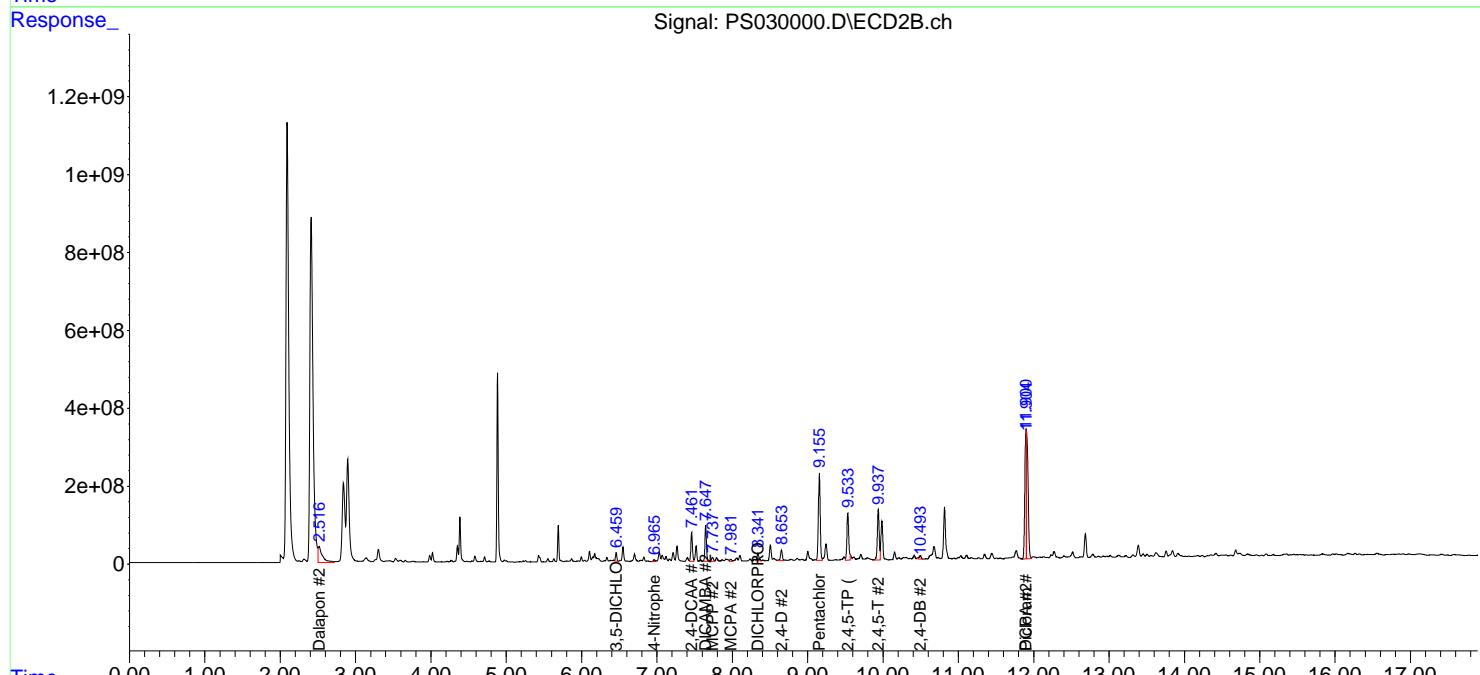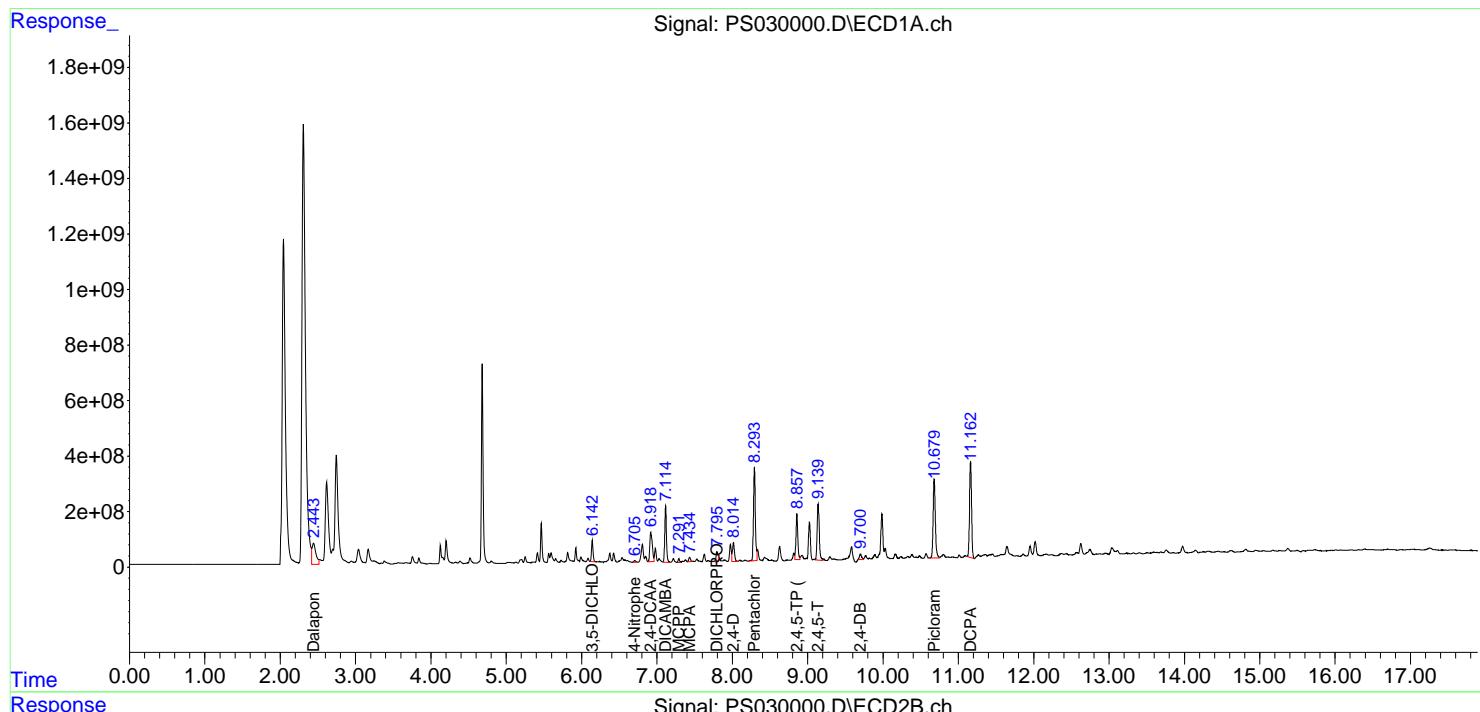

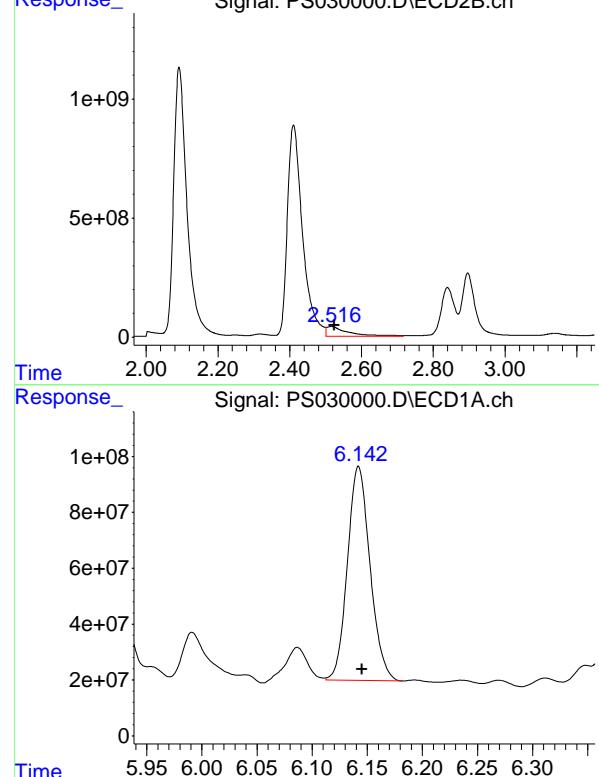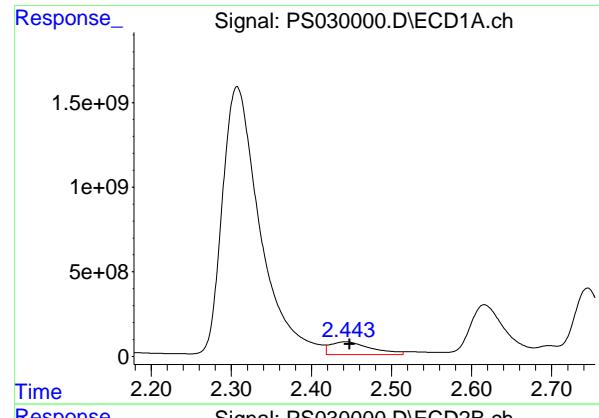

#1 Dalapon

R.T.: 2.443 min  
 Delta R.T.: -0.005 min  
 Response: 2684729749 ECD\_S  
 Conc: 655.57 ng/ml Client SampleId : WC-5MSD

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

#1 Dalapon





R.T.: 2.516 min  
 Delta R.T.: -0.008 min  
 Response: 1670184214  
 Conc: 962.01 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.142 min  
 Delta R.T.: -0.004 min  
 Response: 1091547420  
 Conc: 305.43 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.459 min  
 Delta R.T.: -0.004 min  
 Response: 282032989  
 Conc: 288.50 ng/ml

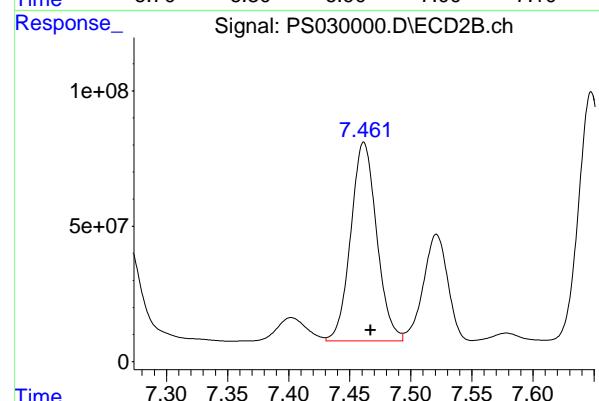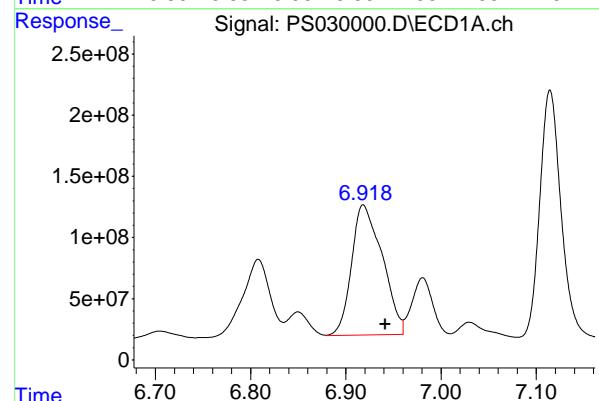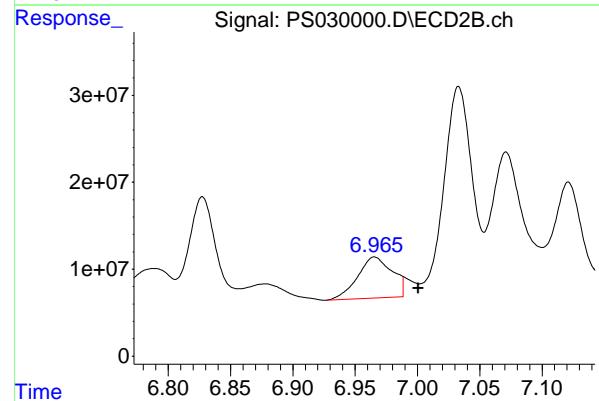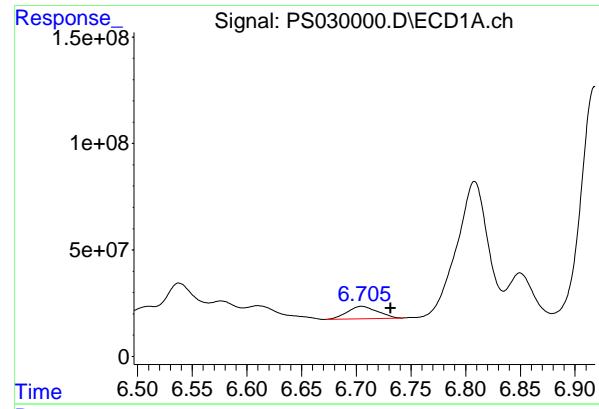

## #3 4-Nitrophenol

R.T.: 6.705 min  
Delta R.T.: -0.026 min  
Response: 111398988 ECD\_S  
Conc: 62.47 ng/ml Client Sample ID : WC-5MSD

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
Supervised By :mohammad ahmed 05/02/2025

## #3 4-Nitrophenol


R.T.: 6.965 min  
Delta R.T.: -0.036 min  
Response: 93163381  
Conc: 121.64 ng/ml

## #4 2,4-DCAA

R.T.: 6.919 min  
Delta R.T.: -0.023 min  
Response: 2383750734  
Conc: 968.58 ng/ml

## #4 2,4-DCAA

R.T.: 7.462 min  
Delta R.T.: -0.005 min  
Response: 1086700629  
Conc: 1542.48 ng/ml

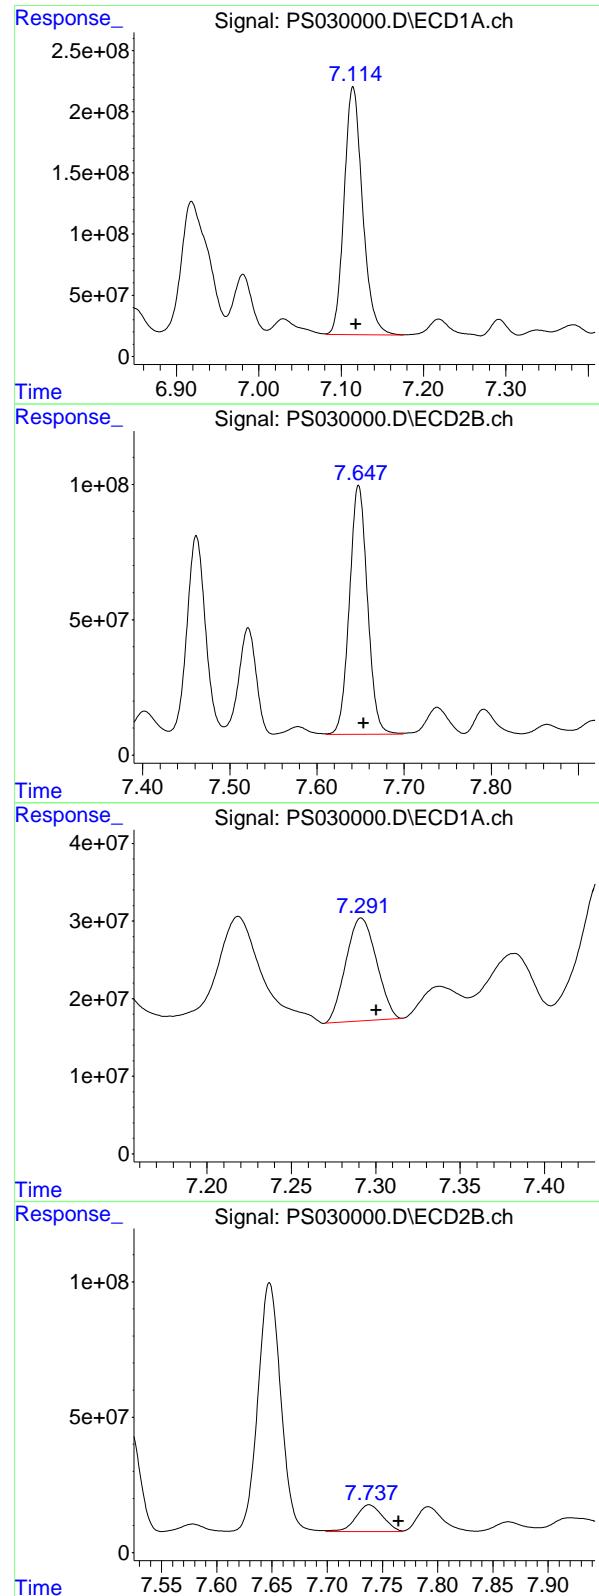

## #5 DICAMBA

R.T.: 7.114 min  
 Delta R.T.: -0.004 min  
 Response: 3137245760 ECD\_S  
 Conc: 316.80 ng/ml Client SampleId : WC-5MSD

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

## #5 DICAMBA


R.T.: 7.648 min  
 Delta R.T.: -0.006 min  
 Response: 1321193549  
 Conc: 334.47 ng/ml

## #6 MCPP

R.T.: 7.292 min  
 Delta R.T.: -0.009 min  
 Response: 166652078  
 Conc: 25.86 ug/ml

## #6 MCPP

R.T.: 7.738 min  
 Delta R.T.: -0.027 min  
 Response: 168151316  
 Conc: 96.14 ug/ml

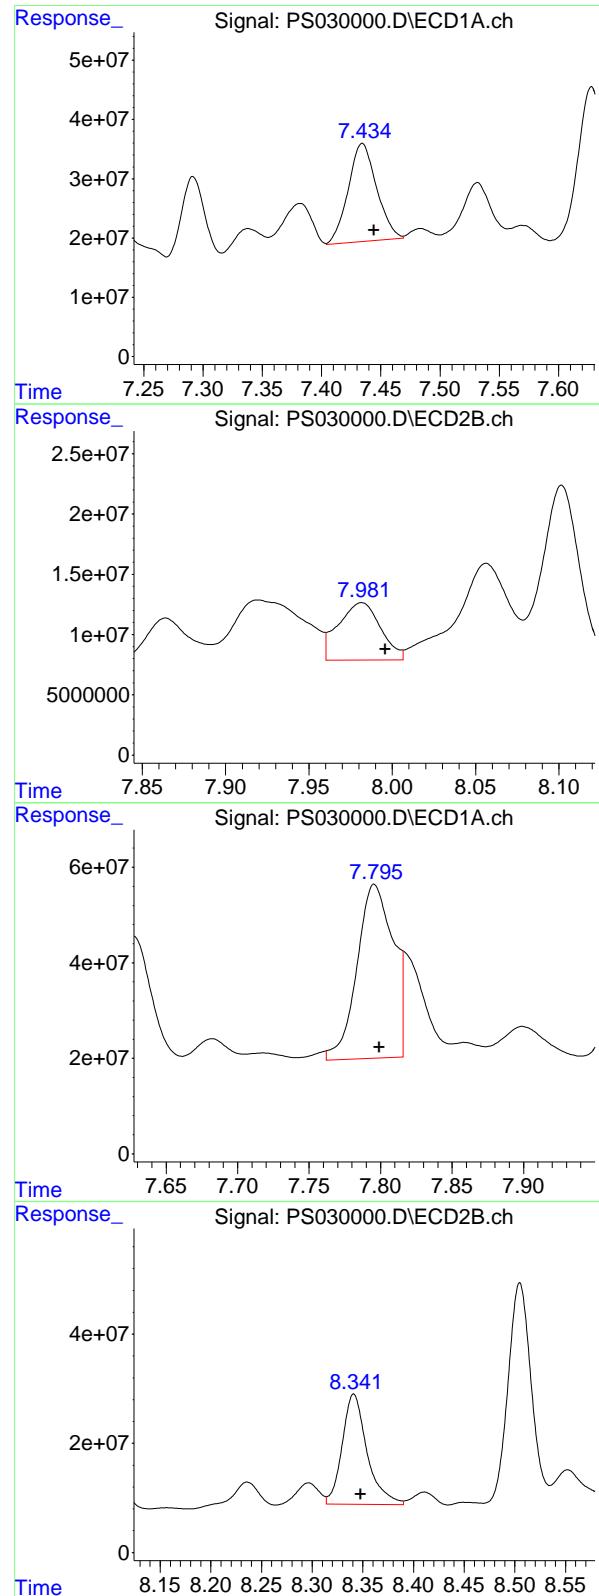

#7 MCPA

R.T.: 7.434 min  
 Delta R.T.: -0.010 min  
 Response: 274972414 ECD\_S  
 Conc: 31.14 ug/ml Client SampleId : WC-5MSD

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

#7 MCPA





R.T.: 7.982 min  
 Delta R.T.: -0.014 min  
 Response: 84049137  
 Conc: 35.53 ug/ml

#8 DICHLORPROP

R.T.: 7.795 min  
 Delta R.T.: -0.004 min  
 Response: 637341151  
 Conc: 251.51 ng/ml

#8 DICHLORPROP

R.T.: 8.341 min  
 Delta R.T.: -0.007 min  
 Response: 345457932  
 Conc: 344.09 ng/ml

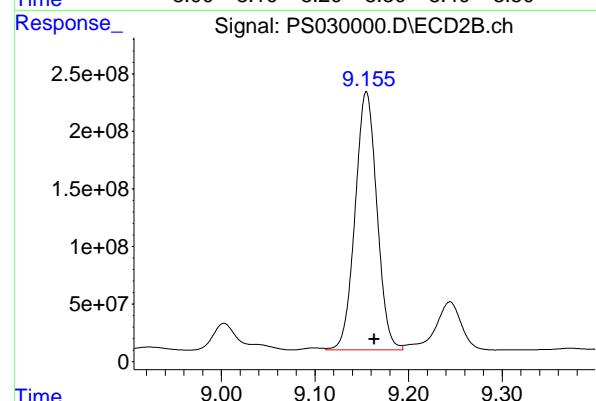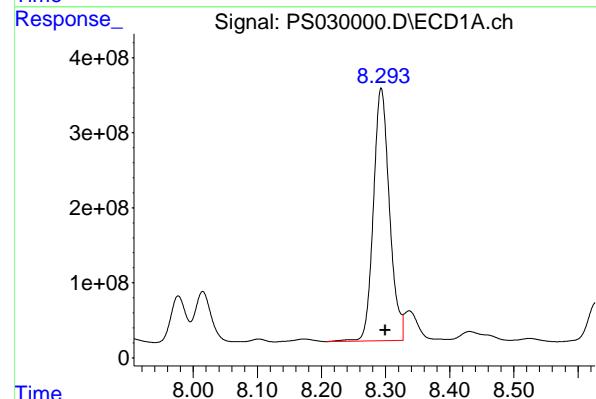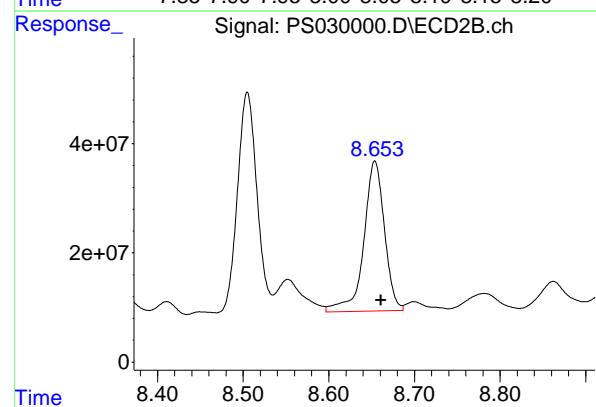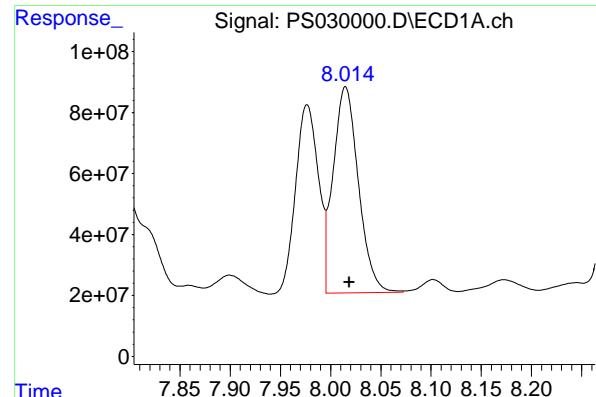

#9 2,4-D

R.T.: 8.015 min  
 Delta R.T.: -0.004 min  
 Response: 1183696641 ECD\_S  
 Conc: 420.81 ng/ml Client SampleId : WC-5MSD

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

#9 2,4-D


R.T.: 8.654 min  
 Delta R.T.: -0.007 min  
 Response: 461368615  
 Conc: 409.34 ng/ml

#10 Pentachlorophenol

R.T.: 8.293 min  
 Delta R.T.: -0.006 min  
 Response: 5829372536  
 Conc: 167.10 ng/ml

#10 Pentachlorophenol

R.T.: 9.155 min  
 Delta R.T.: -0.009 min  
 Response: 3626233908  
 Conc: 178.24 ng/ml

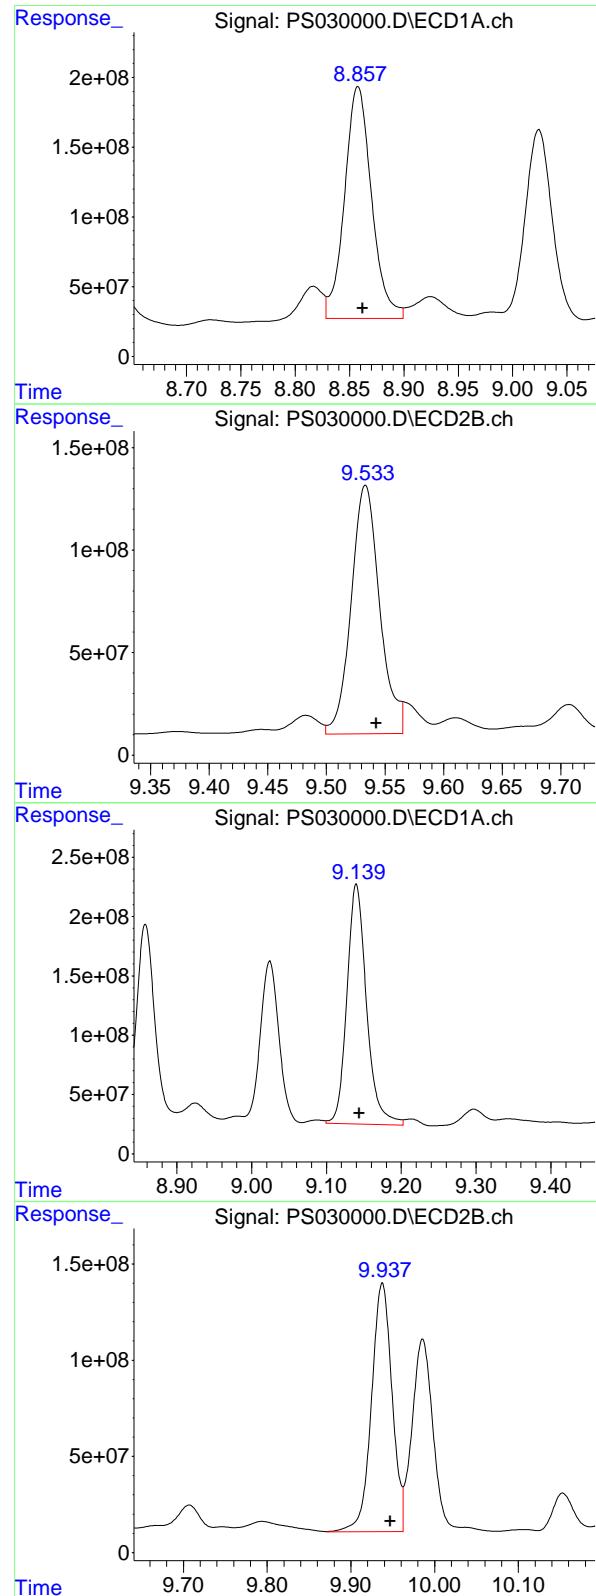

#11 2,4,5-TP (SILVEX)

R.T.: 8.857 min

Delta R.T.: -0.005 min

Instrument: ECD\_S

Response: 2881331277

Conc: 207.85 ng/ml

ClientSampleId: WC-5MSD

**Manual Integrations**  
**APPROVED**

Reviewed By :Abdul Mirza 05/01/2025

Supervised By :mohammad ahmed 05/02/2025

#11 2,4,5-TP (SILVEX)

R.T.: 9.533 min

Delta R.T.: -0.010 min

Response: 2059964649

Conc: 251.78 ng/ml

#12 2,4,5-T

R.T.: 9.140 min

Delta R.T.: -0.004 min

Response: 3680396485

Conc: 261.89 ng/ml


#12 2,4,5-T

R.T.: 9.937 min

Delta R.T.: -0.010 min

Response: 2208455612

Conc: 284.50 ng/ml

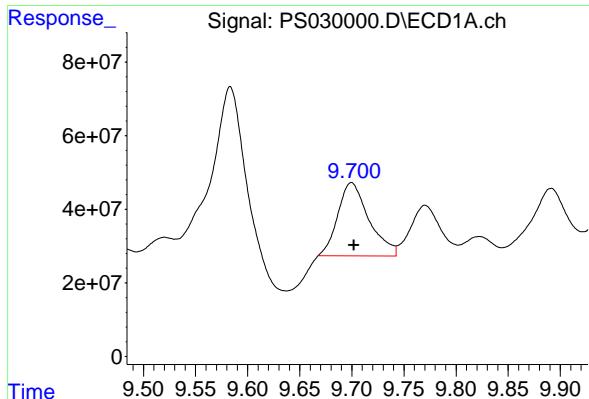


#13 2,4-DB

R.T.: 9.700 min  
 Delta R.T.: -0.002 min  
 Response: 413963725  
 Conc: 181.14 ng/ml

Instrument: ECD\_S  
 Client SampleId: WC-5MSD


Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

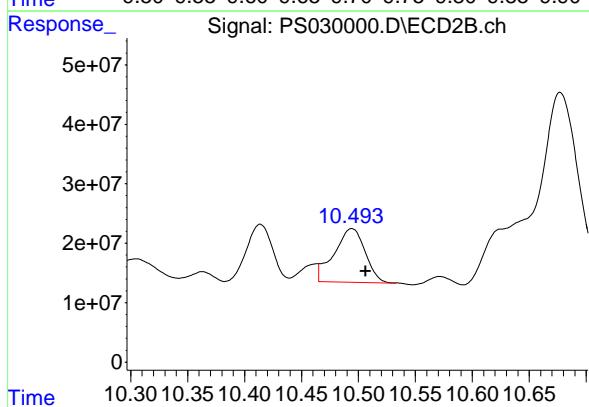


#13 2,4-DB

R.T.: 10.493 min  
 Delta R.T.: -0.013 min  
 Response: 170641685  
 Conc: 212.02 ng/ml

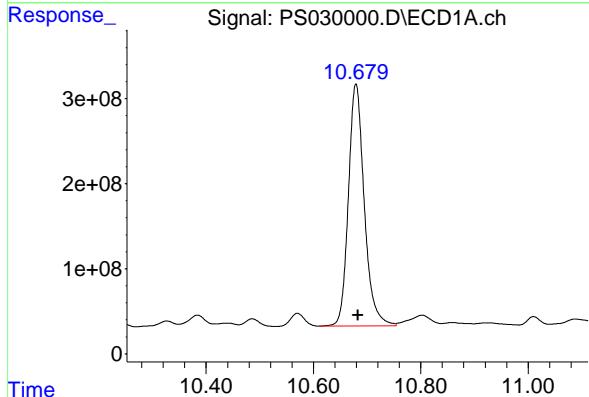


#15 Picloram

R.T.: 10.679 min  
 Delta R.T.: -0.004 min  
 Response: 5832090919  
 Conc: 318.16 ng/ml

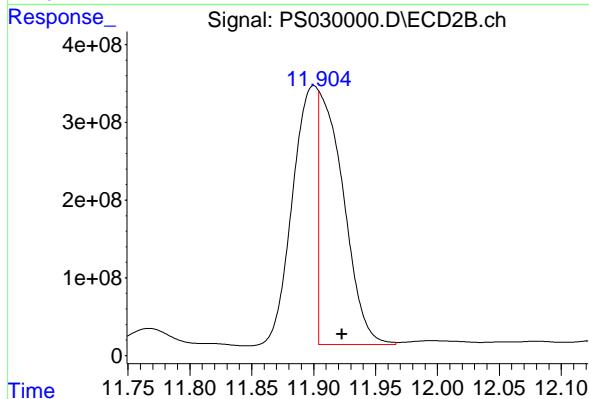

#15 Picloram

R.T.: 11.904 min  
 Delta R.T.: -0.019 min  
 Response: 4481672472  
 Conc: 364.85 ng/ml

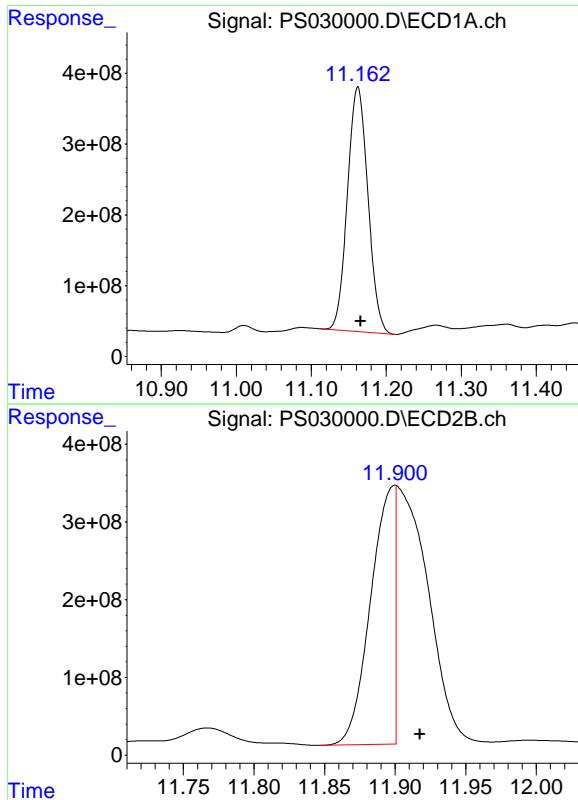

#16 DCPA

R.T.: 11.162 min  
 Delta R.T.: -0.004 min  
 Response: 6578656178 ECD\_S  
 Conc: 386.50 ng/ml Client Sample ID : WC-5MSD

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 05/01/2025  
 Supervised By :mohammad ahmed 05/02/2025

#16 DCPA

R.T.: 11.900 min  
 Delta R.T.: -0.018 min  
 Response: 3900733580  
 Conc: 346.07 ng/ml

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

### Manual Integration Report

Sequence:	PS042325	Instrument	ECD_s
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
HSTDICC200	PS029919.D	Dalapon	Abdul	4/24/2025 8:49:48 AM	mohammad	4/26/2025 2:18:24	Peak Integrated by Software
HSTDICC200	PS029919.D	DCPA #2	Abdul	4/24/2025 8:49:48 AM	mohammad	4/26/2025 2:18:24	Peak Integrated by Software
HSTDICC200	PS029919.D	Picloram #2	Abdul	4/24/2025 8:49:48 AM	mohammad	4/26/2025 2:18:24	Peak Integrated by Software
HSTDICC500	PS029920.D	DCPA #2	Abdul	4/24/2025 8:49:52 AM	mohammad	4/26/2025 2:18:24	Peak Integrated by Software
HSTDICC500	PS029920.D	Picloram #2	Abdul	4/24/2025 8:49:52 AM	mohammad	4/26/2025 2:18:24	Peak Integrated by Software
HSTDICC750	PS029921.D	DCPA #2	Abdul	4/24/2025 8:49:56 AM	mohammad	4/26/2025 2:18:24	Peak Integrated by Software
HSTDICC750	PS029921.D	Picloram #2	Abdul	4/24/2025 8:49:56 AM	mohammad	4/26/2025 2:18:24	Peak Integrated by Software
HSTDICC1000	PS029922.D	DCPA #2	Abdul	4/24/2025 8:49:59 AM	mohammad	4/26/2025 2:18:24	Peak Integrated by Software
HSTDICC1000	PS029922.D	Picloram #2	Abdul	4/24/2025 8:49:59 AM	mohammad	4/26/2025 2:18:24	Peak Integrated by Software
HSTDICC1500	PS029923.D	DCPA #2	Abdul	4/24/2025 8:50:02 AM	mohammad	4/26/2025 2:18:24	Peak Integrated by Software
HSTDICC1500	PS029923.D	Picloram #2	Abdul	4/24/2025 8:50:02 AM	mohammad	4/26/2025 2:18:24	Peak Integrated by Software
HSTDICV750	PS029924.D	DCPA #2	Abdul	4/24/2025 8:50:06 AM	mohammad	4/26/2025 2:18:24	Peak Integrated by Software
HSTDICV750	PS029924.D	Picloram #2	Abdul	4/24/2025 8:50:06 AM	mohammad	4/26/2025 2:18:24	Peak Integrated by Software

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

## Manual Integration Report

Sequence:	PS042325	Instrument	ECD_s
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
HSTDCCC750	PS029926.D	DCPA #2	Abdul	4/24/2025 8:50:10 AM	mohammad	4/26/2025 2:18:24	Peak Integrated by Software
HSTDCCC750	PS029926.D	Picloram #2	Abdul	4/24/2025 8:50:10 AM	mohammad	4/26/2025 2:18:24	Peak Integrated by Software
HSTDCCC750	PS029935.D	DCPA #2	Abdul	4/24/2025 8:50:13 AM	mohammad	4/26/2025 2:18:24	Peak Integrated by Software
HSTDCCC750	PS029935.D	Picloram #2	Abdul	4/24/2025 8:50:13 AM	mohammad	4/26/2025 2:18:24	Peak Integrated by Software
HSTDCCC750	PS029943.D	DCPA #2	Abdul	4/24/2025 8:50:32 AM	mohammad	4/26/2025 2:18:24	Peak Integrated by Software
HSTDCCC750	PS029943.D	Picloram #2	Abdul	4/24/2025 8:50:32 AM	mohammad	4/26/2025 2:18:24	Peak Integrated by Software
HSTDCCC750	PS029954.D	DCPA #2	Abdul	4/24/2025 8:50:56 AM	mohammad	4/26/2025 2:18:24	Peak Integrated by Software
HSTDCCC750	PS029954.D	DICAMBA #2	Abdul	4/24/2025 8:50:56 AM	mohammad	4/26/2025 2:18:24	Peak Integrated by Software
HSTDCCC750	PS029954.D	MCPP #2	Abdul	4/24/2025 8:50:56 AM	mohammad	4/26/2025 2:18:24	Peak Integrated by Software
HSTDCCC750	PS029954.D	Picloram #2	Abdul	4/24/2025 8:50:56 AM	mohammad	4/26/2025 2:18:24	Peak Integrated by Software

### Manual Integration Report

Sequence:	ps043025	Instrument	ECD_s
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
HSTDCCC750	PS029991.D	DCPA #2	Abdul	5/1/2025 8:10:54 AM	mohammad	5/2/2025 3:20:13	Peak Integrated by Software
HSTDCCC750	PS029991.D	Picloram #2	Abdul	5/1/2025 8:10:54 AM	mohammad	5/2/2025 3:20:13	Peak Integrated by Software
Q1906-05MS	PS029999.D	2,4,5-TP (SILVEX)	Abdul	5/1/2025 8:11:19 AM	mohammad	5/2/2025 3:20:33	Peak Integrated by Software
Q1906-05MS	PS029999.D	2,4,5-TP (SILVEX) #2	Abdul	5/1/2025 8:11:19 AM	mohammad	5/2/2025 3:20:33	Peak Integrated by Software
Q1906-05MS	PS029999.D	2,4-DB	Abdul	5/1/2025 8:11:19 AM	mohammad	5/2/2025 3:20:33	Peak Integrated by Software
Q1906-05MS	PS029999.D	2,4-DB #2	Abdul	5/1/2025 8:11:19 AM	mohammad	5/2/2025 3:20:33	Peak Integrated by Software
Q1906-05MS	PS029999.D	3,5-DICHLOROBENZOIC ACID	Abdul	5/1/2025 8:11:19 AM	mohammad	5/2/2025 3:20:33	Peak Integrated by Software
Q1906-05MS	PS029999.D	4-Nitrophenol #2	Abdul	5/1/2025 8:11:19 AM	mohammad	5/2/2025 3:20:33	Peak Integrated by Software
Q1906-05MS	PS029999.D	DCPA	Abdul	5/1/2025 8:11:19 AM	mohammad	5/2/2025 3:20:33	Peak Integrated by Software
Q1906-05MS	PS029999.D	DCPA #2	Abdul	5/1/2025 8:11:19 AM	mohammad	5/2/2025 3:20:33	Peak Integrated by Software
Q1906-05MS	PS029999.D	DICAMBA	Abdul	5/1/2025 8:11:19 AM	mohammad	5/2/2025 3:20:33	Peak Integrated by Software
Q1906-05MS	PS029999.D	DICHLORPROP	Abdul	5/1/2025 8:11:19 AM	mohammad	5/2/2025 3:20:33	Peak Integrated by Software
Q1906-05MS	PS029999.D	Pentachlorophenol	Abdul	5/1/2025 8:11:19 AM	mohammad	5/2/2025 3:20:33	Peak Integrated by Software

### Manual Integration Report

Sequence:	ps043025	Instrument	ECD_s
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
Q1906-05MS	PS029999.D	Picloram #2	Abdul	5/1/2025 8:11:19 AM	mohammad	5/2/2025 3:20:33	Peak Integrated by Software
Q1906-05MSD	PS030000.D	2,4,5-TP (SILVEX)	Abdul	5/1/2025 8:11:24 AM	mohammad	5/2/2025 3:20:35	Peak Integrated by Software
Q1906-05MSD	PS030000.D	2,4,5-TP (SILVEX) #2	Abdul	5/1/2025 8:11:24 AM	mohammad	5/2/2025 3:20:35	Peak Integrated by Software
Q1906-05MSD	PS030000.D	2,4-DB	Abdul	5/1/2025 8:11:24 AM	mohammad	5/2/2025 3:20:35	Peak Integrated by Software
Q1906-05MSD	PS030000.D	2,4-DB #2	Abdul	5/1/2025 8:11:24 AM	mohammad	5/2/2025 3:20:35	Peak Integrated by Software
Q1906-05MSD	PS030000.D	3,5-DICHLOROBENZOIC ACID	Abdul	5/1/2025 8:11:24 AM	mohammad	5/2/2025 3:20:35	Peak Integrated by Software
Q1906-05MSD	PS030000.D	4-Nitrophenol #2	Abdul	5/1/2025 8:11:24 AM	mohammad	5/2/2025 3:20:35	Peak Integrated by Software
Q1906-05MSD	PS030000.D	DCPA #2	Abdul	5/1/2025 8:11:24 AM	mohammad	5/2/2025 3:20:35	Peak Integrated by Software
Q1906-05MSD	PS030000.D	DICAMBA	Abdul	5/1/2025 8:11:24 AM	mohammad	5/2/2025 3:20:35	Peak Integrated by Software
Q1906-05MSD	PS030000.D	DICHLORPROP	Abdul	5/1/2025 8:11:24 AM	mohammad	5/2/2025 3:20:35	Peak Integrated by Software
Q1906-05MSD	PS030000.D	Picloram #2	Abdul	5/1/2025 8:11:24 AM	mohammad	5/2/2025 3:20:35	Peak Integrated by Software
HSTDCCC750	PS030002.D	DCPA #2	Abdul	5/1/2025 8:11:29 AM	mohammad	5/2/2025 3:20:38	Peak Integrated by Software
HSTDCCC750	PS030002.D	Picloram #2	Abdul	5/1/2025 8:11:29 AM	mohammad	5/2/2025 3:20:38	Peak Integrated by Software

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

## Manual Integration Report

Sequence:	ps043025	Instrument	ECD_s
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
HSTDCCC750	PS030013.D	DCPA #2	Abdul	5/2/2025 8:26:37 AM	mohammad	5/5/2025 4:31:22	Peak Integrated by Software
HSTDCCC750	PS030013.D	Picloram #2	Abdul	5/2/2025 8:26:37 AM	mohammad	5/5/2025 4:31:22	Peak Integrated by Software

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

## Manual Integration Report

Sequence:	PS050125	Instrument	ECD_s
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
HSTDCCC750	PS030016.D	DCPA #2	Abdul	5/2/2025 8:18:06 AM	mohammad	5/5/2025 4:41:45	Peak Integrated by Software
HSTDCCC750	PS030016.D	Picloram #2	Abdul	5/2/2025 8:18:06 AM	mohammad	5/5/2025 4:41:45	Peak Integrated by Software
Q1883-01	PS030017.D	2,4-DCAA	Abdul	5/2/2025 8:18:11 AM	mohammad	5/5/2025 4:41:47	Peak Integrated by Software
Q1883-01	PS030017.D	2,4-DCAA #2	Abdul	5/2/2025 8:18:11 AM	mohammad	5/5/2025 4:41:47	Peak Integrated by Software
Q1883-03	PS030018.D	2,4-DCAA	Abdul	5/2/2025 8:18:15 AM	mohammad	5/5/2025 4:41:49	Peak Integrated by Software
Q1883-03	PS030018.D	2,4-DCAA #2	Abdul	5/2/2025 8:18:15 AM	mohammad	5/5/2025 4:41:49	Peak Integrated by Software
Q1883-07	PS030020.D	2,4-DCAA	Abdul	5/2/2025 8:18:19 AM	mohammad	5/5/2025 4:41:51	Peak Integrated by Software
Q1883-07	PS030020.D	2,4-DCAA #2	Abdul	5/2/2025 8:18:19 AM	mohammad	5/5/2025 4:41:51	Peak Integrated by Software
Q1883-09	PS030021.D	2,4-DCAA	Abdul	5/2/2025 8:18:22 AM	mohammad	5/5/2025 4:41:54	Peak Integrated by Software
HSTDCCC750	PS030026.D	DCPA #2	Abdul	5/2/2025 8:18:28 AM	mohammad	5/5/2025 4:41:57	Peak Integrated by Software
HSTDCCC750	PS030026.D	Picloram #2	Abdul	5/2/2025 8:18:28 AM	mohammad	5/5/2025 4:41:57	Peak Integrated by Software

### Manual Integration Report

Sequence:	PS050525	Instrument	ECD_s
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
HSTDCCC750	PS030029.D	DCPA #2	Abdul	5/6/2025 8:15:03 AM	mohammad	5/7/2025 6:08:59	Peak Integrated by Software
HSTDCCC750	PS030029.D	Picloram #2	Abdul	5/6/2025 8:15:03 AM	mohammad	5/7/2025 6:08:59	Peak Integrated by Software
PB167796BS	PS030038.D	DCPA #2	Abdul	5/6/2025 8:15:22 AM	mohammad	5/7/2025 6:08:59	Peak Integrated by Software
PB167796BS	PS030038.D	Picloram #2	Abdul	5/6/2025 8:15:22 AM	mohammad	5/7/2025 6:08:59	Peak Integrated by Software
HSTDCCC750	PS030041.D	4-Nitrophenol #2	Abdul	5/6/2025 8:15:27 AM	mohammad	5/7/2025 6:08:59	Peak Integrated by Software
HSTDCCC750	PS030041.D	DCPA #2	Abdul	5/6/2025 8:15:27 AM	mohammad	5/7/2025 6:08:59	Peak Integrated by Software
HSTDCCC750	PS030041.D	Picloram #2	Abdul	5/6/2025 8:15:27 AM	mohammad	5/7/2025 6:08:59	Peak Integrated by Software
HSTDCCC750	PS030049.D	DCPA #2	Abdul	5/6/2025 8:15:36 AM	mohammad	5/7/2025 6:08:59	Peak Integrated by Software
HSTDCCC750	PS030049.D	Picloram #2	Abdul	5/6/2025 8:15:36 AM	mohammad	5/7/2025 6:08:59	Peak Integrated by Software

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

Instrument ID: ECD\_S

**Daily Analysis Runlog For Sequence/QCBatch ID # PS042325**

Review By	Abdul	Review On	4/24/2025 8:51:25 AM
Supervise By	mohammad	Supervise On	4/26/2025 2:18:24 AM
SubDirectory	PS042325	HP Acquire Method	HP Processing Method ps042325 8151
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24064,PP24065,PP24066,PP24067,PP24068		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24066 PP24069,PP24070		

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PS029917.D	23 Apr 2025 10:13	AR\AJ	Ok
2	I.BLK	PS029918.D	23 Apr 2025 10:37	AR\AJ	Ok
3	HSTDIICC200	PS029919.D	23 Apr 2025 11:01	AR\AJ	Ok,M
4	HSTDIICC500	PS029920.D	23 Apr 2025 11:25	AR\AJ	Ok,M
5	HSTDIICC750	PS029921.D	23 Apr 2025 11:49	AR\AJ	Ok,M
6	HSTDIICC1000	PS029922.D	23 Apr 2025 12:13	AR\AJ	Ok,M
7	HSTDIICC1500	PS029923.D	23 Apr 2025 12:37	AR\AJ	Ok,M
8	HSTDICV750	PS029924.D	23 Apr 2025 13:01	AR\AJ	Ok,M
9	I.BLK	PS029925.D	23 Apr 2025 13:25	AR\AJ	Ok
10	HSTDCCC750	PS029926.D	23 Apr 2025 13:50	AR\AJ	Ok,M
11	Q1842-06	PS029927.D	23 Apr 2025 14:14	AR\AJ	Ok
12	Q1842-12	PS029928.D	23 Apr 2025 14:38	AR\AJ	Ok
13	Q1842-18	PS029929.D	23 Apr 2025 15:02	AR\AJ	Ok
14	Q1842-24	PS029930.D	23 Apr 2025 15:26	AR\AJ	Ok
15	Q1842-30	PS029931.D	23 Apr 2025 15:50	AR\AJ	Ok
16	Q1842-36	PS029932.D	23 Apr 2025 16:14	AR\AJ	Ok
17	Q1842-42	PS029933.D	23 Apr 2025 16:38	AR\AJ	Ok
18	I.BLK	PS029934.D	23 Apr 2025 17:02	AR\AJ	Ok
19	HSTDCCC750	PS029935.D	23 Apr 2025 17:26	AR\AJ	Ok,M
20	Q1842-06MS	PS029936.D	23 Apr 2025 18:14	AR\AJ	Ok,M
21	Q1842-06MSD	PS029937.D	23 Apr 2025 18:38	AR\AJ	Ok,M

Instrument ID: ECD\_S

**Daily Analysis Runlog For Sequence/QCBatch ID # PS042325**

Review By	Abdul	Review On	4/24/2025 8:51:25 AM
Supervise By	mohammad	Supervise On	4/26/2025 2:18:24 AM
SubDirectory	PS042325	HP Acquire Method	HP Processing Method ps042325 8151
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24064,PP24065,PP24066,PP24067,PP24068		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24066 PP24069,PP24070		

22	PB167675BS	PS029938.D	23 Apr 2025 19:02	AR\AJ	Ok,M
23	PB167701BL	PS029939.D	23 Apr 2025 19:27	AR\AJ	Ok
24	PB167701BS	PS029940.D	23 Apr 2025 19:51	AR\AJ	Ok,M
25	PB167660TB	PS029941.D	23 Apr 2025 20:15	AR\AJ	Ok
26	I.BLK	PS029942.D	23 Apr 2025 20:39	AR\AJ	Ok
27	HSTDCCC750	PS029943.D	23 Apr 2025 21:03	AR\AJ	Ok,M
28	PB167710BL	PS029944.D	23 Apr 2025 21:51	AR\AJ	Ok
29	PB167710BS	PS029945.D	23 Apr 2025 22:15	AR\AJ	Ok,M
30	Q1850-01	PS029946.D	23 Apr 2025 22:39	AR\AJ	Ok
31	Q1852-01	PS029947.D	23 Apr 2025 23:03	AR\AJ	Ok
32	Q1852-03	PS029948.D	23 Apr 2025 23:27	AR\AJ	Ok
33	Q1852-05	PS029949.D	23 Apr 2025 23:51	AR\AJ	Ok,M
34	Q1852-07	PS029950.D	24 Apr 2025 00:15	AR\AJ	Ok,M
35	Q1852-07MS	PS029951.D	24 Apr 2025 00:39	AR\AJ	Ok,M
36	Q1852-07MSD	PS029952.D	24 Apr 2025 01:03	AR\AJ	Ok,M
37	I.BLK	PS029953.D	24 Apr 2025 01:27	AR\AJ	Ok
38	HSTDCCC750	PS029954.D	24 Apr 2025 04:15	AR\AJ	Ok,M

M : Manual Integration

Instrument ID: ECD\_S

**Daily Analysis Runlog For Sequence/QCBatch ID # PS043025**

Review By	Abdul	Review On	5/1/2025 8:12:26 AM
Supervise By	mohammad	Supervise On	5/2/2025 3:21:15 AM
SubDirectory	PS043025	HP Acquire Method	HP Processing Method ps042325 8151
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24064,PP24065,PP24066,PP24067,PP24068		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24066 PP24069,PP24070		

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PS029989.D	01 May 2025 00:34	AR\AJ	Ok
2	I.BLK	PS029990.D	01 May 2025 00:58	AR\AJ	Ok
3	HSTDCCC750	PS029991.D	01 May 2025 01:22	AR\AJ	Ok,M
4	PB167796BL	PS029992.D	01 May 2025 01:46	AR\AJ	Not Ok
5	PB167796BS	PS029993.D	01 May 2025 02:10	AR\AJ	Not Ok
6	Q1904-01	PS029994.D	01 May 2025 02:34	AR\AJ	Ok
7	Q1905-01	PS029995.D	01 May 2025 02:58	AR\AJ	Ok,M
8	Q1905-05	PS029996.D	01 May 2025 03:22	AR\AJ	Ok,M
9	Q1906-01	PS029997.D	01 May 2025 03:46	AR\AJ	Ok,M
10	Q1906-05	PS029998.D	01 May 2025 04:10	AR\AJ	Ok
11	Q1906-05MS	PS029999.D	01 May 2025 04:34	AR\AJ	Ok,M
12	Q1906-05MSD	PS030000.D	01 May 2025 04:58	AR\AJ	Ok,M
13	I.BLK	PS030001.D	01 May 2025 06:10	AR\AJ	Ok
14	HSTDCCC750	PS030002.D	01 May 2025 06:59	AR\AJ	Ok,M
15	Q1906-09	PS030003.D	01 May 2025 07:47	AR\AJ	Ok
16	Q1906-13	PS030004.D	01 May 2025 08:11	AR\AJ	Ok,M
17	Q1907-01	PS030005.D	01 May 2025 08:35	AR\AJ	Ok,M
18	Q1912-01	PS030006.D	01 May 2025 08:59	AR\AJ	Ok
19	Q1912-05	PS030007.D	01 May 2025 09:23	AR\AJ	Ok
20	Q1906-05RE	PS030008.D	01 May 2025 10:11	AR\AJ	Not Ok
21	Q1906-05MSRE	PS030009.D	01 May 2025 10:35	AR\AJ	Not Ok

Instrument ID: ECD\_S

**Daily Analysis Runlog For Sequence/QCBatch ID # PS043025**

Review By	Abdul	Review On	5/1/2025 8:12:26 AM
Supervise By	mohammad	Supervise On	5/2/2025 3:21:15 AM
SubDirectory	PS043025	HP Acquire Method	HP Processing Method ps042325 8151
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24064,PP24065,PP24066,PP24067,PP24068		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24066 PP24069,PP24070		

22	Q1906-05MSDRE	PS030010.D	01 May 2025 11:00	AR\AJ	Not Ok
23	PB167796BL	PS030011.D	01 May 2025 11:24	AR\AJ	Ok
24	I.BLK	PS030012.D	01 May 2025 11:48	AR\AJ	Ok
25	HSTDCCC750	PS030013.D	01 May 2025 12:12	AR\AJ	Ok,M

M : Manual Integration

Instrument ID: ECD\_S

**Daily Analysis Runlog For Sequence/QCBatch ID # PS050125**

Review By	Abdul	Review On	5/2/2025 8:21:10 AM
Supervise By	mohammad	Supervise On	5/5/2025 4:42:18 AM
SubDirectory	PS050125	HP Acquire Method	HP Processing Method ps042325 8151
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24064,PP24065,PP24066,PP24067,PP24068		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24066 PP24069,PP24070		

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PS030014.D	01 May 2025 12:36	AR\AJ	Ok
2	I.BLK	PS030015.D	01 May 2025 13:03	AR\AJ	Ok
3	HSTDCCC750	PS030016.D	01 May 2025 13:27	AR\AJ	Ok,M
4	Q1883-01	PS030017.D	01 May 2025 13:51	AR\AJ	Ok,M
5	Q1883-03	PS030018.D	01 May 2025 14:15	AR\AJ	Ok,M
6	Q1883-05	PS030019.D	01 May 2025 14:39	AR\AJ	Ok
7	Q1883-07	PS030020.D	01 May 2025 15:04	AR\AJ	Ok,M
8	Q1883-09	PS030021.D	01 May 2025 15:28	AR\AJ	Ok,M
9	Q1883-11	PS030022.D	01 May 2025 15:52	AR\AJ	Ok
10	Q1883-13	PS030023.D	01 May 2025 16:16	AR\AJ	Ok
11	Q1883-15	PS030024.D	01 May 2025 16:40	AR\AJ	Ok
12	I.BLK	PS030025.D	01 May 2025 17:04	AR\AJ	Ok
13	HSTDCCC750	PS030026.D	01 May 2025 17:28	AR\AJ	Ok,M

M : Manual Integration

Instrument ID: ECD\_S

**Daily Analysis Runlog For Sequence/QCBatch ID # PS050525**

Review By	Abdul	Review On	5/6/2025 8:15:56 AM
Supervise By	mohammad	Supervise On	5/7/2025 6:08:59 AM
SubDirectory	PS050525	HP Acquire Method	HP Processing Method ps042325 8151
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24064,PP24065,PP24066,PP24067,PP24068		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24066 PP24069,PP24070		

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PS030027.D	05 May 2025 08:15	AR\AJ	Ok
2	I.BLK	PS030028.D	05 May 2025 08:38	AR\AJ	Ok
3	HSTDCCC750	PS030029.D	05 May 2025 09:55	AR\AJ	Ok,M
4	PB167830BL	PS030030.D	05 May 2025 10:19	AR\AJ	Ok
5	PB167830BS	PS030031.D	05 May 2025 10:43	AR\AJ	Ok
6	Q1916-01	PS030032.D	05 May 2025 11:23	AR\AJ	Ok
7	Q1917-01	PS030033.D	05 May 2025 11:47	AR\AJ	Ok
8	Q1917-01MS	PS030034.D	05 May 2025 12:11	AR\AJ	Ok,M
9	Q1917-01MSD	PS030035.D	05 May 2025 12:35	AR\AJ	Ok,M
10	Q1922-01	PS030036.D	05 May 2025 12:59	AR\AJ	Ok
11	Q1922-05	PS030037.D	05 May 2025 13:23	AR\AJ	Ok,M
12	PB167796BS	PS030038.D	05 May 2025 13:47	AR\AJ	Ok,M
13	Q1928-01	PS030039.D	05 May 2025 14:11	AR\AJ	Ok
14	I.BLK	PS030040.D	05 May 2025 14:35	AR\AJ	Ok
15	HSTDCCC750	PS030041.D	05 May 2025 16:41	AR\AJ	Ok,M
16	Q1932-01	PS030042.D	05 May 2025 17:05	AR\AJ	Ok
17	Q1932-03	PS030043.D	05 May 2025 17:29	AR\AJ	Ok,M
18	Q1932-05	PS030044.D	05 May 2025 17:53	AR\AJ	Ok
19	Q1932-07	PS030045.D	05 May 2025 18:17	AR\AJ	Ok
20	Q1935-01	PS030046.D	05 May 2025 18:41	AR\AJ	Ok
21	Q1935-05	PS030047.D	05 May 2025 19:06	AR\AJ	Ok

Instrument ID: ECD\_S

**Daily Analysis Runlog For Sequence/QCBatch ID # PS050525**

Review By	Abdul	Review On	5/6/2025 8:15:56 AM
Supervise By	mohammad	Supervise On	5/7/2025 6:08:59 AM
SubDirectory	PS050525	HP Acquire Method	HP Processing Method ps042325 8151
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24064,PP24065,PP24066,PP24067,PP24068		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24066 PP24069,PP24070		

22	I.BLK	PS030048.D	05 May 2025 19:30	AR\AJ	Ok
23	HSTDCCC750	PS030049.D	05 May 2025 20:18	AR\AJ	Ok,M

M : Manual Integration

Instrument ID: ECD\_S

### Daily Analysis Runlog For Sequence/QCBatch ID # PS042325

Review By	Abdul	Review On	4/24/2025 8:51:25 AM
Supervise By	mohammad	Supervise On	4/26/2025 2:18:24 AM
SubDirectory	PS042325	HP Acquire Method	HP Processing Method ps042325 8151
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24064,PP24065,PP24066,PP24067,PP24068		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24066 PP24069,PP24070		

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PS029917.D	23 Apr 2025 10:13		AR\AJ	Ok
2	I.BLK	I.BLK	PS029918.D	23 Apr 2025 10:37		AR\AJ	Ok
3	HSTDICC200	HSTDICC200	PS029919.D	23 Apr 2025 11:01		AR\AJ	Ok,M
4	HSTDICC500	HSTDICC500	PS029920.D	23 Apr 2025 11:25		AR\AJ	Ok,M
5	HSTDICC750	HSTDICC750	PS029921.D	23 Apr 2025 11:49		AR\AJ	Ok,M
6	HSTDICC1000	HSTDICC1000	PS029922.D	23 Apr 2025 12:13		AR\AJ	Ok,M
7	HSTDICC1500	HSTDICC1500	PS029923.D	23 Apr 2025 12:37		AR\AJ	Ok,M
8	HSTDICV750	ICVPS042325	PS029924.D	23 Apr 2025 13:01		AR\AJ	Ok,M
9	I.BLK	I.BLK	PS029925.D	23 Apr 2025 13:25		AR\AJ	Ok
10	HSTDCCC750	HSTDCCC750	PS029926.D	23 Apr 2025 13:50		AR\AJ	Ok,M
11	Q1842-06	PL-714-COMP-08	PS029927.D	23 Apr 2025 14:14		AR\AJ	Ok
12	Q1842-12	PL-714-COMP-09	PS029928.D	23 Apr 2025 14:38		AR\AJ	Ok
13	Q1842-18	PL-714-COMP-10	PS029929.D	23 Apr 2025 15:02		AR\AJ	Ok
14	Q1842-24	PL-714-COMP-11	PS029930.D	23 Apr 2025 15:26		AR\AJ	Ok
15	Q1842-30	PL-714-COMP-12	PS029931.D	23 Apr 2025 15:50		AR\AJ	Ok
16	Q1842-36	PL-714-COMP-13	PS029932.D	23 Apr 2025 16:14		AR\AJ	Ok
17	Q1842-42	PL-714-COMP-14	PS029933.D	23 Apr 2025 16:38		AR\AJ	Ok
18	I.BLK	I.BLK	PS029934.D	23 Apr 2025 17:02		AR\AJ	Ok

Instrument ID: ECD\_S

### Daily Analysis Runlog For Sequence/QCBatch ID # PS042325

Review By	Abdul	Review On	4/24/2025 8:51:25 AM
Supervise By	mohammad	Supervise On	4/26/2025 2:18:24 AM
SubDirectory	PS042325	HP Acquire Method	HP Processing Method ps042325 8151
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24064,PP24065,PP24066,PP24067,PP24068		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24066 PP24069,PP24070		

19	HSTDCCC750	HSTDCCC750	PS029935.D	23 Apr 2025 17:26		AR\AJ	Ok,M
20	Q1842-06MS	PL-714-COMP-08MS	PS029936.D	23 Apr 2025 18:14		AR\AJ	Ok,M
21	Q1842-06MSD	PL-714-COMP-08MSD	PS029937.D	23 Apr 2025 18:38	RPD Fail	AR\AJ	Ok,M
22	PB167675BS	PB167675BS	PS029938.D	23 Apr 2025 19:02		AR\AJ	Ok,M
23	PB167701BL	PB167701BL	PS029939.D	23 Apr 2025 19:27		AR\AJ	Ok
24	PB167701BS	PB167701BS	PS029940.D	23 Apr 2025 19:51		AR\AJ	Ok,M
25	PB167660TB	PB167660TB	PS029941.D	23 Apr 2025 20:15		AR\AJ	Ok
26	I.BLK	I.BLK	PS029942.D	23 Apr 2025 20:39		AR\AJ	Ok
27	HSTDCCC750	HSTDCCC750	PS029943.D	23 Apr 2025 21:03		AR\AJ	Ok,M
28	PB167710BL	PB167710BL	PS029944.D	23 Apr 2025 21:51		AR\AJ	Ok
29	PB167710BS	PB167710BS	PS029945.D	23 Apr 2025 22:15		AR\AJ	Ok,M
30	Q1850-01	CONCRETE-PILE-N-C	PS029946.D	23 Apr 2025 22:39		AR\AJ	Ok
31	Q1852-01	ETGI-354	PS029947.D	23 Apr 2025 23:03		AR\AJ	Ok
32	Q1852-03	72-11977	PS029948.D	23 Apr 2025 23:27		AR\AJ	Ok
33	Q1852-05	ETGI-278	PS029949.D	23 Apr 2025 23:51		AR\AJ	Ok,M
34	Q1852-07	72-12013	PS029950.D	24 Apr 2025 00:15		AR\AJ	Ok,M
35	Q1852-07MS	72-12013MS	PS029951.D	24 Apr 2025 00:39	Some compound recovery fail	AR\AJ	Ok,M
36	Q1852-07MSD	72-12013MSD	PS029952.D	24 Apr 2025 01:03	Some compound recovery fail, RPD fail.	AR\AJ	Ok,M
37	I.BLK	I.BLK	PS029953.D	24 Apr 2025 01:27		AR\AJ	Ok

Instrument ID: ECD\_S

### Daily Analysis Runlog For Sequence/QCBatch ID # PS042325

Review By	Abdul	Review On	4/24/2025 8:51:25 AM
Supervise By	mohammad	Supervise On	4/26/2025 2:18:24 AM
SubDirectory	PS042325	HP Acquire Method	HP Processing Method ps042325 8151
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24064,PP24065,PP24066,PP24067,PP24068		
CCC Internal Standard/PEM	PP24066		
ICV/I.BLK	PP24069,PP24070		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

38	HSTDCCC750	HSTDCCC750	PS029954.D	24 Apr 2025 04:15	All comp fail in 2nd column Except comp#1,6,15,16	AR\AJ	Ok,M
----	------------	------------	------------	-------------------	--	-------	------

M : Manual Integration

Instrument ID: ECD\_S

**Daily Analysis Runlog For Sequence/QCBatch ID # PS043025**

Review By	Abdul	Review On	5/1/2025 8:12:26 AM
Supervise By	mohammad	Supervise On	5/2/2025 3:21:15 AM
SubDirectory	PS043025	HP Acquire Method	HP Processing Method ps042325 8151
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24064,PP24065,PP24066,PP24067,PP24068		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24066 PP24069,PP24070		

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PS029989.D	01 May 2025 00:34		AR\AJ	Ok
2	I.BLK	I.BLK	PS029990.D	01 May 2025 00:58		AR\AJ	Ok
3	HSTDCCC750	HSTDCCC750	PS029991.D	01 May 2025 01:22		AR\AJ	Ok,M
4	PB167796BL	PB167796BL	PS029992.D	01 May 2025 01:46	Looks like hexan	AR\AJ	Not Ok
5	PB167796BS	PB167796BS	PS029993.D	01 May 2025 02:10	Surrogate recovery high	AR\AJ	Not Ok
6	Q1904-01	VNJ-210	PS029994.D	01 May 2025 02:34		AR\AJ	Ok
7	Q1905-01	MH-G	PS029995.D	01 May 2025 02:58		AR\AJ	Ok,M
8	Q1905-05	MH-H	PS029996.D	01 May 2025 03:22		AR\AJ	Ok,M
9	Q1906-01	WC-4	PS029997.D	01 May 2025 03:46		AR\AJ	Ok,M
10	Q1906-05	WC-5	PS029998.D	01 May 2025 04:10	Surrogate high in both column,Confirm in MS-MSD	AR\AJ	Ok
11	Q1906-05MS	WC-5MS	PS029999.D	01 May 2025 04:34	surrogate high in both column , some compound recovery fail	AR\AJ	Ok,M
12	Q1906-05MSD	WC-5MSD	PS030000.D	01 May 2025 04:58	surrogate high in both column , some compound recovery fail	AR\AJ	Ok,M
13	I.BLK	I.BLK	PS030001.D	01 May 2025 06:10		AR\AJ	Ok
14	HSTDCCC750	HSTDCCC750	PS030002.D	01 May 2025 06:59		AR\AJ	Ok,M
15	Q1906-09	WC-6	PS030003.D	01 May 2025 07:47		AR\AJ	Ok
16	Q1906-13	WC-7	PS030004.D	01 May 2025 08:11		AR\AJ	Ok,M

Instrument ID: ECD\_S

### Daily Analysis Runlog For Sequence/QCBatch ID # PS043025

Review By	Abdul	Review On	5/1/2025 8:12:26 AM
Supervise By	mohammad	Supervise On	5/2/2025 3:21:15 AM
SubDirectory	PS043025	HP Acquire Method	HP Processing Method ps042325 8151
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24064,PP24065,PP24066,PP24067,PP24068		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24066 PP24069,PP24070		

17	Q1907-01	CO-8R-WC	PS030005.D	01 May 2025 08:35		AR\AJ	Ok,M
18	Q1912-01	MH-E	PS030006.D	01 May 2025 08:59		AR\AJ	Ok
19	Q1912-05	MH-F	PS030007.D	01 May 2025 09:23		AR\AJ	Ok
20	Q1906-05RE	WC-5RE	PS030008.D	01 May 2025 10:11	Surrogate high in both column	AR\AJ	Not Ok
21	Q1906-05MSRE	WC-5MSRE	PS030009.D	01 May 2025 10:35	F Flag coming , surrogate high in both column , some compound recovery fail	AR\AJ	Not Ok
22	Q1906-05MSDRE	WC-5MSDRE	PS030010.D	01 May 2025 11:00	F Flag coming , surrogate high in both column , some compound recovery fail	AR\AJ	Not Ok
23	PB167796BL	PB167796BL	PS030011.D	01 May 2025 11:24		AR\AJ	Ok
24	I.BLK	I.BLK	PS030012.D	01 May 2025 11:48		AR\AJ	Ok
25	HSTDCCC750	HSTDCCC750	PS030013.D	01 May 2025 12:12		AR\AJ	Ok,M

M : Manual Integration

Instrument ID: ECD\_S

### Daily Analysis Runlog For Sequence/QCBatch ID # PS050125

Review By	Abdul	Review On	5/2/2025 8:21:10 AM
Supervise By	mohammad	Supervise On	5/5/2025 4:42:18 AM
SubDirectory	PS050125	HP Acquire Method	HP Processing Method ps042325 8151
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24064,PP24065,PP24066,PP24067,PP24068		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24066 PP24069,PP24070		

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PS030014.D	01 May 2025 12:36		AR\AJ	Ok
2	I.BLK	I.BLK	PS030015.D	01 May 2025 13:03		AR\AJ	Ok
3	HSTDCCC750	HSTDCCC750	PS030016.D	01 May 2025 13:27		AR\AJ	Ok,M
4	Q1883-01	OU4-PCS-TC-27-04232	PS030017.D	01 May 2025 13:51		AR\AJ	Ok,M
5	Q1883-03	OU4-PCS-TC-28-04232	PS030018.D	01 May 2025 14:15		AR\AJ	Ok,M
6	Q1883-05	OU4-PCS-TC-29-04232	PS030019.D	01 May 2025 14:39		AR\AJ	Ok
7	Q1883-07	OU4-PCS-TC-30-04232	PS030020.D	01 May 2025 15:04		AR\AJ	Ok,M
8	Q1883-09	OU4-PCS-TC-31-04232	PS030021.D	01 May 2025 15:28		AR\AJ	Ok,M
9	Q1883-11	OU4-PCS-TC-32-04232	PS030022.D	01 May 2025 15:52		AR\AJ	Ok
10	Q1883-13	OU4-VSL-18-042325	PS030023.D	01 May 2025 16:16		AR\AJ	Ok
11	Q1883-15	OU4-VSL-19-042325	PS030024.D	01 May 2025 16:40		AR\AJ	Ok
12	I.BLK	I.BLK	PS030025.D	01 May 2025 17:04		AR\AJ	Ok
13	HSTDCCC750	HSTDCCC750	PS030026.D	01 May 2025 17:28		AR\AJ	Ok,M

M : Manual Integration

Instrument ID: ECD\_S

### Daily Analysis Runlog For Sequence/QCBatch ID # PS050525

Review By	Abdul	Review On	5/6/2025 8:15:56 AM
Supervise By	mohammad	Supervise On	5/7/2025 6:08:59 AM
SubDirectory	PS050525	HP Acquire Method	HP Processing Method ps042325 8151
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24064,PP24065,PP24066,PP24067,PP24068		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24066 PP24069,PP24070		

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PS030027.D	05 May 2025 08:15		AR\AJ	Ok
2	I.BLK	I.BLK	PS030028.D	05 May 2025 08:38		AR\AJ	Ok
3	HSTDCCC750	HSTDCCC750	PS030029.D	05 May 2025 09:55		AR\AJ	Ok,M
4	PB167830BL	PB167830BL	PS030030.D	05 May 2025 10:19		AR\AJ	Ok
5	PB167830BS	PB167830BS	PS030031.D	05 May 2025 10:43		AR\AJ	Ok
6	Q1916-01	WC-12	PS030032.D	05 May 2025 11:23		AR\AJ	Ok
7	Q1917-01	MH-JJ	PS030033.D	05 May 2025 11:47		AR\AJ	Ok
8	Q1917-01MS	MH-JJMS	PS030034.D	05 May 2025 12:11	some compound recovery fail	AR\AJ	Ok,M
9	Q1917-01MSD	MH-JJMSD	PS030035.D	05 May 2025 12:35	some compound recovery fail	AR\AJ	Ok,M
10	Q1922-01	MH-R	PS030036.D	05 May 2025 12:59		AR\AJ	Ok
11	Q1922-05	MH-S	PS030037.D	05 May 2025 13:23		AR\AJ	Ok,M
12	PB167796BS	PB167796BS	PS030038.D	05 May 2025 13:47		AR\AJ	Ok,M
13	Q1928-01	MH-Q	PS030039.D	05 May 2025 14:11		AR\AJ	Ok
14	I.BLK	I.BLK	PS030040.D	05 May 2025 14:35		AR\AJ	Ok
15	HSTDCCC750	HSTDCCC750	PS030041.D	05 May 2025 16:41		AR\AJ	Ok,M
16	Q1932-01	COMP-4	PS030042.D	05 May 2025 17:05		AR\AJ	Ok
17	Q1932-03	COMP-5	PS030043.D	05 May 2025 17:29		AR\AJ	Ok,M
18	Q1932-05	COMP-6	PS030044.D	05 May 2025 17:53		AR\AJ	Ok

Instrument ID: ECD\_S

**Daily Analysis Runlog For Sequence/QCBatch ID # PS050525**

Review By	Abdul	Review On	5/6/2025 8:15:56 AM
Supervise By	mohammad	Supervise On	5/7/2025 6:08:59 AM
SubDirectory	PS050525	HP Acquire Method	HP Processing Method ps042325 8151
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP24064,PP24065,PP24066,PP24067,PP24068		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24066 PP24069,PP24070		

19	Q1932-07	COMP-7	PS030045.D	05 May 2025 18:17		AR\AJ	Ok
20	Q1935-01	MH-NN	PS030046.D	05 May 2025 18:41		AR\AJ	Ok
21	Q1935-05	MH-MM	PS030047.D	05 May 2025 19:06		AR\AJ	Ok
22	I.BLK	I.BLK	PS030048.D	05 May 2025 19:30		AR\AJ	Ok
23	HSTDCCC750	HSTDCCC750	PS030049.D	05 May 2025 20:18		AR\AJ	Ok,M

M : Manual Integration

**PERCENT SOLID**

**Supervisor:** Iwona  
**Analyst:** jignesh  
**Date:** 4/28/2025

**OVENTEMP IN Celsius(°C):** 107  
**Time IN:** 17:25  
**In Date:** 04/25/2025  
**Weight Check 1.0g:** 1.00  
**Weight Check 10g:** 10.00  
**OvenID:** M OVEN#1

**OVENTEMP OUT Celsius(°C):** 103  
**Time OUT:** 08:37  
**Out Date:** 04/26/2025  
**Weight Check 1.0g:** 1.00  
**Weight Check 10g:** 10.00  
**BalanceID:** M SC-4  
**Thermometer ID:** % SOLID- OVEN

QC:LB135558

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
Q1883-01	OU4-PCS-TC-27-042325	1	1.18	10.04	11.22	10.67	94.5	
Q1883-03	OU4-PCS-TC-28-042325	2	1.14	9.97	11.11	10.56	94.5	
Q1883-05	OU4-PCS-TC-29-042325	3	1.19	10.54	11.73	11.28	95.7	
Q1883-07	OU4-PCS-TC-30-042325	4	1.17	10.15	11.32	10.96	96.5	
Q1883-09	OU4-PCS-TC-31-042325	5	1.18	10.48	11.66	11.34	96.9	
Q1883-11	OU4-PCS-TC-32-042325	6	1.18	9.96	11.14	10.87	97.3	
Q1883-13	OU4-PCS-18-042325	7	1.15	10.25	11.4	10.86	94.7	
Q1883-15	OU4-PCS-19-042325	8	1.19	10.54	11.73	11.29	95.8	
Q1884-01	P001-SS037-01	9	1.17	10.30	11.47	10.87	94.2	
Q1884-02	P001-SS038-01	10	1.17	10.32	11.49	11.22	97.4	
Q1888-05	SVOC-GPC-BLANK	11	1.00	1.00	2.00	2.00	100.0	
Q1888-06	PEST-GPC-BLANK	12	1.00	1.00	2.00	2.00	100.0	
Q1888-07	PEST-GPC-BLANK-SPIKE	13	1.00	1.00	2.00	2.00	100.0	
Q1888-08	PCB-GPC-BLANK	14	1.00	1.00	2.00	2.00	100.0	
Q1888-09	PCB-GPC-BLANK-SPIKE	15	1.00	1.00	2.00	2.00	100.0	
Q1888-10	SVOC-GPC2-BLANK	16	1.00	1.00	2.00	2.00	100.0	
Q1888-11	PEST-GPC2-BLANK	17	1.00	1.00	2.00	2.00	100.0	
Q1888-12	PEST-GPC2-BLANK-SPIKE	18	1.00	1.00	2.00	2.00	100.0	
Q1888-13	PCB-GPC2-BLANK	19	1.00	1.00	2.00	2.00	100.0	
Q1888-14	PCB-GPC2-BLANK-SPIKE	20	1.00	1.00	2.00	2.00	100.0	
Q1889-01	COMP-1	21	1.19	10.07	11.26	9.5	82.5	
Q1889-02	COMP-2	22	1.16	10.50	11.66	9.61	80.5	
Q1889-03	COMP-3	23	1.11	10.73	11.84	9.77	80.7	
Q1891-01	MH-C	24	1.15	9.48	10.63	9.8	91.2	
Q1891-02	MH-C-EPH	25	1.16	9.82	10.98	10.15	91.5	
Q1891-03	MH-C-VOC	26	1.19	9.94	11.13	10.2	90.6	
Q1891-05	MH-D	27	1.15	10.17	11.32	9.64	83.5	
Q1891-06	MH-D-EPH	28	1.15	9.97	11.12	8.74	76.1	

**PERCENT SOLID**

**Supervisor:** Iwona  
**Analyst:** jignesh  
**Date:** 4/28/2025

**OVENTEMP IN Celsius(°C):** 107  
**Time IN:** 17:25  
**In Date:** 04/25/2025  
**Weight Check 1.0g:** 1.00  
**Weight Check 10g:** 10.00  
**OvenID:** M OVEN#1

**OVENTEMP OUT Celsius(°C):** 103  
**Time OUT:** 08:37  
**Out Date:** 04/26/2025  
**Weight Check 1.0g:** 1.00  
**Weight Check 10g:** 10.00  
**BalanceID:** M SC-4  
**Thermometer ID:** % SOLID- OVEN

QC:LB135558

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
Q1891-07	MH-D-VOC	29	1.18	9.46	10.64	8.83	80.9	
Q1892-01	MH-G	30	1.13	9.61	10.74	9.35	85.5	
Q1892-02	MH-G-EPH	31	1.15	10.29	11.44	9.98	85.8	
Q1892-03	MH-G-VOC	32	1.18	10.45	11.63	9.82	82.7	
Q1892-05	MH-H	33	1.14	9.66	10.8	9.92	90.9	
Q1892-06	MH-H-EPH	34	1.12	10.66	11.78	10.68	89.7	
Q1892-07	MH-H-VOC	35	1.18	10.19	11.37	10.28	89.3	
Q1892-09	MH-U2	36	1.18	10.04	11.22	9.96	87.5	
Q1892-10	MH-U2-EPH	37	1.19	10.34	11.53	10.04	85.6	
Q1892-11	MH-U2-VOC	38	1.18	10.22	11.4	10.14	87.7	
Q1893-01	UGGP-1	39	1.00	1.00	2.00	2.00	100.0	TAR SAMPLE
Q1893-02	UGGP-2	40	1.00	1.00	2.00	2.00	100.0	TAR SAMPLE
Q1893-03	INTERIOR-1	41	1.00	1.00	2.00	2.00	100.0	wipe sample
Q1893-04	INTERIOR-2	42	1.00	1.00	2.00	2.00	100.0	wipe sample
Q1893-05	INTERIOR-3	43	1.00	1.00	2.00	2.00	100.0	wipe sample
Q1893-06	INTERIOR-4	44	1.00	1.00	2.00	2.00	100.0	wipe sample
Q1893-07	EXTERIOR-1	45	1.00	1.00	2.00	2.00	100.0	wipe sample
Q1895-01	COMP-1	55	1.14	10.58	11.72	10.97	92.9	
Q1895-03	COMP-2	56	1.14	10.77	11.91	10.96	91.2	
Q1895-05	COMP-3	57	1.18	10.06	11.24	10.56	93.2	
Q1896-01	295-BERGEN-RO	58	1.14	11.31	12.45	10.91	86.4	
Q1896-02	295-BERGEN-RO	59	1.18	10.01	11.19	9.9	87.1	
Q1898-01	41525A	60	1.00	1.00	2.00	2.00	100.0	wipe sample
Q1898-02	41525B	61	1.00	1.00	2.00	2.00	100.0	wipe sample
Q1898-03	42525A	62	1.00	1.00	2.00	2.00	100.0	wipe sample
Q1898-04	42525B	63	1.00	1.00	2.00	2.00	100.0	wipe sample
Q1900-01	WC-1	46	1.14	9.98	11.12	9.56	84.4	
Q1900-02	WC-1-EPH	47	1.14	10.35	11.49	10.19	87.4	

**PERCENT SOLID**

**Supervisor:** Iwona  
**Analyst:** jignesh  
**Date:** 4/28/2025

**OVENTEMP IN Celsius(°C):** 107  
**Time IN:** 17:25  
**In Date:** 04/25/2025  
**Weight Check 1.0g:** 1.00  
**Weight Check 10g:** 10.00  
**OvenID:** M OVEN#1

**OVENTEMP OUT Celsius(°C):** 103  
**Time OUT:** 08:37  
**Out Date:** 04/26/2025  
**Weight Check 1.0g:** 1.00  
**Weight Check 10g:** 10.00  
**BalanceID:** M SC-4  
**Thermometer ID:** % SOLID- OVEN

QC:LB135558

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
Q1900-03	WC-1-VOC	48	1.14	10.01	11.15	9.73	85.8	
Q1900-05	WC-2	49	1.19	8.82	10.01	8.76	85.8	
Q1900-06	WC-2-EPH	50	1.19	10.08	11.27	9.76	85.0	
Q1900-07	WC-2-VOC	51	1.17	10.79	11.96	10.33	84.9	
Q1900-09	WC-3	52	1.14	9.61	10.75	9.32	85.1	
Q1900-10	WC-3-EPH	53	1.12	10.38	11.5	9.11	77.0	
Q1900-11	WC-3-VOC	54	1.19	10.71	11.9	10.39	85.9	

$$\% \text{ Solid} = \frac{(C-A) * 100}{(B-A)}$$

## WORKLIST(Hardcopy Internal Chain)

WorkList Name : %1-042525

WorkList ID : 189135

Department : Wet-Chemistry

Date : 04-25-2025 08:09:39  
VB135558

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1883-01	OU4-PCS-TC-27-042325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L41	04/23/2025	Chemtech -SO
Q1883-03	OU4-PCS-TC-28-042325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L41	04/23/2025	Chemtech -SO
Q1883-05	OU4-PCS-TC-29-042325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L41	04/23/2025	Chemtech -SO
Q1883-07	OU4-PCS-TC-30-042325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L41	04/23/2025	Chemtech -SO
Q1883-09	OU4-PCS-TC-31-042325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L41	04/23/2025	Chemtech -SO
Q1883-11	OU4-PCS-TC-32-042325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L41	04/23/2025	Chemtech -SO
Q1883-13	OU4-PCS-18-042325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L41	04/23/2025	Chemtech -SO
Q1883-15	OU4-PCS-19-042325	Solid	Percent Solids	Cool 4 deg C	NOBI03	L41	04/23/2025	Chemtech -SO
Q1884-01	P001-SS037-01	Solid	Percent Solids	Cool 4 deg C	ROYF02	L51	04/24/2025	Chemtech -SO
Q1884-02	P001-SS038-01	Solid	Percent Solids	Cool 4 deg C	ROYF02	L51	04/24/2025	Chemtech -SO
Q1888-05	SVOC-GPC-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	L31	04/18/2025	Chemtech -SO
Q1888-06	PEST-GPC-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	L31	04/18/2025	Chemtech -SO
Q1888-07	PEST-GPC-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	L31	04/18/2025	Chemtech -SO
Q1888-08	PCB-GPC-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	L31	04/18/2025	Chemtech -SO
Q1888-09	PCB-GPC-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	L31	04/18/2025	Chemtech -SO
Q1888-10	SVOC-GPC2-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	L31	04/18/2025	Chemtech -SO
Q1888-11	PEST-GPC2-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	L31	04/18/2025	Chemtech -SO
Q1888-12	PEST-GPC2-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	L31	04/18/2025	Chemtech -SO
Q1888-13	PCB-GPC2-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	L31	04/18/2025	Chemtech -SO
Q1888-14	PCB-GPC2-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	L31	04/18/2025	Chemtech -SO
Q1889-01	COMP-1	Solid	Percent Solids	Cool 4 deg C	POWE02	L51	04/24/2025	Chemtech -SO

Date/Time 04/25/25 15:20

Raw Sample Received by: JD (ee)

Raw Sample Relinquished by: JD (SM)

Date/Time 04/25/25 17:30

Raw Sample Received by:

JD (SM)

Raw Sample Relinquished by:

JD (eeC)

## WORKLIST(Hardcopy Internal Chain)

JB B5558

WorkList Name : %1-042525

WorkList ID : 189135

Department : Wet-Chemistry

Date : 04-25-2025 08:09:39

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1889-02	COMP-2	Solid	Percent Solids	Cool 4 deg C	POWE02	L51	04/24/2025	Chemtech -SO
Q1889-03	COMP-3	Solid	Percent Solids	Cool 4 deg C	POWE02	L51	04/24/2025	Chemtech -SO
Q1891-01	MH-C	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO
Q1891-02	MH-C-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO
Q1891-03	MH-C-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO
Q1891-05	MH-D	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO
Q1891-06	MH-D-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO
Q1891-07	MH-D-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO
Q1892-01	MH-G	Solid	Percent Solids	Cool 4 deg C	PSEG03	L51	04/24/2025	Chemtech -SO
Q1892-02	MH-G-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	L51	04/24/2025	Chemtech -SO
Q1892-03	MH-G-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	L51	04/24/2025	Chemtech -SO
Q1892-05	MH-H	Solid	Percent Solids	Cool 4 deg C	PSEG03	L51	04/24/2025	Chemtech -SO
Q1892-06	MH-H-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	L51	04/24/2025	Chemtech -SO
Q1892-07	MH-H-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	L51	04/24/2025	Chemtech -SO
Q1892-09	MH-U2	Solid	Percent Solids	Cool 4 deg C	PSEG03	L51	04/24/2025	Chemtech -SO
Q1892-10	MH-U2-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	L51	04/25/2025	Chemtech -SO
Q1892-11	MH-U2-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	L51	04/25/2025	Chemtech -SO
Q1893-01	UGGP-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO
Q1893-02	UGGP-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO
Q1893-03	INTERIOR-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO
Q1893-04	INTERIOR-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO

Date/Time 04/25/25 15:20

Raw Sample Received by: SO wet 01  
Raw Sample Relinquished by: JD csmDate/Time 04/25/25 17:30  
Raw Sample Received by: JD csm  
Raw Sample Relinquished by: JD cool C1  
317 of 574

## WORKLIST(Hardcopy Internal Chain)

JF 135558

WorkList Name : %1-042525

WorkList ID : 189135

Department : Wet-Chemistry

Date : 04-25-2025 08:09:39

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1893-05	INTERIOR-3	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO
Q1893-06	INTERIOR-4	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO
Q1893-07	EXTERIOR-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO
Q1895-01	COMP-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO
Q1895-03	COMP-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO
Q1895-05	COMP-3	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO
Q1896-01	295-BERGEN-RO	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/25/2025	Chemtech -SO
Q1896-02	295-BERGEN-RO	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	04/25/2025	Chemtech -SO
Q1898-01	41525A	Solid	Percent Solids	Cool 4 deg C	PSEG03	L12	04/25/2025	Chemtech -SO
Q1898-02	41525B	Solid	Percent Solids	Cool 4 deg C	PSEG03	L12	04/25/2025	Chemtech -SO
Q1898-03	42525A	Solid	Percent Solids	Cool 4 deg C	PSEG03	L12	04/25/2025	Chemtech -SO
Q1898-04	42525B	Solid	Percent Solids	Cool 4 deg C	PSEG03	L12	04/25/2025	Chemtech -SO
Q1900-01	WC-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO
Q1900-02	WC-1-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO
Q1900-03	WC-1-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO
Q1900-05	WC-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO
Q1900-06	WC-2-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO
Q1900-07	WC-2-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO
Q1900-09	WC-3	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO
Q1900-10	WC-3-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO
Q1900-11	WC-3-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	04/25/2025	Chemtech -SO

Date/Time 04/23/25 13:20

Raw Sample Received by: SD WEC

Raw Sample Relinquished by: JD CSM

Date/Time 04/25/25 17:30

Raw Sample Received by: JD CSM

Raw Sample Relinquished by: SD WEC

318 of 574

SOP ID:	M8151A-Herbicide-22		
Clean Up SOP #:	N/A	Extraction Start Date :	04/30/2025
Matrix :	Solid	Extraction Start Time :	08:50
Weigh By:	EH	Extraction End Date :	04/30/2025
Balance check:	RJ	Extraction End Time :	16:25
Balance ID:	EX-SC-2	pH Meter ID:	N/A
pH Strip Lot#:	E3880	Hood ID:	3,4,5,7
Extraction Method:	<input type="checkbox"/> Separatory Funnel <input type="checkbox"/> Continous Liquid/Liquid		<input type="checkbox"/> Sonication <input type="checkbox"/> Waste Dilution <input checked="" type="checkbox"/> Soxhlet

Standard Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	1.0ML	5/500 PPM	PP24484
Surrogate	1.0ML	5000 PPB	PP24424
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
MeCl2/Acetone/1:1	N/A	EP2600
Acidified Na2SO4	N/A	EP2576
Sand	N/A	E2865
HCL	N/A	M6151
DI WATER	N/A	N/A
37% KOH	N/A	EP2594
Methylene Chloride	N/A	E3926
1:3 SULPHURIC ACID	N/A	EP2598
Ether	N/A	E3881
ISO OCTANE	N/A	E3554
METHANOL	N/A	V14622
Diazomethane	N/A	EP2603
Hexane	N/A	E3928
N/A	N/A	N/A

**Extraction Conformance/Non-Conformance Comments:**

pH adjusted with HCL <2 for soil Extraction, PH adjusted with 1:3 H2SO4 <2 after Hydrolysis, Derivatization procedure is completed and samples are ready to Analyze,40ML Vial Lot # 03-40 BTS723.


KD Bath ID: N/A      Envap ID: NEVAP-02  
 KD Bath Temperature: N/A      Envap Temperature: 40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
4/30/25	RS (Ext-Lab)	R Pest/PCB Lab
16:30	Preparation Group	Analysis Group

Analytical Method: M8151A-Herbicide-22

Concentration Date: 04/30/2025

Sample ID	Client Sample ID	Test	(g) mL	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB167796BL	HBLK796	Herbicide	30.01	N/A	ritesh	Evelyn	10			U2-1
PB167796BS	HLCS796	Herbicide	30.02	N/A	ritesh	Evelyn	10			2
Q1883-01	OU4-PCS-TC-27-042325	Herbicide Group1	30.01	N/A	ritesh	Evelyn	10	E		3
Q1883-03	OU4-PCS-TC-28-042325	Herbicide Group1	30.06	N/A	ritesh	Evelyn	10	E		4
Q1883-05	OU4-PCS-TC-29-042325	Herbicide Group1	30.05	N/A	ritesh	Evelyn	10	E		5
Q1883-07	OU4-PCS-TC-30-042325	Herbicide Group1	30.03	N/A	ritesh	Evelyn	10	E		6
Q1883-09	OU4-PCS-TC-31-042325	Herbicide Group1	30.04	N/A	ritesh	Evelyn	10	E		U3-1
Q1883-11	OU4-PCS-TC-32-042325	Herbicide Group1	30.02	N/A	ritesh	Evelyn	10	E		2
Q1883-13	OU4-VSL-18-042325	Herbicide Group1	30.04	N/A	ritesh	Evelyn	10	E		3
Q1883-15	OU4-VSL-19-042325	Herbicide Group1	30.07	N/A	ritesh	Evelyn	10	E		4
Q1904-01	VNJ-210	Herbicide	30.04	N/A	ritesh	Evelyn	10			5
Q1905-01	MH-G	Herbicide	30.01	N/A	ritesh	Evelyn	10	D		6
Q1905-05	MH-H	Herbicide	30.03	N/A	ritesh	Evelyn	10	D		U6-1
Q1906-01	WC-4	Herbicide	30.05	N/A	ritesh	Evelyn	10			2
Q1906-05	WC-5	Herbicide	30.02	N/A	ritesh	Evelyn	10			3
Q1906-05MS	WC-5MS	Herbicide	30.06	N/A	ritesh	Evelyn	10			4
Q1906-05MS D	WC-5MSD	Herbicide	30.04	N/A	ritesh	Evelyn	10			5
Q1906-09	WC-6	Herbicide	30.08	N/A	ritesh	Evelyn	10			6
Q1906-13	WC-7	Herbicide	30.01	N/A	ritesh	Evelyn	10			U7-1
Q1907-01	CO-8R-WC	Herbicide	30.06	N/A	ritesh	Evelyn	10	D		2
Q1912-01	MH-E	Herbicide	30.07	N/A	ritesh	Evelyn	10	E		3
Q1912-05	MH-F	Herbicide	30.02	N/A	ritesh	Evelyn	10	D		4

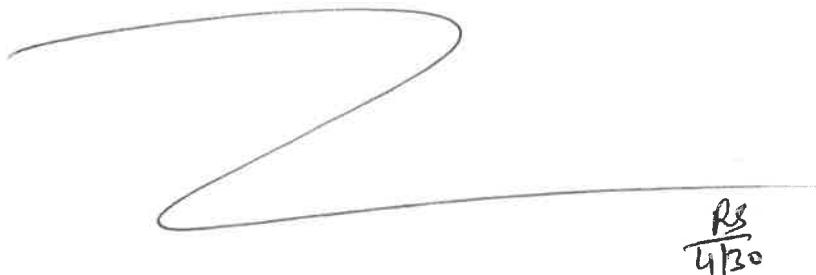

RS  
4/30

\* Extracts relinquished on the same date as received.

167796  
850

## WORKLIST(Hardcopy Internal Chain)

WorkList Name : Q1904

WorkList ID : 189222

Department : Extraction

Date : 04-30-2025 08:35:01

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1883-01	OU4-PCS-TC-27-042325	Solid	Herbicide Group1	Cool 4 deg C	NOBI03	L41	04/23/2025	8151A
Q1883-03	OU4-PCS-TC-28-042325	Solid	Herbicide Group1	Cool 4 deg C	NOBI03	L41	04/23/2025	8151A
Q1883-05	OU4-PCS-TC-29-042325	Solid	Herbicide Group1	Cool 4 deg C	NOBI03	L41	04/23/2025	8151A
Q1883-07	OU4-PCS-TC-30-042325	Solid	Herbicide Group1	Cool 4 deg C	NOBI03	L41	04/23/2025	8151A
Q1883-09	OU4-PCS-TC-31-042325	Solid	Herbicide Group1	Cool 4 deg C	NOBI03	L41	04/23/2025	8151A
Q1883-11	OU4-PCS-TC-32-042325	Solid	Herbicide Group1	Cool 4 deg C	NOBI03	L41	04/23/2025	8151A
Q1883-13	OU4-VSL-18-042325	Solid	Herbicide Group1	Cool 4 deg C	NOBI03	L41	04/23/2025	8151A
Q1883-15	OU4-VSL-19-042325	Solid	Herbicide Group1	Cool 4 deg C	NOBI03	L41	04/23/2025	8151A
Q1904-01	VNJ-210	Solid	Herbicide	Cool 4 deg C	PSEG03	L41	04/28/2025	8151A
Q1905-01	MH-G	Solid	Herbicide	Cool 4 deg C	PSEG03	L51	04/28/2025	8151A
Q1905-05	MH-H	Solid	Herbicide	Cool 4 deg C	PSEG03	L51	04/28/2025	8151A
Q1906-01	WC-4	Solid	Herbicide	Cool 4 deg C	PSEG03	L41	04/28/2025	8151A
Q1906-05	WC-5	Solid	Herbicide	Cool 4 deg C	PSEG03	L41	04/28/2025	8151A
Q1906-09	WC-6	Solid	Herbicide	Cool 4 deg C	PSEG03	L41	04/28/2025	8151A
Q1906-13	WC-7	Solid	Herbicide	Cool 4 deg C	PSEG03	L41	04/28/2025	8151A
Q1907-01	CO-8R-WC	Solid	Herbicide	Cool 4 deg C	WALS01	L51	04/28/2025	8151A
Q1912-01	MH-E	Solid	Herbicide	Cool 4 deg C	PSEG03	L51	04/29/2025	8151A
Q1912-05	MH-F	Solid	Herbicide	Cool 4 deg C	PSEG03	L51	04/29/2025	8151A

Date/Time 04/30/25 8:45  
 Raw Sample Received by: RJ (EST-1ab)  
 Raw Sample Relinquished by: AM sn

Date/Time 04/30/25 9:15  
 Raw Sample Received by: AM sn  
 Raw Sample Relinquished by: RJ (EST-1ab)

**Prep Standard - Chemical Standard Summary****Order ID :** Q1883**Test :** Herbicide Group1**Prepbatch ID :** PB167796,**Sequence ID/Qc Batch ID:** ps043025,PS050125,ps050525,**Standard ID :**

EP2576,EP2600,PP24061,PP24062,PP24064,PP24065,PP24066,PP24067,PP24068,PP24069,PP24070,PP24424,PP24484,

**Chemical ID :**

E2865,E3370,E3551,E3826,E3902,E3904,E3917,E3929,M5173,M6151,P10549,P11180,P11181,P12619,P12629,P12686,P12708,P12709,P13514,P13515,P13532,P13533,P13534,

## Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
601	Acidified Sodium Sulphate 2	<a href="#">EP2576</a>	01/06/2025	06/02/2025	Rajesh Parikh	Extraction_SC_ALE_2	None	RUPESHKUMAR SHAH 01/06/2025

FROM 100.00000ml of E3370 + 150.00000ml of M5173 + 3000.00000ml of E3551 = Final Quantity: 3000.000 gram  
(EX-SC-2)

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2017	1:1 ACETONE/METHYLENE CHLORIDE	<a href="#">EP2600</a>	04/07/2025	10/03/2025	Rajesh Parikh	None	None	Riteshkumar Patel 04/07/2025

FROM 8000.00000ml of E3904 + 8000.00000ml of E3917 = Final Quantity: 16000.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1321	2/200 PPM Herb Mega Mix	<a href="#">PP24061</a>	11/26/2024	05/09/2025	Ankita Jodhani	None	None	Yogesh Patel 11/27/2024

FROM 0.20000ml of P10549 + 1.00000ml of P11180 + 1.00000ml of P12619 + 1.00000ml of P12629 + 1.00000ml of P12686 + 95.80000ml of E3826 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1851	2/200 PPM Herb Mega Mix 2nd Source	<a href="#">PP24062</a>	11/26/2024	05/09/2025	Ankita Jodhani	None	None	Yogesh Patel 11/27/2024

FROM 1.00000ml of P11181 + 1.00000ml of P12708 + 1.00000ml of P12709 + 97.00000ml of E3826 = Final Quantity: 100.000 ml

### Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1452	1500 PPB HERB MIX STD	<a href="#">PP24064</a>	11/26/2024	05/09/2025	Ankita Jodhani	None	None	Yogesh Patel 11/27/2024

FROM 0.25000ml of E3826 + 0.75000ml of PP24061 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1453	1000 PPB Herb MIX STD	<a href="#">PP24065</a>	11/26/2024	05/09/2025	Ankita Jodhani	None	None	Yogesh Patel 11/27/2024

FROM 0.50000ml of E3826 + 0.50000ml of PP24061 = Final Quantity: 1.000 ml

### Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1454	750 PPB Herb MIX STD	<a href="#">PP24066</a>	11/26/2024	05/09/2025	Ankita Jodhani	None	None	Yogesh Patel 11/27/2024

FROM 0.25000ml of E3826 + 0.75000ml of PP24065 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1455	500 PPB Herb MIX STD	<a href="#">PP24067</a>	11/26/2024	05/09/2025	Ankita Jodhani	None	None	Yogesh Patel 11/27/2024

FROM 0.75000ml of E3826 + 0.25000ml of PP24061 = Final Quantity: 1.000 ml

### Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1456	200 PPB Herb MIX STD	<a href="#">PP24068</a>	11/26/2024	05/09/2025	Ankita Jodhani	None	None	Yogesh Patel 11/27/2024

FROM 0.90000ml of E3826 + 0.10000ml of PP24061 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1854	1000 PPB HERB MIX ICV STD	<a href="#">PP24069</a>	11/26/2024	05/09/2025	Ankita Jodhani	None	None	Yogesh Patel 11/27/2024

FROM 0.50000ml of E3826 + 0.50000ml of PP24062 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1691	750 PPB ICV HERB STD	<a href="#">PP24070</a>	11/26/2024	05/09/2025	Ankita Jodhani	None	None	Yogesh Patel 11/27/2024

FROM 0.25000ml of E3826 + 0.75000ml of PP24069 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
60	5000 PPB Herbicide Surg Spike (Free Acid)	<a href="#">PP24424</a>	03/26/2025	09/18/2025	Abdul Mirza	None	None	Yogesh Patel 04/02/2025

FROM 1.25000ml of P13514 + 1.25000ml of P13515 + 97.50000ml of E3902 = Final Quantity: 100.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1848	5000/500000 PPB Herbicide Spike (Free Acid)	<a href="#">PP24484</a>	04/23/2025	10/23/2025	Abdul Mirza	None	None	Yogesh Patel 05/03/2025
<b>FROM</b>	0.50000ml of P13534 + 1.00000ml of P13532 + 1.00000ml of P13533 + 47.75000ml of E3929 = Final Quantity: 50.000 ml							

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-3382-05 / Sand, Purified (cs/4x2.5kg)	0000243821	06/30/2025	04/30/2020 / RAJESH	04/28/2020 / RAJESH	E2865
Seidler Chemical	BA-9244-03 / Ether, Anhydrous, Purified (cs/4x4L)	0000288039	07/17/2025	08/01/2022 / Rajesh	07/13/2022 / Rajesh	E3370
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	313201	07/01/2025	01/03/2024 / Rajesh	07/20/2023 / Rajesh	E3551
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24G1962003	05/09/2025	11/09/2024 / Rajesh	11/07/2024 / Rajesh	E3826
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H2762008	09/18/2025	03/18/2025 / RUPESH	02/12/2025 / RUPESH	E3902
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24K1762005	01/07/2026	03/13/2025 / RUPESH	12/27/2024 / RUPESH	E3904

### CHEMICAL RECEIPT LOG BOOK

<b>Supplier</b>	<b>ItemCode / ItemName</b>	<b>Lot #</b>	<b>Expiration Date</b>	<b>Date Opened / Opened By</b>	<b>Received Date / Received By</b>	<b>Chemtech Lot #</b>
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H2762008	10/03/2025	04/03/2025 / Rajesh	03/31/2025 / Rajesh	E3917
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H2762008	04/18/2027	04/18/2025 / RUPESH	04/16/2025 / RUPESH	E3929
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	0000281827	06/02/2025	06/01/2022 / william	04/05/2022 / william	M5173
Seidler Chemical	BA-9530-33 / Hydrochloric Acid, Instra-Analyzed (cs/6x2.5L)	22G2862015	08/18/2025	02/18/2025 / Sagar	01/15/2025 / Sagar	M6151
Restek	32254 / Dalapon Methyl Ester, 1000 ug/ml	A0170243	05/26/2025	11/26/2024 / Ankita	04/06/2021 / dhaval	P10549
Restek	32050 / Herbicide, 8000 series, 515 Surrogate [ester] 2,4-dichlorophenyl acetic acid methyl ester, 1mL, 200ug/mL, Hexane	A0172864	05/26/2025	11/26/2024 / Ankita	11/01/2021 / Abdul	P11180

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32050 / Herbicide, 8000 series, 515 Surrogate [ester] 2,4-dichlorophenyl acetic acid methyl ester, 1mL, 200ug/mL, Hexane	A0172864	05/26/2025	11/26/2024 / Ankita	11/01/2021 / Abdul	P11181
Restek	32062 / Herbicide Mix, 500/8000, Standard #4 [methyl ester] 200ug/mL, hexane, 1mL/ampul	A0155055	05/26/2025	11/26/2024 / Ankita	07/03/2023 / Abdul	P12619
Restek	32055 / Herbicide Mix, 500/8000, Standard #1 [methyl ester] 200ug/mL, hexane, 1mL/ampul	A192429	05/26/2025	11/26/2024 / Ankita	07/03/2023 / Abdul	P12629
Restek	32059 / Herbicide Mix#3 (Methyl Ester), 20000 ug/ml	A0199844	05/26/2025	11/26/2024 / Ankita	07/24/2023 / Abdul	P12686
Agilent Technologies	HBM-8151M / Chlorinated Herbicide Mixtures, Methyl Esters	0006752480	05/26/2025	11/26/2024 / Ankita	08/09/2023 / Abdul	P12708
Agilent Technologies	HBM-8151M / Chlorinated Herbicide Mixtures, Methyl Esters	0006752480	05/26/2025	11/26/2024 / Ankita	08/09/2023 / Abdul	P12708

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	HBM-8151M / Chlorinated Herbicide Mixtures, Methyl Esters	0006752480	05/26/2025	11/26/2024 / Ankita	08/09/2023 / Abdul	P12709
Agilent Technologies	HBM-8151M / Chlorinated Herbicide Mixtures, Methyl Esters	0006752480	05/26/2025	11/26/2024 / Ankita	08/09/2023 / Abdul	P12709
Restek	32049 / Herbicide, 8000 series, 515 Surrogate [free acid] 2,4-dichlorophenyl acetic acid, 1mL, 200ug/mL, MeOH	A0212676	09/26/2025	03/26/2025 / Abdul	08/16/2024 / yogesh	P13514
Restek	32049 / Herbicide, 8000 series, 515 Surrogate [free acid] 2,4-dichlorophenyl acetic acid, 1mL, 200ug/mL, MeOH	A0212676	09/26/2025	03/26/2025 / Abdul	08/16/2024 / yogesh	P13515
Agilent Technologies	HBM-8151A / Chlorinated Herbicide Mixtures, Free Acids	0006810955	10/23/2025	04/23/2025 / Abdul	09/03/2024 / Abdul	P13532
Agilent Technologies	HBM-8151A / Chlorinated Herbicide Mixtures, Free Acids	0006810955	10/23/2025	04/23/2025 / Abdul	09/03/2024 / Abdul	P13532

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	HBM-8151A / Chlorinated Herbicide Mixtures, Free Acids	0006810955	10/23/2025	04/23/2025 / Abdul	09/03/2024 / Abdul	P13533
Agilent Technologies	HBM-8151A / Chlorinated Herbicide Mixtures, Free Acids	0006810955	10/23/2025	04/23/2025 / Abdul	09/03/2024 / Abdul	P13533
Agilent Technologies	HBM-8151A / Chlorinated Herbicide Mixtures, Free Acids	0006810955	10/23/2025	04/23/2025 / Abdul	09/03/2024 / Abdul	P13534
Agilent Technologies	HBM-8151A / Chlorinated Herbicide Mixtures, Free Acids	0006810955	10/23/2025	04/23/2025 / Abdul	09/03/2024 / Abdul	P13534

Sand  
Purified  
Washed and Ignited



Material No.: 3382-05  
Batch No.: 0000243821  
Manufactured Date: 2018/04/09  
Retest Date: 2025/04/07  
Revision No: 1

## Certificate of Analysis

Test	Specification	Result
Substances Soluble in HCl	<= 0.16 %	0.01

For Laboratory, Research or Manufacturing Use  
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US  
Packaging Site: Paris Mfg Ctr & DC

E 2865

*James T Ethier*  
Jamie Ethier  
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700  
Avantor Performance Materials, LLC  
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Ether, Anhydrous  
BAKER ANALYZED® A.C.S. Reagent  
Contains BHT as a Preservative  
Suitable for Fat Extraction



Material No.: 9244-03  
Batch No.: 0000288039  
Manufactured Date: 2021/07/22  
Expiration Date: 2023/07/22  
Revision No: 1

## Certificate of Analysis

Meets ACS Reagent Chemical Requirements,

Test	Specification	Result
Assay ((C <sub>2</sub> H <sub>5</sub> ) <sub>2</sub> O) (by GC, corrected for water)	>= 99.0 %	100.0
Alcohol (C <sub>2</sub> H <sub>5</sub> OH)	Passes Test	PT
Carbonyl Compounds (as HCHO) (by polarography)	<= 0.001 %	< 0.001
Color (APHA)	<= 10	< 5
Peroxide (as H <sub>2</sub> O <sub>2</sub> )	<= 1 ppm	< 1
Preservative (BHT)	>= 7 ppm	9
Residue after Evaporation	<= 0.0010 %	< 0.0010
Titrable Acid (μeq/g)	<= 0.2	< 0.2
Water (by KF, coulometric)	<= 0.01 %	0.01


For Laboratory, Research or Manufacturing Use

Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US

Recd. by RP on 9/13/22

E 3370

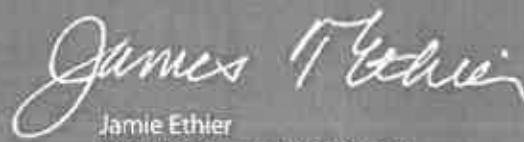  
Jamie Ethier  
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC  
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700



PRODUCTOS  
QUÍMICOS  
MONTERREY, S.A. DE C.V.

MIRADOR 201, COL. MIRADOR  
MONTERREY, N.L. MEXICO  
CP 64070  
TEL +52 81 13 52 57 57  
www.pqm.com.mx

## CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na <sub>2</sub> SO <sub>4</sub>
SPECIFICATION NUMBER :	6399	RELEASE DATE:	ABR/21/2023
LOT NUMBER :	313201		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na <sub>2</sub> SO <sub>4</sub> )	Min. 99.0%	99.7 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.1
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO <sub>4</sub> )	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.003 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreing matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.1 %
Retained on US Standard No. 60 sieve	Min. 94%	97.3 %
Through US Standard No. 60 sieve	Max. 5%	2.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %
COMMENTS		
QC: PhC Irma Belmares		

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/29/23 [E 3551]

RC-02-01, Ed. 3

Material No.: 9262-03  
Batch No.: 24G1962003  
Manufactured Date: 2024-05-23  
Expiration Date: 2025-08-22  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) – Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C <sub>6</sub> Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H <sub>2</sub> SO <sub>4</sub>	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3826

Rec'd by RP on 11/7/24

*J.Croak*

Jamie Croak

Director Quality Operations, Bioscience Production

Acetone  
BAKER RESI-ANALYZED® Reagent  
For Organic Residue Analysis



Material No.: 9254-03  
Batch No.: 24H2762008  
Manufactured Date: 2024-04-18  
Expiration Date: 2027-04-18  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
Assay ((CH <sub>3</sub> ) <sub>2</sub> CO) (by GC, corrected for water)	>= 99.4 %	100.0 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.0 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titrable Acid (μeq/g)	<= 0.3	0.2
Titrable Base (μeq/g)	<= 0.6	<0.1
Water (H <sub>2</sub> O)	<= 0.5 %	<0.1 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States  
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3902

Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA, 19087, U.S.A. Phone 610.386.1700

Acetone

BAKER RESI-ANALYZED® Reagent  
For Organic Residue Analysis



Material No.: 9254-03  
Batch No.: 24H2762008  
Manufactured Date: 2024-04-18  
Expiration Date: 2027-04-18  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
Assay ((CH <sub>3</sub> ) <sub>2</sub> CO) (by GC, corrected for water)	>= 99.4 %	100.0 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.0 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titrable Acid (μeq/g)	<= 0.3	Passes Test
Titrable Base (μeq/g)	<= 0.6	0.2
Water (H <sub>2</sub> O)	<= 0.5 %	<0.1
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	<0.1 %
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 03/31/25

E3917

Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Acetone  
BAKER RESI-ANALYZED® Reagent  
For Organic Residue Analysis



Material No.: 9254-03  
Batch No.: 24H2762008  
Manufactured Date: 2024-04-18  
Expiration Date: 2027-04-18  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
Assay ((CH <sub>3</sub> ) <sub>2</sub> CO) (by GC, corrected for water)	>= 99.4 %	100.0 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.0 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titrable Acid (μeq/g)	<= 0.3	0.2
Titrable Base (μeq/g)	<= 0.6	<0.1
Water (H <sub>2</sub> O)	<= 0.5 %	<0.1 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

E 3929

Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Hydrochloric Acid, 36.5-38.0%  
 BAKER INSTRA-ANALYZED® Reagent  
 For Trace Metal Analysis



Material No.: 9530-33  
 Batch No.: 0000281827  
 Manufactured Date: 2021/03/30  
 Retest Date: 2026/03/29  
 Revision No: 1

## Certificate of Analysis

Test	Specification	Result
ACS - Assay (as HCl) (by acid-base titrn)	36.5 – 38.0 %	37.6
ACS - Color (APHA)	<= 10	5
ACS - Residue after Ignition	<= 3 ppm	1
ACS - Specific Gravity at 60°/60°F	1.185 – 1.192	1.189
ACS - Bromide (Br)	<= 0.005 %	< 0.005
ACS - Extractable Organic Substances	<= 5 ppm	< 1
ACS - Free Chlorine (as Cl <sub>2</sub> )	<= 0.5 ppm	< 0.5
Phosphate (PO <sub>4</sub> )	<= 0.05 ppm	< 0.03
Sulfate (SO <sub>4</sub> )	<= 0.5 ppm	< 0.3
Sulfite (SO <sub>3</sub> )	<= 0.8 ppm	0.3
Ammonium (NH <sub>4</sub> )	<= 3 ppm	< 1
Trace Impurities - Arsenic (As)	<= 0.010 ppm	< 0.003
Trace Impurities - Aluminum (Al)	<= 10.0 ppb	0.5
Arsenic and Antimony (as As)	<= 5 ppb	< 3
Trace Impurities - Barium (Ba)	<= 1.0 ppb	< 0.2
Trace Impurities - Beryllium (Be)	<= 1.0 ppb	< 0.2
Trace Impurities - Bismuth (Bi)	<= 10.0 ppb	< 1.0
Trace Impurities - Boron (B)	<= 20.0 ppb	< 5.0
Trace Impurities - Cadmium (Cd)	<= 1.0 ppb	< 0.3
Trace Impurities - Calcium (Ca)	<= 50.0 ppb	15.0
Trace Impurities - Chromium (Cr)	<= 1.0 ppb	< 0.4
Trace Impurities - Cobalt (Co)	<= 1.0 ppb	< 0.3
Trace Impurities - Copper (Cu)	<= 1.0 ppb	< 0.1
Trace Impurities - Gallium (Ga)	<= 1.0 ppb	< 0.2

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Test	Specification	Result
Trace Impurities – Germanium (Ge)	<= 3.0 ppb	< 2.0
Trace Impurities – Gold (Au)	<= 4.0 ppb	3.0
Heavy Metals (as Pb)	<= 100 ppb	< 50
Trace Impurities – Iron (Fe)	<= 15.0 ppb	1.0
Trace Impurities – Lead (Pb)	<= 1.0 ppb	< 0.5
Trace Impurities – Lithium (Li)	<= 1.0 ppb	< 0.2
Trace Impurities – Magnesium (Mg)	<= 10.0 ppb	< 0.4
Trace Impurities – Manganese (Mn)	<= 1.0 ppb	< 0.4
Trace Impurities – Mercury (Hg)	<= 0.5 ppb	0.2
Trace Impurities – Molybdenum (Mo)	<= 10.0 ppb	< 5.0
Trace Impurities – Nickel (Ni)	<= 4.0 ppb	< 0.3
Trace Impurities – Niobium (Nb)	<= 1.0 ppb	< 0.2
Trace Impurities – Potassium (K)	<= 9.0 ppb	< 2.0
Trace Impurities – Selenium (Se), For Information Only	ppb	1.0
Trace Impurities – Silicon (Si)	<= 100.0 ppb	18.0
Trace Impurities – Silver (Ag)	<= 1.0 ppb	< 0.3
Trace Impurities – Sodium (Na)	<= 100.0 ppb	< 5.0
Trace Impurities – Strontium (Sr)	<= 1.0 ppb	< 0.2
Trace Impurities – Tantalum (Ta)	<= 1.0 ppb	< 0.9
Trace Impurities – Thallium (Tl)	<= 5.0 ppb	< 2.0
Trace Impurities – Tin (Sn)	<= 5.0 ppb	< 0.8
Trace Impurities – Titanium (Ti)	<= 1.0 ppb	< 0.2
Trace Impurities – Vanadium (V)	<= 1.0 ppb	< 0.2
Trace Impurities – Zinc (Zn)	<= 5.0 ppb	0.4
Trace Impurities – Zirconium (Zr)	<= 1.0 ppb	< 0.1

For Laboratory, Research or Manufacturing Use

Product Information (not specifications):

Appearance (clear, fuming liquid)

Meets ACS Specifications

Country of Origin: US

Packaging Site: Phillipsburg Mfg Ctr & DC



Jamie Ethier  
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

M 6151

R → 115125

Material No.: 9530-33  
Batch No.: 22G2862015  
Manufactured Date: 2022-06-15  
Retest Date: 2027-06-14  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
ACS - Assay (as HCl) (by acid-base titrn)	36.5 – 38.0 %	37.9 %
ACS - Color (APHA)	≤ 10	5
ACS - Residue after Ignition	≤ 3 ppm	< 1 ppm
ACS - Specific Gravity at 60°/60°F	1.185 – 1.192	1.191
ACS - Bromide (Br)	≤ 0.005 %	< 0.005 %
ACS - Extractable Organic Substances	≤ 5 ppm	< 1 ppm
ACS - Free Chlorine (as Cl <sub>2</sub> )	≤ 0.5 ppm	< 0.5 ppm
Phosphate (PO <sub>4</sub> )	≤ 0.05 ppm	< 0.03 ppm
Sulfate (SO <sub>4</sub> )	≤ 0.5 ppm	< 0.3 ppm
Sulfite (SO <sub>3</sub> )	≤ 0.8 ppm	0.3 ppm
Ammonium (NH <sub>4</sub> )	≤ 3 ppm	< 1 ppm
Trace Impurities - Arsenic (As)	≤ 0.010 ppm	< 0.003 ppm
Trace Impurities - Aluminum (Al)	≤ 10.0 ppb	1.3 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 3.0 ppb
Trace Impurities - Barium (Ba)	≤ 1.0 ppb	0.2 ppb
Trace Impurities - Beryllium (Be)	≤ 1.0 ppb	< 0.2 ppb
Trace Impurities - Bismuth (Bi)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities - Boron (B)	≤ 20.0 ppb	< 5.0 ppb
Trace Impurities - Cadmium (Cd)	≤ 1.0 ppb	< 0.3 ppb
Trace Impurities - Calcium (Ca)	≤ 50.0 ppb	163.0 ppb
Trace Impurities - Chromium (Cr)	≤ 1.0 ppb	0.7 ppb
Trace Impurities - Cobalt (Co)	≤ 1.0 ppb	< 0.3 ppb
Trace Impurities - Copper (Cu)	≤ 1.0 ppb	< 0.1 ppb
Trace Impurities - Gallium (Ga)	≤ 1.0 ppb	< 0.2 ppb
Trace Impurities - Germanium (Ge)	≤ 3.0 ppb	< 2.0 ppb
Trace Impurities - Gold (Au)	≤ 4.0 ppb	0.6 ppb
Heavy Metals (as Pb)	≤ 100 ppb	< 50 ppb
Trace Impurities - Iron (Fe)	≤ 15 ppb	6 ppb

>>> Continued on page 2 >>>

Material No.: 9530-33  
Batch No.: 22G2862015

Test	Specification	Result
Trace Impurities – Lead (Pb)	≤ 1.0 ppb	< 0.5 ppb
Trace Impurities – Lithium (Li)	≤ 1.0 ppb	< 0.2 ppb
Trace Impurities – Magnesium (Mg)	≤ 10.0 ppb	2.9 ppb
Trace Impurities – Manganese (Mn)	≤ 1.0 ppb	< 0.4 ppb
Trace Impurities – Mercury (Hg)	≤ 0.5 ppb	0.1 ppb
Trace Impurities – Molybdenum (Mo)	≤ 10.0 ppb	< 3.0 ppb
Trace Impurities – Nickel (Ni)	≤ 4.0 ppb	< 0.3 ppb
Trace Impurities – Niobium (Nb)	≤ 1.0 ppb	0.8 ppb
Trace Impurities – Potassium (K)	≤ 9.0 ppb	< 2.0 ppb
Trace Impurities – Selenium (Se), For Information Only		< 1.0 ppb
Trace Impurities – Silicon (Si)	≤ 100.0 ppb	< 10.0 ppb
Trace Impurities – Silver (Ag)	≤ 1.0 ppb	0.5 ppb
Trace Impurities – Sodium (Na)	≤ 100.0 ppb	2.3 ppb
Trace Impurities – Strontium (Sr)	≤ 1.0 ppb	< 0.2 ppb
Trace Impurities – Tantalum (Ta)	≤ 1.0 ppb	1.6 ppb
Trace Impurities – Thallium (Tl)	≤ 5.0 ppb	< 2.0 ppb
Trace Impurities – Tin (Sn)	≤ 5.0 ppb	4.0 ppb
Trace Impurities – Titanium (Ti)	≤ 1.0 ppb	1.5 ppb
Trace Impurities – Vanadium (V)	≤ 1.0 ppb	< 0.2 ppb
Trace Impurities – Zinc (Zn)	≤ 5.0 ppb	0.8 ppb
Trace Impurities – Zirconium (Zr)	≤ 1.0 ppb	0.3 ppb

>>> Continued on page 3 >>>

Hydrochloric Acid, 36.5–38.0%  
BAKER INTRA-ANALYZED® Reagent  
For Trace Metal Analysis



Material No.: 9530-33  
Batch No.: 22G2862015

Test	Specification	Result

For Laboratory, Research, or Manufacturing Use  
Product Information (not specifications):  
Appearance (clear, fuming liquid)  
Meets ACS Specifications  
Storage Condition: Store below 25 °C.

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

*James Ethier*  
Jamie Ethier  
Vice President Global Quality

**Column:**

30m x 0.25mm x 0.25 $\mu$ m  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

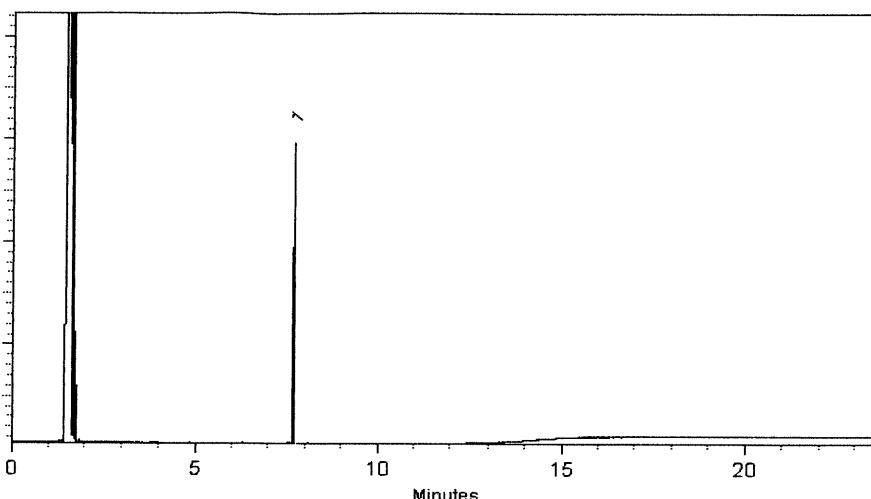

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Katelyn McGinn - Operations Tech I

Date Mixed: 28-May-2021 Balance: B345965662

*Marlina Cowan*  
Marlina Cowan - Operations Tech I

Date Passed: 02-Jun-2021

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

10/11/22  
P 11170  
P 11186  
AP  
11/02/21

# RESTEK® CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

[www.restek.com](http://www.restek.com)



## Certificate of Analysis



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

**Catalog No. :** 32050

**Lot No.:** A0172864

**Description :** 2,4-Dichlorophenylacetic Acid Methyl Ester Standard

515 Surrogate (ester) 2, 4-dichlorophenyl Acetic Acid Methyl Ester  
200 $\mu$ g/mL, Hexane, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** February 29, 2028

**Storage:** 10°C or colder

**Handling:** This product is photosensitive.

**Ship:** Ambient

### C E R T I F I E D V A L U E S

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)		
1	2,4-Dichlorophenyl acetic acid methyl ester <b>CAS #</b> 55954-23-9 <b>Purity</b> 99% (Lot CSC42194-01)	202.0 $\mu$ g/mL	+/- 1.4323 $\mu$ g/mL	+/- 6.8182 $\mu$ g/mL	Gravimetric Unstressed Stressed

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

P11177  
↓  
P11186  
AK  
v102121

**Column:**

30m x 0.25mm x 0.25 $\mu$ m  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

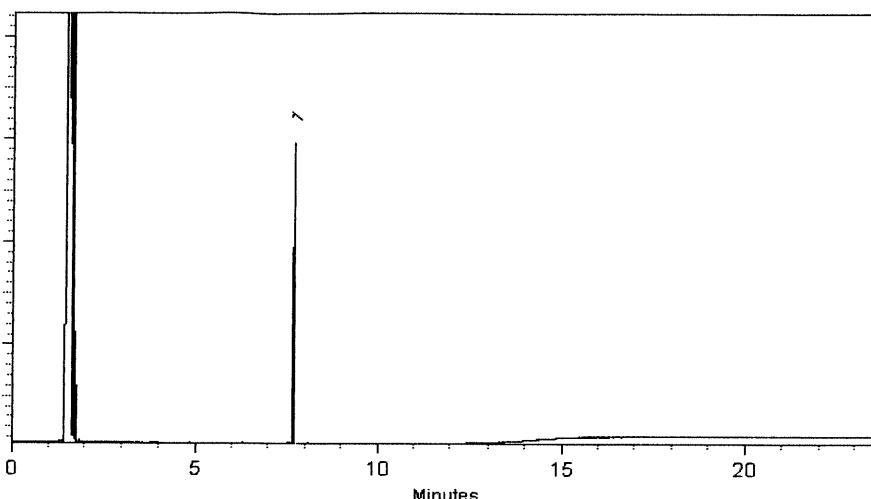

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Katelyn McGinn - Operations Tech I

Date Mixed: 28-May-2021 Balance: B345965662

*Marlina Cowan*  
Marlina Cowan - Operations Tech I

Date Passed: 02-Jun-2021

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

10/11/22  
P 10/11/22  
P 10/11/22  
AP  
10/21/21

# RESTEK® CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

[www.restek.com](http://www.restek.com)



## Certificate of Analysis



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. :	<u>32050</u>	Lot No.:	<u>A0172864</u>
Description :	2,4-Dichlorophenylacetic Acid Methyl Ester Standard		
	515 Surrogate (ester) 2, 4-dichlorophenyl Acetic Acid Methyl Ester 200µg/mL, Hexane, 1mL/ampul		
Container Size :	<u>2 mL</u>	Pkg Amt:	<u>&gt; 1 mL</u>
Expiration Date :	<u>February 29, 2028</u>	Storage:	<u>10°C or colder</u>
Handling:	<u>This product is photosensitive.</u>		
Ship:	<u>Ambient</u>		

### C E R T I F I E D V A L U E S

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)		
1	2,4-Dichlorophenyl acetic acid methyl ester CAS # 55954-23-9 (Lot CSC42194-01) Purity 99%	202.0 µg/mL	+/- 1.4323 µg/mL	+/- 6.8182 µg/mL	Gravimetric Unstressed Stressed

Solvent: Hexane  
CAS # 110-54-3  
Purity 99%

P11177  
↓  
P11186  
AK  
v102121



# CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

[www.restek.com](http://www.restek.com)



## Certificate of Analysis

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32062

Lot No.: A0155055

Description : Herbicide Mix #4/ME (Methyl Ester)

Herbicide Mix #4/ME (Methyl Ester) 200 $\mu$ g/mL,  
Hexane/Methyl-tert-butyl-ether, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : November 30, 2026

Storage: 10°C or colder

P12616 → P12620  
P12620  
Dawn  
1/15/2023

### C E R T I F I E D V A L U E S

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)		
1	3,5-Dichlorobenzoic acid methyl ester <b>CAS #</b> 2905-67-1 <b>Purity</b> 99%	200.0 $\mu$ g/mL (Lot 3903900)	+/- 1.4182 +/- 6.7507 +/- 6.7507	$\mu$ g/mL $\mu$ g/mL $\mu$ g/mL	Gravimetric Unstressed Stressed
2	4-Nitroanisole <b>CAS #</b> 100-17-4 <b>Purity</b> 99%	200.0 $\mu$ g/mL (Lot 24765/7)	+/- 1.4182 +/- 6.7507 +/- 6.7507	$\mu$ g/mL $\mu$ g/mL $\mu$ g/mL	Gravimetric Unstressed Stressed
3	Pentachloroanisole <b>CAS #</b> 1825-21-4 <b>Purity</b> 99%	200.0 $\mu$ g/mL (Lot 7921100)	+/- 1.4182 +/- 6.7507 +/- 6.7507	$\mu$ g/mL $\mu$ g/mL $\mu$ g/mL	Gravimetric Unstressed Stressed
4	Chloramben methyl ester <b>CAS #</b> 7286-84-2 <b>Purity</b> 98%	199.9 $\mu$ g/mL (Lot 6487100)	+/- 1.4176 +/- 6.7480 +/- 6.7480	$\mu$ g/mL $\mu$ g/mL $\mu$ g/mL	Gravimetric Unstressed Stressed
5	Bentazon methyl ester <b>CAS #</b> 61592-45-8 <b>Purity</b> 99%	200.0 $\mu$ g/mL (Lot 817100)	+/- 1.4182 +/- 6.7507 +/- 6.7507	$\mu$ g/mL $\mu$ g/mL $\mu$ g/mL	Gravimetric Unstressed Stressed
6	Picloram methyl ester <b>CAS #</b> 14143-55-6 <b>Purity</b> 98%	201.9 $\mu$ g/mL (Lot 386-21B)	+/- 1.4315 +/- 6.8141 +/- 6.8141	$\mu$ g/mL $\mu$ g/mL $\mu$ g/mL	Gravimetric Unstressed Stressed
7	DCPA methyl ester (Chlorthal-dimethyl) <b>CAS #</b> 1861-32-1 <b>Purity</b> 99%	200.0 $\mu$ g/mL (Lot 8008700)	+/- 1.4182 +/- 6.7507 +/- 6.7507	$\mu$ g/mL $\mu$ g/mL $\mu$ g/mL	Gravimetric Unstressed Stressed

8 Acifluorfen methyl ester  
CAS # 50594-67-7  
Purity 99% (Lot 6282300) 200.0 µg/mL +/- 1.4182 µg/mL Gravimetric  
+/- 6.7507 µg/mL Unstressed  
+/- 6.7507 µg/mL Stressed

Solvent: Hexane/Methyl-tert-butyl-ether  
CAS # 110-54-3/1634-04-4  
Purity 99%

Column:  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)


Carrier Gas:  
hydrogen-constant pressure 10 psi.

Temp. Program:  
75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

Inj. Temp:  
250°C

Det. Temp:  
330°C

Det. Type:  
FID

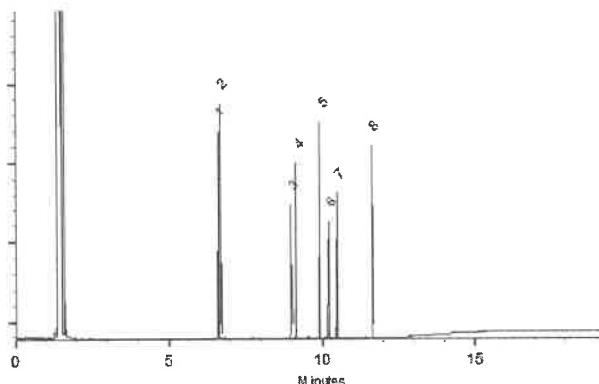

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Michael Maye*

Date Mixed: 14-Nov-2019 Balance: 1128353505

*Justine Albertson*  
Justine Albertson - Operations Tech-ARM QC

Date Passed: 18-Nov-2019

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis *chromatographic plus*



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32055

**Lot No.:** A0192429

**Description :** Herbicide Mix #1/ME (Methyl Ester)

Herbicide Mix #1/ME (Methyl Ester) 200 µg/mL, Hexane, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** December 31, 2029

**Storage:** 10°C or colder

**Handling:** This product is photosensitive.

**Ship:** Ambient

P12626  
1  
P12630  
1  
J. Davis  
7/15/2023

#### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Dicamba methyl ester	6597-78-0	11705400	99%	201.6 µg/mL	+/- 3.4204
2	Dichlorprop methyl ester	57153-17-0	11672100	99%	201.4 µg/mL	+/- 3.4170
3	2,4-D methyl ester	1928-38-7	10048000	99%	201.2 µg/mL	+/- 3.4136
4	2,4,5-TP (silvex) methyl ester	4841-20-7	6364900	99%	201.2 µg/mL	+/- 3.4136
5	2,4,5-T methyl ester	1928-37-6	6875800	98%	200.7 µg/mL	+/- 3.4052
6	Dinoseb methyl ether	6099-79-2	12914300	99%	200.8 µg/mL	+/- 3.4068
7	2,4-DB methyl ester	18625-12-2	12542000	99%	201.0 µg/mL	+/- 3.4102

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane

**CAS #** 110-54-3

**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25 $\mu$ m  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1 $\mu$ l

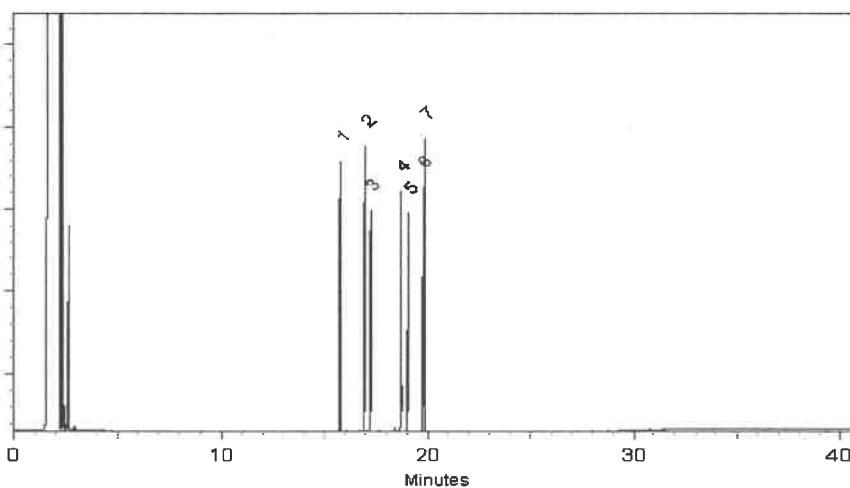

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope Riglin*  
Penelope Riglin - Operations Tech I

Date Mixed: 09-Dec-2022      Balance Serial #: 1128360905

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 12-Dec-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis *chromatographic plus*



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32059

**Lot No.:** A0199844

**Description :** Herbicide Mix #3/ME (Methyl Ester)

Herbicide Mix #3/ME (Methyl Ester) 20,000 µg/mL, Hexane, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** July 31, 2030

**Storage:** 10°C or colder

**Handling:** This product is photosensitive.

**Ship:** Ambient

P 12685 → ↘ S  
P 12689 ↗ ↘  
D. Mau J/24/23

#### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	MCPP (Mecoprop) methyl ester	23844-56-6	14546400	99%	20,035.0 µg/mL	+/- 360.1907
2	MCPA methyl ester	2436-73-9	SL201209	99%	20,055.0 µg/mL	+/- 360.5503

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane

**CAS #** 110-54-3

**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25 $\mu$ m  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1 $\mu$ l

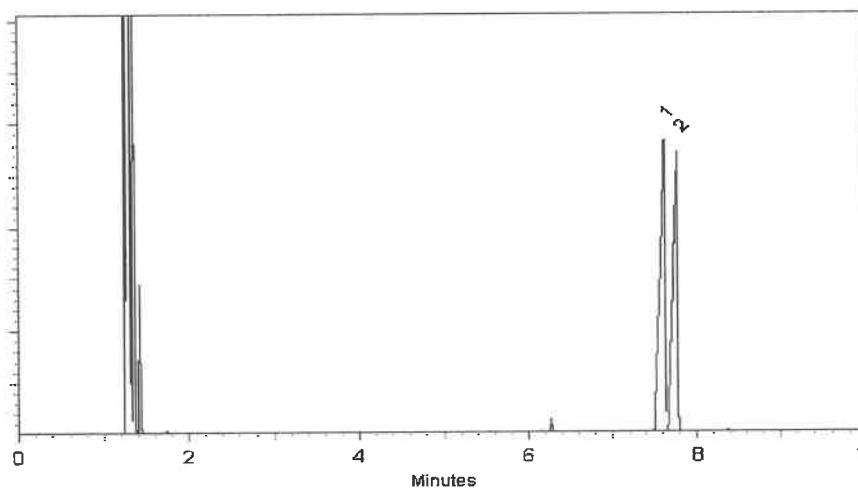

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Morgan Craighead - Mix Technician

Date Mixed: 12-Jul-2023 Balance Serial #: B442140311

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 19-Jul-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



Trusted Answers

P12706  
P12715  
10  
J. Hause  
8/15/23

ISO 17034

## Reference Material Certificate

### Product Information Sheet

**Product Name:** Chlorinated Methylated Herbicides Standard**Lot Number:** 0006752480**Product Number:** HBM-8151M-1**Lot Issue Date:** 18-Jul-2023**Storage Conditions:** Store at Room Temperature (15° to 30°C).**Expiration Date:** 31-Aug-2025

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
acifluorfen methyl ester	100.3	± 0.5 µg/mL	050594-67-7	RM03058
bentazon methyl derivative	100.2	± 0.5 µg/mL	061592-45-8	RM13829
chloramben methyl ester	100.4	± 0.5 µg/mL	007286-84-2	RM03055
2,4-D methyl ester	100.2	± 0.5 µg/mL	001928-38-7	RM03040
dalapon methyl ester	100.4	± 0.5 µg/mL	017640-02-7	RM14219
2,4-DB methyl ester	100.2	± 0.5 µg/mL	018625-12-2	RM03029
DCPA	100.2	± 0.5 µg/mL	001861-32-1	RM13426
dicamba methyl ester	100.4	± 0.5 µg/mL	006597-78-0	RM03039
methyl-3,5-dichlorobenzoate	100.1	± 0.5 µg/mL	002905-67-1	RM03048
dichlorprop methyl ester	100.4	± 0.5 µg/mL	057153-17-0	NT02086
dinoseb methyl ether	100.5	± 0.5 µg/mL	006099-79-2	RM03051
MCPA methyl ester	10031	± 50 µg/mL	002436-73-9	RM12863
MCPP methyl ester	10031	± 50 µg/mL	023844-56-6	RM20060
4-nitroanisole	100.3	± 0.5 µg/mL	000100-17-4	RM02806
pentachloroanisole	100.4	± 0.5 µg/mL	001825-21-4	RM02457
picloram methyl ester	100.2	± 0.5 µg/mL	014143-55-6	RM03044
silvex methyl ester	100.2	± 0.5 µg/mL	004841-20-7	RM03799
2,4,5-T methyl ester	100.4	± 0.5 µg/mL	001928-37-6	RM03033

**Matrix:** methanol (methyl alcohol)**Description:**


This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

**Traceability:**

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

**Homogeneity:**

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

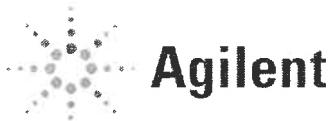

Trusted Answers

**Instructions for Use:**

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

**Safety:**

Refer to the Safety Data Sheet on [www.agilent.com](http://www.agilent.com) for information regarding this analytical reference material.

**Intended Use:**

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

**Expiration of Certification:**

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

**Maintenance of Certification:**

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois  
QMS Representative

P12706  
P12715  
10  
J. Davis  
8.15.23



ISO 17034  
Cert No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015 Quality Management System. Cert# 951215321

Page: 2 of 2

[www.agilent.com/quality/](http://www.agilent.com/quality/)  
CSD-QA-015.2

ISO 17025  
Cert No. AT-1937



Trusted Answers

P12706  
P12715  
J. DRAKE  
8/15/23

ISO 17034

## Reference Material Certificate

### Product Information Sheet

**Product Name:** Chlorinated Methylated Herbicides Standard**Lot Number:** 0006752480**Product Number:** HBM-8151M-1**Lot Issue Date:** 18-Jul-2023**Storage Conditions:** Store at Room Temperature (15° to 30°C).**Expiration Date:** 31-Aug-2025

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
acifluorfen methyl ester	100.3	± 0.5 µg/mL	050594-67-7	RM03058
bentazon methyl derivative	100.2	± 0.5 µg/mL	061592-45-8	RM13829
chloramben methyl ester	100.4	± 0.5 µg/mL	007286-84-2	RM03055
2,4-D methyl ester	100.2	± 0.5 µg/mL	001928-38-7	RM03040
dalapon methyl ester	100.4	± 0.5 µg/mL	017640-02-7	RM14219
2,4-DB methyl ester	100.2	± 0.5 µg/mL	018625-12-2	RM03029
DCPA	100.2	± 0.5 µg/mL	001861-32-1	RM13426
dicamba methyl ester	100.4	± 0.5 µg/mL	006597-78-0	RM03039
methyl-3,5-dichlorobenzoate	100.1	± 0.5 µg/mL	002905-67-1	RM03048
dichlorprop methyl ester	100.4	± 0.5 µg/mL	057153-17-0	NT02086
dinoseb methyl ether	100.5	± 0.5 µg/mL	006099-79-2	RM03051
MCPA methyl ester	10031	± 50 µg/mL	002436-73-9	RM12863
MCPP methyl ester	10031	± 50 µg/mL	023844-56-6	RM20060
4-nitroanisole	100.3	± 0.5 µg/mL	000100-17-4	RM02806
pentachloroanisole	100.4	± 0.5 µg/mL	001825-21-4	RM02457
picloram methyl ester	100.2	± 0.5 µg/mL	014143-55-6	RM03044
silvex methyl ester	100.2	± 0.5 µg/mL	004841-20-7	RM03799
2,4,5-T methyl ester	100.4	± 0.5 µg/mL	001928-37-6	RM03033

**Matrix:** methanol (methyl alcohol)**Description:**


This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

**Traceability:**

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

**Homogeneity:**

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.



# Agilent

Trusted Answers

**Instructions for Use:**

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

**Safety:**

Refer to the Safety Data Sheet on [www.agilent.com](http://www.agilent.com) for information regarding this analytical reference material.

**Intended Use:**

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

**Expiration of Certification:**

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

**Maintenance of Certification:**

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois  
QMS Representative

P12706  
P12715  
10  
J. Davis  
8.15.23



ISO 17034  
Cert No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015 Quality Management System. Cert# 951215321

Page: 2 of 2

[www.agilent.com/quality/](http://www.agilent.com/quality/)  
CSD-QA-015.2

ISO 17025  
Cert No. AT-1937



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



## Certificate of Analysis

*chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32049      **Lot No.:** A0212676

**Description :** 2,4-Dichlorophenylacetic Acid Standard  
2, 4-Dichlorophenyl Acetic Acid 200 $\mu$ g/mL, Methanol, 1mL/ampul

**Container Size :** 2 mL      **Pkg Amt:** > 1 mL

**Expiration Date :** March 31, 2027      **Storage:** 10°C or colder

**Handling:** This product is photosensitive.      **Ship:** Ambient

P13497 } Y.P.  
↓ }  
P13515 } 08/16/2024

### C E R T I F I E D   V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4-dichlorophenylacetic acid	19719-28-9	STBK3827	99%	200.0 $\mu$ g/mL	+/- 2.7154

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methanol  
**CAS #** 67-56-1  
**Purity** 99%

### Specific Reference Material Notes:

Failure to derivatize this standard will lead to incorrect quantitative results.

# Quality Confirmation Test

**Column:**

150mm x 4.6mm  
Allure C18 Cat.(#9164565)

**Flow Rate:**

1.0 ml/min.

**Mobile Phase A:**

0.14% H<sub>3</sub>PO<sub>4</sub> in water

**Mobile Phase B:**


acetonitrile

**Mobile Phase Composition:**

90% B Isocratic

**Det. Type:**

Wavelength: 220 & 254 nm

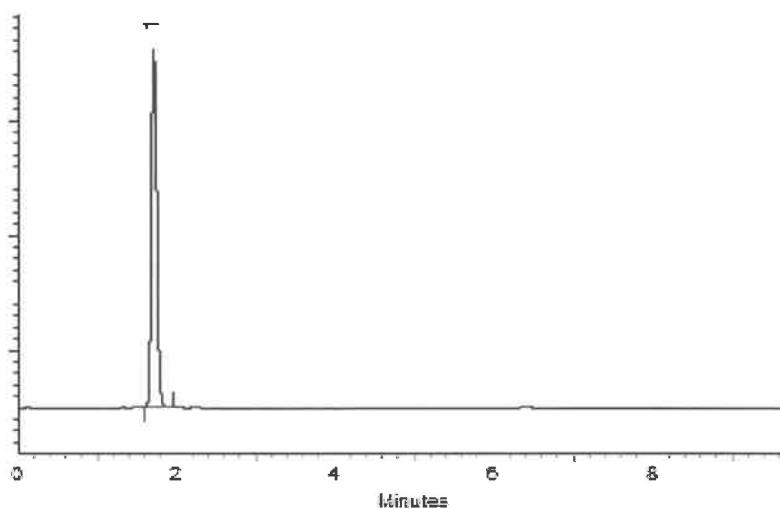

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Ethan Winiarski*  
Ethan Winiarski - Operations Tech I

Date Mixed: 11-Jun-2024 Balance Serial #: B345965662

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 13-Jun-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



## Certificate of Analysis

*chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32049      **Lot No.:** A0212676

**Description :** 2,4-Dichlorophenylacetic Acid Standard  
2, 4-Dichlorophenyl Acetic Acid 200 $\mu$ g/mL, Methanol, 1mL/ampul

**Container Size :** 2 mL      **Pkg Amt:** > 1 mL

**Expiration Date :** March 31, 2027      **Storage:** 10°C or colder

**Handling:** This product is photosensitive.      **Ship:** Ambient

P13497 } Y.P.  
↓ }  
P13515 } 08/16/20

### C E R T I F I E D   V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4-dichlorophenylacetic acid	19719-28-9	STBK3827	99%	200.0 $\mu$ g/mL	+/- 2.7154

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methanol  
**CAS #** 67-56-1  
**Purity** 99%

### Specific Reference Material Notes:

Failure to derivatize this standard will lead to incorrect quantitative results.

# Quality Confirmation Test

**Column:**

150mm x 4.6mm  
Allure C18 Cat.(#9164565)

**Flow Rate:**

1.0 ml/min.

**Mobile Phase A:**

0.14% H<sub>3</sub>PO<sub>4</sub> in water

**Mobile Phase B:**


acetonitrile

**Mobile Phase Composition:**

90% B Isocratic

**Det. Type:**

Wavelength: 220 & 254 nm

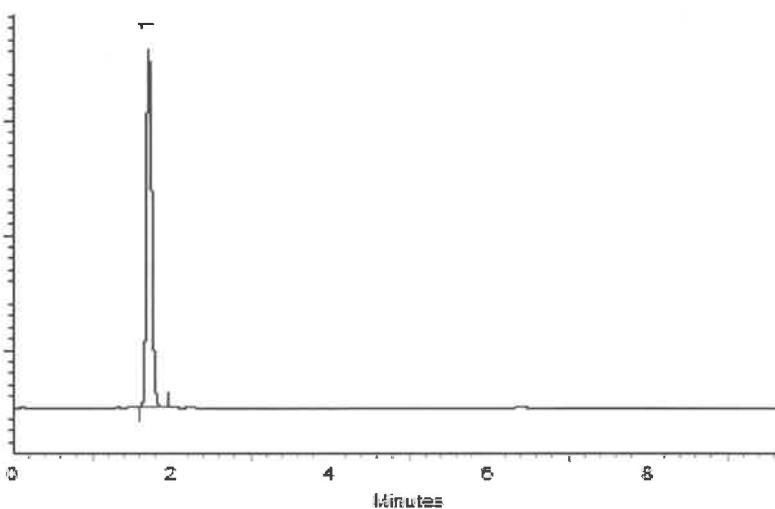

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Ethan Winiarski*  
Ethan Winiarski - Operations Tech I

Date Mixed: 11-Jun-2024 Balance Serial #: B345965662

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 13-Jun-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



Trusted Answers

ISO 17034

18

## Reference Material Certificate

### Product Information Sheet

<b>Product Name:</b>	Chlorinated Herbicides Standard	<b>Lot Number:</b>	0006810955
<b>Product Number:</b>	HBM-8151A-1	<b>Lot Issue Date:</b>	20-Aug-2024
<b>Storage Conditions:</b>	Store at Room Temperature (15° to 30°C).	<b>Expiration Date:</b>	30-Sep-2026

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
acifluorfen	100.2 ±	0.5 µg/mL	050594-66-6	NT02057
bentazon	100.4 ±	0.5 µg/mL	025057-89-0	RM21359
chloramben	100.3 ±	0.5 µg/mL	000133-90-4	RM02698
2,4-D	100.4 ±	0.5 µg/mL	000094-75-7	RM17172
dalapon	100.4 ±	0.5 µg/mL	000075-99-0	RM19677
2,4-DB	100.1 ±	0.5 µg/mL	000094-82-6	RM02866
tetrachloroterephthalic acid	100.4 ±	0.5 µg/mL	002136-79-0	RM15140
dicamba	100.3 ±	0.5 µg/mL	001918-00-9	RM22113
3,5-dichlorobenzoic acid	100.4 ±	0.5 µg/mL	000051-36-5	RM02768
dichlorprop	100.2 ±	0.5 µg/mL	000120-36-5	RM21688
dinoseb	100.3 ±	0.5 µg/mL	000088-85-7	RM22275
MCPA	10019 ±	50 µg/mL	000094-74-6	RM12220
MCPP (mecoprop)	10011 ±	50 µg/mL	000093-65-2	RM09273
4-nitrophenol	100.4 ±	0.5 µg/mL	000100-02-7	RM02391
pentachlorophenol	100.2 ±	0.5 µg/mL	000087-86-5	RM02474
picloram	100.4 ±	0.5 µg/mL	001918-02-1	RM20442
silvex	100.5 ±	0.5 µg/mL	000093-72-1	RM22116
2,4,5-T	100.3 ±	0.5 µg/mL	000093-76-5	RM19314

**Matrix:** methanol (methyl alcohol)

#### Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

#### Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

#### Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Page: 1 of 2

CSD-QA-015.2

ISO 17025  
Cert No. AT-1937

250 Smith Street North Kingstown, Rhode Island 02852   
[www.agilent.com/quality](http://www.agilent.com/quality)



Trusted Answers

ISO 17034

18

## Reference Material Certificate

### Product Information Sheet

<b>Product Name:</b>	Chlorinated Herbicides Standard	<b>Lot Number:</b>	0006810955
<b>Product Number:</b>	HBM-8151A-1	<b>Lot Issue Date:</b>	20-Aug-2024
<b>Storage Conditions:</b>	Store at Room Temperature (15° to 30°C).	<b>Expiration Date:</b>	30-Sep-2026

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
acifluorfen	100.2 ±	0.5 µg/mL	050594-66-6	NT02057
bentazon	100.4 ±	0.5 µg/mL	025057-89-0	RM21359
chloramben	100.3 ±	0.5 µg/mL	000133-90-4	RM02698
2,4-D	100.4 ±	0.5 µg/mL	000094-75-7	RM17172
dalapon	100.4 ±	0.5 µg/mL	000075-99-0	RM19677
2,4-DB	100.1 ±	0.5 µg/mL	000094-82-6	RM02866
tetrachloroterephthalic acid	100.4 ±	0.5 µg/mL	002136-79-0	RM15140
dicamba	100.3 ±	0.5 µg/mL	001918-00-9	RM22113
3,5-dichlorobenzoic acid	100.4 ±	0.5 µg/mL	000051-36-5	RM02768
dichlorprop	100.2 ±	0.5 µg/mL	000120-36-5	RM21688
dinoseb	100.3 ±	0.5 µg/mL	000088-85-7	RM22275
MCPA	10019 ±	50 µg/mL	000094-74-6	RM12220
MCPP (mecoprop)	10011 ±	50 µg/mL	000093-65-2	RM09273
4-nitrophenol	100.4 ±	0.5 µg/mL	000100-02-7	RM02391
pentachlorophenol	100.2 ±	0.5 µg/mL	000087-86-5	RM02474
picloram	100.4 ±	0.5 µg/mL	001918-02-1	RM20442
silvex	100.5 ±	0.5 µg/mL	000093-72-1	RM22116
2,4,5-T	100.3 ±	0.5 µg/mL	000093-76-5	RM19314

**Matrix:** methanol (methyl alcohol)

#### Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

#### Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

#### Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Page: 1 of 2

CSD-QA-015.2

ISO 17025  
Cert No. AT-1937

250 Smith Street North Kingstown, Rhode Island 02852  www.agilent.com/quality



Trusted Answers

ISO 17034

18

## Reference Material Certificate

### Product Information Sheet

<b>Product Name:</b>	Chlorinated Herbicides Standard	<b>Lot Number:</b>	0006810955
<b>Product Number:</b>	HBM-8151A-1	<b>Lot Issue Date:</b>	20-Aug-2024
<b>Storage Conditions:</b>	Store at Room Temperature (15° to 30°C).	<b>Expiration Date:</b>	30-Sep-2026

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
acifluorfen	100.2 ±	0.5 µg/mL	050594-66-6	NT02057
bentazon	100.4 ±	0.5 µg/mL	025057-89-0	RM21359
chloramben	100.3 ±	0.5 µg/mL	000133-90-4	RM02698
2,4-D	100.4 ±	0.5 µg/mL	000094-75-7	RM17172
dalapon	100.4 ±	0.5 µg/mL	000075-99-0	RM19677
2,4-DB	100.1 ±	0.5 µg/mL	000094-82-6	RM02866
tetrachloroterephthalic acid	100.4 ±	0.5 µg/mL	002136-79-0	RM15140
dicamba	100.3 ±	0.5 µg/mL	001918-00-9	RM22113
3,5-dichlorobenzoic acid	100.4 ±	0.5 µg/mL	000051-36-5	RM02768
dichlorprop	100.2 ±	0.5 µg/mL	000120-36-5	RM21688
dinoseb	100.3 ±	0.5 µg/mL	000088-85-7	RM22275
MCPA	10019 ±	50 µg/mL	000094-74-6	RM12220
MCPP (mecoprop)	10011 ±	50 µg/mL	000093-65-2	RM09273
4-nitrophenol	100.4 ±	0.5 µg/mL	000100-02-7	RM02391
pentachlorophenol	100.2 ±	0.5 µg/mL	000087-86-5	RM02474
picloram	100.4 ±	0.5 µg/mL	001918-02-1	RM20442
silvex	100.5 ±	0.5 µg/mL	000093-72-1	RM22116
2,4,5-T	100.3 ±	0.5 µg/mL	000093-76-5	RM19314

**Matrix:** methanol (methyl alcohol)

#### Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

#### Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

#### Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Page: 1 of 2

CSD-QA-015.2

ISO 17025  
Cert No. AT-1937

250 Smith Street North Kingstown, Rhode Island 02852  www.agilent.com/quality



# SHIPPING DOCUMENTS

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

Chemtech

Phone: (908) 789-8900  
Fax: (908) 789-8922

284 Sheffield Street, Mountainside, NJ 07092

**Company Name:** Nobis Group

**Address:** 55 Technology Dr Suite 101, Lowell, MA 01851

Phone: 978-703-6014

Project Name: Raymark

**Project Location:** Stratford, CT

**Project Number:** 95700

Project Manager: Adam Roy

Con-Test Quote Name/Number:

**Invoice Recipient:**

Sampled By: S. Stone

Con-Test      Standard ID / Registration

**Work Order#** **Client Sample ID / Description**

<http://www.contestlabs.com>

Doc # 381 Rev 4\_01/08/2020

Q1883

Page 1 of 1

## **CHAIN OF CUSTODY RECORD**

39 Spruce Street  
East Longmeadow, MA 01028

**Lab Comments:**

3.6<sup>c</sup> ADJUST FACTOR +1  
IR&UN #1

**Disclaimer:** Con-Test Labs is not responsible for any omitted information on the Chain of Custody. The Chain of Custody is a legal document that must be complete and accurate and is used to determine what analyses the laboratory will perform. Any missing information is not the laboratory's responsibility. Con-Test values your partnership on each project and will try to assist with missing information, but will not be held accountable.

### Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

## LOGIN REPORT/SAMPLE TRANSFER

Order ID : Q1883	NOBI03	Order Date : 4/25/2025 10:10:00 AM	Project Mgr :
Client Name : Nobis Group		Project Name : Raymark Superfund Site	Report Type : Level 4
Client Contact : Adam Roy		Receive DateTime : 4/25/2025 9:30:00 AM	EDD Type : EQUIS
Invoice Name : Nobis Group		Purchase Order :	Hard Copy Date :
Invoice Contact : Adam Roy			Date Signoff :

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DU <sup>E</sup> DATES
Q1883-01	OU4-PCS-TC-27-042325	Solid	04/23/2025	12:45	VOCMS Group3		8260D	10 Bus. Days	
Q1883-03	OU4-PCS-TC-28-042325	Solid	04/23/2025	12:50	VOCMS Group3		8260D	10 Bus. Days	
Q1883-05	OU4-PCS-TC-29-042325	Solid	04/23/2025	13:00	VOCMS Group3		8260D	10 Bus. Days	
Q1883-07	OU4-PCS-TC-30-042325	Solid	04/23/2025	13:15	VOCMS Group3		8260D	10 Bus. Days	
Q1883-09	OU4-PCS-TC-31-042325	Solid	04/23/2025	13:20	VOCMS Group3		8260D	10 Bus. Days	
Q1883-11	OU4-PCS-TC-32-042325	Solid	04/23/2025	13:30	VOCMS Group3		8260D	10 Bus. Days	
Q1883-13	OU4-PCS-18-042325 VSL	Solid	04/23/2025	11:20	VOCMS Group3		8260D	10 Bus. Days	
Q1883-15	OU4-PCS-19-042325 VSL	Solid	04/23/2025	11:50	VOCMS Group3		8260D	10 Bus. Days	

## LOGIN REPORT/SAMPLE TRANSFER

Order ID : Q1883	NOBI03	Order Date : 4/25/2025 10:10:00 AM	Project Mgr :
Client Name : Nobis Group		Project Name : Raymark Superfund Site	Report Type : Level 4
Client Contact : Adam Roy		Receive DateTime : 4/25/2025 9:30:00 AM	EDD Type : EQUIS
Invoice Name : Nobis Group		Purchase Order :	Hard Copy Date :
Invoice Contact : Adam Roy			Date Signoff :

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DU <sup>E</sup> DATES
Q1883-17	SO-TB-01-042325	Solid	04/23/2025	08:00	VOCMS Group3		8260D	10 Bus. Days	
					VOCMS Group3		8260D	10 Bus. Days	

Relinquished By :   
 Date / Time : 4/25/25 11:20

Received By : Sem  
 Date / Time : 04/25/25 11:20 0246  
 Storage Area : VOA Refrigerator Room F22

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029919.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 11:01  
 Operator : AR\AJ  
 Sample : HSTDICC200  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**HSTDICC200**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 12:21:29 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:13:04 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.942 7.467 607.6E6 161.5E6 232.374 221.995

Target Compounds

1) T	Dalapon	2.449	2.525	1000.1E6	380.3E6	229.017	208.714
2) T	3,5-DICHL...	6.146	6.463	802.7E6	206.9E6	212.813	205.094
3) T	4-Nitroph...	6.733	7.001	383.7E6	162.2E6	206.288	204.354
5) T	DICAMBA	7.118	7.653	2150.4E6	774.6E6	208.534	196.353
6) T	MCPP	7.295	7.758	112.8E6	31299306	18.132	18.050
7) T	MCPA	7.437	7.988	169.4E6	48918025	19.260	20.374
8) T	DICHLORPROP	7.799	8.348	584.1E6	218.7E6	217.778	210.088
9) T	2,4-D	8.021	8.661	635.4E6	244.2E6	214.810	209.141
10) T	Pentachlo...	8.298	9.163	7828.1E6	4208.5E6	211.528	201.368
11) T	2,4,5-TP ...	8.862	9.542	3080.5E6	1679.9E6	212.416	201.589
12) T	2,4,5-T	9.145	9.947	3136.0E6	1619.8E6	213.126	204.001
13) T	2,4-DB	9.704	10.507	483.4E6	167.7E6	206.590	206.030
14) T	DINOSEB	10.866	10.881	2266.8E6	1229.2E6	211.888	204.977
15) T	Picloram	10.686	11.919	3927.9E6	4718.9E6	208.185	386.108 #
16) T	DCPA	11.167	11.919	3823.9E6	4718.9E6	214.204	402.928 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029919.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 11:01  
 Operator : AR\AJ  
 Sample : HSTDICC200  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDICC200

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 12:21:29 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:13:04 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

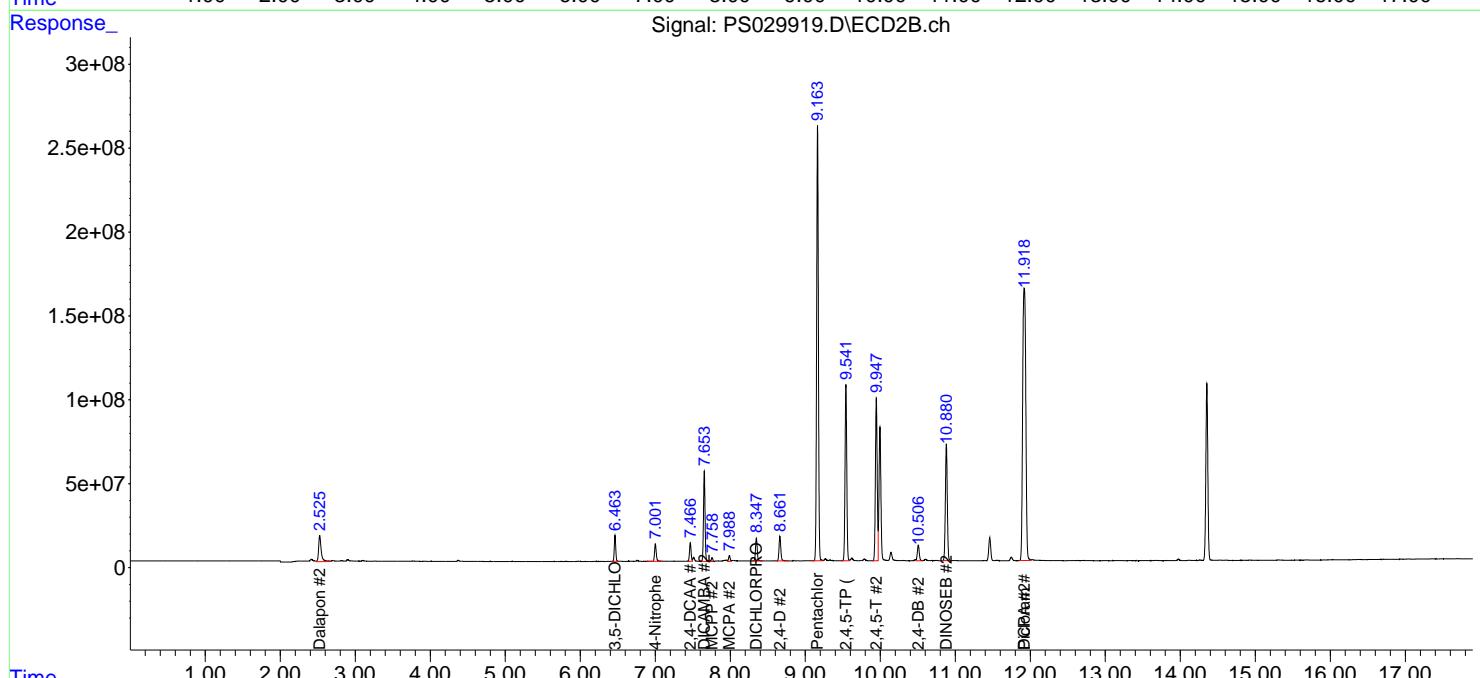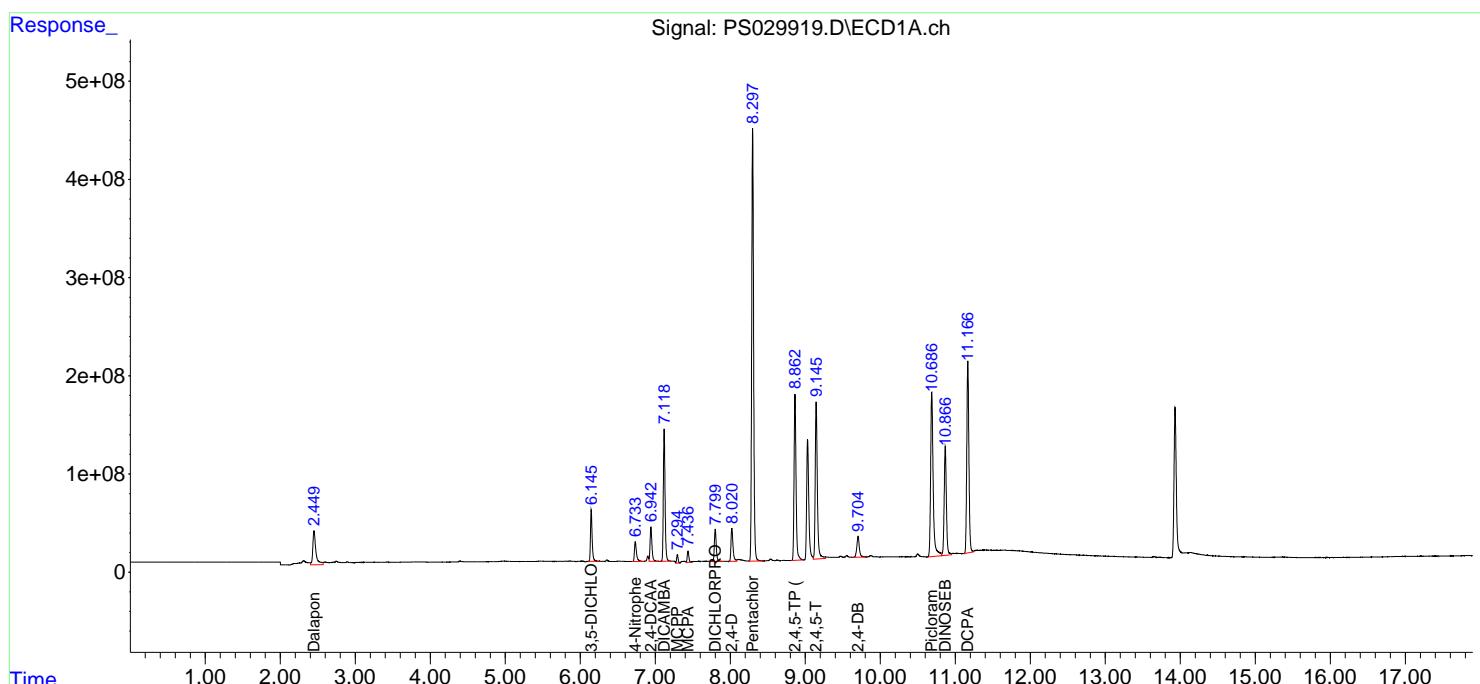

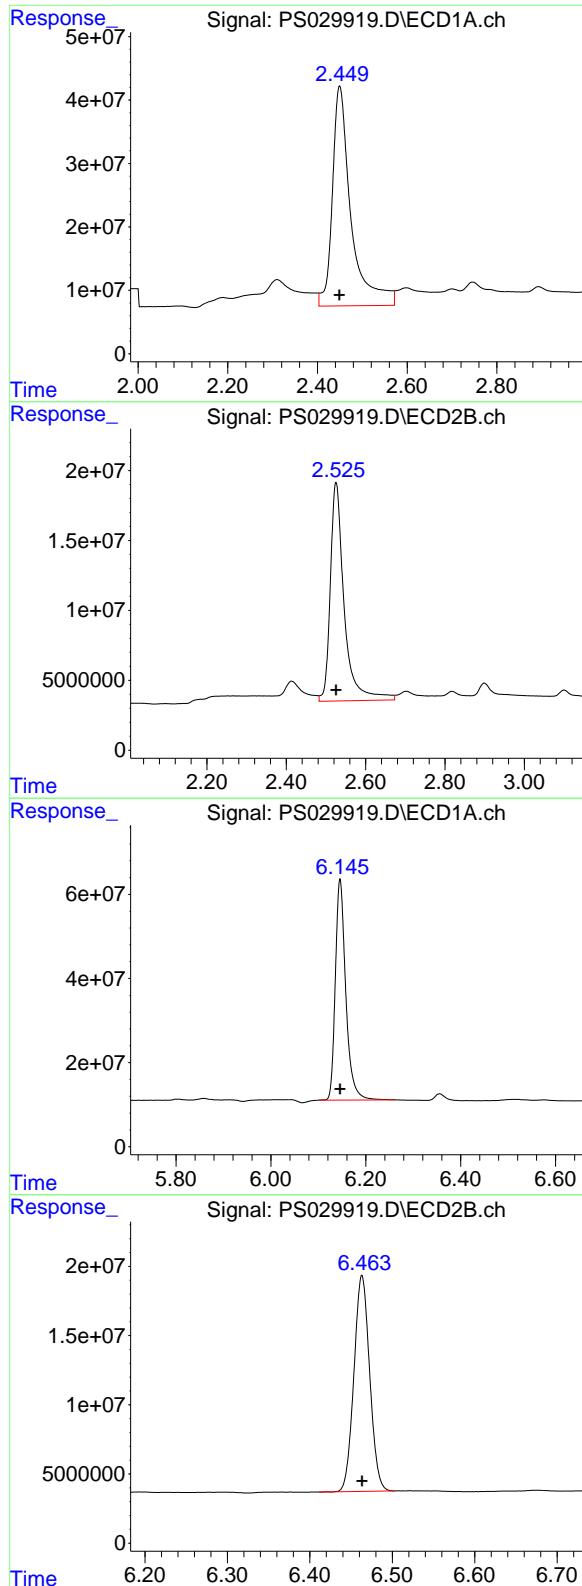

#1 Dalapon

R.T.: 2.449 min  
 Delta R.T.: 0.000 min  
 Response: 1000077310  
 Conc: 229.02 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDICC200

#1 Dalapon


R.T.: 2.525 min  
 Delta R.T.: 0.000 min  
 Response: 380305456  
 Conc: 208.71 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.146 min  
 Delta R.T.: 0.000 min  
 Response: 802682173  
 Conc: 212.81 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.463 min  
 Delta R.T.: 0.000 min  
 Response: 206925954  
 Conc: 205.09 ng/ml

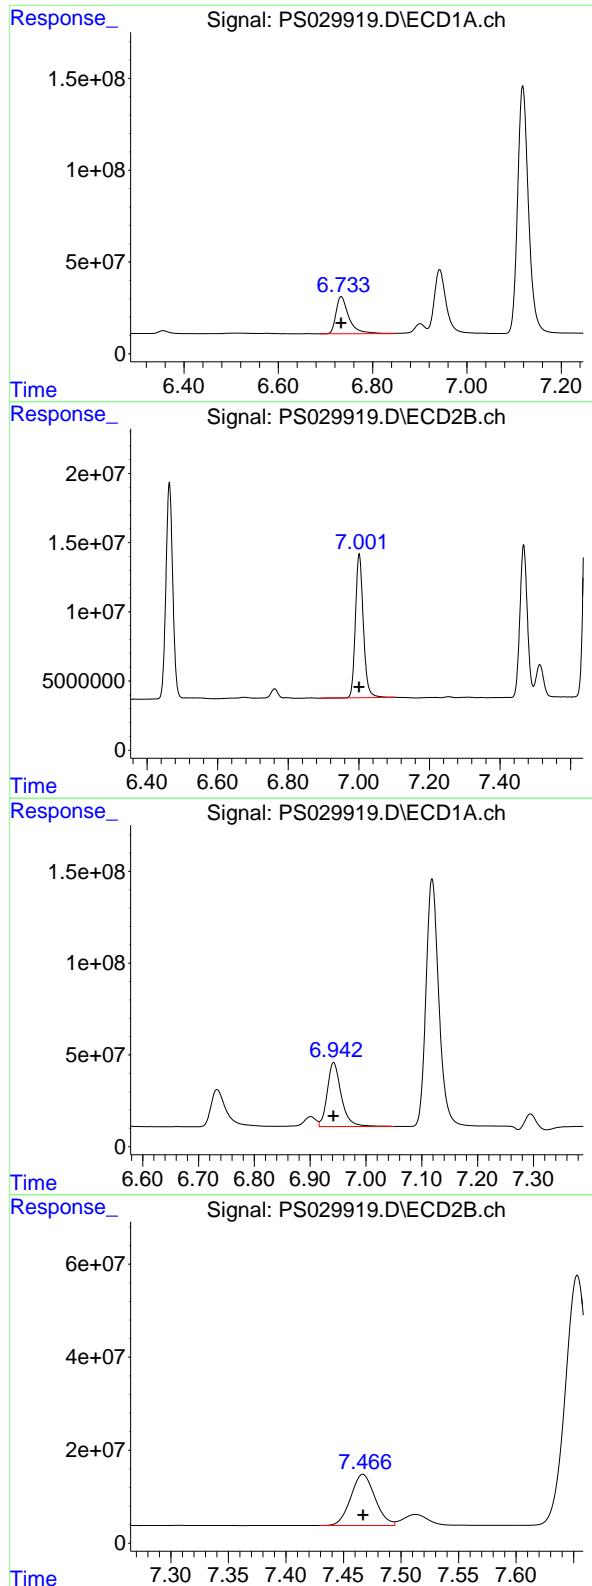

#3 4-Nitrophenol

R.T.: 6.733 min  
Delta R.T.: 0.000 min  
Response: 383695461  
Conc: 206.29 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** HSTDICC200

#3 4-Nitrophenol


R.T.: 7.001 min  
Delta R.T.: 0.000 min  
Response: 162220636  
Conc: 204.35 ng/ml

#4 2,4-DCAA

R.T.: 6.942 min  
Delta R.T.: 0.000 min  
Response: 607649568  
Conc: 232.37 ng/ml

#4 2,4-DCAA

R.T.: 7.467 min  
Delta R.T.: 0.000 min  
Response: 161527736  
Conc: 221.99 ng/ml

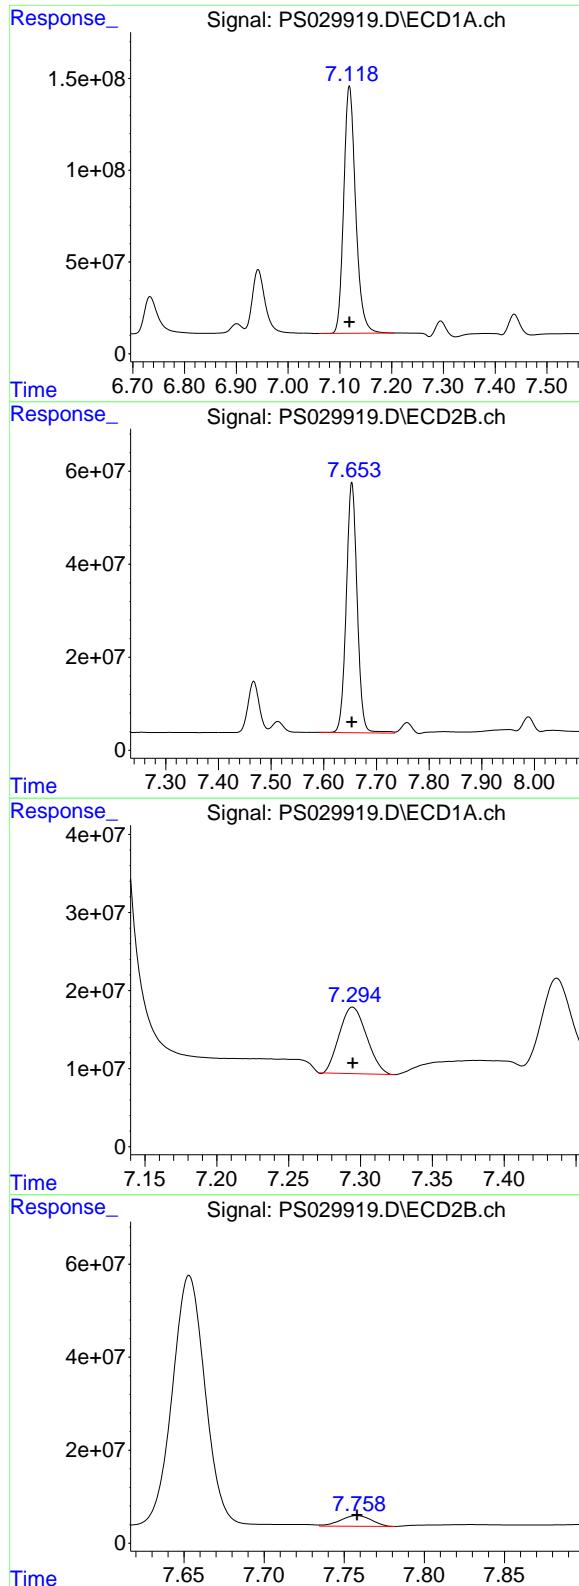

#5 DICAMBA

R.T.: 7.118 min  
Delta R.T.: 0.000 min **Instrument:**  
Response: 2150414141 ECD\_S  
Conc: 208.53 ng/ml **ClientSampleId:**  
HSTDICC200

#5 DICAMBA


R.T.: 7.653 min  
Delta R.T.: 0.000 min  
Response: 774585769  
Conc: 196.35 ng/ml

#6 MCPP

R.T.: 7.295 min  
Delta R.T.: 0.000 min  
Response: 112779199  
Conc: 18.13 ug/ml

#6 MCPP

R.T.: 7.758 min  
Delta R.T.: 0.000 min  
Response: 31299306  
Conc: 18.05 ug/ml

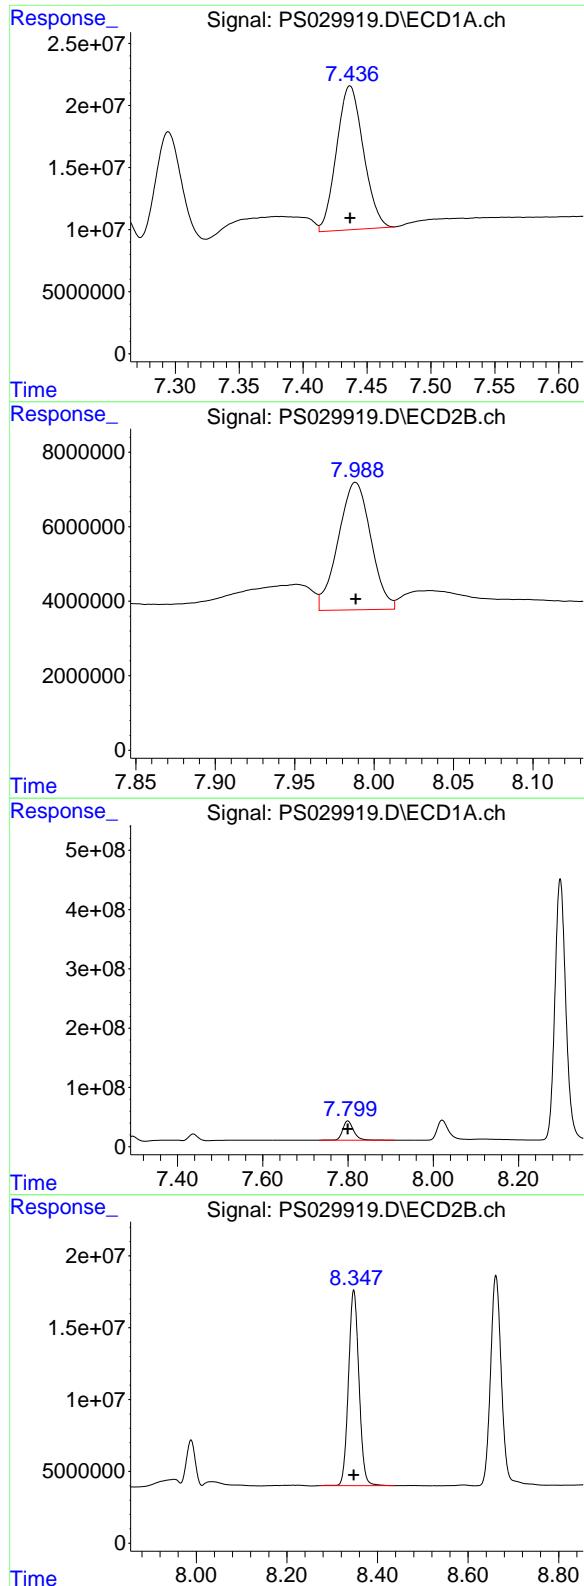

#7 MCPA

R.T.: 7.437 min  
 Delta R.T.: 0.000 min  
 Response: 169402932  
 Conc: 19.26 ug/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDICC200

#7 MCPA


R.T.: 7.988 min  
 Delta R.T.: 0.000 min  
 Response: 48918025  
 Conc: 20.37 ug/ml

#8 DICHLORPROP

R.T.: 7.799 min  
 Delta R.T.: 0.000 min  
 Response: 584067087  
 Conc: 217.78 ng/ml

#8 DICHLORPROP

R.T.: 8.348 min  
 Delta R.T.: 0.000 min  
 Response: 218723918  
 Conc: 210.09 ng/ml

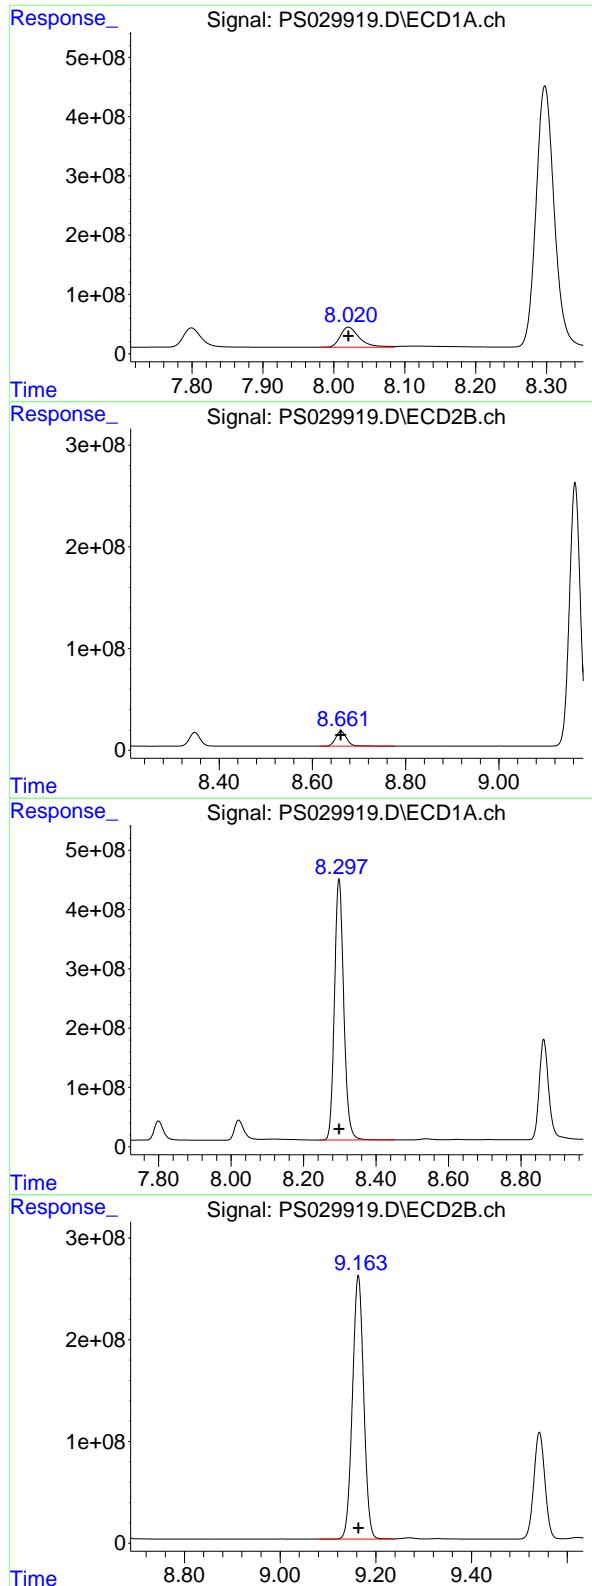

#9 2,4-D

R.T.: 8.021 min  
Delta R.T.: 0.000 min  
Response: 635351443  
Conc: 214.81 ng/ml

Instrument: ECD\_S  
ClientSampleId: HSTDICC200

#9 2,4-D


R.T.: 8.661 min  
Delta R.T.: 0.000 min  
Response: 244229801  
Conc: 209.14 ng/ml

#10 Pentachlorophenol

R.T.: 8.298 min  
Delta R.T.: 0.000 min  
Response: 7828106091  
Conc: 211.53 ng/ml

#10 Pentachlorophenol

R.T.: 9.163 min  
Delta R.T.: 0.000 min  
Response: 4208465177  
Conc: 201.37 ng/ml

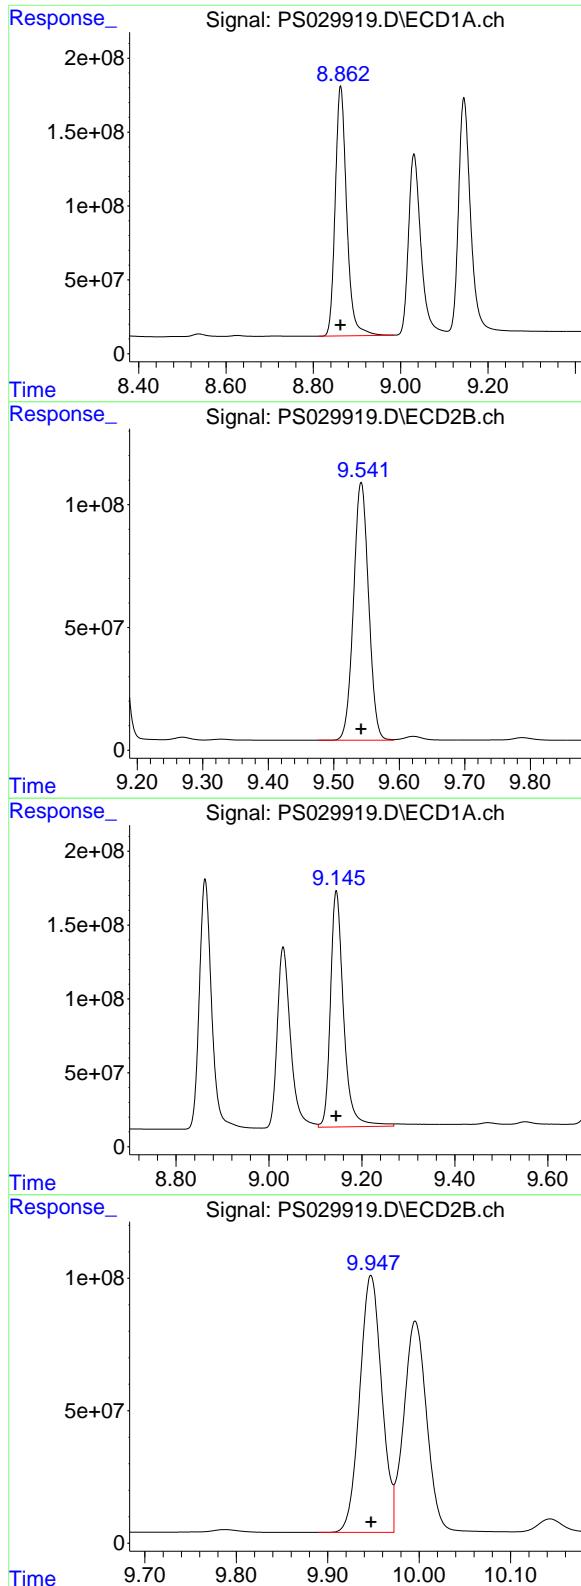

#11 2,4,5-TP (SILVEX)

R.T.: 8.862 min  
Delta R.T.: 0.000 min  
Response: 3080510531  
Conc: 212.42 ng/ml

Instrument: ECD\_S  
ClientSampleId: HSTDICC200

#11 2,4,5-TP (SILVEX)


R.T.: 9.542 min  
Delta R.T.: 0.000 min  
Response: 1679940962  
Conc: 201.59 ng/ml

#12 2,4,5-T

R.T.: 9.145 min  
Delta R.T.: 0.000 min  
Response: 3136007230  
Conc: 213.13 ng/ml

#12 2,4,5-T

R.T.: 9.947 min  
Delta R.T.: 0.000 min  
Response: 1619770655  
Conc: 204.00 ng/ml

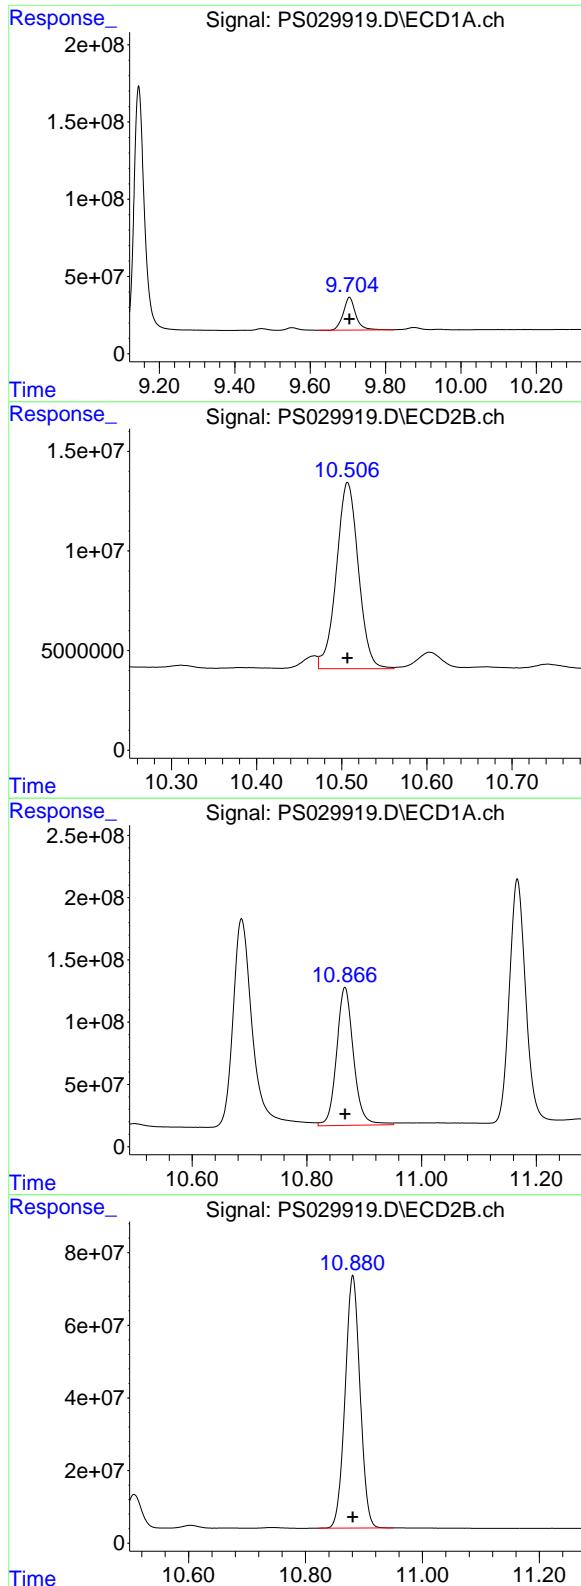

#13 2,4-DB

R.T.: 9.704 min  
Delta R.T.: 0.000 min  
Response: 483428317  
Conc: 206.59 ng/ml

Instrument: ECD\_S  
ClientSampleId: HSTDICC200

#13 2,4-DB


R.T.: 10.507 min  
Delta R.T.: 0.000 min  
Response: 167703688  
Conc: 206.03 ng/ml

#14 DINOSEB

R.T.: 10.866 min  
Delta R.T.: 0.000 min  
Response: 2266806582  
Conc: 211.89 ng/ml

#14 DINOSEB

R.T.: 10.881 min  
Delta R.T.: 0.000 min  
Response: 1229173921  
Conc: 204.98 ng/ml

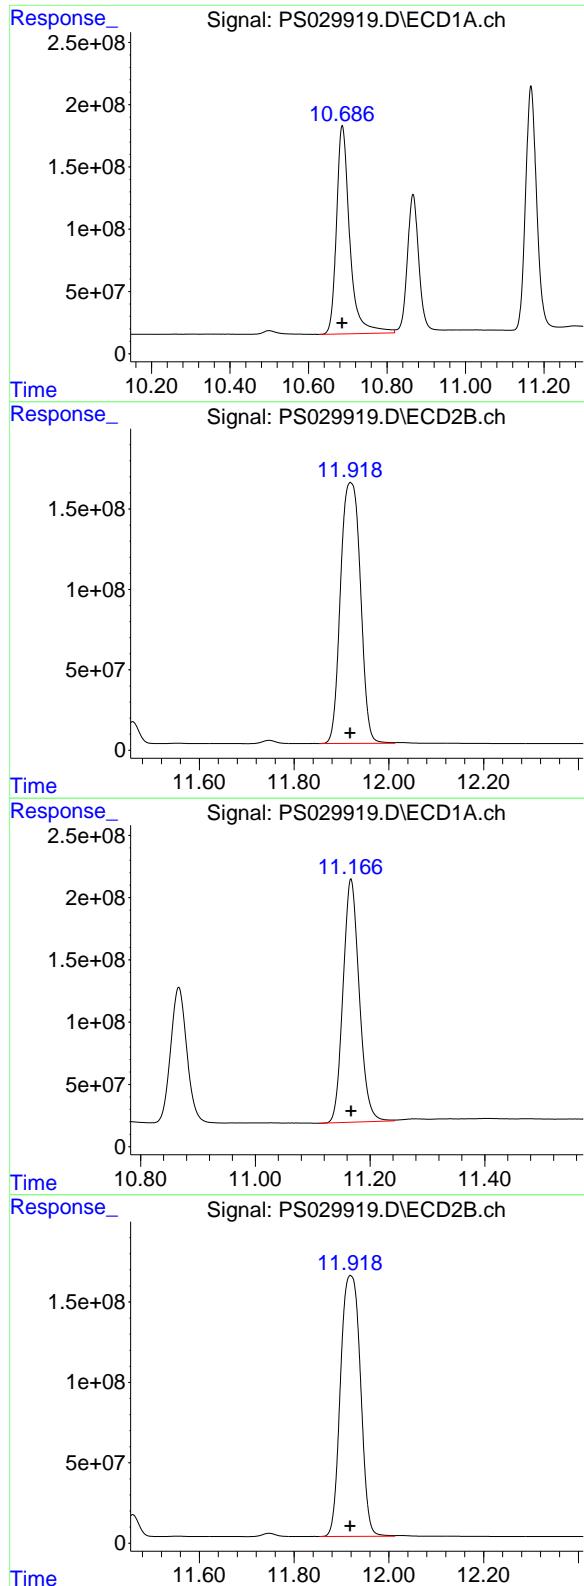

#15 Picloram

R.T.: 10.686 min  
 Delta R.T.: 0.000 min  
 Response: 3927930714  
 Conc: 208.18 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDICC200

#15 Picloram

R.T.: 11.919 min  
 Delta R.T.: 0.000 min  
 Response: 4718859422  
 Conc: 386.11 ng/ml

#16 DCPA

R.T.: 11.167 min  
 Delta R.T.: 0.000 min  
 Response: 3823873526  
 Conc: 214.20 ng/ml

#16 DCPA

R.T.: 11.919 min  
 Delta R.T.: 0.000 min  
 Response: 4718859422  
 Conc: 402.93 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029920.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 11:25  
 Operator : AR\AJ  
 Sample : HSTDICC500  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**HSTDICC500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 12:18:02 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:13:04 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.942 7.467 1231.8E6 346.2E6 512.532 503.455

Target Compounds

1) T	Dalapon	2.449	2.525	1929.5E6	780.3E6	468.186	462.137
2) T	3,5-DICHL...	6.146	6.463	1662.7E6	449.2E6	475.061	469.317
3) T	4-Nitroph...	6.733	7.001	802.3E6	342.6E6	462.200	459.862
5) T	DICAMBA	7.118	7.653	4642.9E6	1792.4E6	476.252	464.683
6) T	MCPP	7.296	7.759	290.7E6	82241844	45.918	46.500
7) T	MCPA	7.438	7.990	399.1E6	105.5E6	46.188	46.156
8) T	DICHLORPROP	7.799	8.347	1186.8E6	464.3E6	480.564	473.759
9) T	2,4-D	8.020	8.661	1315.0E6	523.2E6	478.744	474.742
10) T	Pentachlo...	8.297	9.164	16887.6E6	9661.5E6	483.734	476.543
11) T	2,4,5-TP ...	8.862	9.542	6584.5E6	3838.6E6	482.498	475.108
12) T	2,4,5-T	9.145	9.948	6674.4E6	3641.9E6	482.992	476.224
13) T	2,4-DB	9.703	10.507	1071.1E6	362.7E6	478.618	465.162
14) T	DINOSEB	10.866	10.881	4764.3E6	2699.3E6	475.549	471.423
15) T	Picloram	10.685	11.922	8585.2E6	11084.9E6	477.895	918.963 #
16) T	DCPA	11.167	11.922	8208.3E6	11084.9E6	488.029	986.265 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029920.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 11:25  
 Operator : AR\AJ  
 Sample : HSTDICC500  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1



Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDICC500


Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 12:18:02 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:13:04 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l

Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2

Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

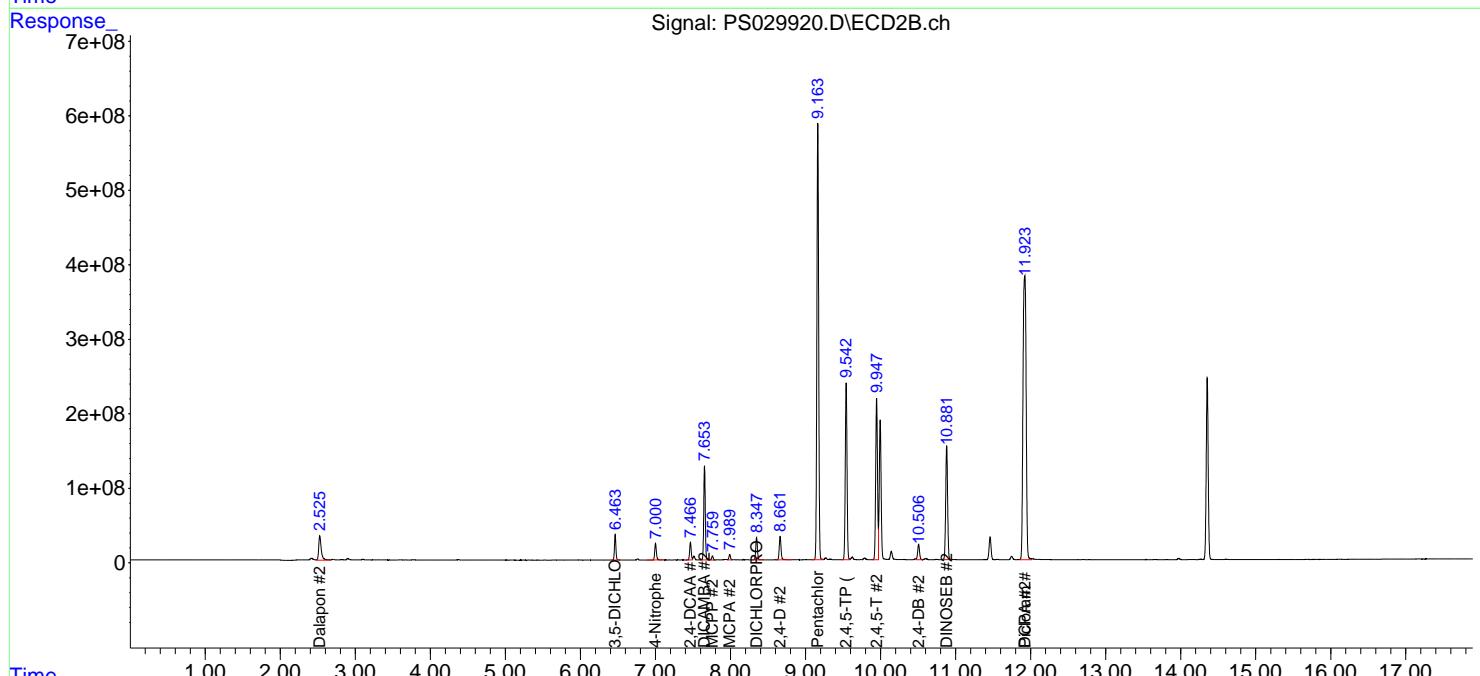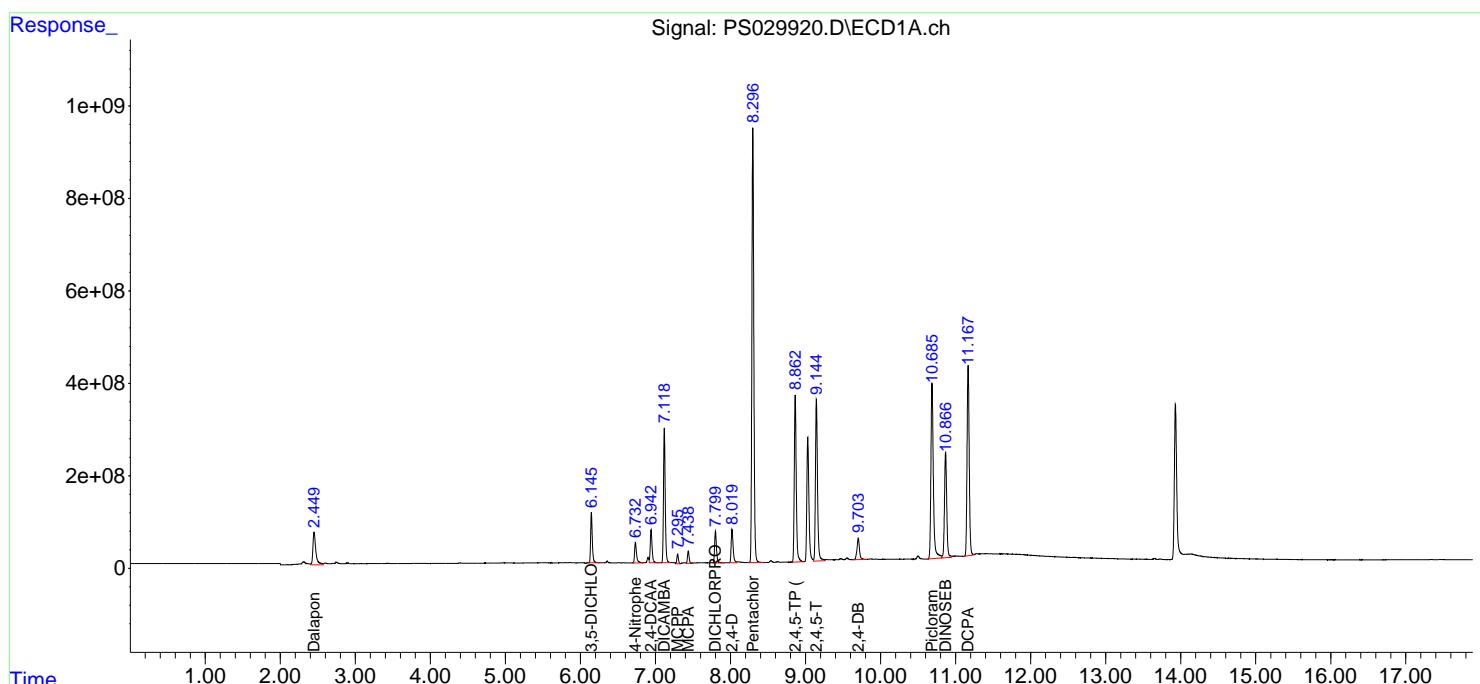

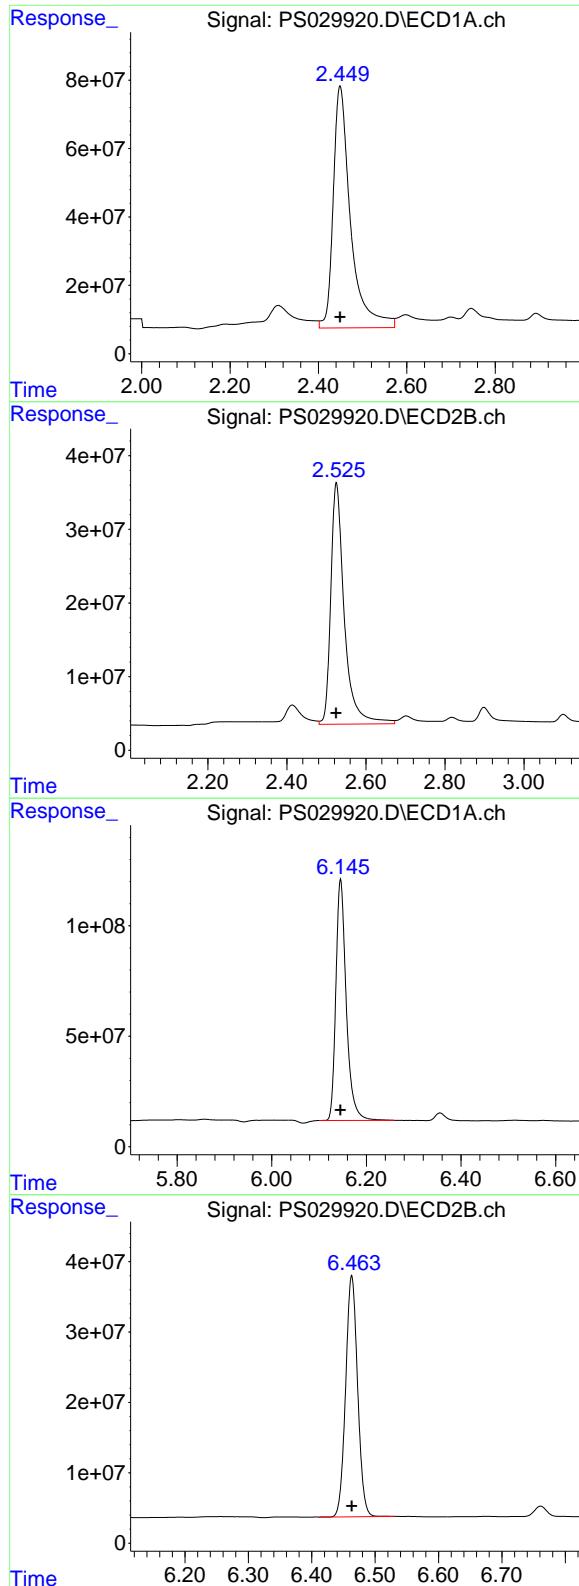

#1 Dalapon

R.T.: 2.449 min  
 Delta R.T.: 0.000 min  
 Response: 1929533765  
 Conc: 468.19 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDICC500

#1 Dalapon


R.T.: 2.525 min  
 Delta R.T.: 0.000 min  
 Response: 780277133  
 Conc: 462.14 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.146 min  
 Delta R.T.: 0.000 min  
 Response: 1662675840  
 Conc: 475.06 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.463 min  
 Delta R.T.: 0.000 min  
 Response: 449204324  
 Conc: 469.32 ng/ml

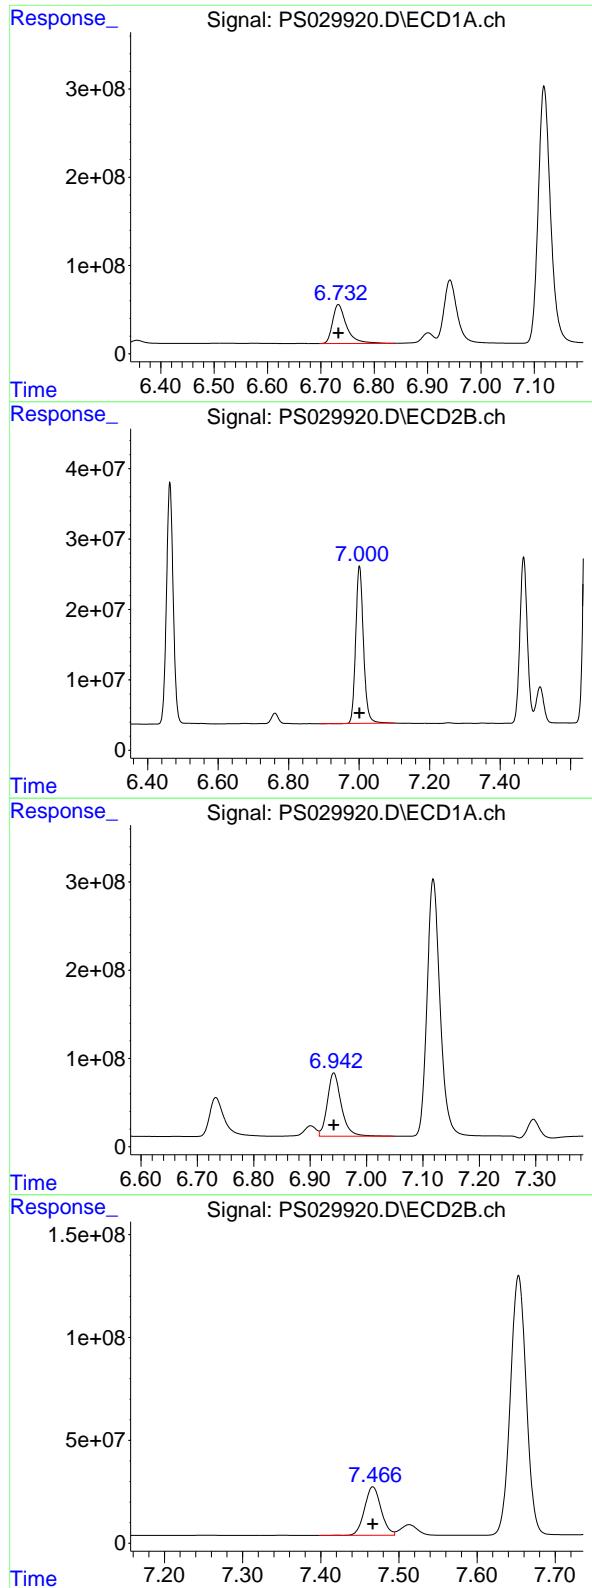

#3 4-Nitrophenol

R.T.: 6.733 min  
 Delta R.T.: 0.000 min  
 Response: 802328512  
 Conc: 462.20 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDICC500

#3 4-Nitrophenol


R.T.: 7.001 min  
 Delta R.T.: 0.000 min  
 Response: 342629938  
 Conc: 459.86 ng/ml

#4 2,4-DCAA

R.T.: 6.942 min  
 Delta R.T.: 0.000 min  
 Response: 1231780921  
 Conc: 512.53 ng/ml

#4 2,4-DCAA

R.T.: 7.467 min  
 Delta R.T.: 0.000 min  
 Response: 346180636  
 Conc: 503.46 ng/ml

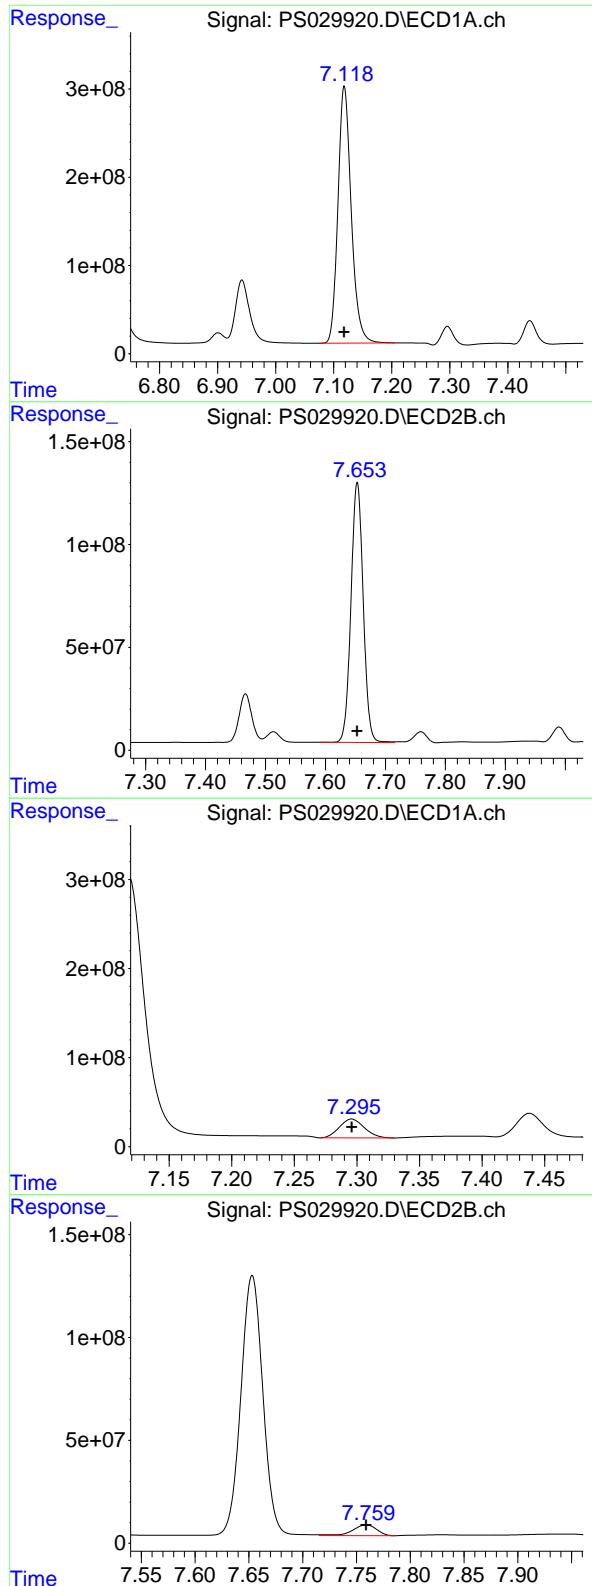

#5 DICAMBA

R.T.: 7.118 min  
 Delta R.T.: 0.000 min **Instrument:**  
 Response: 4642915948 ECD\_S  
 Conc: 476.25 ng/ml **ClientSampleId:**  
 HSTDICC500

#5 DICAMBA


R.T.: 7.653 min  
 Delta R.T.: 0.000 min  
 Response: 1792383950  
 Conc: 464.68 ng/ml

#6 MCPP

R.T.: 7.296 min  
 Delta R.T.: 0.000 min  
 Response: 290670931  
 Conc: 45.92 ug/ml

#6 MCPP

R.T.: 7.759 min  
 Delta R.T.: 0.000 min  
 Response: 82241844  
 Conc: 46.50 ug/ml

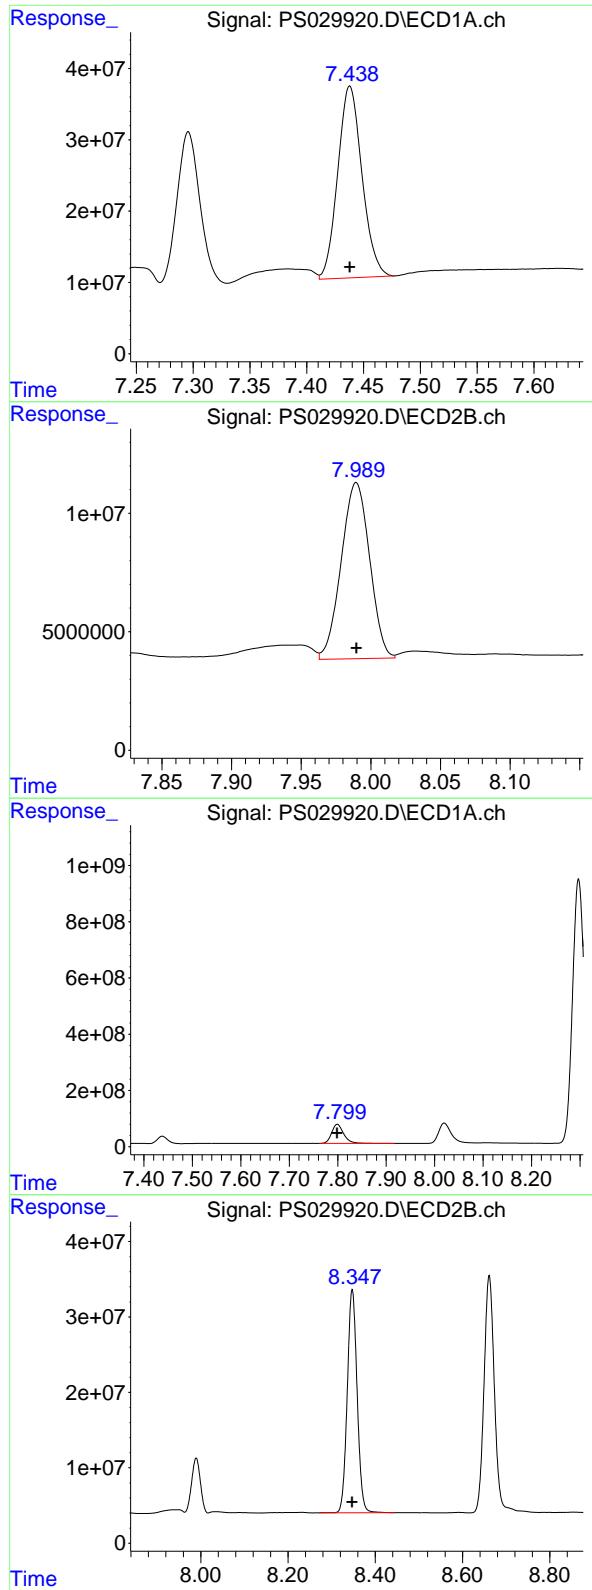

#7 MCPA

R.T.: 7.438 min  
Delta R.T.: 0.000 min  
Response: 399051123  
Conc: 46.19 ug/ml

Instrument: ECD\_S  
ClientSampleId: HSTDICC500

#7 MCPA


R.T.: 7.990 min  
Delta R.T.: 0.000 min  
Response: 105534297  
Conc: 46.16 ug/ml

#8 DICHLOPROP

R.T.: 7.799 min  
Delta R.T.: 0.000 min  
Response: 1186769618  
Conc: 480.56 ng/ml

#8 DICHLOPROP

R.T.: 8.347 min  
Delta R.T.: 0.000 min  
Response: 464258436  
Conc: 473.76 ng/ml

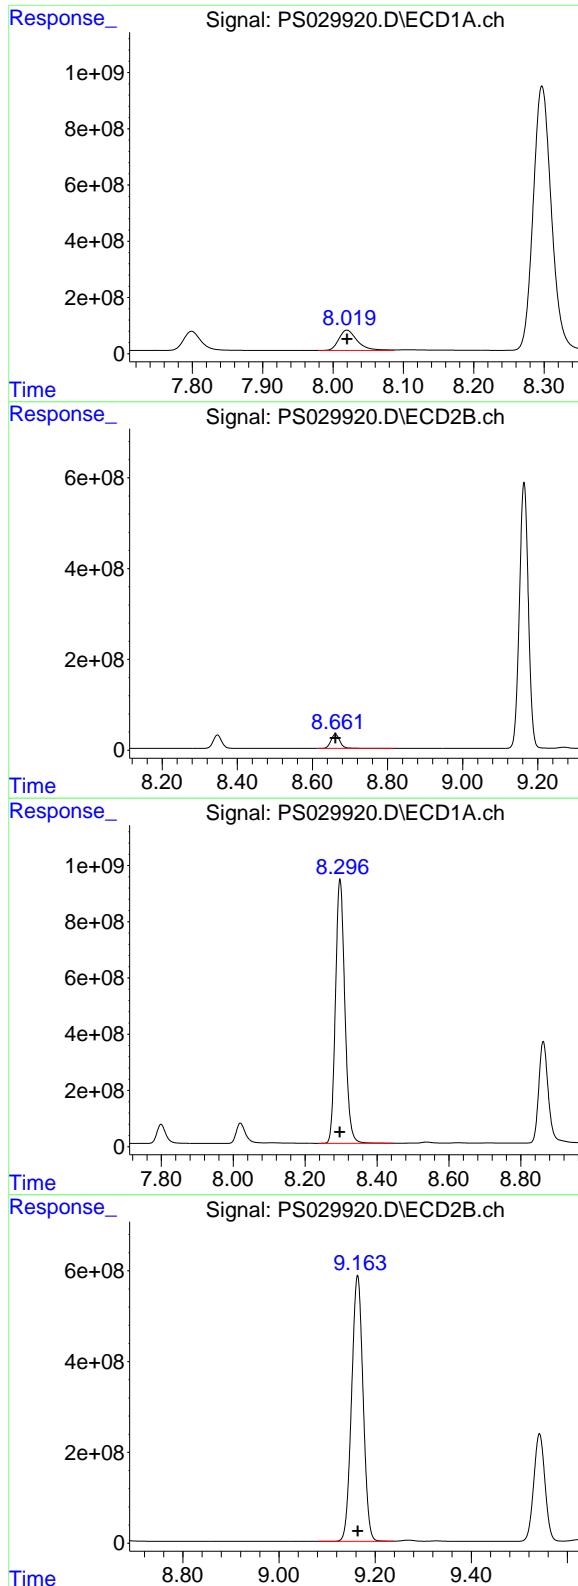

#9 2,4-D

R.T.: 8.020 min  
Delta R.T.: 0.000 min  
Response: 1315035111  
Conc: 478.74 ng/ml

Instrument: ECD\_S  
ClientSampleId: HSTDICC500

#9 2,4-D


R.T.: 8.661 min  
Delta R.T.: 0.000 min  
Response: 523223015  
Conc: 474.74 ng/ml

#10 Pentachlorophenol

R.T.: 8.297 min  
Delta R.T.: 0.000 min  
Response: 16887638820  
Conc: 483.73 ng/ml

#10 Pentachlorophenol

R.T.: 9.164 min  
Delta R.T.: 0.000 min  
Response: 9661508840  
Conc: 476.54 ng/ml

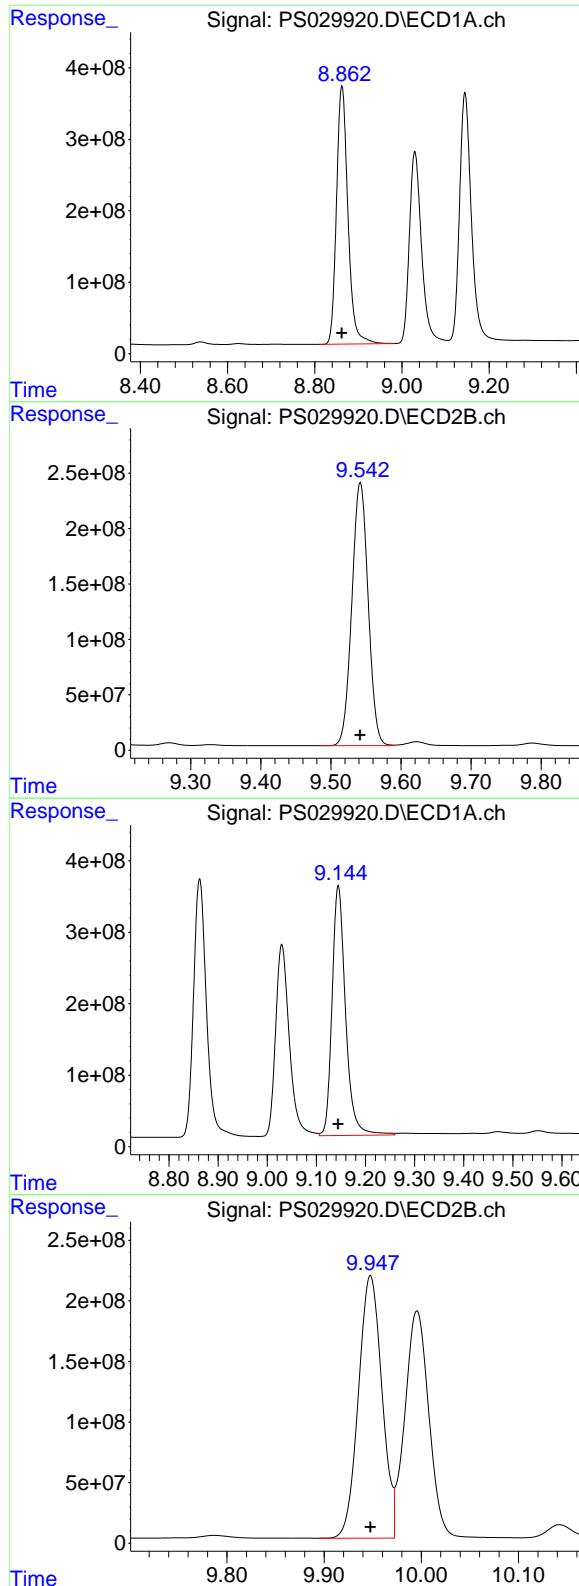

#11 2,4,5-TP (SILVEX)

R.T.: 8.862 min  
 Delta R.T.: 0.000 min  
 Response: 6584545232  
 Conc: 482.50 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDICC500

#11 2,4,5-TP (SILVEX)


R.T.: 9.542 min  
 Delta R.T.: 0.000 min  
 Response: 3838568800  
 Conc: 475.11 ng/ml

#12 2,4,5-T

R.T.: 9.145 min  
 Delta R.T.: 0.000 min  
 Response: 6674392581  
 Conc: 482.99 ng/ml

#12 2,4,5-T

R.T.: 9.948 min  
 Delta R.T.: 0.000 min  
 Response: 3641908671  
 Conc: 476.22 ng/ml

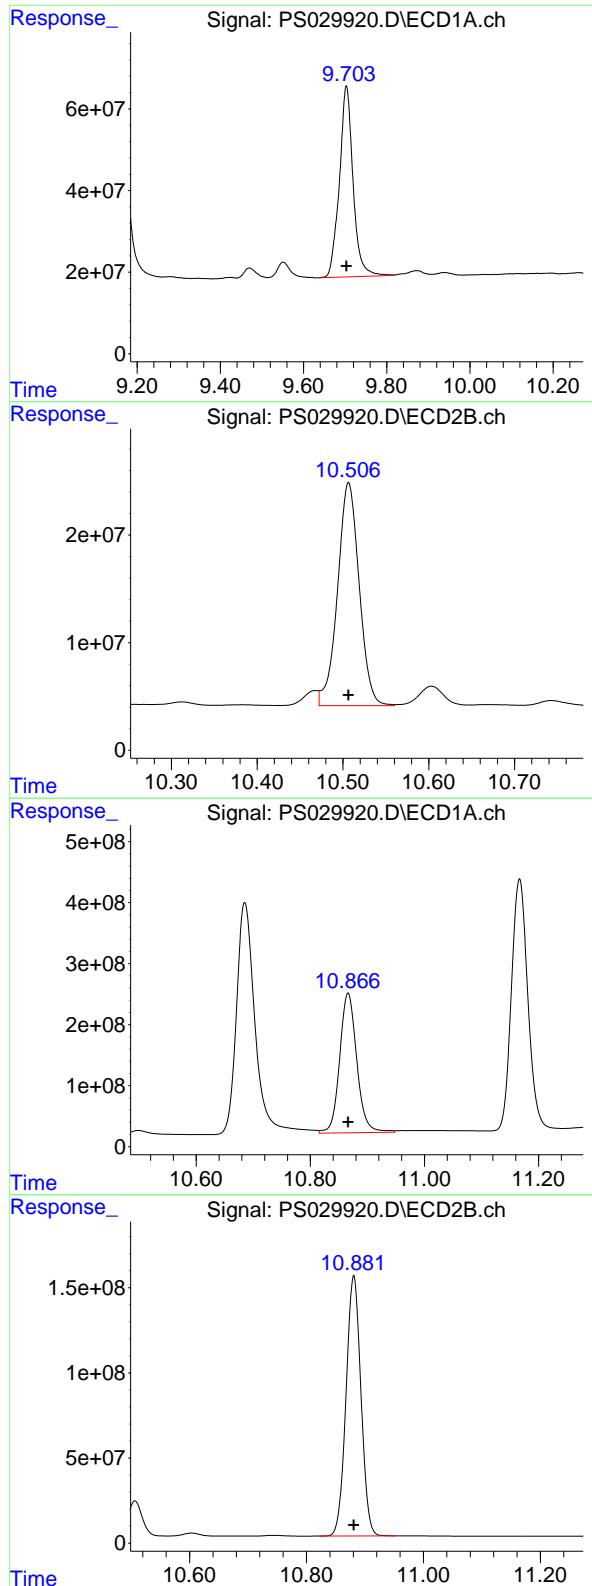

#13 2,4-DB

R.T.: 9.703 min  
 Delta R.T.: 0.000 min  
 Response: 1071085603  
 Conc: 478.62 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDICC500

#13 2,4-DB


R.T.: 10.507 min  
 Delta R.T.: 0.000 min  
 Response: 362659677  
 Conc: 465.16 ng/ml

#14 DINOSEB

R.T.: 10.866 min  
 Delta R.T.: 0.000 min  
 Response: 4764255395  
 Conc: 475.55 ng/ml

#14 DINOSEB

R.T.: 10.881 min  
 Delta R.T.: 0.000 min  
 Response: 2699322247  
 Conc: 471.42 ng/ml

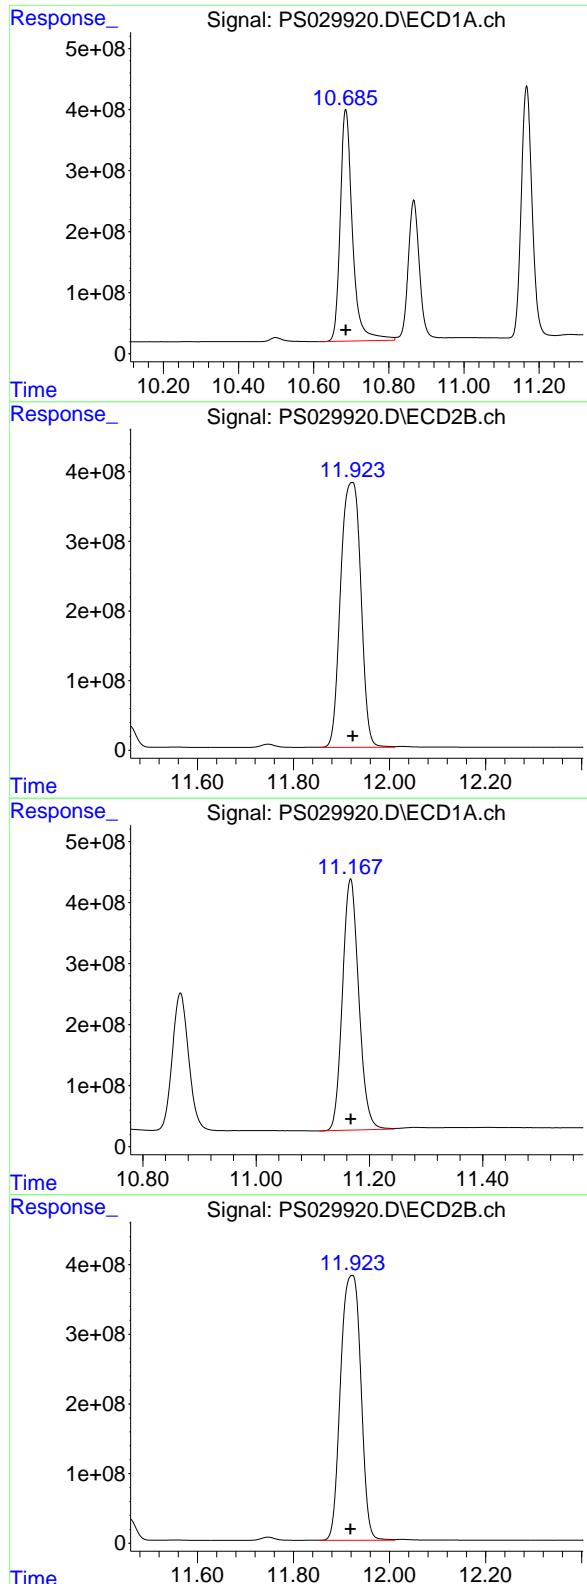

#15 Picloram

R.T.: 10.685 min  
 Delta R.T.: 0.000 min  
 Response: 8585191140  
 Conc: 477.89 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDICC500

#15 Picloram

R.T.: 11.922 min  
 Delta R.T.: -0.001 min  
 Response: 11084895769  
 Conc: 918.96 ng/ml

#16 DCPA

R.T.: 11.167 min  
 Delta R.T.: 0.000 min  
 Response: 8208335626  
 Conc: 488.03 ng/ml

#16 DCPA

R.T.: 11.922 min  
 Delta R.T.: 0.004 min  
 Response: 11084895769  
 Conc: 986.26 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029921.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 11:49  
 Operator : AR\AJ  
 Sample : HSTDICC750  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**HSTDICC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 12:13:23 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:13:04 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.942 7.467 1757.3E6 512.1E6 750.000 750.000

Target Compounds

1) T	Dalapon	2.449	2.525	2731.3E6	1134.3E6	682.500	682.500
2) T	3,5-DICHL...	6.146	6.463	2388.4E6	661.4E6	697.500	697.500
3) T	4-Nitroph...	6.732	7.001	1166.0E6	503.1E6	682.500	682.500
5) T	DICAMBA	7.118	7.653	6781.5E6	2750.1E6	705.000	705.000
6) T	MCPP	7.297	7.761	456.6E6	126.0E6	70.500	70.500
7) T	MCPA	7.440	7.991	606.7E6	160.7E6	69.750	69.750
8) T	DICHLORPROP	7.799	8.348	1701.9E6	685.3E6	705.000	705.000
9) T	2,4-D	8.019	8.661	1900.5E6	769.2E6	705.000	705.000
10) T	Pentachlo...	8.297	9.163	24416.7E6	14398.4E6	712.500	712.500
11) T	2,4,5-TP ...	8.862	9.542	9569.8E6	5755.2E6	712.500	712.500
12) T	2,4,5-T	9.144	9.947	9680.3E6	5434.8E6	712.500	712.500
13) T	2,4-DB	9.703	10.507	1582.3E6	567.0E6	712.500	712.500
14) T	DINOSEB	10.866	10.881	6979.6E6	4024.5E6	705.000	705.000
15) T	Picloram	10.685	11.921	12721.8E6	16794.7E6	712.500	1401.728 #
16) T	DCPA	11.166	11.921	11907.4E6	16794.7E6	720.000	1511.632 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029921.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 11:49  
 Operator : AR\AJ  
 Sample : HSTDICC750  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**HSTDICC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 12:13:23 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:13:04 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

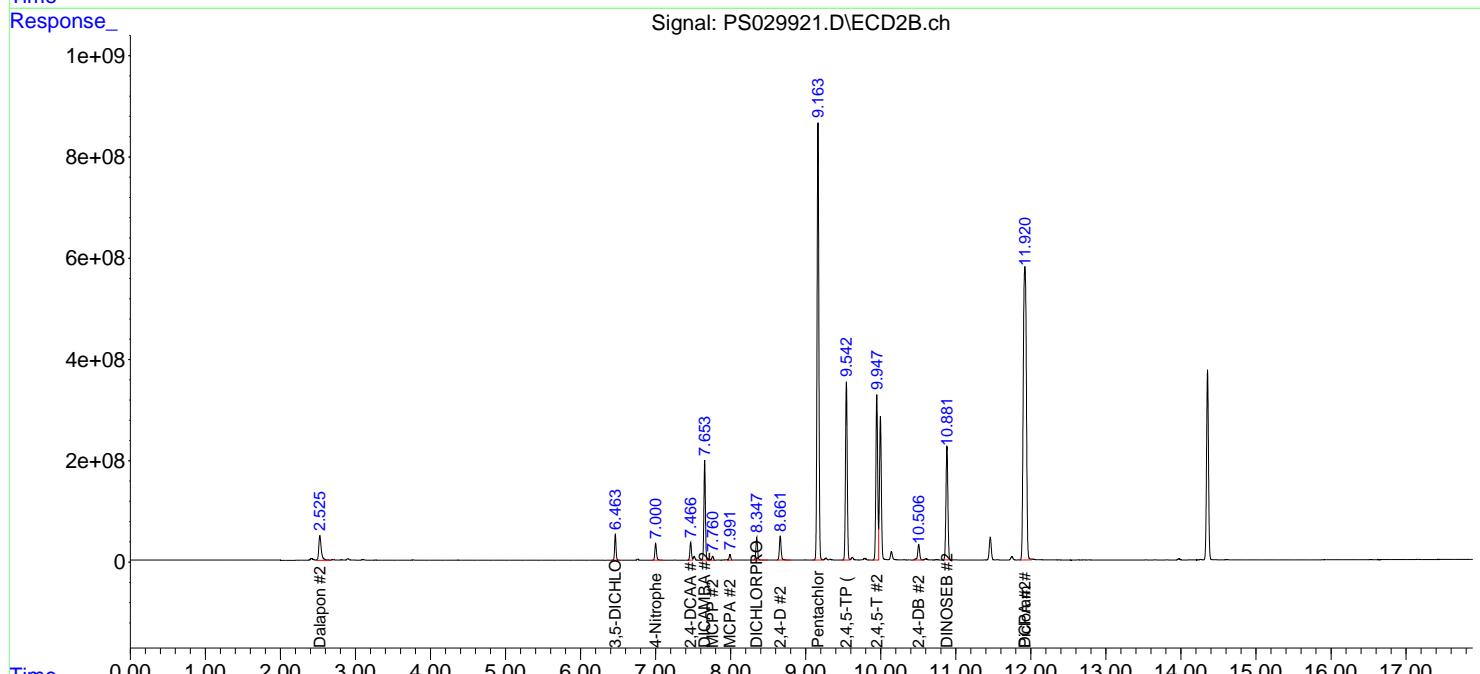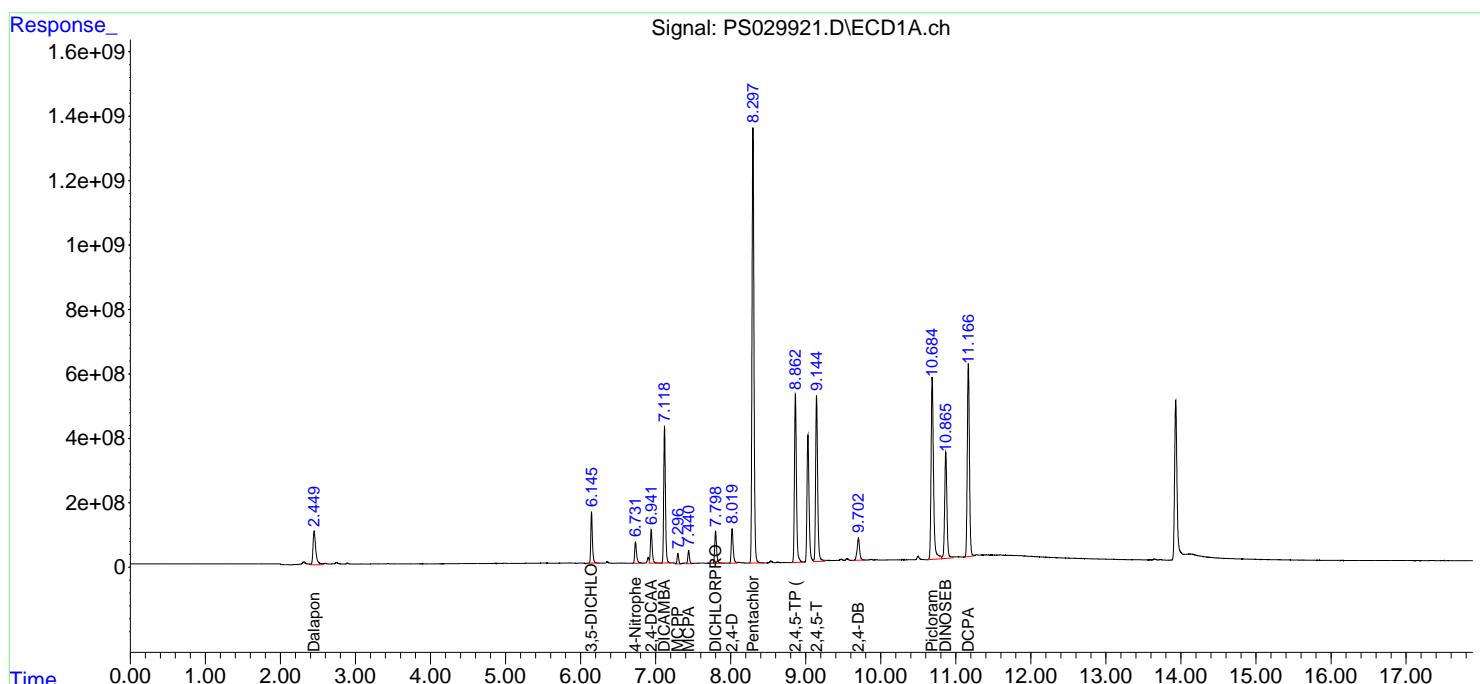

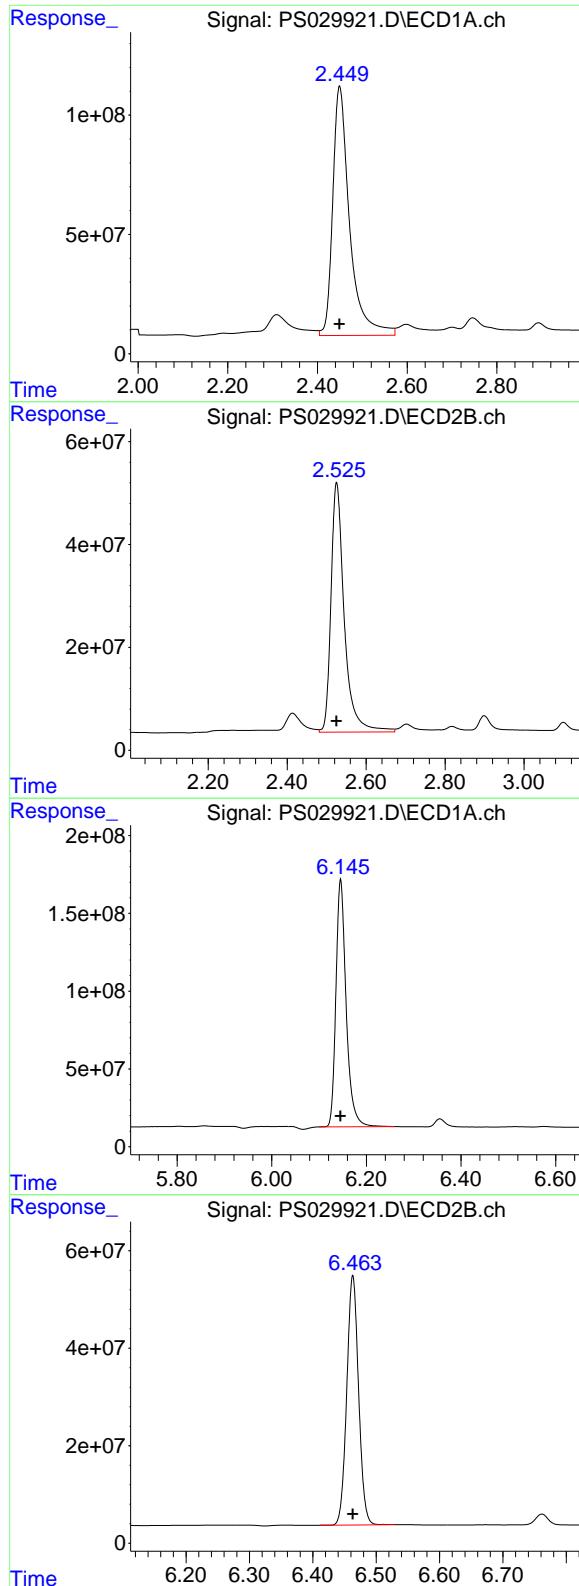

#1 Dalapon

R.T.: 2.449 min  
 Delta R.T.: 0.000 min  
 Response: 2731274284  
 Conc: 682.50 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDICC750

#1 Dalapon


R.T.: 2.525 min  
 Delta R.T.: 0.000 min  
 Response: 1134264471  
 Conc: 682.50 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.146 min  
 Delta R.T.: 0.000 min  
 Response: 2388375809  
 Conc: 697.50 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.463 min  
 Delta R.T.: 0.000 min  
 Response: 661411771  
 Conc: 697.50 ng/ml

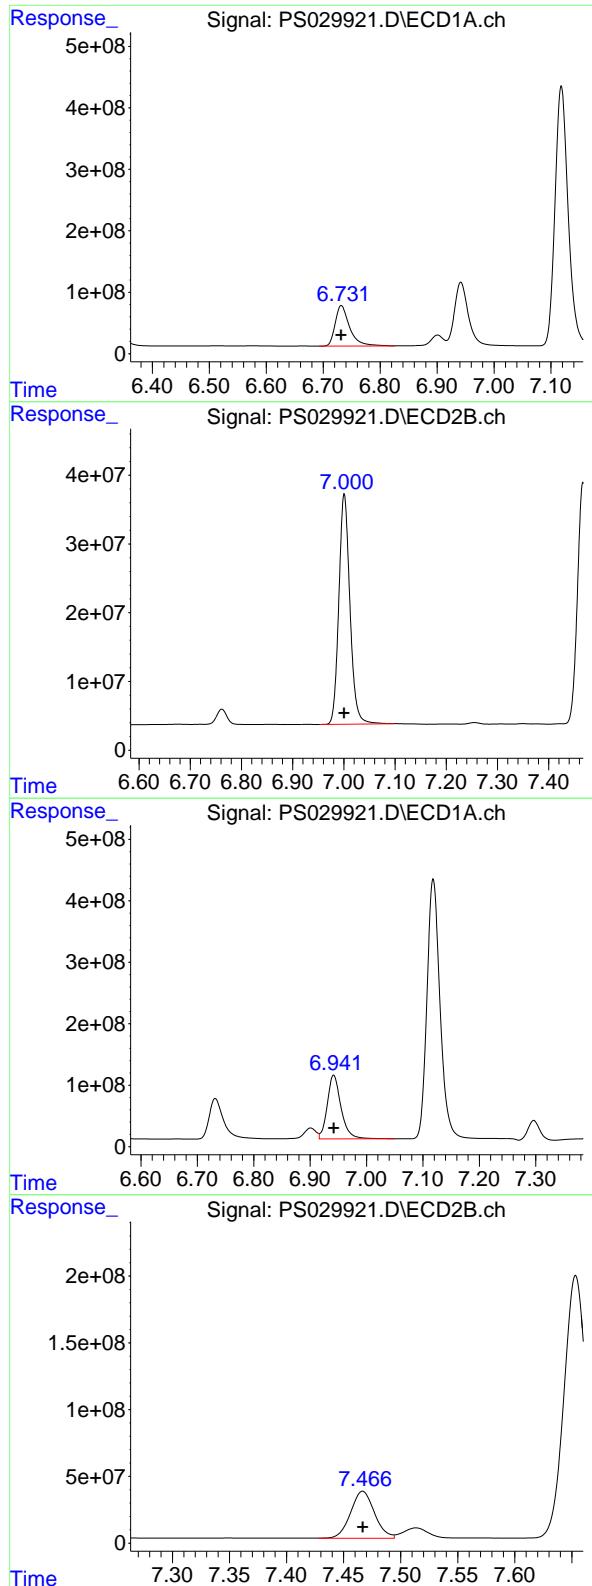

#3 4-Nitrophenol

R.T.: 6.732 min  
 Delta R.T.: 0.000 min  
 Response: 1165994997  
 Conc: 682.50 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** HSTDICC750

#3 4-Nitrophenol


R.T.: 7.001 min  
 Delta R.T.: 0.000 min  
 Response: 503078374  
 Conc: 682.50 ng/ml

#4 2,4-DCAA

R.T.: 6.942 min  
 Delta R.T.: 0.000 min  
 Response: 1757314349  
 Conc: 750.00 ng/ml

#4 2,4-DCAA

R.T.: 7.467 min  
 Delta R.T.: 0.000 min  
 Response: 512143835  
 Conc: 750.00 ng/ml

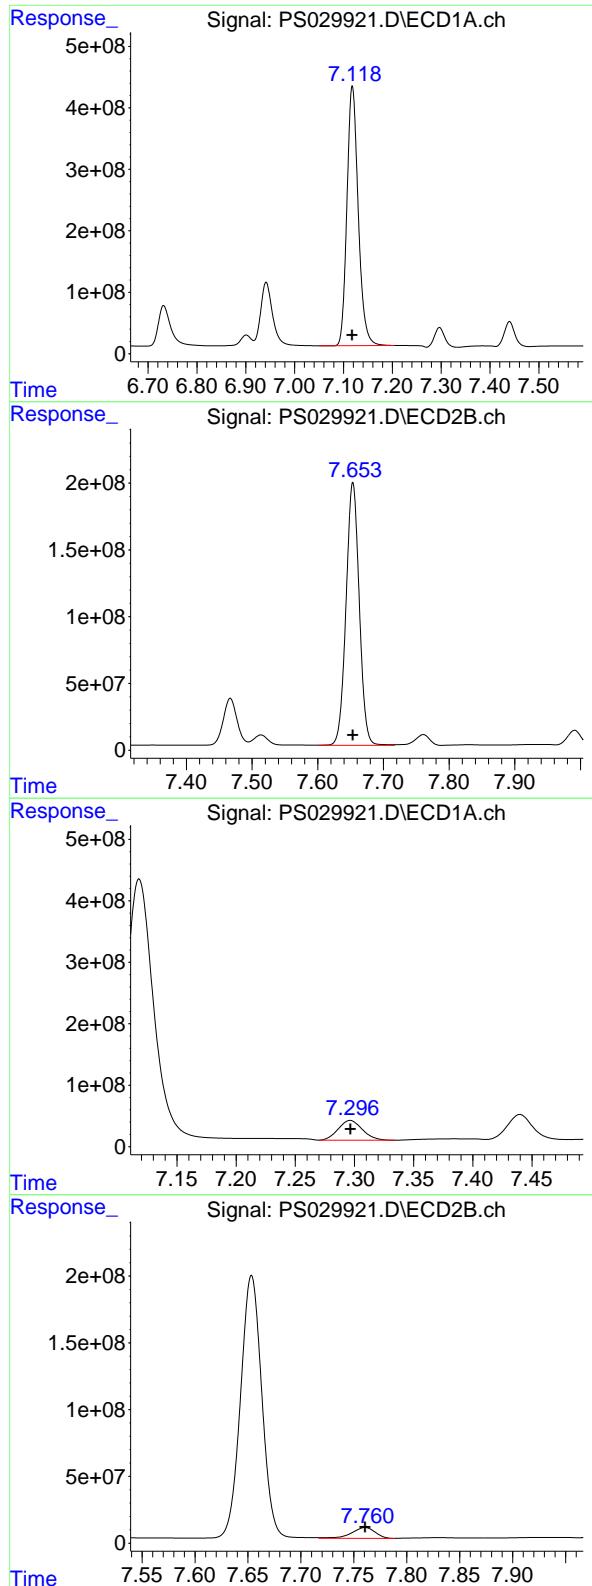

#5 DICAMBA

R.T.: 7.118 min  
Delta R.T.: 0.000 min **Instrument:**  
Response: 6781538346 ECD\_S  
Conc: 705.00 ng/ml **ClientSampleId:**  
HSTDICC750

#5 DICAMBA


R.T.: 7.653 min  
Delta R.T.: 0.000 min  
Response: 2750105949  
Conc: 705.00 ng/ml

#6 MCPP

R.T.: 7.297 min  
Delta R.T.: 0.000 min  
Response: 456554341  
Conc: 70.50 ug/ml

#6 MCPP

R.T.: 7.761 min  
Delta R.T.: 0.000 min  
Response: 126016285  
Conc: 70.50 ug/ml

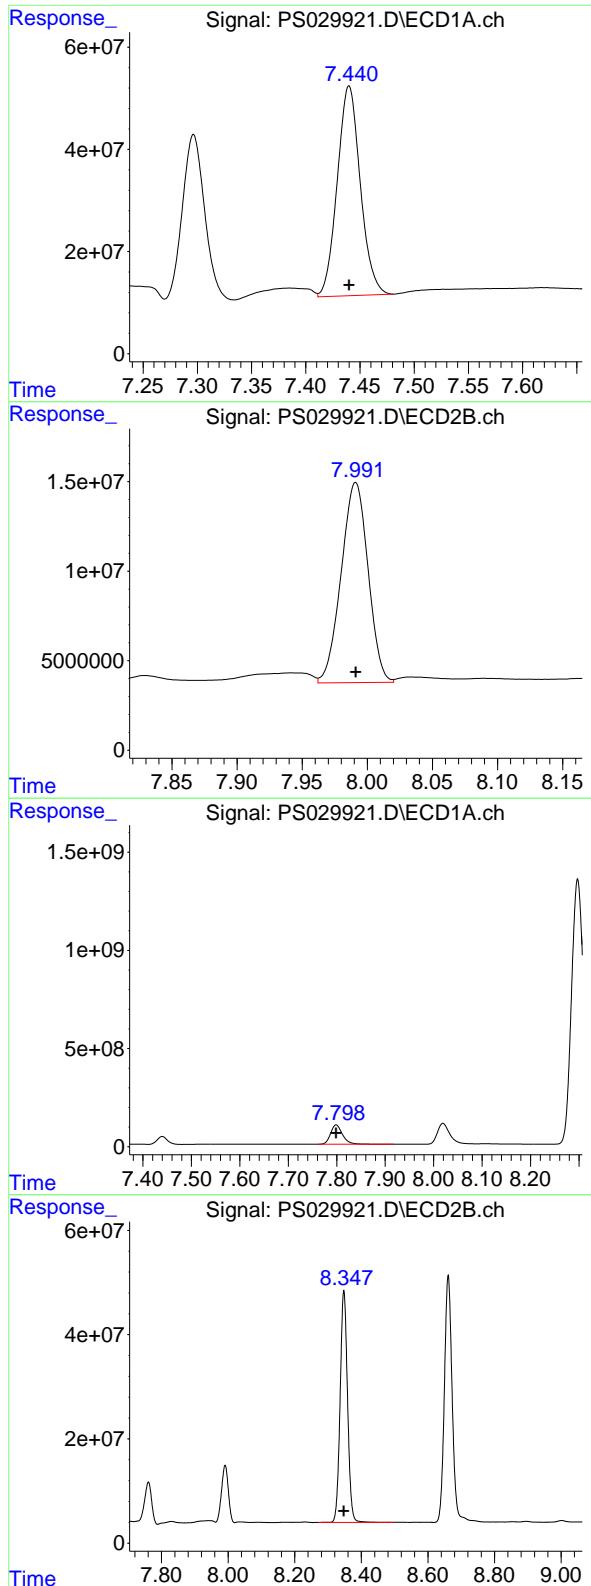

#7 MCPA

R.T.: 7.440 min  
Delta R.T.: 0.000 min  
Response: 606675377  
Conc: 69.75 ug/ml

Instrument: ECD\_S  
ClientSampleId: HSTDICC750

#7 MCPA


R.T.: 7.991 min  
Delta R.T.: 0.000 min  
Response: 160659432  
Conc: 69.75 ug/ml

#8 DICHLORPROP

R.T.: 7.799 min  
Delta R.T.: 0.000 min  
Response: 1701892611  
Conc: 705.00 ng/ml

#8 DICHLORPROP

R.T.: 8.348 min  
Delta R.T.: 0.000 min  
Response: 685337493  
Conc: 705.00 ng/ml

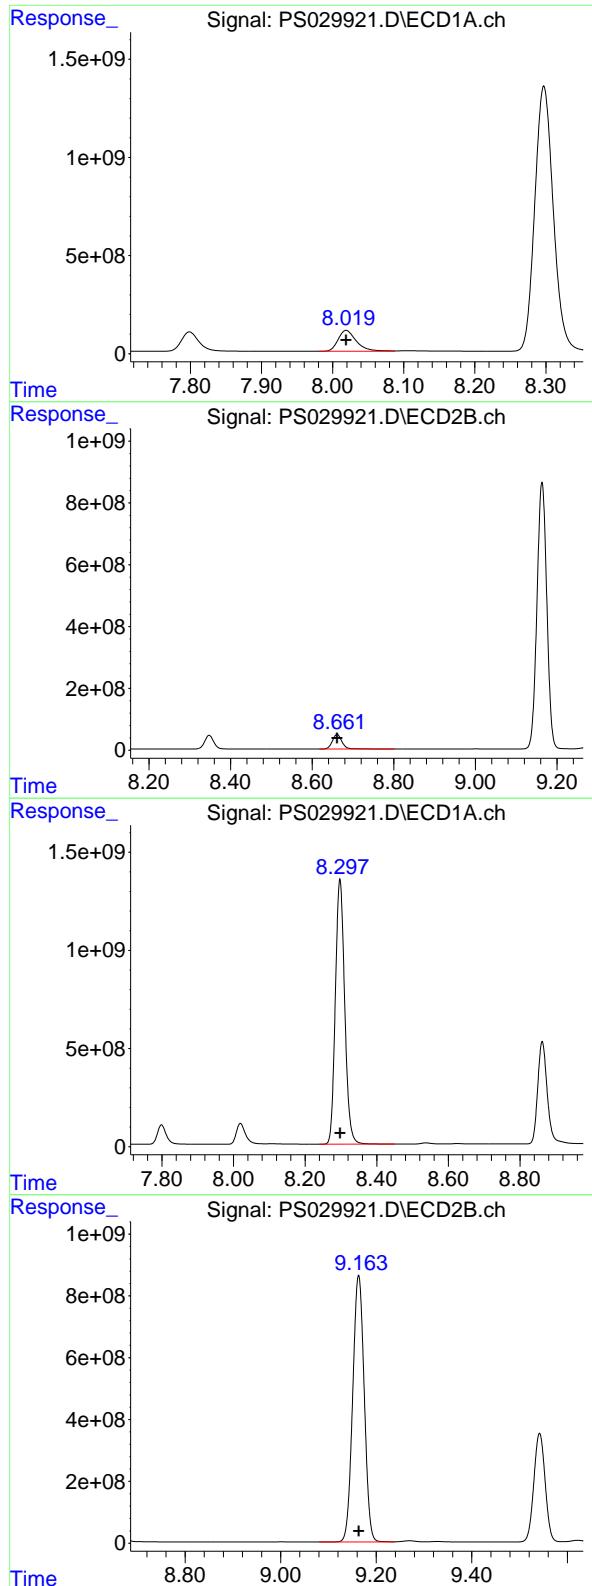

#9 2,4-D

R.T.: 8.019 min  
 Delta R.T.: 0.000 min  
 Response: 1900496204  
 Conc: 705.00 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDICC750

#9 2,4-D


R.T.: 8.661 min  
 Delta R.T.: 0.000 min  
 Response: 769155125  
 Conc: 705.00 ng/ml

#10 Pentachlorophenol

R.T.: 8.297 min  
 Delta R.T.: 0.000 min  
 Response: 24416691751  
 Conc: 712.50 ng/ml

#10 Pentachlorophenol

R.T.: 9.163 min  
 Delta R.T.: 0.000 min  
 Response: 14398444463  
 Conc: 712.50 ng/ml

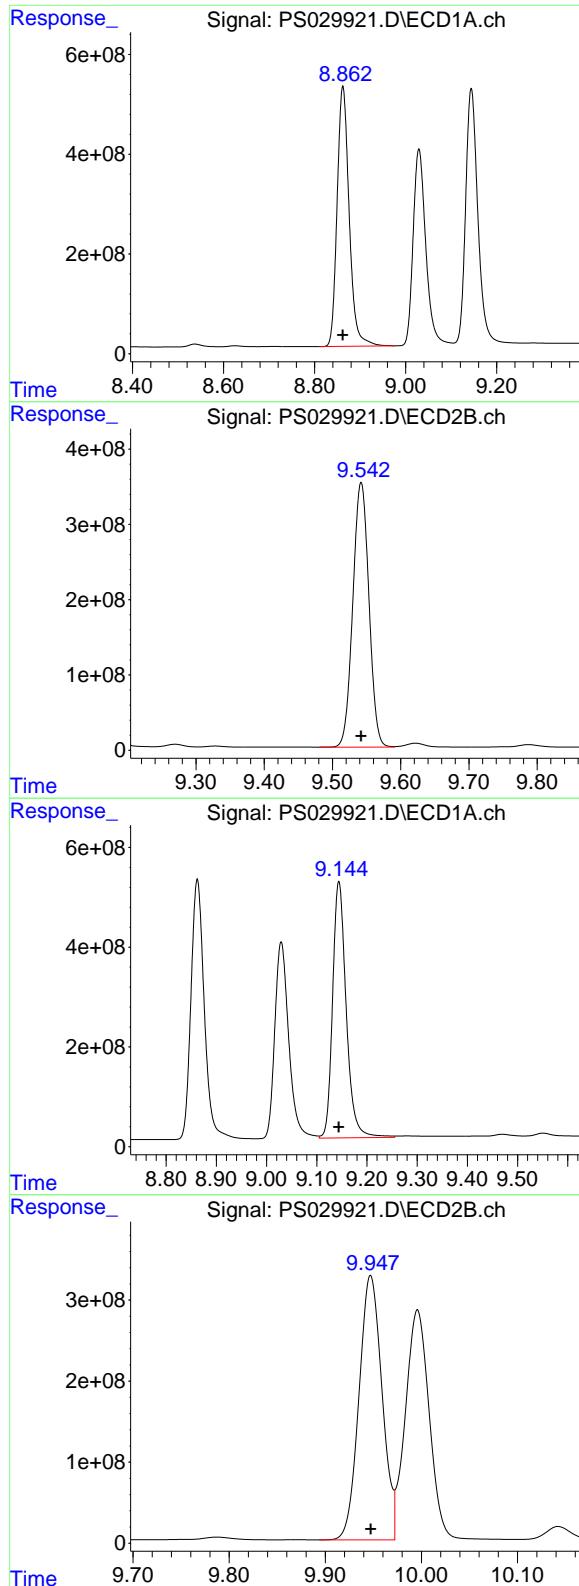

#11 2,4,5-TP (SILVEX)

R.T.: 8.862 min  
 Delta R.T.: 0.000 min  
 Response: 9569830576  
 Conc: 712.50 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDICC750

#11 2,4,5-TP (SILVEX)


R.T.: 9.542 min  
 Delta R.T.: 0.000 min  
 Response: 5755245929  
 Conc: 712.50 ng/ml

#12 2,4,5-T

R.T.: 9.144 min  
 Delta R.T.: 0.000 min  
 Response: 9680261593  
 Conc: 712.50 ng/ml

#12 2,4,5-T

R.T.: 9.947 min  
 Delta R.T.: 0.000 min  
 Response: 5434774786  
 Conc: 712.50 ng/ml

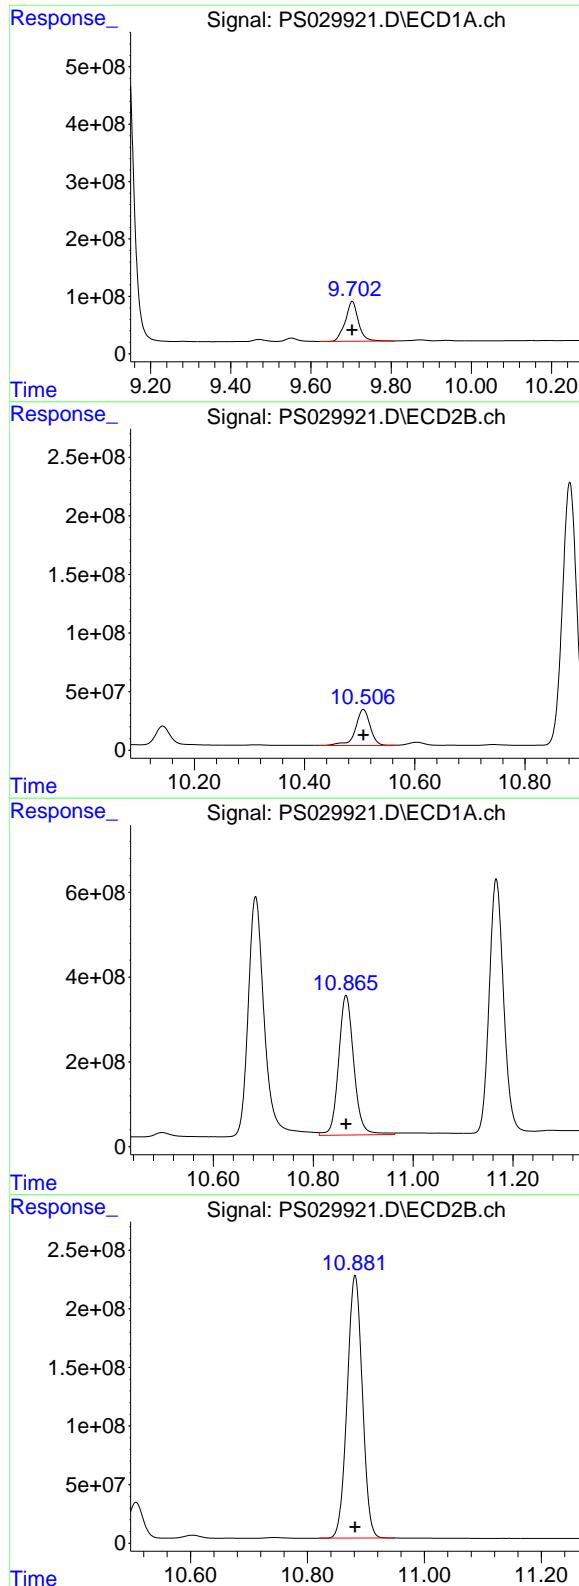

#13 2,4-DB

R.T.: 9.703 min  
 Delta R.T.: 0.000 min  
 Response: 1582337187  
 Conc: 712.50 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDICC750

#13 2,4-DB


R.T.: 10.507 min  
 Delta R.T.: 0.000 min  
 Response: 567000464  
 Conc: 712.50 ng/ml

#14 DINOSEB

R.T.: 10.866 min  
 Delta R.T.: 0.000 min  
 Response: 6979616298  
 Conc: 705.00 ng/ml

#14 DINOSEB

R.T.: 10.881 min  
 Delta R.T.: 0.000 min  
 Response: 4024544896  
 Conc: 705.00 ng/ml

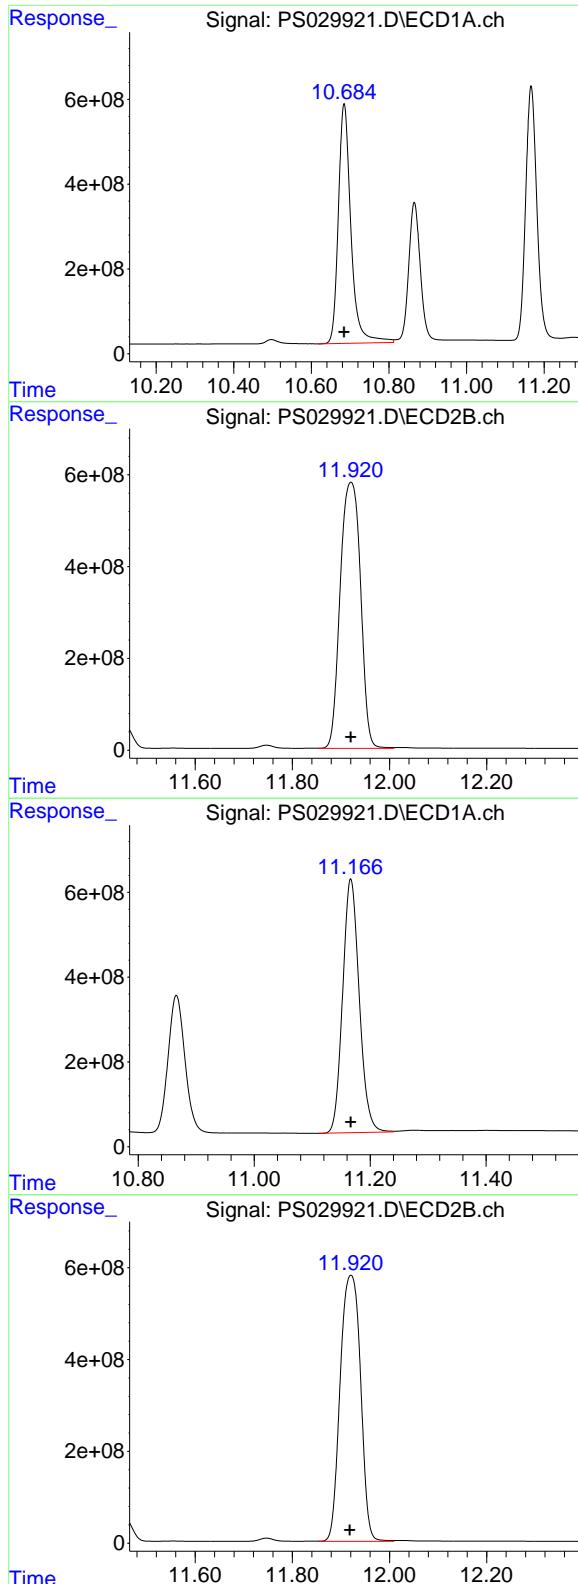

#15 Picloram

R.T.: 10.685 min  
 Delta R.T.: 0.000 min  
 Response: 12721770760 ECD\_S  
 Conc: 712.50 ng/ml ClientSampleId : HSTDICC750

#15 Picloram

R.T.: 11.921 min  
 Delta R.T.: 0.000 min  
 Response: 16794663994  
 Conc: 1401.73 ng/ml

#16 DCPA

R.T.: 11.166 min  
 Delta R.T.: 0.000 min  
 Response: 11907371025  
 Conc: 720.00 ng/ml

#16 DCPA

R.T.: 11.921 min  
 Delta R.T.: 0.002 min  
 Response: 16794663994  
 Conc: 1511.63 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029922.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 12:13  
 Operator : AR\AJ  
 Sample : HSTDICC1000  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**HSTDICC1000**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 12:41:26 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:41:18 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.941 7.466 2233.7E6 662.0E6 886.503 930.792

Target Compounds

1) T	Dalapon	2.448	2.524	3459.2E6	1450.3E6	829.350	821.672
2) T	3,5-DICHL...	6.145	6.463	3047.9E6	855.5E6	835.452	867.026
3) T	4-Nitroph...	6.731	7.000	1500.3E6	650.1E6	830.199	840.006
5) T	DICAMBA	7.118	7.652	8709.4E6	3622.0E6	866.580	923.531
6) T	MCPP	7.297	7.761	613.1E6	163.4E6	97.394	94.159
7) T	MCPA	7.440	7.992	802.4E6	212.9E6	91.664	89.703
8) T	DICHLORPROP	7.798	8.347	2167.0E6	881.3E6	837.398	868.054
9) T	2,4-D	8.018	8.661	2435.4E6	991.5E6	849.738	870.102
10) T	Pentachlo...	8.297	9.163	31038.8E6	18517.9E6	864.019	901.215
11) T	2,4,5-TP ...	8.862	9.542	12264.9E6	7478.1E6	869.588	909.959
12) T	2,4,5-T	9.144	9.947	12428.5E6	7054.1E6	868.738	903.059
13) T	2,4-DB	9.702	10.506	2059.3E6	737.5E6	896.524	916.649
14) T	DINOSEB	10.866	10.881	8807.7E6	5194.8E6	849.671	883.604
15) T	Picloram	10.685	11.921	16510.1E6	21923.5E6	892.660	1757.231 #
16) T	DCPA	11.166	11.921	15201.9E6	21923.5E6	876.317	1927.353 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029922.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 12:13  
 Operator : AR\AJ  
 Sample : HSTDICC1000  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**HSTDICC1000**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 12:41:26 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:41:18 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

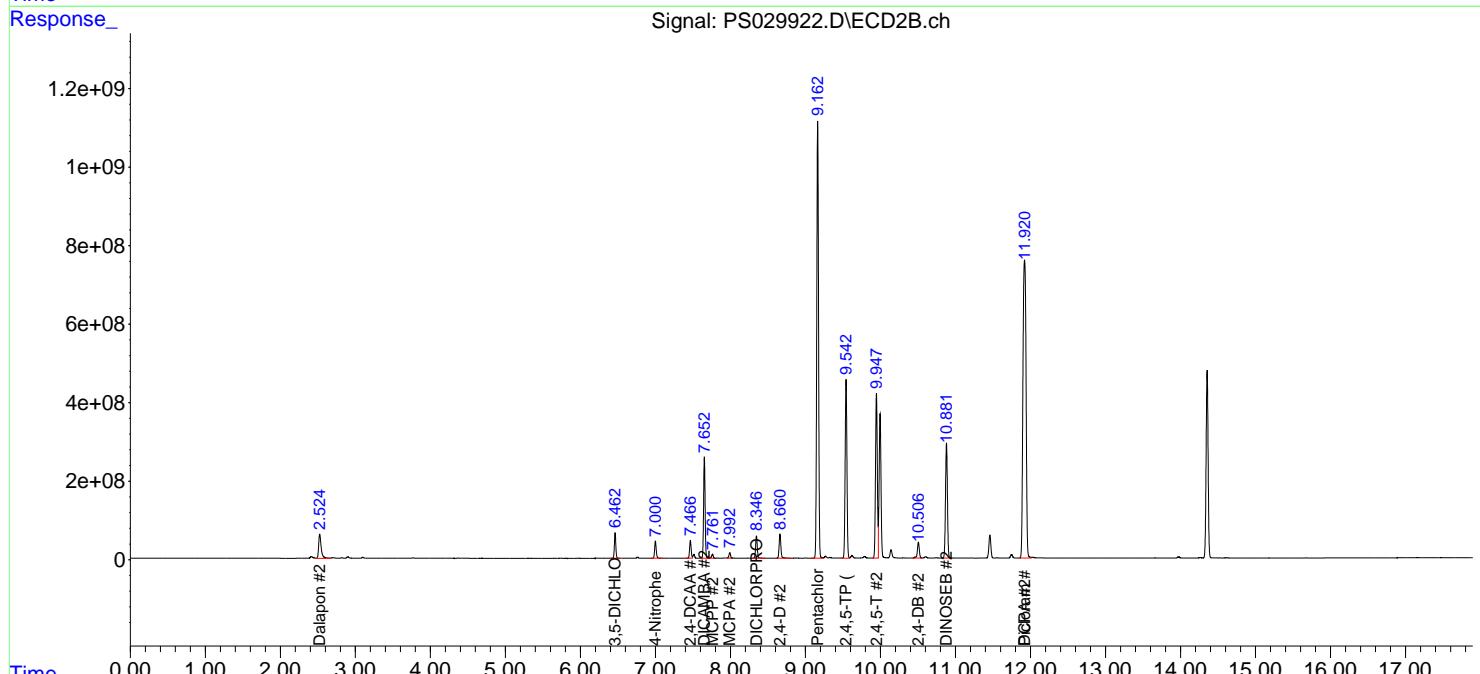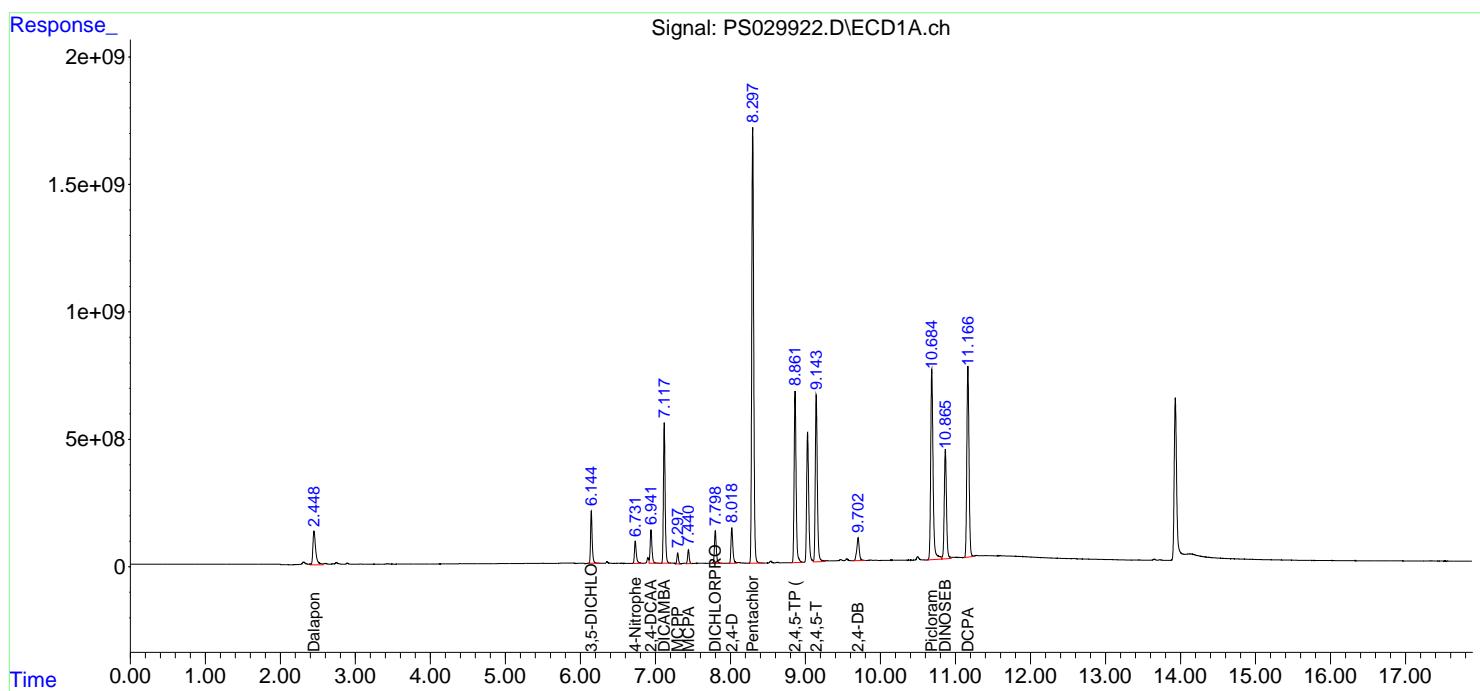

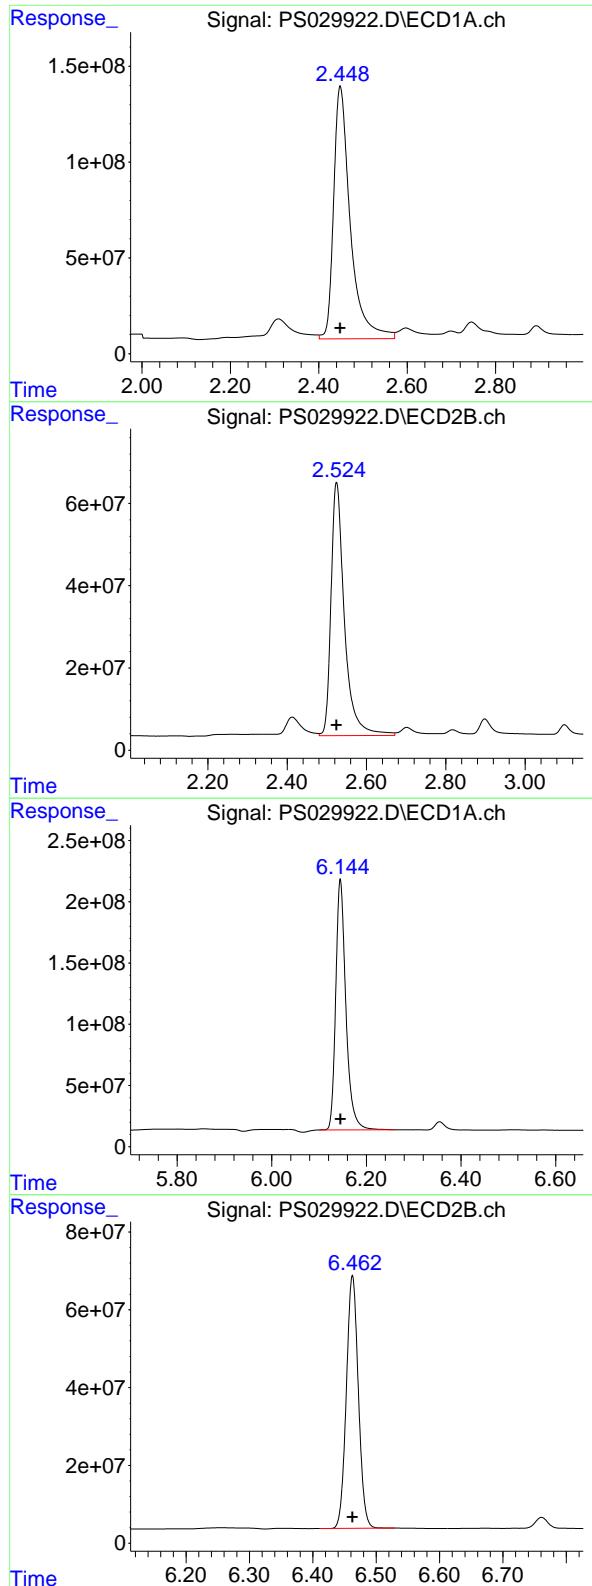

#1 Dalapon

R.T.: 2.448 min  
 Delta R.T.: 0.000 min  
 Response: 3459192542  
 Conc: 829.35 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDICC1000

#1 Dalapon


R.T.: 2.524 min  
 Delta R.T.: 0.000 min  
 Response: 1450275646  
 Conc: 821.67 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.145 min  
 Delta R.T.: 0.000 min  
 Response: 3047853600  
 Conc: 835.45 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.463 min  
 Delta R.T.: 0.000 min  
 Response: 855462143  
 Conc: 867.03 ng/ml

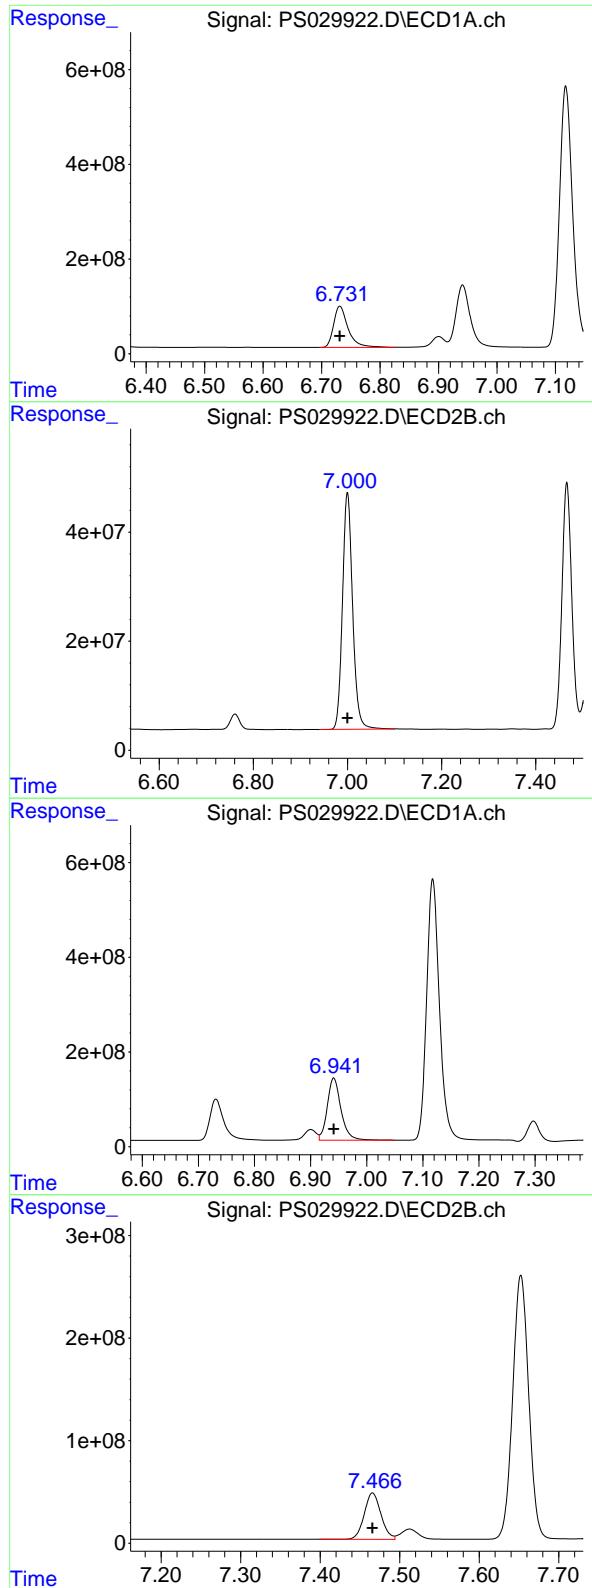

#3 4-Nitrophenol

R.T.: 6.731 min  
 Delta R.T.: 0.000 min  
 Response: 1500313179  
 Conc: 830.20 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** HSTDICC1000

#3 4-Nitrophenol


R.T.: 7.000 min  
 Delta R.T.: 0.000 min  
 Response: 650145921  
 Conc: 840.01 ng/ml

#4 2,4-DCAA

R.T.: 6.941 min  
 Delta R.T.: 0.000 min  
 Response: 2233667943  
 Conc: 886.50 ng/ml

#4 2,4-DCAA

R.T.: 7.466 min  
 Delta R.T.: 0.000 min  
 Response: 661990920  
 Conc: 930.79 ng/ml

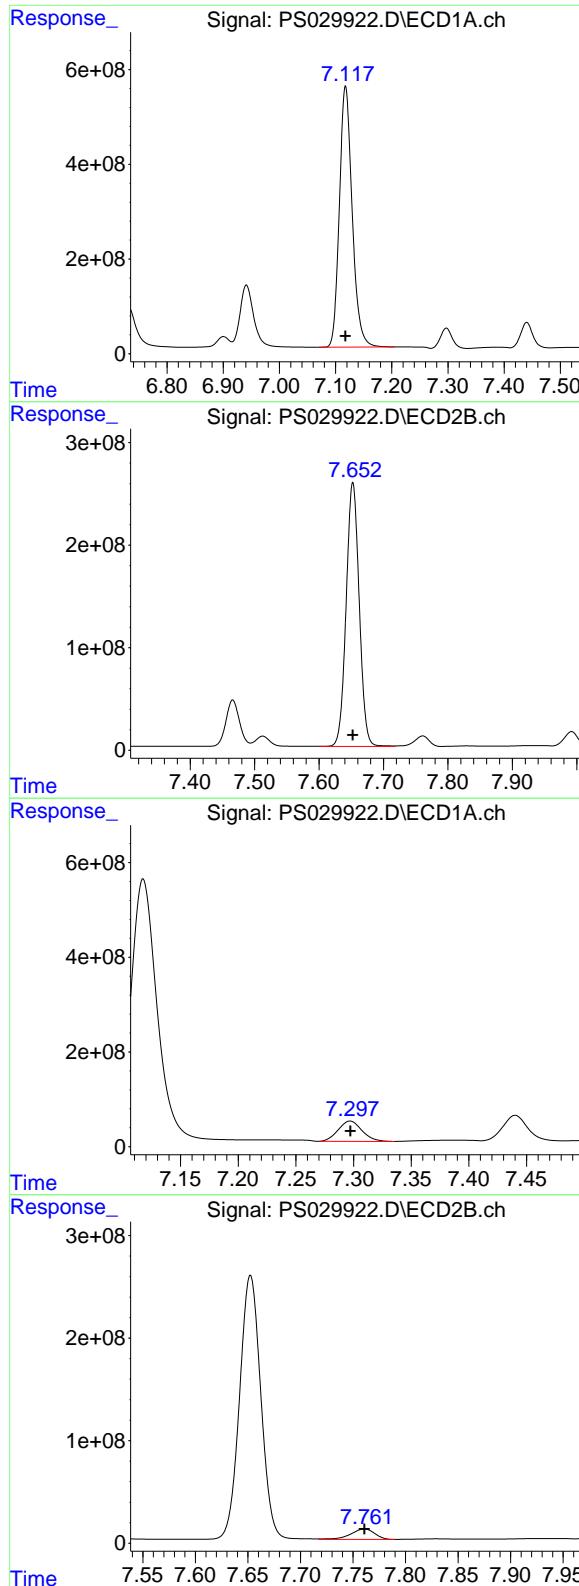

#5 DICAMBA

R.T.: 7.118 min  
Delta R.T.: 0.000 min **Instrument:**  
Response: 8709449271 ECD\_S  
Conc: 866.58 ng/ml **ClientSampleId:**  
HSTDICC1000

#5 DICAMBA


R.T.: 7.652 min  
Delta R.T.: 0.000 min  
Response: 3622048735  
Conc: 923.53 ng/ml

#6 MCPP

R.T.: 7.297 min  
Delta R.T.: 0.000 min  
Response: 613146849  
Conc: 97.39 ug/ml

#6 MCPP


R.T.: 7.761 min  
Delta R.T.: 0.000 min  
Response: 163368164  
Conc: 94.16 ug/ml

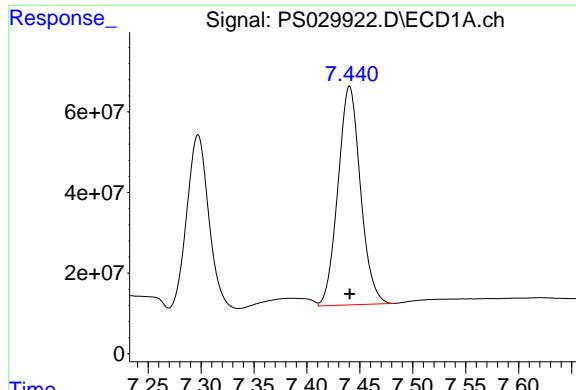

#7 MCPA


R.T.: 7.440 min  
 Delta R.T.: 0.000 min  
 Response: 802417459  
 Conc: 91.66 ug/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDICC1000

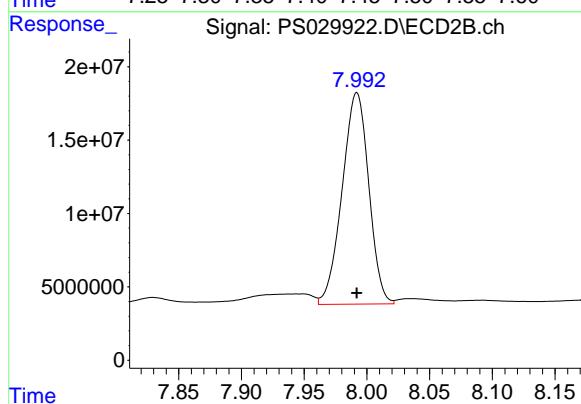


#7 MCPA

R.T.: 7.992 min  
 Delta R.T.: 0.000 min  
 Response: 212857828  
 Conc: 89.70 ug/ml

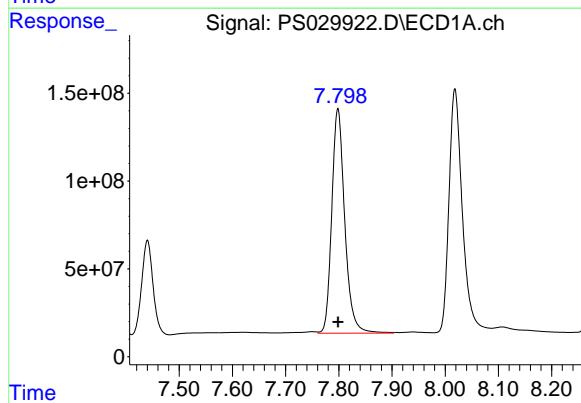


#8 DICHLORPROP

R.T.: 7.798 min  
 Delta R.T.: 0.000 min  
 Response: 2167004704  
 Conc: 837.40 ng/ml

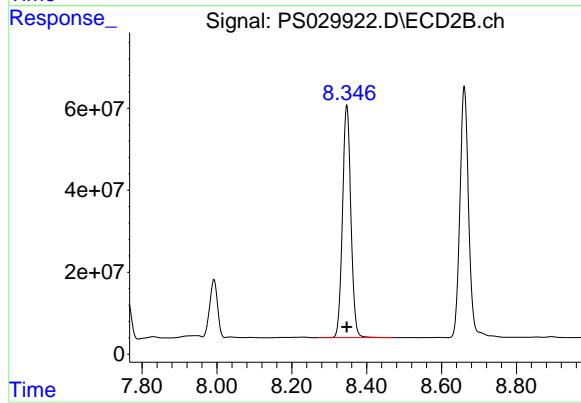

#8 DICHLORPROP

R.T.: 8.347 min  
 Delta R.T.: 0.000 min  
 Response: 881253779  
 Conc: 868.05 ng/ml

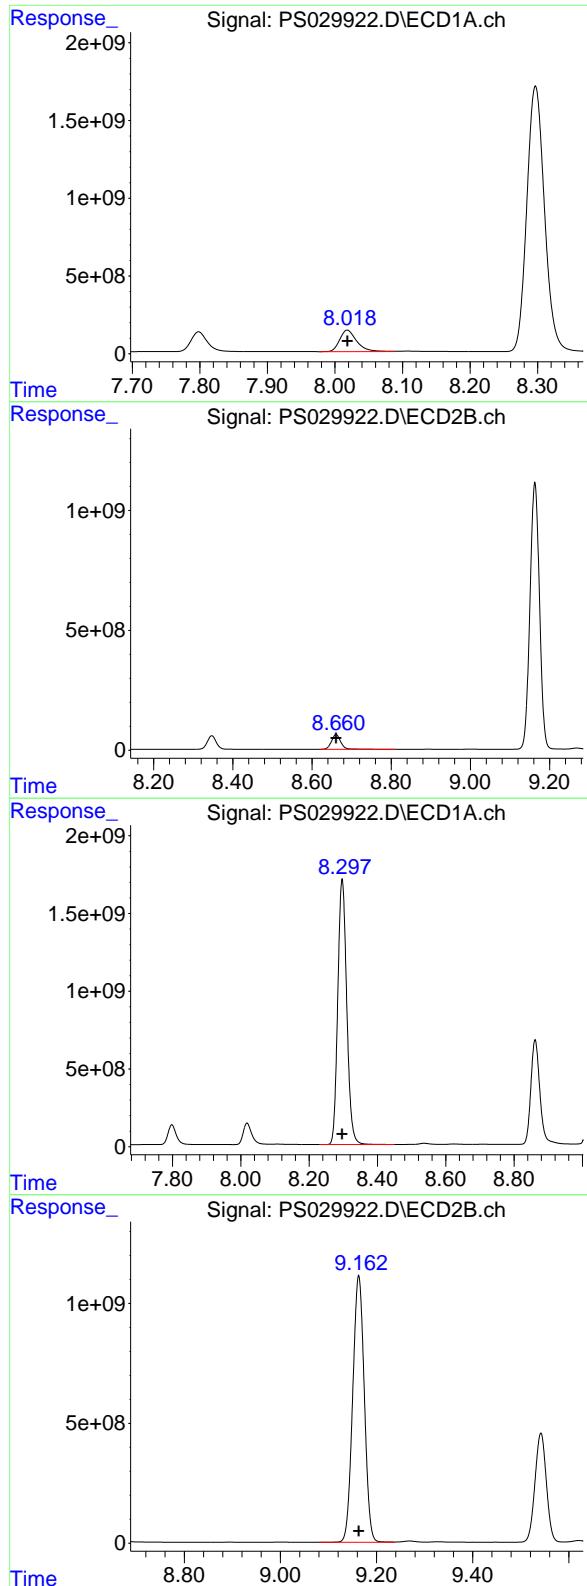

#9 2,4-D

R.T.: 8.018 min  
Delta R.T.: 0.000 min  
Response: 2435353652  
Conc: 849.74 ng/ml

Instrument: ECD\_S  
ClientSampleId: HSTDICC1000

#9 2,4-D


R.T.: 8.661 min  
Delta R.T.: 0.000 min  
Response: 991509756  
Conc: 870.10 ng/ml

#10 Pentachlorophenol

R.T.: 8.297 min  
Delta R.T.: 0.000 min  
Response: 31038781576  
Conc: 864.02 ng/ml

#10 Pentachlorophenol

R.T.: 9.163 min  
Delta R.T.: 0.000 min  
Response: 18517872387  
Conc: 901.22 ng/ml

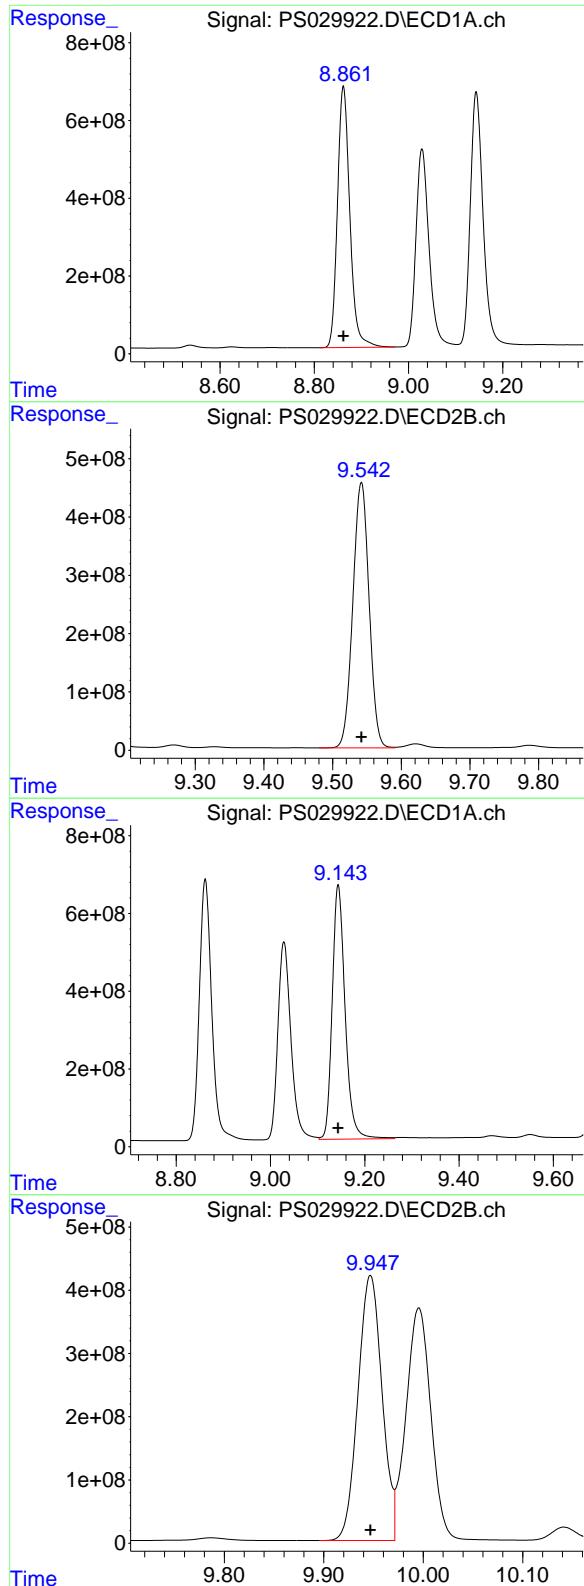

#11 2,4,5-TP (SILVEX)

R.T.: 8.862 min  
 Delta R.T.: 0.000 min  
 Response: 12264939701  
 Conc: 869.59 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDICC1000

#11 2,4,5-TP (SILVEX)


R.T.: 9.542 min  
 Delta R.T.: 0.000 min  
 Response: 7478086402  
 Conc: 909.96 ng/ml

#12 2,4,5-T

R.T.: 9.144 min  
 Delta R.T.: 0.000 min  
 Response: 12428516949  
 Conc: 868.74 ng/ml

#12 2,4,5-T

R.T.: 9.947 min  
 Delta R.T.: 0.000 min  
 Response: 7054117355  
 Conc: 903.06 ng/ml

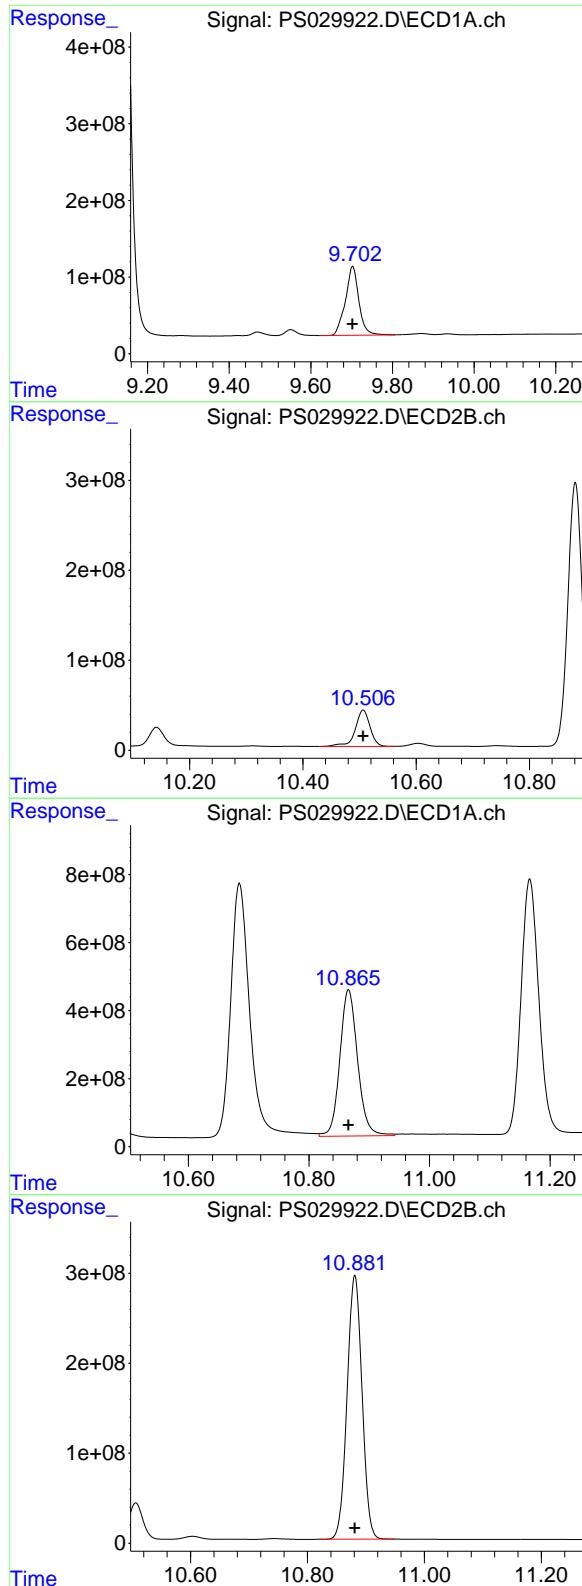

#13 2,4-DB

R.T.: 9.702 min  
 Delta R.T.: 0.000 min  
 Response: 2059257414  
 Conc: 896.52 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDICC1000

#13 2,4-DB


R.T.: 10.506 min  
 Delta R.T.: 0.000 min  
 Response: 737501651  
 Conc: 916.65 ng/ml

#14 DINOSEB

R.T.: 10.866 min  
 Delta R.T.: 0.000 min  
 Response: 8807749773  
 Conc: 849.67 ng/ml

#14 DINOSEB

R.T.: 10.881 min  
 Delta R.T.: 0.000 min  
 Response: 5194780641  
 Conc: 883.60 ng/ml

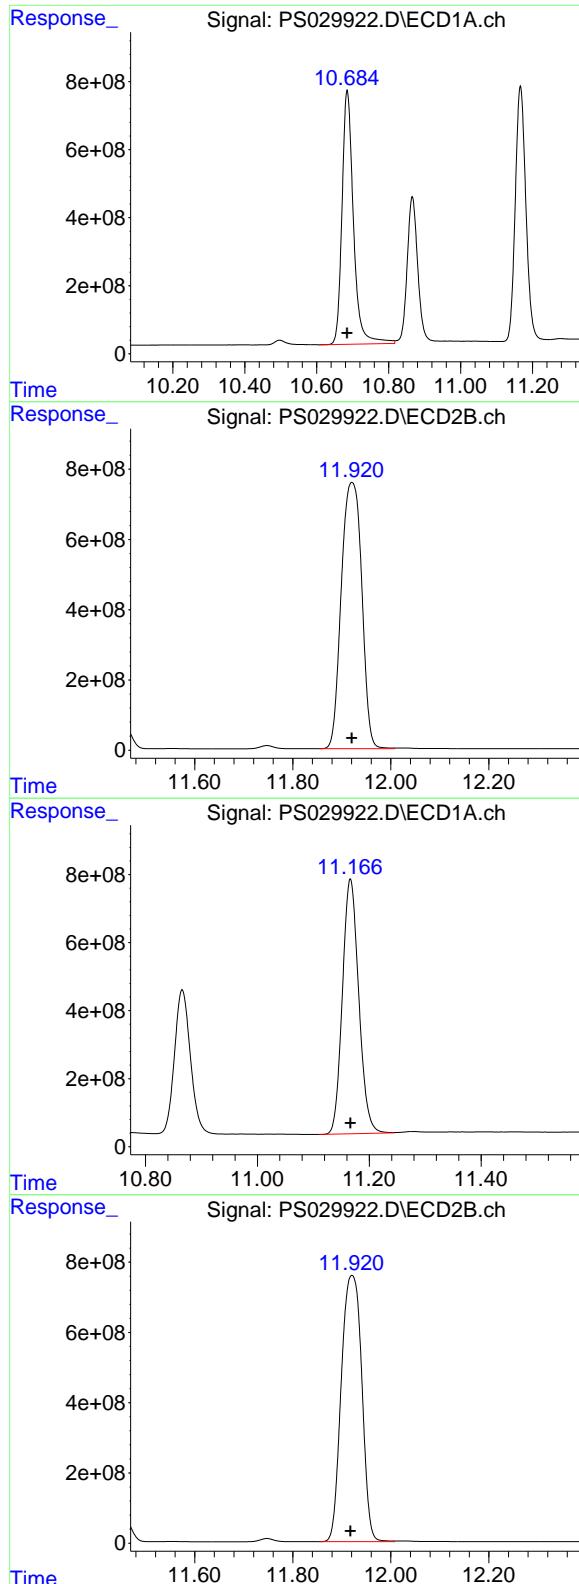

#15 Picloram

R.T.: 10.685 min  
 Delta R.T.: 0.000 min **Instrument:**  
 Response: 16510101945 ECD\_S  
 Conc: 892.66 ng/ml **ClientSampleId:**  
 HSTDICC1000

#15 Picloram

R.T.: 11.921 min  
 Delta R.T.: 0.000 min  
 Response: 21923468689  
 Conc: 1757.23 ng/ml

#16 DCPA

R.T.: 11.166 min  
 Delta R.T.: 0.000 min  
 Response: 15201932980  
 Conc: 876.32 ng/ml

#16 DCPA

R.T.: 11.921 min  
 Delta R.T.: 0.003 min  
 Response: 21923468689  
 Conc: 1927.35 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029923.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 12:37  
 Operator : AR\AJ  
 Sample : HSTDICC1500  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**HSTDICC1500**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 12:55:49 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:55:41 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.941 7.467 3340.2E6 1016.6E6 1357.229 1442.979

Target Compounds

1) T	Dalapon	2.448	2.524	5176.7E6	2212.1E6	1264.064	1274.156
2) T	3,5-DICHL...	6.145	6.463	4570.5E6	1313.0E6	1278.892	1343.156
3) T	4-Nitroph...	6.731	7.001	2304.0E6	1001.5E6	1291.971	1307.566
5) T	DICAMBA	7.118	7.654	13131.1E6	5728.1E6	1325.990	1450.134
6) T	MCPP	7.300	7.765	992.1E6	254.5E6	153.962	145.490
7) T	MCPA	7.444	7.996	1275.2E6	326.1E6	144.397	137.819
8) T	DICHLORPROP	7.799	8.348	3270.4E6	1352.2E6	1290.535	1346.848
9) T	2,4-D	8.019	8.661	3666.5E6	1519.1E6	1303.464	1347.820
10) T	Pentachlo...	8.300	9.164	43790.4E6	27835.1E6	1255.279	1368.166
11) T	2,4,5-TP ...	8.862	9.543	18378.2E6	11452.1E6	1325.717	1399.712
12) T	2,4,5-T	9.144	9.947	18581.8E6	10783.8E6	1322.259	1389.199
13) T	2,4-DB	9.702	10.507	3190.6E6	1148.5E6	1396.120	1426.978
14) T	DINOSEB	10.866	10.881	13258.0E6	7950.4E6	1303.197	1363.473
15) T	Picloram	10.684	11.923	25181.9E6	33589.7E6	1373.763	2722.382 #
16) T	DCPA	11.166	11.923	22629.5E6	33589.7E6	1329.504	2961.816 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029923.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 12:37  
 Operator : AR\AJ  
 Sample : HSTDICC1500  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1



**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**HSTDICC1500**


Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 12:55:49 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:55:41 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l

Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2

Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

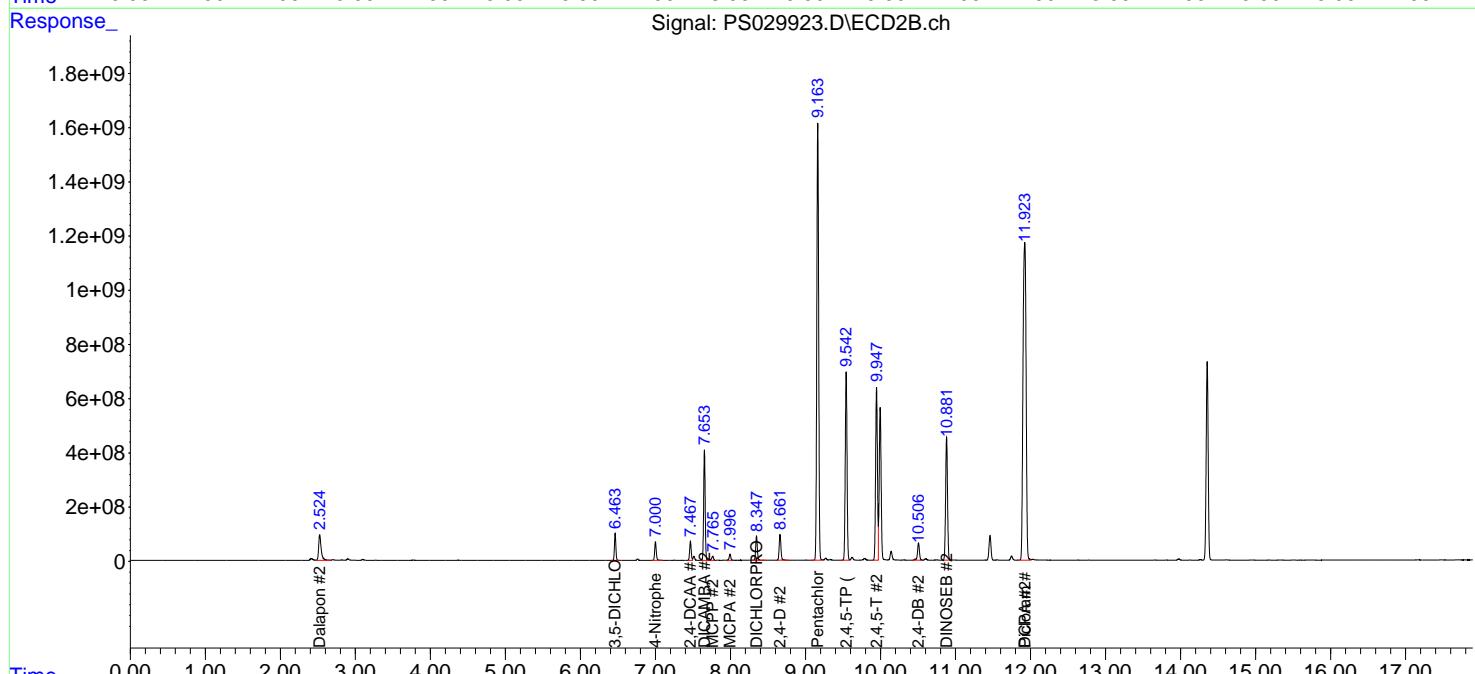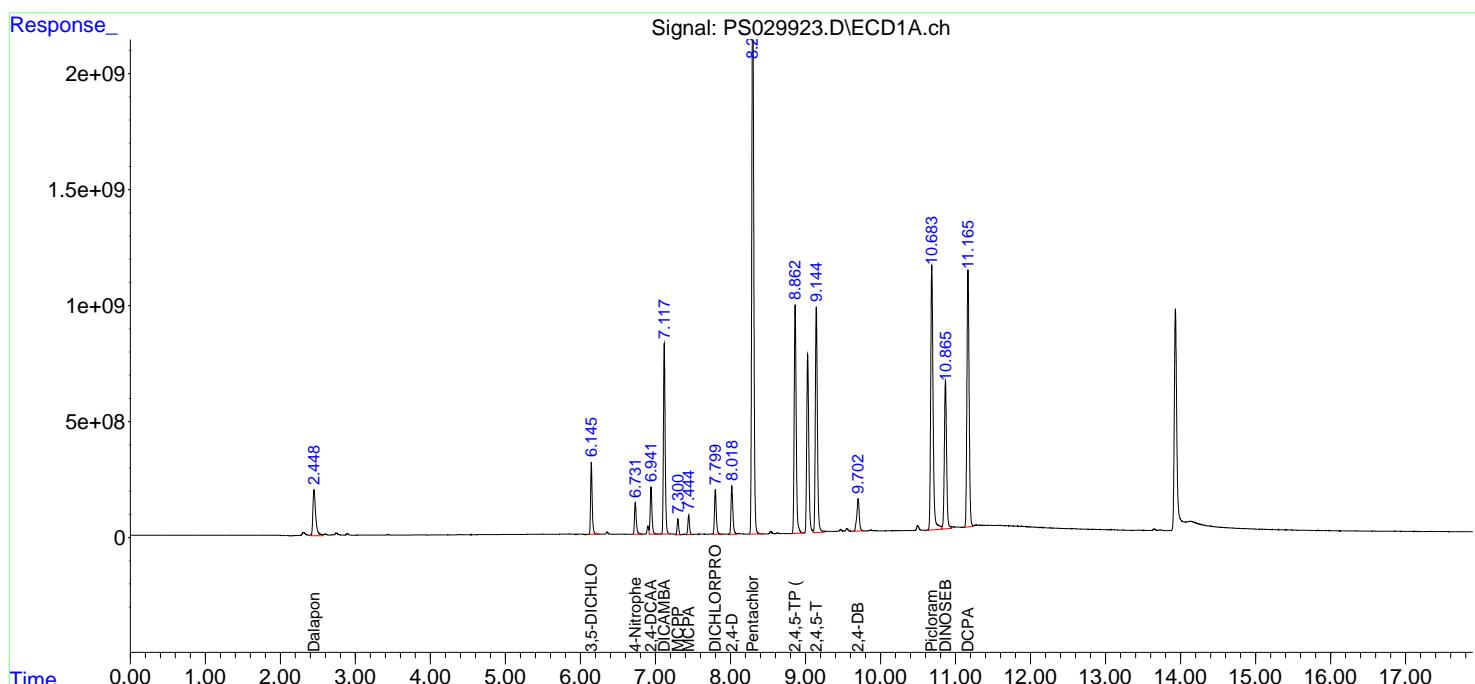

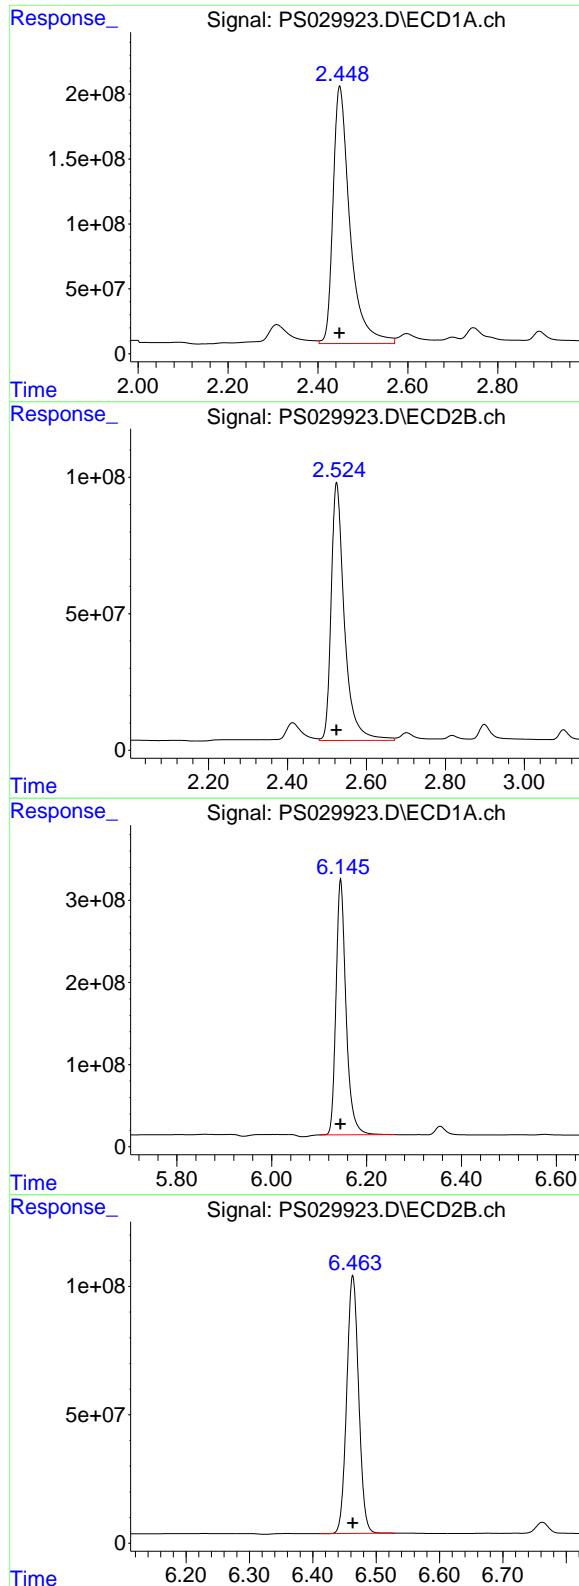

#1 Dalapon

R.T.: 2.448 min  
 Delta R.T.: 0.000 min **Instrument:**  
 Response: 5176670282 ECD\_S  
 Conc: 1264.06 ng/ml **ClientSampleId:**  
 HSTDICC1500

#1 Dalapon


R.T.: 2.524 min  
 Delta R.T.: 0.000 min  
 Response: 2212117489  
 Conc: 1274.16 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.145 min  
 Delta R.T.: 0.000 min  
 Response: 4570485622  
 Conc: 1278.89 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.463 min  
 Delta R.T.: 0.000 min  
 Response: 1313041128  
 Conc: 1343.16 ng/ml

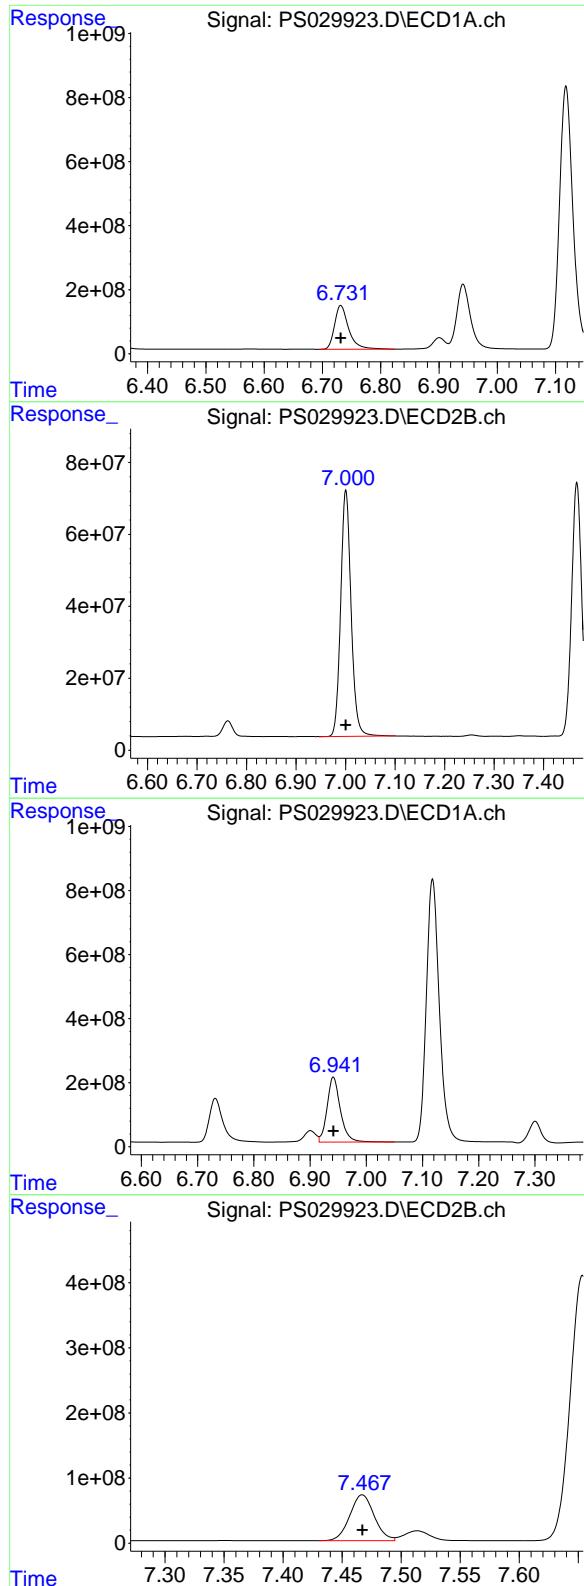

#3 4-Nitrophenol

R.T.: 6.731 min  
 Delta R.T.: 0.000 min  
**Instrument:**  
 Response: 2303997056 ECD\_S  
 Conc: 1291.97 ng/ml  
**ClientSampleId:**  
 HSTDICC1500

#3 4-Nitrophenol


R.T.: 7.001 min  
 Delta R.T.: 0.000 min  
 Response: 1001492635  
 Conc: 1307.57 ng/ml

#4 2,4-DCAA

R.T.: 6.941 min  
 Delta R.T.: 0.000 min  
 Response: 3340247176  
 Conc: 1357.23 ng/ml

#4 2,4-DCAA

R.T.: 7.467 min  
 Delta R.T.: 0.000 min  
 Response: 1016603254  
 Conc: 1442.98 ng/ml

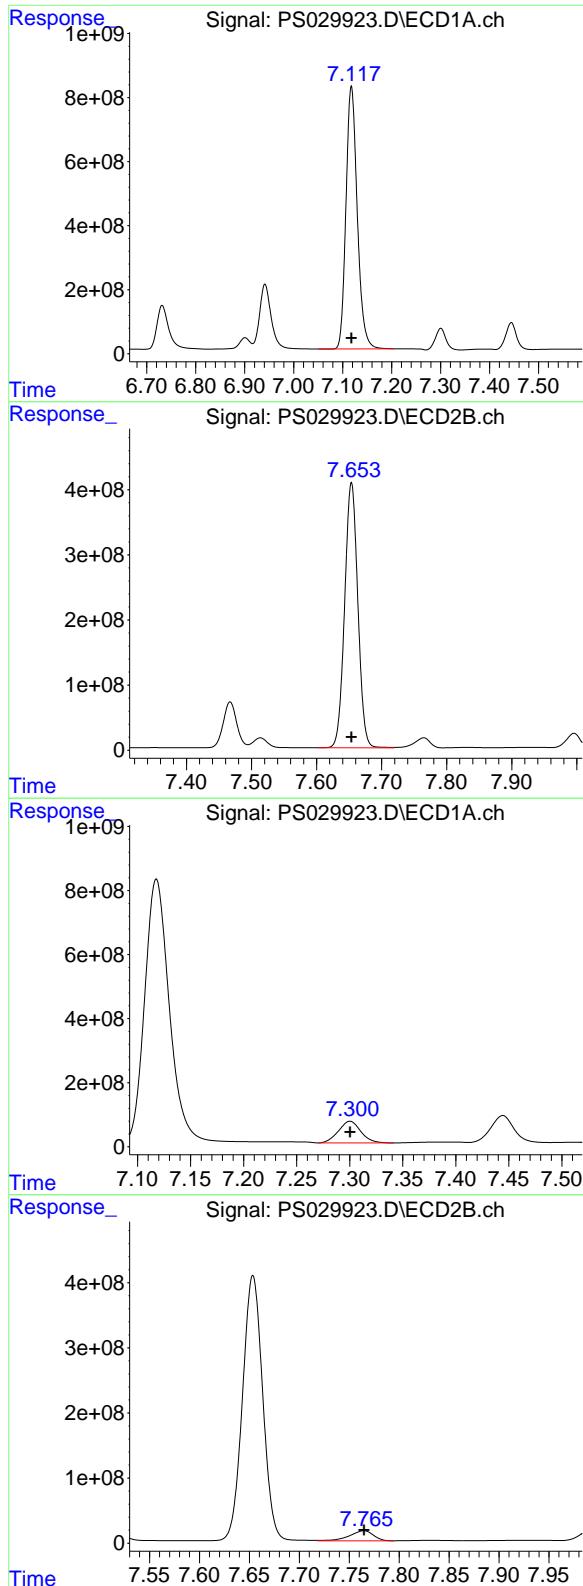

#5 DICAMBA

R.T.: 7.118 min  
 Delta R.T.: 0.000 min **Instrument:**  
 Response: 13131098945 ECD\_S  
 Conc: 1325.99 ng/ml **ClientSampleId:**  
 HSTDICC1500

#5 DICAMBA


R.T.: 7.654 min  
 Delta R.T.: 0.000 min  
 Response: 5728123349  
 Conc: 1450.13 ng/ml

#6 MCPP

R.T.: 7.300 min  
 Delta R.T.: 0.000 min  
 Response: 992077341  
 Conc: 153.96 ug/ml

#6 MCPP

R.T.: 7.765 min  
 Delta R.T.: 0.000 min  
 Response: 254454768  
 Conc: 145.49 ug/ml

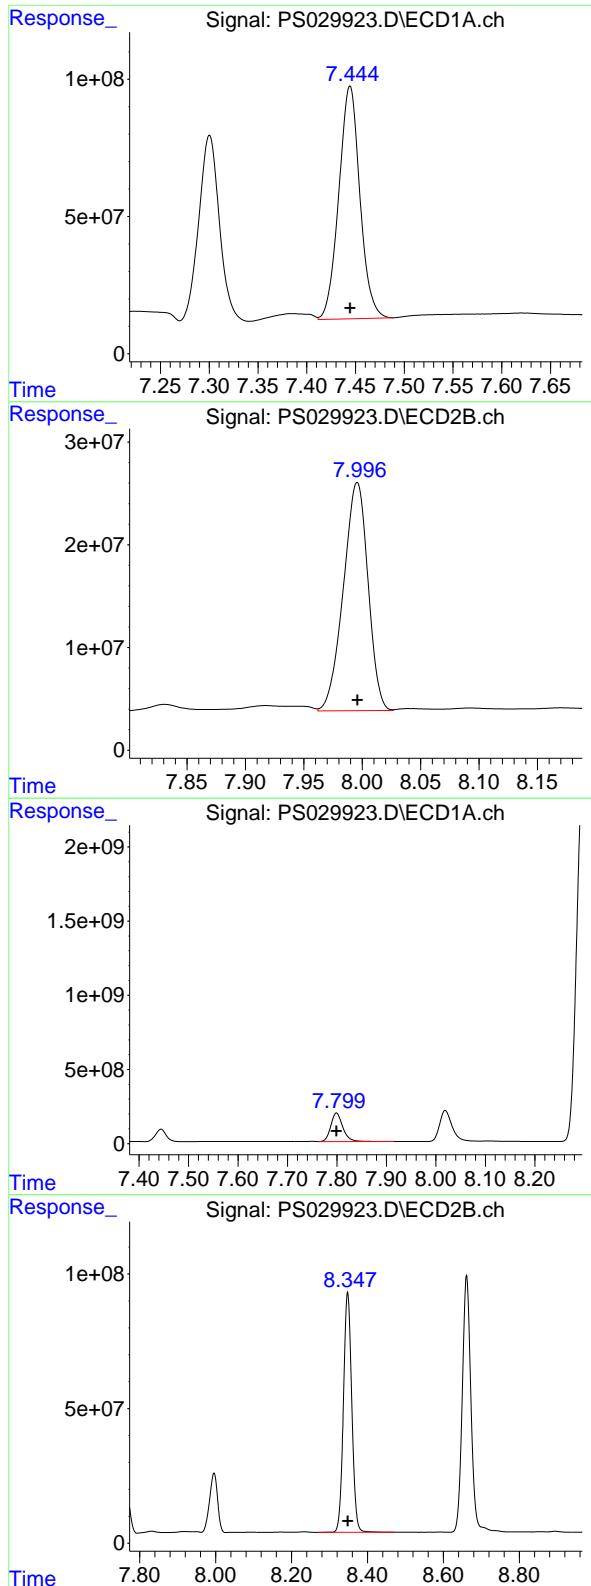

#7 MCPA

R.T.: 7.444 min  
 Delta R.T.: 0.000 min  
 Response: 1275219029  
 Conc: 144.40 ug/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDICC1500

#7 MCPA


R.T.: 7.996 min  
 Delta R.T.: 0.000 min  
 Response: 326053003  
 Conc: 137.82 ug/ml

#8 DICHLOPROP

R.T.: 7.799 min  
 Delta R.T.: 0.000 min  
 Response: 3270356058  
 Conc: 1290.54 ng/ml

#8 DICHLOPROP

R.T.: 8.348 min  
 Delta R.T.: 0.000 min  
 Response: 1352187583  
 Conc: 1346.85 ng/ml

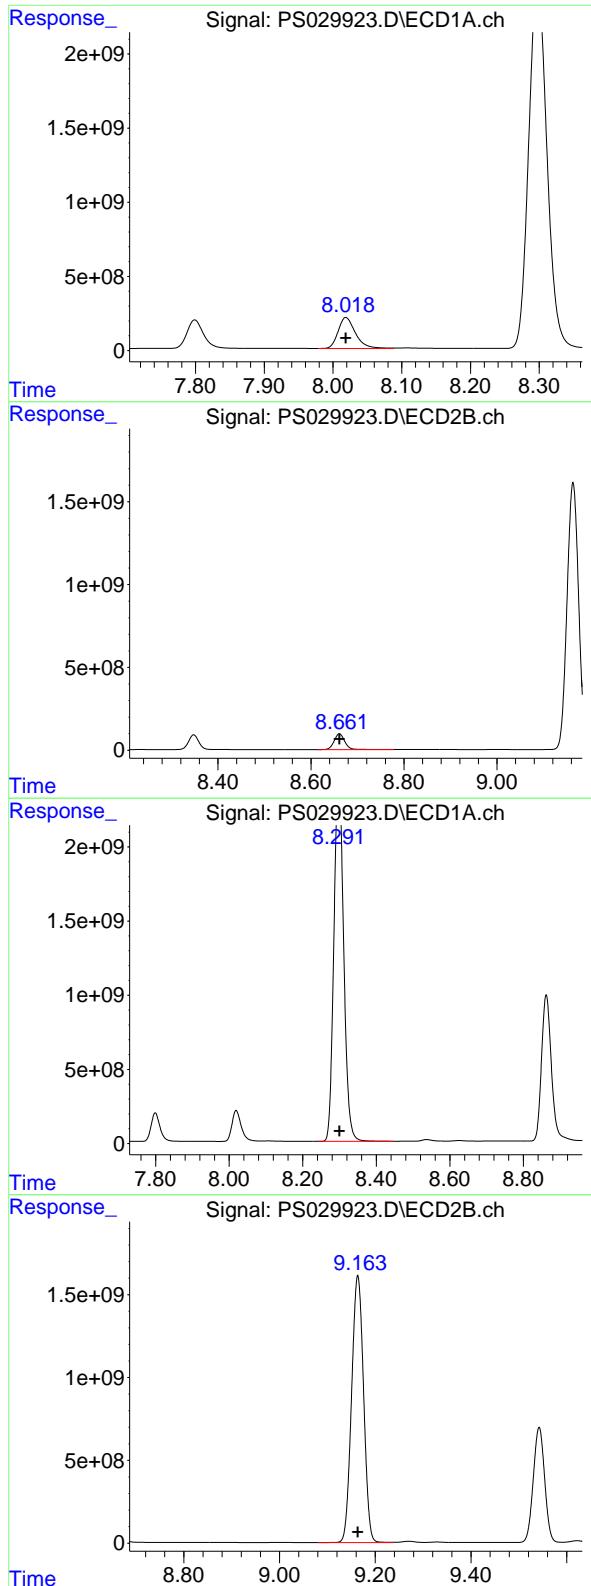

#9 2,4-D

R.T.: 8.019 min  
Delta R.T.: 0.000 min  
Instrument: ECD\_S  
Response: 3666476235  
Conc: 1303.46 ng/ml ClientSampleId : HSTDICC1500

#9 2,4-D


R.T.: 8.661 min  
Delta R.T.: 0.000 min  
Response: 1519137434  
Conc: 1347.82 ng/ml

#10 Pentachlorophenol

R.T.: 8.300 min  
Delta R.T.: 0.000 min  
Response: 43790422023  
Conc: 1255.28 ng/ml

#10 Pentachlorophenol

R.T.: 9.164 min  
Delta R.T.: 0.000 min  
Response: 27835080663  
Conc: 1368.17 ng/ml

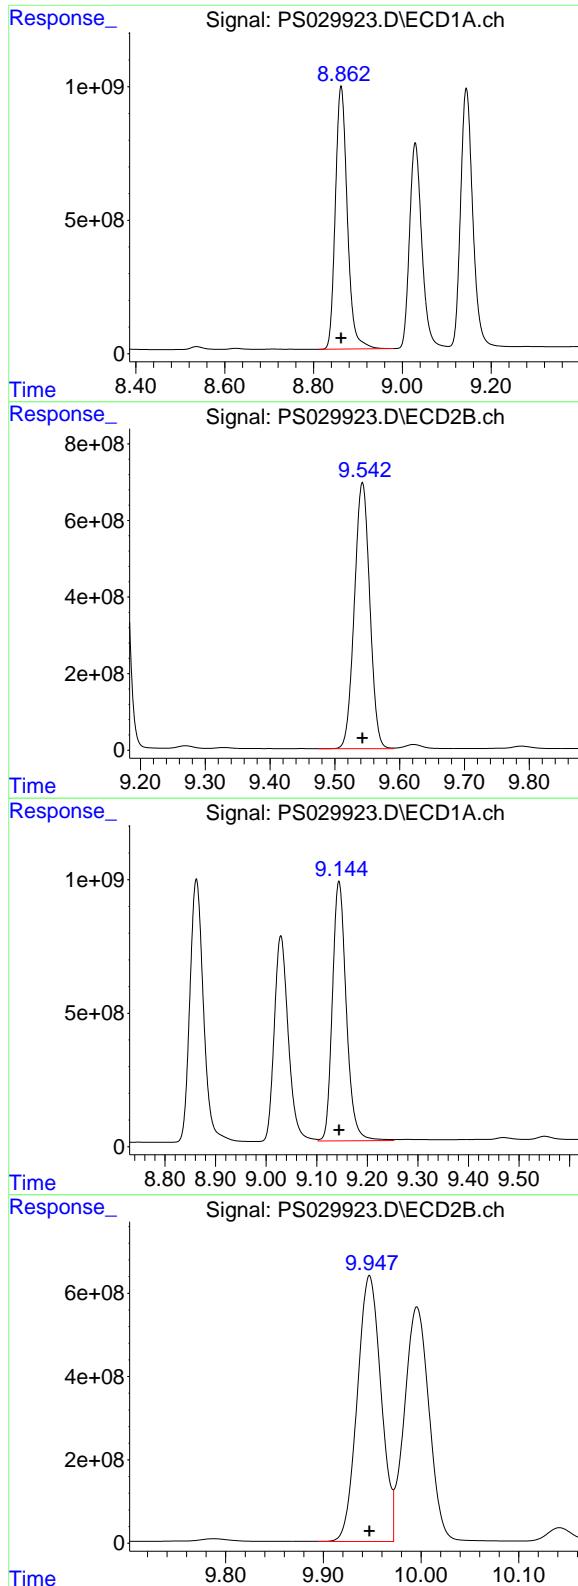

#11 2,4,5-TP (SILVEX)

R.T.: 8.862 min  
 Delta R.T.: 0.000 min  
 Response: 18378203400  
 Conc: 1325.72 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDICC1500

#11 2,4,5-TP (SILVEX)


R.T.: 9.543 min  
 Delta R.T.: 0.000 min  
 Response: 11452091600  
 Conc: 1399.71 ng/ml

#12 2,4,5-T

R.T.: 9.144 min  
 Delta R.T.: 0.000 min  
 Response: 18581844789  
 Conc: 1322.26 ng/ml

#12 2,4,5-T

R.T.: 9.947 min  
 Delta R.T.: 0.000 min  
 Response: 10783792004  
 Conc: 1389.20 ng/ml

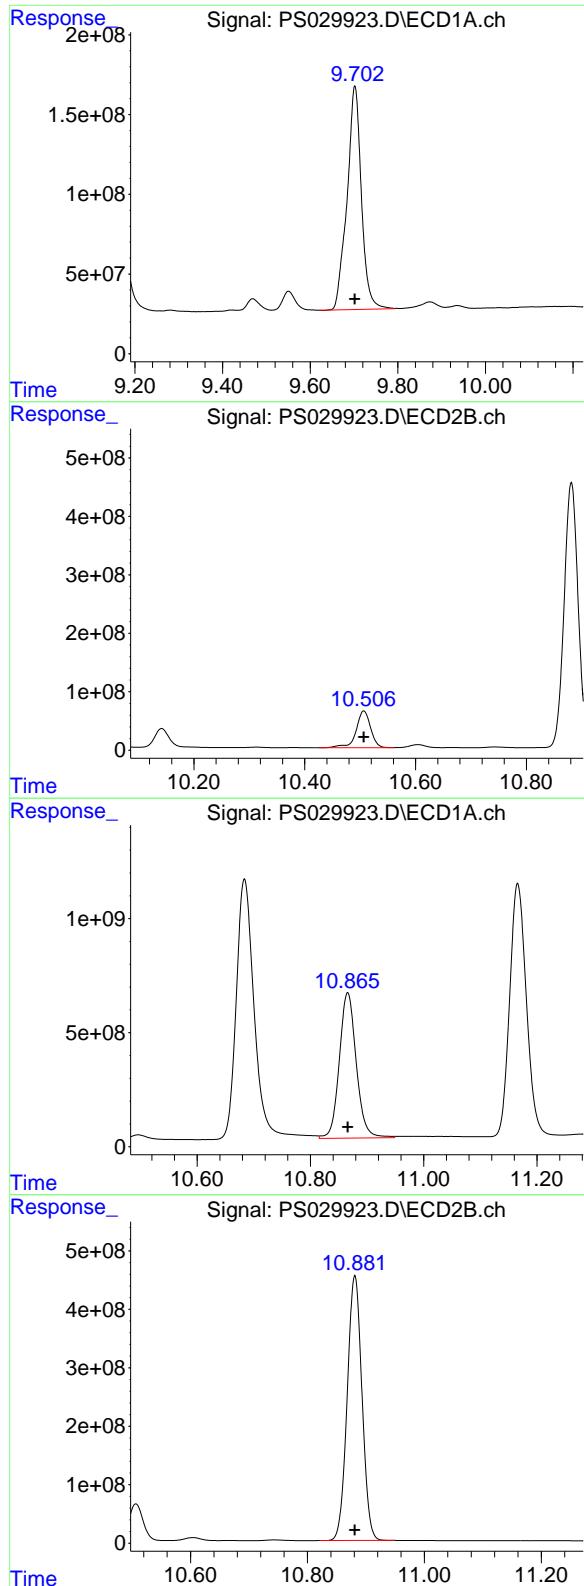

#13 2,4-DB

R.T.: 9.702 min  
 Delta R.T.: 0.000 min  
 Response: 3190632076  
 Conc: 1396.12 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDICC1500

#13 2,4-DB


R.T.: 10.507 min  
 Delta R.T.: 0.000 min  
 Response: 1148492462  
 Conc: 1426.98 ng/ml

#14 DINOSEB

R.T.: 10.866 min  
 Delta R.T.: 0.000 min  
 Response: 13257982778  
 Conc: 1303.20 ng/ml

#14 DINOSEB

R.T.: 10.881 min  
 Delta R.T.: 0.000 min  
 Response: 7950383575  
 Conc: 1363.47 ng/ml

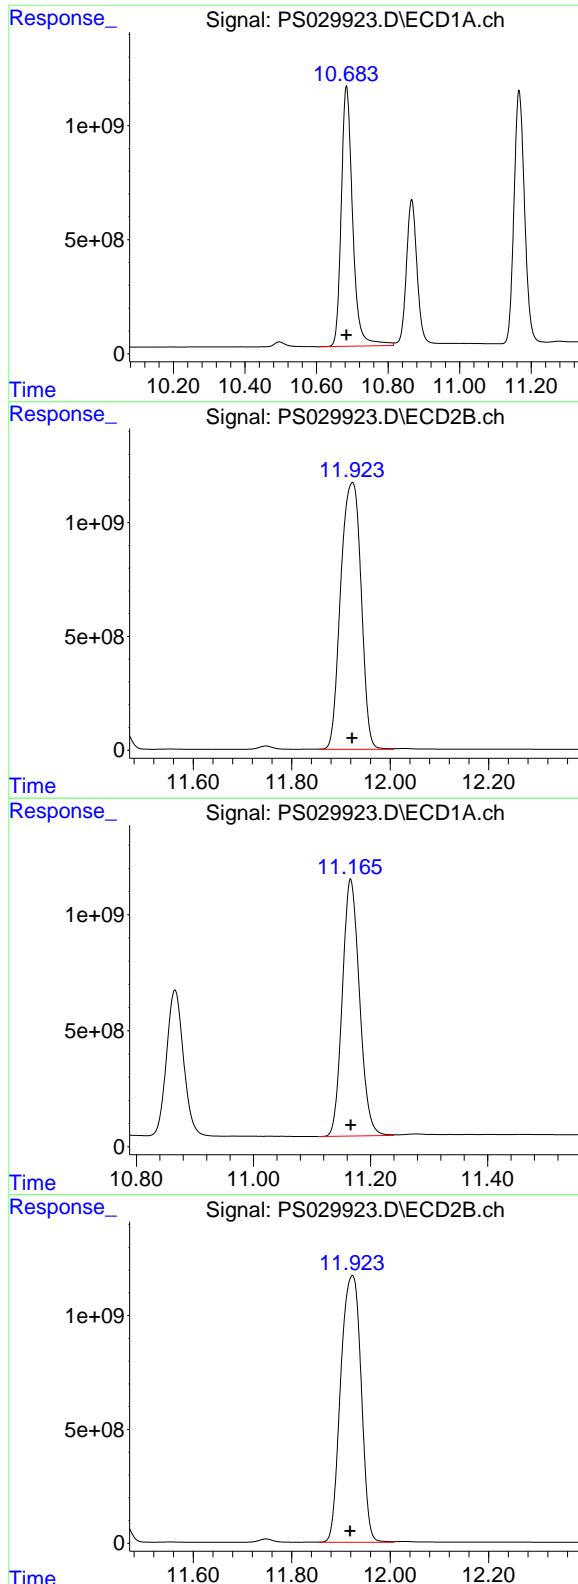

#15 Picloram

R.T.: 10.684 min  
 Delta R.T.: 0.000 min  
**Instrument:**  
 Response: 25181937899 ECD\_S  
 Conc: 1373.76 ng/ml  
**ClientSampleId :**  
 HSTDICC1500

#15 Picloram

R.T.: 11.923 min  
 Delta R.T.: 0.000 min  
 Response: 33589683389  
 Conc: 2722.38 ng/ml

#16 DCPA

R.T.: 11.166 min  
 Delta R.T.: 0.000 min  
 Response: 22629488258  
 Conc: 1329.50 ng/ml

#16 DCPA

R.T.: 11.923 min  
 Delta R.T.: 0.005 min  
 Response: 33589683389  
 Conc: 2961.82 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029924.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 13:01  
 Operator : AR\AJ  
 Sample : HSTDICV750  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**ICVPS042325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 13:20:38 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.941 7.467 1785.1E6 522.8E6 725.315 742.096

Target Compounds

1) T	Dalapon	2.449	2.525	2793.7E6	1167.7E6	682.183	672.600
2) T	3,5-DICHL...	6.145	6.463	2447.4E6	679.4E6	684.816	695.005
3) T	4-Nitroph...	6.732	7.000	1167.8E6	514.6E6	654.846	671.850
5) T	DICAMBA	7.118	7.653	6990.7E6	2822.8E6	705.926	714.619
6) T	MCPP	7.297	7.760	467.2E6	127.4E6	72.508	72.837
7) T	MCPA	7.439	7.991	617.1E6	165.5E6	69.876	69.959
8) T	DICHLORPROP	7.798	8.347	1751.5E6	702.7E6	691.189	699.969
9) T	2,4-D	8.018	8.661	1976.8E6	789.4E6	702.764	700.374
10) T	Pentachlo...	8.297	9.163	25231.5E6	14767.7E6	723.277	725.871
11) T	2,4,5-TP ...	8.862	9.542	9894.0E6	5913.4E6	713.706	722.753
12) T	2,4,5-T	9.144	9.947	9990.5E6	5588.6E6	710.908	719.944
13) T	2,4-DB	9.702	10.506	1649.4E6	582.7E6	721.719	724.013
14) T	DINOSEB	10.866	10.881	7070.7E6	4118.9E6	695.014	706.382
15) T	Picloram	10.685	11.923	13255.1E6	17280.6E6	723.112	1406.800 #
16) T	DCPA	11.167	11.923	12285.5E6	17280.6E6	721.785	1533.105 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS042325\  
 Data File : PS029924.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Apr 2025 13:01  
 Operator : AR\AJ  
 Sample : HSTDICV750  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**ICVPS042325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 23 13:20:38 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

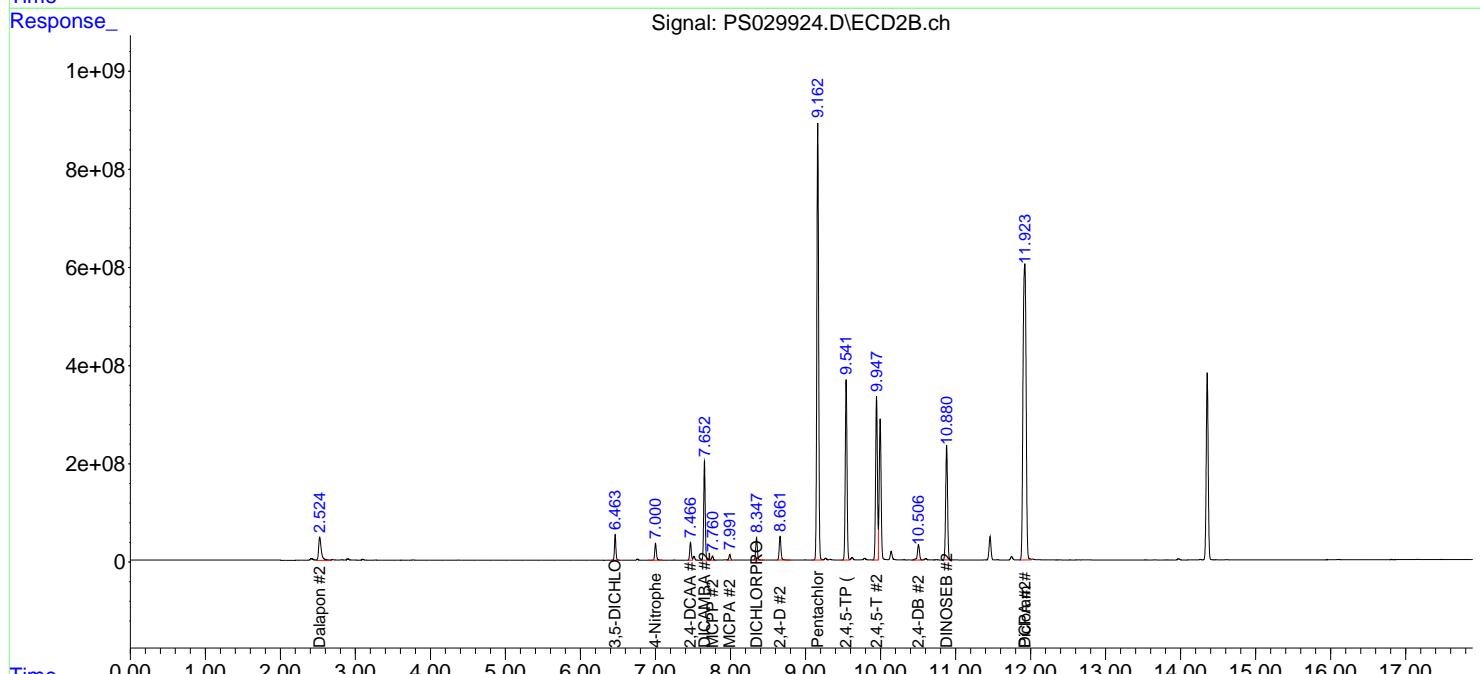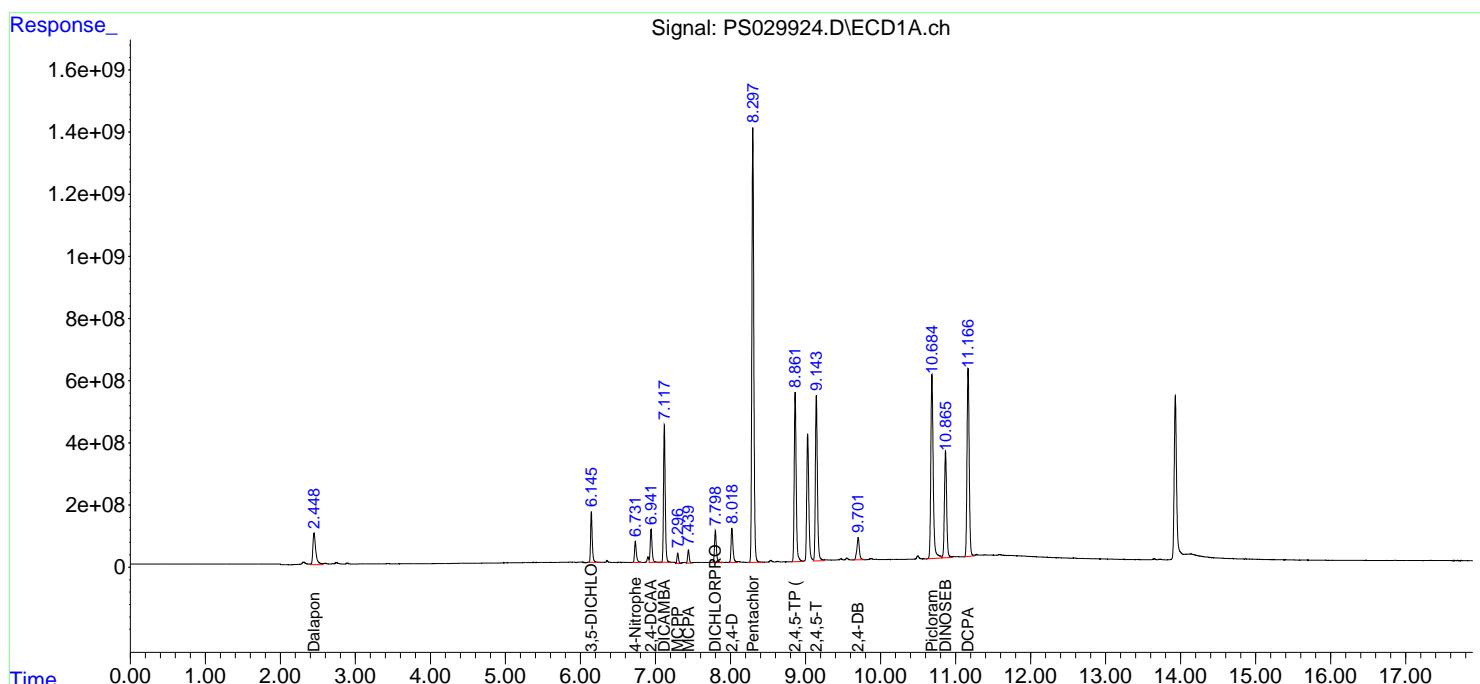

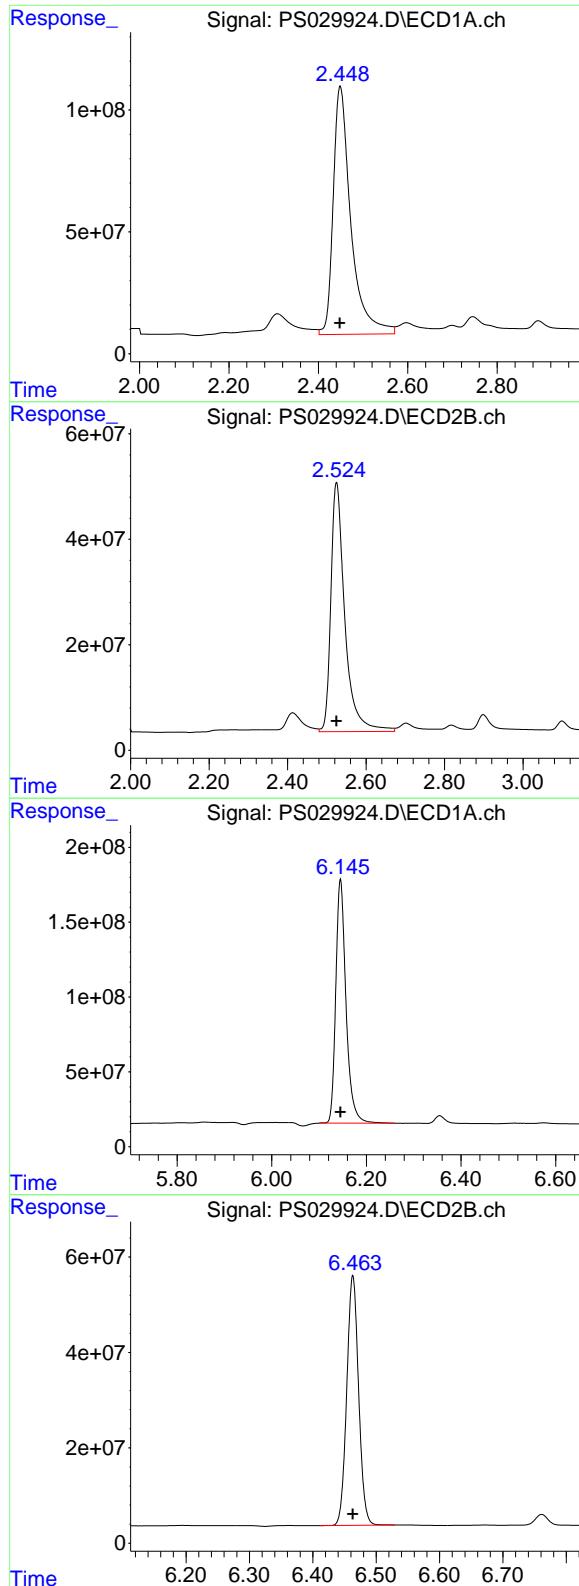

#1 Dalapon

R.T.: 2.449 min  
 Delta R.T.: 0.000 min  
 Response: 2793715347  
 Conc: 682.18 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** ICVPS042325

#1 Dalapon


R.T.: 2.525 min  
 Delta R.T.: 0.000 min  
 Response: 1167729659  
 Conc: 672.60 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.145 min  
 Delta R.T.: 0.000 min  
 Response: 2447386587  
 Conc: 684.82 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.463 min  
 Delta R.T.: 0.000 min  
 Response: 679422841  
 Conc: 695.01 ng/ml

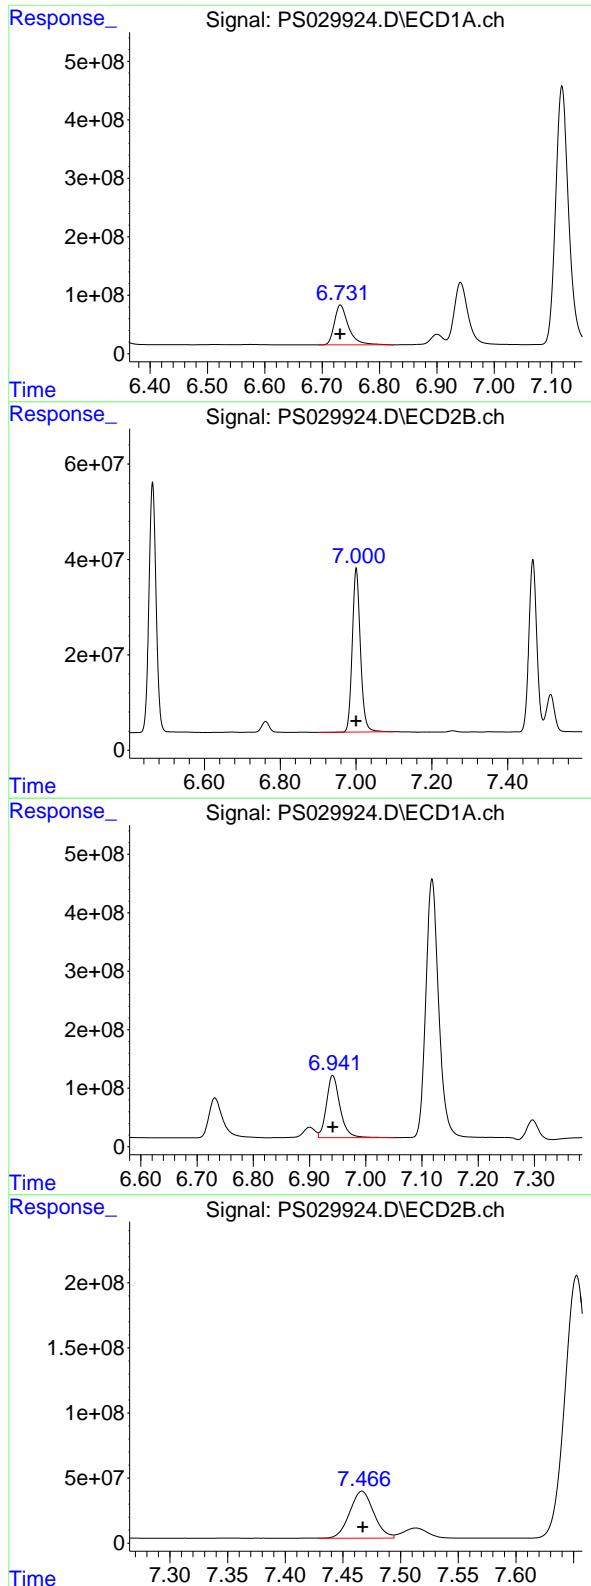

#3 4-Nitrophenol

R.T.: 6.732 min  
 Delta R.T.: 0.000 min  
 Response: 1167800121  
 Conc: 654.85 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** ICVPS042325

#3 4-Nitrophenol


R.T.: 7.000 min  
 Delta R.T.: 0.000 min  
 Response: 514583941  
 Conc: 671.85 ng/ml

#4 2,4-DCAA

R.T.: 6.941 min  
 Delta R.T.: 0.000 min  
 Response: 1785057977  
 Conc: 725.32 ng/ml

#4 2,4-DCAA

R.T.: 7.467 min  
 Delta R.T.: 0.000 min  
 Response: 522819399  
 Conc: 742.10 ng/ml

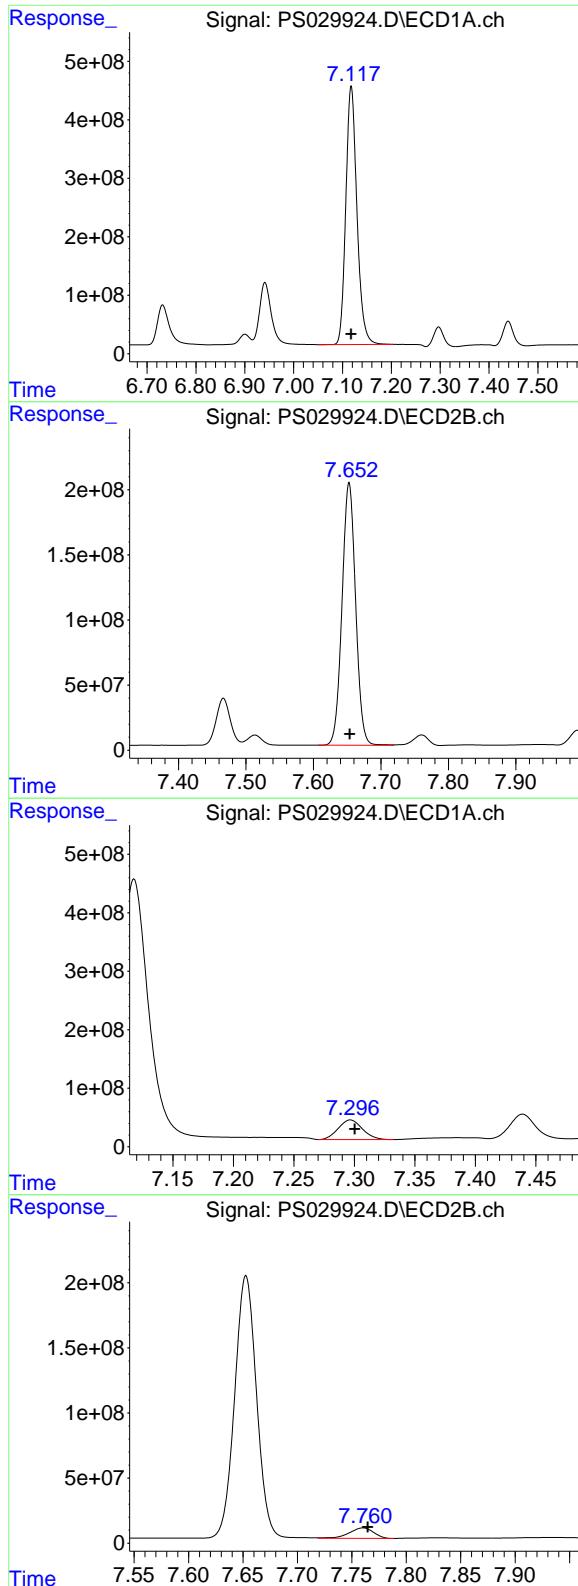

#5 DICAMBA

R.T.: 7.118 min  
 Delta R.T.: 0.000 min  
 Response: 6990688242  
 Conc: 705.93 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** ICVPS042325

#5 DICAMBA


R.T.: 7.653 min  
 Delta R.T.: 0.000 min  
 Response: 2822792480  
 Conc: 714.62 ng/ml

#6 MCPP

R.T.: 7.297 min  
 Delta R.T.: -0.004 min  
 Response: 467215325  
 Conc: 72.51 ug/ml

#6 MCPP

R.T.: 7.760 min  
 Delta R.T.: -0.004 min  
 Response: 127389122  
 Conc: 72.84 ug/ml

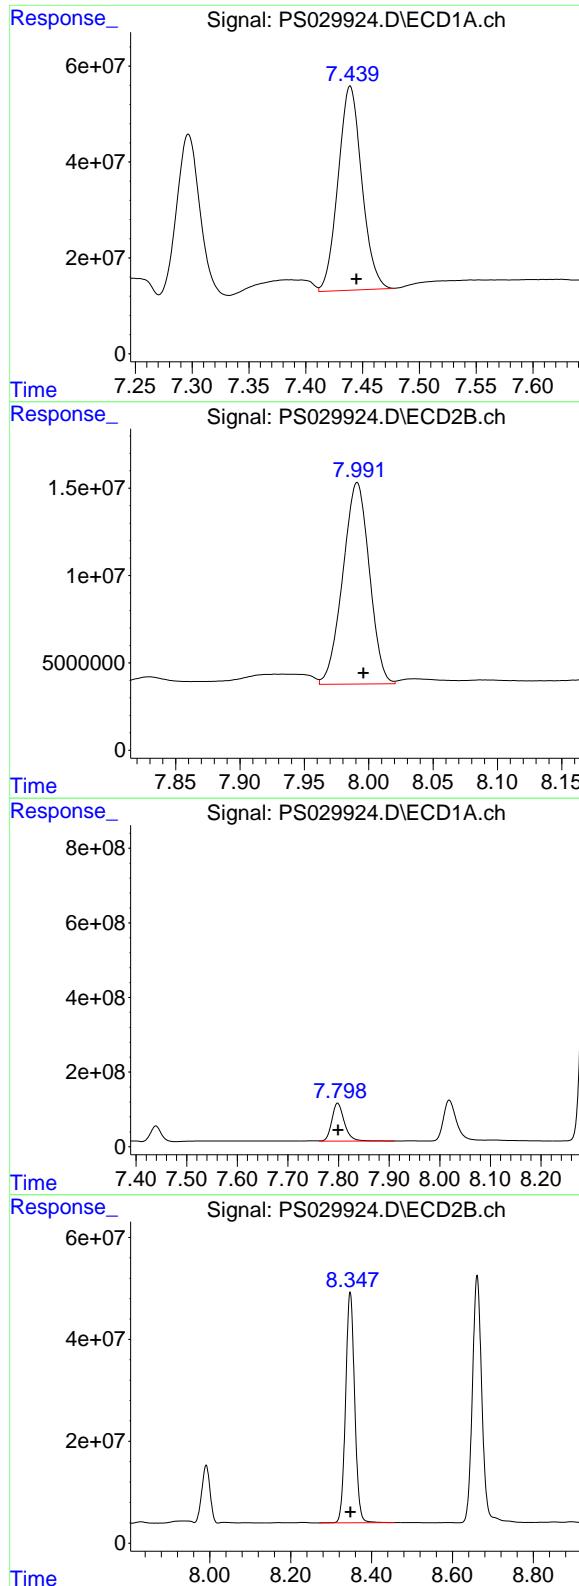

#7 MCPA

R.T.: 7.439 min  
 Delta R.T.: -0.005 min  
 Response: 617101386  
 Conc: 69.88 ug/ml

Instrument: ECD\_S  
 ClientSampleId: ICVPS042325

#7 MCPA


R.T.: 7.991 min  
 Delta R.T.: -0.005 min  
 Response: 165509058  
 Conc: 69.96 ug/ml

#8 DICHLOPROP

R.T.: 7.798 min  
 Delta R.T.: 0.000 min  
 Response: 1751547333  
 Conc: 691.19 ng/ml

#8 DICHLOPROP

R.T.: 8.347 min  
 Delta R.T.: 0.000 min  
 Response: 702743426  
 Conc: 699.97 ng/ml

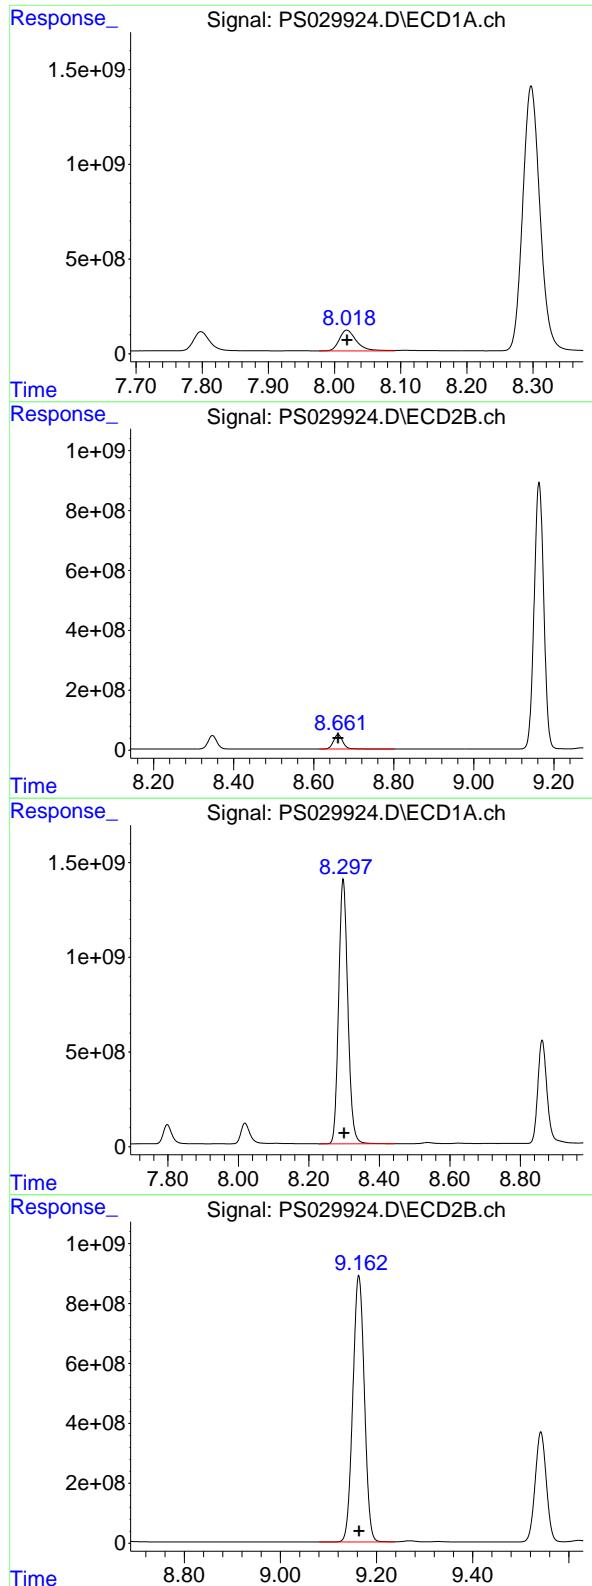

#9 2,4-D

R.T.: 8.018 min  
 Delta R.T.: 0.000 min  
 Response: 1976784235  
 Conc: 702.76 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** ICPVPS042325

#9 2,4-D


R.T.: 8.661 min  
 Delta R.T.: 0.000 min  
 Response: 789396429  
 Conc: 700.37 ng/ml

#10 Pentachlorophenol

R.T.: 8.297 min  
 Delta R.T.: -0.002 min  
 Response: 25231541630  
 Conc: 723.28 ng/ml

#10 Pentachlorophenol

R.T.: 9.163 min  
 Delta R.T.: 0.000 min  
 Response: 14767707242  
 Conc: 725.87 ng/ml

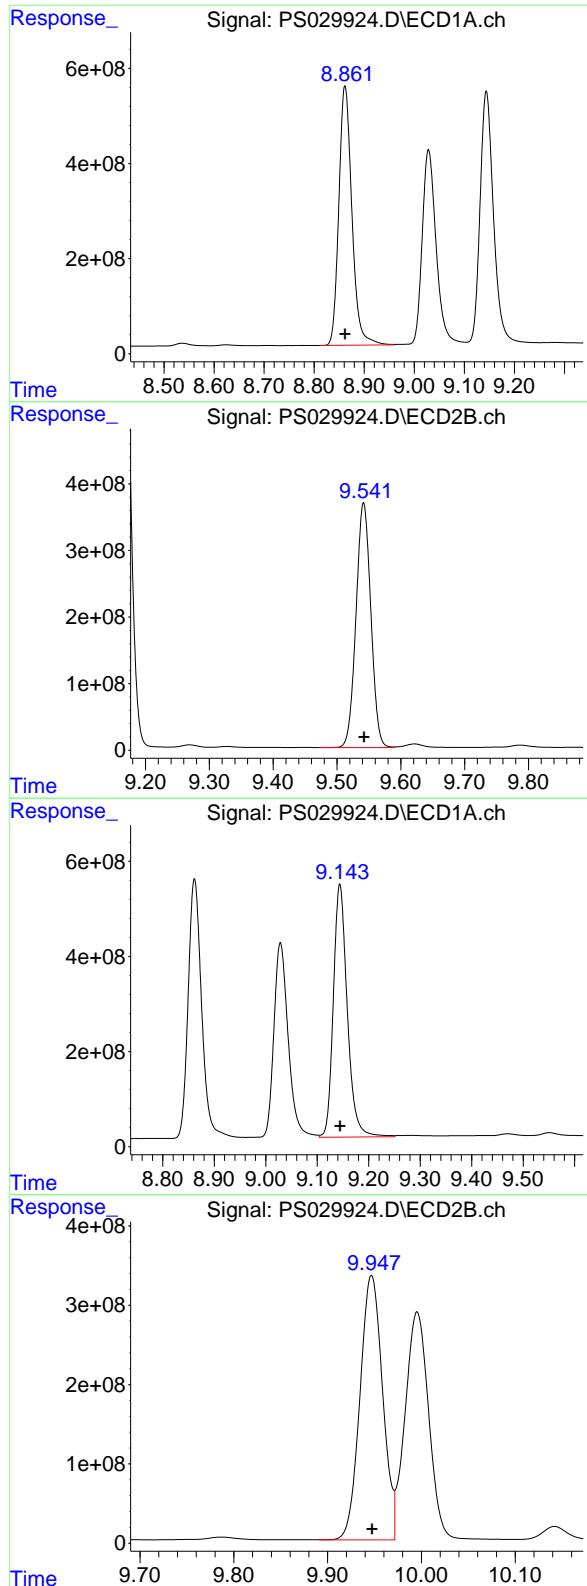

#11 2,4,5-TP (SILVEX)

R.T.: 8.862 min  
 Delta R.T.: 0.000 min  
 Response: 9893987718  
 Conc: 713.71 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** ICVPS042325

#11 2,4,5-TP (SILVEX)


R.T.: 9.542 min  
 Delta R.T.: 0.000 min  
 Response: 5913388172  
 Conc: 722.75 ng/ml

#12 2,4,5-T

R.T.: 9.144 min  
 Delta R.T.: 0.000 min  
 Response: 9990461422  
 Conc: 710.91 ng/ml

#12 2,4,5-T

R.T.: 9.947 min  
 Delta R.T.: 0.000 min  
 Response: 5588639706  
 Conc: 719.94 ng/ml

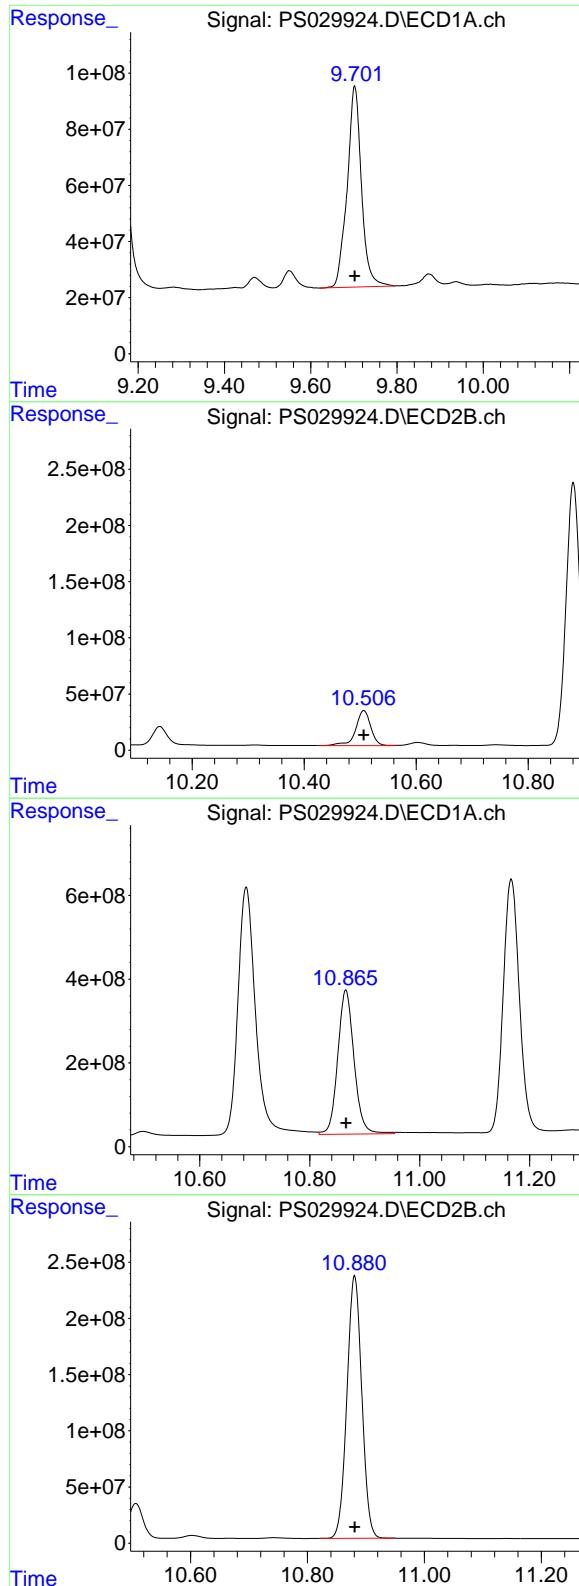

#13 2,4-DB

R.T.: 9.702 min  
 Delta R.T.: 0.000 min  
 Response: 1649385436  
 Conc: 721.72 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** ICVPS042325

#13 2,4-DB


R.T.: 10.506 min  
 Delta R.T.: 0.000 min  
 Response: 582716222  
 Conc: 724.01 ng/ml

#14 DINOSEB

R.T.: 10.866 min  
 Delta R.T.: 0.000 min  
 Response: 7070677904  
 Conc: 695.01 ng/ml

#14 DINOSEB

R.T.: 10.881 min  
 Delta R.T.: 0.000 min  
 Response: 4118901701  
 Conc: 706.38 ng/ml

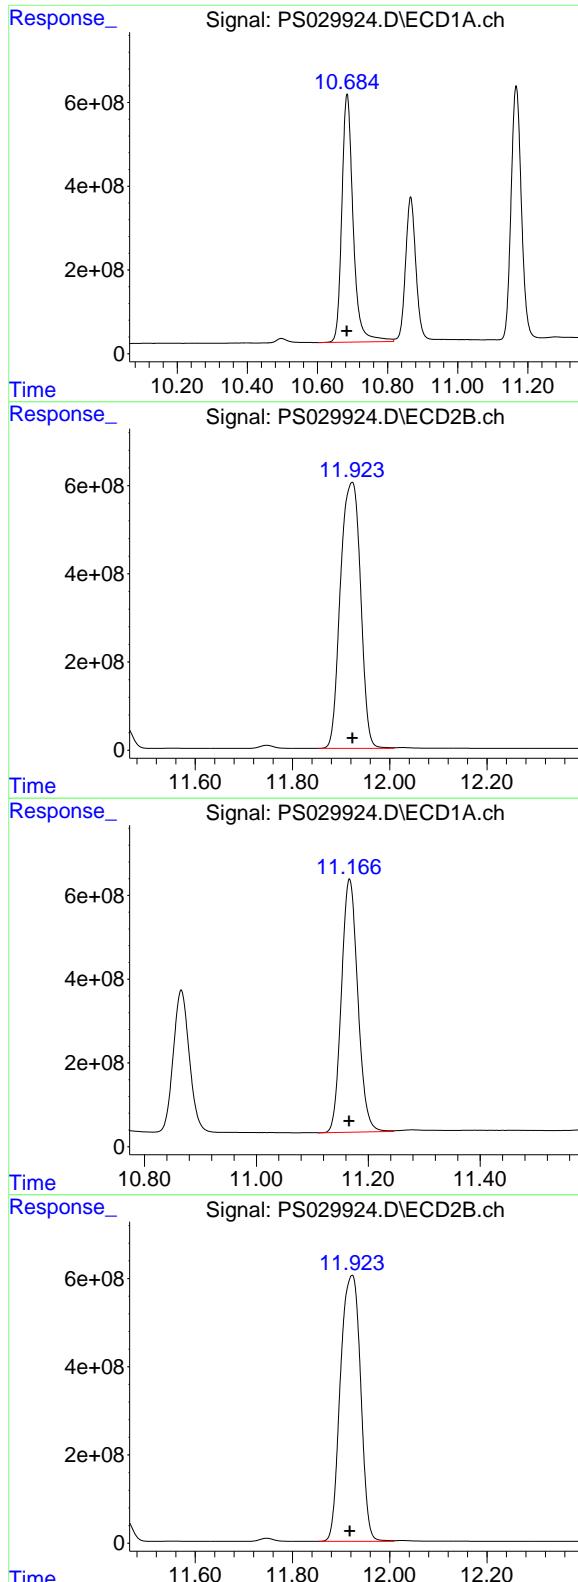

#15 Picloram

R.T.: 10.685 min  
 Delta R.T.: 0.000 min  
 Response: 13255096434 ECD\_S  
 Conc: 723.11 ng/ml ClientSampleId :  
 ICVPS042325

#15 Picloram

R.T.: 11.923 min  
 Delta R.T.: 0.000 min  
 Response: 17280627172  
 Conc: 1406.80 ng/ml

#16 DCPA

R.T.: 11.167 min  
 Delta R.T.: 0.000 min  
 Response: 12285496361  
 Conc: 721.78 ng/ml

#16 DCPA

R.T.: 11.923 min  
 Delta R.T.: 0.005 min  
 Response: 17280627172  
 Conc: 1533.10 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS029991.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 01:22  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**HSTDCCC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 01 01:46:42 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.939 7.463 1866.9E6 564.4E6 758.552 801.051

Target Compounds

1) T	Dalapon	2.449	2.523	2892.9E6	1234.8E6	706.400	711.228
2) T	3,5-DICHL...	6.143	6.460	2518.3E6	726.1E6	704.648	742.792
3) T	4-Nitroph...	6.729	6.996	1243.4E6	555.8E6	697.248	725.719
5) T	DICAMBA	7.116	7.649	7168.2E6	3087.4E6	723.855	781.611
6) T	MCPP	7.294	7.756	466.6E6	129.0E6	72.412	73.739
7) T	MCPA	7.437	7.986	642.6E6	171.6E6	72.763	72.534
8) T	DICHLORPROP	7.796	8.342	1785.1E6	760.6E6	704.424	757.567
9) T	2,4-D	8.016	8.655	2013.0E6	843.4E6	715.648	748.243
10) T	Pentachlo...	8.294	9.156	25792.5E6	16172.6E6	739.359	794.924
11) T	2,4,5-TP ...	8.858	9.534	10127.5E6	6432.9E6	730.547	786.255
12) T	2,4,5-T	9.141	9.938	10350.9E6	6030.3E6	736.554	776.838
13) T	2,4-DB	9.699	10.497	1746.3E6	586.9E6	764.144	729.270
14) T	DINOSEB	10.861	10.870	7271.9E6	4421.7E6	714.798	758.306
15) T	Picloram	10.680	11.908	13551.6E6	18335.9E6	739.289	1492.711 #
16) T	DCPA	11.163	11.908	12619.6E6	18335.9E6	741.412	1626.729 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS029991.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 01:22  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDCCC750

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 01 01:46:42 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

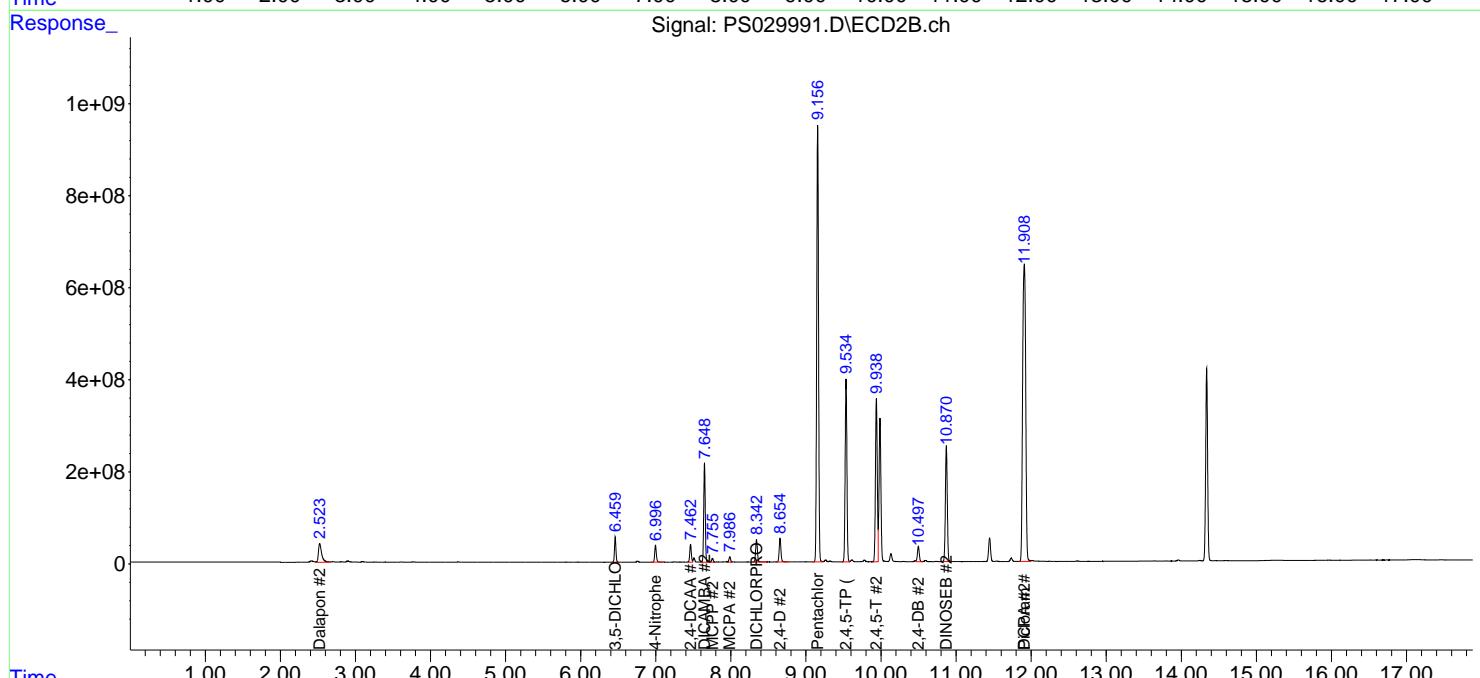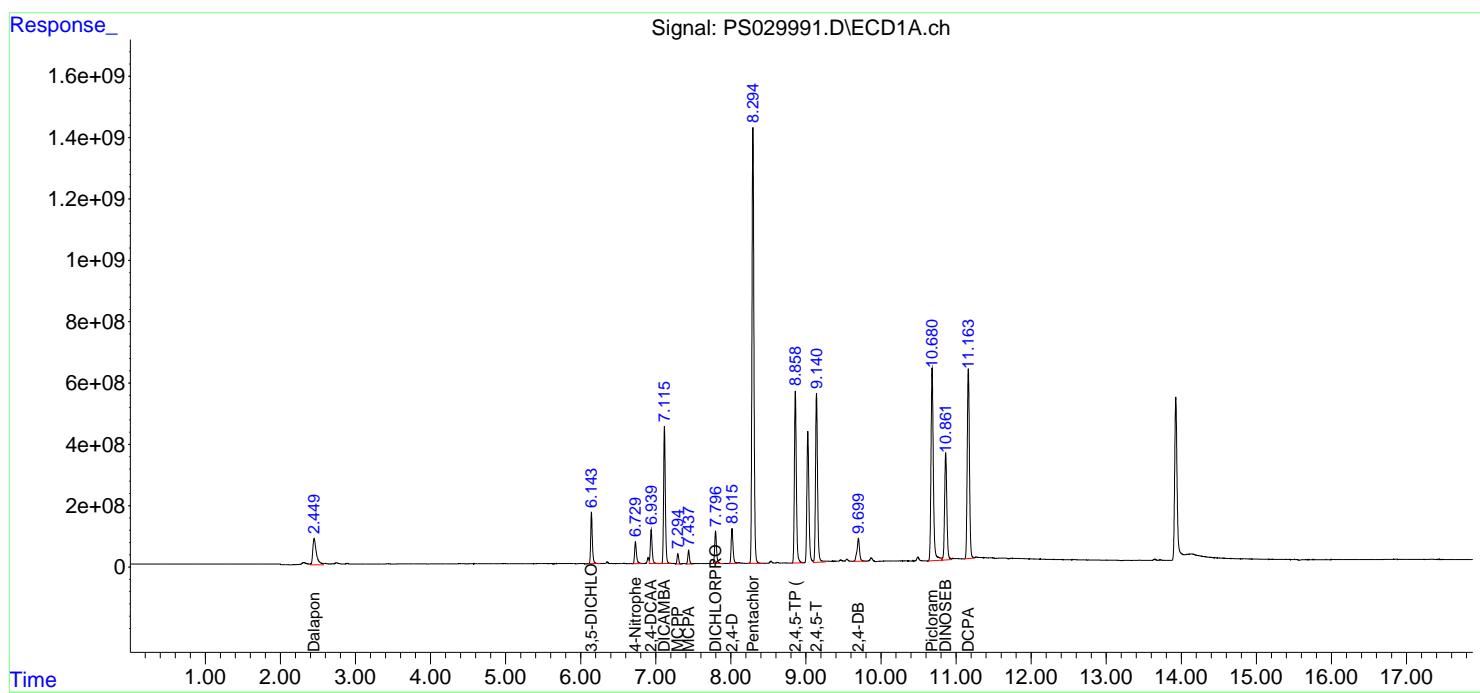

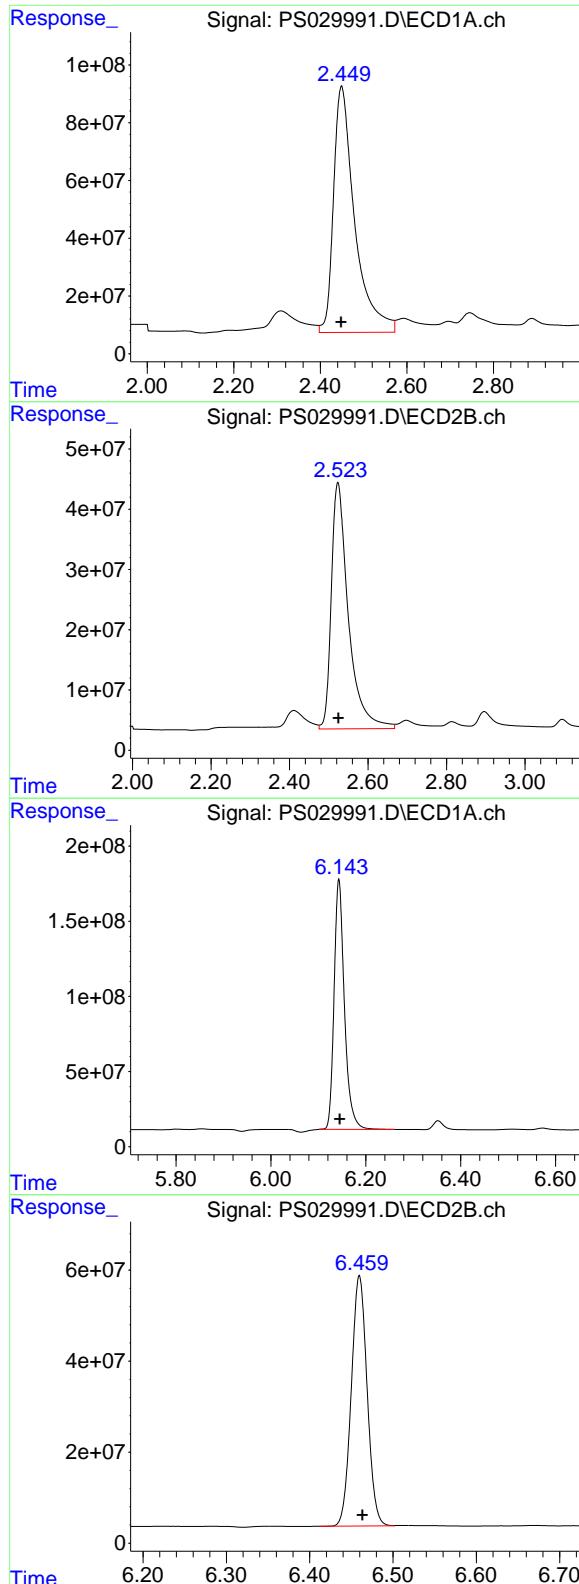

#1 Dalapon

R.T.: 2.449 min  
 Delta R.T.: 0.001 min  
 Response: 2892891563  
 Conc: 706.40 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#1 Dalapon


R.T.: 2.523 min  
 Delta R.T.: -0.001 min  
 Response: 1234794085  
 Conc: 711.23 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.143 min  
 Delta R.T.: -0.002 min  
 Response: 2518260122  
 Conc: 704.65 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.460 min  
 Delta R.T.: -0.003 min  
 Response: 726137732  
 Conc: 742.79 ng/ml

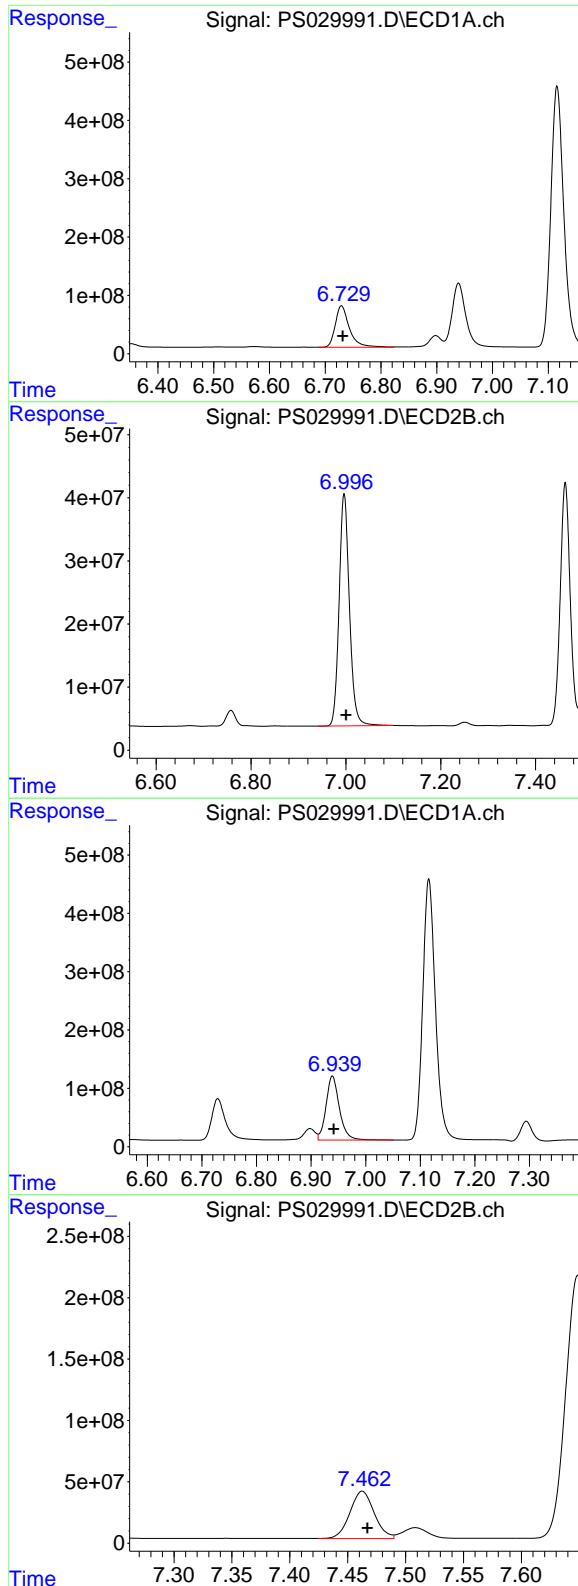

#3 4-Nitrophenol

R.T.: 6.729 min  
 Delta R.T.: -0.002 min  
 Response: 1243415669  
 Conc: 697.25 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** HSTDCCC750

#3 4-Nitrophenol


R.T.: 6.996 min  
 Delta R.T.: -0.004 min  
 Response: 555843920  
 Conc: 725.72 ng/ml

#4 2,4-DCAA

R.T.: 6.939 min  
 Delta R.T.: -0.002 min  
 Response: 1866856353  
 Conc: 758.55 ng/ml

#4 2,4-DCAA

R.T.: 7.463 min  
 Delta R.T.: -0.004 min  
 Response: 564353935  
 Conc: 801.05 ng/ml

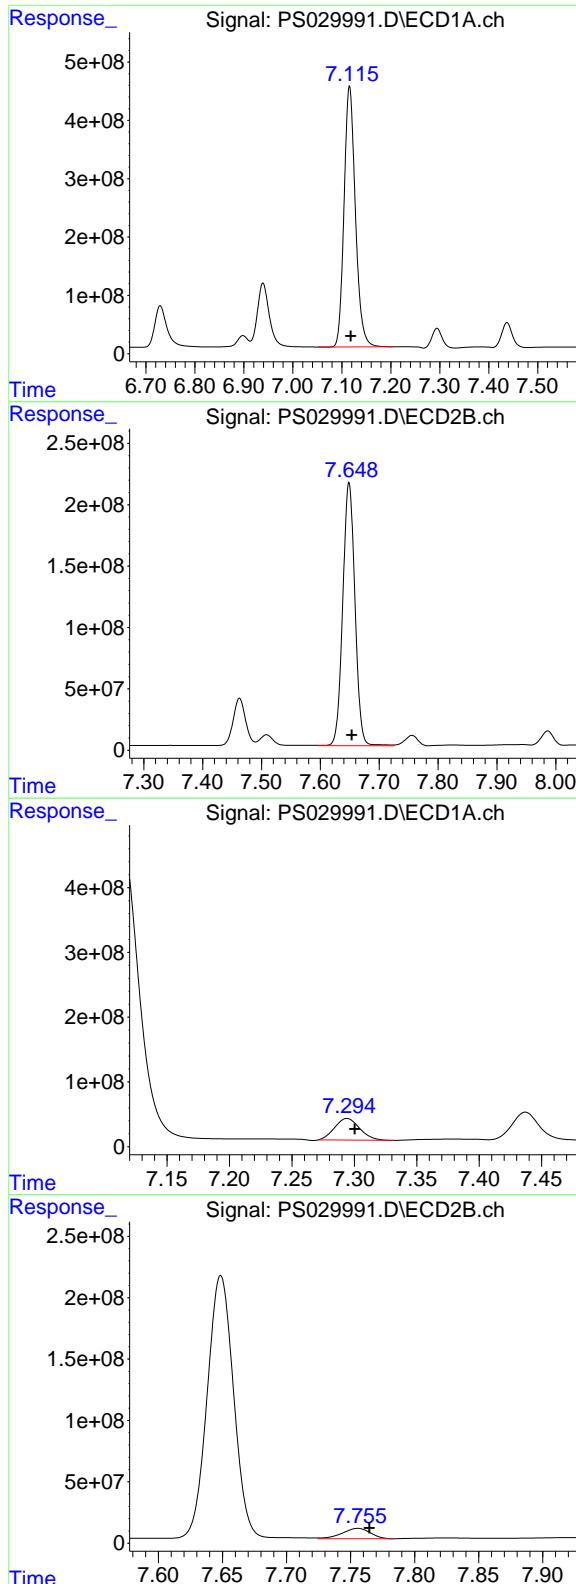

#5 DICAMBA

R.T.: 7.116 min  
 Delta R.T.: -0.002 min  
 Response: 7168239889  
 Conc: 723.86 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** HSTDCCC750

#5 DICAMBA


R.T.: 7.649 min  
 Delta R.T.: -0.005 min  
 Response: 3087414925  
 Conc: 781.61 ng/ml

#6 MCPP

R.T.: 7.294 min  
 Delta R.T.: -0.006 min  
 Response: 466598554  
 Conc: 72.41 ug/ml

#6 MCPP


R.T.: 7.756 min  
 Delta R.T.: -0.009 min  
 Response: 128965896  
 Conc: 73.74 ug/ml

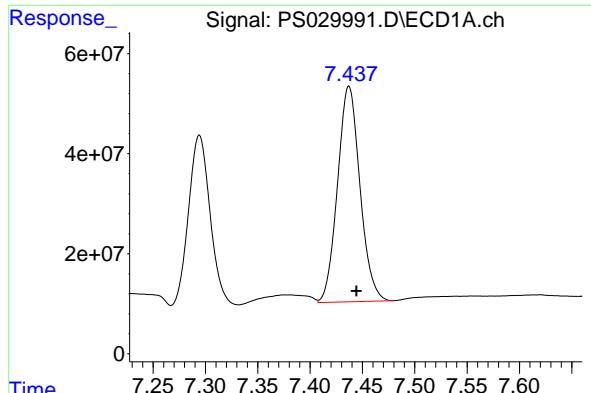

#7 MCPA


R.T.: 7.437 min  
 Delta R.T.: -0.007 min  
 Response: 642595119  
 Conc: 72.76 ug/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

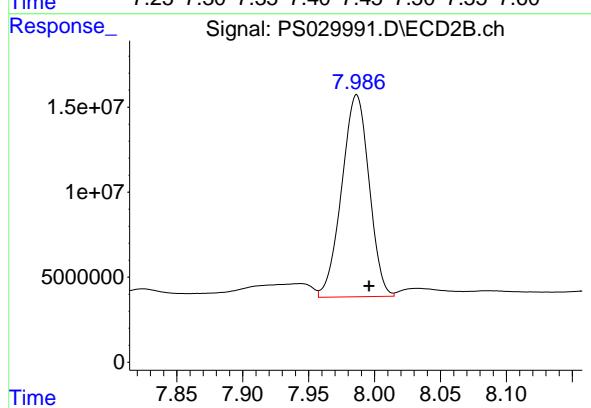


#7 MCPA

R.T.: 7.986 min  
 Delta R.T.: -0.009 min  
 Response: 171601600  
 Conc: 72.53 ug/ml

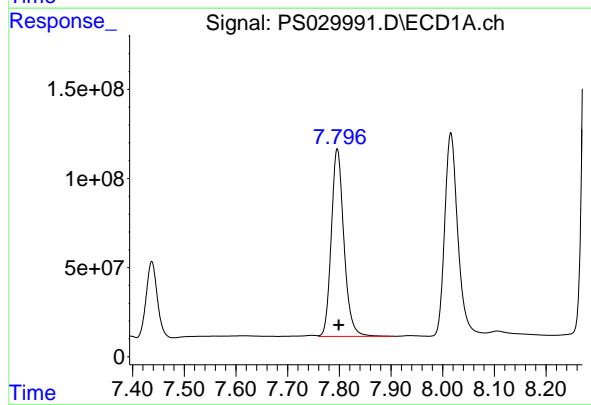


#8 DICHLORPROP

R.T.: 7.796 min  
 Delta R.T.: -0.003 min  
 Response: 1785086910  
 Conc: 704.42 ng/ml

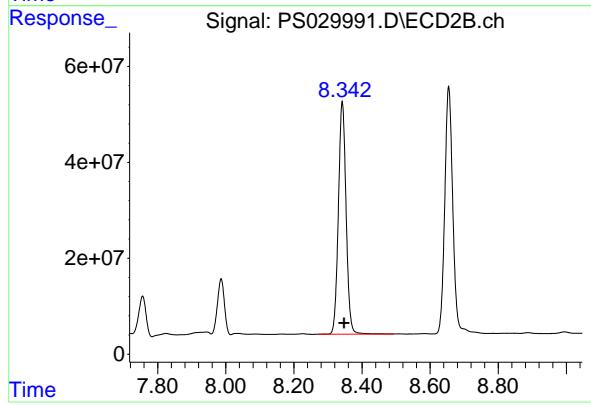

#8 DICHLORPROP

R.T.: 8.342 min  
 Delta R.T.: -0.006 min  
 Response: 760570474  
 Conc: 757.57 ng/ml

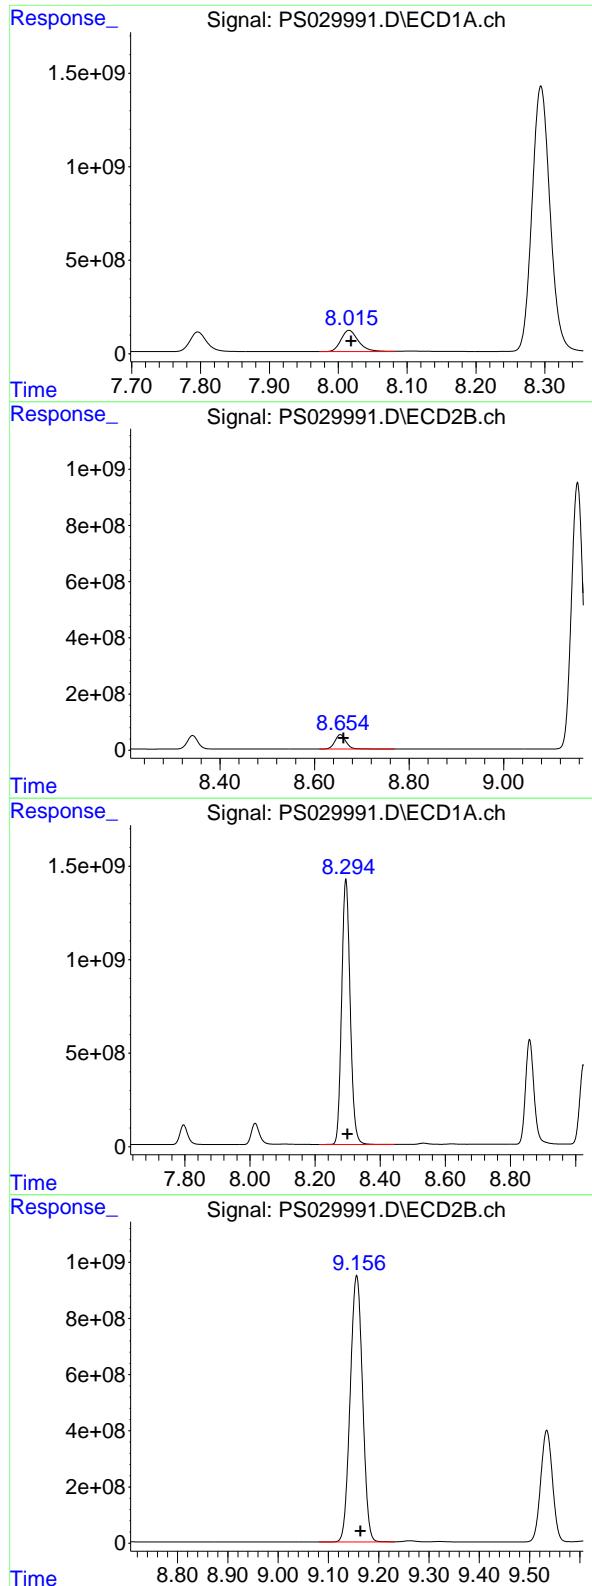

#9 2,4-D

R.T.: 8.016 min  
 Delta R.T.: -0.003 min  
 Response: 2013024091  
 Conc: 715.65 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#9 2,4-D


R.T.: 8.655 min  
 Delta R.T.: -0.007 min  
 Response: 843350175  
 Conc: 748.24 ng/ml

#10 Pentachlorophenol

R.T.: 8.294 min  
 Delta R.T.: -0.005 min  
 Response: 25792542501  
 Conc: 739.36 ng/ml

#10 Pentachlorophenol


R.T.: 9.156 min  
 Delta R.T.: -0.007 min  
 Response: 16172585032  
 Conc: 794.92 ng/ml

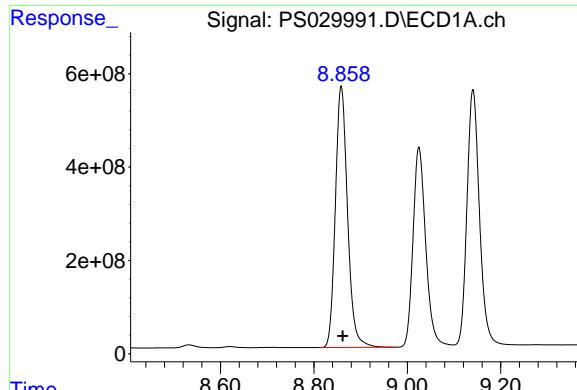

#11 2,4,5-TP (SILVEX)


R.T.: 8.858 min  
 Delta R.T.: -0.004 min  
 Response: 10127462888  
 Conc: 730.55 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

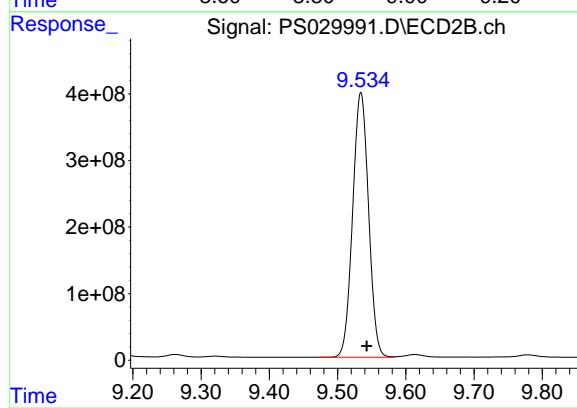


#11 2,4,5-TP (SILVEX)

R.T.: 9.534 min  
 Delta R.T.: -0.008 min  
 Response: 6432945338  
 Conc: 786.26 ng/ml

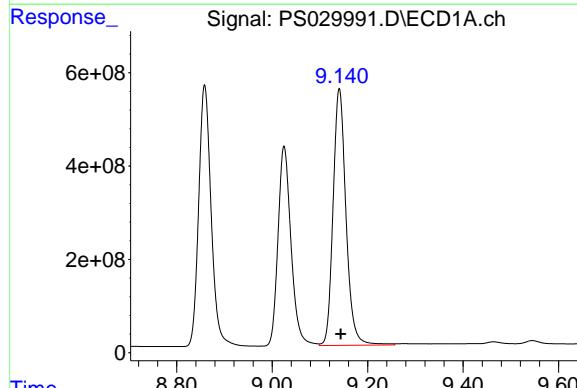


#12 2,4,5-T

R.T.: 9.141 min  
 Delta R.T.: -0.003 min  
 Response: 10350875514  
 Conc: 736.55 ng/ml

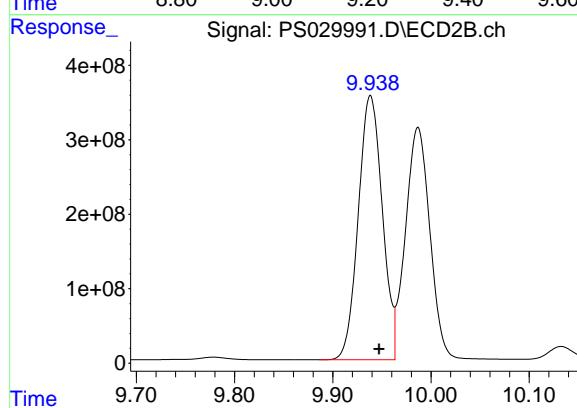

#12 2,4,5-T

R.T.: 9.938 min  
 Delta R.T.: -0.009 min  
 Response: 6030280570  
 Conc: 776.84 ng/ml

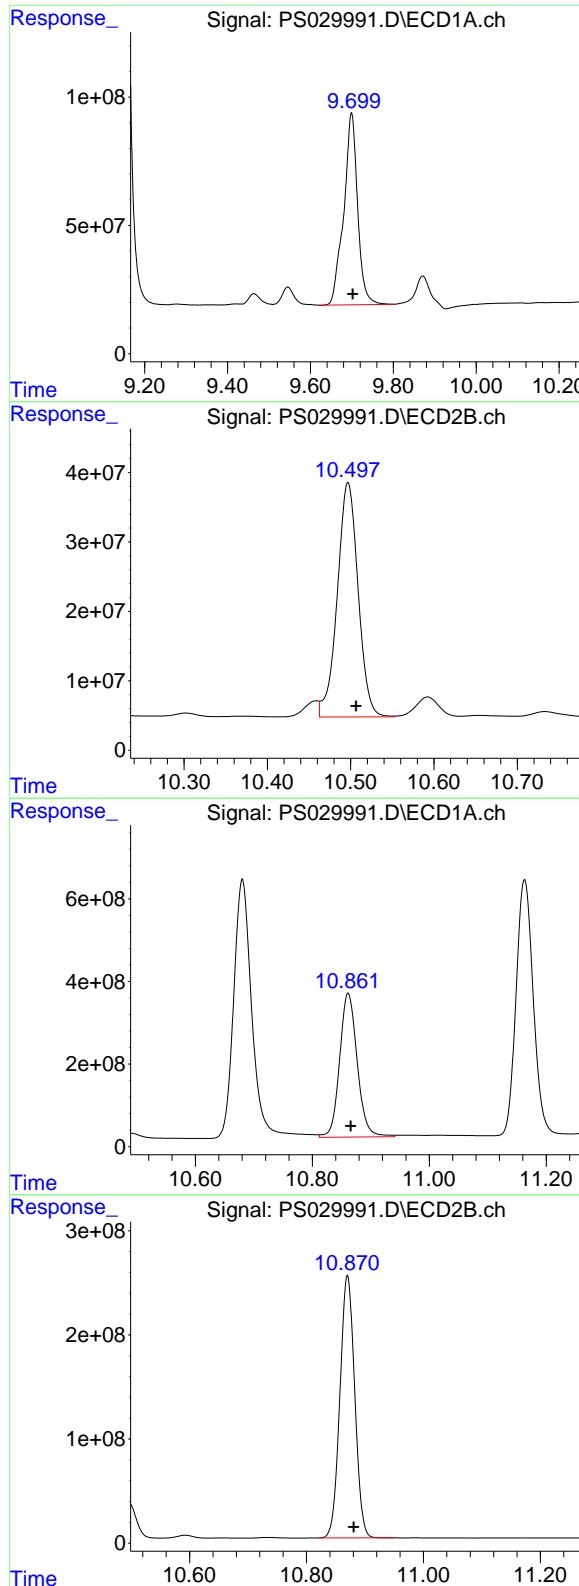

#13 2,4-DB

R.T.: 9.699 min  
 Delta R.T.: -0.003 min  
 Response: 1746342018  
 Conc: 764.14 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#13 2,4-DB


R.T.: 10.497 min  
 Delta R.T.: -0.010 min  
 Response: 586947234  
 Conc: 729.27 ng/ml

#14 DINOSEB

R.T.: 10.861 min  
 Delta R.T.: -0.005 min  
 Response: 7271944355  
 Conc: 714.80 ng/ml

#14 DINOSEB

R.T.: 10.870 min  
 Delta R.T.: -0.011 min  
 Response: 4421665636  
 Conc: 758.31 ng/ml

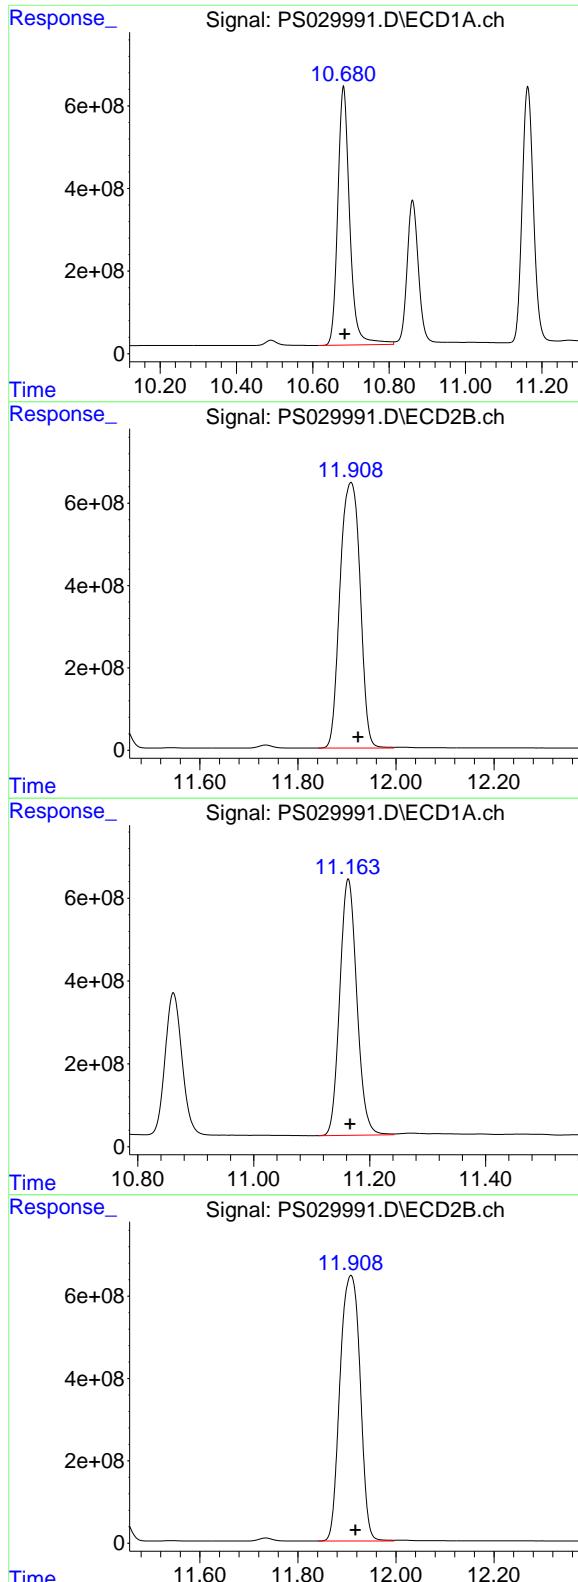

#15 Picloram

R.T.: 10.680 min  
 Delta R.T.: -0.003 min  
 Response: 13551620682  
 Conc: 739.29 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#15 Picloram

R.T.: 11.908 min  
 Delta R.T.: -0.015 min  
 Response: 18335929223  
 Conc: 1492.71 ng/ml

#16 DCPA

R.T.: 11.163 min  
 Delta R.T.: -0.003 min  
 Response: 12619577763  
 Conc: 741.41 ng/ml

#16 DCPA

R.T.: 11.908 min  
 Delta R.T.: -0.009 min  
 Response: 18335929223  
 Conc: 1626.73 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS029999.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 04:34  
 Operator : AR\AJ  
 Sample : Q1906-05MS  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**WC-5MS**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 01 04:56:31 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.919 7.462 2352.7E6 1067.4E6 955.960 1515.125 #

Target Compounds

1) T	Dalapon	2.442	2.515	2778.7E6	1703.5E6	678.528	981.208 #
2) T	3,5-DICHL...	6.143	6.459	1011.1E6	276.7E6	282.908	283.063
3) T	4-Nitroph...	6.705	7.033	108.8E6	299.8E6	60.990	391.398 #
5) T	DICAMBA	7.115	7.647	2969.9E6	1301.2E6	299.901	329.411
6) T	MCPP	7.292	7.739	169.1E6	167.6E6	26.245	95.838 #
7) T	MCPA	7.434	7.981	275.9E6	85484678	31.237	36.133
8) T	DICHLORPROP	7.796	8.341	864.6E6	340.2E6	341.197	338.858
9) T	2,4-D	8.015	8.654	1168.3E6	453.2E6	415.356	402.054
10) T	Pentachlo...	8.294	9.155	5798.7E6	3568.2E6	166.225	175.388
11) T	2,4,5-TP ...	8.858	9.534	2407.1E6	2166.3E6	173.635	264.772 #
12) T	2,4,5-T	9.140	9.938	3632.2E6	2158.8E6	258.462	278.109
13) T	2,4-DB	9.700	10.495	428.5E6	244.5E6	187.506	303.752 #
15) T	Picloram	10.680	11.901	5787.6E6	9016.2E6	315.734	734.001 #
16) T	DCPA	11.163	11.901	6544.8E6	9016.2E6	384.512	799.901 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS029999.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 04:34  
 Operator : AR\AJ  
 Sample : Q1906-05MS  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 WC-5MS

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 01 04:56:31 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

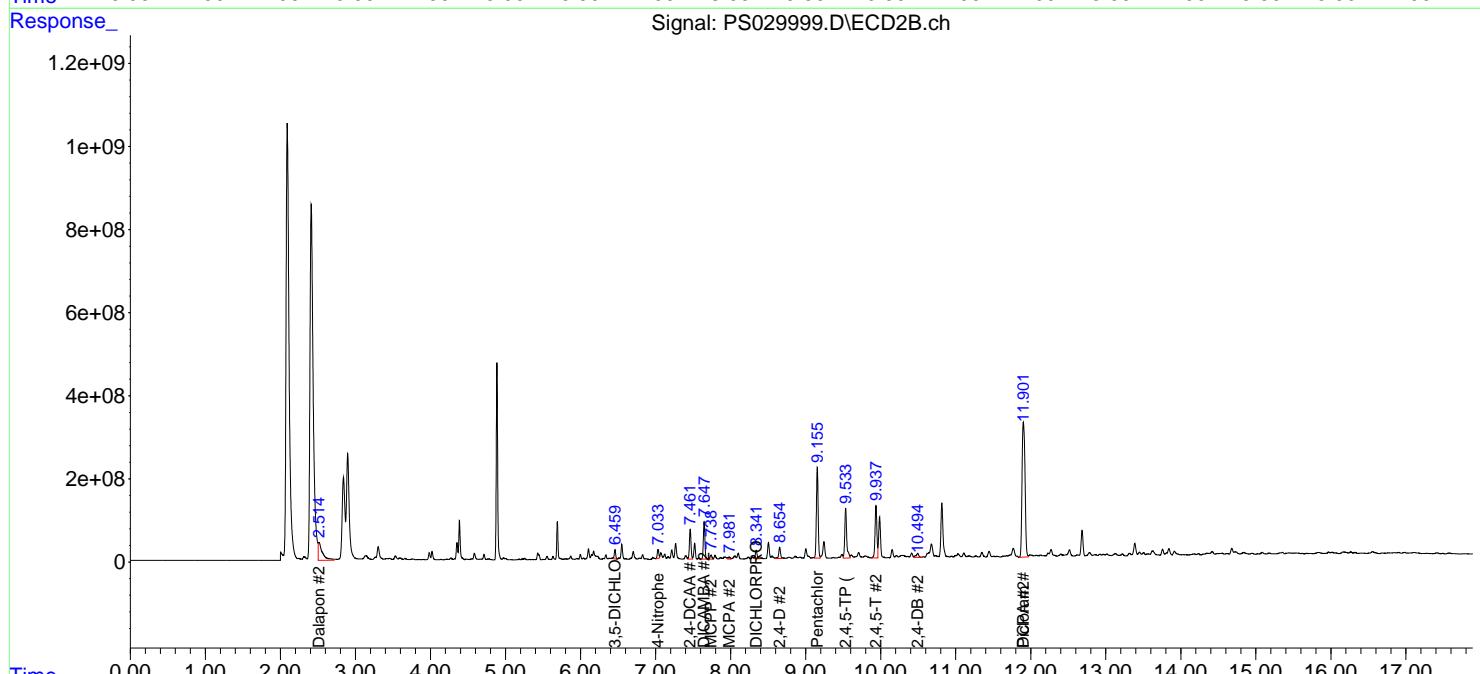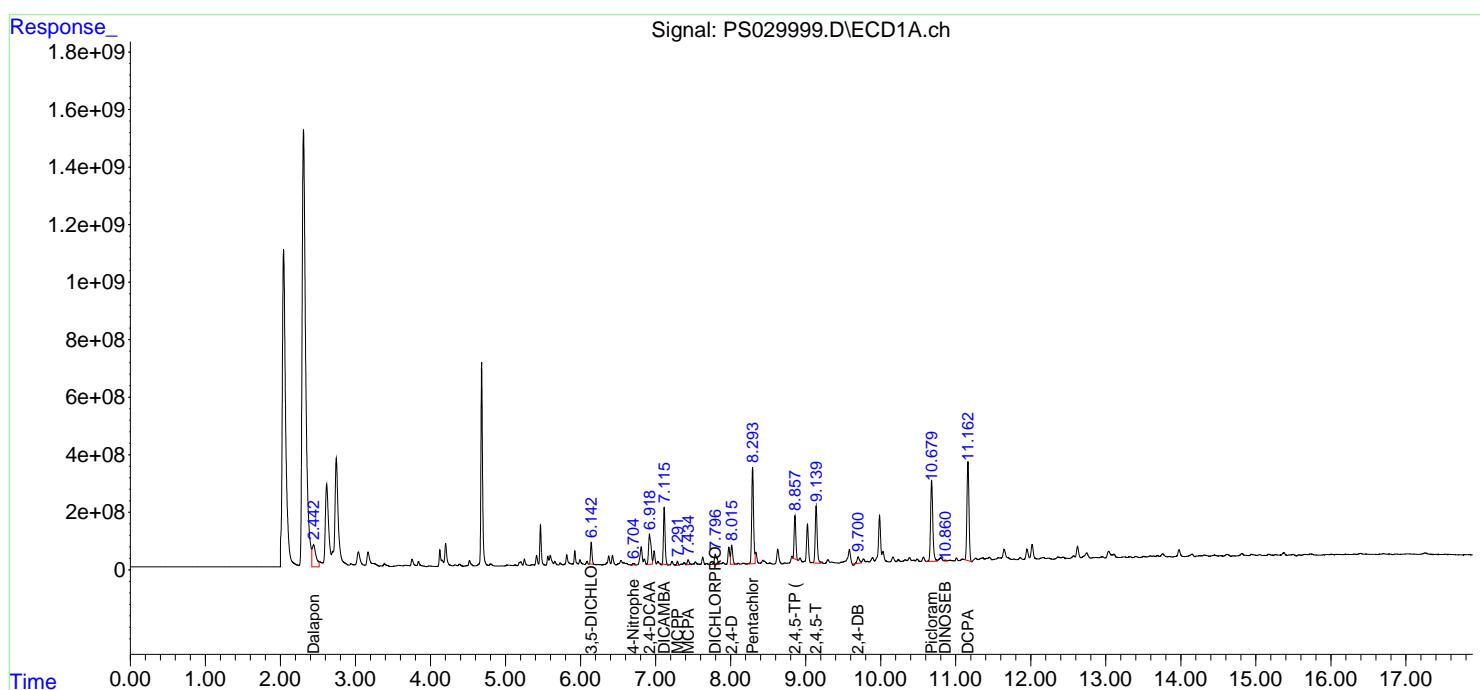

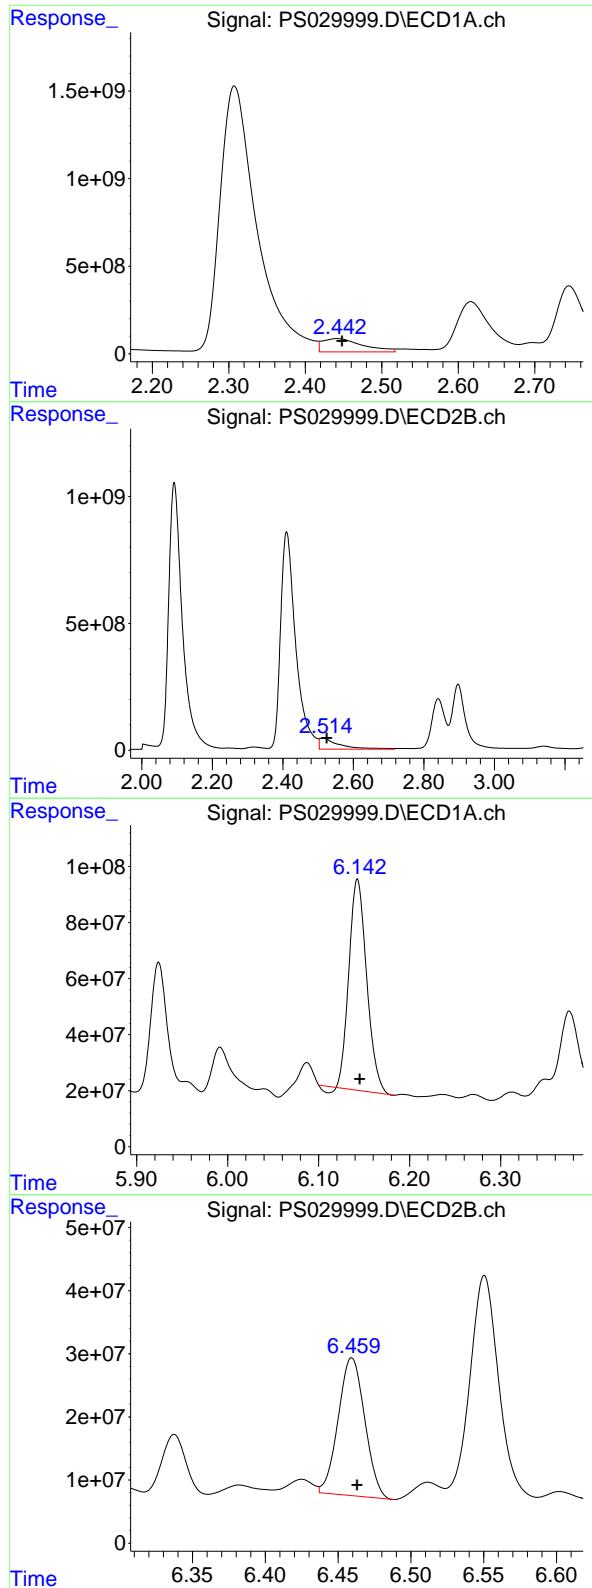

#1 Dalapon

R.T.: 2.442 min  
 Delta R.T.: -0.006 min  
 Response: 2778749021  
 Conc: 678.53 ng/ml

Instrument: ECD\_S  
 ClientSampleId: WC-5MS

#1 Dalapon


R.T.: 2.515 min  
 Delta R.T.: -0.010 min  
 Response: 1703518196  
 Conc: 981.21 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.143 min  
 Delta R.T.: -0.003 min  
 Response: 1011053759  
 Conc: 282.91 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.459 min  
 Delta R.T.: -0.004 min  
 Response: 276716083  
 Conc: 283.06 ng/ml

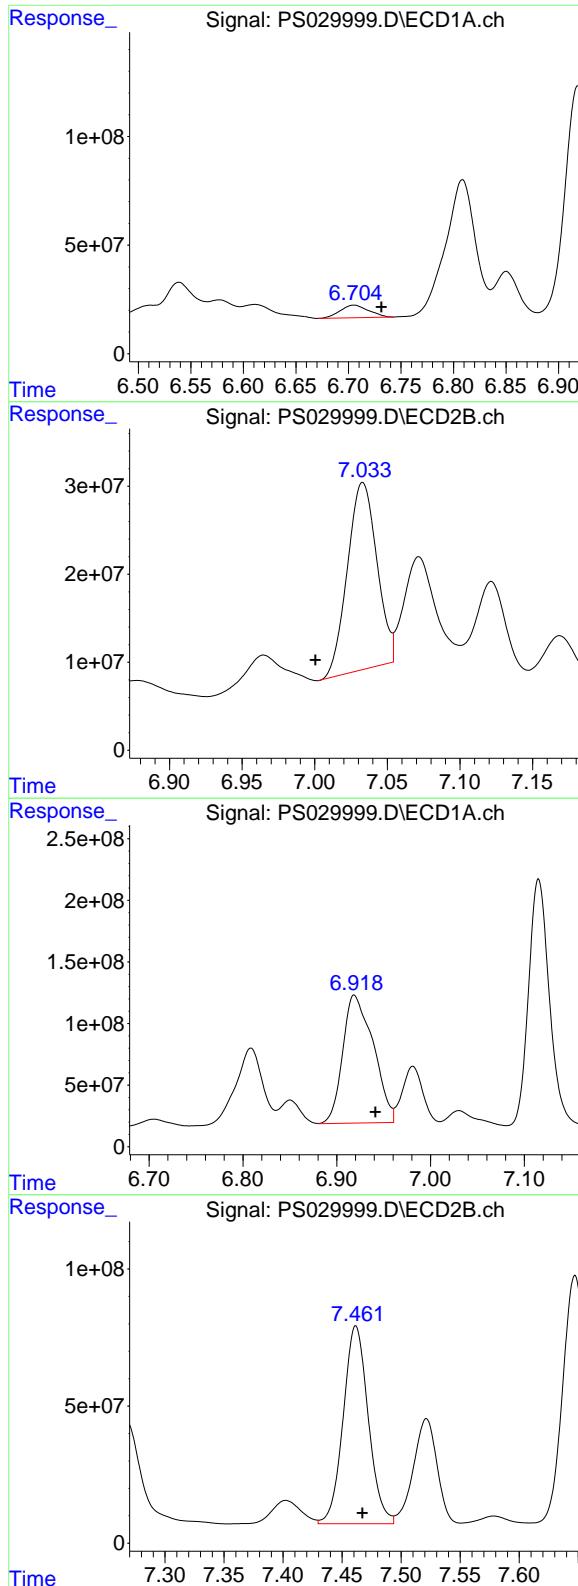

### #3 4-Nitrophenol

R.T.: 6.705 min  
Delta R.T.: -0.026 min  
Response: 108765273  
Conc: 60.99 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** WC-5MS

### #3 4-Nitrophenol


R.T.: 7.033 min  
Delta R.T.: 0.033 min  
Response: 299779817  
Conc: 391.40 ng/ml

### #4 2,4-DCAA

R.T.: 6.919 min  
Delta R.T.: -0.022 min  
Response: 2352694270  
Conc: 955.96 ng/ml

### #4 2,4-DCAA

R.T.: 7.462 min  
Delta R.T.: -0.005 min  
Response: 1067430949  
Conc: 1515.12 ng/ml

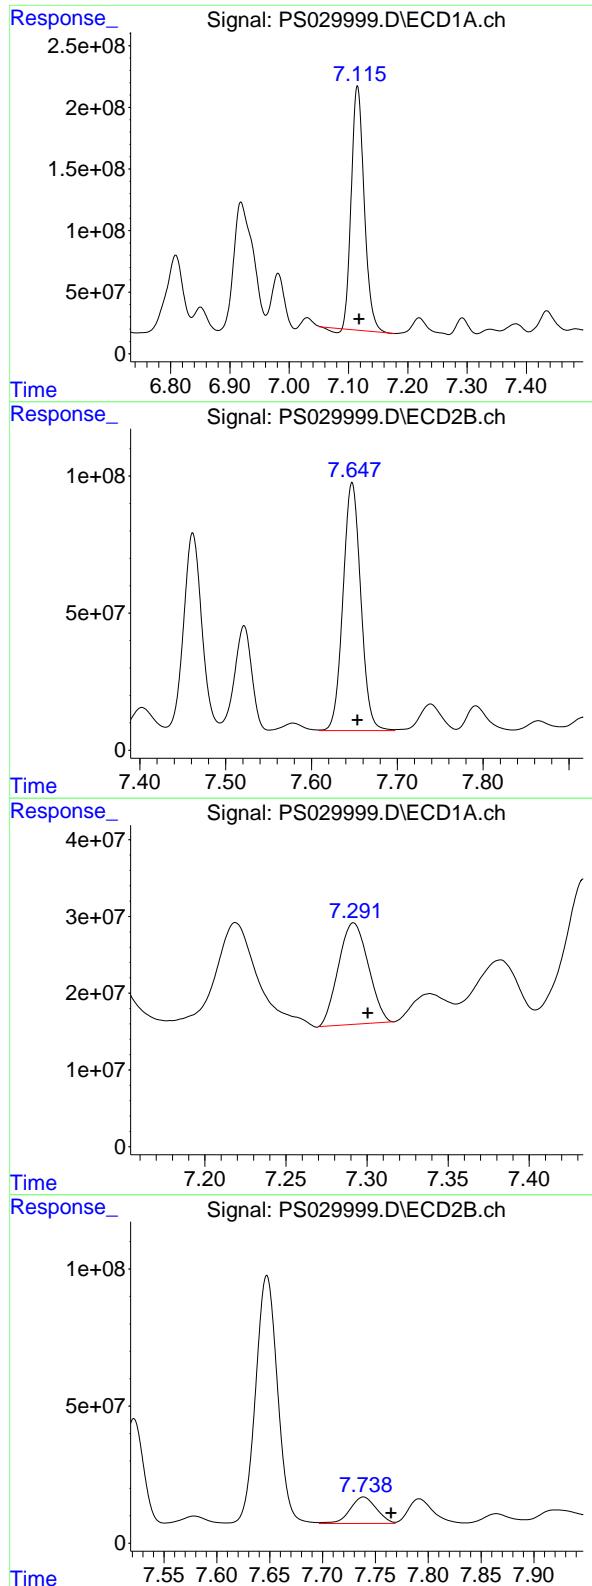

#5 DICAMBA

R.T.: 7.115 min  
 Delta R.T.: -0.003 min  
 Response: 2969877314  
 Conc: 299.90 ng/ml

Instrument: ECD\_S  
 ClientSampleId: WC-5MS

#5 DICAMBA


R.T.: 7.647 min  
 Delta R.T.: -0.006 min  
 Response: 1301192862  
 Conc: 329.41 ng/ml

#6 MCPP

R.T.: 7.292 min  
 Delta R.T.: -0.009 min  
 Response: 169114247  
 Conc: 26.25 ug/ml

#6 MCPP

R.T.: 7.739 min  
 Delta R.T.: -0.026 min  
 Response: 167616033  
 Conc: 95.84 ug/ml

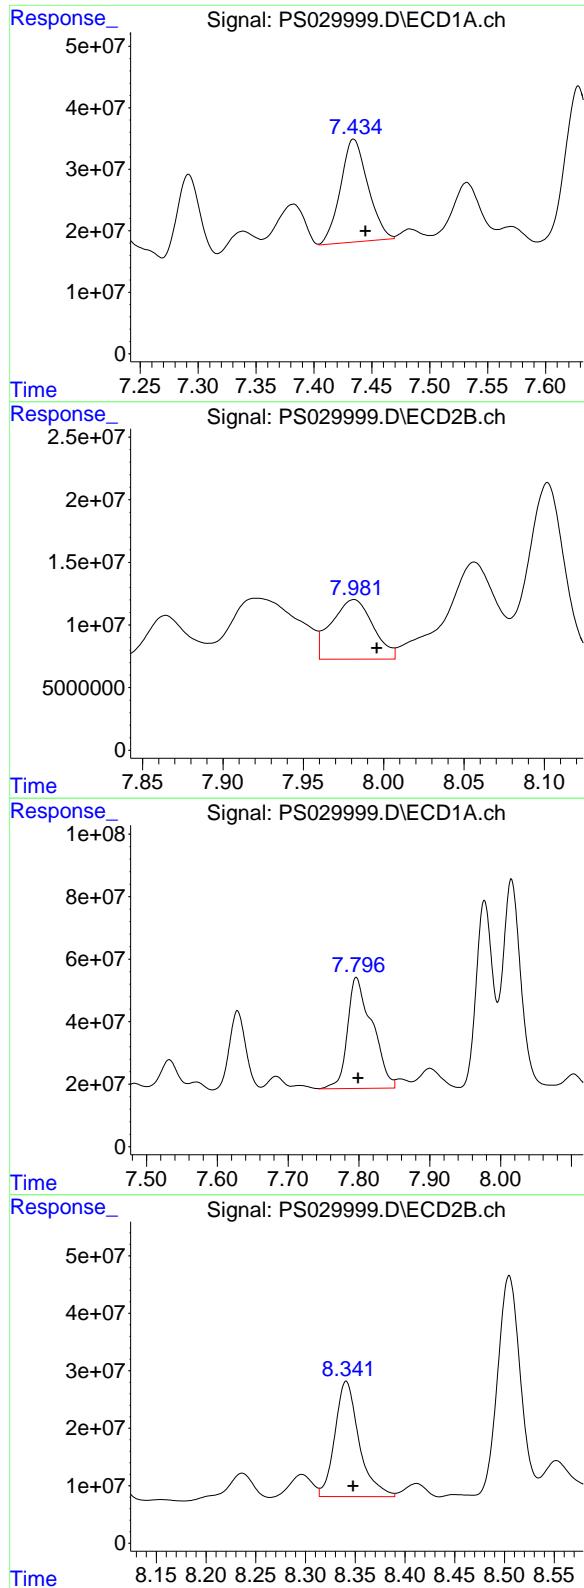

#7 MCPA

R.T.: 7.434 min  
 Delta R.T.: -0.010 min  
 Response: 275866896  
 Conc: 31.24 ug/ml

Instrument: ECD\_S  
 ClientSampleId: WC-5MS

#7 MCPA


R.T.: 7.981 min  
 Delta R.T.: -0.014 min  
 Response: 85484678  
 Conc: 36.13 ug/ml

#8 DICHLOPROP

R.T.: 7.796 min  
 Delta R.T.: -0.003 min  
 Response: 864629774  
 Conc: 341.20 ng/ml

#8 DICHLOPROP


R.T.: 8.341 min  
 Delta R.T.: -0.007 min  
 Response: 340201612  
 Conc: 338.86 ng/ml

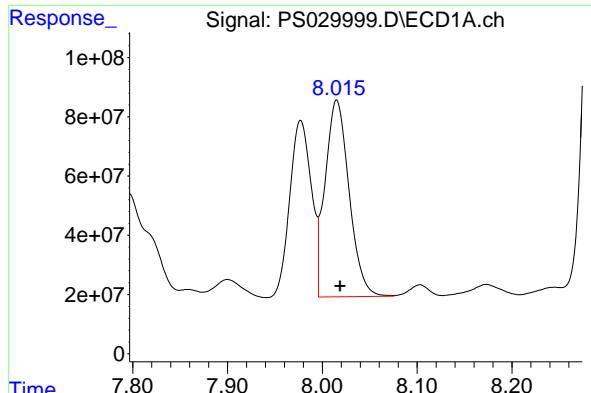

#9 2,4-D


R.T.: 8.015 min  
 Delta R.T.: -0.004 min  
 Response: 1168343085  
 Conc: 415.36 ng/ml

Instrument: ECD\_S  
 ClientSampleId: WC-5MS

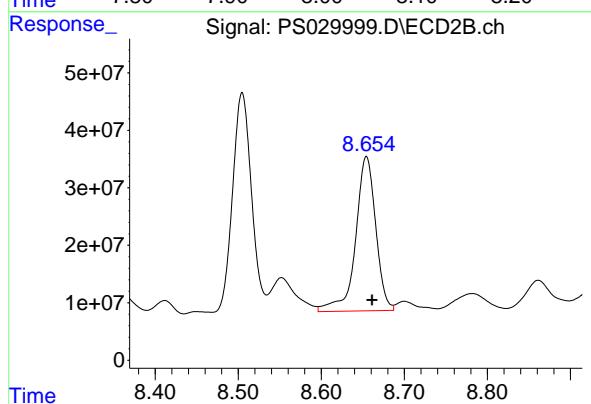


#9 2,4-D

R.T.: 8.654 min  
 Delta R.T.: -0.007 min  
 Response: 453157976  
 Conc: 402.05 ng/ml

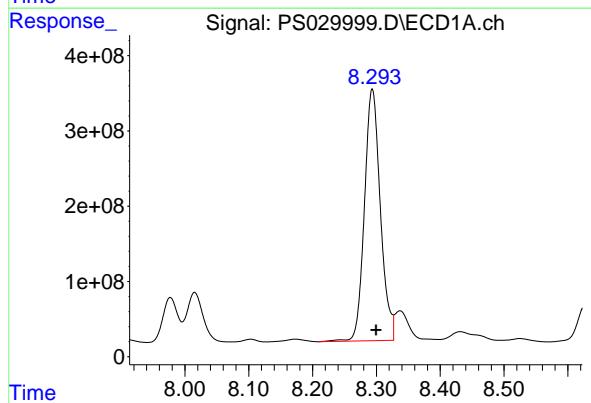


#10 Pentachlorophenol

R.T.: 8.294 min  
 Delta R.T.: -0.006 min  
 Response: 5798748268  
 Conc: 166.22 ng/ml

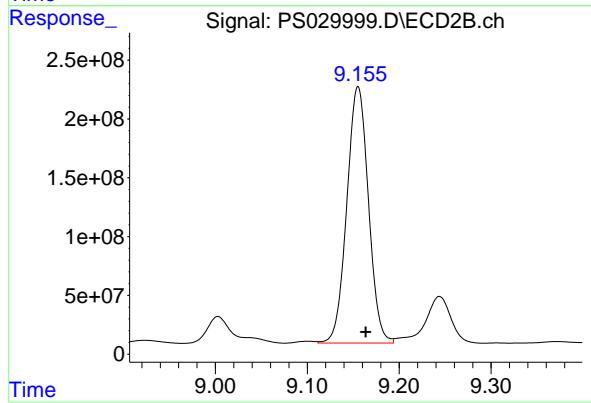

#10 Pentachlorophenol

R.T.: 9.155 min  
 Delta R.T.: -0.008 min  
 Response: 3568229586  
 Conc: 175.39 ng/ml

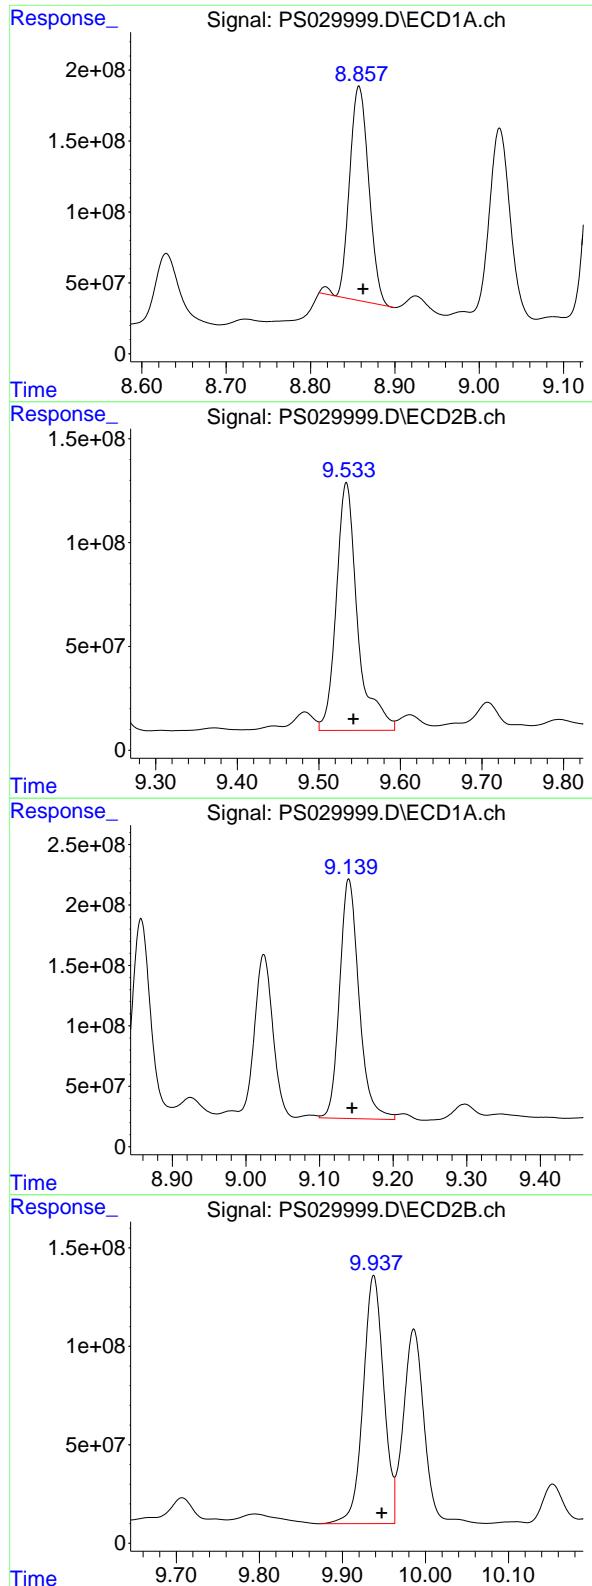

#11 2,4,5-TP (SILVEX)

R.T.: 8.858 min  
Delta R.T.: -0.005 min  
Instrument: ECD\_S  
Response: 2407072323  
Conc: 173.63 ng/ml ClientSampleId : WC-5MS

#11 2,4,5-TP (SILVEX)


R.T.: 9.534 min  
Delta R.T.: -0.009 min  
Response: 2166300266  
Conc: 264.77 ng/ml

#12 2,4,5-T

R.T.: 9.140 min  
Delta R.T.: -0.004 min  
Response: 3632188453  
Conc: 258.46 ng/ml

#12 2,4,5-T

R.T.: 9.938 min  
Delta R.T.: -0.010 min  
Response: 2158849749  
Conc: 278.11 ng/ml

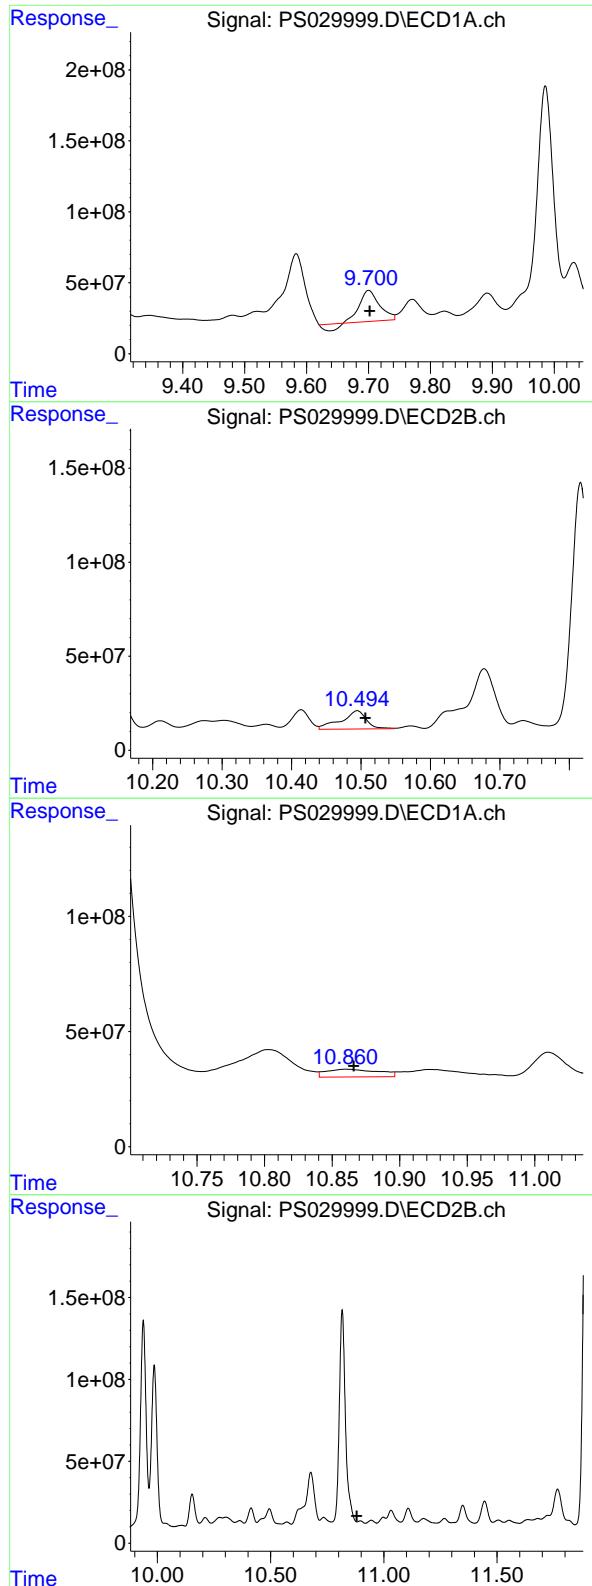

#13 2,4-DB

R.T.: 9.700 min  
 Delta R.T.: -0.002 min  
 Response: 428517754  
 Conc: 187.51 ng/ml

Instrument: ECD\_S  
 ClientSampleId: WC-5MS

#13 2,4-DB


R.T.: 10.495 min  
 Delta R.T.: -0.012 min  
 Response: 244472139  
 Conc: 303.75 ng/ml

#14 DINOSEB

R.T.: 10.861 min  
 Delta R.T.: -0.005 min  
 Response: 90083314  
 Conc: 8.85 ng/ml

#14 DINOSEB

R.T.: 10.896 min  
 Delta R.T.: 0.015 min  
 Response: -167004366  
 Conc: N.D.

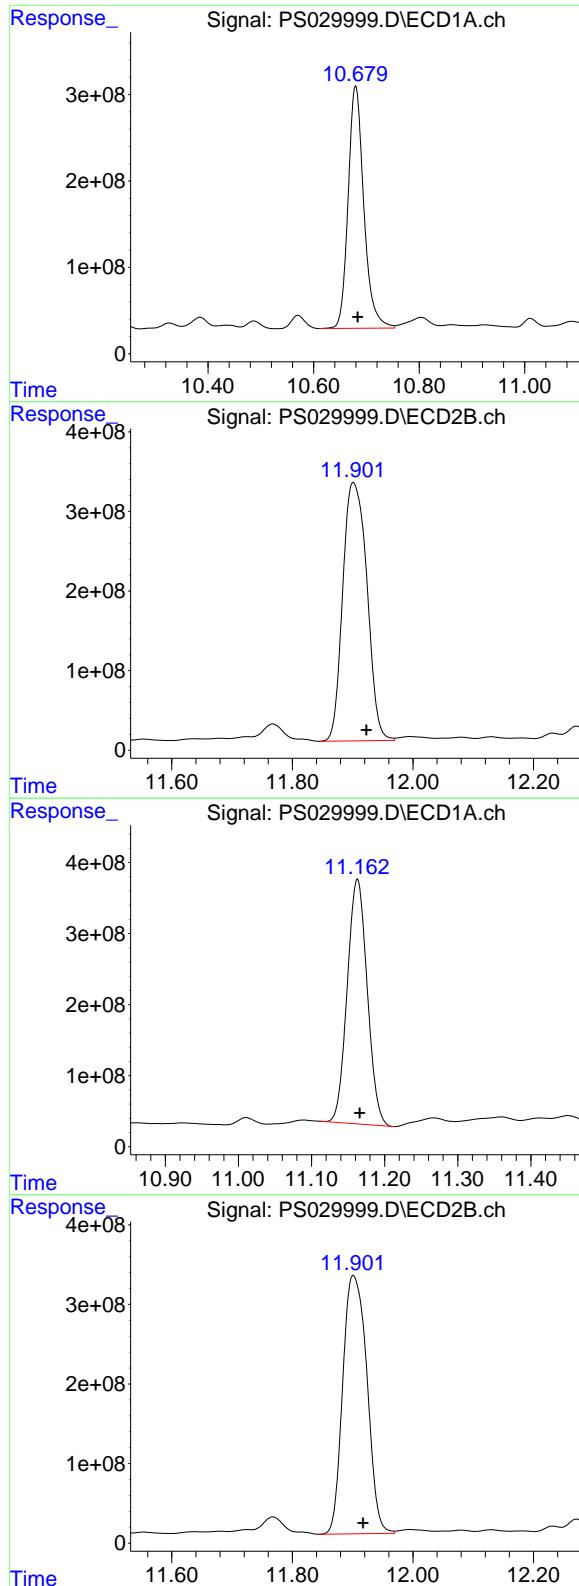

#15 Picloram

R.T.: 10.680 min  
 Delta R.T.: -0.004 min  
 Response: 5787594197  
 Conc: 315.73 ng/ml

Instrument : ECD\_S  
 ClientSampleId : WC-5MS

#15 Picloram

R.T.: 11.901 min  
 Delta R.T.: -0.022 min  
 Response: 9016205321  
 Conc: 734.00 ng/ml

#16 DCPA

R.T.: 11.163 min  
 Delta R.T.: -0.003 min  
 Response: 6544783262  
 Conc: 384.51 ng/ml

#16 DCPA

R.T.: 11.901 min  
 Delta R.T.: -0.016 min  
 Response: 9016205321  
 Conc: 799.90 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS030000.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 04:58  
 Operator : AR\AJ  
 Sample : Q1906-05MSD  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**WC-5MSD**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 01 05:15:48 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.919 7.462 2383.8E6 1086.7E6 968.580 1542.476 #

Target Compounds

1) T	Dalapon	2.443	2.516	2684.7E6	1670.2E6	655.570	962.008 #
2) T	3,5-DICHL...	6.142	6.459	1025.7E6	282.0E6	287.002	288.501
3) T	4-Nitroph...	6.705	7.033	111.4E6	303.5E6	62.467	396.248 #
5) T	DICAMBA	7.114	7.648	2999.4E6	1321.2E6	302.882	334.474
6) T	MCPP	7.292	7.738	166.7E6	168.2E6	25.863	96.144 #
7) T	MCPA	7.434	7.982	275.0E6	84049137	31.136	35.527
8) T	DICHLORPROP	7.796	8.341	878.3E6	345.5E6	346.594	344.094
9) T	2,4-D	8.015	8.654	1183.7E6	461.4E6	420.814	409.339
10) T	Pentachlo...	8.293	9.155	5829.4E6	3626.2E6	167.103	178.239
11) T	2,4,5-TP ...	8.858	9.533	2380.4E6	2214.4E6	171.708	270.656 #
12) T	2,4,5-T	9.140	9.937	3680.4E6	2208.5E6	261.892	284.499
13) T	2,4-DB	9.700	10.494	461.1E6	253.9E6	201.765	315.431 #
15) T	Picloram	10.679	11.901	5832.1E6	9209.8E6	318.161	749.763 #
16) T	DCPA	11.162	11.901	6578.7E6	9209.8E6	386.502	817.078 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS030000.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 04:58  
 Operator : AR\AJ  
 Sample : Q1906-05MSD  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 WC-5MSD

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 01 05:15:48 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

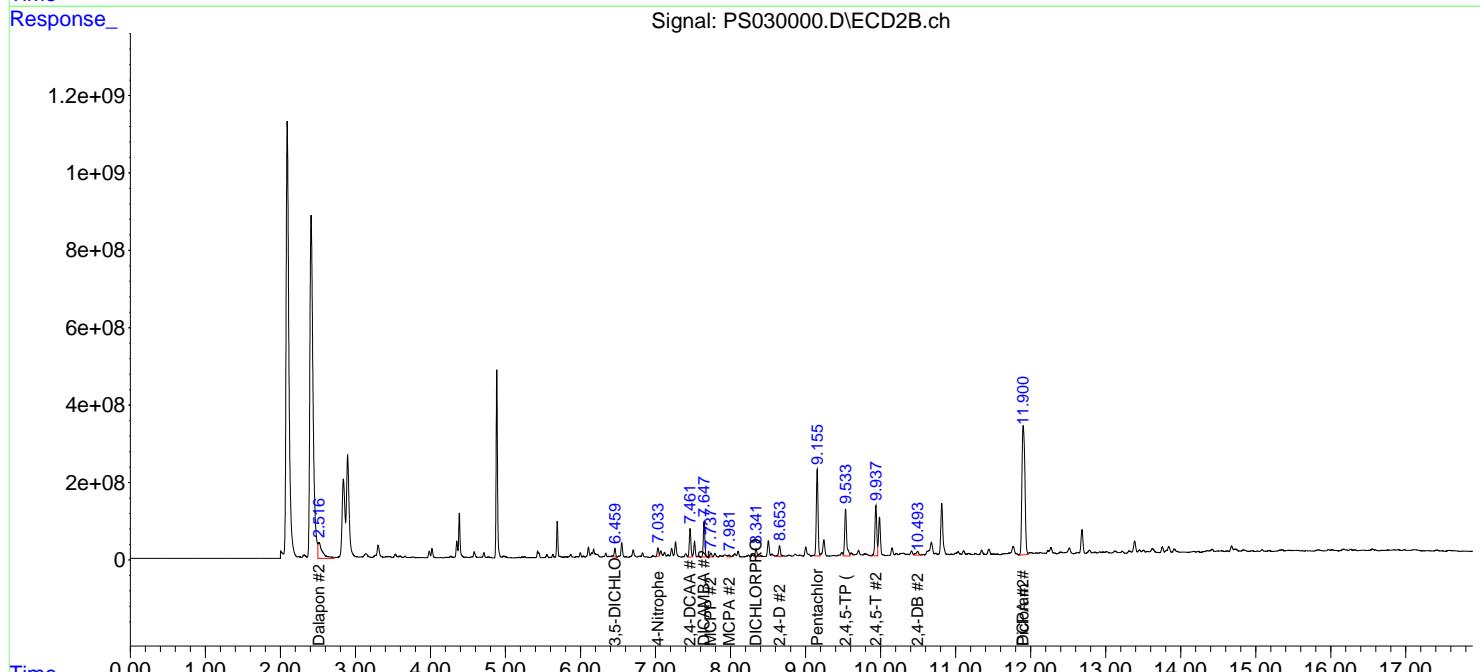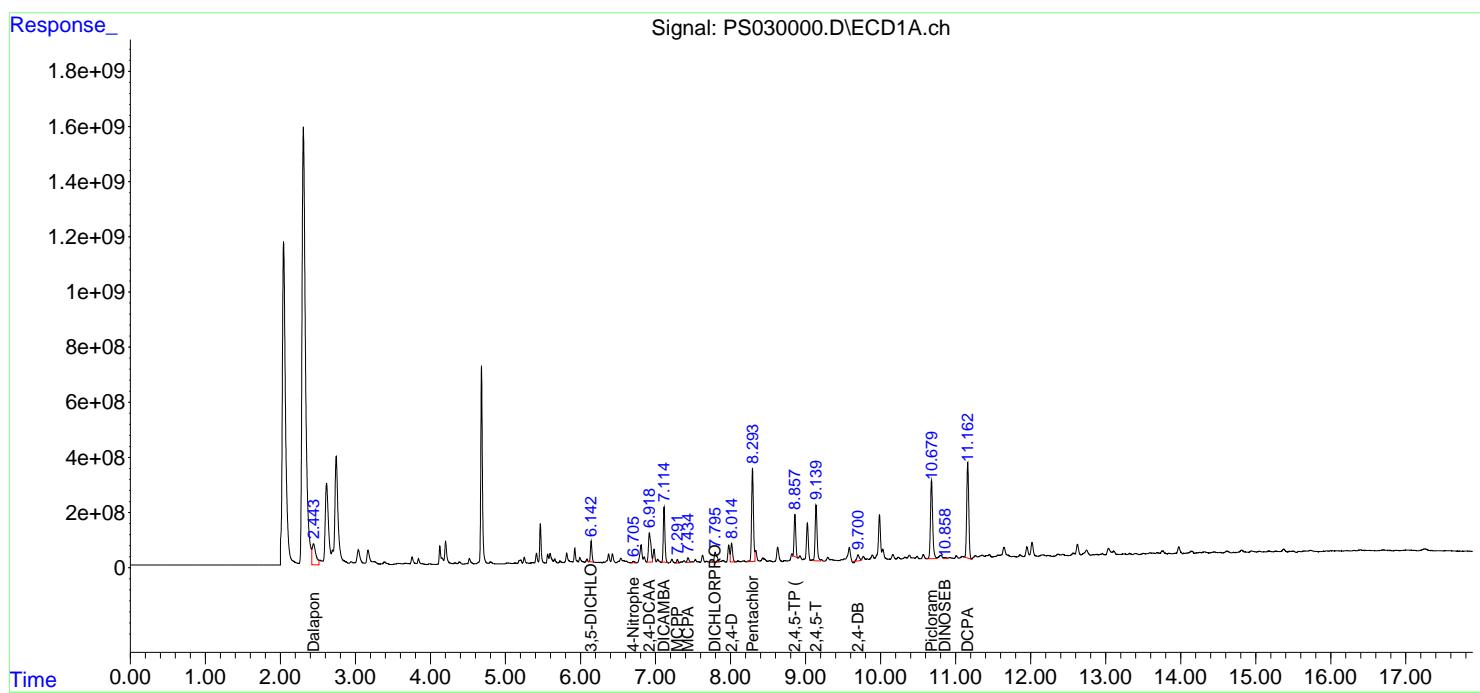

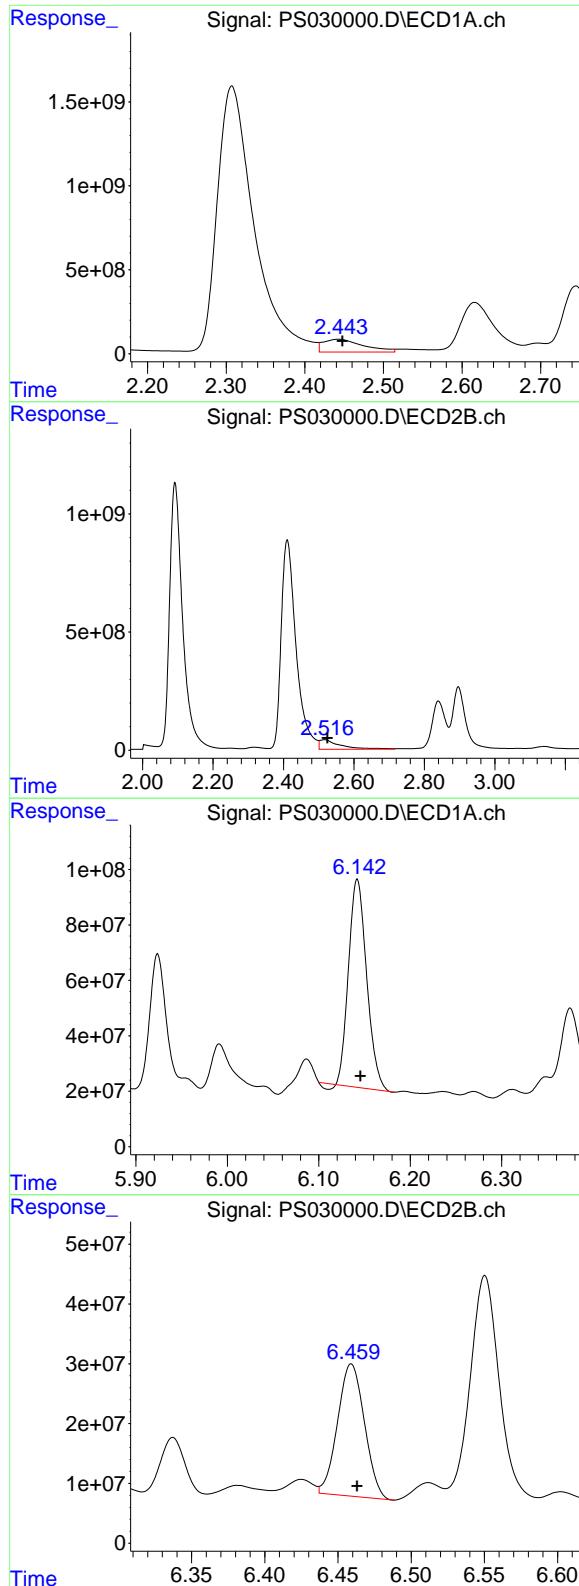

#1 Dalapon

R.T.: 2.443 min  
 Delta R.T.: -0.005 min  
 Response: 2684729749  
 Conc: 655.57 ng/ml

Instrument: ECD\_S  
 ClientSampleId: WC-5MSD

#1 Dalapon


R.T.: 2.516 min  
 Delta R.T.: -0.008 min  
 Response: 1670184214  
 Conc: 962.01 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.142 min  
 Delta R.T.: -0.003 min  
 Response: 1025682749  
 Conc: 287.00 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.459 min  
 Delta R.T.: -0.004 min  
 Response: 282032989  
 Conc: 288.50 ng/ml

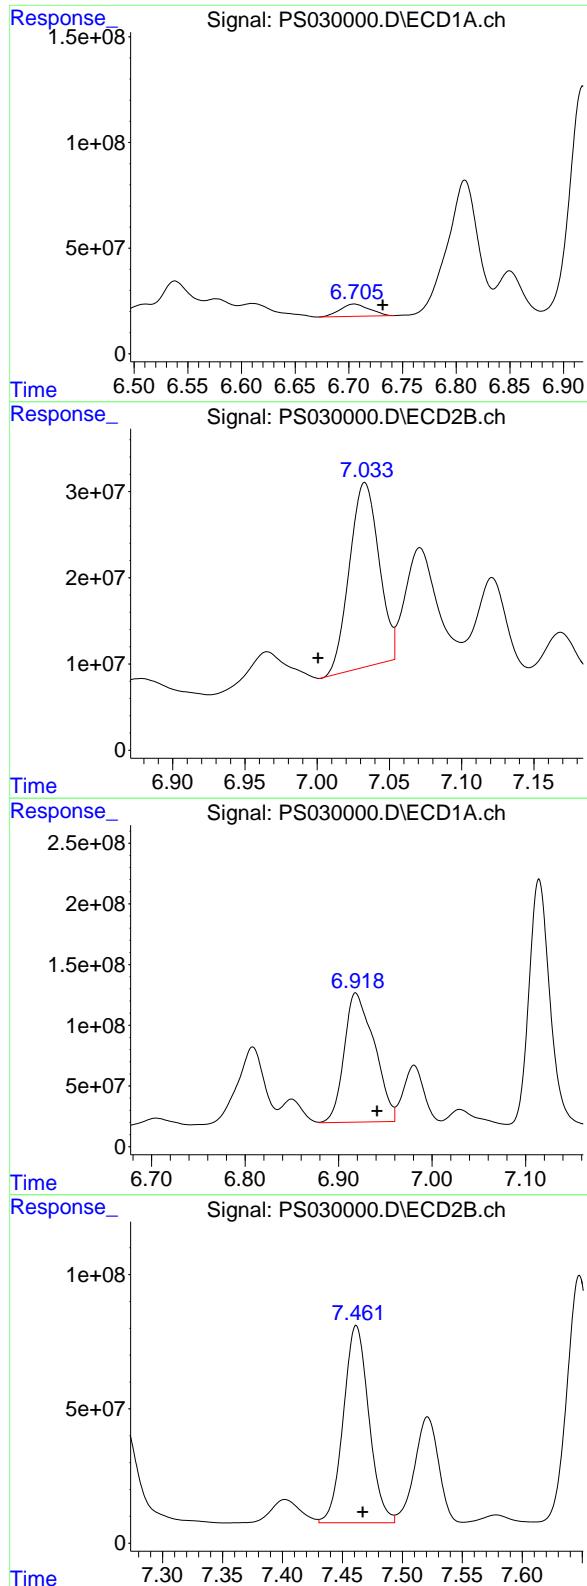

#3 4-Nitrophenol

R.T.: 6.705 min  
Delta R.T.: -0.026 min  
Response: 111398988  
Conc: 62.47 ng/ml

Instrument: ECD\_S  
ClientSampleId: WC-5MSD

#3 4-Nitrophenol


R.T.: 7.033 min  
Delta R.T.: 0.033 min  
Response: 303494987  
Conc: 396.25 ng/ml

#4 2,4-DCAA

R.T.: 6.919 min  
Delta R.T.: -0.023 min  
Response: 2383750734  
Conc: 968.58 ng/ml

#4 2,4-DCAA

R.T.: 7.462 min  
Delta R.T.: -0.005 min  
Response: 1086700629  
Conc: 1542.48 ng/ml

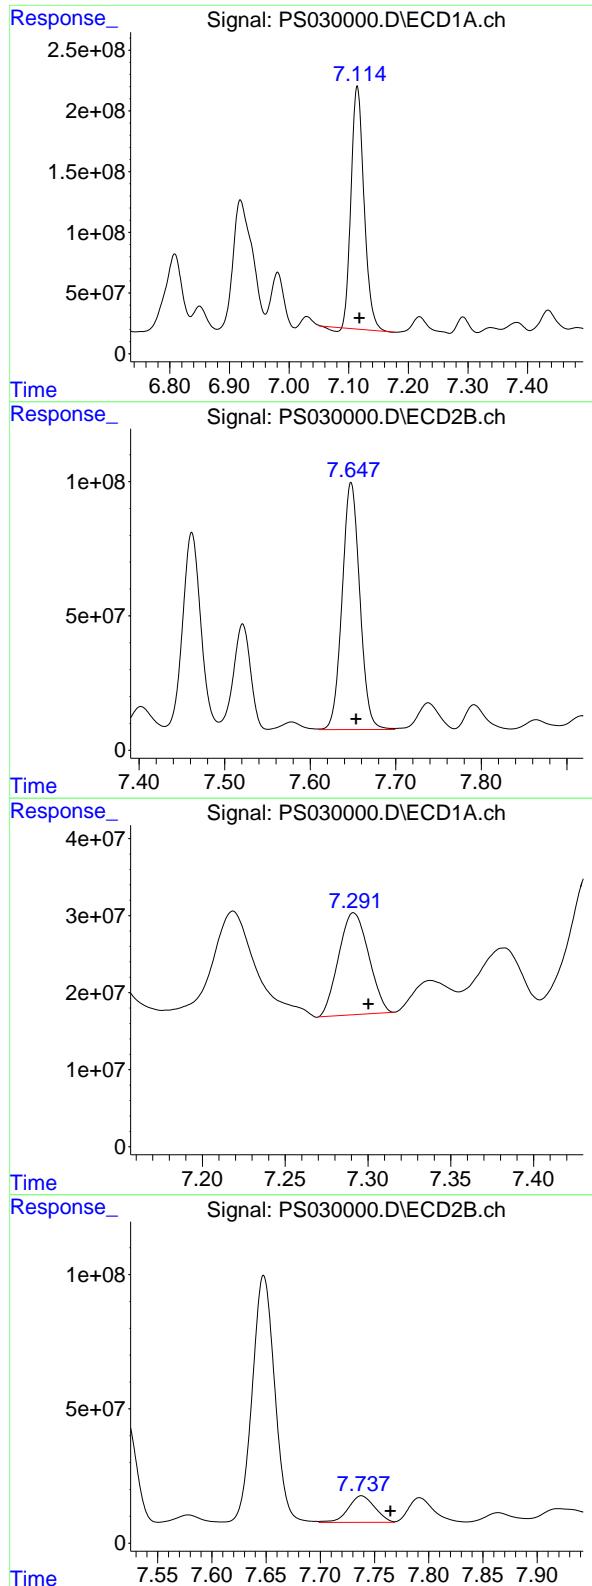

#5 DICAMBA

R.T.: 7.114 min  
 Delta R.T.: -0.003 min  
 Response: 2999399775  
 Conc: 302.88 ng/ml

Instrument: ECD\_S  
 ClientSampleId: WC-5MSD

#5 DICAMBA


R.T.: 7.648 min  
 Delta R.T.: -0.006 min  
 Response: 1321193549  
 Conc: 334.47 ng/ml

#6 MCPP

R.T.: 7.292 min  
 Delta R.T.: -0.009 min  
 Response: 166652078  
 Conc: 25.86 ug/ml

#6 MCPP

R.T.: 7.738 min  
 Delta R.T.: -0.027 min  
 Response: 168151316  
 Conc: 96.14 ug/ml

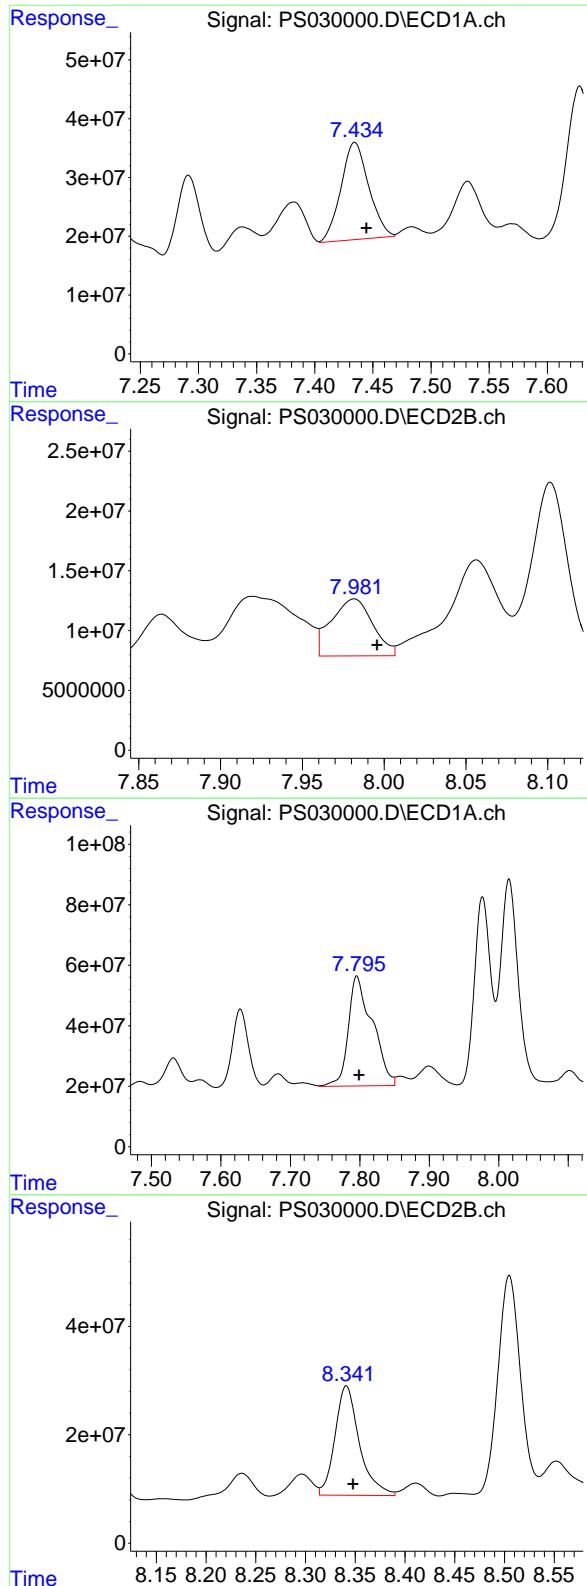

#7 MCPA

R.T.: 7.434 min  
 Delta R.T.: -0.010 min  
 Response: 274972414  
 Conc: 31.14 ug/ml

Instrument: ECD\_S  
 ClientSampleId: WC-5MSD

#7 MCPA


R.T.: 7.982 min  
 Delta R.T.: -0.014 min  
 Response: 84049137  
 Conc: 35.53 ug/ml

#8 DICHLOPROP

R.T.: 7.796 min  
 Delta R.T.: -0.003 min  
 Response: 878307532  
 Conc: 346.59 ng/ml

#8 DICHLOPROP

R.T.: 8.341 min  
 Delta R.T.: -0.007 min  
 Response: 345457932  
 Conc: 344.09 ng/ml

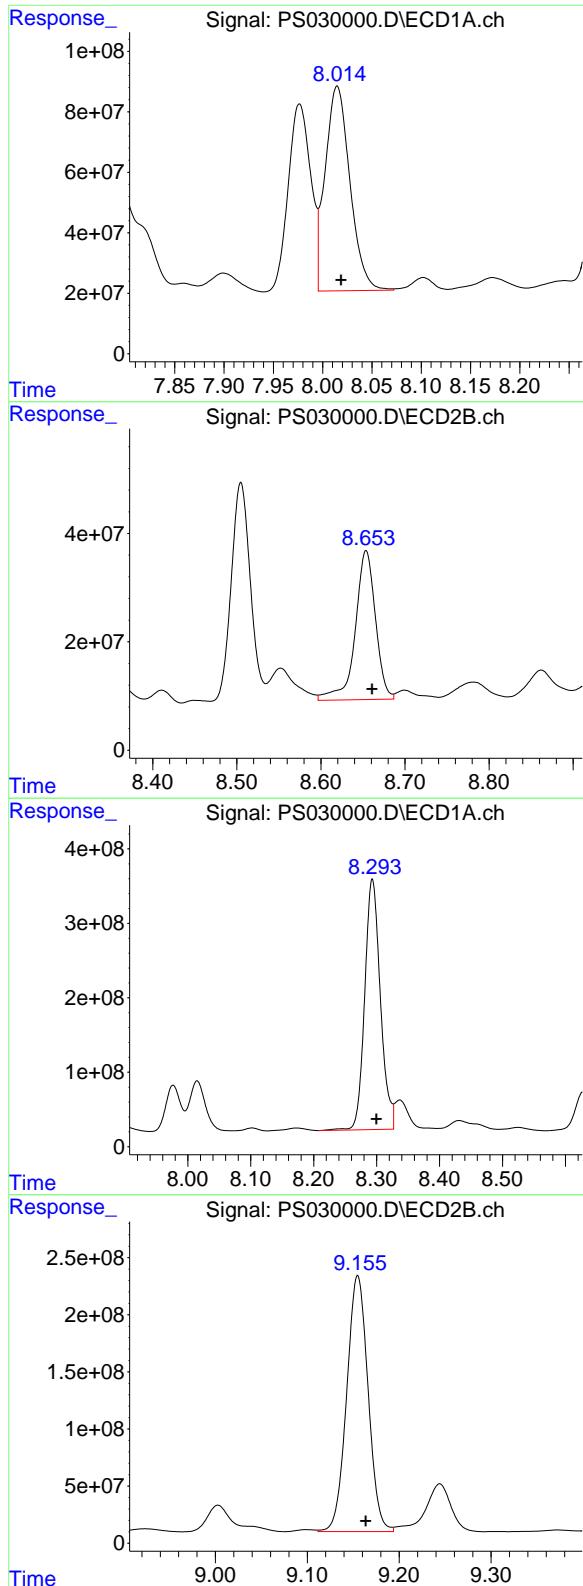

#9 2,4-D

R.T.: 8.015 min  
Delta R.T.: -0.004 min  
Response: 1183696641  
Conc: 420.81 ng/ml

Instrument: ECD\_S  
ClientSampleId: WC-5MSD

#9 2,4-D


R.T.: 8.654 min  
Delta R.T.: -0.007 min  
Response: 461368615  
Conc: 409.34 ng/ml

#10 Pentachlorophenol

R.T.: 8.293 min  
Delta R.T.: -0.006 min  
Response: 5829372536  
Conc: 167.10 ng/ml

#10 Pentachlorophenol

R.T.: 9.155 min  
Delta R.T.: -0.009 min  
Response: 3626233908  
Conc: 178.24 ng/ml

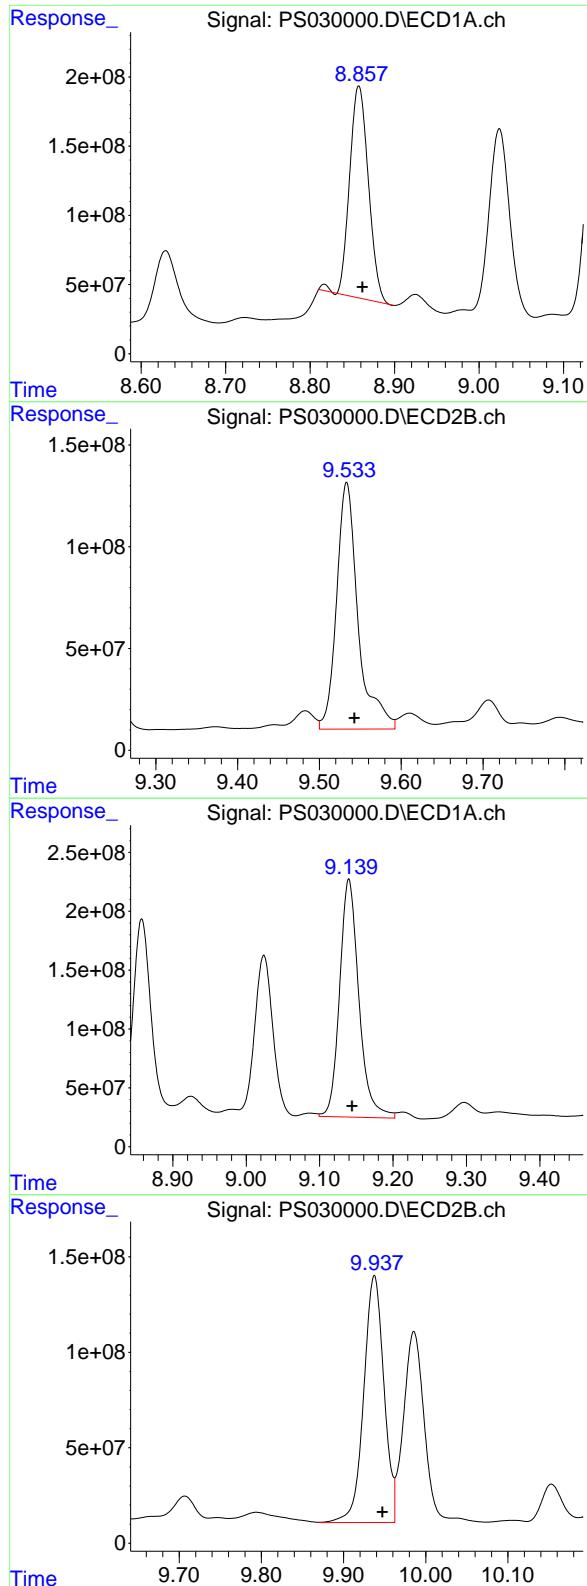

#11 2,4,5-TP (SILVEX)

R.T.: 8.858 min  
 Delta R.T.: -0.004 min  
 Response: 2380360363  
 Conc: 171.71 ng/ml

Instrument: ECD\_S  
 ClientSampleId: WC-5MSD

#11 2,4,5-TP (SILVEX)


R.T.: 9.533 min  
 Delta R.T.: -0.009 min  
 Response: 2214437332  
 Conc: 270.66 ng/ml

#12 2,4,5-T

R.T.: 9.140 min  
 Delta R.T.: -0.004 min  
 Response: 3680396485  
 Conc: 261.89 ng/ml

#12 2,4,5-T

R.T.: 9.937 min  
 Delta R.T.: -0.010 min  
 Response: 2208455612  
 Conc: 284.50 ng/ml

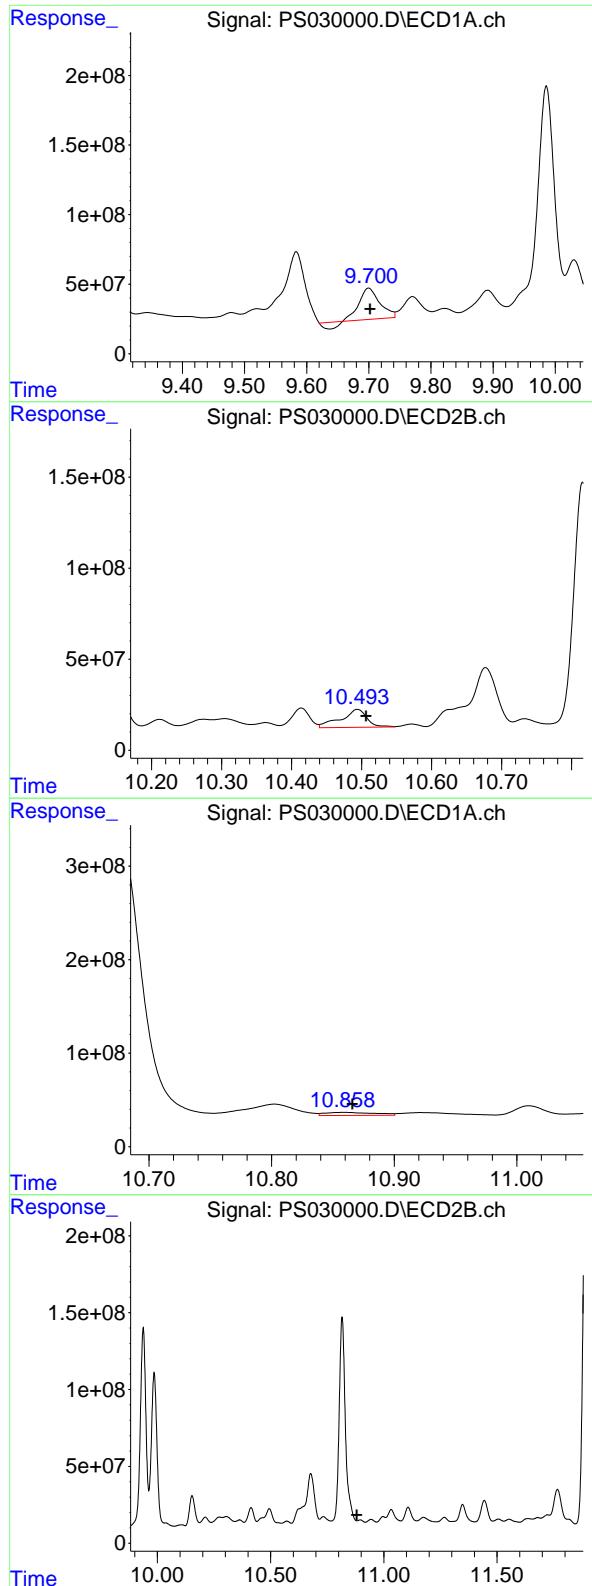

#13 2,4-DB

R.T.: 9.700 min  
 Delta R.T.: -0.002 min  
 Response: 461103799  
 Conc: 201.76 ng/ml

Instrument: ECD\_S  
 ClientSampleId: WC-5MSD

#13 2,4-DB


R.T.: 10.494 min  
 Delta R.T.: -0.012 min  
 Response: 253872450  
 Conc: 315.43 ng/ml

#14 DINOSEB

R.T.: 10.859 min  
 Delta R.T.: -0.007 min  
 Response: 92940543  
 Conc: 9.14 ng/ml

#14 DINOSEB

R.T.: 10.896 min  
 Delta R.T.: 0.015 min  
 Response: -158669769  
 Conc: N.D.

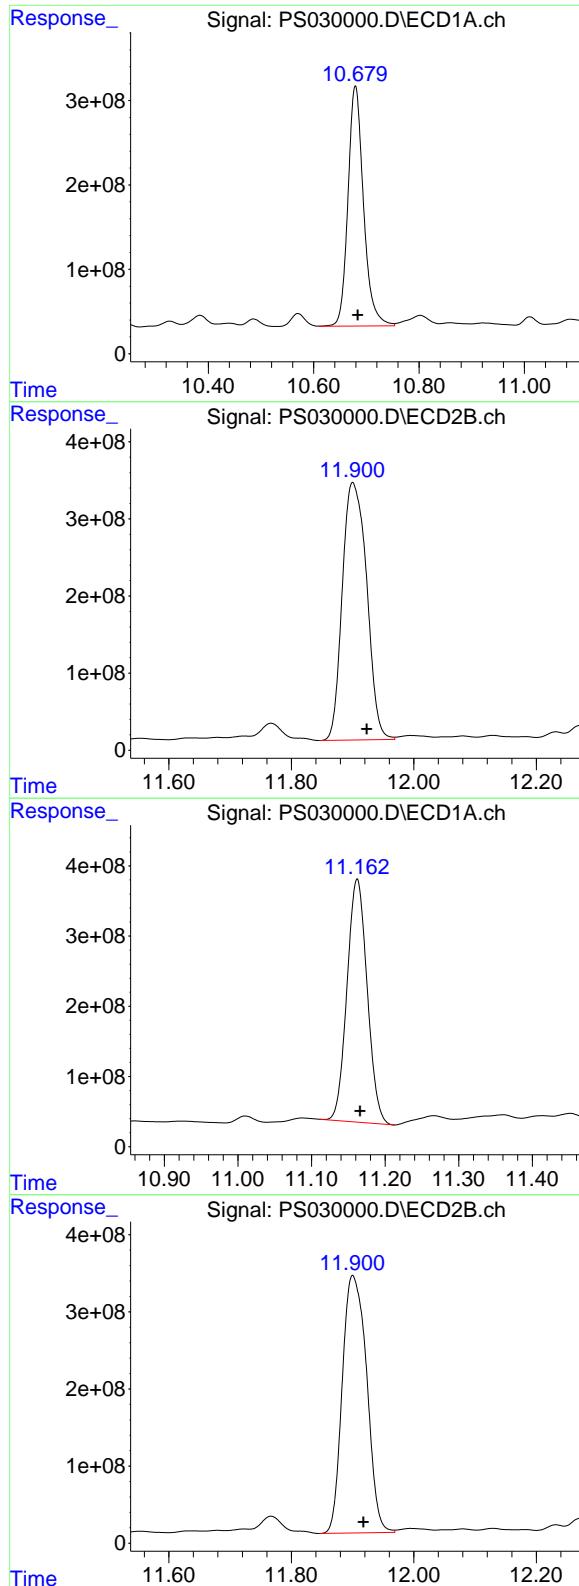

#15 Picloram

R.T.: 10.679 min  
 Delta R.T.: -0.004 min  
 Response: 5832090919  
 Conc: 318.16 ng/ml

Instrument: ECD\_S  
 ClientSampleId: WC-5MSD

#15 Picloram

R.T.: 11.901 min  
 Delta R.T.: -0.022 min  
 Response: 9209822883  
 Conc: 749.76 ng/ml

#16 DCPA

R.T.: 11.162 min  
 Delta R.T.: -0.004 min  
 Response: 6578656178  
 Conc: 386.50 ng/ml

#16 DCPA

R.T.: 11.901 min  
 Delta R.T.: -0.017 min  
 Response: 9209822883  
 Conc: 817.08 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS030002.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 06:59  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**HSTDCCC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 07 06:53:54 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.939 7.462 1810.3E6 559.5E6 735.571 794.137

Target Compounds

1) T	Dalapon	2.449	2.523	2775.4E6	1208.6E6	677.707	696.158
2) T	3,5-DICHL...	6.143	6.459	2465.8E6	721.5E6	689.978	738.090
3) T	4-Nitroph...	6.729	6.996	1209.4E6	555.7E6	678.175	725.560
5) T	DICAMBA	7.115	7.648	6990.3E6	3084.7E6	705.883	780.916
6) T	MCPP	7.294	7.756	452.6E6	123.1E6	70.239	70.364
7) T	MCPA	7.437	7.986	612.8E6	164.2E6	69.392	69.420
8) T	DICHLORPROP	7.796	8.342	1743.1E6	763.8E6	687.852	760.753
9) T	2,4-D	8.015	8.655	1969.4E6	836.1E6	700.153	741.775
10) T	Pentachlo...	8.294	9.155	25274.2E6	16072.4E6	724.501	790.000
11) T	2,4,5-TP ...	8.858	9.534	9981.3E6	6378.1E6	720.003	779.555
12) T	2,4,5-T	9.140	9.938	10149.2E6	5979.9E6	722.205	770.353
13) T	2,4-DB	9.698	10.496	1710.1E6	595.1E6	748.265	739.381
14) T	DINOSEB	10.860	10.870	7020.8E6	4312.3E6	690.113	739.552
15) T	Picloram	10.679	11.906	13213.8E6	18061.0E6	720.858	1470.327 #
16) T	DCPA	11.162	11.906	12337.1E6	18061.0E6	724.817	1602.335 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS030002.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 06:59  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDCCC750

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 07 06:53:54 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

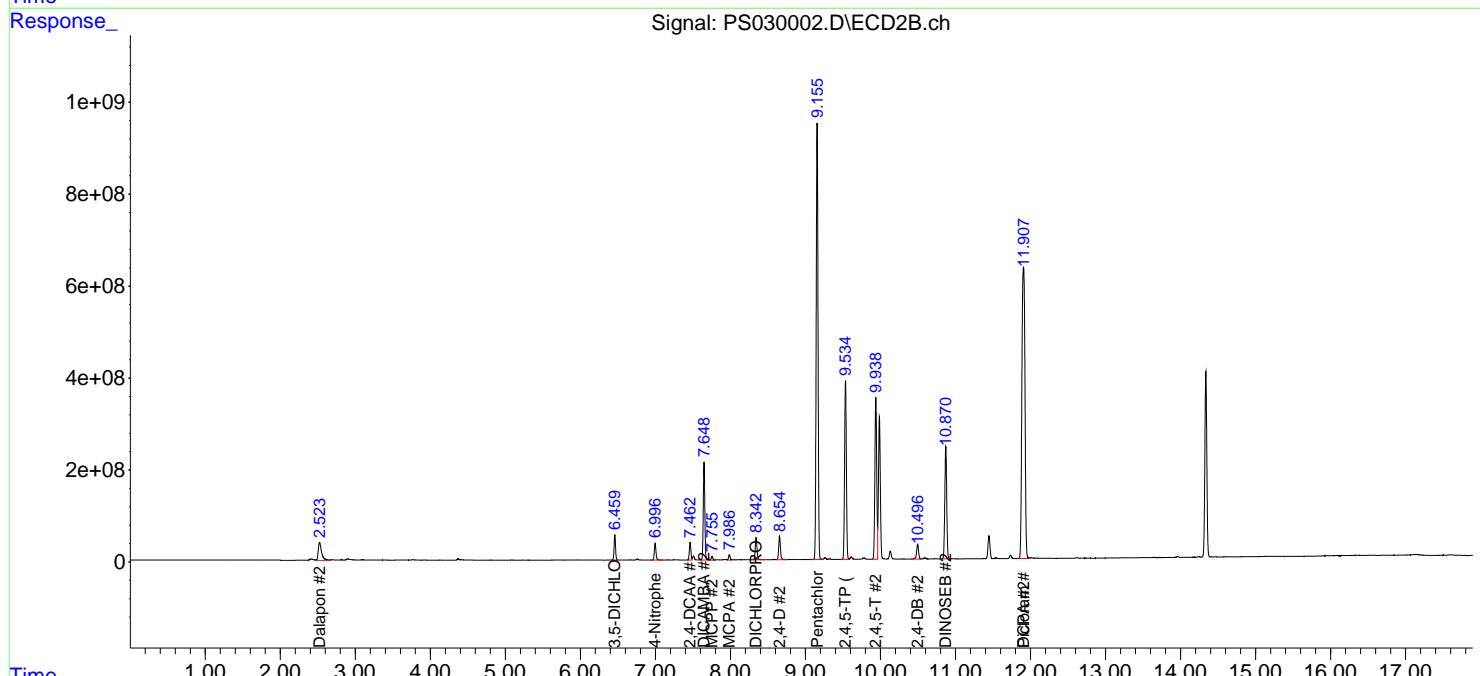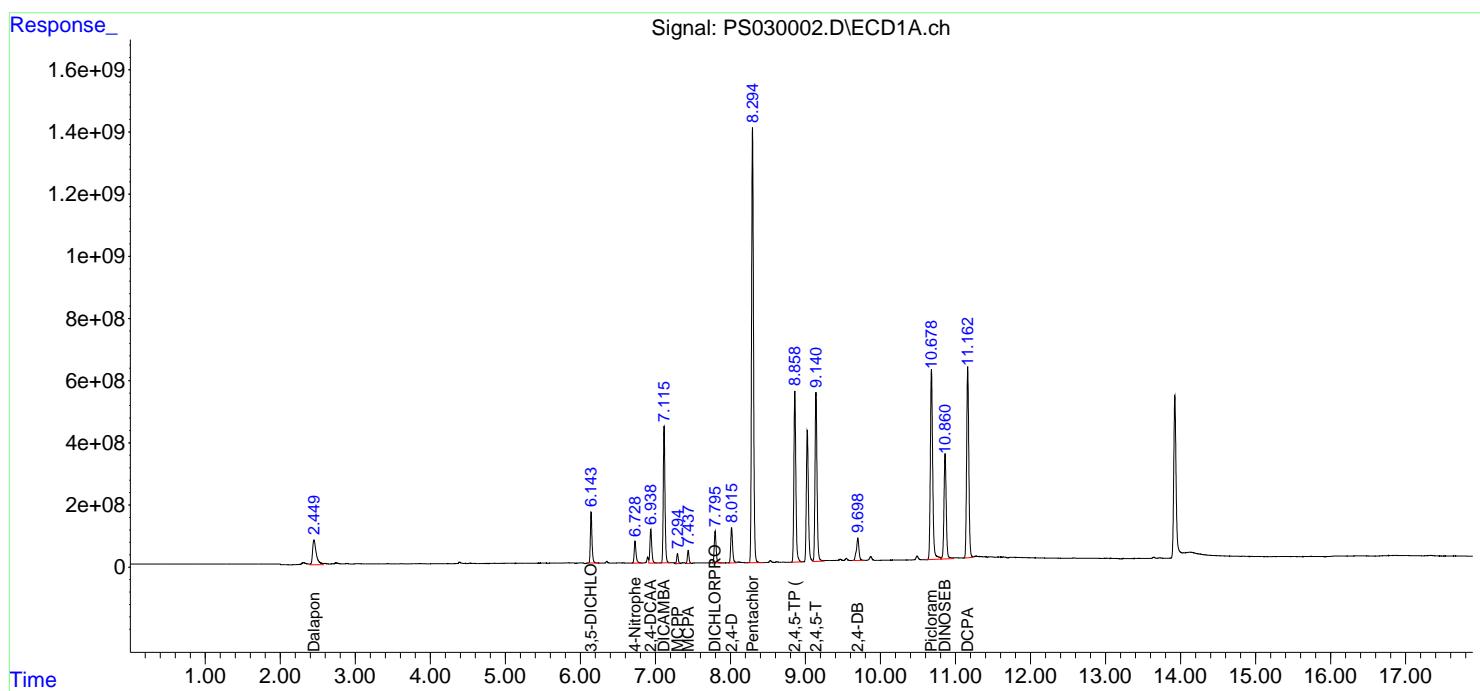

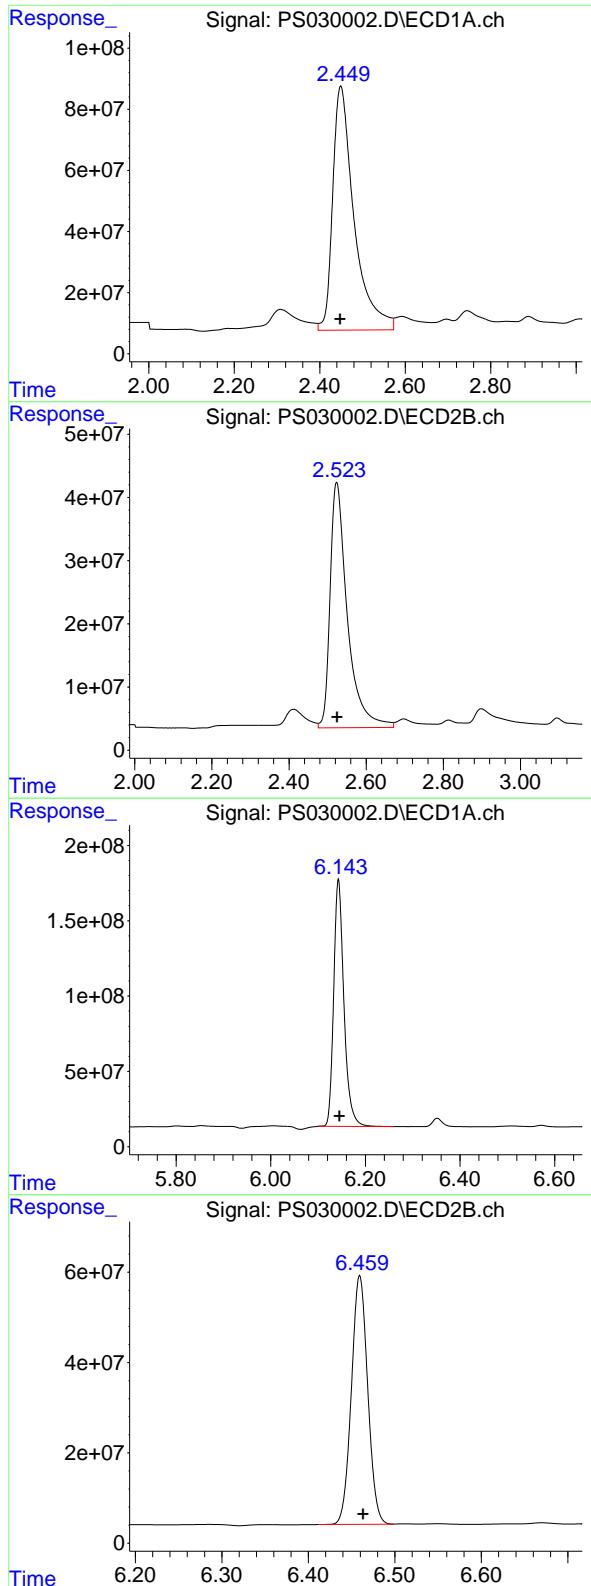

#1 Dalapon

R.T.: 2.449 min  
Delta R.T.: 0.001 min  
Response: 2775385295  
Conc: 677.71 ng/ml

Instrument: ECD\_S  
ClientSampleId: HSTDCCC750

#1 Dalapon


R.T.: 2.523 min  
Delta R.T.: 0.000 min  
Response: 1208630888  
Conc: 696.16 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.143 min  
Delta R.T.: -0.002 min  
Response: 2465834422  
Conc: 689.98 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.459 min  
Delta R.T.: -0.004 min  
Response: 721541539  
Conc: 738.09 ng/ml

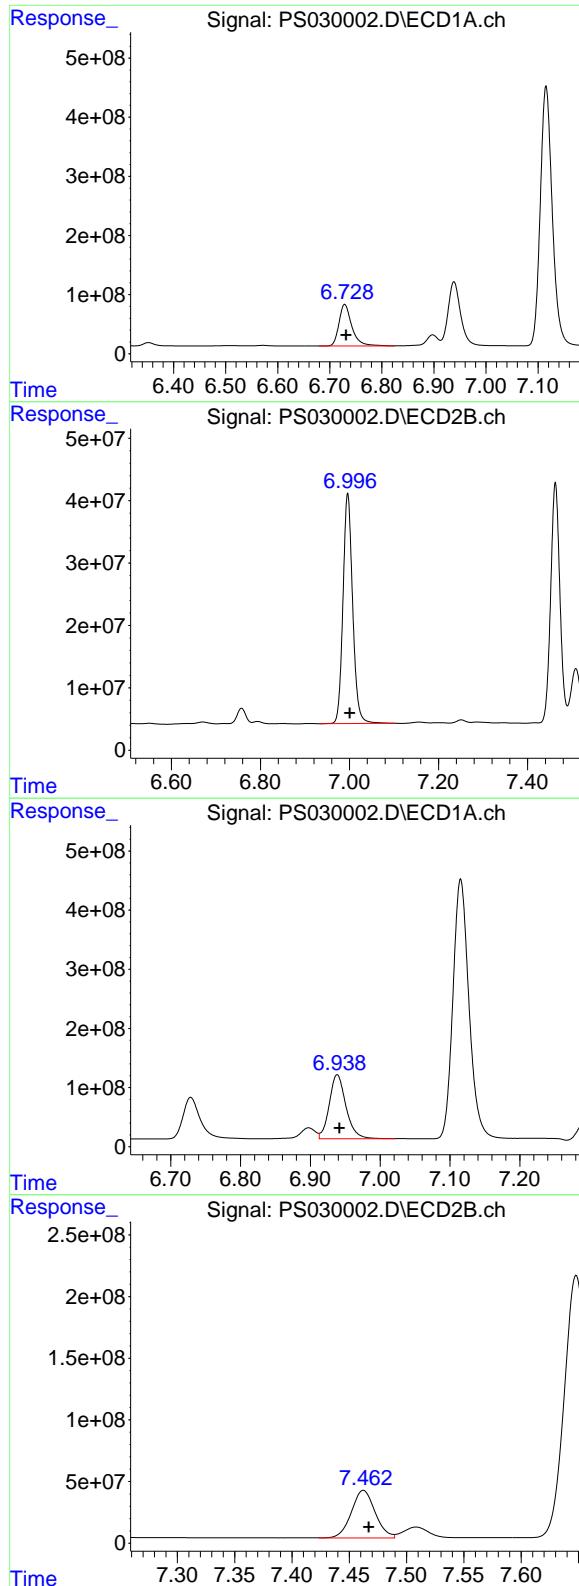

#3 4-Nitrophenol

R.T.: 6.729 min  
 Delta R.T.: -0.003 min  
 Response: 1209402202  
 Conc: 678.17 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#3 4-Nitrophenol


R.T.: 6.996 min  
 Delta R.T.: -0.005 min  
 Response: 555722167  
 Conc: 725.56 ng/ml

#4 2,4-DCAA

R.T.: 6.939 min  
 Delta R.T.: -0.003 min  
 Response: 1810298034  
 Conc: 735.57 ng/ml

#4 2,4-DCAA

R.T.: 7.462 min  
 Delta R.T.: -0.005 min  
 Response: 559483066  
 Conc: 794.14 ng/ml

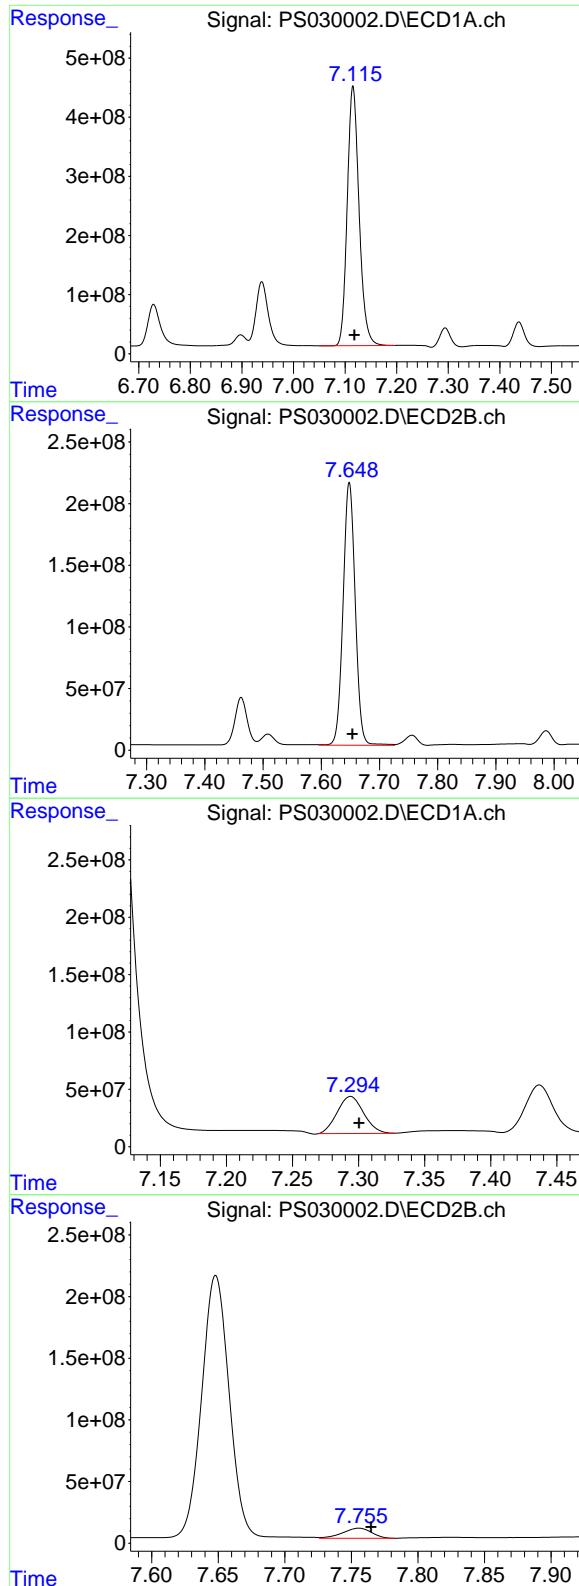

#5 DICAMBA

R.T.: 7.115 min  
Delta R.T.: -0.003 min  
Response: 6990261354  
Conc: 705.88 ng/ml

Instrument: ECD\_S  
ClientSampleId: HSTDCCC750

#5 DICAMBA


R.T.: 7.648 min  
Delta R.T.: -0.005 min  
Response: 3084666816  
Conc: 780.92 ng/ml

#6 MCPP

R.T.: 7.294 min  
Delta R.T.: -0.006 min  
Response: 452596677  
Conc: 70.24 ug/ml

#6 MCPP

R.T.: 7.756 min  
Delta R.T.: -0.009 min  
Response: 123062529  
Conc: 70.36 ug/ml

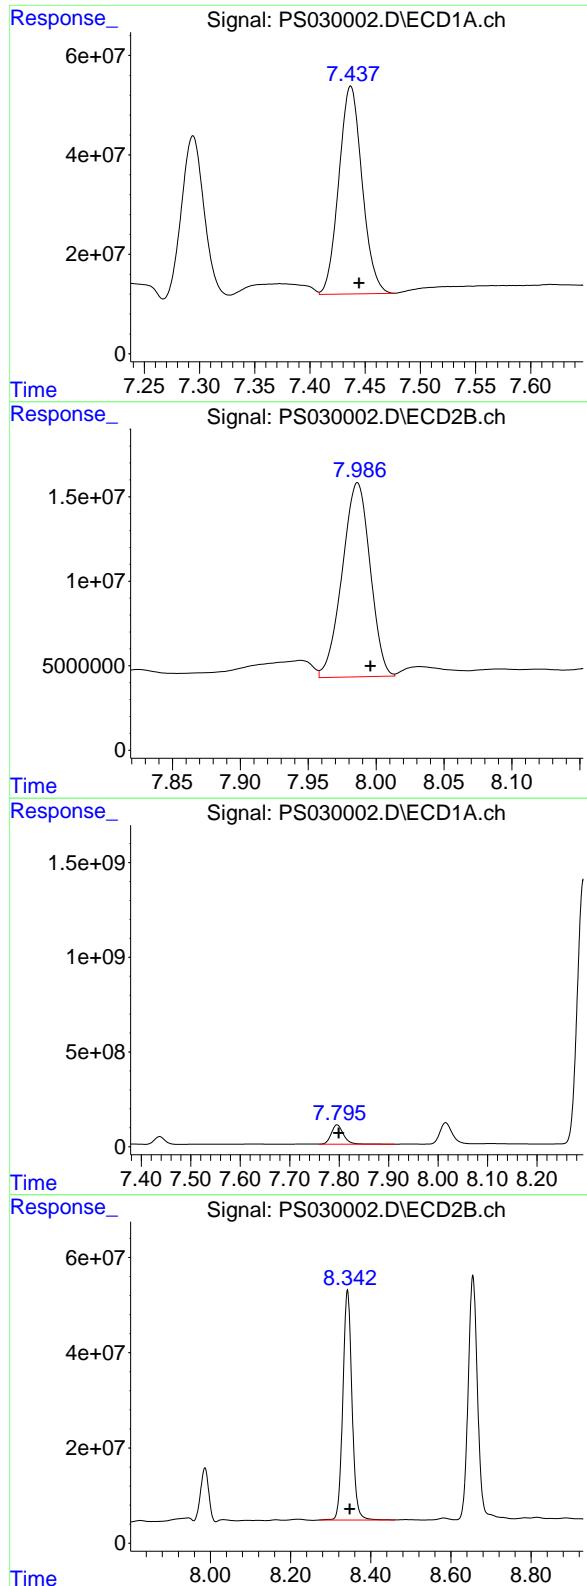

#7 MCPA

R.T.: 7.437 min  
 Delta R.T.: -0.008 min  
 Response: 612821796  
 Conc: 69.39 ug/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#7 MCPA


R.T.: 7.986 min  
 Delta R.T.: -0.009 min  
 Response: 164234366  
 Conc: 69.42 ug/ml

#8 DICHLOPROP

R.T.: 7.796 min  
 Delta R.T.: -0.003 min  
 Response: 1743091262  
 Conc: 687.85 ng/ml

#8 DICHLOPROP

R.T.: 8.342 min  
 Delta R.T.: -0.006 min  
 Response: 763768910  
 Conc: 760.75 ng/ml

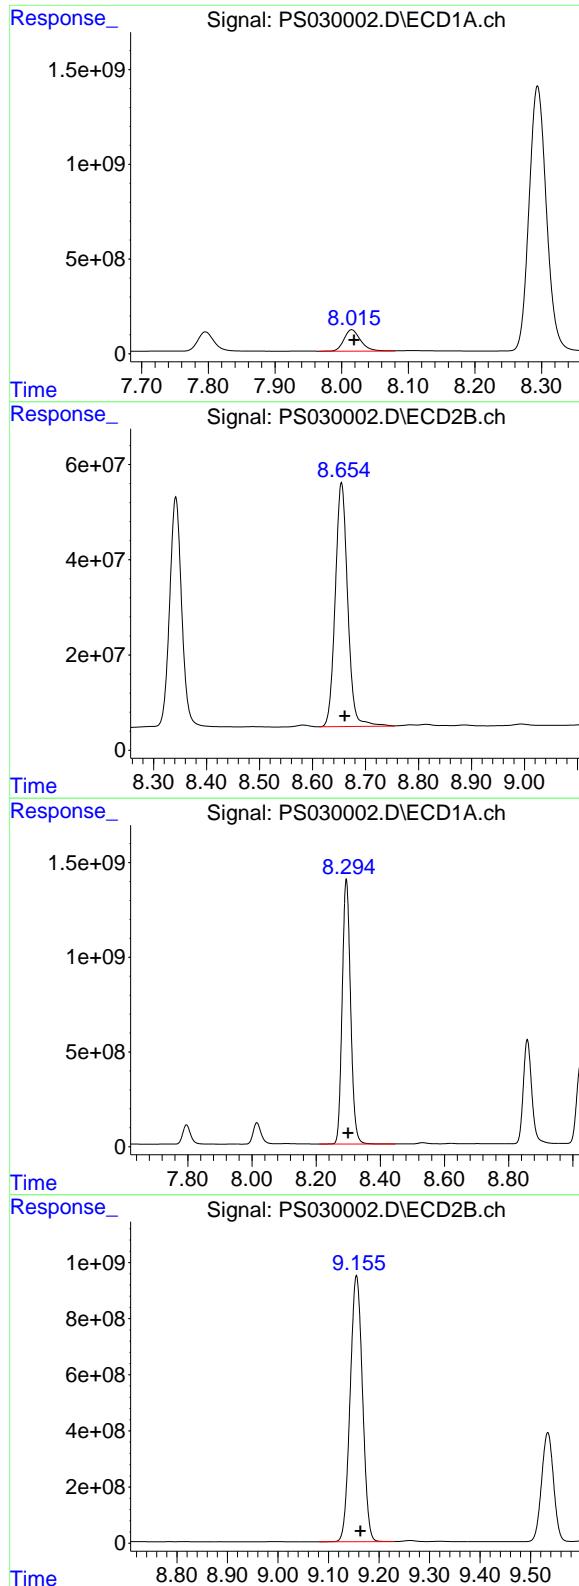

#9 2,4-D

R.T.: 8.015 min  
 Delta R.T.: -0.004 min  
 Response: 1969440235  
 Conc: 700.15 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#9 2,4-D


R.T.: 8.655 min  
 Delta R.T.: -0.006 min  
 Response: 836059988  
 Conc: 741.78 ng/ml

#10 Pentachlorophenol

R.T.: 8.294 min  
 Delta R.T.: -0.006 min  
 Response: 25274216279  
 Conc: 724.50 ng/ml

#10 Pentachlorophenol

R.T.: 9.155 min  
 Delta R.T.: -0.008 min  
 Response: 16072410428  
 Conc: 790.00 ng/ml

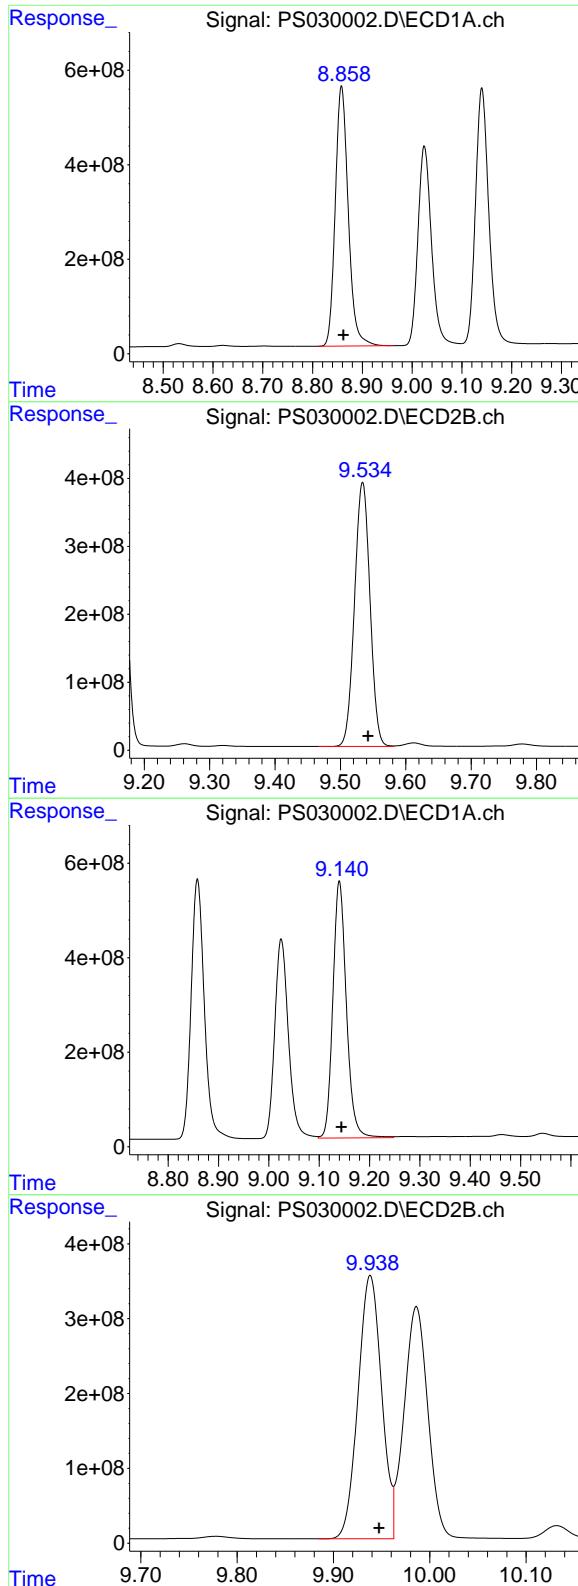

#11 2,4,5-TP (SILVEX)

R.T.: 8.858 min  
 Delta R.T.: -0.004 min  
 Response: 9981291001  
 Conc: 720.00 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#11 2,4,5-TP (SILVEX)


R.T.: 9.534 min  
 Delta R.T.: -0.009 min  
 Response: 6378120993  
 Conc: 779.55 ng/ml

#12 2,4,5-T

R.T.: 9.140 min  
 Delta R.T.: -0.004 min  
 Response: 10149222516  
 Conc: 722.20 ng/ml

#12 2,4,5-T

R.T.: 9.938 min  
 Delta R.T.: -0.009 min  
 Response: 5979942577  
 Conc: 770.35 ng/ml

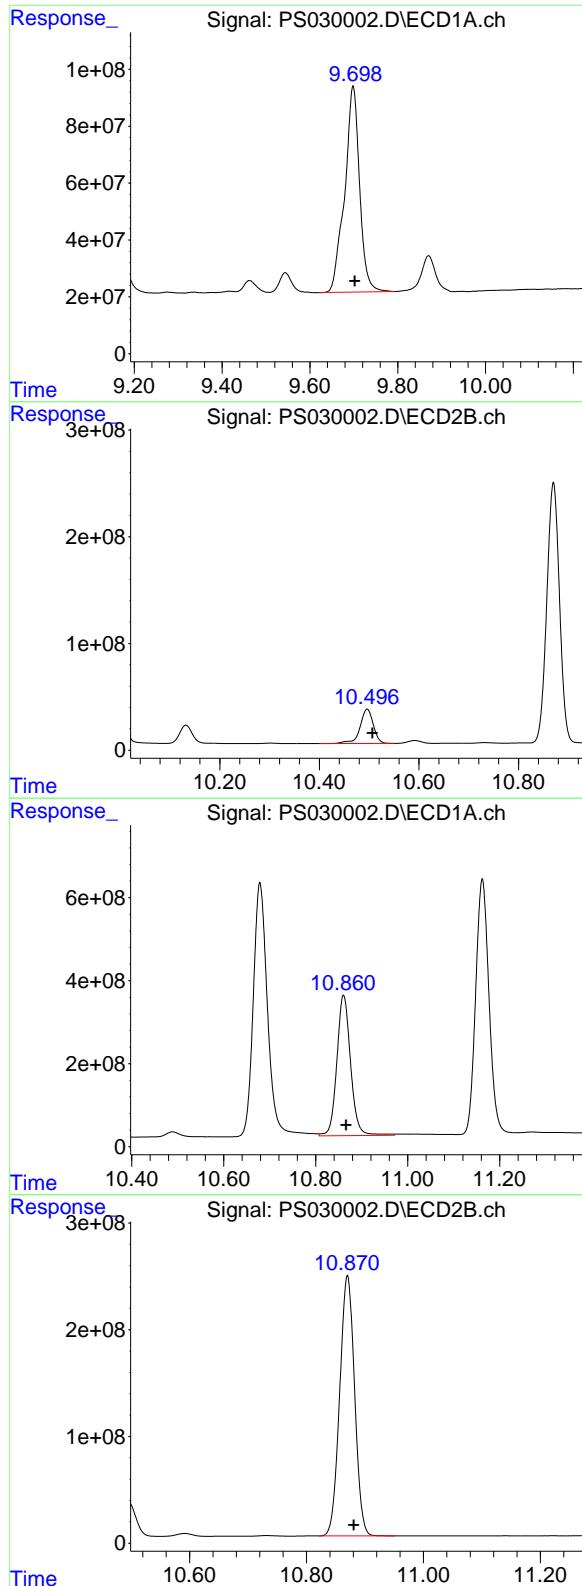

#13 2,4-DB

R.T.: 9.698 min  
 Delta R.T.: -0.004 min  
 Response: 1710051124  
 Conc: 748.26 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#13 2,4-DB


R.T.: 10.496 min  
 Delta R.T.: -0.010 min  
 Response: 595085100  
 Conc: 739.38 ng/ml

#14 DINOSEB

R.T.: 10.860 min  
 Delta R.T.: -0.005 min  
 Response: 7020810578  
 Conc: 690.11 ng/ml

#14 DINOSEB

R.T.: 10.870 min  
 Delta R.T.: -0.011 min  
 Response: 4312313988  
 Conc: 739.55 ng/ml

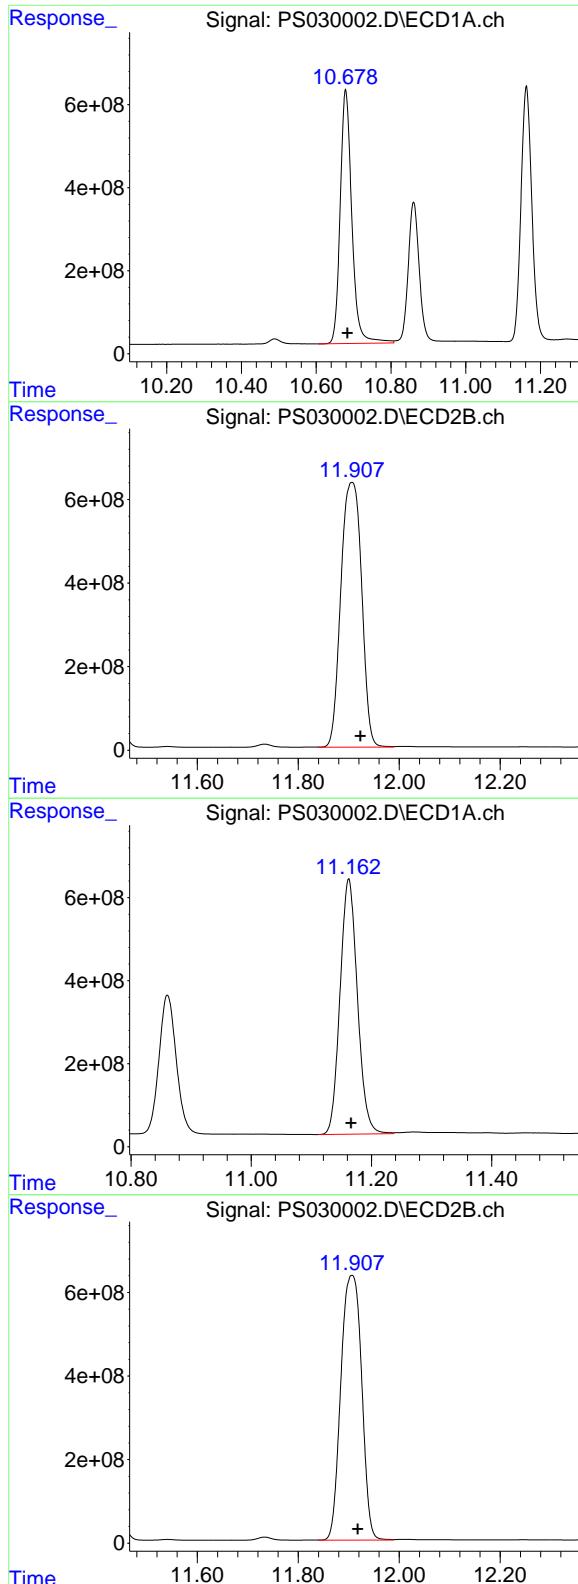

#15 Picloram

R.T.: 10.679 min  
 Delta R.T.: -0.005 min  
 Response: 13213782052  
 Conc: 720.86 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#15 Picloram

R.T.: 11.906 min  
 Delta R.T.: -0.017 min  
 Response: 18060964673  
 Conc: 1470.33 ng/ml

#16 DCPA

R.T.: 11.162 min  
 Delta R.T.: -0.004 min  
 Response: 12337113007  
 Conc: 724.82 ng/ml

#16 DCPA

R.T.: 11.906 min  
 Delta R.T.: -0.011 min  
 Response: 18060964673  
 Conc: 1602.33 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS030013.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 12:12  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**HSTDCCC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 04:57:06 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.939 7.462 1871.5E6 578.1E6 760.455 820.588

Target Compounds

1) T	Dalapon	2.450	2.523	2842.4E6	1225.0E6	694.072	705.564
2) T	3,5-DICHL...	6.143	6.459	2534.7E6	733.0E6	709.256	749.766
3) T	4-Nitroph...	6.729	6.996	1248.9E6	553.9E6	700.337	723.117
5) T	DICAMBA	7.116	7.648	7216.6E6	3162.9E6	728.740	800.727
6) T	MCPP	7.294	7.755	476.8E6	127.0E6	73.990	72.588
7) T	MCPA	7.437	7.986	642.0E6	173.5E6	72.694	73.321
8) T	DICHLORPROP	7.796	8.341	1795.0E6	771.3E6	708.332	768.253
9) T	2,4-D	8.015	8.654	2025.4E6	853.4E6	720.064	757.125
10) T	Pentachlo...	8.294	9.155	25966.6E6	16440.0E6	744.350	808.069
11) T	2,4,5-TP ...	8.858	9.533	10286.3E6	6518.3E6	742.007	796.691
12) T	2,4,5-T	9.140	9.937	10478.0E6	6086.5E6	745.600	784.085
13) T	2,4-DB	9.698	10.495	1745.4E6	609.4E6	763.742	757.220
14) T	DINOSEB	10.861	10.869	7317.8E6	4408.0E6	719.308	755.957
15) T	Picloram	10.680	11.905	13288.4E6	18055.4E6	724.926	1469.870 #
16) T	DCPA	11.162	11.905	12725.4E6	18055.4E6	747.629	1601.837 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS043025\  
 Data File : PS030013.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 12:12  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDCCC750

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 04:57:06 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

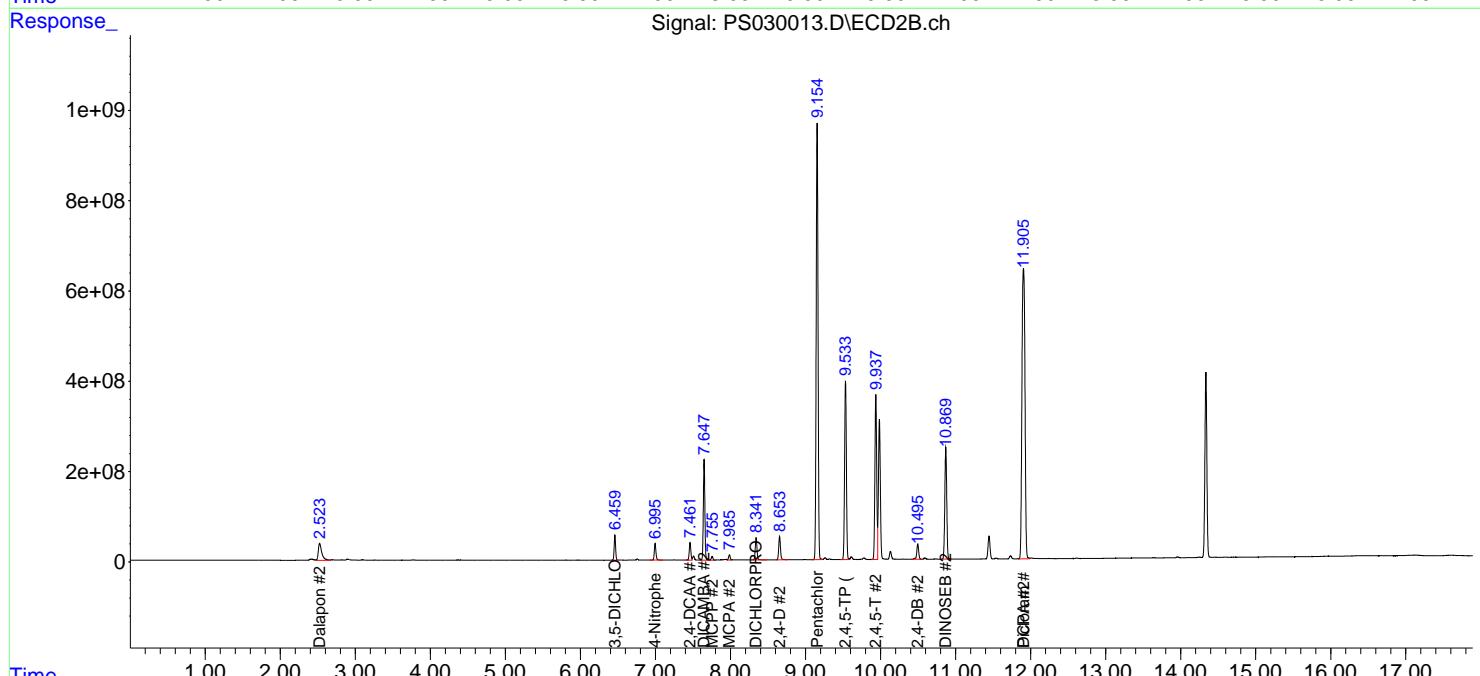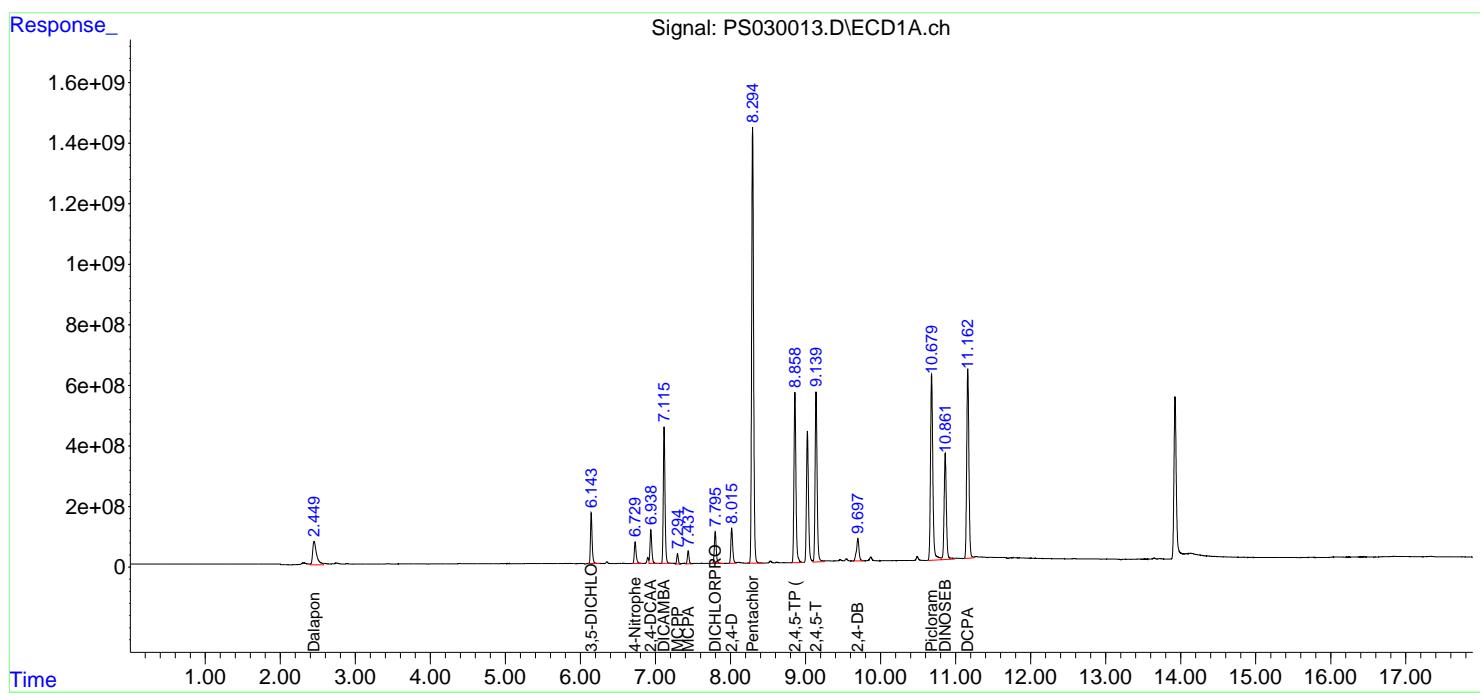

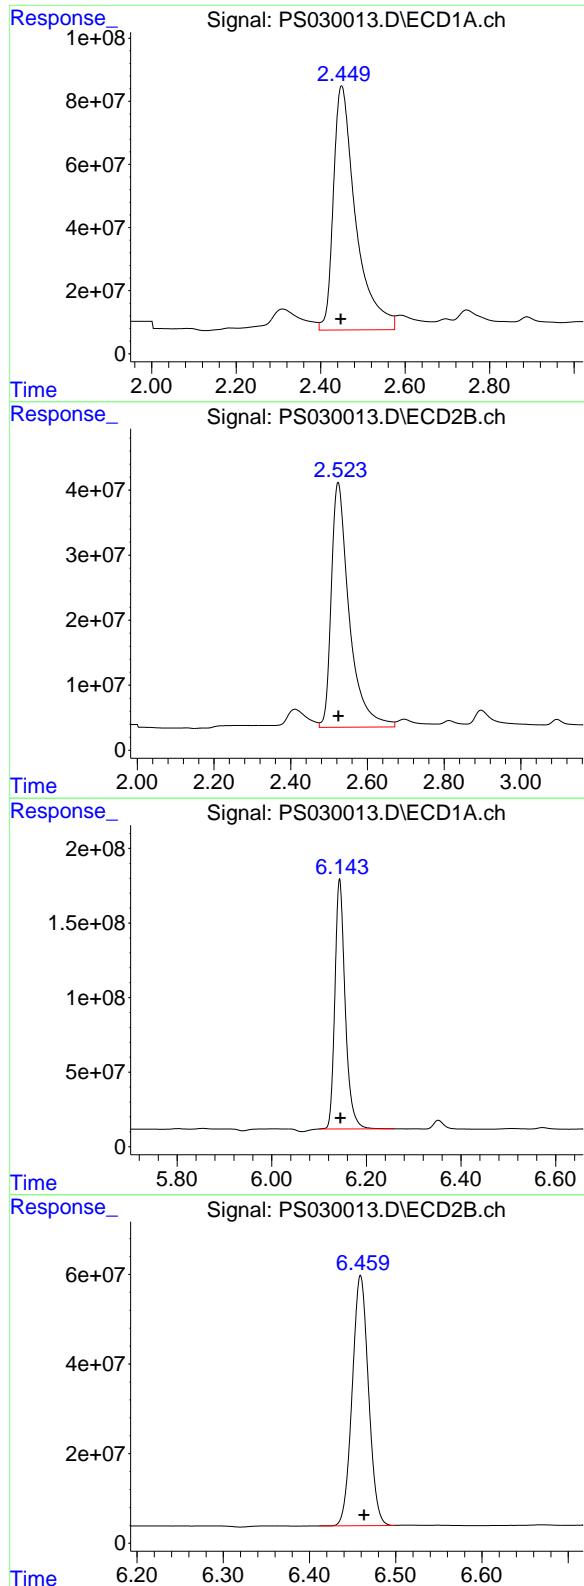

#1 Dalapon

R.T.: 2.450 min  
Delta R.T.: 0.002 min  
Response: 2842405390  
Conc: 694.07 ng/ml

Instrument: ECD\_S  
ClientSampleId: HSTDCCC750

#1 Dalapon


R.T.: 2.523 min  
Delta R.T.: -0.001 min  
Response: 1224960796  
Conc: 705.56 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.143 min  
Delta R.T.: -0.002 min  
Response: 2534729517  
Conc: 709.26 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.459 min  
Delta R.T.: -0.004 min  
Response: 732955479  
Conc: 749.77 ng/ml

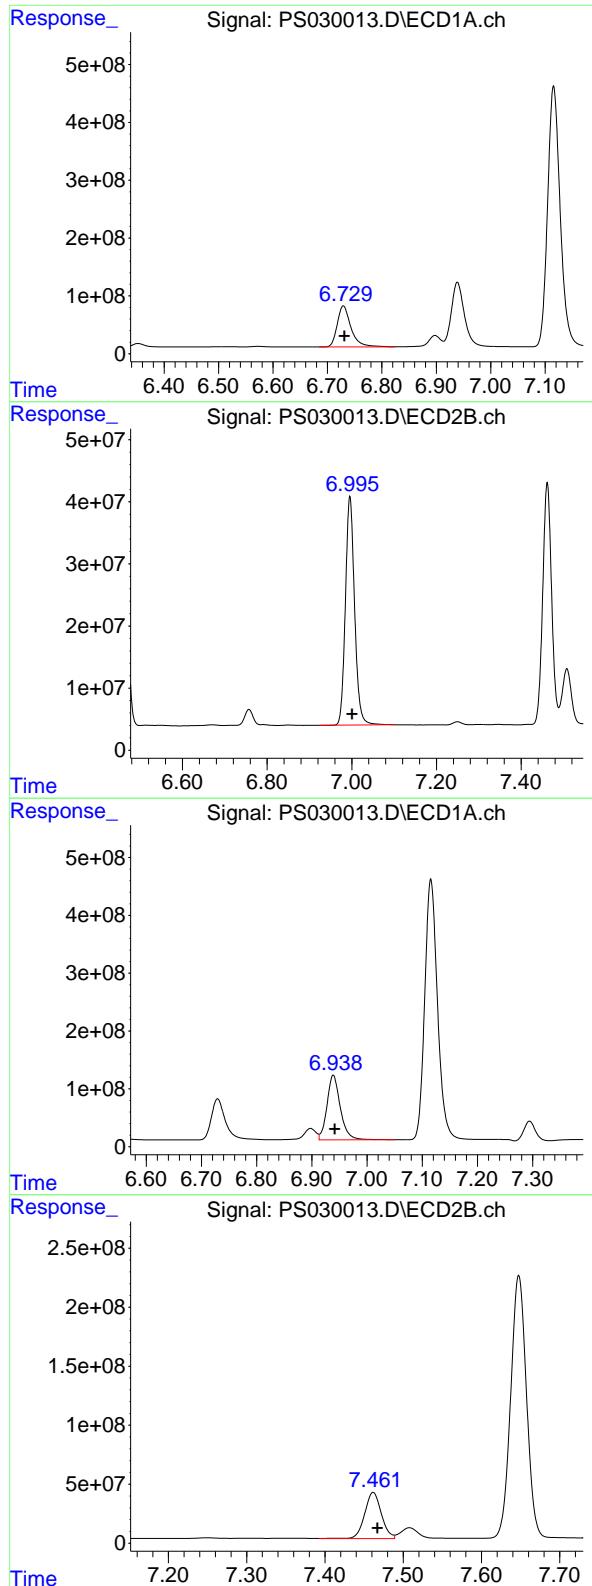

#3 4-Nitrophenol

R.T.: 6.729 min  
 Delta R.T.: -0.002 min  
 Response: 1248924020  
 Conc: 700.34 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#3 4-Nitrophenol


R.T.: 6.996 min  
 Delta R.T.: -0.005 min  
 Response: 553850837  
 Conc: 723.12 ng/ml

#4 2,4-DCAA

R.T.: 6.939 min  
 Delta R.T.: -0.003 min  
 Response: 1871539269  
 Conc: 760.45 ng/ml

#4 2,4-DCAA

R.T.: 7.462 min  
 Delta R.T.: -0.005 min  
 Response: 578117969  
 Conc: 820.59 ng/ml

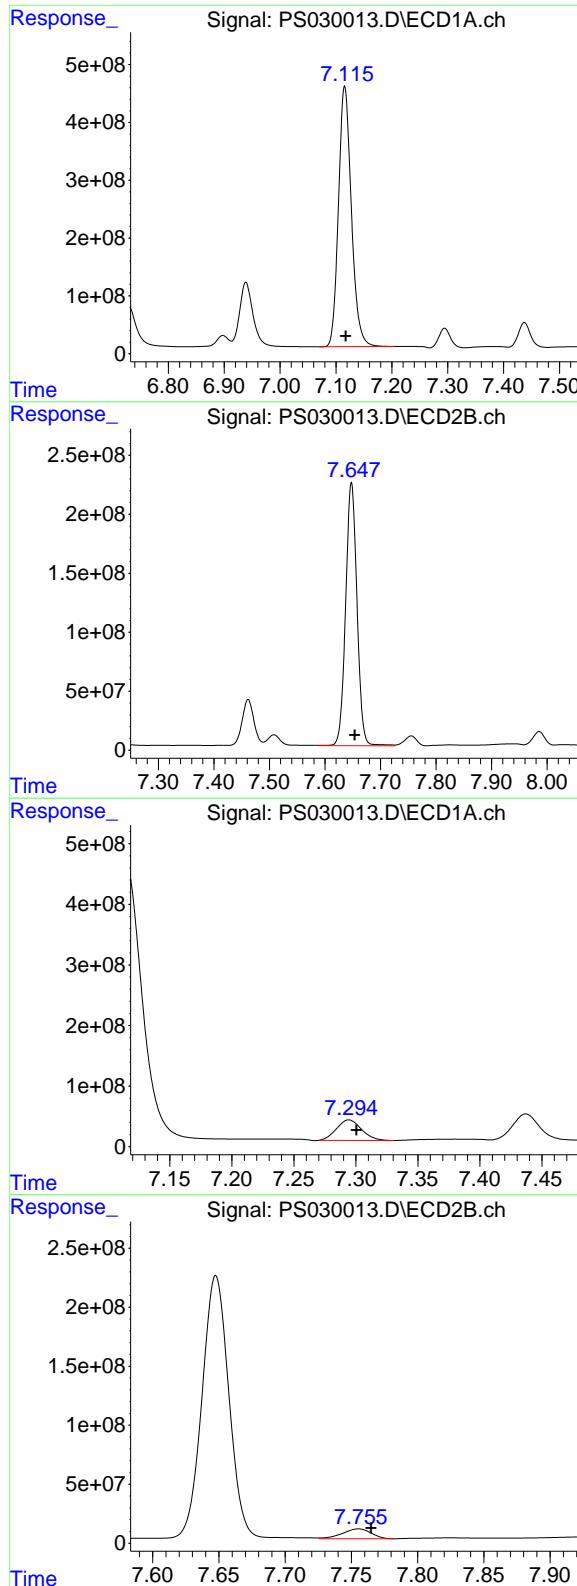

#5 DICAMBA

R.T.: 7.116 min  
 Delta R.T.: -0.002 min  
 Response: 7216610889  
 Conc: 728.74 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#5 DICAMBA


R.T.: 7.648 min  
 Delta R.T.: -0.006 min  
 Response: 3162921794  
 Conc: 800.73 ng/ml

#6 MCPP

R.T.: 7.294 min  
 Delta R.T.: -0.006 min  
 Response: 476765864  
 Conc: 73.99 ug/ml

#6 MCPP

R.T.: 7.755 min  
 Delta R.T.: -0.009 min  
 Response: 126951961  
 Conc: 72.59 ug/ml

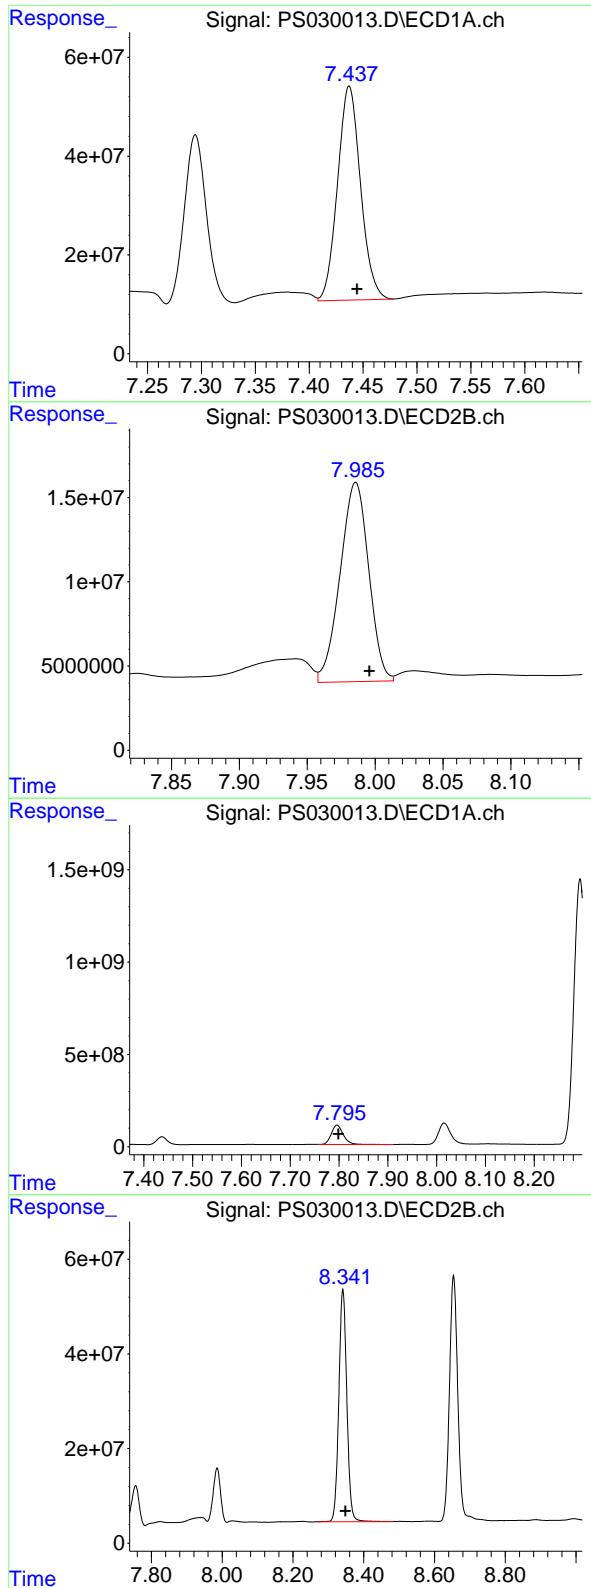

#7 MCPA

R.T.: 7.437 min  
 Delta R.T.: -0.007 min  
 Response: 641986097  
 Conc: 72.69 ug/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#7 MCPA


R.T.: 7.986 min  
 Delta R.T.: -0.010 min  
 Response: 173462992  
 Conc: 73.32 ug/ml

#8 DICHLOPROP

R.T.: 7.796 min  
 Delta R.T.: -0.003 min  
 Response: 1794988816  
 Conc: 708.33 ng/ml

#8 DICHLOPROP

R.T.: 8.341 min  
 Delta R.T.: -0.007 min  
 Response: 771298752  
 Conc: 768.25 ng/ml

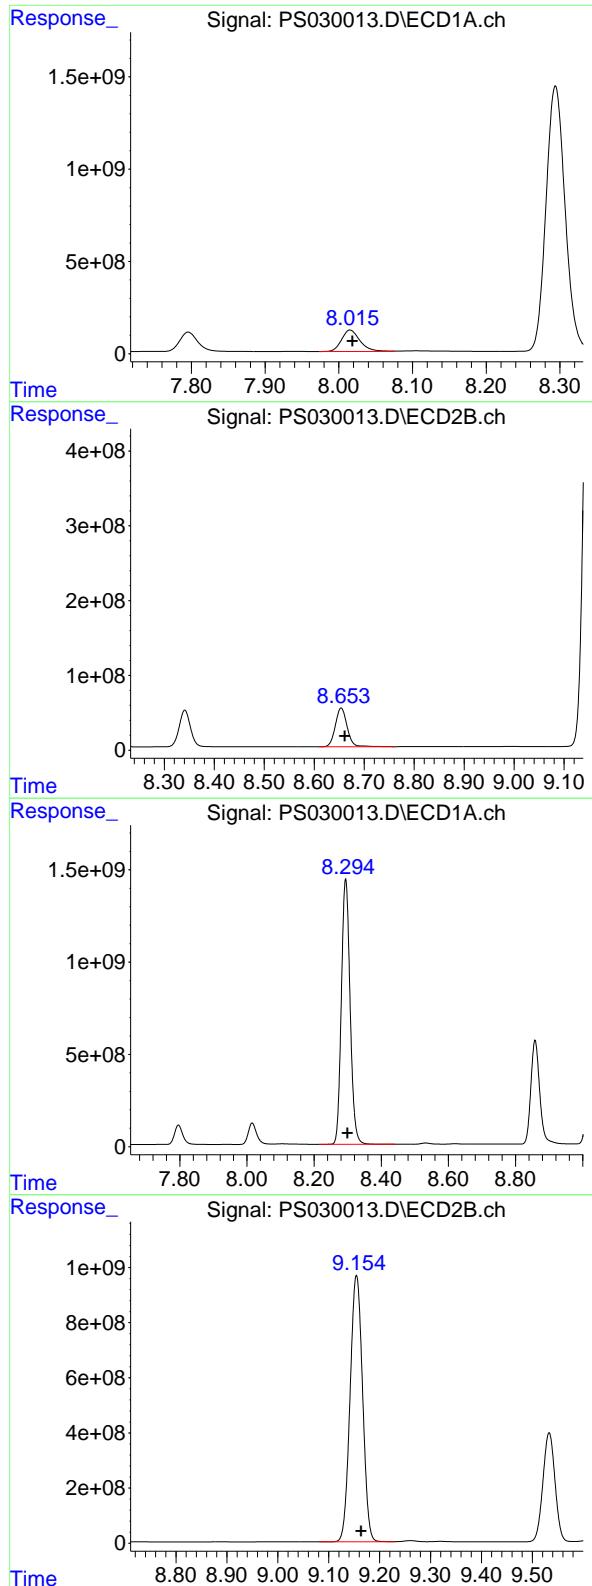

#9 2,4-D

R.T.: 8.015 min  
 Delta R.T.: -0.003 min  
 Response: 2025447050  
 Conc: 720.06 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#9 2,4-D


R.T.: 8.654 min  
 Delta R.T.: -0.007 min  
 Response: 853360684  
 Conc: 757.12 ng/ml

#10 Pentachlorophenol

R.T.: 8.294 min  
 Delta R.T.: -0.006 min  
 Response: 25966648022  
 Conc: 744.35 ng/ml

#10 Pentachlorophenol

R.T.: 9.155 min  
 Delta R.T.: -0.009 min  
 Response: 16440020170  
 Conc: 808.07 ng/ml

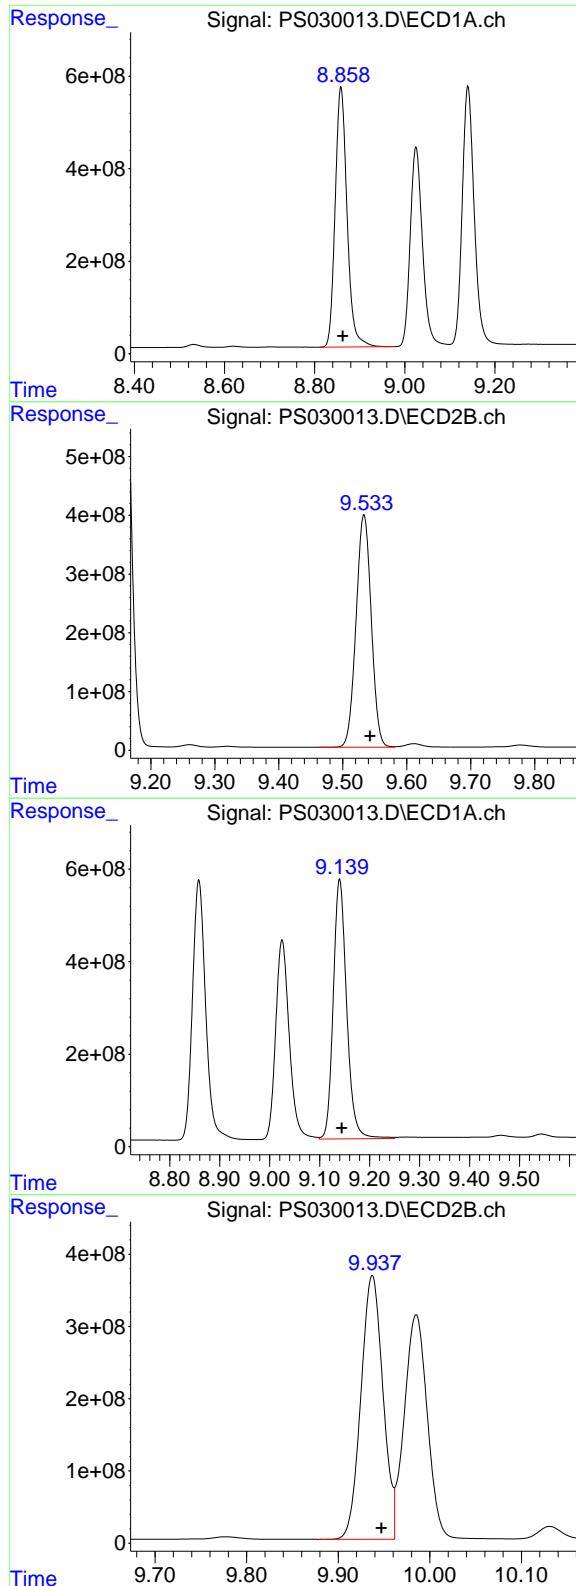

#11 2,4,5-TP (SILVEX)

R.T.: 8.858 min  
Delta R.T.: -0.004 min  
Instrument: ECD\_S  
Response: 10286319183  
Conc: 742.01 ng/ml  
ClientSampleId: HSTDCCC750

#11 2,4,5-TP (SILVEX)


R.T.: 9.533 min  
Delta R.T.: -0.010 min  
Response: 6518329316  
Conc: 796.69 ng/ml

#12 2,4,5-T

R.T.: 9.140 min  
Delta R.T.: -0.004 min  
Response: 10478000956  
Conc: 745.60 ng/ml

#12 2,4,5-T

R.T.: 9.937 min  
Delta R.T.: -0.010 min  
Response: 6086536736  
Conc: 784.08 ng/ml

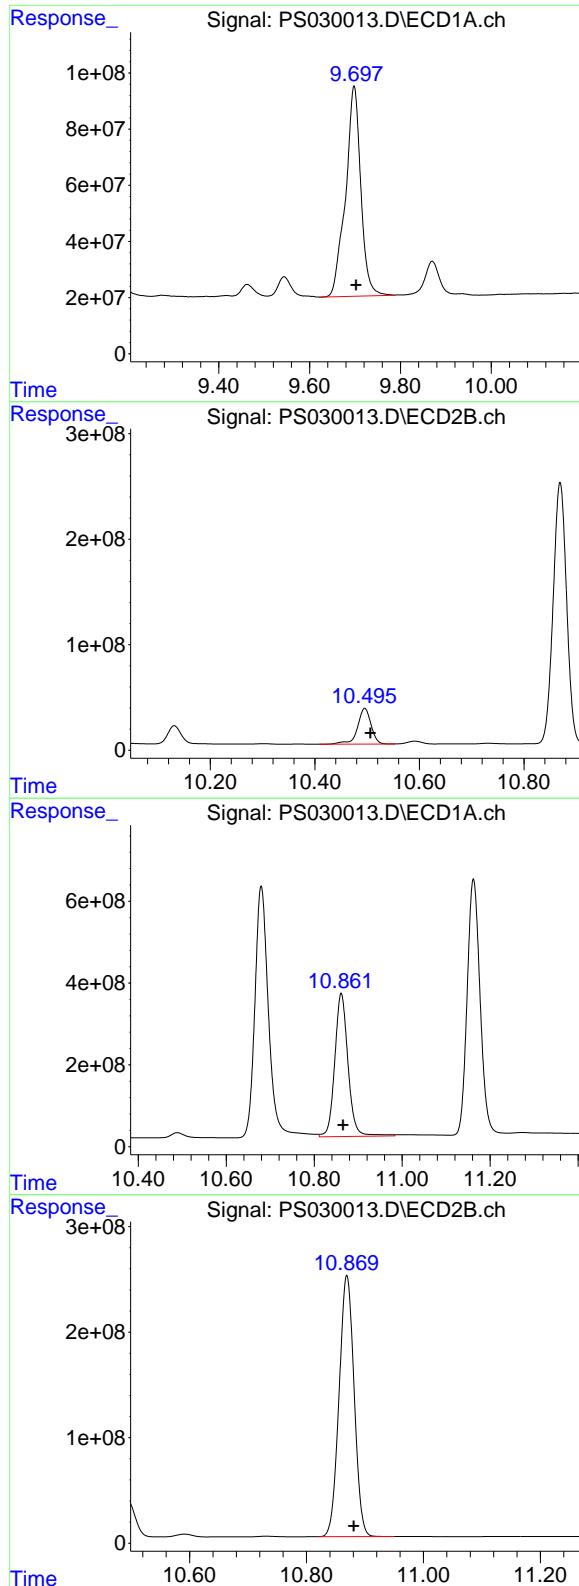

#13 2,4-DB

R.T.: 9.698 min  
 Delta R.T.: -0.004 min  
 Response: 1745423457  
 Conc: 763.74 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#13 2,4-DB


R.T.: 10.495 min  
 Delta R.T.: -0.011 min  
 Response: 609442670  
 Conc: 757.22 ng/ml

#14 DINOSEB

R.T.: 10.861 min  
 Delta R.T.: -0.005 min  
 Response: 7317825824  
 Conc: 719.31 ng/ml

#14 DINOSEB

R.T.: 10.869 min  
 Delta R.T.: -0.012 min  
 Response: 4407971468  
 Conc: 755.96 ng/ml

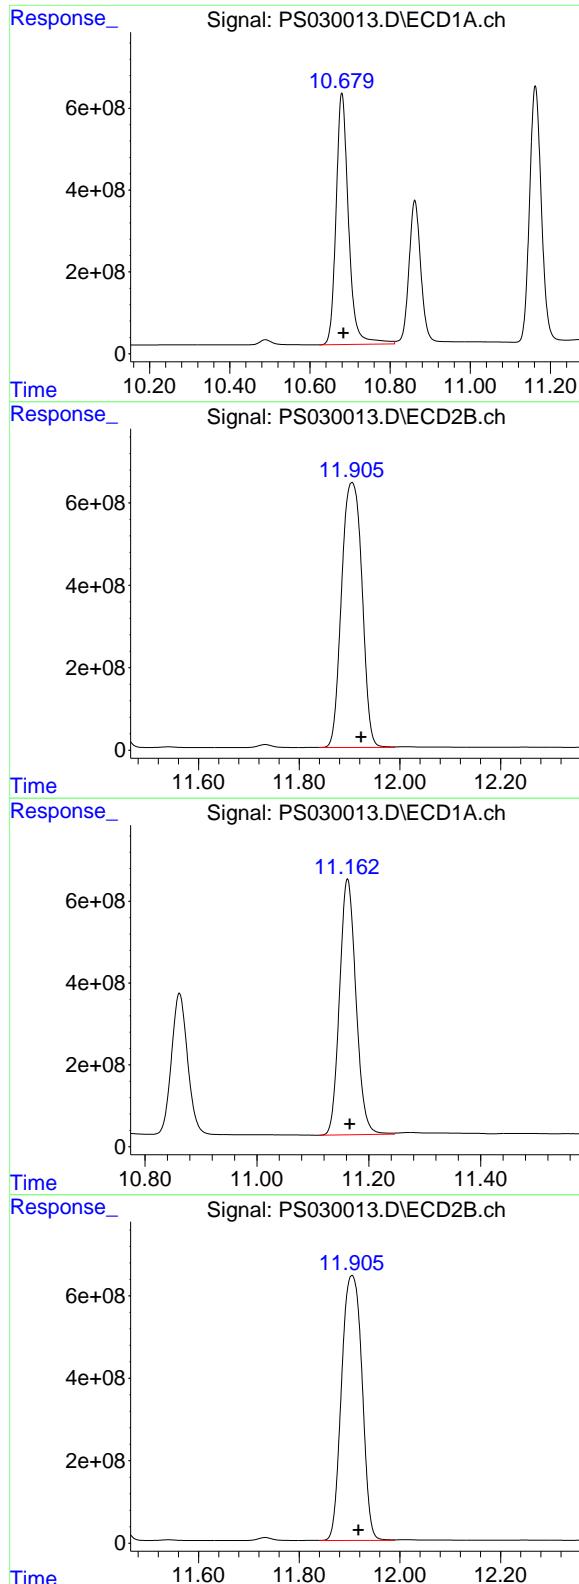

#15 Picloram

R.T.: 10.680 min  
 Delta R.T.: -0.004 min  
 Response: 13288353705  
 Conc: 724.93 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#15 Picloram

R.T.: 11.905 min  
 Delta R.T.: -0.018 min  
 Response: 18055353858  
 Conc: 1469.87 ng/ml

#16 DCPA

R.T.: 11.162 min  
 Delta R.T.: -0.004 min  
 Response: 12725385376  
 Conc: 747.63 ng/ml

#16 DCPA

R.T.: 11.905 min  
 Delta R.T.: -0.013 min  
 Response: 18055353858  
 Conc: 1601.84 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030016.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 13:27  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**HSTDCCC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:28:08 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.938 7.462 1884.6E6 575.4E6 765.767 816.786

Target Compounds

1) T	Dalapon	2.449	2.523	2798.1E6	1209.5E6	683.247	696.662
2) T	3,5-DICHL...	6.143	6.459	2544.7E6	733.9E6	712.034	750.706
3) T	4-Nitroph...	6.728	6.996	1257.5E6	552.2E6	705.169	720.931
5) T	DICAMBA	7.115	7.648	7244.6E6	3144.8E6	731.569	796.146
6) T	MCPP	7.294	7.755	469.8E6	129.0E6	72.914	73.740
7) T	MCPA	7.436	7.986	645.8E6	171.6E6	73.130	72.542
8) T	DICHLORPROP	7.795	8.341	1809.7E6	774.5E6	714.123	771.491
9) T	2,4-D	8.014	8.654	2042.0E6	854.2E6	725.956	757.867
10) T	Pentachlo...	8.293	9.155	26148.2E6	16409.8E6	749.553	806.585
11) T	2,4,5-TP ...	8.858	9.533	10392.9E6	6513.9E6	749.693	796.152
12) T	2,4,5-T	9.139	9.937	10599.2E6	6089.9E6	754.227	784.513
13) T	2,4-DB	9.698	10.495	1756.3E6	619.2E6	768.523	769.370
14) T	DINOSEB	10.860	10.869	7372.8E6	4425.3E6	724.708	758.937
15) T	Picloram	10.679	11.905	13694.5E6	18404.4E6	747.085	1498.289 #
16) T	DCPA	11.161	11.905	12916.6E6	18404.4E6	758.863	1632.808 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030016.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 13:27  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1



Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDCCC750


Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:28:08 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l

Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2

Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

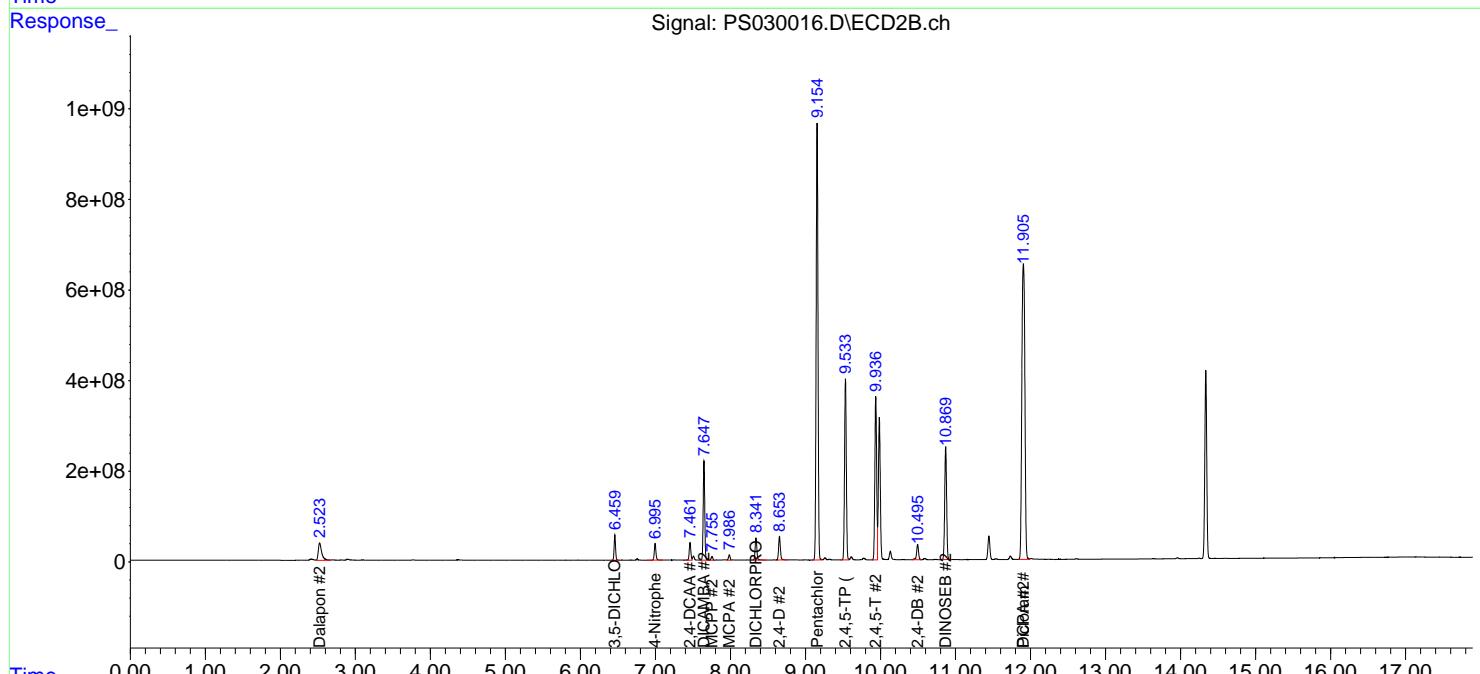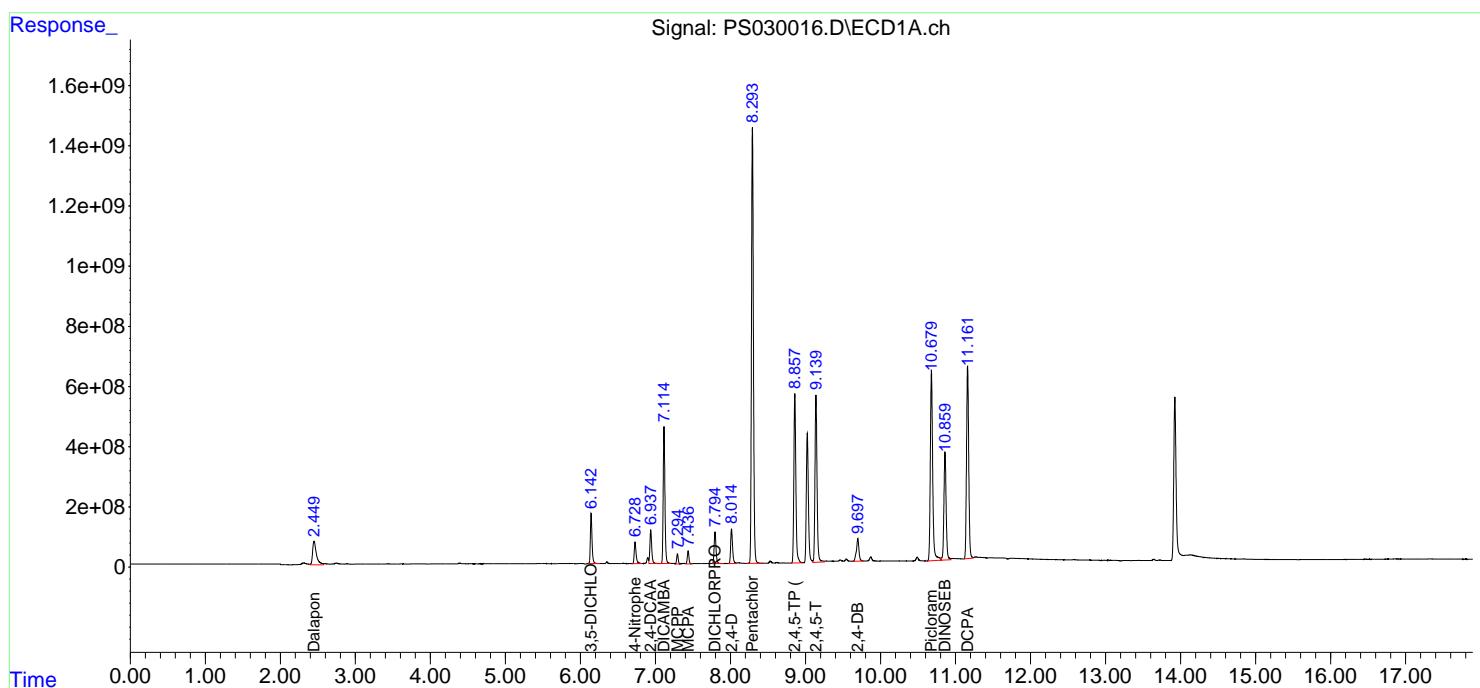

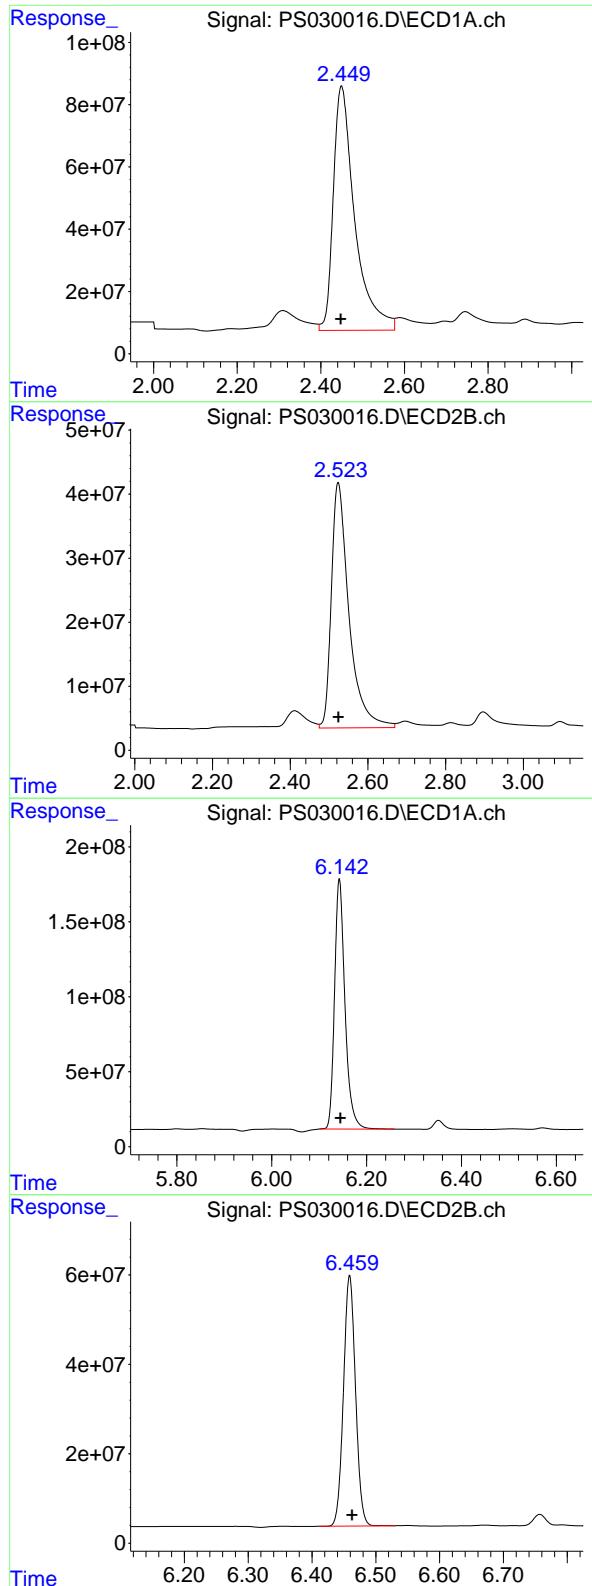

#1 Dalapon

R.T.: 2.449 min  
Delta R.T.: 0.001 min  
Response: 2798074434  
Conc: 683.25 ng/ml

Instrument: ECD\_S  
ClientSampleId: HSTDCCC750

#1 Dalapon


R.T.: 2.523 min  
Delta R.T.: 0.000 min  
Response: 1209506191  
Conc: 696.66 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.143 min  
Delta R.T.: -0.003 min  
Response: 2544656484  
Conc: 712.03 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.459 min  
Delta R.T.: -0.004 min  
Response: 733875039  
Conc: 750.71 ng/ml

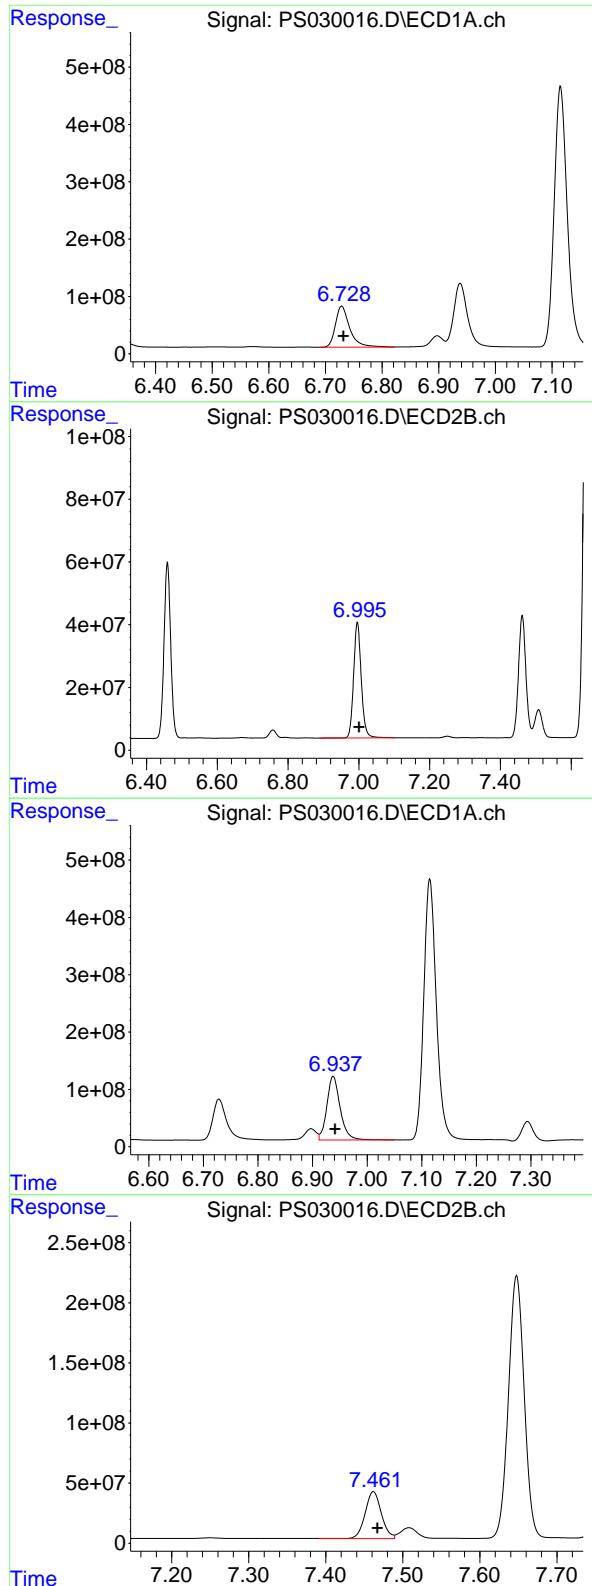

#3 4-Nitrophenol

R.T.: 6.728 min  
 Delta R.T.: -0.003 min  
 Response: 1257541620  
 Conc: 705.17 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#3 4-Nitrophenol


R.T.: 6.996 min  
 Delta R.T.: -0.005 min  
 Response: 552176387  
 Conc: 720.93 ng/ml

#4 2,4-DCAA

R.T.: 6.938 min  
 Delta R.T.: -0.004 min  
 Response: 1884613932  
 Conc: 765.77 ng/ml

#4 2,4-DCAA

R.T.: 7.462 min  
 Delta R.T.: -0.005 min  
 Response: 575439313  
 Conc: 816.79 ng/ml

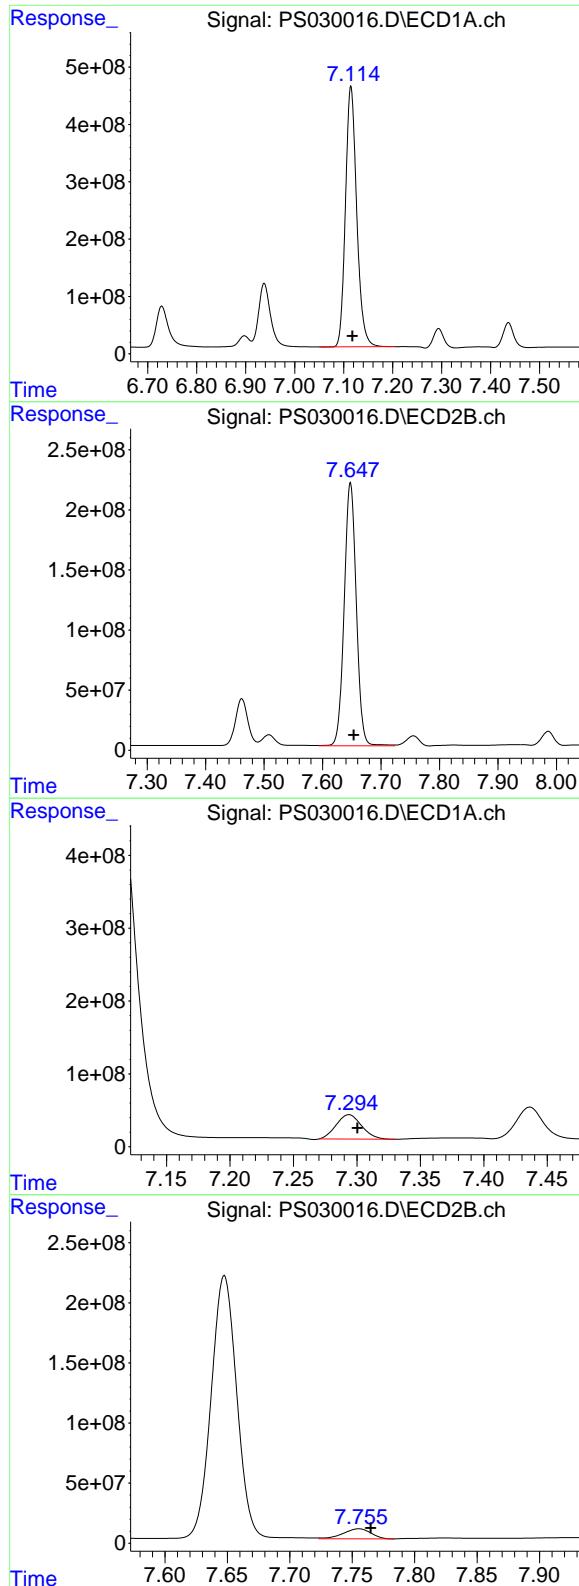

#5 DICAMBA

R.T.: 7.115 min  
Delta R.T.: -0.003 min  
Response: 7244628718  
Conc: 731.57 ng/ml

Instrument: ECD\_S  
ClientSampleId: HSTDCCC750

#5 DICAMBA


R.T.: 7.648 min  
Delta R.T.: -0.006 min  
Response: 3144828216  
Conc: 796.15 ng/ml

#6 MCPP

R.T.: 7.294 min  
Delta R.T.: -0.006 min  
Response: 469831489  
Conc: 72.91 ug/ml

#6 MCPP


R.T.: 7.755 min  
Delta R.T.: -0.010 min  
Response: 128968282  
Conc: 73.74 ug/ml

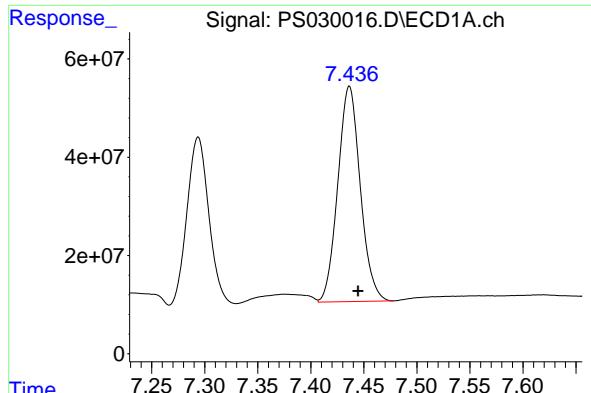

#7 MCPA


R.T.: 7.436 min  
Delta R.T.: -0.008 min  
Response: 645840618  
Conc: 73.13 ug/ml

Instrument: ECD\_S  
ClientSampleId: HSTDCCC750

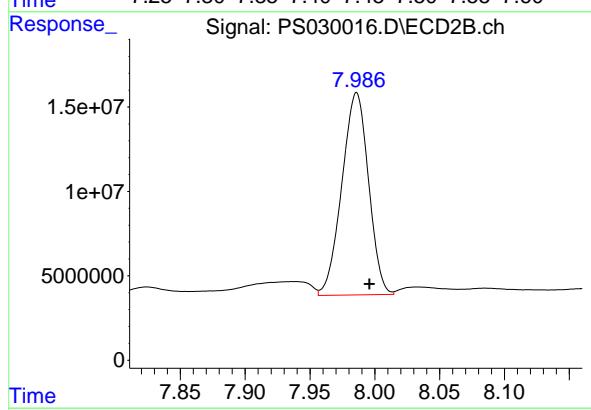


#7 MCPA

R.T.: 7.986 min  
Delta R.T.: -0.010 min  
Response: 171619066  
Conc: 72.54 ug/ml

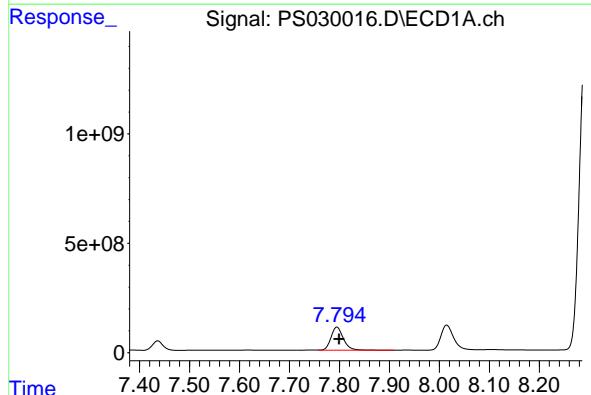


#8 DICHLORPROP

R.T.: 7.795 min  
Delta R.T.: -0.004 min  
Response: 1809664833  
Conc: 714.12 ng/ml

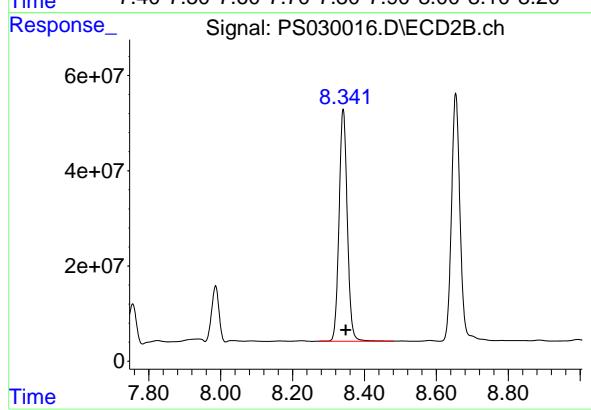

#8 DICHLORPROP

R.T.: 8.341 min  
Delta R.T.: -0.007 min  
Response: 774549366  
Conc: 771.49 ng/ml

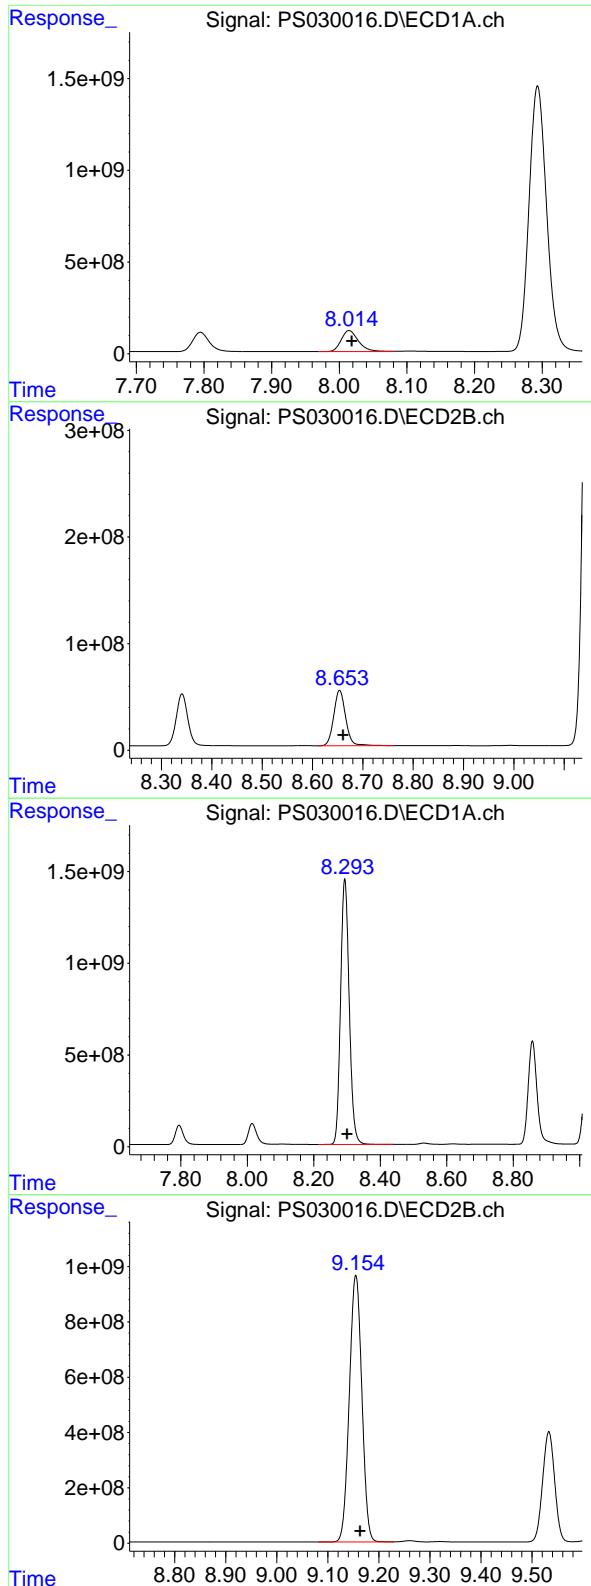

#9 2,4-D

R.T.: 8.014 min  
 Delta R.T.: -0.004 min  
 Response: 2042021191  
 Conc: 725.96 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#9 2,4-D


R.T.: 8.654 min  
 Delta R.T.: -0.007 min  
 Response: 854197073  
 Conc: 757.87 ng/ml

#10 Pentachlorophenol

R.T.: 8.293 min  
 Delta R.T.: -0.006 min  
 Response: 26148171863  
 Conc: 749.55 ng/ml

#10 Pentachlorophenol


R.T.: 9.155 min  
 Delta R.T.: -0.009 min  
 Response: 16409812223  
 Conc: 806.58 ng/ml

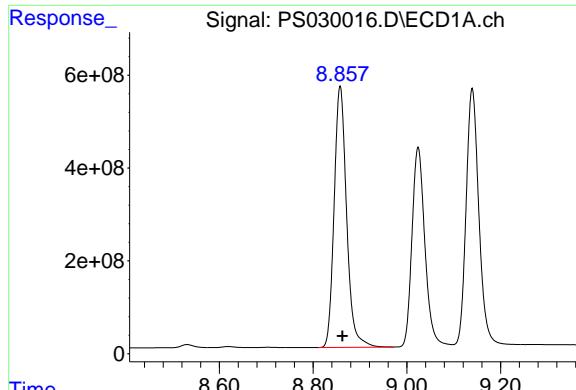

#11 2,4,5-TP (SILVEX)


R.T.: 8.858 min  
 Delta R.T.: -0.004 min  
 Response: 10392876642  
 Conc: 749.69 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

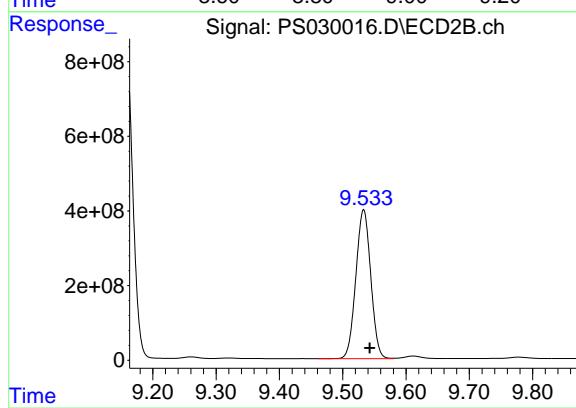


#11 2,4,5-TP (SILVEX)

R.T.: 9.533 min  
 Delta R.T.: -0.010 min  
 Response: 6513919285  
 Conc: 796.15 ng/ml

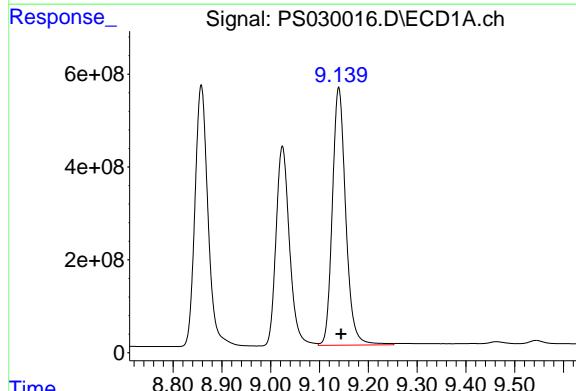


#12 2,4,5-T

R.T.: 9.139 min  
 Delta R.T.: -0.005 min  
 Response: 10599227676  
 Conc: 754.23 ng/ml

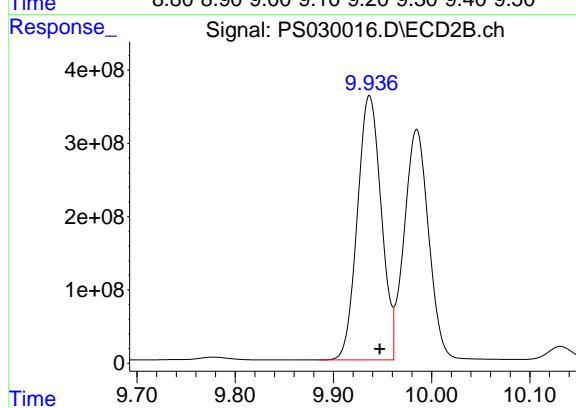

#12 2,4,5-T

R.T.: 9.937 min  
 Delta R.T.: -0.010 min  
 Response: 6089857207  
 Conc: 784.51 ng/ml

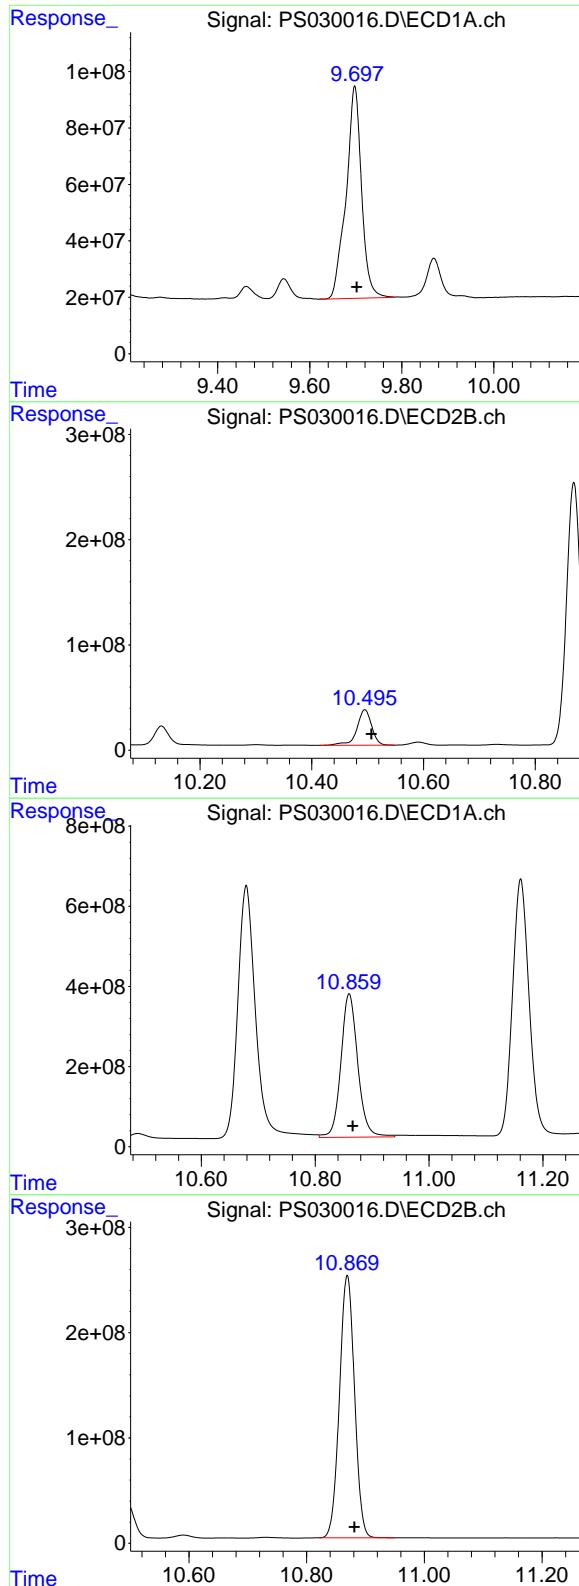

#13 2,4-DB

R.T.: 9.698 min  
 Delta R.T.: -0.004 min  
 Response: 1756348858  
 Conc: 768.52 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#13 2,4-DB


R.T.: 10.495 min  
 Delta R.T.: -0.011 min  
 Response: 619221462  
 Conc: 769.37 ng/ml

#14 DINOSEB

R.T.: 10.860 min  
 Delta R.T.: -0.006 min  
 Response: 7372763225  
 Conc: 724.71 ng/ml

#14 DINOSEB

R.T.: 10.869 min  
 Delta R.T.: -0.012 min  
 Response: 4425346841  
 Conc: 758.94 ng/ml

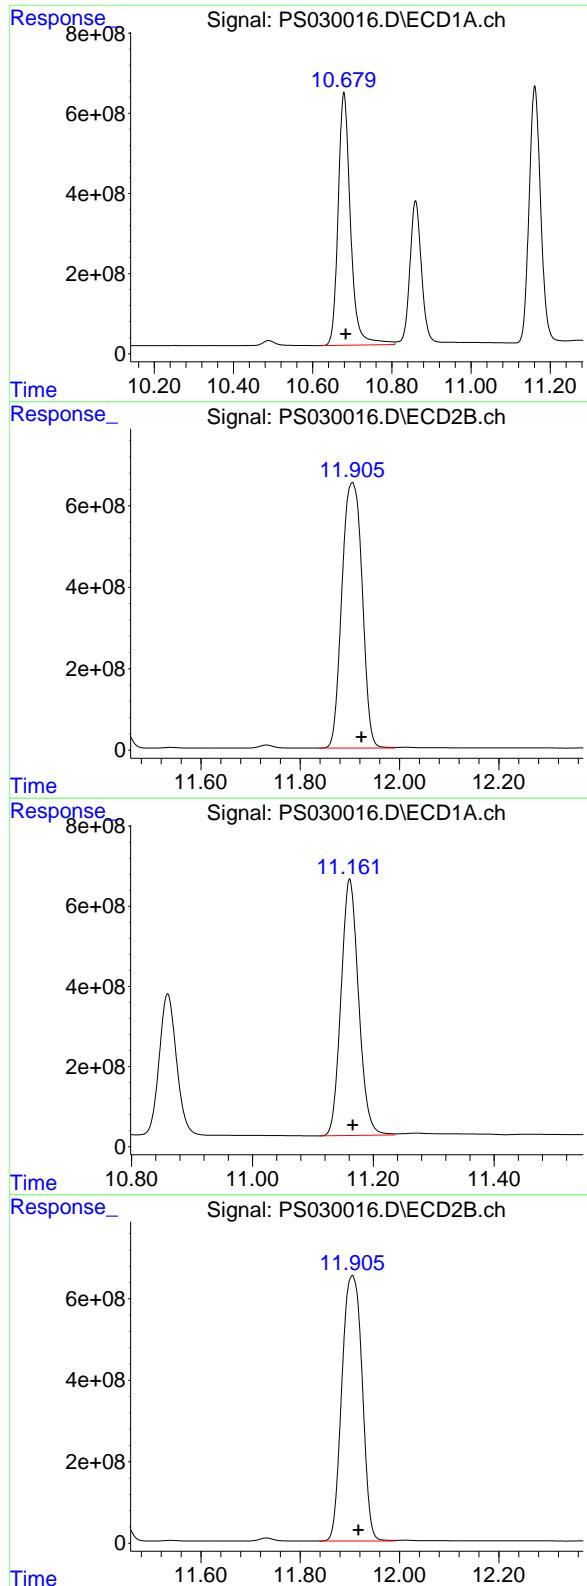

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030017.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 13:51  
 Operator : AR\AJ  
 Sample : Q1983-01  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**OU4-PCS-TC-27-042325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:28:26 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.938 7.462 1078.1E6 293.0E6 438.074 415.858

Target Compounds

1) T	Dalapon	2.432	2.499f	198.5E6	30851519	48.460	17.770 #
2) T	3,5-DICHL...	6.136	6.469	5065169	19736620	1.417	20.189 #
3) T	4-Nitroph...	6.719	6.988	34601750	12204445	19.403	15.934
5) T	DICAMBA	7.130	7.629	20840115	10292797	2.104	2.606
6) T	MCPP	7.286	7.789	2374565	11599435	<MDL	6.632 #
7) T	MCPA	7.446	8.021f	18185276	21087650	2.059	8.914 #
8) T	DICHLORPROP	7.799	8.362	48423986	83292801	19.109	82.964 #
9) T	2,4-D	8.027	8.631f	54131730	14339780	19.244	12.723 #
10) T	Pentachlo...	8.290	9.152	140.3E6	26158906	4.023	1.286 #
11) T	2,4,5-TP ...	8.883	9.550	12123631	50827137	<MDL	6.212 #
12) T	2,4,5-T	9.181f	9.914f	91226312	86813759	6.492	11.184 #
13) T	2,4-DB	9.720	10.473f	232.3E6	52968504	101.658	65.812 #
14) T	DINOSEB	10.851	10.893	54420857	5942261	5.349	1.019 #
15) T	Picloram	10.680	11.917	520.4E6	250.0E6	28.389	20.349 #
16) T	DCPA	11.151	11.917	109.0E6	250.0E6	6.406	22.176 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030017.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 13:51  
 Operator : AR\AJ  
 Sample : Q1983-01  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**OU4-PCS-TC-27-042325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:28:26 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

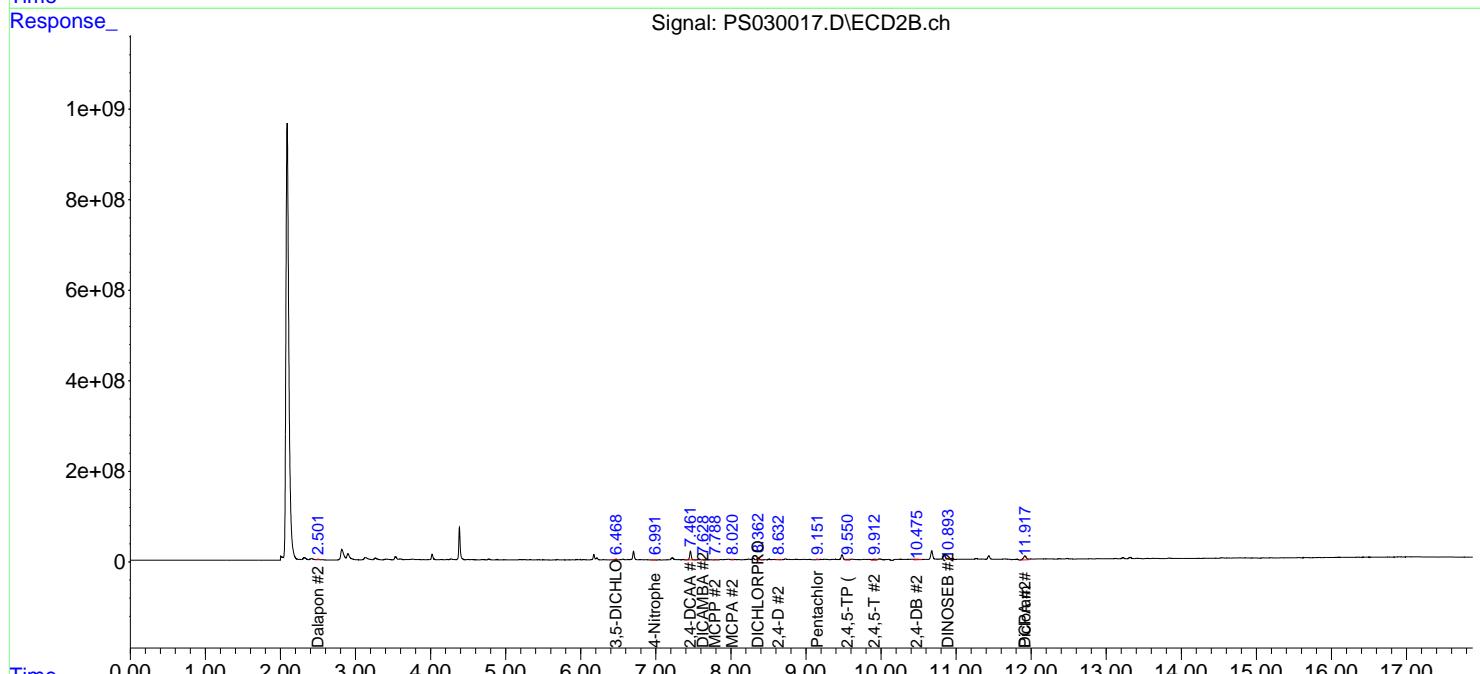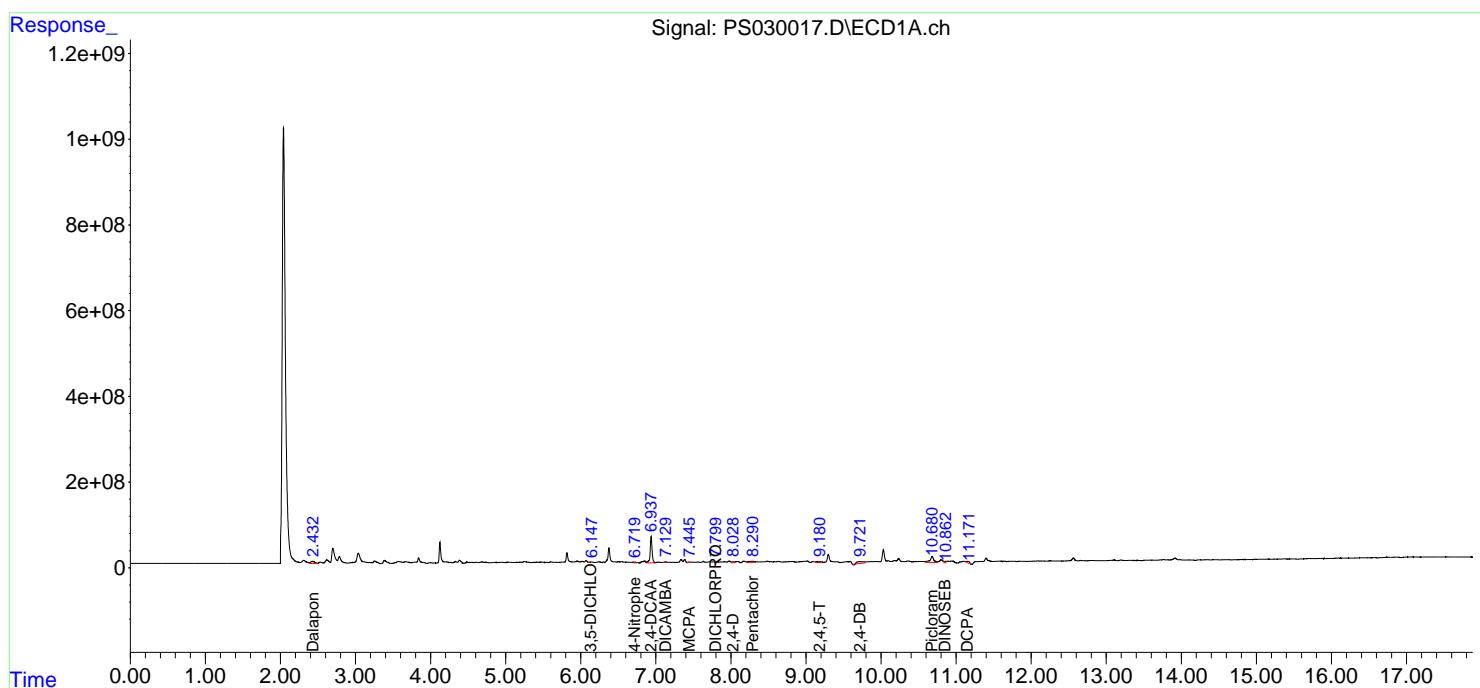

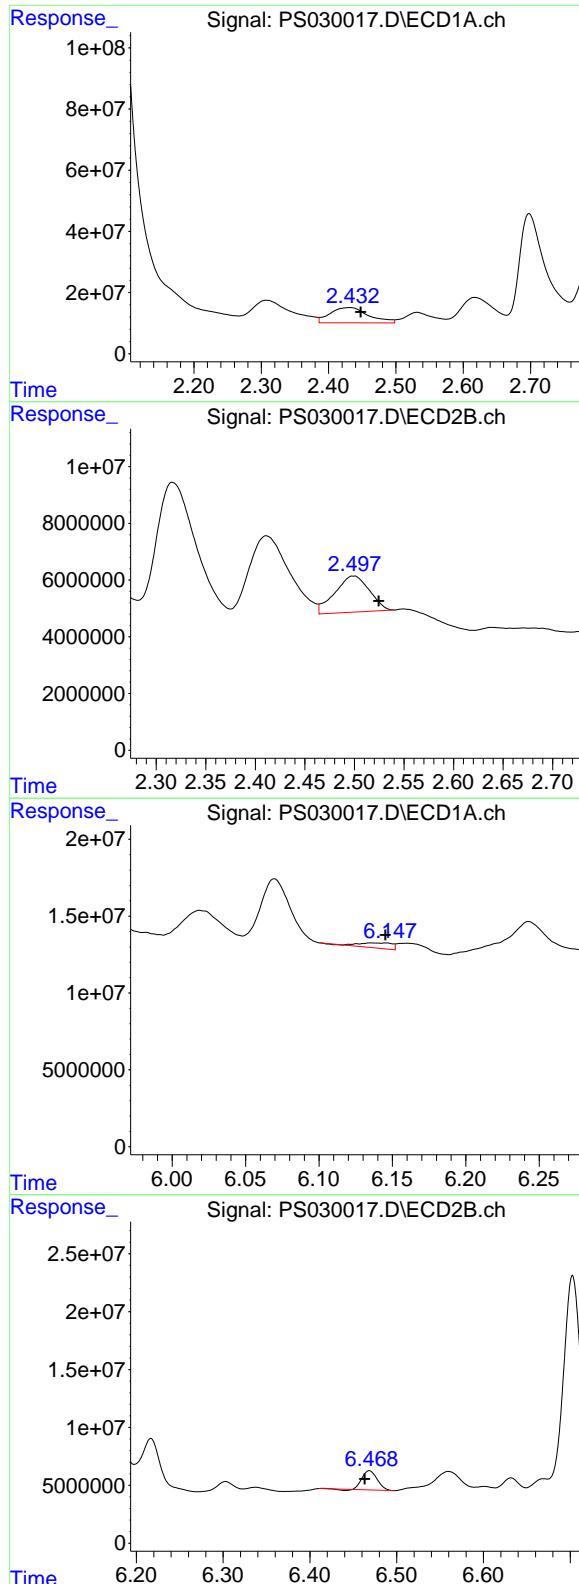

#1 Dalapon

R.T.: 2.432 min  
Delta R.T.: -0.016 min  
Response: 198456442  
Conc: 48.46 ng/ml

Instrument: ECD\_S  
ClientSampleId: Q1883-Herbicide Group1

#1 Dalapon


R.T.: 2.499 min  
Delta R.T.: -0.025 min  
Response: 30851519  
Conc: 17.77 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.136 min  
Delta R.T.: -0.010 min  
Response: 5065169  
Conc: 1.42 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.469 min  
Delta R.T.: 0.005 min  
Response: 19736620  
Conc: 20.19 ng/ml

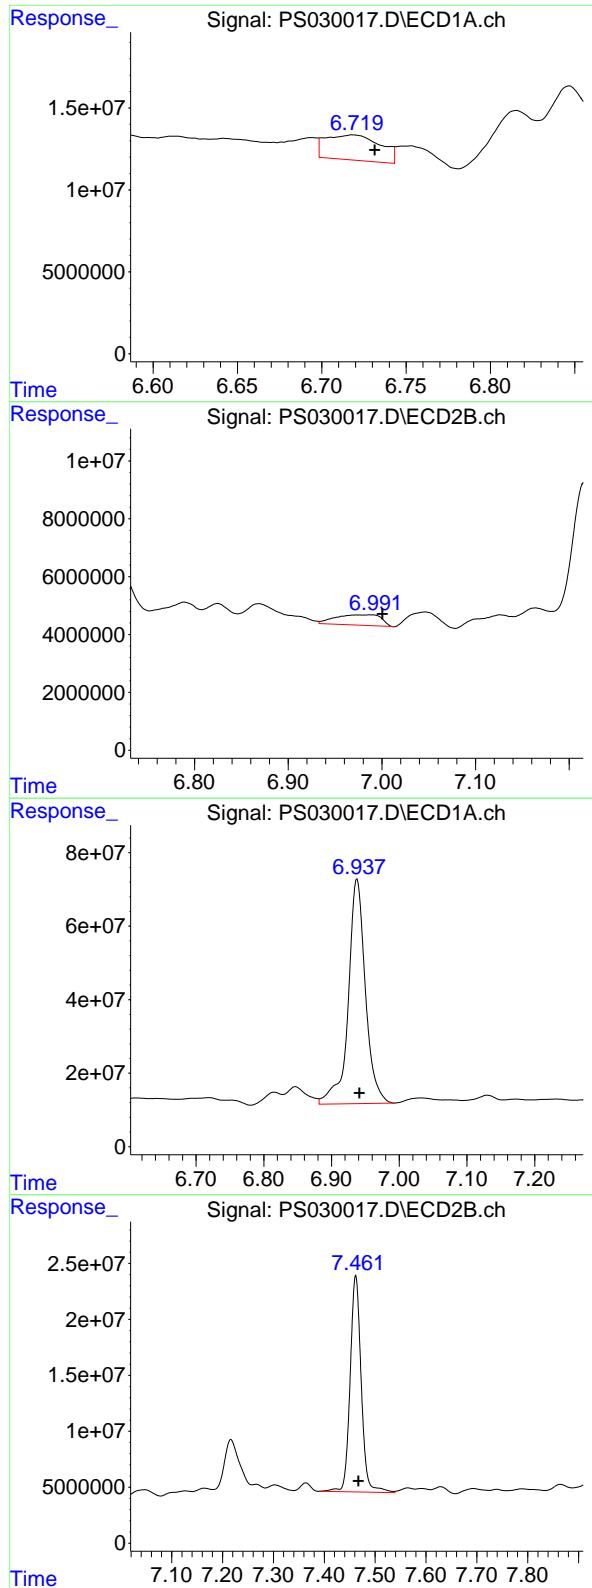

#3 4-Nitrophenol

R.T.: 6.719 min  
 Delta R.T.: -0.013 min  
 Response: 34601750  
 Conc: 19.40 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** OU4-PCS-TC-27-042325

#3 4-Nitrophenol


R.T.: 6.988 min  
 Delta R.T.: -0.013 min  
 Response: 12204445  
 Conc: 15.93 ng/ml

#4 2,4-DCAA

R.T.: 6.938 min  
 Delta R.T.: -0.004 min  
 Response: 1078133489  
 Conc: 438.07 ng/ml

#4 2,4-DCAA


R.T.: 7.462 min  
 Delta R.T.: -0.005 min  
 Response: 292978773  
 Conc: 415.86 ng/ml

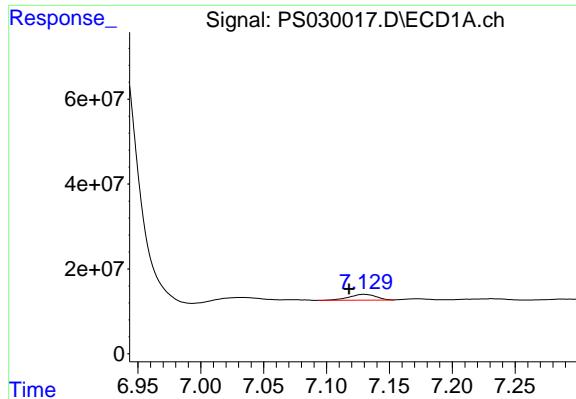

#5 DICAMBA


R.T.: 7.130 min  
 Delta R.T.: 0.012 min  
 Response: 20840115  
 Conc: 2.10 ng/ml

Instrument: ECD\_S  
 ClientSampleId: Q1883-Herbicide Group1

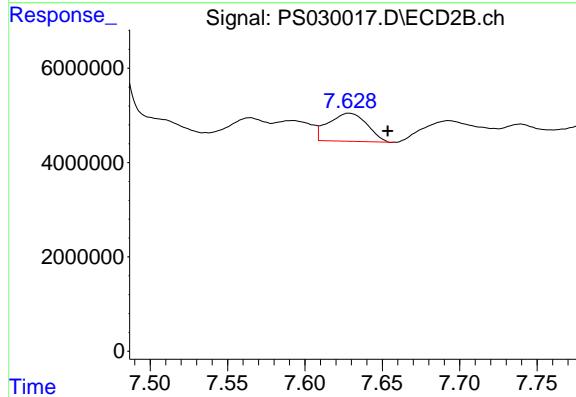


#5 DICAMBA

R.T.: 7.629 min  
 Delta R.T.: -0.025 min  
 Response: 10292797  
 Conc: 2.61 ng/ml

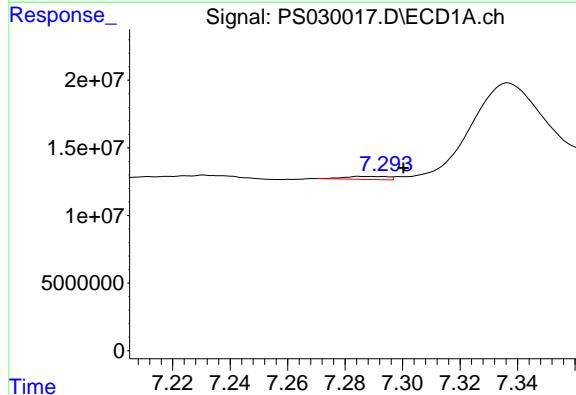


#6 MCPP

R.T.: 7.286 min  
 Delta R.T.: -0.015 min  
 Response: 2374565  
 Conc: N.D.

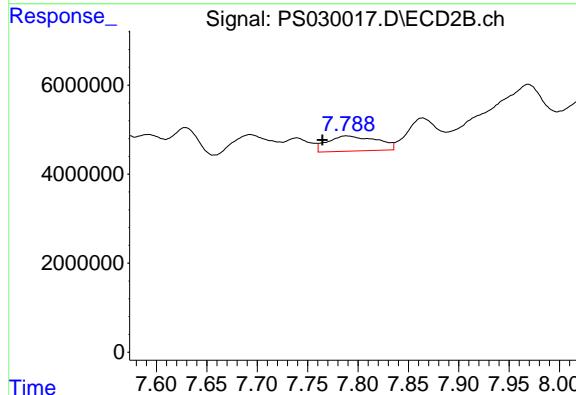

#6 MCPP

R.T.: 7.789 min  
 Delta R.T.: 0.024 min  
 Response: 11599435  
 Conc: 6.63 ug/ml

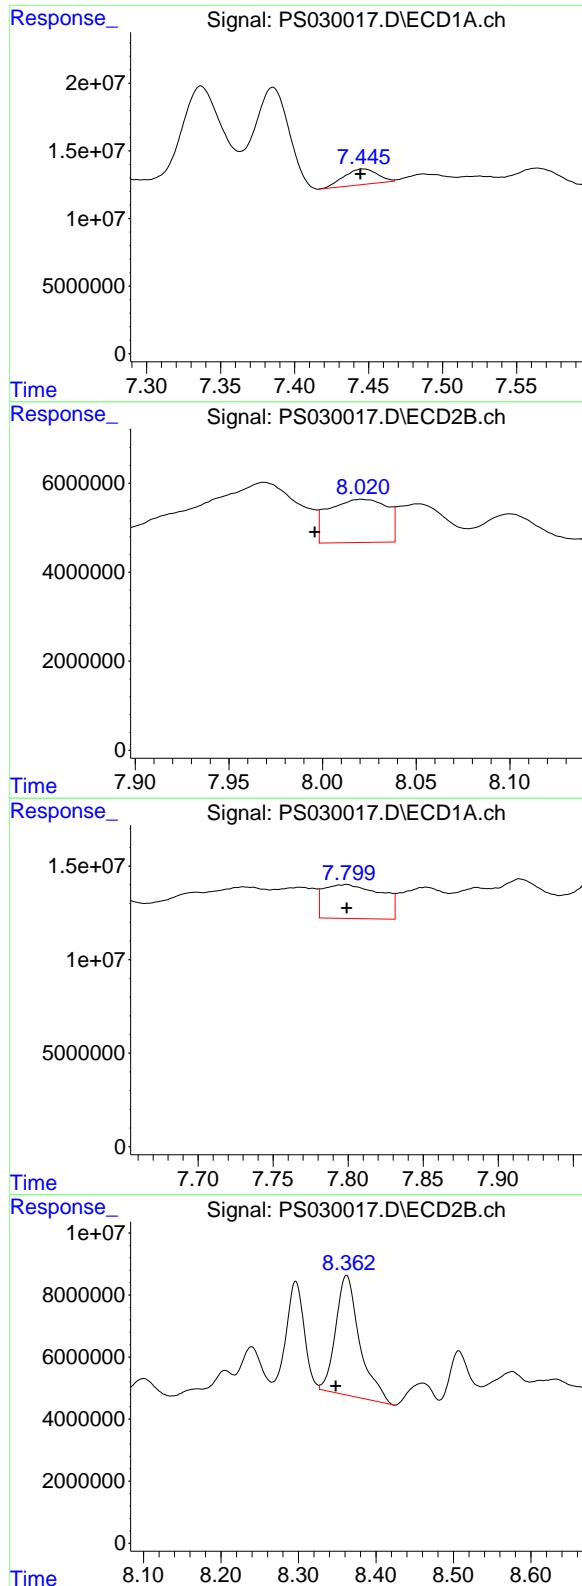

#7 MCPA

R.T.: 7.446 min  
 Delta R.T.: 0.002 min  
 Response: 18185276  
 Conc: 2.06 ug/ml

Instrument: ECD\_S  
 ClientSampleId: OU4-PCS-TC-27-042325

#7 MCPA


R.T.: 8.021 min  
 Delta R.T.: 0.025 min  
 Response: 21087650  
 Conc: 8.91 ug/ml

#8 DICHLOPROP

R.T.: 7.799 min  
 Delta R.T.: 0.000 min  
 Response: 48423986  
 Conc: 19.11 ng/ml

#8 DICHLOPROP

R.T.: 8.362 min  
 Delta R.T.: 0.014 min  
 Response: 83292801  
 Conc: 82.96 ng/ml

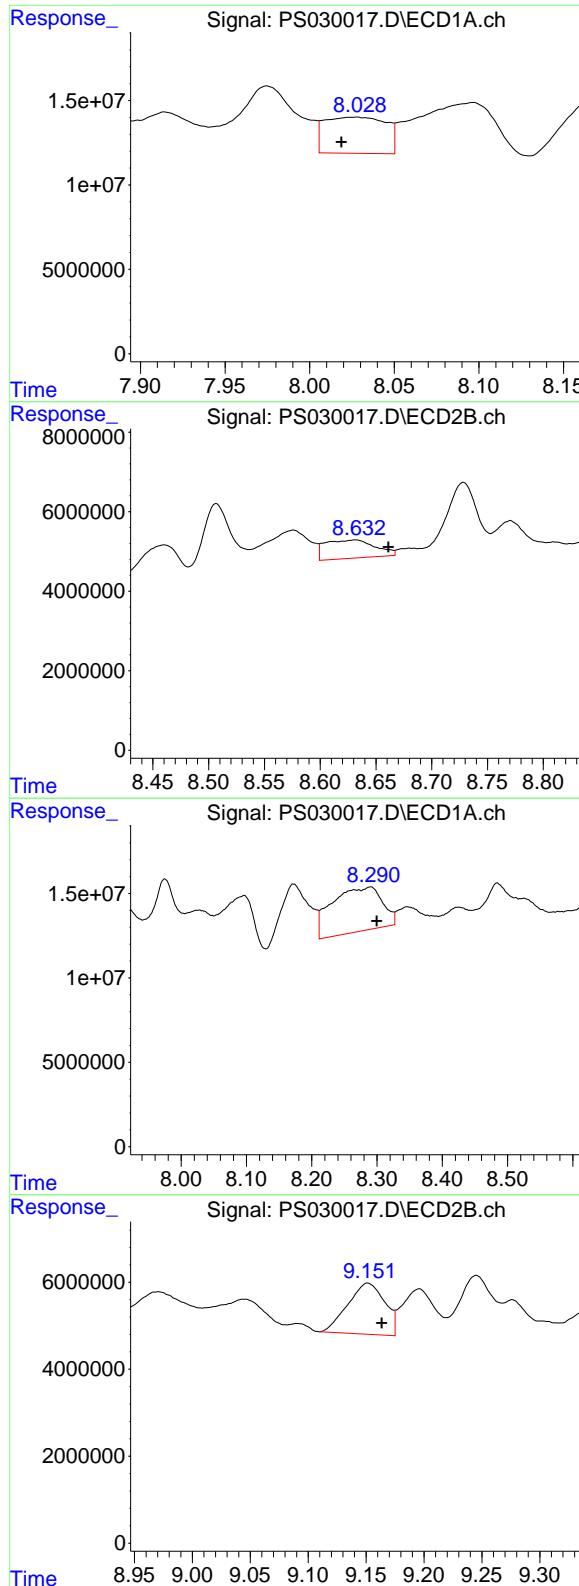

#9 2,4-D

R.T.: 8.027 min  
 Delta R.T.: 0.009 min  
 Response: 54131730  
 Conc: 19.24 ng/ml

Instrument: ECD\_S  
 ClientSampleId: OU4-PCS-TC-27-042325

#9 2,4-D


R.T.: 8.631 min  
 Delta R.T.: -0.030 min  
 Response: 14339780  
 Conc: 12.72 ng/ml

#10 Pentachlorophenol

R.T.: 8.290 min  
 Delta R.T.: -0.009 min  
 Response: 140338157  
 Conc: 4.02 ng/ml

#10 Pentachlorophenol

R.T.: 9.152 min  
 Delta R.T.: -0.012 min  
 Response: 26158906  
 Conc: 1.29 ng/ml

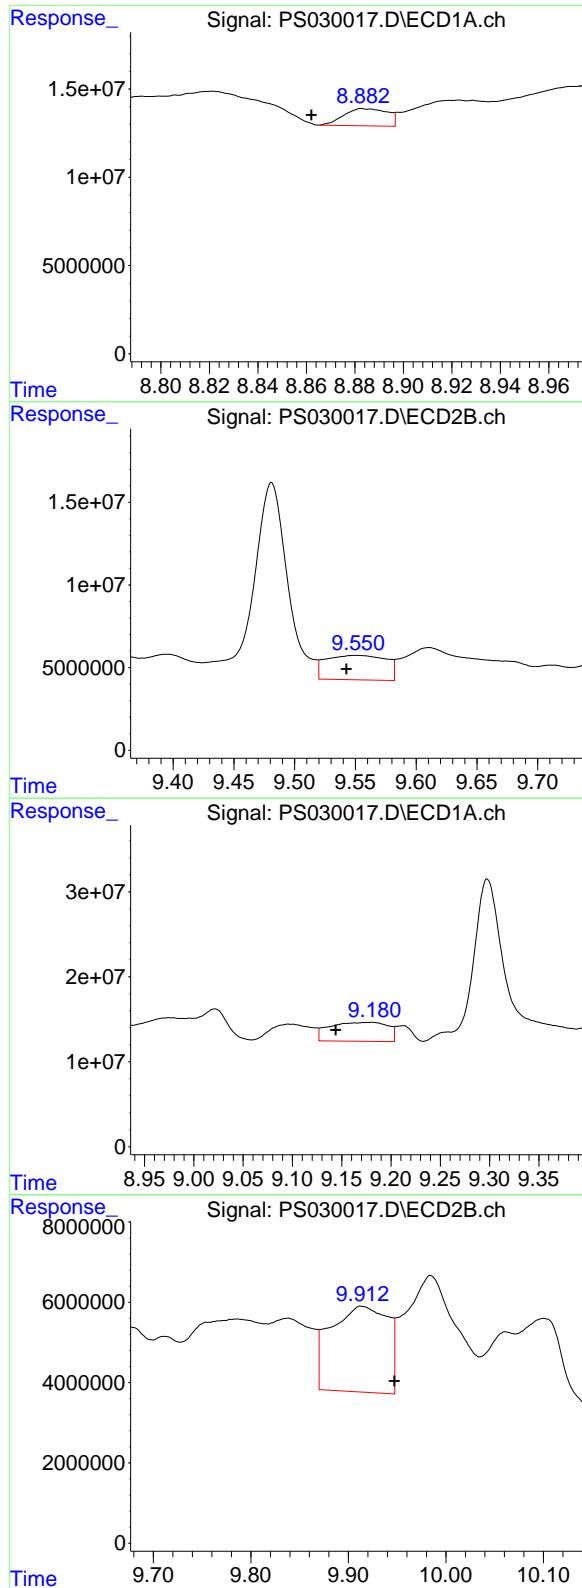

#11 2,4,5-TP (SILVEX)

R.T.: 8.883 min  
 Delta R.T.: 0.021 min  
 Response: 12123631  
 Conc: N.D.

**Instrument:** ECD\_S  
**ClientSampleId:** OU4-PCS-TC-27-042325

#11 2,4,5-TP (SILVEX)


R.T.: 9.550 min  
 Delta R.T.: 0.008 min  
 Response: 50827137  
 Conc: 6.21 ng/ml

#12 2,4,5-T

R.T.: 9.181 min  
 Delta R.T.: 0.037 min  
 Response: 91226312  
 Conc: 6.49 ng/ml

#12 2,4,5-T

R.T.: 9.914 min  
 Delta R.T.: -0.034 min  
 Response: 86813759  
 Conc: 11.18 ng/ml

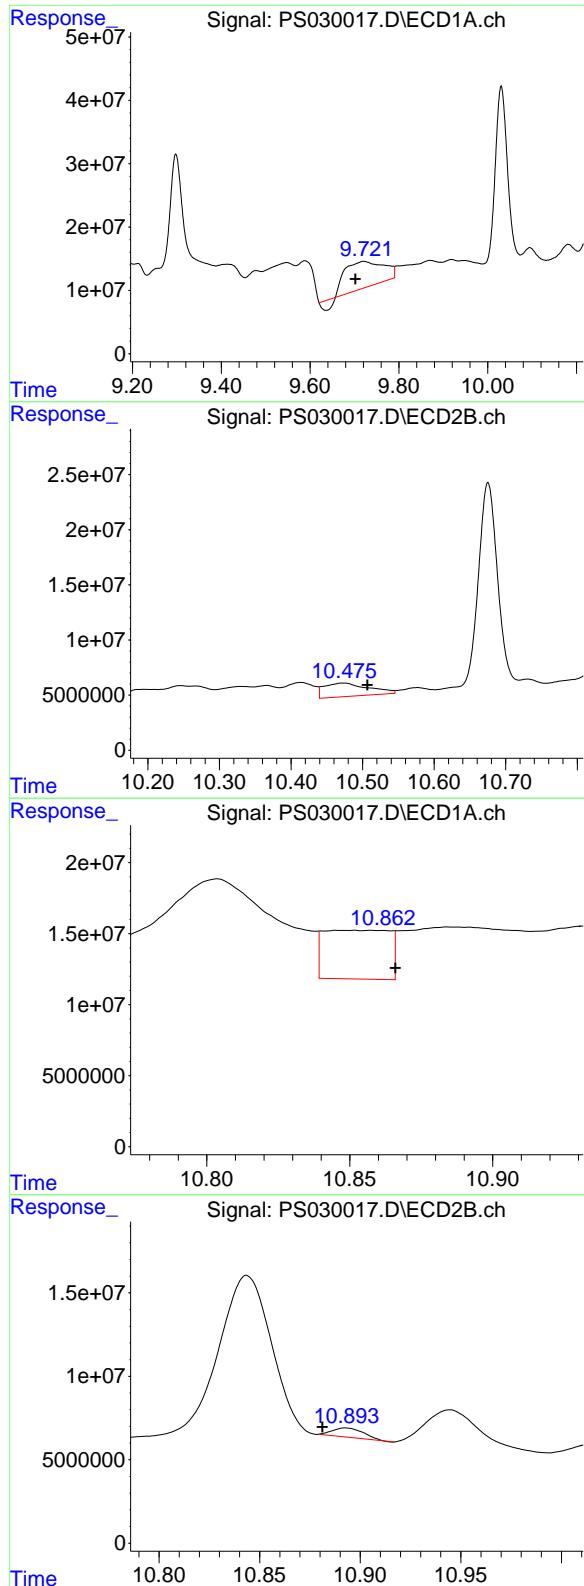

#13 2,4-DB

R.T.: 9.720 min  
 Delta R.T.: 0.018 min  
 Response: 232323707  
 Conc: 101.66 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** OU4-PCS-TC-27-042325

#13 2,4-DB


R.T.: 10.473 min  
 Delta R.T.: -0.034 min  
 Response: 52968504  
 Conc: 65.81 ng/ml

#14 DINOSEB

R.T.: 10.851 min  
 Delta R.T.: -0.015 min  
 Response: 54420857  
 Conc: 5.35 ng/ml

#14 DINOSEB

R.T.: 10.893 min  
 Delta R.T.: 0.012 min  
 Response: 5942261  
 Conc: 1.02 ng/ml

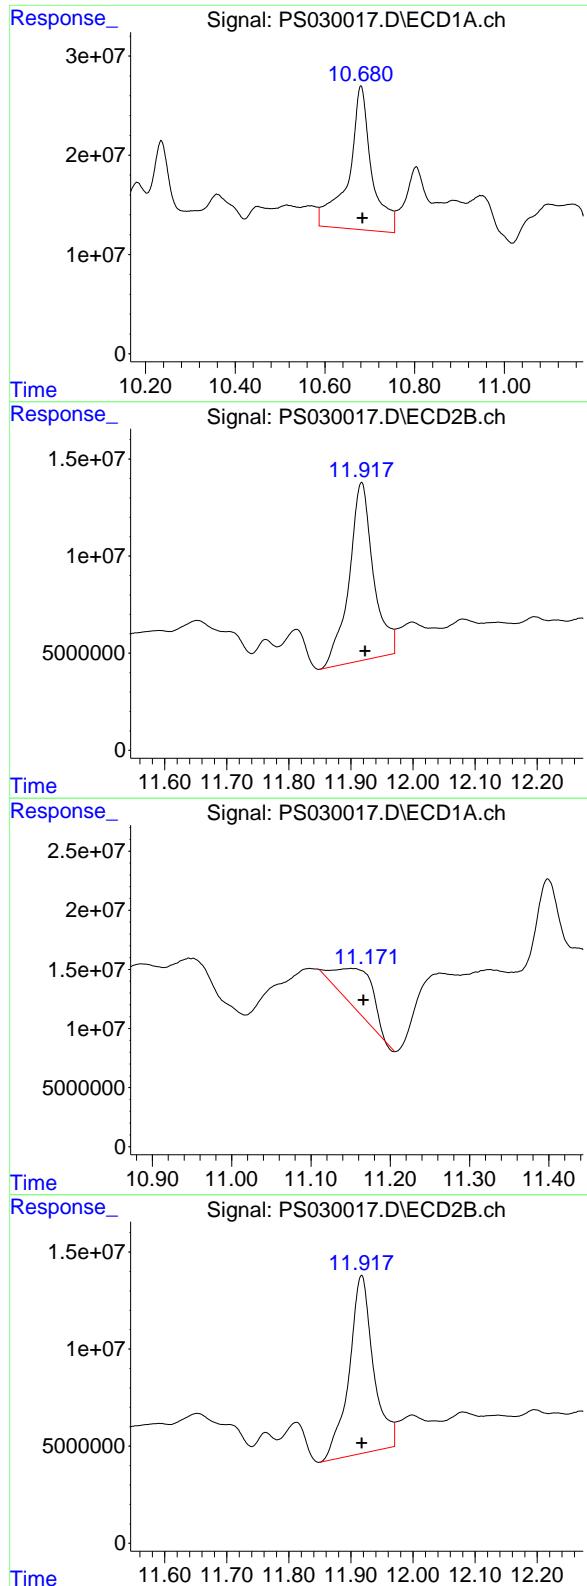

#15 Picloram

R.T.: 10.680 min  
 Delta R.T.: -0.003 min  
 Response: 520392778  
 Conc: 28.39 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** OU4-PCS-TC-27-042325

#15 Picloram

R.T.: 11.917 min  
 Delta R.T.: -0.006 min  
 Response: 249965755  
 Conc: 20.35 ng/ml

#16 DCPA

R.T.: 11.151 min  
 Delta R.T.: -0.015 min  
 Response: 109033727  
 Conc: 6.41 ng/ml

#16 DCPA

R.T.: 11.917 min  
 Delta R.T.: 0.000 min  
 Response: 249965755  
 Conc: 22.18 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030018.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 14:15  
 Operator : AR\AJ  
 Sample : Q1983-03  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**OU4-PCS-TC-28-042325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:28:39 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.938 7.462 880.7E6 241.3E6 357.869 342.520

Target Compounds

1) T	Dalapon	2.433	2.500	241.1E6	155.8E6	58.872	89.727 #
2) T	3,5-DICHL...	6.160	6.468	13818390	3115871	3.867	3.187
3) T	4-Nitroph...	6.723	6.991	28819651	7553129	16.161	9.861 #
5) T	DICAMBA	7.129	7.629	3320906	8767724	<MDL	2.220 #
6) T	MCPP	7.336f	7.740	200.4E6	2585095	31.104	1.478 #
7) T	MCPA	7.446	7.968f	25321584	49645689	2.867	20.985 #
8) T	DICHLORPROP	7.801	8.361	17331087	86121013	6.839	85.781 #
9) T	2,4-D	8.031	8.652	24834517	4518274	8.829	4.009 #
10) T	Pentachlo...	8.291	9.152	79060471	22504972	2.266	1.106 #
11) T	2,4,5-TP ...	8.848	0.000	2382231	0	<MDL	N.D. #
12) T	2,4,5-T	9.160	9.981f	81848958	84007451	5.824	10.822 #
13) T	2,4-DB	9.721	10.463f	176.4E6	90222853	77.208	112.100 #
14) T	DINOSEB	10.849	10.843f	106.9E6	158.2E6	10.508	27.132 #
15) T	Picloram	10.680	11.921	212.4E6	134.8E6	11.587	10.973
16) T	DCPA	11.154	11.921	96251824	134.8E6	5.655	11.958 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030018.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 14:15  
 Operator : AR\AJ  
 Sample : Q1983-03  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**OU4-PCS-TC-28-042325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:28:39 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

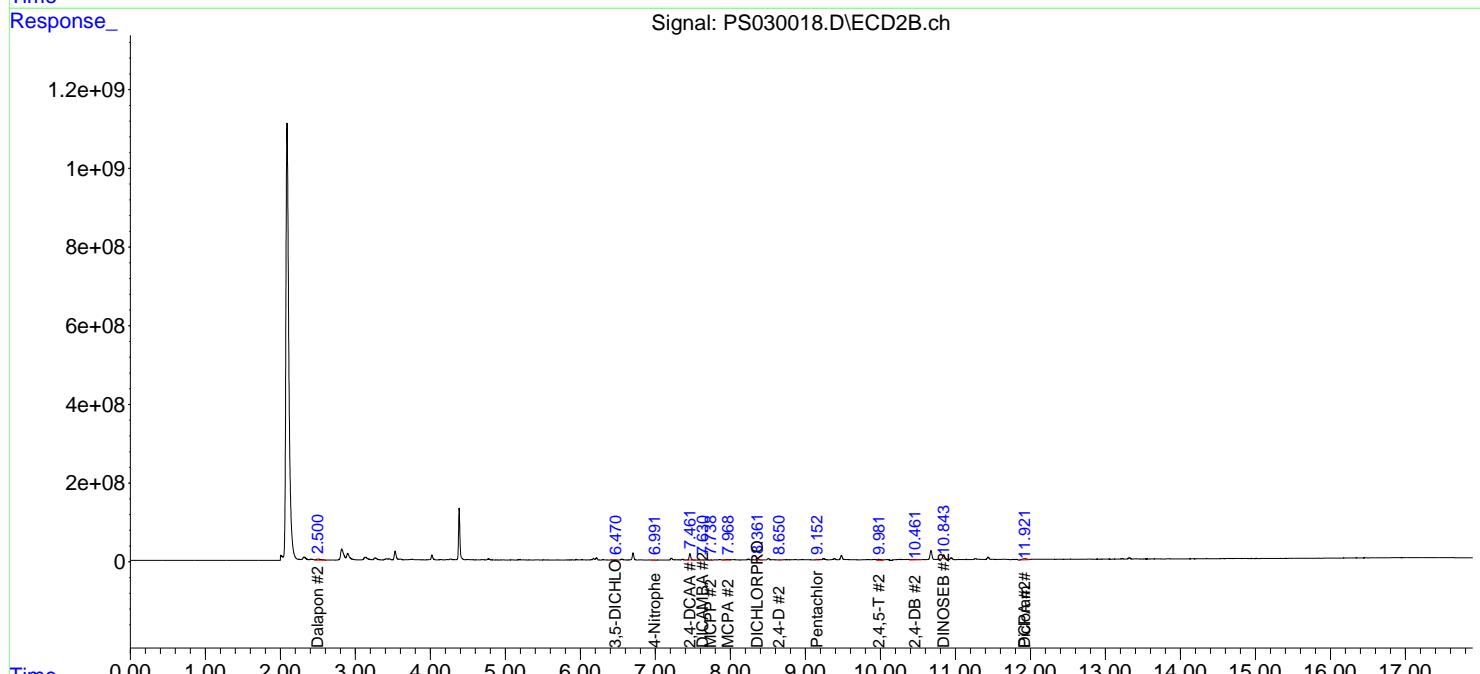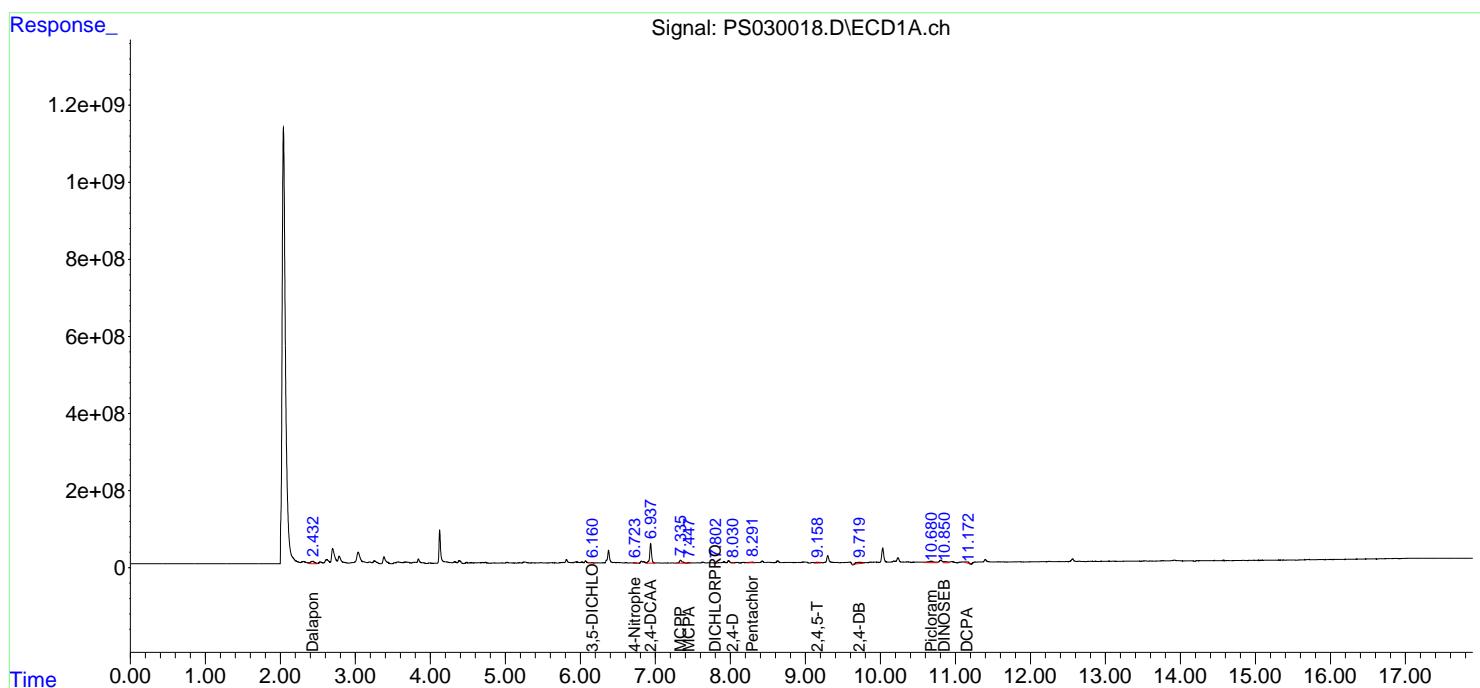


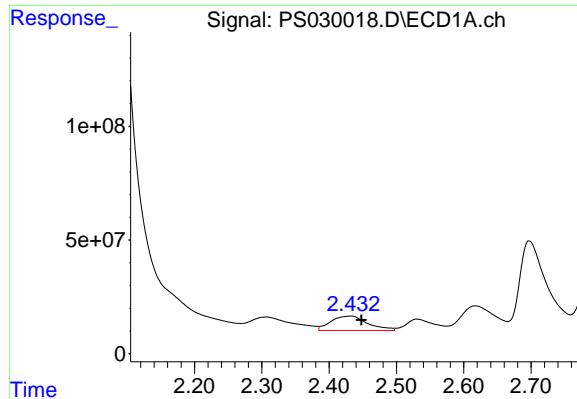

#1 Dalapon


R.T.: 2.433 min  
Delta R.T.: -0.015 min  
Response: 241097359  
Conc: 58.87 ng/ml

Instrument: ECD\_S  
ClientSampleId: Q4-PCS-TC-28-042325

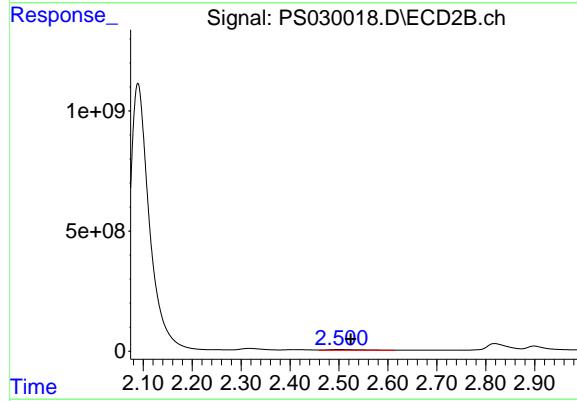


#1 Dalapon

R.T.: 2.500 min  
Delta R.T.: -0.024 min  
Response: 155778371  
Conc: 89.73 ng/ml

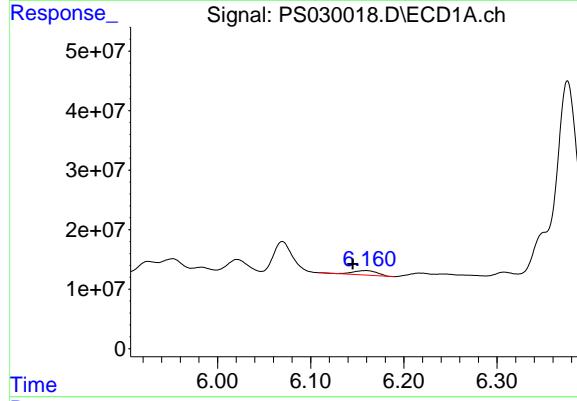


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.160 min  
Delta R.T.: 0.014 min  
Response: 13818390  
Conc: 3.87 ng/ml

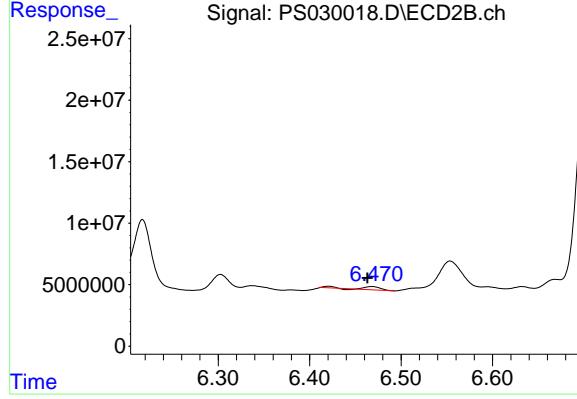

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.468 min  
Delta R.T.: 0.005 min  
Response: 3115871  
Conc: 3.19 ng/ml

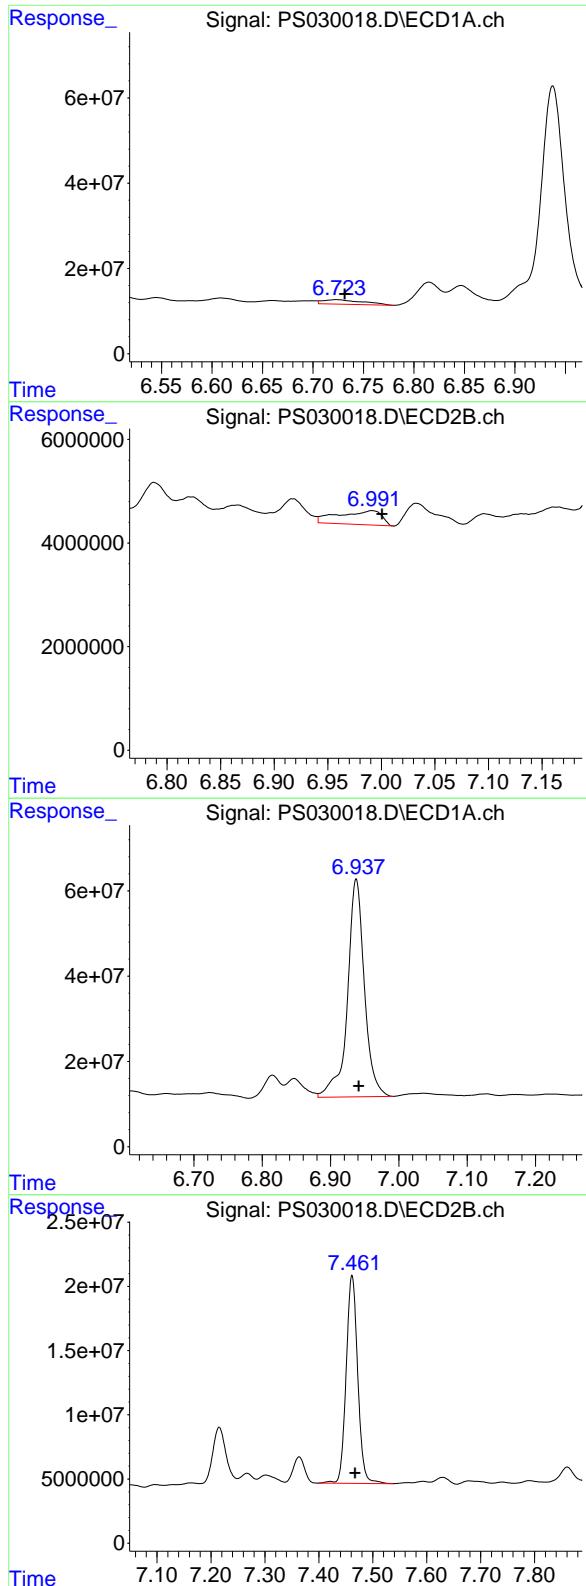

#3 4-Nitrophenol

R.T.: 6.723 min  
 Delta R.T.: -0.008 min  
 Response: 28819651  
 Conc: 16.16 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** OU4-PCS-TC-28-042325

#3 4-Nitrophenol


R.T.: 6.991 min  
 Delta R.T.: -0.009 min  
 Response: 7553129  
 Conc: 9.86 ng/ml

#4 2,4-DCAA

R.T.: 6.938 min  
 Delta R.T.: -0.004 min  
 Response: 880743174  
 Conc: 357.87 ng/ml

#4 2,4-DCAA


R.T.: 7.462 min  
 Delta R.T.: -0.005 min  
 Response: 241311020  
 Conc: 342.52 ng/ml

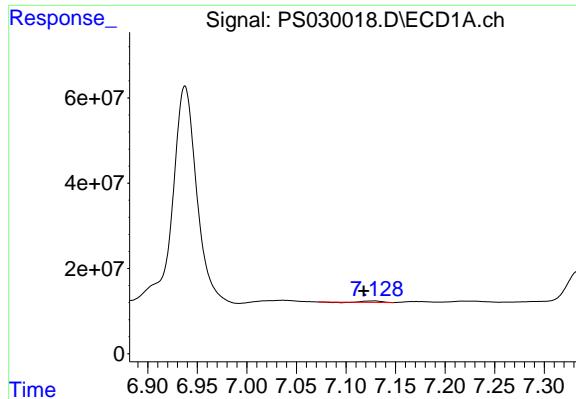

#5 DICAMBA


R.T.: 7.129 min  
Delta R.T.: 0.011 min  
Response: 3320906  
Conc: N.D.

Instrument: ECD\_S  
ClientSampleId: OU4-PCS-TC-28-042325

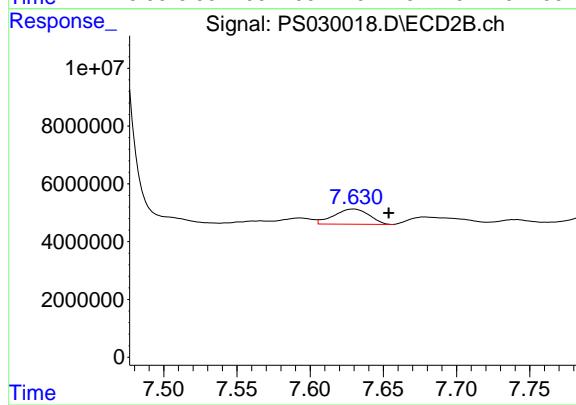


#5 DICAMBA

R.T.: 7.629 min  
Delta R.T.: -0.024 min  
Response: 8767724  
Conc: 2.22 ng/ml

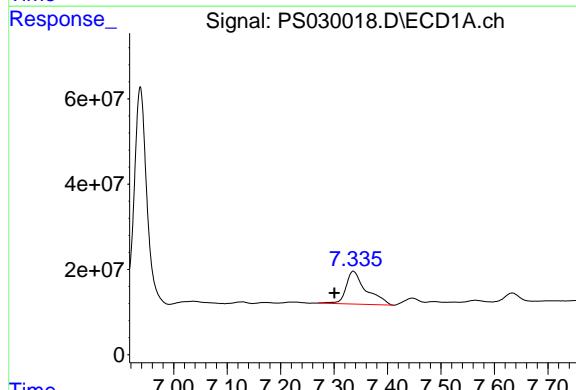


#6 MCPP

R.T.: 7.336 min  
Delta R.T.: 0.036 min  
Response: 200419917  
Conc: 31.10 ug/ml

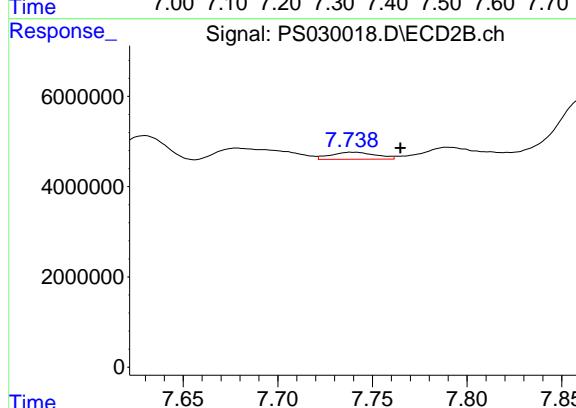

#6 MCPP


R.T.: 7.740 min  
Delta R.T.: -0.025 min  
Response: 2585095  
Conc: 1.48 ug/ml

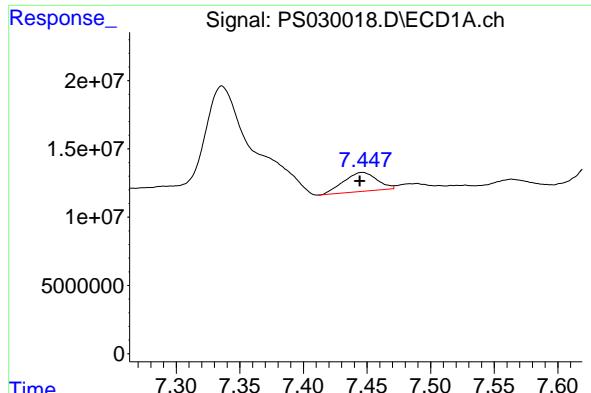

#7 MCPA


R.T.: 7.446 min  
 Delta R.T.: 0.002 min  
 Response: 25321584  
 Conc: 2.87 ug/ml

Instrument: ECD\_S  
 ClientSampleId: OU4-PCS-TC-28-042325

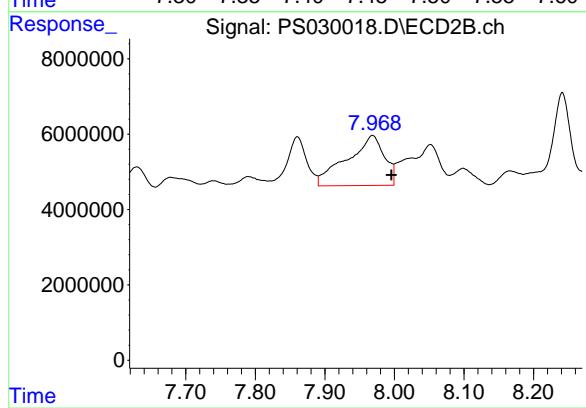


#7 MCPA

R.T.: 7.968 min  
 Delta R.T.: -0.027 min  
 Response: 49645689  
 Conc: 20.98 ug/ml

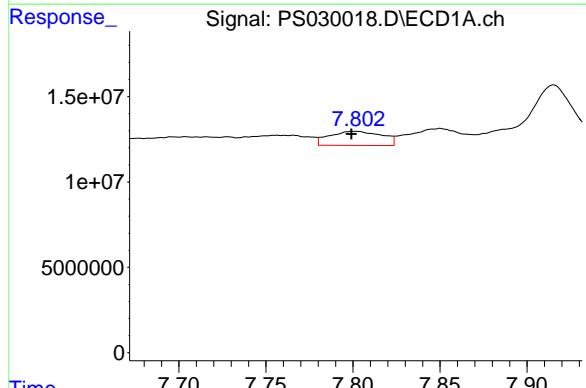


#8 DICHLOPROP

R.T.: 7.801 min  
 Delta R.T.: 0.002 min  
 Response: 17331087  
 Conc: 6.84 ng/ml

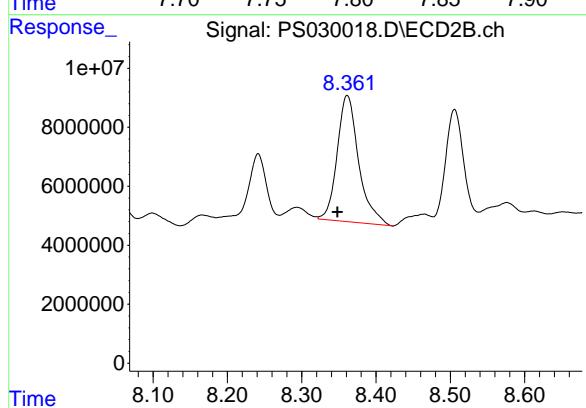


#8 DICHLOPROP


R.T.: 8.361 min  
 Delta R.T.: 0.013 min  
 Response: 86121013  
 Conc: 85.78 ng/ml

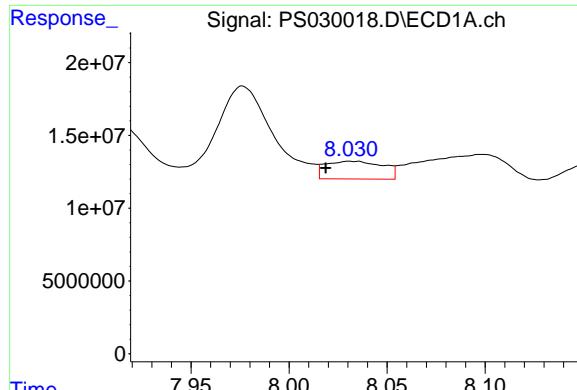


#9 2,4-D  
R.T.: 8.031 min  
Delta R.T.: 0.012 min  
Response: 24834517  
Conc: 8.83 ng/ml  
**Instrument:** ECD\_S  
**ClientSampleId:** OU4-PCS-TC-28-042325

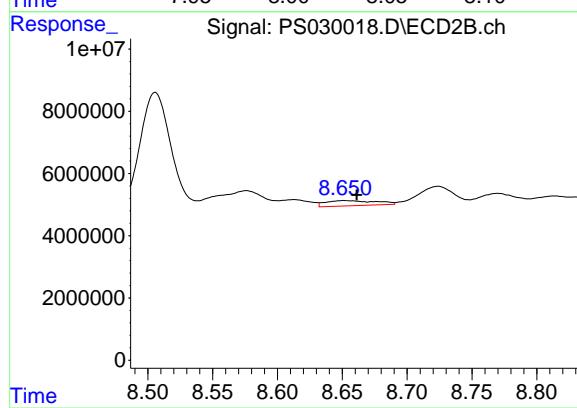


#9 2,4-D  
R.T.: 8.652 min  
Delta R.T.: -0.009 min  
Response: 4518274  
Conc: 4.01 ng/ml

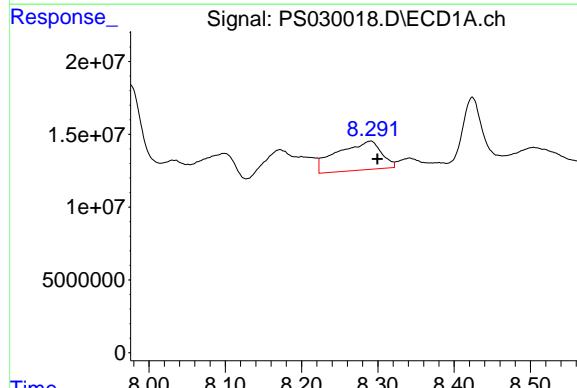

#10 Pentachlorophenol  
R.T.: 8.291 min  
Delta R.T.: -0.009 min  
Response: 79060471  
Conc: 2.27 ng/ml

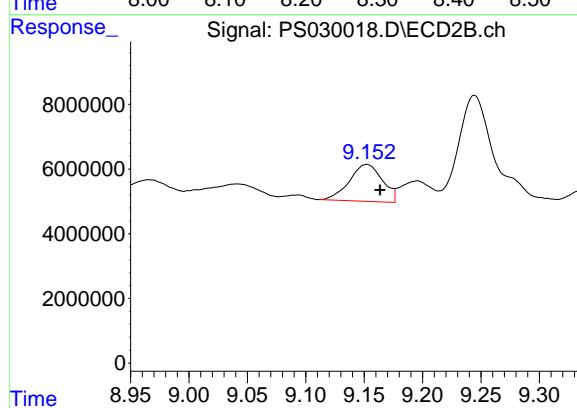

#10 Pentachlorophenol  
R.T.: 9.152 min  
Delta R.T.: -0.011 min  
Response: 22504972  
Conc: 1.11 ng/ml

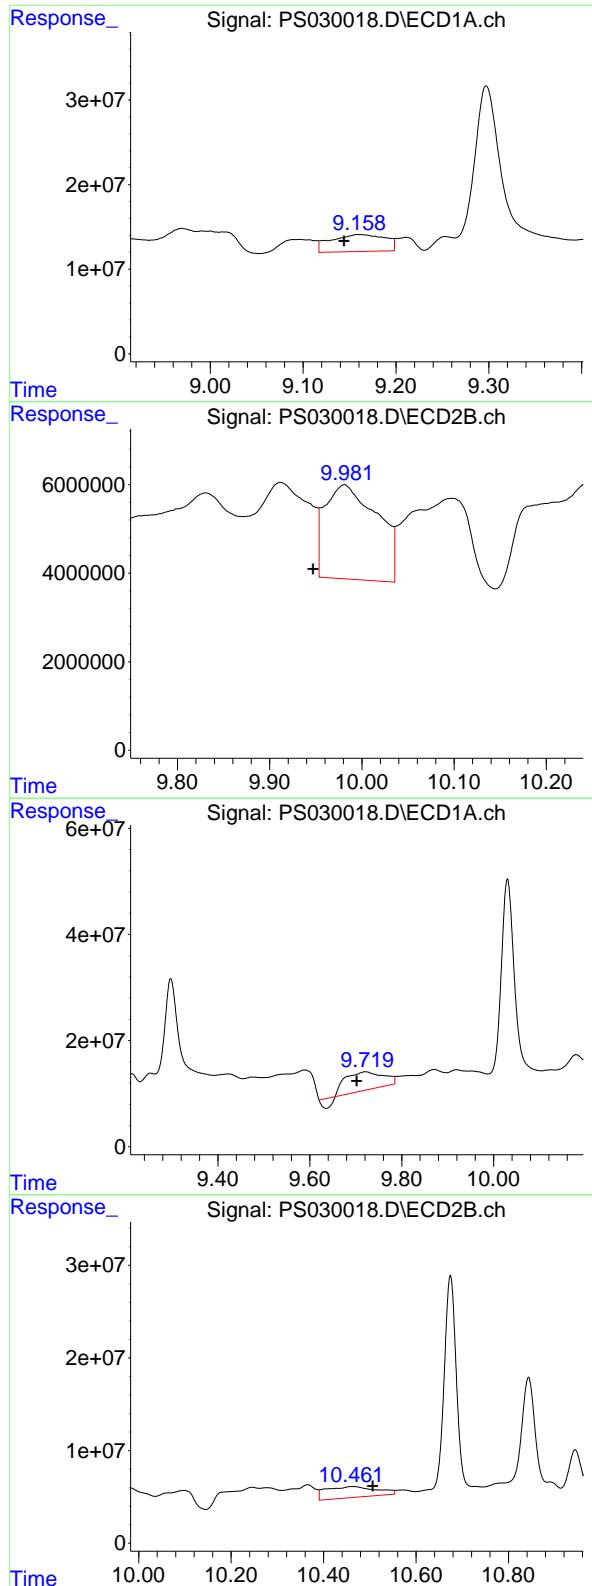

#12 2,4,5-T

R.T.: 9.160 min  
 Delta R.T.: 0.016 min  
 Response: 81848958  
 Conc: 5.82 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** OU4-PCS-TC-28-042325

#12 2,4,5-T


R.T.: 9.981 min  
 Delta R.T.: 0.034 min  
 Response: 84007451  
 Conc: 10.82 ng/ml

#13 2,4-DB

R.T.: 9.721 min  
 Delta R.T.: 0.019 min  
 Response: 176447167  
 Conc: 77.21 ng/ml

#13 2,4-DB

R.T.: 10.463 min  
 Delta R.T.: -0.044 min  
 Response: 90222853  
 Conc: 112.10 ng/ml

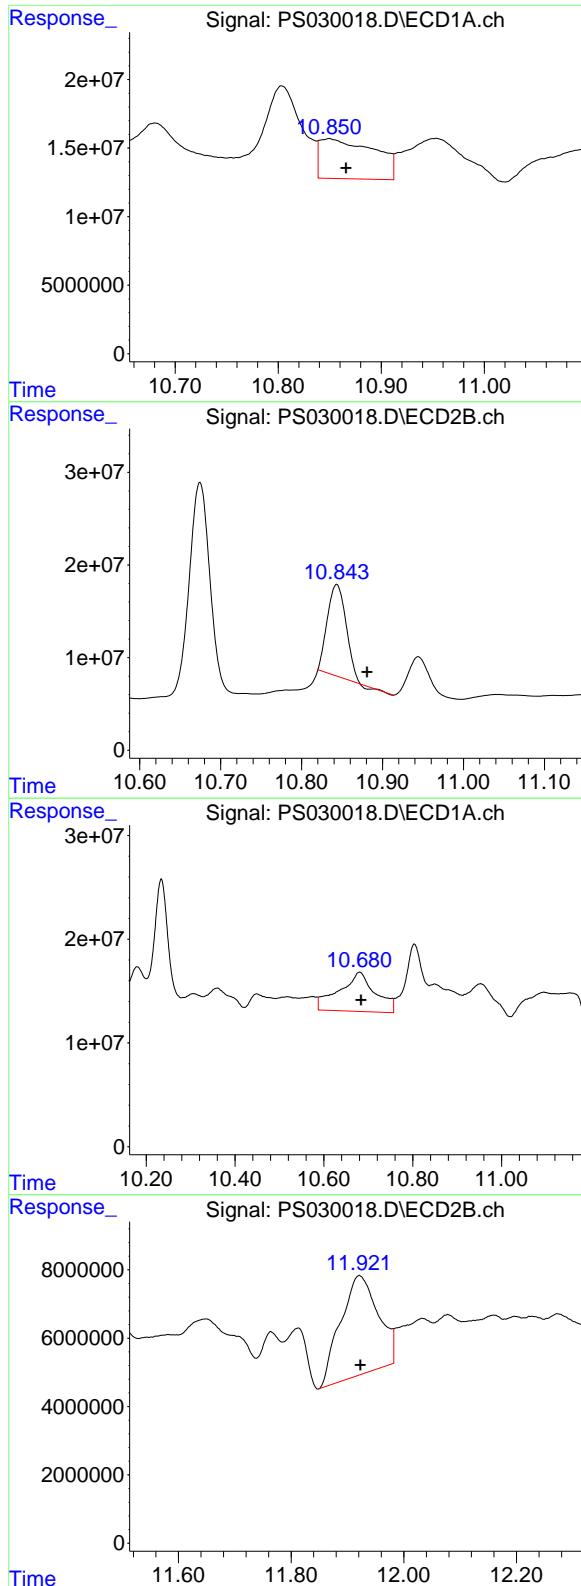

#14 DINOSEB

R.T.: 10.849 min  
 Delta R.T.: -0.017 min  
 Response: 106903416  
 Conc: 10.51 ng/ml

Instrument: ECD\_S  
 ClientSampleId: OU4-PCS-TC-28-042325

#14 DINOSEB


R.T.: 10.843 min  
 Delta R.T.: -0.038 min  
 Response: 158207178  
 Conc: 27.13 ng/ml

#15 Picloram

R.T.: 10.680 min  
 Delta R.T.: -0.003 min  
 Response: 212391053  
 Conc: 11.59 ng/ml

#15 Picloram

R.T.: 11.921 min  
 Delta R.T.: -0.002 min  
 Response: 134786278  
 Conc: 10.97 ng/ml

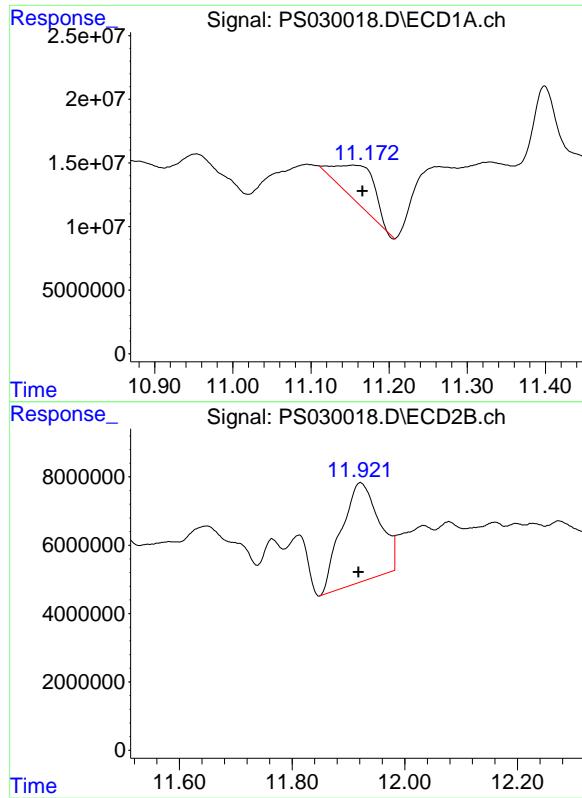

#16 DCPA

R.T.: 11.154 min  
 Delta R.T.: -0.012 min  
 Response: 96251824  
 Conc: 5.65 ng/ml

Instrument: ECD\_S  
 ClientSampleId: OU4-PCS-TC-28-042325

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030020.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 15:04  
 Operator : AR\AJ  
 Sample : Q1983-07  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**OU4-PCS-TC-30-042325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:29:04 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.938 7.461 939.5E6 250.4E6 381.738 355.382

Target Compounds

1) T	Dalapon	2.434	2.499	276.1E6	159.5E6	67.415	91.861 #
2) T	3,5-DICHL...	6.162	6.468	7741288	11003325	2.166	11.256 #
3) T	4-Nitroph...	6.723	6.982	46188406	19777464	25.900	25.822
5) T	DICAMBA	7.131	7.627f	44301703	17622450	4.474	4.461
6) T	MCPP	7.336f	7.741	166.5E6	3687325	25.837	2.108 #
7) T	MCPA	7.445	8.022f	9843728	34989917	1.115	14.790 #
8) T	DICHLORPROP	7.795	8.361	65892516	98492487	26.002	98.104 #
9) T	2,4-D	8.021	0.000	34475421	0	12.256	N.D. #
10) T	Pentachlo...	8.267f	9.150	101.5E6	16183448	2.910	<MDL #
11) T	2,4,5-TP ...	8.883	9.550	-475133	53425910	N.D.	6.530
12) T	2,4,5-T	9.175f	9.981f	95586070	81923977	6.802	10.554 #
13) T	2,4-DB	9.718	10.469f	240.3E6	50036189	105.136	62.169 #
14) T	DINOSEB	10.885	10.893	134.3E6	3605831	13.203	<MDL #
15) T	Picloram	10.682	11.928	130.7E6	111.3E6	7.132	9.065 #
16) T	DCPA	11.157	11.928	87839378	111.3E6	5.161	9.878 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030020.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 15:04  
 Operator : AR\AJ  
 Sample : Q1983-07  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**OU4-PCS-TC-30-042325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:29:04 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

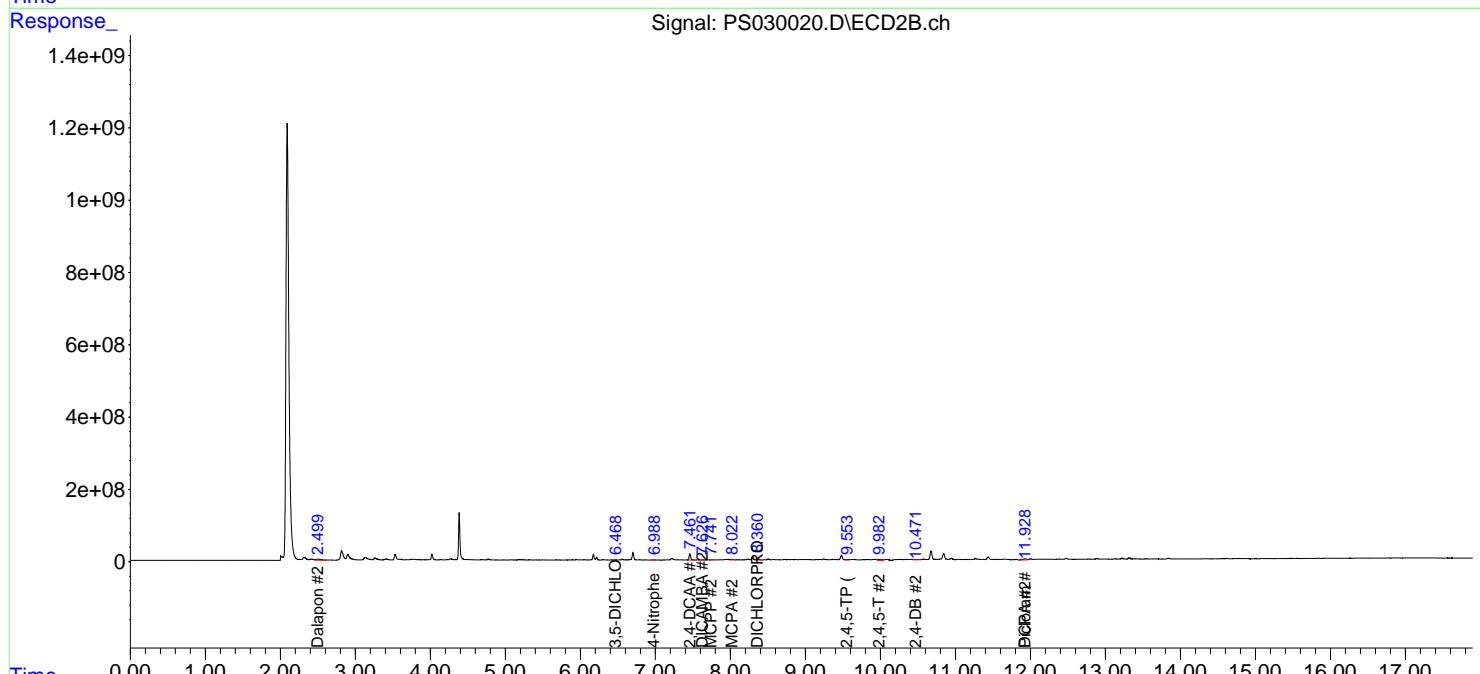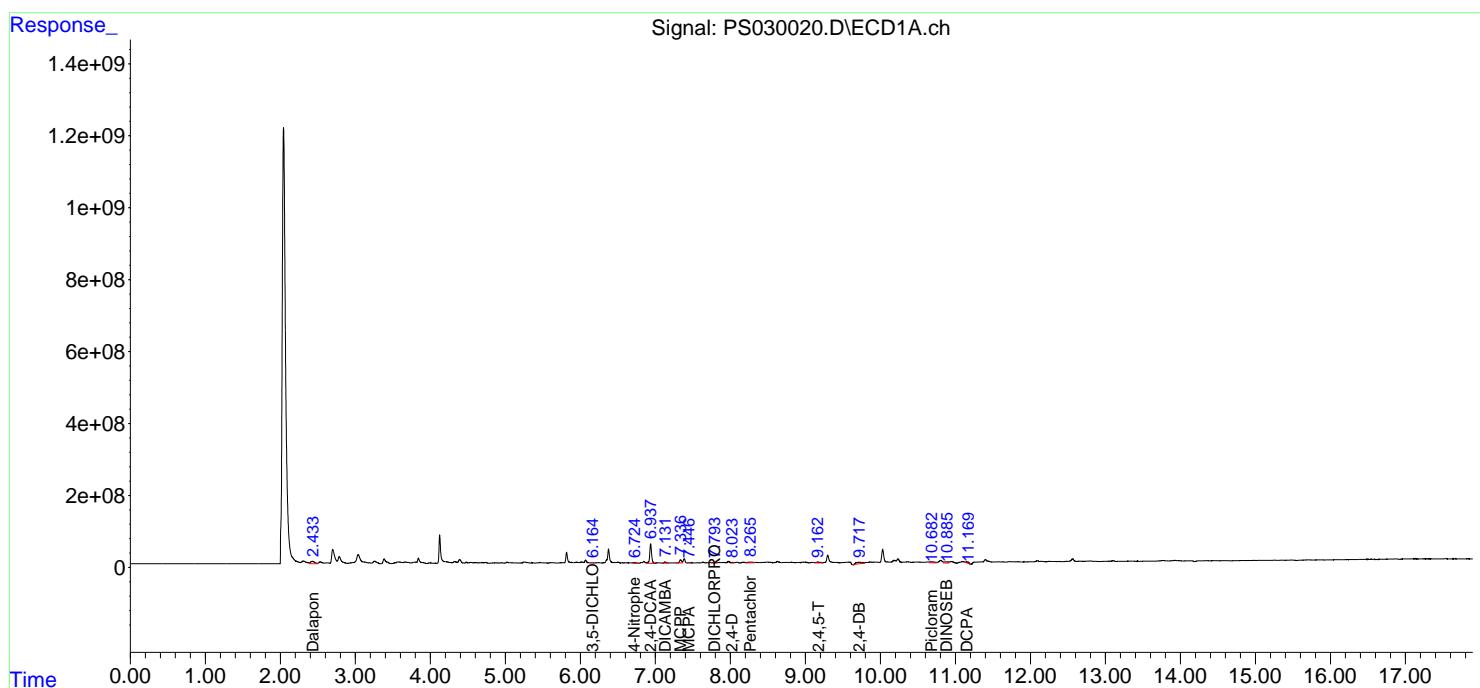

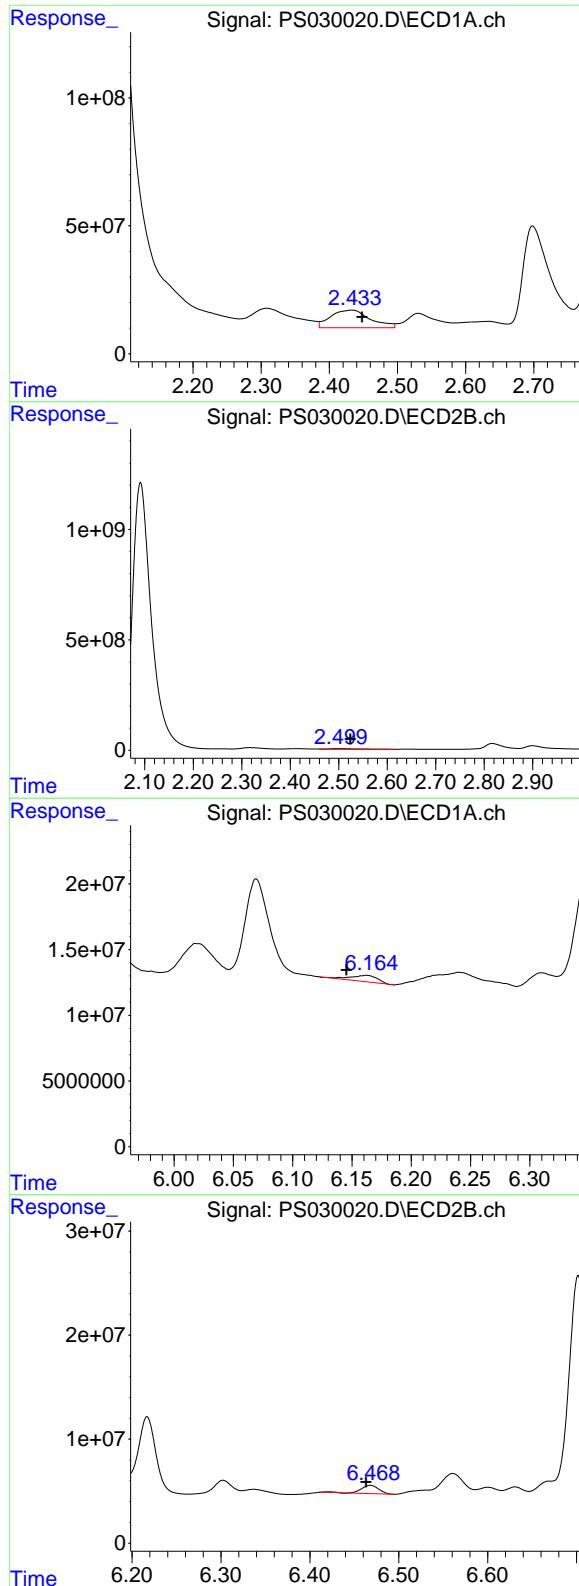

#1 Dalapon

R.T.: 2.434 min  
 Delta R.T.: -0.014 min  
 Response: 276080173  
 Conc: 67.41 ng/ml

Instrument: ECD\_S  
 ClientSampleId: Q1883-Herbicide Group1

#1 Dalapon


R.T.: 2.499 min  
 Delta R.T.: -0.025 min  
 Response: 159484228  
 Conc: 91.86 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.162 min  
 Delta R.T.: 0.017 min  
 Response: 7741288  
 Conc: 2.17 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.468 min  
 Delta R.T.: 0.005 min  
 Response: 11003325  
 Conc: 11.26 ng/ml

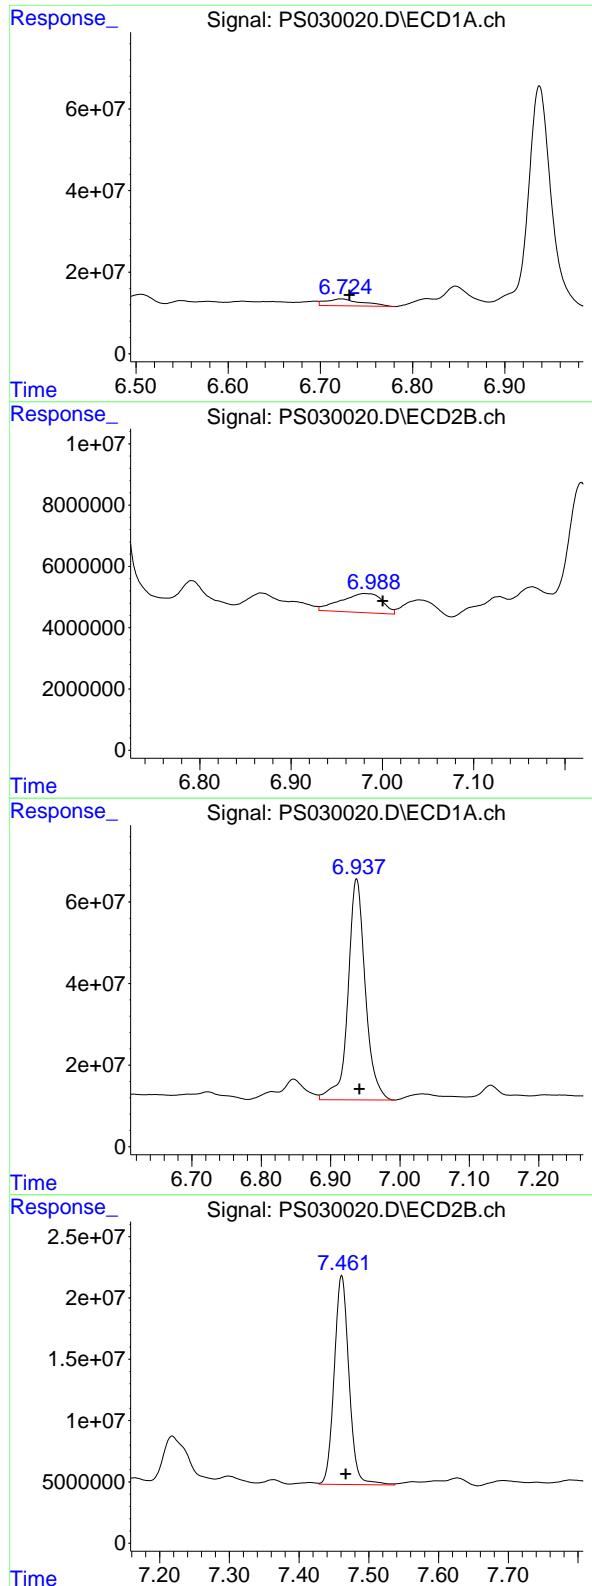

### #3 4-Nitrophenol

R.T.: 6.723 min  
 Delta R.T.: -0.009 min  
 Response: 46188406  
 Conc: 25.90 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** OU4-PCS-TC-30-042325

### #3 4-Nitrophenol


R.T.: 6.982 min  
 Delta R.T.: -0.019 min  
 Response: 19777464  
 Conc: 25.82 ng/ml

### #4 2,4-DCAA

R.T.: 6.938 min  
 Delta R.T.: -0.004 min  
 Response: 939487720  
 Conc: 381.74 ng/ml

### #4 2,4-DCAA

R.T.: 7.461 min  
 Delta R.T.: -0.006 min  
 Response: 250372814  
 Conc: 355.38 ng/ml

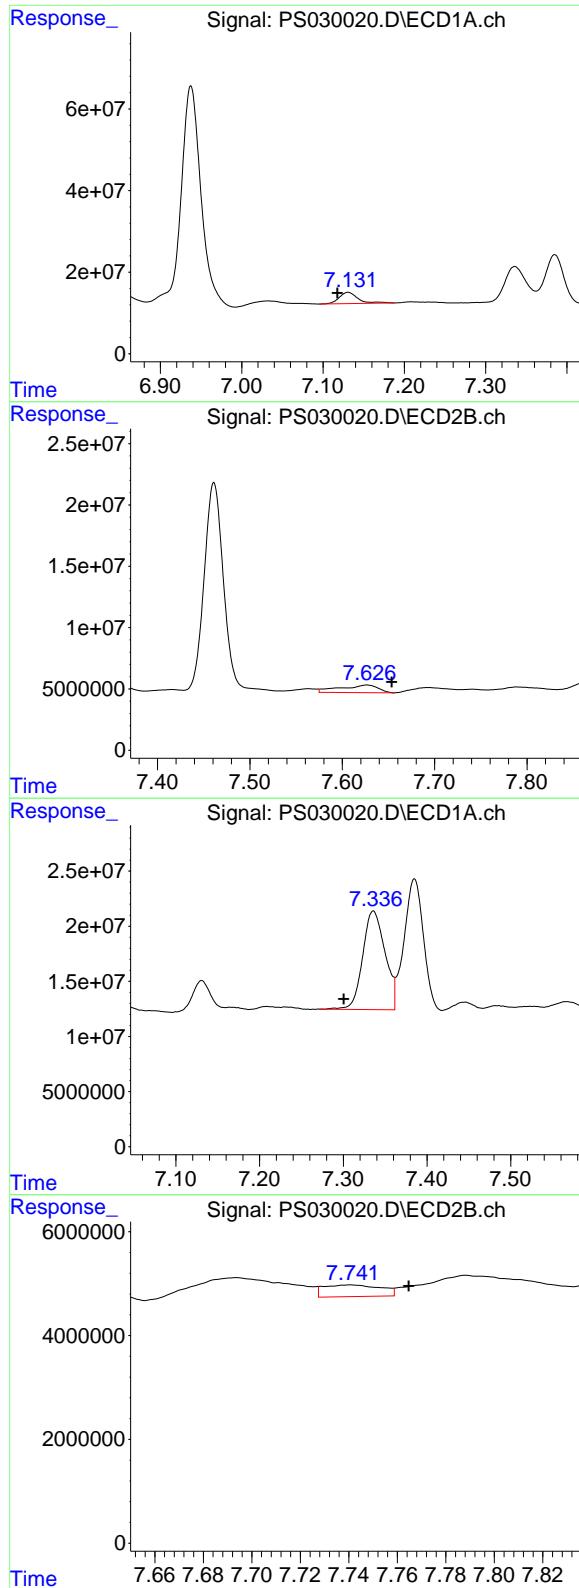

#5 DICAMBA

R.T.: 7.131 min  
 Delta R.T.: 0.013 min  
 Response: 44301703  
 Conc: 4.47 ng/ml

Instrument: ECD\_S  
 ClientSampleId: Q1883-Herbicide Group1

#5 DICAMBA


R.T.: 7.627 min  
 Delta R.T.: -0.027 min  
 Response: 17622450  
 Conc: 4.46 ng/ml

#6 MCPP

R.T.: 7.336 min  
 Delta R.T.: 0.036 min  
 Response: 166483955  
 Conc: 25.84 ug/ml

#6 MCPP


R.T.: 7.741 min  
 Delta R.T.: -0.024 min  
 Response: 3687325  
 Conc: 2.11 ug/ml

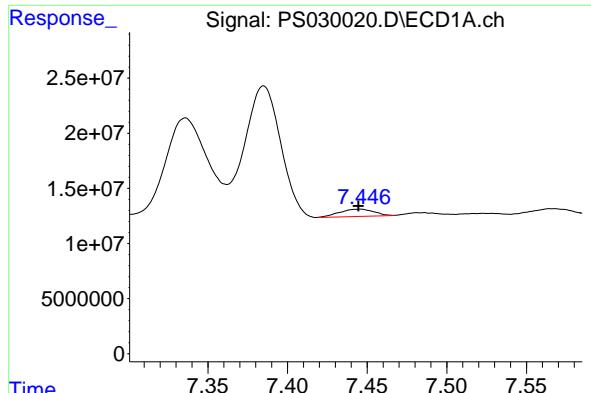

#7 MCPA


R.T.: 7.445 min  
 Delta R.T.: 0.000 min  
 Response: 9843728  
 Conc: 1.11 ug/ml

Instrument: ECD\_S  
 ClientSampleId: OU4-PCS-TC-30-042325

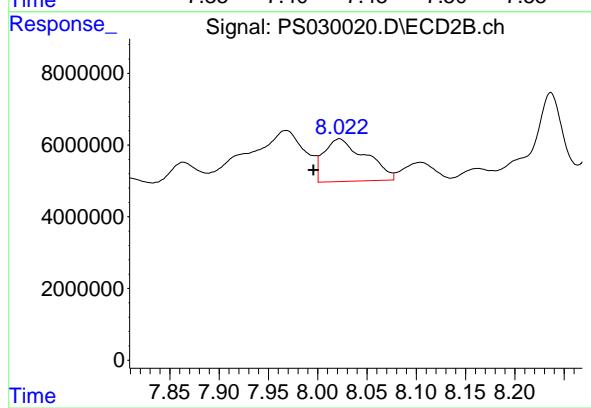


#7 MCPA

R.T.: 8.022 min  
 Delta R.T.: 0.026 min  
 Response: 34989917  
 Conc: 14.79 ug/ml

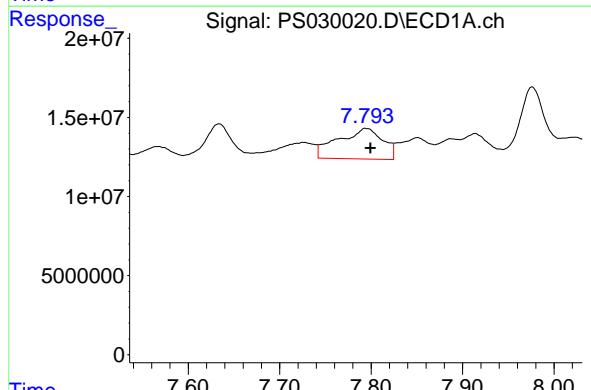


#8 DICHLOPROP

R.T.: 7.795 min  
 Delta R.T.: -0.004 min  
 Response: 65892516  
 Conc: 26.00 ng/ml

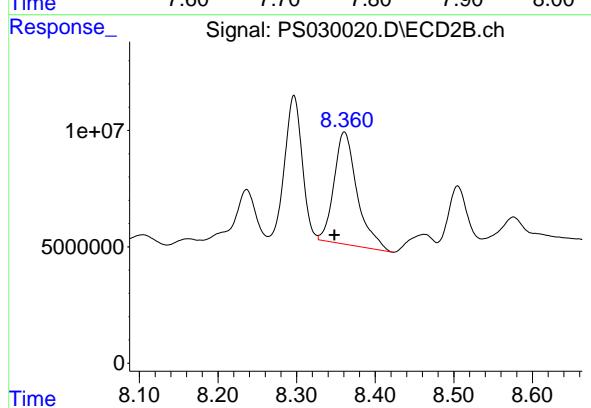

#8 DICHLOPROP

R.T.: 8.361 min  
 Delta R.T.: 0.013 min  
 Response: 98492487  
 Conc: 98.10 ng/ml

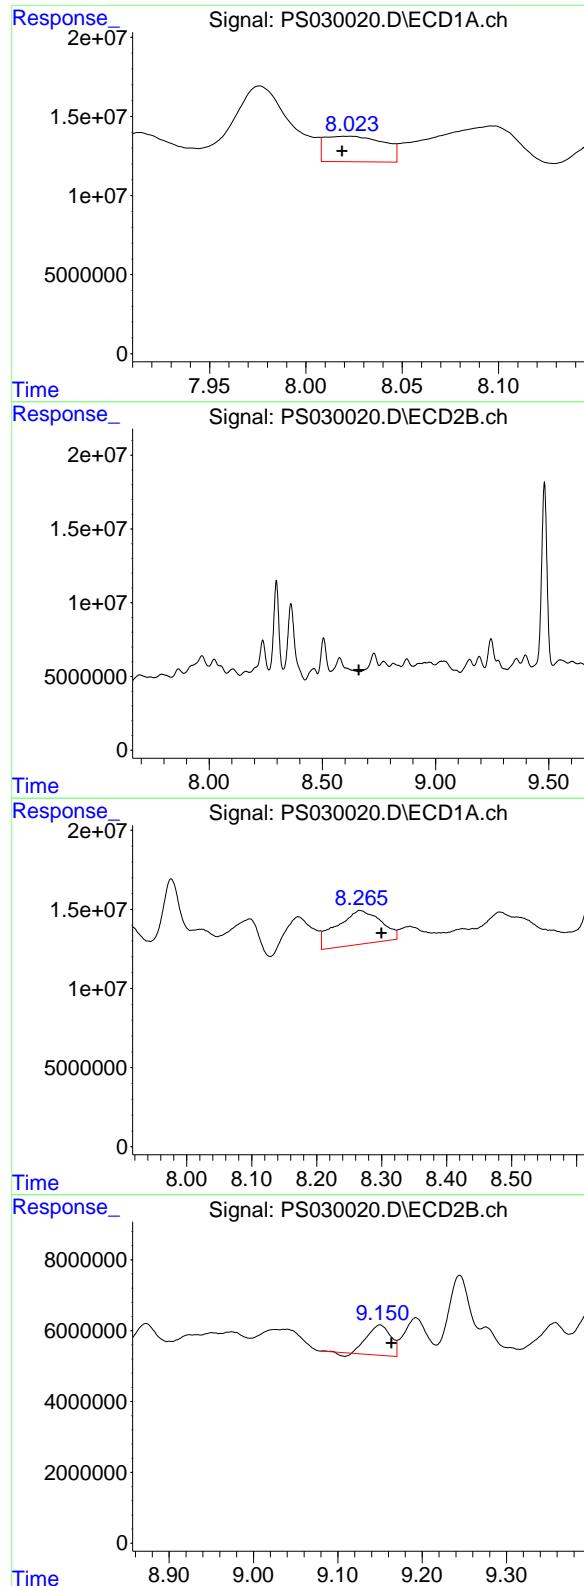

#9 2,4-D

R.T.: 8.021 min  
Delta R.T.: 0.003 min  
Response: 34475421  
Conc: 12.26 ng/ml

Instrument: ECD\_S  
ClientSampleId : OU4-PCS-TC-30-042325

#9 2,4-D


R.T.: 0.000 min  
Exp R.T. : 8.661 min  
Response: 0  
Conc: N.D.

#10 Pentachlorophenol

R.T.: 8.267 min  
Delta R.T.: -0.032 min  
Response: 101518737  
Conc: 2.91 ng/ml

#10 Pentachlorophenol

R.T.: 9.150 min  
Delta R.T.: -0.014 min  
Response: 16183448  
Conc: N.D.

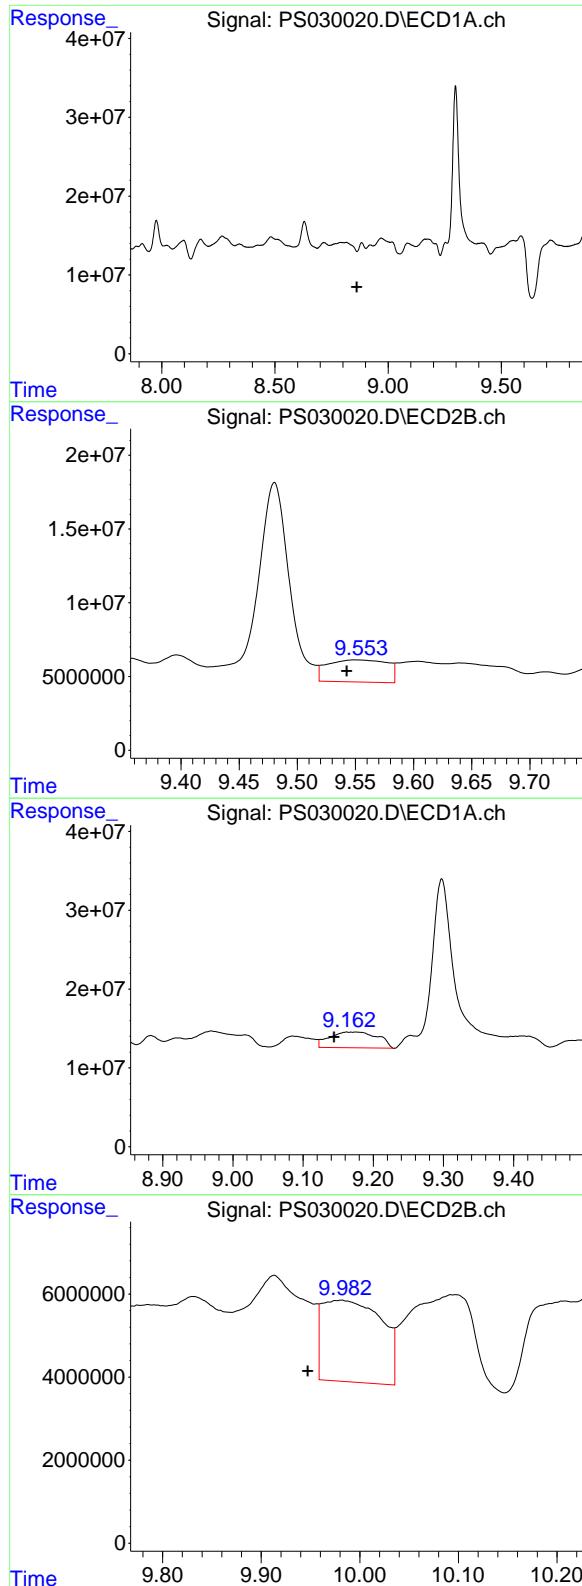

#11 2,4,5-TP (SILVEX)

R.T.: 8.883 min  
 Delta R.T.: 0.021 min  
 Response: -475133  
 Conc: N.D.

Instrument :  
 ECD\_S  
 ClientSampleId :  
 OU4-PCS-TC-30-042325

#11 2,4,5-TP (SILVEX)


R.T.: 9.550 min  
 Delta R.T.: 0.008 min  
 Response: 53425910  
 Conc: 6.53 ng/ml

#12 2,4,5-T

R.T.: 9.175 min  
 Delta R.T.: 0.031 min  
 Response: 95586070  
 Conc: 6.80 ng/ml

#12 2,4,5-T

R.T.: 9.981 min  
 Delta R.T.: 0.033 min  
 Response: 81923977  
 Conc: 10.55 ng/ml

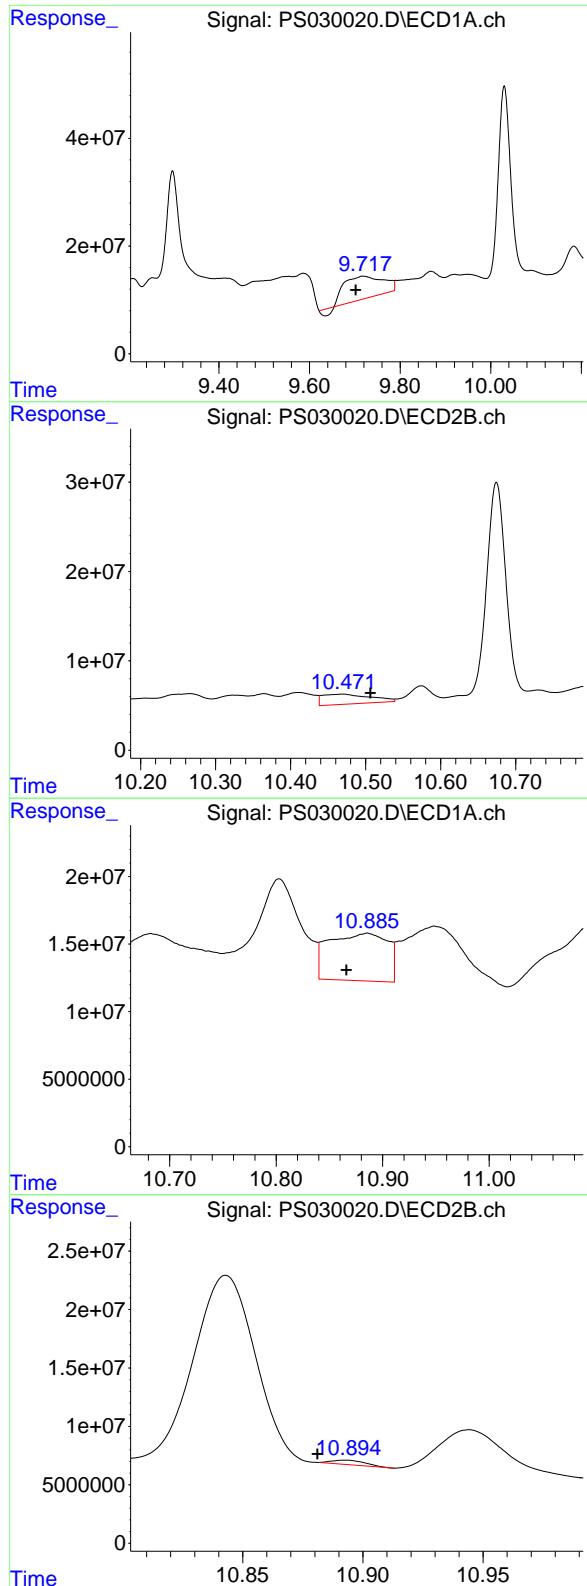

#13 2,4-DB

R.T.: 9.718 min  
 Delta R.T.: 0.016 min  
 Response: 240273509  
 Conc: 105.14 ng/ml

Instrument: ECD\_S  
 ClientSampleId: OU4-PCS-TC-30-042325

#13 2,4-DB


R.T.: 10.469 min  
 Delta R.T.: -0.037 min  
 Response: 50036189  
 Conc: 62.17 ng/ml

#14 DINOSEB

R.T.: 10.885 min  
 Delta R.T.: 0.019 min  
 Response: 134322664  
 Conc: 13.20 ng/ml

#14 DINOSEB

R.T.: 10.893 min  
 Delta R.T.: 0.011 min  
 Response: 3605831  
 Conc: N.D.

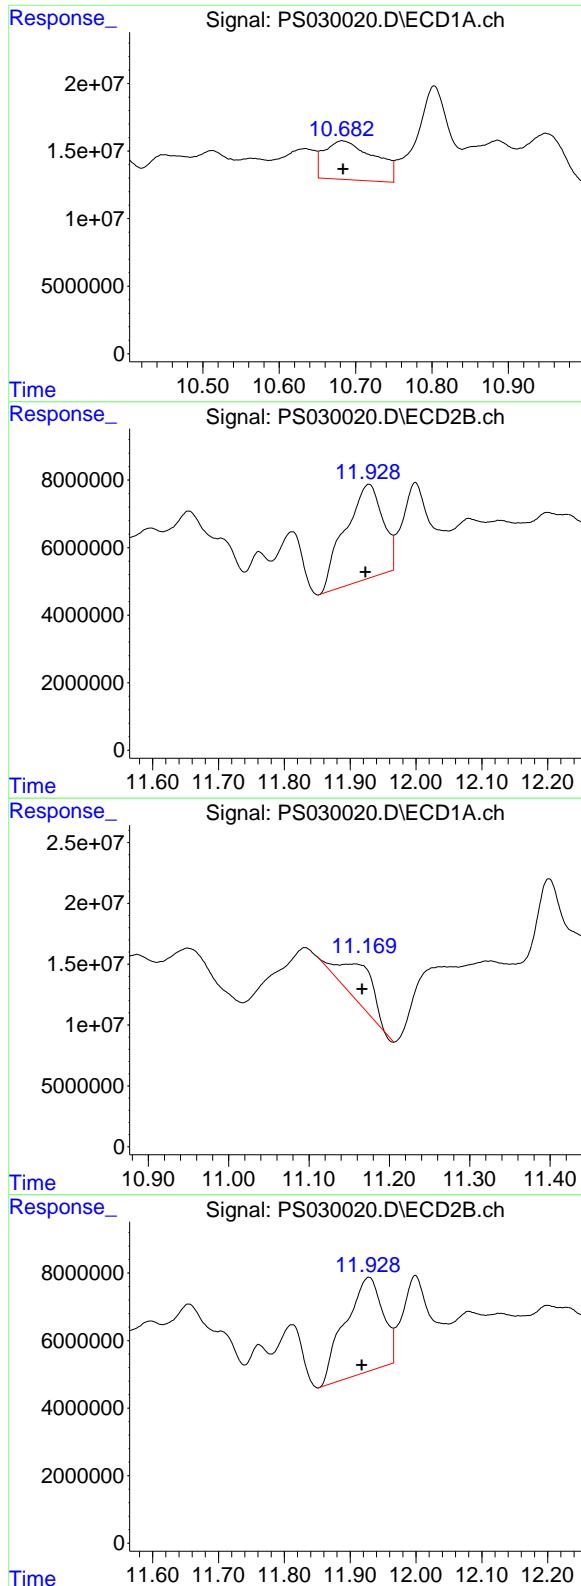

#15 Picloram

R.T.: 10.682 min  
 Delta R.T.: -0.001 min  
 Response: 130727697  
 Conc: 7.13 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** OU4-PCS-TC-30-042325

#15 Picloram

R.T.: 11.928 min  
 Delta R.T.: 0.005 min  
 Response: 111346825  
 Conc: 9.06 ng/ml

#16 DCPA

R.T.: 11.157 min  
 Delta R.T.: -0.009 min  
 Response: 87839378  
 Conc: 5.16 ng/ml

#16 DCPA

R.T.: 11.928 min  
 Delta R.T.: 0.011 min  
 Response: 111346825  
 Conc: 9.88 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030021.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 15:28  
 Operator : AR\AJ  
 Sample : Q1983-09  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**OU4-PCS-TC-31-042325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:29:18 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.938 7.461 983.0E6 267.8E6 399.422 380.058

Target Compounds

1) T	Dalapon	2.434	2.499f	228.3E6	132.5E6	55.738	76.341 #
2) T	3,5-DICHL...	6.162	6.468	6228037	10179898	1.743	10.413 #
3) T	4-Nitroph...	6.722	6.981	54657362	15030114	30.649	19.624 #
5) T	DICAMBA	7.131	7.627f	28640387	18138562	2.892	4.592 #
6) T	MCPP	7.278	7.739f	227934	2001920	<MDL	1.145 #
7) T	MCPA	7.445	8.022f	14260114	23597897	1.615	9.975 #
8) T	DICHLORPROP	7.798	8.361	47603925	91068506	18.785	90.709 #
9) T	2,4-D	7.977f	8.613f	215.4E6	7327934	76.559	6.502 #
10) T	Pentachlo...	8.288	9.151	102.6E6	18715528	2.940	<MDL #
11) T	2,4,5-TP ...	8.885	9.556	5649395	57866025	<MDL	7.073 #
12) T	2,4,5-T	9.164	9.982f	100.8E6	81225598	7.176	10.464 #
13) T	2,4-DB	9.721	10.523	235.2E6	10154346	102.915	12.617 #
14) T	DINOSEB	10.855	10.844f	42002587	149.1E6	4.129	25.575 #
15) T	Picloram	10.690	11.930	126.0E6	109.7E6	6.876	8.929 #
16) T	DCPA	11.156	11.930	81394330	109.7E6	4.782	9.731 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030021.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 15:28  
 Operator : AR\AJ  
 Sample : Q1983-09  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**OU4-PCS-TC-31-042325**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:29:18 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

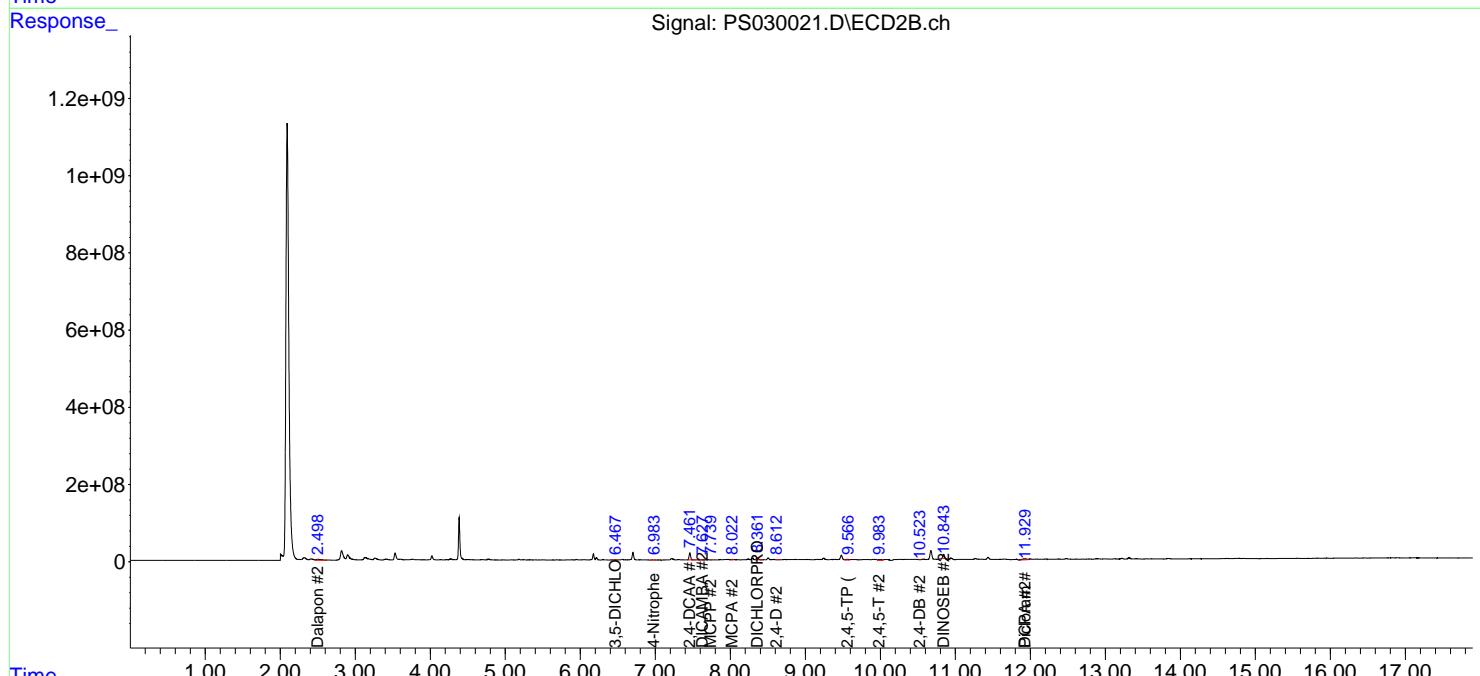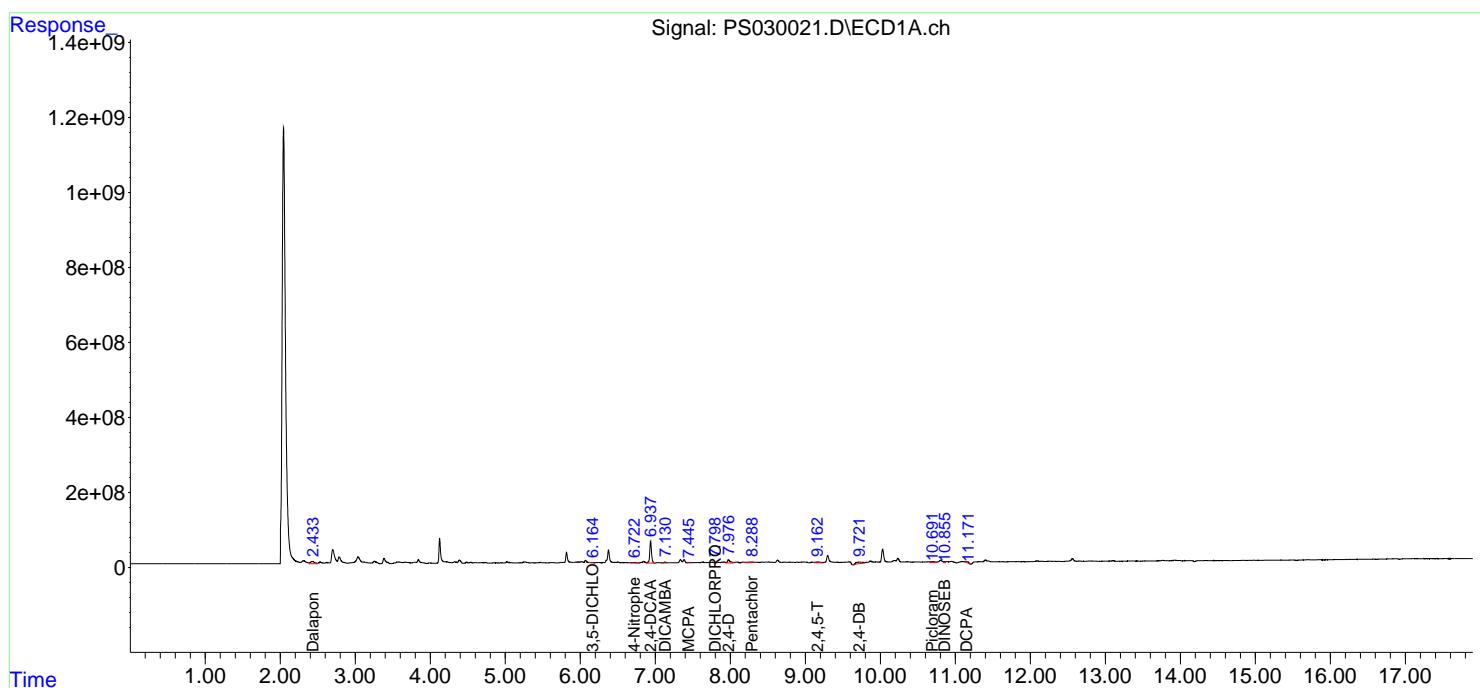


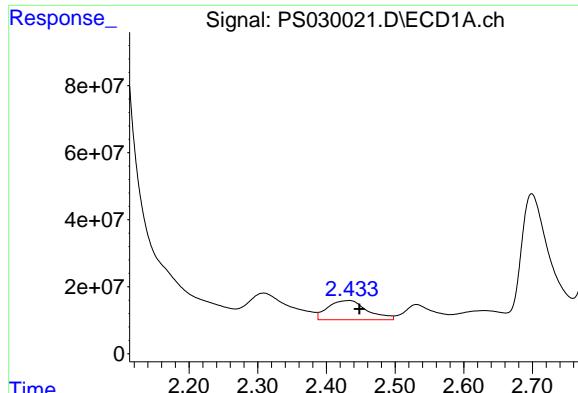

#1 Dalapon


R.T.: 2.434 min  
Delta R.T.: -0.014 min  
Response: 228262990  
Conc: 55.74 ng/ml

Instrument: ECD\_S  
ClientSampleId: Q1883-Herbicide Group1

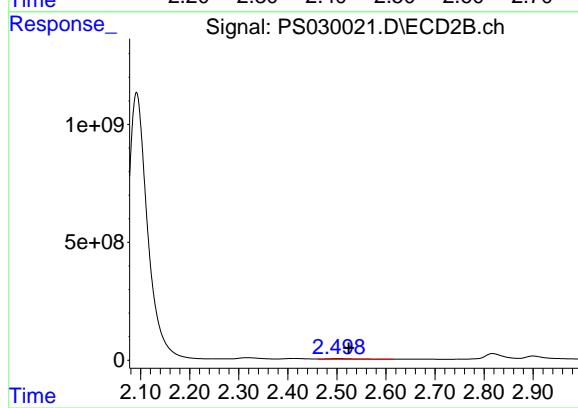


#1 Dalapon

R.T.: 2.499 min  
Delta R.T.: -0.025 min  
Response: 132539566  
Conc: 76.34 ng/ml

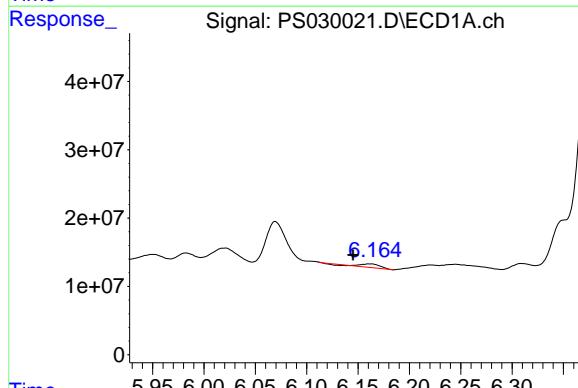


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.162 min  
Delta R.T.: 0.017 min  
Response: 6228037  
Conc: 1.74 ng/ml

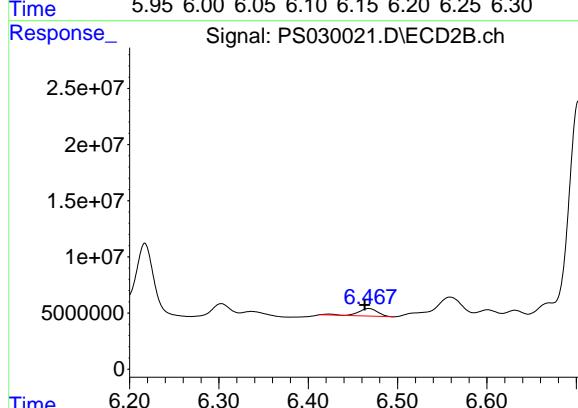

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.468 min  
Delta R.T.: 0.005 min  
Response: 10179898  
Conc: 10.41 ng/ml

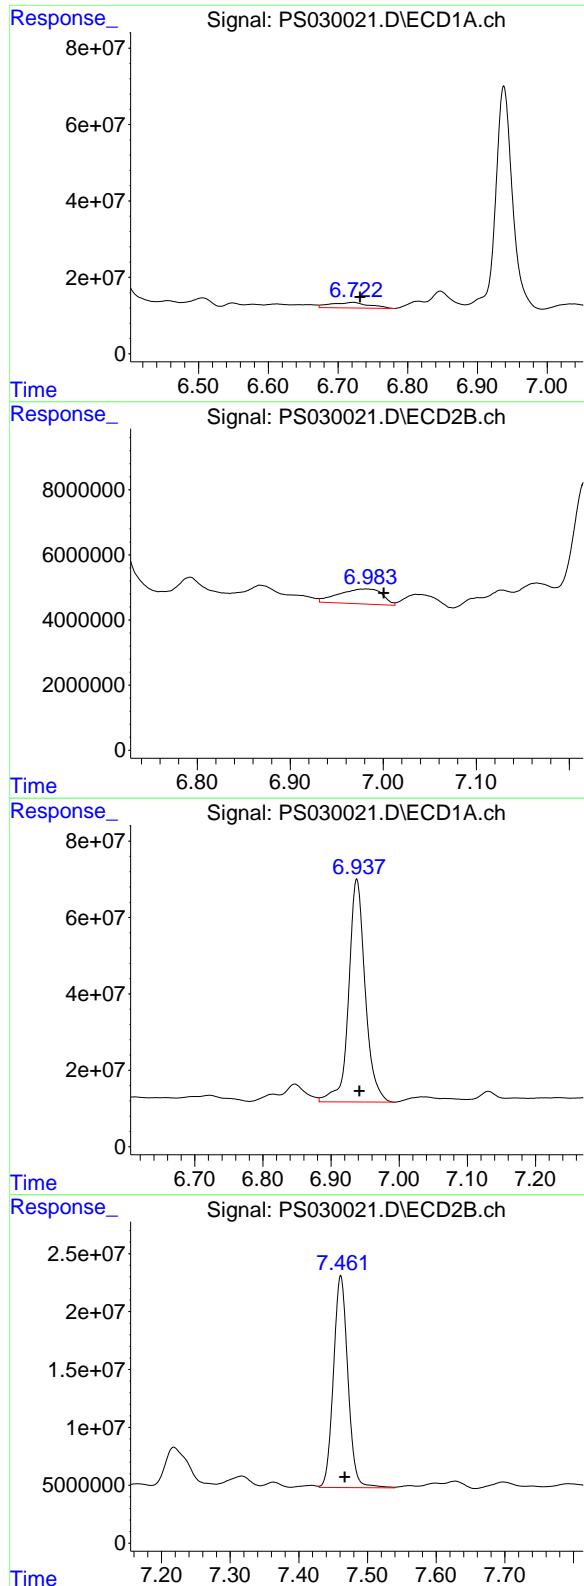

#3 4-Nitrophenol

R.T.: 6.722 min  
Delta R.T.: -0.010 min  
Response: 54657362  
Conc: 30.65 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** OU4-PCS-TC-31-042325

#3 4-Nitrophenol


R.T.: 6.981 min  
Delta R.T.: -0.019 min  
Response: 15030114  
Conc: 19.62 ng/ml

#4 2,4-DCAA

R.T.: 6.938 min  
Delta R.T.: -0.004 min  
Response: 983009744  
Conc: 399.42 ng/ml

#4 2,4-DCAA


R.T.: 7.461 min  
Delta R.T.: -0.006 min  
Response: 267757330  
Conc: 380.06 ng/ml

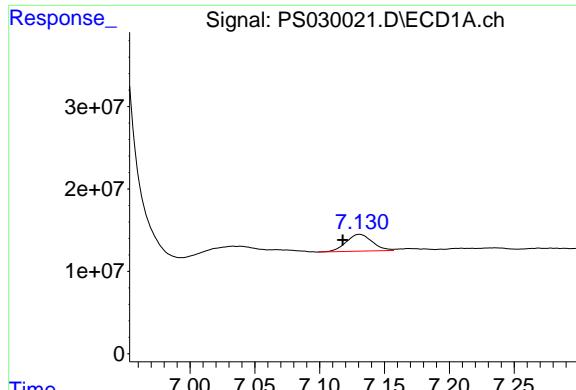

#5 DICAMBA


R.T.: 7.131 min  
 Delta R.T.: 0.013 min  
 Response: 28640387  
 Conc: 2.89 ng/ml

Instrument: ECD\_S  
 ClientSampleId: Q1883-Herbicide Group1-042325.M

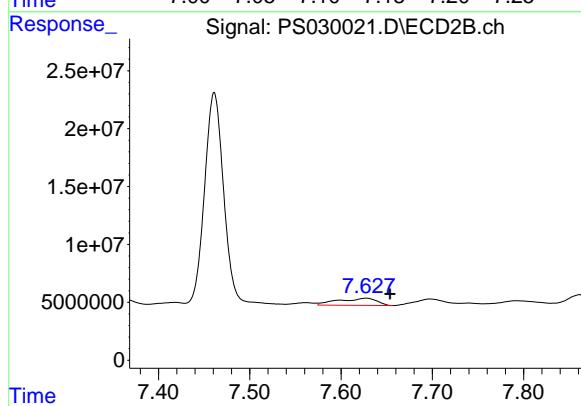


#5 DICAMBA

R.T.: 7.627 min  
 Delta R.T.: -0.026 min  
 Response: 18138562  
 Conc: 4.59 ng/ml

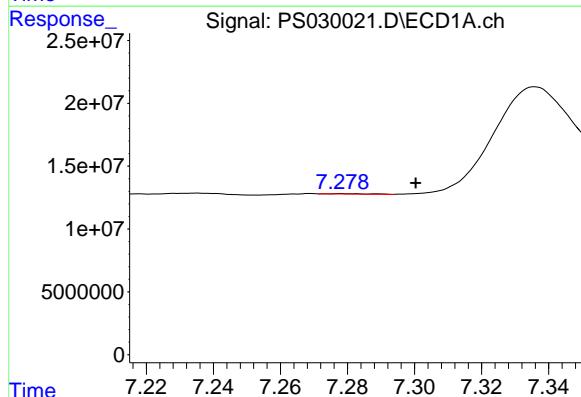


#6 MCPP

R.T.: 7.278 min  
 Delta R.T.: -0.022 min  
 Response: 227934  
 Conc: N.D.

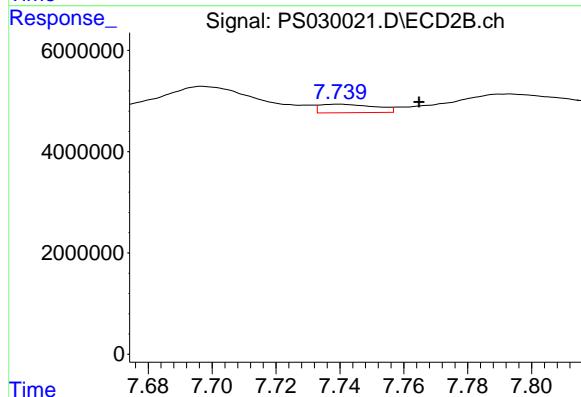

#6 MCPP

R.T.: 7.739 min  
 Delta R.T.: -0.025 min  
 Response: 2001920  
 Conc: 1.14 ug/ml

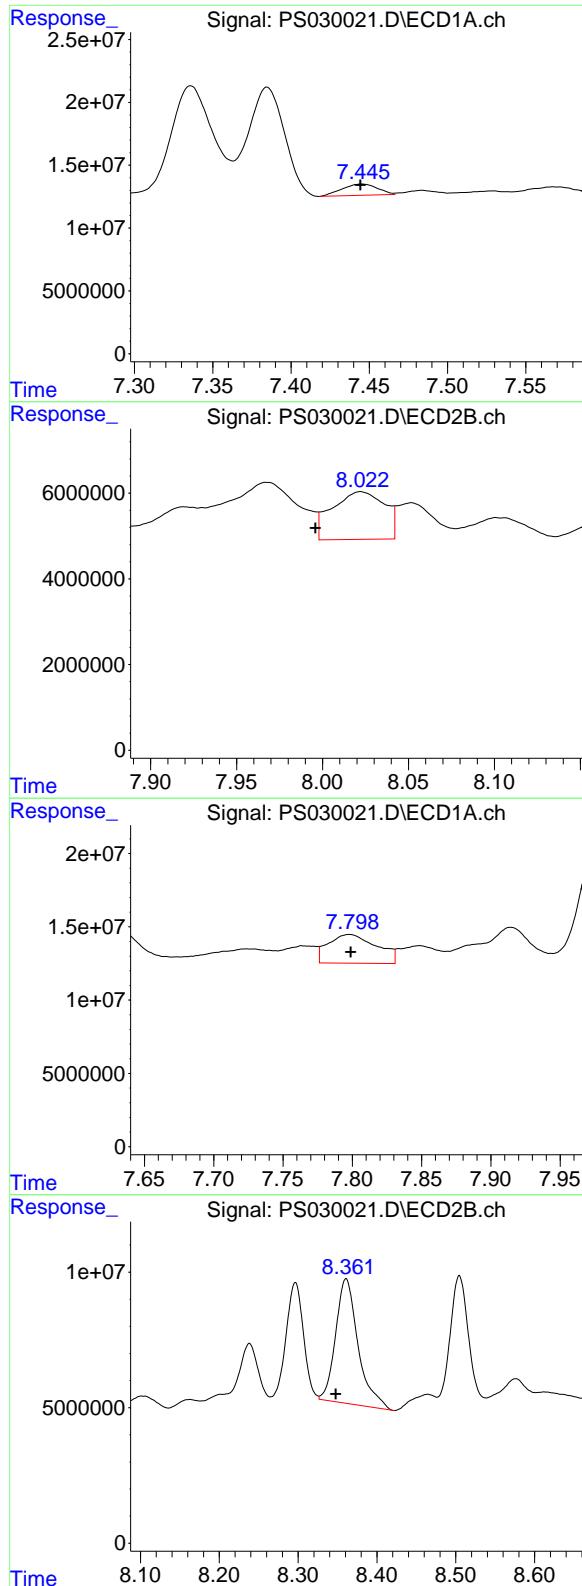

#7 MCPA

R.T.: 7.445 min  
 Delta R.T.: 0.000 min  
 Response: 14260114  
 Conc: 1.61 ug/ml

**Instrument:** ECD\_S  
**ClientSampleId:** OU4-PCS-TC-31-042325

#7 MCPA


R.T.: 8.022 min  
 Delta R.T.: 0.027 min  
 Response: 23597897  
 Conc: 9.97 ug/ml

#8 DICHLORPROP

R.T.: 7.798 min  
 Delta R.T.: 0.000 min  
 Response: 47603925  
 Conc: 18.79 ng/ml

#8 DICHLORPROP

R.T.: 8.361 min  
 Delta R.T.: 0.013 min  
 Response: 91068506  
 Conc: 90.71 ng/ml

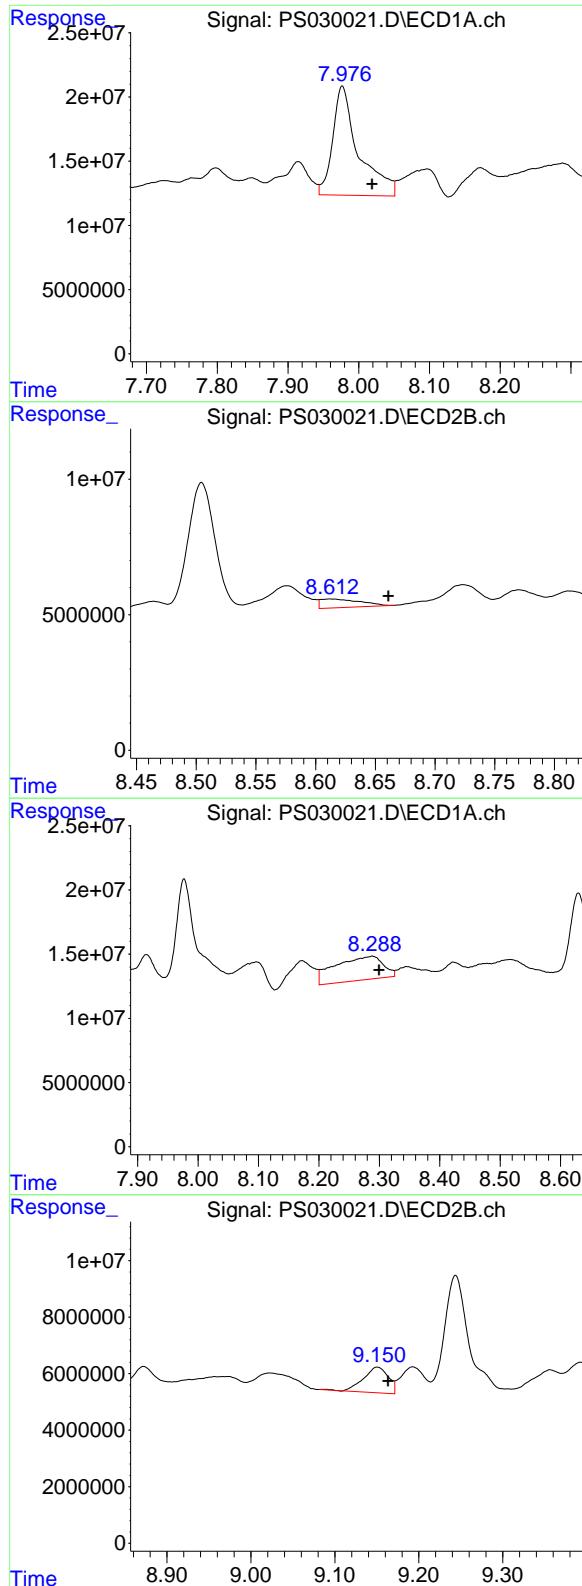

#9 2,4-D

R.T.: 7.977 min  
Delta R.T.: -0.042 min  
Response: 215350295  
Conc: 76.56 ng/ml

Instrument: ECD\_S  
ClientSampleId: OU4-PCS-TC-31-042325

#9 2,4-D


R.T.: 8.613 min  
Delta R.T.: -0.049 min  
Response: 7327934  
Conc: 6.50 ng/ml

#10 Pentachlorophenol

R.T.: 8.288 min  
Delta R.T.: -0.011 min  
Response: 102556293  
Conc: 2.94 ng/ml

#10 Pentachlorophenol

R.T.: 9.151 min  
Delta R.T.: -0.013 min  
Response: 18715528  
Conc: N.D.

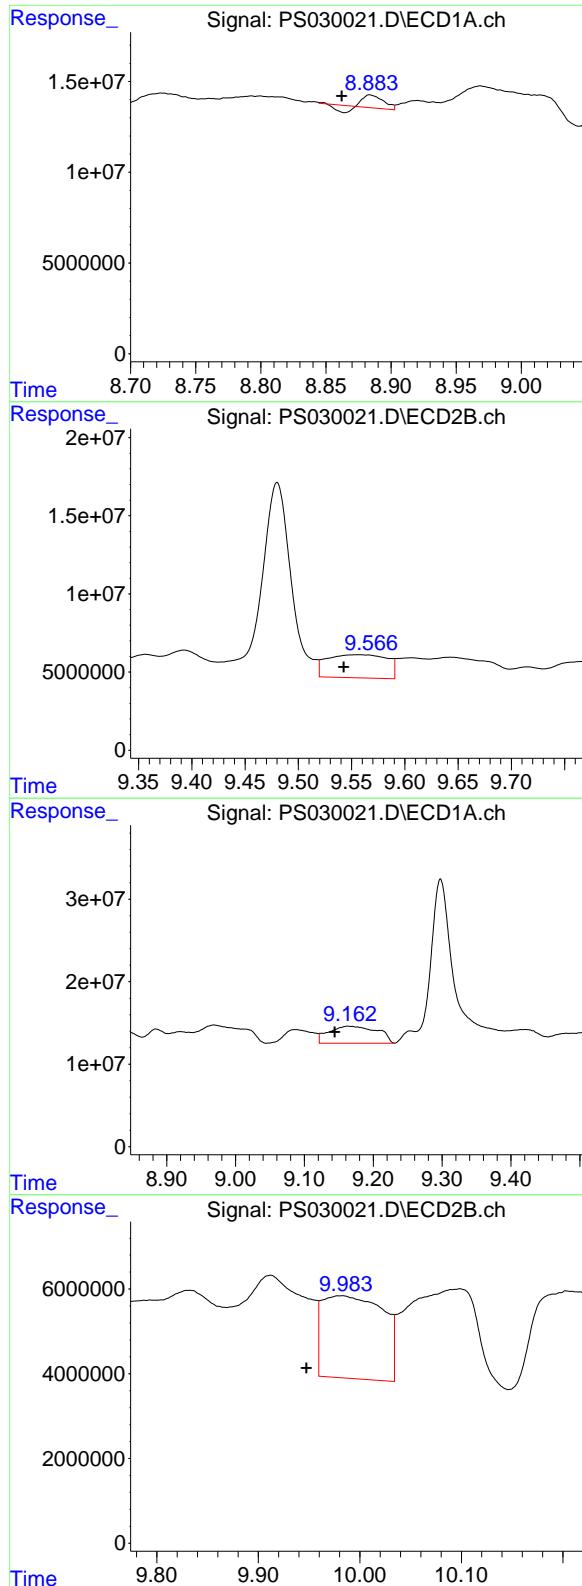

#11 2,4,5-TP (SILVEX)

R.T.: 8.885 min  
 Delta R.T.: 0.022 min  
 Response: 5649395  
 Conc: N.D.

Instrument: ECD\_S  
 ClientSampleId: OU4-PCS-TC-31-042325

#11 2,4,5-TP (SILVEX)


R.T.: 9.556 min  
 Delta R.T.: 0.013 min  
 Response: 57866025  
 Conc: 7.07 ng/ml

#12 2,4,5-T

R.T.: 9.164 min  
 Delta R.T.: 0.020 min  
 Response: 100842308  
 Conc: 7.18 ng/ml

#12 2,4,5-T

R.T.: 9.982 min  
 Delta R.T.: 0.034 min  
 Response: 81225598  
 Conc: 10.46 ng/ml

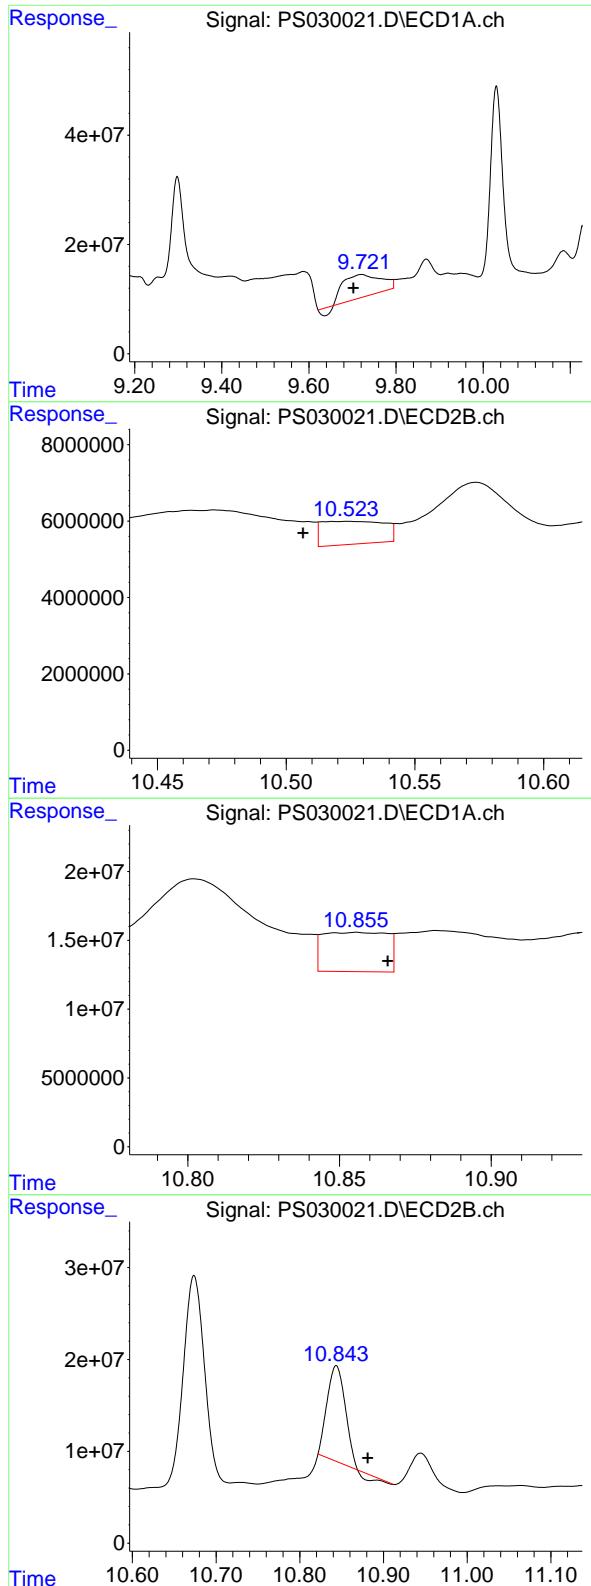

#13 2,4-DB

R.T.: 9.721 min  
 Delta R.T.: 0.019 min  
 Response: 235197606  
 Conc: 102.92 ng/ml

Instrument: ECD\_S  
 ClientSampleId: Q1883-Herbicide Group1

#13 2,4-DB


R.T.: 10.523 min  
 Delta R.T.: 0.017 min  
 Response: 10154346  
 Conc: 12.62 ng/ml

#14 DINOSEB

R.T.: 10.855 min  
 Delta R.T.: -0.011 min  
 Response: 42002587  
 Conc: 4.13 ng/ml

#14 DINOSEB

R.T.: 10.844 min  
 Delta R.T.: -0.038 min  
 Response: 149128200  
 Conc: 25.58 ng/ml

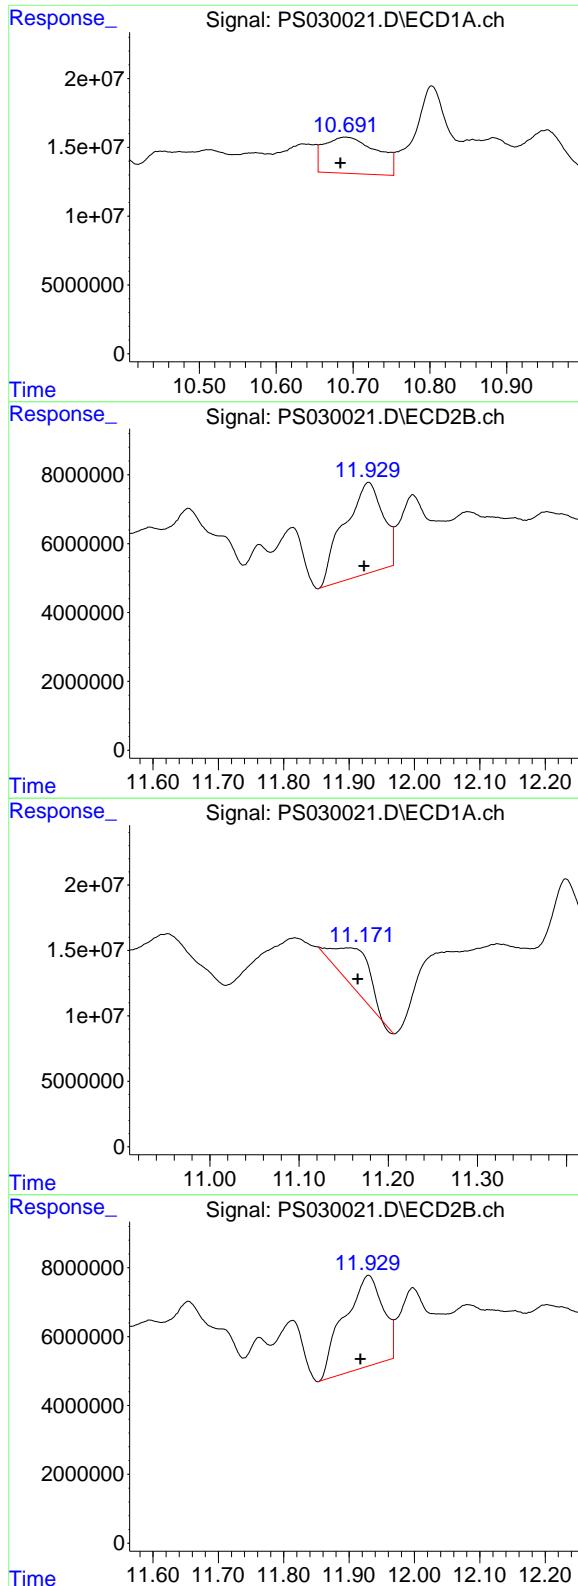

#15 Picloram

R.T.: 10.690 min  
 Delta R.T.: 0.007 min  
 Response: 126036632  
 Conc: 6.88 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** OU4-PCS-TC-31-042325

#15 Picloram

R.T.: 11.930 min  
 Delta R.T.: 0.007 min  
 Response: 109680135  
 Conc: 8.93 ng/ml

#16 DCPA

R.T.: 11.156 min  
 Delta R.T.: -0.010 min  
 Response: 81394330  
 Conc: 4.78 ng/ml

#16 DCPA

R.T.: 11.930 min  
 Delta R.T.: 0.012 min  
 Response: 109680135  
 Conc: 9.73 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030026.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 17:28  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**HSTDCCC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:30:46 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.938 7.462 1888.4E6 569.7E6 767.297 808.568

Target Compounds

1) T	Dalapon	2.448	2.523	2794.7E6	1185.1E6	682.429	682.626
2) T	3,5-DICHL...	6.142	6.459	2569.7E6	738.2E6	719.036	755.171
3) T	4-Nitroph...	6.728	6.995	1269.3E6	560.2E6	711.772	731.395
5) T	DICAMBA	7.114	7.648	7247.0E6	3150.6E6	731.806	797.615
6) T	MCPP	7.293	7.755	448.3E6	125.9E6	69.578	72.009
7) T	MCPA	7.436	7.985	641.0E6	170.3E6	72.586	71.966
8) T	DICHLORPROP	7.795	8.341	1817.9E6	801.4E6	717.354	798.239
9) T	2,4-D	8.015	8.653	2045.8E6	862.5E6	727.283	765.272
10) T	Pentachlo...	8.293	9.154	26237.5E6	16512.9E6	752.115	811.653
11) T	2,4,5-TP ...	8.857	9.533	10417.0E6	6556.3E6	751.434	801.336
12) T	2,4,5-T	9.139	9.937	10641.3E6	6136.4E6	757.218	790.511
13) T	2,4-DB	9.698	10.495	1757.6E6	617.9E6	769.084	767.700
14) T	DINOSEB	10.860	10.869	7519.2E6	4438.6E6	739.099	761.205
15) T	Picloram	10.678	11.903	13425.7E6	18182.7E6	732.418	1480.233 #
16) T	DCPA	11.161	11.903	12986.2E6	18182.7E6	762.952	1613.131 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050125\  
 Data File : PS030026.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 May 2025 17:28  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDCCC750

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 02 01:30:46 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

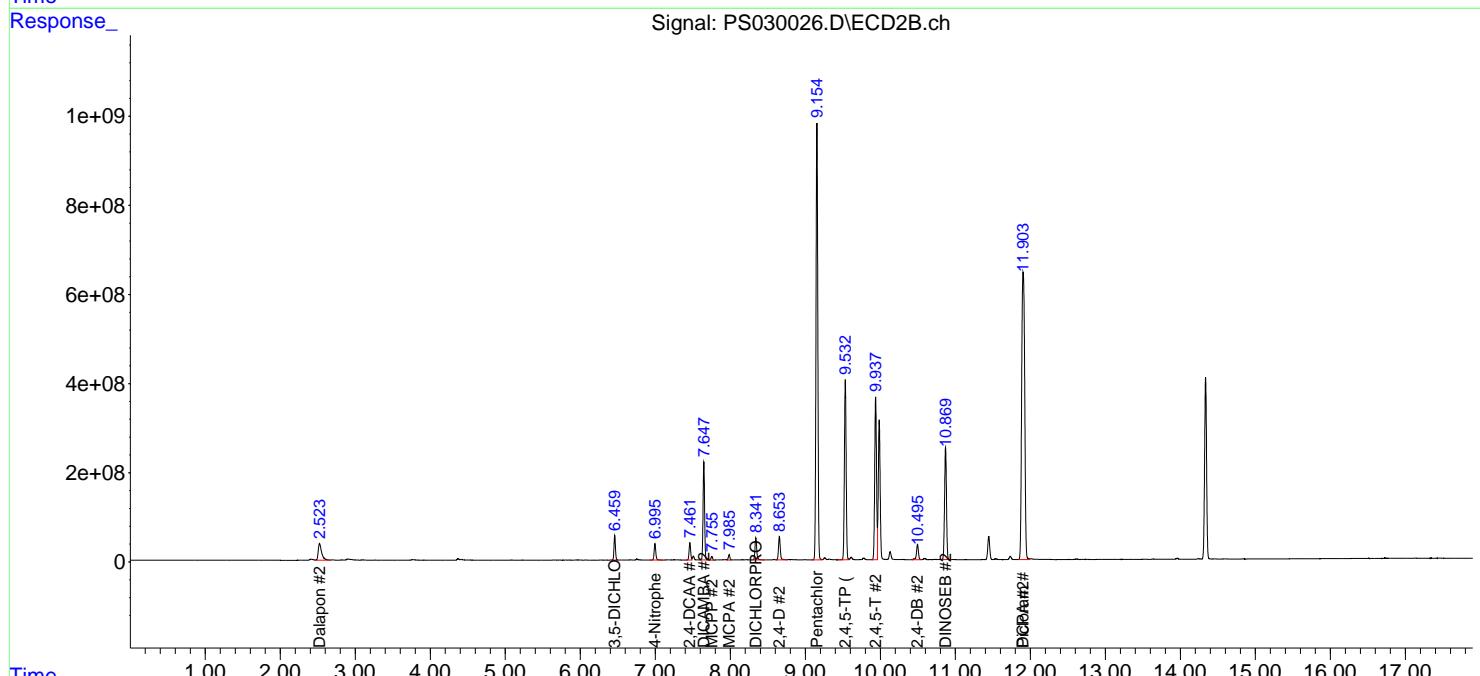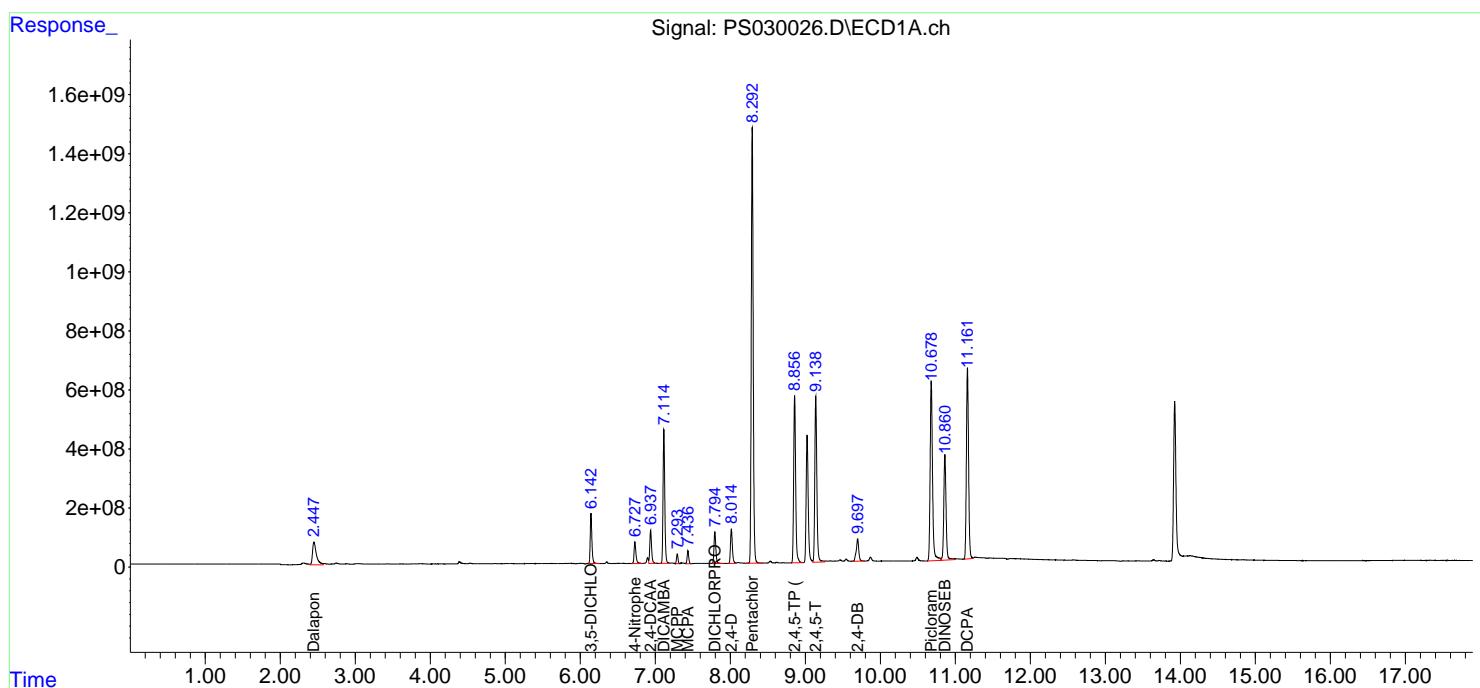

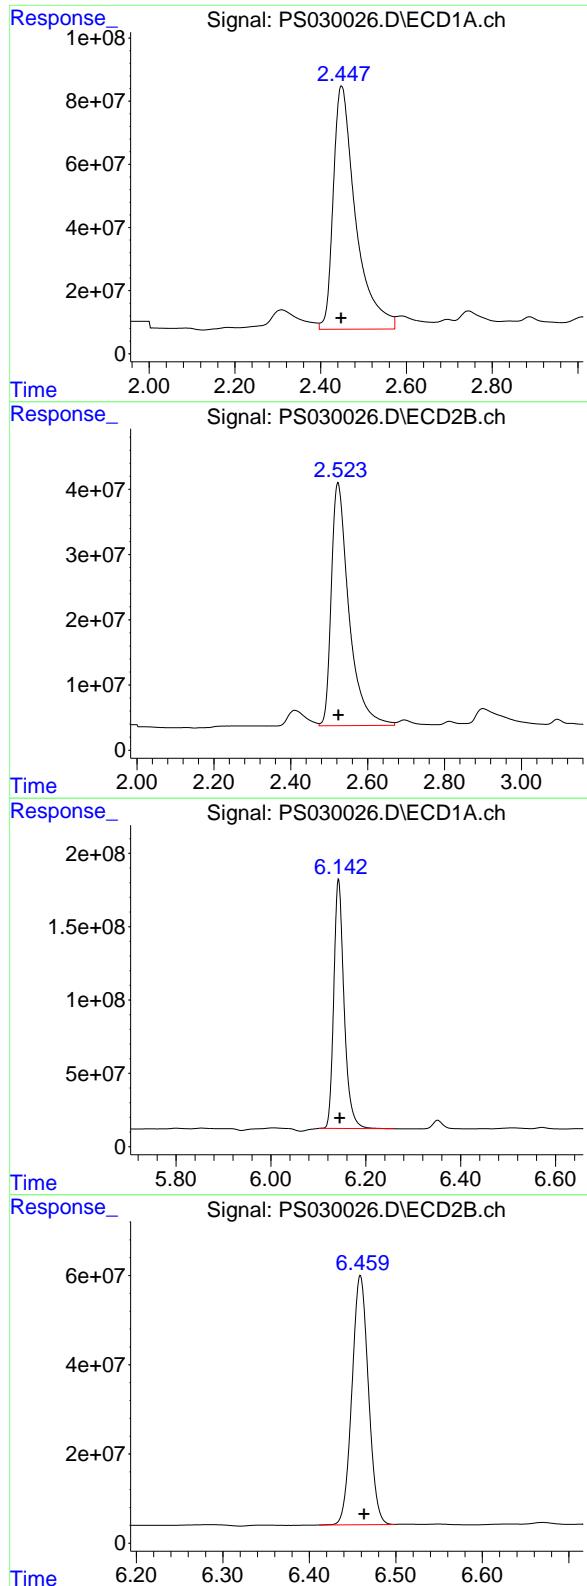

#1 Dalapon

R.T.: 2.448 min  
Delta R.T.: 0.000 min **Instrument:**  
Response: 2794723971 ECD\_S  
Conc: 682.43 ng/ml **ClientSampleId:**  
HSTDCCC750

#1 Dalapon


R.T.: 2.523 min  
Delta R.T.: -0.002 min  
Response: 1185136689  
Conc: 682.63 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.142 min  
Delta R.T.: -0.003 min  
Response: 2569680983  
Conc: 719.04 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.459 min  
Delta R.T.: -0.004 min  
Response: 738239496  
Conc: 755.17 ng/ml

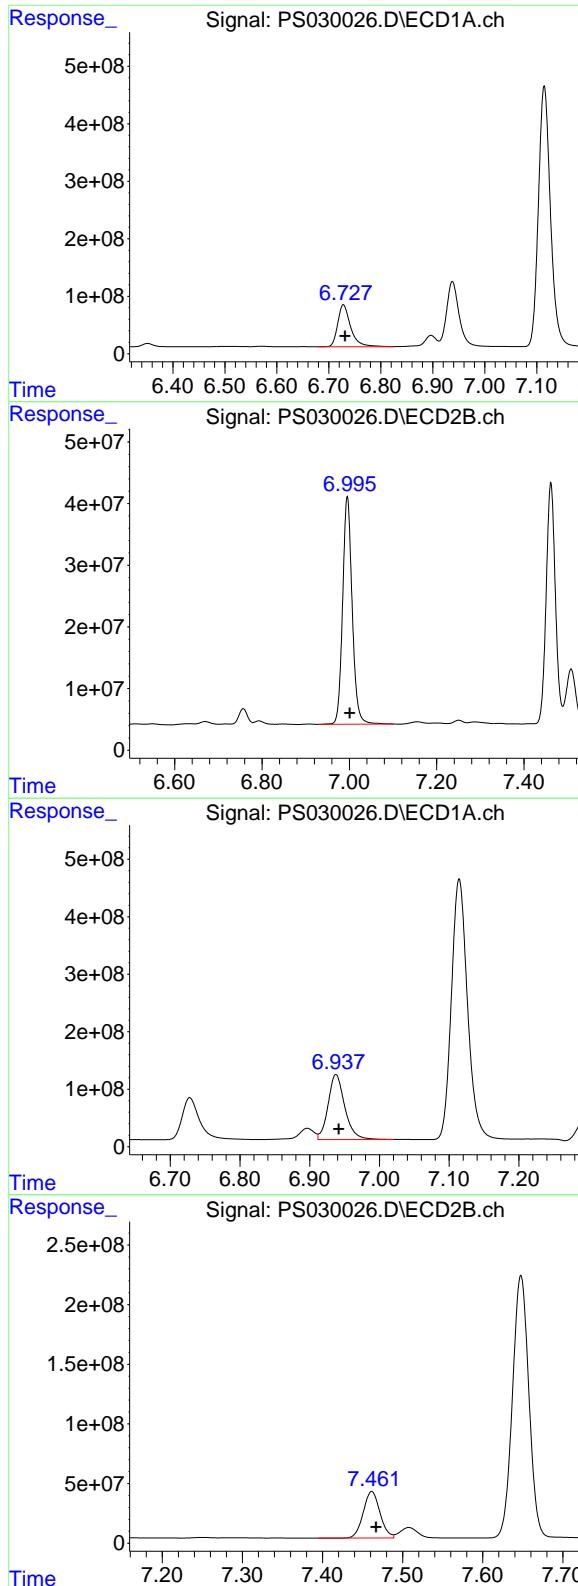

#3 4-Nitrophenol

R.T.: 6.728 min  
 Delta R.T.: -0.003 min  
 Response: 1269317960  
 Conc: 711.77 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#3 4-Nitrophenol


R.T.: 6.995 min  
 Delta R.T.: -0.005 min  
 Response: 560191374  
 Conc: 731.40 ng/ml

#4 2,4-DCAA

R.T.: 6.938 min  
 Delta R.T.: -0.004 min  
 Response: 1888378898  
 Conc: 767.30 ng/ml

#4 2,4-DCAA

R.T.: 7.462 min  
 Delta R.T.: -0.006 min  
 Response: 569650088  
 Conc: 808.57 ng/ml

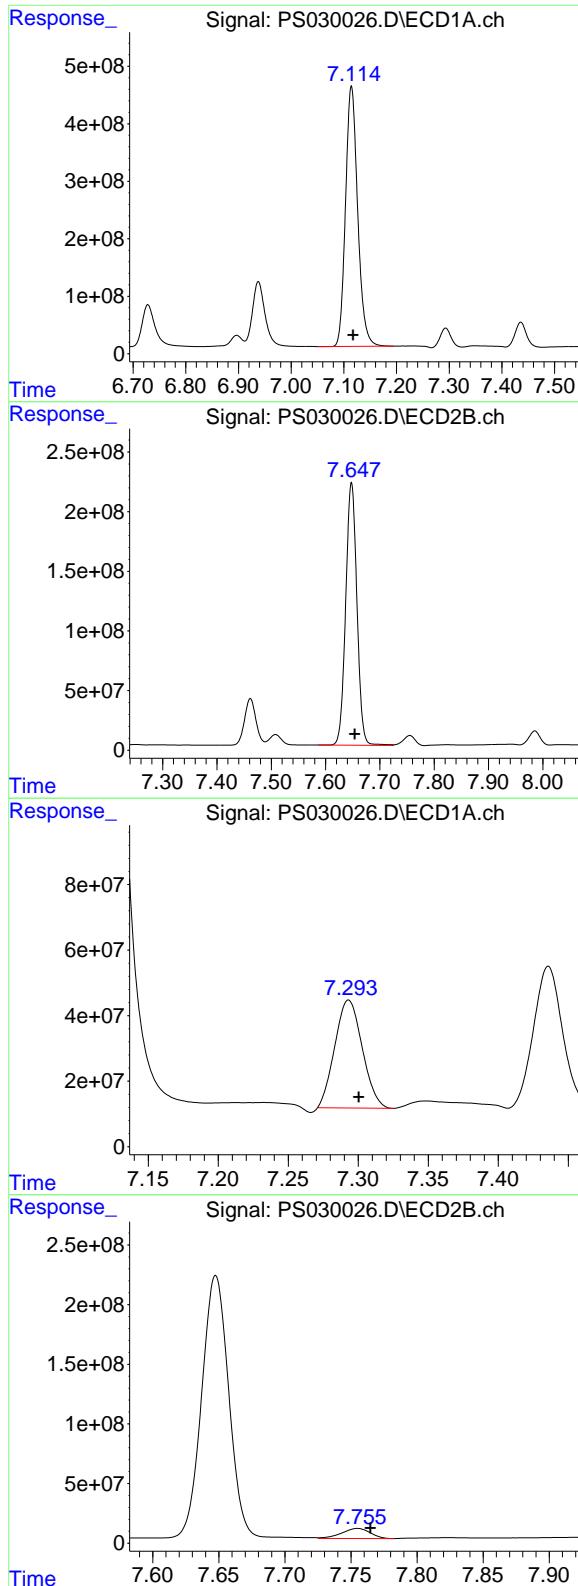

#5 DICAMBA

R.T.: 7.114 min  
 Delta R.T.: -0.003 min  
 Response: 7246972846  
 Conc: 731.81 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** HSTDCCC750

#5 DICAMBA


R.T.: 7.648 min  
 Delta R.T.: -0.006 min  
 Response: 3150630491  
 Conc: 797.61 ng/ml

#6 MCPP

R.T.: 7.293 min  
 Delta R.T.: -0.007 min  
 Response: 448334279  
 Conc: 69.58 ug/ml

#6 MCPP

R.T.: 7.755 min  
 Delta R.T.: -0.010 min  
 Response: 125940998  
 Conc: 72.01 ug/ml

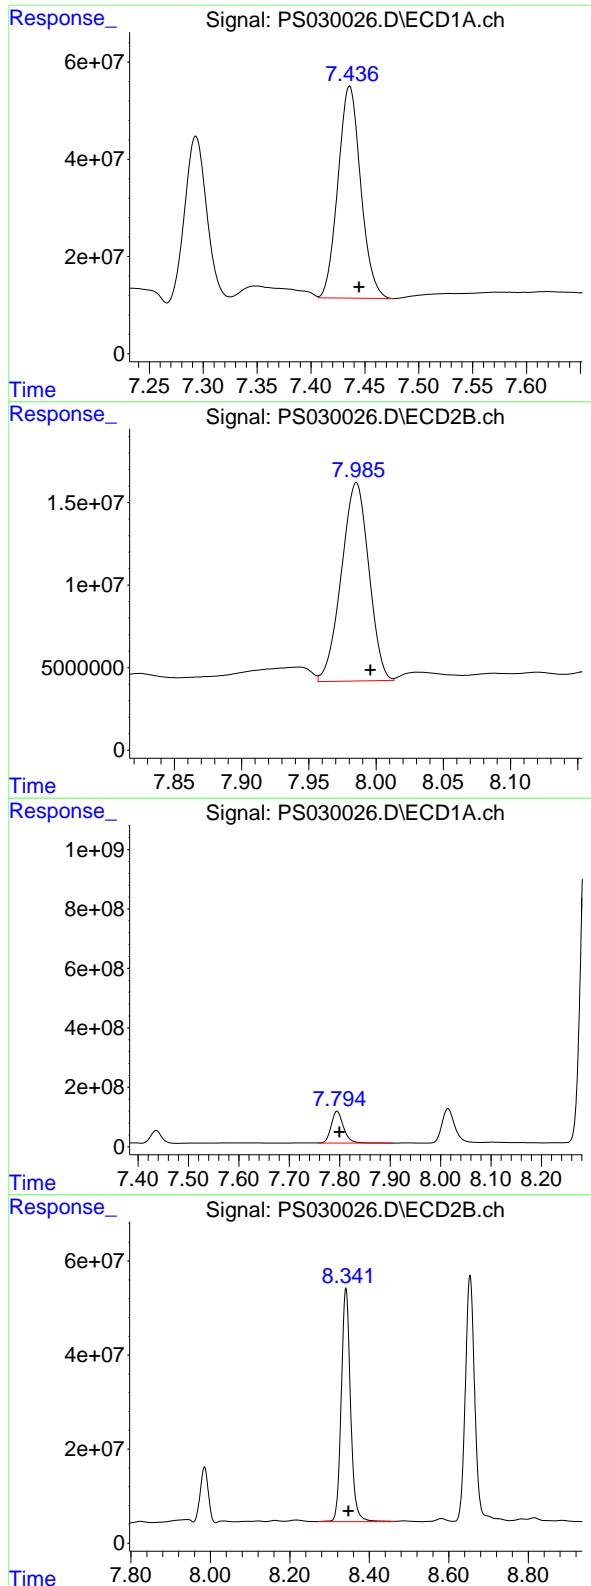

#7 MCPA

R.T.: 7.436 min  
 Delta R.T.: -0.009 min  
 Response: 641028979  
 Conc: 72.59 ug/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#7 MCPA


R.T.: 7.985 min  
 Delta R.T.: -0.010 min  
 Response: 170258090  
 Conc: 71.97 ug/ml

#8 DICHLOPROP

R.T.: 7.795 min  
 Delta R.T.: -0.004 min  
 Response: 1817853046  
 Conc: 717.35 ng/ml

#8 DICHLOPROP

R.T.: 8.341 min  
 Delta R.T.: -0.007 min  
 Response: 801403222  
 Conc: 798.24 ng/ml

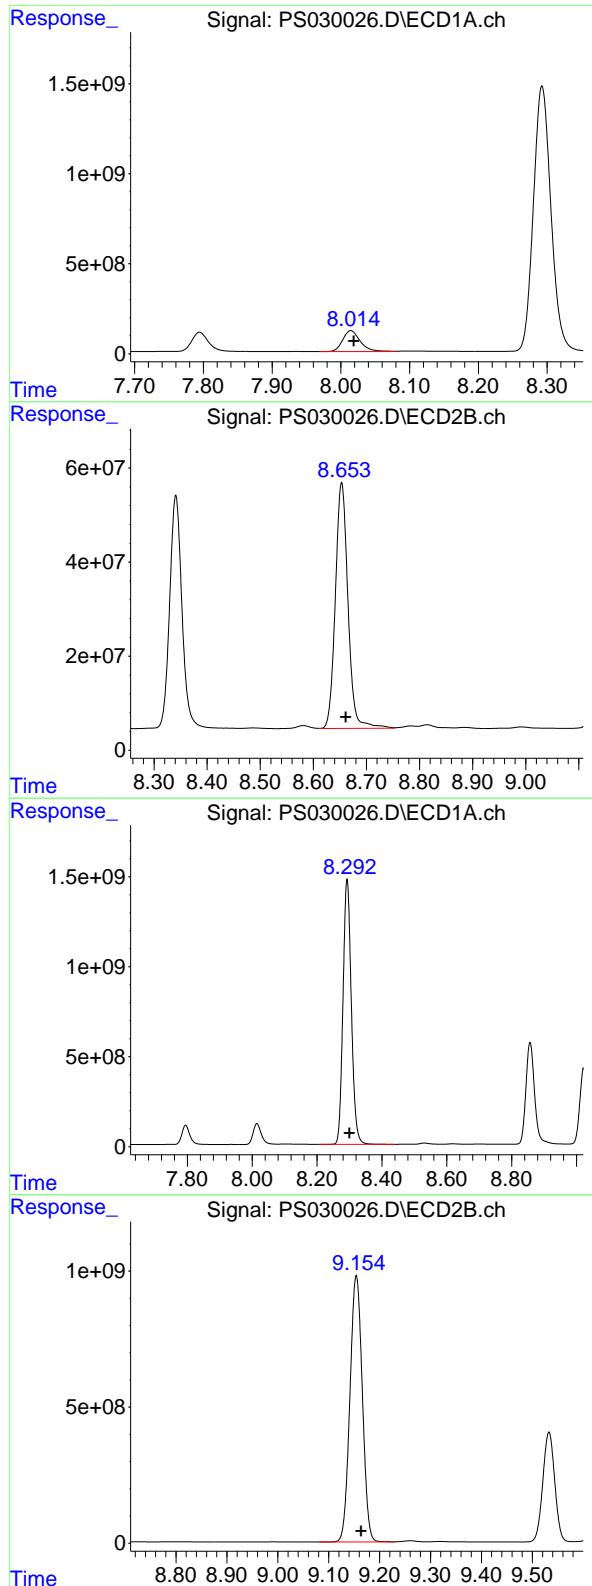

#9 2,4-D

R.T.: 8.015 min  
 Delta R.T.: -0.004 min  
 Response: 2045753582  
 Conc: 727.28 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#9 2,4-D


R.T.: 8.653 min  
 Delta R.T.: -0.008 min  
 Response: 862543014  
 Conc: 765.27 ng/ml

#10 Pentachlorophenol

R.T.: 8.293 min  
 Delta R.T.: -0.007 min  
 Response: 26237549087  
 Conc: 752.12 ng/ml

#10 Pentachlorophenol

R.T.: 9.154 min  
 Delta R.T.: -0.009 min  
 Response: 16512921319  
 Conc: 811.65 ng/ml

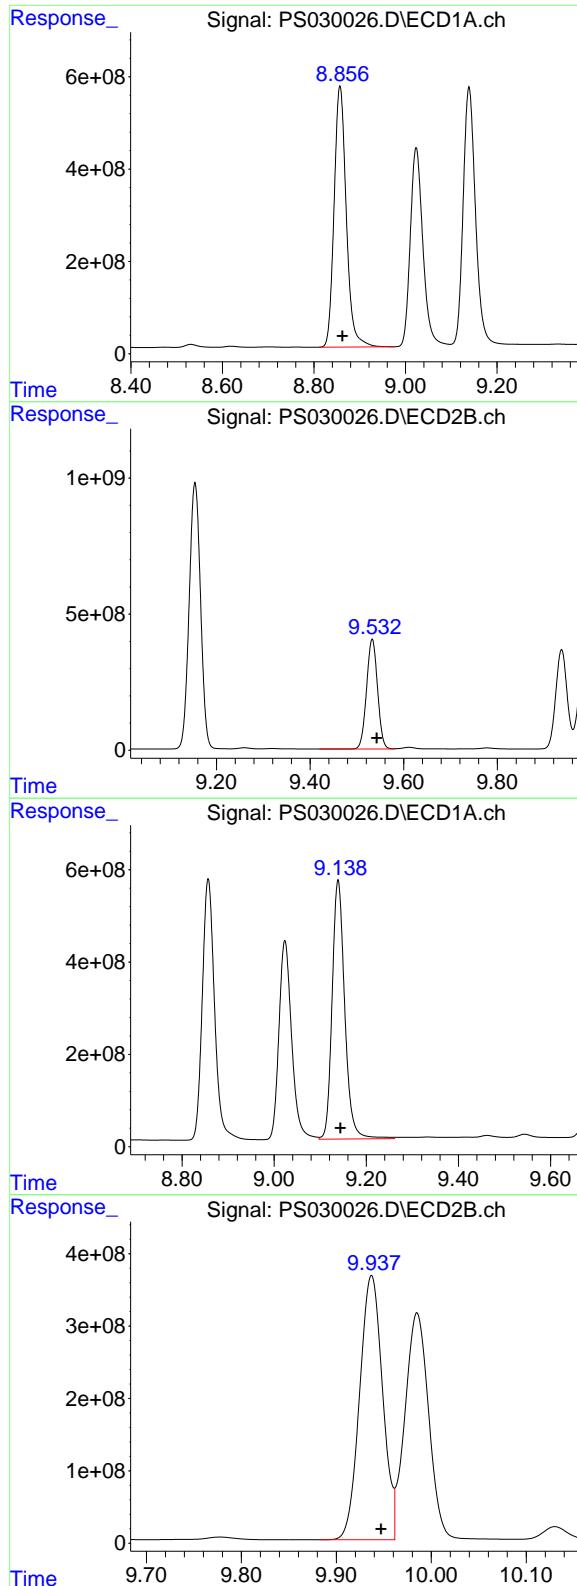

#11 2,4,5-TP (SILVEX)

R.T.: 8.857 min  
 Delta R.T.: -0.005 min  
**Instrument:**  
 Response: 10417003423 ECD\_S  
 Conc: 751.43 ng/ml  
**ClientSampleId:** HSTDCCC750

#11 2,4,5-TP (SILVEX)


R.T.: 9.533 min  
 Delta R.T.: -0.010 min  
 Response: 6556330082  
 Conc: 801.34 ng/ml

#12 2,4,5-T

R.T.: 9.139 min  
 Delta R.T.: -0.005 min  
 Response: 10641265427  
 Conc: 757.22 ng/ml

#12 2,4,5-T

R.T.: 9.937 min  
 Delta R.T.: -0.010 min  
 Response: 6136416767  
 Conc: 790.51 ng/ml

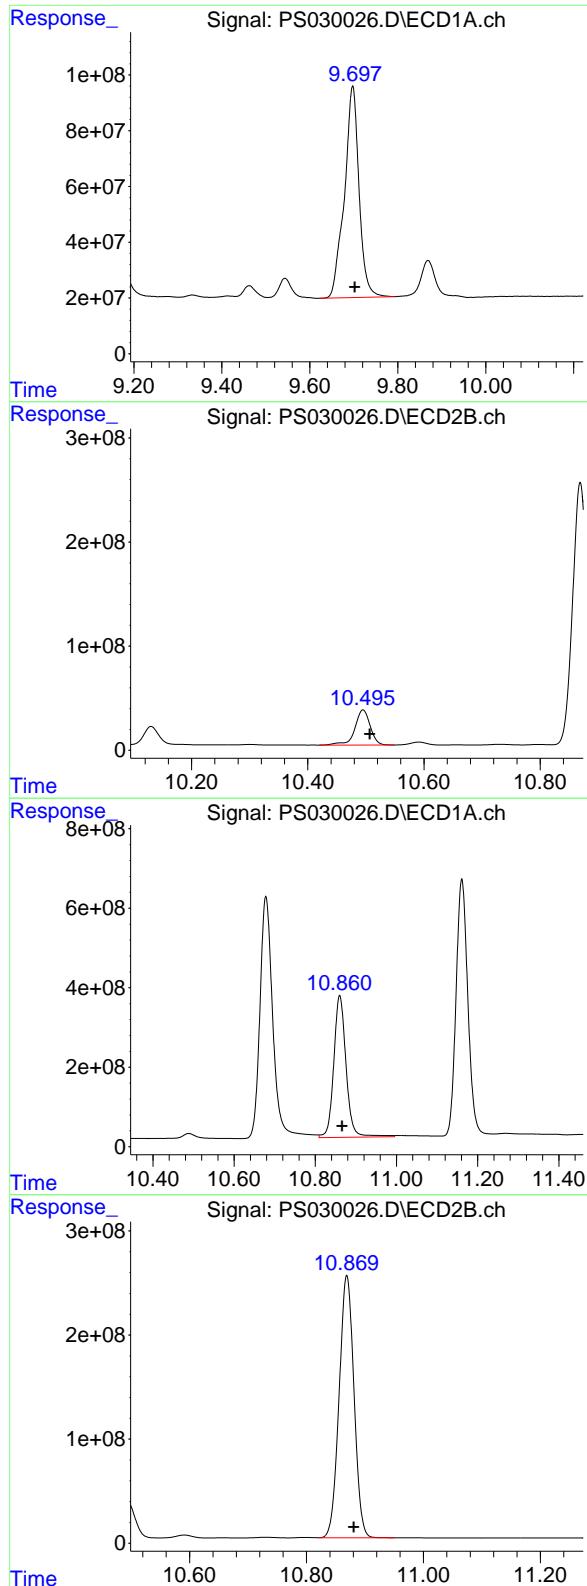

#13 2,4-DB

R.T.: 9.698 min  
 Delta R.T.: -0.004 min  
 Response: 1757631293  
 Conc: 769.08 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#13 2,4-DB


R.T.: 10.495 min  
 Delta R.T.: -0.011 min  
 Response: 617877165  
 Conc: 767.70 ng/ml

#14 DINOSEB

R.T.: 10.860 min  
 Delta R.T.: -0.006 min  
 Response: 7519170257  
 Conc: 739.10 ng/ml

#14 DINOSEB

R.T.: 10.869 min  
 Delta R.T.: -0.012 min  
 Response: 4438570711  
 Conc: 761.20 ng/ml

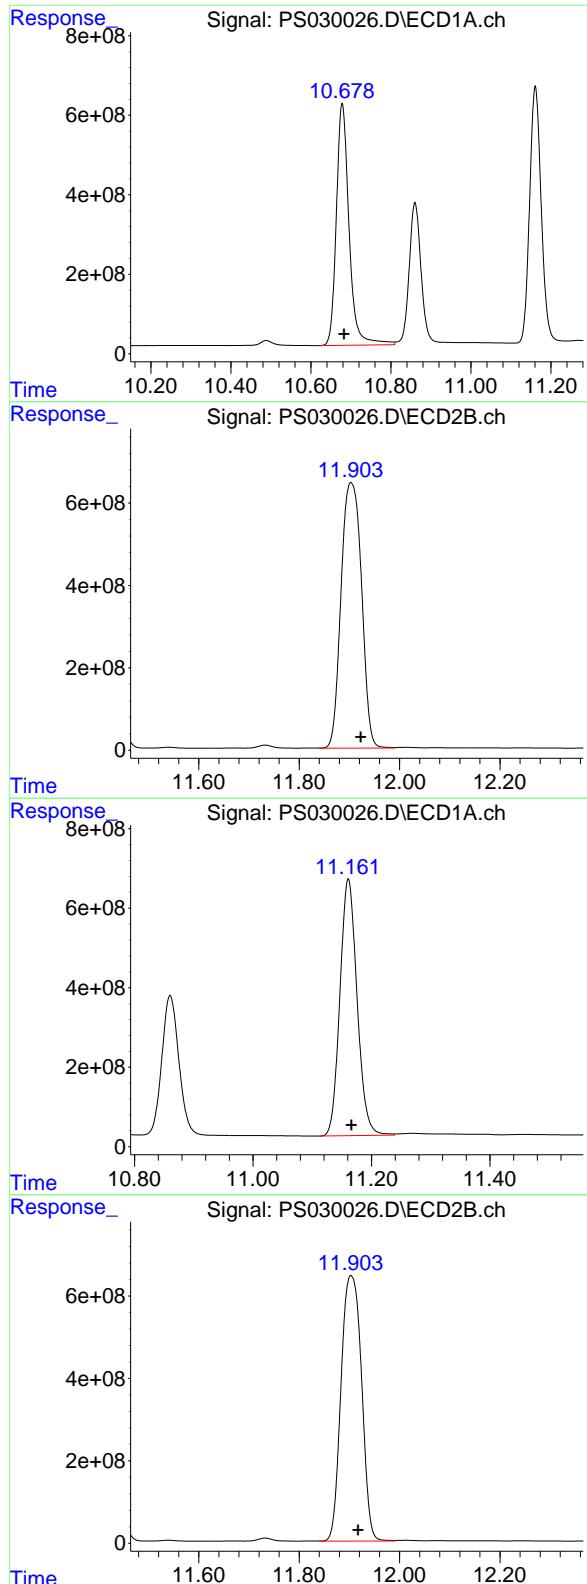

#15 Picloram

R.T.: 10.678 min  
 Delta R.T.: -0.005 min  
 Response: 13425673369  
 Conc: 732.42 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#15 Picloram

R.T.: 11.903 min  
 Delta R.T.: -0.020 min  
 Response: 18182652631  
 Conc: 1480.23 ng/ml

#16 DCPA

R.T.: 11.161 min  
 Delta R.T.: -0.005 min  
 Response: 12986203927  
 Conc: 762.95 ng/ml

#16 DCPA

R.T.: 11.903 min  
 Delta R.T.: -0.014 min  
 Response: 18182652631  
 Conc: 1613.13 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050525\  
 Data File : PS030029.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 05 May 2025 09:55  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**HSTDCCC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 05 12:26:58 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

#### System Monitoring Compounds

4) S 2,4-DCAA 6.938 7.456 1902.1E6 555.4E6 772.860 788.396

#### Target Compounds

1) T	Dalapon	2.446	2.517	3152.3E6	1268.0E6	769.749	730.345
2) T	3,5-DICHL...	6.142	6.454	2580.1E6	718.9E6	721.950	735.376
3) T	4-Nitroph...	6.728	6.990	1270.3E6	554.2E6	712.324	723.635
5) T	DICAMBA	7.114	7.642	7384.3E6	3117.7E6	745.677	789.285
6) T	MCPP	7.293	7.750	474.5E6	139.3E6	73.642	79.630
7) T	MCPA	7.436	7.981	643.1E6	166.0E6	72.816	70.169
8) T	DICHLORPROP	7.795	8.336	1922.1E6	752.9E6	758.477	749.952
9) T	2,4-D	8.015	8.649	2185.1E6	840.8E6	776.807	745.962
10) T	Pentachlo...	8.293	9.150	26374.8E6	16140.6E6	756.051	793.353
11) T	2,4,5-TP ...	8.857	9.528	10510.0E6	6415.5E6	758.140	784.122
12) T	2,4,5-T	9.140	9.933	10639.4E6	5978.3E6	757.082	770.140
13) T	2,4-DB	9.698	10.491	1760.4E6	609.3E6	770.297	757.064
14) T	DINOSEB	10.861	10.865	7541.6E6	4394.3E6	741.305	753.615
15) T	Picloram	10.679	11.901	13895.4E6	18197.0E6	758.042	1481.400 #
16) T	DCPA	11.162	11.901	12980.1E6	18197.0E6	762.591	1614.403 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050525\  
 Data File : PS030029.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 05 May 2025 09:55  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDCCC750

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 05 12:26:58 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

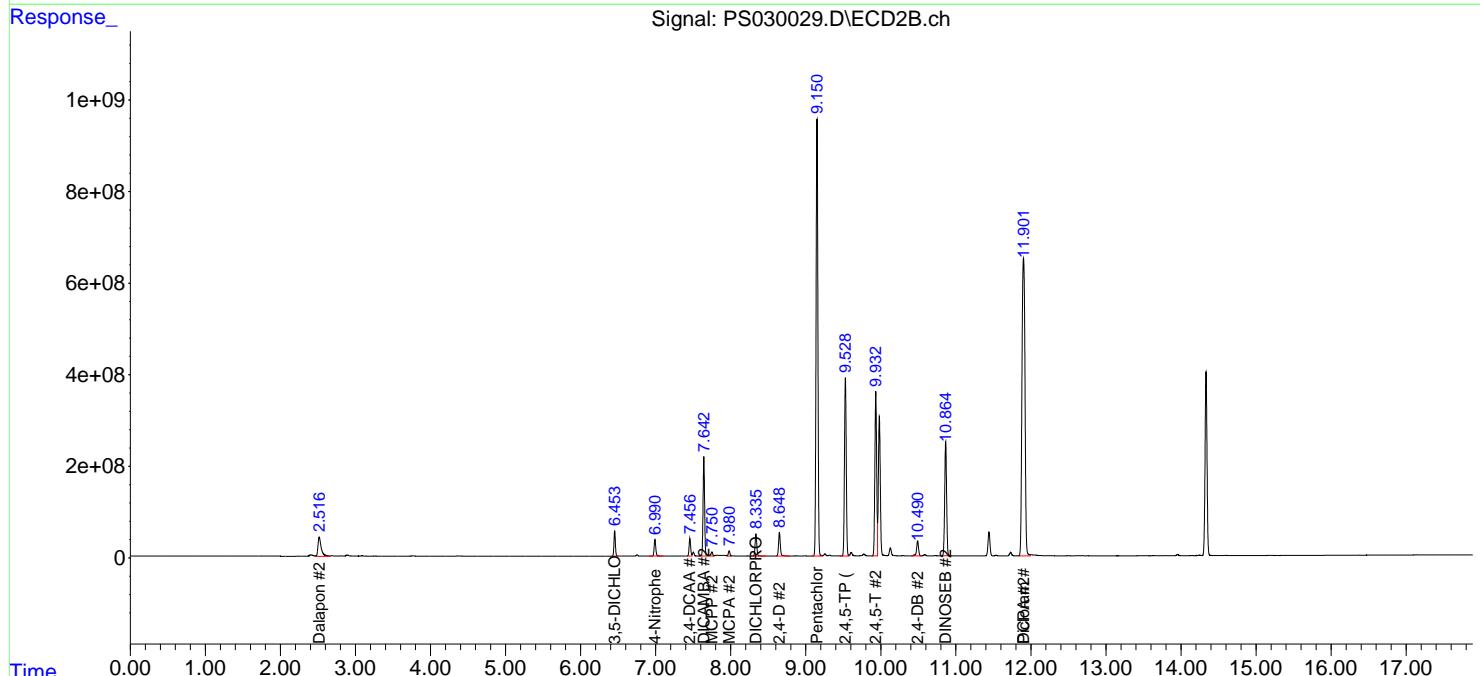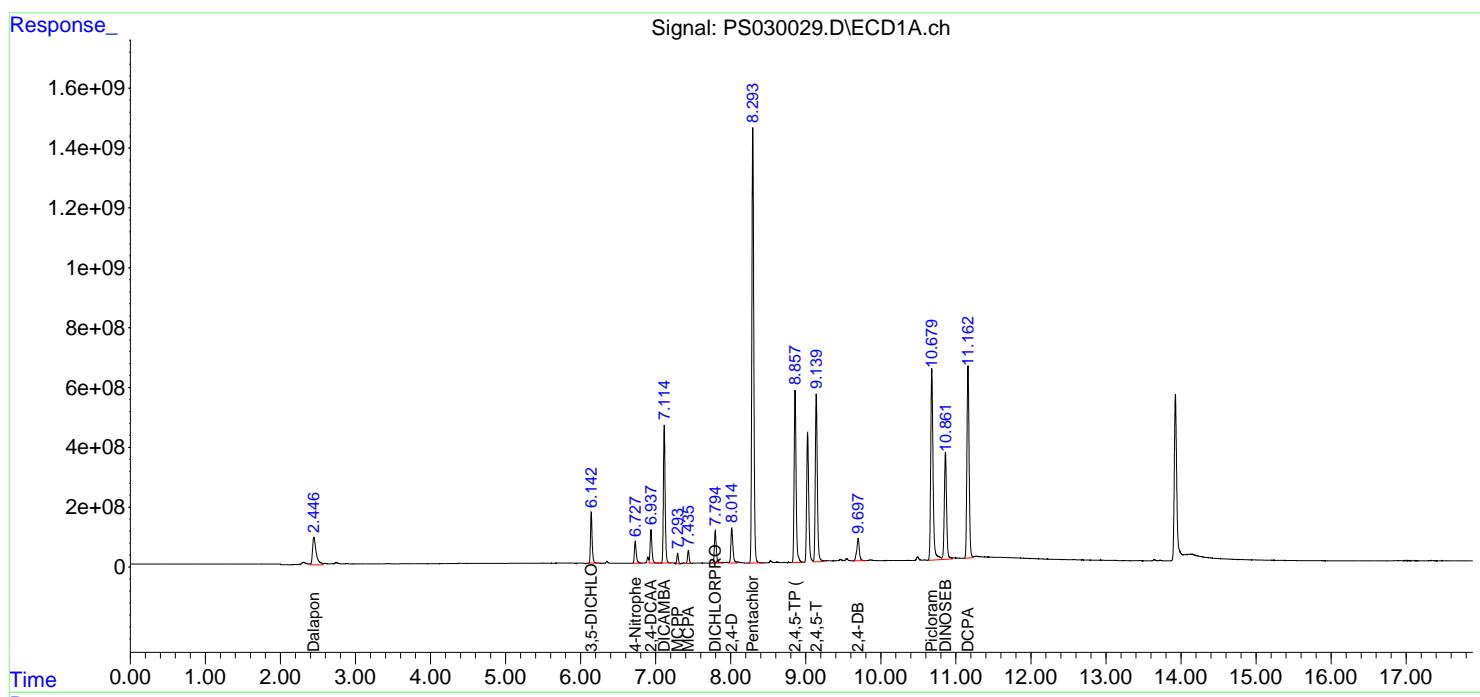

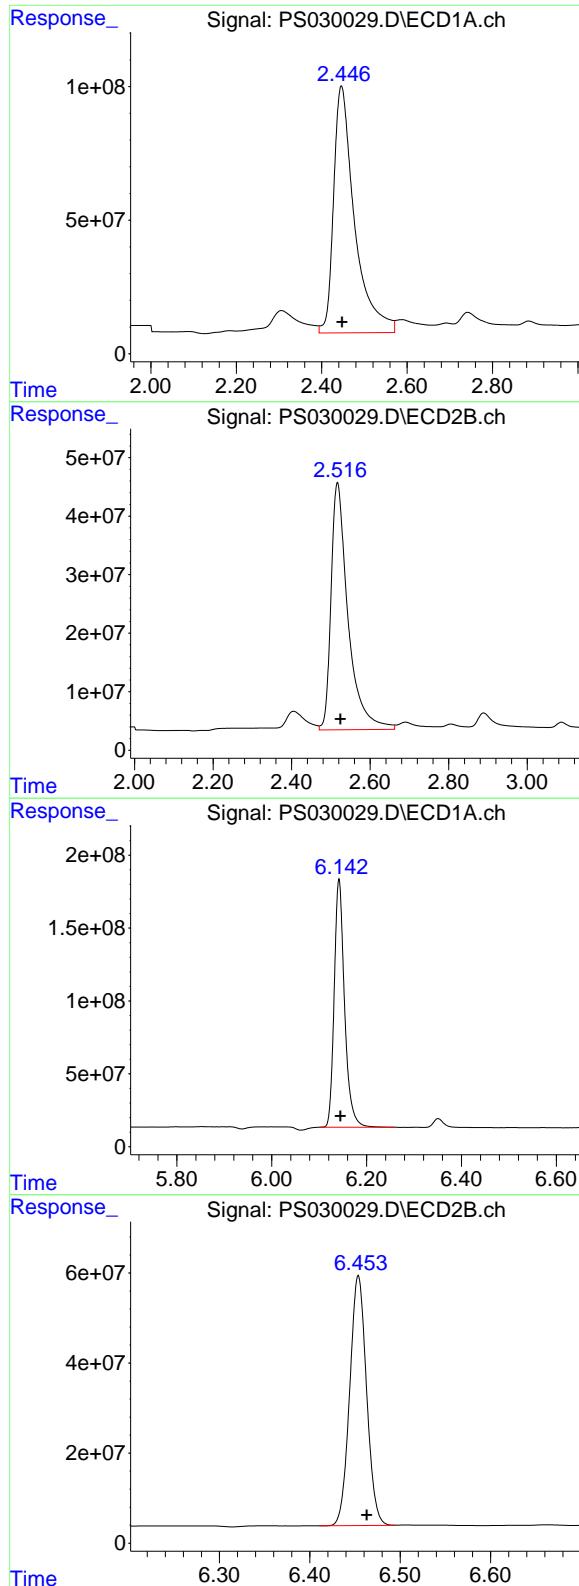

#1 Dalapon

R.T.: 2.446 min  
 Delta R.T.: -0.002 min  
 Response: 3152321923  
 Conc: 769.75 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#1 Dalapon


R.T.: 2.517 min  
 Delta R.T.: -0.008 min  
 Response: 1267983437  
 Conc: 730.34 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.142 min  
 Delta R.T.: -0.003 min  
 Response: 2580095757  
 Conc: 721.95 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.454 min  
 Delta R.T.: -0.009 min  
 Response: 718888293  
 Conc: 735.38 ng/ml

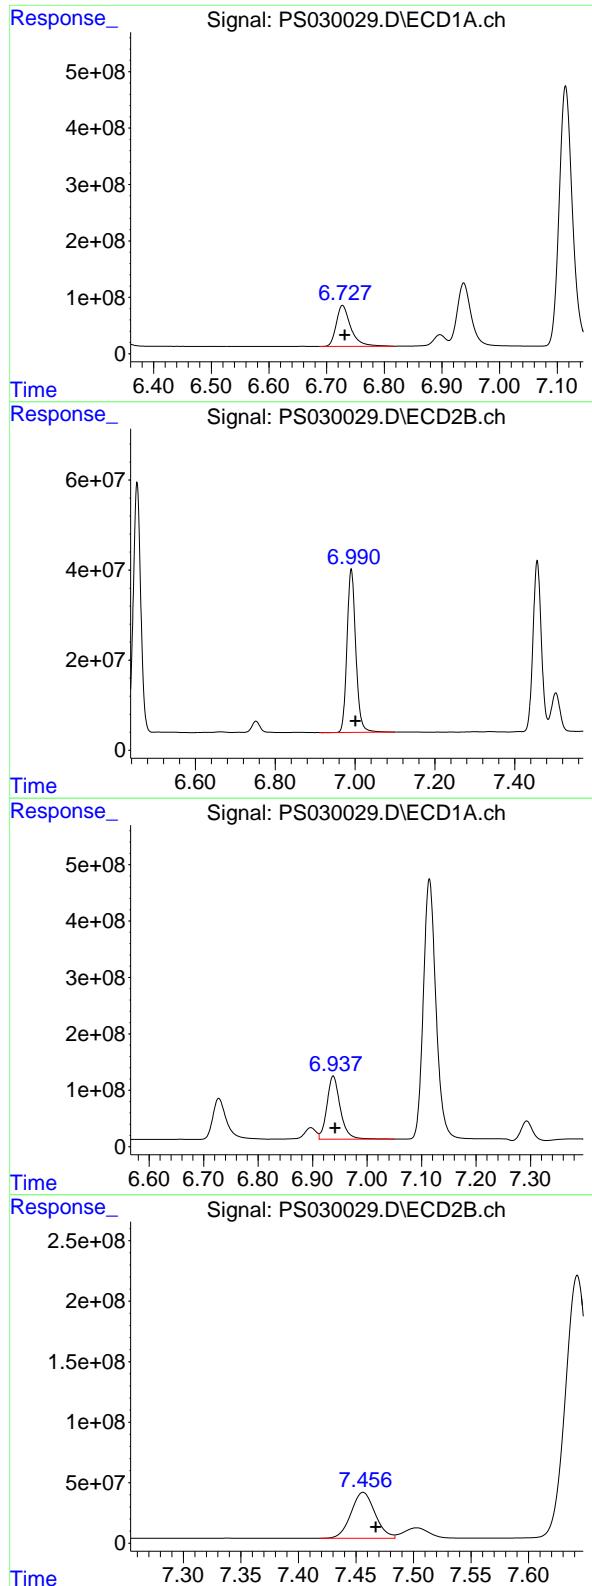

#3 4-Nitrophenol

R.T.: 6.728 min  
 Delta R.T.: -0.004 min  
 Response: 1270301802  
 Conc: 712.32 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#3 4-Nitrophenol


R.T.: 6.990 min  
 Delta R.T.: -0.010 min  
 Response: 554247176  
 Conc: 723.63 ng/ml

#4 2,4-DCAA

R.T.: 6.938 min  
 Delta R.T.: -0.004 min  
 Response: 1902069709  
 Conc: 772.86 ng/ml

#4 2,4-DCAA


R.T.: 7.456 min  
 Delta R.T.: -0.011 min  
 Response: 555438378  
 Conc: 788.40 ng/ml

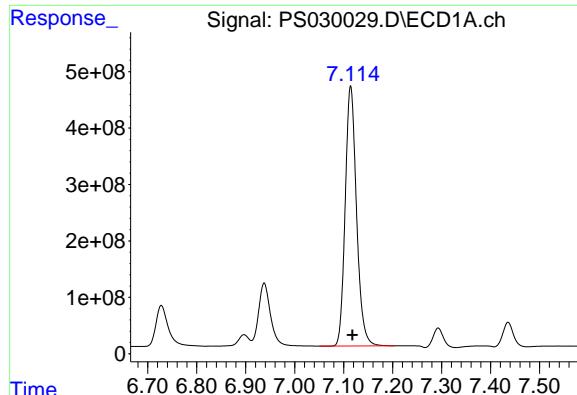

#5 DICAMBA


R.T.: 7.114 min  
 Delta R.T.: -0.004 min  
 Response: 7384334899  
 Conc: 745.68 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

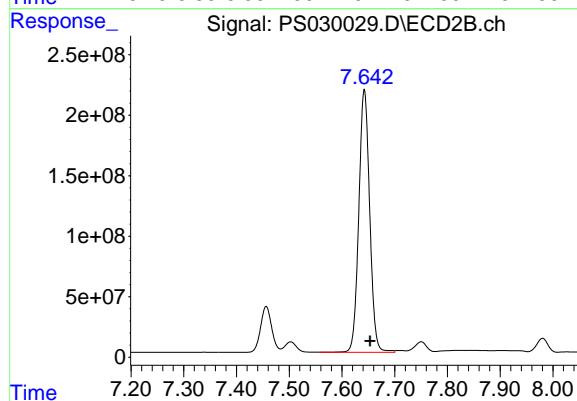


#5 DICAMBA

R.T.: 7.642 min  
 Delta R.T.: -0.011 min  
 Response: 3117725389  
 Conc: 789.28 ng/ml

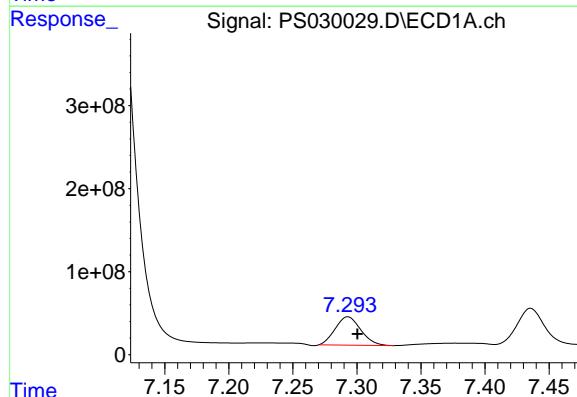


#6 MCPP

R.T.: 7.293 min  
 Delta R.T.: -0.007 min  
 Response: 474519993  
 Conc: 73.64 ug/ml

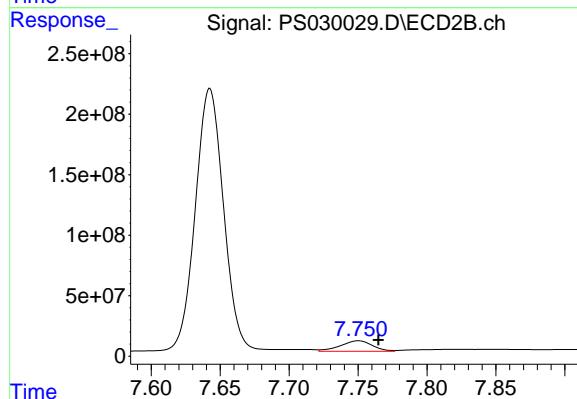

#6 MCPP


R.T.: 7.750 min  
 Delta R.T.: -0.014 min  
 Response: 139269003  
 Conc: 79.63 ug/ml

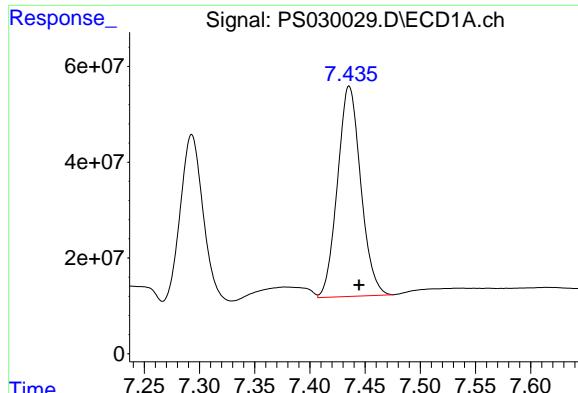

#7 MCPA


R.T.: 7.436 min  
 Delta R.T.: -0.009 min  
 Response: 643063428  
 Conc: 72.82 ug/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

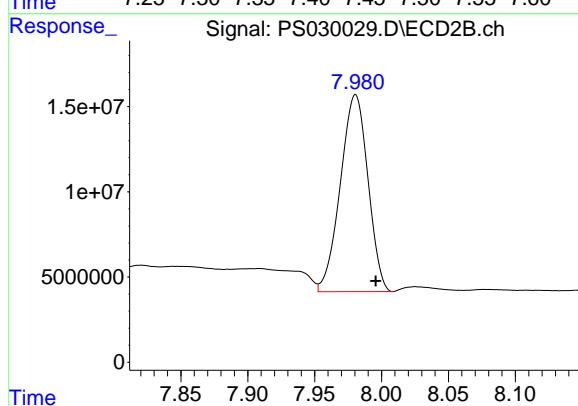


#7 MCPA

R.T.: 7.981 min  
 Delta R.T.: -0.015 min  
 Response: 166006369  
 Conc: 70.17 ug/ml

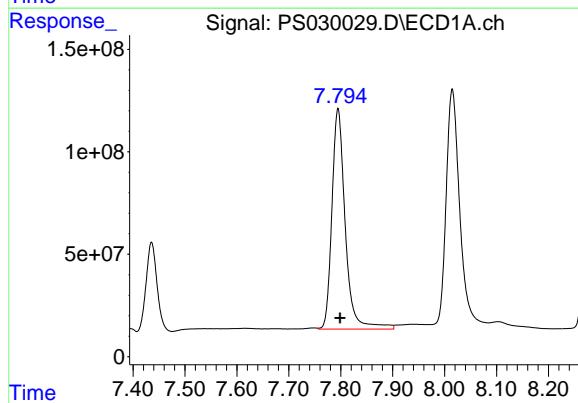


#8 DICHLOPROP

R.T.: 7.795 min  
 Delta R.T.: -0.004 min  
 Response: 1922063526  
 Conc: 758.48 ng/ml

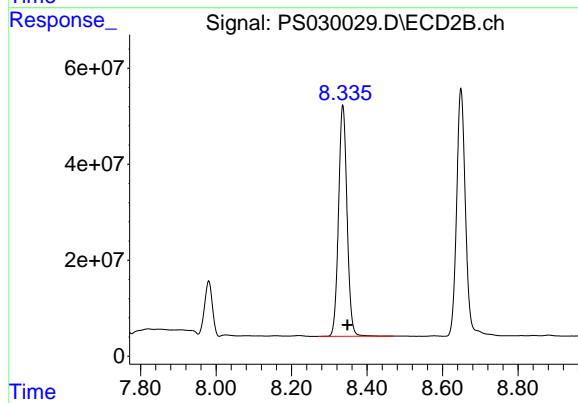

#8 DICHLOPROP

R.T.: 8.336 min  
 Delta R.T.: -0.012 min  
 Response: 752925374  
 Conc: 749.95 ng/ml

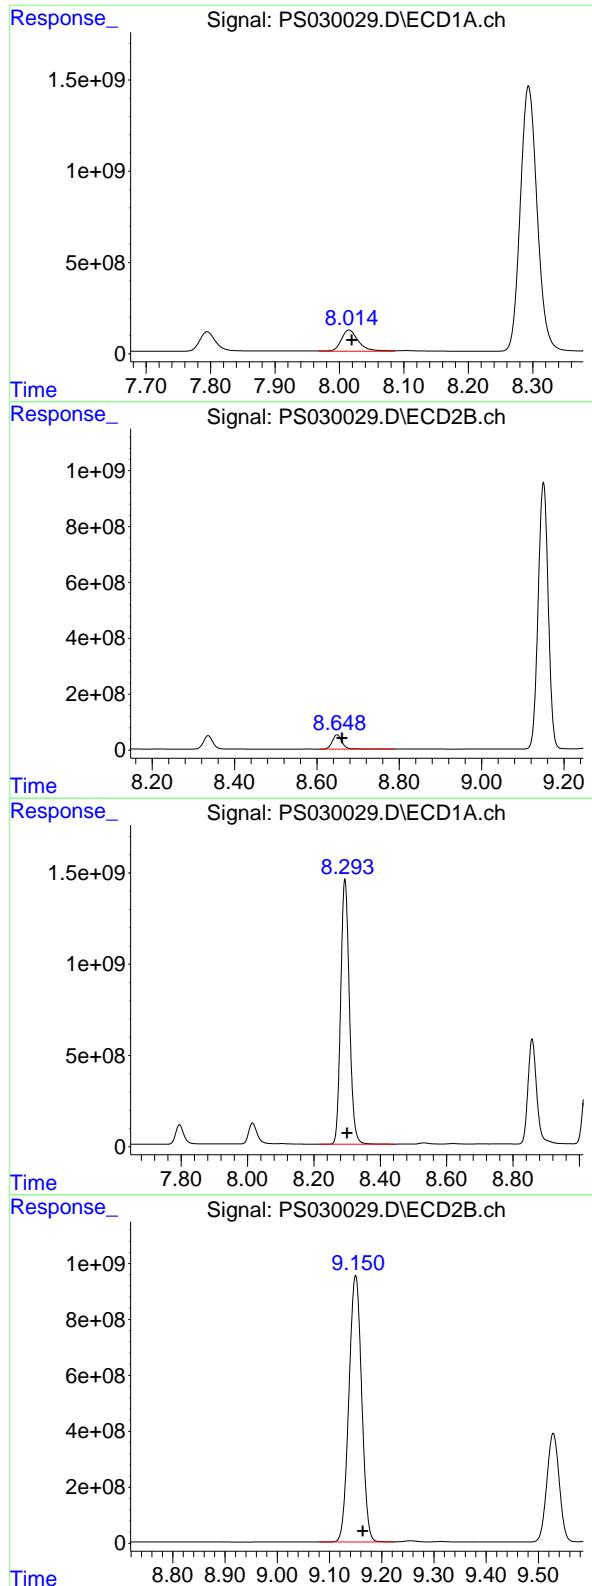

#9 2,4-D

R.T.: 8.015 min  
 Delta R.T.: -0.004 min  
 Response: 2185058539  
 Conc: 776.81 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#9 2,4-D


R.T.: 8.649 min  
 Delta R.T.: -0.012 min  
 Response: 840778929  
 Conc: 745.96 ng/ml

#10 Pentachlorophenol

R.T.: 8.293 min  
 Delta R.T.: -0.006 min  
 Response: 26374849284  
 Conc: 756.05 ng/ml

#10 Pentachlorophenol


R.T.: 9.150 min  
 Delta R.T.: -0.013 min  
 Response: 16140623302  
 Conc: 793.35 ng/ml

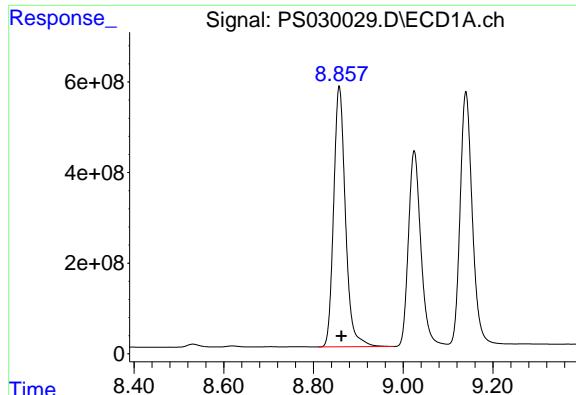

#11 2,4,5-TP (SILVEX)


R.T.: 8.857 min  
 Delta R.T.: -0.005 min  
 Response: 10509968082  
 Conc: 758.14 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

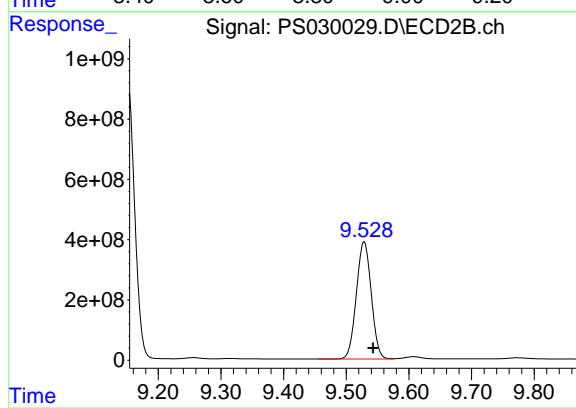


#11 2,4,5-TP (SILVEX)

R.T.: 9.528 min  
 Delta R.T.: -0.014 min  
 Response: 6415490809  
 Conc: 784.12 ng/ml

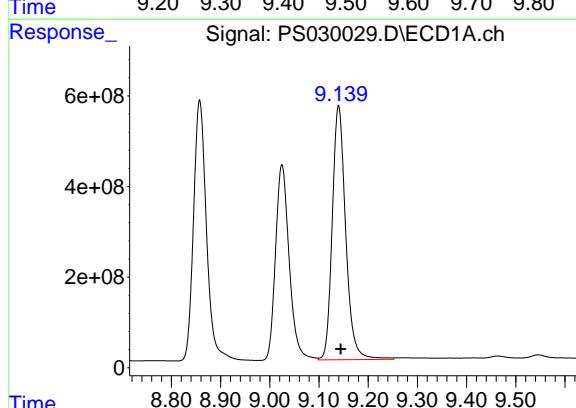


#12 2,4,5-T

R.T.: 9.140 min  
 Delta R.T.: -0.004 min  
 Response: 10639353854  
 Conc: 757.08 ng/ml

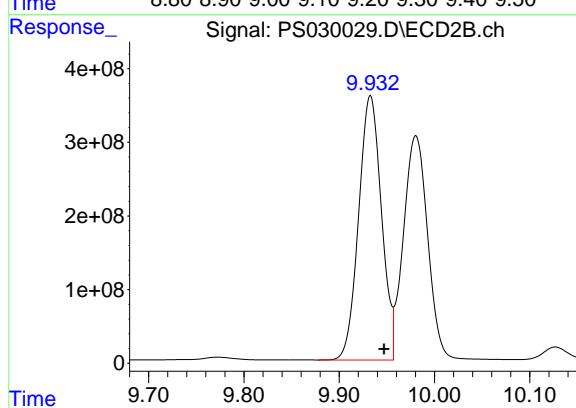

#12 2,4,5-T

R.T.: 9.933 min  
 Delta R.T.: -0.015 min  
 Response: 5978287108  
 Conc: 770.14 ng/ml

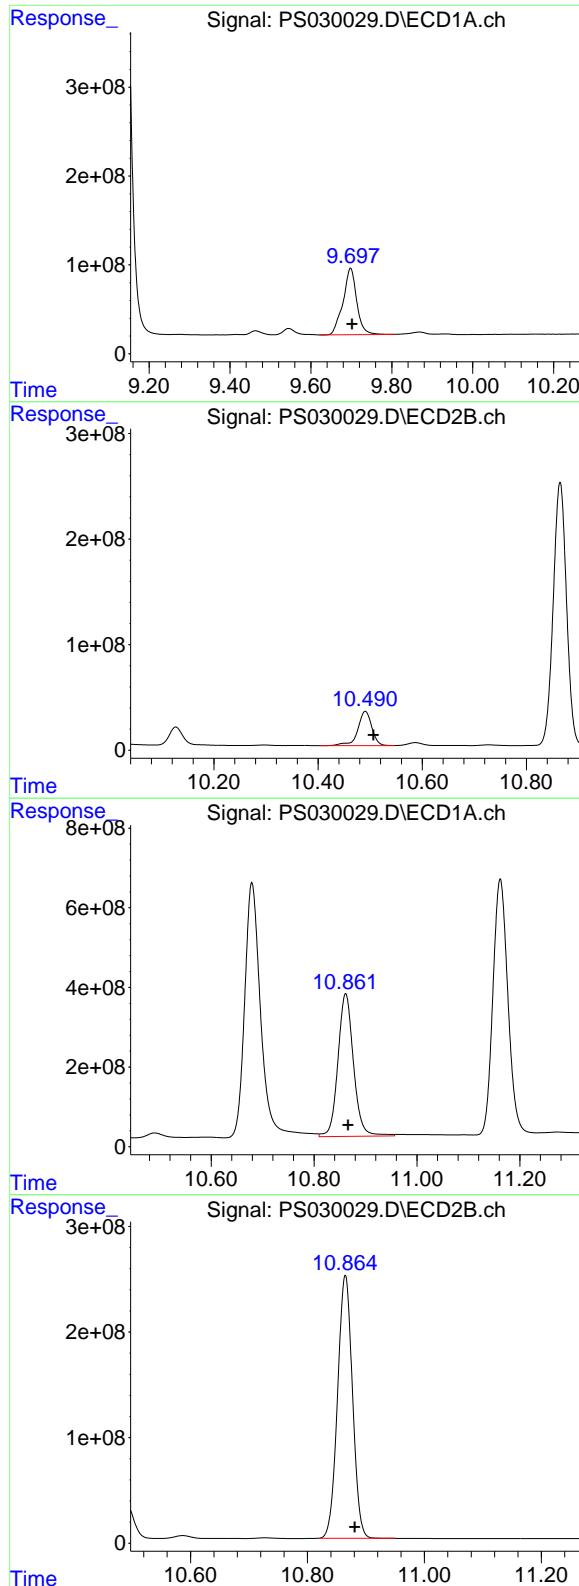

#13 2,4-DB

R.T.: 9.698 min  
 Delta R.T.: -0.004 min  
 Response: 1760403680  
 Conc: 770.30 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#13 2,4-DB


R.T.: 10.491 min  
 Delta R.T.: -0.016 min  
 Response: 609316861  
 Conc: 757.06 ng/ml

#14 DINOSEB

R.T.: 10.861 min  
 Delta R.T.: -0.004 min  
 Response: 7541611717  
 Conc: 741.30 ng/ml

#14 DINOSEB

R.T.: 10.865 min  
 Delta R.T.: -0.016 min  
 Response: 4394315725  
 Conc: 753.62 ng/ml

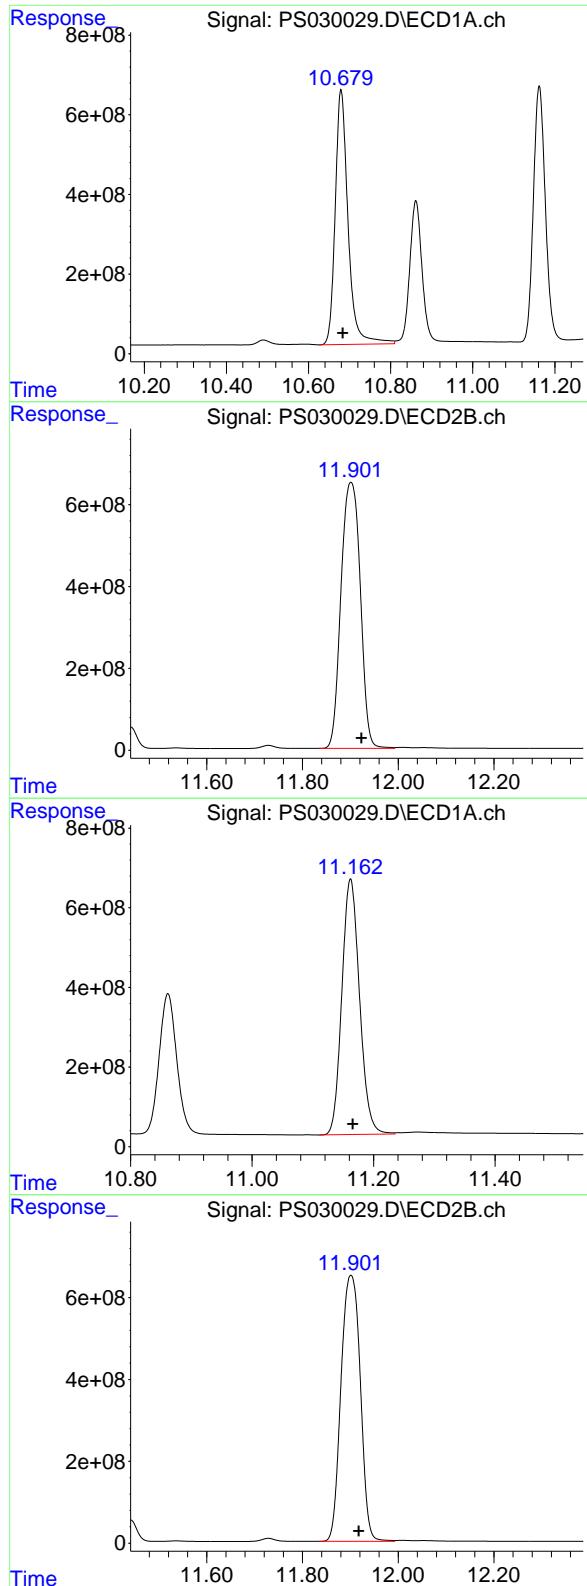

#15 Picloram

R.T.: 10.679 min  
 Delta R.T.: -0.004 min  
 Response: 13895378925  
 Conc: 758.04 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#15 Picloram

R.T.: 11.901 min  
 Delta R.T.: -0.022 min  
 Response: 18196986696  
 Conc: 1481.40 ng/ml

#16 DCPA

R.T.: 11.162 min  
 Delta R.T.: -0.004 min  
 Response: 12980066848  
 Conc: 762.59 ng/ml

#16 DCPA

R.T.: 11.901 min  
 Delta R.T.: -0.016 min  
 Response: 18196986696  
 Conc: 1614.40 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050525\  
 Data File : PS030038.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 05 May 2025 13:47  
 Operator : AR\AJ  
 Sample : PB167796BS  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**PB167796BS**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 06 01:38:53 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.937 7.461 1303.7E6 380.1E6 529.742 539.538

Target Compounds

1) T	Dalapon	2.449	2.523	2026.9E6	836.0E6	494.933	481.542
2) T	3,5-DICHL...	6.142	6.459	1748.8E6	487.0E6	489.353	498.167
3) T	4-Nitroph...	6.728	6.996	852.1E6	376.7E6	477.797	491.891
5) T	DICAMBA	7.114	7.647	4939.4E6	2039.7E6	498.784	516.364
6) T	MCPP	7.292	7.753	295.3E6	80604259	45.824	46.087
7) T	MCPA	7.434	7.983	412.6E6	112.5E6	46.719	47.564
8) T	DICHLORPROP	7.794	8.340	1243.9E6	517.9E6	490.874	515.829
9) T	2,4-D	8.014	8.653	1407.4E6	573.8E6	500.356	509.096
10) T	Pentachlo...	8.292	9.154	18046.0E6	10930.7E6	517.300	537.274
11) T	2,4,5-TP ...	8.856	9.532	7064.9E6	4305.5E6	509.626	526.230
12) T	2,4,5-T	9.138	9.936	7219.0E6	4034.3E6	513.694	519.714
13) T	2,4-DB	9.697	10.495	1180.4E6	404.5E6	516.485	502.607
14) T	DINOSEB	10.859	10.868	5116.9E6	2968.0E6	502.969	509.004
15) T	Picloram	10.678	11.903	9032.0E6	11894.2E6	492.728	968.299 #
16) T	DCPA	11.160	11.903	8804.0E6	11894.2E6	517.242	1055.234 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050525\  
 Data File : PS030038.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 05 May 2025 13:47  
 Operator : AR\AJ  
 Sample : PB167796BS  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 PB167796BS

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 06 01:38:53 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

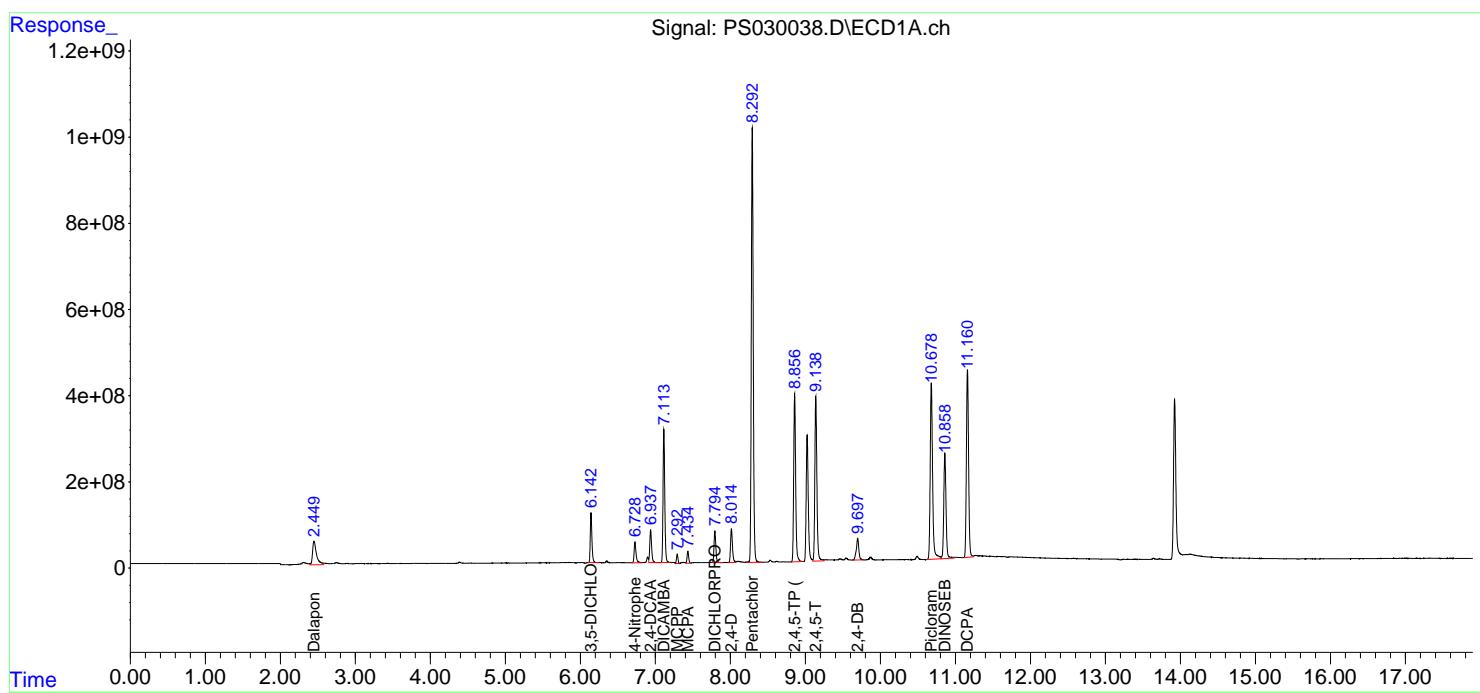

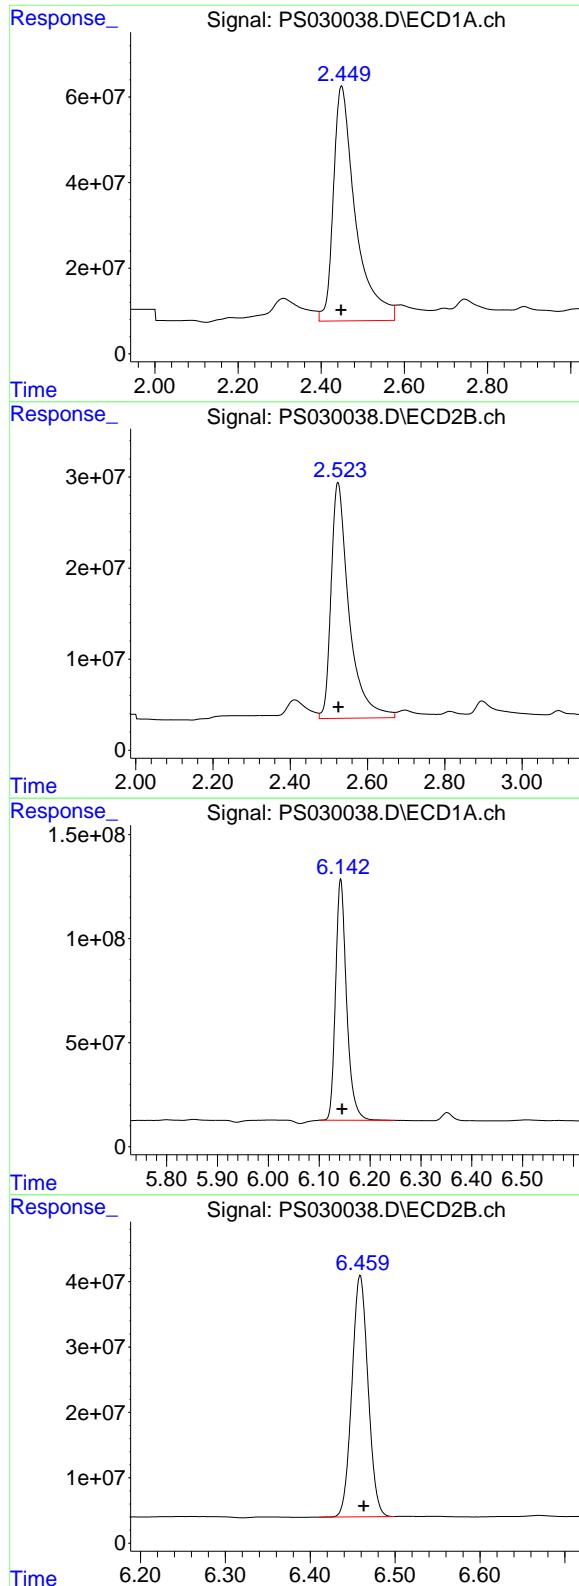

#1 Dalapon

R.T.: 2.449 min  
Delta R.T.: 0.000 min  
Response: 2026876943  
Conc: 494.93 ng/ml

Instrument: ECD\_S  
ClientSampleId: PB167796BS

#1 Dalapon


R.T.: 2.523 min  
Delta R.T.: -0.001 min  
Response: 836026719  
Conc: 481.54 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.142 min  
Delta R.T.: -0.003 min  
Response: 1748841469  
Conc: 489.35 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.459 min  
Delta R.T.: -0.004 min  
Response: 486997904  
Conc: 498.17 ng/ml

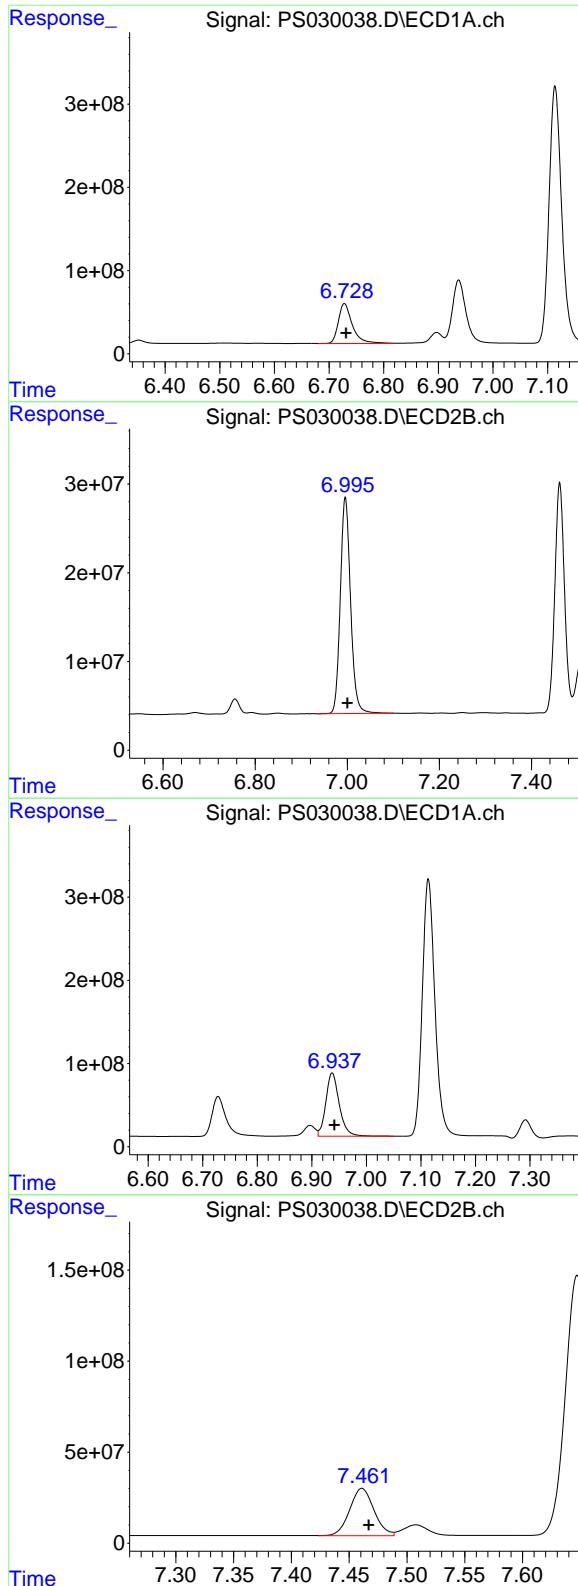

#3 4-Nitrophenol

R.T.: 6.728 min  
 Delta R.T.: -0.003 min  
 Response: 852065133  
 Conc: 477.80 ng/ml

Instrument: ECD\_S  
 ClientSampleId: PB167796BS

#3 4-Nitrophenol


R.T.: 6.996 min  
 Delta R.T.: -0.005 min  
 Response: 376749767  
 Conc: 491.89 ng/ml

#4 2,4-DCAA

R.T.: 6.937 min  
 Delta R.T.: -0.004 min  
 Response: 1303737946  
 Conc: 529.74 ng/ml

#4 2,4-DCAA

R.T.: 7.461 min  
 Delta R.T.: -0.006 min  
 Response: 380113891  
 Conc: 539.54 ng/ml

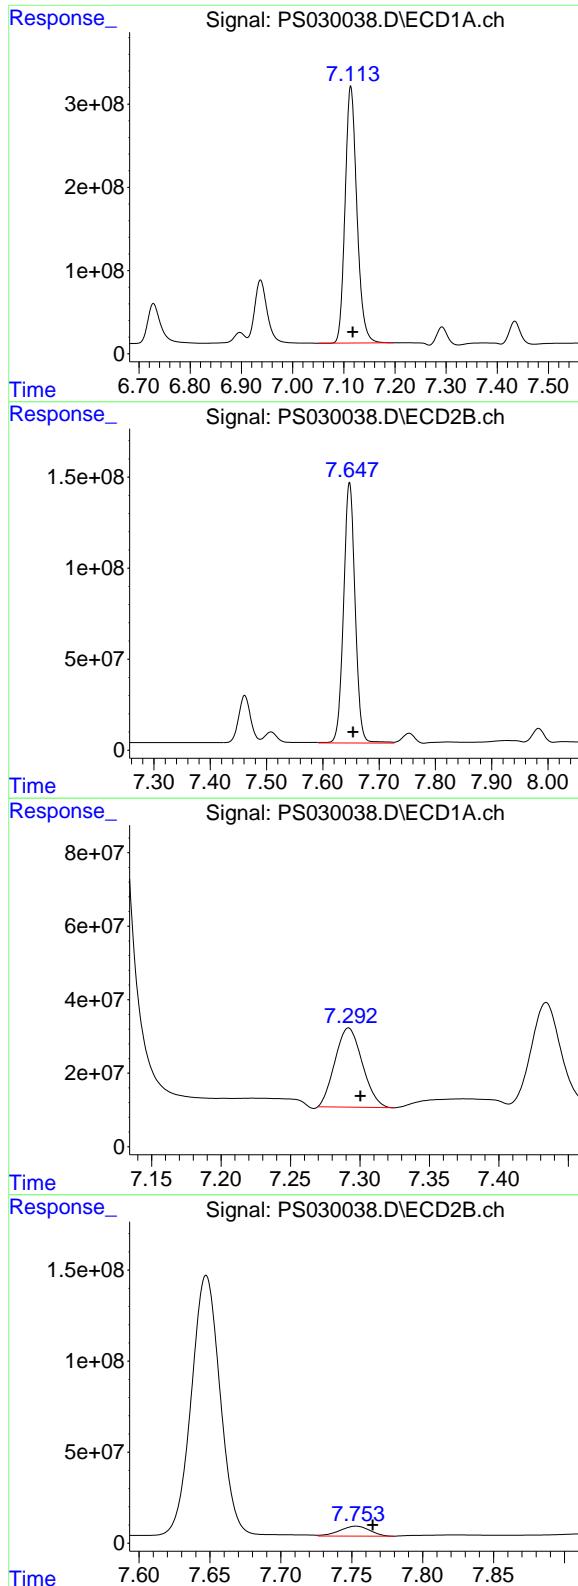

#5 DICAMBA

R.T.: 7.114 min  
 Delta R.T.: -0.004 min  
 Response: 4939392609  
 Conc: 498.78 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** PB167796BS

#5 DICAMBA


R.T.: 7.647 min  
 Delta R.T.: -0.006 min  
 Response: 2039671767  
 Conc: 516.36 ng/ml

#6 MCPP

R.T.: 7.292 min  
 Delta R.T.: -0.008 min  
 Response: 295272711  
 Conc: 45.82 ug/ml

#6 MCPP

R.T.: 7.753 min  
 Delta R.T.: -0.012 min  
 Response: 80604259  
 Conc: 46.09 ug/ml

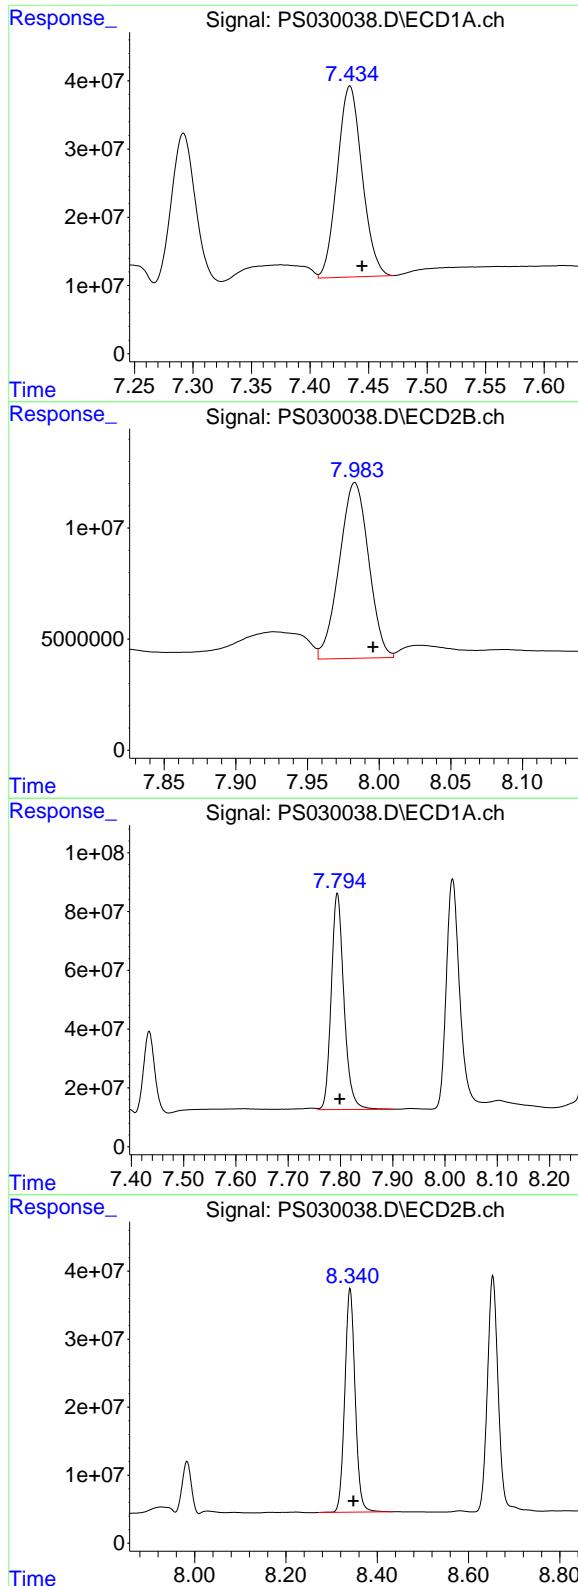

#7 MCPA

R.T.: 7.434 min  
 Delta R.T.: -0.010 min  
 Response: 412595382  
 Conc: 46.72 ug/ml

Instrument: ECD\_S  
 ClientSampleId: PB167796BS

#7 MCPA


R.T.: 7.983 min  
 Delta R.T.: -0.013 min  
 Response: 112526574  
 Conc: 47.56 ug/ml

#8 DICHLOPROP

R.T.: 7.794 min  
 Delta R.T.: -0.005 min  
 Response: 1243928182  
 Conc: 490.87 ng/ml

#8 DICHLOPROP

R.T.: 8.340 min  
 Delta R.T.: -0.007 min  
 Response: 517874081  
 Conc: 515.83 ng/ml

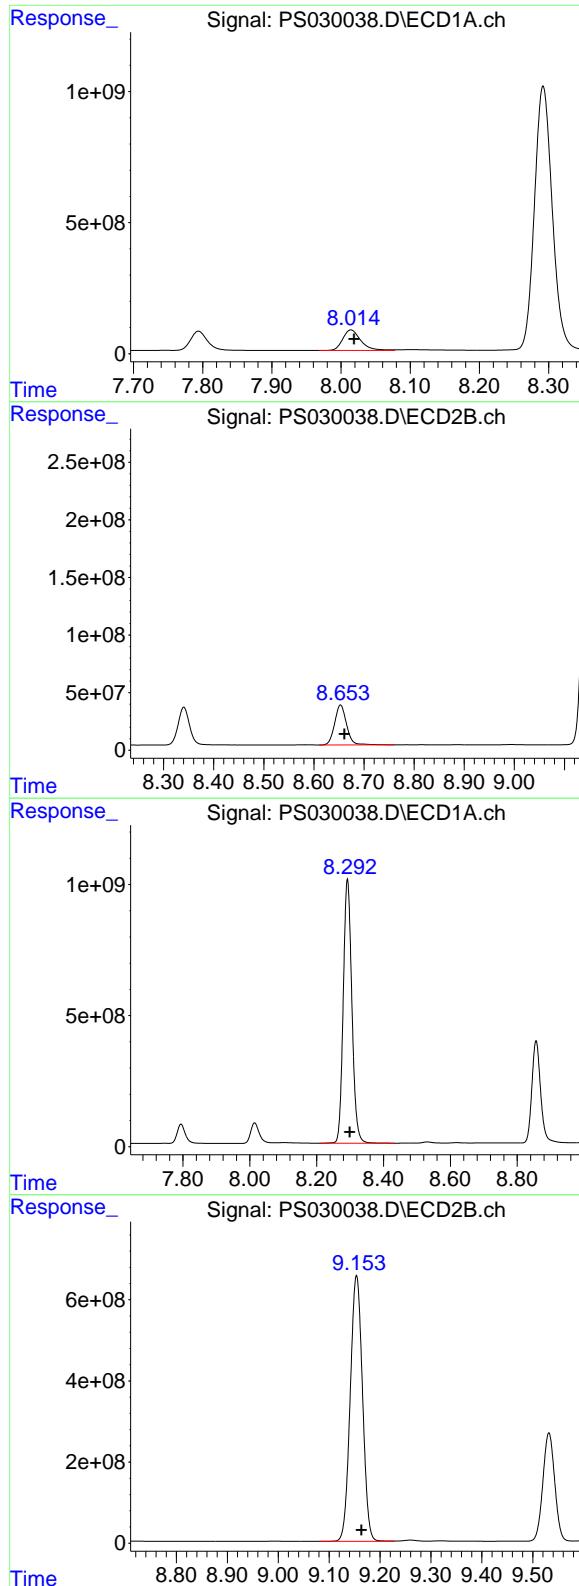

#9 2,4-D

R.T.: 8.014 min  
 Delta R.T.: -0.004 min  
 Response: 1407438073  
 Conc: 500.36 ng/ml

Instrument: ECD\_S  
 ClientSampleId: PB167796BS

#9 2,4-D


R.T.: 8.653 min  
 Delta R.T.: -0.008 min  
 Response: 573806176  
 Conc: 509.10 ng/ml

#10 Pentachlorophenol

R.T.: 8.292 min  
 Delta R.T.: -0.008 min  
 Response: 18046010957  
 Conc: 517.30 ng/ml

#10 Pentachlorophenol

R.T.: 9.154 min  
 Delta R.T.: -0.010 min  
 Response: 10930731101  
 Conc: 537.27 ng/ml

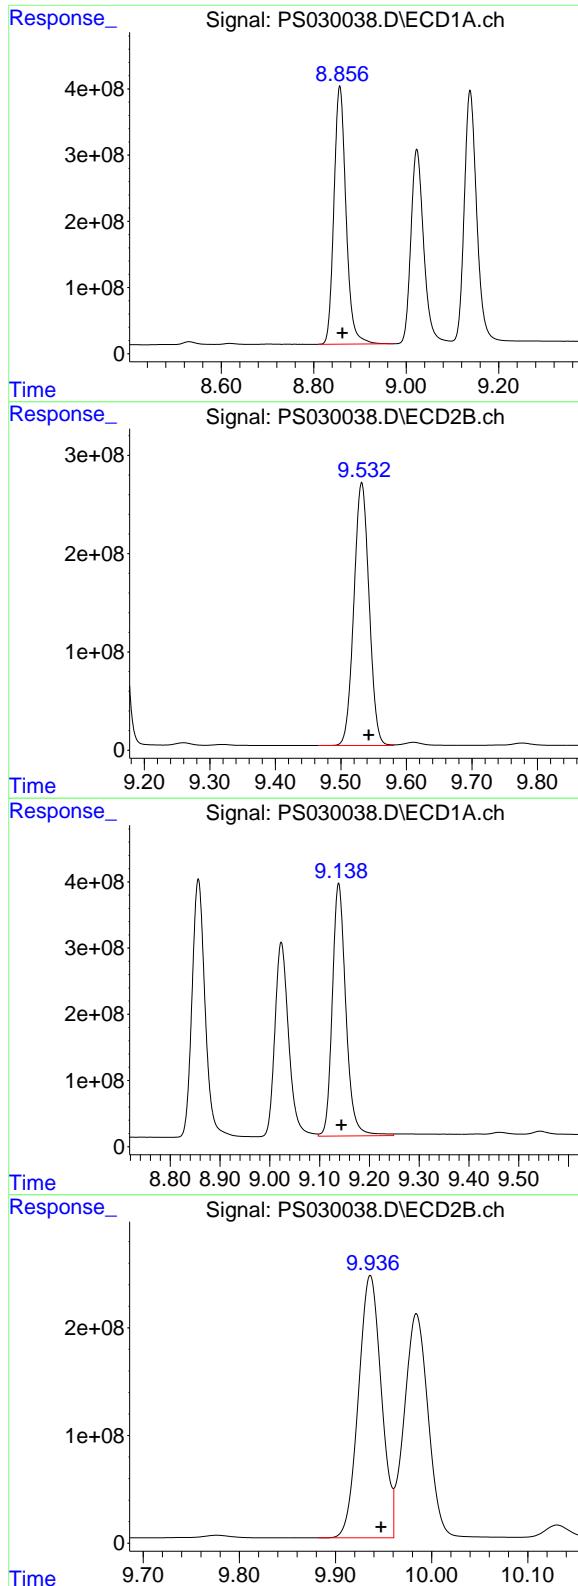

#11 2,4,5-TP (SILVEX)

R.T.: 8.856 min  
 Delta R.T.: -0.006 min  
 Response: 7064866109  
 Conc: 509.63 ng/ml

Instrument: ECD\_S  
 ClientSampleId: PB167796BS

#11 2,4,5-TP (SILVEX)


R.T.: 9.532 min  
 Delta R.T.: -0.011 min  
 Response: 4305484681  
 Conc: 526.23 ng/ml

#12 2,4,5-T

R.T.: 9.138 min  
 Delta R.T.: -0.006 min  
 Response: 7218996712  
 Conc: 513.69 ng/ml

#12 2,4,5-T

R.T.: 9.936 min  
 Delta R.T.: -0.011 min  
 Response: 4034329145  
 Conc: 519.71 ng/ml

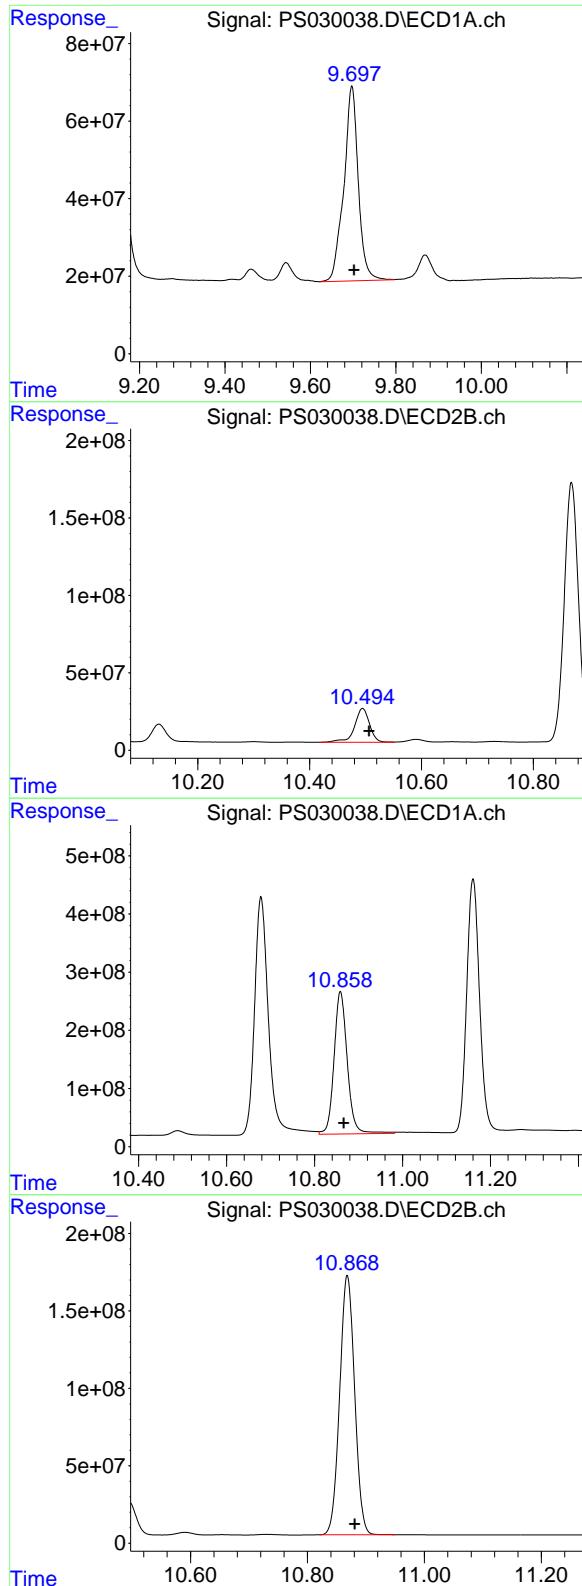

#13 2,4-DB

R.T.: 9.697 min  
 Delta R.T.: -0.005 min **Instrument:**  
 Response: 1180351095 ECD\_S  
 Conc: 516.48 ng/ml **ClientSampleId:**  
 PB167796BS

#13 2,4-DB


R.T.: 10.495 min  
 Delta R.T.: -0.012 min  
 Response: 404519772  
 Conc: 502.61 ng/ml

#14 DINOSEB

R.T.: 10.859 min  
 Delta R.T.: -0.007 min  
 Response: 5116917707  
 Conc: 502.97 ng/ml

#14 DINOSEB

R.T.: 10.868 min  
 Delta R.T.: -0.013 min  
 Response: 2967993353  
 Conc: 509.00 ng/ml

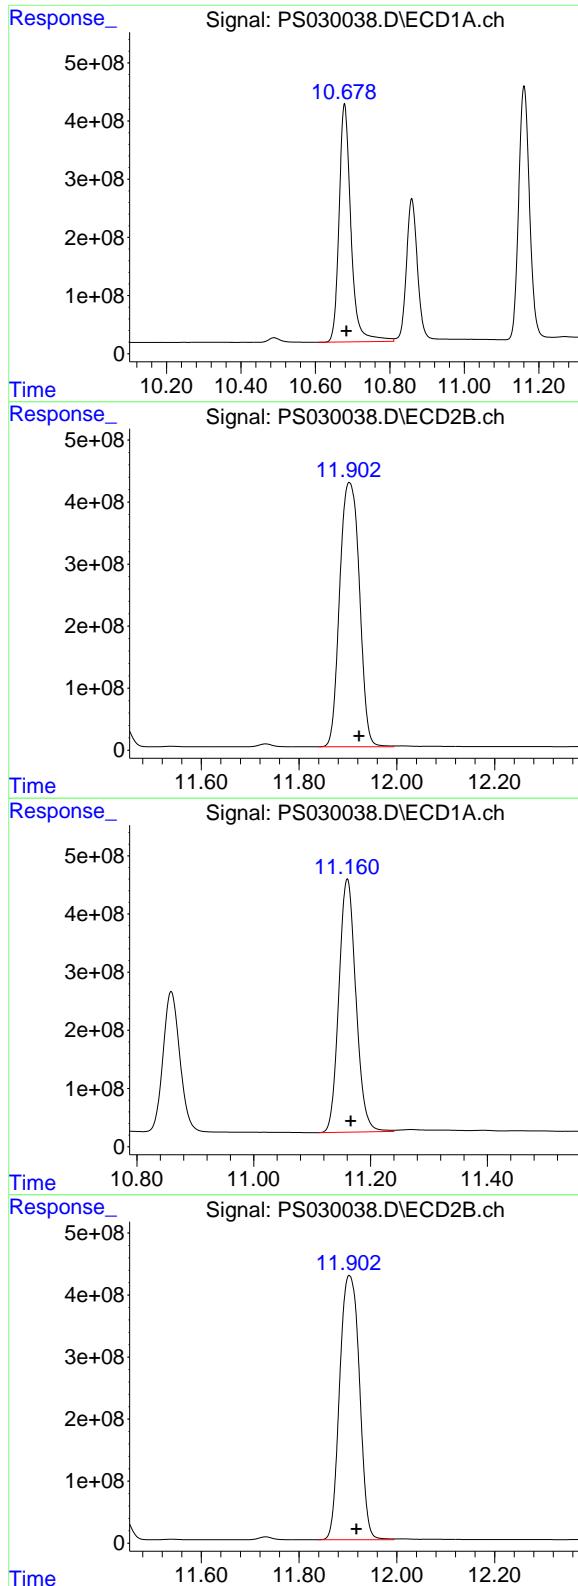

#15 Picloram

R.T.: 10.678 min  
 Delta R.T.: -0.005 min  
 Response: 9032014243  
 Conc: 492.73 ng/ml

Instrument: ECD\_S  
 ClientSampleId: PB167796BS

#15 Picloram

R.T.: 11.903 min  
 Delta R.T.: -0.020 min  
 Response: 11894233948  
 Conc: 968.30 ng/ml

#16 DCPA

R.T.: 11.160 min  
 Delta R.T.: -0.006 min  
 Response: 8803982200  
 Conc: 517.24 ng/ml

#16 DCPA

R.T.: 11.903 min  
 Delta R.T.: -0.015 min  
 Response: 11894233948  
 Conc: 1055.23 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050525\  
 Data File : PS030041.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 05 May 2025 16:41  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
**ECD\_S**  
**ClientSampleId :**  
**HSTDCCC750**

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 06 01:40:04 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S 2,4-DCAA 6.936 7.455 1774.9E6 519.6E6 721.191 737.501

Target Compounds

1) T	Dalapon	2.445	2.516	2952.4E6	1171.6E6	720.926	674.830
2) T	3,5-DICHL...	6.141	6.453	2409.7E6	672.1E6	674.261	687.519
3) T	4-Nitroph...	6.727	6.989	1181.1E6	497.0E6	662.301	648.827
5) T	DICAMBA	7.114	7.642	6817.6E6	2886.7E6	688.443	730.789
6) T	MCPP	7.292	7.748	422.5E6	110.6E6	65.574	63.223
7) T	MCPA	7.435	7.979	581.0E6	149.4E6	65.784	63.137
8) T	DICHLORPROP	7.794	8.335	1709.9E6	711.0E6	674.770	708.151
9) T	2,4-D	8.014	8.648	1935.2E6	785.2E6	687.965	696.646
10) T	Pentachlo...	8.292	9.149	24554.7E6	15042.3E6	703.874	739.367
11) T	2,4,5-TP ...	8.857	9.527	9759.5E6	5967.9E6	704.004	729.413
12) T	2,4,5-T	9.139	9.932	9937.7E6	5585.4E6	707.156	719.532
13) T	2,4-DB	9.699	10.490	1639.3E6	557.8E6	717.316	693.045
14) T	DINOSEB	10.861	10.864	7113.6E6	4063.2E6	699.237	696.838
15) T	Picloram	10.680	11.902	13035.9E6	16973.2E6	711.154	1381.772 #
16) T	DCPA	11.162	11.902	12175.4E6	16973.2E6	715.318	1505.830 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS050525\  
 Data File : PS030041.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 05 May 2025 16:41  
 Operator : AR\AJ  
 Sample : HSTDCCC750  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 HSTDCCC750

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 06 01:40:04 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS042325.M  
 Quant Title : 8080.M  
 QLast Update : Wed Apr 23 12:57:40 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25 $\mu$ m

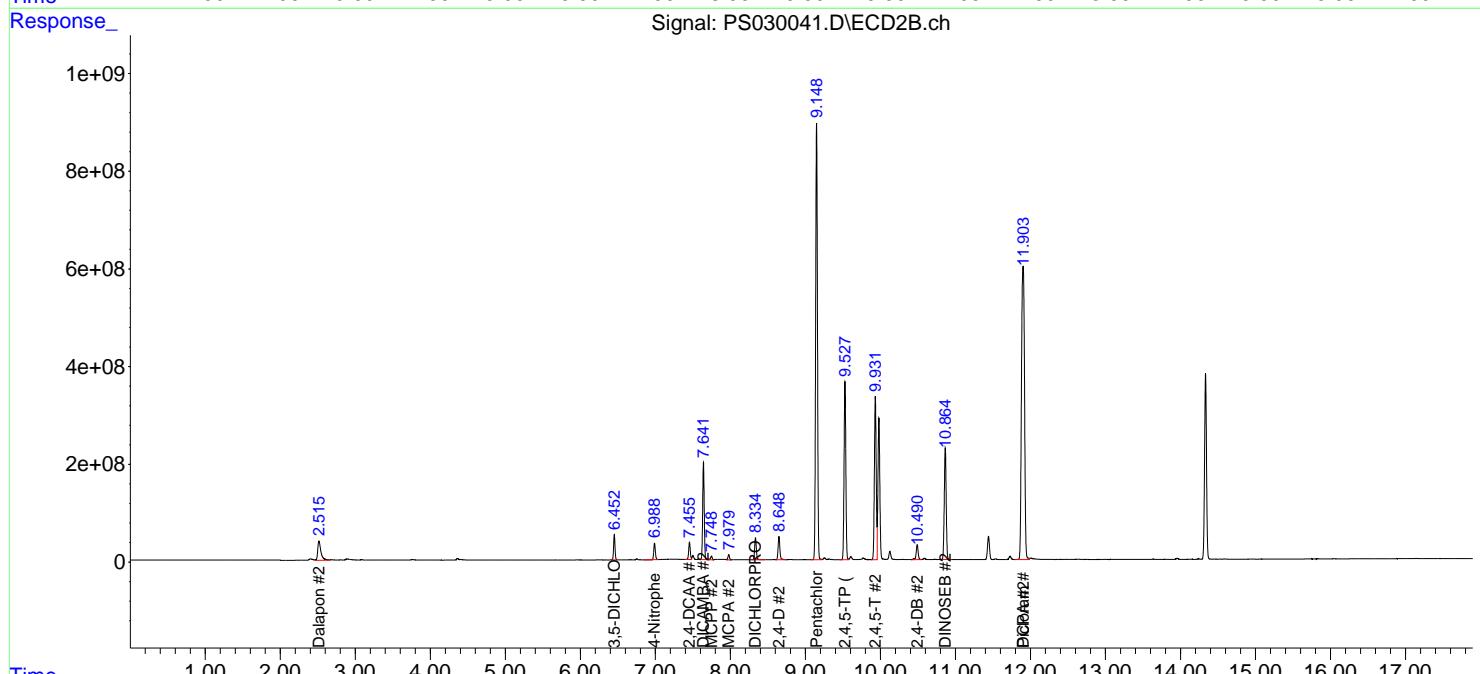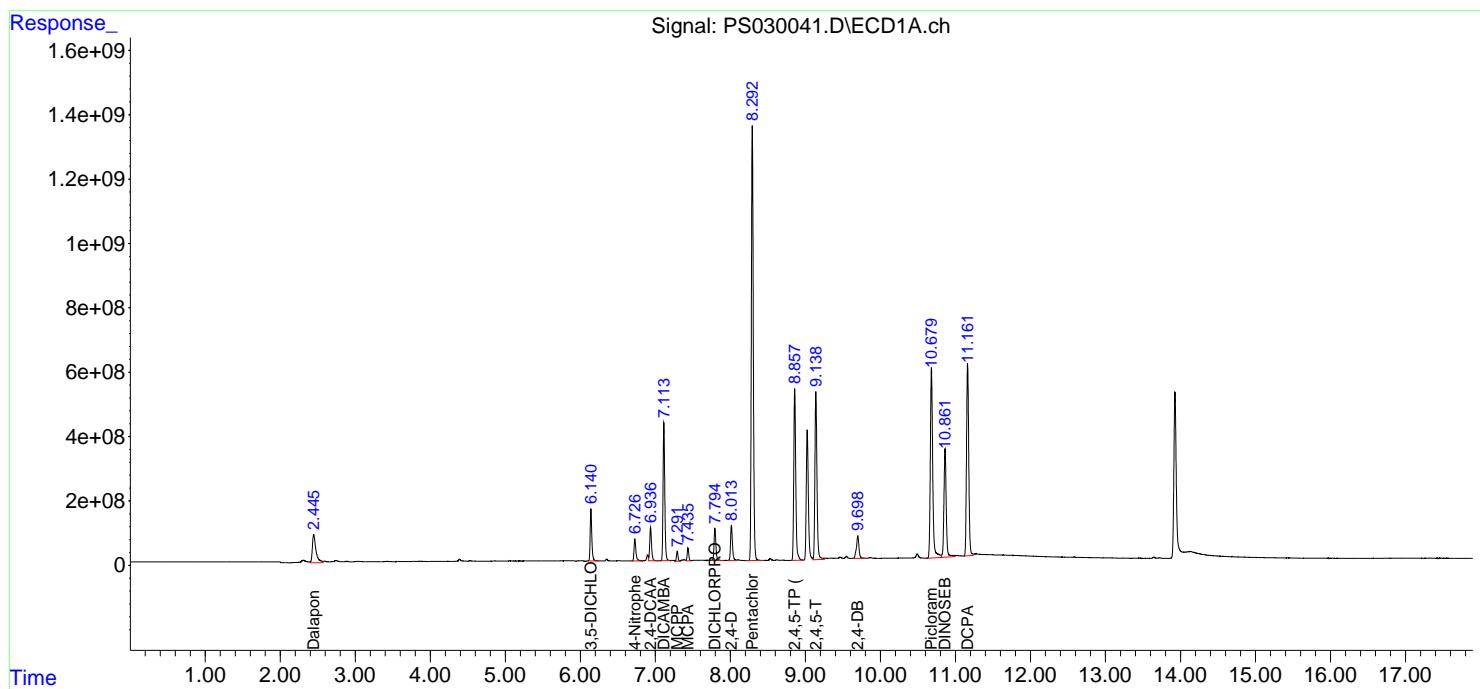

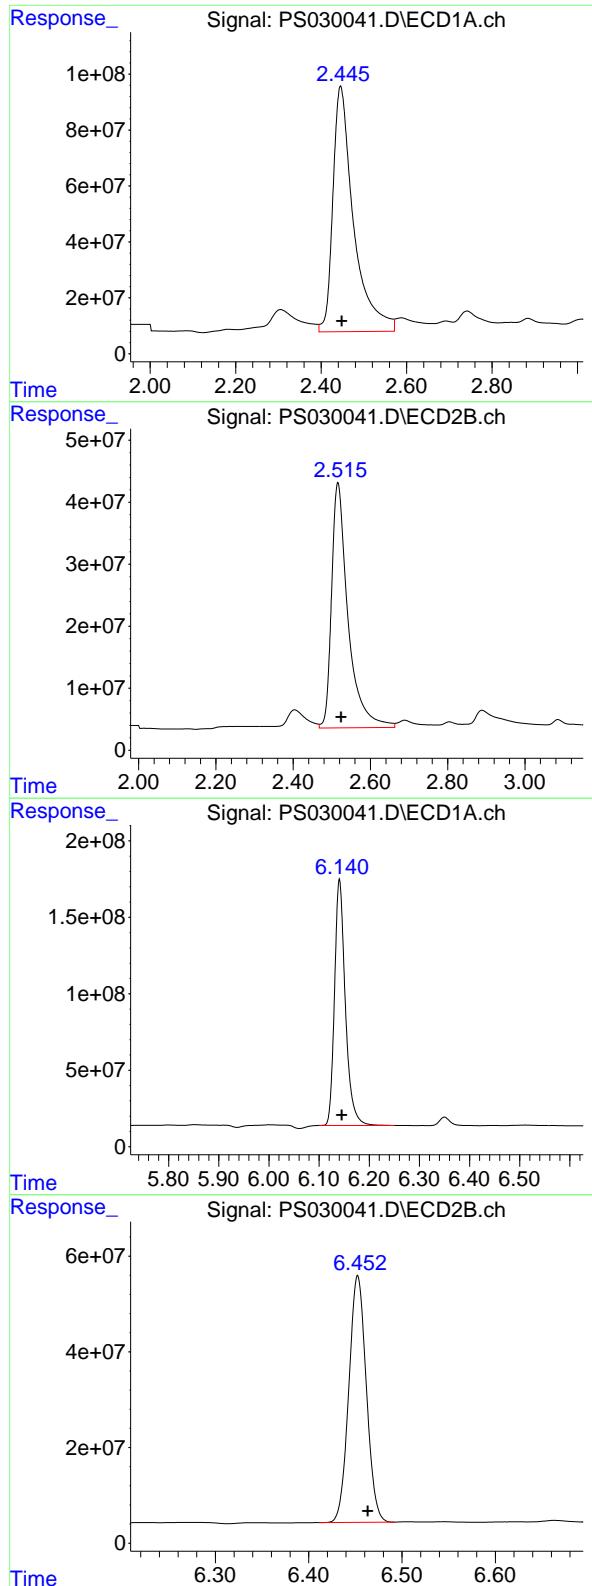

#1 Dalapon

R.T.: 2.445 min  
 Delta R.T.: -0.003 min  
 Response: 2952377655  
 Conc: 720.93 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#1 Dalapon


R.T.: 2.516 min  
 Delta R.T.: -0.009 min  
 Response: 1171602771  
 Conc: 674.83 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.141 min  
 Delta R.T.: -0.005 min  
 Response: 2409663155  
 Conc: 674.26 ng/ml

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.453 min  
 Delta R.T.: -0.010 min  
 Response: 672104770  
 Conc: 687.52 ng/ml

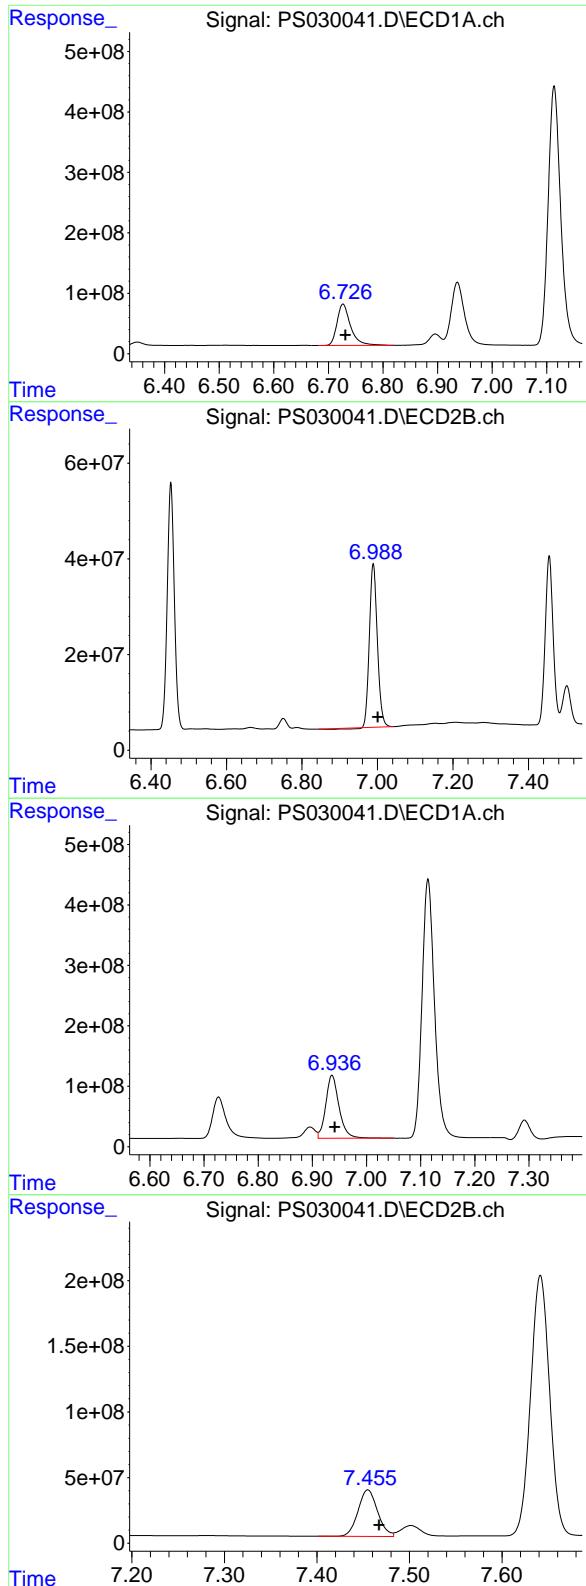

#3 4-Nitrophenol

R.T.: 6.727 min  
 Delta R.T.: -0.005 min  
 Response: 1181094054  
 Conc: 662.30 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** HSTDCCC750

#3 4-Nitrophenol


R.T.: 6.989 min  
 Delta R.T.: -0.012 min  
 Response: 496950659  
 Conc: 648.83 ng/ml

#4 2,4-DCAA

R.T.: 6.936 min  
 Delta R.T.: -0.005 min  
 Response: 1774908871  
 Conc: 721.19 ng/ml

#4 2,4-DCAA

R.T.: 7.455 min  
 Delta R.T.: -0.012 min  
 Response: 519581780  
 Conc: 737.50 ng/ml

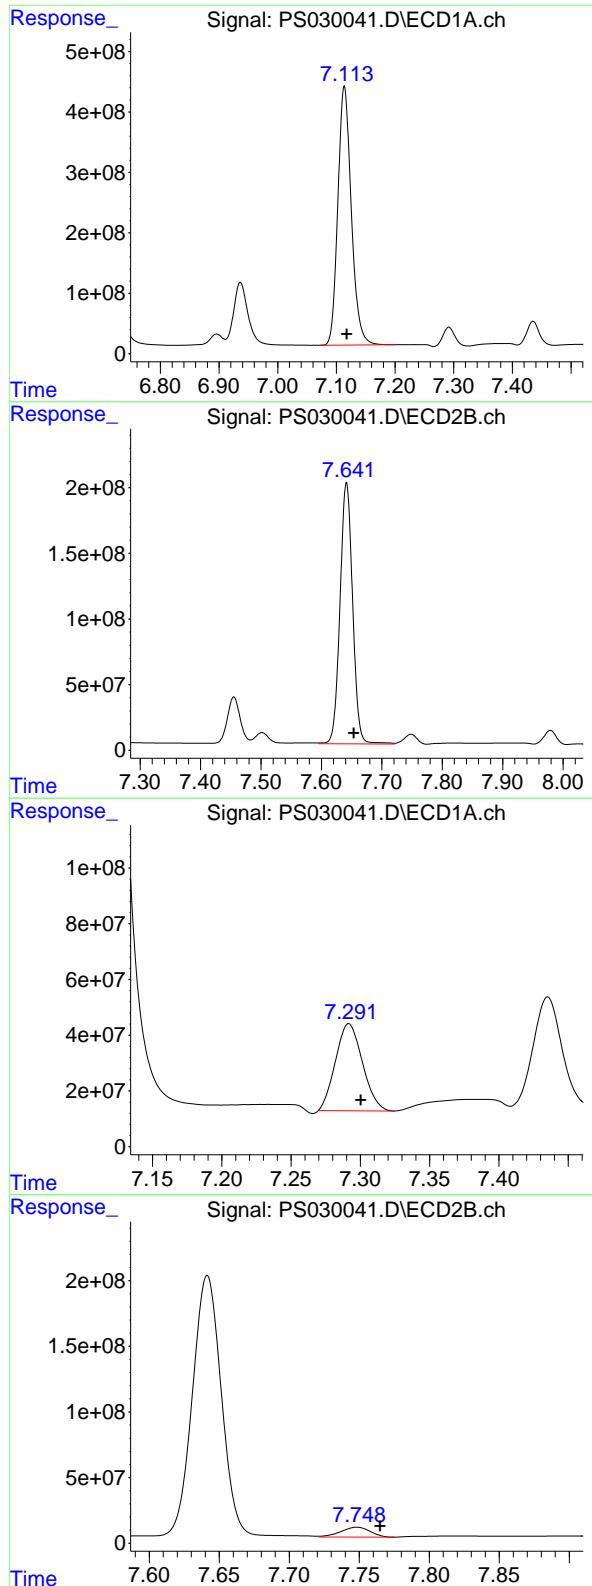

#5 DICAMBA

R.T.: 7.114 min  
 Delta R.T.: -0.004 min  
 Response: 6817562025  
 Conc: 688.44 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#5 DICAMBA


R.T.: 7.642 min  
 Delta R.T.: -0.012 min  
 Response: 2886665237  
 Conc: 730.79 ng/ml

#6 MCPP

R.T.: 7.292 min  
 Delta R.T.: -0.009 min  
 Response: 422534047  
 Conc: 65.57 ug/ml

#6 MCPP


R.T.: 7.748 min  
 Delta R.T.: -0.016 min  
 Response: 110573744  
 Conc: 63.22 ug/ml

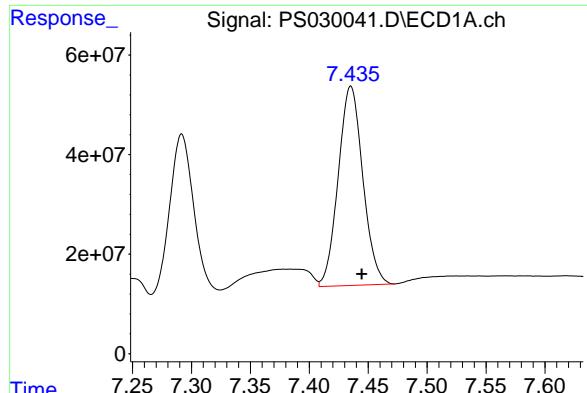

#7 MCPA


R.T.: 7.435 min  
 Delta R.T.: -0.009 min  
 Response: 580958132  
 Conc: 65.78 ug/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

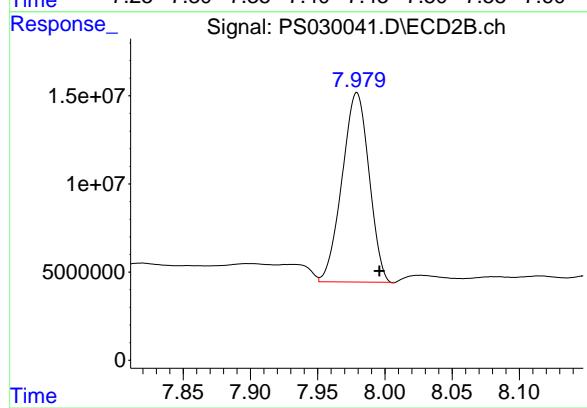


#7 MCPA

R.T.: 7.979 min  
 Delta R.T.: -0.017 min  
 Response: 149368796  
 Conc: 63.14 ug/ml

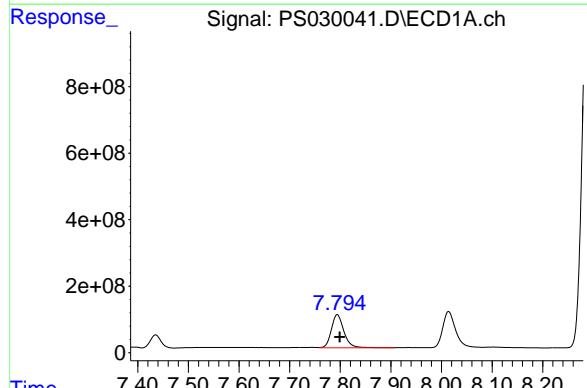


#8 DICHLOPROP

R.T.: 7.794 min  
 Delta R.T.: -0.005 min  
 Response: 1709939199  
 Conc: 674.77 ng/ml

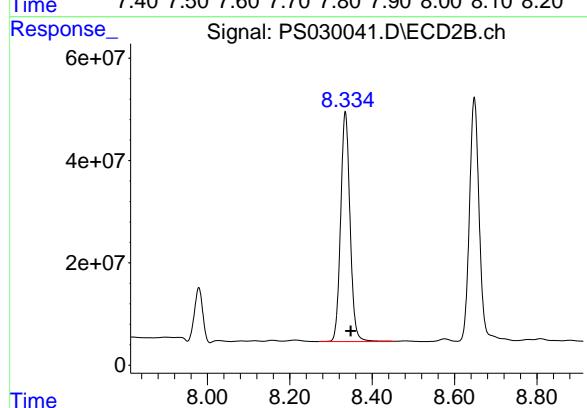

#8 DICHLOPROP

R.T.: 8.335 min  
 Delta R.T.: -0.013 min  
 Response: 710958723  
 Conc: 708.15 ng/ml

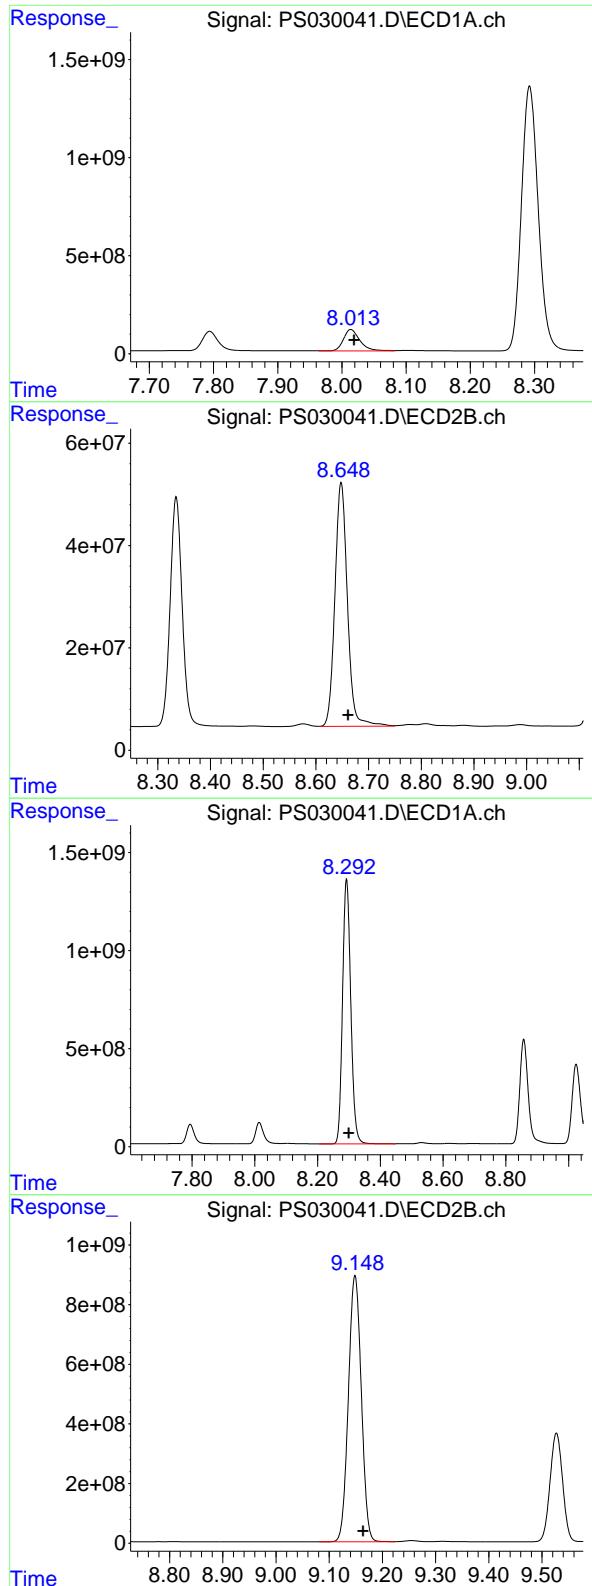

#9 2,4-D

R.T.: 8.014 min  
Delta R.T.: -0.005 min  
Response: 1935157953  
Conc: 687.97 ng/ml

Instrument: ECD\_S  
ClientSampleId: HSTDCCC750

#9 2,4-D


R.T.: 8.648 min  
Delta R.T.: -0.013 min  
Response: 785195057  
Conc: 696.65 ng/ml

#10 Pentachlorophenol

R.T.: 8.292 min  
Delta R.T.: -0.007 min  
Response: 24554651193  
Conc: 703.87 ng/ml

#10 Pentachlorophenol

R.T.: 9.149 min  
Delta R.T.: -0.015 min  
Response: 15042285138  
Conc: 739.37 ng/ml

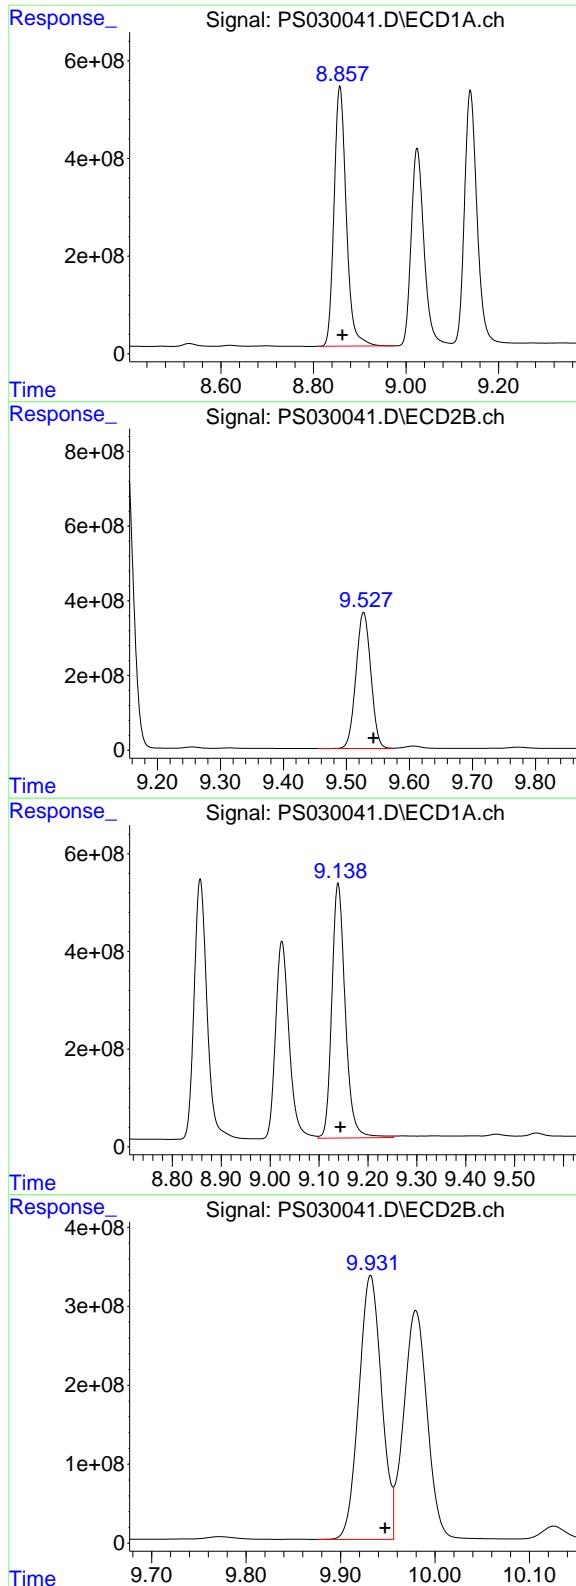

#11 2,4,5-TP (SILVEX)

R.T.: 8.857 min  
 Delta R.T.: -0.005 min  
 Response: 9759498519  
 Conc: 704.00 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#11 2,4,5-TP (SILVEX)


R.T.: 9.527 min  
 Delta R.T.: -0.015 min  
 Response: 5967877580  
 Conc: 729.41 ng/ml

#12 2,4,5-T

R.T.: 9.139 min  
 Delta R.T.: -0.005 min  
 Response: 9937744206  
 Conc: 707.16 ng/ml

#12 2,4,5-T

R.T.: 9.932 min  
 Delta R.T.: -0.015 min  
 Response: 5585441010  
 Conc: 719.53 ng/ml

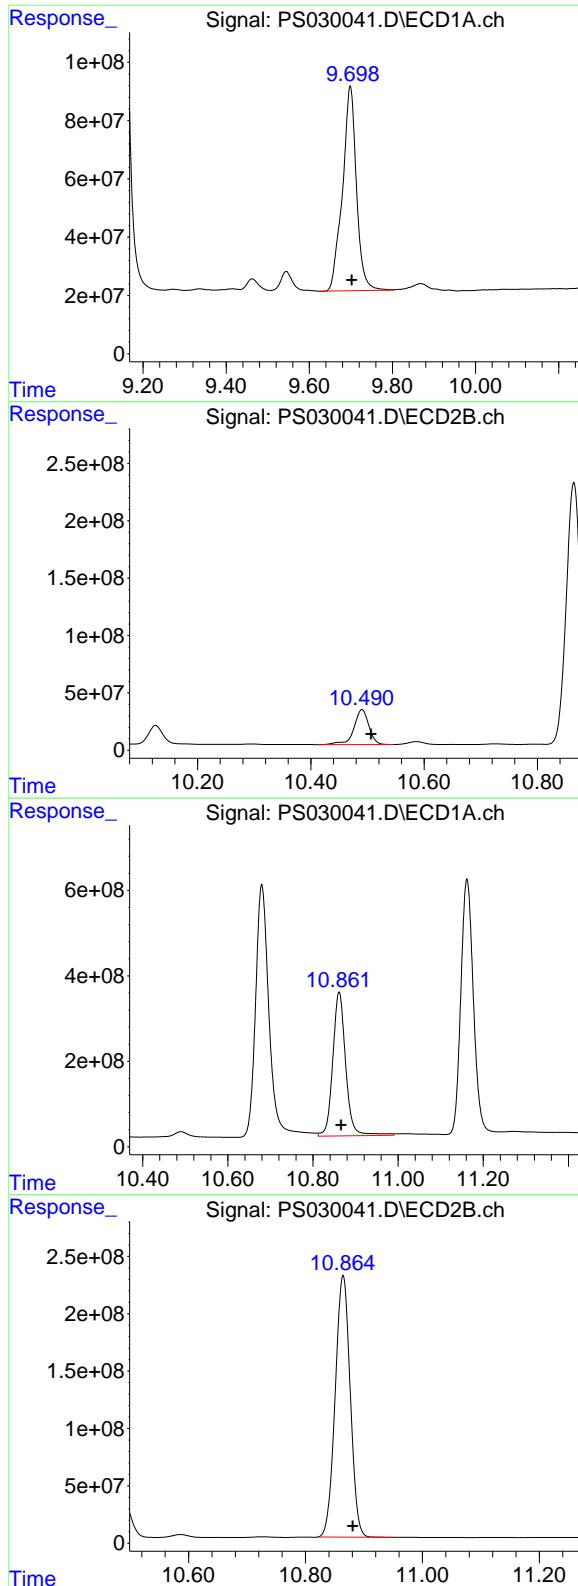

#13 2,4-DB

R.T.: 9.699 min  
 Delta R.T.: -0.003 min  
 Response: 1639322217  
 Conc: 717.32 ng/ml

**Instrument:** ECD\_S  
**ClientSampleId:** HSTDCCC750

#13 2,4-DB


R.T.: 10.490 min  
 Delta R.T.: -0.016 min  
 Response: 557791820  
 Conc: 693.04 ng/ml

#14 DINOSEB

R.T.: 10.861 min  
 Delta R.T.: -0.004 min  
 Response: 7113634891  
 Conc: 699.24 ng/ml

#14 DINOSEB

R.T.: 10.864 min  
 Delta R.T.: -0.017 min  
 Response: 4063249852  
 Conc: 696.84 ng/ml

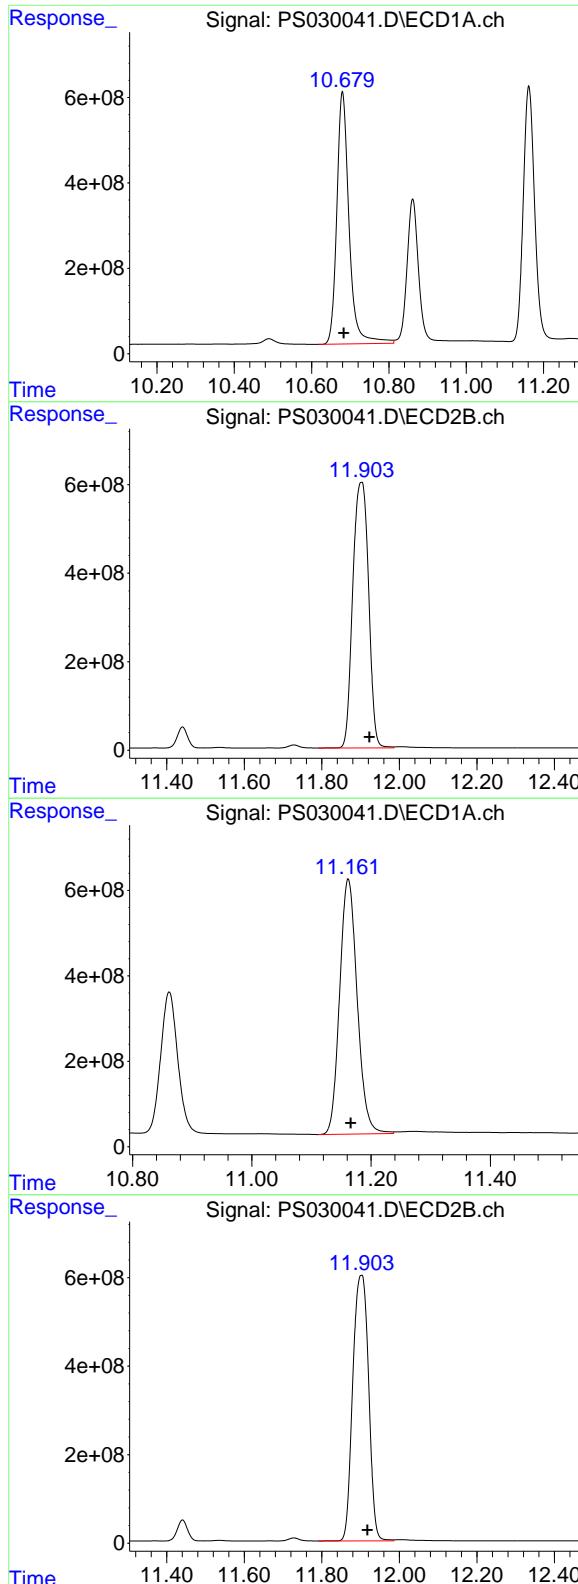

#15 Picloram

R.T.: 10.680 min  
 Delta R.T.: -0.004 min  
 Response: 13035887532  
 Conc: 711.15 ng/ml

Instrument: ECD\_S  
 ClientSampleId: HSTDCCC750

#15 Picloram

R.T.: 11.902 min  
 Delta R.T.: -0.021 min  
 Response: 16973196390  
 Conc: 1381.77 ng/ml

#16 DCPA

R.T.: 11.162 min  
 Delta R.T.: -0.004 min  
 Response: 12175434673  
 Conc: 715.32 ng/ml

#16 DCPA

R.T.: 11.902 min  
 Delta R.T.: -0.016 min  
 Response: 16973196390  
 Conc: 1505.83 ng/ml