

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL043025\
 Data File : PL095440.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Apr 2025 16:01
 Operator : AR\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 01:34:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 23 16:23:18 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.593	2.904	167.3E6	159.8E6	51.234	50.269
28)	SA Decachlor...	9.116	8.083	154.3E6	161.8E6	55.674	54.678
Target Compounds							
2)	A alpha-BHC	4.044	3.414	257.1E6	232.3E6	51.895	52.209
3)	MA gamma-BHC...	4.375	3.747	243.7E6	223.0E6	51.469	50.705
4)	MA Heptachlor	4.972	4.101	235.2E6	215.4E6	51.415	49.436
5)	MB Aldrin	5.314	4.386	239.1E6	205.7E6	52.062	49.991
6)	B beta-BHC	4.560	4.040	104.8E6	102.1E6	50.683	49.198
7)	B delta-BHC	0.000	4.277	0	223.5E6	N.D.	50.996 #
8)	B Heptachlo...	5.735	4.889	215.0E6	191.0E6	53.673	49.436
9)	A Endosulfan I	6.118	5.262	205.5E6	183.9E6	54.126	50.236
10)	B gamma-Chl...	5.989	5.141	220.5E6	204.2E6	54.052	50.397
11)	B alpha-Chl...	6.070	5.206	226.5E6	197.8E6	55.700	49.673
12)	B 4,4'-DDE	6.239	5.392	219.9E6	193.0E6	56.088	47.455
13)	MA Dieldrin	6.391	5.527	209.2E6	198.2E6	54.261	48.724
14)	MA Endrin	6.619	5.802	166.9E6	155.7E6	52.421	42.778
15)	B Endosulfa...	6.831	6.092	186.9E6	178.7E6	58.563	49.756
16)	A 4,4'-DDD	6.748	5.944	166.2E6	165.7E6	58.711	50.708
17)	MA 4,4'-DDT	7.064	6.198	159.4E6	146.2E6	55.966	42.538
18)	B Endrin al...	6.960	6.270	132.7E6	134.5E6	57.199	51.464
19)	B Endosulfa...	7.193	6.493	156.8E6	173.0E6	55.948	52.133
20)	A Methoxychlor	7.535	6.768	73516314	88053321	52.695	46.163
21)	B Endrin ke...	7.674	6.999	169.3E6	199.6E6	59.372	56.679
22)	Mirex	8.155	7.195	132.3E6	184.1E6	55.691	63.860
24)	Chlordane-2	5.314f	0.000	239.1E6	0	1129.456	N.D. #
25)	Chlordane-3	5.989	5.141	220.5E6	204.2E6	283.076	395.339 #
26)	Chlordane-4	6.070	5.206	226.5E6	197.8E6	240.189	455.005 #
27)	Chlordane-5	0.000	6.092	0	178.7E6	N.D.	967.204 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL043025\
Data File : PL095440.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Apr 2025 16:01
Operator : AR\AJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 01:34:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
Quant Title : GC Extractables
QLast Update : Wed Apr 23 16:23:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

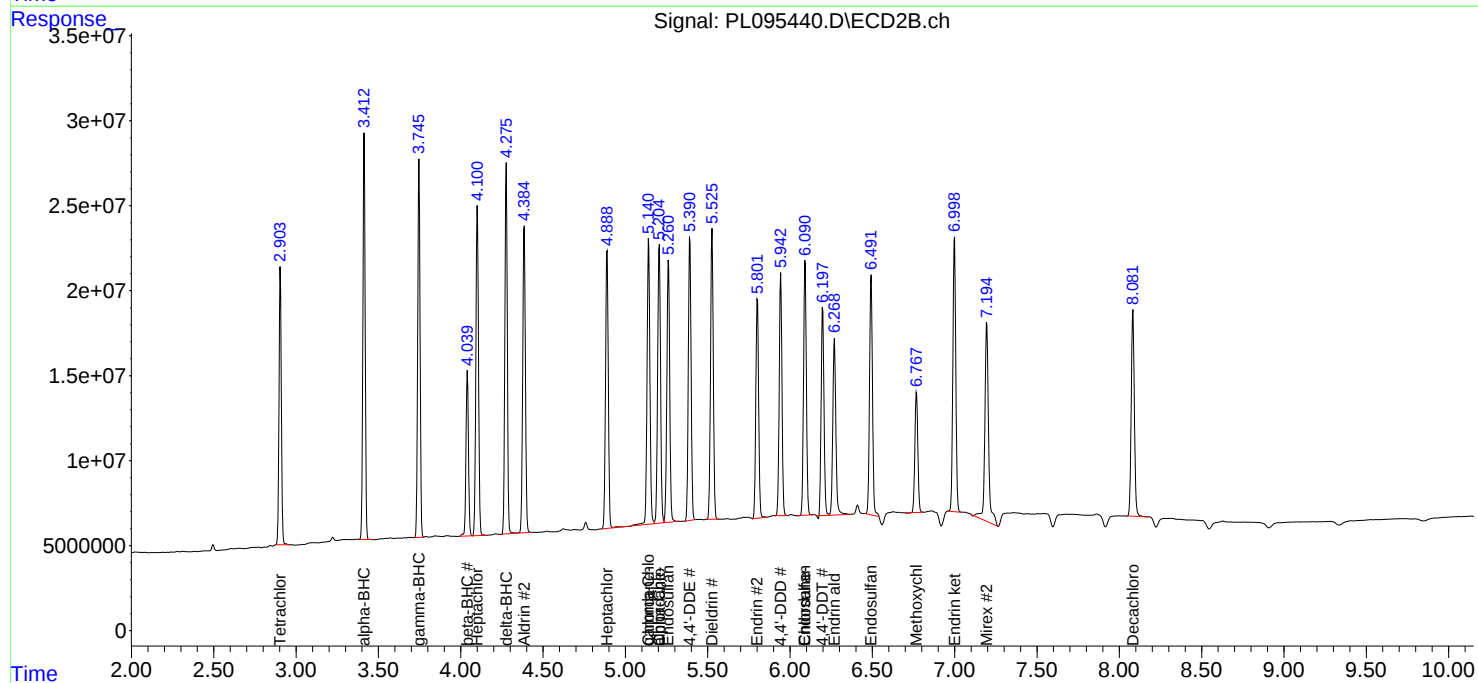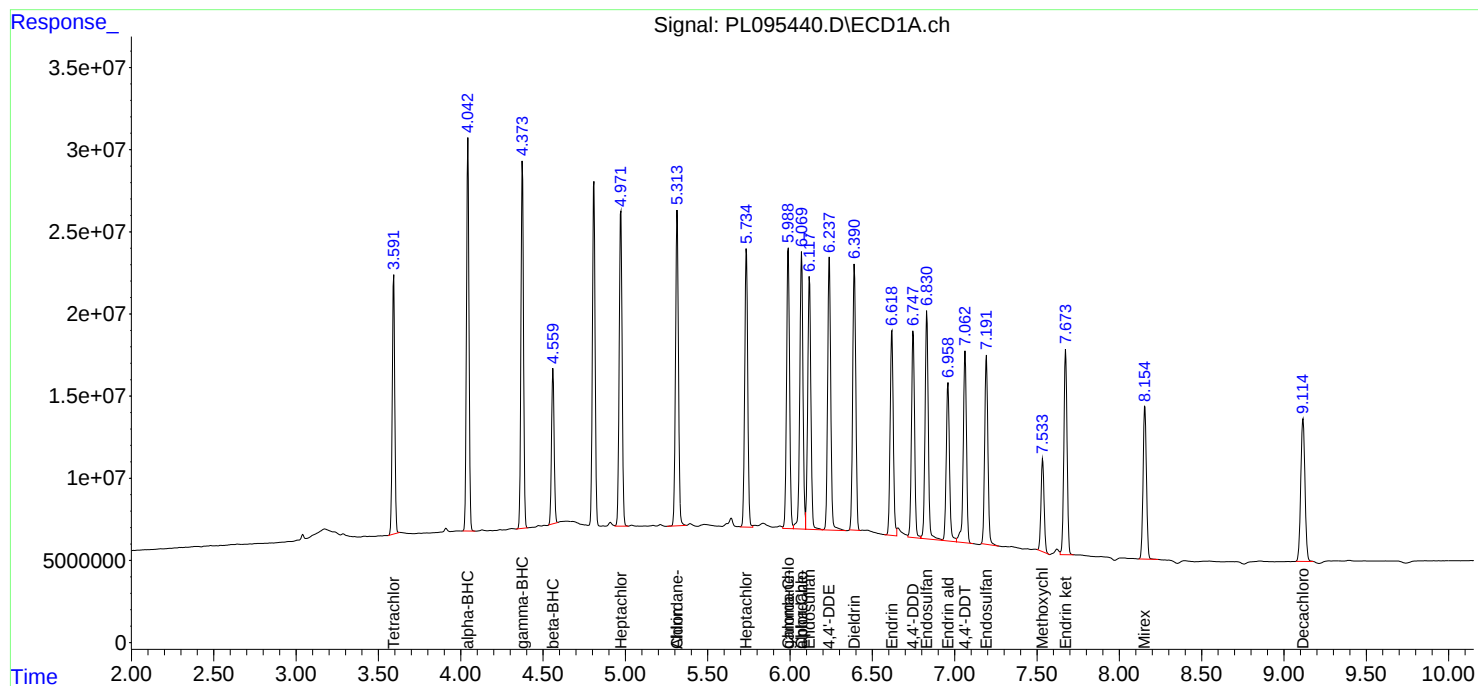


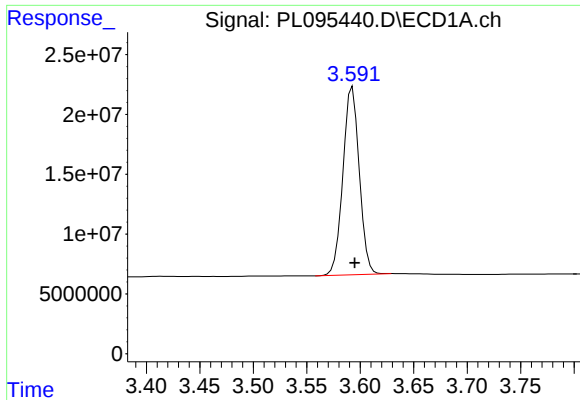

#1 Tetrachloro-m-xylene


R.T.: 3.593 min
Delta R.T.: -0.002 min
Response: 167262219
Conc: 51.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

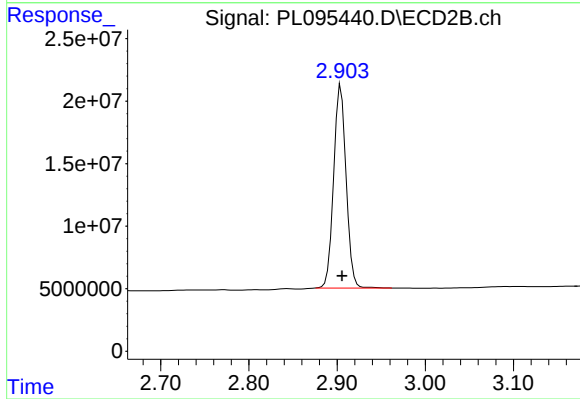


#1 Tetrachloro-m-xylene

R.T.: 2.904 min
Delta R.T.: -0.001 min
Response: 159843978
Conc: 50.27 ng/ml

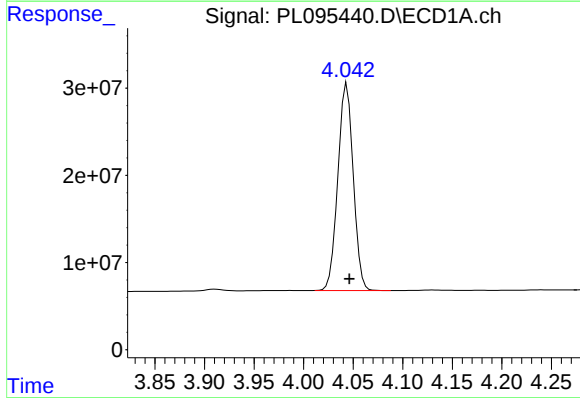


#2 alpha-BHC

R.T.: 4.044 min
Delta R.T.: -0.003 min
Response: 257072845
Conc: 51.89 ng/ml

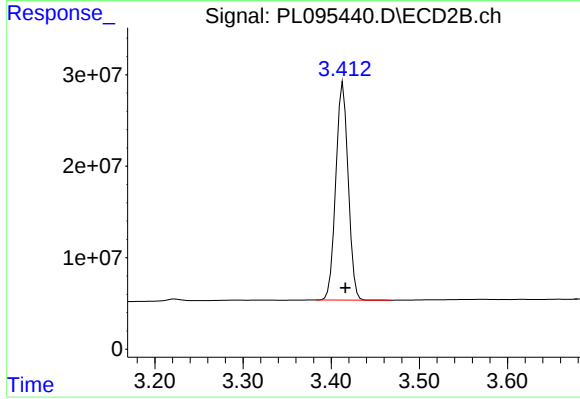

#2 alpha-BHC


R.T.: 3.414 min
Delta R.T.: -0.003 min
Response: 232264928
Conc: 52.21 ng/ml

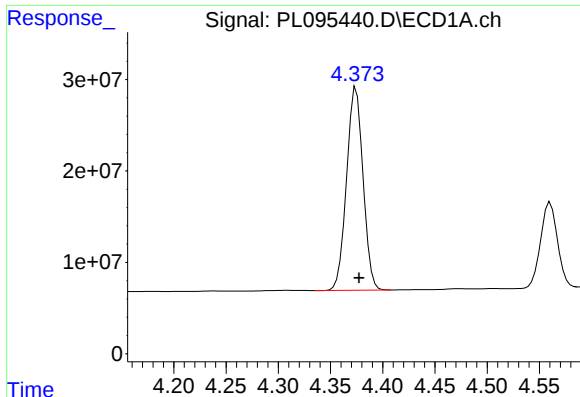

#3 gamma-BHC (Lindane)


R.T.: 4.375 min
Delta R.T.: -0.003 min
Response: 243652188
Conc: 51.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

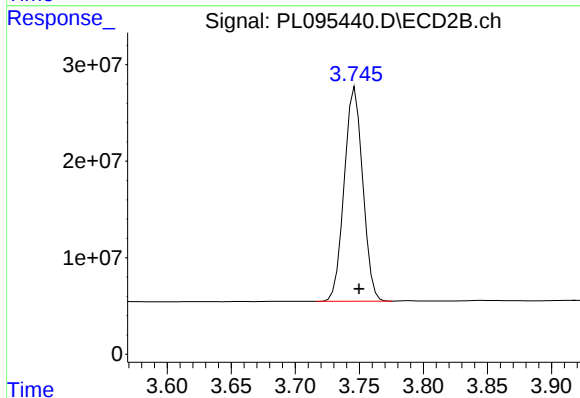


#3 gamma-BHC (Lindane)

R.T.: 3.747 min
Delta R.T.: -0.003 min
Response: 223013873
Conc: 50.71 ng/ml

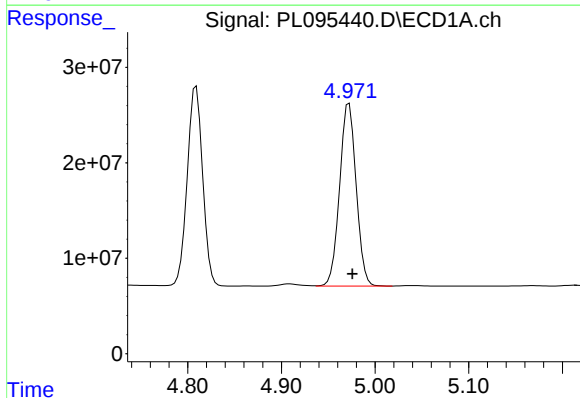


#4 Heptachlor

R.T.: 4.972 min
Delta R.T.: -0.004 min
Response: 235195258
Conc: 51.41 ng/ml

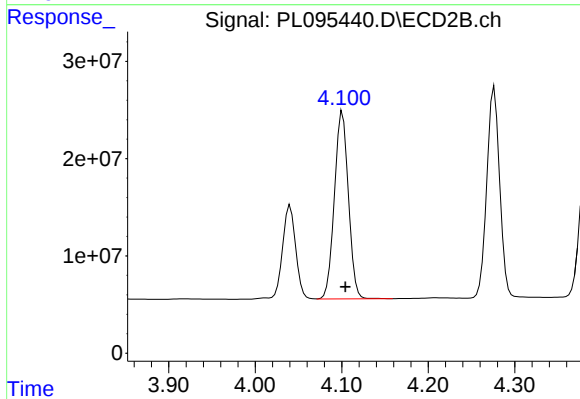

#4 Heptachlor


R.T.: 4.101 min
Delta R.T.: -0.003 min
Response: 215375667
Conc: 49.44 ng/ml

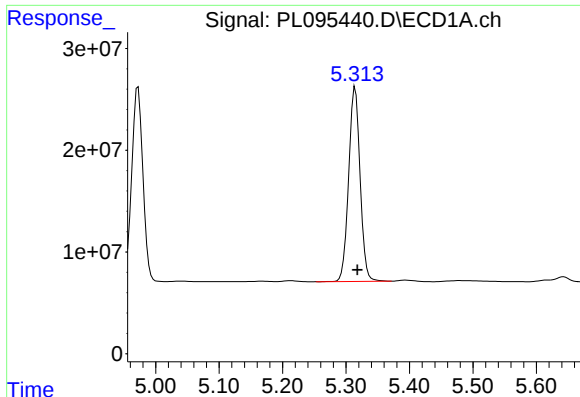

#5 Aldrin


R.T.: 5.314 min
Delta R.T.: -0.004 min
Response: 239123618
Conc: 52.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

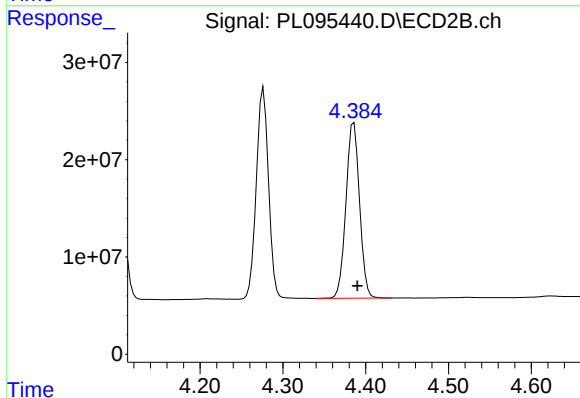


#5 Aldrin

R.T.: 4.386 min
Delta R.T.: -0.004 min
Response: 205747698
Conc: 49.99 ng/ml

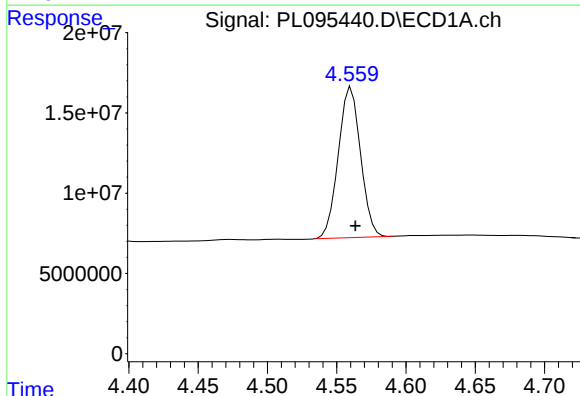


#6 beta-BHC

R.T.: 4.560 min
Delta R.T.: -0.003 min
Response: 104788017
Conc: 50.68 ng/ml

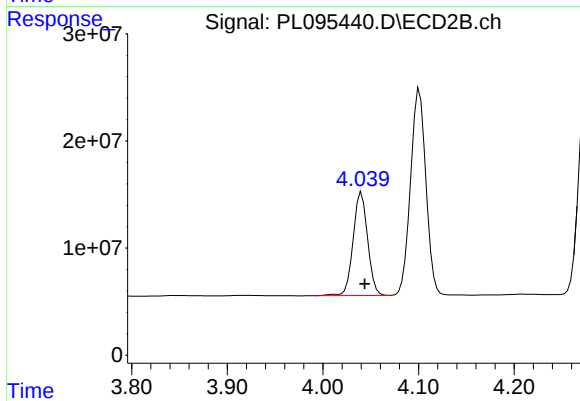

#6 beta-BHC


R.T.: 4.040 min
Delta R.T.: -0.003 min
Response: 102128920
Conc: 49.20 ng/ml

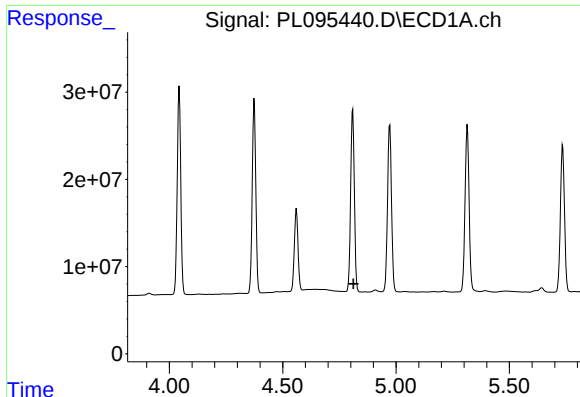

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.812 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

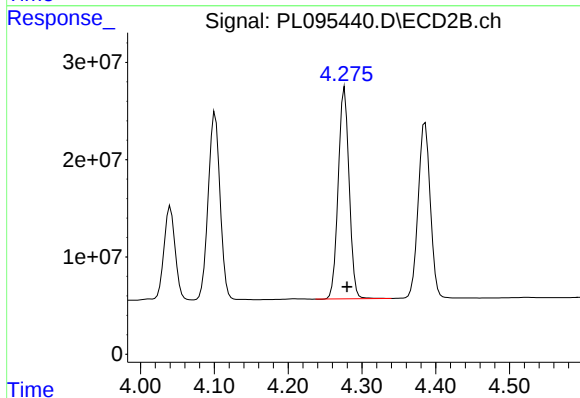


#7 delta-BHC

R.T.: 4.277 min
Delta R.T.: -0.003 min
Response: 223463127
Conc: 51.00 ng/ml

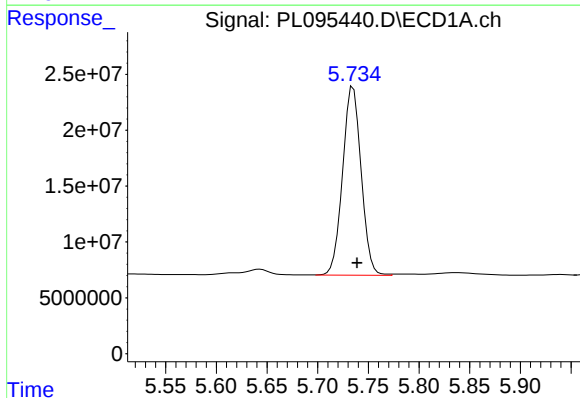


#8 Heptachlor epoxide

R.T.: 5.735 min
Delta R.T.: -0.004 min
Response: 214968820
Conc: 53.67 ng/ml

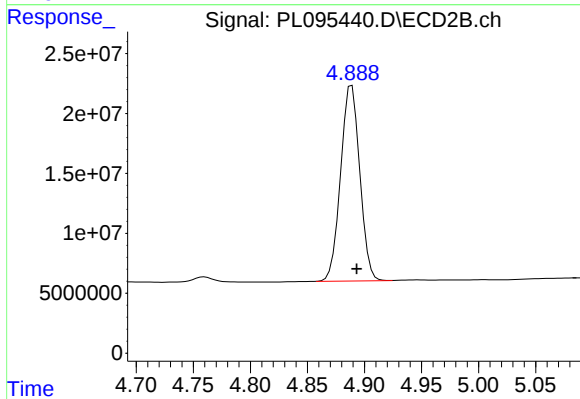

#8 Heptachlor epoxide


R.T.: 4.889 min
Delta R.T.: -0.004 min
Response: 190953783
Conc: 49.44 ng/ml

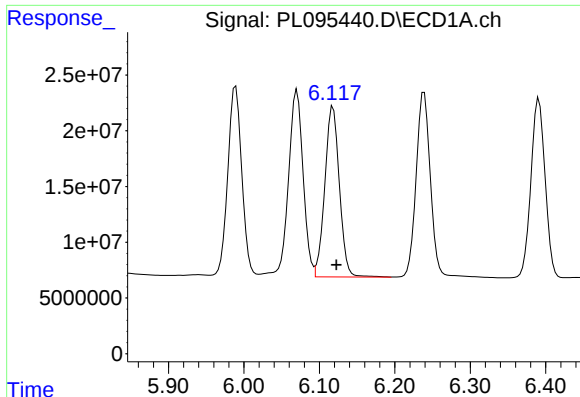

#9 Endosulfan I


R.T.: 6.118 min
Delta R.T.: -0.004 min
Response: 205545727
Conc: 54.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

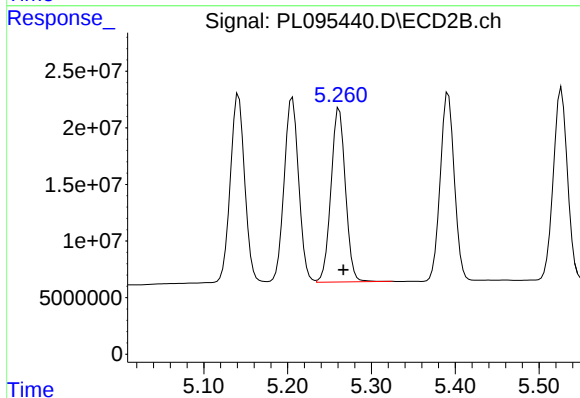


#9 Endosulfan I

R.T.: 5.262 min
Delta R.T.: -0.005 min
Response: 183883855
Conc: 50.24 ng/ml

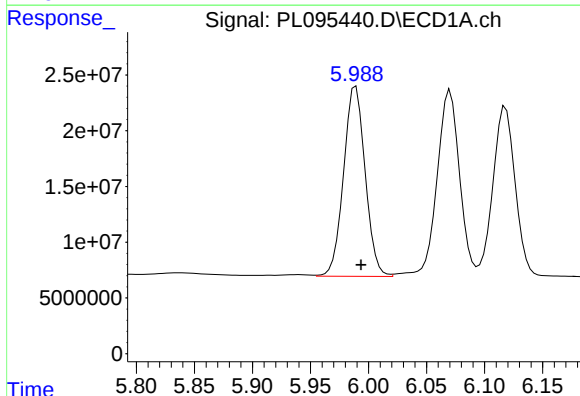


#10 gamma-Chlordane

R.T.: 5.989 min
Delta R.T.: -0.004 min
Response: 220495708
Conc: 54.05 ng/ml

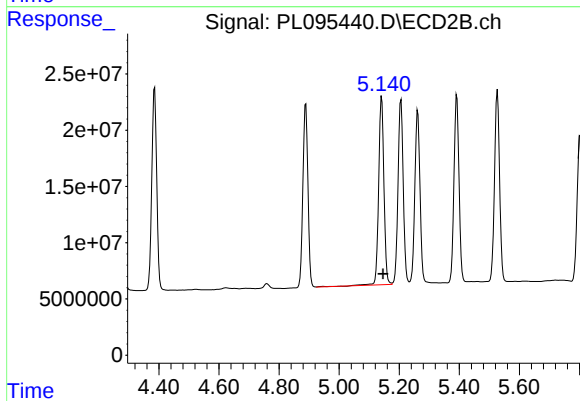

#10 gamma-Chlordane


R.T.: 5.141 min
Delta R.T.: -0.005 min
Response: 204240956
Conc: 50.40 ng/ml

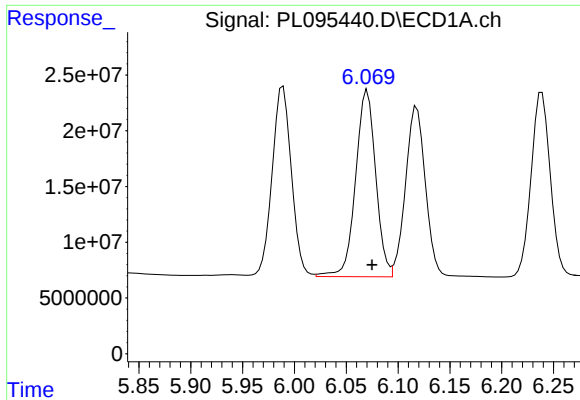

#11 alpha-Chlordane


R.T.: 6.070 min
Delta R.T.: -0.004 min
Response: 226480961
Conc: 55.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

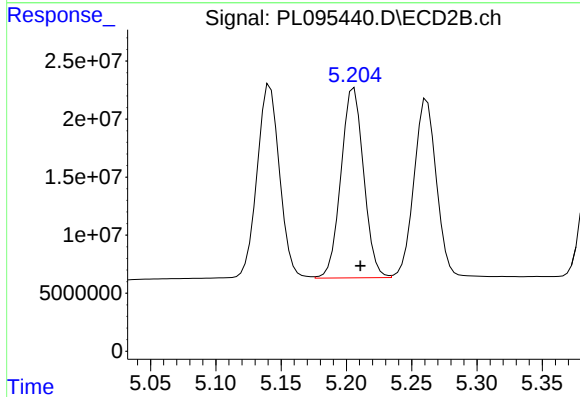


#11 alpha-Chlordane

R.T.: 5.206 min
Delta R.T.: -0.005 min
Response: 197750673
Conc: 49.67 ng/ml

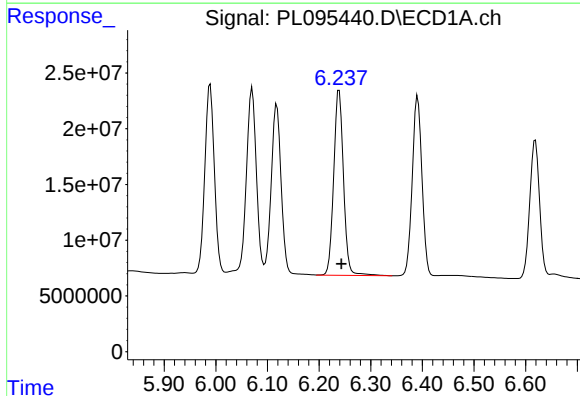


#12 4,4'-DDE

R.T.: 6.239 min
Delta R.T.: -0.004 min
Response: 219897725
Conc: 56.09 ng/ml

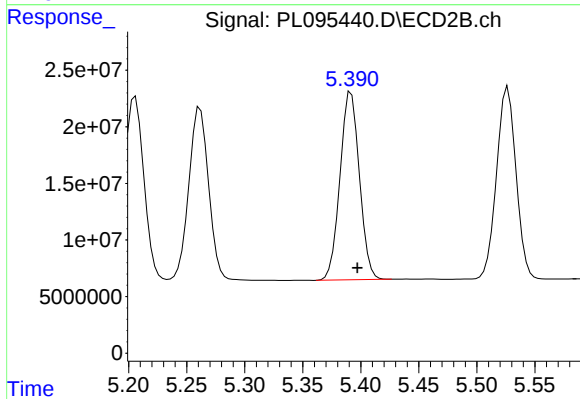

#12 4,4'-DDE


R.T.: 5.392 min
Delta R.T.: -0.005 min
Response: 192997790
Conc: 47.45 ng/ml

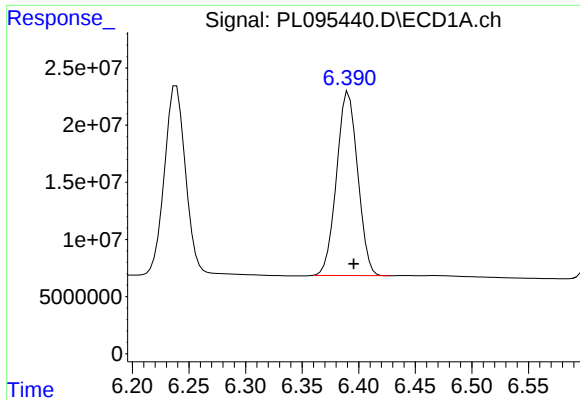

#13 Dieldrin


R.T.: 6.391 min
Delta R.T.: -0.005 min
Response: 209166326
Conc: 54.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

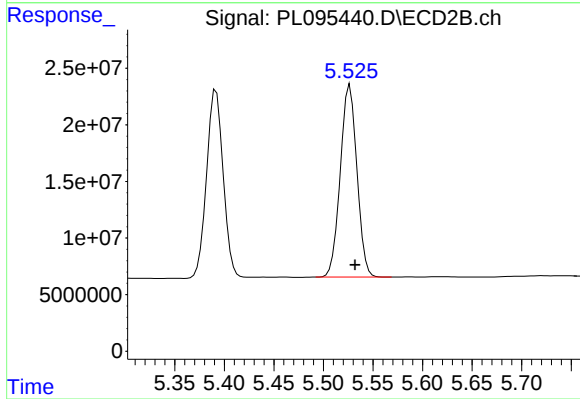


#13 Dieldrin

R.T.: 5.527 min
Delta R.T.: -0.005 min
Response: 198164030
Conc: 48.72 ng/ml

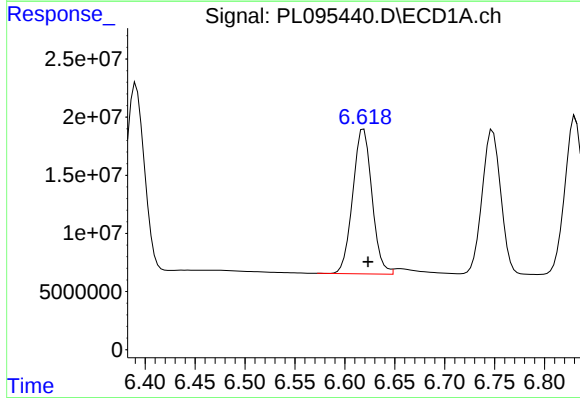


#14 Endrin

R.T.: 6.619 min
Delta R.T.: -0.004 min
Response: 166947576
Conc: 52.42 ng/ml

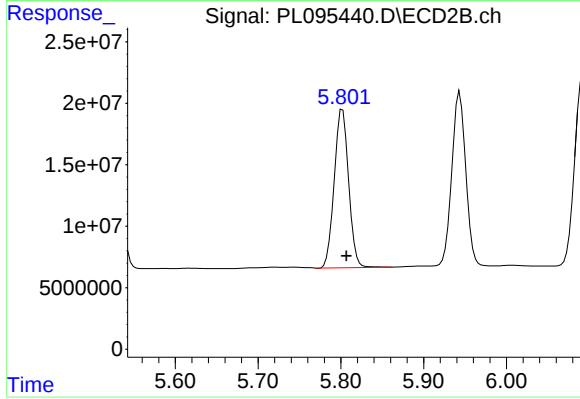

#14 Endrin


R.T.: 5.802 min
Delta R.T.: -0.005 min
Response: 155741444
Conc: 42.78 ng/ml

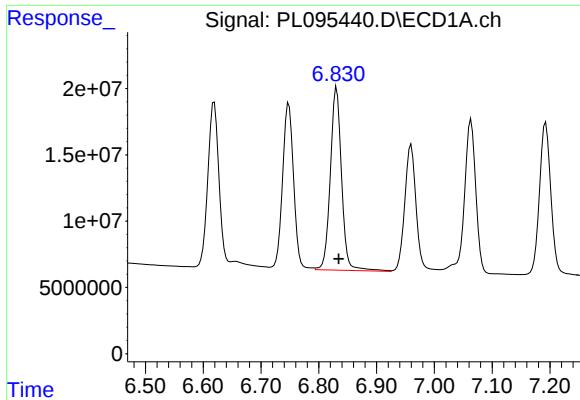

#15 Endosulfan II


R.T.: 6.831 min
Delta R.T.: -0.004 min
Response: 186940626
Conc: 58.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

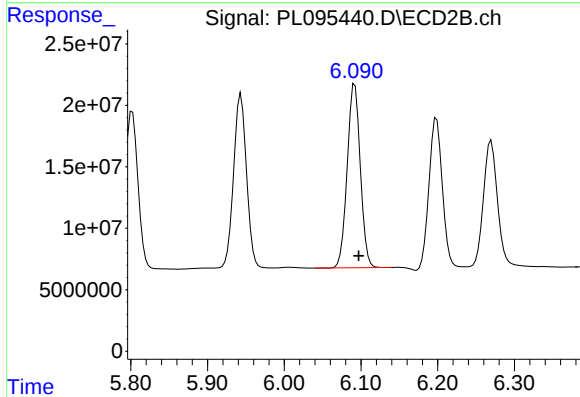


#15 Endosulfan II

R.T.: 6.092 min
Delta R.T.: -0.005 min
Response: 178680070
Conc: 49.76 ng/ml

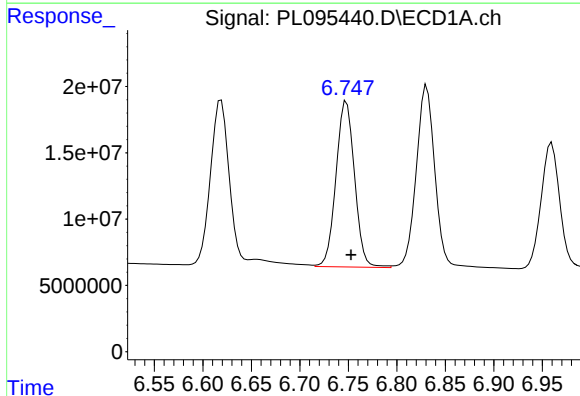


#16 4,4'-DDD

R.T.: 6.748 min
Delta R.T.: -0.005 min
Response: 166208955
Conc: 58.71 ng/ml

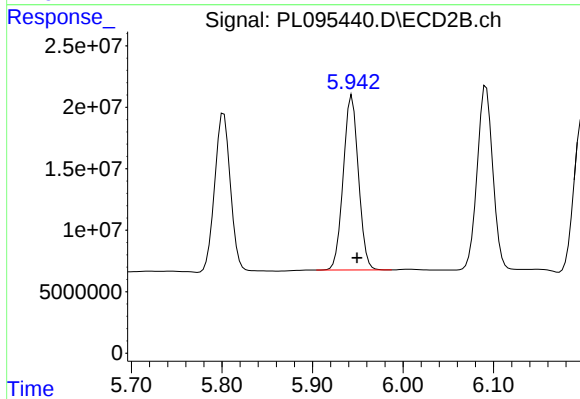

#16 4,4'-DDD


R.T.: 5.944 min
Delta R.T.: -0.006 min
Response: 165652788
Conc: 50.71 ng/ml

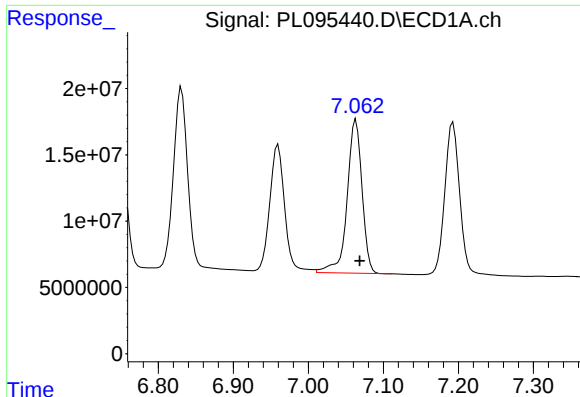

#17 4,4'-DDT


R.T.: 7.064 min
Delta R.T.: -0.005 min
Response: 159422273
Conc: 55.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

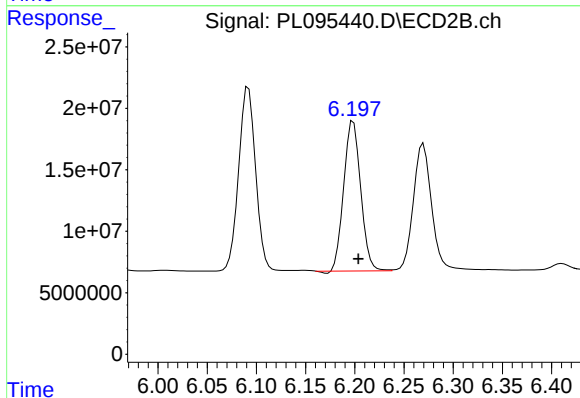


#17 4,4'-DDT

R.T.: 6.198 min
Delta R.T.: -0.005 min
Response: 146167973
Conc: 42.54 ng/ml

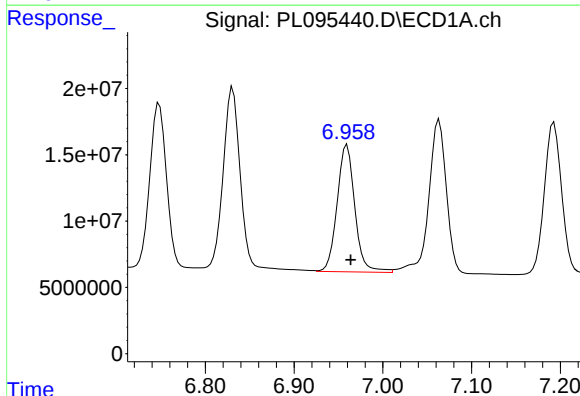


#18 Endrin aldehyde

R.T.: 6.960 min
Delta R.T.: -0.004 min
Response: 132747755
Conc: 57.20 ng/ml

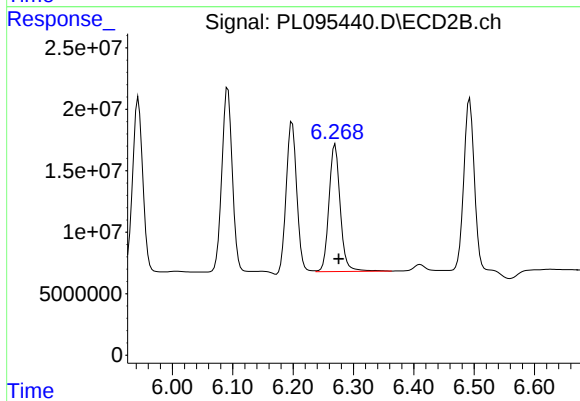

#18 Endrin aldehyde


R.T.: 6.270 min
Delta R.T.: -0.006 min
Response: 134483009
Conc: 51.46 ng/ml

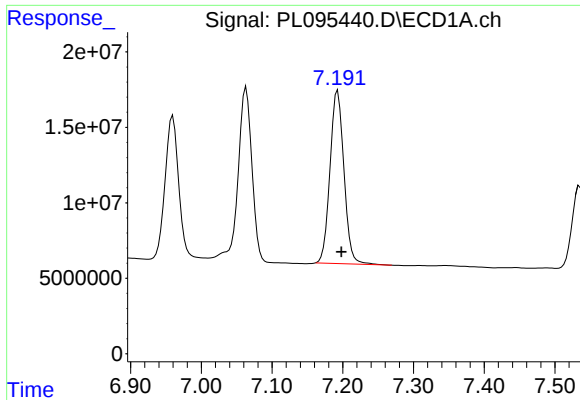

#19 Endosulfan Sulfate


R.T.: 7.193 min
Delta R.T.: -0.005 min
Response: 156753947
Conc: 55.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

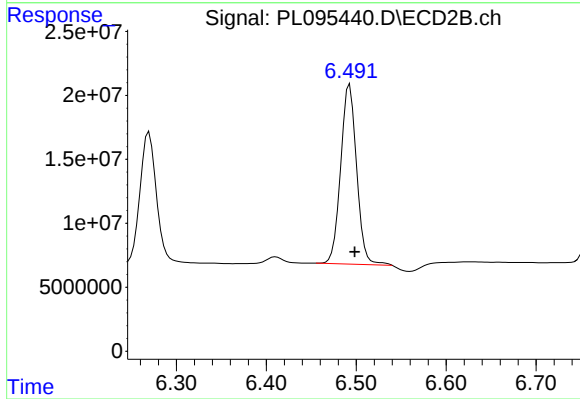


#19 Endosulfan Sulfate

R.T.: 6.493 min
Delta R.T.: -0.006 min
Response: 172972314
Conc: 52.13 ng/ml

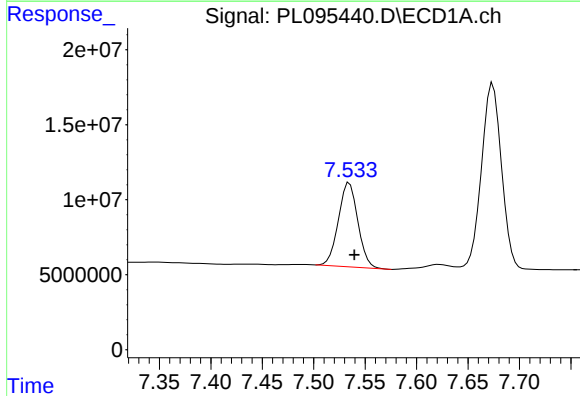


#20 Methoxychlor

R.T.: 7.535 min
Delta R.T.: -0.005 min
Response: 73516314
Conc: 52.69 ng/ml

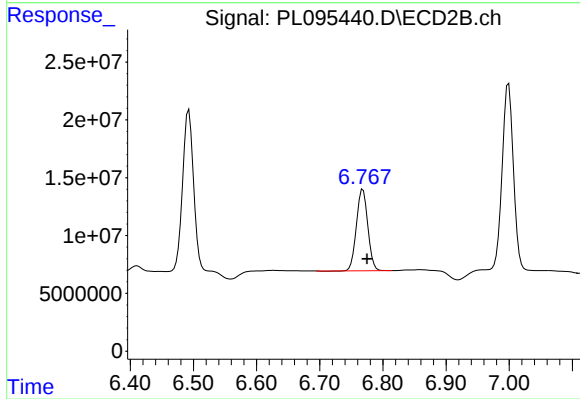

#20 Methoxychlor


R.T.: 6.768 min
Delta R.T.: -0.006 min
Response: 88053321
Conc: 46.16 ng/ml

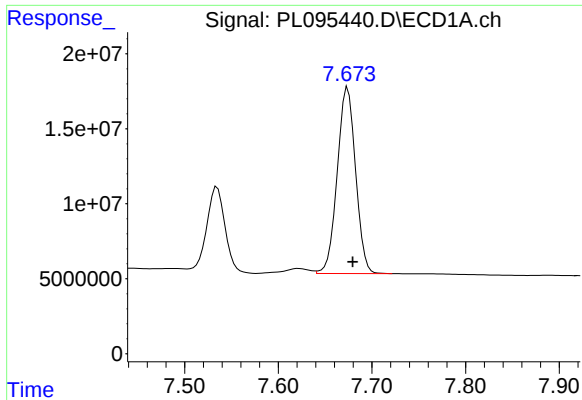

#21 Endrin ketone


R.T.: 7.674 min
Delta R.T.: -0.005 min
Response: 169263018
Conc: 59.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

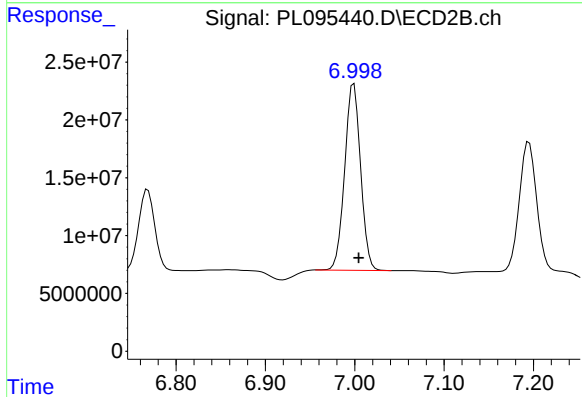


#21 Endrin ketone

R.T.: 6.999 min
Delta R.T.: -0.005 min
Response: 199582150
Conc: 56.68 ng/ml

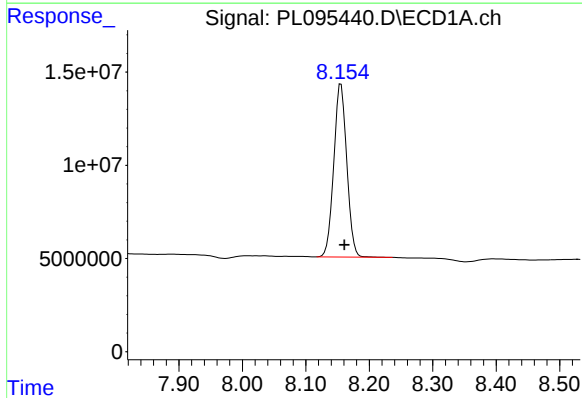


#22 Mirex

R.T.: 8.155 min
Delta R.T.: -0.005 min
Response: 132324817
Conc: 55.69 ng/ml

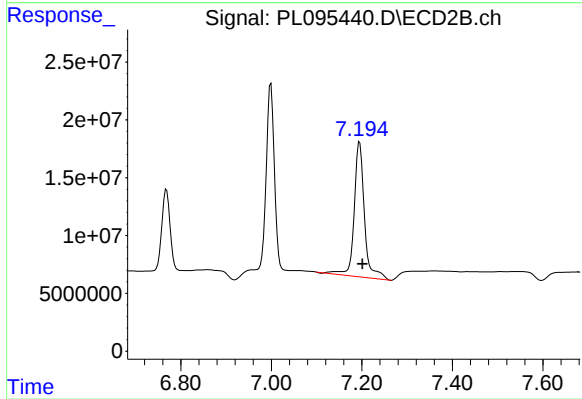

#22 Mirex


R.T.: 7.195 min
Delta R.T.: -0.007 min
Response: 184069814
Conc: 63.86 ng/ml

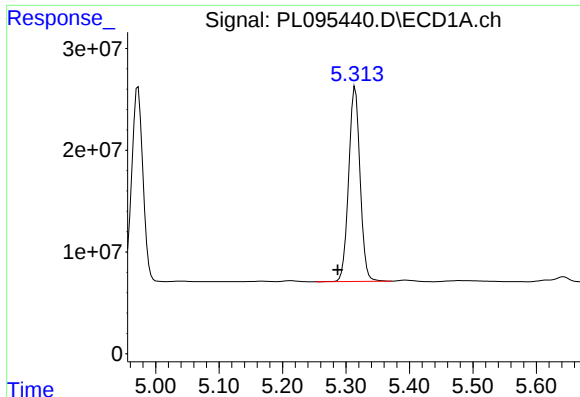

#24 Chlordane-2


R.T.: 5.314 min
Delta R.T.: 0.028 min
Response: 239123618
Conc: 1129.46 ng/m

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

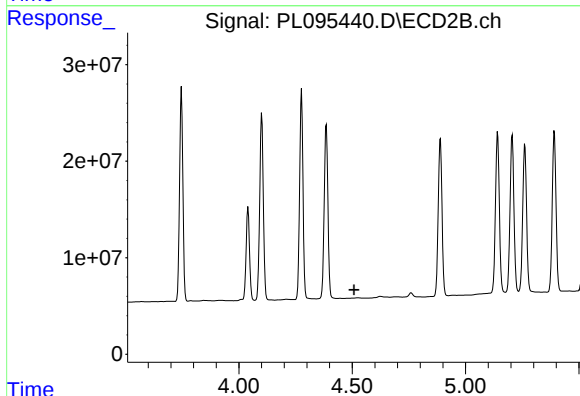


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.508 min
Response: 0
Conc: N.D.

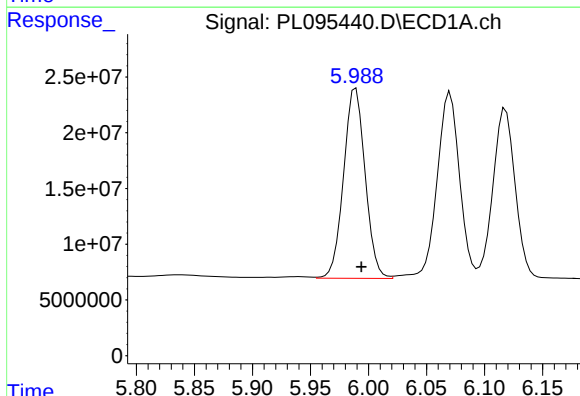


#25 Chlordane-3

R.T.: 5.989 min
Delta R.T.: -0.005 min
Response: 220495708
Conc: 283.08 ng/ml

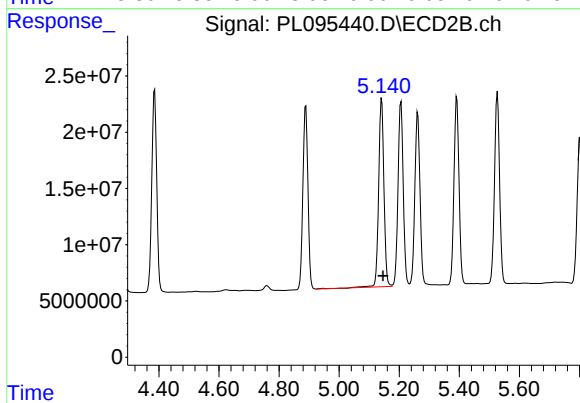

#25 Chlordane-3


R.T.: 5.141 min
Delta R.T.: -0.005 min
Response: 204240956
Conc: 395.34 ng/ml

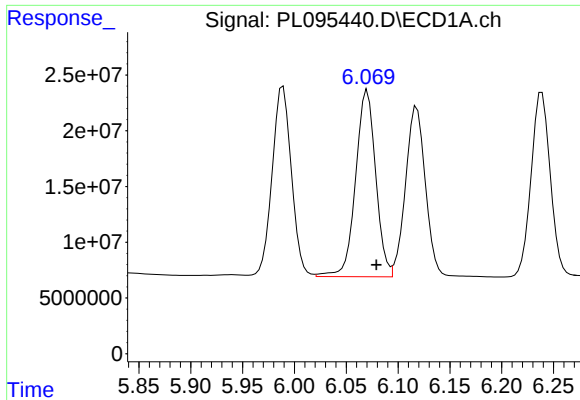

#26 Chlordane-4


R.T.: 6.070 min
Delta R.T.: -0.009 min
Response: 226480961
Conc: 240.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

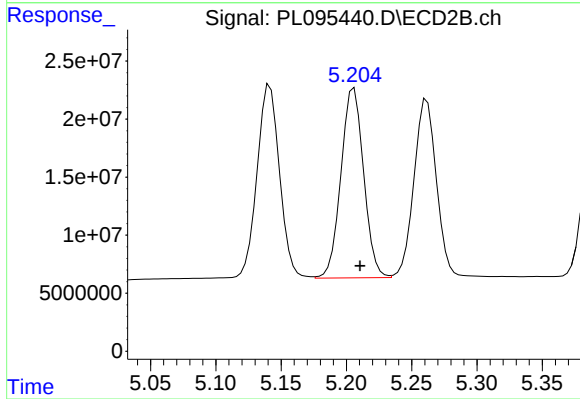


#26 Chlordane-4

R.T.: 5.206 min
Delta R.T.: -0.005 min
Response: 197750673
Conc: 455.01 ng/ml

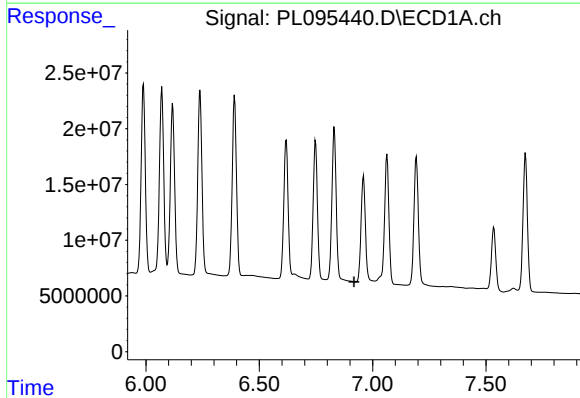


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.919 min
Response: 0
Conc: N.D.

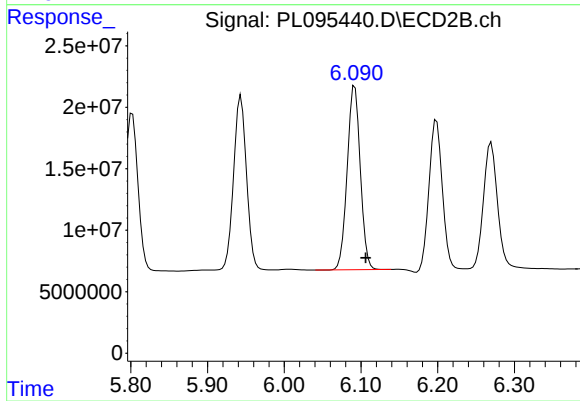

#27 Chlordane-5


R.T.: 6.092 min
Delta R.T.: -0.014 min
Response: 178680070
Conc: 967.20 ng/ml

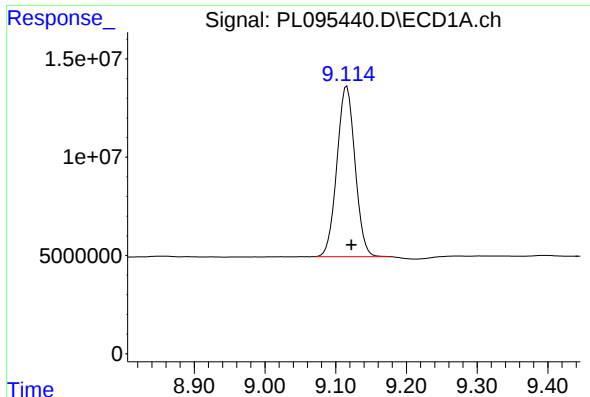

#28 Decachlorobiphenyl

R.T.: 9.116 min
Delta R.T.: -0.006 min
Response: 154263194
Conc: 55.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

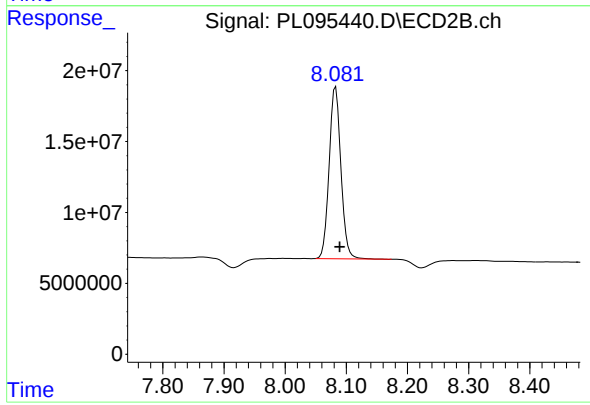

#28 Decachlorobiphenyl

R.T.: 8.083 min
Delta R.T.: -0.007 min
Response: 161807409
Conc: 54.68 ng/ml