


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050525\
Data File : BP024521.D
Acq On : 05 May 2025 11:57
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 18 12:04:48 2025

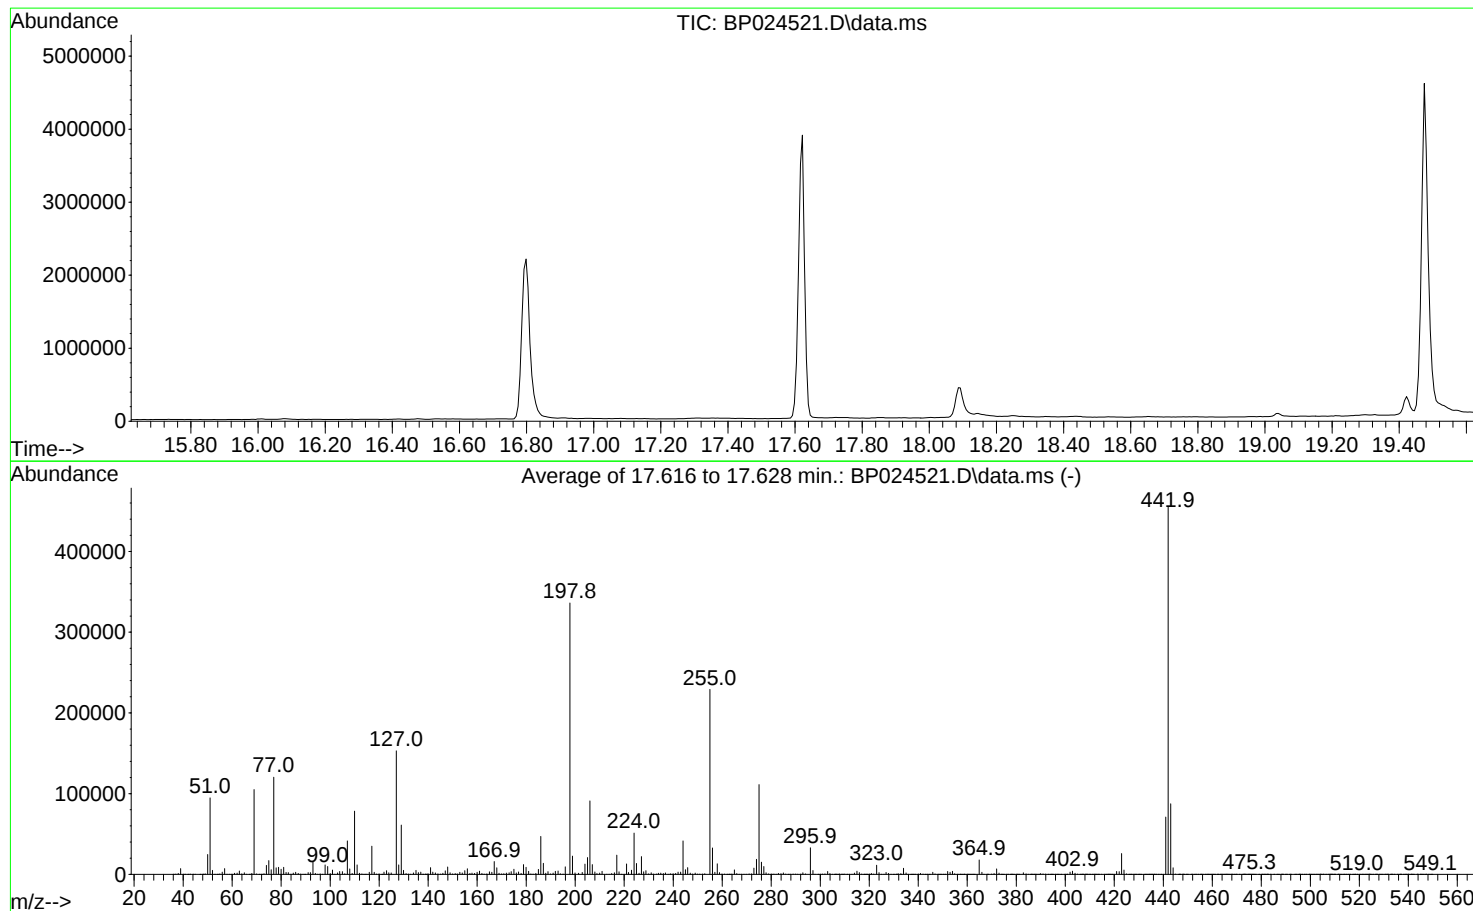

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.2	94677	PASS
68	69	0.00	2	1.1	1105	PASS
69	198	0.00	100	31.3	105085	PASS
70	69	0.00	2	0.6	601	PASS
127	198	10	80	45.5	153112	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	336159	PASS
199	198	5	9	6.7	22574	PASS
275	198	10	60	33.1	111207	PASS
365	198	1	100	5.3	17800	PASS
441	198	0.01	100	21.1	71014	PASS
442	442	100	100	100.0	455698	PASS
443	442	15	24	19.2	87372	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/5/2025	BNA_P	<u>BP024521.D</u>
Compound Name	Response	Retention Time
DDT	1294320	20.763
DDD	38430	20.316
DDE	2470	19.775
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
40900	1335220	3.06

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050525\
Data File : BP024521.D
Acq On : 05 May 2025 11:57
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 05 13:04:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

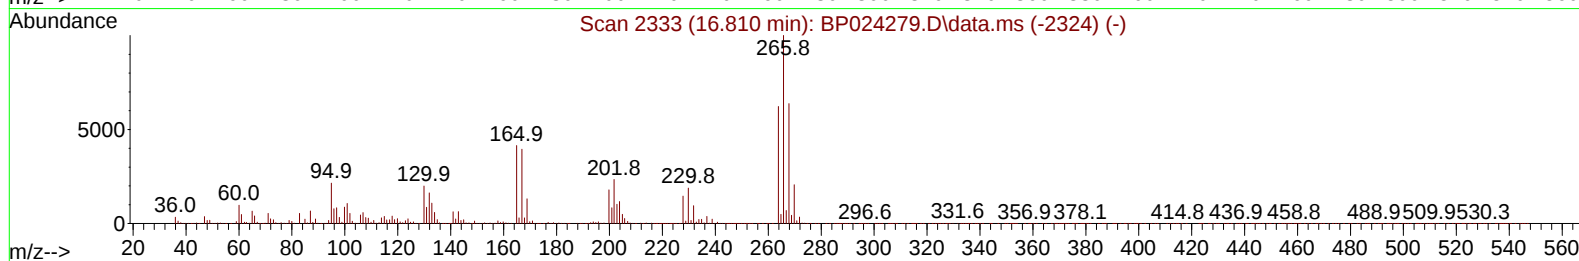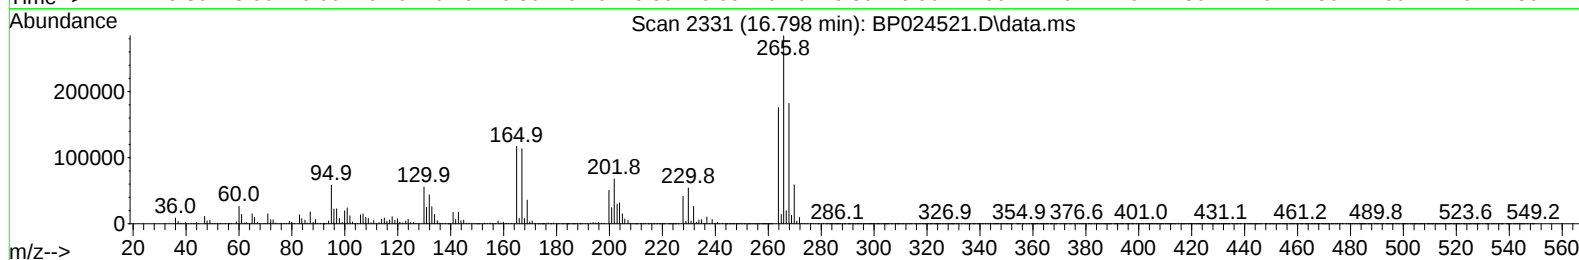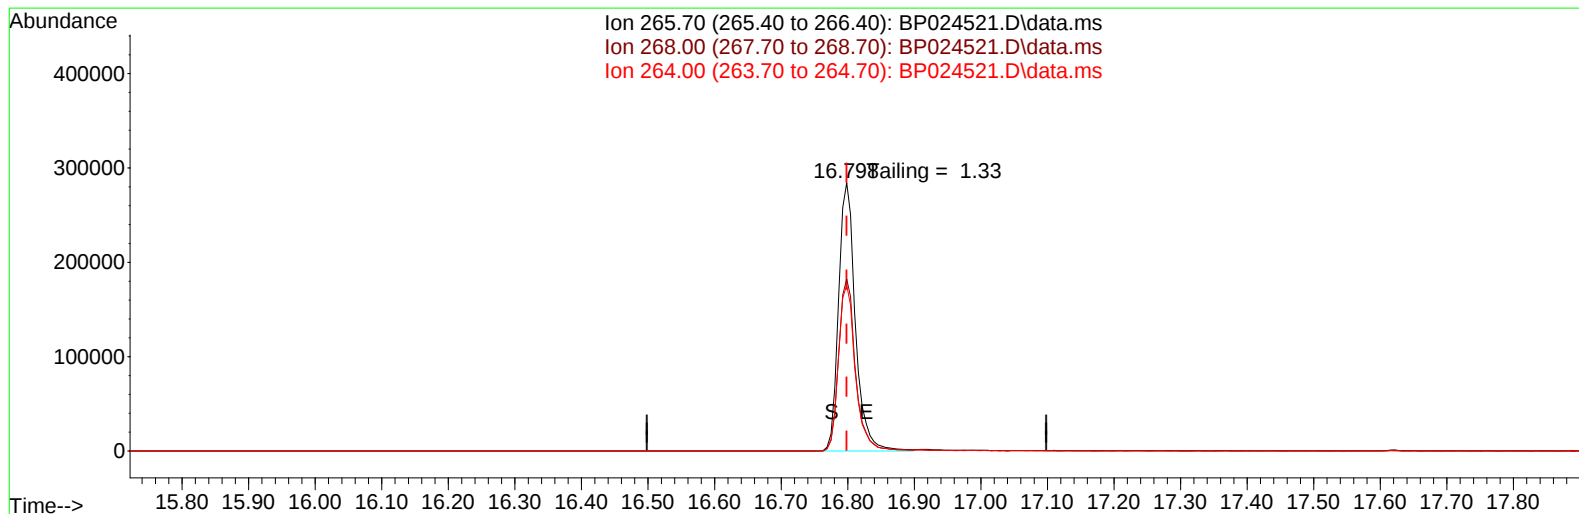

TIC: BP024521.D\data.ms

(70) Pentachlorophenol (C)

16.798min (+ 0.000) 40429.31 ng




response 499235

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.03
264.00	62.20	61.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050525\
Data File : BP024521.D
Acq On : 05 May 2025 11:57
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 05 13:04:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

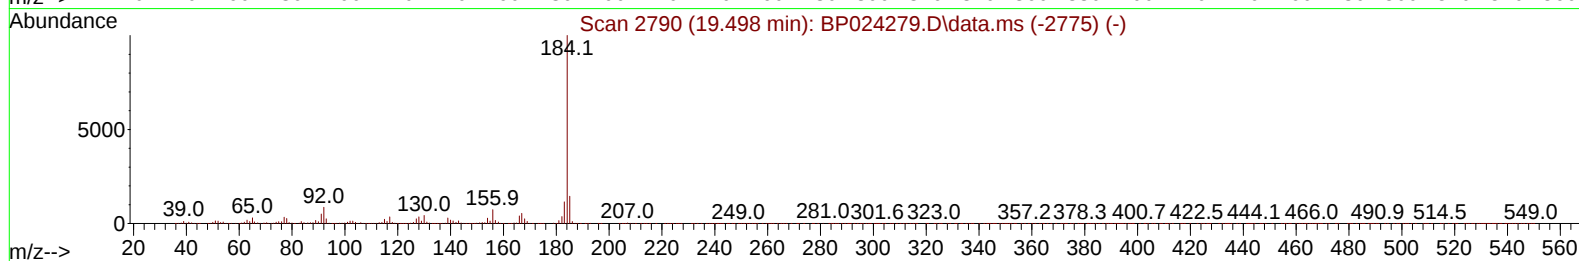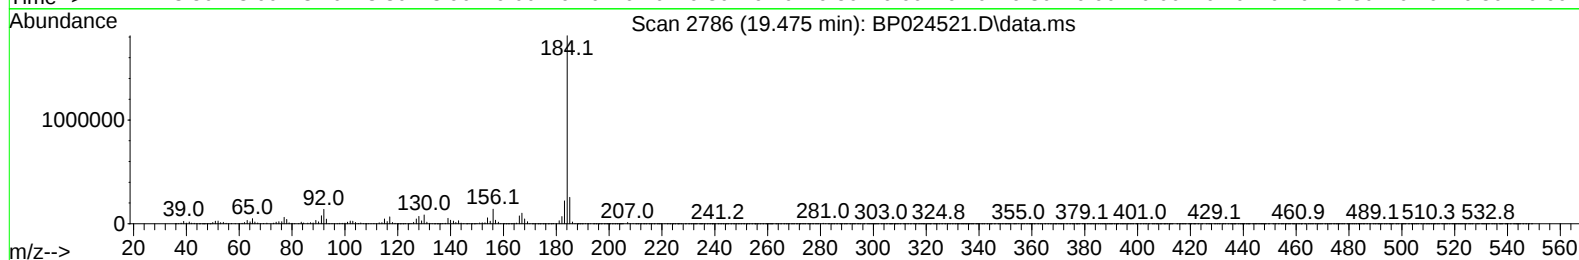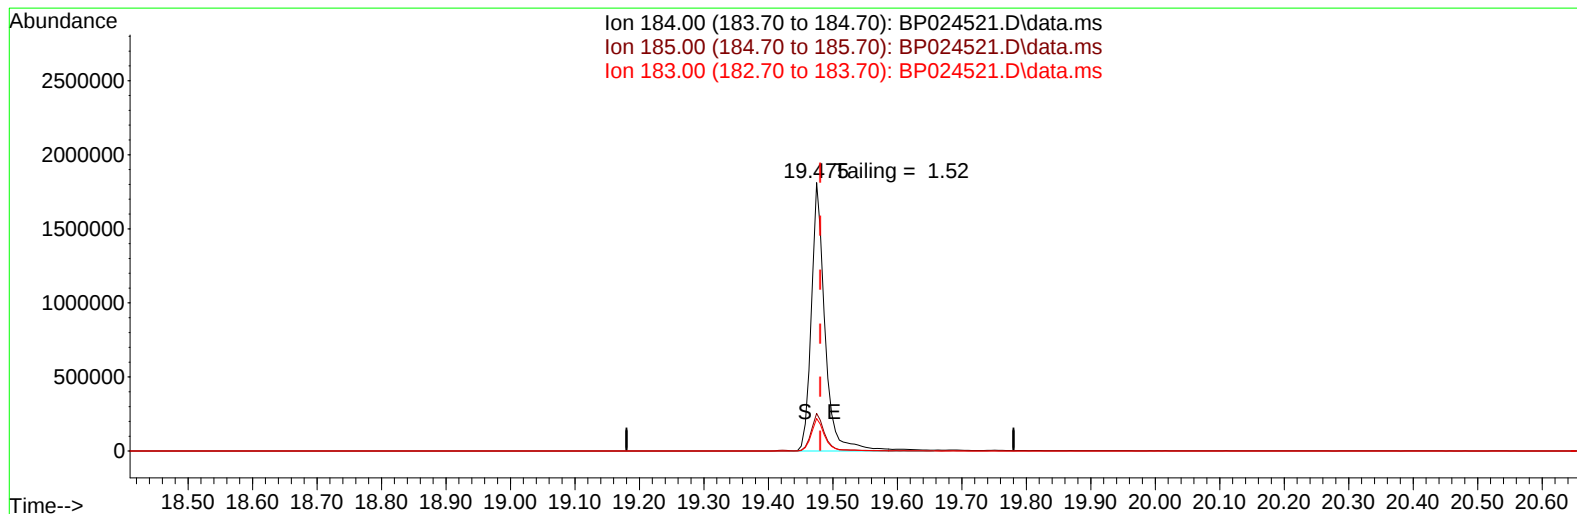

TIC: BP024521.D\data.ms

(77) Benzidine

19.475min (-0.006) 48141.36 ng

response 2700279

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.03
183.00	11.50	12.14
0.00	0.00	0.00