


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050725\
Data File : BP024557.D
Acq On : 07 May 2025 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 18 12:04:48 2025

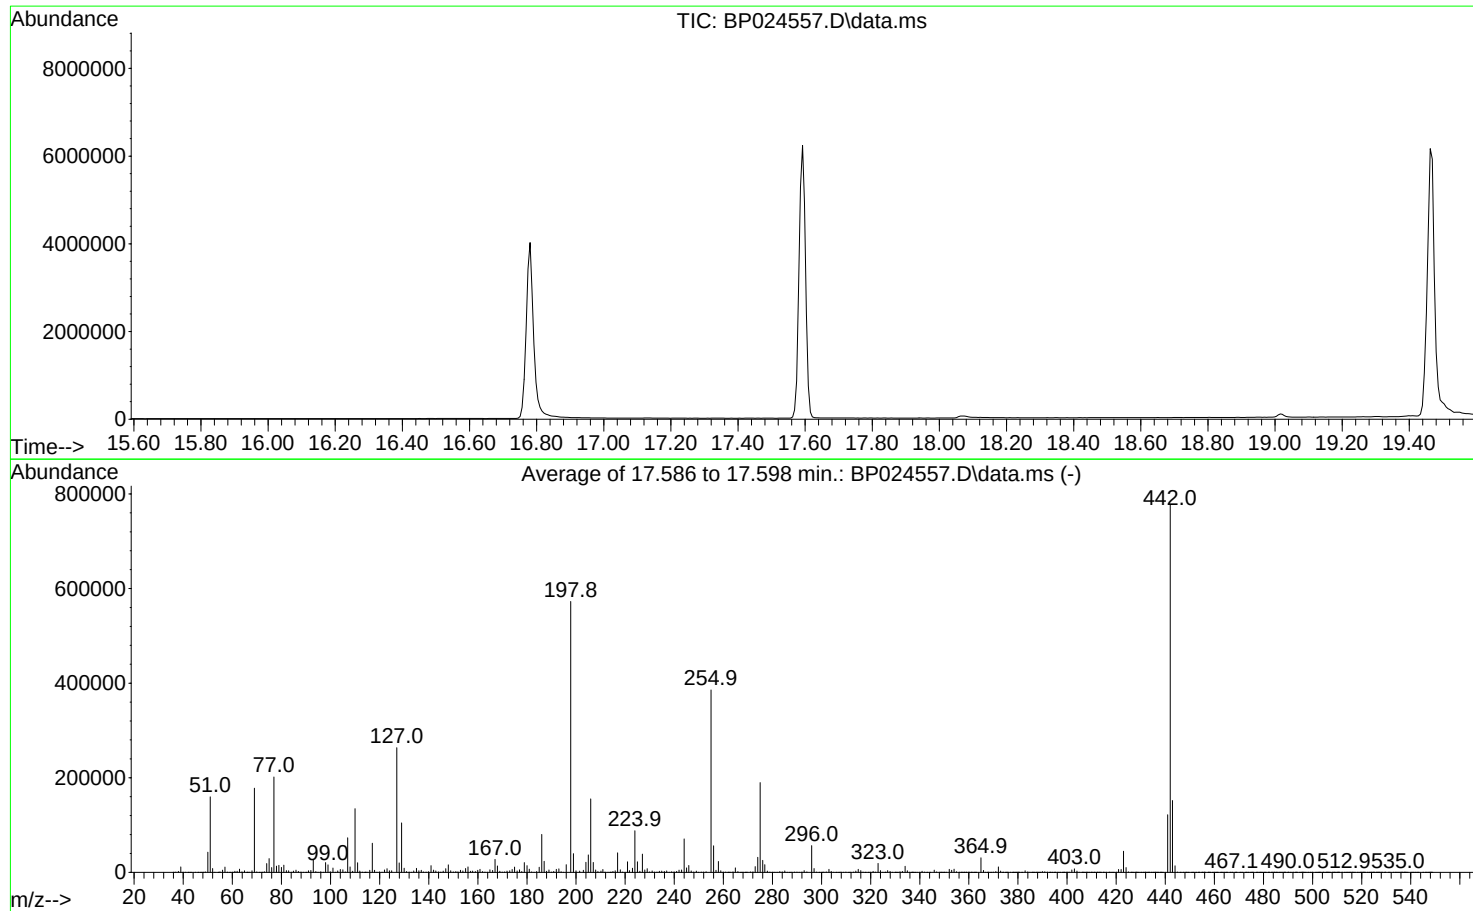

AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.9	159760	PASS
68	69	0.00	2	1.9	3352	PASS
69	198	0.00	100	31.0	177861	PASS
70	69	0.00	2	0.5	888	PASS
127	198	10	80	46.0	263616	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	572840	PASS
199	198	5	9	6.9	39443	PASS
275	198	10	60	33.1	189781	PASS
365	198	1	100	5.4	30664	PASS
441	198	0.01	100	21.3	121821	PASS
442	442	100	100	100.0	777747	PASS
443	442	15	24	19.5	151941	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/7/2025	BNA_P	<u>BP024557.D</u>
Compound Name	Response	Retention Time
DDT	2130375	20.751
DDD	42109	20.292
DDE	3380	19.763
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
45489	2175864	2.09

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050725\
Data File : BP024557.D
Acq On : 07 May 2025 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 08 01:19:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

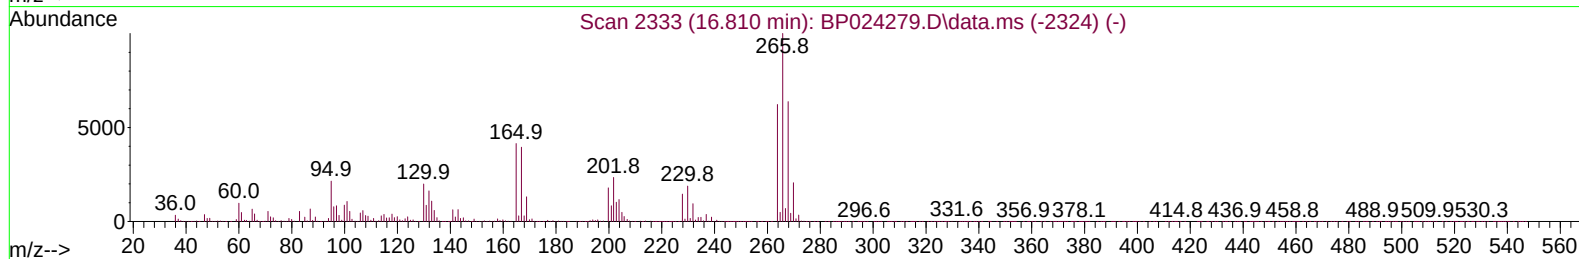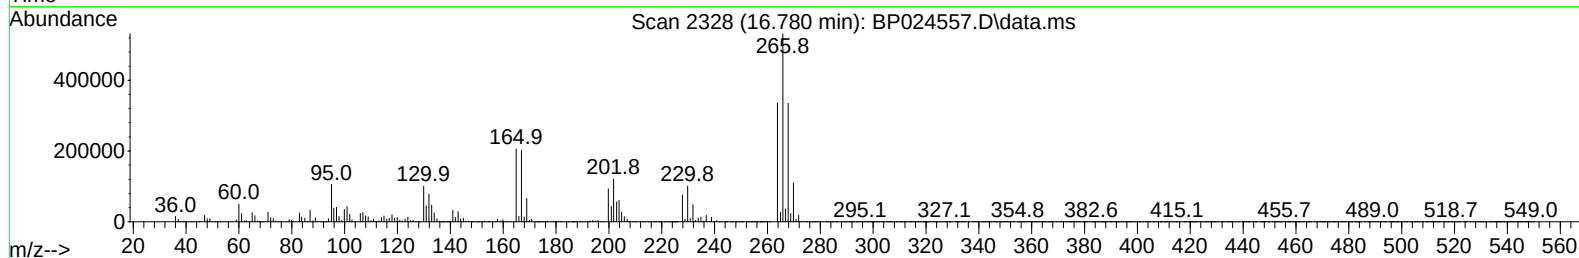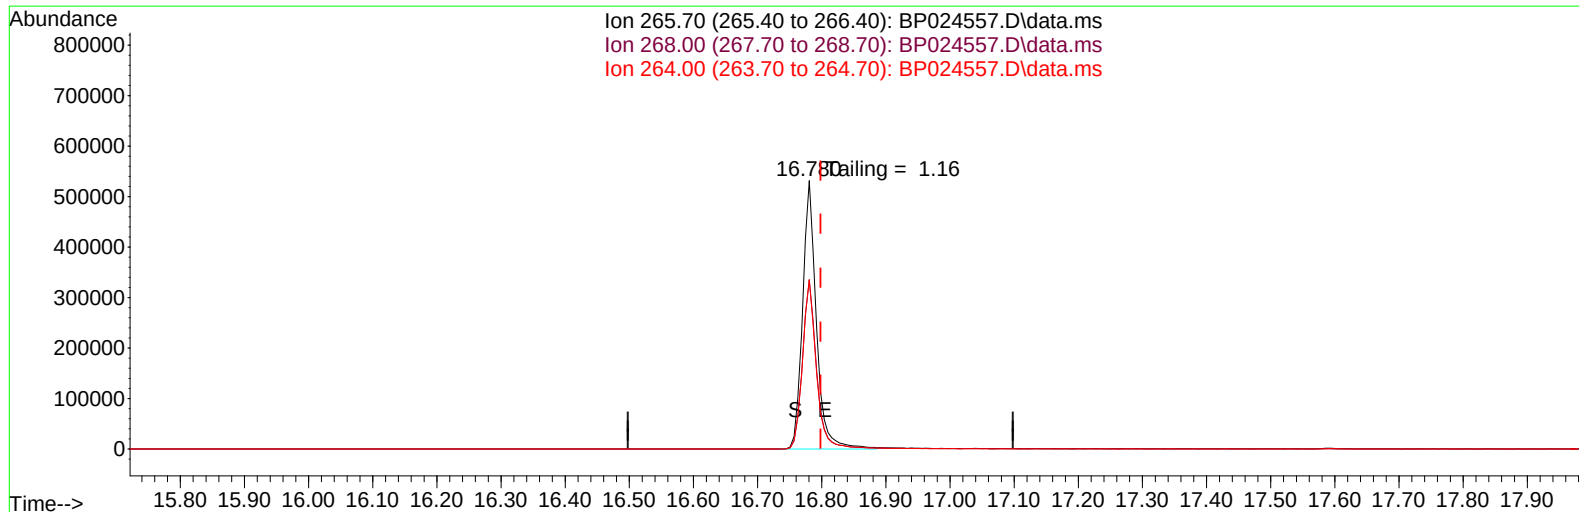

TIC: BP024557.D\data.ms

(70) Pentachlorophenol (C)

16.780min (-0.018) 41423.64 ng




response 804826

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.04
264.00	62.20	63.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050725\
Data File : BP024557.D
Acq On : 07 May 2025 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 07 12:20:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

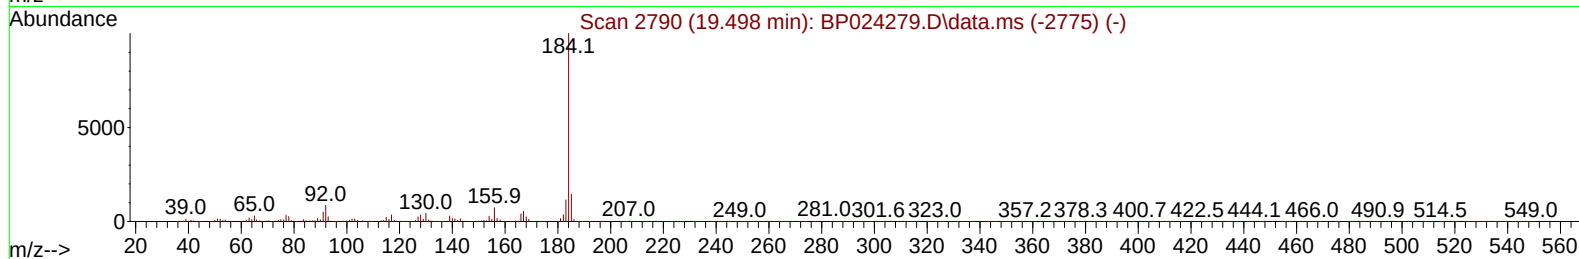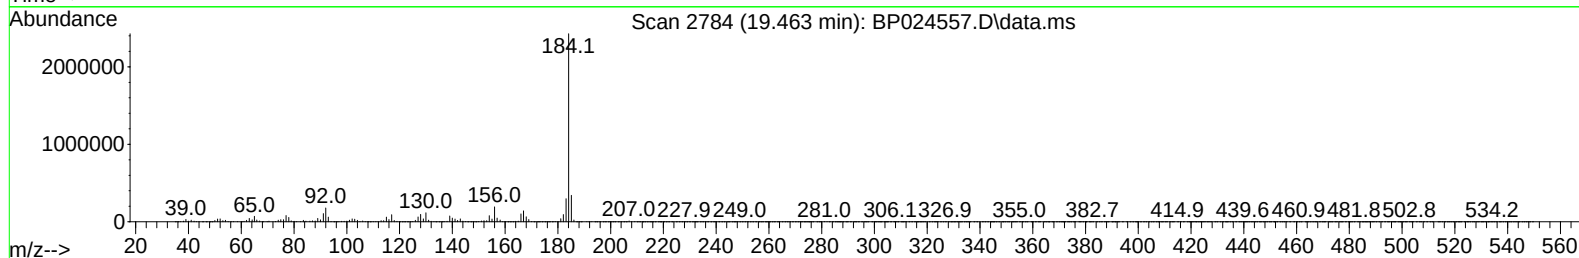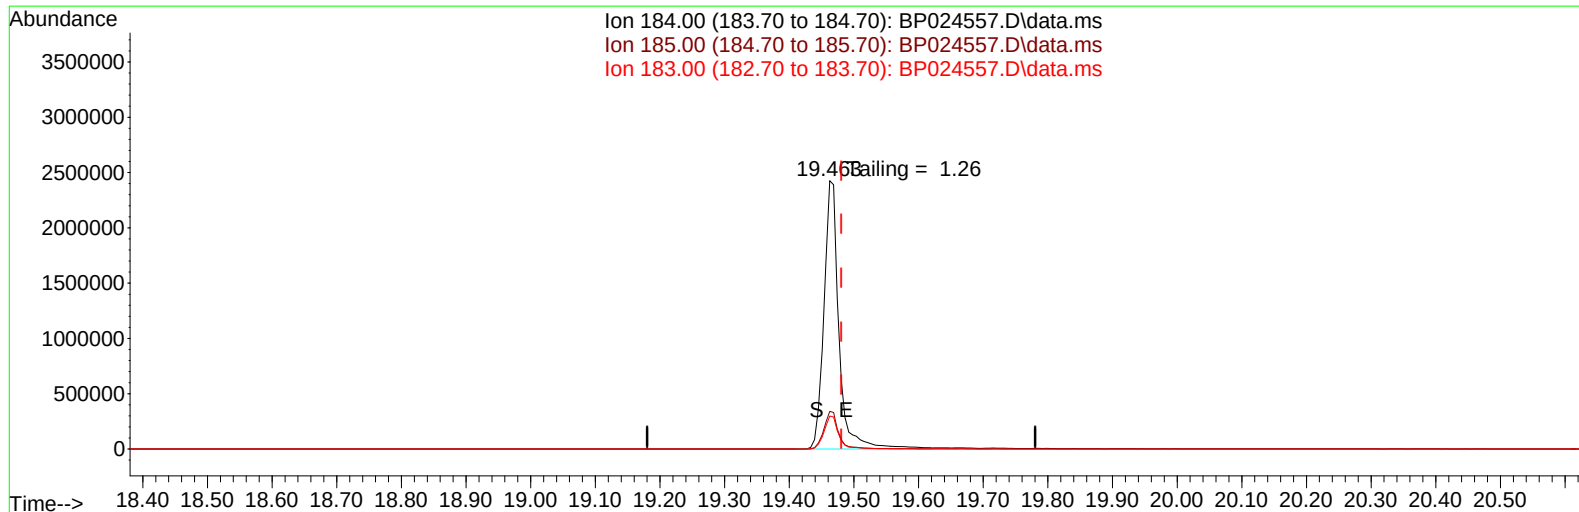

TIC: BP024557.D\data.ms

(77) Benzidine

19.463min (-0.018) 65812.29 ng

response 3926704

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.00
183.00	11.50	12.30
0.00	0.00	0.00