

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050125\
 Data File : VY022106.D
 Acq On : 01 May 2025 14:38
 Operator : SY/MD
 Sample : Q1883-13
 Misc : 14.29g/5.0mL/MSVOA_Y/SOIL/B
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 OU4-VSL-18-042325

Quant Time: May 02 01:30:33 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 23 02:30:30 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.713	168	307701	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.615	114	584162	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.420	117	521346	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	197125	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	156205	54.960	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	109.920%
35) Dibromofluoromethane	7.634	113	198196	51.356	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	102.720%
50) Toluene-d8	10.109	98	696993	47.905	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	95.800%
62) 4-Bromofluorobenzene	12.407	95	276478	56.448	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	112.900%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050125\
Data File : VY022106.D
Acq On : 01 May 2025 14:38
Operator : SY/MD
Sample : Q1883-13
Misc : 14.29g/5.0mL/MSVOA_Y/SOIL/B
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
OU4-VSL-18-042325

Quant Time: May 02 01:30:33 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042225S.M
Quant Title : SW846 8260
QLast Update : Wed Apr 23 02:30:30 2025
Response via : Initial Calibration




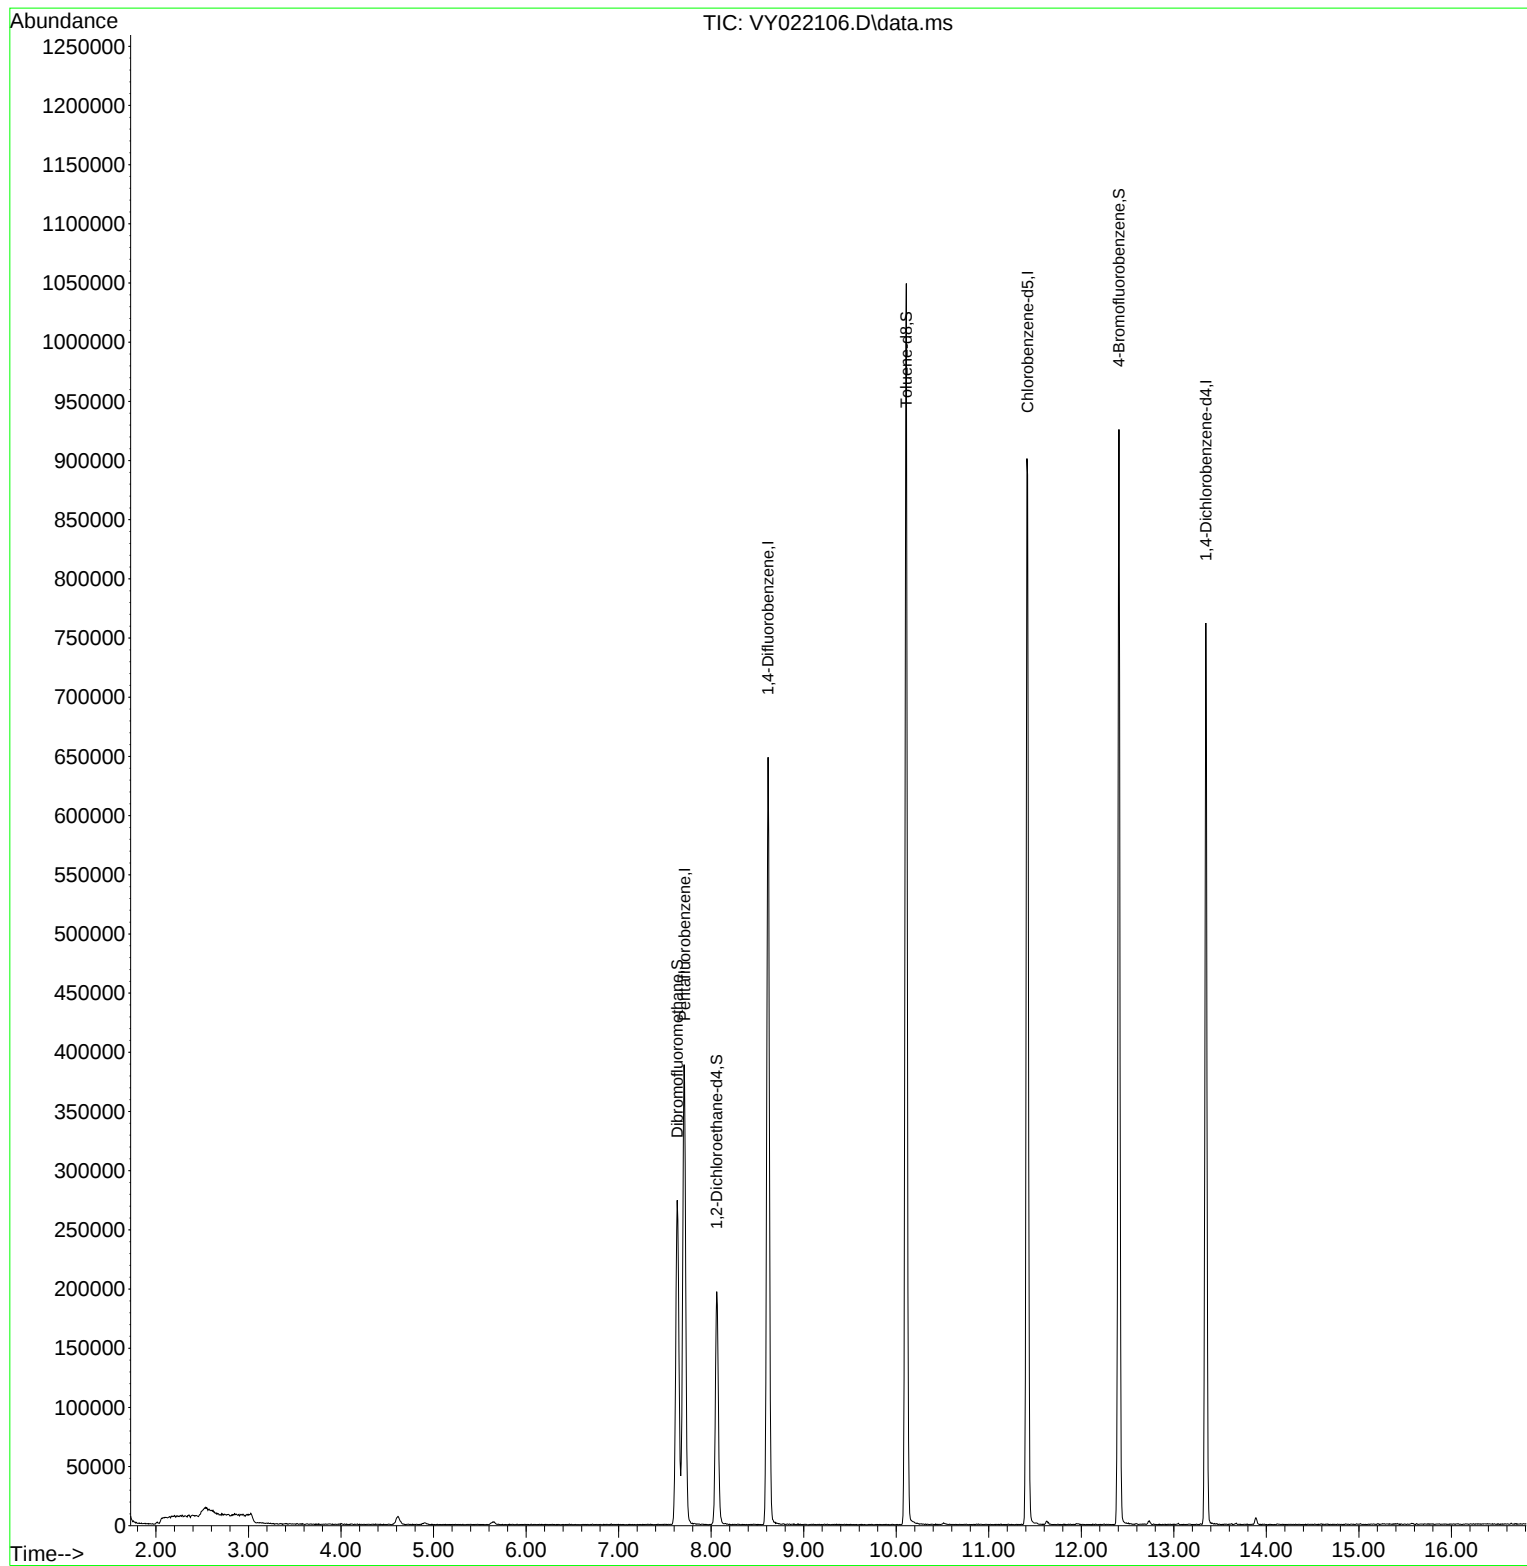


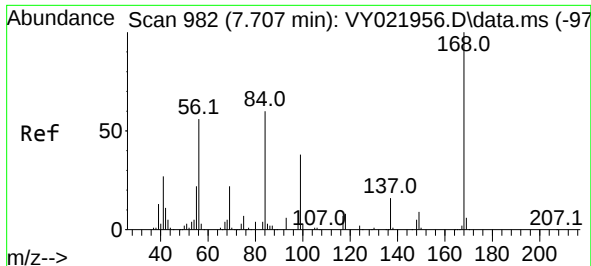

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 982
Delta R.T. 0.006 min
Lab File: VY022106.D
Acq: 01 May 2025 14:38




Instrument :
MSVOA_Y
ClientSampleId :
OU4-VSL-18-042325


Tgt Ion:168 Resp: 307701
Ion Ratio Lower Upper
168 100
99 51.8 43.1 64.7

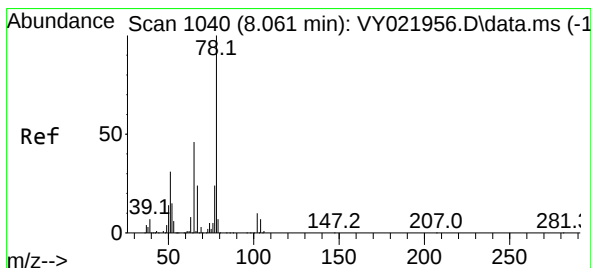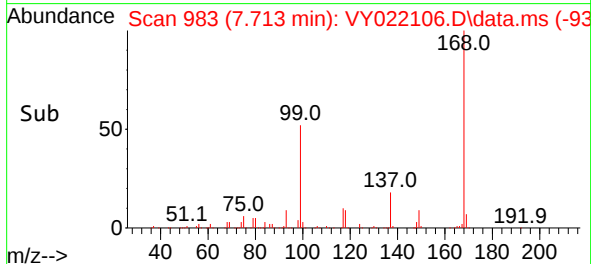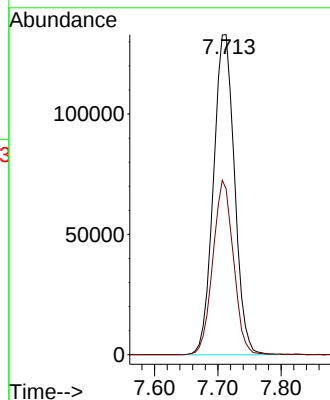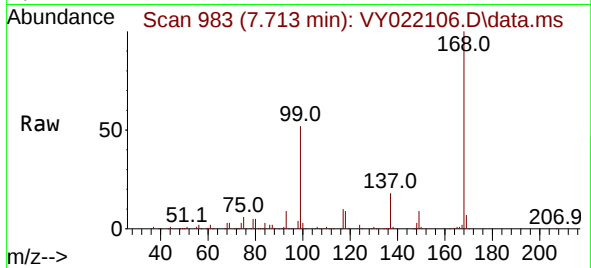

#33
1,2-Dichloroethane-d4
Concen: 54.960 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VY022106.D
Acq: 01 May 2025 14:38

Tgt Ion: 65 Resp: 156205
Ion Ratio Lower Upper
65 100
67 53.9 0.0 105.8

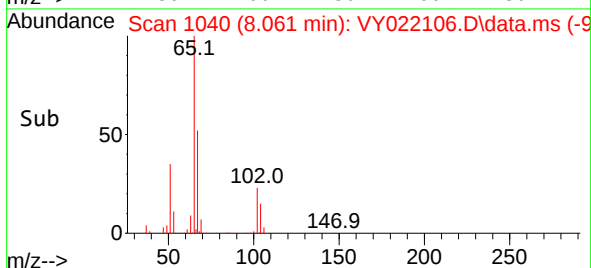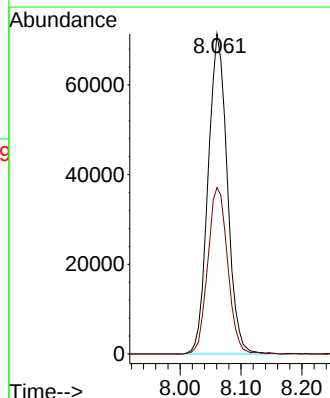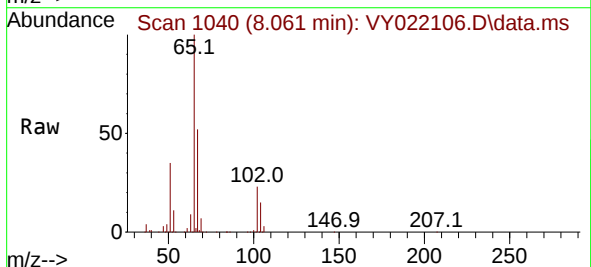

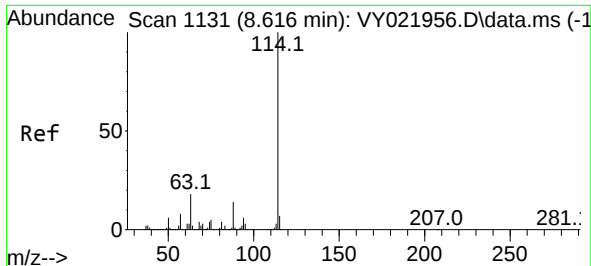

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.615 min Scan# 1131

Delta R.T. -0.000 min

Lab File: VY022106.D

Acq: 01 May 2025 14:38

Instrument :

MSVOA_Y

ClientSampleId :

OU4-VSL-18-042325





Tgt Ion:114 Resp: 584162

Ion Ratio Lower Upper

114 100

63 16.9 0.0 35.4

88 14.6 0.0 28.2

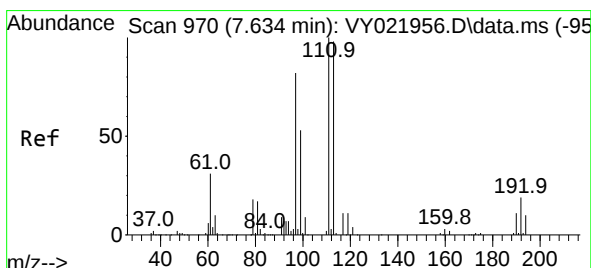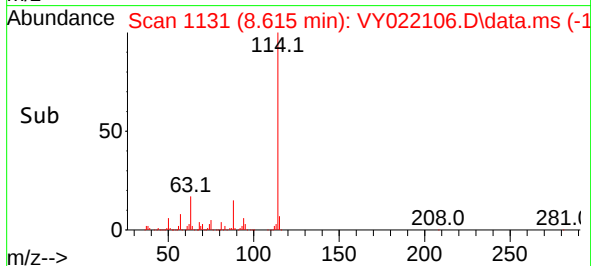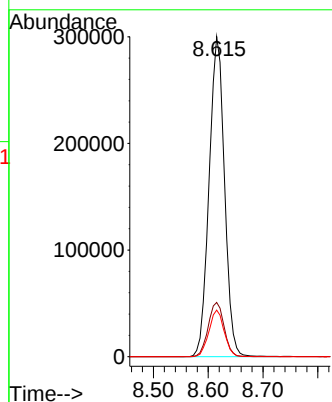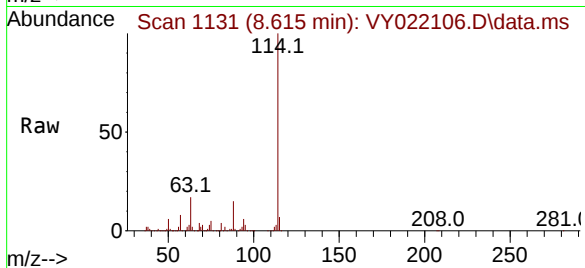

#35

Dibromofluoromethane

Concen: 51.356 ug/l

RT: 7.634 min Scan# 970

Delta R.T. -0.000 min

Lab File: VY022106.D

Acq: 01 May 2025 14:38




Tgt Ion:113 Resp: 198196


Ion Ratio Lower Upper

113 100

111 102.7 81.8 122.8

192 20.8 15.6 23.4


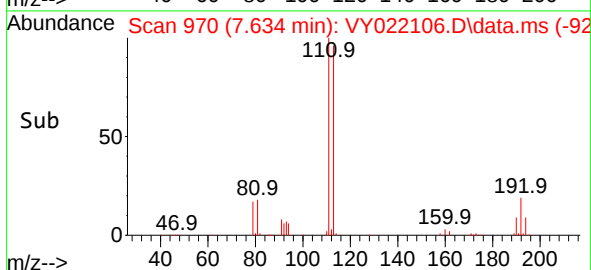
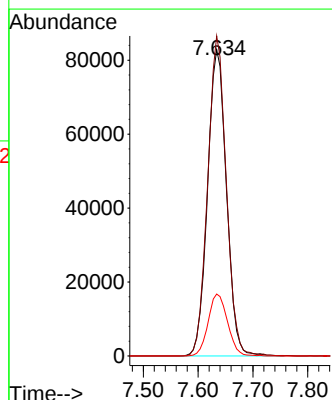
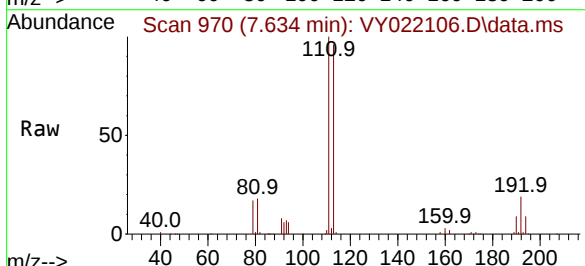


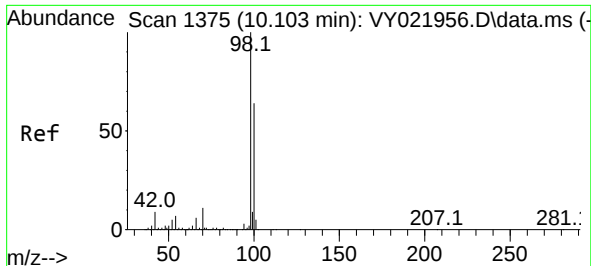

#50
Toluene-d8
Concen: 47.905 ug/l
RT: 10.109 min Scan# 1375
Delta R.T. 0.006 min
Lab File: VY022106.D
Acq: 01 May 2025 14:38




Instrument :
MSVOA_Y
ClientSampleId :
OU4-VSL-18-042325


Tgt Ion: 98 Resp: 696993
Ion Ratio Lower Upper
98 100
100 64.3 51.6 77.4

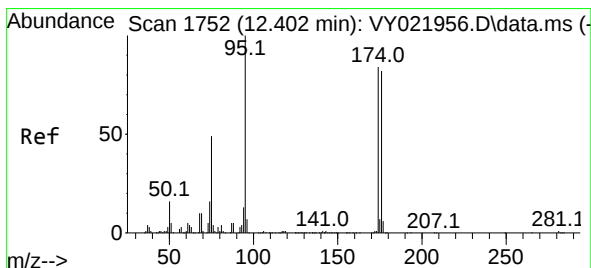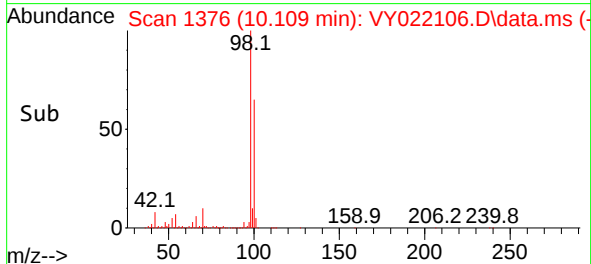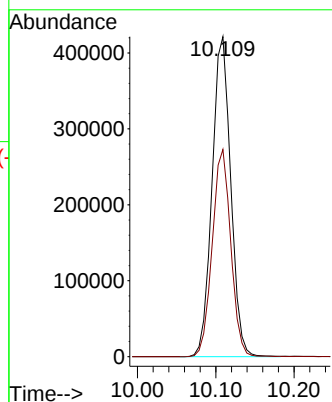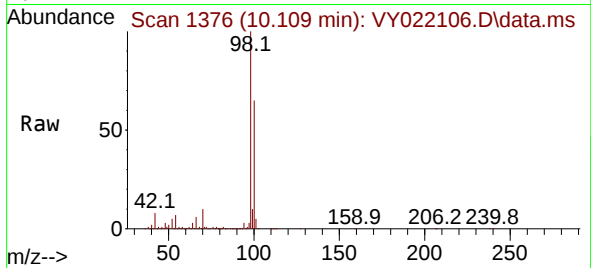

#62
4-Bromofluorobenzene
Concen: 56.448 ug/l
RT: 12.407 min Scan# 1753
Delta R.T. 0.006 min
Lab File: VY022106.D
Acq: 01 May 2025 14:38

Tgt Ion: 95 Resp: 276478
Ion Ratio Lower Upper
95 100
174 89.2 0.0 179.0
176 85.3 0.0 171.8


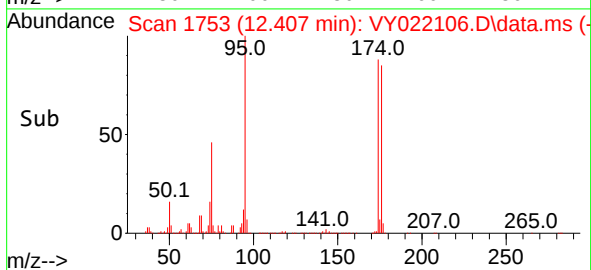
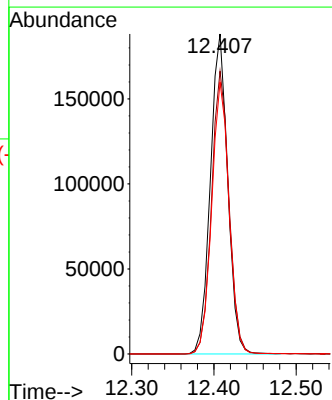
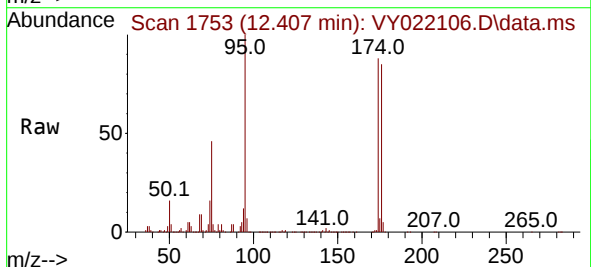


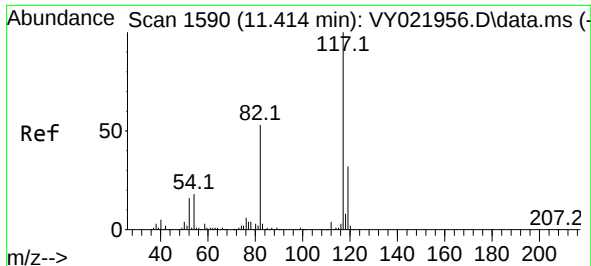

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.420 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY022106.D
Acq: 01 May 2025 14:38

Instrument :
MSVOA_Y
ClientSampleId :
OU4-VSL-18-042325

Tgt Ion:117 Resp: 521346
Ion Ratio Lower Upper
117 100
82 49.5 42.1 63.1
119 32.4 25.7 38.5

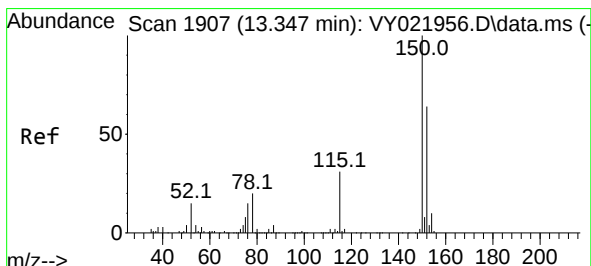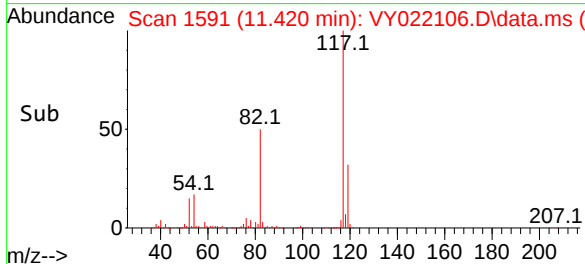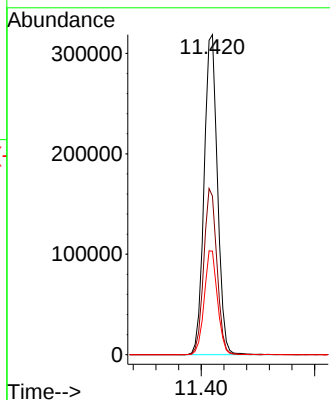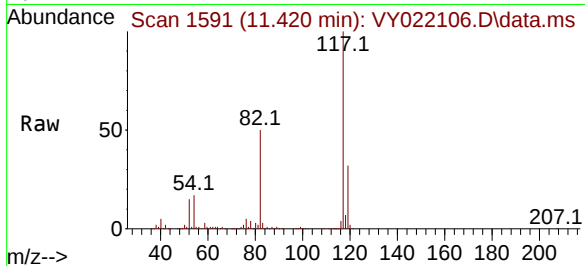

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.346 min Scan# 1907
Delta R.T. -0.000 min
Lab File: VY022106.D
Acq: 01 May 2025 14:38

Tgt Ion:152 Resp: 197125
Ion Ratio Lower Upper
152 100
115 56.6 28.0 84.0
150 156.6 0.0 345.6

