


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043025\
Data File : BM050041.D
Acq On : 30 Apr 2025 10:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 28 18:09:16 2025

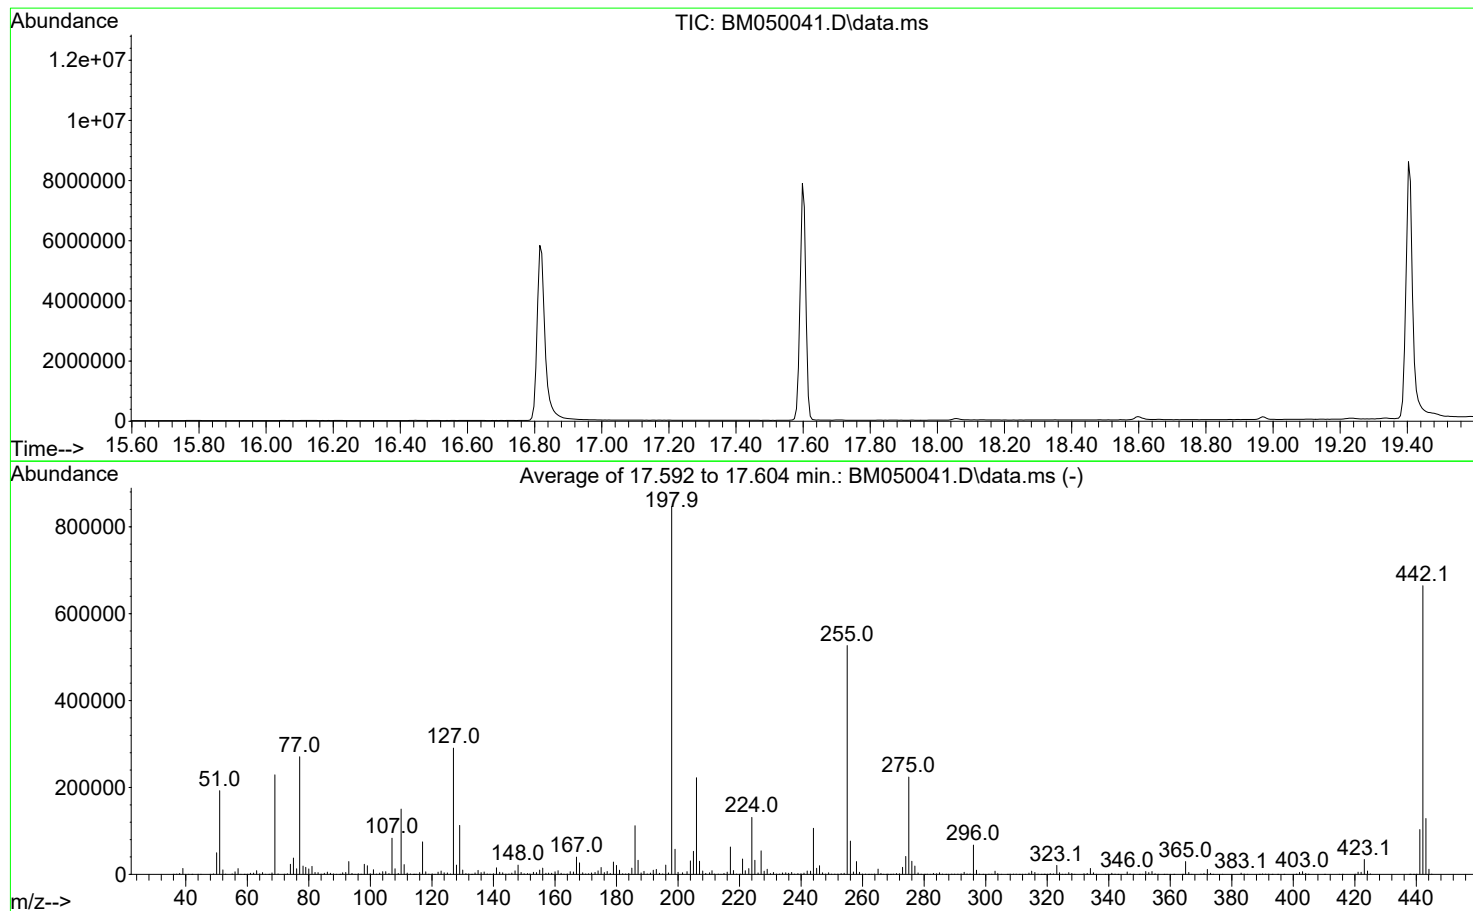

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	22.7	192613	PASS
68	69	0.00	2	1.5	3336	PASS
69	198	0.00	100	27.1	229021	PASS
70	69	0.00	2	0.5	1166	PASS
127	198	10	80	34.3	290581	PASS
197	198	0.00	2	0.4	3307	PASS
198	198	100	100	100.0	846656	PASS
199	198	5	9	6.8	57872	PASS
275	198	10	60	26.5	224064	PASS
365	198	1	100	3.5	29493	PASS
441	198	0.01	100	12.2	102997	PASS
442	442	50	100	100.0	664192	PASS
443	442	15	24	19.4	128672	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/30/2025	BNA_M	<u>BM050041.D</u>
Compound Name	Response	Retention Time
DDT	2852498	20.639
DDD	23676	20.251
DDE	1927	19.692
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25603	2878101	0.89

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043025\
Data File : BM050041.D
Acq On : 30 Apr 2025 10:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 30 11:54:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

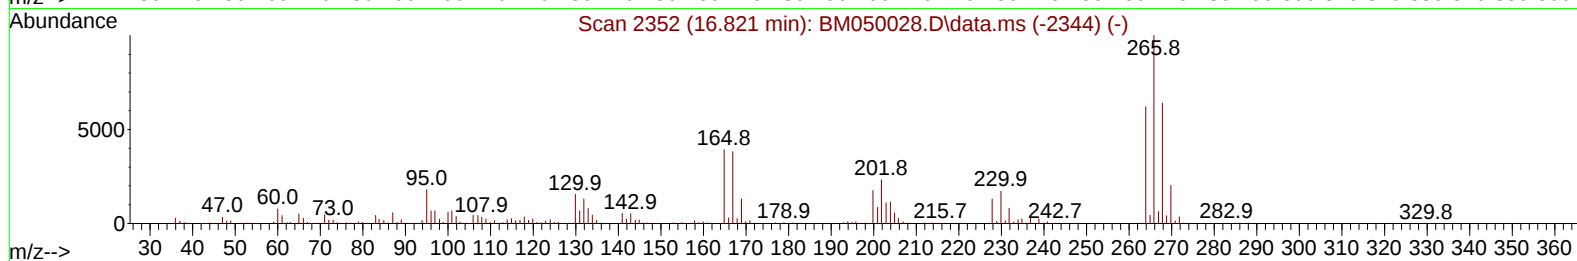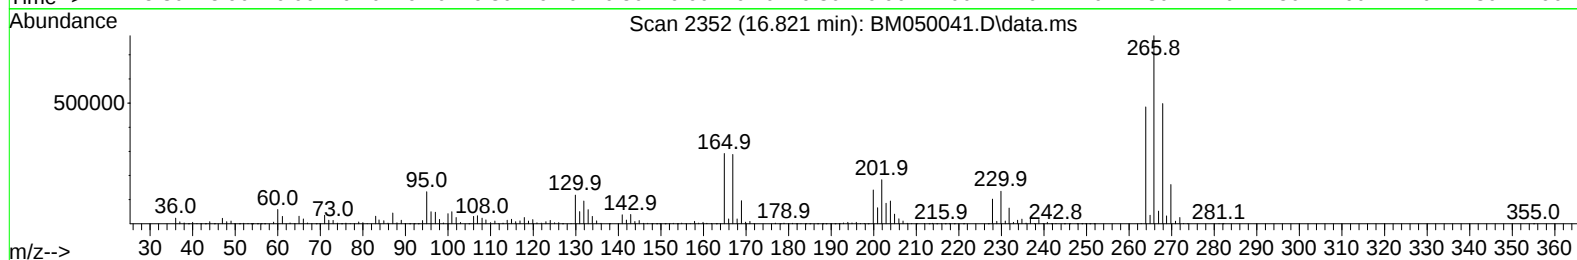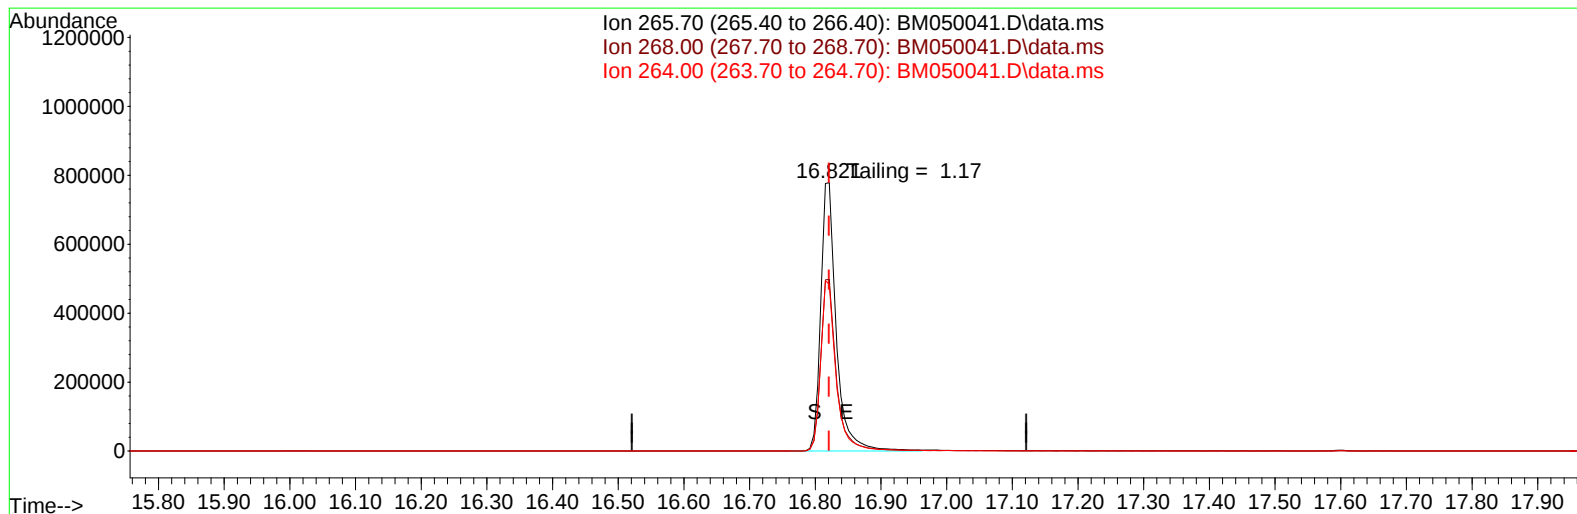

TIC: BM050041.D\data.ms

(70) Pentachlorophenol (C)

16.821min (+ 0.000) 47790.89 ng




response 1282068

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.93
264.00	62.00	62.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043025\
Data File : BM050041.D
Acq On : 30 Apr 2025 10:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 30 11:54:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

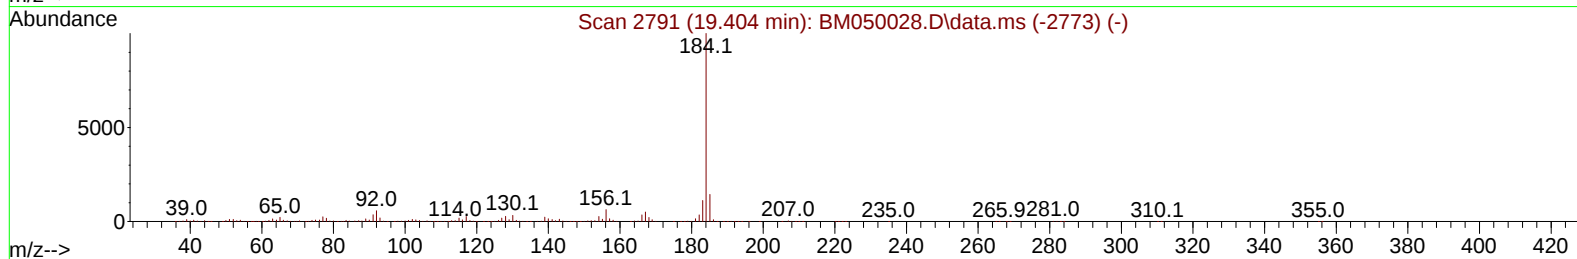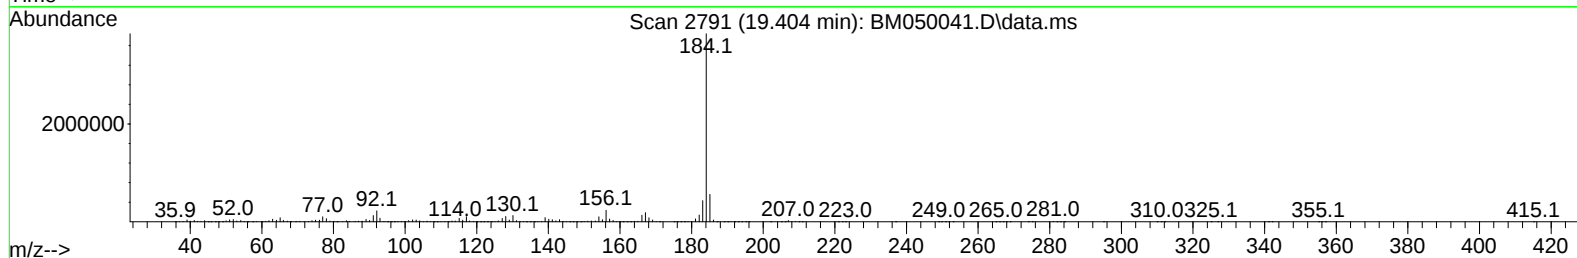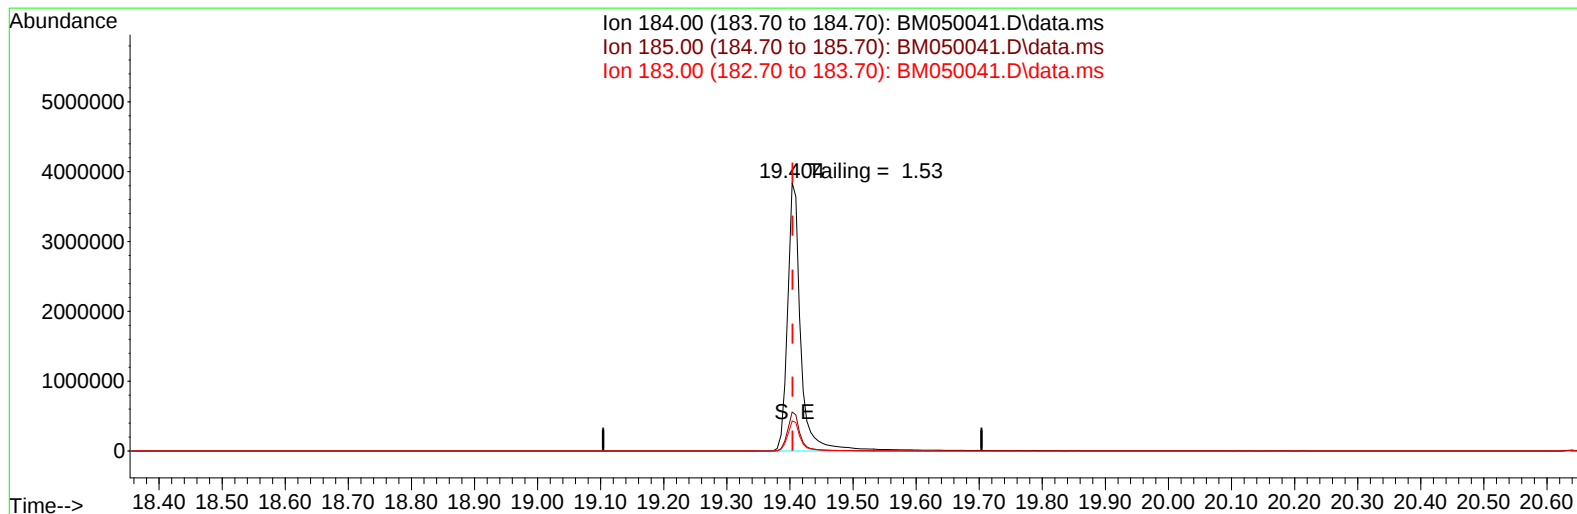

TIC: BM050041.D\data.ms

(77) Benzidine

19.404min (-0.000) 7947.43 ng

response 5627615

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.56
183.00	11.10	11.24
0.00	0.00	0.00