
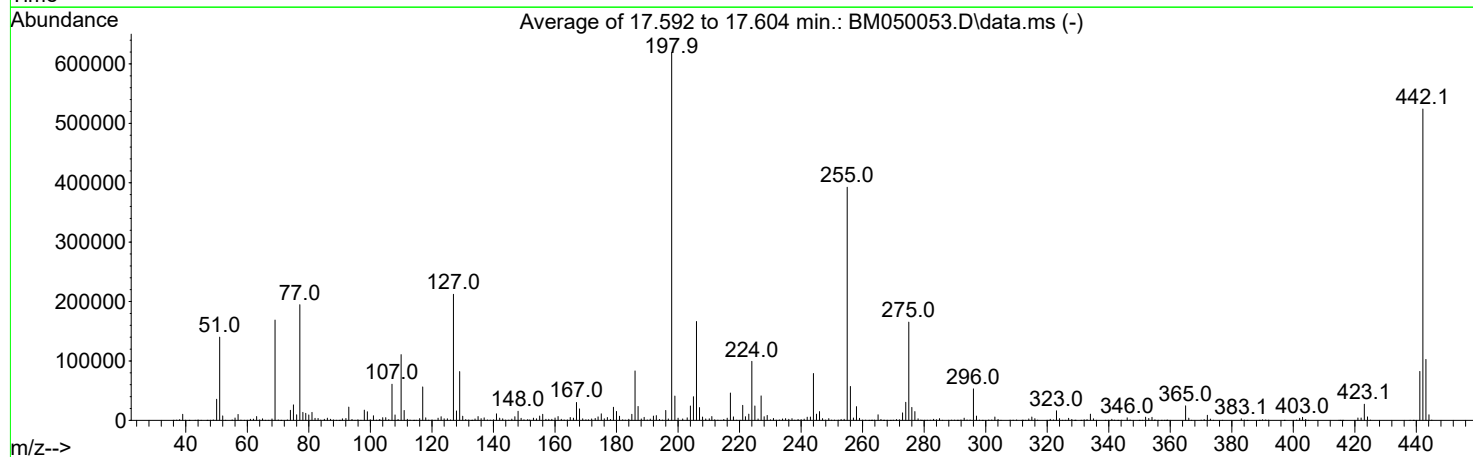


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043025\
Data File : BM050053.D
Acq On : 30 Apr 2025 20:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 28 18:09:16 2025

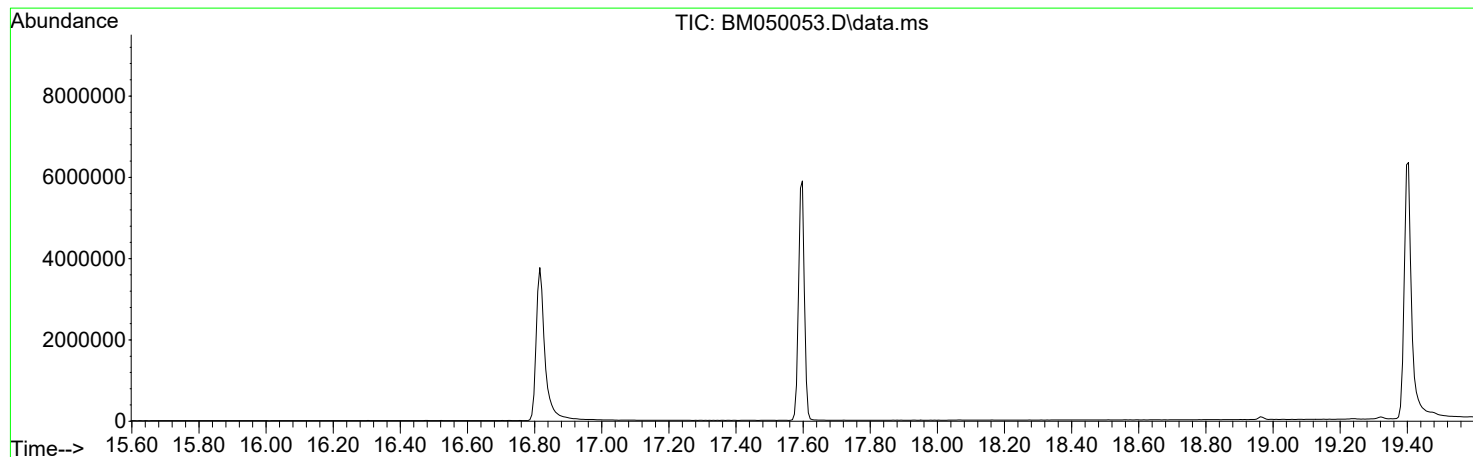

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.6	140036	PASS
68	69	0.00	2	1.5	2536	PASS
69	198	0.00	100	27.3	169029	PASS
70	69	0.00	2	0.5	902	PASS
127	198	10	80	34.3	212203	PASS
197	198	0.00	2	0.4	2425	PASS
198	198	100	100	100.0	619264	PASS
199	198	5	9	6.6	40851	PASS
275	198	10	60	26.7	165312	PASS
365	198	1	100	4.0	24624	PASS
441	198	0.01	100	13.3	82312	PASS
442	442	50	100	100.0	524203	PASS
443	442	15	24	19.6	102515	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/30/2025	BNA_M	<u>BM050053.D</u>
Compound Name	Response	Retention Time
DDT	2117616	20.633
DDD	64903	20.198
DDE	1456	19.686
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
66359	2183975	3.04

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043025\
Data File : BM050053.D
Acq On : 30 Apr 2025 20:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 01 01:52:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

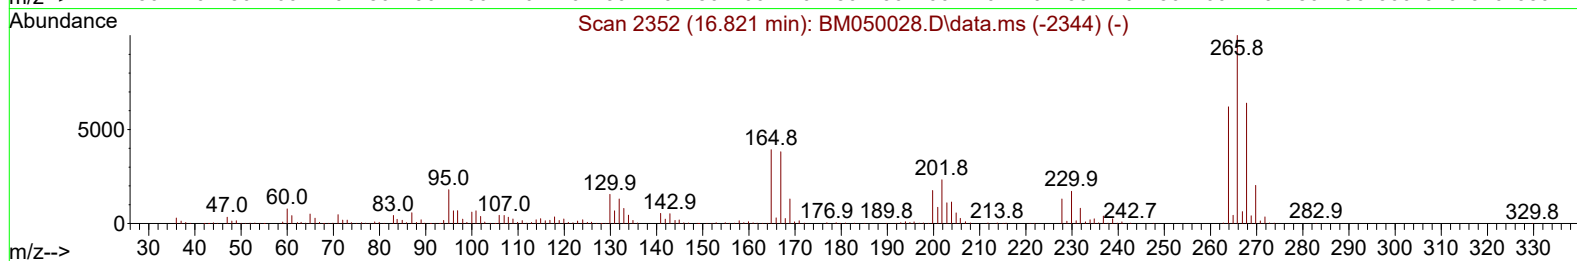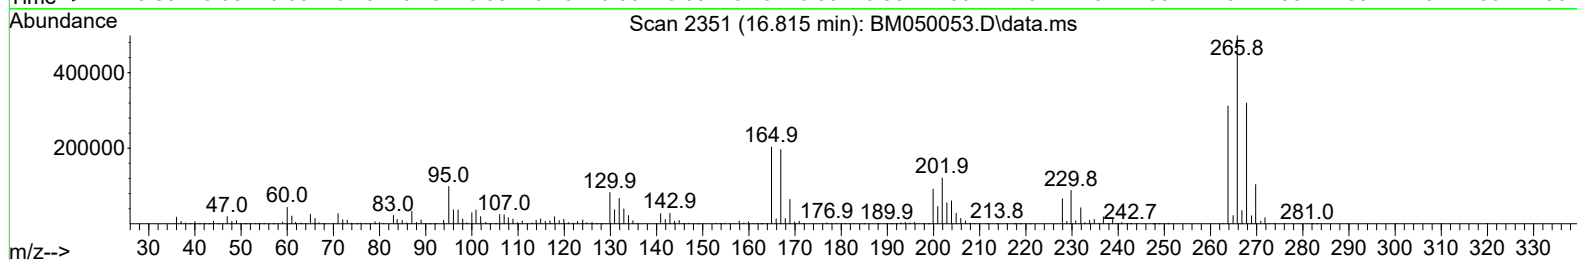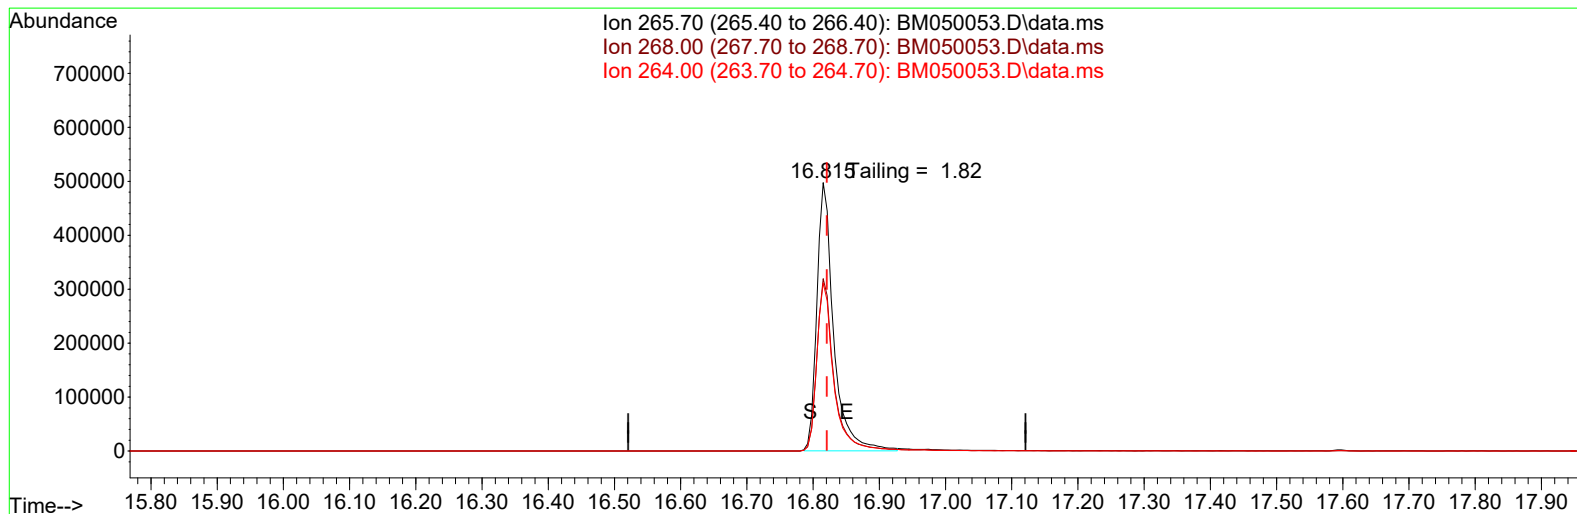

TIC: BM050053.D\data.ms

(70) Pentachlorophenol (C)

16.815min (-0.006) 998032.02 ng




response 884891

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	64.19
264.00	62.00	62.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043025\
Data File : BM050053.D
Acq On : 30 Apr 2025 20:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 01 01:52:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

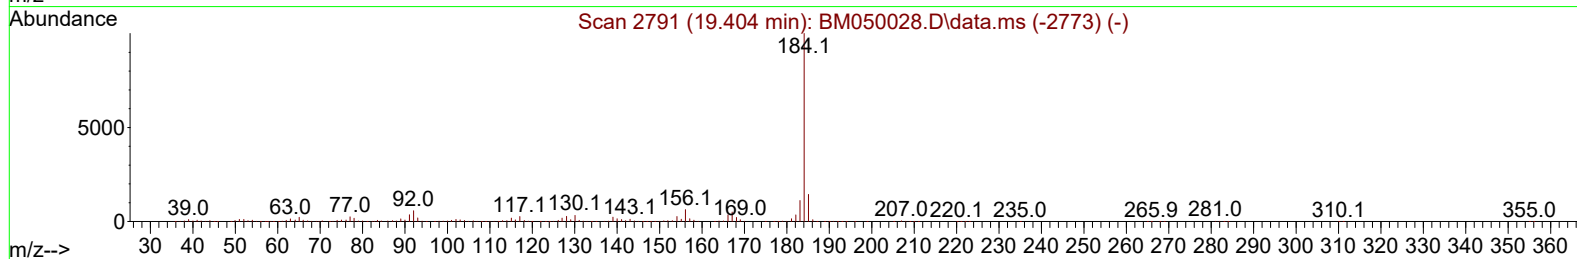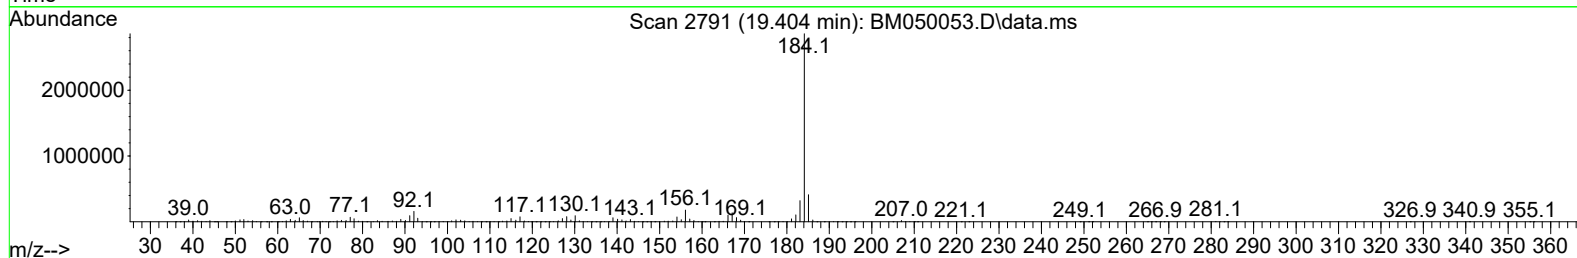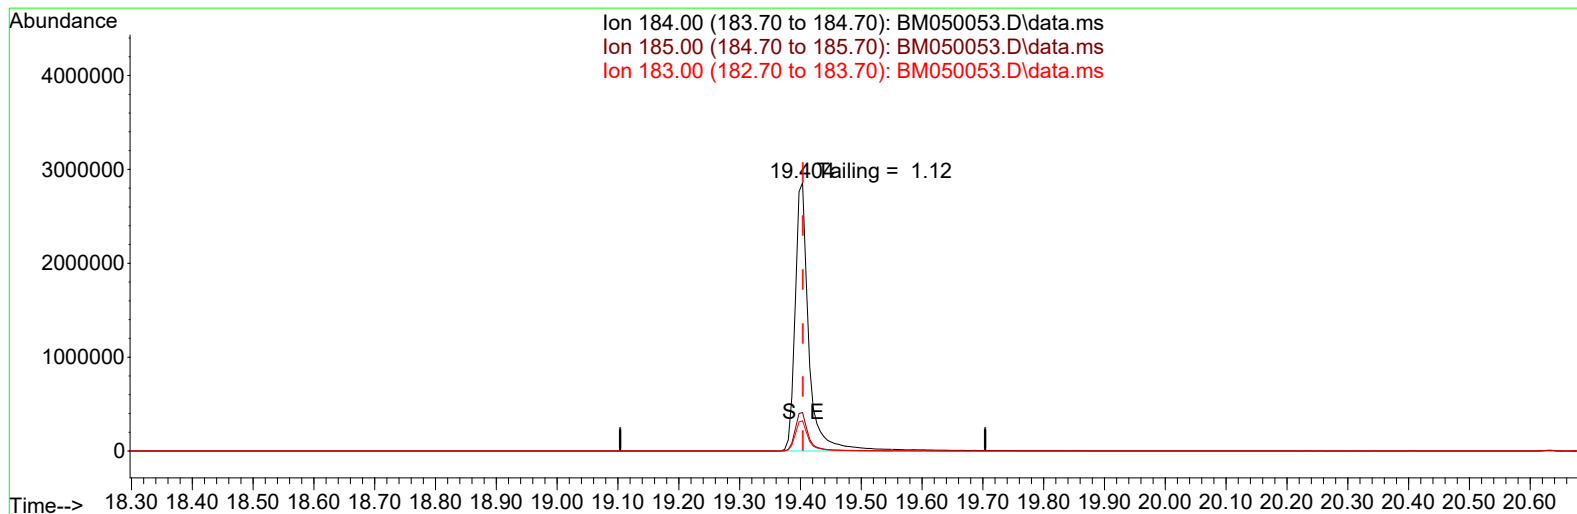

TIC: BM050053.D\data.ms

(77) Benzidine

19.404min (-0.000) 132996.89 ng m

response 4440691

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.39
183.00	11.10	11.28
0.00	0.00	0.00