


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042825\
Data File : BP024434.D
Acq On : 28 Apr 2025 12:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 18 12:04:48 2025

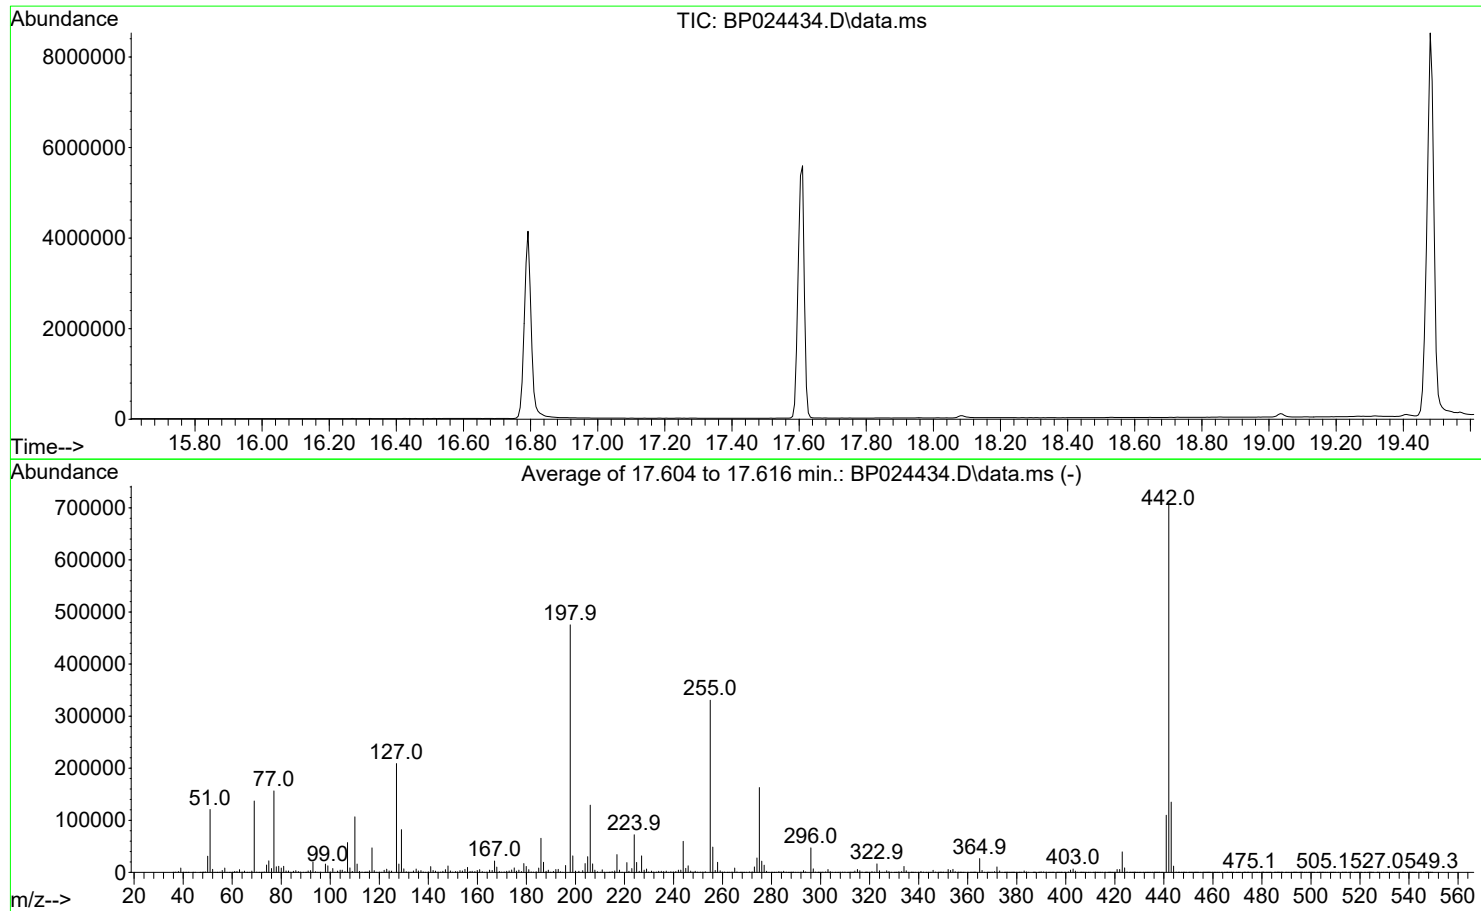

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.4	120703	PASS
68	69	0.00	2	1.9	2619	PASS
69	198	0.00	100	28.8	136965	PASS
70	69	0.00	2	0.5	694	PASS
127	198	10	80	44.0	209032	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	475407	PASS
199	198	5	9	6.6	31521	PASS
275	198	10	60	34.2	162789	PASS
365	198	1	100	5.6	26400	PASS
441	198	0.01	100	23.1	109685	PASS
442	442	100	100	100.0	706347	PASS
443	442	15	24	19.1	134960	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/28/2025	BNA_P	<u>BP024434.D</u>
Compound Name	Response	Retention Time
DDT	1970155	20.769
DDD	46360	20.304
DDE	3338	19.775
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
49698	2019853	2.46

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042825\
Data File : BP024434.D
Acq On : 28 Apr 2025 12:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 28 14:02:25 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

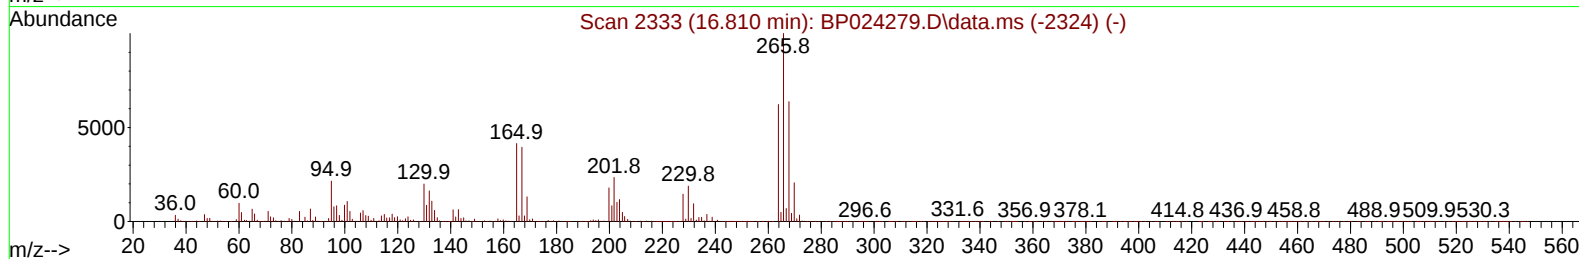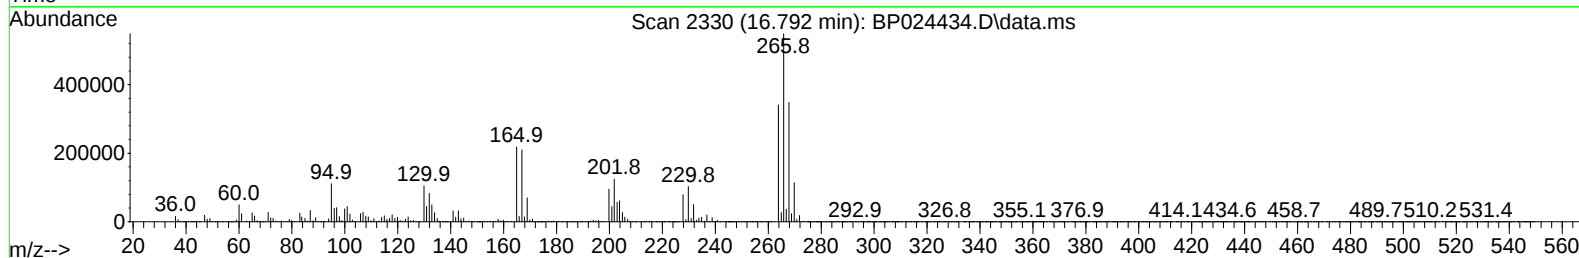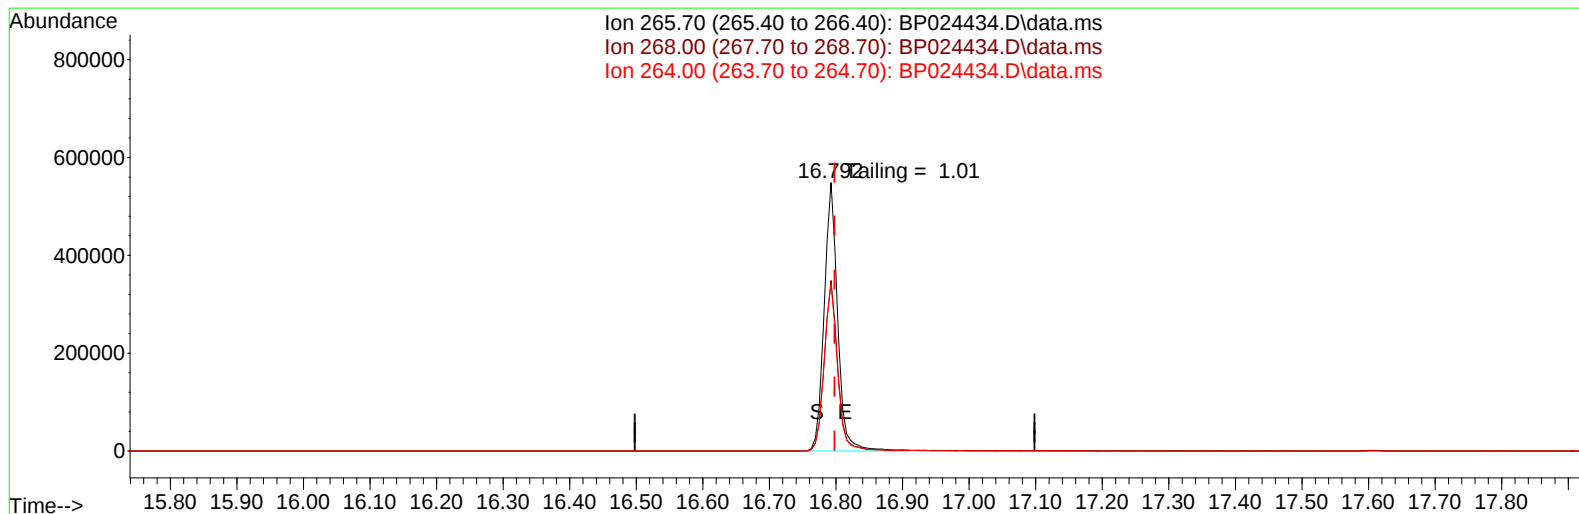

TIC: BP024434.D\data.ms

(70) Pentachlorophenol (C)

16.792min (-0.006) 264266.31 ng




response 776280

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.49
264.00	62.20	62.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042825\
Data File : BP024434.D
Acq On : 28 Apr 2025 12:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 28 14:02:25 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

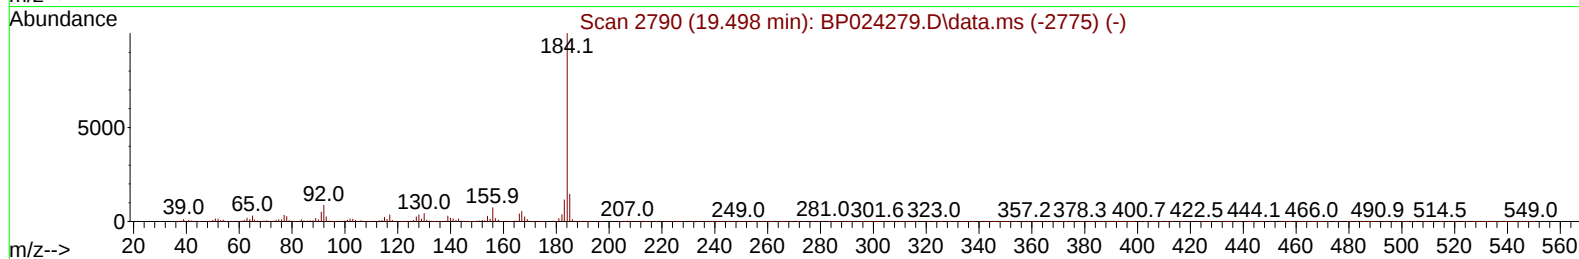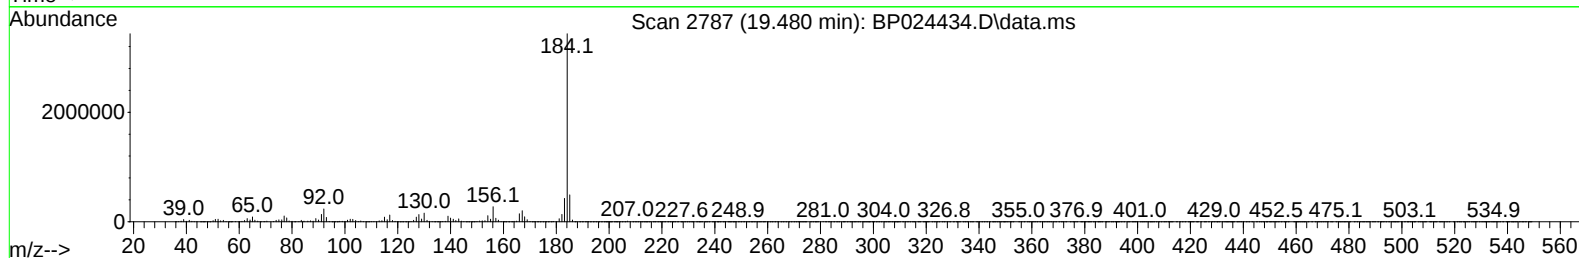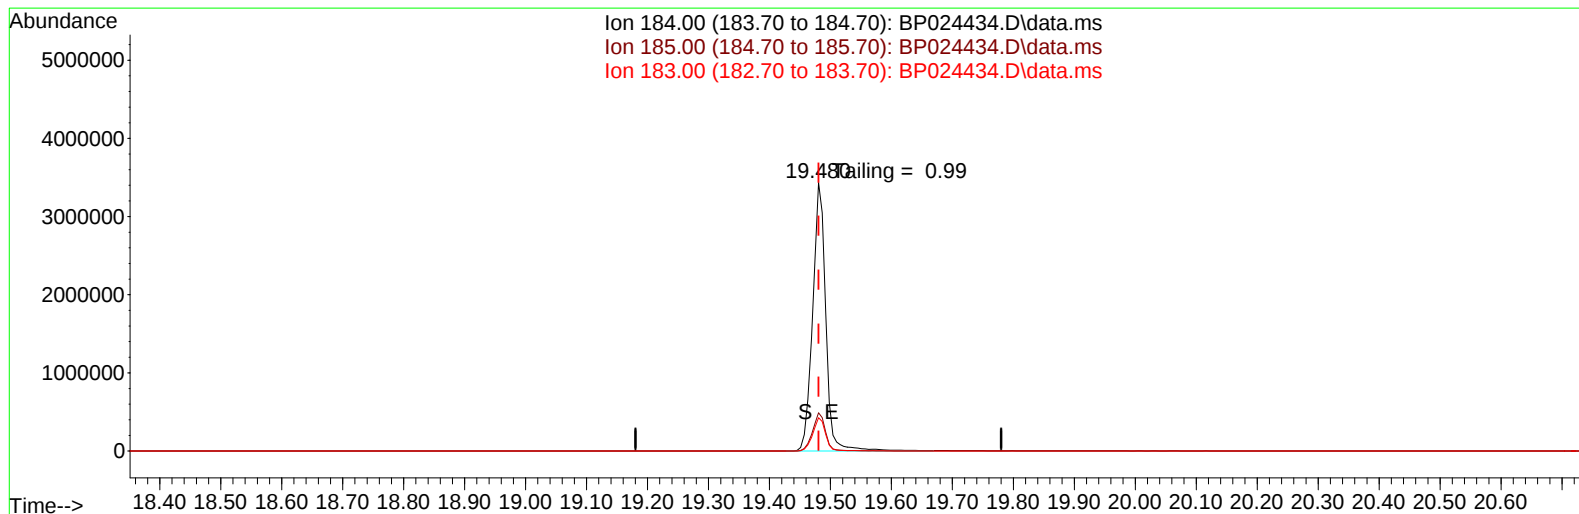

TIC: BP024434.D\data.ms

(77) Benzidine

19.480min (+ 0.000) 246689.07 ng

response 5178300

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.27
183.00	11.50	12.41
0.00	0.00	0.00