

## Prep Standard - Chemical Standard Summary

**Order ID :** Q1901

**Test :** EPH

**Prepbatch ID :** PB167840,PB167903,

**Sequence ID/Qc Batch ID:** FC050225AL,FC050825AL,FD050225AR,FD050825AR,

**Standard ID :**

EP2569,EP2600,EP2607,PP24170,PP24174,PP24175,PP24176,PP24177,PP24178,PP24179,PP24462,PP24465,PP24491,PP24499,PP24500,PP24501,PP24502,PP24503,PP24504,PP24505,PP24506,

**Chemical ID :**

E2865,E3551,E3757,E3904,E3916,E3917,E3926,E3928,E3929,E3930,E3933,M6121,P10758,P11140,P12363,P12981,P12983,P12989,P12990,P13050,P13279,P13596,P13650,P13660,P13662,P13664,P13667,P13671,P13673,P13674,P13709,P13762,P13764,P13865,P13896,P13897,P13898,P13899,P13900,P13901,P13903,P13905,P13906,P13912,P13919,P13920,P13921,P13923,P13926,P13927,P13928,P13931,P13947,P13948,P13950,P13951,P13952,P13953,P13954,P13955,W3112,W3177,

## Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3319	6N HCL	<a href="#">EP2569</a>	12/02/2024	05/13/2025	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 12/02/2024

**FROM** 219.00000ml of M6121 + 781.00000ml of W3112 = Final Quantity: 1000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2017	1:1 ACETONE/METHYLENE CHLORIDE	<a href="#">EP2600</a>	04/07/2025	10/03/2025	Rajesh Parikh	None	None	Riteshkumar Patel 04/07/2025

**FROM** 8000.00000ml of E3904 + 8000.00000ml of E3917 = Final Quantity: 16000.000 ml



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	<a href="#">EP2607</a>	04/25/2025	07/01/2025	RUPESHKUMAR SHAH	Extraction_SC ALE_2 (EX-SC-2)	None	Riteshkumar Patel  04/25/2025
<b><u>FROM</u></b> 4000.00000gram of E3551 = Final Quantity: 4000.000 gram								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
781	100 PPM Aliphatic HC Working STD (Restek)	<a href="#">PP24170</a>	02/03/2025	08/03/2025	Yogesh Patel	None	None	Ankita Jodhani 02/03/2025
<b><u>FROM</u></b> 0.25000ml of P12981 + 0.25000ml of P13671 + 1.25000ml of P12363 + 23.25000ml of W3177 = Final Quantity: 25.000 ml								

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2900	100 PPM Aliphatic HC STD (Absolute)	<a href="#">PP24174</a>	02/03/2025	08/03/2025	Yogesh Patel	None	None	Ankita Jodhani
								02/03/2025

**FROM** 0.25000ml of P12983 + 0.25000ml of P13650 + 2.50000ml of P13279 + 22.00000ml of W3177 = Final Quantity: 25.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
783	50 PPM Aliphatic HC STD	<a href="#">PP24175</a>	02/03/2025	08/03/2025	Yogesh Patel	None	None	Ankita Jodhani
								02/03/2025

**FROM** 0.50000ml of W3177 + 0.50000ml of PP24170 = Final Quantity: 1.000 ml



## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
784	20 PPM Aliphatic HC STD	<a href="#">PP24176</a>	02/03/2025	08/03/2025	Yogesh Patel	None	None	Ankita Jodhani
02/03/2025								

**FROM** 0.80000ml of W3177 + 0.20000ml of PP24170 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
785	10 PPM Aliphatic HC STD	<a href="#">PP24177</a>	02/03/2025	08/03/2025	Yogesh Patel	None	None	Ankita Jodhani
02/03/2025								

**FROM** 0.90000ml of W3177 + 0.10000ml of PP24170 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
786	5 PPM Aliphatic HC STD	<a href="#">PP24178</a>	02/03/2025	08/03/2025	Yogesh Patel	None	None	Ankita Jodhani
								02/03/2025

**FROM** 0.90000ml of W3177 + 0.10000ml of PP24175 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2901	20 PPM Aliphatic HC STD ICV (Absolute)	<a href="#">PP24179</a>	02/03/2025	08/03/2025	Yogesh Patel	None	None	Ankita Jodhani
								02/03/2025

**FROM** 0.80000ml of W3177 + 0.20000ml of PP24174 = Final Quantity: 1.000 ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1330	100 PPM NJEPH Spike Solution	<a href="#">PP24462</a>	04/15/2025	10/15/2025	Yogesh Patel	None	None	Abdul Mirza 04/21/2025
<u>FROM</u>	5.00000ml of P13709 + 5.00000ml of P13865 + 5.00000ml of P13896 + 5.00000ml of P13897 + 5.00000ml of P13898 + 5.00000ml of P13899 + 5.00000ml of P13900 + 5.00000ml of P13901 + 5.00000ml of P13903 + 5.00000ml of P13905 + 5.00000ml of P13906 + 5.00000ml of P13912 + 5.00000ml of P13919 + 5.00000ml of P13920 + 5.00000ml of P13921 + 5.00000ml of P13923 + 5.00000ml of P13926 + 5.00000ml of P13927 + 5.00000ml of P13928 + 5.00000ml of P13931 = Final Quantity: 100.000 ml							

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1331	100 PPM NJEPH Fractionating Surrogate	<a href="#">PP24465</a>	04/18/2025	10/03/2025	Abdul Mirza	None	None	Yogesh Patel 05/03/2025
<b><u>FROM</u></b> 1.25000ml of P13762 + 1.25000ml of P13764 + 1.25000ml of P13947 + 1.25000ml of P13948 + 195.00000ml of E3916 = Final Quantity: 200.000 ml								



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
782	100 PPM Aromatic HC Working STD	<a href="#">PP24500</a>	05/01/2025	10/08/2025	Yogesh Patel	None	None	Abdul Mirza
								05/08/2025

**FROM** 0.25000ml of P13673 + 0.62500ml of P13954 + 1.25000ml of P10758 + 22.87500ml of E3926 = Final Quantity: 25.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2945	100 PPM Aromatic HC Working STD (Absolute)	<a href="#">PP24501</a>	05/01/2025	10/08/2025	Yogesh Patel	None	None	Abdul Mirza
								05/08/2025

**FROM** 0.25000ml of P13674 + 0.62500ml of P13955 + 1.25000ml of P11140 + 22.87500ml of E3926 = Final Quantity: 25.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
787	50 PPM Aromatic HC STD	<a href="#">PP24502</a>	05/01/2025	10/08/2025	Yogesh Patel	None	None	Abdul Mirza
								05/08/2025

**FROM** 0.50000ml of E3926 + 0.50000ml of PP24500 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
788	20 PPM Aromatic HC STD	<a href="#">PP24503</a>	05/01/2025	10/08/2025	Yogesh Patel	None	None	Abdul Mirza
								05/08/2025

**FROM** 0.80000ml of E3926 + 0.20000ml of PP24500 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
789	10 PPM Aromatic HC STD	<a href="#">PP24504</a>	05/01/2025	10/08/2025	Yogesh Patel	None	None	Abdul Mirza
								05/08/2025

**FROM** 0.90000ml of E3926 + 0.10000ml of PP24500 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
790	5 PPM Aromatic HC STD	<a href="#">PP24505</a>	05/01/2025	10/08/2025	Yogesh Patel	None	None	Abdul Mirza
								05/08/2025

**FROM** 0.90000ml of E3926 + 0.10000ml of PP24502 = Final Quantity: 1.000 ml



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2946	20 PPM Aromatic HC STD ICV (Absolute)	<a href="#">PP24506</a>	05/01/2025	10/08/2025	Yogesh Patel	None	None	Abdul Mirza 05/08/2025
<u>FROM</u>	0.80000ml of E3926 + 0.20000ml of PP24501 = Final Quantity: 1.000 ml							



## CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-3382-05 / Sand, Purified (cs/4x2.5kg)	0000243821	06/30/2025	04/30/2020 / RAJESH	04/28/2020 / RAJESH	E2865

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	313201	07/01/2025	01/03/2024 / Rajesh	07/20/2023 / Rajesh	E3551

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
phenomenex	SI500025-30 / Cleanert SPE Silica, 5000 mg/25 ml	Z0513CK1	09/04/2025	09/04/2024 / Rajesh	04/03/2024 / Rajesh	E3757

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24K1762005	01/07/2026	03/13/2025 /	12/27/2024 / RUPESH	E3904

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	243570	10/03/2025	04/03/2025 / Rajesh	03/31/2025 / Rajesh	E3916

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H2762008	10/03/2025	04/03/2025 / Rajesh	03/31/2025 / Rajesh	E3917

## CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	25A0262002	10/08/2025	04/08/2025 / Rajesh	02/07/2025 / Rajesh	E3926

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	25C0362005	10/22/2025	04/18/2025 / RUPESH	04/16/2025 / RUPESH	E3928

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H2762008	04/18/2027	04/18/2025 / RUPESH	04/16/2025 / RUPESH	E3929

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	25A0262002	02/20/2026	05/02/2025 / RUPESH	03/09/2025 / RUPESH	E3930

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	25C0362005	11/05/2025	05/05/2025 / RUPESH	04/23/2025 / RUPESH	E3933

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9530-33 / Hydrochloric Acid, Instra-Analyzed (cs/6x2.5L)	0000275677	05/13/2025	11/13/2024 / Eman	10/13/2024 / Eman	M6121

## CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30541 / Custom NJEPH Aromatics Calibration Standard	A0172403	11/01/2025	05/01/2025 / yogesh	06/17/2021 / dhaval	P10758

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	95709 / NJ EPH Aromatic Hydrocarbons, 2000 PPM	060420	11/01/2025	05/01/2025 / yogesh	10/29/2021 / Abdul	P11140

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30540 / Custom NJEPH Aliphatics Calibration Standard	A0190424	08/03/2025	02/03/2025 / yogesh	03/16/2023 / Yogesh	P12363

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0204989	08/03/2025	02/03/2025 / yogesh	12/20/2023 / Yogesh	P12981

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0204989	08/03/2025	02/03/2025 / yogesh	12/20/2023 / Yogesh	P12983

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0204989	10/25/2025	04/25/2025 / Abdul	12/20/2023 / Yogesh	P12989

## CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0204989	10/25/2025	04/25/2025 / Abdul	12/20/2023 / Yogesh	P12990

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0200707	10/25/2025	04/25/2025 / Abdul	12/26/2023 / Yogesh	P13050

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	95899 / NJ EPH Aliphatic n-Hydrocarbons-Revised, 1000 PPM	040524	08/03/2025	02/03/2025 / yogesh	04/11/2024 / yogesh	P13279

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0213283	10/25/2025	04/25/2025 / Abdul	10/16/2024 / yogesh	P13596

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0216631	08/03/2025	02/03/2025 / yogesh	10/16/2024 / yogesh	P13650

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0216631	10/25/2025	04/25/2025 / Abdul	10/16/2024 / yogesh	P13660

## CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0216631	10/25/2025	04/25/2025 / Abdul	10/16/2024 / yogesh	P13662

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0216631	10/25/2025	04/25/2025 / Abdul	10/16/2024 / yogesh	P13664

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0216631	10/25/2025	04/25/2025 / Abdul	10/16/2024 / yogesh	P13667

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0216631	08/03/2025	02/03/2025 / yogesh	10/16/2024 / yogesh	P13671

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0216631	11/01/2025	05/01/2025 / yogesh	10/16/2024 / yogesh	P13673

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0216631	11/01/2025	05/01/2025 / yogesh	10/16/2024 / yogesh	P13674

## CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0211254	10/15/2025	04/15/2025 / yogesh	10/24/2024 / yogesh	P13709

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0214879	10/18/2025	04/18/2025 / Abdul	11/01/2024 / yogesh	P13762

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0214879	10/18/2025	04/18/2025 / Abdul	11/01/2024 / yogesh	P13764

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0220580	10/15/2025	04/15/2025 / yogesh	01/08/2025 / yogesh	P13865

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0217408	10/15/2025	04/15/2025 / yogesh	03/06/2025 / yogesh	P13896

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0217408	10/15/2025	04/15/2025 / yogesh	03/06/2025 / yogesh	P13897

## CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0217408	10/15/2025	04/15/2025 / yogesh	03/06/2025 / yogesh	P13898

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0217408	10/15/2025	04/15/2025 / yogesh	03/06/2025 / yogesh	P13899

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0217408	10/15/2025	04/15/2025 / yogesh	03/06/2025 / yogesh	P13900

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0217408	10/15/2025	04/15/2025 / yogesh	03/06/2025 / yogesh	P13901

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0217408	10/15/2025	04/15/2025 / yogesh	03/06/2025 / yogesh	P13903

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0217408	10/15/2025	04/15/2025 / yogesh	03/06/2025 / yogesh	P13905

## CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0217408	10/15/2025	04/15/2025 / yogesh	03/06/2025 / yogesh	P13906

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0220449	10/15/2025	04/15/2025 / yogesh	03/06/2025 / yogesh	P13912

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A022580	10/15/2025	04/15/2025 / yogesh	03/06/2025 / yogesh	P13919

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A022580	10/15/2025	04/15/2025 / yogesh	03/06/2025 / yogesh	P13920

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A022580	10/15/2025	04/15/2025 / yogesh	03/06/2025 / yogesh	P13921

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A022580	10/15/2025	04/15/2025 / yogesh	03/06/2025 / yogesh	P13923



## CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A022580	10/15/2025	04/15/2025 / yogesh	03/06/2025 / yogesh	P13926

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A022580	10/15/2025	04/15/2025 / yogesh	03/06/2025 / yogesh	P13927

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A022580	10/15/2025	04/15/2025 / yogesh	03/06/2025 / yogesh	P13928

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A022580	10/15/2025	04/15/2025 / yogesh	03/06/2025 / yogesh	P13931

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0219106	10/31/2030	04/18/2025 / Abdul	03/10/2025 / yogesh	P13947

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0219106	10/18/2025	04/18/2025 / Abdul	03/10/2025 / yogesh	P13948

## CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0219106	11/01/2025	05/01/2025 / Abdul	03/10/2025 / yogesh	P13950

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0219106	11/01/2025	05/01/2025 / Abdul	03/10/2025 / yogesh	P13951

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0219106	11/01/2025	05/01/2025 / Abdul	03/10/2025 / yogesh	P13952

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0219106	11/01/2025	05/01/2025 / Abdul	03/10/2025 / yogesh	P13953

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0219106	11/01/2025	05/01/2025 / yogesh	03/10/2025 / yogesh	P13954

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0221895	11/01/2025	05/01/2025 / yogesh	03/10/2025 / yogesh	P13955

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / lwona	07/03/2024 / lwona	W3112

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24G1962003	08/22/2025	02/03/2025 / jignesh	01/31/2025 / jignesh	W3177




110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

# CERTIFIED REFERENCE MATERIAL

## Certificate of Analysis



**FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.**

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

DD  
06/17/2021

**Catalog No. :** 30541 **Lot No.:** A0172403

**Description :** NJEPH Aromatics Calibration Standard

NJEPH Aromatics Calibration Standard 2,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** April 30, 2027 **Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

P10758  
TO  
P10762  
(S)

### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene CAS # 526-73-8 (Lot 8776.10-36) Purity 98%	2,010.0 µg/mL	+/- 11.7957 µg/mL Gravimetric +/- 90.5449 µg/mL Unstressed +/- 100.4678 µg/mL Stressed
2	Naphthalene CAS # 91-20-3 (Lot MKBZ8680V) Purity 99%	2,006.0 µg/mL	+/- 11.7723 µg/mL Gravimetric +/- 90.3656 µg/mL Unstressed +/- 100.2689 µg/mL Stressed
3	2-Methylnaphthalene CAS # 91-57-6 (Lot STBG8884) Purity 99%	2,008.0 µg/mL	+/- 11.7841 µg/mL Gravimetric +/- 90.4557 µg/mL Unstressed +/- 100.3688 µg/mL Stressed
4	Acenaphthylene CAS # 208-96-8 (Lot N19U) Purity 95%	2,002.6 µg/mL	+/- 11.7524 µg/mL Gravimetric +/- 90.2125 µg/mL Unstressed +/- 100.0989 µg/mL Stressed
5	Acenaphthene CAS # 83-32-9 (Lot MKCN0610) Purity 99%	2,000.0 µg/mL	+/- 11.7371 µg/mL Gravimetric +/- 90.0953 µg/mL Unstressed +/- 99.9689 µg/mL Stressed
6	Fluorene CAS # 86-73-7 (Lot 10217947) Purity 99%	2,016.0 µg/mL	+/- 11.8310 µg/mL Gravimetric +/- 90.8161 µg/mL Unstressed +/- 100.7687 µg/mL Stressed
7	Phenanthrene CAS # 85-01-8 (Lot MKCL7390) Purity 99%	2,012.0 µg/mL	+/- 11.8075 µg/mL Gravimetric +/- 90.6359 µg/mL Unstressed +/- 100.5688 µg/mL Stressed

8	Anthracene <b>CAS #</b> 120-12-7 <b>Purity</b> 99%	(Lot MKCM0015)	2,002.0 µg/mL	+/-	11.7489	µg/mL	Gravimetric
				+/-	90.1854	µg/mL	Unstressed
				+/-	100.0689	µg/mL	Stressed
9	Fluoranthene <b>CAS #</b> 206-44-0 <b>Purity</b> 99%	(Lot MKCF7378)	2,003.0 µg/mL	+/-	11.7547	µg/mL	Gravimetric
				+/-	90.2305	µg/mL	Unstressed
				+/-	100.1189	µg/mL	Stressed
10	Pyrene <b>CAS #</b> 129-00-0 <b>Purity</b> 99%	(Lot BCCB9880)	2,011.0 µg/mL	+/-	11.8017	µg/mL	Gravimetric
				+/-	90.5909	µg/mL	Unstressed
				+/-	100.5188	µg/mL	Stressed
11	Benz(a)anthracene <b>CAS #</b> 56-55-3 <b>Purity</b> 98%	(Lot P0022018-0505)	2,011.0 µg/mL	+/-	11.8014	µg/mL	Gravimetric
				+/-	90.5890	µg/mL	Unstressed
				+/-	100.5168	µg/mL	Stressed
12	Chrysene <b>CAS #</b> 218-01-9 <b>Purity</b> 99%	(Lot STBJ8094)	2,000.0 µg/mL	+/-	11.7371	µg/mL	Gravimetric
				+/-	90.0953	µg/mL	Unstressed
				+/-	99.9689	µg/mL	Stressed
13	Benzo(b)fluoranthene <b>CAS #</b> 205-99-2 <b>Purity</b> 97%	(Lot 012012B)	2,006.0 µg/mL	+/-	11.7721	µg/mL	Gravimetric
				+/-	90.3638	µg/mL	Unstressed
				+/-	100.2669	µg/mL	Stressed
14	Benzo(k)fluoranthene <b>CAS #</b> 207-08-9 <b>Purity</b> 99%	(Lot 012019K)	2,010.0 µg/mL	+/-	11.7958	µg/mL	Gravimetric
				+/-	90.5458	µg/mL	Unstressed
				+/-	100.4688	µg/mL	Stressed
15	Benzo(a)pyrene <b>CAS #</b> 50-32-8 <b>Purity</b> 99%	(Lot RP210113)	2,004.0 µg/mL	+/-	11.7606	µg/mL	Gravimetric
				+/-	90.2755	µg/mL	Unstressed
				+/-	100.1689	µg/mL	Stressed
16	Indeno(1,2,3-cd)pyrene <b>CAS #</b> 193-39-5 <b>Purity</b> 99%	(Lot 1-RAK-33-4)	2,010.0 µg/mL	+/-	11.7958	µg/mL	Gravimetric
				+/-	90.5458	µg/mL	Unstressed
				+/-	100.4688	µg/mL	Stressed
17	Dibenz(a,h)anthracene <b>CAS #</b> 53-70-3 <b>Purity</b> 99%	(Lot ER032211-01)	2,017.0 µg/mL	+/-	11.8369	µg/mL	Gravimetric
				+/-	90.8611	µg/mL	Unstressed
				+/-	100.8187	µg/mL	Stressed
18	Benzo(g,h,i)perylene <b>CAS #</b> 191-24-2 <b>Purity</b> 99%	(Lot 8GFYJ)	2,003.0 µg/mL	+/-	11.7547	µg/mL	Gravimetric
				+/-	90.2305	µg/mL	Unstressed
				+/-	100.1189	µg/mL	Stressed
<b>Solvent:</b>	Methylene chloride <b>CAS #</b> 75-09-2 <b>Purity</b> 99%						

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)


**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

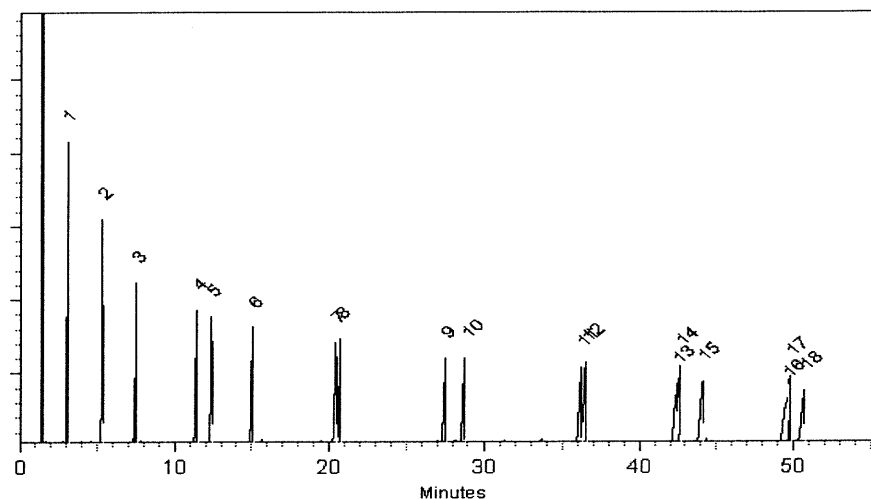

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Lane Kibe - Mix Technician

Date Mixed: 14-May-2021      Balance: B345965662

  
Alexis Shelow - Operations Tech I

Date Passed: 18-May-2021

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.

Sand  
Purified  
Washed and Ignited



Material No.: 3382-05  
Batch No.: 0000243821  
Manufactured Date: 2018/04/09  
Retest Date: 2025/04/07  
Revision No: 1

## Certificate of Analysis

Test	Specification	Result
Substances Soluble in HCl	$\leq 0.16\%$	0.01

For Laboratory, Research or Manufacturing Use  
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US  
Packaging Site: Paris Mfg Ctr & DC

E 2865

  
Jamie Ethier  
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC  
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700





**PRODUCTOS  
QUÍMICOS  
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR  
MONTERREY, N.L. MEXICO  
CP 64070  
TEL +52 81 13 52 57 57  
www.pqm.com.mx

## CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na <sub>2</sub> SO <sub>4</sub>
SPECIFICATION NUMBER :	6399	RELEASE DATE:	ABR/21/2023
LOT NUMBER :	313201		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na <sub>2</sub> SO <sub>4</sub> )	Min. 99.0%	99.7 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.1
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO <sub>4</sub> )	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.003 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.1 %
Retained on US Standard No. 60 sieve	Min. 94%	97.3 %
Through US Standard No. 60 sieve	Max. 5%	2.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

### COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/24/23 E 3551

RC-02-01, Ed. 3

**Cleanert EPH**

5g/25ml 15/pkg

固相萃取产品

LOT#:Z0513CK1



MFG#:F04005



Made in China



**CAT# SI500025-30**

Agela Technologies

E 3757



## Certificate of Analysis

1 Reagent Lane  
 Fair Lawn, NJ 07410  
 201.796.7100 tel  
 201.796.1329 fax

Thermo Fisher Scientific's Quality System has been found to conform to Quality Management System  
 Standard ISO9001:2015 by SAI Global Certificate Number CERT - 0120633

This is to certify that units of the lot number below were tested and found to comply with the specifications of the grade listed. Certain data have been supplied by third parties. Thermo Fisher Scientific expressly disclaims all warranties, expressed or implied, including the implied warranties of merchantability and fitness for a particular purpose. Products are for research use or further manufacturing. Not for direct administration to humans or animals. It is the responsibility of the final formulator and end user to determine suitability based upon the intended use of the end product. Products are tested to meet the analytical requirements of the noted grade. The following information is the actual analytical results obtained.

Catalog Number	H303	Quality Test / Release Date	11/07/2024
Lot Number	243570		
Description	HEXANES - OPTIMA		
Country of Origin	United States	Suggested Retest Date	Nov/2029
Chemical Origin	Organic - non animal		
BSE/TSE Comment	No animal products are used as starting raw material ingredients, or used in processing, including lubricants, processing aids, or any other material that might migrate to the finished product.		

N/A

Result Name	Units	Specifications	Test Value
APPEARANCE		REPORT	Clear, colorless liquid
ASSAY (N-HEXANE)	%	>= 60	69
ASSAY (SUM C6 HYDROCARBONS)	%	>= 99.9	>99.9
COLOR	APHA	<= 5	<5
DENSITY AT 25 DEGREES C	GM/ML	Inclusive Between 0.653 - 0.673	0.669
EVAPORATION RESIDUE	ppm	<= 1	<1
FLUORESCENCE BACKGROUND	ppb	<= 1	<1
IDENTIFICATION	PASS/FAIL	= PASS TEST	PASS TEST
OPTICAL ABS AT 195 NM	ABS. UNITS	<= 1	0.74
OPTICAL ABS AT 210 NM	ABS. UNITS	<= 0.25	0.17
OPTICAL ABS AT 220 NM	ABS. UNITS	<= 0.07	0.05
OPTICAL ABS AT 254 NM	ABS. UNITS	<= 0.005	0.001
PESTICIDE RESIDUE ANALYSIS	NG/L	<= 10	<10
REFRACTIVE INDEX @ 25 DEG C		Inclusive Between 1.375 - 1.385	1.379
SUITABILITY FOR GC/MS		= PASS TEST	PASS TEST
SULFUR COMPOUNDS	%	<= 0.005	<0.005
THIOPHENE	PASS/FAIL	= PASS TEST	PASS TEST
WATER (H2O)	%	<= 0.01	<0.01
WATER-SOLUBLE TITRABLE ACID	MEQ/G	<= 0.0003	0.0001

*Harout Sahagian*

Harout Sahagian - Quality Control Manager - Fair Lawn

Recd by RP on 3/31/25

E 3946

Note: The data listed is valid for all package sizes of this lot of this product, expressed as an extension of this catalog number listed above.  
 If there are any questions with this certificate, please call at (800) 227-6701.  
 \*Based on suggested storage condition.

Acetone

BAKER RESI-ANALYZED® Reagent  
For Organic Residue Analysis

avantor™



Material No.: 9254-03

Batch No.: 24H2762008

Manufactured Date: 2024-04-18

Expiration Date: 2027-04-18

Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
Assay ((CH <sub>3</sub> ) <sub>2</sub> CO) (by GC, corrected for water)	>= 99.4 %	100.0 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.0 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (μeq/g)	<= 0.3	0.2
Titration Base (μeq/g)	<= 0.6	<0.1
Water (H <sub>2</sub> O)	<= 0.5 %	<0.1 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

Recd by RP on 03/31/25

E3917

Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)

avantor



Material No.: 9266-A4  
Batch No.: 25A0262002  
Manufactured Date: 2024-11-21  
Expiration Date: 2026-02-20  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	$\leq 10$	4
Assay ( $\text{CH}_2\text{Cl}_2$ ) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8\%$	99.9%
Color (APHA)	$\leq 10$	10
Residue after Evaporation	$\leq 1.0$ ppm	0.8 ppm
Titration Acid ( $\mu\text{eq/g}$ )	$\leq 0.3$	$< 0.1$
Chloride (Cl)	$\leq 10$ ppm	$< 5$ ppm
Water (by KF, coulometric)	$\leq 0.02\%$	$< 0.01\%$

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States  
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3926

*J. Croak*

Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA, 19087, U.S.A. Phone 610.386.1700

n-Hexane 95%  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis

 **avantors<sup>™</sup>**



Material No.: 9262-03

Batch No.: 25C0362005

Manufactured Date: 2025-01-29

Expiration Date: 2026-04-30

Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	$\leq 10$	6
ECD-Sensitive Impurities (as EthyleneDibromide) - Single Impurity Peak (ng/mL)	$\leq 5$	5
Assay (Total Saturated C <sub>6</sub> Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	100.0 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	100 %
Color (APHA)	$\leq 10$	10
Residue after Evaporation	$\leq 1.0$ ppm	0.1 ppm
Substances Darkened by H <sub>2</sub> SO <sub>4</sub>	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	$< 0.01 \%$

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States  
Packaging Site: Phillipsburg Mfg Ctr & DC

E3928



Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials U.S.

Acetone

BAKER RESI-ANALYZED® Reagent

For Organic Residue Analysis

avantor™



Material No.: 9254-03

Batch No.: 24H2762008

Manufactured Date: 2024-04-18

Expiration Date: 2027-04-18

Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
Assay ((CH <sub>3</sub> ) <sub>2</sub> CO) (by GC, corrected for water)	>= 99.4 %	100.0 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.0 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (µeq/g)	<= 0.3	0.2
Titration Base (µeq/g)	<= 0.6	<0.1
Water (H <sub>2</sub> O)	<= 0.5 %	<0.1 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

E 3929

Jamie Croak

Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4  
Batch No.: 25A0262002  
Manufactured Date: 2024-11-21  
Expiration Date: 2026-02-20  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	$\leq 10$	4
Assay (CH <sub>2</sub> Cl <sub>2</sub> ) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	99.9 %
Color (APHA)	$\leq 10$	10
Residue after Evaporation	$\leq 1.0$ ppm	0.8 ppm
Titration Acid ( $\mu$ eq/g)	$\leq 0.3$	<0.1
Chloride (Cl)	$\leq 10$ ppm	<5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	<0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States  
Packaging Site: Phillipsburg Mfg Ctr & DC

E3930

Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA, 19087, U.S.A. Phone 610.386.1700



n-Hexane 95%  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis

 **avantors**<sup>TM</sup>



Material No.: 9262-03

Batch No.: 25C0362005

Manufactured Date: 2025-01-29

Expiration Date: 2026-04-30

Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	$\leq 10$	6
ECD-Sensitive Impurities (as EthyleneDibromide) - Single Impurity Peak (ng/mL)	$\leq 5$	5
Assay (Total Saturated C <sub>6</sub> Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	100.0 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	100 %
Color (APHA)	$\leq 10$	10
Residue after Evaporation	$\leq 1.0$ ppm	0.1 ppm
Substances Darkened by H <sub>2</sub> SO <sub>4</sub>	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	$< 0.01 \%$

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

E3933



Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

Hydrochloric Acid, 36.5-38.0%  
BAKER INSTRA-ANALYZED® Reagent  
For Trace Metal Analysis



R → 16/13/24  
Met dig

M 6121

Material No.: 9530-33  
Batch No.: 0000275677  
Manufactured Date: 2020/12/16  
Retest Date: 2025/12/15  
Revision No: 1

## Certificate of Analysis

Test	Specification	Result
ACS - Assay (as HCl) (by acid-base titrn)	36.5 - 38.0 %	37.6
ACS - Color (APHA)	<= 10	5
ACS - Residue after Ignition	<= 3 ppm	1
ACS - Specific Gravity at 60°/60°F	1.185 - 1.192	1.190
ACS - Bromide (Br)	<= 0.005 %	< 0.005
ACS - Extractable Organic Substances	<= 5 ppm	1
ACS - Free Chlorine (as Cl <sub>2</sub> )	<= 0.5 ppm	< 0.5
Phosphate (PO <sub>4</sub> )	<= 0.05 ppm	< 0.03
Sulfate (SO <sub>4</sub> )	<= 0.5 ppm	< 0.3
Sulfite (SO <sub>3</sub> )	<= 0.8 ppm	0.3
Ammonium (NH <sub>4</sub> )	<= 3 ppm	< 1
Trace Impurities - Arsenic (As)	<= 0.010 ppm	< 0.003
Trace Impurities - Aluminum (Al)	<= 10.0 ppb	< 0.2
Arsenic and Antimony (as As)	<= 5 ppb	< 3
Trace Impurities - Barium (Ba)	<= 1.0 ppb	< 0.2
Trace Impurities - Beryllium (Be)	<= 1.0 ppb	< 0.2
Trace Impurities - Bismuth (Bi)	<= 10.0 ppb	< 1.0
Trace Impurities - Boron (B)	<= 20.0 ppb	< 5.0
Trace Impurities - Cadmium (Cd)	<= 1.0 ppb	< 0.3
Trace Impurities - Calcium (Ca)	<= 50.0 ppb	29.7
Trace Impurities - Chromium (Cr)	<= 1.0 ppb	< 0.4
Trace Impurities - Cobalt (Co)	<= 1.0 ppb	< 0.3
Trace Impurities - Copper (Cu)	<= 1.0 ppb	< 0.1
Trace Impurities - Gallium (Ga)	<= 1.0 ppb	< 0.2

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Material No.: 9530-33  
Batch No.: 0000275677

Test	Specification	Result
Trace Impurities – Germanium (Ge)	<= 3.0 ppb	< 2.0
Trace Impurities – Gold (Au)	<= 4.0 ppb	< 0.2
Heavy Metals (as Pb)	<= 100 ppb	< 50
Trace Impurities – Iron (Fe)	<= 15.0 ppb	< 1
Trace Impurities – Lead (Pb)	<= 1.0 ppb	< 0.5
Trace Impurities – Lithium (Li)	<= 1.0 ppb	0.2
Trace Impurities – Magnesium (Mg)	<= 10.0 ppb	0.4
Trace Impurities – Manganese (Mn)	<= 1.0 ppb	< 0.4
Trace Impurities – Mercury (Hg)	<= 0.5 ppb	0.1
Trace Impurities – Molybdenum (Mo)	<= 10.0 ppb	< 5.0
Trace Impurities – Nickel (Ni)	<= 4.0 ppb	< 0.3
Trace Impurities – Niobium (Nb)	<= 1.0 ppb	< 0.2
Trace Impurities – Potassium (K)	<= 9.0 ppb	< 2.0
Trace Impurities – Selenium (Se), For Information Only	ppb	1.0
Trace Impurities – Silicon (Si)	<= 100.0 ppb	< 10.0
Trace Impurities – Silver (Ag)	<= 1.0 ppb	< 0.3
Trace Impurities – Sodium (Na)	<= 100.0 ppb	< 5.0
Trace Impurities – Strontium (Sr)	<= 1.0 ppb	< 0.2
Trace Impurities – Tantalum (Ta)	<= 1.0 ppb	< 0.9
Trace Impurities – Thallium (Tl)	<= 5.0 ppb	< 2.0
Trace Impurities – Tin (Sn)	<= 5.0 ppb	< 0.8
Trace Impurities – Titanium (Ti)	<= 1.0 ppb	0.2
Trace Impurities – Vanadium (V)	<= 1.0 ppb	< 0.2
Trace Impurities – Zinc (Zn)	<= 5.0 ppb	0.3
Trace Impurities – Zirconium (Zr)	<= 1.0 ppb	< 0.1

For Laboratory, Research or Manufacturing Use


Product Information (not specifications):

Appearance (clear, fuming liquid)

Meets ACS Specifications

Country of Origin: US

Packaging Site: Phillipsburg Mfg Ctr & DC

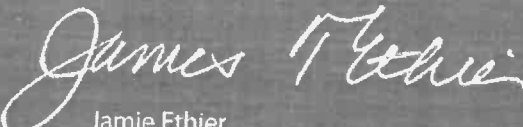  
Jamie Ethier  
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700



**CERTIFIED WEIGHT REPORT**

**Part Number:** 95709  
**Lot Number:** 060420  
**Description:** NJ EPH Aromatic Hydrocarbons  
18 components  
**Expiration Date:** 060425  
**Recommended Storage:** Refrigerate (4 °C)  
**Nominal Concentration (µg/mL):** 2000  
**NIST Test ID#:** 23060  
**Weight(s) shown below were combined and diluted to (mL):** 500.0  
**Balance Uncertainty:** 5E-05  
**Flask Uncertainty:** 0.058

**Solvent(s):** Methylene chloride  
**Lot#** 104923

Formulated By:	Benson Chan	060420
Reviewed By:	Pedro L. Renteria	060420
		DATE

Compound	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	CAS#	SDS Information (Solvent Safety Info. On Attached pg.)	LD50
----------	------------	----------------------	------------	--------------------	------------------	------------------	---------------------	----------------------------------	------	--	------


1. Acenaphthene	1	MKB14871V	2000	99	0.2	1.01003	1.01010	2000.1	8.1	83-32-9	N/A	ip-tral 600mg/kg
2. Acenaphthylene	3	012014	2000	98	0.2	1.02033	1.02053	2000.4	8.2	208-96-6	N/A	N/A
3. Anthracene	13	A0210580	2000	99	0.2	1.01003	1.01009	2000.1	8.1	120-12-7	0.2mg/m3 (8h)	ip-trus 430mg/kg
4. Benz(a)anthracene	28	JY2TD-JT	2000	98	0.2	1.02033	1.02051	2000.3	8.2	56-55-3	N/A	N/A
5. Benz(a)pyrene	30	012012	2000	99.5	0.2	1.00495	1.00511	2000.3	8.1	50-32-8	0.2mg/m3 (8h)	scu-tral 50mg/kg
6. Benz(b)fluoranthene	31	012012b	2000	99	0.2	1.01003	1.01012	2000.2	8.1	205-99-2	N/A	N/A
7. Benz(k)fluoranthene	33	012012k	2000	99	0.2	1.01003	1.01018	2000.3	8.1	207-08-9	N/A	N/A
8. Benz(g,h,i)perylene	32	012018	2000	99	0.2	1.01003	1.01019	2000.3	8.1	191-24-2	N/A	N/A
9. Chrysene	91	012015	2000	98	0.2	1.02033	1.02040	2000.1	8.2	218-01-9	0.2mg/m3	N/A
10. Dibenzo(a,h)anthracene	112	012011	2000	98	0.2	1.02033	1.02050	2000.3	8.2	53-70-3	0.2mg/m3	N/A
11. Fluoranthene	183	04221PV	2000	98	0.2	1.02033	1.02050	2000.3	8.2	206-44-0	N/A	of-tral 2000mg/kg
12. Fluorene	184	07211MV	2000	98	0.2	1.02033	1.02047	2000.3	8.2	86-73-7	N/A	ip-trus 2 g/kg
13. Indeno(1,2,3-cd)pyrene	202	012014	2000	99.9	0.2	1.00093	1.00119	2000.5	8.0	193-39-5	N/A	N/A
14. 2-Methylnaphthalene	214	MKB13783V	2000	97	0.2	1.03085	1.03090	2000.1	8.3	91-57-6	N/A	of-tral 1630mg/kg
15. Naphthalene	222	MKB28690V	2000	100	0.2	0.99993	0.99999	2000.1	8.0	91-20-3	10 ppm (50mg/m3/8h)	of-tral 490mg/kg
16. Phenanthrene	248	03410PV	2000	99	0.2	1.01003	1.01030	2000.5	8.1	85-01-8	0.2mg/m3/8h	of-trus 700mg/kg
17. Pyrene	259	010197	2000	98	0.2	1.02033	1.02042	2000.2	8.2	129-00-0	0.2mg/m3/8h	of-tral 2700mg/kg
18. 1,2,3-trimethylbenzene	944	031097	2000	99	0.2	1.01003	1.01025	2000.4	8.1	526-73-8	N/A	N/A

\* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.  
\* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).  
\* Standards are certified (±) 0.5% of the stated value, unless otherwise stated.  
\* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.  
\* Uncertainty Reference: Taylor, B.N. and Kuyat, C.F., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

P11137  
P11141  
11/10/21



**Method GC8MSD-2.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (14min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Melissa Stonier.**

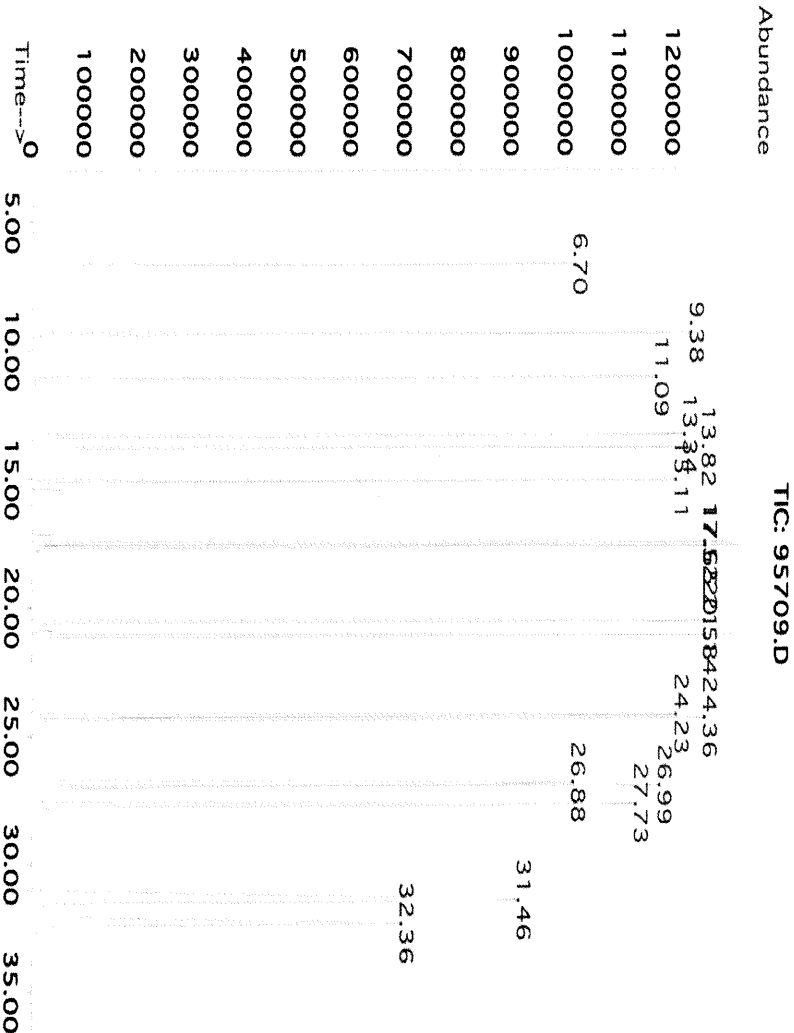

Peak No.	Name	MSD RT (min.)
1	1,2,3-Trimethylbenzene	6.70
2	Naphthalene	9.38
3	2-Methylnaphthalene	11.09
4	Acenaphthylene	13.34
5	Acenaphthene	13.82
6	Fluorene	15.11
7	Phenanthrene	17.52
8	Anthracene	17.65
9	Fluoranthene	20.58
10	Pyrene	21.14
11	Chrysene	24.23
12	Benzo(a)anthracene	24.36
13	Benzo(b)fluoranthene/Benzo(k)fluoranthene	26.98
14	Benzo(a)pyrene	27.73
15	Indeno(1,2,3-cd)pyrene/Dibenzo(a,h)anthracene	31.46
16	Benzo(g,h,i)perylene	32.36



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

# CERTIFIED REFERENCE MATERIAL

## Certificate of Analysis



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30540 **Lot No.:** A0190424

**Description :** NJEPH Aliphatics Calibration Standard

Aliphatics Calibration Standard 2000µg/mL, Hexane/Carbon Disulfide (80:20), 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** November 30, 2029 **Storage:** 25°C nominal

**Handling:** Sonicate prior to use. **Ship:** Ambient

P12361  
↓  
P12370 } Y.P.  
031/6/23

### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)	
1	n-Nonane (C9) CAS # 111-84-2 Purity 99% (Lot SHBN5361)	2,014.0 µg/mL	+/- 11.8193 +/- 50.0027 +/- 59.9491	µg/mL Gravimetric Unstressed Stressed
2	n-Decane (C10) CAS # 124-18-5 Purity 99% (Lot SHBN8619)	2,014.7 µg/mL	+/- 11.8232 +/- 50.0193 +/- 59.9689	µg/mL Gravimetric Unstressed Stressed
3	Naphthalene CAS # 91-20-3 Purity 99% (Lot MKCH0219)	2,015.3 µg/mL	+/- 11.8271 +/- 50.0358 +/- 59.9888	µg/mL Gravimetric Unstressed Stressed
4	n-Dodecane (C12) CAS # 112-40-3 Purity 99% (Lot SHBN7174)	2,008.0 µg/mL	+/- 11.7841 +/- 49.8538 +/- 59.7705	µg/mL Gravimetric Unstressed Stressed
5	2-Methylnaphthalene CAS # 91-57-6 Purity 96% (Lot STBK0259)	2,007.0 µg/mL	+/- 11.7784 +/- 49.8299 +/- 59.7419	µg/mL Gravimetric Unstressed Stressed
6	n-Tetradecane (C14) CAS # 629-59-4 Purity 99% (Lot STBK2282)	2,016.7 µg/mL	+/- 11.8349 +/- 50.0689 +/- 60.0284	µg/mL Gravimetric Unstressed Stressed
7	n-Hexadecane (C16) CAS # 544-76-3 Purity 98% (Lot SHBM4146)	2,014.9 µg/mL	+/- 11.8244 +/- 50.0246 +/- 59.9753	µg/mL Gravimetric Unstressed Stressed

8	n-Octadecane (C18) CAS # 593-45-3 Purity 97%	(Lot VZKOJ)	2,004.7 µg/mL	+/- 11.7645 +/- 49.7710 +/- 59.6712	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
9	n-Eicosane (C20) CAS # 112-95-8 Purity 99%	(Lot MKCF7888)	2,018.0 µg/mL	+/- 11.8428 +/- 50.1020 +/- 60.0681	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
10	n-Heneicosane (C21) CAS # 629-94-7 Purity 99%	(Lot MKCL3226)	2,000.7 µg/mL	+/- 11.7410 +/- 49.6717 +/- 59.5522	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
11	n-Docosane (C22) CAS # 629-97-0 Purity 99%	(Lot MKCL8918)	2,005.3 µg/mL	+/- 11.7684 +/- 49.7876 +/- 59.6911	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
12	n-Tetracosane (C24) CAS # 646-31-1 Purity 99%	(Lot MKCN2863)	2,018.0 µg/mL	+/- 11.8428 +/- 50.1020 +/- 60.0681	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
13	n-Hexacosane (C26) CAS # 630-01-3 Purity 99%	(Lot MKCD4540)	2,014.0 µg/mL	+/- 11.8193 +/- 50.0027 +/- 59.9491	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
14	n-Octacosane (C28) CAS # 630-02-4 Purity 99%	(Lot BCCG0084)	2,002.0 µg/mL	+/- 11.7489 +/- 49.7048 +/- 59.5919	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
15	n-Triacontane (C30) CAS # 638-68-6 Purity 97%	(Lot MKCQ9436)	2,011.1 µg/mL	+/- 11.8025 +/- 49.9316 +/- 59.8637	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
16	n-Dotriacontane (C32) CAS # 544-85-4 Purity 99%	(Lot BCBW0661)	2,012.0 µg/mL	+/- 11.8075 +/- 49.9531 +/- 59.8895	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
17	n-Tetratriacontane (C34) CAS # 14167-59-0 Purity 99%	(Lot OML4N)	2,006.7 µg/mL	+/- 11.7762 +/- 49.8207 +/- 59.7308	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
18	n-Hexatriacontane (C36) CAS # 630-06-8 Purity 99%	(Lot Z27H018)	2,017.3 µg/mL	+/- 11.8388 +/- 50.0855 +/- 60.0483	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
19	n-Octatriacontane (C38) CAS # 7194-85-6 Purity 96%	(Lot 0000145137)	2,017.3 µg/mL	+/- 11.8385 +/- 50.0842 +/- 60.0467	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
20	n-Tetracontane (C40) CAS # 4181-95-7 Purity 99%	(Lot BSBME)	2,008.7 µg/mL	+/- 11.7880 +/- 49.8703 +/- 59.7903	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
Solvent: Hexane/Carbon disulfide (80:20) CAS # 110-54-3/75-15-0 Purity 99%						

**Column:**  
30m x 0.25mm x 0.25µm  
Pxx-5 (cat.#10223)


**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

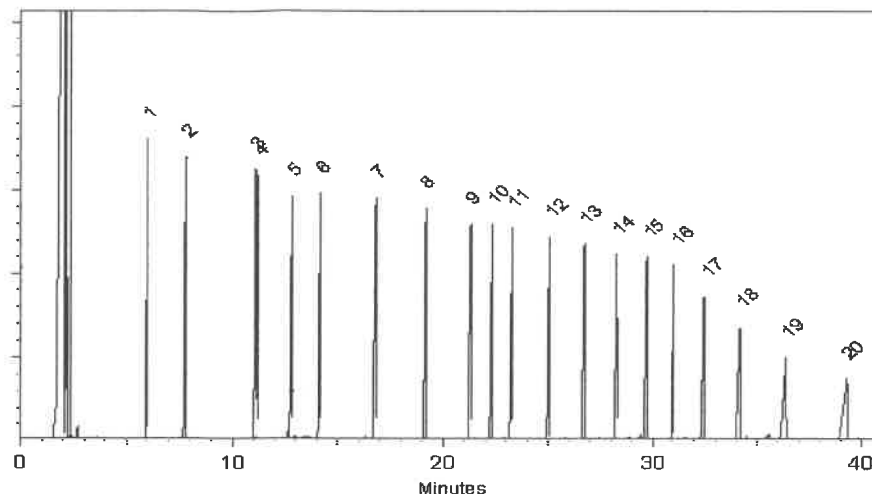

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Morgan Craighead - Mix Technician

Date Mixed: 10-Oct-2022      Balance: 1128360905

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 20-Oct-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No.:** 31098 **Lot No.:** A0204989  
**Description:** 1-Chlorooctadecane Standard  
1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul  
**Container Size:** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date:** January 31, 2031 **Storage:** 10°C or colder  
**Ship:** Ambient

P12960  
↓  
P12991 } Y.P.  
12/21/2023

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Chlorooctadecane	3386-33-2	14738400	99%	10,097.3 µg/mL	+/- 567.2675

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

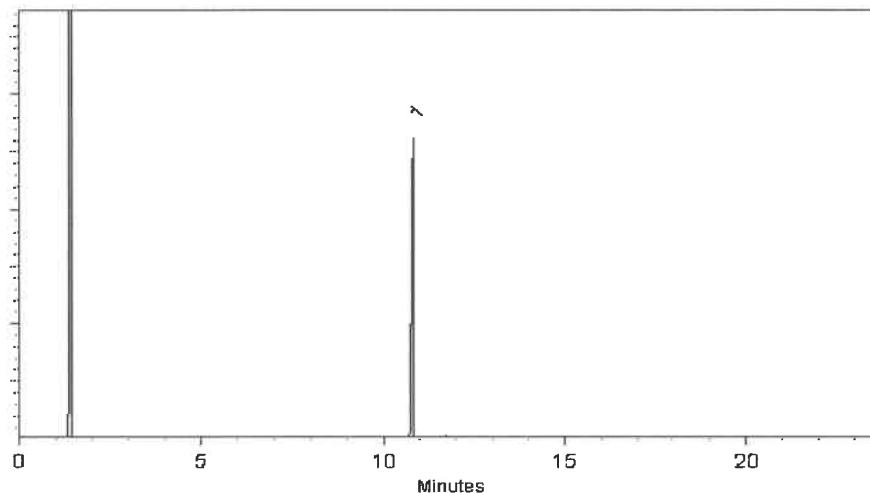

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Peter Robbins - Operations Technician I

Date Mixed: 02-Dec-2023

Balance Serial # B345965662

Christie Mills - Operations Lead Tech - ARM QC

Date Passed: 08-Dec-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No.:** 31098 **Lot No.:** A0204989

**Description:** 1-Chlorooctadecane Standard

1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size:** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date:** January 31, 2031 **Storage:** 10°C or colder

**Ship:** Ambient

P12960  
↓  
P12991 } Y.P.  
12/21/2023

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Chlorooctadecane	3386-33-2	14738400	99%	10,097.3 µg/mL	+/- 567.2675

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

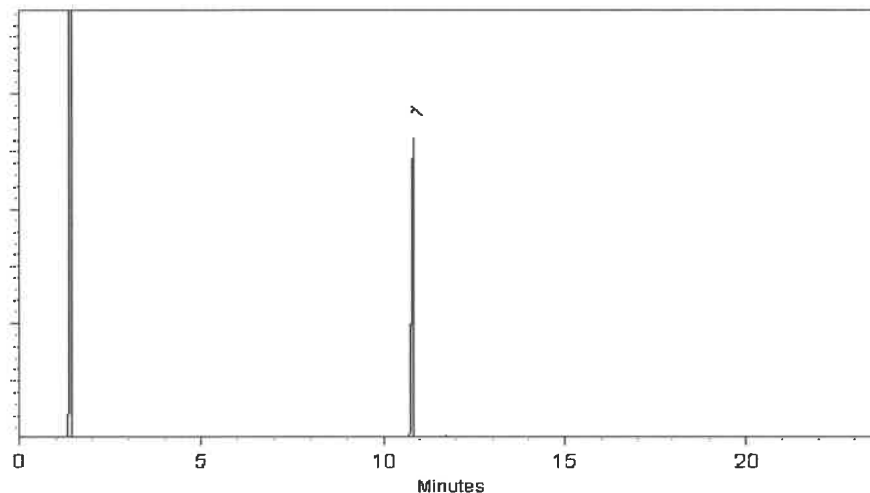

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Peter Robbins - Operations Technician I

Date Mixed: 02-Dec-2023

Balance Serial # B345965662

Christie Mills - Operations Lead Tech - ARM QC

Date Passed: 08-Dec-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No.:** 31098 **Lot No.:** A0204989

**Description:** 1-Chlorooctadecane Standard

1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size:** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date:** January 31, 2031 **Storage:** 10°C or colder

**Ship:** Ambient

P12960  
↓  
P12991 } Y.P.  
12/21/2023

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Chlorooctadecane	3386-33-2	14738400	99%	10,097.3 µg/mL	+/- 567.2675

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

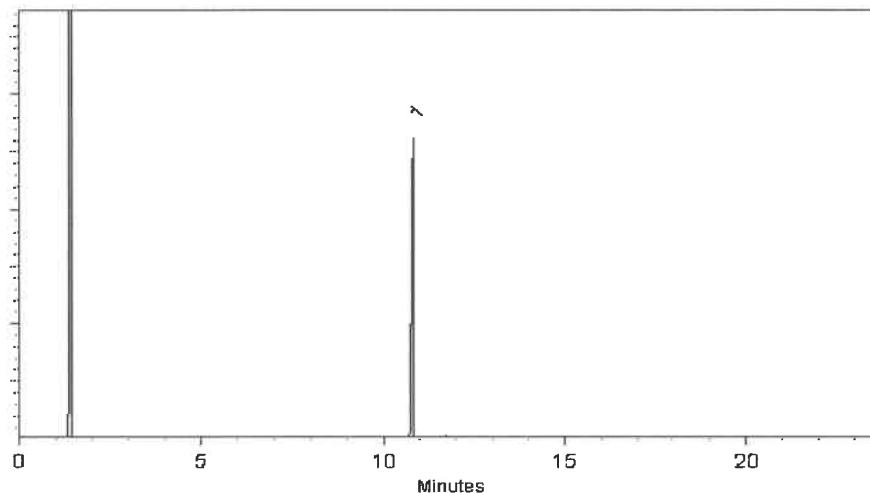

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Peter Robbins - Operations Technician I

Date Mixed: 02-Dec-2023

Balance Serial # B345965662

Christie Mills - Operations Lead Tech - ARM QC

Date Passed: 08-Dec-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No.:** 31098 **Lot No.:** A0204989

**Description:** 1-Chlorooctadecane Standard

1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size:** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date:** January 31, 2031 **Storage:** 10°C or colder

**Ship:** Ambient

P12960  
↓  
P12991 } Y.P.  
12/21/2023

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Chlorooctadecane	3386-33-2	14738400	99%	10,097.3 µg/mL	+/- 567.2675

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

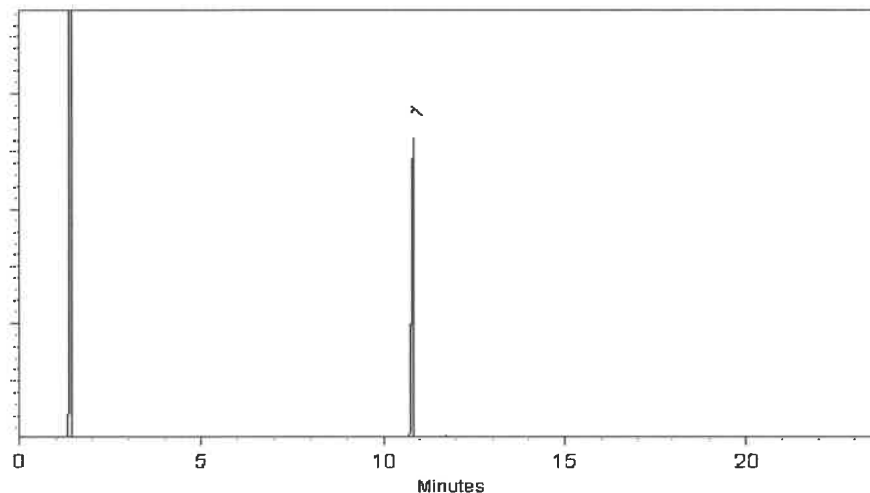

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Peter Robbins - Operations Technician I

Date Mixed: 02-Dec-2023

Balance Serial # B345965662

Christie Mills - Operations Lead Tech - ARM QC

Date Passed: 08-Dec-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31098 **Lot No.:** A0200707

**Description :** 1-Chlorooctadecane Standard  
1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride,  
1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** September 30, 2030 **Storage:** 10°C or colder  
**Ship:** Ambient

P130hh  
2  
P13051 } Y.B.  
12/26/23

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Chlorooctadecane	3386-33-2	E230426RSRB	99%	10,018.0 µg/mL	+/- 562.8106

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

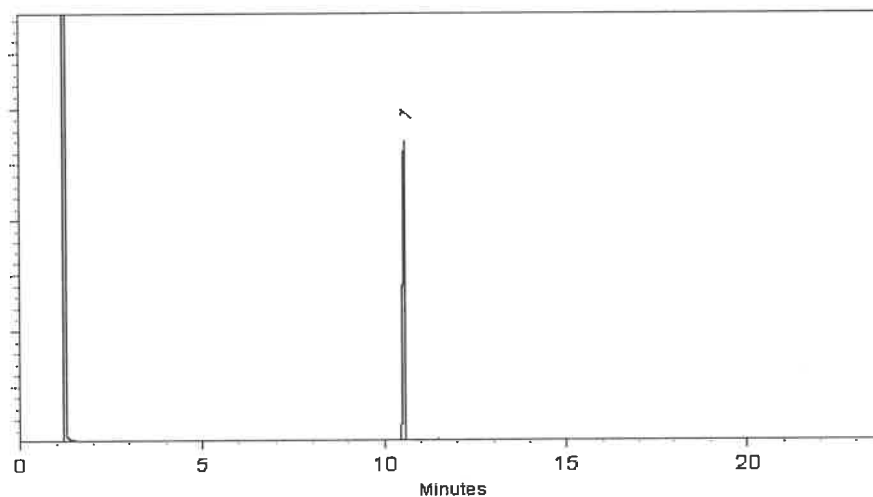

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Ashley Frantz - Quoting Technician

Date Mixed: 07-Aug-2023

Balance Serial # 1128360905

  
Dillan Murphy - Operations Technician I

Date Passed: 10-Aug-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



CERTIFIED WEIGHT REPORT

Part Number: 95999

Lot Number: 040524

Description: NJ EPH Aliphatic n-Hydrocarbons - Revised  
20 components

Expiration Date: 040534

Recommended Storage: Ambient (20 °C)

Nominal Concentration (µg/mL): 1000

NIST Test ID#: 6UTB

Weight(s) shown below were combined and diluted to (mL):

CAUTION: Sonicate Before Use

Solvent(s):  
Cyclohexane

Lot#  
28930

Formulated By:	Anthony Mahoney	040524	DATE
Reviewed By:	Pedro L. Rentas	040524	DATE

P13278  
Y.P.  
P13287  
04/11/24

5E-05 Balance Uncertainty  
0.001 Flask Uncertainty

CAUTION: Sonicate Before Use

Compound															SDS Information		
(RM#)	Lot	Dil.	Initial	Initial	Nominal	Purity	Purity	Uncertainty	Target	Actual	Expanded	(Solvent Safety Info. On Attached pg.)					
Part Number	Number	Factor	Vol. (mL)	Conc.(µg/mL)	Conc (µg/mL)	(%)	Uncertainty	Pipette	Weight(g)	Conc (µg/mL)	Uncertainty	CAS#	OSHA PEL (TWA)	LD50			
1. 2-Methylnaphthalene	(0214)	MKB3783V	NA	NA	NA	1000	97	0.2	NA	0.02579	0.02594	1005.7	91-57-6	N/A	or-rat 1630mg/kg		
2. Naphthalene	(0222)	MKB28680V	NA	NA	NA	1000	100	0.2	NA	0.02502	0.02511	1003.7	91-20-3	10 ppm (50mg/m3/8H)	or-rat 490mg/kg		
3. n-Nonane	95708	120222	1.00	25.00	1000.7	1000	NA	0.013	NA	NA	NA	1000.0	4.2	111-84-2	200 ppm (1050mg/m3/8H)	ivn-mus 218mg/kg	
4. n-Decane	95708	120222	1.00	25.00	1000.9	1000	NA	0.013	NA	NA	NA	1000.2	4.2	124-18-5	N/A	N/A	
5. n-Dodecane	95708	120222	1.00	25.00	1000.7	1000	NA	0.013	NA	NA	NA	1000.0	4.2	112-40-3	N/A	ivn-mus 3494mg/kg	
6. n-Tetradecane	95708	120222	1.00	25.00	1002.1	1000	NA	0.013	NA	NA	NA	1001.3	4.2	629-59-4	N/A	N/A	
7. n-Hexadecane	95708	120222	1.00	25.00	1000.5	1000	NA	0.013	NA	NA	NA	999.7	4.2	544-76-3	N/A	N/A	
8. n-Octadecane	95708	120222	1.00	25.00	1001.0	1000	NA	0.013	NA	NA	NA	1000.3	4.1	593-45-3	N/A	N/A	
9. n-Eicosane	95708	120222	1.00	25.00	1001.0	1000	NA	0.013	NA	NA	NA	1000.3	4.2	112-95-8	N/A	N/A	
10. n-Henelcosane	95708	120222	1.00	25.00	1002.4	1000	NA	0.013	NA	NA	NA	1001.6	4.2	628-94-7	N/A	N/A	
11. n-Docosane	95708	120222	1.00	25.00	1001.9	1000	NA	0.013	NA	NA	NA	1001.2	4.2	629-97-0	N/A	N/A	
12. n-Tetracosane	95708	120222	1.00	25.00	1000.8	1000	NA	0.013	NA	NA	NA	1000.1	4.2	646-31-1	N/A	N/A	
13. n-Hexacosane	95708	120222	1.00	25.00	1001.2	1000	NA	0.013	NA	NA	NA	1000.4	4.2	630-01-3	N/A	N/A	
14. n-Octacosane	95708	120222	1.00	25.00	1000.5	1000	NA	0.013	NA	NA	NA	999.8	4.2	630-02-4	N/A	N/A	
15. n-Triacontane	95708	120222	1.00	25.00	1000.5	1000	NA	0.013	NA	NA	NA	999.8	4.2	638-68-6	N/A	N/A	
16. n-Dotriacontane	95708	120222	1.00	25.00	1000.5	1000	NA	0.013	NA	NA	NA	999.8	4.3	544-85-4	N/A	ivn-mus 100mg/kg	
17. n-Tetra triacontane	95708	120222	1.00	25.00	1000.4	1000	NA	0.013	NA	NA	NA	999.7	4.2	14167-59-0	N/A	N/A	
18. n-Hexatri acontane	95708	120222	1.00	25.00	1000.4	1000	NA	0.013	NA	NA	NA	1000.8	4.2	630-08-8	N/A	N/A	
19. n-Octatri acontane	95708	120222	1.00	25.00	1001.5	1000	NA	0.013	NA	NA	NA	999.6	4.3	7194-85-6	N/A	N/A	
20. n-Tetracontane	95708	120222	1.00	25.00	1000.3	1000	NA	0.013	NA	NA	NA	999.9	4.3	4181-95-7	N/A	N/A	

\* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.  
\* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).  
\* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.  
\* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.  
\* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31098 **Lot No.:** A0213283

**Description :** 1-Chlorooctadecane Standard

1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** July 31, 2031 **Storage:** 10°C or colder

**Ship:** Ambient

P13595  
↓  
P13624 } Y.P.  
10/16/24

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Chlorooctadecane	3386-33-2	15018900	99%	10,058.0 µg/mL	+/- 565.0578

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-S (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

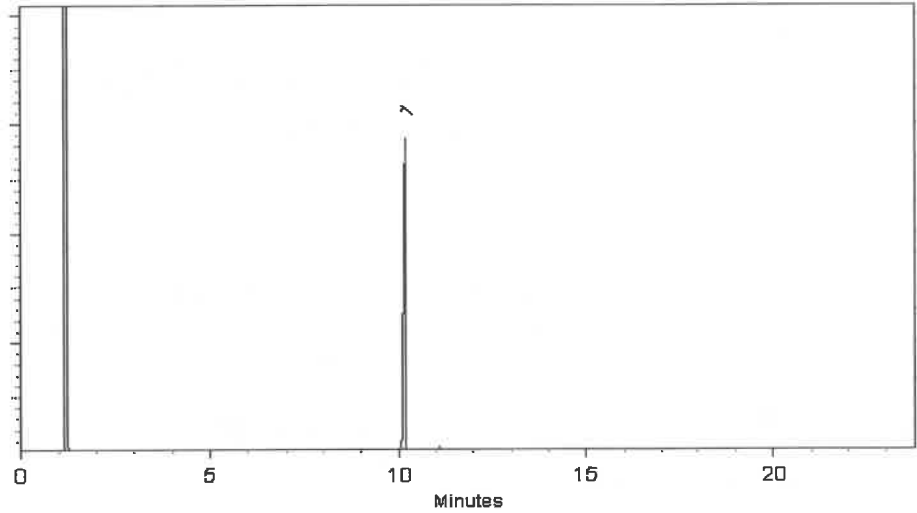

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Stacey Wanner - Operations Technician I

Date Mixed: 28-Jun-2024

Balance Serial # B345965662

Dillan Murphy - Operations Technician I

Date Passed: 01-Jul-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31097 **Lot No.:** A0216631  
**Description :** o-Terphenyl Standard  
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** April 30, 2028 **Storage:** 10°C or colder  
**Handling:** Sonicate prior to use. **Ship:** Ambient

P13645 } Y.P.  
↓  
P13694 } 10/16/24

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	o-Terphenyl	84-15-1	GKSSA	99%	10,065.0 µg/mL	+/- 453.3336

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

# Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

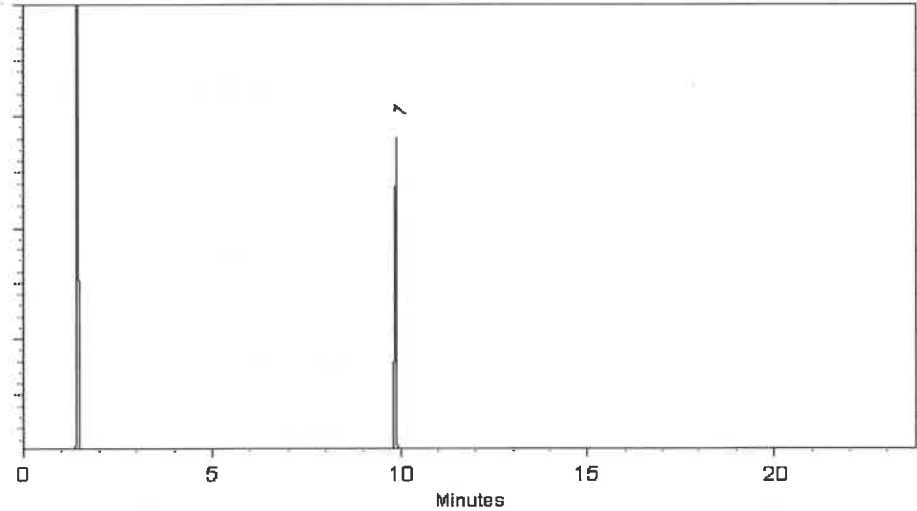

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ven Kelley - Operations Tech I

Date Mixed: 17-Sep-2024

Balance Serial # 1128353505

Dillan Murphy - Operations Technician I

Date Passed: 23-Sep-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31097 **Lot No.:** A0216631  
**Description :** o-Terphenyl Standard  
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** April 30, 2028 **Storage:** 10°C or colder  
**Handling:** Sonicate prior to use. **Ship:** Ambient

P13645 } Y.P.  
↓  
P13694 } 10/16/24

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	o-Terphenyl	84-15-1	GKSSA	99%	10,065.0 µg/mL	+/- 453.3336

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

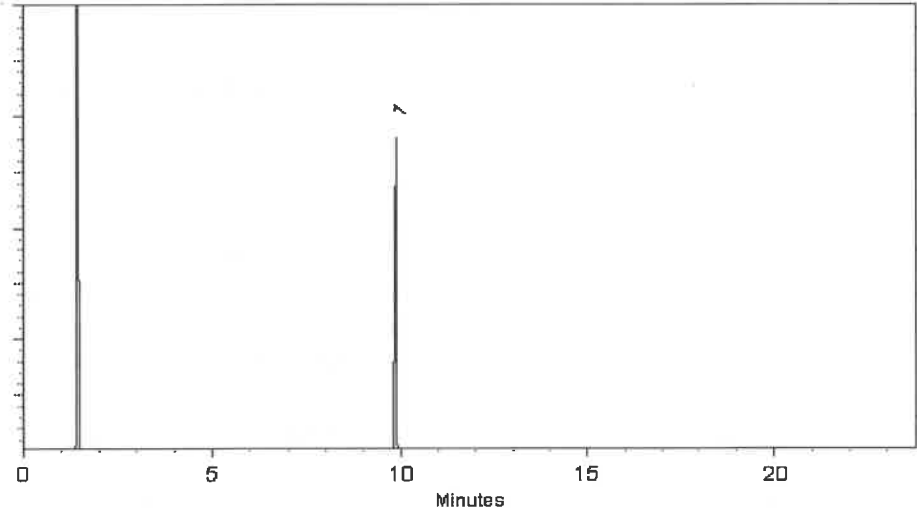

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ven Kelley - Operations Tech I

Date Mixed: 17-Sep-2024

Balance Serial # 1128353505

Dillan Murphy - Operations Technician I

Date Passed: 23-Sep-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31097 **Lot No.:** A0216631  
**Description :** o-Terphenyl Standard  
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** April 30, 2028 **Storage:** 10°C or colder  
**Handling:** Sonicate prior to use. **Ship:** Ambient

P13645 } Y.P.  
↓  
P13694 } 10/16/24

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	o-Terphenyl	84-15-1	GKSSA	99%	10,065.0 µg/mL	+/- 453.3336

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

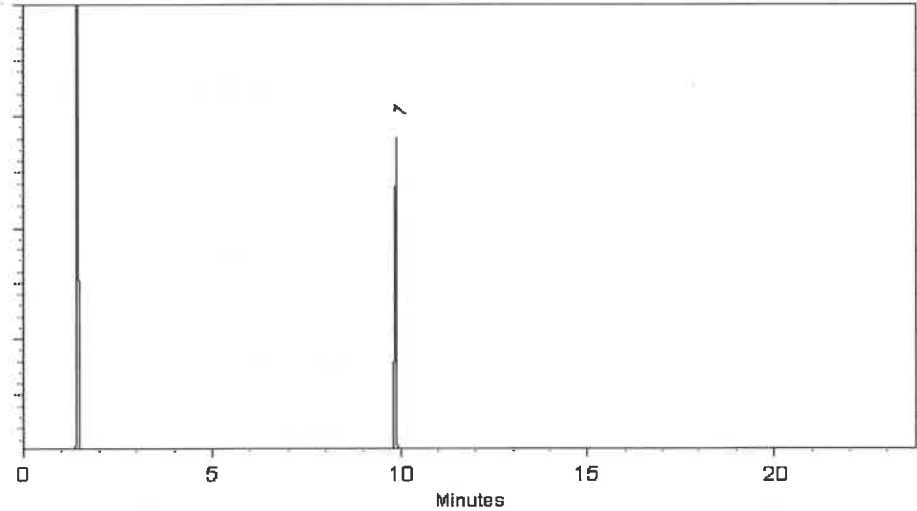

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ven Kelley - Operations Tech I

Date Mixed: 17-Sep-2024

Balance Serial # 1128353505

Dillan Murphy - Operations Technician I

Date Passed: 23-Sep-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31097 **Lot No.:** A0216631  
**Description :** o-Terphenyl Standard  
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** April 30, 2028 **Storage:** 10°C or colder  
**Handling:** Sonicate prior to use. **Ship:** Ambient

P13645 } Y.P.  
↓  
P13694 } 10/16/24

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	o-Terphenyl	84-15-1	GKSSA	99%	10,065.0 µg/mL	+/- 453.3336

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

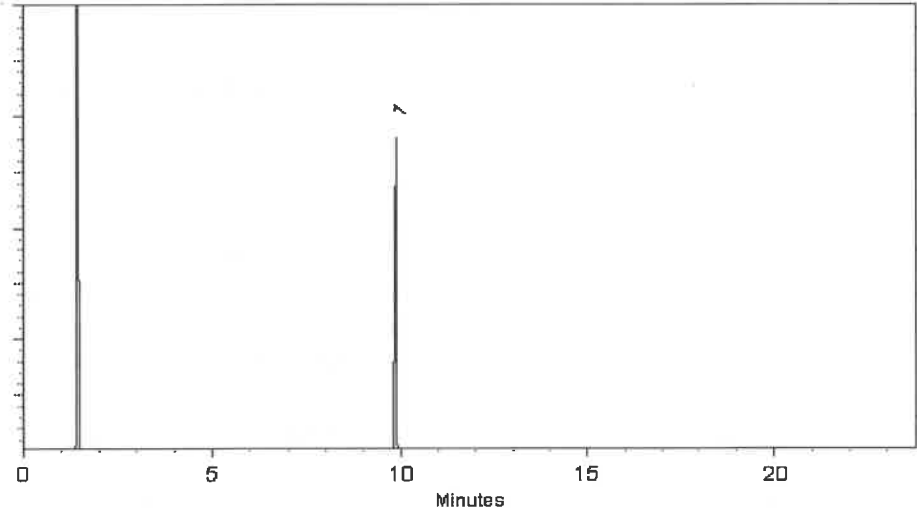

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ven Kelley - Operations Tech I

Date Mixed: 17-Sep-2024

Balance Serial # 1128353505

Dillan Murphy - Operations Technician I

Date Passed: 23-Sep-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31097 **Lot No.:** A0216631  
**Description :** o-Terphenyl Standard  
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** April 30, 2028 **Storage:** 10°C or colder  
**Handling:** Sonicate prior to use. **Ship:** Ambient

P13645 } Y.P.  
↓  
P13694 } 10/16/24

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	o-Terphenyl	84-15-1	GKSSA	99%	10,065.0 µg/mL	+/- 453.3336

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

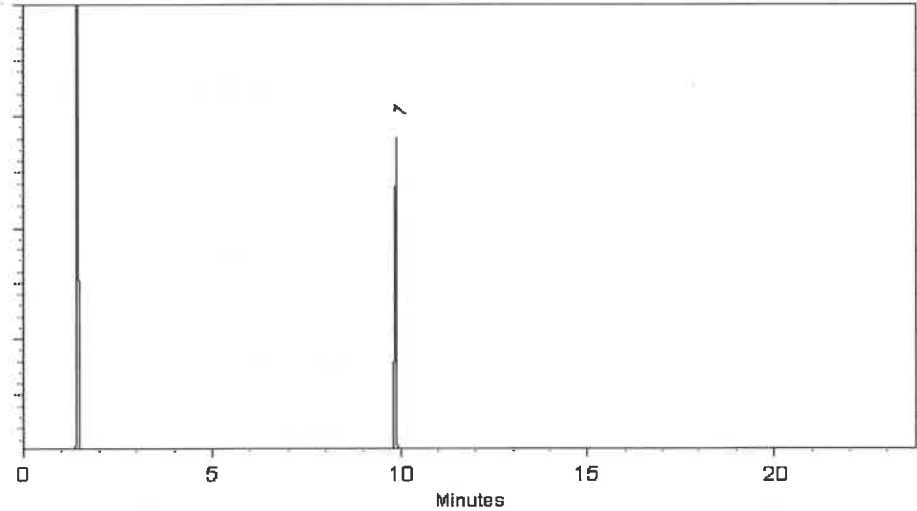

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ven Kelley - Operations Tech I

Date Mixed: 17-Sep-2024

Balance Serial # 1128353505

Dillan Murphy - Operations Technician I

Date Passed: 23-Sep-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31097 **Lot No.:** A0216631  
**Description :** o-Terphenyl Standard  
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** April 30, 2028 **Storage:** 10°C or colder  
**Handling:** Sonicate prior to use. **Ship:** Ambient

P13645 } Y.P.  
↓  
P13694 } 10/16/24

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	o-Terphenyl	84-15-1	GKSSA	99%	10,065.0 µg/mL	+/- 453.3336

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

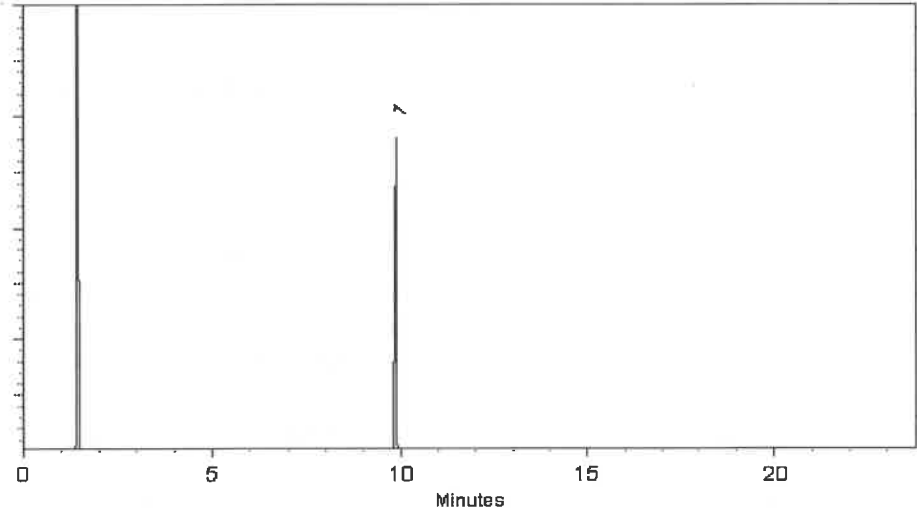

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ven Kelley - Operations Tech I

Date Mixed: 17-Sep-2024

Balance Serial # 1128353505

Dillan Murphy - Operations Technician I

Date Passed: 23-Sep-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31097 **Lot No.:** A0216631  
**Description :** o-Terphenyl Standard  
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** April 30, 2028 **Storage:** 10°C or colder  
**Handling:** Sonicate prior to use. **Ship:** Ambient

P13645 } Y.P.  
↓  
P13694 } 10/16/24

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	o-Terphenyl	84-15-1	GKSSA	99%	10,065.0 µg/mL	+/- 453.3336

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

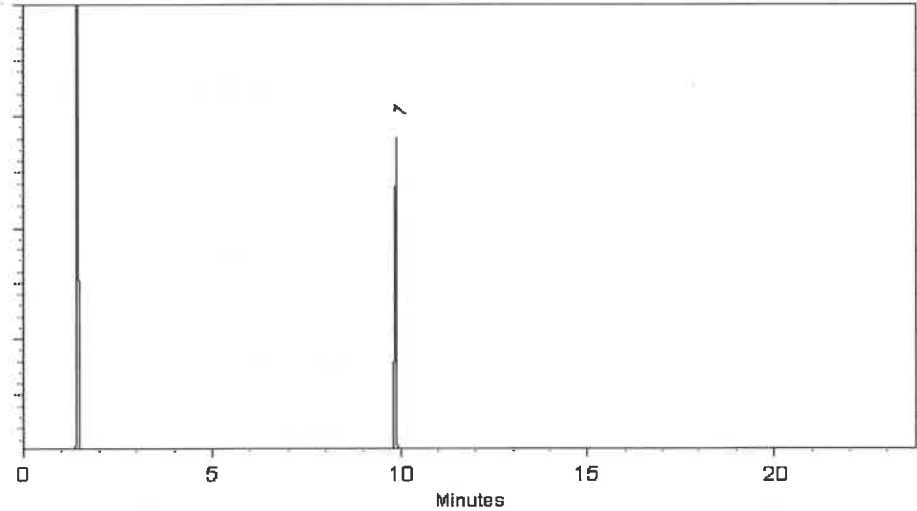

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ven Kelley - Operations Tech I

Date Mixed: 17-Sep-2024

Balance Serial # 1128353505

Dillan Murphy - Operations Technician I

Date Passed: 23-Sep-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543

**Lot No.:** A0211254

**Description :** NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

**Container Size :** 5 mL

**Pkg Amt:** > 5 mL

**Expiration Date :** April 30, 2030

**Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive.

**Ship:** Ambient

P13408  
↓  
P13716 } Y.P.  
10/26/24

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	200.0 µg/mL	+/- 9.0114
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBK0259	96%	200.4 µg/mL	+/- 9.0316
4	Acenaphthylene	208-96-8	214935L31M	98%	200.3 µg/mL	+/- 9.0255
5	Acenaphthene	83-32-9	MKCR7169	99%	202.0 µg/mL	+/- 9.1015
6	Fluorene	86-73-7	10241100	99%	201.2 µg/mL	+/- 9.0655
7	Phenanthrene	85-01-8	MKCS5188	99%	200.4 µg/mL	+/- 9.0294
8	Anthracene	120-12-7	MKCR0570	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.8 µg/mL	+/- 9.0474
10	Pyrene	129-00-0	BCCK2592	99%	201.2 µg/mL	+/- 9.0655
11	Benz(a)anthracene	56-55-3	I30012022BAA	99%	200.8 µg/mL	+/- 9.0474
12	Chrysene	218-01-9	RP231206RSR	99%	200.4 µg/mL	+/- 9.0294
13	Benzo(b)fluoranthene	205-99-2	012013B	99%	200.4 µg/mL	+/- 9.0294
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.0 µg/mL	+/- 9.0114
15	Benzo(a)pyrene	50-32-8	O45GL	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	199.8 µg/mL	+/- 9.0033

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	200.0	µg/mL	+/- 9.0114
18	Benzo(g,h,i)perylene	191-24-2	RP240105ECS	99%	200.8	µg/mL	+/- 9.0474

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rbx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

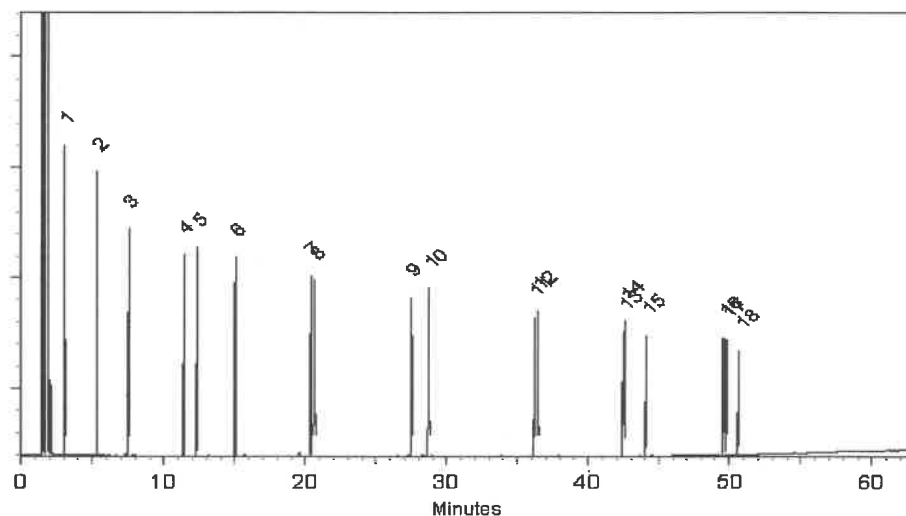

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Michael Maye*  
Michael Maye - Operations Tech I

**Date Mixed:** 09-May-2024 **Balance Serial #** 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 13-May-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31480 **Lot No.:** A0214879  
**Description :** MA Fractionation Surrogate Spike Mix  
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** July 31, 2030 **Storage:** 10°C or colder  
**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

P13743  
↓  
P13772 } Y.P.  
11/01/24

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,009.0 µg/mL	+/- 180.5961
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,008.5 µg/mL	+/- 180.5736

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

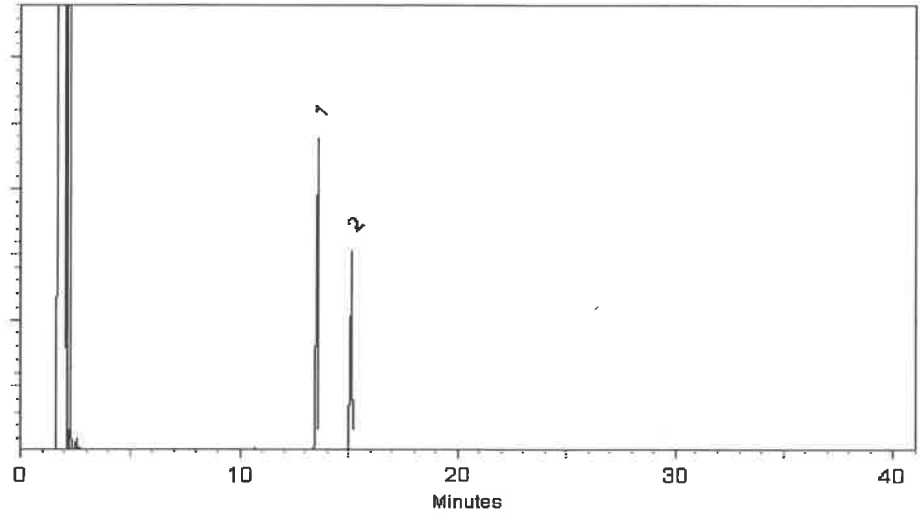

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Scott McNeil - Operations Tech I

Date Mixed: 06-Aug-2024

Balance Serial # 1128360905

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 14-Aug-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31480 **Lot No.:** A0214879  
**Description :** MA Fractionation Surrogate Spike Mix  
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** July 31, 2030 **Storage:** 10°C or colder  
**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

P13743  
↓  
P13772 } Y.P.  
11/01/24

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,009.0 µg/mL	+/- 180.5961
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,008.5 µg/mL	+/- 180.5736

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

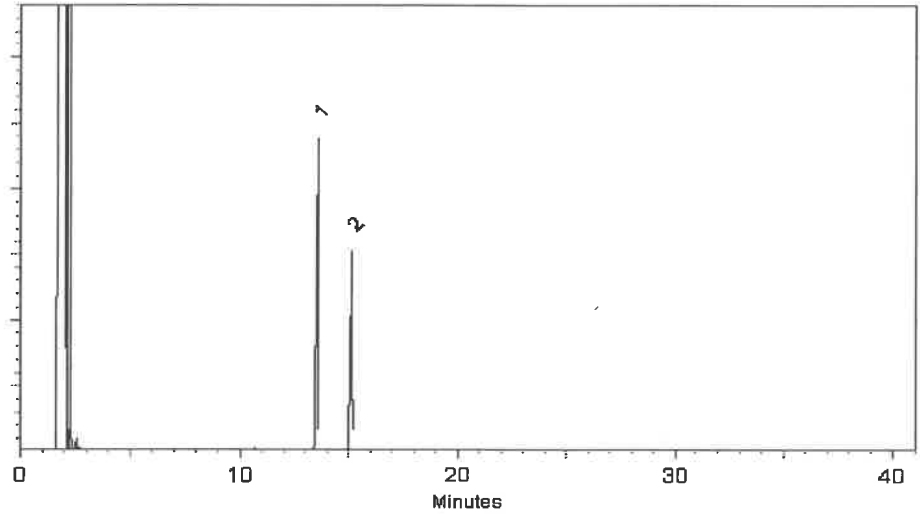

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Scott McNeil - Operations Tech I

Date Mixed: 06-Aug-2024

Balance Serial # 1128360905

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 14-Aug-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



## FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543 **Lot No.:** A0220580

**Description :** NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2030 **Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

P13863 } y.p.  
↓  
P13866 } 01/08/25

## CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-39	98%	201.9 µg/mL	+/- 9.0961
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	RP241029RSR	98%	201.9 µg/mL	+/- 9.0961
5	Acenaphthene	83-32-9	MKCR7169	99%	200.4 µg/mL	+/- 9.0294
6	Fluorene	86-73-7	10246250	98%	201.9 µg/mL	+/- 9.0961
7	Phenanthrene	85-01-8	MKCT3391	99%	200.8 µg/mL	+/- 9.0474
8	Anthracene	120-12-7	MKCW9141	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCL8032	99%	201.6 µg/mL	+/- 9.0835
11	Benz(a)anthracene	56-55-3	I220012022BAA	99%	202.0 µg/mL	+/- 9.1015
12	Chrysene	218-01-9	RP240719RSR	99%	202.0 µg/mL	+/- 9.1015
13	Benzo(b)fluoranthene	205-99-2	SBS-BBF-FINAL-2	99%	202.0 µg/mL	+/- 9.1015
14	Benzo(k)fluoranthene	207-08-9	012022K	98%	201.5 µg/mL	+/- 9.0784
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0383

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	201.2 µg/mL	+/- 9.0655
18	Benzo(g,h,i)perylene	191-24-2	RP241014RSR	98%	200.3 µg/mL	+/- 9.0255

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

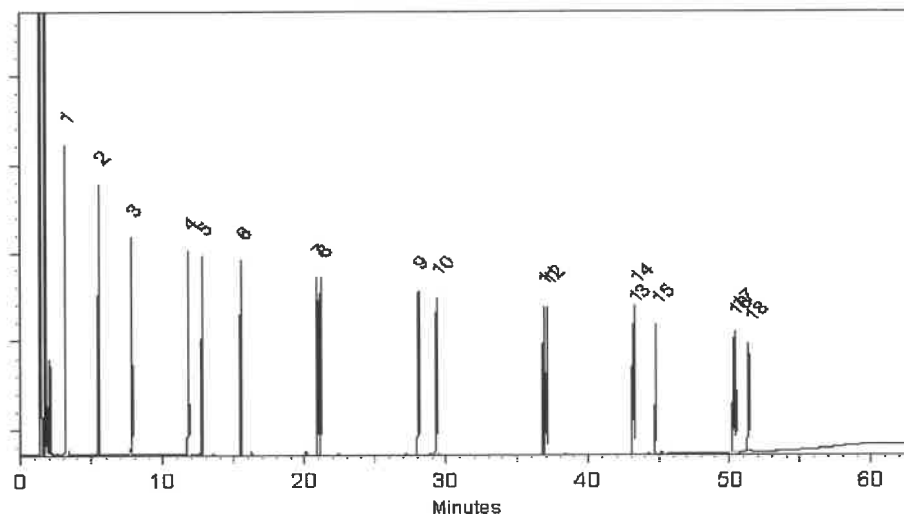

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Ven Kelley*  
**Ven Kelley - Operations Tech I**

**Date Mixed:** 30-Dec-2024 **Balance Serial #** 1128360905

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 03-Jan-2025

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30542 **Lot No.:** A0217408

**Description :** NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2031 **Storage:** 10°C or colder

**Handling:** Sonicate prior to use. **Ship:** Ambient

P13896  
↓  
P13906 } Y.P.  
03/06/25

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.7 µg/mL	+/- 5.1839
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	201.0 µg/mL	+/- 5.1917
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.5 µg/mL	+/- 5.1805
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.5 µg/mL	+/- 5.1805
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.7 µg/mL	+/- 5.1857
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.7 µg/mL	+/- 5.1857
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.9 µg/mL	+/- 5.1888
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.5 µg/mL	+/- 5.1805
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.5 µg/mL	+/- 5.1788
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.6 µg/mL	+/- 5.1822
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCJ4566	99%	200.6 µg/mL	+/- 5.1822
13	n-Triacontane (C30)	638-68-6	MKCV7007	98%	201.1 µg/mL	+/- 5.1942
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.9 µg/mL	+/- 5.1891
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.8 µg/mL	+/- 5.1865
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	199.3 µg/mL	+/- 5.1477

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane**CAS #** 109-66-0**Purity** 99%

## Quality Confirmation Test

**Column:**30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

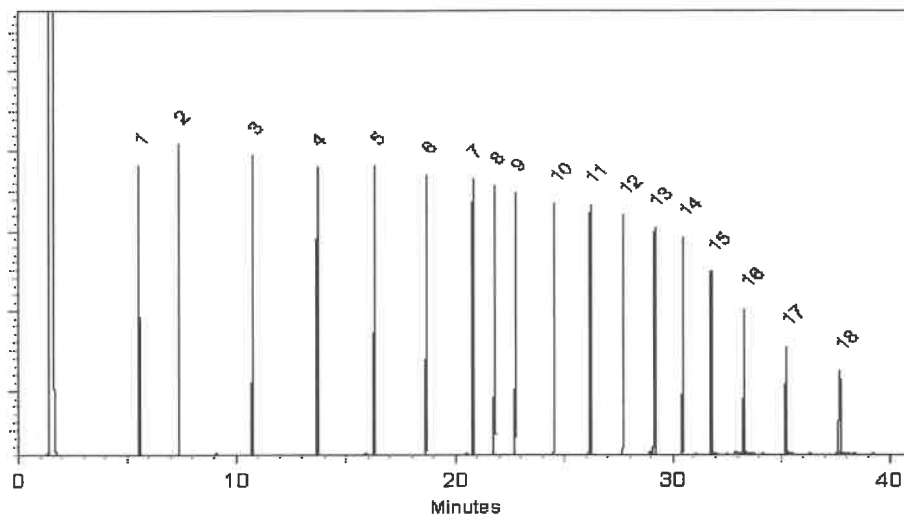

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope B. Riglin*  
Penelope Riglin - Operations Tech I

**Date Mixed:** 03-Oct-2024**Balance Serial #** 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30542 **Lot No.:** A0217408

**Description :** NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2031 **Storage:** 10°C or colder

**Handling:** Sonicate prior to use. **Ship:** Ambient

P13896  
↓  
P13906 } Y.P.  
03/06/25

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.7 µg/mL	+/- 5.1839
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	201.0 µg/mL	+/- 5.1917
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.5 µg/mL	+/- 5.1805
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.5 µg/mL	+/- 5.1805
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.7 µg/mL	+/- 5.1857
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.7 µg/mL	+/- 5.1857
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.9 µg/mL	+/- 5.1888
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.5 µg/mL	+/- 5.1805
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.5 µg/mL	+/- 5.1788
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.6 µg/mL	+/- 5.1822
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCJ4566	99%	200.6 µg/mL	+/- 5.1822
13	n-Triacontane (C30)	638-68-6	MKCV7007	98%	201.1 µg/mL	+/- 5.1942
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.9 µg/mL	+/- 5.1891
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.8 µg/mL	+/- 5.1865
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	199.3 µg/mL	+/- 5.1477

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane  
**CAS #** 109-66-0  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)  
**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
2 ml/min.

**Inj. Vol**  
1µl

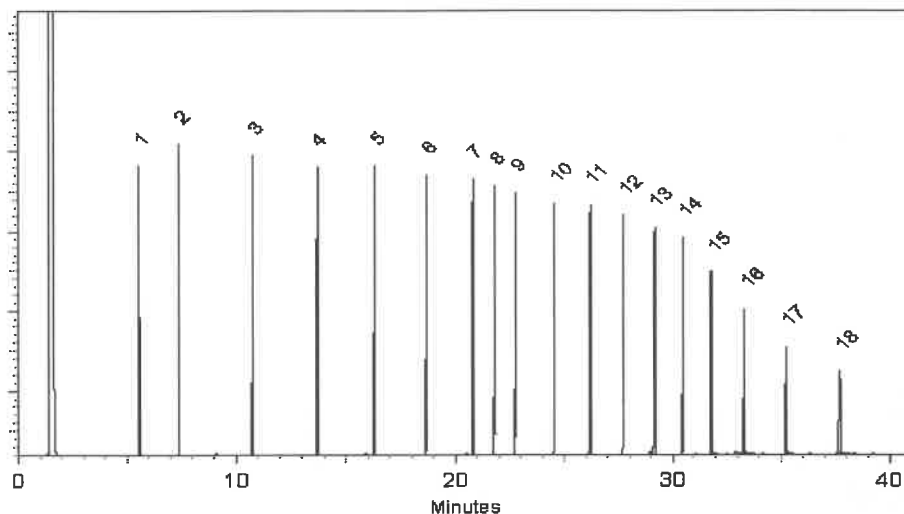

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope B. Riglin*  
Penelope Riglin - Operations Tech I

**Date Mixed:** 03-Oct-2024

**Balance Serial #** 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30542 **Lot No.:** A0217408

**Description :** NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2031 **Storage:** 10°C or colder

**Handling:** Sonicate prior to use. **Ship:** Ambient

P13896  
↓  
P13906 } Y.P.  
03/06/25

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.7 µg/mL	+/- 5.1839
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	201.0 µg/mL	+/- 5.1917
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.5 µg/mL	+/- 5.1805
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.5 µg/mL	+/- 5.1805
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.7 µg/mL	+/- 5.1857
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.7 µg/mL	+/- 5.1857
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.9 µg/mL	+/- 5.1888
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.5 µg/mL	+/- 5.1805
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.5 µg/mL	+/- 5.1788
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.6 µg/mL	+/- 5.1822
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCJ4566	99%	200.6 µg/mL	+/- 5.1822
13	n-Triacontane (C30)	638-68-6	MKCV7007	98%	201.1 µg/mL	+/- 5.1942
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.9 µg/mL	+/- 5.1891
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.8 µg/mL	+/- 5.1865
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	199.3 µg/mL	+/- 5.1477

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane**CAS #** 109-66-0**Purity** 99%

## Quality Confirmation Test

**Column:**30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

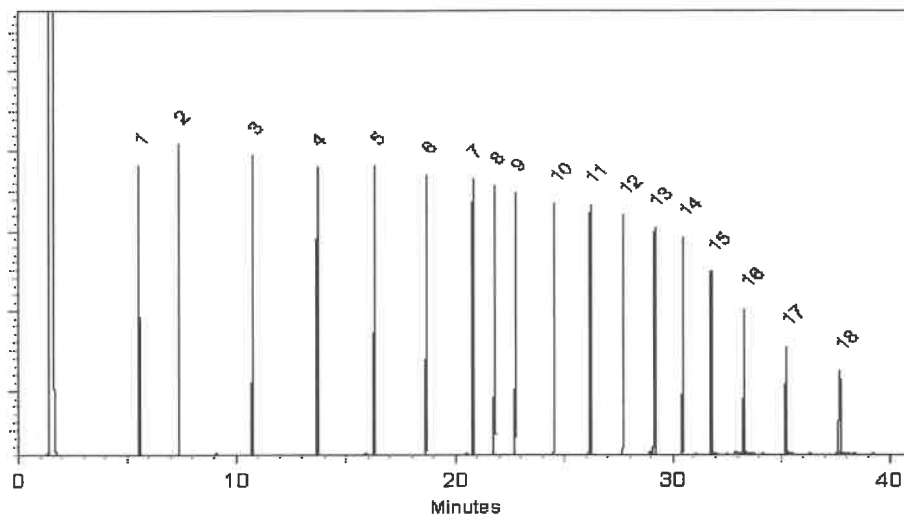

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope B. Riglin*  
Penelope Riglin - Operations Tech I

**Date Mixed:** 03-Oct-2024**Balance Serial #** 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30542 **Lot No.:** A0217408

**Description :** NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2031 **Storage:** 10°C or colder

**Handling:** Sonicate prior to use. **Ship:** Ambient

P13896  
↓  
P13906 } Y.P.  
03/06/25

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.7 µg/mL	+/- 5.1839
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	201.0 µg/mL	+/- 5.1917
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.5 µg/mL	+/- 5.1805
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.5 µg/mL	+/- 5.1805
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.7 µg/mL	+/- 5.1857
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.7 µg/mL	+/- 5.1857
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.9 µg/mL	+/- 5.1888
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.5 µg/mL	+/- 5.1805
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.5 µg/mL	+/- 5.1788
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.6 µg/mL	+/- 5.1822
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCJ4566	99%	200.6 µg/mL	+/- 5.1822
13	n-Triacontane (C30)	638-68-6	MKCV7007	98%	201.1 µg/mL	+/- 5.1942
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.9 µg/mL	+/- 5.1891
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.8 µg/mL	+/- 5.1865
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	199.3 µg/mL	+/- 5.1477

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane**CAS #** 109-66-0**Purity** 99%

## Quality Confirmation Test

**Column:**30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

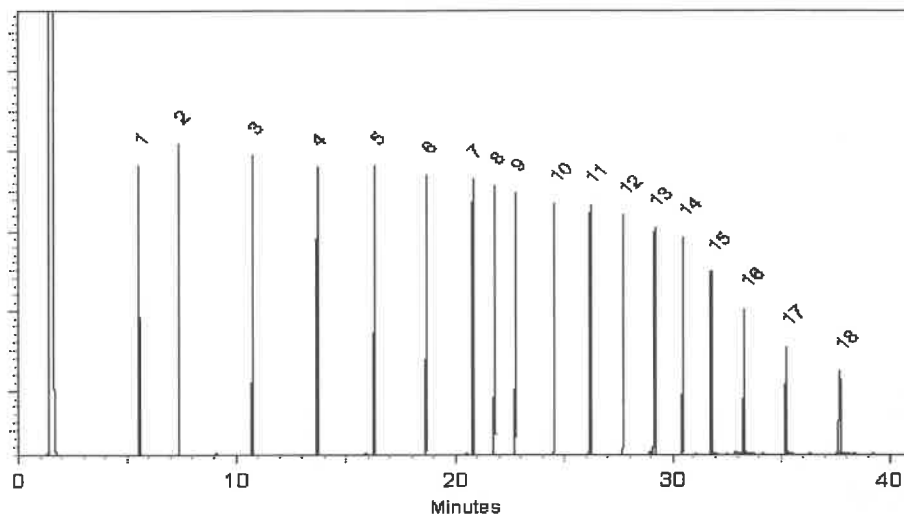

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope B. Riglin*  
Penelope Riglin - Operations Tech I

**Date Mixed:** 03-Oct-2024**Balance Serial #** 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30542 **Lot No.:** A0217408

**Description :** NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2031 **Storage:** 10°C or colder

**Handling:** Sonicate prior to use. **Ship:** Ambient

P13896  
↓  
P13906 } Y.P.  
03/06/25

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.7 µg/mL	+/- 5.1839
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	201.0 µg/mL	+/- 5.1917
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.5 µg/mL	+/- 5.1805
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.5 µg/mL	+/- 5.1805
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.7 µg/mL	+/- 5.1857
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.7 µg/mL	+/- 5.1857
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.9 µg/mL	+/- 5.1888
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.5 µg/mL	+/- 5.1805
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.5 µg/mL	+/- 5.1788
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.6 µg/mL	+/- 5.1822
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCJ4566	99%	200.6 µg/mL	+/- 5.1822
13	n-Triacontane (C30)	638-68-6	MKCV7007	98%	201.1 µg/mL	+/- 5.1942
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.9 µg/mL	+/- 5.1891
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.8 µg/mL	+/- 5.1865
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	199.3 µg/mL	+/- 5.1477

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane**CAS #** 109-66-0**Purity** 99%

## Quality Confirmation Test

**Column:**30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

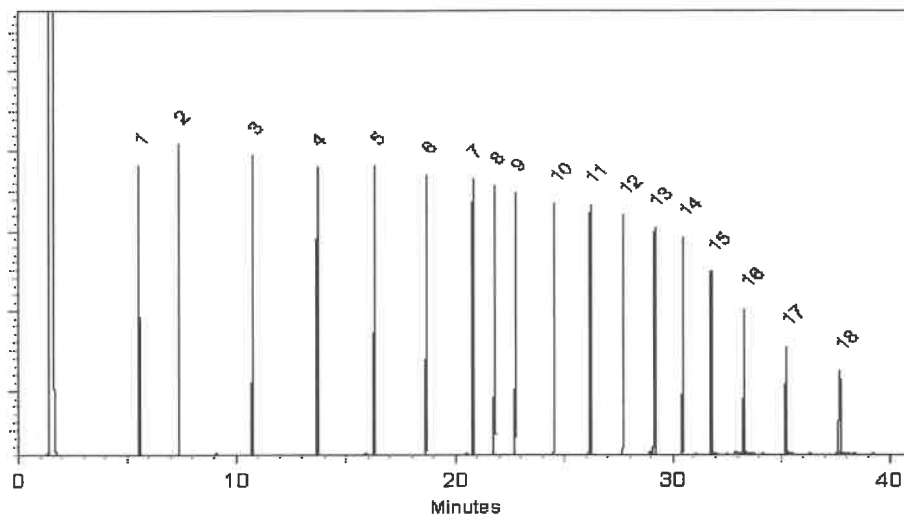

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope B. Riglin*  
Penelope Riglin - Operations Tech I

**Date Mixed:** 03-Oct-2024**Balance Serial #** 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30542 **Lot No.:** A0217408

**Description :** NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2031 **Storage:** 10°C or colder

**Handling:** Sonicate prior to use. **Ship:** Ambient

P13896  
↓  
P13906 } Y.P.  
03/06/25

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.7 µg/mL	+/- 5.1839
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	201.0 µg/mL	+/- 5.1917
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.5 µg/mL	+/- 5.1805
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.5 µg/mL	+/- 5.1805
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.7 µg/mL	+/- 5.1857
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.7 µg/mL	+/- 5.1857
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.9 µg/mL	+/- 5.1888
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.5 µg/mL	+/- 5.1805
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.5 µg/mL	+/- 5.1788
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.6 µg/mL	+/- 5.1822
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCJ4566	99%	200.6 µg/mL	+/- 5.1822
13	n-Triacontane (C30)	638-68-6	MKCV7007	98%	201.1 µg/mL	+/- 5.1942
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.9 µg/mL	+/- 5.1891
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.8 µg/mL	+/- 5.1865
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	199.3 µg/mL	+/- 5.1477

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane  
**CAS #** 109-66-0  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)  
**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
2 ml/min.

**Inj. Vol**  
1µl

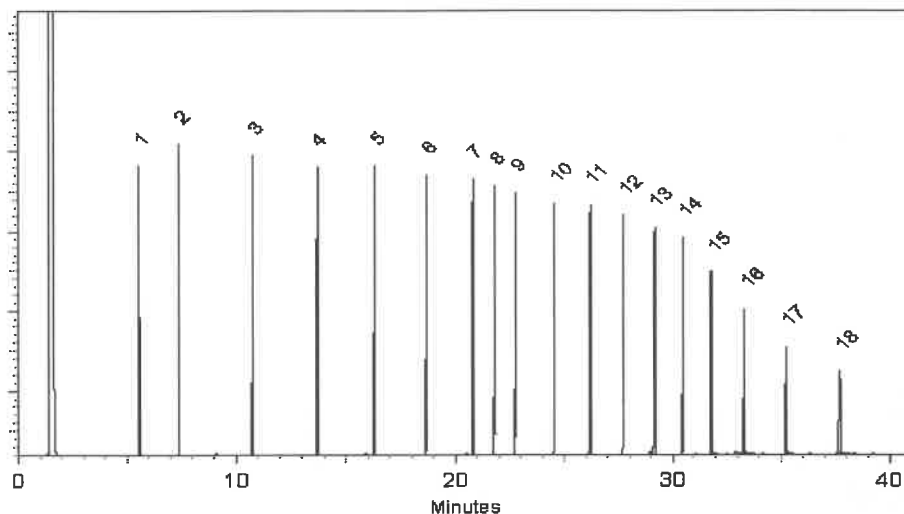


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Penelope Riglin - Operations Tech I

**Date Mixed:** 03-Oct-2024

**Balance Serial #** 1128353505

  
Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30542 **Lot No.:** A0217408

**Description :** NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2031 **Storage:** 10°C or colder

**Handling:** Sonicate prior to use. **Ship:** Ambient

P13896  
↓  
P13906 } Y.P.  
03/06/25

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.7 µg/mL	+/- 5.1839
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	201.0 µg/mL	+/- 5.1917
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.5 µg/mL	+/- 5.1805
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.5 µg/mL	+/- 5.1805
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.7 µg/mL	+/- 5.1857
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.7 µg/mL	+/- 5.1857
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.9 µg/mL	+/- 5.1888
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.5 µg/mL	+/- 5.1805
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.5 µg/mL	+/- 5.1788
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.6 µg/mL	+/- 5.1822
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCJ4566	99%	200.6 µg/mL	+/- 5.1822
13	n-Triacontane (C30)	638-68-6	MKCV7007	98%	201.1 µg/mL	+/- 5.1942
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.9 µg/mL	+/- 5.1891
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.8 µg/mL	+/- 5.1865
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	199.3 µg/mL	+/- 5.1477

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane**CAS #** 109-66-0**Purity** 99%

## Quality Confirmation Test

**Column:**30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

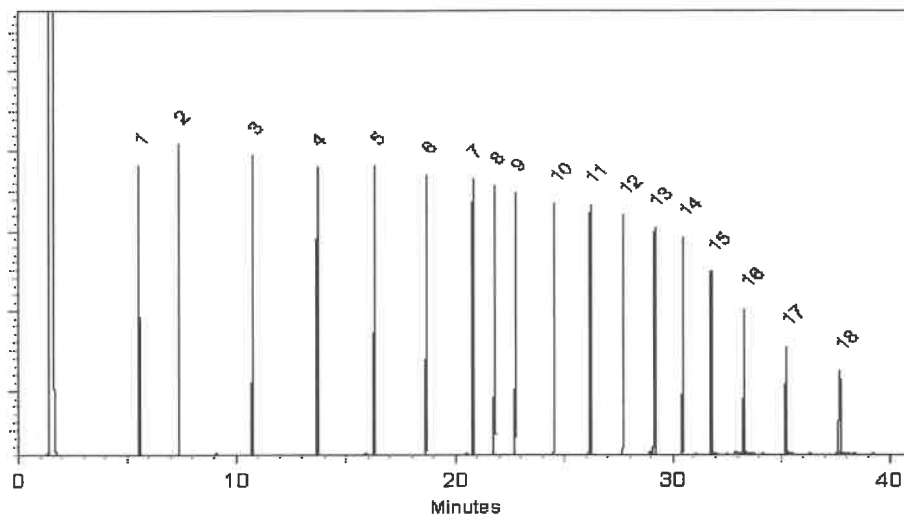

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope B. Riglin*  
Penelope Riglin - Operations Tech I

**Date Mixed:** 03-Oct-2024**Balance Serial #** 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30542 **Lot No.:** A0217408

**Description :** NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2031 **Storage:** 10°C or colder

**Handling:** Sonicate prior to use. **Ship:** Ambient

P13896  
↓  
P13906 } Y.P.  
03/06/25

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.7 µg/mL	+/- 5.1839
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	201.0 µg/mL	+/- 5.1917
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.5 µg/mL	+/- 5.1805
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.5 µg/mL	+/- 5.1805
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.7 µg/mL	+/- 5.1857
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.7 µg/mL	+/- 5.1857
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.9 µg/mL	+/- 5.1888
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.5 µg/mL	+/- 5.1805
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.5 µg/mL	+/- 5.1788
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.6 µg/mL	+/- 5.1822
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCJ4566	99%	200.6 µg/mL	+/- 5.1822
13	n-Triacontane (C30)	638-68-6	MKCV7007	98%	201.1 µg/mL	+/- 5.1942
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.9 µg/mL	+/- 5.1891
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.8 µg/mL	+/- 5.1865
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	199.3 µg/mL	+/- 5.1477

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane  
**CAS #** 109-66-0  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)  
**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
2 ml/min.

**Inj. Vol**  
1µl

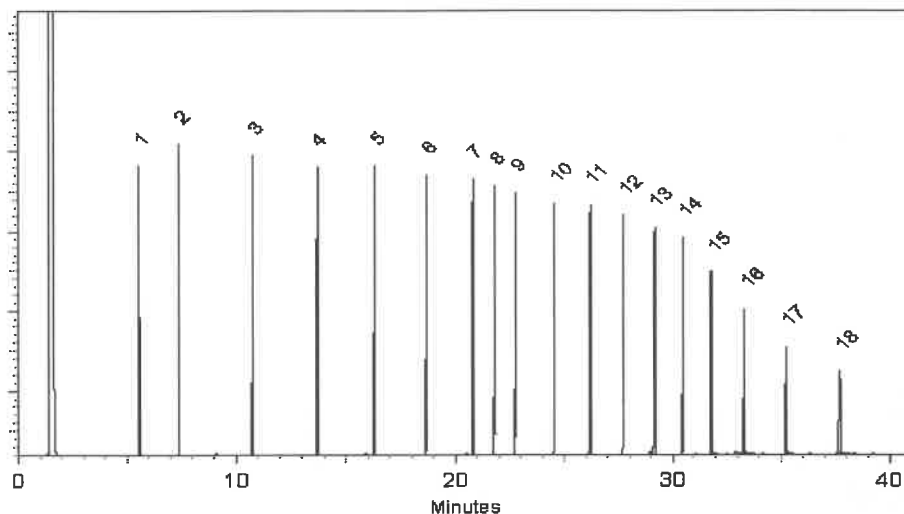

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope B. Riglin*  
Penelope Riglin - Operations Tech I

**Date Mixed:** 03-Oct-2024

**Balance Serial #** 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30542 **Lot No.:** A0217408

**Description :** NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2031 **Storage:** 10°C or colder

**Handling:** Sonicate prior to use. **Ship:** Ambient

P13896  
↓  
P13906 } Y.P.  
03/06/25

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.7 µg/mL	+/- 5.1839
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	201.0 µg/mL	+/- 5.1917
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.5 µg/mL	+/- 5.1805
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.5 µg/mL	+/- 5.1805
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.7 µg/mL	+/- 5.1857
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.7 µg/mL	+/- 5.1857
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.9 µg/mL	+/- 5.1888
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.5 µg/mL	+/- 5.1805
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.5 µg/mL	+/- 5.1788
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.6 µg/mL	+/- 5.1822
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCJ4566	99%	200.6 µg/mL	+/- 5.1822
13	n-Triacontane (C30)	638-68-6	MKCV7007	98%	201.1 µg/mL	+/- 5.1942
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.9 µg/mL	+/- 5.1891
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.8 µg/mL	+/- 5.1865
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	199.3 µg/mL	+/- 5.1477

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane  
**CAS #** 109-66-0  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
2 ml/min.

**Inj. Vol**  
1µl

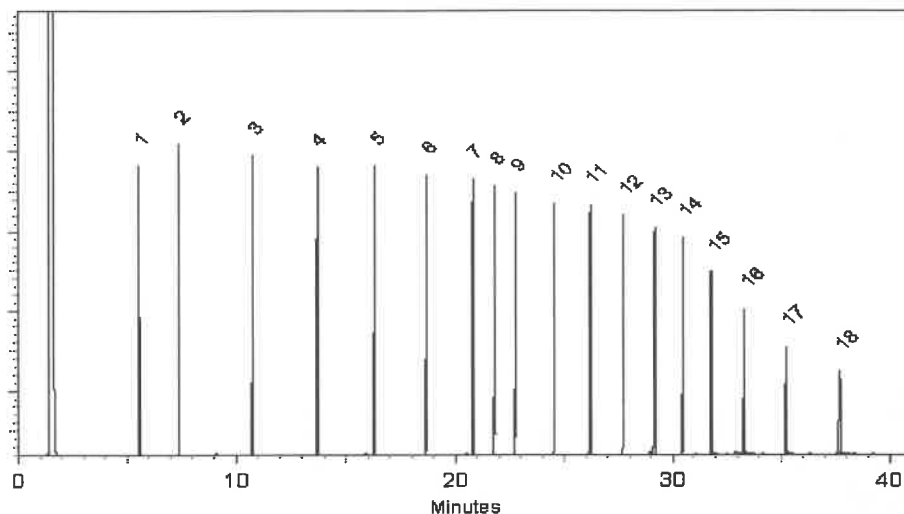

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope B. Riglin*  
Penelope Riglin - Operations Tech I

**Date Mixed:** 03-Oct-2024 **Balance Serial #** 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30542 **Lot No.:** A0220449

**Description :** NJEPH Aliphatics Matrix Spike Mix  
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** January 31, 2032 **Storage:** 10°C or colder

**Handling:** Sonicate prior to use. **Ship:** Ambient

P13909  
↓  
P1395 } Y.P.  
03/06/25

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	201.3 µg/mL	+/- 5.2012
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	201.7 µg/mL	+/- 5.2098
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	201.3 µg/mL	+/- 5.2012
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.7 µg/mL	+/- 5.1839
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.3 µg/mL	+/- 5.1753
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.7 µg/mL	+/- 5.1839
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.1 µg/mL	+/- 5.1704
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.7 µg/mL	+/- 5.1839
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.3 µg/mL	+/- 5.1753
10	n-Tetracosane (C24)	646-31-1	UH5GN	99%	201.3 µg/mL	+/- 5.2012
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	201.0 µg/mL	+/- 5.1926
12	n-Octacosane (C28)	630-02-4	BCCJ4566	99%	200.3 µg/mL	+/- 5.1753
13	n-Triacontane (C30)	638-68-6	MKCV7007	98%	201.2 µg/mL	+/- 5.1984
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	201.7 µg/mL	+/- 5.2098
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	201.3 µg/mL	+/- 5.2012
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	201.7 µg/mL	+/- 5.2098
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	201.6 µg/mL	+/- 5.2081

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane  
**CAS #** 109-66-0  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
2 ml/min.

**Inj. Vol**  
1µl

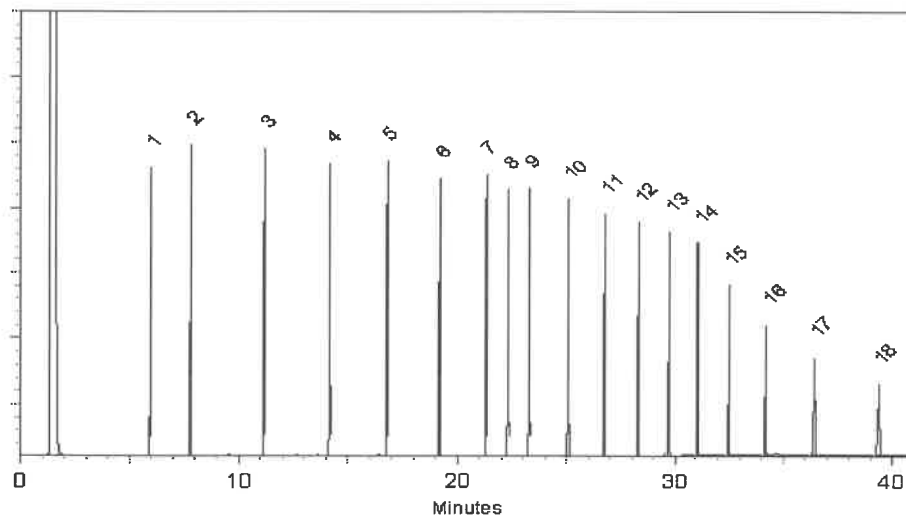

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Brandon Reish*  
Brandon Reish - Operations Technician III

**Date Mixed:** 23-Dec-2024 **Balance Serial #** C322230531

*Dylan Murphy*  
Dylan Murphy - Operations Technician I

**Date Passed:** 27-Dec-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543

**Lot No.:** A0220580

**Description :** NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

**Container Size :** 5 mL

**Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2030

**Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive.

**Ship:** Ambient

P13916 } Y.P.  
↓  
P13935 } 08/06/25

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-39	98%	201.9 µg/mL	+/- 9.0961
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	RP241029RSR	98%	201.9 µg/mL	+/- 9.0961
5	Acenaphthene	83-32-9	MKCR7169	99%	200.4 µg/mL	+/- 9.0294
6	Fluorene	86-73-7	10246250	98%	201.9 µg/mL	+/- 9.0961
7	Phenanthrene	85-01-8	MKCT3391	99%	200.8 µg/mL	+/- 9.0474
8	Anthracene	120-12-7	MKCW9141	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCL8032	99%	201.6 µg/mL	+/- 9.0835
11	Benz(a)anthracene	56-55-3	I220012022BAA	99%	202.0 µg/mL	+/- 9.1015
12	Chrysene	218-01-9	RP240719RSR	99%	202.0 µg/mL	+/- 9.1015
13	Benzo(b)fluoranthene	205-99-2	SBS-BBF-FINAL-2	99%	202.0 µg/mL	+/- 9.1015
14	Benzo(k)fluoranthene	207-08-9	012022K	98%	201.5 µg/mL	+/- 9.0784
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0383

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	201.2 µg/mL	+/- 9.0655
18	Benzo(g,h,i)perylene	191-24-2	RP241014RSR	98%	200.3 µg/mL	+/- 9.0255

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

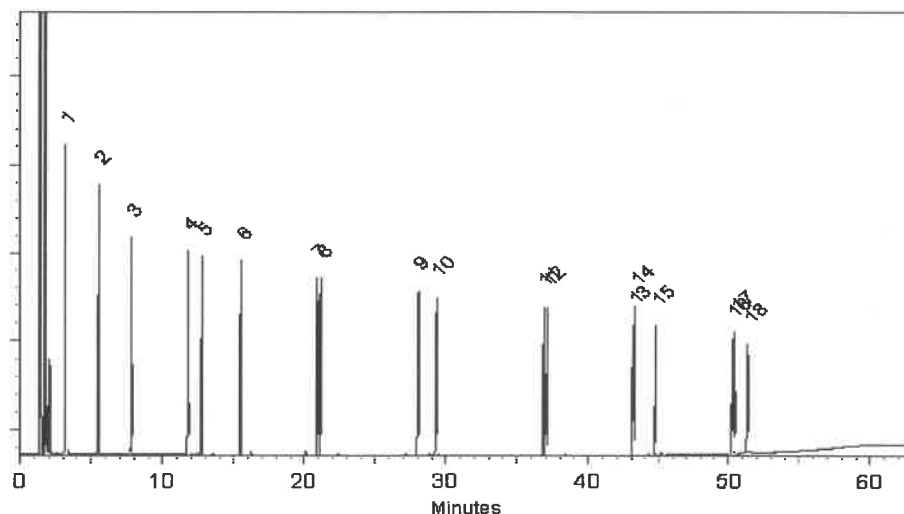

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*VenKelley*  
**Ven Kelley - Operations Tech I**

**Date Mixed:** 30-Dec-2024 **Balance Serial #** 1128360905

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 03-Jan-2025

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543

**Lot No.:** A0220580

**Description :** NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

**Container Size :** 5 mL

**Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2030

**Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive.

**Ship:** Ambient

P13916 } Y.P.  
↓  
P13935 } 08/06/25

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-39	98%	201.9 µg/mL	+/- 9.0961
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	RP241029RSR	98%	201.9 µg/mL	+/- 9.0961
5	Acenaphthene	83-32-9	MKCR7169	99%	200.4 µg/mL	+/- 9.0294
6	Fluorene	86-73-7	10246250	98%	201.9 µg/mL	+/- 9.0961
7	Phenanthrene	85-01-8	MKCT3391	99%	200.8 µg/mL	+/- 9.0474
8	Anthracene	120-12-7	MKCW9141	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCL8032	99%	201.6 µg/mL	+/- 9.0835
11	Benz(a)anthracene	56-55-3	I220012022BAA	99%	202.0 µg/mL	+/- 9.1015
12	Chrysene	218-01-9	RP240719RSR	99%	202.0 µg/mL	+/- 9.1015
13	Benzo(b)fluoranthene	205-99-2	SBS-BBF-FINAL-2	99%	202.0 µg/mL	+/- 9.1015
14	Benzo(k)fluoranthene	207-08-9	012022K	98%	201.5 µg/mL	+/- 9.0784
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0383

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	201.2 µg/mL	+/- 9.0655
18	Benzo(g,h,i)perylene	191-24-2	RP241014RSR	98%	200.3 µg/mL	+/- 9.0255

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

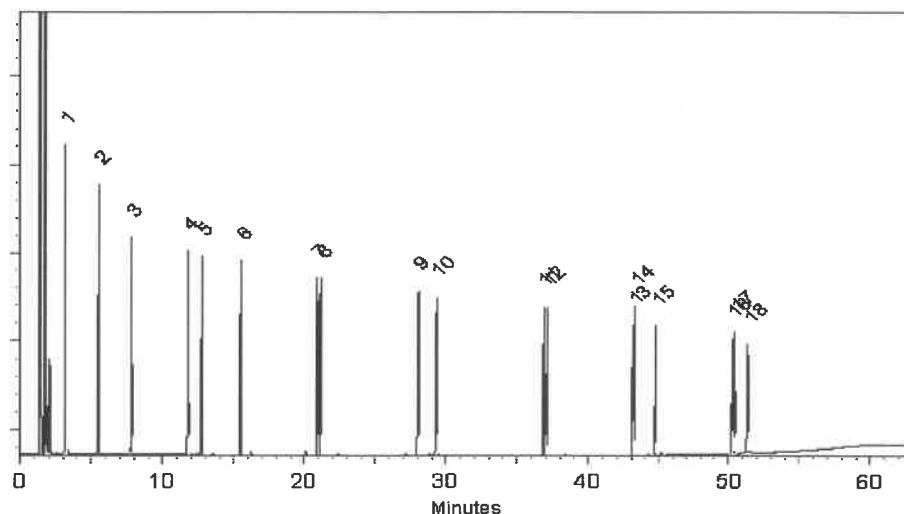

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*VenKelley*  
**Ven Kelley - Operations Tech I**

**Date Mixed:** 30-Dec-2024 **Balance Serial #** 1128360905

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 03-Jan-2025

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543

**Lot No.:** A0220580

**Description :** NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

**Container Size :** 5 mL

**Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2030

**Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive.

**Ship:** Ambient

P13916 } Y.P.  
↓  
P13935 } 08/06/25

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-39	98%	201.9 µg/mL	+/- 9.0961
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	RP241029RSR	98%	201.9 µg/mL	+/- 9.0961
5	Acenaphthene	83-32-9	MKCR7169	99%	200.4 µg/mL	+/- 9.0294
6	Fluorene	86-73-7	10246250	98%	201.9 µg/mL	+/- 9.0961
7	Phenanthrene	85-01-8	MKCT3391	99%	200.8 µg/mL	+/- 9.0474
8	Anthracene	120-12-7	MKCW9141	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCL8032	99%	201.6 µg/mL	+/- 9.0835
11	Benz(a)anthracene	56-55-3	I220012022BAA	99%	202.0 µg/mL	+/- 9.1015
12	Chrysene	218-01-9	RP240719RSR	99%	202.0 µg/mL	+/- 9.1015
13	Benzo(b)fluoranthene	205-99-2	SBS-BBF-FINAL-2	99%	202.0 µg/mL	+/- 9.1015
14	Benzo(k)fluoranthene	207-08-9	012022K	98%	201.5 µg/mL	+/- 9.0784
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0383

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	201.2 µg/mL	+/- 9.0655
18	Benzo(g,h,i)perylene	191-24-2	RP241014RSR	98%	200.3 µg/mL	+/- 9.0255

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

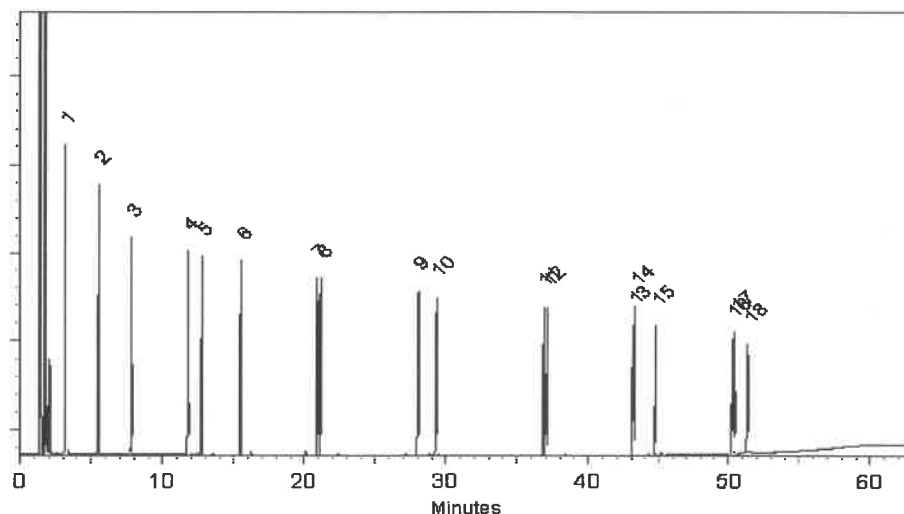

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*VenKelley*  
**Ven Kelley - Operations Tech I**

**Date Mixed:** 30-Dec-2024 **Balance Serial #** 1128360905

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 03-Jan-2025

**Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397**

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543

**Lot No.:** A0220580

**Description :** NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

**Container Size :** 5 mL

**Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2030

**Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive.

**Ship:** Ambient

P13916 } Y.P.  
↓  
P13935 } 08/06/25

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-39	98%	201.9 µg/mL	+/- 9.0961
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	RP241029RSR	98%	201.9 µg/mL	+/- 9.0961
5	Acenaphthene	83-32-9	MKCR7169	99%	200.4 µg/mL	+/- 9.0294
6	Fluorene	86-73-7	10246250	98%	201.9 µg/mL	+/- 9.0961
7	Phenanthrene	85-01-8	MKCT3391	99%	200.8 µg/mL	+/- 9.0474
8	Anthracene	120-12-7	MKCW9141	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCL8032	99%	201.6 µg/mL	+/- 9.0835
11	Benz(a)anthracene	56-55-3	I220012022BAA	99%	202.0 µg/mL	+/- 9.1015
12	Chrysene	218-01-9	RP240719RSR	99%	202.0 µg/mL	+/- 9.1015
13	Benzo(b)fluoranthene	205-99-2	SBS-BBF-FINAL-2	99%	202.0 µg/mL	+/- 9.1015
14	Benzo(k)fluoranthene	207-08-9	012022K	98%	201.5 µg/mL	+/- 9.0784
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0383

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	201.2 µg/mL	+/- 9.0655
18	Benzo(g,h,i)perylene	191-24-2	RP241014RSR	98%	200.3 µg/mL	+/- 9.0255

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

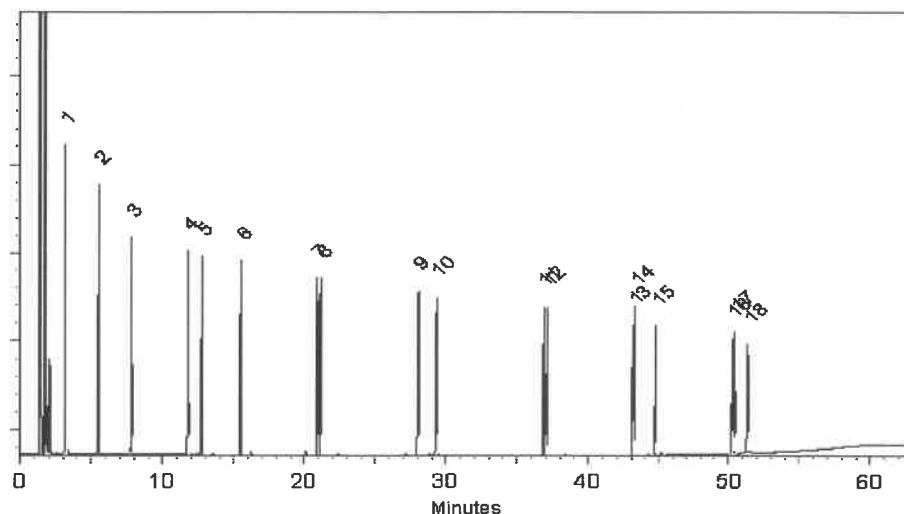

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*VenKelley*  
**Ven Kelley - Operations Tech I**

**Date Mixed:** 30-Dec-2024 **Balance Serial #** 1128360905

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 03-Jan-2025

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543

**Lot No.:** A0220580

**Description :** NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

**Container Size :** 5 mL

**Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2030

**Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive.

**Ship:** Ambient

P13916 } Y.P.  
↓  
P13935 } 08/06/25

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-39	98%	201.9 µg/mL	+/- 9.0961
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	RP241029RSR	98%	201.9 µg/mL	+/- 9.0961
5	Acenaphthene	83-32-9	MKCR7169	99%	200.4 µg/mL	+/- 9.0294
6	Fluorene	86-73-7	10246250	98%	201.9 µg/mL	+/- 9.0961
7	Phenanthrene	85-01-8	MKCT3391	99%	200.8 µg/mL	+/- 9.0474
8	Anthracene	120-12-7	MKCW9141	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCL8032	99%	201.6 µg/mL	+/- 9.0835
11	Benz(a)anthracene	56-55-3	I220012022BAA	99%	202.0 µg/mL	+/- 9.1015
12	Chrysene	218-01-9	RP240719RSR	99%	202.0 µg/mL	+/- 9.1015
13	Benzo(b)fluoranthene	205-99-2	SBS-BBF-FINAL-2	99%	202.0 µg/mL	+/- 9.1015
14	Benzo(k)fluoranthene	207-08-9	012022K	98%	201.5 µg/mL	+/- 9.0784
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0383

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	201.2 µg/mL	+/- 9.0655
18	Benzo(g,h,i)perylene	191-24-2	RP241014RSR	98%	200.3 µg/mL	+/- 9.0255

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

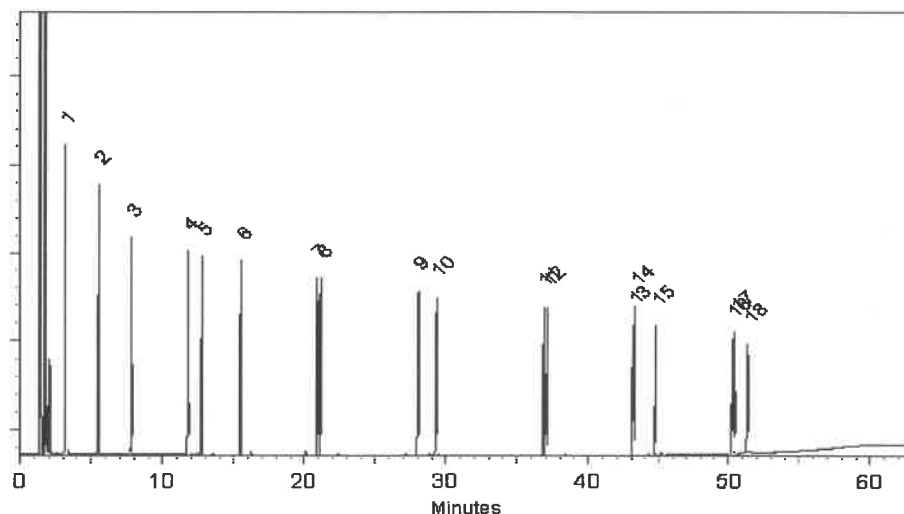

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*VenKelley*  
**Ven Kelley - Operations Tech I**

**Date Mixed:** 30-Dec-2024 **Balance Serial #** 1128360905

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 03-Jan-2025

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543

**Lot No.:** A0220580

**Description :** NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

**Container Size :** 5 mL

**Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2030

**Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive.

**Ship:** Ambient

P13916 } Y.P.  
↓  
P13935 } 08/06/25

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-39	98%	201.9 µg/mL	+/- 9.0961
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	RP241029RSR	98%	201.9 µg/mL	+/- 9.0961
5	Acenaphthene	83-32-9	MKCR7169	99%	200.4 µg/mL	+/- 9.0294
6	Fluorene	86-73-7	10246250	98%	201.9 µg/mL	+/- 9.0961
7	Phenanthrene	85-01-8	MKCT3391	99%	200.8 µg/mL	+/- 9.0474
8	Anthracene	120-12-7	MKCW9141	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCL8032	99%	201.6 µg/mL	+/- 9.0835
11	Benz(a)anthracene	56-55-3	I220012022BAA	99%	202.0 µg/mL	+/- 9.1015
12	Chrysene	218-01-9	RP240719RSR	99%	202.0 µg/mL	+/- 9.1015
13	Benzo(b)fluoranthene	205-99-2	SBS-BBF-FINAL-2	99%	202.0 µg/mL	+/- 9.1015
14	Benzo(k)fluoranthene	207-08-9	012022K	98%	201.5 µg/mL	+/- 9.0784
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0383

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	201.2 µg/mL	+/- 9.0655
18	Benzo(g,h,i)perylene	191-24-2	RP241014RSR	98%	200.3 µg/mL	+/- 9.0255

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

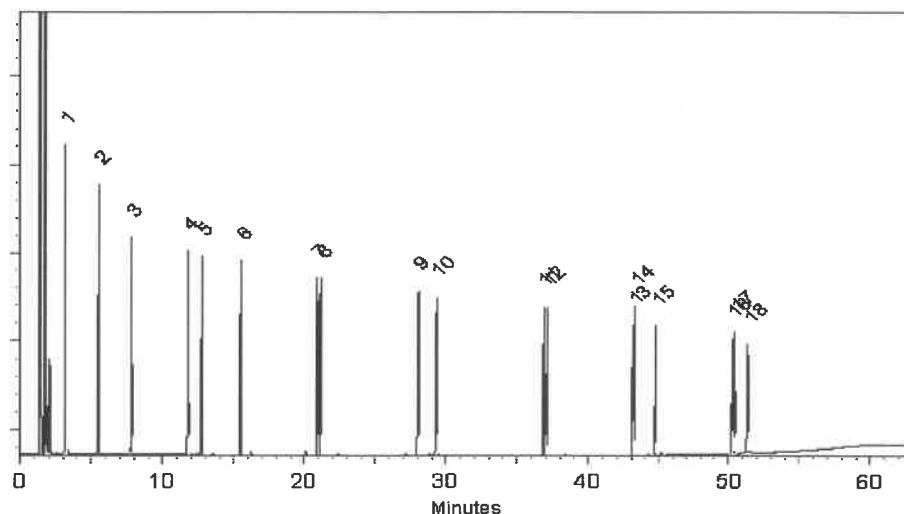

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*VenKelley*  
**Ven Kelley - Operations Tech I**

**Date Mixed:** 30-Dec-2024 **Balance Serial #** 1128360905

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 03-Jan-2025

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543

**Lot No.:** A0220580

**Description :** NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

**Container Size :** 5 mL

**Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2030

**Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive.

**Ship:** Ambient

P13916 } Y.P.  
↓  
P13935 } 08/06/25

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-39	98%	201.9 µg/mL	+/- 9.0961
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	RP241029RSR	98%	201.9 µg/mL	+/- 9.0961
5	Acenaphthene	83-32-9	MKCR7169	99%	200.4 µg/mL	+/- 9.0294
6	Fluorene	86-73-7	10246250	98%	201.9 µg/mL	+/- 9.0961
7	Phenanthrene	85-01-8	MKCT3391	99%	200.8 µg/mL	+/- 9.0474
8	Anthracene	120-12-7	MKCW9141	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCL8032	99%	201.6 µg/mL	+/- 9.0835
11	Benz(a)anthracene	56-55-3	I220012022BAA	99%	202.0 µg/mL	+/- 9.1015
12	Chrysene	218-01-9	RP240719RSR	99%	202.0 µg/mL	+/- 9.1015
13	Benzo(b)fluoranthene	205-99-2	SBS-BBF-FINAL-2	99%	202.0 µg/mL	+/- 9.1015
14	Benzo(k)fluoranthene	207-08-9	012022K	98%	201.5 µg/mL	+/- 9.0784
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0383

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	201.2 µg/mL	+/- 9.0655
18	Benzo(g,h,i)perylene	191-24-2	RP241014RSR	98%	200.3 µg/mL	+/- 9.0255

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

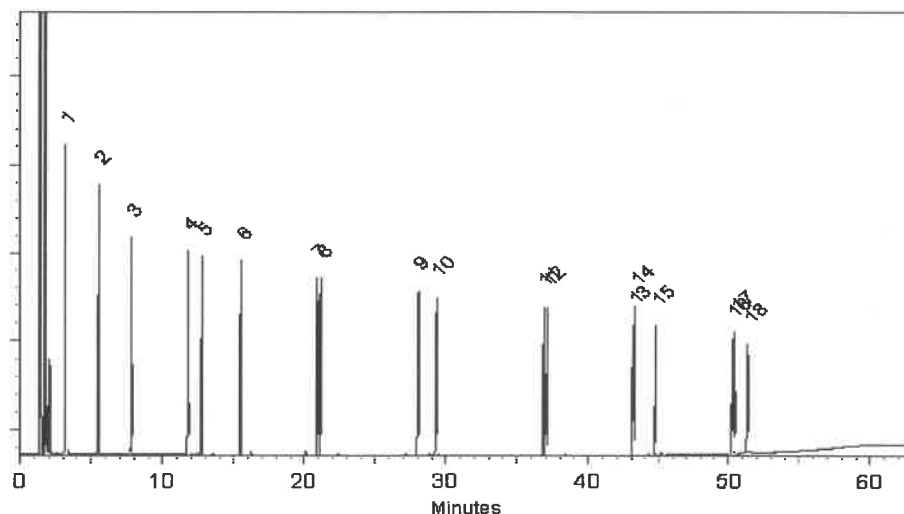

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*VenKelley*  
**Ven Kelley - Operations Tech I**

**Date Mixed:** 30-Dec-2024 **Balance Serial #** 1128360905

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 03-Jan-2025

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543

**Lot No.:** A0220580

**Description :** NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

**Container Size :** 5 mL

**Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2030

**Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive.

**Ship:** Ambient

P13916 } Y.P.  
↓  
P13935 } 08/06/25

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-39	98%	201.9 µg/mL	+/- 9.0961
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	RP241029RSR	98%	201.9 µg/mL	+/- 9.0961
5	Acenaphthene	83-32-9	MKCR7169	99%	200.4 µg/mL	+/- 9.0294
6	Fluorene	86-73-7	10246250	98%	201.9 µg/mL	+/- 9.0961
7	Phenanthrene	85-01-8	MKCT3391	99%	200.8 µg/mL	+/- 9.0474
8	Anthracene	120-12-7	MKCW9141	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCL8032	99%	201.6 µg/mL	+/- 9.0835
11	Benz(a)anthracene	56-55-3	I220012022BAA	99%	202.0 µg/mL	+/- 9.1015
12	Chrysene	218-01-9	RP240719RSR	99%	202.0 µg/mL	+/- 9.1015
13	Benzo(b)fluoranthene	205-99-2	SBS-BBF-FINAL-2	99%	202.0 µg/mL	+/- 9.1015
14	Benzo(k)fluoranthene	207-08-9	012022K	98%	201.5 µg/mL	+/- 9.0784
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0383

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	201.2 µg/mL	+/- 9.0655
18	Benzo(g,h,i)perylene	191-24-2	RP241014RSR	98%	200.3 µg/mL	+/- 9.0255

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

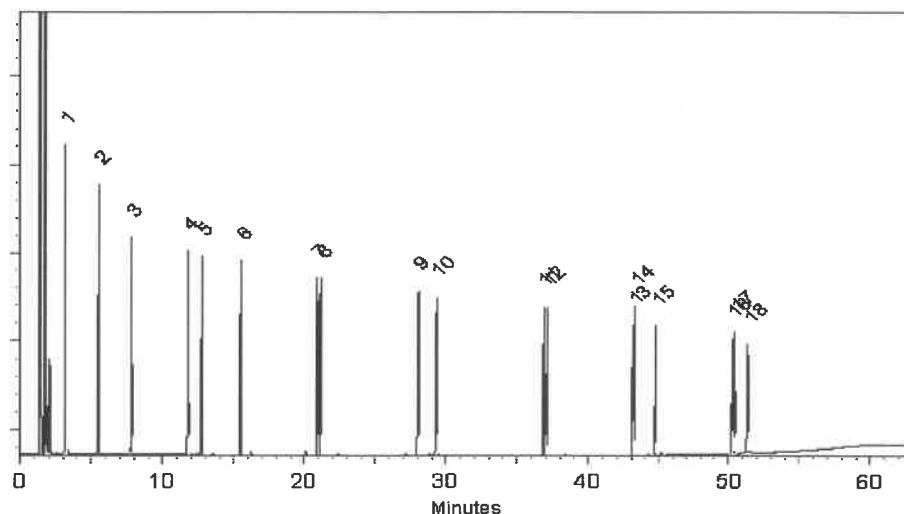

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*VenKelley*  
**Ven Kelley - Operations Tech I**

**Date Mixed:** 30-Dec-2024 **Balance Serial #** 1128360905

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 03-Jan-2025

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



**FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.**

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31480 **Lot No.:** A0219106  
**Description :** MA Fractionation Surrogate Spike Mix  
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** October 31, 2030 **Storage:** 10°C or colder  
**Handling:** Sonication required. Mix is **Ship:** Ambient  
photosensitive.

p13947  
L  
p1395h

**CERTIFIED VALUES**

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,013.5 µg/mL	+/- 180.7988
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,011.0 µg/mL	+/- 180.6862

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-S (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

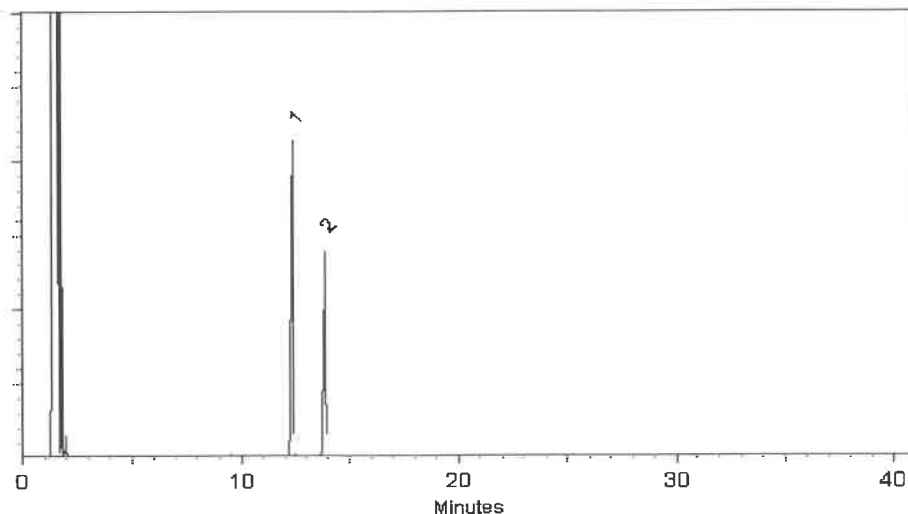

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Wilner Torres*  
Wilner Torres - Operation Tech I

Date Mixed: 14-Nov-2024

Balance Serial # 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 20-Nov-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31480 **Lot No.:** A0219106  
**Description :** MA Fractionation Surrogate Spike Mix  
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** October 31, 2030 **Storage:** 10°C or colder  
**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

P13947  
L  
P13954

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,013.5 µg/mL	+/- 180.7988
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,011.0 µg/mL	+/- 180.6862

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-S (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

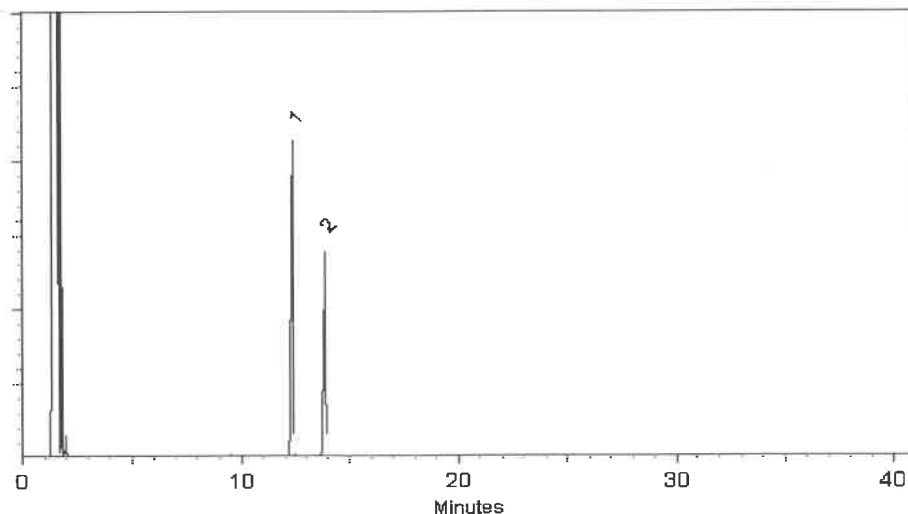

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Wilner Torres*  
Wilner Torres - Operation Tech I

Date Mixed: 14-Nov-2024

Balance Serial # 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 20-Nov-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



**FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.**

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31480 **Lot No.:** A0219106  
**Description :** MA Fractionation Surrogate Spike Mix  
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** October 31, 2030 **Storage:** 10°C or colder  
**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

p13947  
L  
p1395h

**CERTIFIED VALUES**

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,013.5 µg/mL	+/- 180.7988
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,011.0 µg/mL	+/- 180.6862

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-S (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

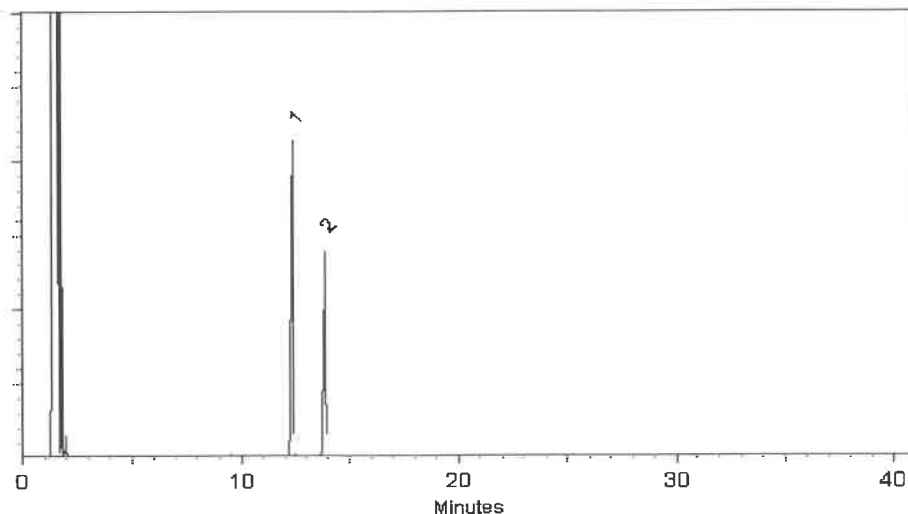

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Wilner Torres*  
Wilner Torres - Operation Tech I

Date Mixed: 14-Nov-2024

Balance Serial # 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 20-Nov-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31480 **Lot No.:** A0219106  
**Description :** MA Fractionation Surrogate Spike Mix  
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** October 31, 2030 **Storage:** 10°C or colder  
**Handling:** Sonication required. Mix is **Ship:** Ambient  
photosensitive.

p13947  
L  
p1395h

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,013.5 µg/mL	+/- 180.7988
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,011.0 µg/mL	+/- 180.6862

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-S (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

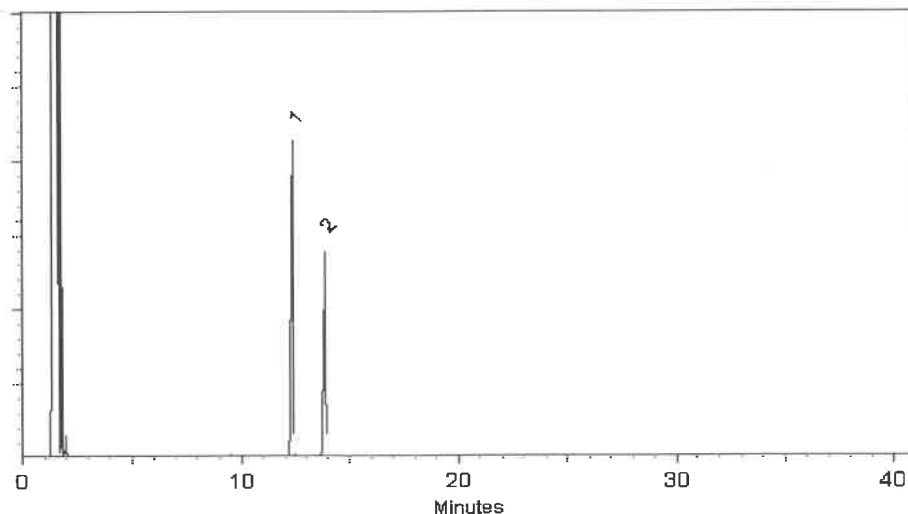

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Wilner Torres*  
Wilner Torres - Operation Tech I

Date Mixed: 14-Nov-2024

Balance Serial # 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 20-Nov-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31480 **Lot No.:** A0219106  
**Description :** MA Fractionation Surrogate Spike Mix  
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** October 31, 2030 **Storage:** 10°C or colder  
**Handling:** Sonication required. Mix is **Ship:** Ambient  
photosensitive.

P13947  
L  
P13954

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,013.5 µg/mL	+/- 180.7988
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,011.0 µg/mL	+/- 180.6862

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-S (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

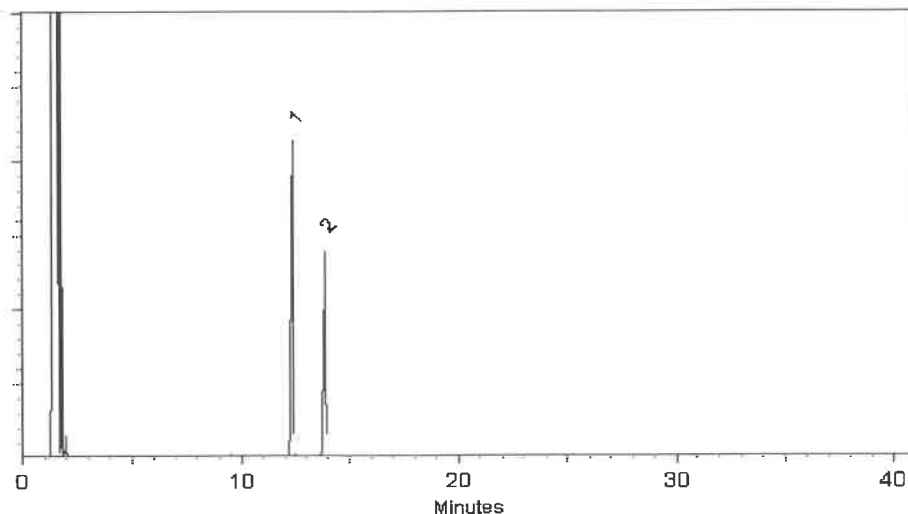

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Wilner Torres*  
Wilner Torres - Operation Tech I

Date Mixed: 14-Nov-2024

Balance Serial # 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 20-Nov-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31480 **Lot No.:** A0219106  
**Description :** MA Fractionation Surrogate Spike Mix  
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** October 31, 2030 **Storage:** 10°C or colder  
**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

P13947  
L  
P13954

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,013.5 µg/mL	+/- 180.7988
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,011.0 µg/mL	+/- 180.6862

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-S (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

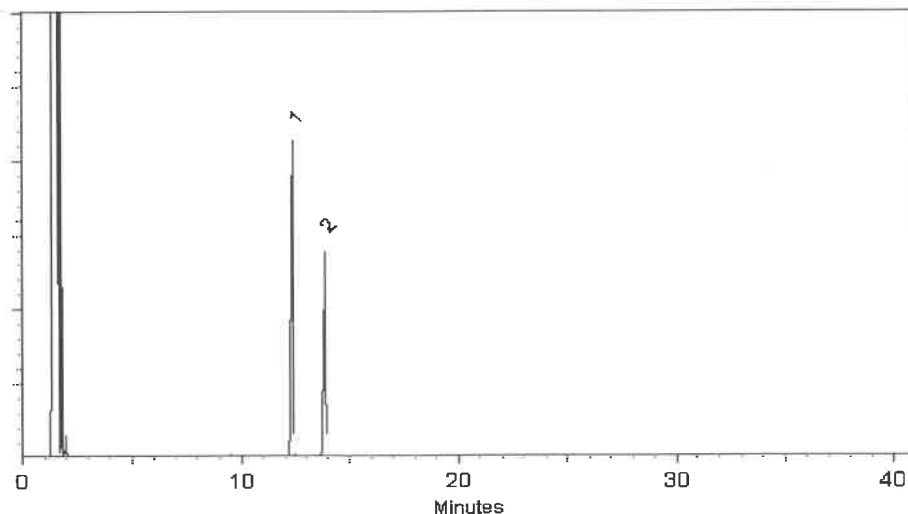

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Wilner Torres*  
Wilner Torres - Operation Tech I

Date Mixed: 14-Nov-2024

Balance Serial # 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 20-Nov-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31480 **Lot No.:** A0219106  
**Description :** MA Fractionation Surrogate Spike Mix  
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** October 31, 2030 **Storage:** 10°C or colder  
**Handling:** Sonication required. Mix is **Ship:** Ambient  
photosensitive.

P13947  
L  
P13954

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,013.5 µg/mL	+/- 180.7988
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,011.0 µg/mL	+/- 180.6862

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-S (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

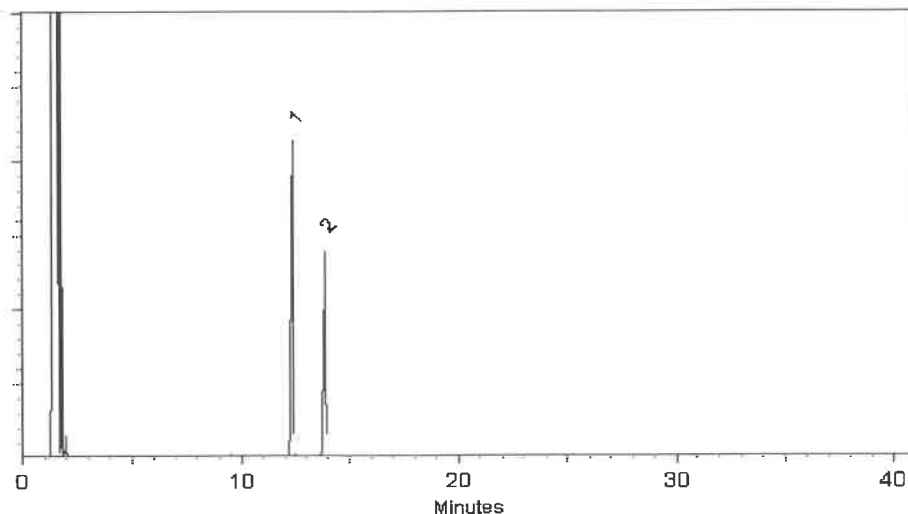

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Wilner Torres*  
Wilner Torres - Operation Tech I

Date Mixed: 14-Nov-2024

Balance Serial # 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 20-Nov-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31480 **Lot No.:** A0221895  
**Description :** MA Fractionation Surrogate Spike Mix  
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** January 31, 2031 **Storage:** 10°C or colder  
**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

P1395  
↓  
P13966.

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,032.5 µg/mL	+/- 181.6547
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,033.0 µg/mL	+/- 181.6772

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

# Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

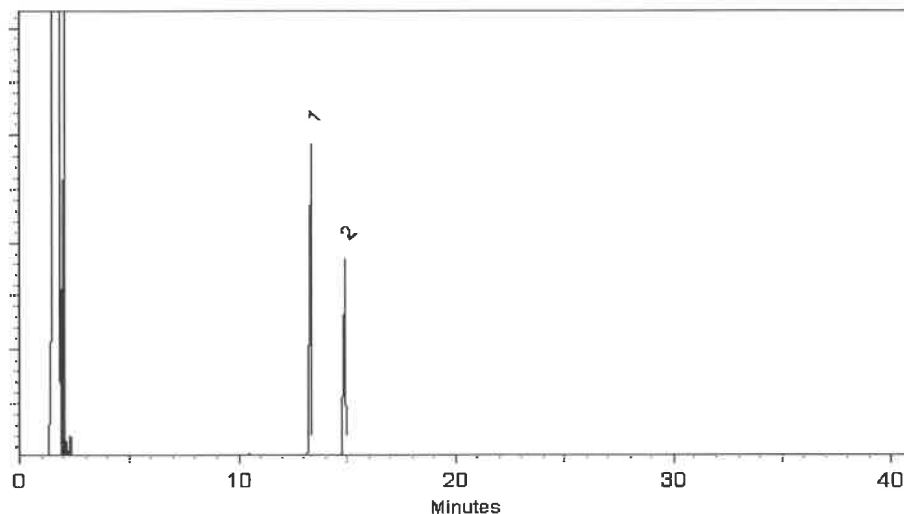

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ven Kelley - Operations Tech I

Date Mixed: 04-Feb-2025

Balance Serial # 1128360905

Dillan Murphy - Operations Technician I

Date Passed: 12-Feb-2025

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



n-Hexane 95%  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis



Material No.: 9262-03  
Batch No.: 24G1962003  
Manufactured Date: 2024-05-23  
Expiration Date: 2025-08-22  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	$\leq 10$	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	$\leq 5$	1
Assay (Total Saturated C <sub>6</sub> Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	98 %
Color (APHA)	$\leq 10$	5
Residue after Evaporation	$\leq 1.0$ ppm	0.1 ppm
Substances Darkened by H <sub>2</sub> SO <sub>4</sub>	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Croak  
Director Quality Operations, Bioscience Production