
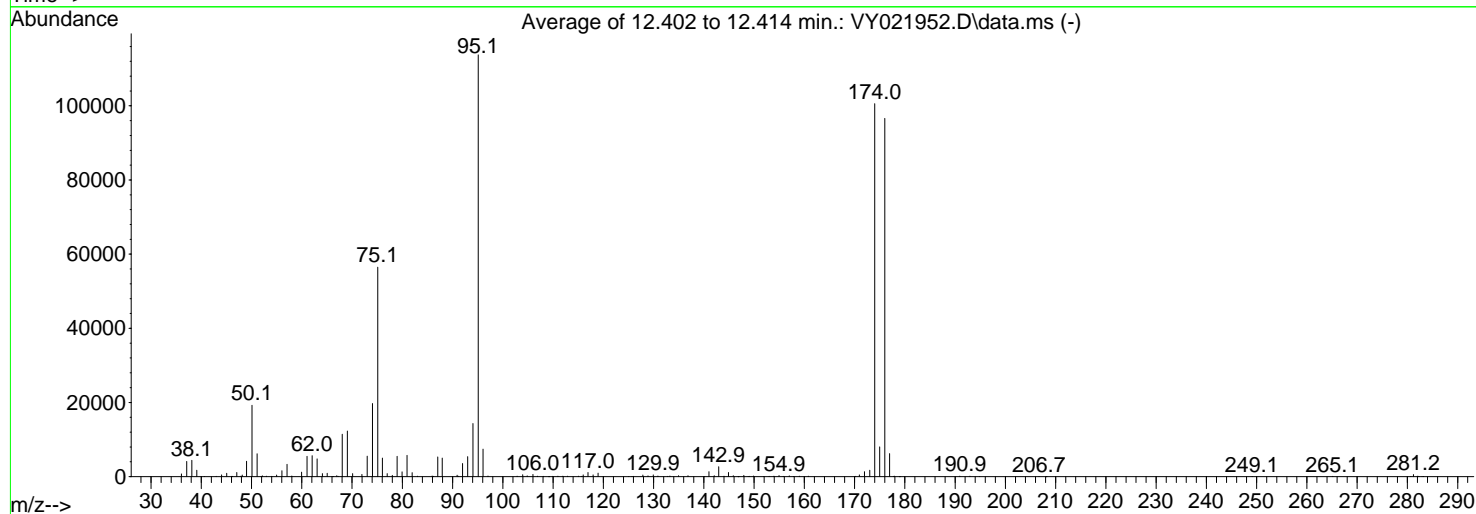


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY042225\  
 Data File : VY021952.D  
 Acq On : 22 Apr 2025 11:33  
 Operator : SY/MD  
 Sample : BFB  
 Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y042225S.M  
 Title : SW846 8260  
 Last Update : Wed Apr 23 02:30:30 2025

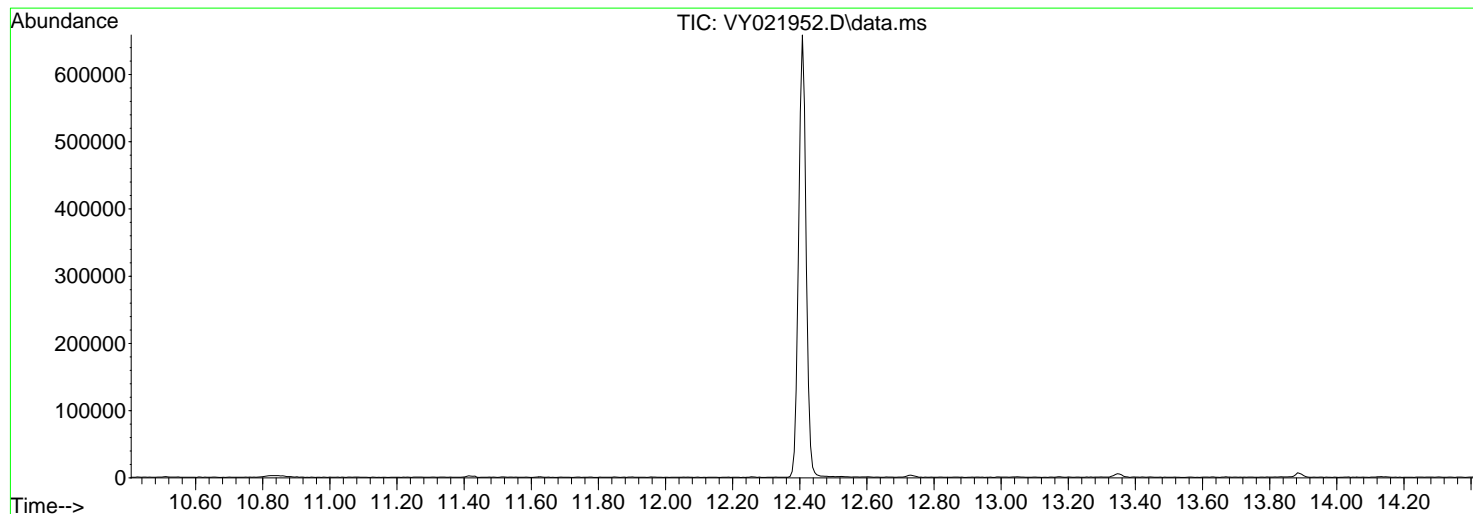

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	19237	PASS
75	95	30	60	49.7	56504	PASS
95	95	100	100	100.0	113749	PASS
96	95	5	9	6.5	7410	PASS
173	174	0.00	2	1.7	1741	PASS
174	95	50	100	88.4	100587	PASS
175	174	5	9	8.0	8046	PASS
176	174	95	101	96.1	96621	PASS
177	176	5	9	6.4	6205	PASS