

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042925\
 Data File : P0110858.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2025 14:12
 Operator : YP/AJ
 Sample : Q1903-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 02:25:18 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0041025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 11 02:12:41 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.685	3.682	209.4E6	108.7E6	23.930	21.776
2) SA Decachlor...	8.727	8.678	158.7E6	38386838	20.106	19.941

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO042925\
Data File : PO110858.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2025 14:12
Operator : YP/AJ
Sample : Q1903-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
COMP-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 02:25:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO041025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 11 02:12:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

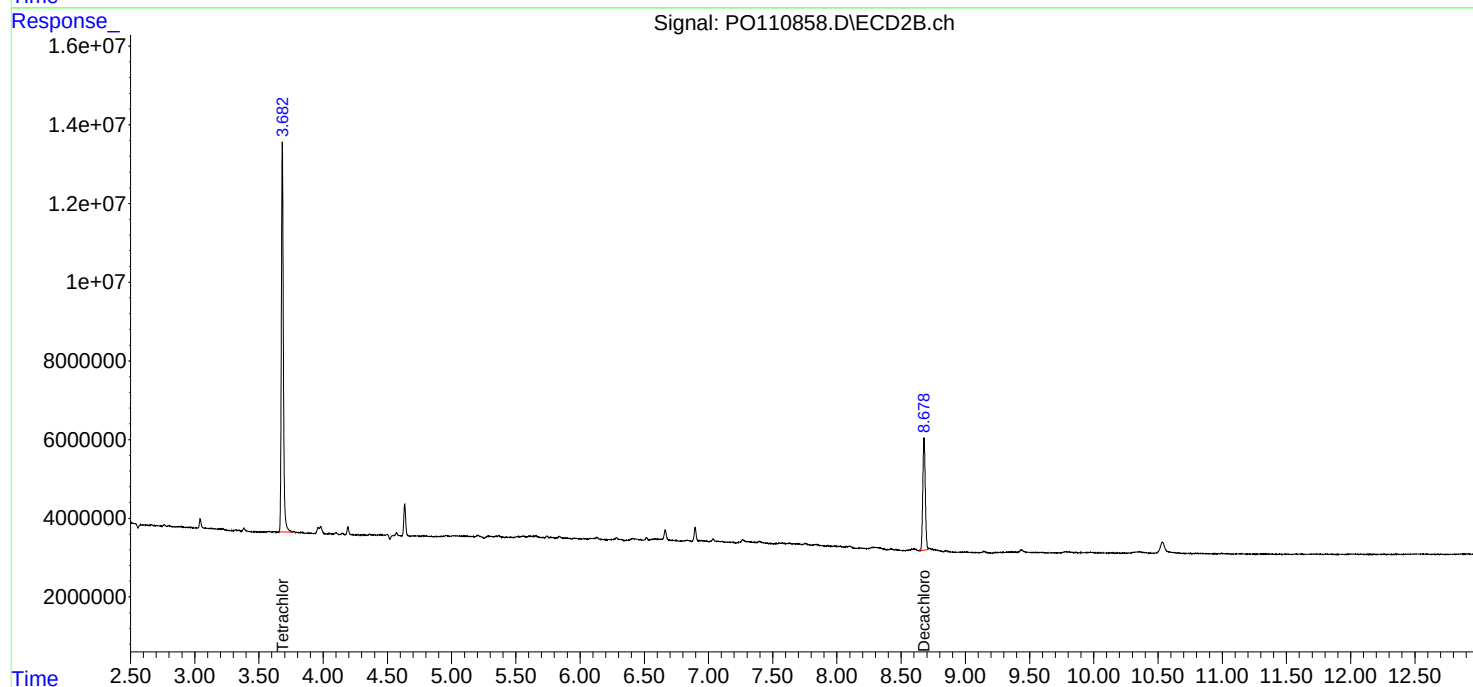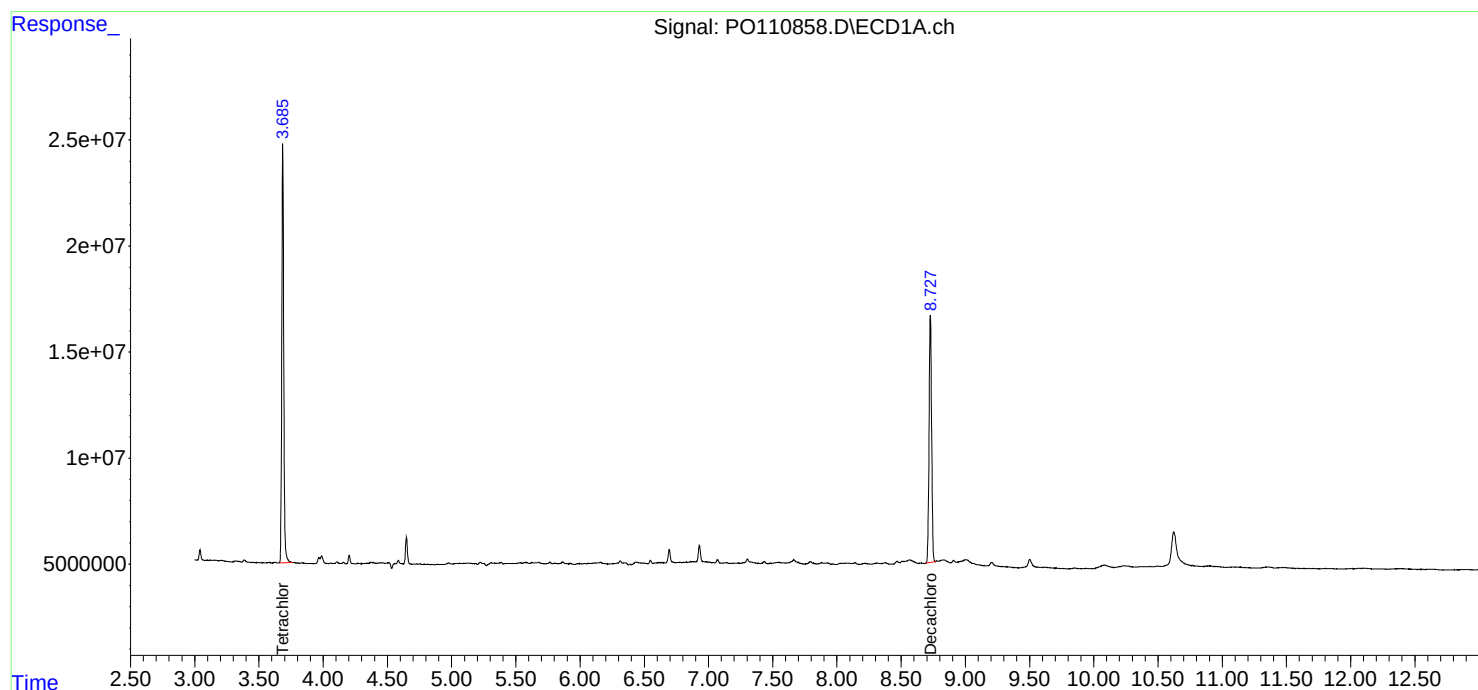


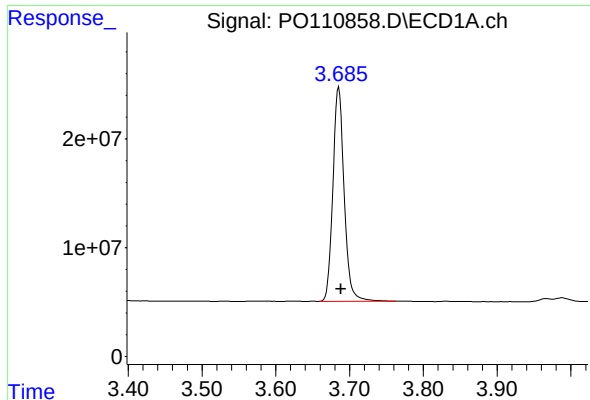

#1 Tetrachloro-m-xylene


R.T.: 3.685 min
Delta R.T.: -0.003 min
Response: 209367041
Conc: 23.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-4

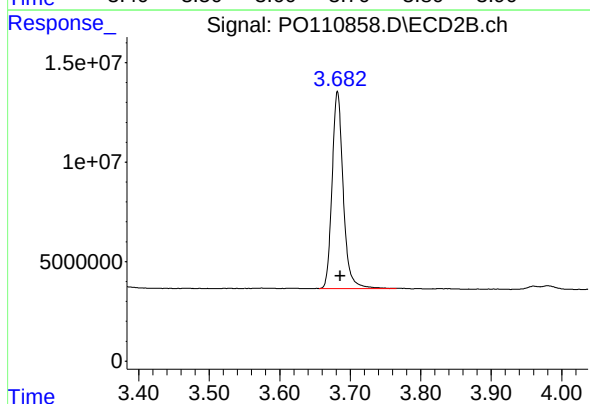


#1 Tetrachloro-m-xylene

R.T.: 3.682 min
Delta R.T.: -0.004 min
Response: 108659232
Conc: 21.78 ng/ml

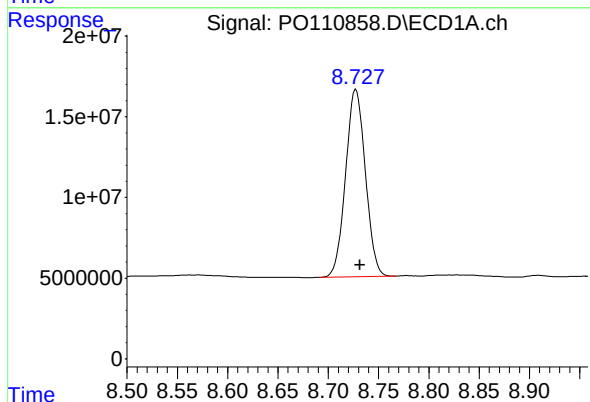

#2 Decachlorobiphenyl

R.T.: 8.727 min
Delta R.T.: -0.004 min
Response: 158734565
Conc: 20.11 ng/ml

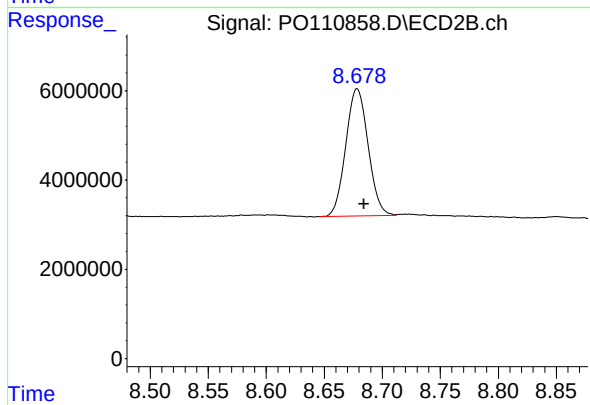

#2 Decachlorobiphenyl

R.T.: 8.678 min
Delta R.T.: -0.006 min
Response: 38386838
Conc: 19.94 ng/ml