


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050125\
Data File : BP024485.D
Acq On : 01 May 2025 09:57
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 18 12:04:48 2025

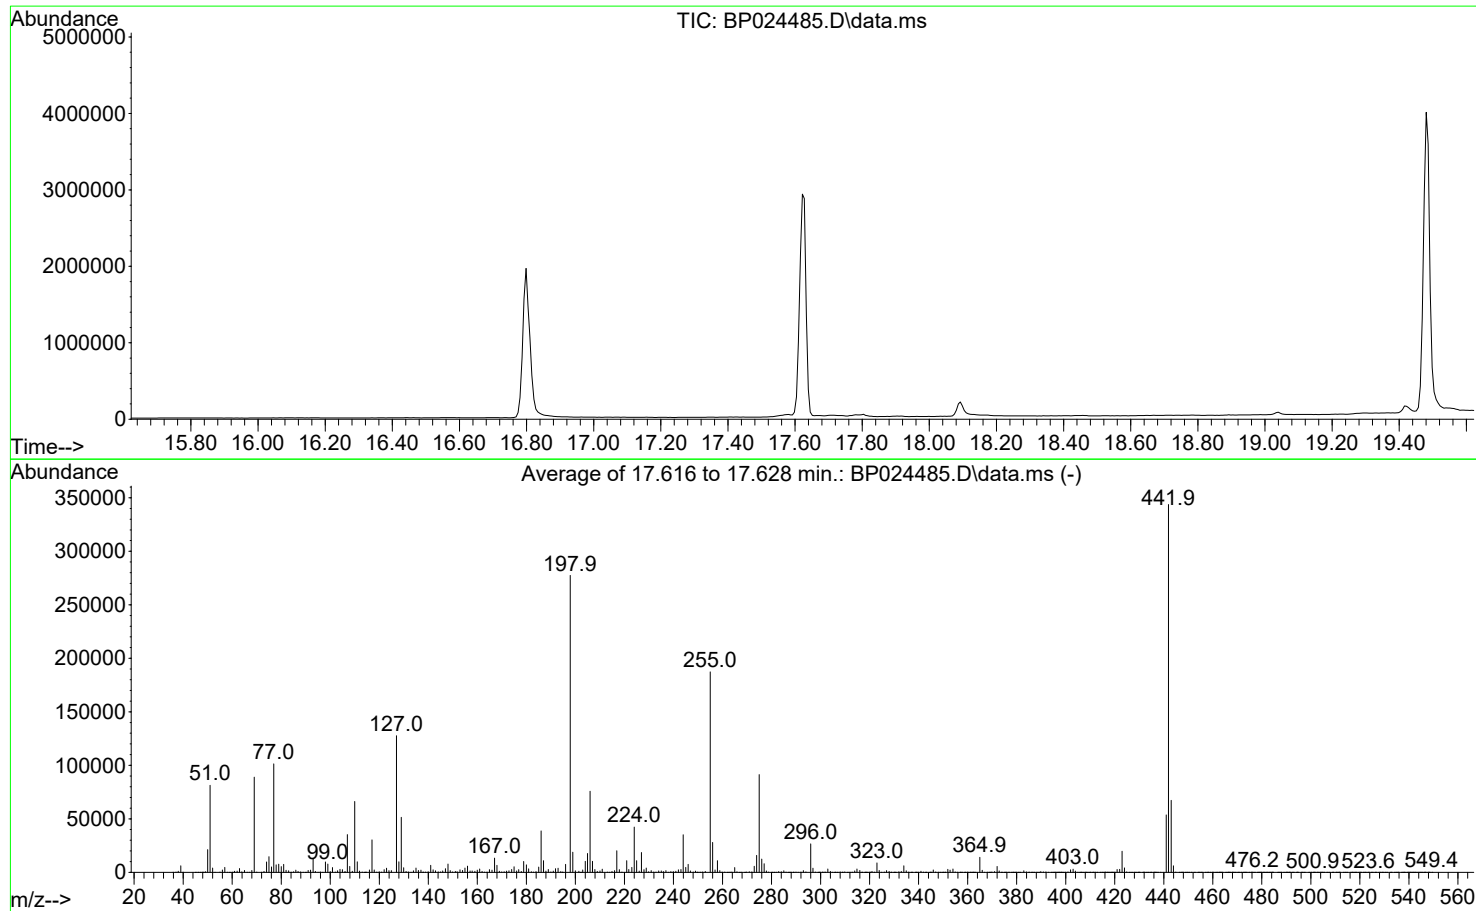

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.3	81389	PASS
68	69	0.00	2	2.0	1760	PASS
69	198	0.00	100	32.1	89017	PASS
70	69	0.00	2	0.3	263	PASS
127	198	10	80	46.0	127653	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	277445	PASS
199	198	5	9	6.8	18837	PASS
275	198	10	60	32.9	91363	PASS
365	198	1	100	5.1	14133	PASS
441	198	0.01	100	19.3	53685	PASS
442	442	100	100	100.0	343720	PASS
443	442	15	24	19.6	67272	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/1/2025	BNA_P	<u>BP024485.D</u>
Compound Name	Response	Retention Time
DDT	1029568	20.763
DDD	20115	20.369
DDE	1747	19.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21862	1051430	2.08

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050125\
Data File : BP024485.D
Acq On : 01 May 2025 09:57
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 01 12:07:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

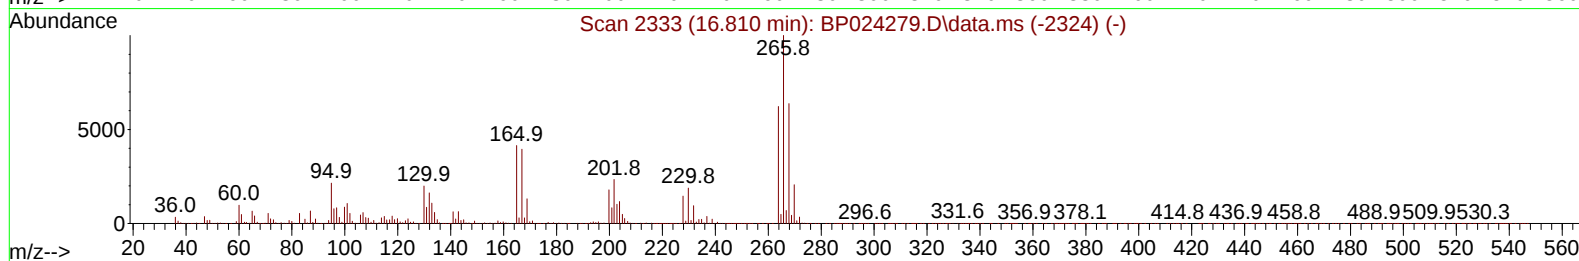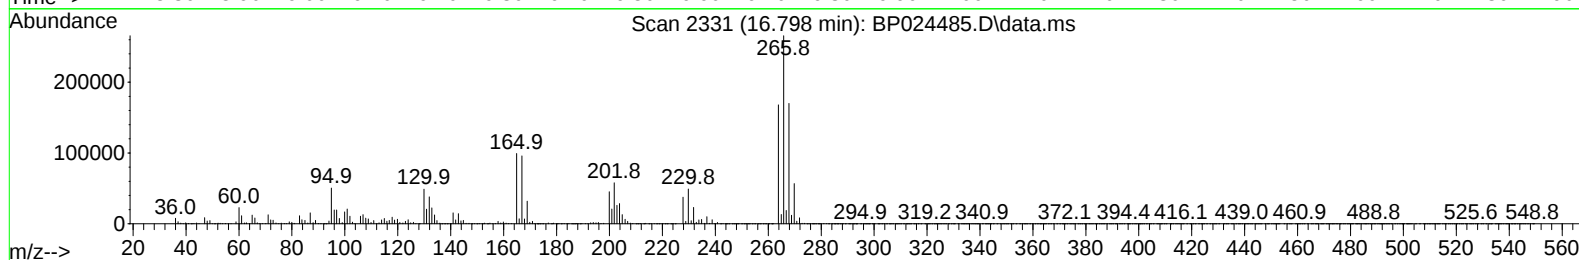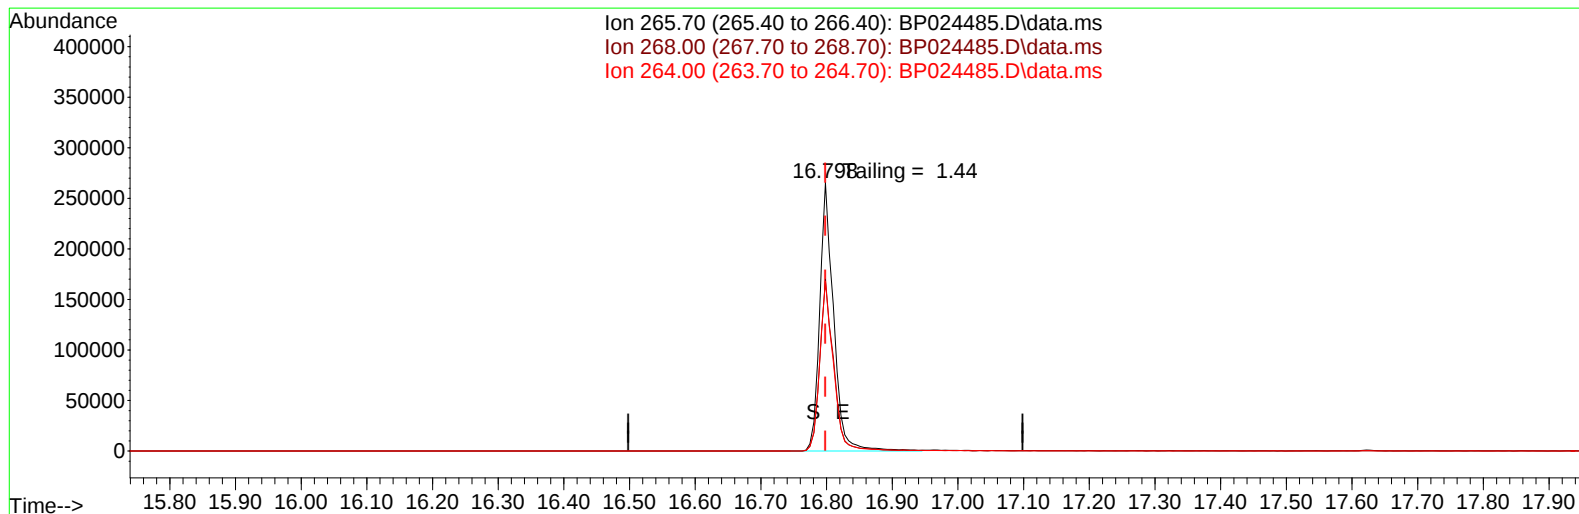

TIC: BP024485.D\data.ms

(70) Pentachlorophenol (C)

16.798min (+ 0.000) 32510.41 ng




response 391723

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.04
264.00	62.20	63.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050125\
Data File : BP024485.D
Acq On : 01 May 2025 09:57
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 01 12:07:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

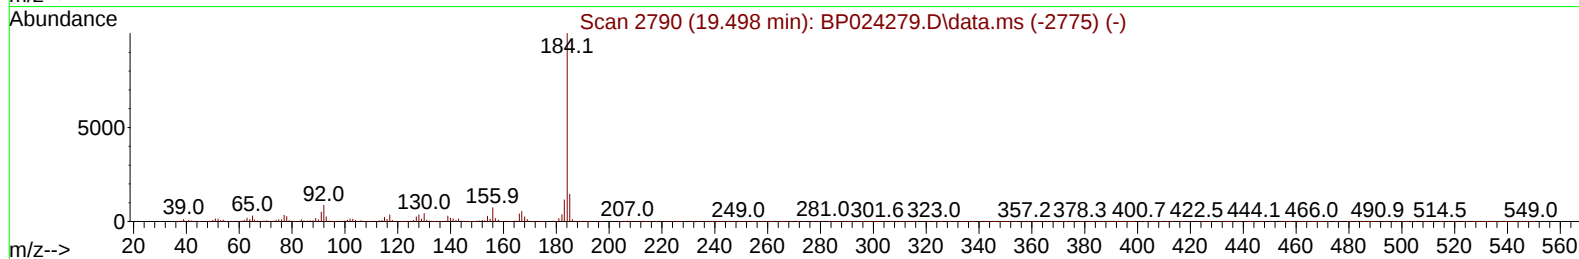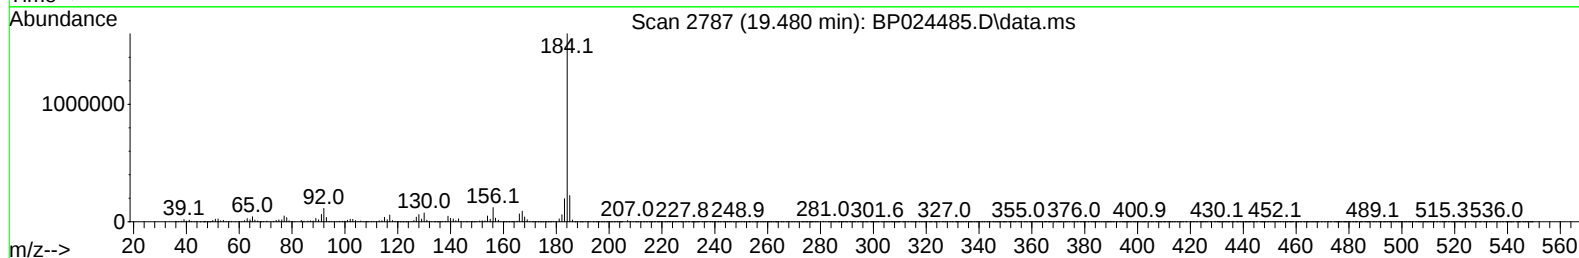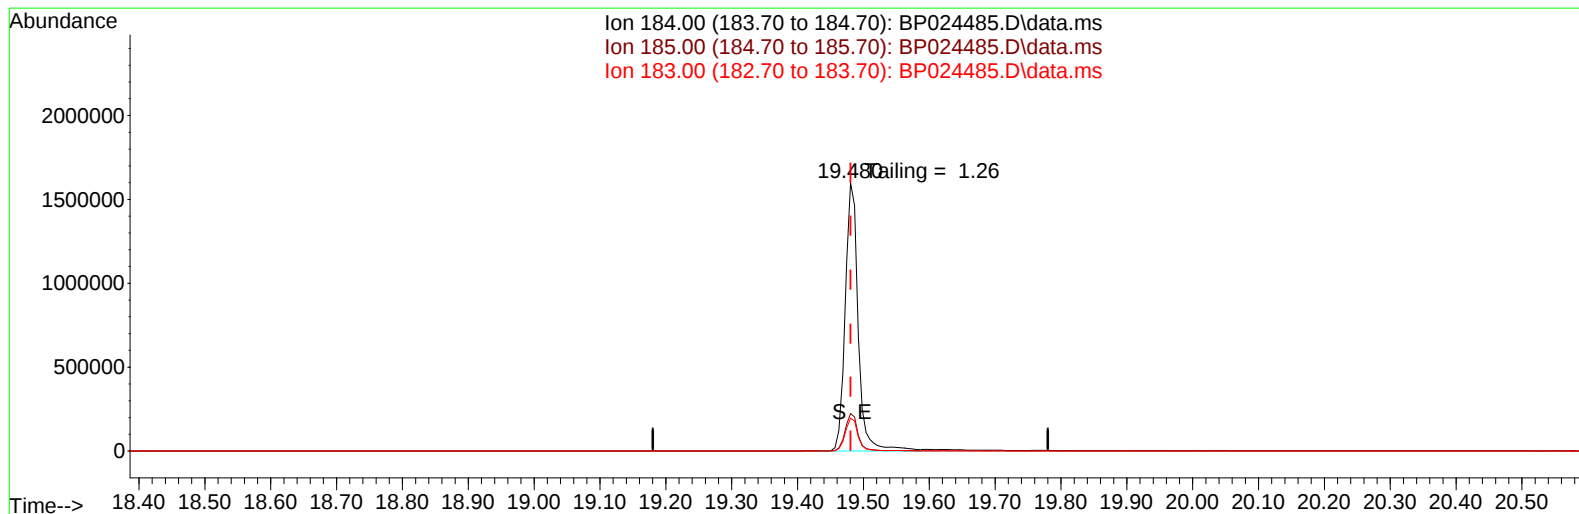

TIC: BP024485.D\data.ms

(77) Benzidine

19.480min (+ 0.000) 35967.83 ng

response 2183414

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.97
183.00	11.50	12.25
0.00	0.00	0.00