
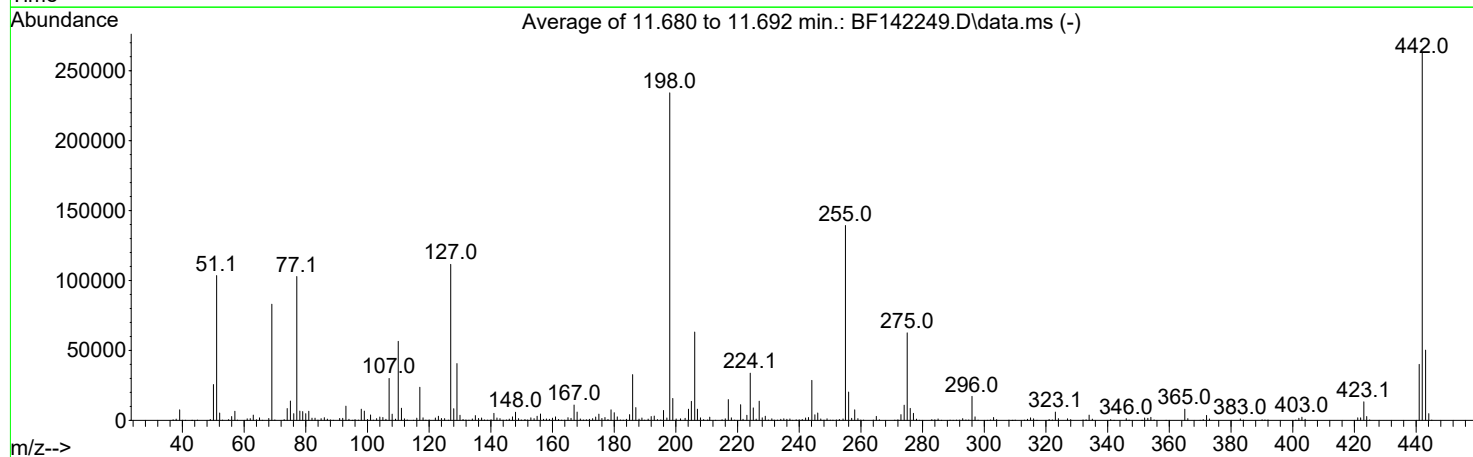


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050125\
Data File : BF142249.D
Acq On : 01 May 2025 09:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 30 16:00:01 2025

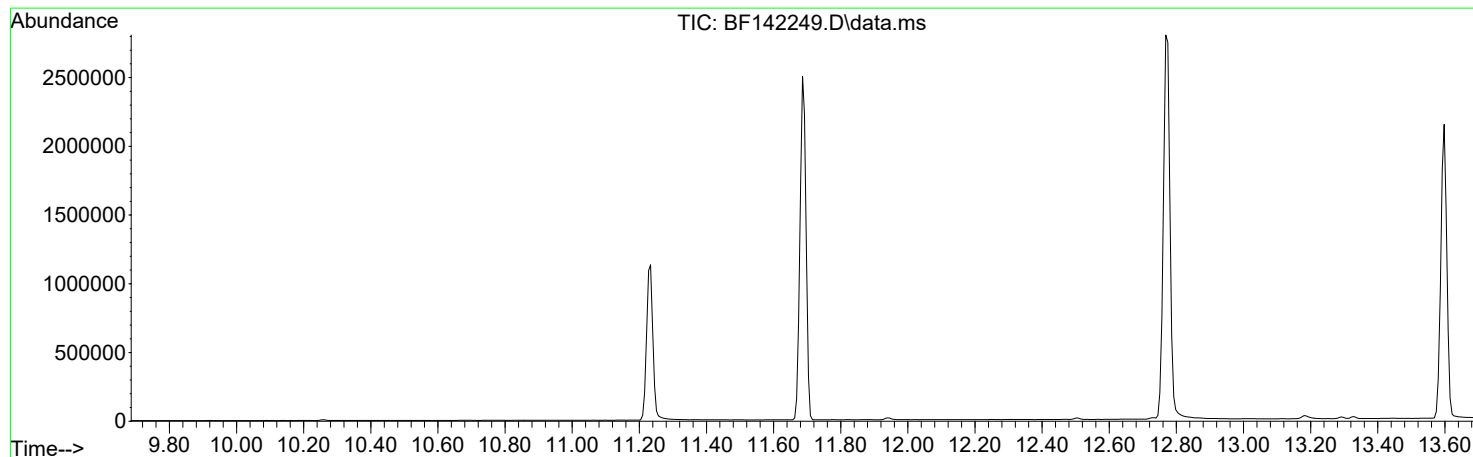

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.2	103579	PASS
68	69	0.00	2	1.6	1339	PASS
69	198	0.00	100	35.5	83059	PASS
70	69	0.00	2	0.5	413	PASS
127	198	10	80	47.7	111579	PASS
197	198	0.00	2	0.7	1704	PASS
198	198	100	100	100.0	234155	PASS
199	198	5	9	6.7	15632	PASS
275	198	10	60	26.7	62555	PASS
365	198	1	100	3.4	8074	PASS
441	198	0.01	100	17.1	40008	PASS
442	442	50	100	100.0	263019	PASS
443	442	15	24	19.1	50208	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/1/2025	BNA_F	<u>BF142249.D</u>
Compound Name	Response	Retention Time
DDT	427368	13.598
DDD	6172	13.327
DDE	0	12.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6172	433540	1.42

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050125\
Data File : BF142249.D
Acq On : 01 May 2025 09:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 01 12:00:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 30 16:00:01 2025
Response via : Initial Calibration

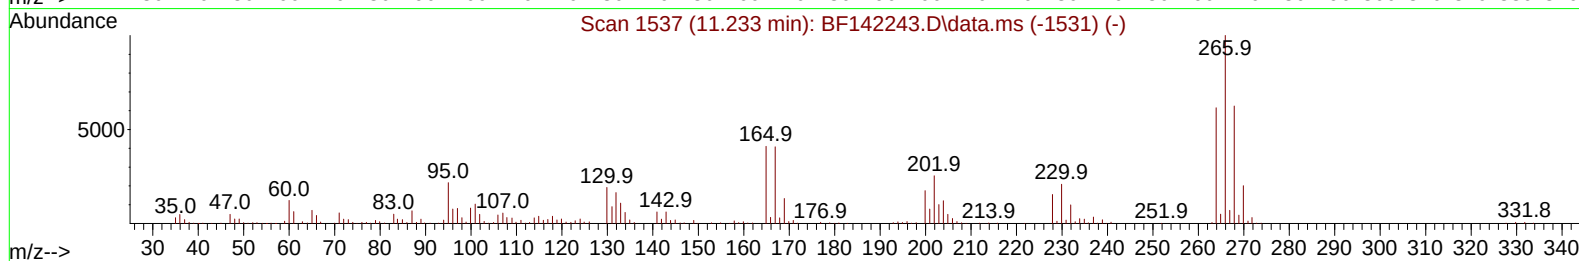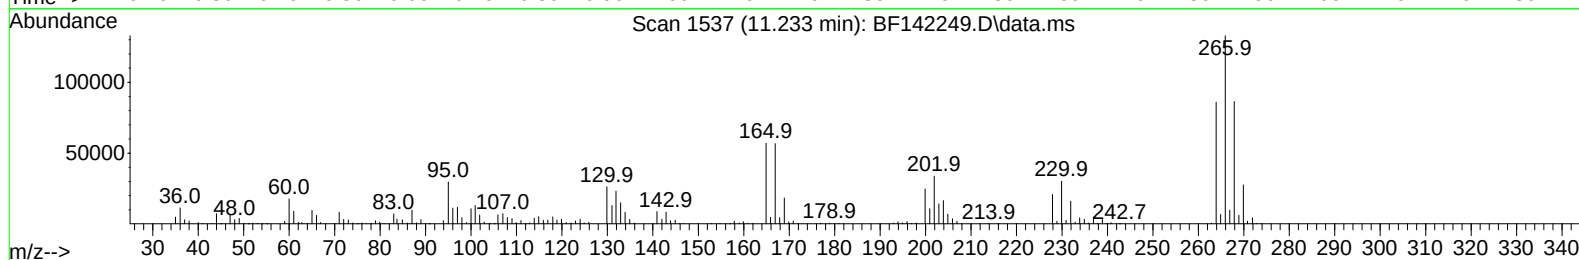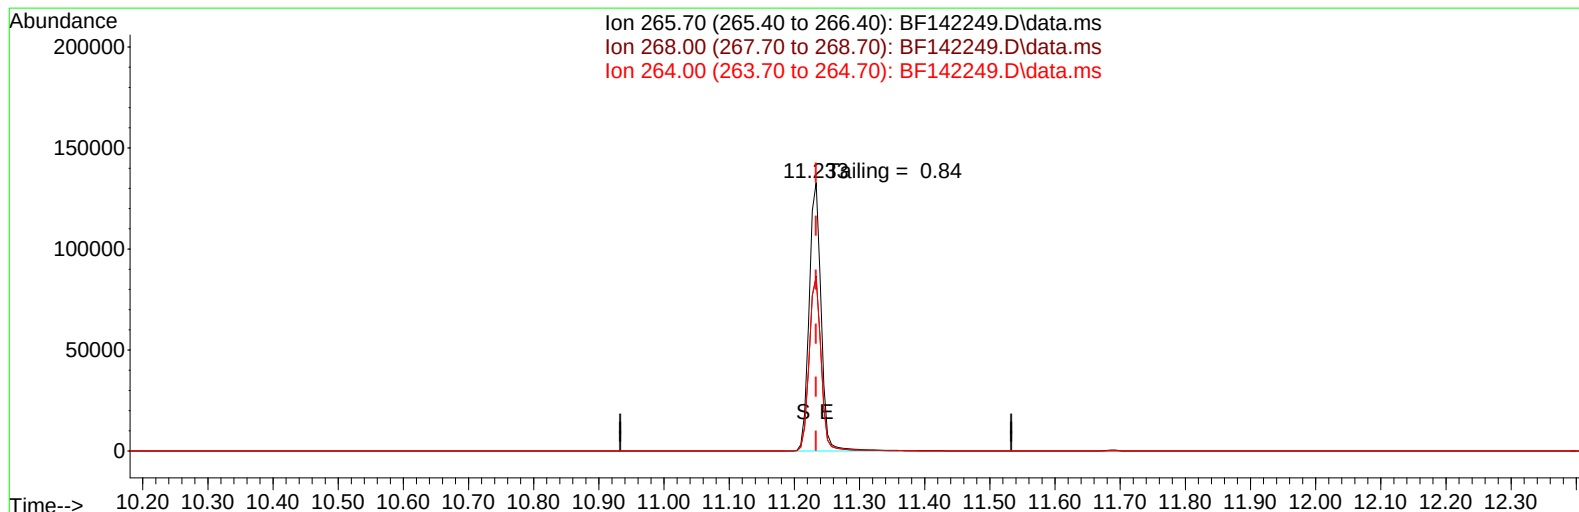

TIC: BF142249.D\data.ms

(70) Pentachlorophenol (C)

11.233min (+ 0.000) 113470.87 ng




response 170474

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	65.06
264.00	61.60	64.75
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050125\  
Data File : BF142249.D  
Acq On    : 01 May 2025  09:48  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 01 12:00:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 30 16:00:01 2025
Response via : Initial Calibration

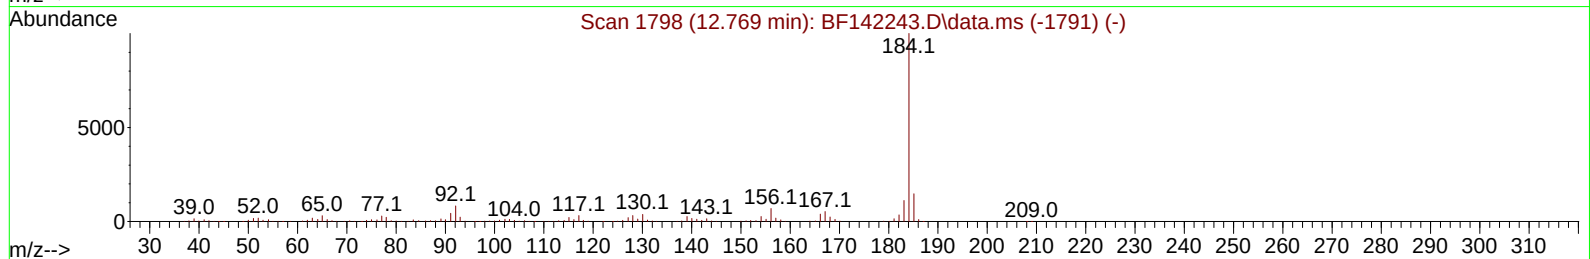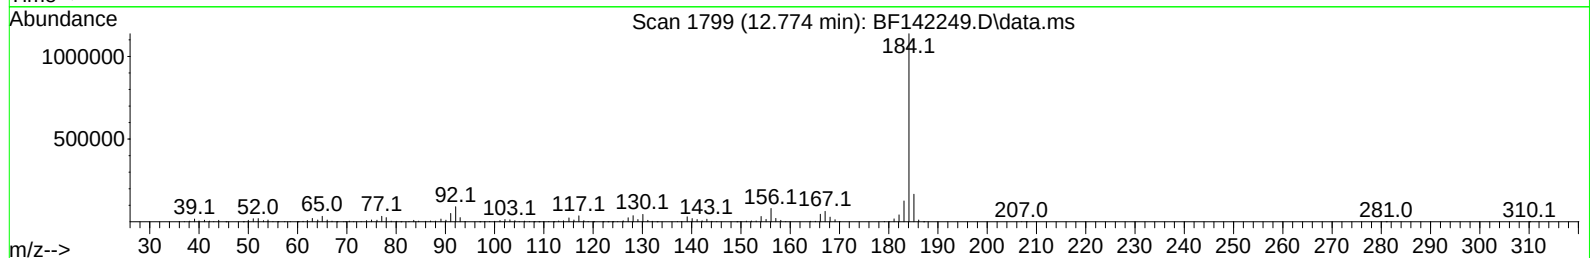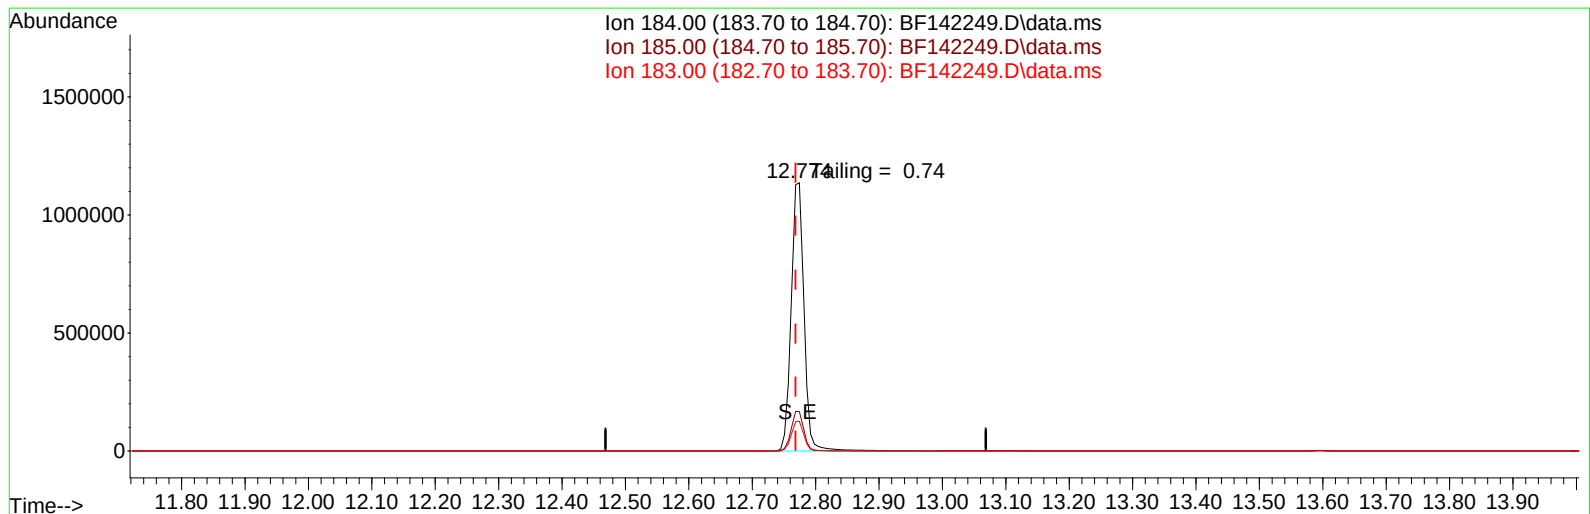

TIC: BF142249.D\data.ms

(77) Benzidine

12.774min (+ 0.006) 156734.40 ng

```
response      1611689
```

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.68
183.00	11.10	11.08
0.00	0.00	0.00