


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050125\
Data File : BM050061.D
Acq On : 01 May 2025 12:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 28 18:09:16 2025

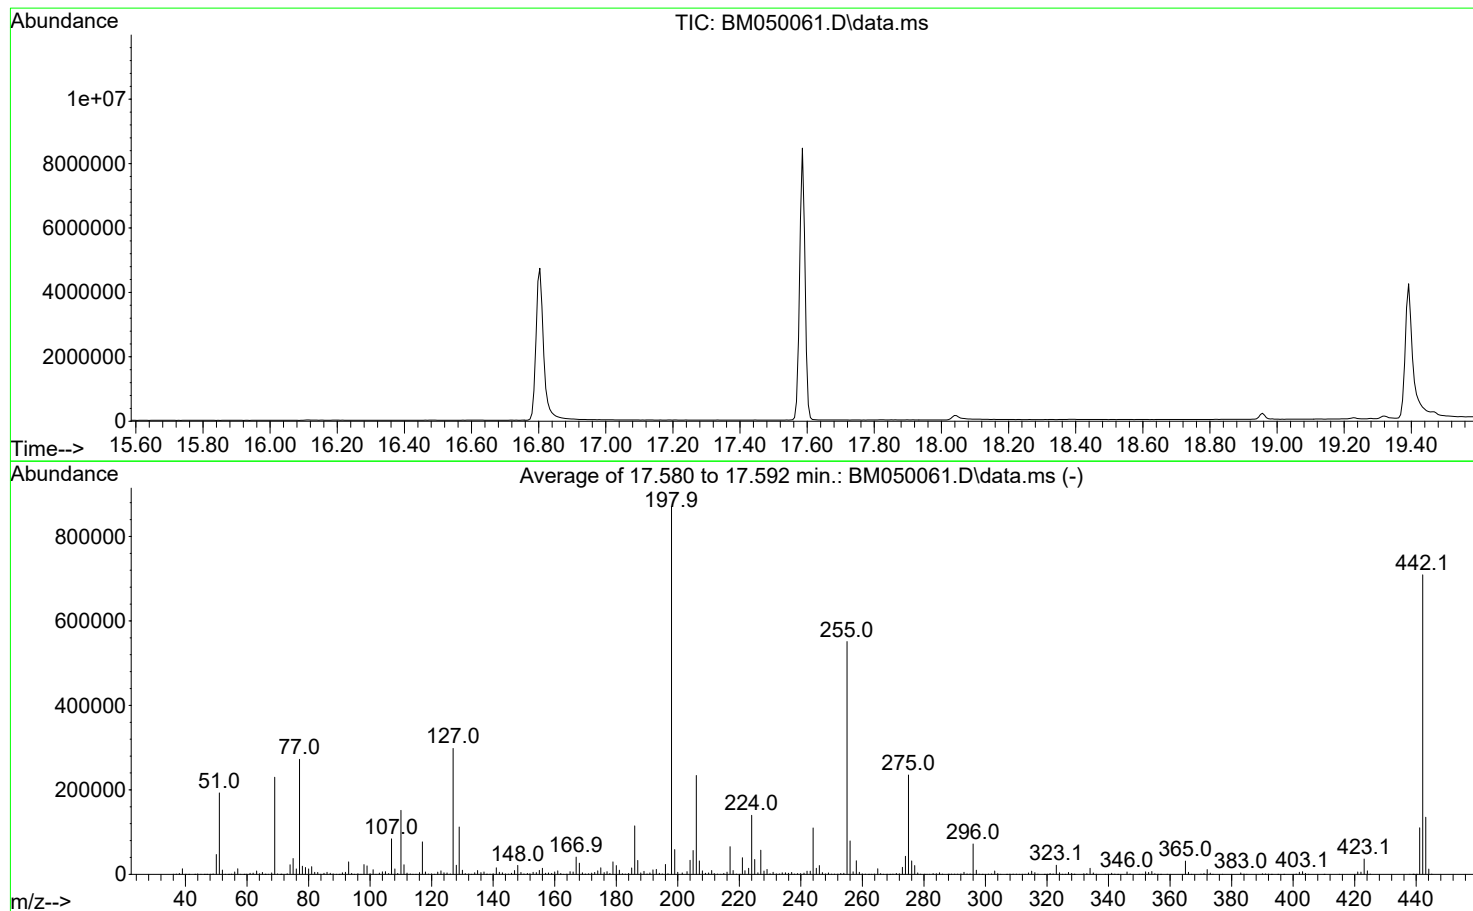

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.1	192815	PASS
68	69	0.00	2	1.5	3449	PASS
69	198	0.00	100	26.4	230047	PASS
70	69	0.00	2	0.4	961	PASS
127	198	10	80	34.3	298304	PASS
197	198	0.00	2	0.2	1539	PASS
198	198	100	100	100.0	870933	PASS
199	198	5	9	6.7	58768	PASS
275	198	10	60	27.0	235264	PASS
365	198	1	100	3.6	31597	PASS
441	198	0.01	100	12.6	110144	PASS
442	442	50	100	100.0	709184	PASS
443	442	15	24	19.1	135272	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/1/2025	BNA_M	<u>BM050061.D</u>
Compound Name	Response	Retention Time
DDT	2747273	20.621
DDD	53335	20.186
DDE	3538	19.68
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
56873	2804146	2.03

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050125\
Data File : BM050061.D
Acq On : 01 May 2025 12:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 01 13:23:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

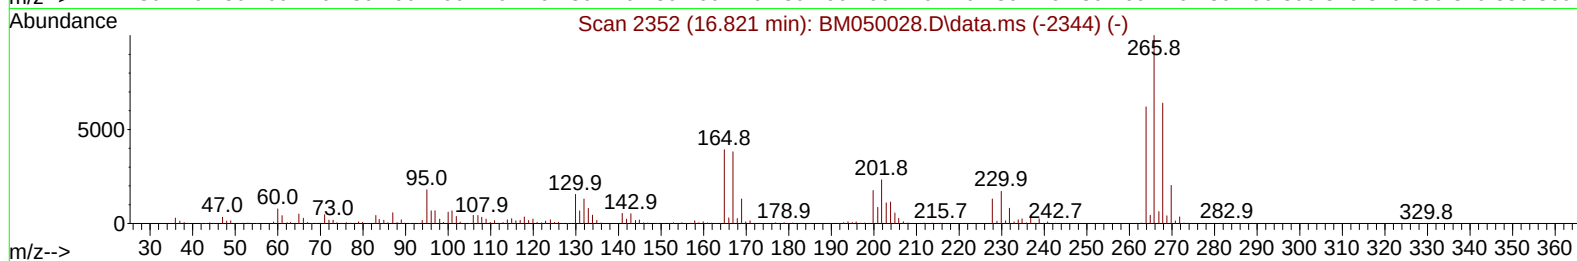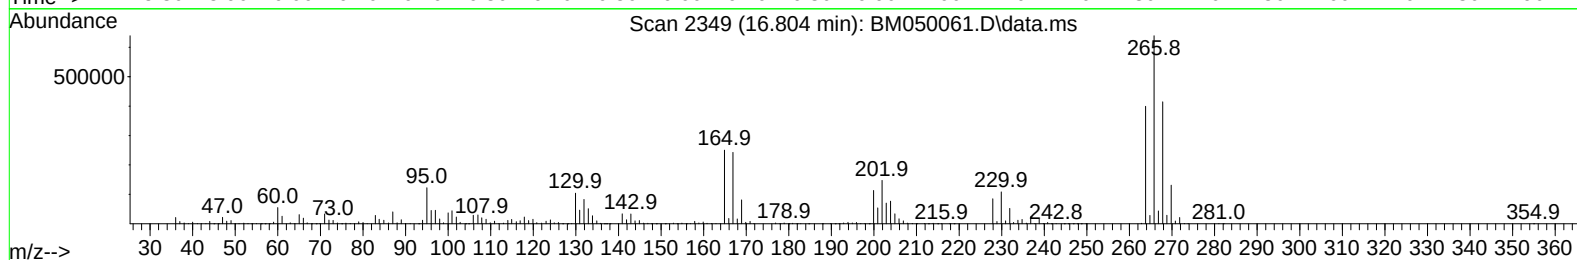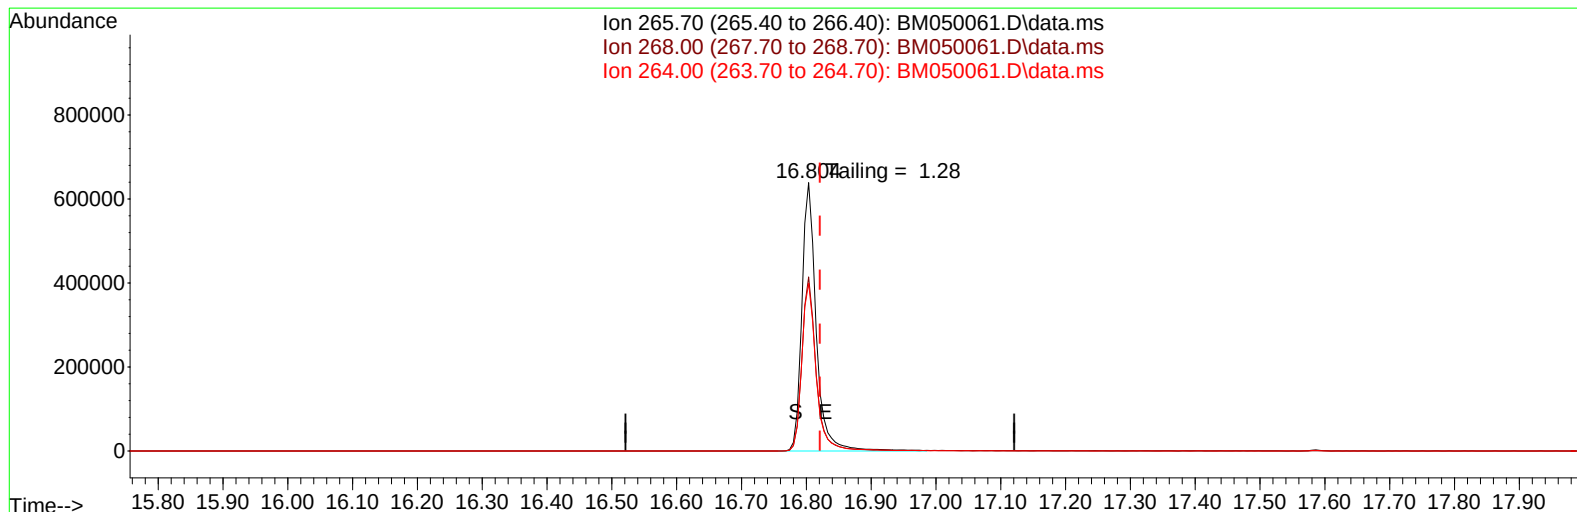

TIC: BM050061.D\data.ms

(70) Pentachlorophenol (C)

16.804min (-0.017) 298828.62 ng




response 984778

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	64.86
264.00	62.00	62.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050125\
Data File : BM050061.D
Acq On : 01 May 2025 12:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 01 13:23:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

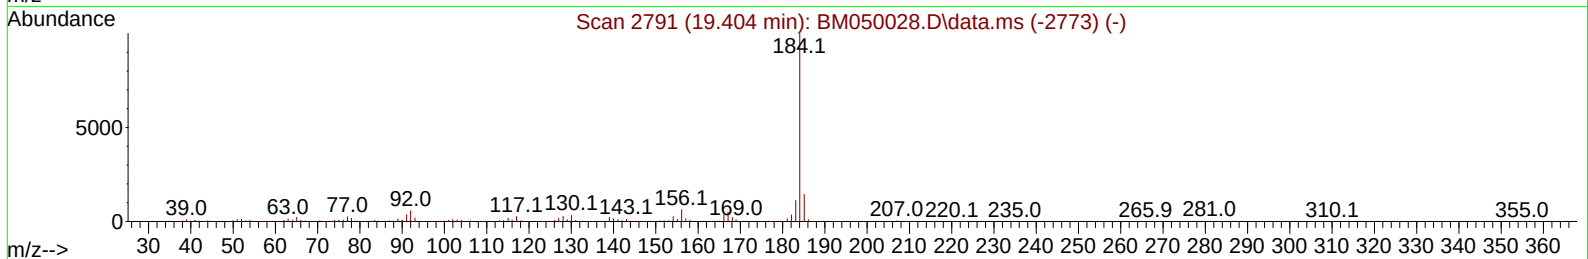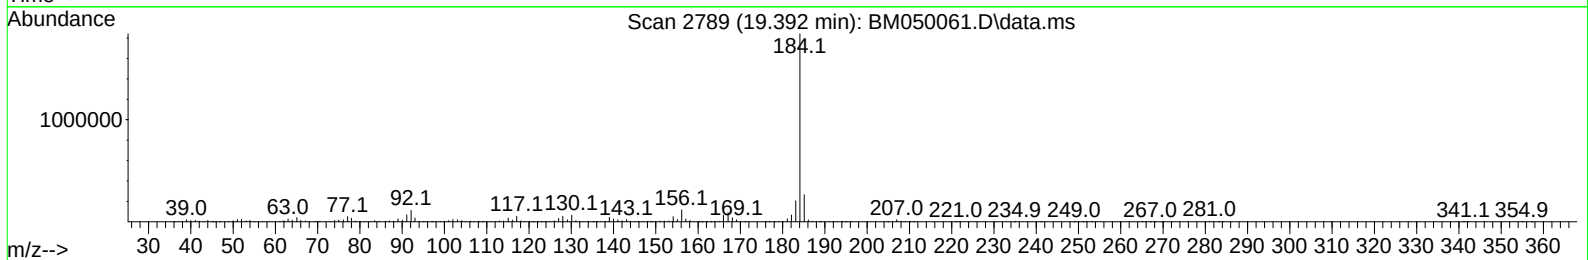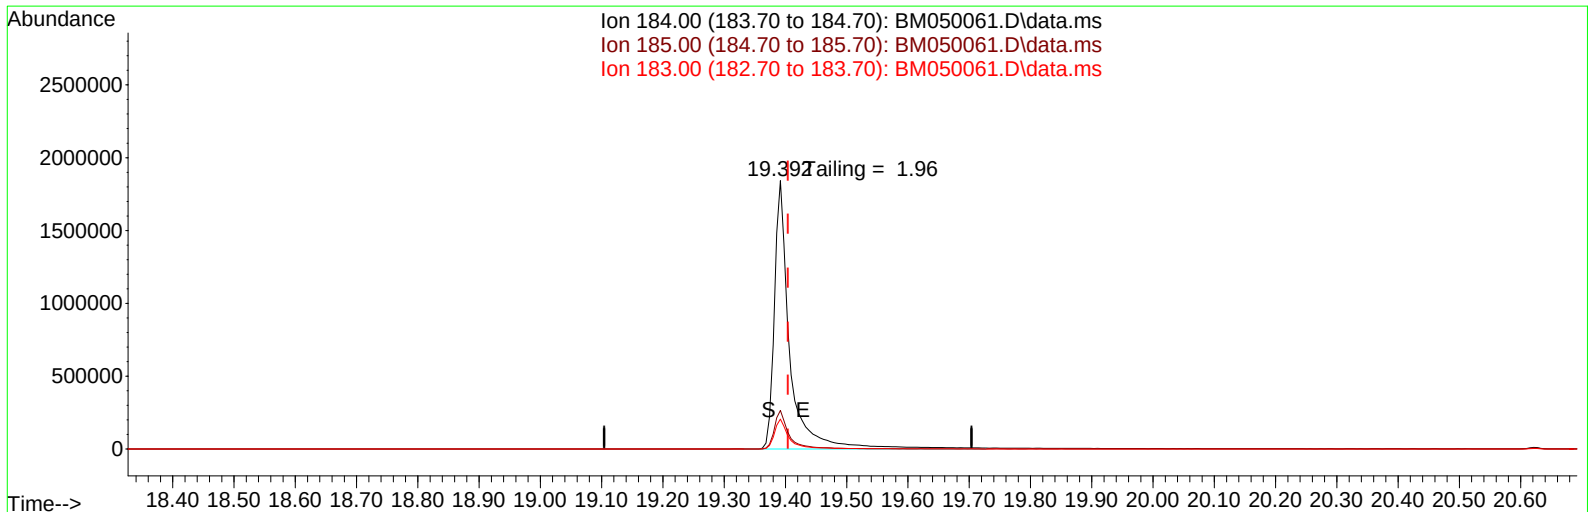

TIC: BM050061.D\data.ms

(77) Benzidine

19.392min (-0.012) 77464.20 ng

response 3260623

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.41
183.00	11.10	11.16
0.00	0.00	0.00