
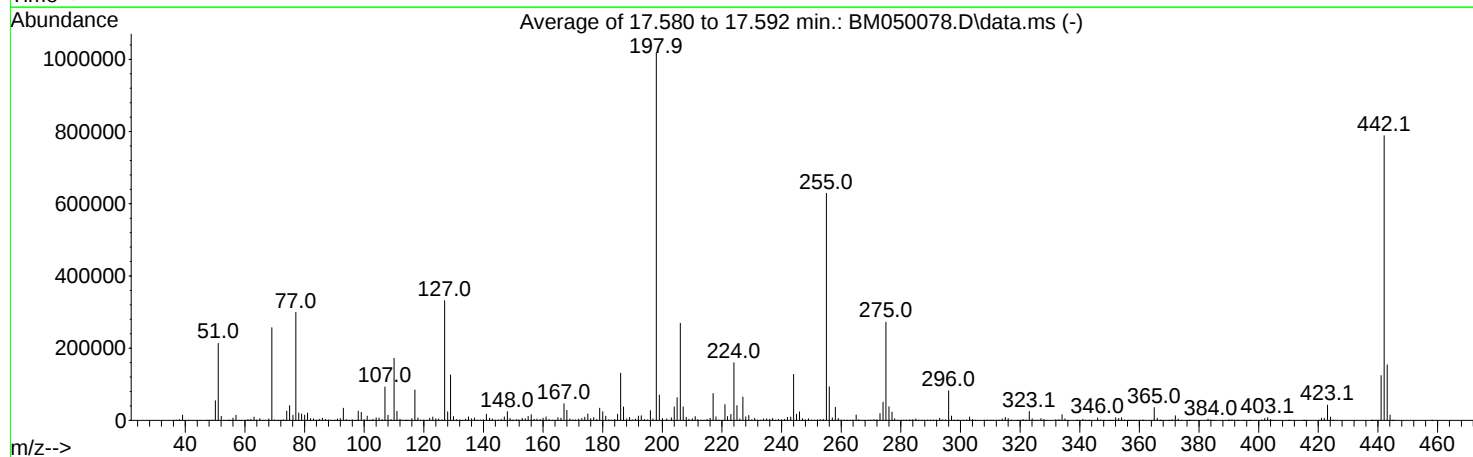


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050225\
Data File : BM050078.D
Acq On : 02 May 2025 09:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 28 18:09:16 2025

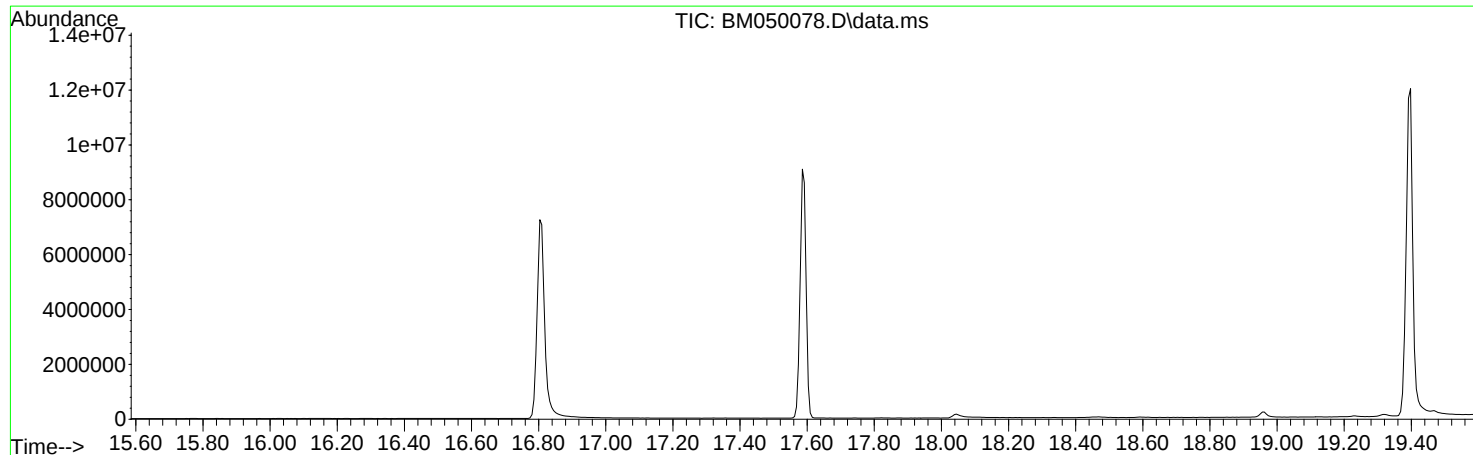

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.9	213274	PASS
68	69	0.00	2	1.5	3940	PASS
69	198	0.00	100	25.2	256603	PASS
70	69	0.00	2	0.5	1404	PASS
127	198	10	80	32.5	331392	PASS
197	198	0.00	2	0.4	4038	PASS
198	198	100	100	100.0	1019051	PASS
199	198	5	9	6.9	70171	PASS
275	198	10	60	26.7	272043	PASS
365	198	1	100	3.5	35432	PASS
441	198	0.01	100	12.2	124285	PASS
442	442	50	100	100.0	788395	PASS
443	442	15	24	19.5	153928	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/2/2025	BNA_M	<u>BM050078.D</u>
Compound Name	Response	Retention Time
DDT	3643029	20.627
DDD	45893	20.233
DDE	2791	19.68
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
48684	3691713	1.32

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050225\
Data File : BM050078.D
Acq On : 02 May 2025 09:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 02 11:44:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

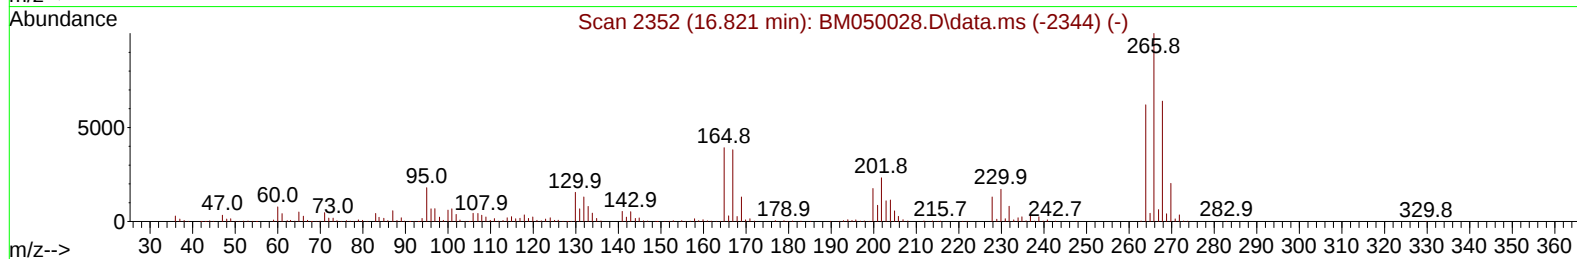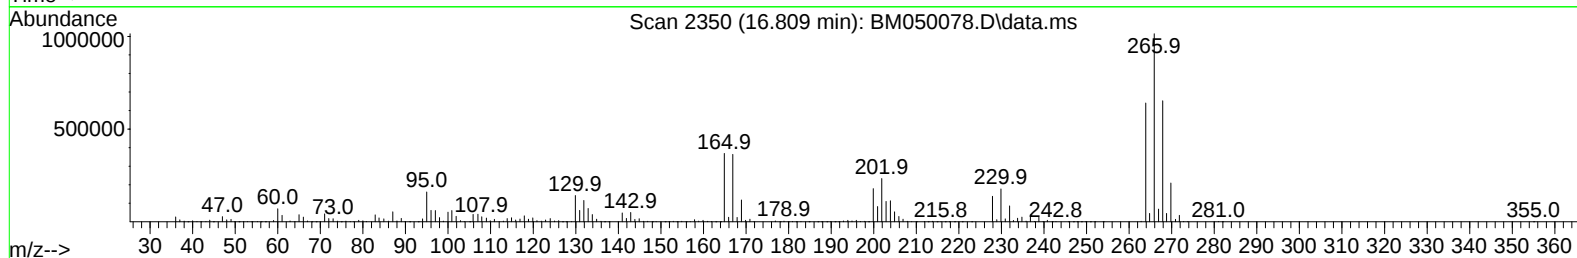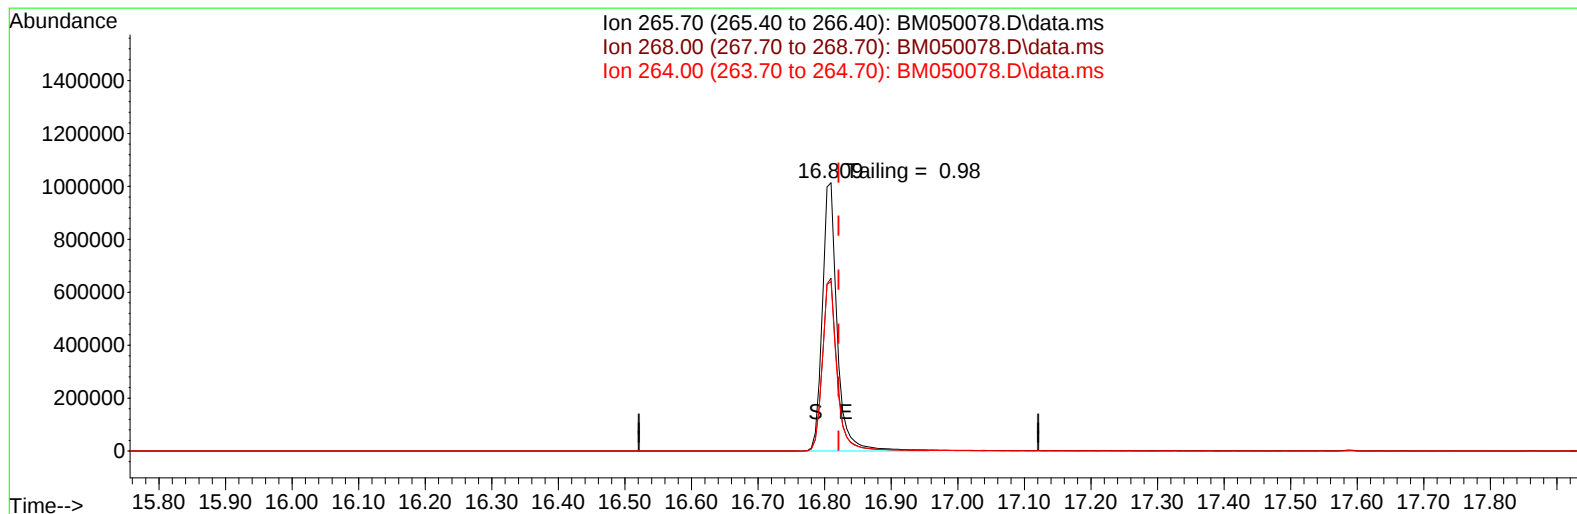

TIC: BM050078.D\data.ms

(70) Pentachlorophenol (C)

16.809min (-0.012) 427399.30 ng




response 1566093

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	64.32
264.00	62.00	63.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050225\
Data File : BM050078.D
Acq On : 02 May 2025 09:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 02 11:44:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

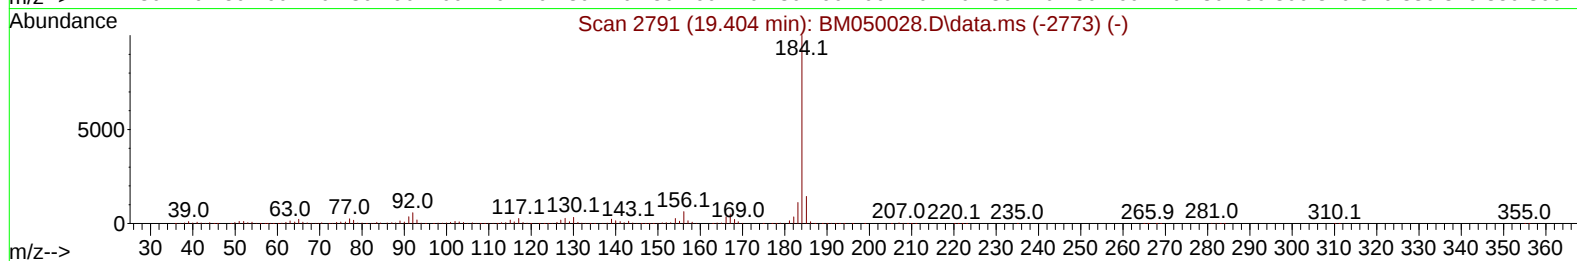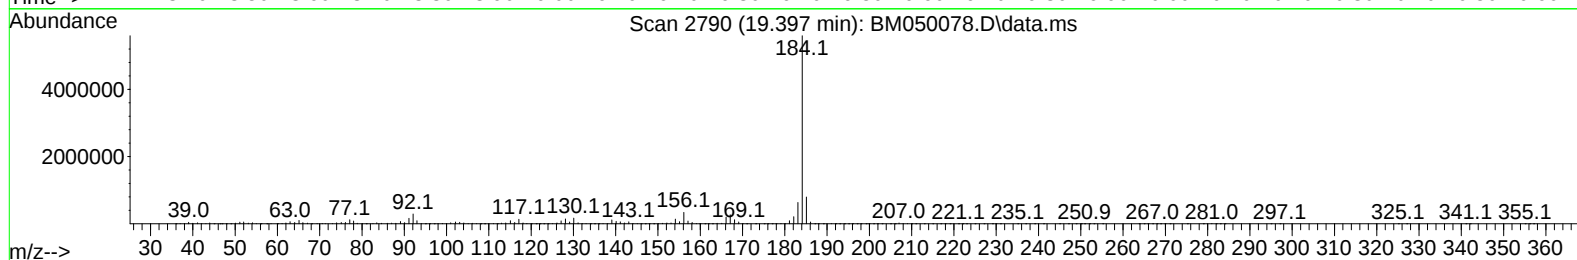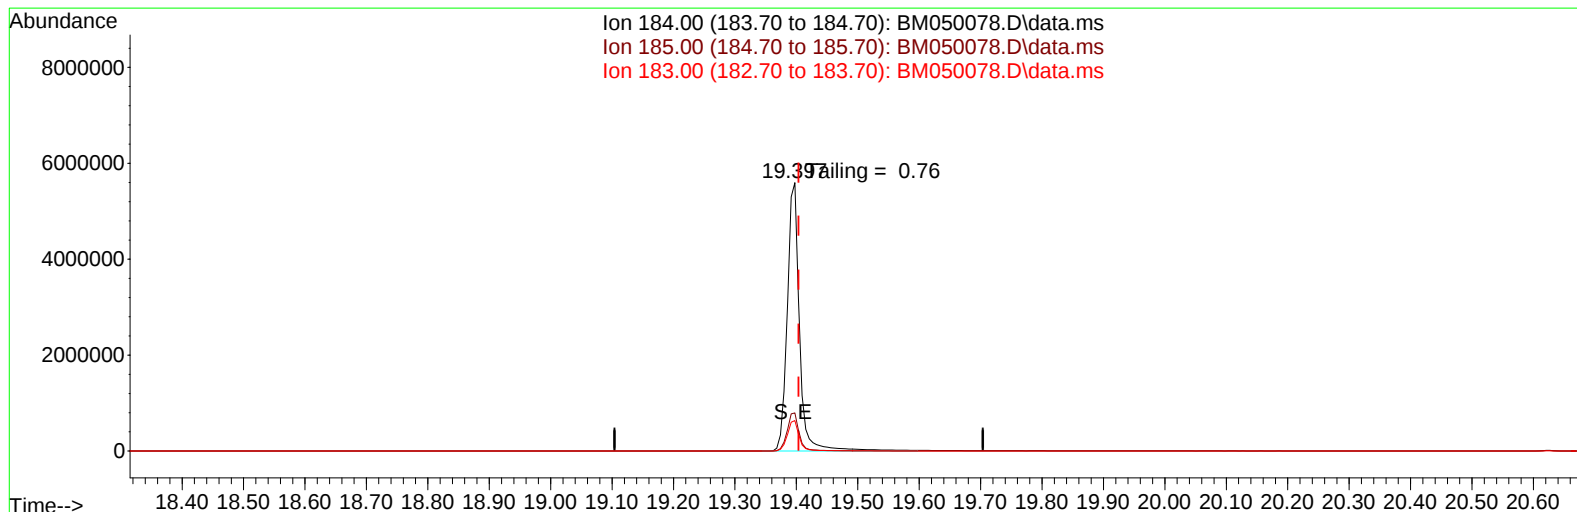

TIC: BM050078.D\data.ms

(77) Benzidine

19.397min (-0.007) 114069.32 ng

response 7848374

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.21
183.00	11.10	11.35
0.00	0.00	0.00