


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050525\
Data File : BM050095.D
Acq On : 05 May 2025 11:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 28 18:09:16 2025

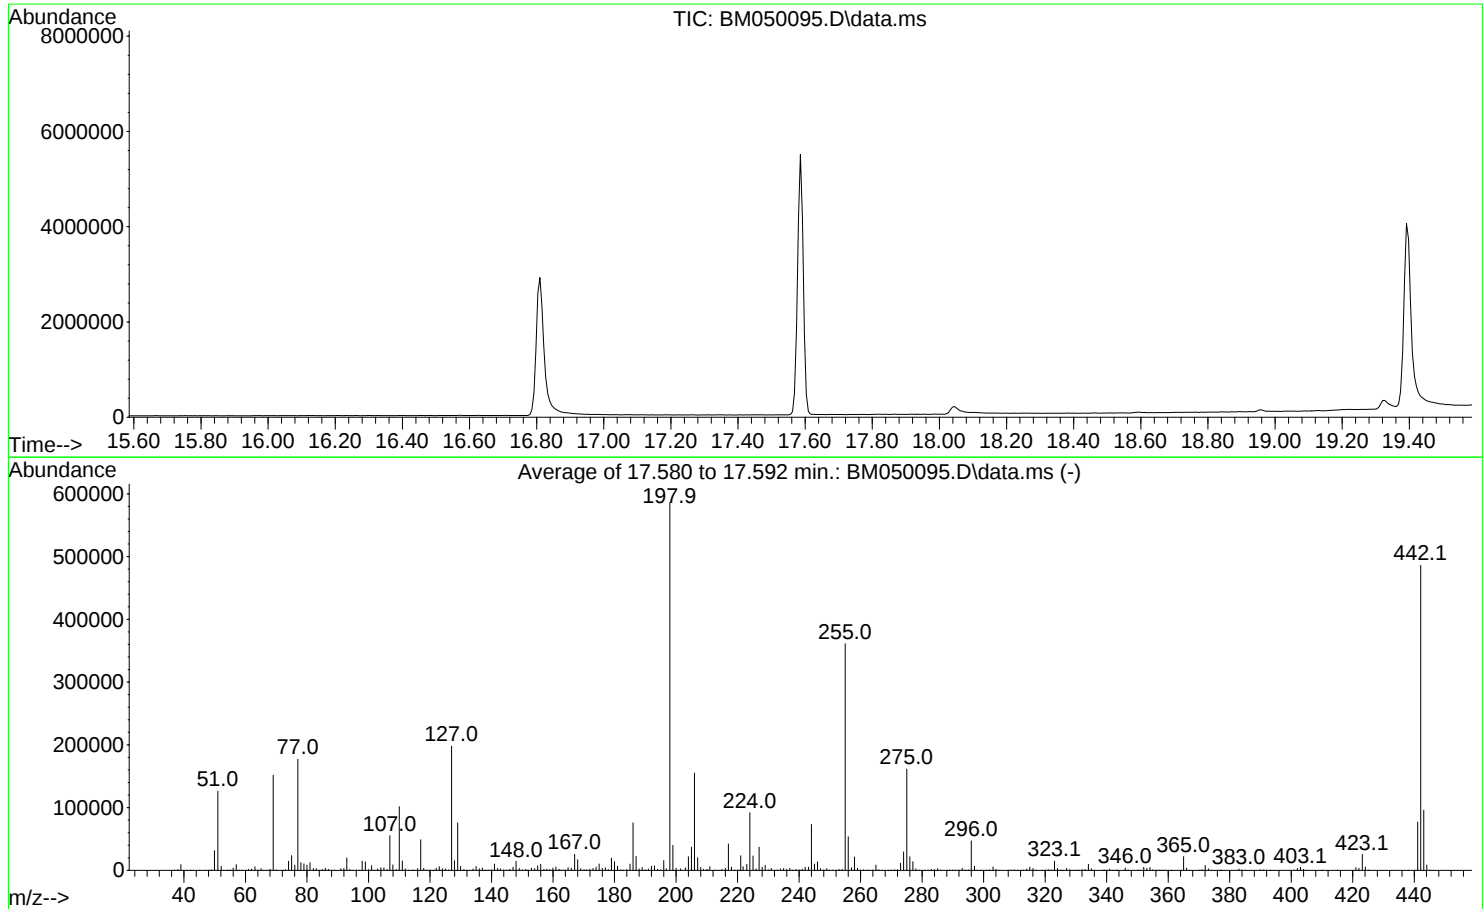

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.5	126193	PASS
68	69	0.00	2	1.4	2128	PASS
69	198	0.00	100	25.9	151749	PASS
70	69	0.00	2	0.5	753	PASS
127	198	10	80	33.8	197867	PASS
197	198	0.00	2	0.4	2535	PASS
198	198	100	100	100.0	586155	PASS
199	198	5	9	6.8	39909	PASS
275	198	10	60	27.5	161365	PASS
365	198	1	100	3.8	21988	PASS
441	198	0.01	100	13.2	77099	PASS
442	442	50	100	100.0	485995	PASS
443	442	15	24	19.7	95787	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/5/2025	BNA_M	<u>BM050095.D</u>
Compound Name	Response	Retention Time
DDT	1857543	20.627
DDD	41765	20.192
DDE	2860	19.68
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
44625	1902168	2.35

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050525\
Data File : BM050095.D
Acq On : 05 May 2025 11:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 05 12:15:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

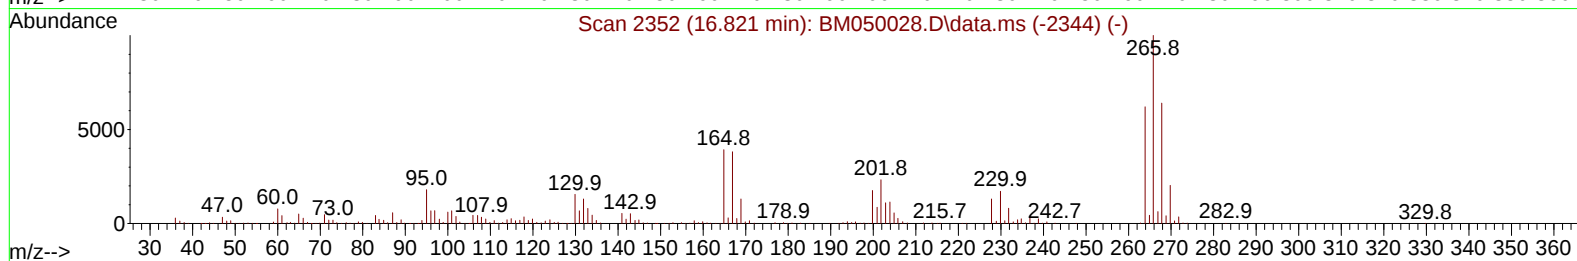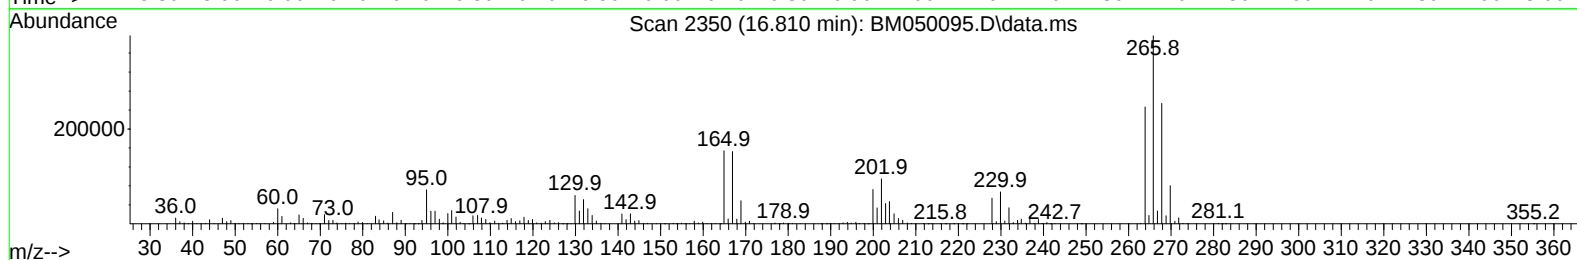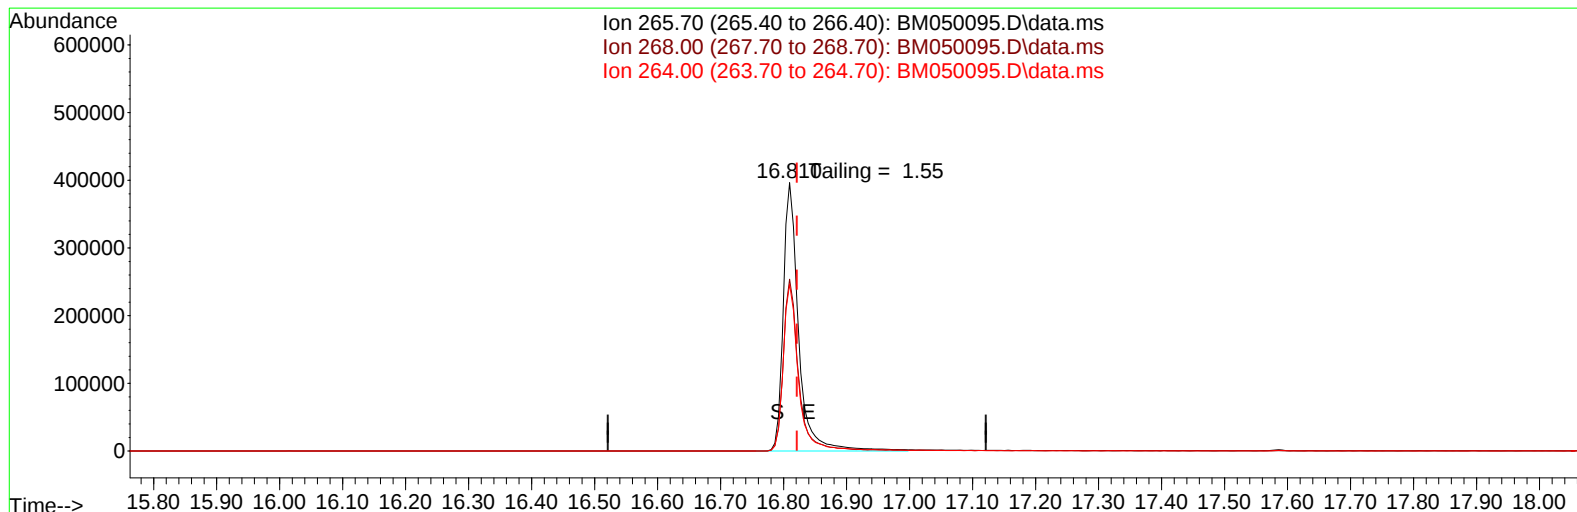

TIC: BM050095.D\data.ms

(70) Pentachlorophenol (C)

16.810min (-0.011) 1373115.00 ng




response 678757

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	64.04
264.00	62.00	62.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050525\
Data File : BM050095.D
Acq On : 05 May 2025 11:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 05 12:15:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

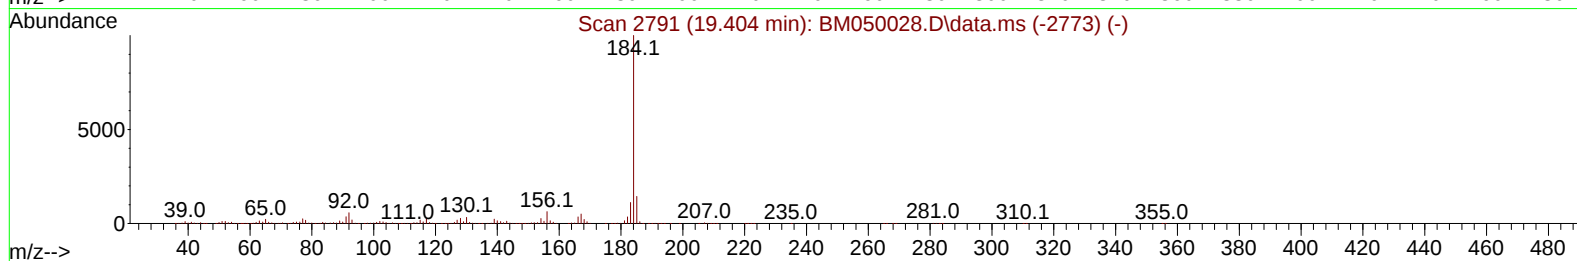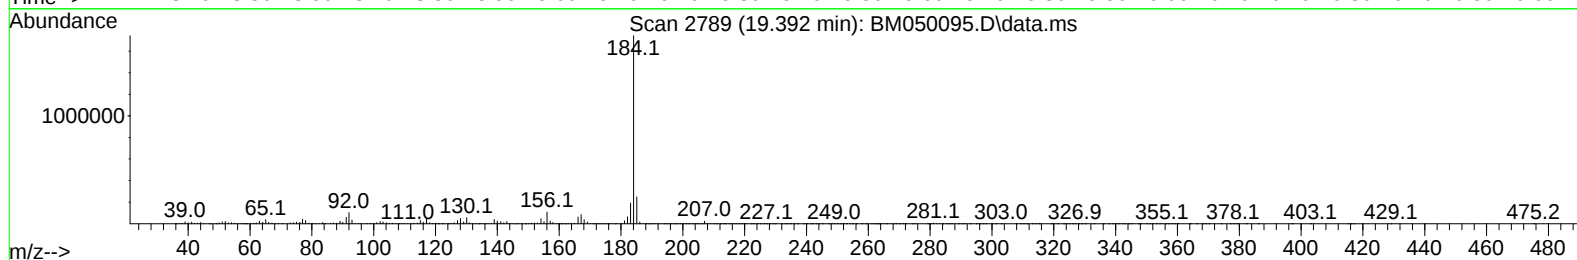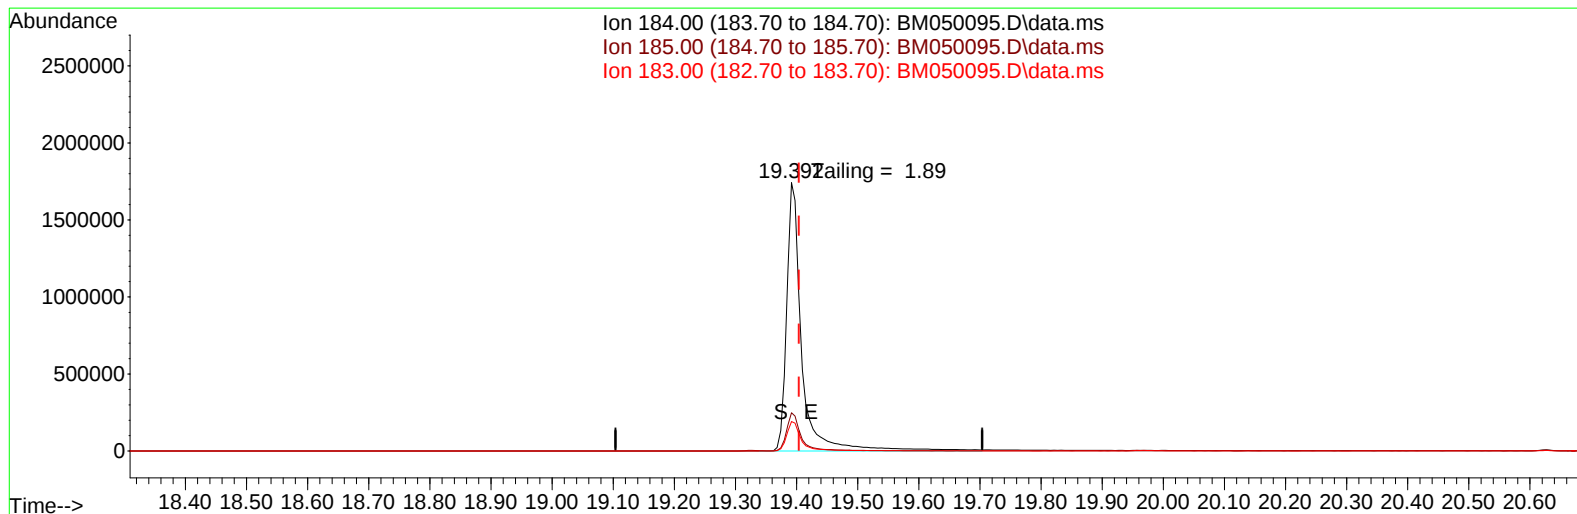

TIC: BM050095.D\data.ms

(77) Benzidine

19.392min (-0.012) 74251.17 ng

response 2996145

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.25
183.00	11.10	11.02
0.00	0.00	0.00