
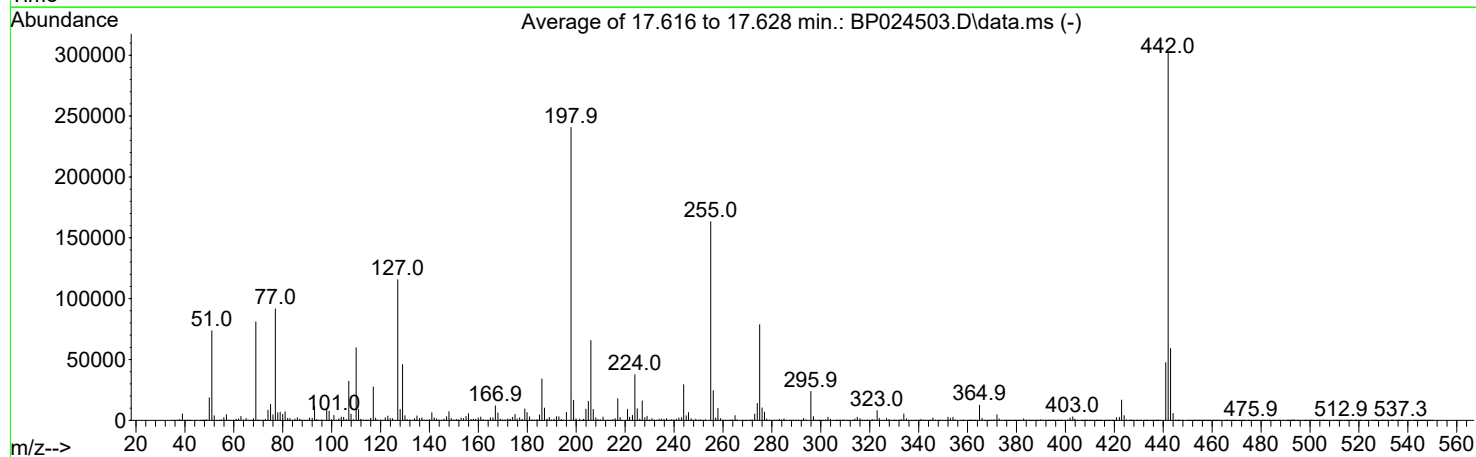


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050225\
Data File : BP024503.D
Acq On : 02 May 2025 10:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 18 12:04:48 2025

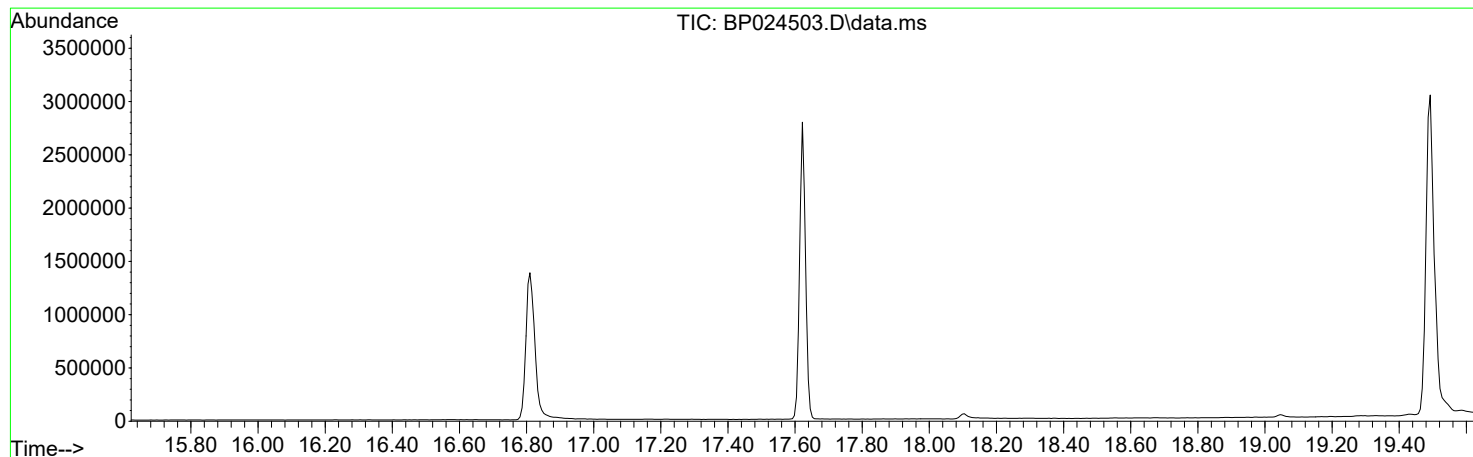

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	73567	PASS
68	69	0.00	2	1.8	1492	PASS
69	198	0.00	100	33.6	80914	PASS
70	69	0.00	2	0.5	423	PASS
127	198	10	80	48.0	115613	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	240640	PASS
199	198	5	9	6.9	16608	PASS
275	198	10	60	32.7	78648	PASS
365	198	1	100	5.2	12516	PASS
441	198	0.01	100	19.7	47454	PASS
442	442	100	100	100.0	302205	PASS
443	442	15	24	19.5	58966	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/2/2025	BNA_P	<u>BP024503.D</u>
Compound Name	Response	Retention Time
DDT	933214	20.786
DDD	18421	20.316
DDE	1625	19.786
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20046	953260	2.10

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050225\
Data File : BP024503.D
Acq On : 02 May 2025 10:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 03 06:17:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

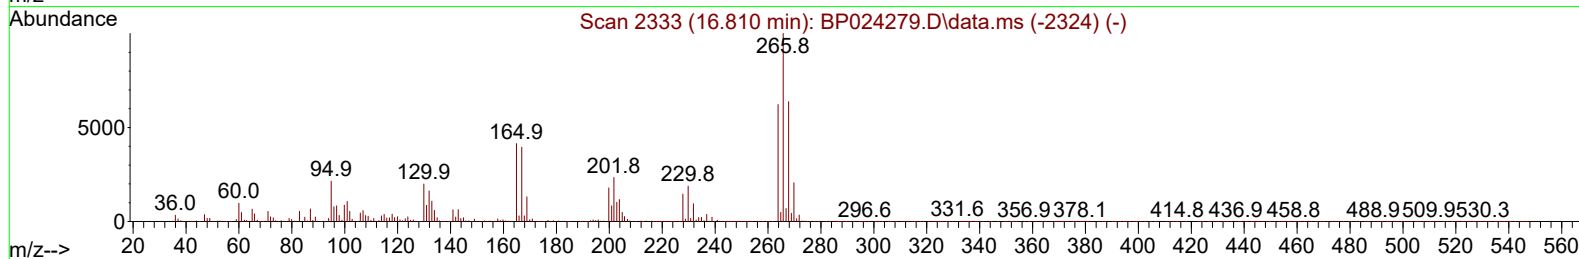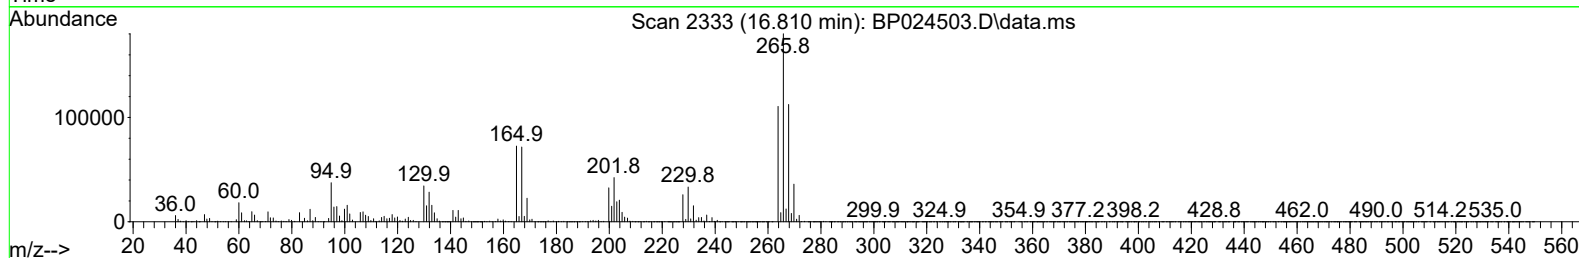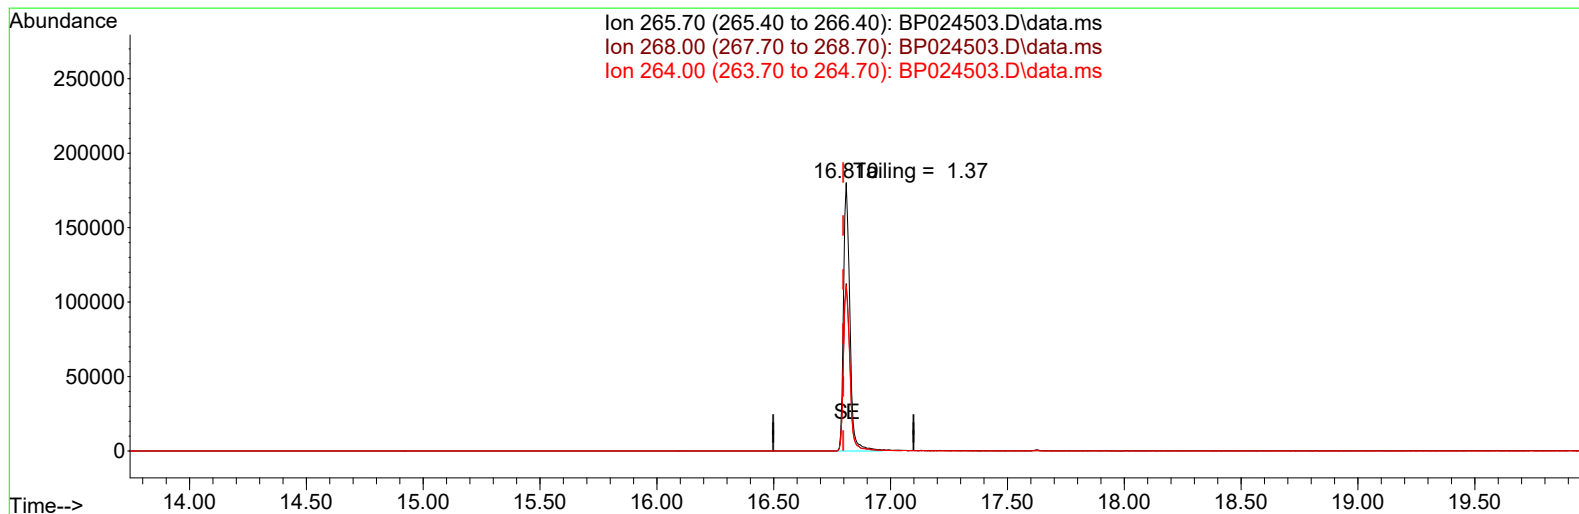

TIC: BP024503.D\data.ms

(70) Pentachlorophenol (C)

16.810min (+ 0.012) 32777.46 ng m




response 339964

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.35
264.00	62.20	61.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050225\
Data File : BP024503.D
Acq On : 02 May 2025 10:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 03 06:17:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

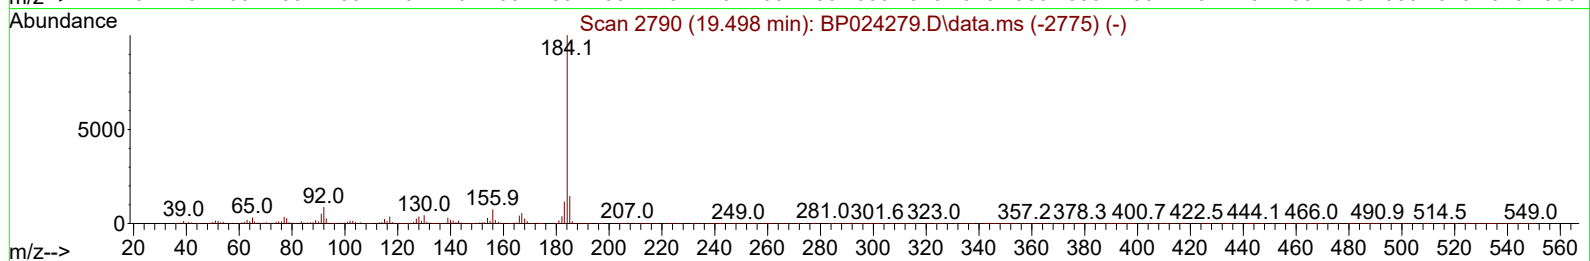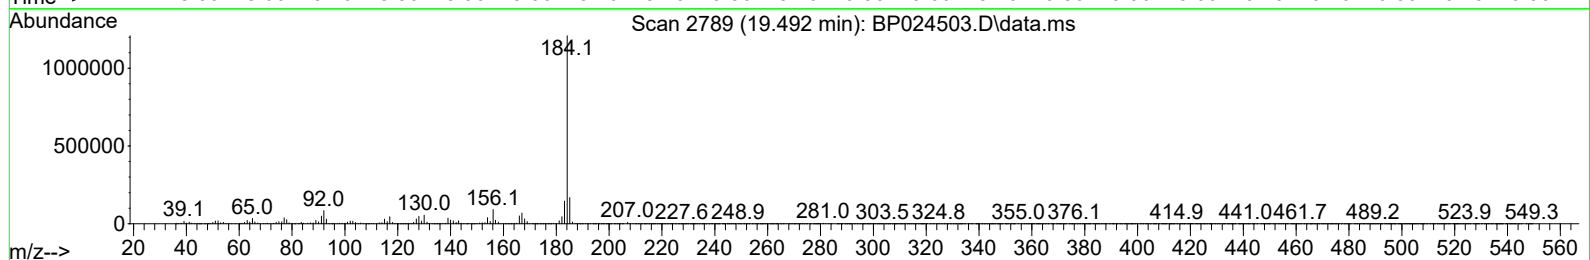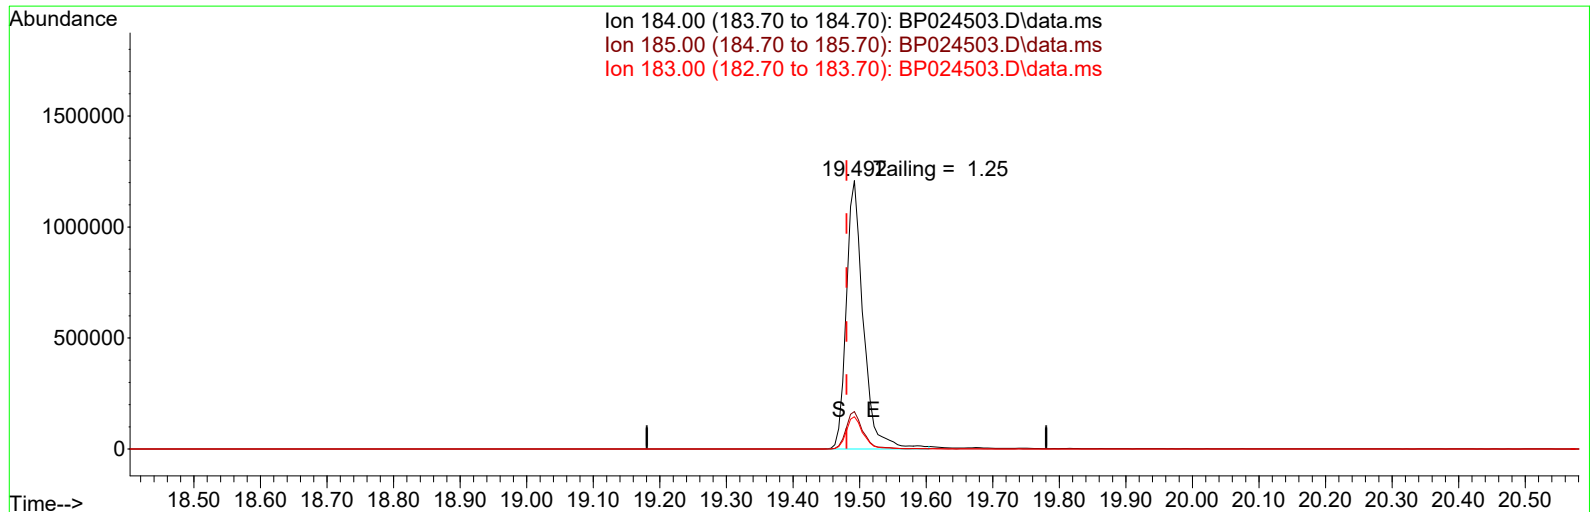

TIC: BP024503.D\data.ms

(77) Benzidine

19.492min (+ 0.012) 40497.92 ng

response 2137057

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.97
183.00	11.50	12.09
0.00	0.00	0.00