
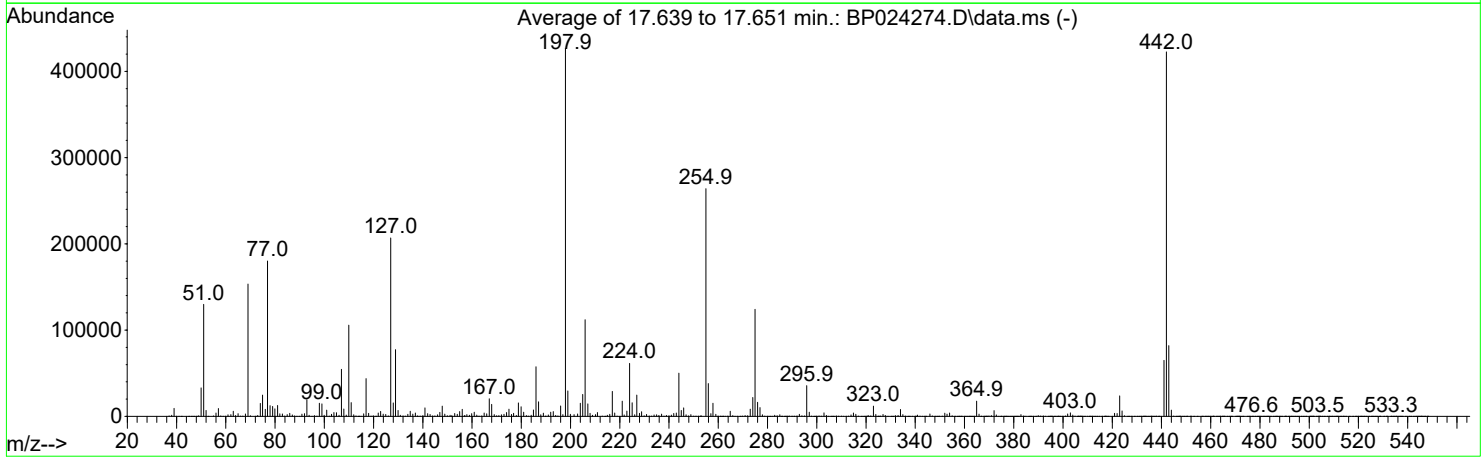


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041425\
 Data File : BP024274.D
 Acq On : 14 Apr 2025 10:25
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 15 04:48:42 2025

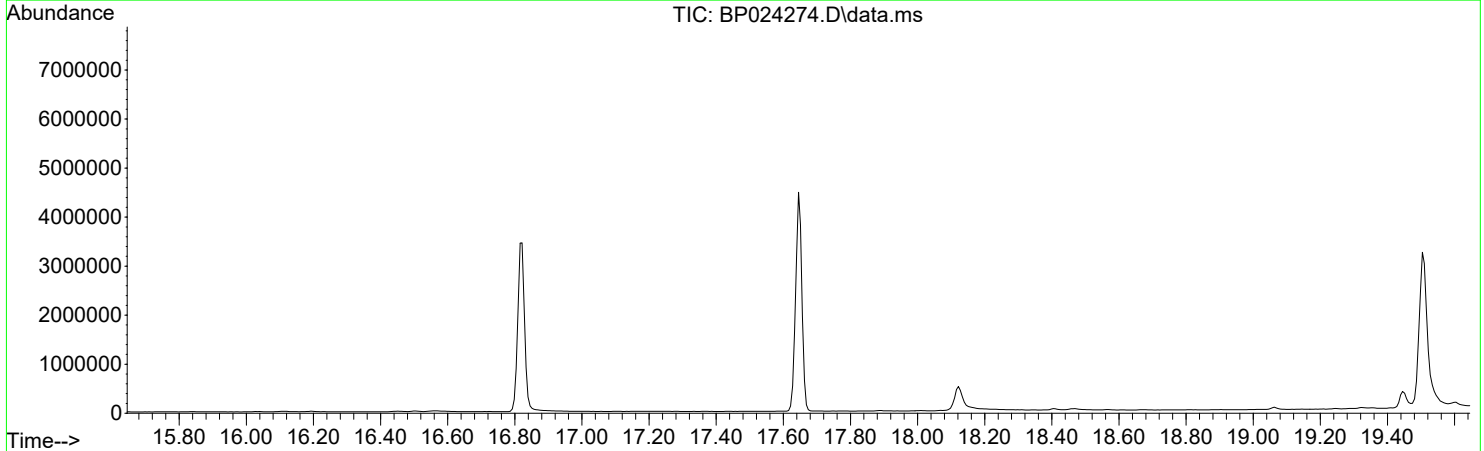

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.4	129796	PASS
68	69	0.00	2	1.8	2815	PASS
69	198	0.00	100	36.0	153442	PASS
70	69	0.00	2	0.5	836	PASS
127	198	10	80	48.5	206858	PASS
197	198	0.00	2	0.5	2122	PASS
198	198	100	100	100.0	426527	PASS
199	198	5	9	6.9	29549	PASS
275	198	10	60	29.1	124199	PASS
365	198	1	100	4.1	17663	PASS
441	198	0.01	100	15.2	64862	PASS
442	442	100	100	100.0	422528	PASS
443	442	15	24	19.4	82090	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/14/2025	BNA_P	<u>BP024274.D</u>
Compound Name	Response	Retention Time
DDT	1715151	20.798
DDD	26002	20.386
DDE	1572	19.81
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27574	1742725	1.58

Instrument :
 BNA_P
 ClientSampled :
 DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041425\
 Data File : BP024274.D
 Acq On : 14 Apr 2025 10:25
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Apr 14 15:07:47 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 14 15:04:09 2025
 Response via : Initial Calibration

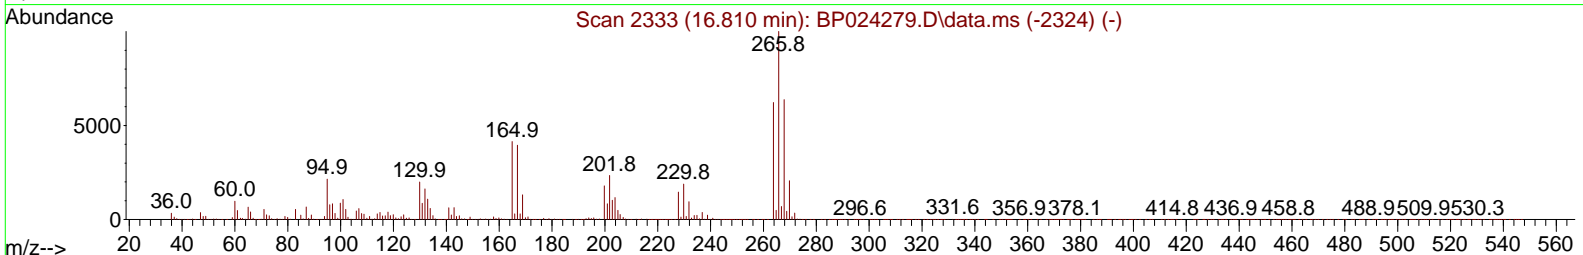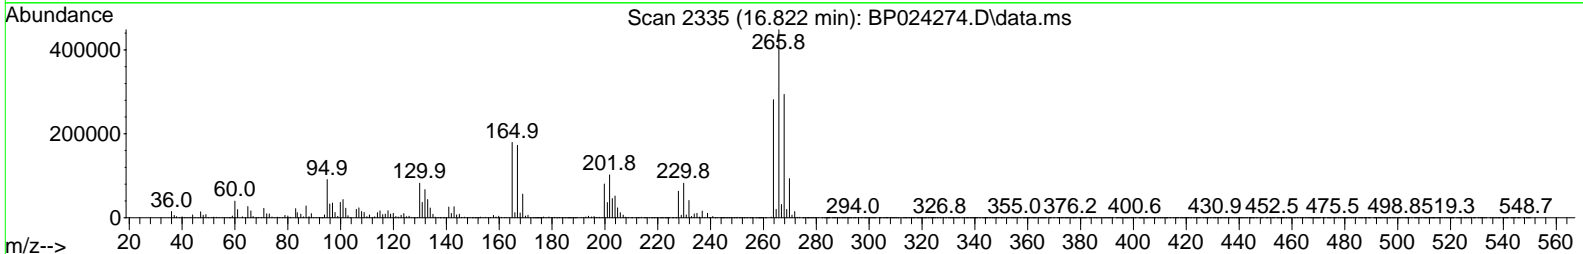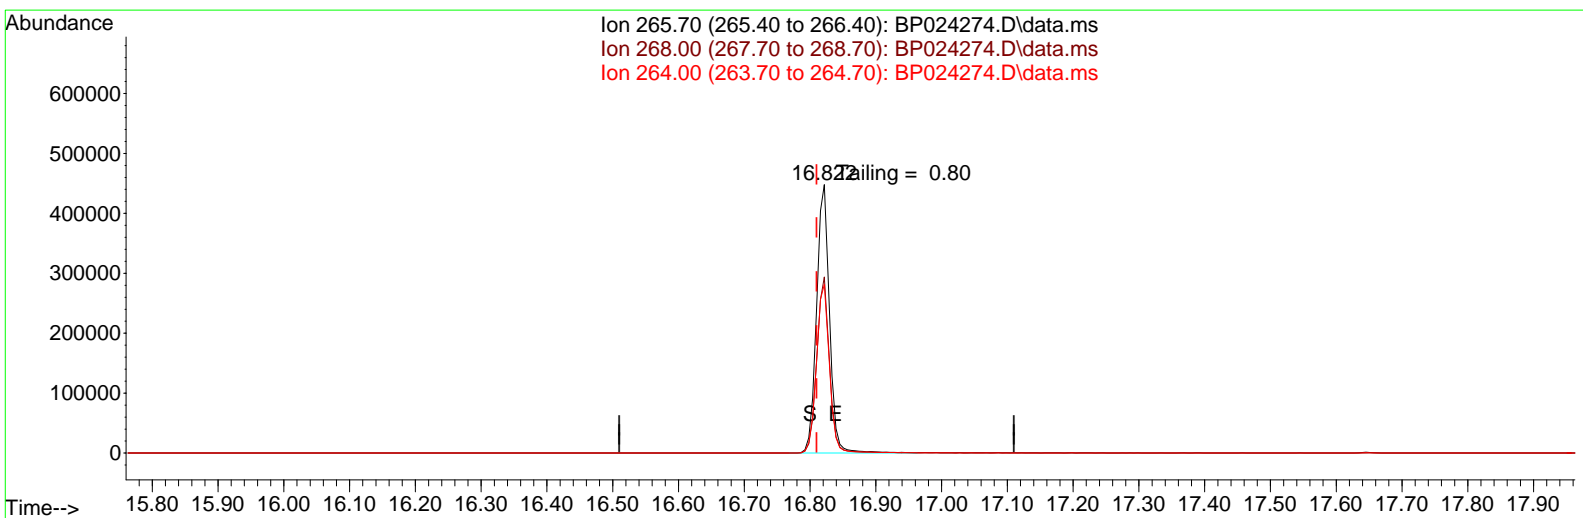

TIC: BP024274.D\data.ms

(70) Pentachlorophenol (C)

16.822min (+ 0.012) 3117222.42 ng




response 611847

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	65.61
264.00	62.20	62.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP041425\
 Data File : BP024274.D
 Acq On : 14 Apr 2025 10:25
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
ClientSampleId :
 DFTPP

Quant Time: Apr 14 15:07:47 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 14 15:04:09 2025
 Response via : Initial Calibration

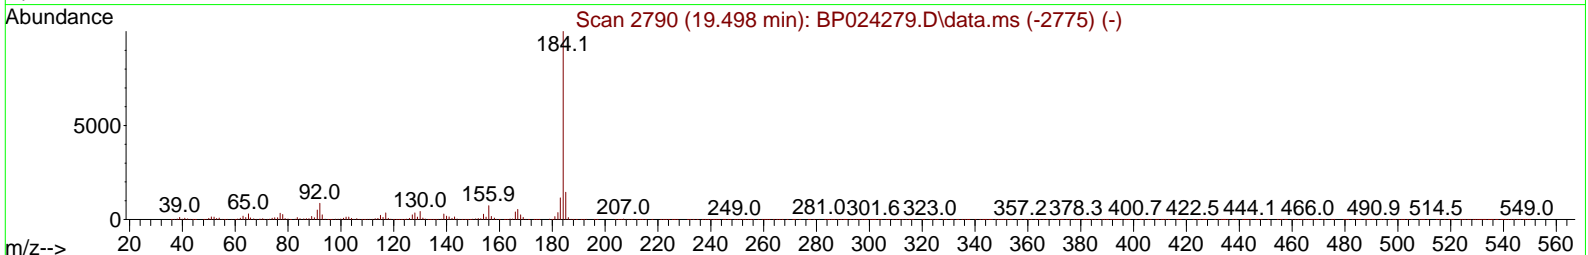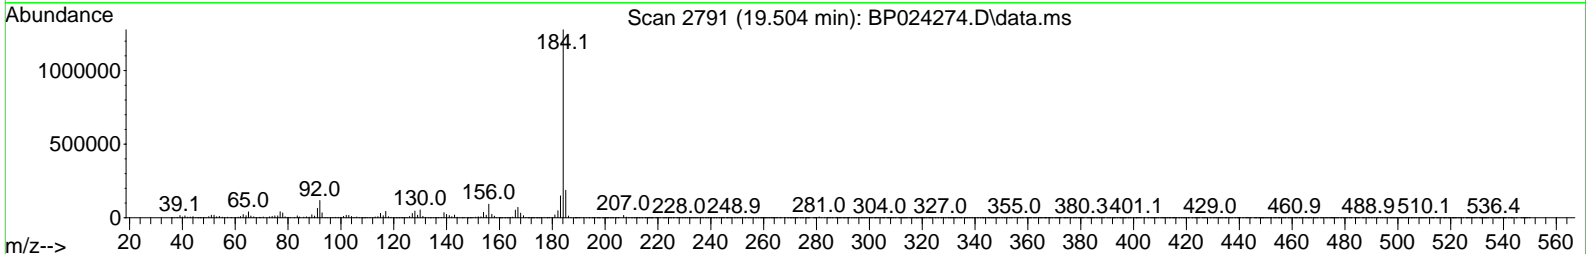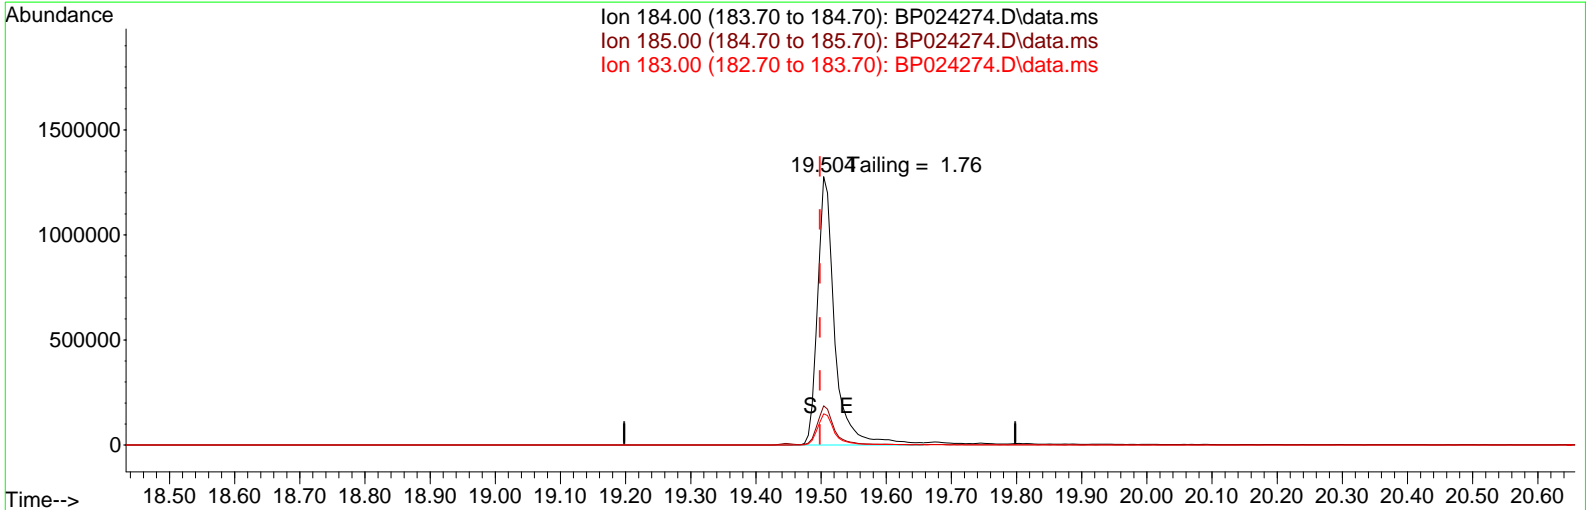

TIC: BP024274.D\data.ms

(77) Benzidine

19.504min (+ 0.006) 7415471.13 ng

response 2354373

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.60
183.00	11.50	11.64
0.00	0.00	0.00