
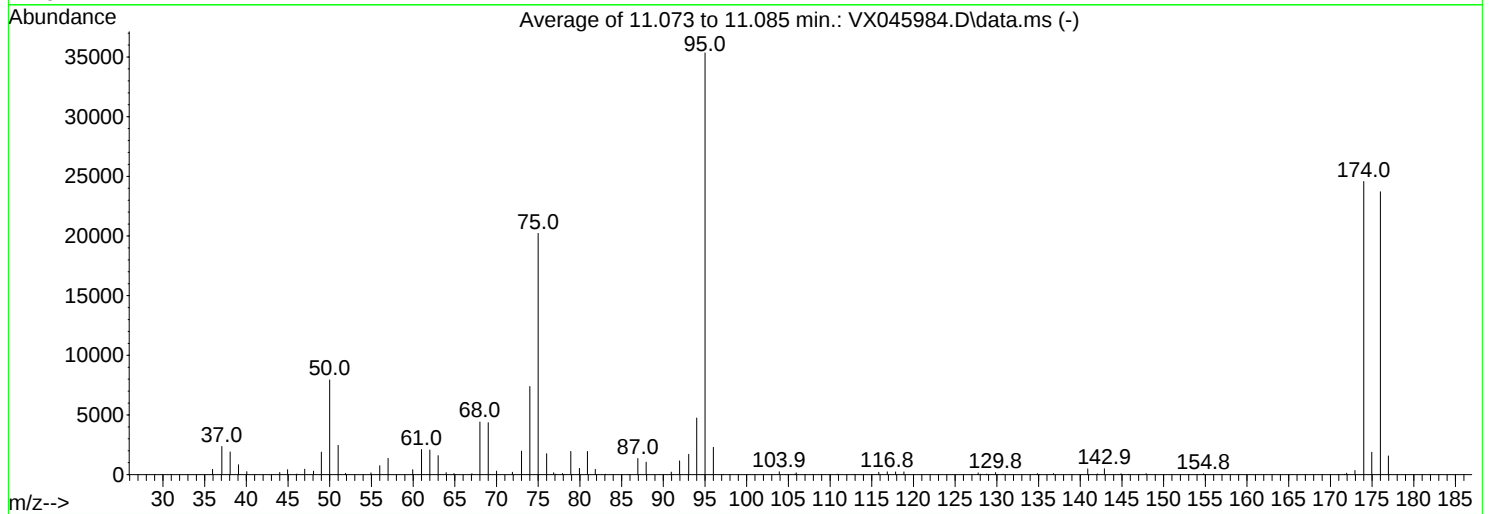


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX043025\
Data File : VX045984.D
Acq On : 30 Apr 2025 09:32
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Title : SW846 8260
Last Update : Wed Apr 02 03:11:43 2025

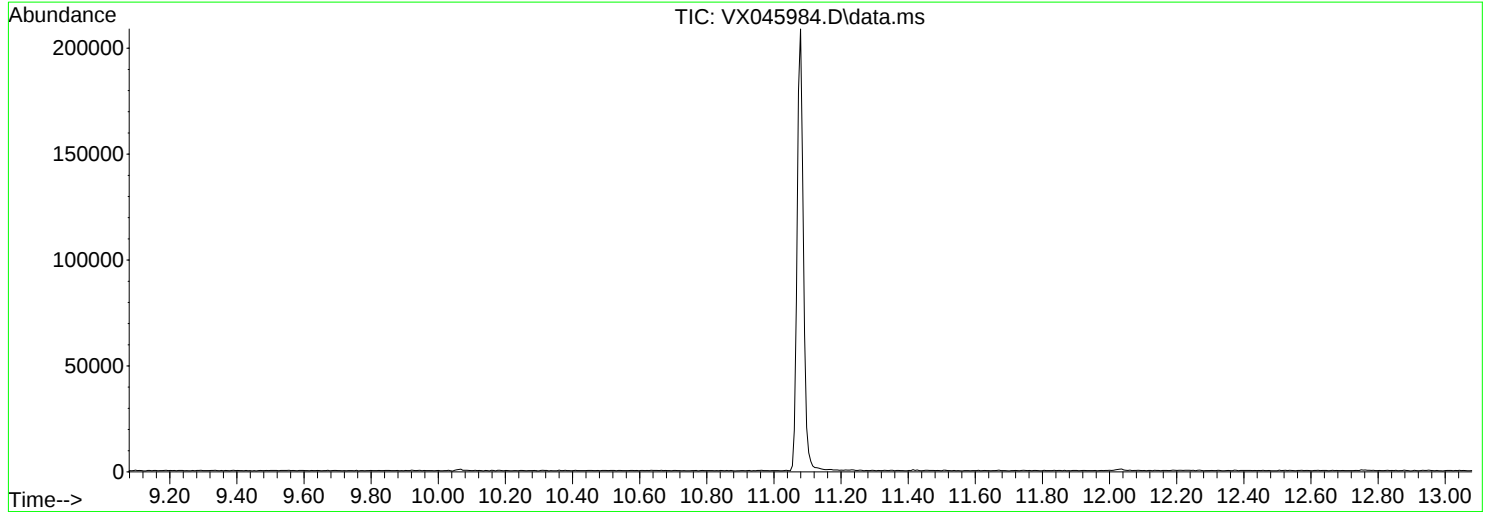

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.5	7942	PASS
75	95	30	60	57.2	20221	PASS
95	95	100	100	100.0	35349	PASS
96	95	5	9	6.5	2291	PASS
173	174	0.00	2	1.4	345	PASS
174	95	50	100	69.5	24563	PASS
175	174	5	9	7.7	1882	PASS
176	174	95	101	96.5	23704	PASS
177	176	5	9	6.6	1575	PASS