
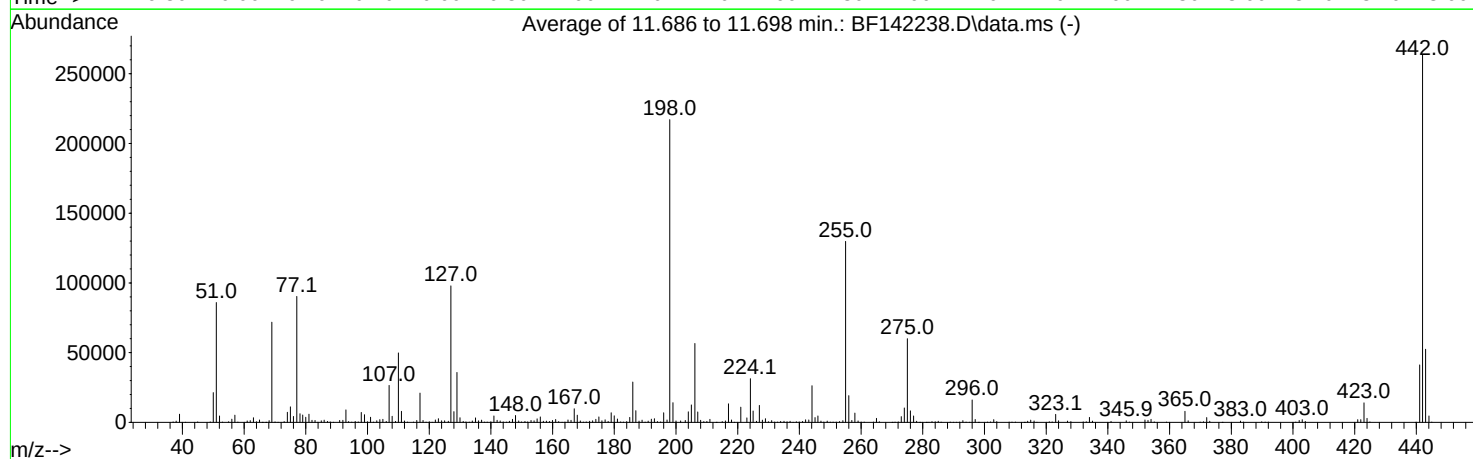


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF043025\
Data File : BF142238.D
Acq On : 30 Apr 2025 10:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 30 16:00:01 2025

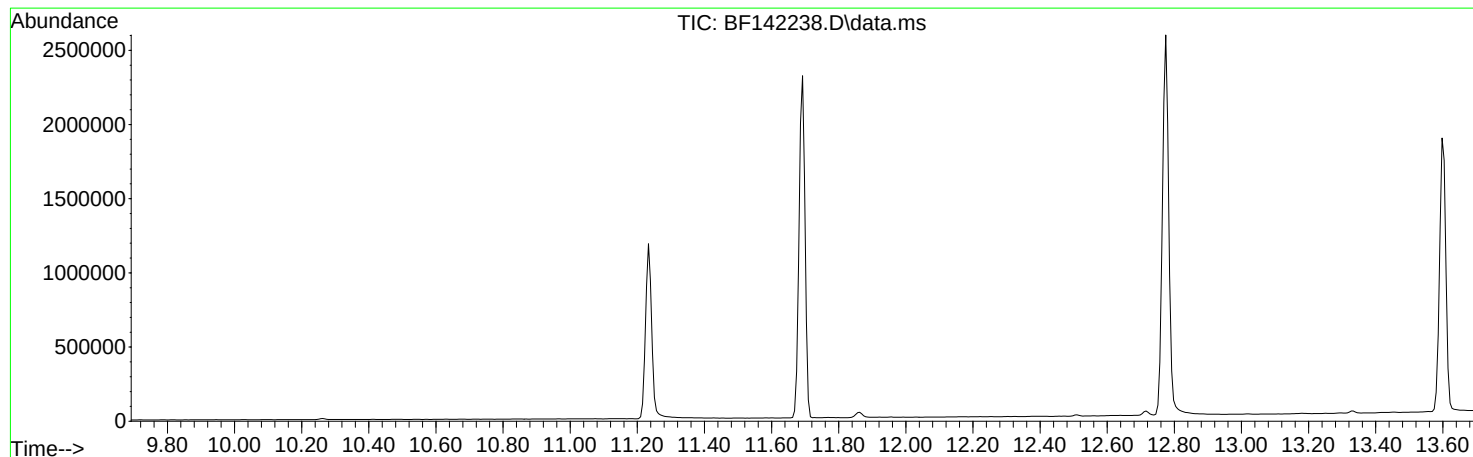




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	86007	PASS
68	69	0.00	2	1.8	1316	PASS
69	198	0.00	100	33.1	71903	PASS
70	69	0.00	2	0.5	377	PASS
127	198	10	80	45.1	97928	PASS
197	198	0.00	2	0.8	1760	PASS
198	198	100	100	100.0	217131	PASS
199	198	5	9	6.5	14095	PASS
275	198	10	60	27.6	60019	PASS
365	198	1	100	3.7	7976	PASS
441	198	0.01	100	19.0	41171	PASS
442	442	50	100	100.0	263808	PASS
443	442	15	24	19.9	52467	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF043025\
Data File : BF142238.D
Acq On : 30 Apr 2025 10:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 30 16:04:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 30 16:00:01 2025
Response via : Initial Calibration

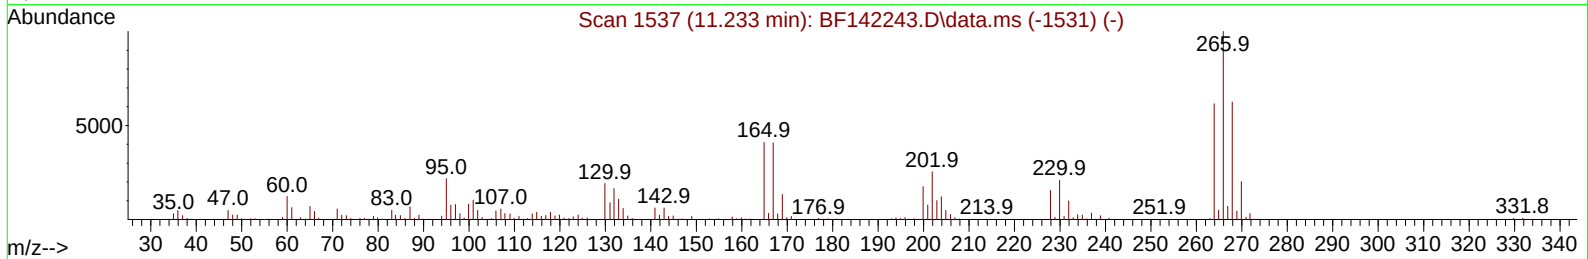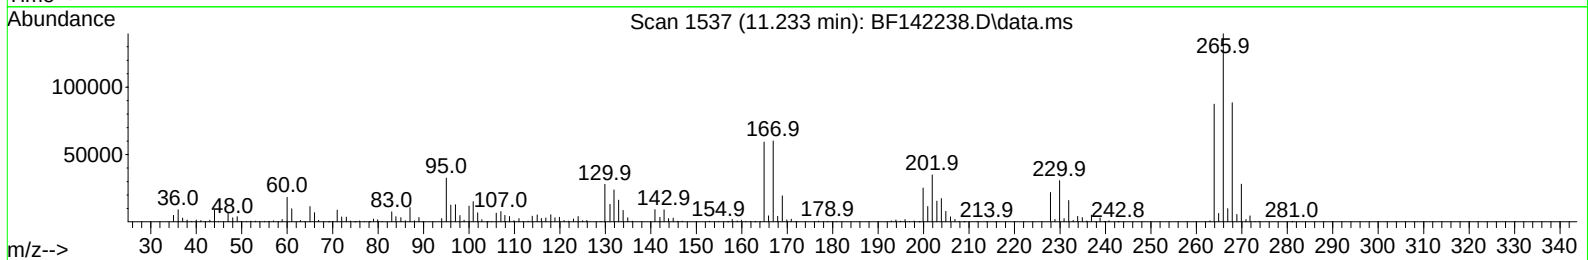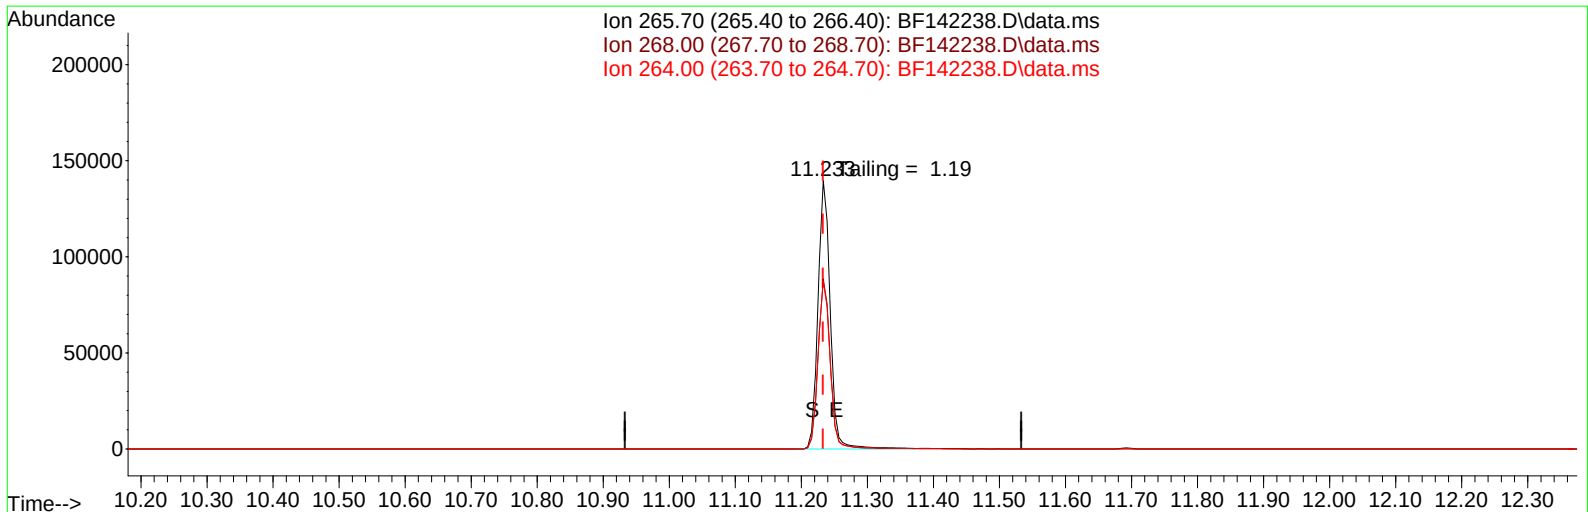

TIC: BF142238.D\data.ms

(70) Pentachlorophenol (C)

11.233min (+ 0.000) 69575.24 ng




response 180630

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	63.39
264.00	61.60	62.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF043025\
Data File : BF142238.D
Acq On : 30 Apr 2025 10:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 30 16:04:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 30 16:00:01 2025
Response via : Initial Calibration

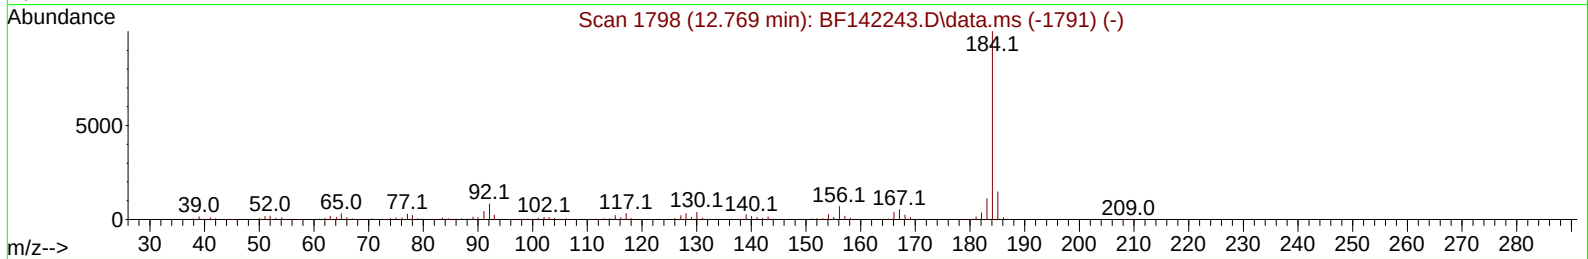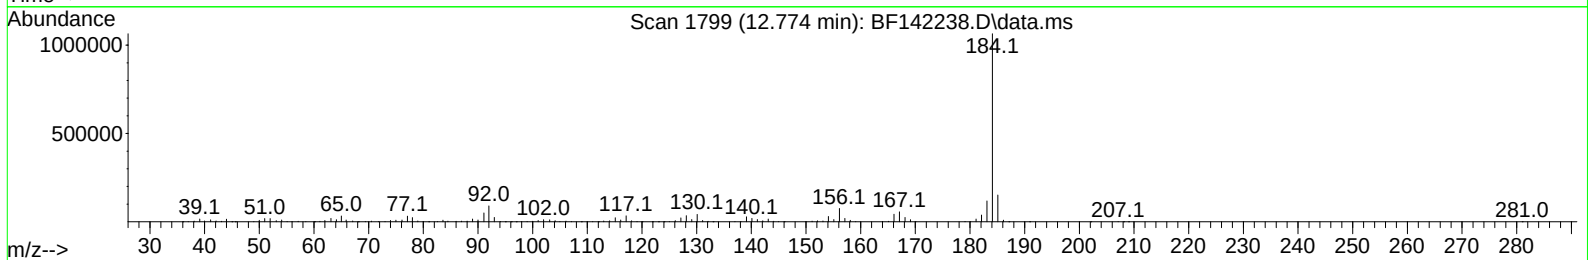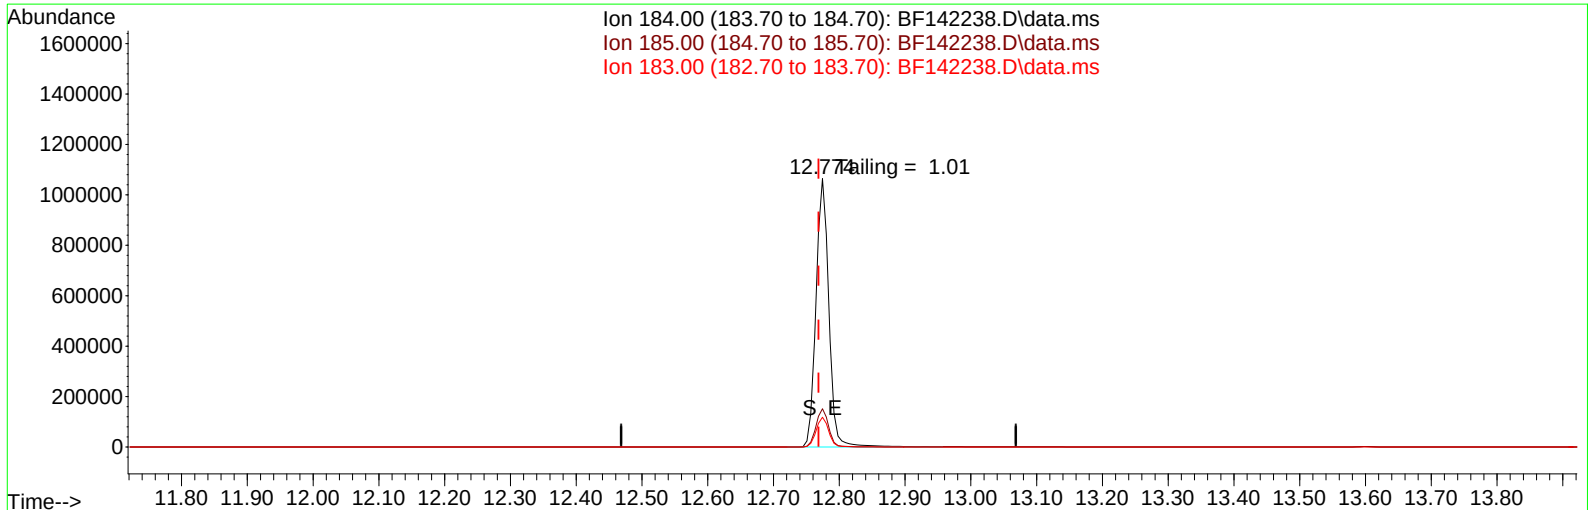

TIC: BF142238.D\data.ms

(77) Benzidine

12.774min (+ 0.006) 97416.22 ng

response 1440496

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.25
183.00	11.10	11.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/30/2025	BNA_F	<u>BF142238.D</u>
Compound Name	Response	Retention Time
DDT	378546	13.598
DDD	2841	13.333
DDE	0	12.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2841	381387	0.74

Instrument :
BNA_F
ClientSampleId :
DFTPP