
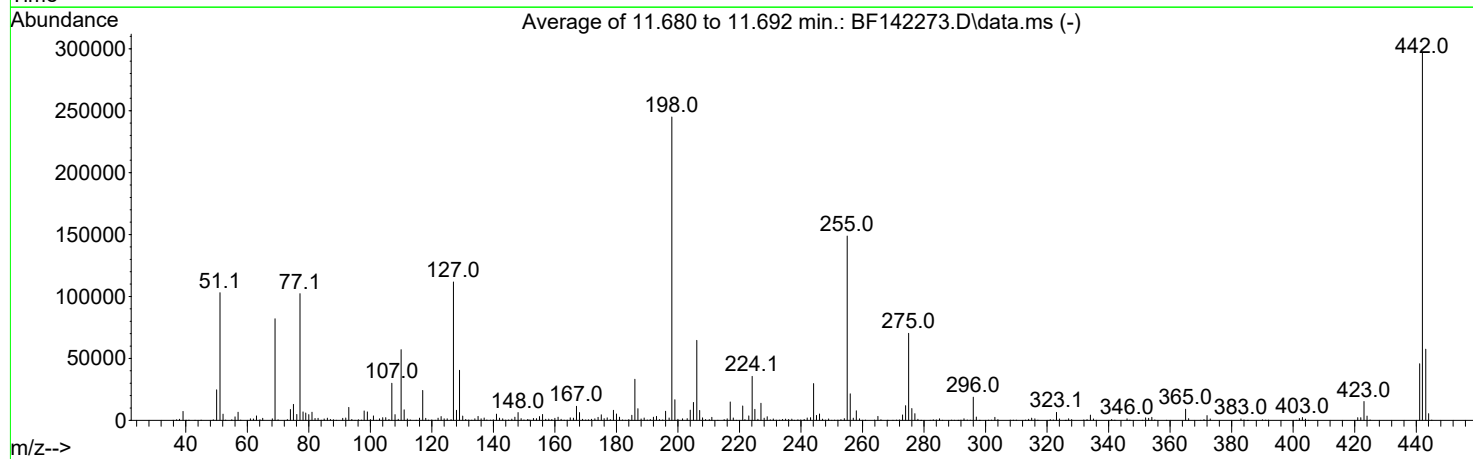


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050225\
Data File : BF142273.D
Acq On : 02 May 2025 10:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 30 16:00:01 2025

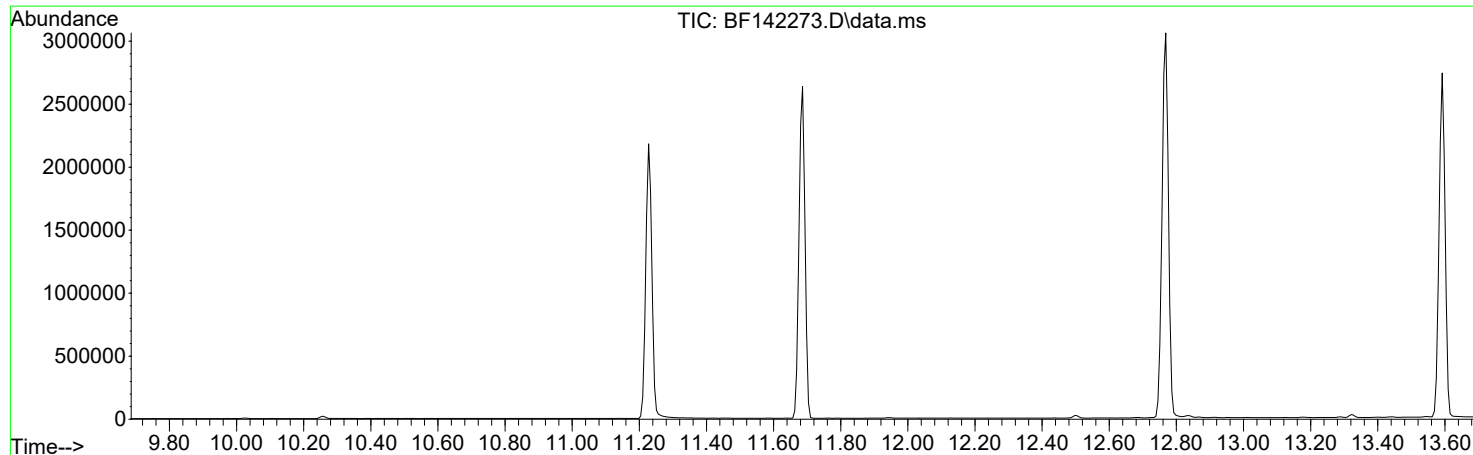

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	103072	PASS
68	69	0.00	2	1.6	1298	PASS
69	198	0.00	100	33.5	82011	PASS
70	69	0.00	2	0.6	473	PASS
127	198	10	80	45.6	111691	PASS
197	198	0.00	2	0.8	2015	PASS
198	198	100	100	100.0	244928	PASS
199	198	5	9	6.8	16632	PASS
275	198	10	60	28.7	70309	PASS
365	198	1	100	3.7	9025	PASS
441	198	0.01	100	18.7	45787	PASS
442	442	50	100	100.0	296981	PASS
443	442	15	24	19.3	57432	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/2/2025	BNA_F	<u>BF142273.D</u>
Compound Name	Response	Retention Time
DDT	646019	13.592
DDD	7521	13.322
DDE	403	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7924	653943	1.21

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050225\
Data File : BF142273.D
Acq On : 02 May 2025 10:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 02 11:49:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 30 16:00:01 2025
Response via : Initial Calibration

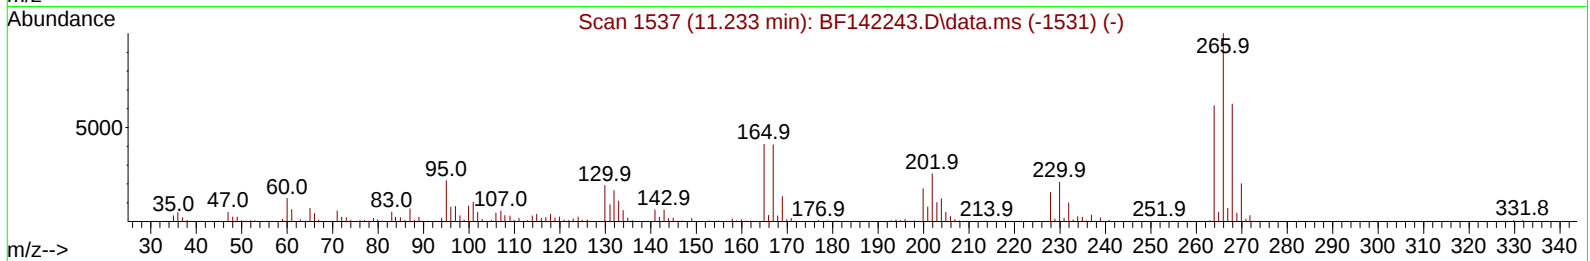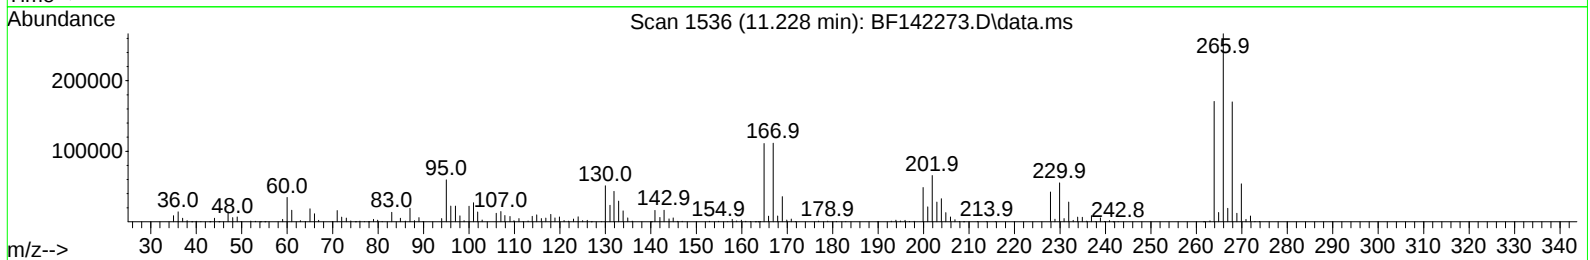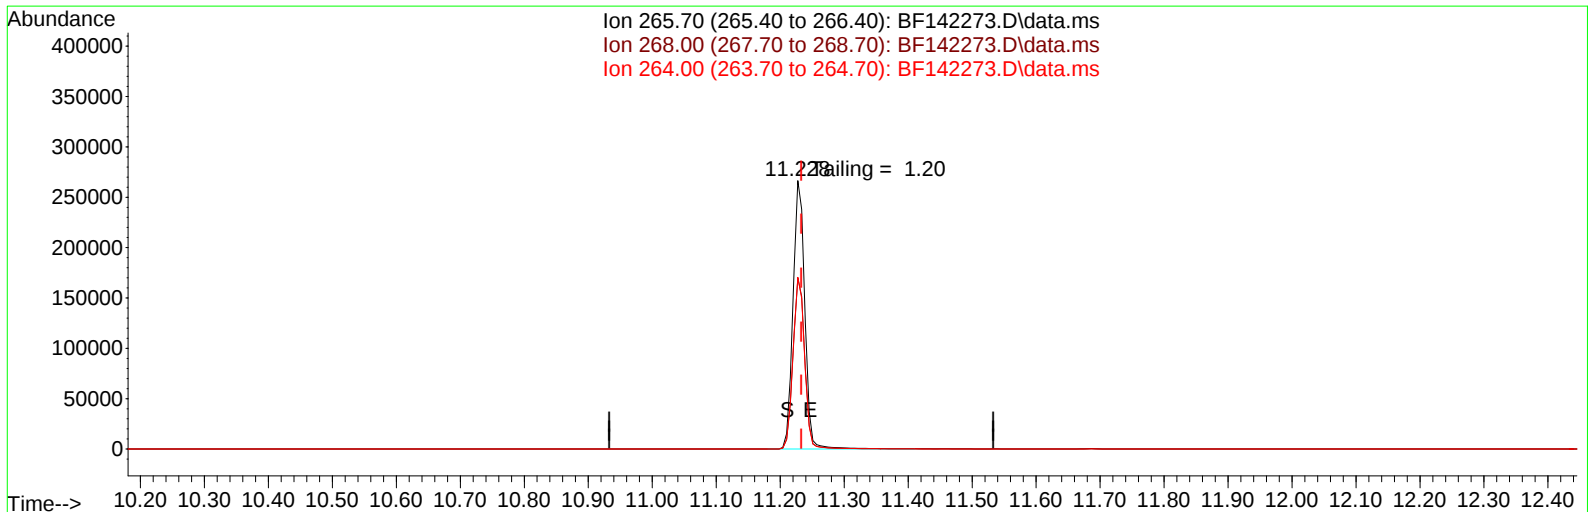

TIC: BF142273.D\data.ms

(70) Pentachlorophenol (C)

11.228min (-0.005) 200113.05 ng




response 342837

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	63.76
264.00	61.60	64.00
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050225\  
Data File : BF142273.D  
Acq On    : 02 May 2025  10:11  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 02 11:49:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 30 16:00:01 2025
Response via : Initial Calibration

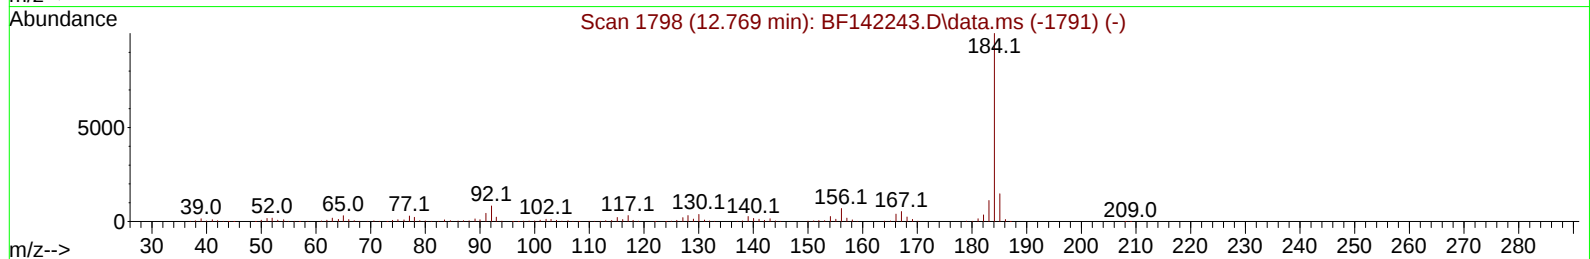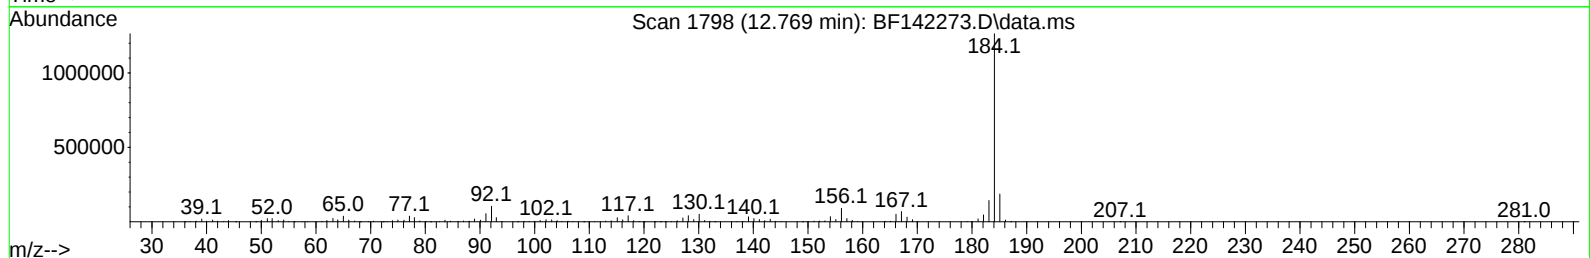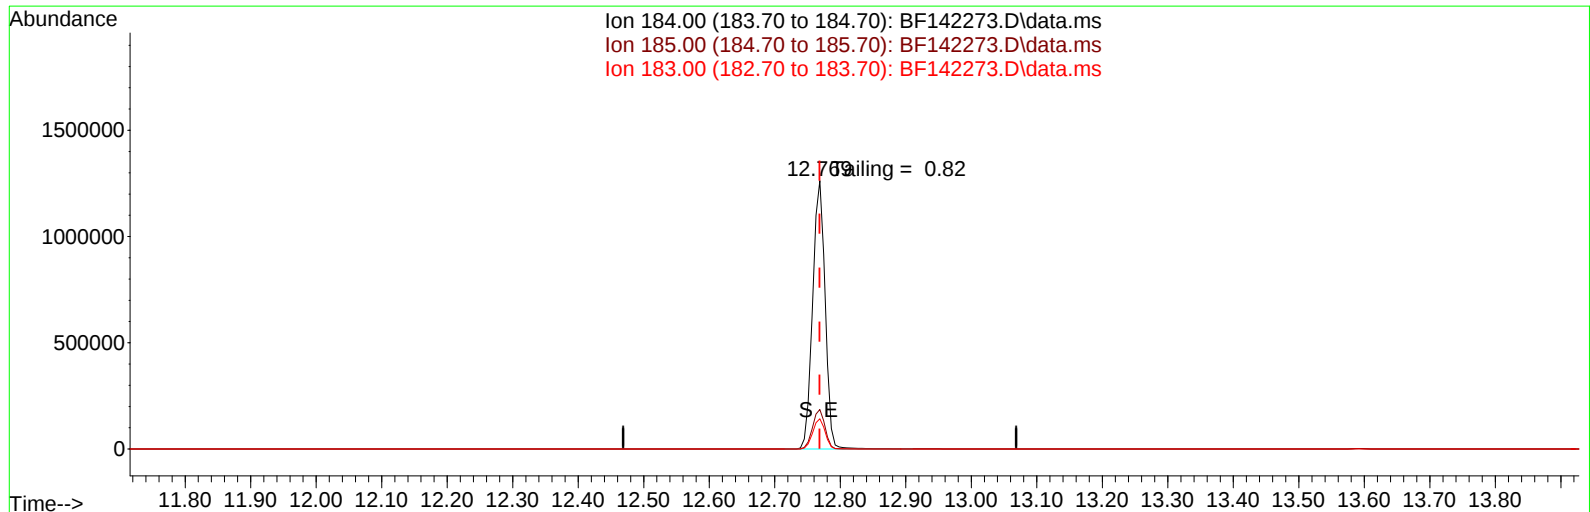

TIC: BF142273.D\data.ms

(77) Benzidine

12.769min (-0.000) 120826.54 ng

response **1673715**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.73
183.00	11.10	11.31
0.00	0.00	0.00