


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050525\
Data File : VN086477.D
Acq On : 05 May 2025 10:23
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
Title : SW846 8260
Last Update : Wed Apr 16 04:19:23 2025

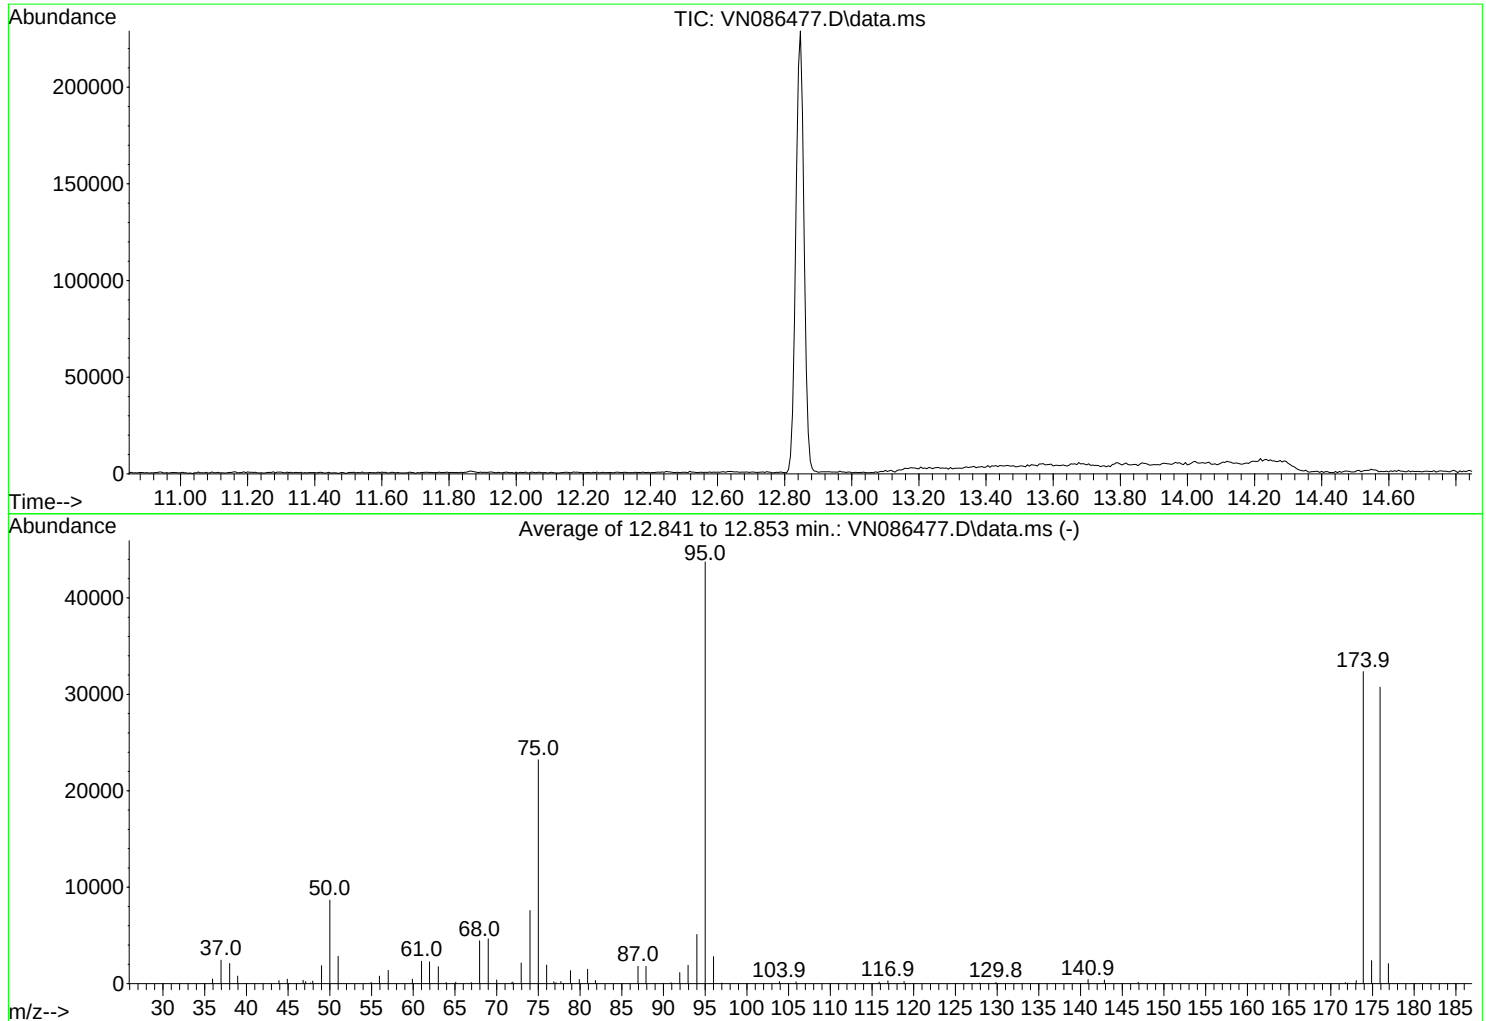

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.8	8661	PASS
75	95	30	60	53.1	23221	PASS
95	95	100	100	100.0	43739	PASS
96	95	5	9	6.4	2801	PASS
173	174	0.00	2	1.0	319	PASS
174	95	50	100	74.0	32349	PASS
175	174	5	9	7.4	2398	PASS
176	174	95	101	95.0	30739	PASS
177	176	5	9	6.8	2079	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	478	50.00	8661	66.95	115	77.10	101
36.95	2433	51.00	2835	67.95	4441	77.70	211
38.00	2086	54.95	140	69.00	4646	78.85	134
38.95	787	55.95	782	70.00	386	79.90	43
43.90	320	57.00	1377	71.80	89	80.90	1487
44.90	463	59.90	462	71.95	170	81.85	333
46.80	352	61.00	2317	72.95	2149	86.95	1803
47.10	210	61.95	2250	74.00	7577	87.90	1800
47.70	83	63.00	1766	75.00	23221	90.90	107
47.95	261	63.95	129	76.00	1918	91.95	1145
49.00	1858	65.10	145	76.85	201	92.95	1909

Average of 12.841 to 12.853 min.: VN086477.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.00	5096	140.90	431				
95.00	43739	142.85	380				
96.00	2801	146.90	148				
97.00	64	171.75	119				
103.90	213	172.00	59				
105.90	178	173.05	319				
115.85	164	173.90	32349				
116.90	299	174.90	2398				
118.85	240	175.90	30739				
127.90	50	176.90	2079				
129.85	136						

Instrument :

MSVOA_N

ClientSampleId :

BFB