

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050625\
 Data File : PL095532.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 May 2025 13:25
 Operator : AR\AJ
 Sample : PB167854BS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB167854BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 01:38:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 23 16:23:18 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.595	2.910	59205924	75217001	18.135	23.655 #
28)	SA Decachlor...	9.118	8.087	57125092	66896101	20.617	22.606
Target Compounds							
2)	A alpha-BHC	4.046	3.419	225.3E6	272.7E6	45.473	61.294 #
3)	MA gamma-BHC...	4.377	3.752	214.3E6	258.2E6	45.258	58.698 #
4)	MA Heptachlor	4.974	4.106	207.0E6	247.5E6	45.254	56.812 #
5)	MB Aldrin	5.316	4.391	223.2E6	250.1E6	48.603	60.770 #
6)	B beta-BHC	4.562	4.046	93978270	114.0E6	45.455	54.929
7)	B delta-BHC	0.000	4.282	0	262.6E6	N.D.	59.917 #
8)	B Heptachlo...	5.737	4.894	203.6E6	225.8E6	50.828	58.469
9)	A Endosulfan I	6.120	5.267	195.5E6	215.5E6	51.487	58.871
10)	B gamma-Chl...	5.991	5.147	208.1E6	236.1E6	51.007	58.247
11)	B alpha-Chl...	6.072	5.211	205.2E6	229.0E6	50.473	57.513
12)	B 4,4'-DDE	6.241	5.397	198.9E6	222.2E6	50.726	54.629
13)	MA Dieldrin	6.393	5.532	193.8E6	238.9E6	50.273	58.743
14)	MA Endrin	6.620	5.808	152.6E6	186.0E6	47.904	51.093
15)	B Endosulfa...	6.832	6.097	168.3E6	208.2E6	52.725	57.977
16)	A 4,4'-DDD	6.750	5.949	152.3E6	199.8E6	53.787	61.151
17)	MA 4,4'-DDT	7.065	6.203	137.6E6	172.3E6	48.316	50.149
18)	B Endrin al...	6.961	6.275	121.8E6	156.2E6	52.484	59.783
19)	B Endosulfa...	7.195	6.498	143.0E6	192.6E6	51.031	58.045
20)	A Methoxychlor	7.536	6.772	62467040	139.4E6	44.775	73.077 #
21)	B Endrin ke...	7.675	7.004	150.2E6	226.4E6	52.687	64.305
22)	Mirex	8.157	7.200	117.9E6	183.2E6	49.637	63.547 #
24)	Chlordane-2	5.316f	0.000	223.2E6	0	1054.409	N.D. #
25)	Chlordane-3	5.991	5.147	208.1E6	236.1E6	267.131	456.923 #
26)	Chlordane-4	6.072	5.211	205.2E6	229.0E6	217.651	526.824 #
27)	Chlordane-5	0.000	6.097	0	208.2E6	N.D.	1126.998 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050625\
Data File : PL095532.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2025 13:25
Operator : AR\AJ
Sample : PB167854BS
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB167854BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 01:38:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
Quant Title : GC Extractables
QLast Update : Wed Apr 23 16:23:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

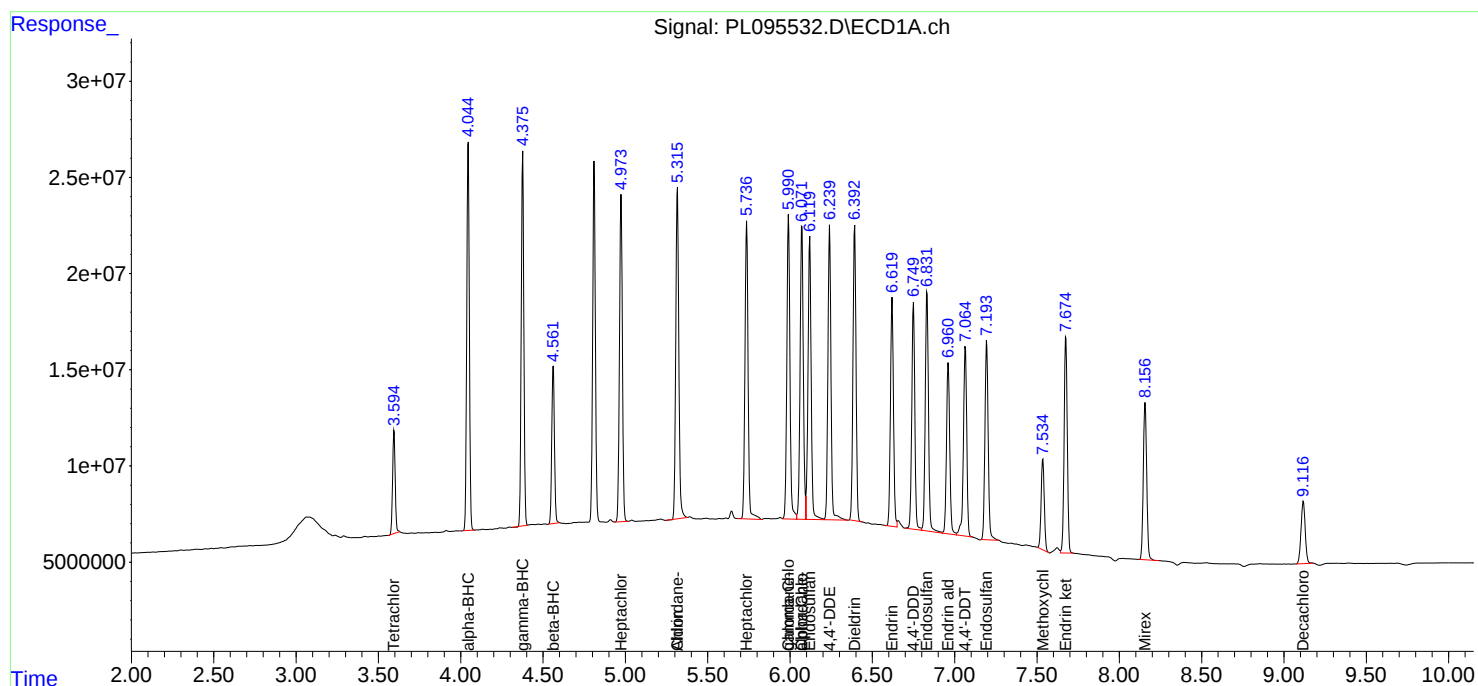


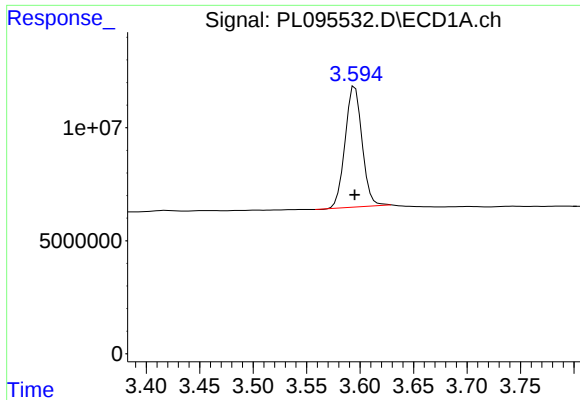

#1 Tetrachloro-m-xylene


R.T.: 3.595 min
Delta R.T.: 0.000 min
Response: 59205924
Conc: 18.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB167854BS

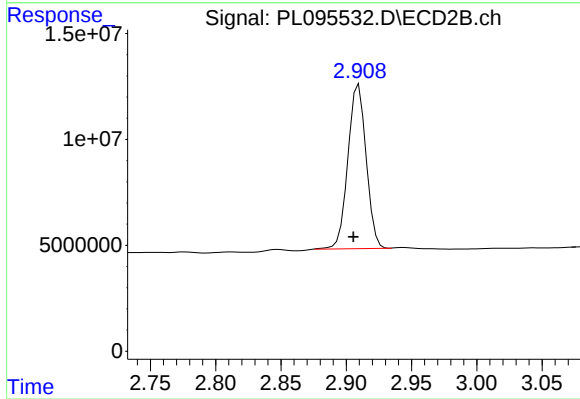


#1 Tetrachloro-m-xylene

R.T.: 2.910 min
Delta R.T.: 0.004 min
Response: 75217001
Conc: 23.65 ng/ml

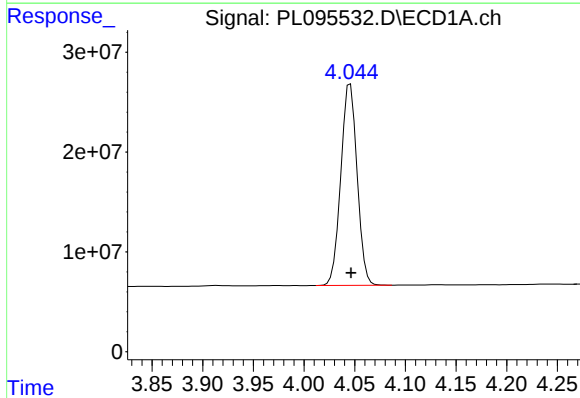


#2 alpha-BHC

R.T.: 4.046 min
Delta R.T.: 0.000 min
Response: 225264012
Conc: 45.47 ng/ml

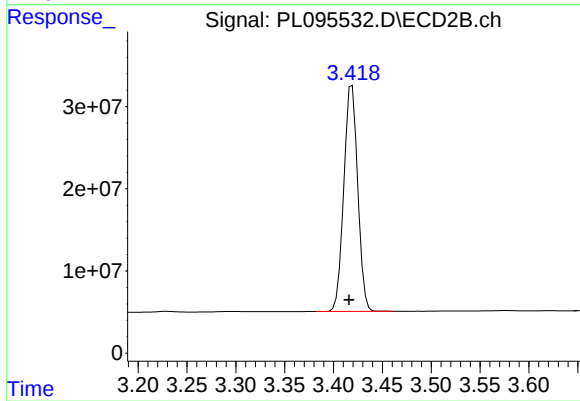

#2 alpha-BHC


R.T.: 3.419 min
Delta R.T.: 0.003 min
Response: 272680033
Conc: 61.29 ng/ml

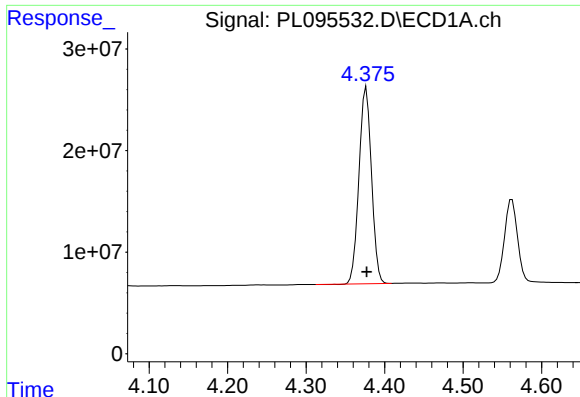

#3 gamma-BHC (Lindane)


R.T.: 4.377 min
Delta R.T.: 0.000 min
Response: 214250372
Conc: 45.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB167854BS

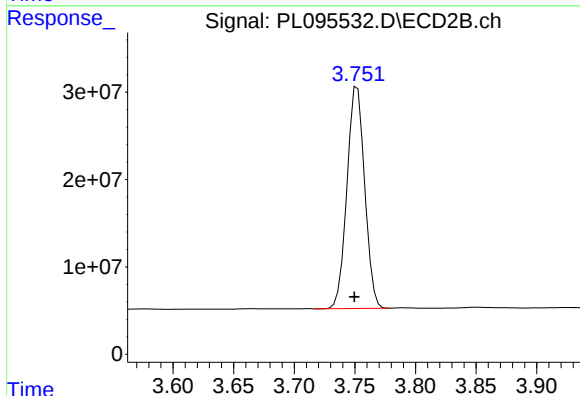


#3 gamma-BHC (Lindane)

R.T.: 3.752 min
Delta R.T.: 0.002 min
Response: 258166044
Conc: 58.70 ng/ml

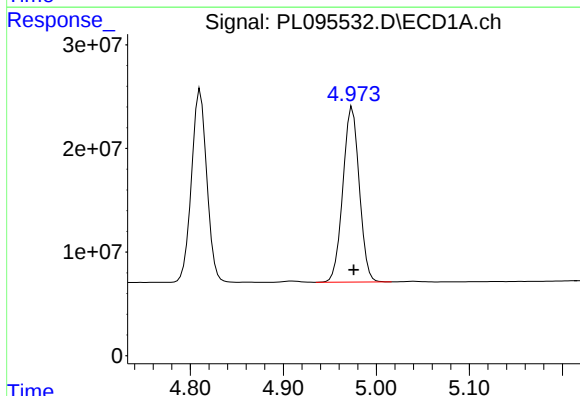


#4 Heptachlor

R.T.: 4.974 min
Delta R.T.: -0.002 min
Response: 207011288
Conc: 45.25 ng/ml

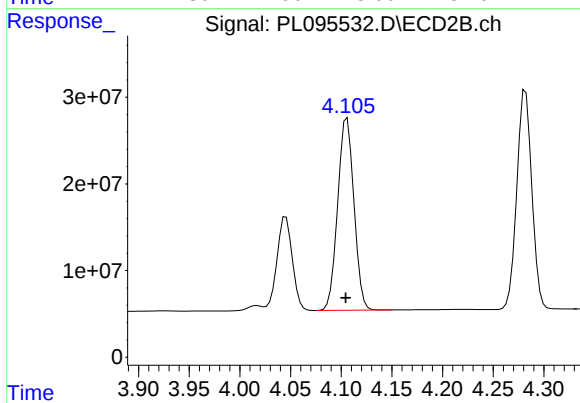

#4 Heptachlor


R.T.: 4.106 min
Delta R.T.: 0.001 min
Response: 247513256
Conc: 56.81 ng/ml

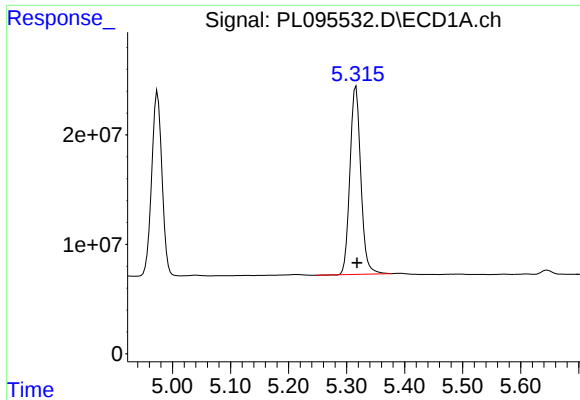

#5 Aldrin


R.T.: 5.316 min
Delta R.T.: -0.002 min
Response: 223234915
Conc: 48.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB167854BS

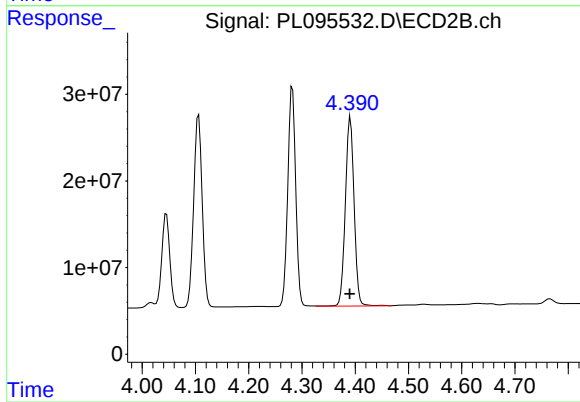


#5 Aldrin

R.T.: 4.391 min
Delta R.T.: 0.000 min
Response: 250111035
Conc: 60.77 ng/ml

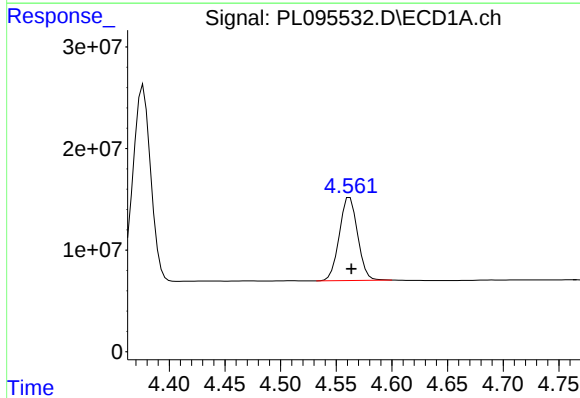


#6 beta-BHC

R.T.: 4.562 min
Delta R.T.: -0.001 min
Response: 93978270
Conc: 45.45 ng/ml

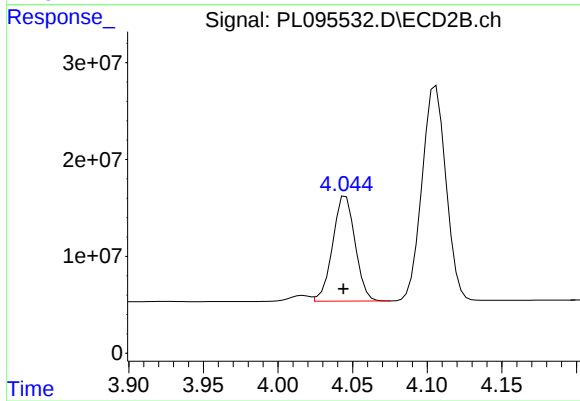

#6 beta-BHC


R.T.: 4.046 min
Delta R.T.: 0.002 min
Response: 114025774
Conc: 54.93 ng/ml

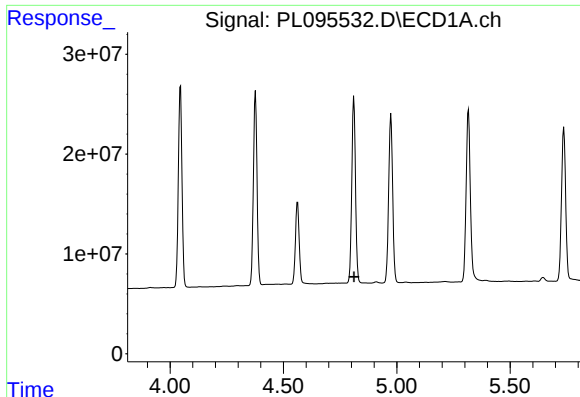

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.812 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB167854BS

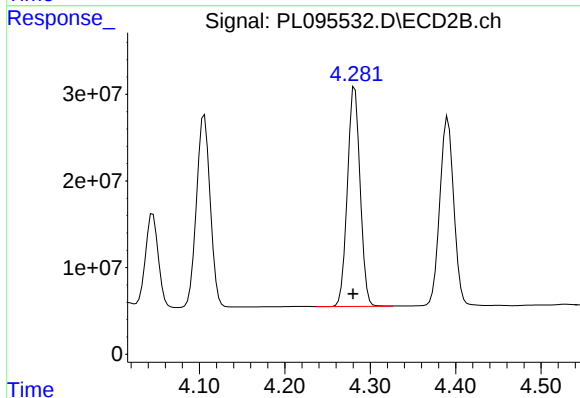


#7 delta-BHC

R.T.: 4.282 min
Delta R.T.: 0.002 min
Response: 262552092
Conc: 59.92 ng/ml

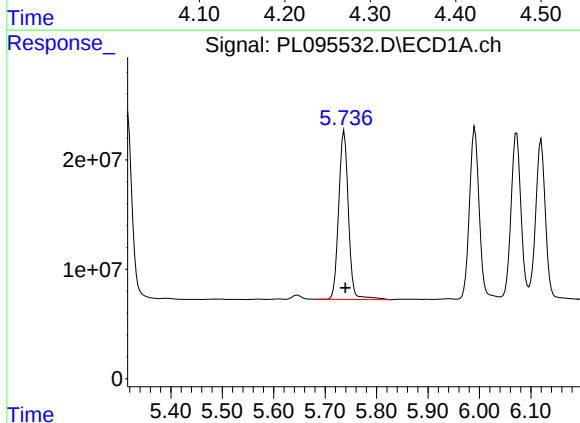


#8 Heptachlor epoxide

R.T.: 5.737 min
Delta R.T.: -0.002 min
Response: 203574483
Conc: 50.83 ng/ml

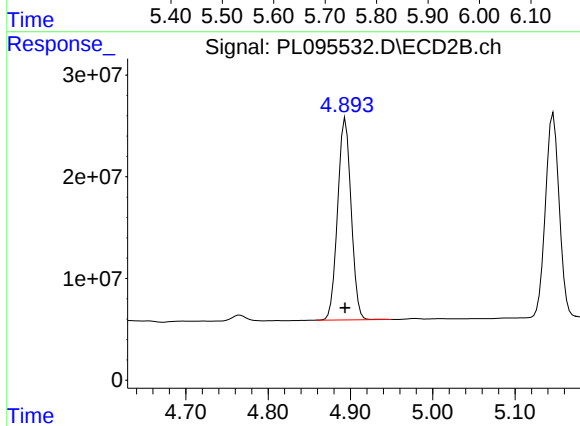

#8 Heptachlor epoxide


R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 225846599
Conc: 58.47 ng/ml

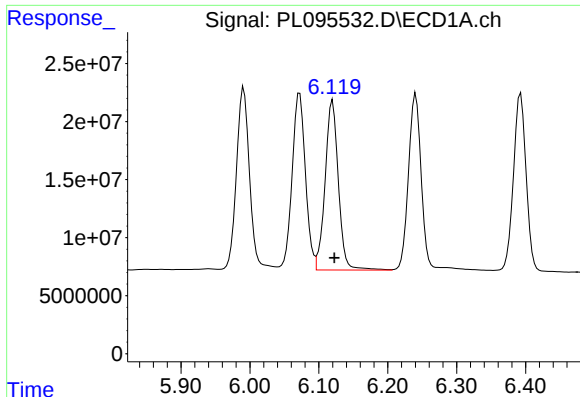

#9 Endosulfan I


R.T.: 6.120 min
Delta R.T.: -0.002 min
Response: 195521782
Conc: 51.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB167854BS

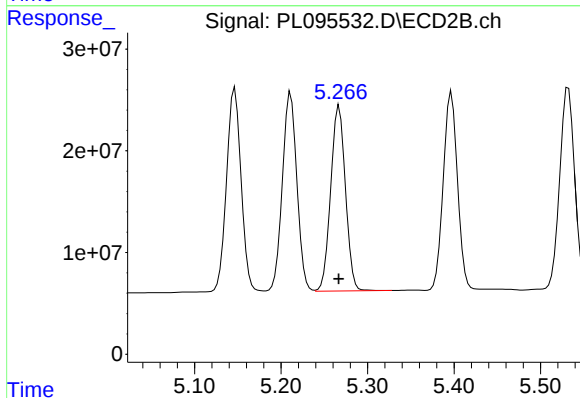


#9 Endosulfan I

R.T.: 5.267 min
Delta R.T.: 0.000 min
Response: 215493118
Conc: 58.87 ng/ml

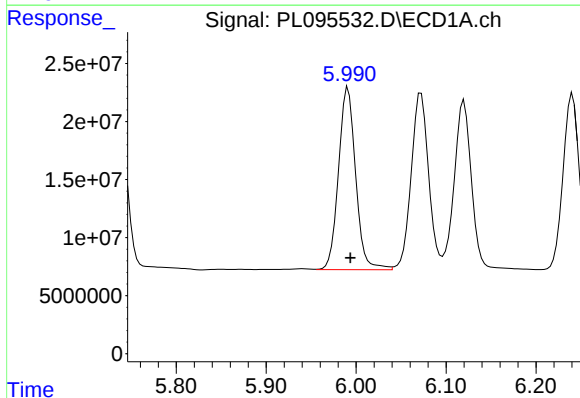


#10 gamma-Chlordane

R.T.: 5.991 min
Delta R.T.: -0.002 min
Response: 208075693
Conc: 51.01 ng/ml

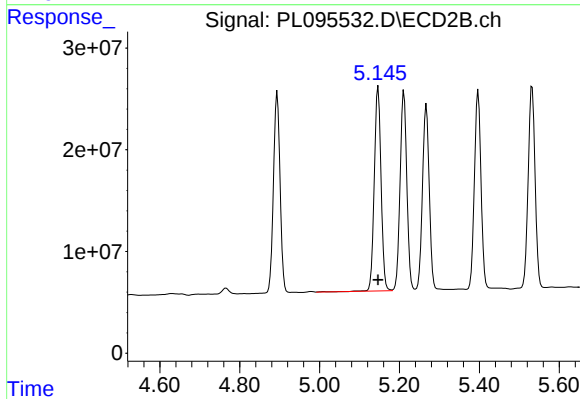

#10 gamma-Chlordane


R.T.: 5.147 min
Delta R.T.: 0.000 min
Response: 236056472
Conc: 58.25 ng/ml

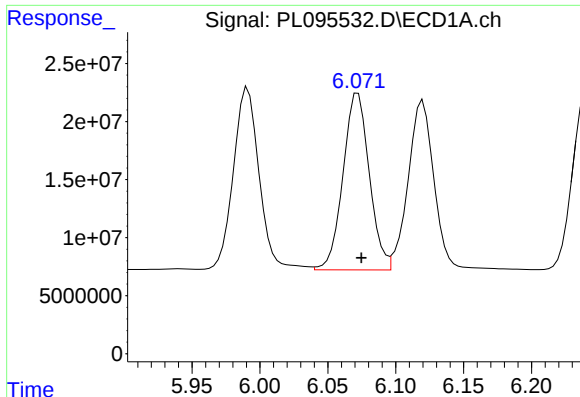

#11 alpha-Chlordane


R.T.: 6.072 min
Delta R.T.: -0.003 min
Response: 205229272
Conc: 50.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB167854BS

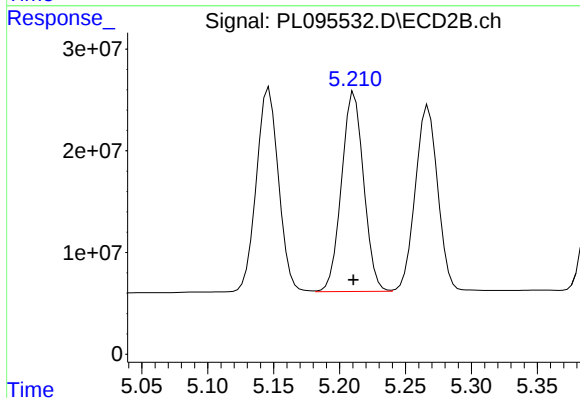


#11 alpha-Chlordane

R.T.: 5.211 min
Delta R.T.: 0.000 min
Response: 228963999
Conc: 57.51 ng/ml

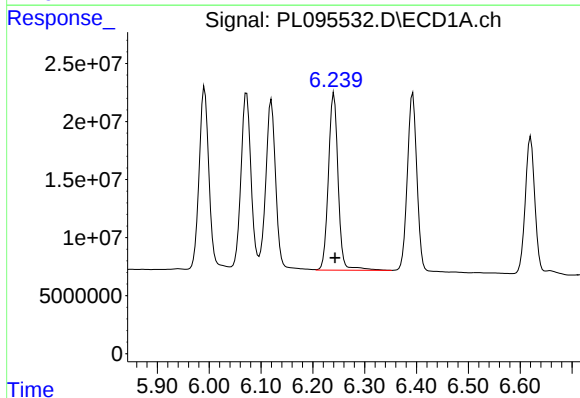


#12 4,4'-DDE

R.T.: 6.241 min
Delta R.T.: -0.002 min
Response: 198872490
Conc: 50.73 ng/ml

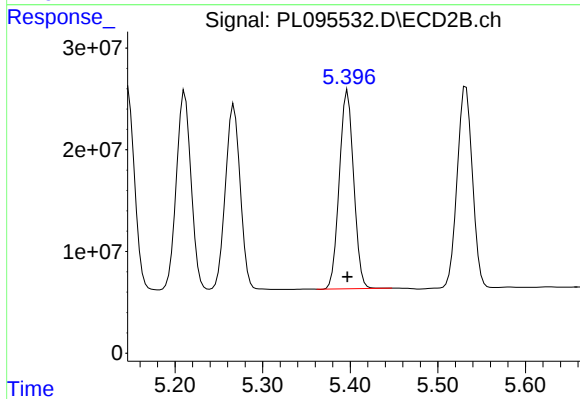

#12 4,4'-DDE


R.T.: 5.397 min
Delta R.T.: 0.000 min
Response: 222176370
Conc: 54.63 ng/ml

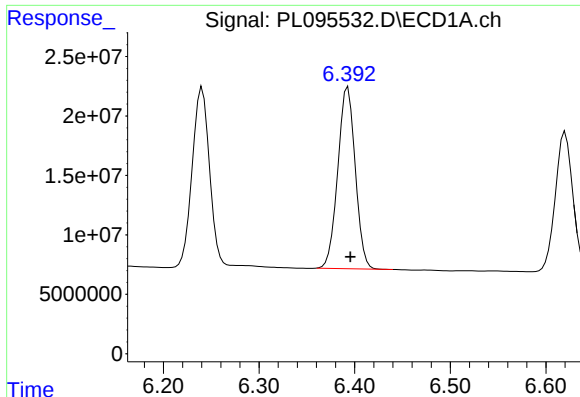

#13 Dieldrin


R.T.: 6.393 min
Delta R.T.: -0.003 min
Response: 193793802
Conc: 50.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB167854BS

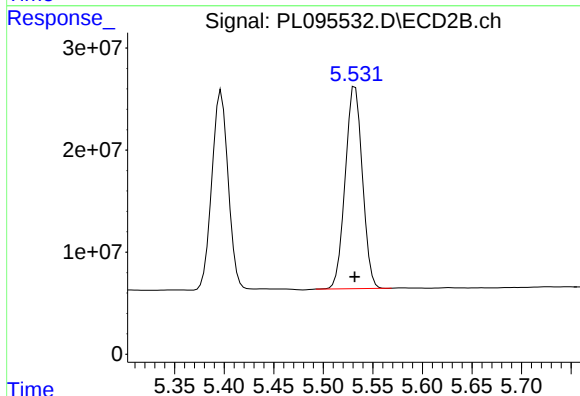


#13 Dieldrin

R.T.: 5.532 min
Delta R.T.: 0.000 min
Response: 238913582
Conc: 58.74 ng/ml

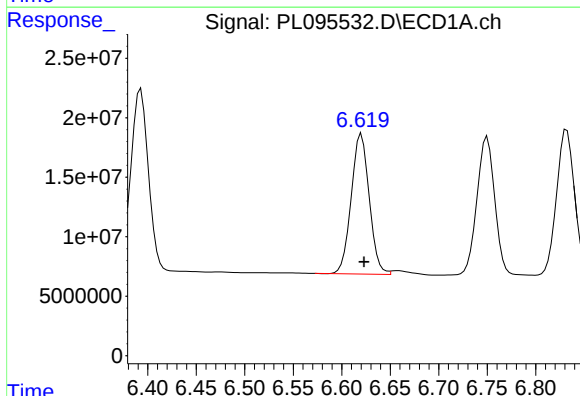


#14 Endrin

R.T.: 6.620 min
Delta R.T.: -0.003 min
Response: 152560839
Conc: 47.90 ng/ml

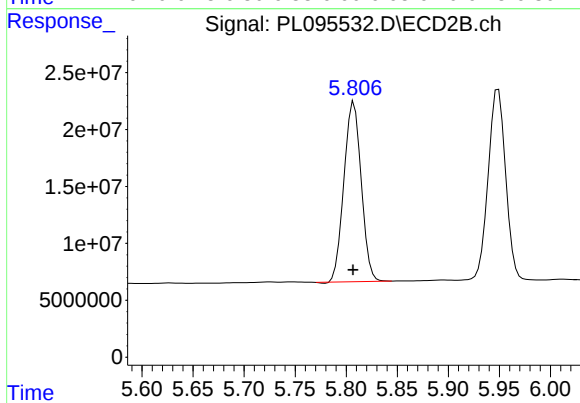

#14 Endrin


R.T.: 5.808 min
Delta R.T.: 0.000 min
Response: 186014130
Conc: 51.09 ng/ml

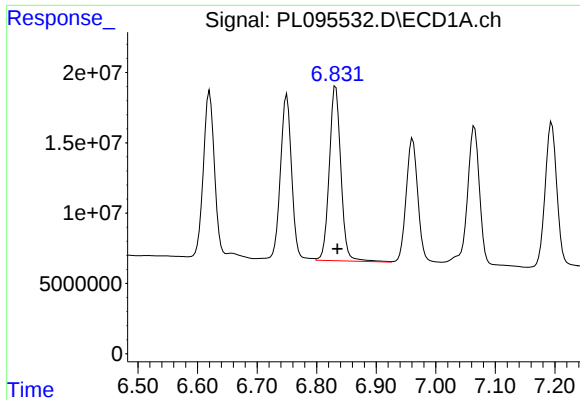

#15 Endosulfan II


R.T.: 6.832 min
Delta R.T.: -0.003 min
Response: 168306143
Conc: 52.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB167854BS

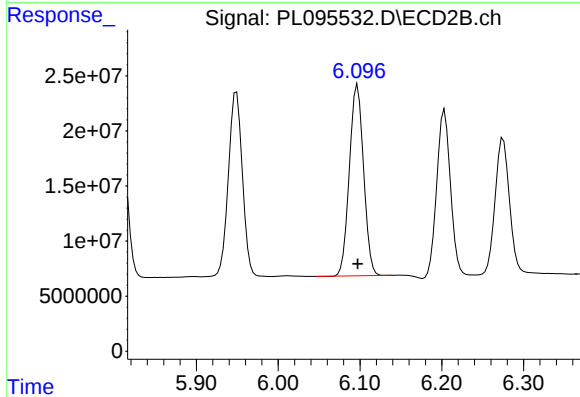


#15 Endosulfan II

R.T.: 6.097 min
Delta R.T.: 0.000 min
Response: 208200241
Conc: 57.98 ng/ml

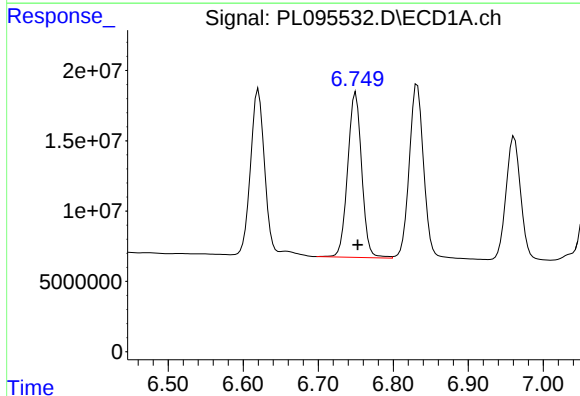


#16 4,4'-DDD

R.T.: 6.750 min
Delta R.T.: -0.003 min
Response: 152269168
Conc: 53.79 ng/ml

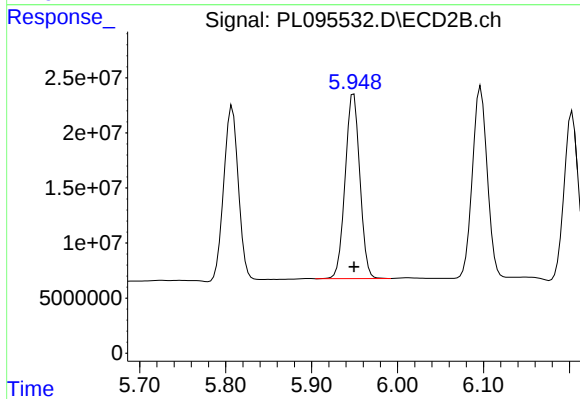

#16 4,4'-DDD


R.T.: 5.949 min
Delta R.T.: 0.000 min
Response: 199767830
Conc: 61.15 ng/ml

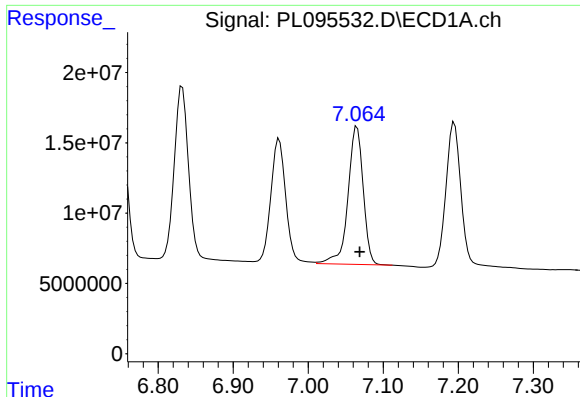

#17 4,4'-DDT


R.T.: 7.065 min
Delta R.T.: -0.004 min
Response: 137631752
Conc: 48.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB167854BS

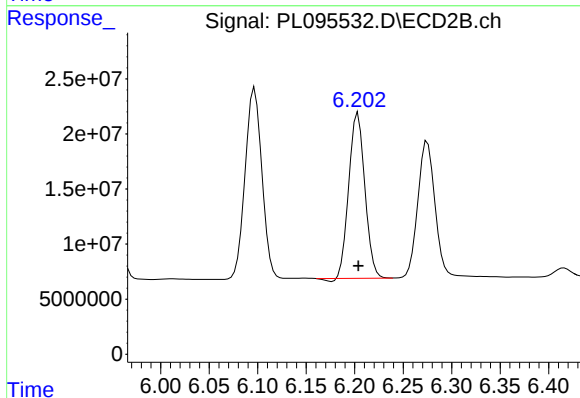


#17 4,4'-DDT

R.T.: 6.203 min
Delta R.T.: 0.000 min
Response: 172320528
Conc: 50.15 ng/ml

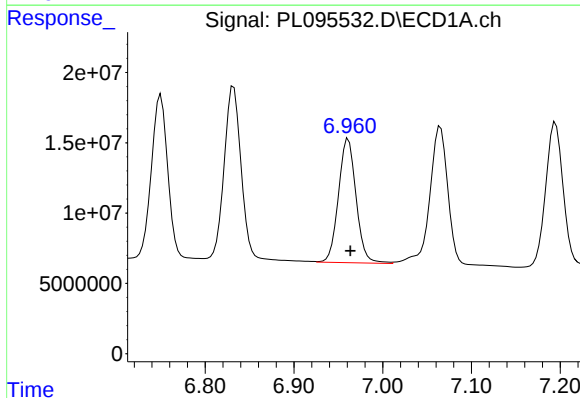


#18 Endrin aldehyde

R.T.: 6.961 min
Delta R.T.: -0.002 min
Response: 121804709
Conc: 52.48 ng/ml

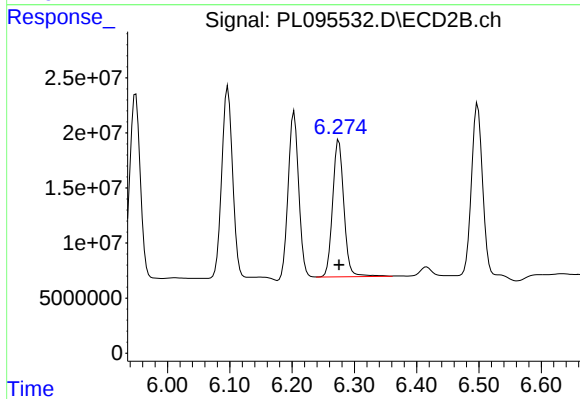

#18 Endrin aldehyde


R.T.: 6.275 min
Delta R.T.: 0.000 min
Response: 156222153
Conc: 59.78 ng/ml

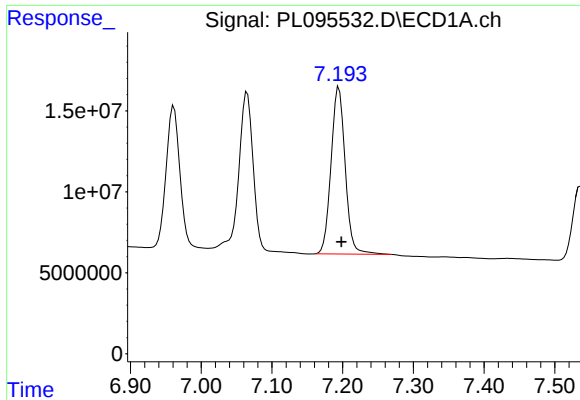

#19 Endosulfan Sulfate


R.T.: 7.195 min
Delta R.T.: -0.003 min
Response: 142977143
Conc: 51.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB167854BS

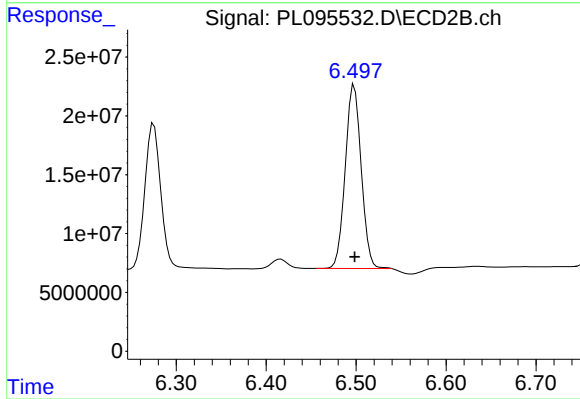


#19 Endosulfan Sulfate

R.T.: 6.498 min
Delta R.T.: 0.000 min
Response: 192590373
Conc: 58.05 ng/ml

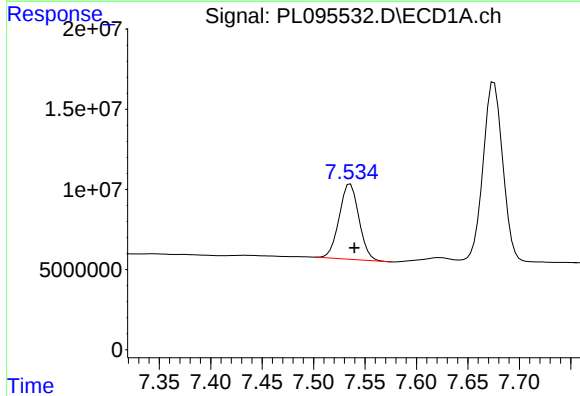


#20 Methoxychlor

R.T.: 7.536 min
Delta R.T.: -0.004 min
Response: 62467040
Conc: 44.78 ng/ml

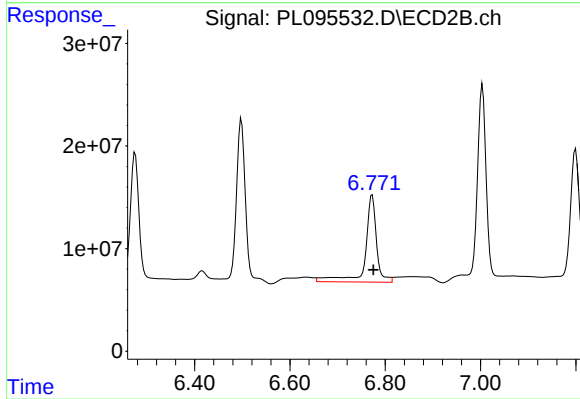

#20 Methoxychlor


R.T.: 6.772 min
Delta R.T.: -0.002 min
Response: 139389759
Conc: 73.08 ng/ml

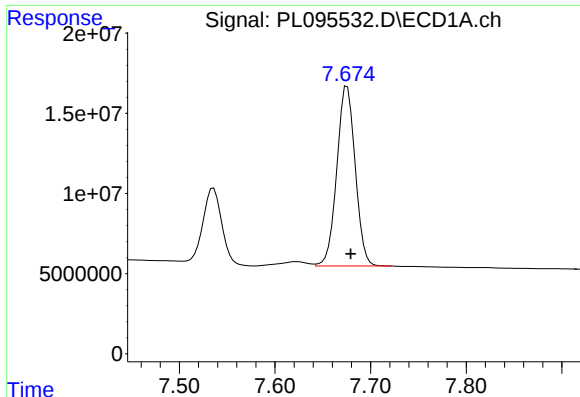

#21 Endrin ketone


R.T.: 7.675 min
Delta R.T.: -0.004 min
Response: 150204921
Conc: 52.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB167854BS

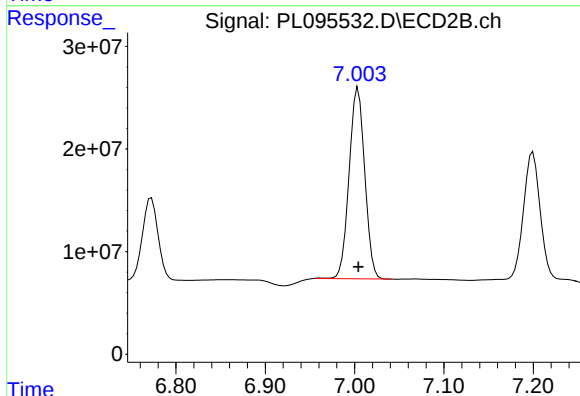


#21 Endrin ketone

R.T.: 7.004 min
Delta R.T.: 0.000 min
Response: 226438108
Conc: 64.31 ng/ml

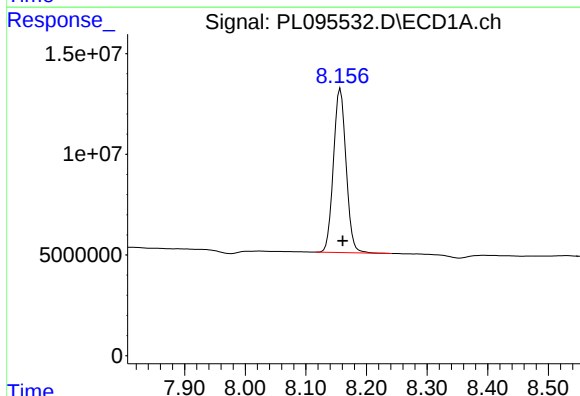


#22 Mirex

R.T.: 8.157 min
Delta R.T.: -0.004 min
Response: 117938847
Conc: 49.64 ng/ml

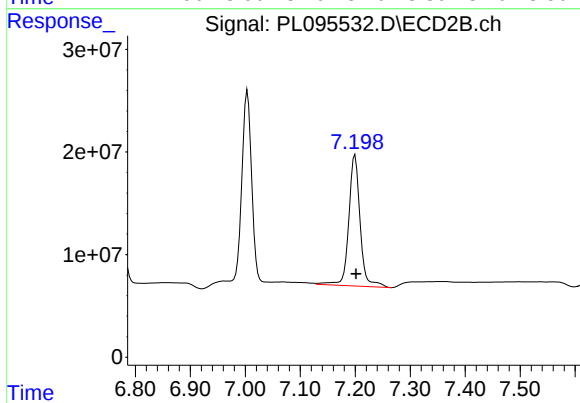

#22 Mirex


R.T.: 7.200 min
Delta R.T.: -0.002 min
Response: 183166555
Conc: 63.55 ng/ml

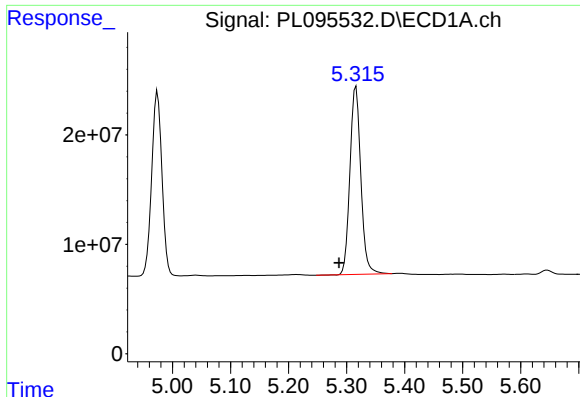

#24 Chlordane-2


R.T.: 5.316 min
Delta R.T.: 0.029 min
Response: 223234915
Conc: 1054.41 ng/m

Instrument :
ECD_L
ClientSampleId :
PB167854BS

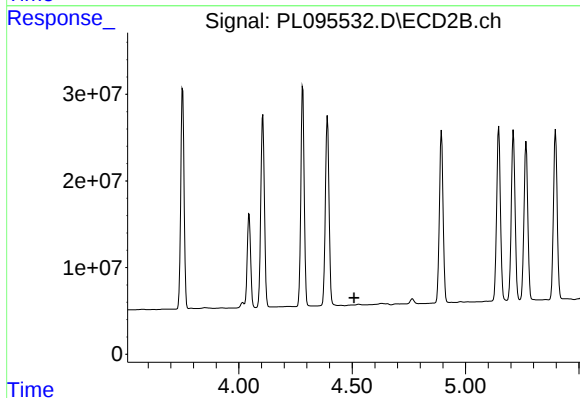


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.508 min
Response: 0
Conc: N.D.

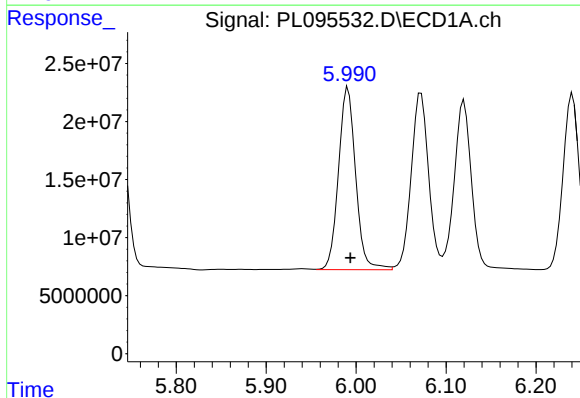


#25 Chlordane-3

R.T.: 5.991 min
Delta R.T.: -0.003 min
Response: 208075693
Conc: 267.13 ng/ml

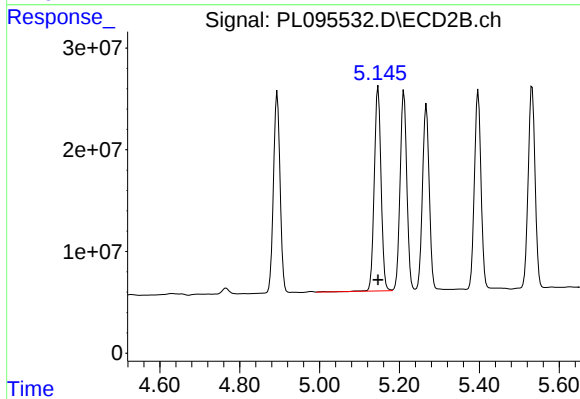

#25 Chlordane-3


R.T.: 5.147 min
Delta R.T.: 0.000 min
Response: 236056472
Conc: 456.92 ng/ml

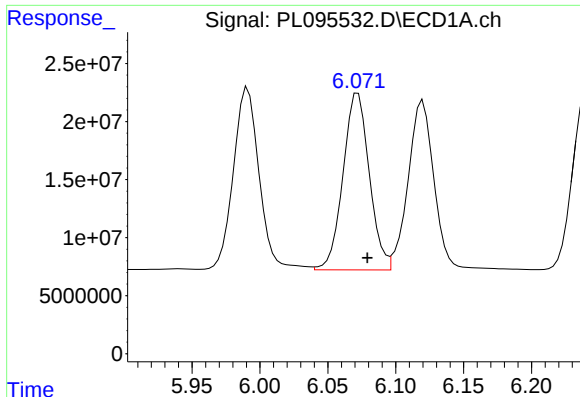

#26 Chlordane-4


R.T.: 6.072 min
Delta R.T.: -0.007 min
Response: 205229272
Conc: 217.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB167854BS

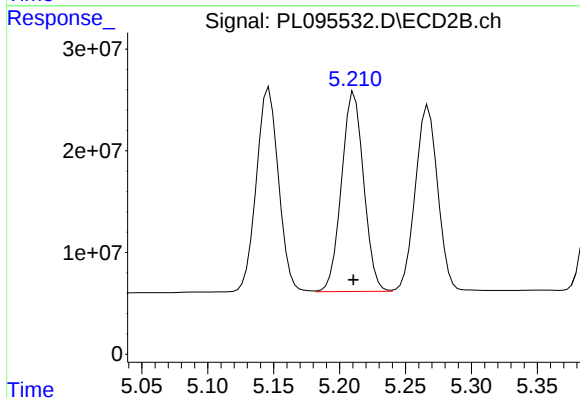


#26 Chlordane-4

R.T.: 5.211 min
Delta R.T.: 0.000 min
Response: 228963999
Conc: 526.82 ng/ml

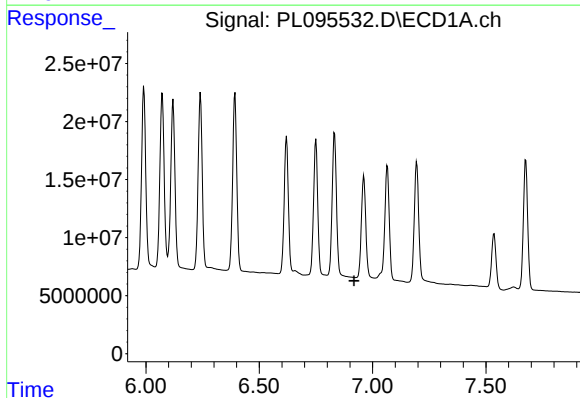


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.919 min
Response: 0
Conc: N.D.

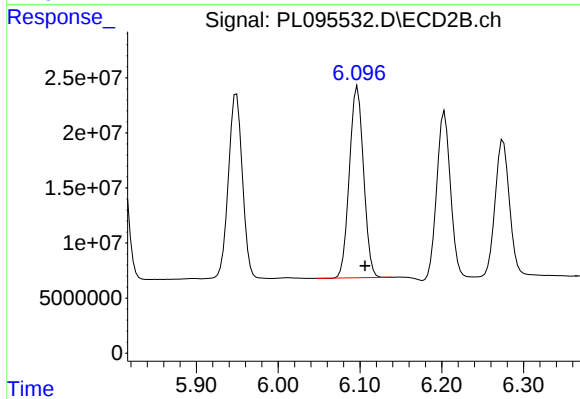

#27 Chlordane-5


R.T.: 6.097 min
Delta R.T.: -0.009 min
Response: 208200241
Conc: 1127.00 ng/ml

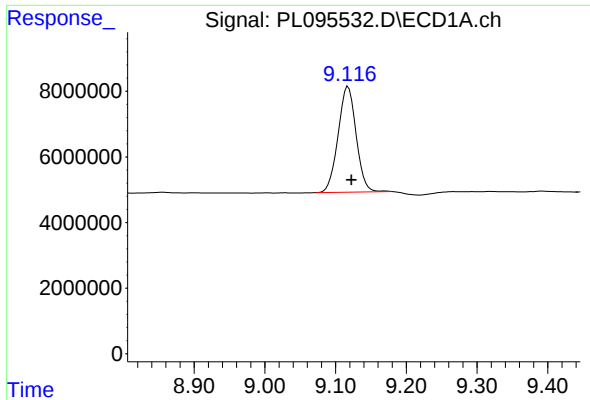

#28 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: -0.004 min
Response: 57125092
Conc: 20.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB167854BS

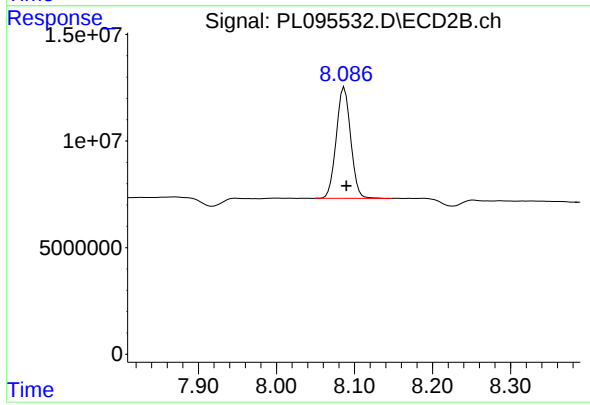

#28 Decachlorobiphenyl

R.T.: 8.087 min
Delta R.T.: -0.002 min
Response: 66896101
Conc: 22.61 ng/ml