

## Prep Standard - Chemical Standard Summary

**Order ID :** Q1939

**Test :** EPH\_NF

**Prepbatch ID :** PB167833,

**Sequence ID/Qc Batch ID:** FC050225AL,FC050525AL,FE050225AL,FE050525AL,FE050625AL,

**Standard ID :**

EP2600,EP2607,PP24170,PP24174,PP24175,PP24176,PP24177,PP24178,PP24179,PP24462,PP24465,PP24491,

**Chemical ID :**

E2865,E3551,E3904,E3916,E3917,E3928,E3929,P12363,P12981,P12983,P12989,P12990,P13050,P13279,P13596,P13650,P13660,P13662,P13664,P13667,P13671,P13709,P13762,P13764,P13865,P13896,P13897,P13898,P13899,P13900,P13901,P13903,P13905,P13906,P13912,P13919,P13920,P13921,P13923,P13926,P13927,P13928,P13931,P13947,P13948,W3177,

## Extractions STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>                    | <u>NO.</u>             | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------------------|------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 2017             | 1:1 ACETONE/METHYLENE CHLORIDE | <a href="#">EP2600</a> | 04/07/2025       | 10/03/2025             | Rajesh Parikh      | None           | None             | Riteshkumar Patel    |
|                  |                                |                        |                  |                        |                    |                |                  | 04/07/2025           |

**FROM** 8000.00000ml of E3904 + 8000.00000ml of E3917 = Final Quantity: 16000.000 ml

| <u>Recipe ID</u> | <u>NAME</u>          | <u>NO.</u>             | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u>                | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|----------------------|------------------------|------------------|------------------------|--------------------|-------------------------------|------------------|----------------------|
| 3923             | Baked Sodium Sulfate | <a href="#">EP2607</a> | 04/25/2025       | 07/01/2025             | RUPESEKUMAR SHAH   | Extraction_SC ALE_2 (EX-SC-2) | None             | Riteshkumar Patel    |
|                  |                      |                        |                  |                        |                    |                               |                  | 04/25/2025           |

**FROM** 4000.00000gram of E3551 = Final Quantity: 4000.000 gram

## Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>                               | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 781              | 100 PPM Aliphatic HC Working STD (Restek) | <a href="#">PP24170</a> | 02/03/2025       | 08/03/2025             | Yogesh Patel       | None           | None             | Ankita Jodhani       |
|                  |                                           |                         |                  |                        |                    |                |                  | 02/03/2025           |

**FROM** 0.25000ml of P12981 + 0.25000ml of P13671 + 1.25000ml of P12363 + 23.25000ml of W3177 = Final Quantity: 25.000 ml

| <u>Recipe ID</u> | <u>NAME</u>                         | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 2900             | 100 PPM Aliphatic HC STD (Absolute) | <a href="#">PP24174</a> | 02/03/2025       | 08/03/2025             | Yogesh Patel       | None           | None             | Ankita Jodhani       |
|                  |                                     |                         |                  |                        |                    |                |                  | 02/03/2025           |

**FROM** 0.25000ml of P12983 + 0.25000ml of P13650 + 2.50000ml of P13279 + 22.00000ml of W3177 = Final Quantity: 25.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>             | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 783              | 50 PPM Aliphatic HC STD | <a href="#">PP24175</a> | 02/03/2025       | 08/03/2025             | Yogesh Patel       | None           | None             | Ankita Jodhani       |
|                  |                         |                         |                  |                        |                    |                |                  | 02/03/2025           |

**FROM** 0.50000ml of W3177 + 0.50000ml of PP24170 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u>             | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 784              | 20 PPM Aliphatic HC STD | <a href="#">PP24176</a> | 02/03/2025       | 08/03/2025             | Yogesh Patel       | None           | None             | Ankita Jodhani       |
|                  |                         |                         |                  |                        |                    |                |                  | 02/03/2025           |

**FROM** 0.80000ml of W3177 + 0.20000ml of PP24170 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>             | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 785              | 10 PPM Aliphatic HC STD | <a href="#">PP24177</a> | 02/03/2025       | 08/03/2025             | Yogesh Patel       | None           | None             | Ankita Jodhani       |
|                  |                         |                         |                  |                        |                    |                |                  | 02/03/2025           |

**FROM** 0.90000ml of W3177 + 0.10000ml of PP24170 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u>            | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 786              | 5 PPM Aliphatic HC STD | <a href="#">PP24178</a> | 02/03/2025       | 08/03/2025             | Yogesh Patel       | None           | None             | Ankita Jodhani       |
|                  |                        |                         |                  |                        |                    |                |                  | 02/03/2025           |

**FROM** 0.90000ml of W3177 + 0.10000ml of PP24175 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>                            | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|----------------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 2901             | 20 PPM Aliphatic HC STD ICV (Absolute) | <a href="#">PP24179</a> | 02/03/2025       | 08/03/2025             | Yogesh Patel       | None           | None             | Ankita Jodhani       |
|                  |                                        |                         |                  |                        |                    |                |                  | 02/03/2025           |

**FROM** 0.80000ml of W3177 + 0.20000ml of PP24174 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u>                  | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 1330             | 100 PPM NJEPH Spike Solution | <a href="#">PP24462</a> | 04/15/2025       | 10/15/2025             | Yogesh Patel       | None           | None             | Abdul Mirza          |
|                  |                              |                         |                  |                        |                    |                |                  | 04/21/2025           |

**FROM** 5.00000ml of P13709 + 5.00000ml of P13865 + 5.00000ml of P13896 + 5.00000ml of P13897 + 5.00000ml of P13898 + 5.00000ml of P13899 + 5.00000ml of P13900 + 5.00000ml of P13901 + 5.00000ml of P13903 + 5.00000ml of P13905 + 5.00000ml of P13906 + 5.00000ml of P13912 + 5.00000ml of P13919 + 5.00000ml of P13920 + 5.00000ml of P13921 + 5.00000ml of P13923 + 5.00000ml of P13926 + 5.00000ml of P13927 + 5.00000ml of P13928 + 5.00000ml of P13931 = Final Quantity: 100.000 ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## CHEMICAL RECEIPT LOG BOOK

| Supplier         | ItemCode / ItemName                      | Lot #      | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|------------------------------------------|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-3382-05 / Sand, Purified (cs/4x2.5kg) | 0000243821 | 06/30/2025      | 04/30/2020 / RAJESH     | 04/28/2020 / RAJESH         | E2865          |

| Supplier                    | ItemCode / ItemName                                    | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|-----------------------------|--------------------------------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| PCI Scientific Supply, Inc. | PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1 | 313201 | 07/01/2025      | 01/03/2024 / Rajesh     | 07/20/2023 / Rajesh         | E3551          |

| Supplier         | ItemCode / ItemName                                         | Lot #      | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|-------------------------------------------------------------|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L) | 24K1762005 | 01/07/2026      | 03/13/2025 /            | 12/27/2024 / RUPESH         | E3904          |

| Supplier         | ItemCode / ItemName                       | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|-------------------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L) | 243570 | 10/03/2025      | 04/03/2025 / Rajesh     | 03/31/2025 / Rajesh         | E3916          |

| Supplier         | ItemCode / ItemName                        | Lot #      | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|--------------------------------------------|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9254-03 / Acetone, Ultra Resi (cs/4x4L) | 24H2762008 | 10/03/2025      | 04/03/2025 / Rajesh     | 03/31/2025 / Rajesh         | E3917          |

| Supplier         | ItemCode / ItemName                       | Lot #      | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|-------------------------------------------|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L) | 25C0362005 | 10/22/2025      | 04/18/2025 / RUPESH     | 04/16/2025 / RUPESH         | E3928          |



## CHEMICAL RECEIPT LOG BOOK

| Supplier         | ItemCode / ItemName                        | Lot #      | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|--------------------------------------------|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9254-03 / Acetone, Ultra Resi (cs/4x4L) | 24H2762008 | 04/18/2027      | 04/18/2025 / RUPESH     | 04/16/2025 / RUPESH         | E3929          |

| Supplier | ItemCode / ItemName                                  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|------------------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 30540 / Custom NJEPH Aliphatics Calibration Standard | A0190424 | 08/03/2025      | 02/03/2025 / yogesh     | 03/16/2023 / Yogesh         | P12363         |

| Supplier | ItemCode / ItemName                 | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31098 / 1-Chlorooctadecane Standard | A0204989 | 08/03/2025      | 02/03/2025 / yogesh     | 12/20/2023 / Yogesh         | P12981         |

| Supplier | ItemCode / ItemName                 | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31098 / 1-Chlorooctadecane Standard | A0204989 | 08/03/2025      | 02/03/2025 / yogesh     | 12/20/2023 / Yogesh         | P12983         |

| Supplier | ItemCode / ItemName                 | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31098 / 1-Chlorooctadecane Standard | A0204989 | 10/25/2025      | 04/25/2025 / Abdul      | 12/20/2023 / Yogesh         | P12989         |

| Supplier | ItemCode / ItemName                 | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31098 / 1-Chlorooctadecane Standard | A0204989 | 10/25/2025      | 04/25/2025 / Abdul      | 12/20/2023 / Yogesh         | P12990         |

## CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName                       | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31098 /<br>1-Chlorooctadecane<br>Standard | A0200707 | 10/25/2025      | 04/25/2025 /<br>Abdul   | 12/26/2023 /<br>Yogesh      | P13050         |

| Supplier                 | ItemCode / ItemName                                             | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|-----------------------------------------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 95899 / NJ EPH Aliphatic<br>n-Hydrocarbons-Revised,<br>1000 PPM | 040524 | 08/03/2025      | 02/03/2025 /<br>yogesh  | 04/11/2024 /<br>yogesh      | P13279         |

| Supplier | ItemCode / ItemName                       | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31098 /<br>1-Chlorooctadecane<br>Standard | A0213283 | 10/25/2025      | 04/25/2025 /<br>Abdul   | 10/16/2024 /<br>yogesh      | P13596         |

| Supplier | ItemCode / ItemName             | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31097 / o-Terphenyl<br>Standard | A0216631 | 08/03/2025      | 02/03/2025 /<br>yogesh  | 10/16/2024 /<br>yogesh      | P13650         |

| Supplier | ItemCode / ItemName             | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31097 / o-Terphenyl<br>Standard | A0216631 | 10/25/2025      | 04/25/2025 /<br>Abdul   | 10/16/2024 /<br>yogesh      | P13660         |

| Supplier | ItemCode / ItemName             | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|---------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31097 / o-Terphenyl<br>Standard | A0216631 | 10/25/2025      | 04/25/2025 /<br>Abdul   | 10/16/2024 /<br>yogesh      | P13662         |

## CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName          | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31097 / o-Terphenyl Standard | A0216631 | 10/25/2025      | 04/25/2025 / Abdul      | 10/16/2024 / yogesh         | P13664         |

| Supplier | ItemCode / ItemName          | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31097 / o-Terphenyl Standard | A0216631 | 10/25/2025      | 04/25/2025 / Abdul      | 10/16/2024 / yogesh         | P13667         |

| Supplier | ItemCode / ItemName          | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31097 / o-Terphenyl Standard | A0216631 | 08/03/2025      | 02/03/2025 / yogesh     | 10/16/2024 / yogesh         | P13671         |

| Supplier | ItemCode / ItemName                             | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-------------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 30543 / Custom NJEPH Aromatics Matrix Spike Mix | A0211254 | 10/15/2025      | 04/15/2025 / yogesh     | 10/24/2024 / yogesh         | P13709         |

| Supplier | ItemCode / ItemName                          | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|----------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31480 / MA Fractionation Surrogate Spike Mix | A0214879 | 10/18/2025      | 04/18/2025 / Abdul      | 11/01/2024 / yogesh         | P13762         |

| Supplier | ItemCode / ItemName                          | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|----------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31480 / MA Fractionation Surrogate Spike Mix | A0214879 | 10/18/2025      | 04/18/2025 / Abdul      | 11/01/2024 / yogesh         | P13764         |

## CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName                             | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-------------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 30543 / Custom NJEPH Aromatics Matrix Spike Mix | A0220580 | 10/15/2025      | 04/15/2025 / yogesh     | 01/08/2025 / yogesh         | P13865         |

| Supplier | ItemCode / ItemName                              | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--------------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 30542 / Custom NJEPH Aliphatics Matrix Spike Mix | A0217408 | 10/15/2025      | 04/15/2025 / yogesh     | 03/06/2025 / yogesh         | P13896         |

| Supplier | ItemCode / ItemName                              | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--------------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 30542 / Custom NJEPH Aliphatics Matrix Spike Mix | A0217408 | 10/15/2025      | 04/15/2025 / yogesh     | 03/06/2025 / yogesh         | P13897         |

| Supplier | ItemCode / ItemName                              | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--------------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 30542 / Custom NJEPH Aliphatics Matrix Spike Mix | A0217408 | 10/15/2025      | 04/15/2025 / yogesh     | 03/06/2025 / yogesh         | P13898         |

| Supplier | ItemCode / ItemName                              | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--------------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 30542 / Custom NJEPH Aliphatics Matrix Spike Mix | A0217408 | 10/15/2025      | 04/15/2025 / yogesh     | 03/06/2025 / yogesh         | P13899         |

| Supplier | ItemCode / ItemName                              | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--------------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 30542 / Custom NJEPH Aliphatics Matrix Spike Mix | A0217408 | 10/15/2025      | 04/15/2025 / yogesh     | 03/06/2025 / yogesh         | P13900         |

## CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName                              | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--------------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 30542 / Custom NJEPH Aliphatics Matrix Spike Mix | A0217408 | 10/15/2025      | 04/15/2025 / yogesh     | 03/06/2025 / yogesh         | P13901         |

| Supplier | ItemCode / ItemName                              | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--------------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 30542 / Custom NJEPH Aliphatics Matrix Spike Mix | A0217408 | 10/15/2025      | 04/15/2025 / yogesh     | 03/06/2025 / yogesh         | P13903         |

| Supplier | ItemCode / ItemName                              | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--------------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 30542 / Custom NJEPH Aliphatics Matrix Spike Mix | A0217408 | 10/15/2025      | 04/15/2025 / yogesh     | 03/06/2025 / yogesh         | P13905         |

| Supplier | ItemCode / ItemName                              | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--------------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 30542 / Custom NJEPH Aliphatics Matrix Spike Mix | A0217408 | 10/15/2025      | 04/15/2025 / yogesh     | 03/06/2025 / yogesh         | P13906         |

| Supplier | ItemCode / ItemName                              | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--------------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 30542 / Custom NJEPH Aliphatics Matrix Spike Mix | A0220449 | 10/15/2025      | 04/15/2025 / yogesh     | 03/06/2025 / yogesh         | P13912         |

| Supplier | ItemCode / ItemName                             | Lot #   | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-------------------------------------------------|---------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 30543 / Custom NJEPH Aromatics Matrix Spike Mix | A022580 | 10/15/2025      | 04/15/2025 / yogesh     | 03/06/2025 / yogesh         | P13919         |

## CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName                             | Lot #   | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-------------------------------------------------|---------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 30543 / Custom NJEPH Aromatics Matrix Spike Mix | A022580 | 10/15/2025      | 04/15/2025 / yogesh     | 03/06/2025 / yogesh         | P13920         |

| Supplier | ItemCode / ItemName                             | Lot #   | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-------------------------------------------------|---------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 30543 / Custom NJEPH Aromatics Matrix Spike Mix | A022580 | 10/15/2025      | 04/15/2025 / yogesh     | 03/06/2025 / yogesh         | P13921         |

| Supplier | ItemCode / ItemName                             | Lot #   | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-------------------------------------------------|---------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 30543 / Custom NJEPH Aromatics Matrix Spike Mix | A022580 | 10/15/2025      | 04/15/2025 / yogesh     | 03/06/2025 / yogesh         | P13923         |

| Supplier | ItemCode / ItemName                             | Lot #   | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-------------------------------------------------|---------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 30543 / Custom NJEPH Aromatics Matrix Spike Mix | A022580 | 10/15/2025      | 04/15/2025 / yogesh     | 03/06/2025 / yogesh         | P13926         |

| Supplier | ItemCode / ItemName                             | Lot #   | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-------------------------------------------------|---------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 30543 / Custom NJEPH Aromatics Matrix Spike Mix | A022580 | 10/15/2025      | 04/15/2025 / yogesh     | 03/06/2025 / yogesh         | P13927         |

| Supplier | ItemCode / ItemName                             | Lot #   | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-------------------------------------------------|---------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 30543 / Custom NJEPH Aromatics Matrix Spike Mix | A022580 | 10/15/2025      | 04/15/2025 / yogesh     | 03/06/2025 / yogesh         | P13928         |

## CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName                             | Lot #   | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-------------------------------------------------|---------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 30543 / Custom NJEPH Aromatics Matrix Spike Mix | A022580 | 10/15/2025      | 04/15/2025 / yogesh     | 03/06/2025 / yogesh         | P13931         |

| Supplier | ItemCode / ItemName                          | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|----------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31480 / MA Fractionation Surrogate Spike Mix | A0219106 | 10/31/2030      | 04/18/2025 / Abdul      | 03/10/2025 / yogesh         | P13947         |

| Supplier | ItemCode / ItemName                          | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|----------------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek   | 31480 / MA Fractionation Surrogate Spike Mix | A0219106 | 10/18/2025      | 04/18/2025 / Abdul      | 03/10/2025 / yogesh         | P13948         |

| Supplier         | ItemCode / ItemName                       | Lot #      | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|-------------------------------------------|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L) | 24G1962003 | 08/22/2025      | 02/03/2025 / jignesh    | 01/31/2025 / jignesh        | W3177          |

Sand  
Purified  
Washed and Ignited



Material No.: 3382-05  
Batch No.: 0000243821  
Manufactured Date: 2018/04/09  
Retest Date: 2025/04/07  
Revision No: 1

## Certificate of Analysis

| Test                      | Specification | Result |
|---------------------------|---------------|--------|
| Substances Soluble in HCl | $\leq 0.16\%$ | 0.01   |

For Laboratory, Research or Manufacturing Use  
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US  
Packaging Site: Paris Mfg Ctr & DC

E 2865

  
Jamie Ethier  
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC  
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700





**PRODUCTOS  
QUÍMICOS  
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR  
MONTERREY, N.L. MEXICO  
CP 64070  
TEL +52 81 13 52 57 57  
www.pqm.com.mx

## CERTIFICATE OF ANALYSIS

|                        |                                   |               |                                 |
|------------------------|-----------------------------------|---------------|---------------------------------|
| PRODUCT :              | SODIUM SULFATE CRYSTALS ANHYDROUS |               |                                 |
| QUALITY :              | ACS (CODE RMB3375)                | FORMULA :     | Na <sub>2</sub> SO <sub>4</sub> |
| SPECIFICATION NUMBER : | 6399                              | RELEASE DATE: | ABR/21/2023                     |
| LOT NUMBER :           | 313201                            |               |                                 |

| TEST                                     | SPECIFICATIONS | LOT VALUES  |
|------------------------------------------|----------------|-------------|
| Assay (Na <sub>2</sub> SO <sub>4</sub> ) | Min. 99.0%     | 99.7 %      |
| pH of a 5% solution at 25°C              | 5.2 - 9.2      | 6.1         |
| Insoluble matter                         | Max. 0.01%     | 0.005 %     |
| Loss on ignition                         | Max. 0.5%      | 0.1 %       |
| Chloride (Cl)                            | Max. 0.001%    | <0.001 %    |
| Nitrogen compounds (as N)                | Max. 5 ppm     | <5 ppm      |
| Phosphate (PO <sub>4</sub> )             | Max. 0.001%    | <0.001 %    |
| Heavy metals (as Pb)                     | Max. 5 ppm     | <5 ppm      |
| Iron (Fe)                                | Max. 0.001%    | <0.001 %    |
| Calcium (Ca)                             | Max. 0.01%     | 0.002 %     |
| Magnesium (Mg)                           | Max. 0.005%    | 0.001 %     |
| Potassium (K)                            | Max. 0.008%    | 0.003 %     |
| Extraction-concentration suitability     | Passes test    | Passes test |
| Appearance                               | Passes test    | Passes test |
| Identification                           | Passes test    | Passes test |
| Solubility and foreign matter            | Passes test    | Passes test |
| Retained on US Standard No. 10 sieve     | Max. 1%        | 0.1 %       |
| Retained on US Standard No. 60 sieve     | Min. 94%       | 97.3 %      |
| Through US Standard No. 60 sieve         | Max. 5%        | 2.5 %       |
| Through US Standard No. 100 sieve        | Max. 10%       | 0.1 %       |

### COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/24/23 E 3551

RC-02-01, Ed. 3

## Certificate of Analysis

1 Reagent Lane  
 Fair Lawn, NJ 07410  
 201.796.7100 tel  
 201.796.1329 fax

Thermo Fisher Scientific's Quality System has been found to conform to Quality Management System  
 Standard ISO9001:2015 by SAI Global Certificate Number CERT - 0120633

This is to certify that units of the lot number below were tested and found to comply with the specifications of the grade listed. Certain data have been supplied by third parties. Thermo Fisher Scientific expressly disclaims all warranties, expressed or implied, including the implied warranties of merchantability and fitness for a particular purpose. Products are for research use or further manufacturing. Not for direct administration to humans or animals. It is the responsibility of the final formulator and end user to determine suitability based upon the intended use of the end product. Products are tested to meet the analytical requirements of the noted grade. The following information is the actual analytical results obtained.

|                   |                                                                                                                                                                                                   |                             |            |
|-------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-----------------------------|------------|
| Catalog Number    | H303                                                                                                                                                                                              | Quality Test / Release Date | 11/07/2024 |
| Lot Number        | 243570                                                                                                                                                                                            |                             |            |
| Description       | HEXANES - OPTIMA                                                                                                                                                                                  |                             |            |
| Country of Origin | United States                                                                                                                                                                                     | Suggested Retest Date       | Nov/2029   |
| Chemical Origin   | Organic - non animal                                                                                                                                                                              |                             |            |
| BSE/TSE Comment   | No animal products are used as starting raw material ingredients, or used in processing, including lubricants, processing aids, or any other material that might migrate to the finished product. |                             |            |

N/A

| Result Name                 | Units      | Specifications                  | Test Value              |
|-----------------------------|------------|---------------------------------|-------------------------|
| APPEARANCE                  |            | REPORT                          | Clear, colorless liquid |
| ASSAY (N-HEXANE)            | %          | >= 60                           | 69                      |
| ASSAY (SUM C6 HYDROCARBONS) | %          | >= 99.9                         | >99.9                   |
| COLOR                       | APHA       | <= 5                            | <5                      |
| DENSITY AT 25 DEGREES C     | GM/ML      | Inclusive Between 0.653 - 0.673 | 0.669                   |
| EVAPORATION RESIDUE         | ppm        | <= 1                            | <1                      |
| FLUORESCENCE BACKGROUND     | ppb        | <= 1                            | <1                      |
| IDENTIFICATION              | PASS/FAIL  | = PASS TEST                     | PASS TEST               |
| OPTICAL ABS AT 195 NM       | ABS. UNITS | <= 1                            | 0.74                    |
| OPTICAL ABS AT 210 NM       | ABS. UNITS | <= 0.25                         | 0.17                    |
| OPTICAL ABS AT 220 NM       | ABS. UNITS | <= 0.07                         | 0.05                    |
| OPTICAL ABS AT 254 NM       | ABS. UNITS | <= 0.005                        | 0.001                   |
| PESTICIDE RESIDUE ANALYSIS  | NG/L       | <= 10                           | <10                     |
| REFRACTIVE INDEX @ 25 DEG C |            | Inclusive Between 1.375 - 1.385 | 1.379                   |
| SUITABILITY FOR GC/MS       |            | = PASS TEST                     | PASS TEST               |
| SULFUR COMPOUNDS            | %          | <= 0.005                        | <0.005                  |
| THIOPHENE                   | PASS/FAIL  | = PASS TEST                     | PASS TEST               |
| WATER (H2O)                 | %          | <= 0.01                         | <0.01                   |
| WATER-SOLUBLE TITRABLE ACID | MEQ/G      | <= 0.0003                       | 0.0001                  |

*Harout Sahagian*

Harout Sahagian - Quality Control Manager - Fair Lawn

Recd by RP on 3/31/25

E 3946

Note: The data listed is valid for all package sizes of this lot of this product, expressed as an extension of this catalog number listed above.  
 If there are any questions with this certificate, please call at (800) 227-6701.  
 \*Based on suggested storage condition.

Acetone

BAKER RESI-ANALYZED® Reagent  
For Organic Residue Analysis

Avantor™



Material No.: 9254-03

Batch No.: 24H2762008

Manufactured Date: 2024-04-18

Expiration Date: 2027-04-18

Revision No.: 0

## Certificate of Analysis

| Test                                                                    | Specification | Result      |
|-------------------------------------------------------------------------|---------------|-------------|
| Assay ((CH <sub>3</sub> ) <sub>2</sub> CO) (by GC, corrected for water) | >= 99.4 %     | 100.0 %     |
| Color (APHA)                                                            | <= 10         | 5           |
| Residue after Evaporation                                               | <= 1.0 ppm    | 0.0 ppm     |
| Substances Reducing Permanganate                                        | Passes Test   | Passes Test |
| Titration Acid (μeq/g)                                                  | <= 0.3        | 0.2         |
| Titration Base (μeq/g)                                                  | <= 0.6        | <0.1        |
| Water (H <sub>2</sub> O)                                                | <= 0.5 %      | <0.1 %      |
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)    | <= 5          | 1           |
| ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)    | <= 10         | 1           |

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

Recd by RP on 03/31/25

E3917

Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

n-Hexane 95%  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis

 **avantors<sup>TM</sup>**



Material No.: 9262-03

Batch No.: 25C0362005

Manufactured Date: 2025-01-29

Expiration Date: 2026-04-30

Revision No.: 0

## Certificate of Analysis

| Test                                                                           | Specification  | Result      |
|--------------------------------------------------------------------------------|----------------|-------------|
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)           | $\leq 5$       | 1           |
| ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)            | $\leq 10$      | 6           |
| ECD-Sensitive Impurities (as EthyleneDibromide) - Single Impurity Peak (ng/mL) | $\leq 5$       | 5           |
| Assay (Total Saturated C <sub>6</sub> Isomers) (by GC, corrected for water)    | $\geq 99.5 \%$ | 100.0 %     |
| Assay (as n-Hexane) (by GC, corrected for water)                               | $\geq 95 \%$   | 100 %       |
| Color (APHA)                                                                   | $\leq 10$      | 10          |
| Residue after Evaporation                                                      | $\leq 1.0$ ppm | 0.1 ppm     |
| Substances Darkened by H <sub>2</sub> SO <sub>4</sub>                          | Passes Test    | Passes Test |
| Water (by KF, coulometric)                                                     | $\leq 0.05 \%$ | $< 0.01 \%$ |

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States  
Packaging Site: Phillipsburg Mfg Ctr & DC

E3928



Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials U.S.

Acetone

BAKER RESI-ANALYZED® Reagent

For Organic Residue Analysis

avantor™



Material No.: 9254-03

Batch No.: 24H2762008

Manufactured Date: 2024-04-18

Expiration Date: 2027-04-18

Revision No.: 0

## Certificate of Analysis

| Test                                                                    | Specification | Result      |
|-------------------------------------------------------------------------|---------------|-------------|
| Assay ((CH <sub>3</sub> ) <sub>2</sub> CO) (by GC, corrected for water) | >= 99.4 %     | 100.0 %     |
| Color (APHA)                                                            | <= 10         | 5           |
| Residue after Evaporation                                               | <= 1.0 ppm    | 0.0 ppm     |
| Substances Reducing Permanganate                                        | Passes Test   | Passes Test |
| Titration Acid (µeq/g)                                                  | <= 0.3        | 0.2         |
| Titration Base (µeq/g)                                                  | <= 0.6        | <0.1        |
| Water (H <sub>2</sub> O)                                                | <= 0.5 %      | <0.1 %      |
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)    | <= 5          | 1           |
| ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)    | <= 10         | 1           |

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

E 3929

Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

# CERTIFIED REFERENCE MATERIAL

## Certificate of Analysis



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30540 **Lot No.:** A0190424

**Description :** NJEPH Aliphatics Calibration Standard

Aliphatics Calibration Standard 2000µg/mL, Hexane/Carbon Disulfide (80:20), 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** November 30, 2029 **Storage:** 25°C nominal

**Handling:** Sonicate prior to use. **Ship:** Ambient

P12361  
↓  
P12370 } Y.P.  
031/6/23

### CERTIFIED VALUES

| Elution Order | Compound                                                              | Grav. Conc. (weight/volume) | Expanded Uncertainty (95% C.L.; K=2)      |                                                |
|---------------|-----------------------------------------------------------------------|-----------------------------|-------------------------------------------|------------------------------------------------|
| 1             | n-Nonane (C9)<br>CAS # 111-84-2<br>Purity 99%<br>(Lot SHBN5361)       | 2,014.0 µg/mL               | +/- 11.8193<br>+/- 50.0027<br>+/- 59.9491 | µg/mL<br>Gravimetric<br>Unstressed<br>Stressed |
| 2             | n-Decane (C10)<br>CAS # 124-18-5<br>Purity 99%<br>(Lot SHBN8619)      | 2,014.7 µg/mL               | +/- 11.8232<br>+/- 50.0193<br>+/- 59.9689 | µg/mL<br>Gravimetric<br>Unstressed<br>Stressed |
| 3             | Naphthalene<br>CAS # 91-20-3<br>Purity 99%<br>(Lot MKCH0219)          | 2,015.3 µg/mL               | +/- 11.8271<br>+/- 50.0358<br>+/- 59.9888 | µg/mL<br>Gravimetric<br>Unstressed<br>Stressed |
| 4             | n-Dodecane (C12)<br>CAS # 112-40-3<br>Purity 99%<br>(Lot SHBN7174)    | 2,008.0 µg/mL               | +/- 11.7841<br>+/- 49.8538<br>+/- 59.7705 | µg/mL<br>Gravimetric<br>Unstressed<br>Stressed |
| 5             | 2-Methylnaphthalene<br>CAS # 91-57-6<br>Purity 96%<br>(Lot STBK0259)  | 2,007.0 µg/mL               | +/- 11.7784<br>+/- 49.8299<br>+/- 59.7419 | µg/mL<br>Gravimetric<br>Unstressed<br>Stressed |
| 6             | n-Tetradecane (C14)<br>CAS # 629-59-4<br>Purity 99%<br>(Lot STBK2282) | 2,016.7 µg/mL               | +/- 11.8349<br>+/- 50.0689<br>+/- 60.0284 | µg/mL<br>Gravimetric<br>Unstressed<br>Stressed |
| 7             | n-Hexadecane (C16)<br>CAS # 544-76-3<br>Purity 98%<br>(Lot SHBM4146)  | 2,014.9 µg/mL               | +/- 11.8244<br>+/- 50.0246<br>+/- 59.9753 | µg/mL<br>Gravimetric<br>Unstressed<br>Stressed |

|                                                 |                                                            |                  |               |     |         |       |             |
|-------------------------------------------------|------------------------------------------------------------|------------------|---------------|-----|---------|-------|-------------|
| 8                                               | n-Octadecane (C18)<br>CAS # 593-45-3<br>Purity 97%         | (Lot VZKOJ)      | 2,004.7 µg/mL | +/- | 11.7645 | µg/mL | Gravimetric |
|                                                 |                                                            |                  |               | +/- | 49.7710 | µg/mL | Unstressed  |
|                                                 |                                                            |                  |               | +/- | 59.6712 | µg/mL | Stressed    |
| 9                                               | n-Eicosane (C20)<br>CAS # 112-95-8<br>Purity 99%           | (Lot MKCF7888)   | 2,018.0 µg/mL | +/- | 11.8428 | µg/mL | Gravimetric |
|                                                 |                                                            |                  |               | +/- | 50.1020 | µg/mL | Unstressed  |
|                                                 |                                                            |                  |               | +/- | 60.0681 | µg/mL | Stressed    |
| 10                                              | n-Heneicosane (C21)<br>CAS # 629-94-7<br>Purity 99%        | (Lot MKCL3226)   | 2,000.7 µg/mL | +/- | 11.7410 | µg/mL | Gravimetric |
|                                                 |                                                            |                  |               | +/- | 49.6717 | µg/mL | Unstressed  |
|                                                 |                                                            |                  |               | +/- | 59.5522 | µg/mL | Stressed    |
| 11                                              | n-Docosane (C22)<br>CAS # 629-97-0<br>Purity 99%           | (Lot MKCL8918)   | 2,005.3 µg/mL | +/- | 11.7684 | µg/mL | Gravimetric |
|                                                 |                                                            |                  |               | +/- | 49.7876 | µg/mL | Unstressed  |
|                                                 |                                                            |                  |               | +/- | 59.6911 | µg/mL | Stressed    |
| 12                                              | n-Tetracosane (C24)<br>CAS # 646-31-1<br>Purity 99%        | (Lot MKCN2863)   | 2,018.0 µg/mL | +/- | 11.8428 | µg/mL | Gravimetric |
|                                                 |                                                            |                  |               | +/- | 50.1020 | µg/mL | Unstressed  |
|                                                 |                                                            |                  |               | +/- | 60.0681 | µg/mL | Stressed    |
| 13                                              | n-Hexacosane (C26)<br>CAS # 630-01-3<br>Purity 99%         | (Lot MKCD4540)   | 2,014.0 µg/mL | +/- | 11.8193 | µg/mL | Gravimetric |
|                                                 |                                                            |                  |               | +/- | 50.0027 | µg/mL | Unstressed  |
|                                                 |                                                            |                  |               | +/- | 59.9491 | µg/mL | Stressed    |
| 14                                              | n-Octacosane (C28)<br>CAS # 630-02-4<br>Purity 99%         | (Lot BCCG0084)   | 2,002.0 µg/mL | +/- | 11.7489 | µg/mL | Gravimetric |
|                                                 |                                                            |                  |               | +/- | 49.7048 | µg/mL | Unstressed  |
|                                                 |                                                            |                  |               | +/- | 59.5919 | µg/mL | Stressed    |
| 15                                              | n-Triacontane (C30)<br>CAS # 638-68-6<br>Purity 97%        | (Lot MKCQ9436)   | 2,011.1 µg/mL | +/- | 11.8025 | µg/mL | Gravimetric |
|                                                 |                                                            |                  |               | +/- | 49.9316 | µg/mL | Unstressed  |
|                                                 |                                                            |                  |               | +/- | 59.8637 | µg/mL | Stressed    |
| 16                                              | n-Dotriacontane (C32)<br>CAS # 544-85-4<br>Purity 99%      | (Lot BCBW0661)   | 2,012.0 µg/mL | +/- | 11.8075 | µg/mL | Gravimetric |
|                                                 |                                                            |                  |               | +/- | 49.9531 | µg/mL | Unstressed  |
|                                                 |                                                            |                  |               | +/- | 59.8895 | µg/mL | Stressed    |
| 17                                              | n-Tetratriacontane (C34)<br>CAS # 14167-59-0<br>Purity 99% | (Lot OML4N)      | 2,006.7 µg/mL | +/- | 11.7762 | µg/mL | Gravimetric |
|                                                 |                                                            |                  |               | +/- | 49.8207 | µg/mL | Unstressed  |
|                                                 |                                                            |                  |               | +/- | 59.7308 | µg/mL | Stressed    |
| 18                                              | n-Hexatriacontane (C36)<br>CAS # 630-06-8<br>Purity 99%    | (Lot Z27H018)    | 2,017.3 µg/mL | +/- | 11.8388 | µg/mL | Gravimetric |
|                                                 |                                                            |                  |               | +/- | 50.0855 | µg/mL | Unstressed  |
|                                                 |                                                            |                  |               | +/- | 60.0483 | µg/mL | Stressed    |
| 19                                              | n-Octatriacontane (C38)<br>CAS # 7194-85-6<br>Purity 96%   | (Lot 0000145137) | 2,017.3 µg/mL | +/- | 11.8385 | µg/mL | Gravimetric |
|                                                 |                                                            |                  |               | +/- | 50.0842 | µg/mL | Unstressed  |
|                                                 |                                                            |                  |               | +/- | 60.0467 | µg/mL | Stressed    |
| 20                                              | n-Tetracontane (C40)<br>CAS # 4181-95-7<br>Purity 99%      | (Lot BSBME)      | 2,008.7 µg/mL | +/- | 11.7880 | µg/mL | Gravimetric |
|                                                 |                                                            |                  |               | +/- | 49.8703 | µg/mL | Unstressed  |
|                                                 |                                                            |                  |               | +/- | 59.7903 | µg/mL | Stressed    |
| <b>Solvent:</b> Hexane/Carbon disulfide (80:20) |                                                            |                  |               |     |         |       |             |
|                                                 | CAS # 110-54-3/75-15-0                                     |                  |               |     |         |       |             |
|                                                 | Purity 99%                                                 |                  |               |     |         |       |             |

**Column:**  
30m x 0.25mm x 0.25µm  
Pxx-5 (cat.#10223)


**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

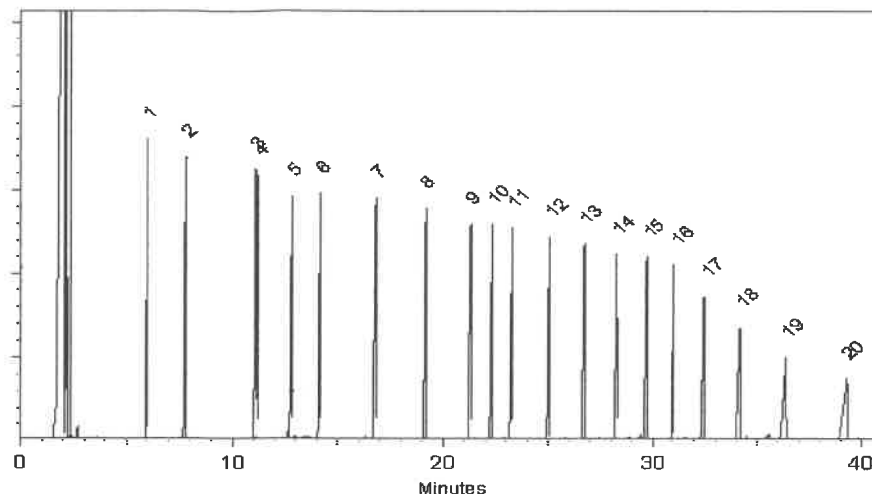

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Morgan Craighead - Mix Technician

Date Mixed: 10-Oct-2022

Balance: 1128360905

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 20-Oct-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

| Label Conditions                                          | Standard Conditions | Non-Standard Conditions |
|-----------------------------------------------------------|---------------------|-------------------------|
| 25°C Nominal (Room Temperature)                           | < 60°C              | ≥ 60°C up to 7 days     |
| 10°C or colder (Refrigerate)                              | < 40°C              | ≥ 40°C up to 7 days     |
| 0°C or colder (Freezer)<br>-20°C or colder (Deep Freezer) | < 25°C              | ≥ 25°C up to 7 days     |

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No.:** 31098 **Lot No.:** A0204989  
**Description:** 1-Chlorooctadecane Standard  
1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul  
**Container Size:** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date:** January 31, 2031 **Storage:** 10°C or colder  
**Ship:** Ambient

P12960  
↓  
P12991 } Y.P.  
12/21/2023

### CERTIFIED VALUES

| Elution Order | Compound           | CAS #     | Lot #    | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------|-----------|----------|--------|-----------------------------|----------------------------------------|
| 1             | 1-Chlorooctadecane | 3386-33-2 | 14738400 | 99%    | 10,097.3 µg/mL              | +/- 567.2675                           |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

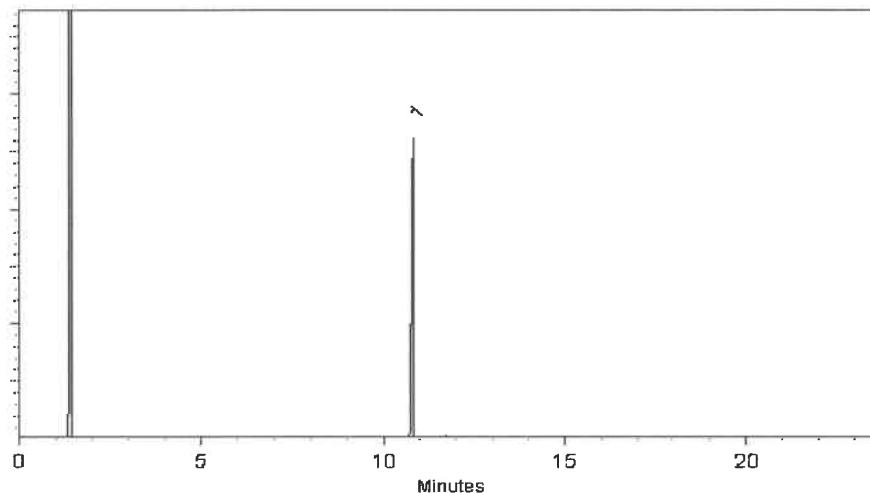

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Peter Robbins - Operations Technician I

Date Mixed: 02-Dec-2023

Balance Serial # B345965662

Christie Mills - Operations Lead Tech - ARM QC

Date Passed: 08-Dec-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No.:** 31098 **Lot No.:** A0204989  
**Description:** 1-Chlorooctadecane Standard  
1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul  
**Container Size:** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date:** January 31, 2031 **Storage:** 10°C or colder  
**Ship:** Ambient

P12960  
↓  
P12991 } Y.P.  
12/21/2023

### CERTIFIED VALUES

| Elution Order | Compound           | CAS #     | Lot #    | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------|-----------|----------|--------|-----------------------------|----------------------------------------|
| 1             | 1-Chlorooctadecane | 3386-33-2 | 14738400 | 99%    | 10,097.3 µg/mL              | +/- 567.2675                           |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

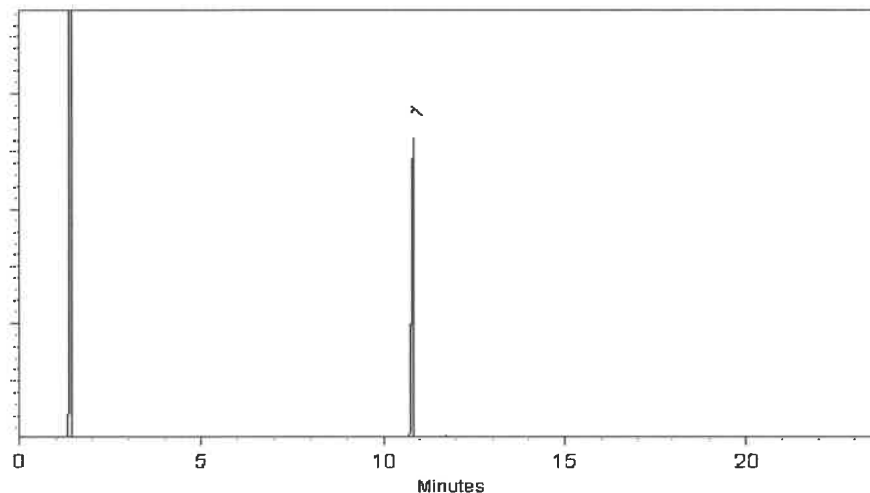

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Peter Robbins - Operations Technician I

Date Mixed: 02-Dec-2023

Balance Serial # B345965662

Christie Mills - Operations Lead Tech - ARM QC

Date Passed: 08-Dec-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No.:** 31098 **Lot No.:** A0204989  
**Description:** 1-Chlorooctadecane Standard  
1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul  
**Container Size:** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date:** January 31, 2031 **Storage:** 10°C or colder  
**Ship:** Ambient

P12960  
↓  
P12991 } Y.P.  
12/21/2023

### CERTIFIED VALUES

| Elution Order | Compound           | CAS #     | Lot #    | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------|-----------|----------|--------|-----------------------------|----------------------------------------|
| 1             | 1-Chlorooctadecane | 3386-33-2 | 14738400 | 99%    | 10,097.3 µg/mL              | +/- 567.2675                           |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

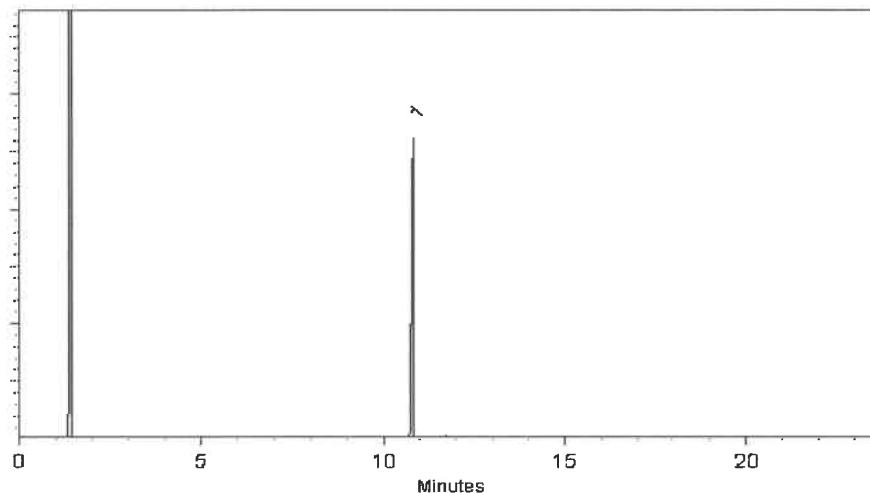

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Peter Robbins - Operations Technician I

Date Mixed: 02-Dec-2023

Balance Serial # B345965662

Christie Mills - Operations Lead Tech - ARM QC

Date Passed: 08-Dec-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No.:** 31098 **Lot No.:** A0204989

**Description:** 1-Chlorooctadecane Standard

1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size:** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date:** January 31, 2031 **Storage:** 10°C or colder

**Ship:** Ambient

P12960  
↓  
P12991 } Y.P.  
12/21/2023

### CERTIFIED VALUES

| Elution Order | Compound           | CAS #     | Lot #    | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------|-----------|----------|--------|-----------------------------|----------------------------------------|
| 1             | 1-Chlorooctadecane | 3386-33-2 | 14738400 | 99%    | 10,097.3 µg/mL              | +/- 567.2675                           |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

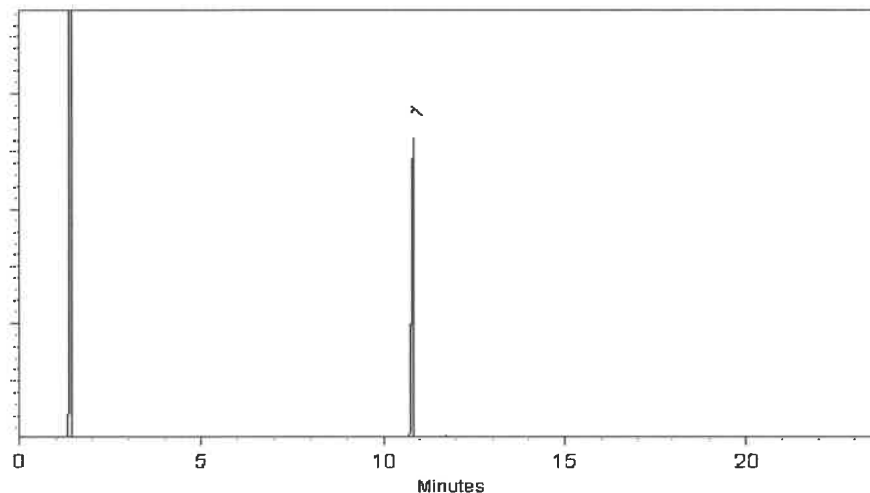

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Peter Robbins - Operations Technician I

Date Mixed: 02-Dec-2023

Balance Serial # B345965662

Christie Mills - Operations Lead Tech - ARM QC

Date Passed: 08-Dec-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31098 **Lot No.:** A0200707

**Description :** 1-Chlorooctadecane Standard

1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** September 30, 2030 **Storage:** 10°C or colder

**Ship:** Ambient

P130hh  
2  
P13051 } Y.B.  
12/26/23

### CERTIFIED VALUES

| Elution Order | Compound           | CAS #     | Lot #       | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------|-----------|-------------|--------|-----------------------------|----------------------------------------|
| 1             | 1-Chlorooctadecane | 3386-33-2 | E230426RSRB | 99%    | 10,018.0 µg/mL              | +/- 562.8106                           |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

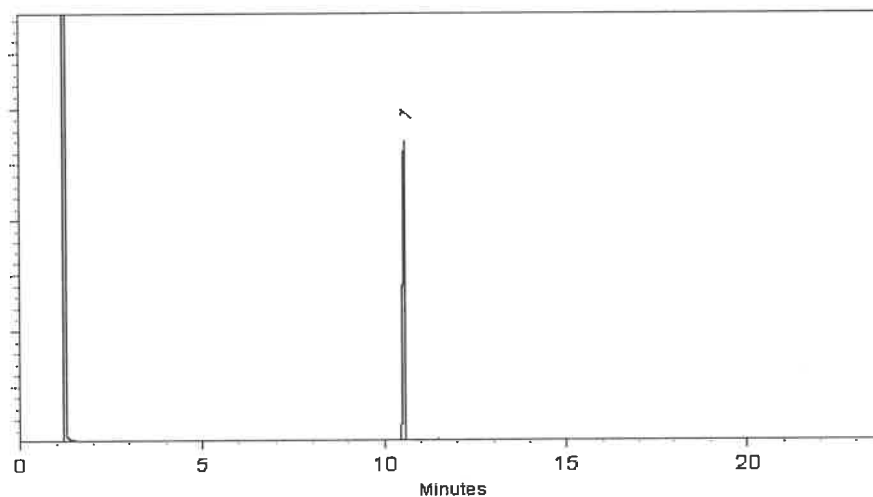

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Ashley Frantz - Quoting Technician

Date Mixed: 07-Aug-2023

Balance Serial # 1128360905

  
Dillan Murphy - Operations Technician I

Date Passed: 10-Aug-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



CERTIFIED WEIGHT REPORT

Part Number: 95999

Lot Number: 040524

Description: NJ EPH Aliphatic n-Hydrocarbons - Revised  
20 components

Expiration Date: 040534

Recommended Storage: Ambient (20 °C)

Nominal Concentration (µg/mL): 1000

NIST Test ID#: 6UTB

Weight(s) shown below were combined and diluted to (mL):

CAUTION: Sonicate Before Use

Solvent(s):  
Cyclohexane

Lot#  
28930

P13278  
2  
P13287  
Y.P.  
04/11/24

5E-05 Balance Uncertainty  
0.001 Flask Uncertainty

|                |                 |        |      |
|----------------|-----------------|--------|------|
| Formulated By: | Anthony Mahoney | 040524 | DATE |
| Reviewed By:   | Pedro L. Rentas | 040524 | DATE |

| Compound |                     | Part Number | (RM#)     | Lot Number | DIL Factor | Initial Vol. (mL) | Initial Conc (µg/mL) | Nominal Conc (µg/mL) | Purity (%) | Purity Uncertainty | Pipette | Target Weight(g) | Actual Weight(g) | Actual Conc (µg/mL) | Expanded Uncertainty (+/-) (µg/mL) | SDS Information<br>(Solvent Safety Info. On Attached pg.) |                                     |                   |
|----------|---------------------|-------------|-----------|------------|------------|-------------------|----------------------|----------------------|------------|--------------------|---------|------------------|------------------|---------------------|------------------------------------|-----------------------------------------------------------|-------------------------------------|-------------------|
|          |                     |             |           |            |            |                   |                      |                      |            |                    |         |                  |                  |                     |                                    | CAS#                                                      | OSHA PEL (TWA)                      | LD50              |
| 1.       | 2-Methylnaphthalene | (0214)      | MKBF3783V | NA         | NA         | NA                | NA                   | 1000                 | 97         | 0.2                | NA      | 0.02579          | 0.02594          | 1005.7              | 5.7                                | 91-57-6                                                   | N/A                                 | or-rat 1630mg/kg  |
| 2.       | Naphthalene         | (0222)      | MKB28680V | NA         | NA         | NA                | NA                   | 1000                 | 100        | 0.2                | NA      | 0.02502          | 0.02511          | 1003.7              | 5.7                                | 91-20-3                                                   | 10 ppm (50mg/m <sup>3</sup> /8H)    | or-rat 490mg/kg   |
| 3.       | n-Nonane            | 95708       | 120222    | 1.00       | 25.00      | 1000.7            | 1000.7               | 1000                 | NA         | 0.013              | NA      | 0.013            | NA               | 1000.0              | 4.2                                | 111-84-2                                                  | 200 ppm (1050mg/m <sup>3</sup> /8H) | ivn-mus 218mg/kg  |
| 4.       | n-Decane            | 95708       | 120222    | 1.00       | 25.00      | 1000.9            | 1000.9               | 1000                 | NA         | 0.013              | NA      | 0.013            | NA               | 1000.2              | 4.2                                | 124-18-5                                                  | N/A                                 | N/A               |
| 5.       | n-Dodecane          | 95708       | 120222    | 1.00       | 25.00      | 1000.7            | 1000.7               | 1000                 | NA         | 0.013              | NA      | 0.013            | NA               | 1000.0              | 4.2                                | 112-40-3                                                  | N/A                                 | ivn-mus 3494mg/kg |
| 6.       | n-Tetradecane       | 95708       | 120222    | 1.00       | 25.00      | 1002.1            | 1002.1               | 1000                 | NA         | 0.013              | NA      | 0.013            | NA               | 1001.3              | 4.2                                | 629-59-4                                                  | N/A                                 | N/A               |
| 7.       | n-Hexadecane        | 95708       | 120222    | 1.00       | 25.00      | 1000.5            | 1000.5               | 1000                 | NA         | 0.013              | NA      | 0.013            | NA               | 999.7               | 4.2                                | 544-76-3                                                  | N/A                                 | N/A               |
| 8.       | n-Octadecane        | 95708       | 120222    | 1.00       | 25.00      | 1001.0            | 1001.0               | 1000                 | NA         | 0.013              | NA      | 0.013            | NA               | 1000.3              | 4.1                                | 583-45-3                                                  | N/A                                 | N/A               |
| 9.       | n-Eicosane          | 95708       | 120222    | 1.00       | 25.00      | 1001.0            | 1001.0               | 1000                 | NA         | 0.013              | NA      | 0.013            | NA               | 1000.3              | 4.2                                | 112-95-8                                                  | N/A                                 | N/A               |
| 10.      | n-Henicosane        | 95708       | 120222    | 1.00       | 25.00      | 1002.4            | 1002.4               | 1000                 | NA         | 0.013              | NA      | 0.013            | NA               | 1001.6              | 4.2                                | 629-94-7                                                  | N/A                                 | N/A               |
| 11.      | n-Docosane          | 95708       | 120222    | 1.00       | 25.00      | 1001.9            | 1001.9               | 1000                 | NA         | 0.013              | NA      | 0.013            | NA               | 1001.2              | 4.2                                | 629-97-0                                                  | N/A                                 | N/A               |
| 12.      | n-Tetracosane       | 95708       | 120222    | 1.00       | 25.00      | 1000.8            | 1000.8               | 1000                 | NA         | 0.013              | NA      | 0.013            | NA               | 1000.1              | 4.2                                | 646-31-1                                                  | N/A                                 | N/A               |
| 13.      | n-Hexacosane        | 95708       | 120222    | 1.00       | 25.00      | 1001.2            | 1001.2               | 1000                 | NA         | 0.013              | NA      | 0.013            | NA               | 1000.4              | 4.2                                | 630-01-3                                                  | N/A                                 | N/A               |
| 14.      | n-Octacosane        | 95708       | 120222    | 1.00       | 25.00      | 1000.5            | 1000.5               | 1000                 | NA         | 0.013              | NA      | 0.013            | NA               | 999.8               | 4.2                                | 630-02-4                                                  | N/A                                 | N/A               |
| 15.      | n-Triacontane       | 95708       | 120222    | 1.00       | 25.00      | 1000.5            | 1000.5               | 1000                 | NA         | 0.013              | NA      | 0.013            | NA               | 999.8               | 4.2                                | 638-68-6                                                  | N/A                                 | N/A               |
| 16.      | n-Dotriacontane     | 95708       | 120222    | 1.00       | 25.00      | 1000.5            | 1000.5               | 1000                 | NA         | 0.013              | NA      | 0.013            | NA               | 999.8               | 4.3                                | 544-85-4                                                  | N/A                                 | ivn-mus 100mg/kg  |
| 17.      | n-Tetracontane      | 95708       | 120222    | 1.00       | 25.00      | 1000.4            | 1000.4               | 1000                 | NA         | 0.013              | NA      | 0.013            | NA               | 999.7               | 4.2                                | 14167-59-0                                                | N/A                                 | N/A               |
| 18.      | n-Hexatriacontane   | 95708       | 120222    | 1.00       | 25.00      | 1001.5            | 1001.5               | 1000                 | NA         | 0.013              | NA      | 0.013            | NA               | 1000.8              | 4.2                                | 630-08-8                                                  | N/A                                 | N/A               |
| 19.      | n-Octatriacontane   | 95708       | 120222    | 1.00       | 25.00      | 1000.3            | 1000.3               | 1000                 | NA         | 0.013              | NA      | 0.013            | NA               | 999.6               | 4.3                                | 7184-86-6                                                 | N/A                                 | N/A               |
| 20.      | n-Tetracontane      | 95708       | 120222    | 1.00       | 25.00      | 1000.6            | 1000.6               | 1000                 | NA         | 0.013              | NA      | 0.013            | NA               | 999.9               | 4.3                                | 4181-95-7                                                 | N/A                                 | N/A               |

\* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.  
\* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).  
\* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.  
\* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.  
\* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31098 **Lot No.:** A0213283

**Description :** 1-Chlorooctadecane Standard

1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** July 31, 2031 **Storage:** 10°C or colder

**Ship:** Ambient

P13595  
↓  
P13624 } Y.P.  
10/16/24

### CERTIFIED VALUES

| Elution Order | Compound           | CAS #     | Lot #    | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------|-----------|----------|--------|-----------------------------|----------------------------------------|
| 1             | 1-Chlorooctadecane | 3386-33-2 | 15018900 | 99%    | 10,058.0 µg/mL              | +/- 565.0578                           |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-S (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

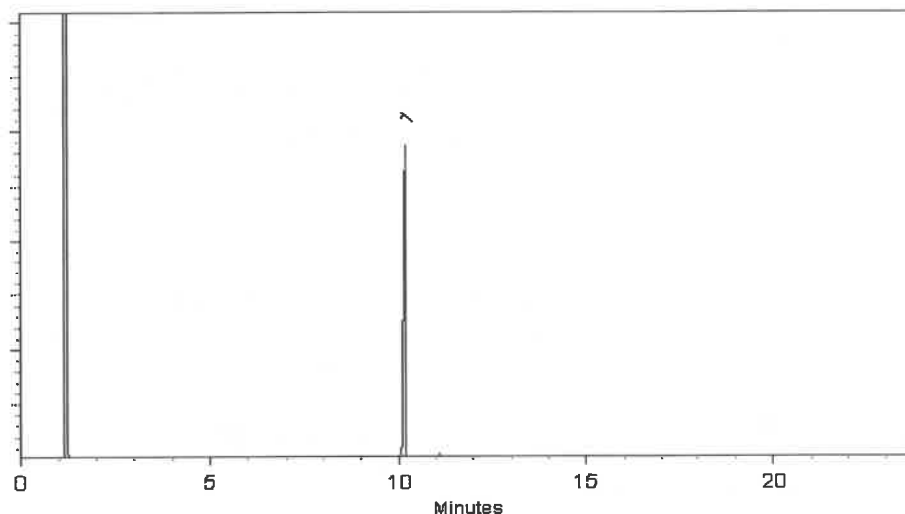

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Stacey Wanner - Operations Technician I

Date Mixed: 28-Jun-2024

Balance Serial # B345965662

Dillan Murphy - Operations Technician I

Date Passed: 01-Jul-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31097 **Lot No.:** A0216631  
**Description :** o-Terphenyl Standard  
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** April 30, 2028 **Storage:** 10°C or colder  
**Handling:** Sonicate prior to use. **Ship:** Ambient

P13645 } Y.P.  
↓  
P13694 } 10/16/24

### CERTIFIED VALUES

| Elution Order | Compound    | CAS #   | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|-------------|---------|-------|--------|-----------------------------|----------------------------------------|
| 1             | o-Terphenyl | 84-15-1 | GKSSA | 99%    | 10,065.0 µg/mL              | +/- 453.3336                           |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

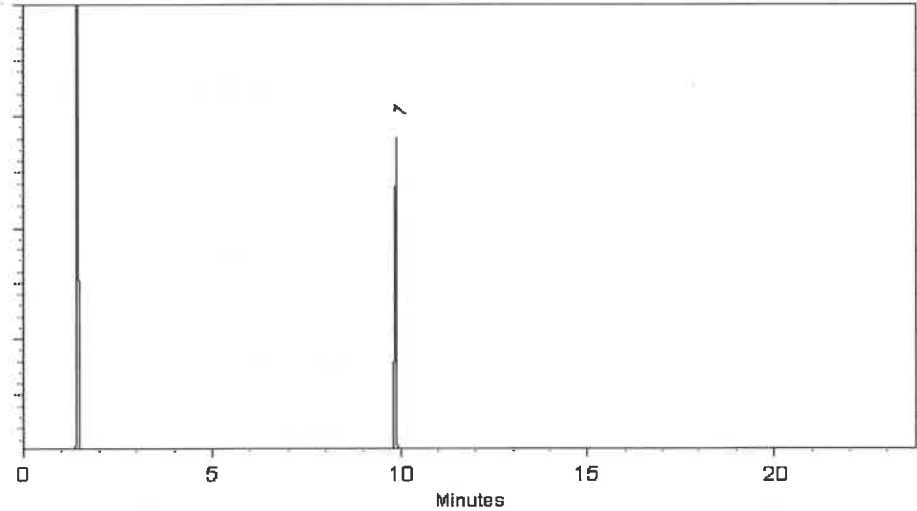

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ven Kelley - Operations Tech I

Date Mixed: 17-Sep-2024

Balance Serial # 1128353505

Dillan Murphy - Operations Technician I

Date Passed: 23-Sep-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31097 **Lot No.:** A0216631  
**Description :** o-Terphenyl Standard  
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** April 30, 2028 **Storage:** 10°C or colder  
**Handling:** Sonicate prior to use. **Ship:** Ambient

P13645 } Y.P.  
↓  
P13694 } 10/16/24

### CERTIFIED VALUES

| Elution Order | Compound    | CAS #   | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|-------------|---------|-------|--------|-----------------------------|----------------------------------------|
| 1             | o-Terphenyl | 84-15-1 | GKSSA | 99%    | 10,065.0 µg/mL              | +/- 453.3336                           |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

# Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

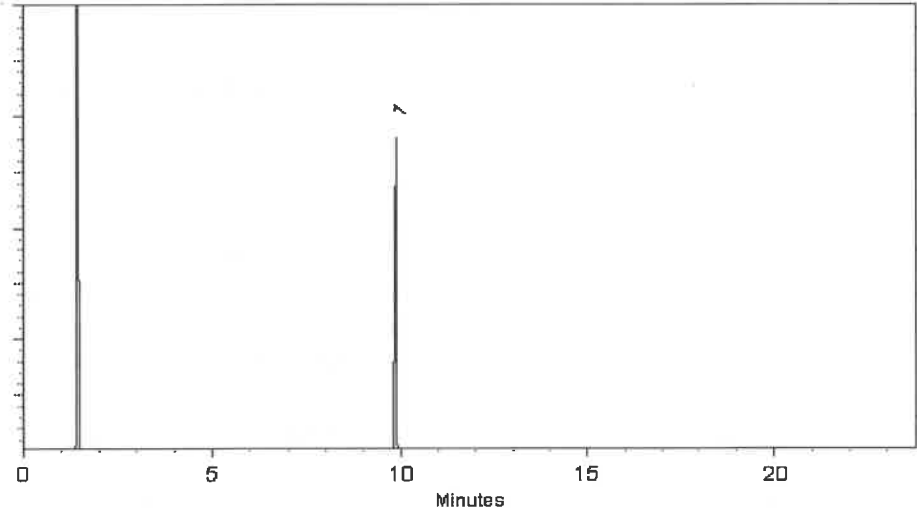

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ven Kelley - Operations Tech I

Date Mixed: 17-Sep-2024

Balance Serial # 1128353505

Dillan Murphy - Operations Technician I

Date Passed: 23-Sep-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31097 **Lot No.:** A0216631  
**Description :** o-Terphenyl Standard  
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** April 30, 2028 **Storage:** 10°C or colder  
**Handling:** Sonicate prior to use. **Ship:** Ambient

P13645 } Y.P.  
↓  
P13694 } 10/16/24

### CERTIFIED VALUES

| Elution Order | Compound    | CAS #   | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|-------------|---------|-------|--------|-----------------------------|----------------------------------------|
| 1             | o-Terphenyl | 84-15-1 | GKSSA | 99%    | 10,065.0 µg/mL              | +/- 453.3336                           |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

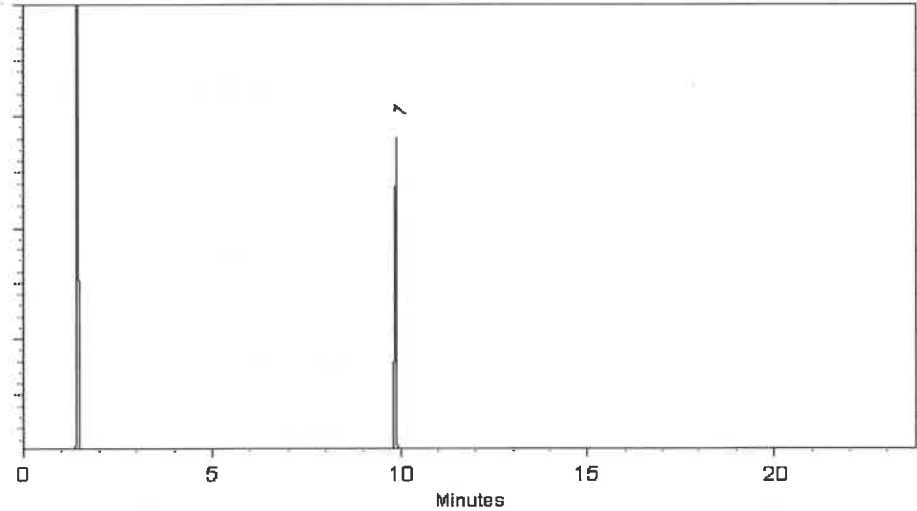

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ven Kelley - Operations Tech I

Date Mixed: 17-Sep-2024

Balance Serial # 1128353505

Dillan Murphy - Operations Technician I

Date Passed: 23-Sep-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31097 **Lot No.:** A0216631  
**Description :** o-Terphenyl Standard  
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** April 30, 2028 **Storage:** 10°C or colder  
**Handling:** Sonicate prior to use. **Ship:** Ambient

P13645 } Y.P.  
↓  
P13694 } 10/16/24

### CERTIFIED VALUES

| Elution Order | Compound    | CAS #   | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|-------------|---------|-------|--------|-----------------------------|----------------------------------------|
| 1             | o-Terphenyl | 84-15-1 | GKSSA | 99%    | 10,065.0 µg/mL              | +/- 453.3336                           |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

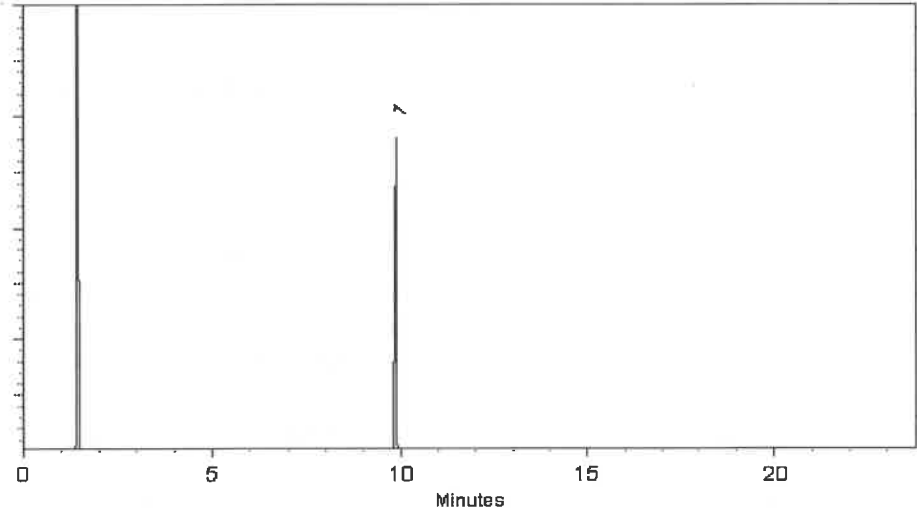

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ven Kelley - Operations Tech I

Date Mixed: 17-Sep-2024

Balance Serial # 1128353505

Dillan Murphy - Operations Technician I

Date Passed: 23-Sep-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31097 **Lot No.:** A0216631  
**Description :** o-Terphenyl Standard  
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** April 30, 2028 **Storage:** 10°C or colder  
**Handling:** Sonicate prior to use. **Ship:** Ambient

P13645 } Y.P.  
↓  
P13694 } 10/16/24

### CERTIFIED VALUES

| Elution Order | Compound    | CAS #   | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|-------------|---------|-------|--------|-----------------------------|----------------------------------------|
| 1             | o-Terphenyl | 84-15-1 | GKSSA | 99%    | 10,065.0 µg/mL              | +/- 453.3336                           |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

# Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

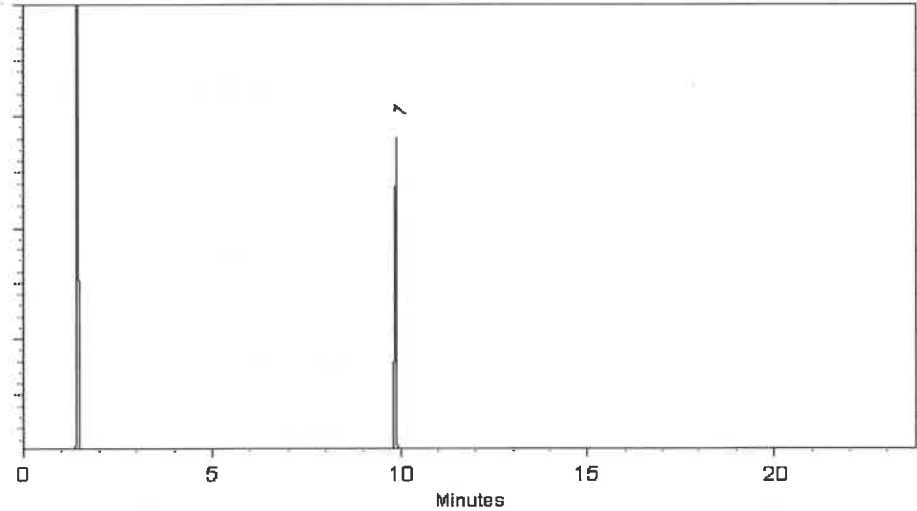

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ven Kelley - Operations Tech I

Date Mixed: 17-Sep-2024

Balance Serial # 1128353505

Dillan Murphy - Operations Technician I

Date Passed: 23-Sep-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543

**Lot No.:** A0211254

**Description :** NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

**Container Size :** 5 mL

**Pkg Amt:** > 5 mL

**Expiration Date :** April 30, 2030

**Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive.

**Ship:** Ambient

P13408  
↓  
P13716 } Y.P.  
10/26/24

### CERTIFIED VALUES

| Elution Order | Compound               | CAS #    | Lot #        | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------|----------|--------------|--------|-----------------------------|----------------------------------------|
| 1             | 1,2,3-Trimethylbenzene | 526-73-8 | 8776.10-38   | 99%    | 200.0 µg/mL                 | +/- 9.0114                             |
| 2             | Naphthalene            | 91-20-3  | STBL1057     | 99%    | 200.8 µg/mL                 | +/- 9.0474                             |
| 3             | 2-Methylnaphthalene    | 91-57-6  | STBK0259     | 96%    | 200.4 µg/mL                 | +/- 9.0316                             |
| 4             | Acenaphthylene         | 208-96-8 | 214935L31M   | 98%    | 200.3 µg/mL                 | +/- 9.0255                             |
| 5             | Acenaphthene           | 83-32-9  | MKCR7169     | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 6             | Fluorene               | 86-73-7  | 10241100     | 99%    | 201.2 µg/mL                 | +/- 9.0655                             |
| 7             | Phenanthrene           | 85-01-8  | MKCS5188     | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 8             | Anthracene             | 120-12-7 | MKCR0570     | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 9             | Fluoranthene           | 206-44-0 | MKCQ4728     | 99%    | 200.8 µg/mL                 | +/- 9.0474                             |
| 10            | Pyrene                 | 129-00-0 | BCCK2592     | 99%    | 201.2 µg/mL                 | +/- 9.0655                             |
| 11            | Benz(a)anthracene      | 56-55-3  | I30012022BAA | 99%    | 200.8 µg/mL                 | +/- 9.0474                             |
| 12            | Chrysene               | 218-01-9 | RP231206RSR  | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 13            | Benzo(b)fluoranthene   | 205-99-2 | 012013B      | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 14            | Benzo(k)fluoranthene   | 207-08-9 | 012022K      | 99%    | 200.0 µg/mL                 | +/- 9.0114                             |
| 15            | Benzo(a)pyrene         | 50-32-8  | O45GL        | 98%    | 200.7 µg/mL                 | +/- 9.0431                             |
| 16            | Indeno(1,2,3-cd)pyrene | 193-39-5 | 12-JKL-118-9 | 97%    | 199.8 µg/mL                 | +/- 9.0033                             |

|    |                       |          |             |     |       |       |            |
|----|-----------------------|----------|-------------|-----|-------|-------|------------|
| 17 | Dibenz(a,h)anthracene | 53-70-3  | 2-ASA-59-1  | 99% | 200.0 | µg/mL | +/- 9.0114 |
| 18 | Benzo(g,h,i)perylene  | 191-24-2 | RP240105ECS | 99% | 200.8 | µg/mL | +/- 9.0474 |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rbx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

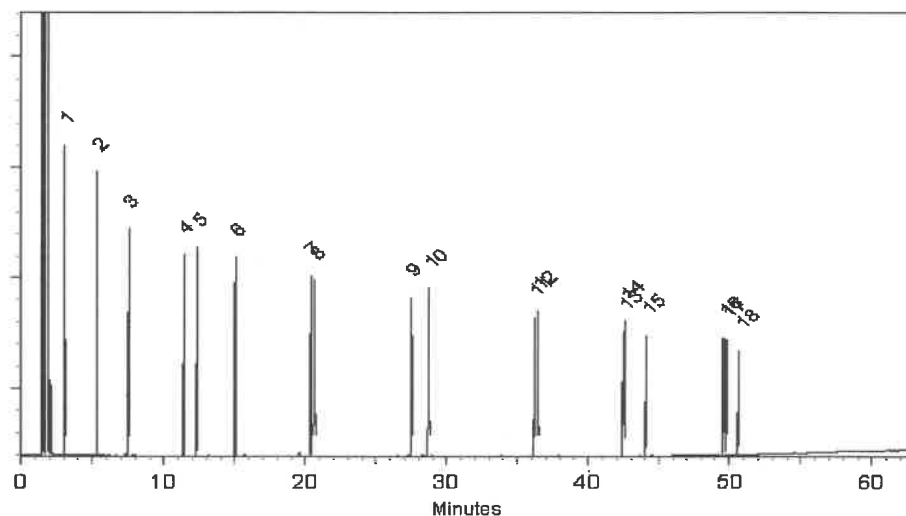

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Michael Maye*  
Michael Maye - Operations Tech I

**Date Mixed:** 09-May-2024 **Balance Serial #** 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 13-May-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31480 **Lot No.:** A0214879  
**Description :** MA Fractionation Surrogate Spike Mix  
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** July 31, 2030 **Storage:** 10°C or colder  
**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

P13743  
↓  
P13772 } Y.P.  
11/01/24

### CERTIFIED VALUES

| Elution Order | Compound           | CAS #    | Lot #     | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------|----------|-----------|--------|-----------------------------|----------------------------------------|
| 1             | 2-Fluorobiphenyl   | 321-60-8 | 00021384  | 99%    | 4,009.0 µg/mL               | +/- 180.5961                           |
| 2             | 2-Bromonaphthalene | 580-13-2 | STBC5362V | 99%    | 4,008.5 µg/mL               | +/- 180.5736                           |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

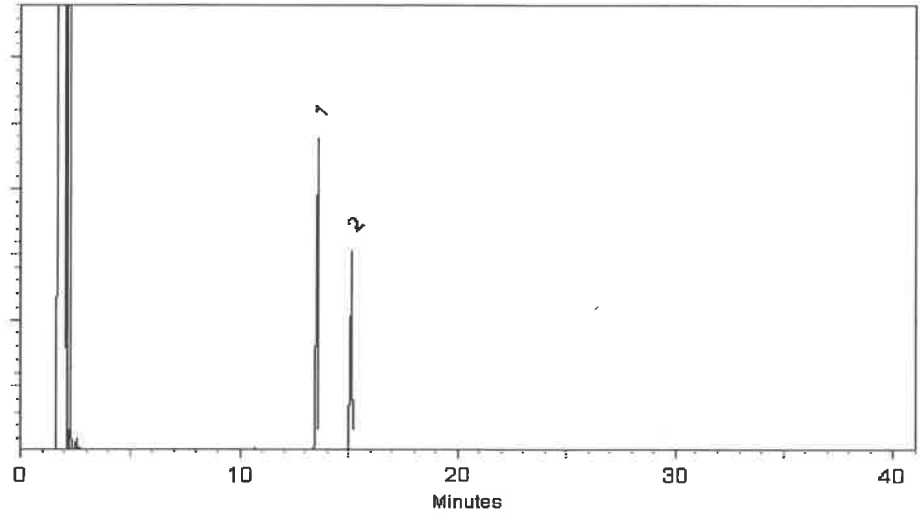

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Scott McNeil - Operations Tech I

Date Mixed: 06-Aug-2024

Balance Serial # 1128360905

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 14-Aug-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31480 **Lot No.:** A0214879  
**Description :** MA Fractionation Surrogate Spike Mix  
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** July 31, 2030 **Storage:** 10°C or colder  
**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

P13743  
↓  
P13772 } Y.P.  
11/01/24

### CERTIFIED VALUES

| Elution Order | Compound           | CAS #    | Lot #     | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------|----------|-----------|--------|-----------------------------|----------------------------------------|
| 1             | 2-Fluorobiphenyl   | 321-60-8 | 00021384  | 99%    | 4,009.0 µg/mL               | +/- 180.5961                           |
| 2             | 2-Bromonaphthalene | 580-13-2 | STBC5362V | 99%    | 4,008.5 µg/mL               | +/- 180.5736                           |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

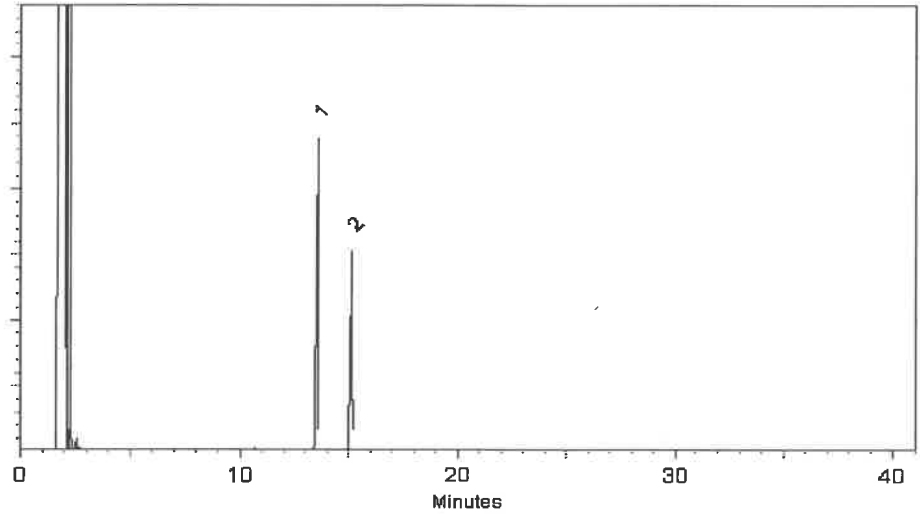

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Scott McNeil - Operations Tech I

Date Mixed: 06-Aug-2024

Balance Serial # 1128360905

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 14-Aug-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



## FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543 **Lot No.:** A0220580

**Description :** NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2030 **Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

P13863 } y.p.  
↓  
P13866 } 01/08/25

## CERTIFIED VALUES

| Elution Order | Compound               | CAS #    | Lot #           | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------|----------|-----------------|--------|-----------------------------|----------------------------------------|
| 1             | 1,2,3-Trimethylbenzene | 526-73-8 | 8776.10-39      | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 2             | Naphthalene            | 91-20-3  | STBL1057        | 99%    | 200.8 µg/mL                 | +/- 9.0474                             |
| 3             | 2-Methylnaphthalene    | 91-57-6  | STBL3028        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 4             | Acenaphthylene         | 208-96-8 | RP241029RSR     | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 5             | Acenaphthene           | 83-32-9  | MKCR7169        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 6             | Fluorene               | 86-73-7  | 10246250        | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 7             | Phenanthrene           | 85-01-8  | MKCT3391        | 99%    | 200.8 µg/mL                 | +/- 9.0474                             |
| 8             | Anthracene             | 120-12-7 | MKCW9141        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 9             | Fluoranthene           | 206-44-0 | MKCQ4728        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 10            | Pyrene                 | 129-00-0 | BCCL8032        | 99%    | 201.6 µg/mL                 | +/- 9.0835                             |
| 11            | Benz(a)anthracene      | 56-55-3  | I220012022BAA   | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 12            | Chrysene               | 218-01-9 | RP240719RSR     | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 13            | Benzo(b)fluoranthene   | 205-99-2 | SBS-BBF-FINAL-2 | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 14            | Benzo(k)fluoranthene   | 207-08-9 | 012022K         | 98%    | 201.5 µg/mL                 | +/- 9.0784                             |
| 15            | Benzo(a)pyrene         | 50-32-8  | NQLXA           | 98%    | 200.7 µg/mL                 | +/- 9.0431                             |
| 16            | Indeno(1,2,3-cd)pyrene | 193-39-5 | 12-JKL-118-9    | 97%    | 200.6 µg/mL                 | +/- 9.0383                             |

|    |                       |          |             |     |       |       |            |
|----|-----------------------|----------|-------------|-----|-------|-------|------------|
| 17 | Dibenz(a,h)anthracene | 53-70-3  | 2-ASA-59-1  | 99% | 201.2 | µg/mL | +/- 9.0655 |
| 18 | Benzo(g,h,i)perylene  | 191-24-2 | RP241014RSR | 98% | 200.3 | µg/mL | +/- 9.0255 |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

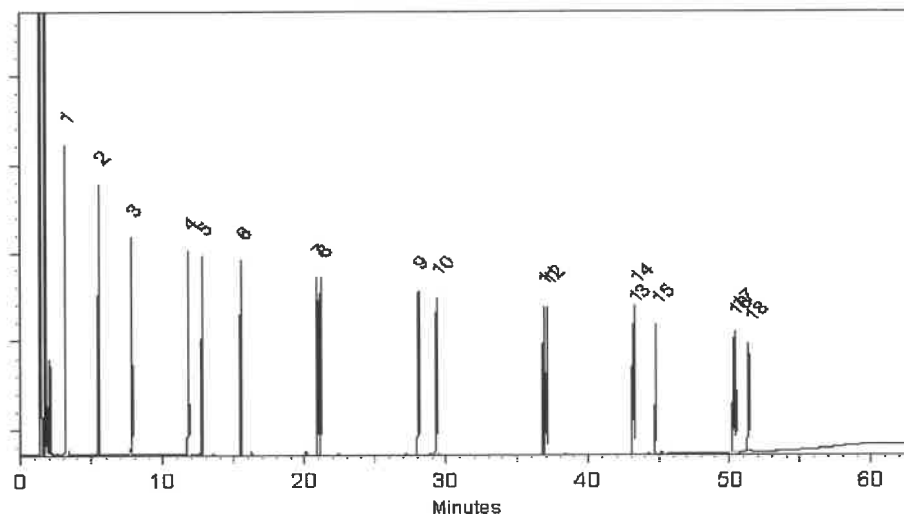

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Ven Kelley*  
**Ven Kelley - Operations Tech I**

**Date Mixed:** 30-Dec-2024 **Balance Serial #** 1128360905

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 03-Jan-2025

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30542 **Lot No.:** A0217408

**Description :** NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2031 **Storage:** 10°C or colder

**Handling:** Sonicate prior to use. **Ship:** Ambient

P13896  
↓  
P13906 } Y.P.  
03/06/25

### CERTIFIED VALUES

| Elution Order | Compound                 | CAS #      | Lot #      | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------------|------------|------------|--------|-----------------------------|----------------------------------------|
| 1             | n-Nonane (C9)            | 111-84-2   | SHBP9752   | 99%    | 200.7 µg/mL                 | +/- 5.1839                             |
| 2             | n-Decane (C10)           | 124-18-5   | SHBQ1342   | 99%    | 201.0 µg/mL                 | +/- 5.1917                             |
| 3             | n-Dodecane (C12)         | 112-40-3   | SHBP7054   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 4             | n-Tetradecane (C14)      | 629-59-4   | STBL0465   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 5             | n-Hexadecane (C16)       | 544-76-3   | SHBR0669   | 99%    | 200.7 µg/mL                 | +/- 5.1857                             |
| 6             | n-Octadecane (C18)       | 593-45-3   | UE5NG      | 99%    | 200.7 µg/mL                 | +/- 5.1857                             |
| 7             | n-Eicosane (C20)         | 112-95-8   | MKCN8767   | 97%    | 200.9 µg/mL                 | +/- 5.1888                             |
| 8             | n-Heneicosane (C21)      | 629-94-7   | MKCP1960   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 9             | n-Docosane (C22)         | 629-97-0   | MKCQ3882   | 99%    | 200.5 µg/mL                 | +/- 5.1788                             |
| 10            | n-Tetracosane (C24)      | 646-31-1   | MKCS9978   | 99%    | 200.6 µg/mL                 | +/- 5.1822                             |
| 11            | n-Hexacosane (C26)       | 630-01-3   | MKCQ4814   | 99%    | 200.5 µg/mL                 | +/- 5.1796                             |
| 12            | n-Octacosane (C28)       | 630-02-4   | BCCJ4566   | 99%    | 200.6 µg/mL                 | +/- 5.1822                             |
| 13            | n-Triacontane (C30)      | 638-68-6   | MKCV7007   | 98%    | 201.1 µg/mL                 | +/- 5.1942                             |
| 14            | n-Dotriacontane (C32)    | 544-85-4   | BCBW0661   | 99%    | 200.9 µg/mL                 | +/- 5.1891                             |
| 15            | n-Tetratriacontane (C34) | 14167-59-0 | 6JNHB      | 99%    | 200.8 µg/mL                 | +/- 5.1865                             |
| 16            | n-Hexatriacontane (C36)  | 630-06-8   | Z27H018    | 99%    | 200.6 µg/mL                 | +/- 5.1814                             |
| 17            | n-Octatriacontane (C38)  | 7194-85-6  | 0000207852 | 96%    | 199.3 µg/mL                 | +/- 5.1477                             |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane**CAS #** 109-66-0**Purity** 99%

## Quality Confirmation Test

**Column:**30m x 0.25mm x 0.25µm  
Rtx-S (cat.#10223)**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

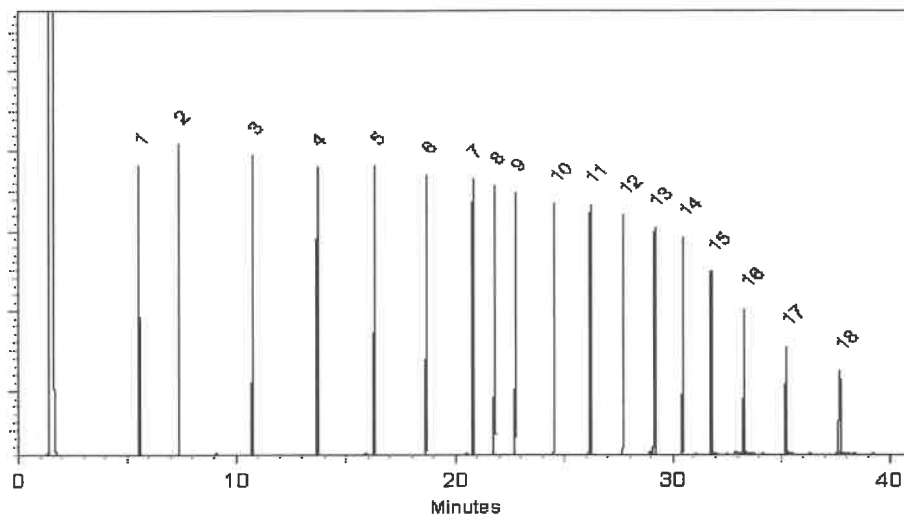

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope B. Riglin*  
Penelope Riglin - Operations Tech I

**Date Mixed:** 03-Oct-2024**Balance Serial #** 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30542 **Lot No.:** A0217408

**Description :** NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2031 **Storage:** 10°C or colder

**Handling:** Sonicate prior to use. **Ship:** Ambient

P13896  
↓  
P13906 } Y.P.  
03/06/25

### CERTIFIED VALUES

| Elution Order | Compound                 | CAS #      | Lot #      | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------------|------------|------------|--------|-----------------------------|----------------------------------------|
| 1             | n-Nonane (C9)            | 111-84-2   | SHBP9752   | 99%    | 200.7 µg/mL                 | +/- 5.1839                             |
| 2             | n-Decane (C10)           | 124-18-5   | SHBQ1342   | 99%    | 201.0 µg/mL                 | +/- 5.1917                             |
| 3             | n-Dodecane (C12)         | 112-40-3   | SHBP7054   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 4             | n-Tetradecane (C14)      | 629-59-4   | STBL0465   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 5             | n-Hexadecane (C16)       | 544-76-3   | SHBR0669   | 99%    | 200.7 µg/mL                 | +/- 5.1857                             |
| 6             | n-Octadecane (C18)       | 593-45-3   | UE5NG      | 99%    | 200.7 µg/mL                 | +/- 5.1857                             |
| 7             | n-Eicosane (C20)         | 112-95-8   | MKCN8767   | 97%    | 200.9 µg/mL                 | +/- 5.1888                             |
| 8             | n-Heneicosane (C21)      | 629-94-7   | MKCP1960   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 9             | n-Docosane (C22)         | 629-97-0   | MKCQ3882   | 99%    | 200.5 µg/mL                 | +/- 5.1788                             |
| 10            | n-Tetracosane (C24)      | 646-31-1   | MKCS9978   | 99%    | 200.6 µg/mL                 | +/- 5.1822                             |
| 11            | n-Hexacosane (C26)       | 630-01-3   | MKCQ4814   | 99%    | 200.5 µg/mL                 | +/- 5.1796                             |
| 12            | n-Octacosane (C28)       | 630-02-4   | BCCJ4566   | 99%    | 200.6 µg/mL                 | +/- 5.1822                             |
| 13            | n-Triacontane (C30)      | 638-68-6   | MKCV7007   | 98%    | 201.1 µg/mL                 | +/- 5.1942                             |
| 14            | n-Dotriacontane (C32)    | 544-85-4   | BCBW0661   | 99%    | 200.9 µg/mL                 | +/- 5.1891                             |
| 15            | n-Tetratriacontane (C34) | 14167-59-0 | 6JNHB      | 99%    | 200.8 µg/mL                 | +/- 5.1865                             |
| 16            | n-Hexatriacontane (C36)  | 630-06-8   | Z27H018    | 99%    | 200.6 µg/mL                 | +/- 5.1814                             |
| 17            | n-Octatriacontane (C38)  | 7194-85-6  | 0000207852 | 96%    | 199.3 µg/mL                 | +/- 5.1477                             |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane**CAS #** 109-66-0**Purity** 99%

## Quality Confirmation Test

**Column:**30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

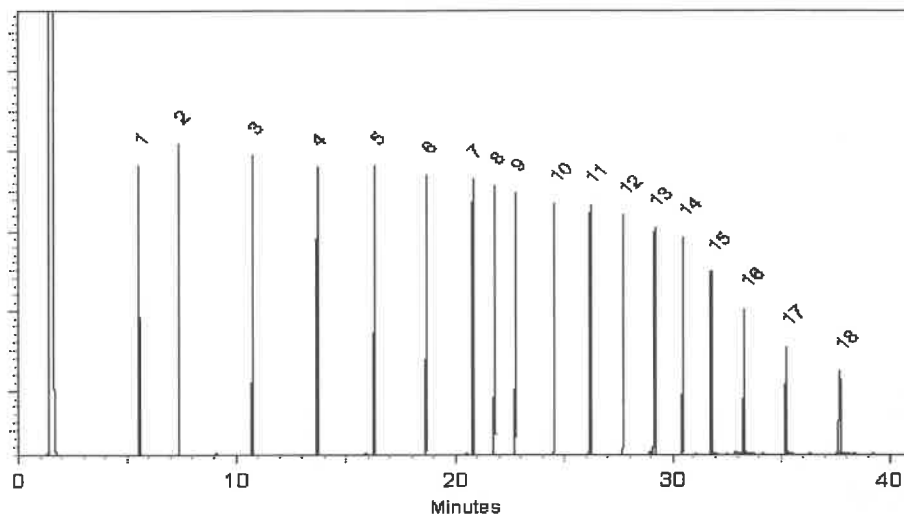

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope B. Riglin*  
Penelope Riglin - Operations Tech I

**Date Mixed:** 03-Oct-2024**Balance Serial #** 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30542 **Lot No.:** A0217408

**Description :** NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2031 **Storage:** 10°C or colder

**Handling:** Sonicate prior to use. **Ship:** Ambient

P13896  
↓  
P13906 } Y.P.  
03/06/25

### CERTIFIED VALUES

| Elution Order | Compound                 | CAS #      | Lot #      | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------------|------------|------------|--------|-----------------------------|----------------------------------------|
| 1             | n-Nonane (C9)            | 111-84-2   | SHBP9752   | 99%    | 200.7 µg/mL                 | +/- 5.1839                             |
| 2             | n-Decane (C10)           | 124-18-5   | SHBQ1342   | 99%    | 201.0 µg/mL                 | +/- 5.1917                             |
| 3             | n-Dodecane (C12)         | 112-40-3   | SHBP7054   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 4             | n-Tetradecane (C14)      | 629-59-4   | STBL0465   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 5             | n-Hexadecane (C16)       | 544-76-3   | SHBR0669   | 99%    | 200.7 µg/mL                 | +/- 5.1857                             |
| 6             | n-Octadecane (C18)       | 593-45-3   | UE5NG      | 99%    | 200.7 µg/mL                 | +/- 5.1857                             |
| 7             | n-Eicosane (C20)         | 112-95-8   | MKCN8767   | 97%    | 200.9 µg/mL                 | +/- 5.1888                             |
| 8             | n-Heneicosane (C21)      | 629-94-7   | MKCP1960   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 9             | n-Docosane (C22)         | 629-97-0   | MKCQ3882   | 99%    | 200.5 µg/mL                 | +/- 5.1788                             |
| 10            | n-Tetracosane (C24)      | 646-31-1   | MKCS9978   | 99%    | 200.6 µg/mL                 | +/- 5.1822                             |
| 11            | n-Hexacosane (C26)       | 630-01-3   | MKCQ4814   | 99%    | 200.5 µg/mL                 | +/- 5.1796                             |
| 12            | n-Octacosane (C28)       | 630-02-4   | BCCJ4566   | 99%    | 200.6 µg/mL                 | +/- 5.1822                             |
| 13            | n-Triacontane (C30)      | 638-68-6   | MKCV7007   | 98%    | 201.1 µg/mL                 | +/- 5.1942                             |
| 14            | n-Dotriacontane (C32)    | 544-85-4   | BCBW0661   | 99%    | 200.9 µg/mL                 | +/- 5.1891                             |
| 15            | n-Tetratriacontane (C34) | 14167-59-0 | 6JNHB      | 99%    | 200.8 µg/mL                 | +/- 5.1865                             |
| 16            | n-Hexatriacontane (C36)  | 630-06-8   | Z27H018    | 99%    | 200.6 µg/mL                 | +/- 5.1814                             |
| 17            | n-Octatriacontane (C38)  | 7194-85-6  | 0000207852 | 96%    | 199.3 µg/mL                 | +/- 5.1477                             |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane**CAS #** 109-66-0**Purity** 99%

## Quality Confirmation Test

**Column:**30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

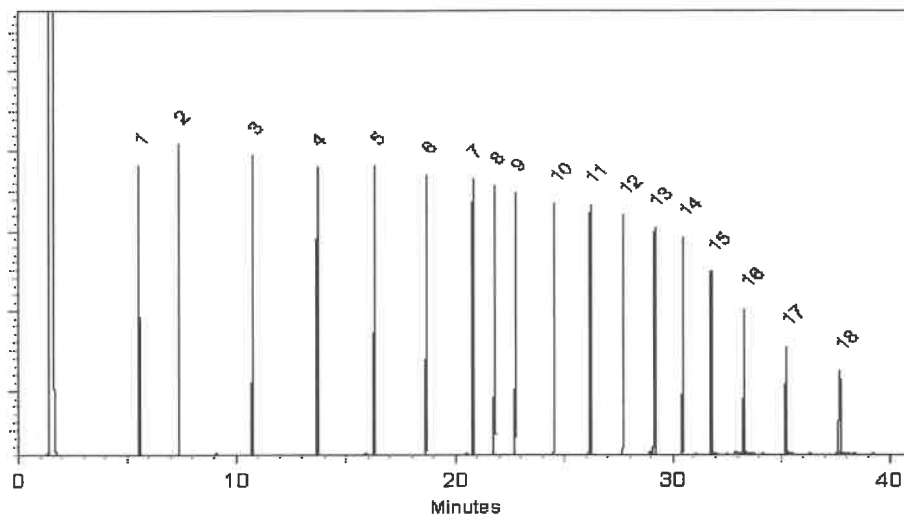

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope B. Riglin*  
Penelope Riglin - Operations Tech I

**Date Mixed:** 03-Oct-2024**Balance Serial #** 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30542 **Lot No.:** A0217408

**Description :** NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2031 **Storage:** 10°C or colder

**Handling:** Sonicate prior to use. **Ship:** Ambient

P13896  
↓  
P13906 } Y.P.  
03/06/25

### CERTIFIED VALUES

| Elution Order | Compound                 | CAS #      | Lot #      | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------------|------------|------------|--------|-----------------------------|----------------------------------------|
| 1             | n-Nonane (C9)            | 111-84-2   | SHBP9752   | 99%    | 200.7 µg/mL                 | +/- 5.1839                             |
| 2             | n-Decane (C10)           | 124-18-5   | SHBQ1342   | 99%    | 201.0 µg/mL                 | +/- 5.1917                             |
| 3             | n-Dodecane (C12)         | 112-40-3   | SHBP7054   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 4             | n-Tetradecane (C14)      | 629-59-4   | STBL0465   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 5             | n-Hexadecane (C16)       | 544-76-3   | SHBR0669   | 99%    | 200.7 µg/mL                 | +/- 5.1857                             |
| 6             | n-Octadecane (C18)       | 593-45-3   | UE5NG      | 99%    | 200.7 µg/mL                 | +/- 5.1857                             |
| 7             | n-Eicosane (C20)         | 112-95-8   | MKCN8767   | 97%    | 200.9 µg/mL                 | +/- 5.1888                             |
| 8             | n-Heneicosane (C21)      | 629-94-7   | MKCP1960   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 9             | n-Docosane (C22)         | 629-97-0   | MKCQ3882   | 99%    | 200.5 µg/mL                 | +/- 5.1788                             |
| 10            | n-Tetracosane (C24)      | 646-31-1   | MKCS9978   | 99%    | 200.6 µg/mL                 | +/- 5.1822                             |
| 11            | n-Hexacosane (C26)       | 630-01-3   | MKCQ4814   | 99%    | 200.5 µg/mL                 | +/- 5.1796                             |
| 12            | n-Octacosane (C28)       | 630-02-4   | BCCJ4566   | 99%    | 200.6 µg/mL                 | +/- 5.1822                             |
| 13            | n-Triacontane (C30)      | 638-68-6   | MKCV7007   | 98%    | 201.1 µg/mL                 | +/- 5.1942                             |
| 14            | n-Dotriacontane (C32)    | 544-85-4   | BCBW0661   | 99%    | 200.9 µg/mL                 | +/- 5.1891                             |
| 15            | n-Tetratriacontane (C34) | 14167-59-0 | 6JNHB      | 99%    | 200.8 µg/mL                 | +/- 5.1865                             |
| 16            | n-Hexatriacontane (C36)  | 630-06-8   | Z27H018    | 99%    | 200.6 µg/mL                 | +/- 5.1814                             |
| 17            | n-Octatriacontane (C38)  | 7194-85-6  | 0000207852 | 96%    | 199.3 µg/mL                 | +/- 5.1477                             |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane**CAS #** 109-66-0**Purity** 99%

## Quality Confirmation Test

**Column:**30m x 0.25mm x 0.25µm  
Rtx-S (cat.#10223)**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

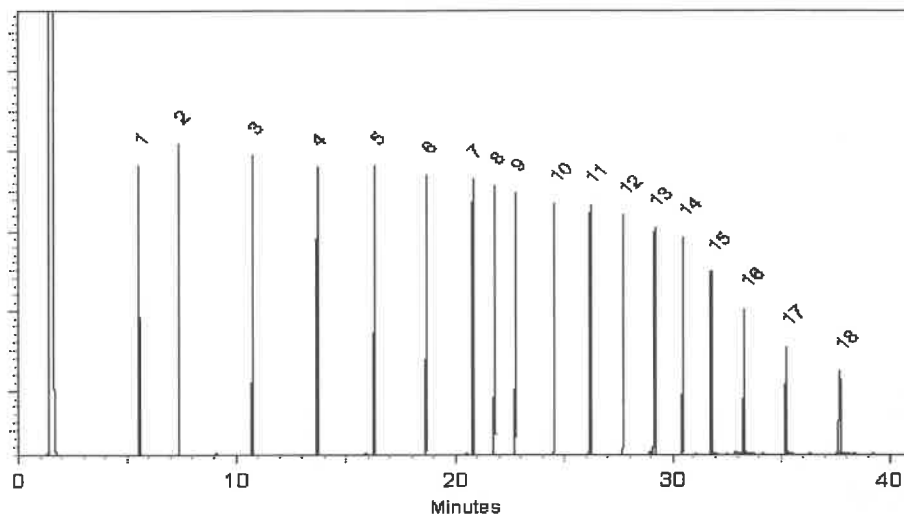

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope B. Riglin*  
Penelope Riglin - Operations Tech I

**Date Mixed:** 03-Oct-2024**Balance Serial #** 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30542 **Lot No.:** A0217408

**Description :** NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2031 **Storage:** 10°C or colder

**Handling:** Sonicate prior to use. **Ship:** Ambient

P13896  
↓  
P13906 } Y.P.  
03/06/25

### CERTIFIED VALUES

| Elution Order | Compound                 | CAS #      | Lot #      | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------------|------------|------------|--------|-----------------------------|----------------------------------------|
| 1             | n-Nonane (C9)            | 111-84-2   | SHBP9752   | 99%    | 200.7 µg/mL                 | +/- 5.1839                             |
| 2             | n-Decane (C10)           | 124-18-5   | SHBQ1342   | 99%    | 201.0 µg/mL                 | +/- 5.1917                             |
| 3             | n-Dodecane (C12)         | 112-40-3   | SHBP7054   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 4             | n-Tetradecane (C14)      | 629-59-4   | STBL0465   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 5             | n-Hexadecane (C16)       | 544-76-3   | SHBR0669   | 99%    | 200.7 µg/mL                 | +/- 5.1857                             |
| 6             | n-Octadecane (C18)       | 593-45-3   | UE5NG      | 99%    | 200.7 µg/mL                 | +/- 5.1857                             |
| 7             | n-Eicosane (C20)         | 112-95-8   | MKCN8767   | 97%    | 200.9 µg/mL                 | +/- 5.1888                             |
| 8             | n-Heneicosane (C21)      | 629-94-7   | MKCP1960   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 9             | n-Docosane (C22)         | 629-97-0   | MKCQ3882   | 99%    | 200.5 µg/mL                 | +/- 5.1788                             |
| 10            | n-Tetracosane (C24)      | 646-31-1   | MKCS9978   | 99%    | 200.6 µg/mL                 | +/- 5.1822                             |
| 11            | n-Hexacosane (C26)       | 630-01-3   | MKCQ4814   | 99%    | 200.5 µg/mL                 | +/- 5.1796                             |
| 12            | n-Octacosane (C28)       | 630-02-4   | BCCJ4566   | 99%    | 200.6 µg/mL                 | +/- 5.1822                             |
| 13            | n-Triacontane (C30)      | 638-68-6   | MKCV7007   | 98%    | 201.1 µg/mL                 | +/- 5.1942                             |
| 14            | n-Dotriacontane (C32)    | 544-85-4   | BCBW0661   | 99%    | 200.9 µg/mL                 | +/- 5.1891                             |
| 15            | n-Tetratriacontane (C34) | 14167-59-0 | 6JNHB      | 99%    | 200.8 µg/mL                 | +/- 5.1865                             |
| 16            | n-Hexatriacontane (C36)  | 630-06-8   | Z27H018    | 99%    | 200.6 µg/mL                 | +/- 5.1814                             |
| 17            | n-Octatriacontane (C38)  | 7194-85-6  | 0000207852 | 96%    | 199.3 µg/mL                 | +/- 5.1477                             |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane**CAS #** 109-66-0**Purity** 99%

## Quality Confirmation Test

**Column:**30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

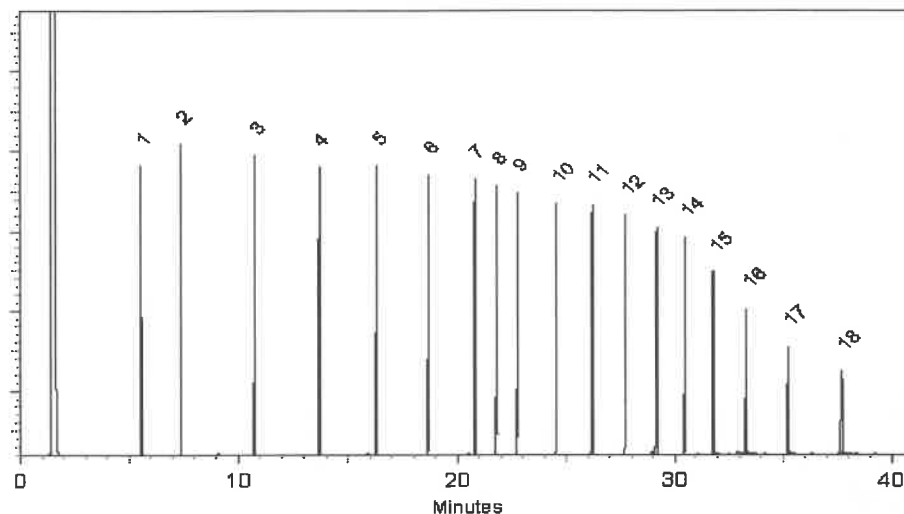

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope B. Riglin*  
Penelope Riglin - Operations Tech I

**Date Mixed:** 03-Oct-2024**Balance Serial #** 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30542 **Lot No.:** A0217408

**Description :** NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2031 **Storage:** 10°C or colder

**Handling:** Sonicate prior to use. **Ship:** Ambient

P13896  
↓  
P13906 } Y.P.  
03/06/25

### CERTIFIED VALUES

| Elution Order | Compound                 | CAS #      | Lot #      | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------------|------------|------------|--------|-----------------------------|----------------------------------------|
| 1             | n-Nonane (C9)            | 111-84-2   | SHBP9752   | 99%    | 200.7 µg/mL                 | +/- 5.1839                             |
| 2             | n-Decane (C10)           | 124-18-5   | SHBQ1342   | 99%    | 201.0 µg/mL                 | +/- 5.1917                             |
| 3             | n-Dodecane (C12)         | 112-40-3   | SHBP7054   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 4             | n-Tetradecane (C14)      | 629-59-4   | STBL0465   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 5             | n-Hexadecane (C16)       | 544-76-3   | SHBR0669   | 99%    | 200.7 µg/mL                 | +/- 5.1857                             |
| 6             | n-Octadecane (C18)       | 593-45-3   | UE5NG      | 99%    | 200.7 µg/mL                 | +/- 5.1857                             |
| 7             | n-Eicosane (C20)         | 112-95-8   | MKCN8767   | 97%    | 200.9 µg/mL                 | +/- 5.1888                             |
| 8             | n-Heneicosane (C21)      | 629-94-7   | MKCP1960   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 9             | n-Docosane (C22)         | 629-97-0   | MKCQ3882   | 99%    | 200.5 µg/mL                 | +/- 5.1788                             |
| 10            | n-Tetracosane (C24)      | 646-31-1   | MKCS9978   | 99%    | 200.6 µg/mL                 | +/- 5.1822                             |
| 11            | n-Hexacosane (C26)       | 630-01-3   | MKCQ4814   | 99%    | 200.5 µg/mL                 | +/- 5.1796                             |
| 12            | n-Octacosane (C28)       | 630-02-4   | BCCJ4566   | 99%    | 200.6 µg/mL                 | +/- 5.1822                             |
| 13            | n-Triacontane (C30)      | 638-68-6   | MKCV7007   | 98%    | 201.1 µg/mL                 | +/- 5.1942                             |
| 14            | n-Dotriacontane (C32)    | 544-85-4   | BCBW0661   | 99%    | 200.9 µg/mL                 | +/- 5.1891                             |
| 15            | n-Tetratriacontane (C34) | 14167-59-0 | 6JNHB      | 99%    | 200.8 µg/mL                 | +/- 5.1865                             |
| 16            | n-Hexatriacontane (C36)  | 630-06-8   | Z27H018    | 99%    | 200.6 µg/mL                 | +/- 5.1814                             |
| 17            | n-Octatriacontane (C38)  | 7194-85-6  | 0000207852 | 96%    | 199.3 µg/mL                 | +/- 5.1477                             |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane**CAS #** 109-66-0**Purity** 99%

## Quality Confirmation Test

**Column:**30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

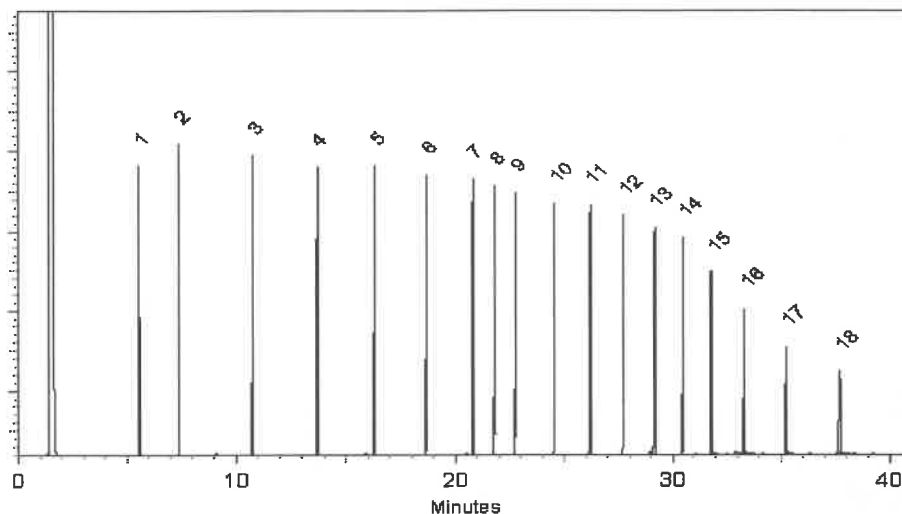

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope B. Riglin*  
Penelope Riglin - Operations Tech I

**Date Mixed:** 03-Oct-2024**Balance Serial #** 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30542 **Lot No.:** A0217408

**Description :** NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2031 **Storage:** 10°C or colder

**Handling:** Sonicate prior to use. **Ship:** Ambient

P13896  
↓  
P13906 } Y.P.  
03/06/25

### CERTIFIED VALUES

| Elution Order | Compound                 | CAS #      | Lot #      | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------------|------------|------------|--------|-----------------------------|----------------------------------------|
| 1             | n-Nonane (C9)            | 111-84-2   | SHBP9752   | 99%    | 200.7 µg/mL                 | +/- 5.1839                             |
| 2             | n-Decane (C10)           | 124-18-5   | SHBQ1342   | 99%    | 201.0 µg/mL                 | +/- 5.1917                             |
| 3             | n-Dodecane (C12)         | 112-40-3   | SHBP7054   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 4             | n-Tetradecane (C14)      | 629-59-4   | STBL0465   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 5             | n-Hexadecane (C16)       | 544-76-3   | SHBR0669   | 99%    | 200.7 µg/mL                 | +/- 5.1857                             |
| 6             | n-Octadecane (C18)       | 593-45-3   | UE5NG      | 99%    | 200.7 µg/mL                 | +/- 5.1857                             |
| 7             | n-Eicosane (C20)         | 112-95-8   | MKCN8767   | 97%    | 200.9 µg/mL                 | +/- 5.1888                             |
| 8             | n-Heneicosane (C21)      | 629-94-7   | MKCP1960   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 9             | n-Docosane (C22)         | 629-97-0   | MKCQ3882   | 99%    | 200.5 µg/mL                 | +/- 5.1788                             |
| 10            | n-Tetracosane (C24)      | 646-31-1   | MKCS9978   | 99%    | 200.6 µg/mL                 | +/- 5.1822                             |
| 11            | n-Hexacosane (C26)       | 630-01-3   | MKCQ4814   | 99%    | 200.5 µg/mL                 | +/- 5.1796                             |
| 12            | n-Octacosane (C28)       | 630-02-4   | BCCJ4566   | 99%    | 200.6 µg/mL                 | +/- 5.1822                             |
| 13            | n-Triacontane (C30)      | 638-68-6   | MKCV7007   | 98%    | 201.1 µg/mL                 | +/- 5.1942                             |
| 14            | n-Dotriacontane (C32)    | 544-85-4   | BCBW0661   | 99%    | 200.9 µg/mL                 | +/- 5.1891                             |
| 15            | n-Tetratriacontane (C34) | 14167-59-0 | 6JNHB      | 99%    | 200.8 µg/mL                 | +/- 5.1865                             |
| 16            | n-Hexatriacontane (C36)  | 630-06-8   | Z27H018    | 99%    | 200.6 µg/mL                 | +/- 5.1814                             |
| 17            | n-Octatriacontane (C38)  | 7194-85-6  | 0000207852 | 96%    | 199.3 µg/mL                 | +/- 5.1477                             |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane  
**CAS #** 109-66-0  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)  
**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
2 ml/min.

**Inj. Vol**  
1µl

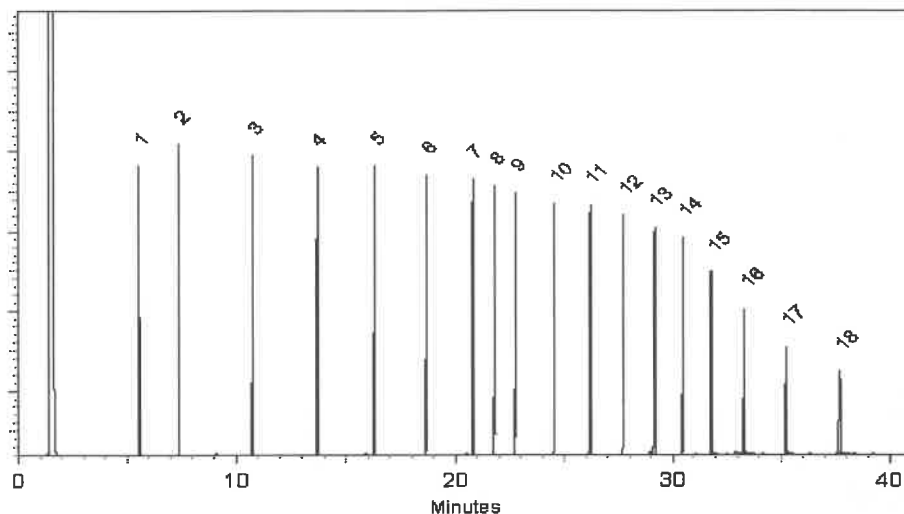

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope B. Riglin*  
Penelope Riglin - Operations Tech I

**Date Mixed:** 03-Oct-2024

**Balance Serial #** 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30542 **Lot No.:** A0217408

**Description :** NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2031 **Storage:** 10°C or colder

**Handling:** Sonicate prior to use. **Ship:** Ambient

P13896  
↓  
P13906 } Y.P.  
03/06/25

### CERTIFIED VALUES

| Elution Order | Compound                 | CAS #      | Lot #      | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------------|------------|------------|--------|-----------------------------|----------------------------------------|
| 1             | n-Nonane (C9)            | 111-84-2   | SHBP9752   | 99%    | 200.7 µg/mL                 | +/- 5.1839                             |
| 2             | n-Decane (C10)           | 124-18-5   | SHBQ1342   | 99%    | 201.0 µg/mL                 | +/- 5.1917                             |
| 3             | n-Dodecane (C12)         | 112-40-3   | SHBP7054   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 4             | n-Tetradecane (C14)      | 629-59-4   | STBL0465   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 5             | n-Hexadecane (C16)       | 544-76-3   | SHBR0669   | 99%    | 200.7 µg/mL                 | +/- 5.1857                             |
| 6             | n-Octadecane (C18)       | 593-45-3   | UE5NG      | 99%    | 200.7 µg/mL                 | +/- 5.1857                             |
| 7             | n-Eicosane (C20)         | 112-95-8   | MKCN8767   | 97%    | 200.9 µg/mL                 | +/- 5.1888                             |
| 8             | n-Heneicosane (C21)      | 629-94-7   | MKCP1960   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 9             | n-Docosane (C22)         | 629-97-0   | MKCQ3882   | 99%    | 200.5 µg/mL                 | +/- 5.1788                             |
| 10            | n-Tetracosane (C24)      | 646-31-1   | MKCS9978   | 99%    | 200.6 µg/mL                 | +/- 5.1822                             |
| 11            | n-Hexacosane (C26)       | 630-01-3   | MKCQ4814   | 99%    | 200.5 µg/mL                 | +/- 5.1796                             |
| 12            | n-Octacosane (C28)       | 630-02-4   | BCCJ4566   | 99%    | 200.6 µg/mL                 | +/- 5.1822                             |
| 13            | n-Triacontane (C30)      | 638-68-6   | MKCV7007   | 98%    | 201.1 µg/mL                 | +/- 5.1942                             |
| 14            | n-Dotriacontane (C32)    | 544-85-4   | BCBW0661   | 99%    | 200.9 µg/mL                 | +/- 5.1891                             |
| 15            | n-Tetratriacontane (C34) | 14167-59-0 | 6JNHB      | 99%    | 200.8 µg/mL                 | +/- 5.1865                             |
| 16            | n-Hexatriacontane (C36)  | 630-06-8   | Z27H018    | 99%    | 200.6 µg/mL                 | +/- 5.1814                             |
| 17            | n-Octatriacontane (C38)  | 7194-85-6  | 0000207852 | 96%    | 199.3 µg/mL                 | +/- 5.1477                             |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane**CAS #** 109-66-0**Purity** 99%

## Quality Confirmation Test

**Column:**30m x 0.25mm x 0.25µm  
Rtx-S (cat.#10223)**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

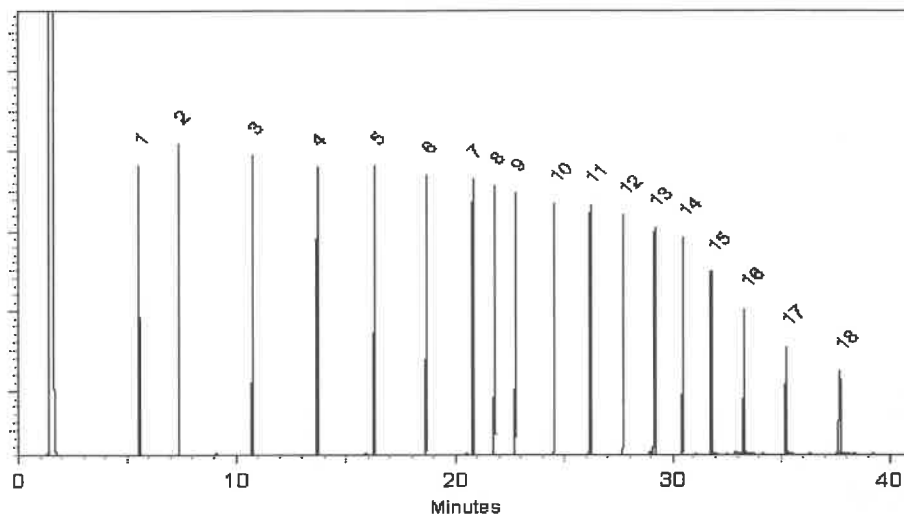

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope B. Riglin*  
Penelope Riglin - Operations Tech I

**Date Mixed:** 03-Oct-2024**Balance Serial #** 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30542 **Lot No.:** A0217408

**Description :** NJEPH Aliphatics Matrix Spike Mix

NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2031 **Storage:** 10°C or colder

**Handling:** Sonicate prior to use. **Ship:** Ambient

P13896  
↓  
P13906 } Y.P.  
03/06/25

### CERTIFIED VALUES

| Elution Order | Compound                 | CAS #      | Lot #      | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------------|------------|------------|--------|-----------------------------|----------------------------------------|
| 1             | n-Nonane (C9)            | 111-84-2   | SHBP9752   | 99%    | 200.7 µg/mL                 | +/- 5.1839                             |
| 2             | n-Decane (C10)           | 124-18-5   | SHBQ1342   | 99%    | 201.0 µg/mL                 | +/- 5.1917                             |
| 3             | n-Dodecane (C12)         | 112-40-3   | SHBP7054   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 4             | n-Tetradecane (C14)      | 629-59-4   | STBL0465   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 5             | n-Hexadecane (C16)       | 544-76-3   | SHBR0669   | 99%    | 200.7 µg/mL                 | +/- 5.1857                             |
| 6             | n-Octadecane (C18)       | 593-45-3   | UE5NG      | 99%    | 200.7 µg/mL                 | +/- 5.1857                             |
| 7             | n-Eicosane (C20)         | 112-95-8   | MKCN8767   | 97%    | 200.9 µg/mL                 | +/- 5.1888                             |
| 8             | n-Heneicosane (C21)      | 629-94-7   | MKCP1960   | 99%    | 200.5 µg/mL                 | +/- 5.1805                             |
| 9             | n-Docosane (C22)         | 629-97-0   | MKCQ3882   | 99%    | 200.5 µg/mL                 | +/- 5.1788                             |
| 10            | n-Tetracosane (C24)      | 646-31-1   | MKCS9978   | 99%    | 200.6 µg/mL                 | +/- 5.1822                             |
| 11            | n-Hexacosane (C26)       | 630-01-3   | MKCQ4814   | 99%    | 200.5 µg/mL                 | +/- 5.1796                             |
| 12            | n-Octacosane (C28)       | 630-02-4   | BCCJ4566   | 99%    | 200.6 µg/mL                 | +/- 5.1822                             |
| 13            | n-Triacontane (C30)      | 638-68-6   | MKCV7007   | 98%    | 201.1 µg/mL                 | +/- 5.1942                             |
| 14            | n-Dotriacontane (C32)    | 544-85-4   | BCBW0661   | 99%    | 200.9 µg/mL                 | +/- 5.1891                             |
| 15            | n-Tetratriacontane (C34) | 14167-59-0 | 6JNHB      | 99%    | 200.8 µg/mL                 | +/- 5.1865                             |
| 16            | n-Hexatriacontane (C36)  | 630-06-8   | Z27H018    | 99%    | 200.6 µg/mL                 | +/- 5.1814                             |
| 17            | n-Octatriacontane (C38)  | 7194-85-6  | 0000207852 | 96%    | 199.3 µg/mL                 | +/- 5.1477                             |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane**CAS #** 109-66-0**Purity** 99%

## Quality Confirmation Test

**Column:**30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

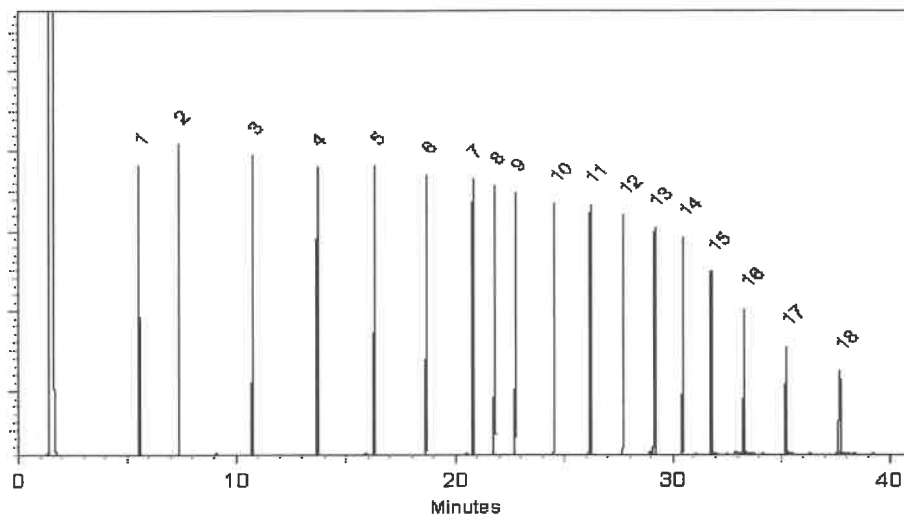

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope B. Riglin*  
Penelope Riglin - Operations Tech I

**Date Mixed:** 03-Oct-2024**Balance Serial #** 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30542 **Lot No.:** A0220449

**Description :** NJEPH Aliphatics Matrix Spike Mix  
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

**Container Size :** 5 mL **Pkg Amt:** > 5 mL

**Expiration Date :** January 31, 2032 **Storage:** 10°C or colder

**Handling:** Sonicate prior to use. **Ship:** Ambient

P13909  
↓  
P1395 } Y.P.  
03/06/25

### CERTIFIED VALUES

| Elution Order | Compound                 | CAS #      | Lot #      | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------------|------------|------------|--------|-----------------------------|----------------------------------------|
| 1             | n-Nonane (C9)            | 111-84-2   | SHBP9752   | 99%    | 201.3 µg/mL                 | +/- 5.2012                             |
| 2             | n-Decane (C10)           | 124-18-5   | SHBQ1342   | 99%    | 201.7 µg/mL                 | +/- 5.2098                             |
| 3             | n-Dodecane (C12)         | 112-40-3   | SHBP7054   | 99%    | 201.3 µg/mL                 | +/- 5.2012                             |
| 4             | n-Tetradecane (C14)      | 629-59-4   | STBL0465   | 99%    | 200.7 µg/mL                 | +/- 5.1839                             |
| 5             | n-Hexadecane (C16)       | 544-76-3   | SHBR0669   | 99%    | 200.3 µg/mL                 | +/- 5.1753                             |
| 6             | n-Octadecane (C18)       | 593-45-3   | UE5NG      | 99%    | 200.7 µg/mL                 | +/- 5.1839                             |
| 7             | n-Eicosane (C20)         | 112-95-8   | MKCN8767   | 97%    | 200.1 µg/mL                 | +/- 5.1704                             |
| 8             | n-Heneicosane (C21)      | 629-94-7   | MKCP1960   | 99%    | 200.7 µg/mL                 | +/- 5.1839                             |
| 9             | n-Docosane (C22)         | 629-97-0   | MKCQ3882   | 99%    | 200.3 µg/mL                 | +/- 5.1753                             |
| 10            | n-Tetracosane (C24)      | 646-31-1   | UH5GN      | 99%    | 201.3 µg/mL                 | +/- 5.2012                             |
| 11            | n-Hexacosane (C26)       | 630-01-3   | MKCQ4814   | 99%    | 201.0 µg/mL                 | +/- 5.1926                             |
| 12            | n-Octacosane (C28)       | 630-02-4   | BCCJ4566   | 99%    | 200.3 µg/mL                 | +/- 5.1753                             |
| 13            | n-Triacontane (C30)      | 638-68-6   | MKCV7007   | 98%    | 201.2 µg/mL                 | +/- 5.1984                             |
| 14            | n-Dotriacontane (C32)    | 544-85-4   | BCBW0661   | 99%    | 201.7 µg/mL                 | +/- 5.2098                             |
| 15            | n-Tetratriacontane (C34) | 14167-59-0 | 6JNHB      | 99%    | 201.3 µg/mL                 | +/- 5.2012                             |
| 16            | n-Hexatriacontane (C36)  | 630-06-8   | Z27H018    | 99%    | 201.7 µg/mL                 | +/- 5.2098                             |
| 17            | n-Octatriacontane (C38)  | 7194-85-6  | 0000207852 | 96%    | 201.6 µg/mL                 | +/- 5.2081                             |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane  
**CAS #** 109-66-0  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
2 ml/min.

**Inj. Vol**  
1µl

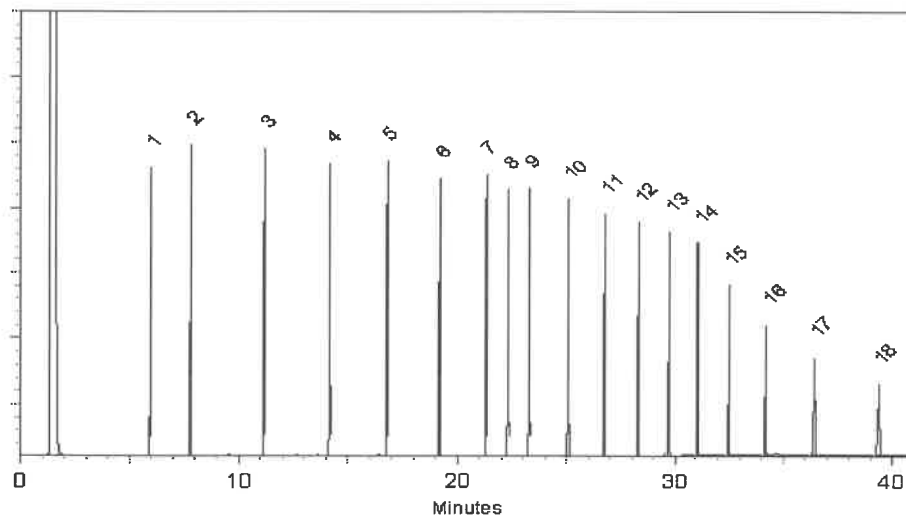

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Brandon Reish*  
Brandon Reish - Operations Technician III

**Date Mixed:** 23-Dec-2024 **Balance Serial #** C322230531

*Dillan Murphy*  
Dillan Murphy - Operations Technician I

**Date Passed:** 27-Dec-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 30543

Lot No.: A0220580

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL

Pkg Amt: > 5 mL

Expiration Date : November 30, 2030

Storage: 10°C or colder

Handling: Sonication required. Mix is photosensitive.

Ship: Ambient

P13916 } Y.P.  
↓  
P13935 } 08/06/25

### CERTIFIED VALUES

| Elution Order | Compound               | CAS #    | Lot #           | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------|----------|-----------------|--------|-----------------------------|----------------------------------------|
| 1             | 1,2,3-Trimethylbenzene | 526-73-8 | 8776.10-39      | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 2             | Naphthalene            | 91-20-3  | STBL1057        | 99%    | 200.8 µg/mL                 | +/- 9.0474                             |
| 3             | 2-Methylnaphthalene    | 91-57-6  | STBL3028        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 4             | Acenaphthylene         | 208-96-8 | RP241029RSR     | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 5             | Acenaphthene           | 83-32-9  | MKCR7169        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 6             | Fluorene               | 86-73-7  | 10246250        | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 7             | Phenanthrene           | 85-01-8  | MKCT3391        | 99%    | 200.8 µg/mL                 | +/- 9.0474                             |
| 8             | Anthracene             | 120-12-7 | MKCW9141        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 9             | Fluoranthene           | 206-44-0 | MKCQ4728        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 10            | Pyrene                 | 129-00-0 | BCCL8032        | 99%    | 201.6 µg/mL                 | +/- 9.0835                             |
| 11            | Benz(a)anthracene      | 56-55-3  | I220012022BAA   | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 12            | Chrysene               | 218-01-9 | RP240719RSR     | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 13            | Benzo(b)fluoranthene   | 205-99-2 | SBS-BBF-FINAL-2 | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 14            | Benzo(k)fluoranthene   | 207-08-9 | 012022K         | 98%    | 201.5 µg/mL                 | +/- 9.0784                             |
| 15            | Benzo(a)pyrene         | 50-32-8  | NQLXA           | 98%    | 200.7 µg/mL                 | +/- 9.0431                             |
| 16            | Indeno(1,2,3-cd)pyrene | 193-39-5 | 12-JKL-118-9    | 97%    | 200.6 µg/mL                 | +/- 9.0383                             |

|    |                       |          |             |     |             |            |
|----|-----------------------|----------|-------------|-----|-------------|------------|
| 17 | Dibenz(a,h)anthracene | 53-70-3  | 2-ASA-59-1  | 99% | 201.2 µg/mL | +/- 9.0655 |
| 18 | Benzo(g,h,i)perylene  | 191-24-2 | RP241014RSR | 98% | 200.3 µg/mL | +/- 9.0255 |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

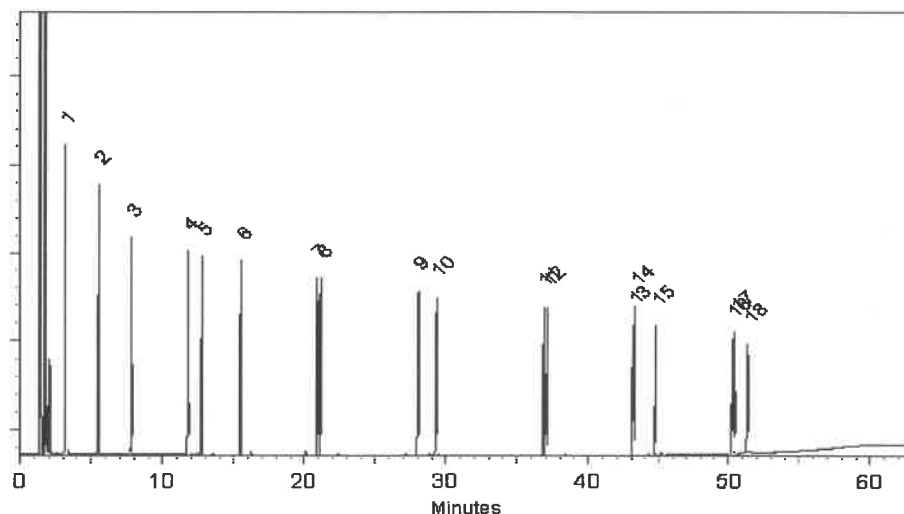

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*VenKelley*  
**Ven Kelley - Operations Tech I**

**Date Mixed:** 30-Dec-2024 **Balance Serial #** 1128360905

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 03-Jan-2025

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543

**Lot No.:** A0220580

**Description :** NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

**Container Size :** 5 mL

**Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2030

**Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive.

**Ship:** Ambient

P13916 } Y.P.  
↓  
P13935 } 08/06/25

### CERTIFIED VALUES

| Elution Order | Compound               | CAS #    | Lot #           | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------|----------|-----------------|--------|-----------------------------|----------------------------------------|
| 1             | 1,2,3-Trimethylbenzene | 526-73-8 | 8776.10-39      | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 2             | Naphthalene            | 91-20-3  | STBL1057        | 99%    | 200.8 µg/mL                 | +/- 9.0474                             |
| 3             | 2-Methylnaphthalene    | 91-57-6  | STBL3028        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 4             | Acenaphthylene         | 208-96-8 | RP241029RSR     | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 5             | Acenaphthene           | 83-32-9  | MKCR7169        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 6             | Fluorene               | 86-73-7  | 10246250        | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 7             | Phenanthrene           | 85-01-8  | MKCT3391        | 99%    | 200.8 µg/mL                 | +/- 9.0474                             |
| 8             | Anthracene             | 120-12-7 | MKCW9141        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 9             | Fluoranthene           | 206-44-0 | MKCQ4728        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 10            | Pyrene                 | 129-00-0 | BCCL8032        | 99%    | 201.6 µg/mL                 | +/- 9.0835                             |
| 11            | Benz(a)anthracene      | 56-55-3  | I220012022BAA   | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 12            | Chrysene               | 218-01-9 | RP240719RSR     | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 13            | Benzo(b)fluoranthene   | 205-99-2 | SBS-BBF-FINAL-2 | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 14            | Benzo(k)fluoranthene   | 207-08-9 | 012022K         | 98%    | 201.5 µg/mL                 | +/- 9.0784                             |
| 15            | Benzo(a)pyrene         | 50-32-8  | NQLXA           | 98%    | 200.7 µg/mL                 | +/- 9.0431                             |
| 16            | Indeno(1,2,3-cd)pyrene | 193-39-5 | 12-JKL-118-9    | 97%    | 200.6 µg/mL                 | +/- 9.0383                             |

|    |                       |          |             |     |             |            |
|----|-----------------------|----------|-------------|-----|-------------|------------|
| 17 | Dibenz(a,h)anthracene | 53-70-3  | 2-ASA-59-1  | 99% | 201.2 µg/mL | +/- 9.0655 |
| 18 | Benzo(g,h,i)perylene  | 191-24-2 | RP241014RSR | 98% | 200.3 µg/mL | +/- 9.0255 |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

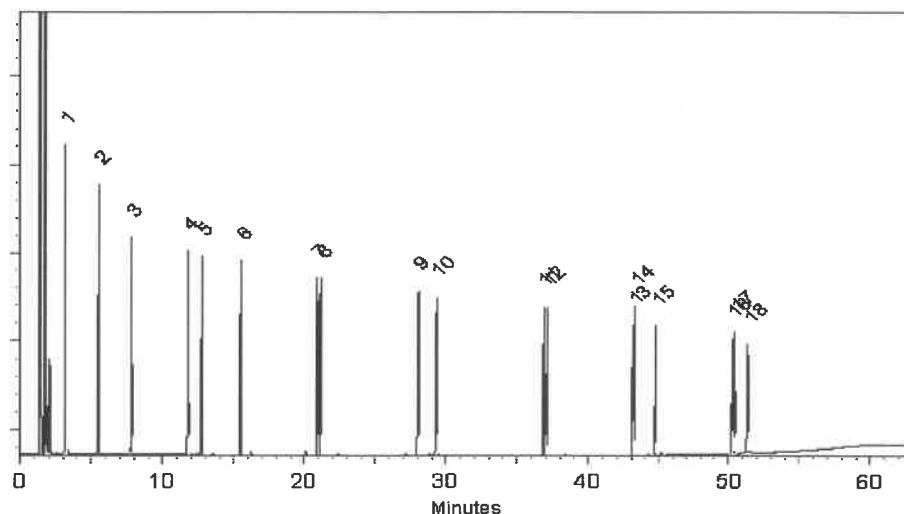

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*VenKelley*  
**Ven Kelley - Operations Tech I**

**Date Mixed:** 30-Dec-2024 **Balance Serial #** 1128360905

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 03-Jan-2025

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543

**Lot No.:** A0220580

**Description :** NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

**Container Size :** 5 mL

**Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2030

**Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive.

**Ship:** Ambient

P13916 } Y.P.  
↓  
P13935 } 08/06/25

### CERTIFIED VALUES

| Elution Order | Compound               | CAS #    | Lot #           | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------|----------|-----------------|--------|-----------------------------|----------------------------------------|
| 1             | 1,2,3-Trimethylbenzene | 526-73-8 | 8776.10-39      | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 2             | Naphthalene            | 91-20-3  | STBL1057        | 99%    | 200.8 µg/mL                 | +/- 9.0474                             |
| 3             | 2-Methylnaphthalene    | 91-57-6  | STBL3028        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 4             | Acenaphthylene         | 208-96-8 | RP241029RSR     | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 5             | Acenaphthene           | 83-32-9  | MKCR7169        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 6             | Fluorene               | 86-73-7  | 10246250        | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 7             | Phenanthrene           | 85-01-8  | MKCT3391        | 99%    | 200.8 µg/mL                 | +/- 9.0474                             |
| 8             | Anthracene             | 120-12-7 | MKCW9141        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 9             | Fluoranthene           | 206-44-0 | MKCQ4728        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 10            | Pyrene                 | 129-00-0 | BCCL8032        | 99%    | 201.6 µg/mL                 | +/- 9.0835                             |
| 11            | Benz(a)anthracene      | 56-55-3  | I220012022BAA   | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 12            | Chrysene               | 218-01-9 | RP240719RSR     | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 13            | Benzo(b)fluoranthene   | 205-99-2 | SBS-BBF-FINAL-2 | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 14            | Benzo(k)fluoranthene   | 207-08-9 | 012022K         | 98%    | 201.5 µg/mL                 | +/- 9.0784                             |
| 15            | Benzo(a)pyrene         | 50-32-8  | NQLXA           | 98%    | 200.7 µg/mL                 | +/- 9.0431                             |
| 16            | Indeno(1,2,3-cd)pyrene | 193-39-5 | 12-JKL-118-9    | 97%    | 200.6 µg/mL                 | +/- 9.0383                             |

|    |                       |          |             |     |             |            |
|----|-----------------------|----------|-------------|-----|-------------|------------|
| 17 | Dibenz(a,h)anthracene | 53-70-3  | 2-ASA-59-1  | 99% | 201.2 µg/mL | +/- 9.0655 |
| 18 | Benzo(g,h,i)perylene  | 191-24-2 | RP241014RSR | 98% | 200.3 µg/mL | +/- 9.0255 |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

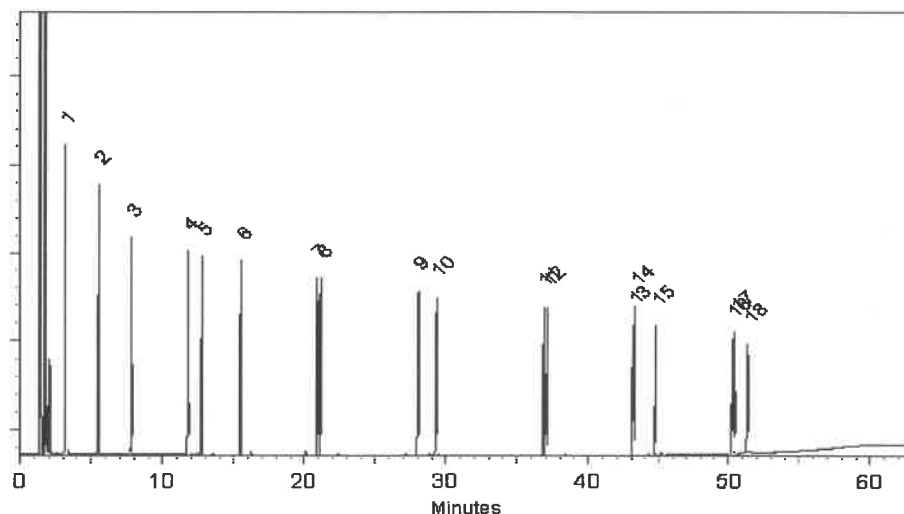

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*VenKelley*  
**Ven Kelley - Operations Tech I**

**Date Mixed:** 30-Dec-2024 **Balance Serial #** 1128360905

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 03-Jan-2025

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543

**Lot No.:** A0220580

**Description :** NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

**Container Size :** 5 mL

**Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2030

**Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive.

**Ship:** Ambient

P13916 } Y.P.  
↓  
P13935 } 08/06/25

### CERTIFIED VALUES

| Elution Order | Compound               | CAS #    | Lot #           | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------|----------|-----------------|--------|-----------------------------|----------------------------------------|
| 1             | 1,2,3-Trimethylbenzene | 526-73-8 | 8776.10-39      | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 2             | Naphthalene            | 91-20-3  | STBL1057        | 99%    | 200.8 µg/mL                 | +/- 9.0474                             |
| 3             | 2-Methylnaphthalene    | 91-57-6  | STBL3028        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 4             | Acenaphthylene         | 208-96-8 | RP241029RSR     | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 5             | Acenaphthene           | 83-32-9  | MKCR7169        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 6             | Fluorene               | 86-73-7  | 10246250        | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 7             | Phenanthrene           | 85-01-8  | MKCT3391        | 99%    | 200.8 µg/mL                 | +/- 9.0474                             |
| 8             | Anthracene             | 120-12-7 | MKCW9141        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 9             | Fluoranthene           | 206-44-0 | MKCQ4728        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 10            | Pyrene                 | 129-00-0 | BCCL8032        | 99%    | 201.6 µg/mL                 | +/- 9.0835                             |
| 11            | Benz(a)anthracene      | 56-55-3  | I220012022BAA   | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 12            | Chrysene               | 218-01-9 | RP240719RSR     | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 13            | Benzo(b)fluoranthene   | 205-99-2 | SBS-BBF-FINAL-2 | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 14            | Benzo(k)fluoranthene   | 207-08-9 | 012022K         | 98%    | 201.5 µg/mL                 | +/- 9.0784                             |
| 15            | Benzo(a)pyrene         | 50-32-8  | NQLXA           | 98%    | 200.7 µg/mL                 | +/- 9.0431                             |
| 16            | Indeno(1,2,3-cd)pyrene | 193-39-5 | 12-JKL-118-9    | 97%    | 200.6 µg/mL                 | +/- 9.0383                             |

|    |                       |          |             |     |             |            |
|----|-----------------------|----------|-------------|-----|-------------|------------|
| 17 | Dibenz(a,h)anthracene | 53-70-3  | 2-ASA-59-1  | 99% | 201.2 µg/mL | +/- 9.0655 |
| 18 | Benzo(g,h,i)perylene  | 191-24-2 | RP241014RSR | 98% | 200.3 µg/mL | +/- 9.0255 |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

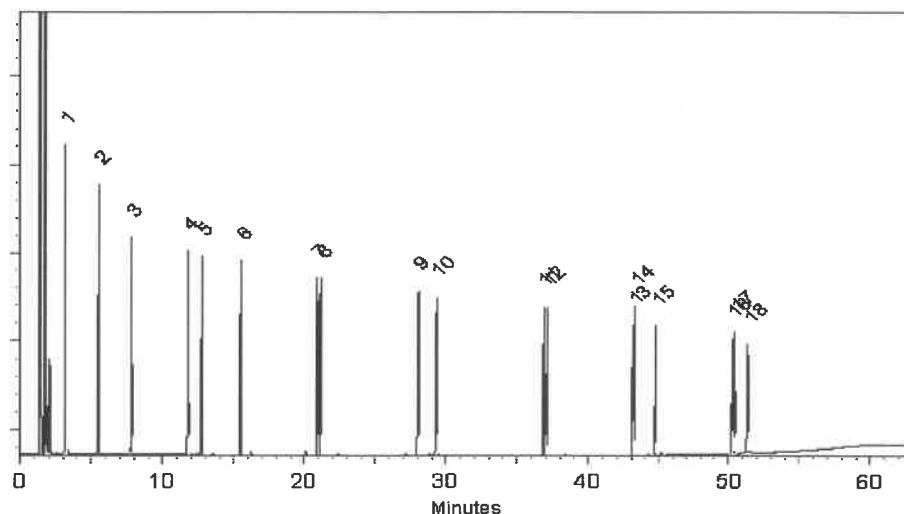

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*VenKelley*  
**Ven Kelley - Operations Tech I**

**Date Mixed:** 30-Dec-2024 **Balance Serial #** 1128360905

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 03-Jan-2025

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543

**Lot No.:** A0220580

**Description :** NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

**Container Size :** 5 mL

**Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2030

**Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive.

**Ship:** Ambient

P13916 } Y.P.  
↓  
P13935 } 08/06/25

### CERTIFIED VALUES

| Elution Order | Compound               | CAS #    | Lot #           | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------|----------|-----------------|--------|-----------------------------|----------------------------------------|
| 1             | 1,2,3-Trimethylbenzene | 526-73-8 | 8776.10-39      | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 2             | Naphthalene            | 91-20-3  | STBL1057        | 99%    | 200.8 µg/mL                 | +/- 9.0474                             |
| 3             | 2-Methylnaphthalene    | 91-57-6  | STBL3028        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 4             | Acenaphthylene         | 208-96-8 | RP241029RSR     | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 5             | Acenaphthene           | 83-32-9  | MKCR7169        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 6             | Fluorene               | 86-73-7  | 10246250        | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 7             | Phenanthrene           | 85-01-8  | MKCT3391        | 99%    | 200.8 µg/mL                 | +/- 9.0474                             |
| 8             | Anthracene             | 120-12-7 | MKCW9141        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 9             | Fluoranthene           | 206-44-0 | MKCQ4728        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 10            | Pyrene                 | 129-00-0 | BCCL8032        | 99%    | 201.6 µg/mL                 | +/- 9.0835                             |
| 11            | Benz(a)anthracene      | 56-55-3  | I220012022BAA   | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 12            | Chrysene               | 218-01-9 | RP240719RSR     | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 13            | Benzo(b)fluoranthene   | 205-99-2 | SBS-BBF-FINAL-2 | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 14            | Benzo(k)fluoranthene   | 207-08-9 | 012022K         | 98%    | 201.5 µg/mL                 | +/- 9.0784                             |
| 15            | Benzo(a)pyrene         | 50-32-8  | NQLXA           | 98%    | 200.7 µg/mL                 | +/- 9.0431                             |
| 16            | Indeno(1,2,3-cd)pyrene | 193-39-5 | 12-JKL-118-9    | 97%    | 200.6 µg/mL                 | +/- 9.0383                             |

|    |                       |          |             |     |             |            |
|----|-----------------------|----------|-------------|-----|-------------|------------|
| 17 | Dibenz(a,h)anthracene | 53-70-3  | 2-ASA-59-1  | 99% | 201.2 µg/mL | +/- 9.0655 |
| 18 | Benzo(g,h,i)perylene  | 191-24-2 | RP241014RSR | 98% | 200.3 µg/mL | +/- 9.0255 |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

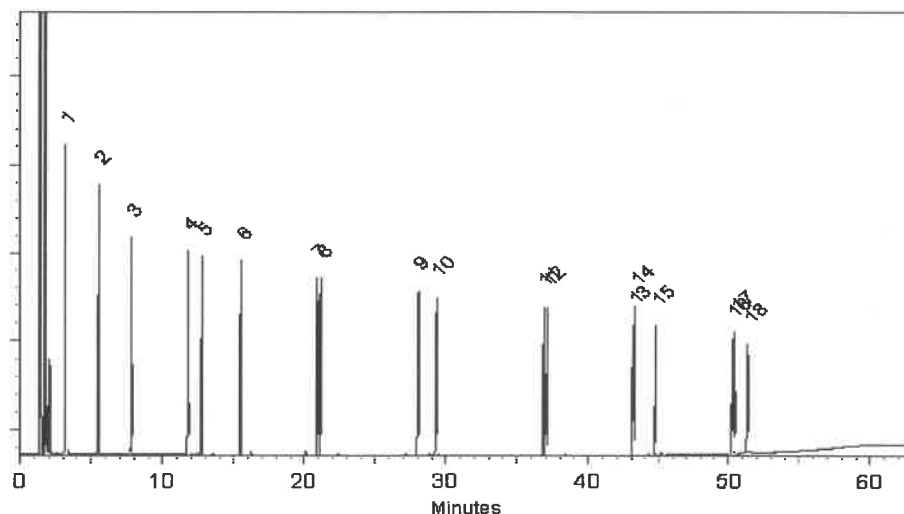

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*VenKelley*  
**Ven Kelley - Operations Tech I**

**Date Mixed:** 30-Dec-2024 **Balance Serial #** 1128360905

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 03-Jan-2025

**Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397**

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543

**Lot No.:** A0220580

**Description :** NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

**Container Size :** 5 mL

**Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2030

**Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive.

**Ship:** Ambient

P13916 } Y.P.  
↓  
P13935 } 08/06/25

### CERTIFIED VALUES

| Elution Order | Compound               | CAS #    | Lot #           | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------|----------|-----------------|--------|-----------------------------|----------------------------------------|
| 1             | 1,2,3-Trimethylbenzene | 526-73-8 | 8776.10-39      | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 2             | Naphthalene            | 91-20-3  | STBL1057        | 99%    | 200.8 µg/mL                 | +/- 9.0474                             |
| 3             | 2-Methylnaphthalene    | 91-57-6  | STBL3028        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 4             | Acenaphthylene         | 208-96-8 | RP241029RSR     | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 5             | Acenaphthene           | 83-32-9  | MKCR7169        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 6             | Fluorene               | 86-73-7  | 10246250        | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 7             | Phenanthrene           | 85-01-8  | MKCT3391        | 99%    | 200.8 µg/mL                 | +/- 9.0474                             |
| 8             | Anthracene             | 120-12-7 | MKCW9141        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 9             | Fluoranthene           | 206-44-0 | MKCQ4728        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 10            | Pyrene                 | 129-00-0 | BCCL8032        | 99%    | 201.6 µg/mL                 | +/- 9.0835                             |
| 11            | Benz(a)anthracene      | 56-55-3  | I220012022BAA   | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 12            | Chrysene               | 218-01-9 | RP240719RSR     | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 13            | Benzo(b)fluoranthene   | 205-99-2 | SBS-BBF-FINAL-2 | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 14            | Benzo(k)fluoranthene   | 207-08-9 | 012022K         | 98%    | 201.5 µg/mL                 | +/- 9.0784                             |
| 15            | Benzo(a)pyrene         | 50-32-8  | NQLXA           | 98%    | 200.7 µg/mL                 | +/- 9.0431                             |
| 16            | Indeno(1,2,3-cd)pyrene | 193-39-5 | 12-JKL-118-9    | 97%    | 200.6 µg/mL                 | +/- 9.0383                             |

|    |                       |          |             |     |             |            |
|----|-----------------------|----------|-------------|-----|-------------|------------|
| 17 | Dibenz(a,h)anthracene | 53-70-3  | 2-ASA-59-1  | 99% | 201.2 µg/mL | +/- 9.0655 |
| 18 | Benzo(g,h,i)perylene  | 191-24-2 | RP241014RSR | 98% | 200.3 µg/mL | +/- 9.0255 |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

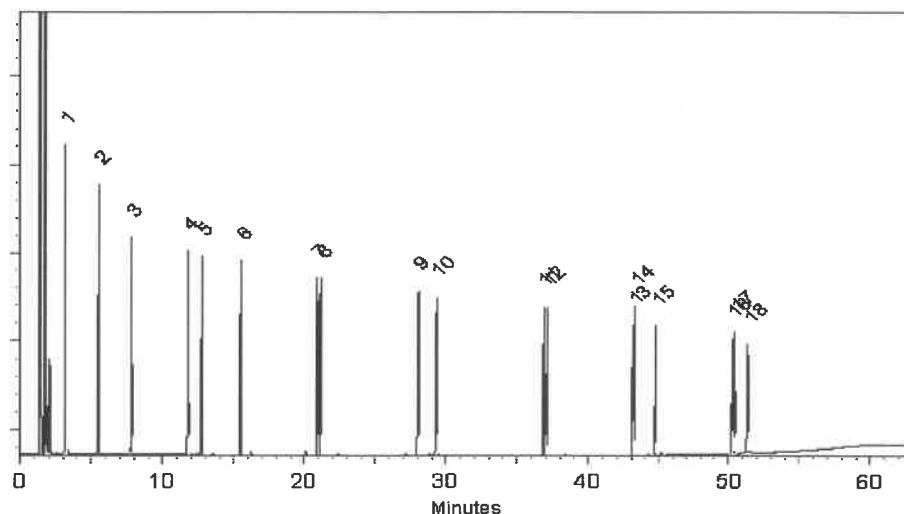

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*VenKelley*  
**Ven Kelley - Operations Tech I**

**Date Mixed:** 30-Dec-2024 **Balance Serial #** 1128360905

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 03-Jan-2025

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543

**Lot No.:** A0220580

**Description :** NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

**Container Size :** 5 mL

**Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2030

**Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive.

**Ship:** Ambient

P13916 } Y.P.  
↓  
P13935 } 08/06/25

### CERTIFIED VALUES

| Elution Order | Compound               | CAS #    | Lot #           | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------|----------|-----------------|--------|-----------------------------|----------------------------------------|
| 1             | 1,2,3-Trimethylbenzene | 526-73-8 | 8776.10-39      | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 2             | Naphthalene            | 91-20-3  | STBL1057        | 99%    | 200.8 µg/mL                 | +/- 9.0474                             |
| 3             | 2-Methylnaphthalene    | 91-57-6  | STBL3028        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 4             | Acenaphthylene         | 208-96-8 | RP241029RSR     | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 5             | Acenaphthene           | 83-32-9  | MKCR7169        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 6             | Fluorene               | 86-73-7  | 10246250        | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 7             | Phenanthrene           | 85-01-8  | MKCT3391        | 99%    | 200.8 µg/mL                 | +/- 9.0474                             |
| 8             | Anthracene             | 120-12-7 | MKCW9141        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 9             | Fluoranthene           | 206-44-0 | MKCQ4728        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 10            | Pyrene                 | 129-00-0 | BCCL8032        | 99%    | 201.6 µg/mL                 | +/- 9.0835                             |
| 11            | Benz(a)anthracene      | 56-55-3  | I220012022BAA   | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 12            | Chrysene               | 218-01-9 | RP240719RSR     | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 13            | Benzo(b)fluoranthene   | 205-99-2 | SBS-BBF-FINAL-2 | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 14            | Benzo(k)fluoranthene   | 207-08-9 | 012022K         | 98%    | 201.5 µg/mL                 | +/- 9.0784                             |
| 15            | Benzo(a)pyrene         | 50-32-8  | NQLXA           | 98%    | 200.7 µg/mL                 | +/- 9.0431                             |
| 16            | Indeno(1,2,3-cd)pyrene | 193-39-5 | 12-JKL-118-9    | 97%    | 200.6 µg/mL                 | +/- 9.0383                             |

|    |                       |          |             |     |             |            |
|----|-----------------------|----------|-------------|-----|-------------|------------|
| 17 | Dibenz(a,h)anthracene | 53-70-3  | 2-ASA-59-1  | 99% | 201.2 µg/mL | +/- 9.0655 |
| 18 | Benzo(g,h,i)perylene  | 191-24-2 | RP241014RSR | 98% | 200.3 µg/mL | +/- 9.0255 |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

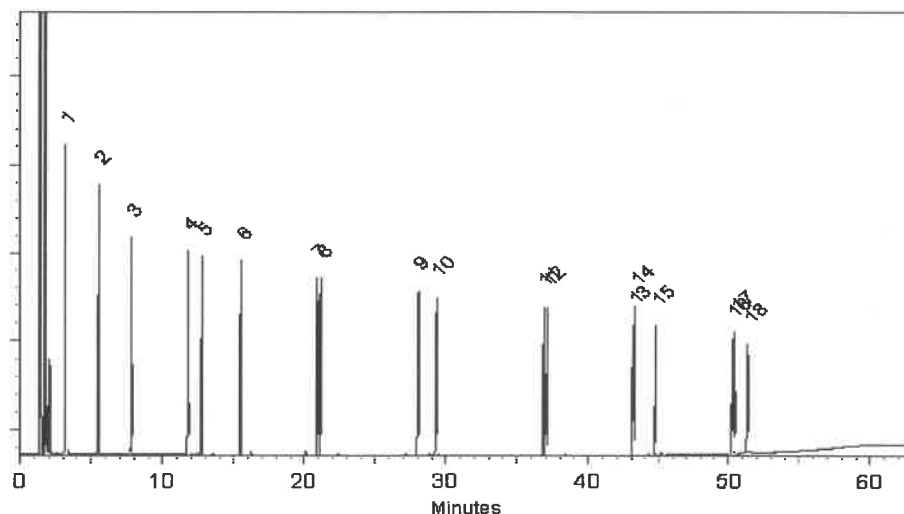

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*VenKelley*  
**Ven Kelley - Operations Tech I**

**Date Mixed:** 30-Dec-2024 **Balance Serial #** 1128360905

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 03-Jan-2025

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543

**Lot No.:** A0220580

**Description :** NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

**Container Size :** 5 mL

**Pkg Amt:** > 5 mL

**Expiration Date :** November 30, 2030

**Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive.

**Ship:** Ambient

P13916 } Y.P.  
↓  
P13935 } 08/06/25

### CERTIFIED VALUES

| Elution Order | Compound               | CAS #    | Lot #           | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------|----------|-----------------|--------|-----------------------------|----------------------------------------|
| 1             | 1,2,3-Trimethylbenzene | 526-73-8 | 8776.10-39      | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 2             | Naphthalene            | 91-20-3  | STBL1057        | 99%    | 200.8 µg/mL                 | +/- 9.0474                             |
| 3             | 2-Methylnaphthalene    | 91-57-6  | STBL3028        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 4             | Acenaphthylene         | 208-96-8 | RP241029RSR     | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 5             | Acenaphthene           | 83-32-9  | MKCR7169        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 6             | Fluorene               | 86-73-7  | 10246250        | 98%    | 201.9 µg/mL                 | +/- 9.0961                             |
| 7             | Phenanthrene           | 85-01-8  | MKCT3391        | 99%    | 200.8 µg/mL                 | +/- 9.0474                             |
| 8             | Anthracene             | 120-12-7 | MKCW9141        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 9             | Fluoranthene           | 206-44-0 | MKCQ4728        | 99%    | 200.4 µg/mL                 | +/- 9.0294                             |
| 10            | Pyrene                 | 129-00-0 | BCCL8032        | 99%    | 201.6 µg/mL                 | +/- 9.0835                             |
| 11            | Benz(a)anthracene      | 56-55-3  | I220012022BAA   | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 12            | Chrysene               | 218-01-9 | RP240719RSR     | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 13            | Benzo(b)fluoranthene   | 205-99-2 | SBS-BBF-FINAL-2 | 99%    | 202.0 µg/mL                 | +/- 9.1015                             |
| 14            | Benzo(k)fluoranthene   | 207-08-9 | 012022K         | 98%    | 201.5 µg/mL                 | +/- 9.0784                             |
| 15            | Benzo(a)pyrene         | 50-32-8  | NQLXA           | 98%    | 200.7 µg/mL                 | +/- 9.0431                             |
| 16            | Indeno(1,2,3-cd)pyrene | 193-39-5 | 12-JKL-118-9    | 97%    | 200.6 µg/mL                 | +/- 9.0383                             |

|    |                       |          |             |     |             |            |
|----|-----------------------|----------|-------------|-----|-------------|------------|
| 17 | Dibenz(a,h)anthracene | 53-70-3  | 2-ASA-59-1  | 99% | 201.2 µg/mL | +/- 9.0655 |
| 18 | Benzo(g,h,i)perylene  | 191-24-2 | RP241014RSR | 98% | 200.3 µg/mL | +/- 9.0255 |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

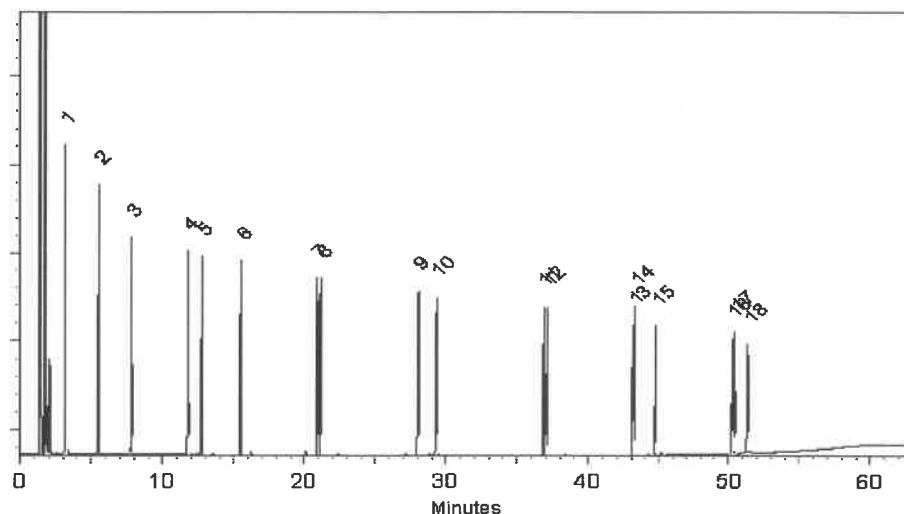

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*VenKelley*  
**Ven Kelley - Operations Tech I**

**Date Mixed:** 30-Dec-2024 **Balance Serial #** 1128360905

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 03-Jan-2025

**Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397**

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31480 **Lot No.:** A0219106  
**Description :** MA Fractionation Surrogate Spike Mix  
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** October 31, 2030 **Storage:** 10°C or colder  
**Handling:** Sonication required. Mix is **Ship:** Ambient  
photosensitive.

p13947  
L  
p1395h

### CERTIFIED VALUES

| Elution Order | Compound           | CAS #    | Lot #     | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------|----------|-----------|--------|-----------------------------|----------------------------------------|
| 1             | 2-Fluorobiphenyl   | 321-60-8 | 00021384  | 99%    | 4,013.5 µg/mL               | +/- 180.7988                           |
| 2             | 2-Bromonaphthalene | 580-13-2 | STBC5362V | 99%    | 4,011.0 µg/mL               | +/- 180.6862                           |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-S (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

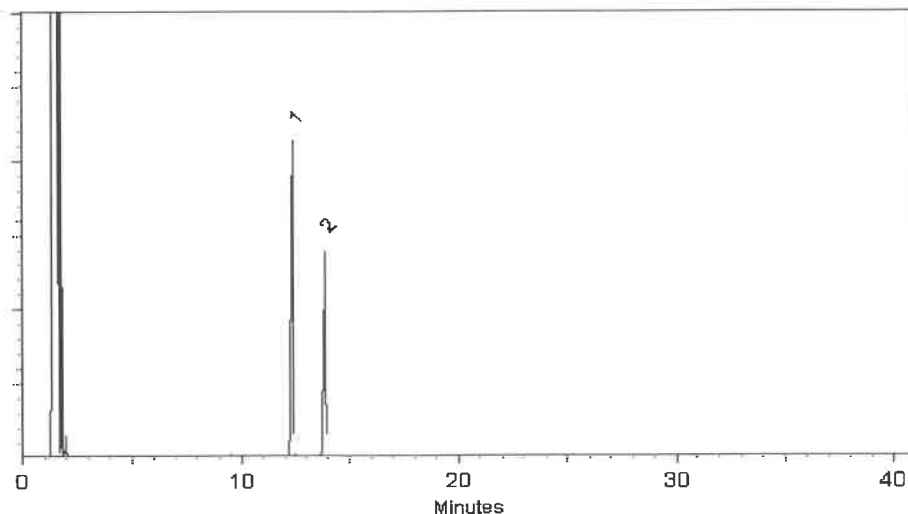

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Wilner Torres*  
Wilner Torres - Operation Tech I

Date Mixed: 14-Nov-2024

Balance Serial # 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 20-Nov-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31480 **Lot No.:** A0219106  
**Description :** MA Fractionation Surrogate Spike Mix  
MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** October 31, 2030 **Storage:** 10°C or colder  
**Handling:** Sonication required. Mix is **Ship:** Ambient  
photosensitive.

P13947  
L  
P13954

### CERTIFIED VALUES

| Elution Order | Compound           | CAS #    | Lot #     | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------|----------|-----------|--------|-----------------------------|----------------------------------------|
| 1             | 2-Fluorobiphenyl   | 321-60-8 | 00021384  | 99%    | 4,013.5 µg/mL               | +/- 180.7988                           |
| 2             | 2-Bromonaphthalene | 580-13-2 | STBC5362V | 99%    | 4,011.0 µg/mL               | +/- 180.6862                           |

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-S (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

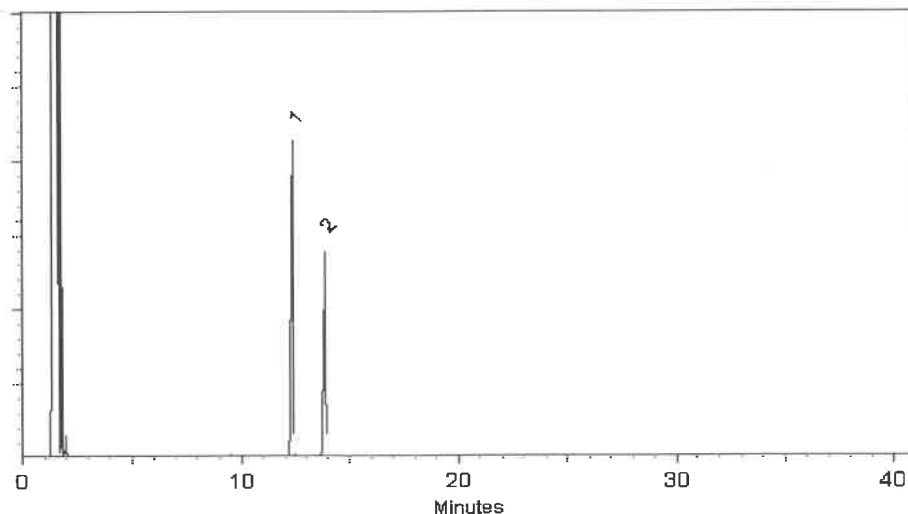

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Wilner Torres*  
Wilner Torres - Operation Tech I

Date Mixed: 14-Nov-2024

Balance Serial # 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 20-Nov-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



n-Hexane 95%  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis



Material No.: 9262-03  
Batch No.: 24G1962003  
Manufactured Date: 2024-05-23  
Expiration Date: 2025-08-22  
Revision No.: 0

## Certificate of Analysis

| Test                                                                            | Specification  | Result      |
|---------------------------------------------------------------------------------|----------------|-------------|
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)            | $\leq 5$       | 3           |
| ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)            | $\leq 10$      | 1           |
| ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL) | $\leq 5$       | 1           |
| Assay (Total Saturated C <sub>6</sub> Isomers) (by GC, corrected for water)     | $\geq 99.5 \%$ | 99.7 %      |
| Assay (as n-Hexane) (by GC, corrected for water)                                | $\geq 95 \%$   | 98 %        |
| Color (APHA)                                                                    | $\leq 10$      | 5           |
| Residue after Evaporation                                                       | $\leq 1.0$ ppm | 0.1 ppm     |
| Substances Darkened by H <sub>2</sub> SO <sub>4</sub>                           | Passes Test    | Passes Test |
| Water (by KF, coulometric)                                                      | $\leq 0.05 \%$ | < 0.01 %    |

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Croak  
Director Quality Operations, Bioscience Production