
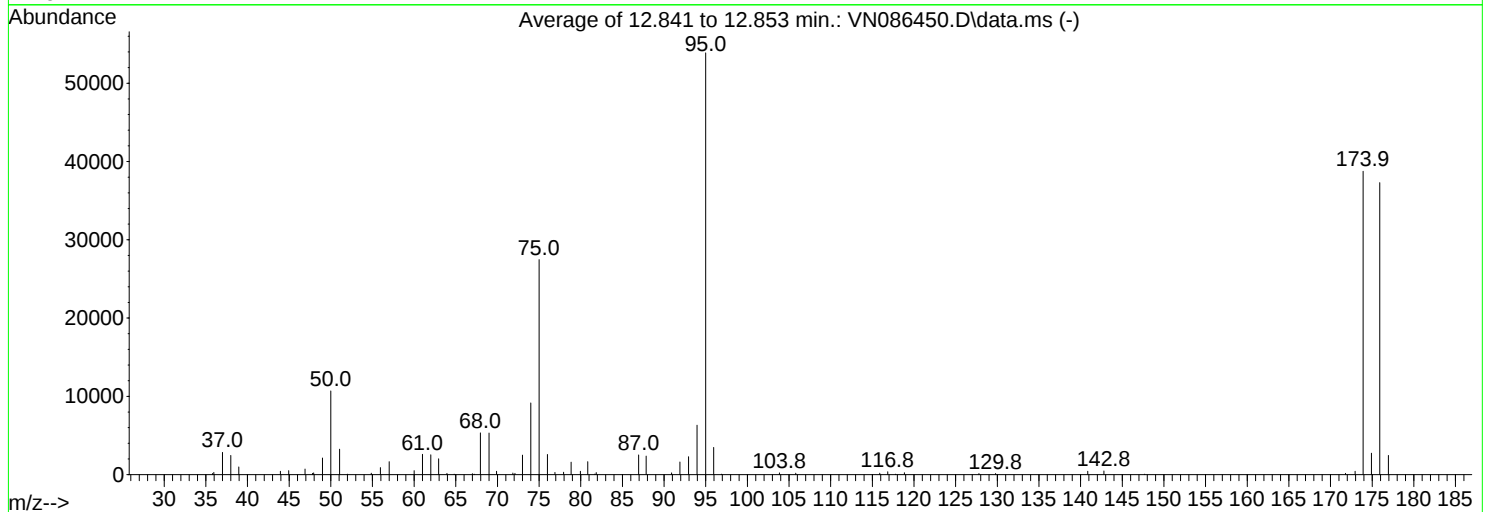


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050225\
Data File : VN086450.D
Acq On : 02 May 2025 08:47
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
Title : SW846 8260
Last Update : Wed Apr 16 04:19:23 2025

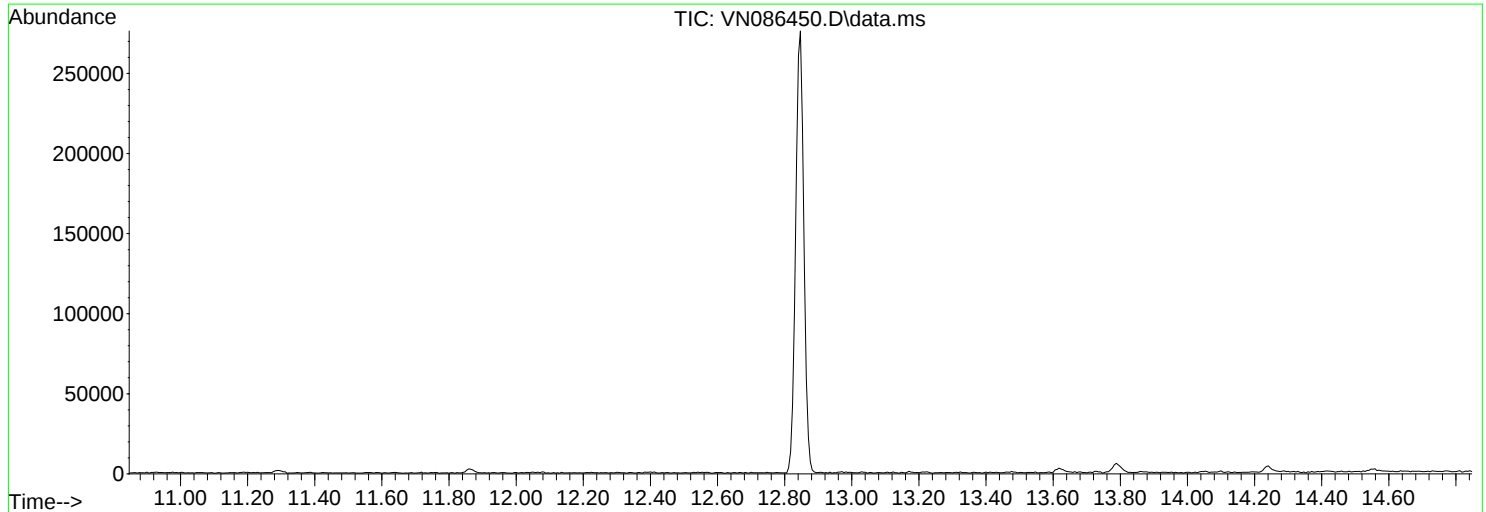

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	10692	PASS
75	95	30	60	51.0	27472	PASS
95	95	100	100	100.0	53880	PASS
96	95	5	9	6.5	3485	PASS
173	174	0.00	2	1.1	430	PASS
174	95	50	100	71.9	38757	PASS
175	174	5	9	7.1	2734	PASS
176	174	95	101	96.3	37307	PASS
177	176	5	9	6.6	2450	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	144	50.00	10692	64.80	69	76.00	2584
35.95	288	51.05	3261	67.00	125	76.90	270
37.00	2843	52.00	66	67.20	63	77.95	300
38.00	2447	54.85	190	67.95	5336	78.85	1598
38.95	990	55.95	911	69.00	5315	79.95	431
43.95	420	57.00	1646	69.90	435	80.85	1659
44.95	510	60.00	513	71.85	202	81.70	89
46.90	722	61.00	2591	72.10	174	81.85	259
47.80	163	62.00	2545	73.00	2500	86.95	2508
47.95	232	62.95	2032	74.00	9148	87.85	2366
49.00	2134	63.95	164	75.00	27472	90.90	230

Average of 12.841 to 12.853 min.: VN086450.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
91.90	1609	118.85	241	176.95	2450		
92.95	2293	127.80	139				
93.95	6307	129.80	147				
95.00	53880	140.85	433				
95.95	3485	142.80	477				
96.90	70	147.70	56				
103.85	216	171.80	167				
105.80	185	172.95	430				
115.90	183	173.90	38757				
116.85	374	174.90	2734				
117.80	60	175.90	37307				

Instrument :

MSVOA_N

ClientSampleId :

BFB