

DATA REPORTING QUALIFIERS- ORGANIC

For reporting results, the following "Results Qualifiers" are used:

Value	If the result is a value greater than or equal to the detection limit, report the value
U	Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. "10 U". This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
ND	Indicates the analyte was analyzed for, but not detected
J	Indicates an estimated value. This flag is used: (1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.) (2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
B	Indicates the analyte was found in the blank as well as the sample report as "12 B".
E	Indicates the analyte 's concentration exceeds the calibrated range of the instrument for that specific analysis.
D	This flag identifies all compounds identified in an analysis at a secondary dilution factor.
P	This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a "P".
N	This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
A	This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
Q	Indicates the LCS did not meet the control limits requirements

LAB CHRONICLE

OrderID: Q1942
Client: Chemtech Consulting Group
Contact: QA Officer

OrderDate: 5/2/2025 11:11:00 AM
Project: Weekly Storage Blanks
Location: L41,VOA Ref. #3 Water

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q1942-13	PCB-GPC2-BLANK	SOIL	PCB	SFAM_PCB	04/25/25	05/05/25	05/06/25	05/02/25
Q1942-14	PCB-GPC2-BLANK-SPI KE	SOIL	PCB	SFAM_PCB	04/25/25	05/05/25	05/06/25	05/02/25

Hit Summary Sheet
SW-846

SDG No.: Q1942

Order ID: Q1942

Client: Chemtech Consulting Group

Project ID: Weekly Storage Blanks

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	RDL	Units
Client ID : PCB-GPC2-BLANK-SPIKE								
Q1942-14	PCB-GPC2-BLANK-§ SOIL	§ SOIL	Aroclor-1016	360		4.50	100	ug/kg
Q1942-14	PCB-GPC2-BLANK-§ SOIL	§ SOIL	Aroclor-1260	380		4.80	100	ug/kg
Total Concentration:				740.000				



QC SUMMARY

Surrogate Summary

SDG No.: Q1942

Client: Chemtech Consulting Group

Analytical Method: SFAM_PCB

Lab Sample ID	Client ID	Parameter	Column	Spike	Result	Rec	Qual	Limits	
								Low	High
Q1942-13	PCB-GPC2-BLANK	TCX	1	20	0	0	*	30	150
		DCB	1	40	0	0	*	30	150
		TCX	2	20	0	0	*	30	150
		DCB	2	40	0	0	*	30	150
Q1942-14	PCB-GPC2-BLANK-SPIKE	TCX	1	20	0	0	*	30	150
		DCB	1	40	0	0	*	30	150
		TCX	2	20	0	0	*	30	150
		DCB	2	40	0	0	*	30	150

4C

PESTICIDE METHOD BLANK SUMMARY

EPA SAMPLE NO.

Lab Name: CHEMTECH

Contract: CHEM02

Lab Code: CHEM Case No.: Q1942

SAS No.: Q1942 SDG NO.: Q1942

Lab Sample ID: _____

Lab File ID: _____

Matrix: (soil/water) _____

Extraction: (Type) _____

Sulfur Cleanup: (Y/N) _____

Date Extracted: _____

Date Analyzed (1): _____

Date Analyzed (2): _____

Time Analyzed (1): _____

Time Analyzed (2): _____

Instrument ID (1): _____

Instrument ID (2): _____

GC Column (1): _____ ID: _____ (mm)

GC Column (2): _____ ID: _____ (mm)

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED 1	DATE ANALYZED 2

COMMENTS: _____



SAMPLE DATA

Report of Analysis

Client:	Chemtech Consulting Group	Date Collected:	04/25/25
Project:	Weekly Storage Blanks	Date Received:	05/02/25
Client Sample ID:	PCB-GPC2-BLANK	SDG No.:	Q1942
Lab Sample ID:	Q1942-13	Matrix:	SOIL
Analytical Method:	SFAM_PCB	% Solid:	100
Sample Wt/Vol:	10 Units: g	Final Vol:	5000 uL
Soil Aliquot Vol:	uL	Test:	PCB
Extraction Type:		Injection Volume :	
GPC Factor :	2.0	PH :	
Prep Method :			

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PQ070236.D	1	05/05/25 10:42	05/06/25 10:42	PB167862

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	4.50	U	4.50	100	ug/kg
11104-28-2	Aroclor-1221	4.80	U	4.80	100	ug/kg
11141-16-5	Aroclor-1232	4.80	U	4.80	100	ug/kg
53469-21-9	Aroclor-1242	4.80	U	4.80	100	ug/kg
12672-29-6	Aroclor-1248	4.80	U	4.80	100	ug/kg
11097-69-1	Aroclor-1254	4.80	U	4.80	100	ug/kg
11096-82-5	Aroclor-1260	4.80	U	4.80	100	ug/kg
37324-23-5	Aroclor-1262	4.80	U	4.80	100	ug/kg
11100-14-4	Aroclor-1268	4.80	U	4.80	100	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	0	*	30 - 150	%	SPK: 20
2051-24-3	Decachlorobiphenyl	0	*	30 - 150	%	SPK: 40

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ050625\
Data File : PQ070236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2025 10:42
Operator : YP\AJ
Sample : Q1942-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
PCB-GPC2-BLANK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 12:35:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 10 09:58:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ050625\
Data File : PQ070236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2025 10:42
Operator : YP\AJ
Sample : Q1942-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
PCB-GPC2-BLANK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 12:35:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 10 09:58:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

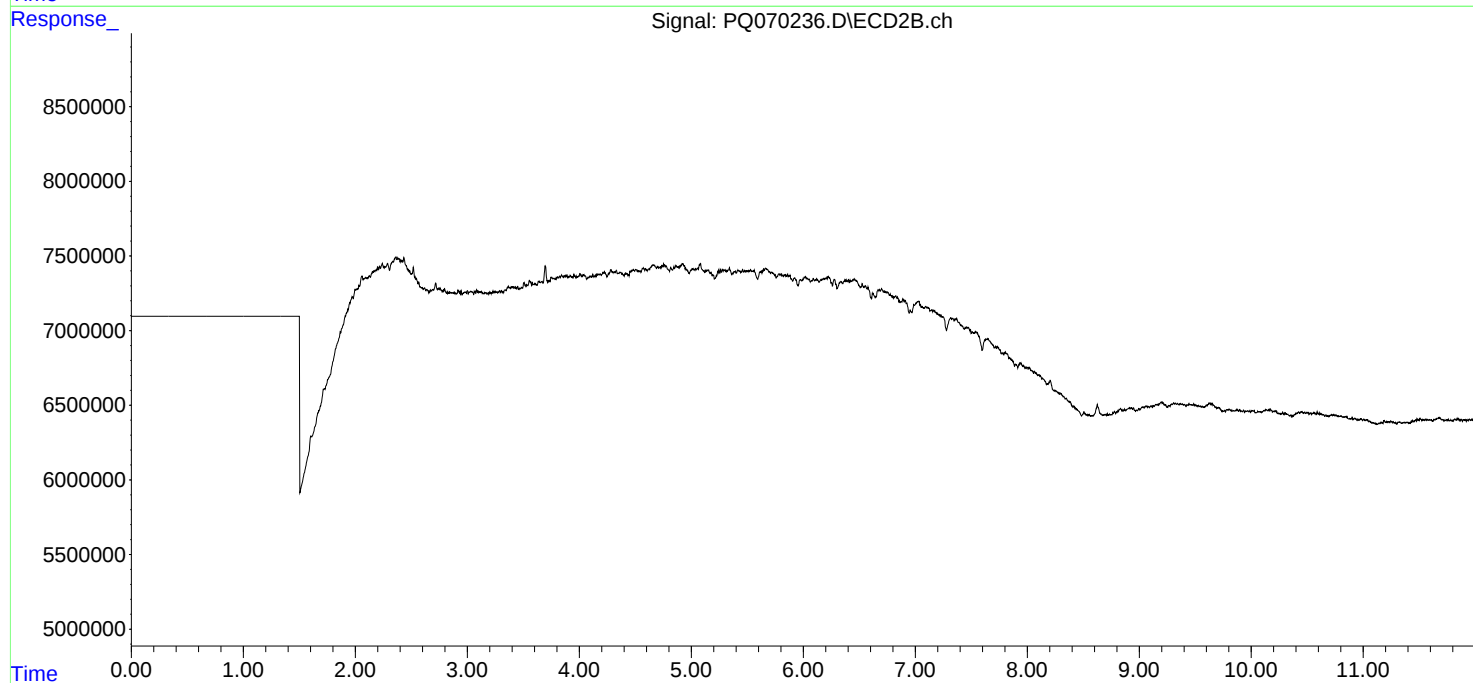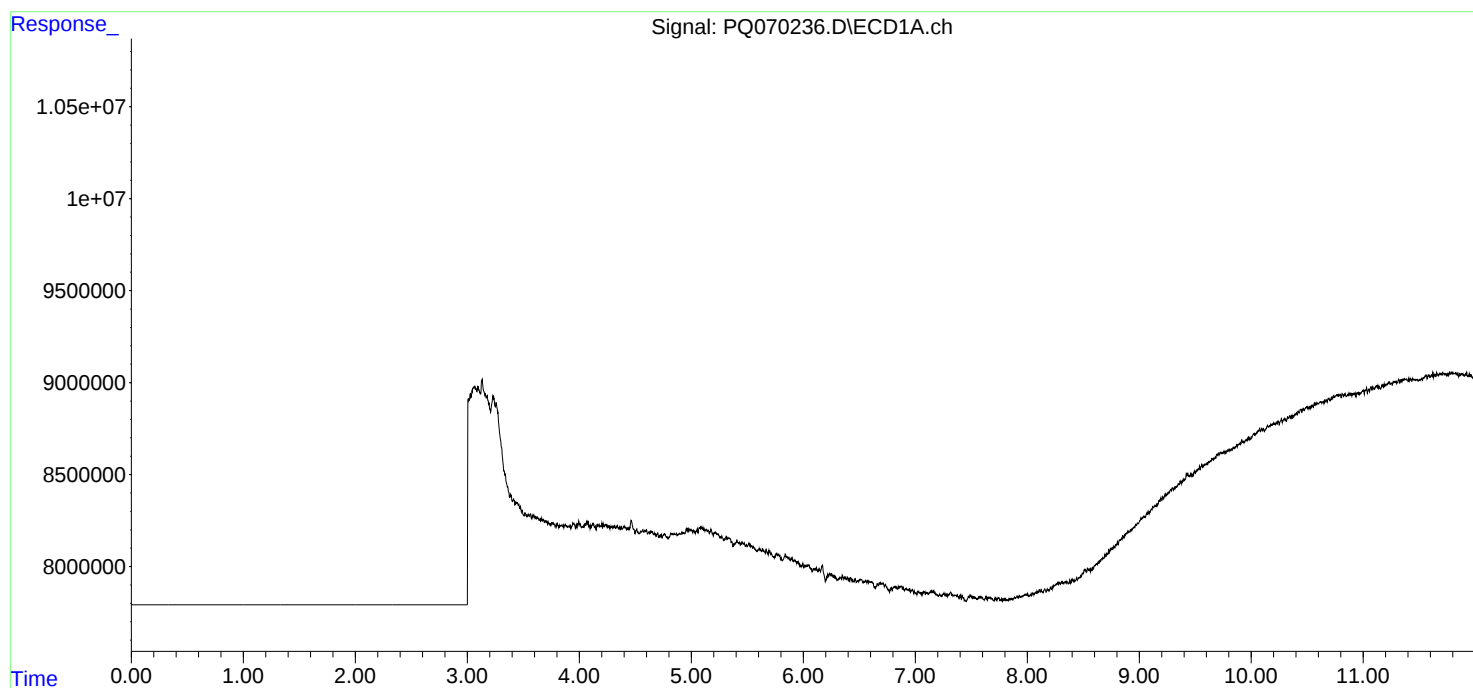

Report of Analysis

Client:	Chemtech Consulting Group	Date Collected:	04/25/25
Project:	Weekly Storage Blanks	Date Received:	05/02/25
Client Sample ID:	PCB-GPC2-BLANK-SPIKE	SDG No.:	Q1942
Lab Sample ID:	Q1942-14	Matrix:	SOIL
Analytical Method:	SFAM_PCB	% Solid:	100
Sample Wt/Vol:	10 Units: g	Final Vol:	5000 uL
Soil Aliquot Vol:	uL	Test:	PCB
Extraction Type:		Injection Volume :	
GPC Factor :	2.0	PH :	
Prep Method :			

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PQ070237.D	1	05/05/25 10:42	05/06/25 10:56	PB167862

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	360		4.50	100	ug/kg
11104-28-2	Aroclor-1221	4.80	U	4.80	100	ug/kg
11141-16-5	Aroclor-1232	4.80	U	4.80	100	ug/kg
53469-21-9	Aroclor-1242	4.80	U	4.80	100	ug/kg
12672-29-6	Aroclor-1248	4.80	U	4.80	100	ug/kg
11097-69-1	Aroclor-1254	4.80	U	4.80	100	ug/kg
11096-82-5	Aroclor-1260	380		4.80	100	ug/kg
37324-23-5	Aroclor-1262	4.80	U	4.80	100	ug/kg
11100-14-4	Aroclor-1268	4.80	U	4.80	100	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	0	*	30 - 150	%	SPK: 20
2051-24-3	Decachlorobiphenyl	0	*	30 - 150	%	SPK: 40

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ050625\
 Data File : PQ070237.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2025 10:56
 Operator : YP\AJ
 Sample : Q1942-14
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 PCB-GCP2-BLANK-SPIKE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 12:35:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 10 09:58:55 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
3)	L1	AR-1016-1	4.486	3.785	74544762	83201818	356.492 377.189
4)	L1	AR-1016-2	4.505	3.801	124.1E6	145.8E6	379.348 437.085
5)	L1	AR-1016-3	4.563	3.961	76878849	69670103	373.394 376.755
6)	L1	AR-1016-4	4.652	4.009	61460457	58866234	364.684 364.297
7)	L1	AR-1016-5	4.936	4.204	56550245	72341860	344.056 369.726
31)	L7	AR-1260-1	6.026	5.197	118.0E6	155.8E6	407.400 439.704
32)	L7	AR-1260-2	6.282	5.387	135.4E6	186.2E6	402.237 436.067
33)	L7	AR-1260-3	6.632	5.528	86451431	174.6E6	336.136 433.952 #
34)	L7	AR-1260-4	6.847	5.988	107.3E6	131.3E6	376.994 372.507
35)	L7	AR-1260-5	7.152	6.233	205.0E6	325.8E6	373.779 408.950



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ050625\
Data File : PQ070237.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2025 10:56
Operator : YP\AJ
Sample : Q1942-14
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
PCB-GCP2-BLANK-SPIKE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 12:35:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 10 09:58:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

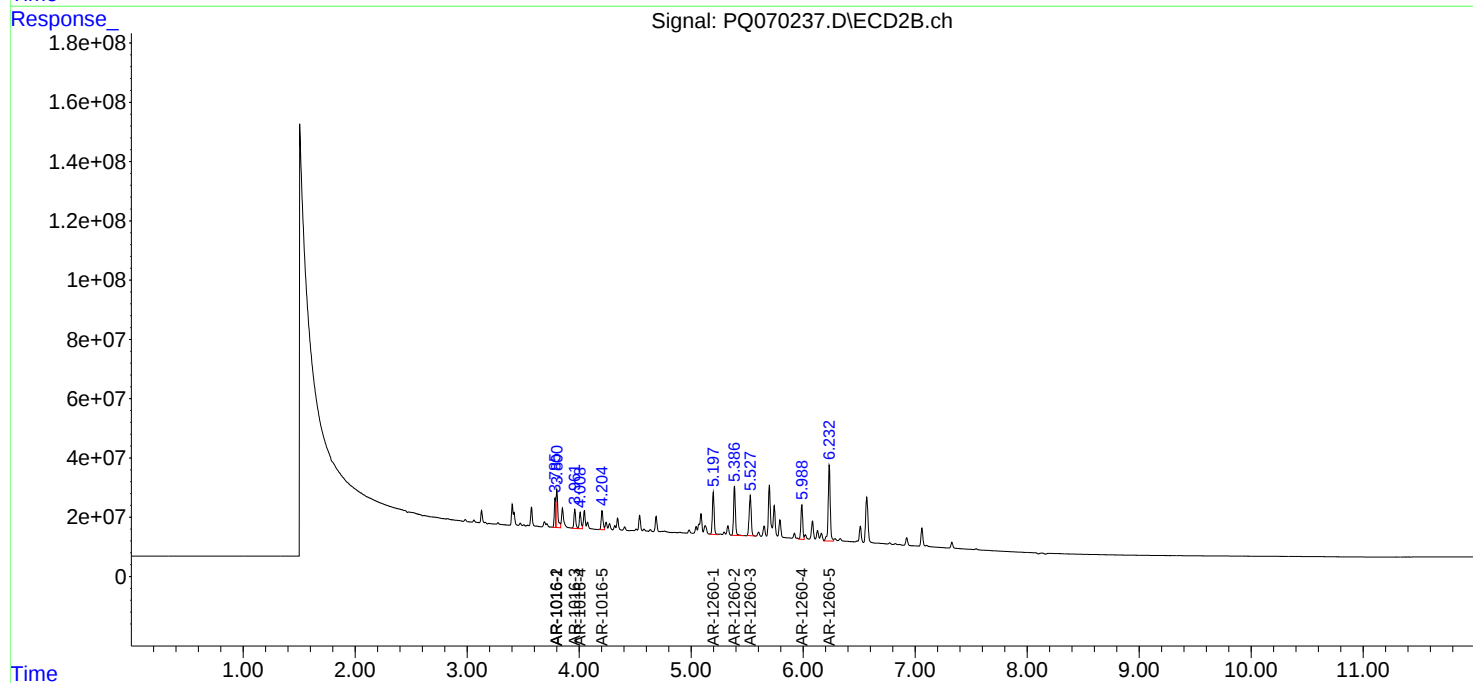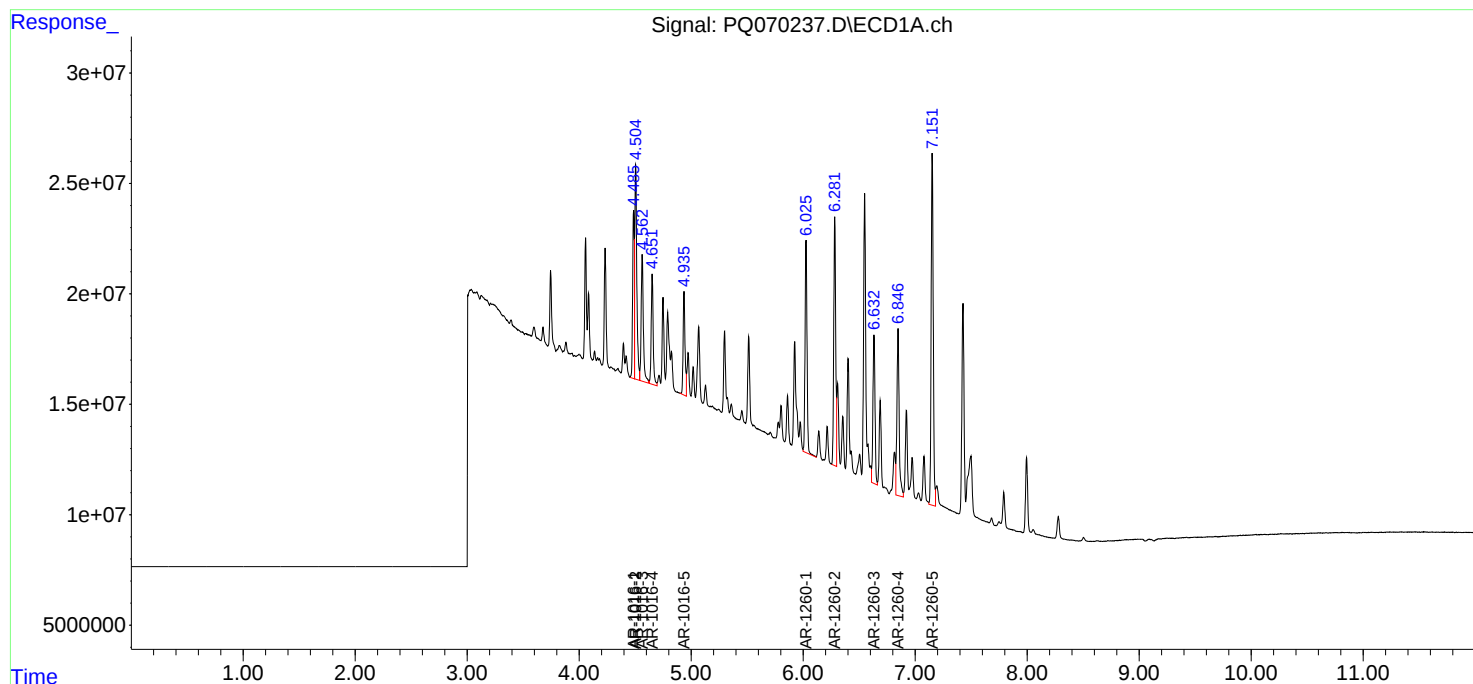



CALIBRATION SUMMARY

RETENTION TIMES OF INITIAL CALIBRATION

Contract: CHEM02

Lab Code: CHEM Case No.: Q1942 SAS No.: Q1942 SDG NO.: Q1942

Instrument ID: ECD_Q Calibration Date(s): 04/09/2025 04/09/2025

Calibration Times: 09:41 19:09

GC Column: ZB-MR1 ID: 0.32 (mm)

LAB FILE ID: RT 100 = PQ070136.D RT 200 = PQ070137.D

RT 400 = PQ070138.D RT 800 = PQ070139.D RT 1600 = PQ070140.D

COMPOUND		RT 100	RT 200	RT 400	RT 800	RT 1600	MEAN RT	RT WINDOW	
								FROM	TO
Aroclor-1016-1	(1)	4.48	4.49	4.48	4.49	4.49	4.49	4.42	4.56
Aroclor-1016-2	(2)	4.50	4.50	4.50	4.50	4.50	4.50	4.43	4.57
Aroclor-1016-3	(3)	4.56	4.56	4.56	4.56	4.56	4.56	4.49	4.63
Aroclor-1016-4	(4)	4.65	4.65	4.65	4.65	4.65	4.65	4.58	4.72
Aroclor-1016-5	(5)	4.94	4.94	4.94	4.94	4.94	4.94	4.87	5.01
Aroclor-1260-1	(1)	6.03	6.03	6.03	6.03	6.03	6.03	5.96	6.10
Aroclor-1260-2	(2)	6.28	6.28	6.28	6.28	6.28	6.28	6.21	6.35
Aroclor-1260-3	(3)	6.63	6.63	6.63	6.63	6.63	6.63	6.56	6.70
Aroclor-1260-4	(4)	6.85	6.85	6.85	6.85	6.85	6.85	6.78	6.92
Aroclor-1260-5	(5)	7.15	7.15	7.15	7.15	7.15	7.15	7.08	7.22
DCB		8.50	8.50	8.50	8.50	8.50	8.50	8.40	8.60
TCX		3.40	3.41	3.40	3.41	3.41	3.41	3.36	3.46
Aroclor-1221-1	(1)	3.60	3.60	3.60	3.60	3.60	3.60	3.53	3.67
Aroclor-1221-2	(2)	3.68	3.68	3.68	3.68	3.68	3.68	3.61	3.75
Aroclor-1221-3	(3)	3.74	3.74	3.74	3.74	3.74	3.74	3.67	3.81
DCB		8.50	8.50	8.50	8.50	8.50	8.50	8.40	8.60
TCX		3.41	3.41	3.40	3.41	3.41	3.41	3.36	3.46
Aroclor-1232-1	(1)	3.74	3.74	3.74	3.74	3.74	3.74	3.67	3.81
Aroclor-1232-2	(2)	4.23	4.23	4.23	4.23	4.23	4.23	4.16	4.30
Aroclor-1232-3	(3)	4.50	4.50	4.50	4.50	4.50	4.50	4.43	4.57
Aroclor-1232-4	(4)	4.65	4.65	4.65	4.65	4.65	4.65	4.58	4.72
Aroclor-1232-5	(5)	4.75	4.75	4.75	4.75	4.75	4.75	4.68	4.82
DCB		8.50	8.50	8.50	8.50	8.50	8.50	8.40	8.60
TCX		3.40	3.41	3.40	3.41	3.40	3.40	3.35	3.45
Aroclor-1242-1	(1)	4.48	4.49	4.49	4.48	4.49	4.49	4.42	4.56
Aroclor-1242-2	(2)	4.50	4.50	4.50	4.50	4.50	4.50	4.43	4.57
Aroclor-1242-3	(3)	4.56	4.56	4.56	4.56	4.56	4.56	4.49	4.63
Aroclor-1242-4	(4)	4.65	4.65	4.65	4.65	4.65	4.65	4.58	4.72
Aroclor-1242-5	(5)	5.36	5.36	5.36	5.36	5.36	5.36	5.29	5.43
DCB		8.50	8.50	8.50	8.50	8.50	8.50	8.40	8.60
TCX		3.40	3.41	3.40	3.40	3.40	3.40	3.35	3.45
Aroclor-1248-1	(1)	4.48	4.49	4.48	4.48	4.48	4.48	4.41	4.55
Aroclor-1248-2	(2)	4.75	4.75	4.75	4.75	4.75	4.75	4.68	4.82
Aroclor-1248-3	(3)	4.94	4.94	4.94	4.94	4.94	4.94	4.87	5.01
Aroclor-1248-4	(4)	5.32	5.32	5.32	5.32	5.32	5.32	5.25	5.39
Aroclor-1248-5	(5)	5.36	5.36	5.36	5.36	5.36	5.36	5.29	5.43
DCB		8.50	8.50	8.50	8.50	8.50	8.50	8.40	8.60
TCX		3.40	3.41	3.40	3.40	3.41	3.40	3.35	3.45

RETENTION TIMES OF INITIAL CALIBRATION

Aroclor-1254-1	(1)	5.30	5.30	5.30	5.30	5.30	5.30	5.23	5.37
Aroclor-1254-2	(2)	5.51	5.51	5.51	5.51	5.51	5.51	5.44	5.58
Aroclor-1254-3	(3)	5.86	5.86	5.86	5.86	5.86	5.86	5.79	5.93
Aroclor-1254-4	(4)	6.14	6.14	6.14	6.14	6.14	6.14	6.07	6.21
Aroclor-1254-5	(5)	6.55	6.55	6.55	6.55	6.55	6.55	6.48	6.62
DCB		8.50	8.50	8.50	8.50	8.50	8.50	8.40	8.60
TCX		3.40	3.41	3.40	3.40	3.40	3.40	3.35	3.45
Aroclor-1262-1	(1)	6.85	6.85	6.85	6.85	6.85	6.85	6.78	6.92
Aroclor-1262-2	(2)	7.15	7.15	7.15	7.15	7.15	7.15	7.08	7.22
Aroclor-1262-3	(3)	7.42	7.42	7.42	7.43	7.42	7.42	7.35	7.49
Aroclor-1262-4	(4)	7.50	7.50	7.50	7.50	7.50	7.50	7.43	7.57
Aroclor-1262-5	(5)	7.99	7.99	7.99	7.99	7.99	7.99	7.92	8.06
DCB		8.50	8.50	8.50	8.50	8.50	8.50	8.40	8.60
TCX		3.40	3.41	3.40	3.40	3.40	3.40	3.35	3.45
Aroclor-1268-1	(1)	7.42	7.42	7.42	7.42	7.42	7.42	7.35	7.49
Aroclor-1268-2	(2)	7.50	7.50	7.50	7.50	7.50	7.50	7.43	7.57
Aroclor-1268-3	(3)	7.68	7.68	7.68	7.68	7.68	7.68	7.61	7.75
Aroclor-1268-4	(4)	7.99	7.99	7.99	7.99	7.99	7.99	7.92	8.06
Aroclor-1268-5	(5)	8.28	8.28	8.28	8.28	8.28	8.28	8.21	8.35
DCB		8.50	8.50	8.50	8.50	8.50	8.50	8.40	8.60
TCX		3.41	3.41	3.40	3.40	3.41	3.41	3.36	3.46

Contract:	<u>CHEM02</u>						
Lab Code:	<u>CHEM</u>	Case No.:	<u>Q1942</u>	SAS No.:	<u>Q1942</u>	SDG NO.:	<u>Q1942</u>
Instrument ID:	<u>ECD_Q</u>	Calibration Date(s):		<u>04/09/2025</u>	<u>04/09/2025</u>		
		Calibration Times:		<u>09:41</u>	<u>19:09</u>		

LAB FILE ID:		RT 100 =	<u>PQ070136.D</u>	RT 200 =	<u>PQ070137.D</u>
RT 400 =	PQ070138.D	RT 800 =	PQ070139.D	RT 1600 =	PQ070140.D

[illegible]

RETENTION TIMES OF INITIAL CALIBRATION

[illegible]

CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: CHEM02

Lab Code: CHEM **Case No.:** Q1942 **SAS No.:** Q1942 **SDG NO.:** Q1942

Instrument ID: ECD_Q **Calibration Date(s):** 04/09/2025 04/09/2025
Calibration Times: 09:41 19:09

GC Column: ZB-MR1 **ID:** 0.32 (mm)

LAB FILE ID:		CF 100 = <u>PQ070136.D</u>		CF 200 = <u>PQ070137.D</u>			
CF 400 = <u>PQ070138.D</u>		CF 800 = <u>PQ070139.D</u>		CF 1600 = <u>PQ070140.D</u>			
COMPOUND		CF 100	CF 200	CF 400	CF 800	CF 1600	% RSD
Aroclor-1016-1	(1)	249763050	224775150	204155215	186161255	180676488	209106232
Aroclor-1016-2	(2)	384976690	351460750	323806283	294880266	281216291	327268056
Aroclor-1016-3	(3)	244527460	220764925	204373900	184653395	175140664	205892069
Aroclor-1016-4	(4)	200404980	181110060	165723520	151280245	144135296	168530820
Aroclor-1016-5	(5)	194892690	176771980	162665350	148098721	139388661	164363480
Aroclor-1260-1	(1)	344597770	307765250	284829255	259977844	250559227	289545869
Aroclor-1260-2	(2)	403345070	355839390	327234215	303176460	293137811	336546589
Aroclor-1260-3	(3)	300037390	274824575	252370055	232970993	225755974	257191797
Aroclor-1260-4	(4)	335321590	300263950	280280703	257292511	250260739	284683899
Aroclor-1260-5	(5)	626224630	578658625	535046863	503058616	499290124	548455772
DCB		3852041000	3616857350	3367328525	3095901850	3028387594	3392103264
TCX		8453367000	7803085600	7162715300	6652607350	6439273738	7302209798
Aroclor-1221-1	(1)	99985590	90199425	83271005	76395416	71421911	84254669
Aroclor-1221-2	(2)	69042840	61184150	56742780	52797200	48990068	57751408
Aroclor-1221-3	(3)	230369300	199658620	182985365	168427125	154975430	187283168
DCB		3824402900	3521747800	3357980200	3181631463	3033366988	3383825870
TCX		8678124200	8031927000	7454699150	7027083700	6726203988	7583607608
Aroclor-1232-1	(1)	178066420	159011455	147372078	136366765	125092483	149181840
Aroclor-1232-2	(2)	103584510	89009000	81307485	74752030	69913703	83713346
Aroclor-1232-3	(3)	182024280	164644930	151912513	141098261	132757514	154487500
Aroclor-1232-4	(4)	94645710	82631940	78160283	71539890	67361971	78867959
Aroclor-1232-5	(5)	63101380	54348725	51917020	47870774	44697929	52387166
DCB		3934139600	3587764300	3391018250	3181704463	3055915325	3430108388
TCX		8971385400	8052367400	7399591750	6978983575	6706179013	7621701428
Aroclor-1242-1	(1)	213603080	198703975	177018540	163968976	154304205	181519755
Aroclor-1242-2	(2)	328307680	302808275	278882430	257652641	249307827	283391771
Aroclor-1242-3	(3)	210055910	193062480	175865913	163370901	154452037	179361448
Aroclor-1242-4	(4)	169794630	154949690	143459175	133036525	126991226	145646249
Aroclor-1242-5	(5)	155561720	150410045	140501235	130674215	125811173	140591678
DCB		3883102600	3686509700	3413574800	3228196050	3134234106	3469123451
TCX		8450671400	8070960800	7491548450	7034362875	6818019613	7573112628
Aroclor-1248-1	(1)	164605890	145266540	136378668	125716768	115227908	137439155
Aroclor-1248-2	(2)	233809720	199502095	189341295	173068164	158480831	190840421
Aroclor-1248-3	(3)	277138600	240806610	226244858	208075665	192649591	228983065

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1248-4	(4)	290049390	253343145	239807183	223278169	209330638	243161705	13
Aroclor-1248-5	(5)	272889530	233804265	234790728	216664286	205333548	232696471	11
DCB		4057944600	3784720900	3464210375	3265882075	3113655913	3537822773	11
TCX		8879608200	7942057800	7352740200	6851244875	6501803488	7505490913	13
Aroclor-1254-1	(1)	302854610	279411805	254446368	226108266	213120638	255188337	15
Aroclor-1254-2	(2)	464147800	430952225	389204123	347971921	331035789	392662372	14
Aroclor-1254-3	(3)	475648200	444165230	409054165	370493481	354980801	410868375	12
Aroclor-1254-4	(4)	328403150	300047185	281022058	255040681	247413060	282385227	12
Aroclor-1254-5	(5)	366157740	342098460	319837540	288456235	279202967	319150588	11
DCB		4064620400	3777196350	3537407075	3232911213	3108644906	3544155989	11
TCX		8296091200	7917615900	7330357150	6620248675	6332071275	7299276840	11
Aroclor-1262-1	(1)	415137180	374665495	355371995	325227399	319018834	357884181	11
Aroclor-1262-2	(2)	745177040	672958940	625537058	592185150	586546946	644481027	10
Aroclor-1262-3	(3)	433891230	436762110	417179538	379273571	382323369	409885964	7
Aroclor-1262-4	(4)	373605980	348125720	338384735	310807106	305468103	335278329	8
Aroclor-1262-5	(5)	231273680	214143825	199096500	188017520	181527519	202811809	10
DCB		4317220100	3826260000	3557739075	3300433825	3197257900	3639782180	12
TCX		8539875000	7921745300	7186249900	6522050950	6429636125	7319911455	12
Aroclor-1268-1	(1)	851867840	816190885	727096280	680668058	655637546	746292122	11
Aroclor-1268-2	(2)	792919400	760581365	686802638	636628110	612661784	697918659	11
Aroclor-1268-3	(3)	673906890	627904940	569259908	523691860	505189009	579990521	12
Aroclor-1268-4	(4)	262772550	256240655	230264760	210831920	201799756	232381928	12
Aroclor-1268-5	(5)	1884061310	1784761040	1638320858	1520636569	1483204471	1662196849	10
DCB		8060966100	7515239050	6769809200	6202952513	5888748550	6887543083	13
TCX		8589194400	8040753200	7212303650	6653681875	6289940125	7357174650	13

CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: CHEM02

Lab Code: CHEM **Case No.:** Q1942 **SAS No.:** Q1942 **SDG NO.:** Q1942

Instrument ID: ECD_Q **Calibration Date(s):** 04/09/2025 04/09/2025
Calibration Times: 09:41 19:09

GC Column: ZB-MR2 **ID:** 0.32 (mm)

LAB FILE ID: CF 100 = PQ070136.D CF 200 = PQ070137.D								
CF 400 = PQ070138.D CF 800 = PQ070139.D CF 1600 = PQ070140.D								
COMPOUND		CF 100	CF 200	CF 400	CF 800	CF 1600	CF	% RSD
Aroclor-1016-1	(1)	267706380	240149510	215617863	195076538	184368240	220583706	15
Aroclor-1016-2	(2)	398799990	357631625	325418048	297729016	288608279	333637392	14
Aroclor-1016-3	(3)	223358650	200653035	179940028	163355350	157299829	184921378	15
Aroclor-1016-4	(4)	198859160	177775385	158179853	140714338	132415214	161588790	17
Aroclor-1016-5	(5)	241987510	211088515	190979875	171021975	163239005	195663376	16
Aroclor-1260-1	(1)	423427040	379556595	344405948	318514340	305369473	354254679	14
Aroclor-1260-2	(2)	504309150	457295850	416490358	386146059	370486350	426945553	13
Aroclor-1260-3	(3)	476308260	428023580	391463698	363603344	352197272	402319231	13
Aroclor-1260-4	(4)	420036920	372615210	343535138	317648710	308142144	352395624	13
Aroclor-1260-5	(5)	907130970	841414240	756997773	744475633	733281271	796659977	9
DCB		6535604400	5852947600	5380023725	5035407675	4899016056	5540599891	12
TCX		8131999400	7443437200	6888261700	6456898025	6236661550	7031451575	11
Aroclor-1221-1	(1)	102650310	94151785	83595913	78608001	72942361	86389674	14
Aroclor-1221-2	(2)	73994600	65421480	59864215	55348631	51783409	61282467	14
Aroclor-1221-3	(3)	233765870	208136675	189628173	172930146	159329051	192757983	15
DCB		6481435000	5883893900	5370720450	5098018588	4889196425	5544652873	12
TCX		8099340600	7346610500	6739527150	6418585575	6192109800	6959234725	11
Aroclor-1232-1	(1)	188507030	173261055	152964000	138815121	125676611	155844763	16
Aroclor-1232-2	(2)	186302530	168460415	152863605	139764006	131031050	155684321	14
Aroclor-1232-3	(3)	102354730	89756075	82396380	76131875	70310489	84189910	15
Aroclor-1232-4	(4)	90000150	77455130	71377800	64871604	59285185	72597974	16
Aroclor-1232-5	(5)	102278410	86074350	79274728	72168070	66629351	81284982	17
DCB		6704351200	5925502000	5536721775	5152150500	4915175206	5646780136	12
TCX		8087265800	7461421900	6837631050	6455598150	6187239325	7005831245	11
Aroclor-1242-1	(1)	226399990	205837620	177449193	161209293	157327211	185644661	16
Aroclor-1242-2	(2)	335014360	304161420	272261593	247436299	242587584	280292251	14
Aroclor-1242-3	(3)	185128690	170203865	149501653	137477609	133187764	155099916	14
Aroclor-1242-4	(4)	176767690	162934115	141567113	128493226	122068773	146366183	16
Aroclor-1242-5	(5)	221216690	204998190	179077545	163439771	157983109	185343061	15
DCB		6656627800	6224051750	5490437225	5145624225	5056216013	5714591403	12
TCX		8176444800	7734070000	6988443300	6539849375	6448004175	7177362330	11
Aroclor-1248-1	(1)	172551350	150026530	138233948	125131790	114679439	140124611	16
Aroclor-1248-2	(2)	265596080	226910660	211885993	190284878	174331772	213801876	16
Aroclor-1248-3	(3)	259487790	220864925	205843245	185130823	169614557	208188268	17

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1248-4	(4)	316203260	265890980	249991765	226792396	209369018	253649484	16
Aroclor-1248-5	(5)	307761630	261844580	245137418	223445620	208434931	249324836	15
DCB		6821876300	6330252400	5590001050	5286447313	4894995394	5784714491	14
TCX		8587323200	7625509300	7220146150	6689572525	6364480838	7297406403	12
Aroclor-1254-1	(1)	452232520	415810180	374659888	327881964	312113079	376539526	16
Aroclor-1254-2	(2)	401965440	368052650	329043383	286694086	271991447	331549401	16
Aroclor-1254-3	(3)	630751260	583781200	524959120	461083610	447915403	529698119	15
Aroclor-1254-4	(4)	377369540	350771460	319312268	281666679	274425016	320708993	14
Aroclor-1254-5	(5)	567209870	531535745	480961875	428681108	408777653	483433250	14
DCB		6718161800	6274237100	5623043850	5080971700	4863532681	5711989426	14
TCX		8302043200	7742535400	7146211800	6364580475	6193526938	7149779563	13
Aroclor-1262-1	(1)	549175570	526412150	484975778	432665170	423525525	483350839	11
Aroclor-1262-2	(2)	503484530	509047360	445327908	417300923	395341229	454100390	11
Aroclor-1262-3	(3)	433072560	385250720	348805213	315340720	311690518	358831946	14
Aroclor-1262-4	(4)	724255690	649670675	633651833	571123538	580952826	631930912	10
Aroclor-1262-5	(5)	321409280	315736790	301302245	275456958	273716904	297524435	7
DCB		6270711900	6081579900	5487790150	5051265950	4893711225	5557011825	11
TCX		7650151400	7163812600	6960953350	6105068425	6217091550	6819415465	10
Aroclor-1268-1	(1)	1172688790	1110342955	997292465	922425329	892346753	1019019258	12
Aroclor-1268-2	(2)	1059649520	1014686725	902528473	848879576	827722193	930693297	11
Aroclor-1268-3	(3)	970600990	891422115	828495370	744677306	719980218	831035200	12
Aroclor-1268-4	(4)	392452430	378314640	345218365	319673034	305341517	348199997	11
Aroclor-1268-5	(5)	2931717850	2702209675	2458251545	2289988123	2235926499	2523618738	12
DCB		12477463300	11548770550	10490532075	9472314313	9012424938	10600301035	14
TCX		7945200600	7733277400	6856583350	6386768525	6064278800	6997221735	12

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: CHEM02

Lab Code: CHEM Case No.: Q1942 SAS No.: Q1942 SDG NO.: Q1942

Instrument ID: _____ Date(s) Analyzed: _____

GC Column: _____ ID: _____ (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
		1				
		2				
		3				
		4				
		5				

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070136.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 09:41
 Operator : YP\AJ
 Sample : AR1660ICC100
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR16601038

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 11:12:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 11:02:03 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.783	42266835	40659997	5.788	5.783
2) SA Decachlor...	8.503	7.547	38520410	65356044	11.356	11.796
Target Compounds						
3) L1 AR-1016-1	4.484	3.785	24976305	26770638	119.443	121.363
4) L1 AR-1016-2	4.503	3.801	38497669	39879999	117.633	119.531
5) L1 AR-1016-3	4.561	3.961	24452746	22335865	118.765	120.786
6) L1 AR-1016-4	4.651	4.010	20040498	19885916	118.913	123.065
7) L1 AR-1016-5	4.935	4.205	19489269	24198751	118.574	123.675
31) L7 AR-1260-1	6.025	5.199	34459777	42342704	119.013	119.526
32) L7 AR-1260-2	6.281	5.387	40334507	50430915	119.848	118.120
33) L7 AR-1260-3	6.632	5.529	30003739	47630826	116.659	118.391
34) L7 AR-1260-4	6.845	5.990	33532159	42003692	117.787	119.195
35) L7 AR-1260-5	7.151	6.233	62622463	90713097	114.180	113.867



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070136.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 09:41
Operator : YP\AJ
Sample : AR1660ICC100
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR16601038

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 11:12:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 11:02:03 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

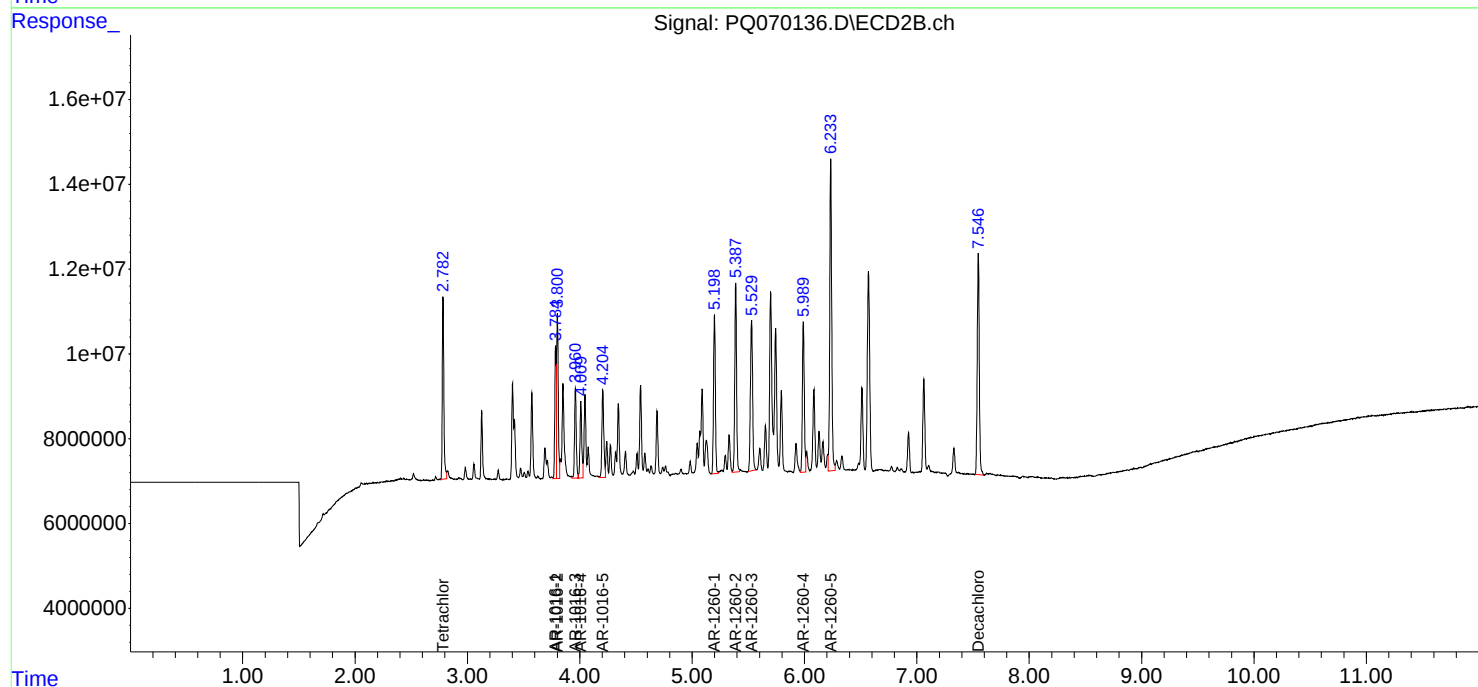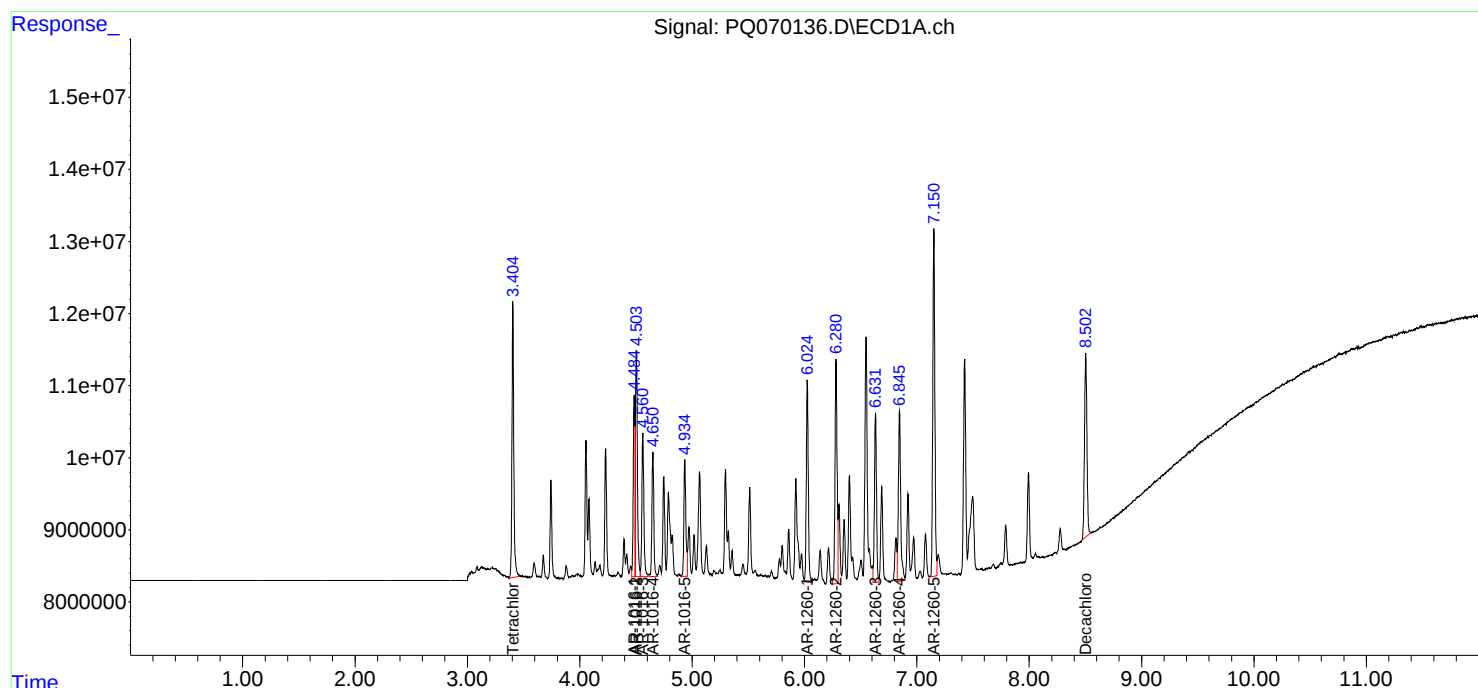

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070137.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 09:55
 Operator : YP\AJ
 Sample : AR1660ICC200
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR16602039

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 11:09:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 11:02:03 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.405	2.783	78030856	74434372	11.124	11.017
2) SA Decachlor...	8.504	7.547	72337147	117.1E6	22.073	22.121
Target Compounds						
3) L1 AR-1016-1	4.485	3.785	44955030	48029902	225.971	230.025
4) L1 AR-1016-2	4.503	3.801	70292150	71526325	224.690	225.389
5) L1 AR-1016-3	4.562	3.961	44152985	40130607	225.003	228.910
6) L1 AR-1016-4	4.651	4.010	36222012	35555077	225.595	233.498
7) L1 AR-1016-5	4.935	4.205	35354396	42217703	225.573	229.341
31) L7 AR-1260-1	6.025	5.199	61553050	75911319	223.194	225.282
32) L7 AR-1260-2	6.281	5.388	71167878	91459170	222.506	224.382
33) L7 AR-1260-3	6.632	5.529	54964915	85604716	222.999	223.032
34) L7 AR-1260-4	6.846	5.990	60052790	74523042	220.762	222.135
35) L7 AR-1260-5	7.152	6.235	115.7E6	168.3E6	218.769	218.821



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070137.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 09:55
Operator : YP\AJ
Sample : AR1660ICC200
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR16602039

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 11:09:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 11:02:03 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

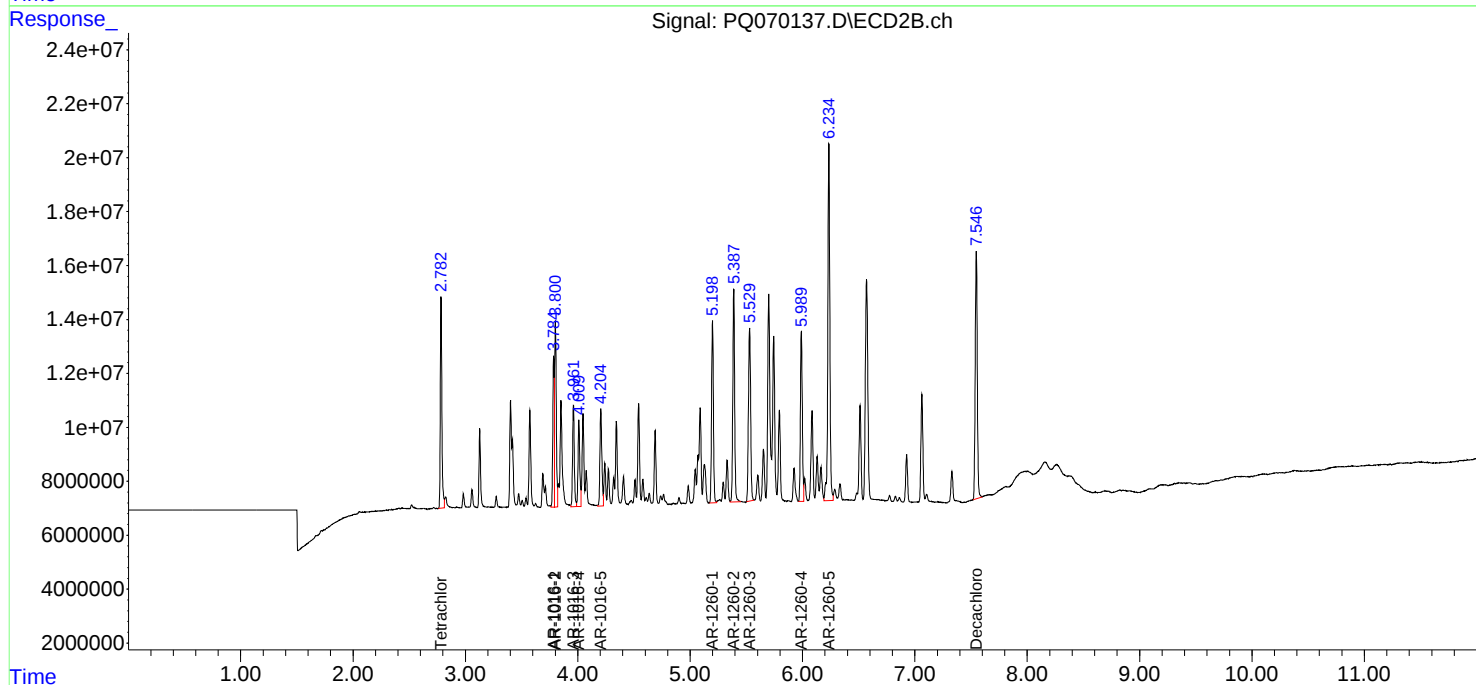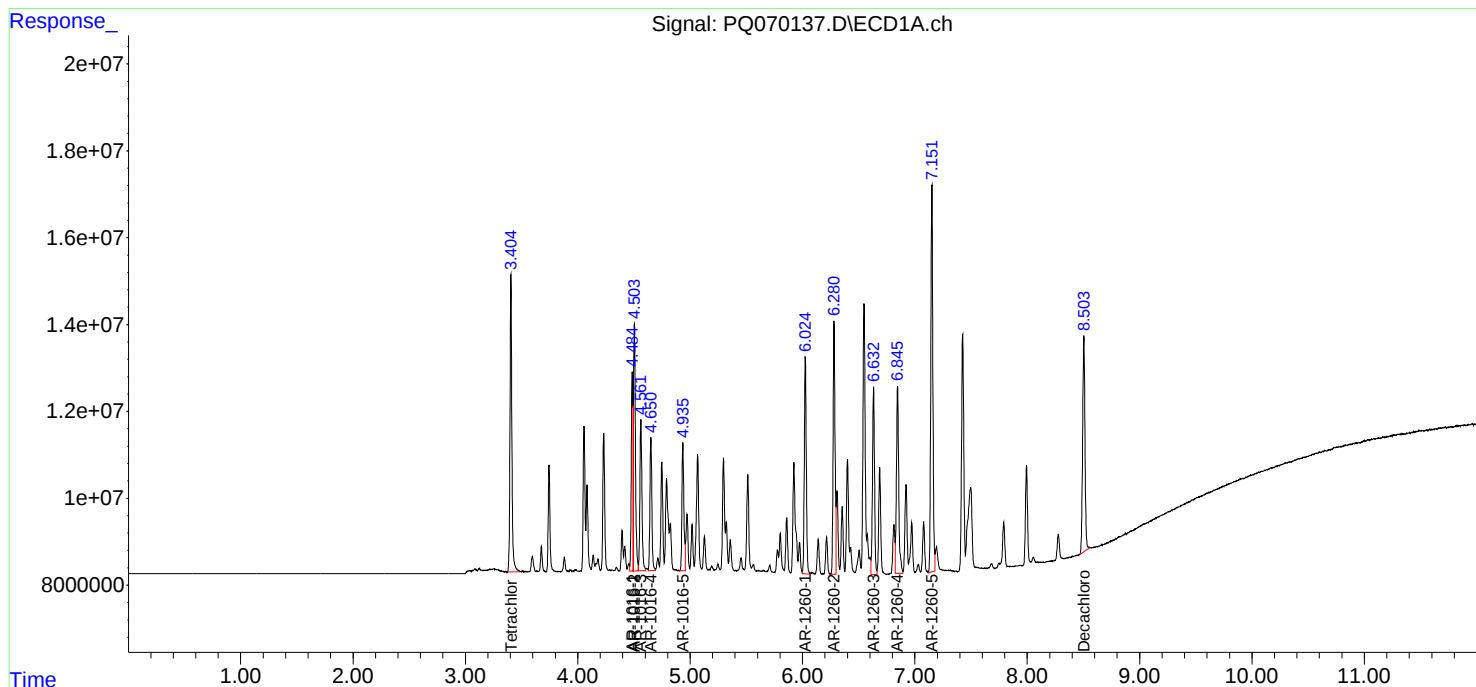

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070138.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 10:10
 Operator : YP\AJ
 Sample : AR1660ICC400
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR16603040

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 11:02:25 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 11:02:03 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.783	143.3E6	137.8E6	20.000	20.000
2) SA Decachlor...	8.502	7.546	134.7E6	215.2E6	40.000	40.000
Target Compounds						
3) L1 AR-1016-1	4.484	3.785	81662086	86247145	400.000	400.000
4) L1 AR-1016-2	4.503	3.800	129.5E6	130.2E6	400.000	400.000
5) L1 AR-1016-3	4.561	3.961	81749560	71976011	400.000	400.000
6) L1 AR-1016-4	4.651	4.009	66289408	63271941	400.000	400.000
7) L1 AR-1016-5	4.935	4.205	65066140	76391950	400.000	400.000
31) L7 AR-1260-1	6.025	5.198	113.9E6	137.8E6	400.000	400.000
32) L7 AR-1260-2	6.280	5.387	130.9E6	166.6E6	400.000	400.000
33) L7 AR-1260-3	6.631	5.529	100.9E6	156.6E6	400.000	400.000
34) L7 AR-1260-4	6.845	5.990	112.1E6	137.4E6	400.000	400.000
35) L7 AR-1260-5	7.151	6.234	214.0E6	302.8E6	400.000	400.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070138.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 10:10
Operator : YP\AJ
Sample : AR1660ICC400
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR16603040

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 11:02:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 11:02:03 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

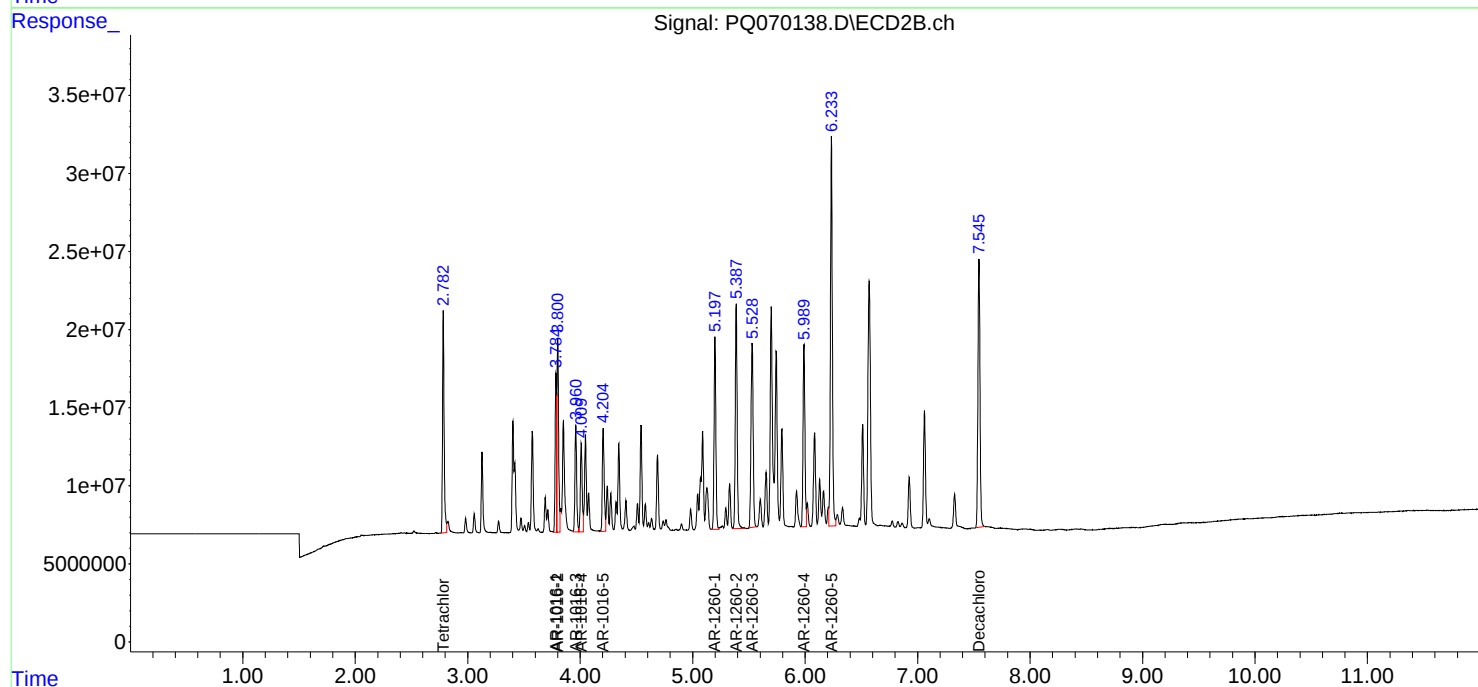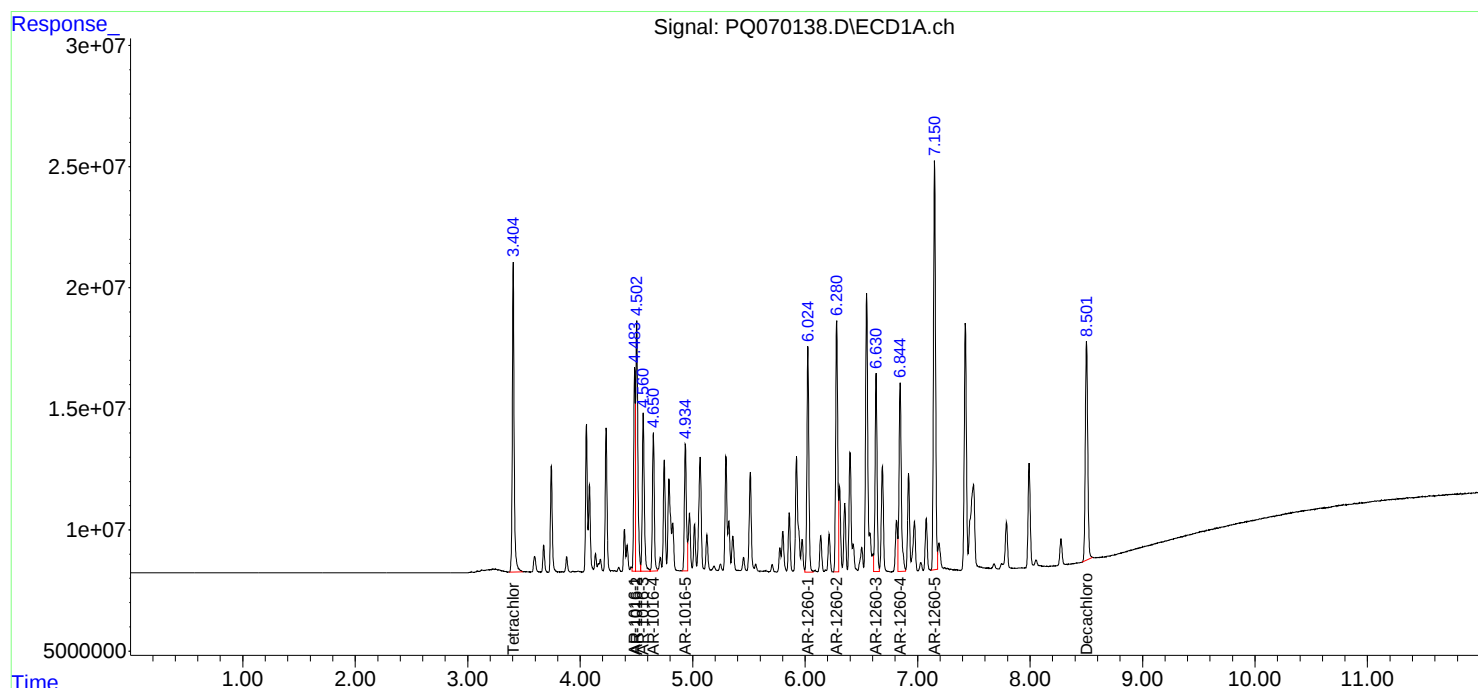

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070139.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 10:25
 Operator : YP\AJ
 Sample : AR1660ICC800
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR16604041

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 11:07:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 11:02:03 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.405	2.783	266.1E6	258.3E6	39.414	39.569
2) SA Decachlor...	8.502	7.547	247.7E6	402.8E6	78.281	78.912
Target Compounds						
3) L1 AR-1016-1	4.485	3.785	148.9E6	156.1E6	782.474	786.781
4) L1 AR-1016-2	4.503	3.801	235.9E6	238.2E6	786.432	783.708
5) L1 AR-1016-3	4.561	3.961	147.7E6	130.7E6	785.525	783.173
6) L1 AR-1016-4	4.650	4.010	121.0E6	112.6E6	787.339	782.998
7) L1 AR-1016-5	4.935	4.205	118.5E6	136.8E6	789.592	781.456
31) L7 AR-1260-1	6.025	5.199	208.0E6	254.8E6	784.477	789.469
32) L7 AR-1260-2	6.281	5.388	242.5E6	308.9E6	787.856	789.986
33) L7 AR-1260-3	6.632	5.530	186.4E6	290.9E6	786.293	788.112
34) L7 AR-1260-4	6.846	5.991	205.8E6	254.1E6	783.797	786.481
35) L7 AR-1260-5	7.151	6.235	402.4E6	595.6E6	785.316	799.525



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070139.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 10:25
Operator : YP\AJ
Sample : AR1660ICC800
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR16604041

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 11:07:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 11:02:03 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

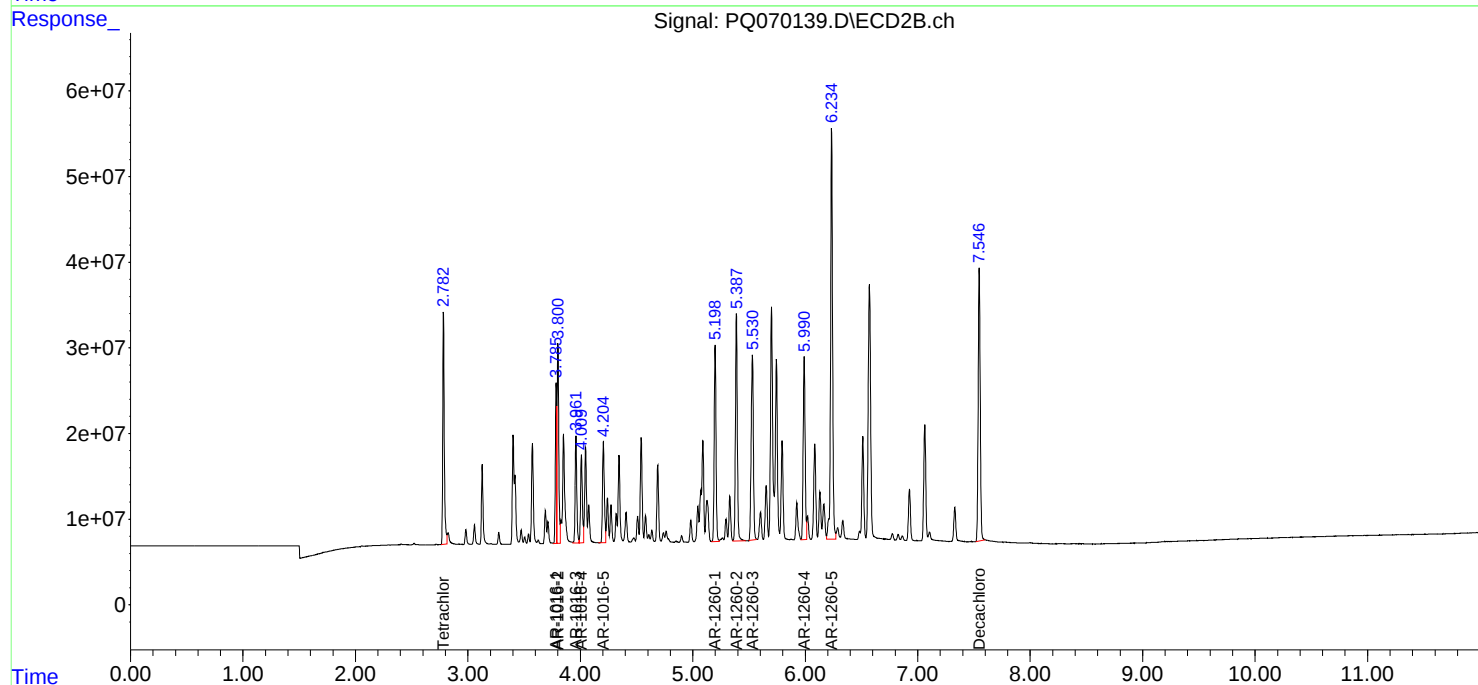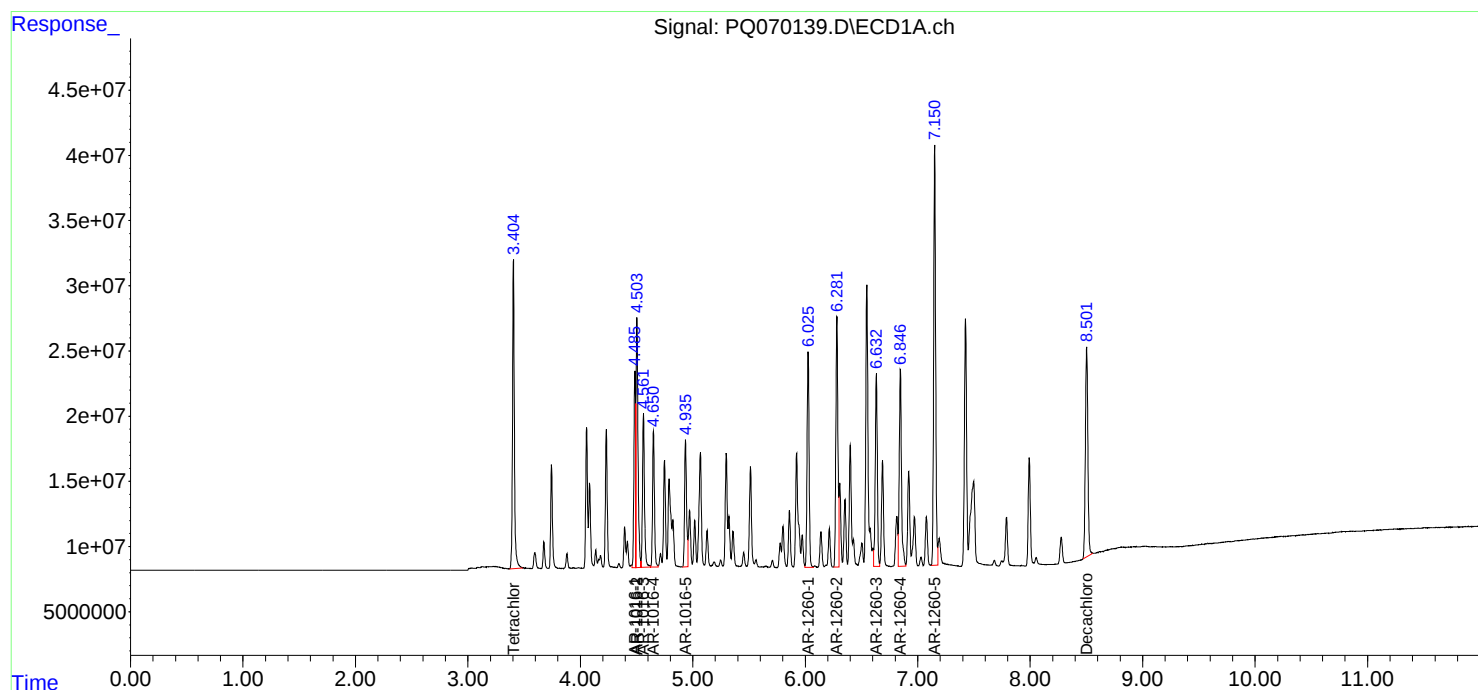

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070140.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 10:39
 Operator : YP\AJ
 Sample : AR1660ICC1600
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR16605042

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 11:04:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 11:02:03 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.405	2.783	515.1E6	498.9E6	75.745	76.028
2) SA Decachlor...	8.502	7.547	484.5E6	783.8E6	151.521	152.513
Target Compounds						
3) L1 AR-1016-1	4.485	3.785	289.1E6	295.0E6	1502.383	1474.997
4) L1 AR-1016-2	4.503	3.801	449.9E6	461.8E6	1487.370	1504.083
5) L1 AR-1016-3	4.561	3.961	280.2E6	251.7E6	1476.755	1492.586
6) L1 AR-1016-4	4.650	4.010	230.6E6	211.9E6	1488.526	1458.141
7) L1 AR-1016-5	4.935	4.205	223.0E6	261.2E6	1476.702	1474.695
31) L7 AR-1260-1	6.025	5.198	400.9E6	488.6E6	1497.585	1503.877
32) L7 AR-1260-2	6.280	5.388	469.0E6	592.8E6	1512.062	1506.469
33) L7 AR-1260-3	6.631	5.529	361.2E6	563.5E6	1510.939	1515.518
34) L7 AR-1260-4	6.845	5.990	400.4E6	493.0E6	1509.466	1513.103
35) L7 AR-1260-5	7.151	6.234	798.9E6	1173.3E6	1544.688	1574.537



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070140.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 10:39
Operator : YP\AJ
Sample : AR1660ICC1600
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR16605042

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 11:04:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 11:02:03 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

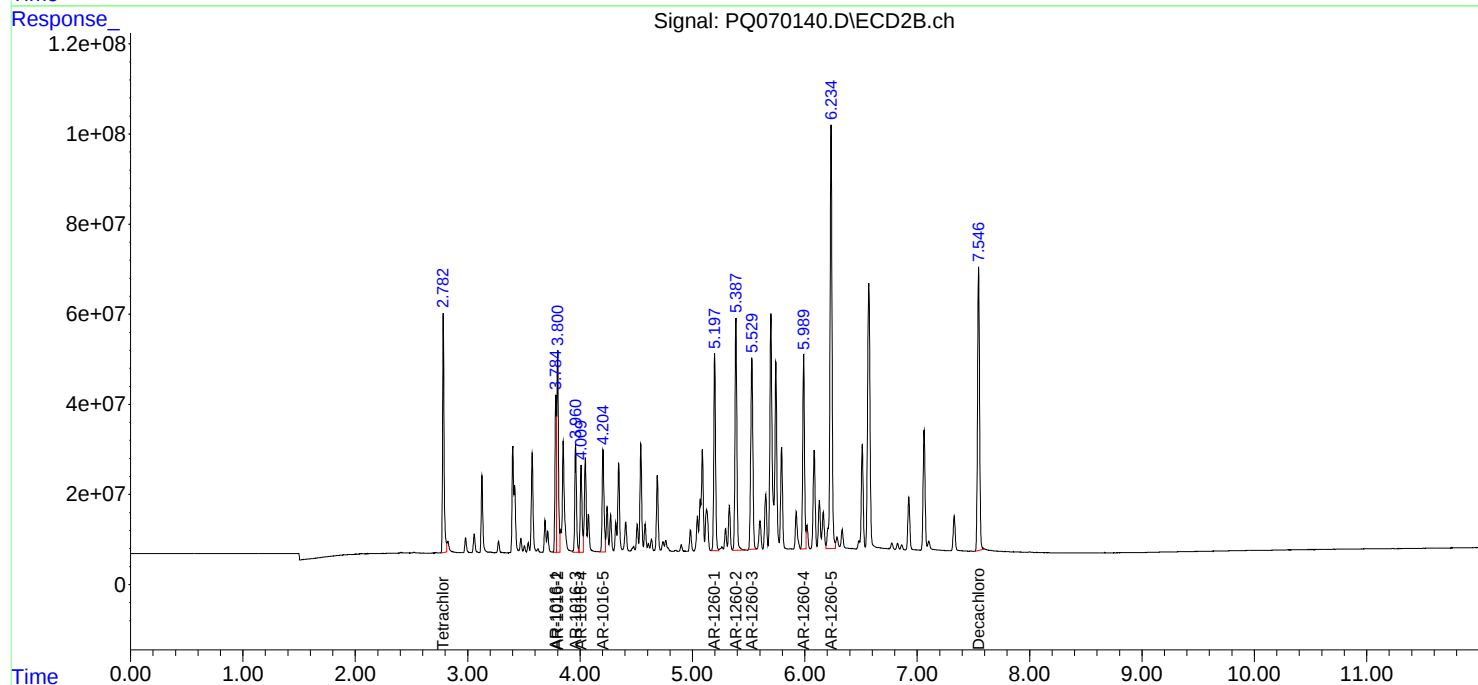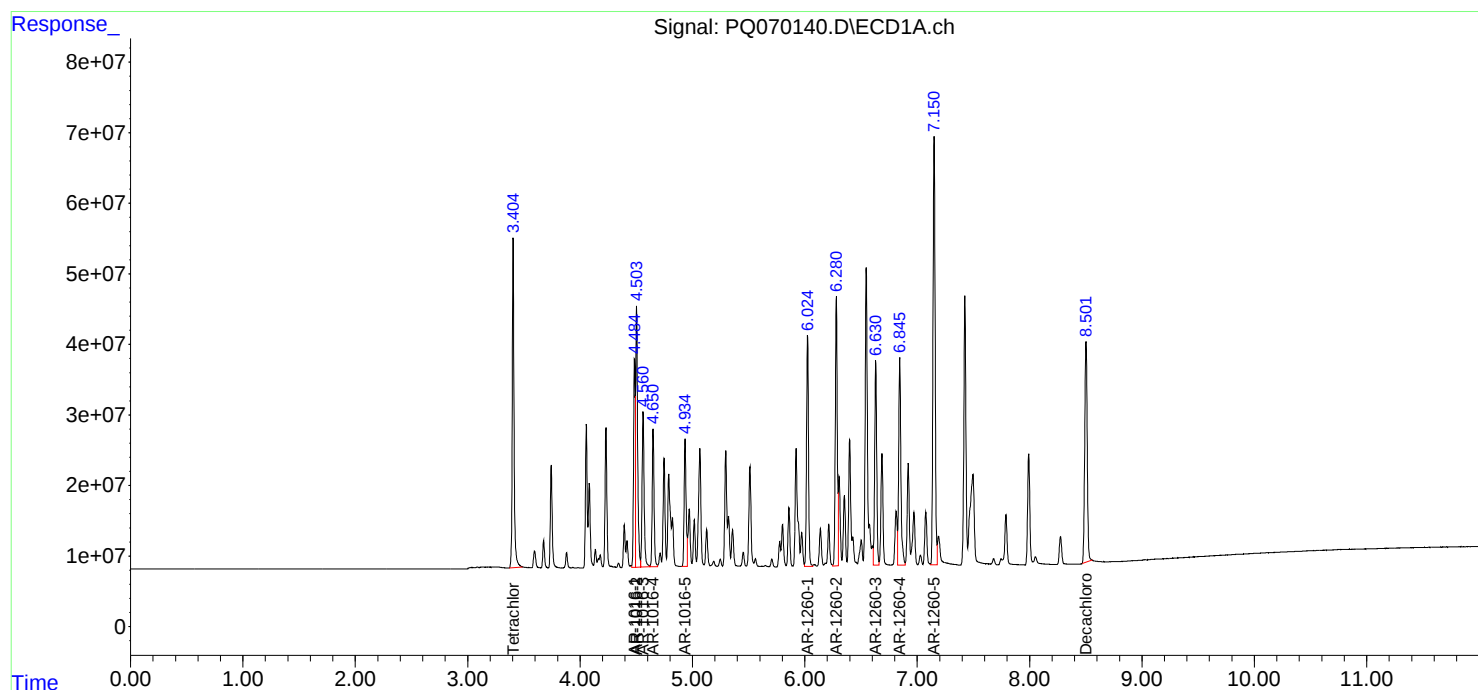

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070141.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 10:54
 Operator : YP\AJ
 Sample : AR1221ICC100
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12211043

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 11:40:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 11:35:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.405	2.783	43390621	40496703	5.387	5.476
2) SA Decachlor...	8.503	7.547	38244029	64814350	10.718	10.963
Target Compounds						
8) L2 AR-1221-1	3.597	2.983	9998559	10265031	109.691	109.826
9) L2 AR-1221-2	3.676	3.059	6904284	7399460	110.782	111.393
10) L2 AR-1221-3	3.743	3.128	23036930	23376587	112.739	111.047



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070141.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 10:54
Operator : YP\AJ
Sample : AR1221ICC100
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12211043

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 11:40:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 11:35:47 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

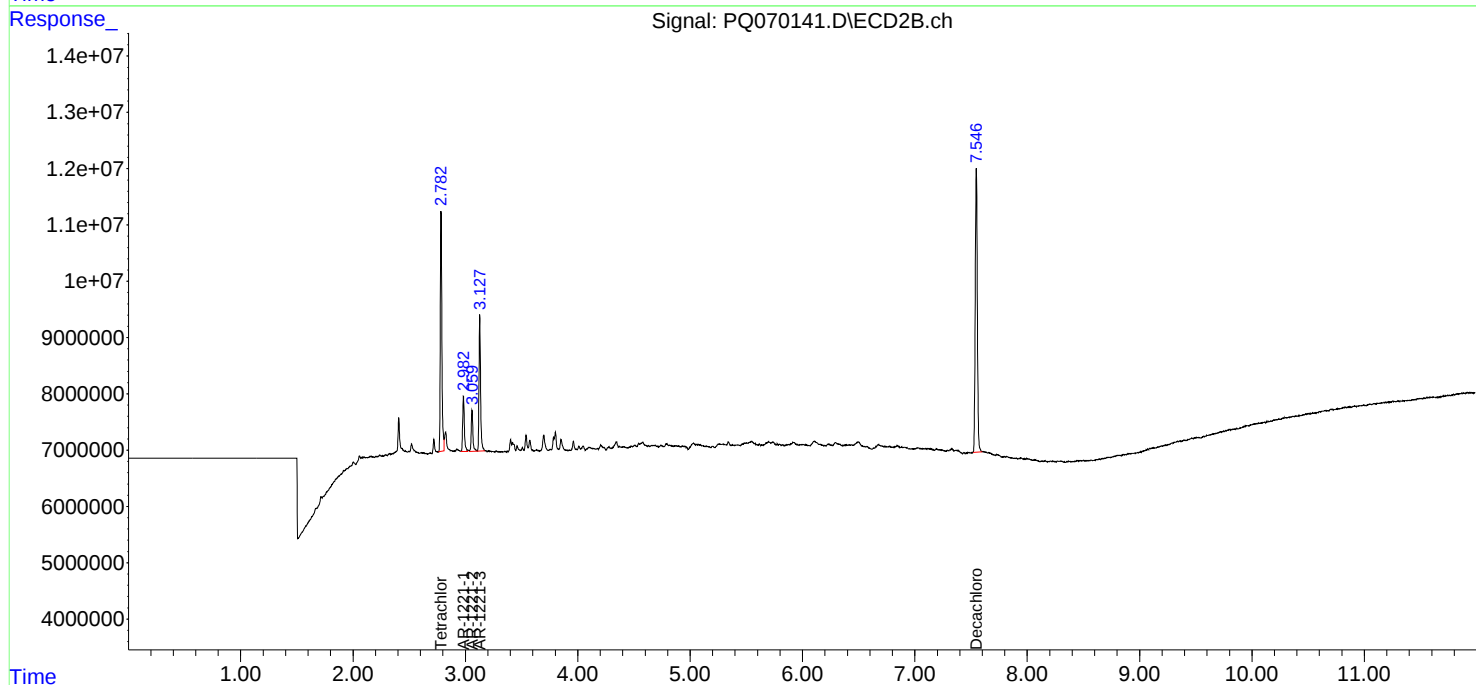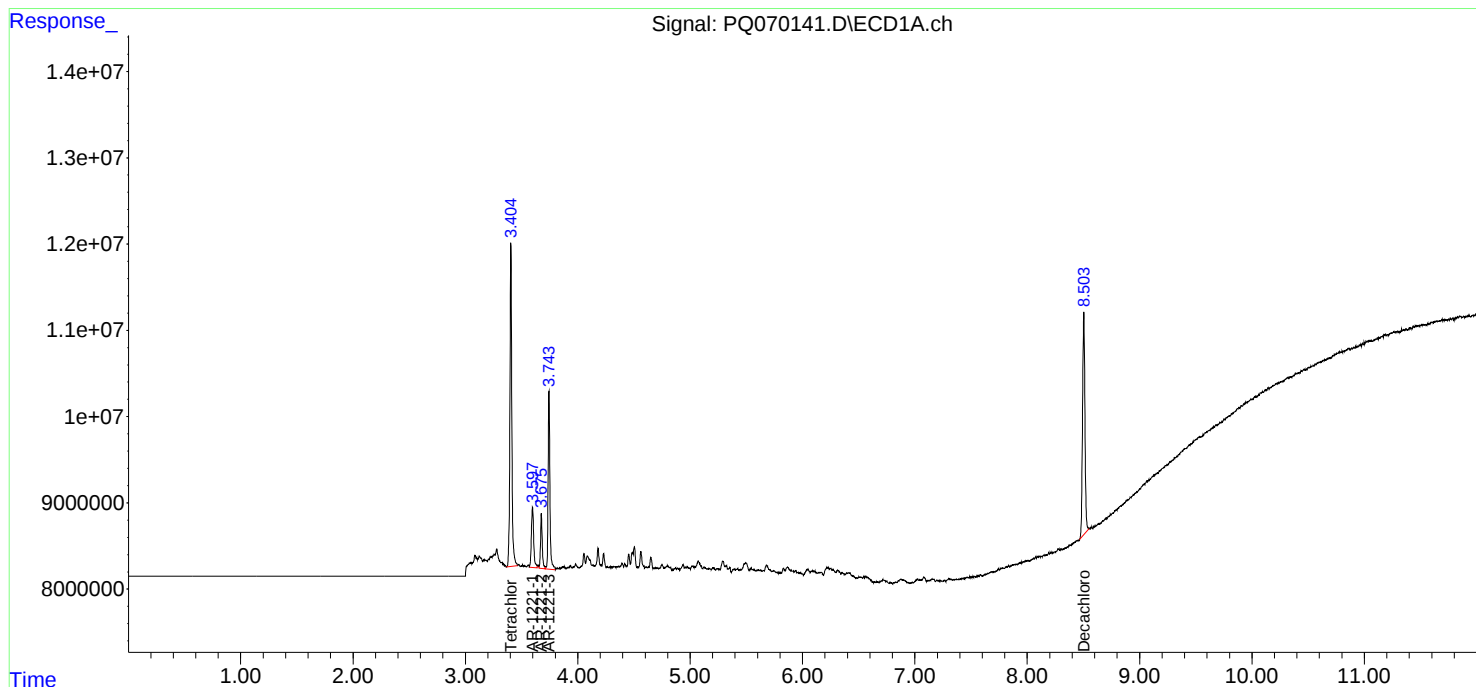

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070142.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 11:08
 Operator : YP\AJ
 Sample : AR1221ICC200
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12212044

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 11:38:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 11:35:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.405	2.783	80319270	73466105	10.373	10.431
2) SA Decachlor...	8.502	7.547	70434956	117.7E6	20.476	20.912
Target Compounds						
8) L2 AR-1221-1	3.598	2.983	18039885	18830357	207.988	211.877
9) L2 AR-1221-2	3.676	3.059	12236830	13084296	207.532	208.871
10) L2 AR-1221-3	3.744	3.128	39931724	41627335	208.715	209.306



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070142.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 11:08
Operator : YP\AJ
Sample : AR1221ICC200
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12212044

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 11:38:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 11:35:47 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

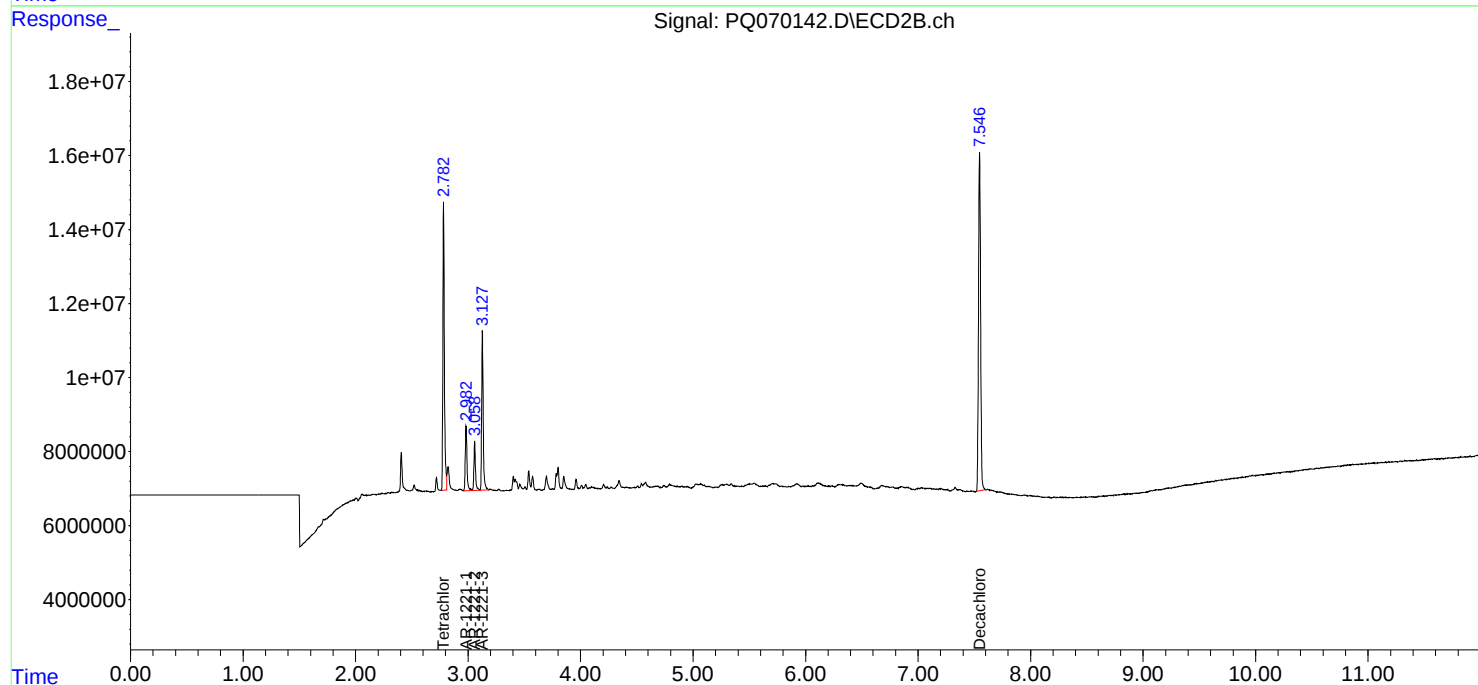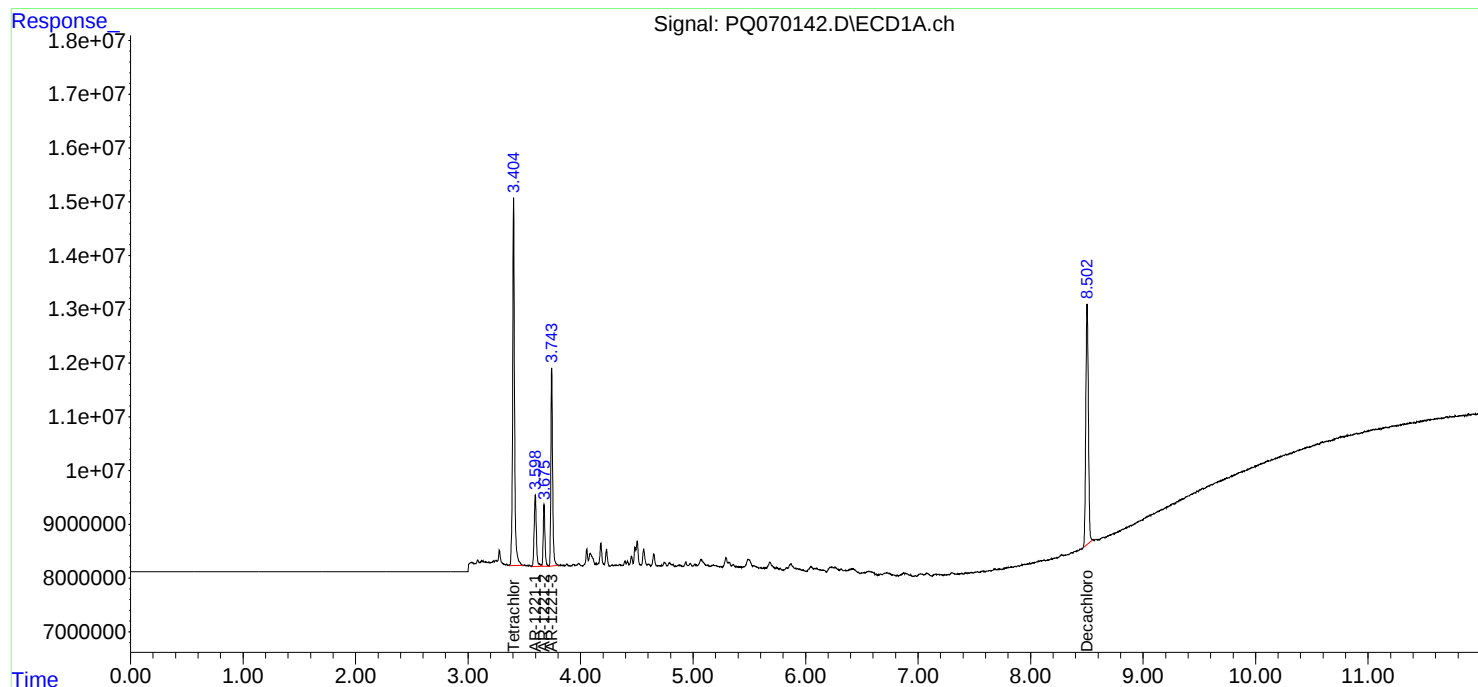

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070143.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 11:23
 Operator : YP\AJ
 Sample : AR1221ICC400
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12213045

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 11:36:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 11:35:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.783	149.1E6	134.8E6	20.000	20.000
2) SA Decachlor...	8.502	7.546	134.3E6	214.8E6	40.000	40.000
Target Compounds						
8) L2 AR-1221-1	3.598	2.982	33308402	33438365	400.000	400.000
9) L2 AR-1221-2	3.676	3.058	22697112	23945686	400.000	400.000
10) L2 AR-1221-3	3.743	3.127	73194146	75851269	400.000	400.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070143.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 11:23
Operator : YP\AJ
Sample : AR1221ICC400
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12213045

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 11:36:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 11:35:47 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

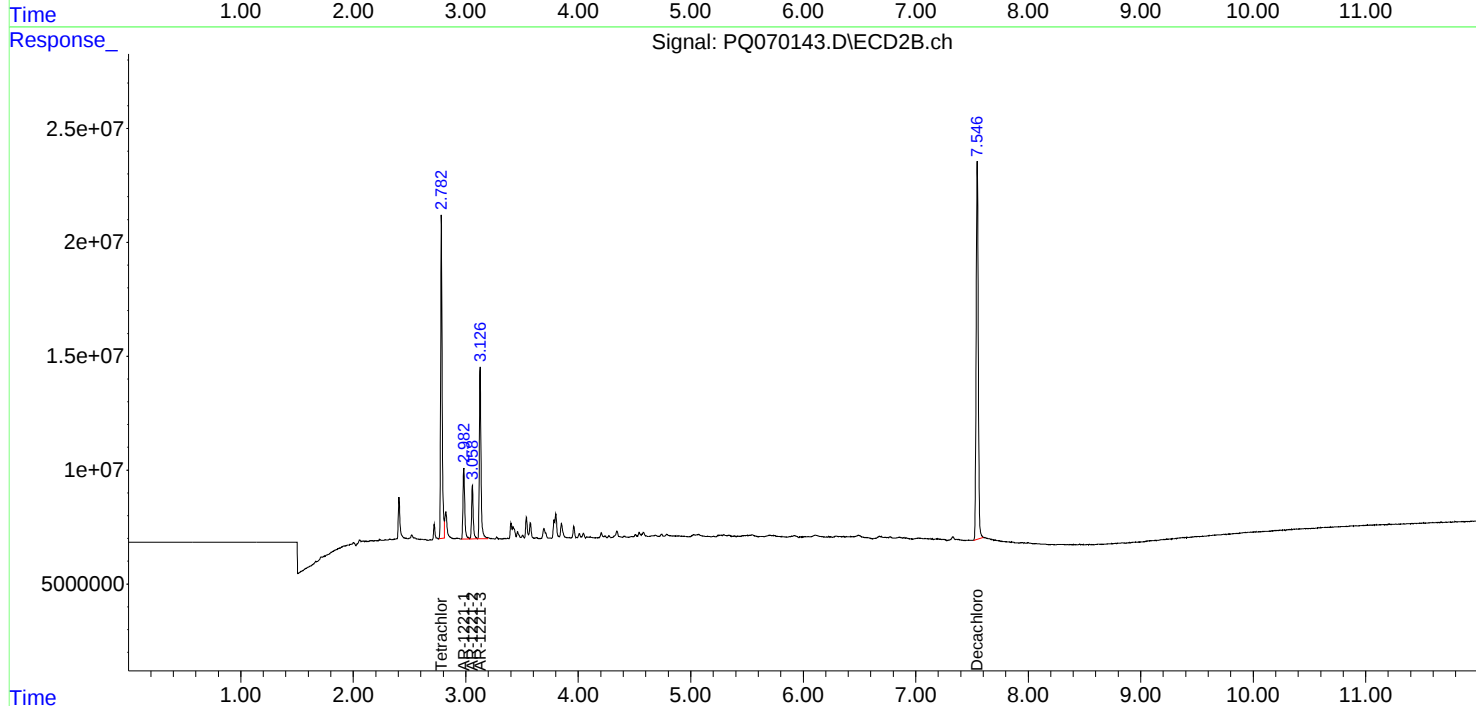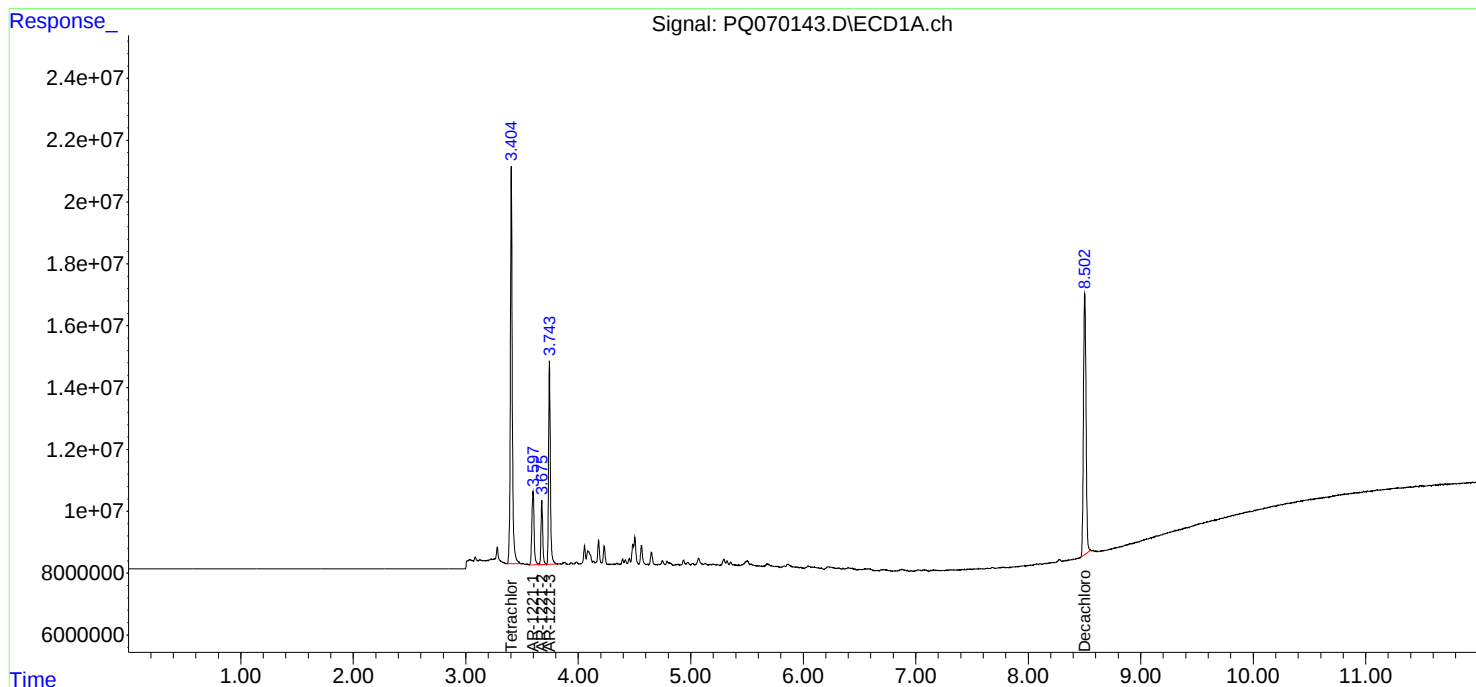

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070144.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 11:37
 Operator : YP\AJ
 Sample : AR1221ICC800
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12214046

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 11:49:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 11:49:02 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.405	2.783	281.1E6	256.7E6	36.046	35.903
2) SA Decachlor...	8.502	7.546	254.5E6	407.8E6	73.321	71.444
Target Compounds						
8) L2 AR-1221-1	3.598	2.983	61116333	62886401	698.769	700.672
9) L2 AR-1221-2	3.676	3.059	42237760	44278905	704.647	695.583
10) L2 AR-1221-3	3.743	3.127	134.7E6	138.3E6	689.709	687.885



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070144.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 11:37
Operator : YP\AJ
Sample : AR1221ICC800
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12214046

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 11:49:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 11:49:02 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

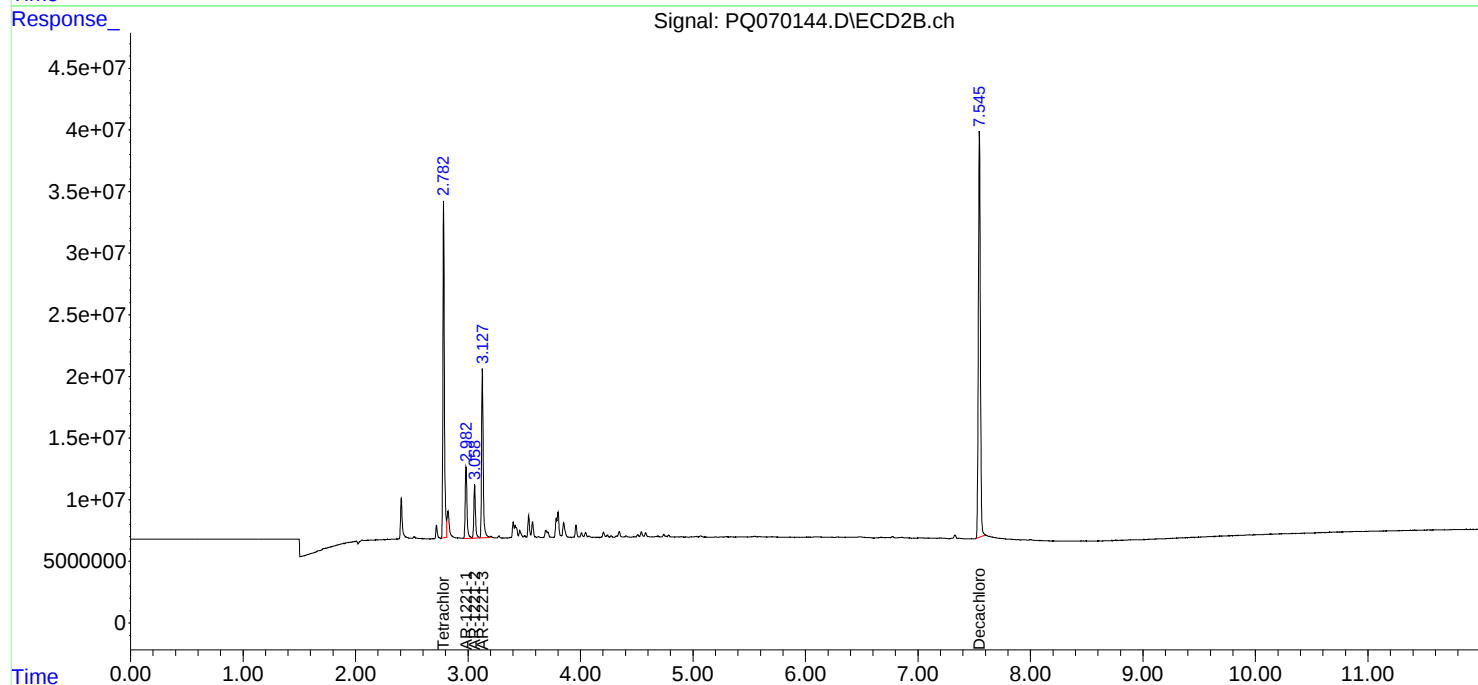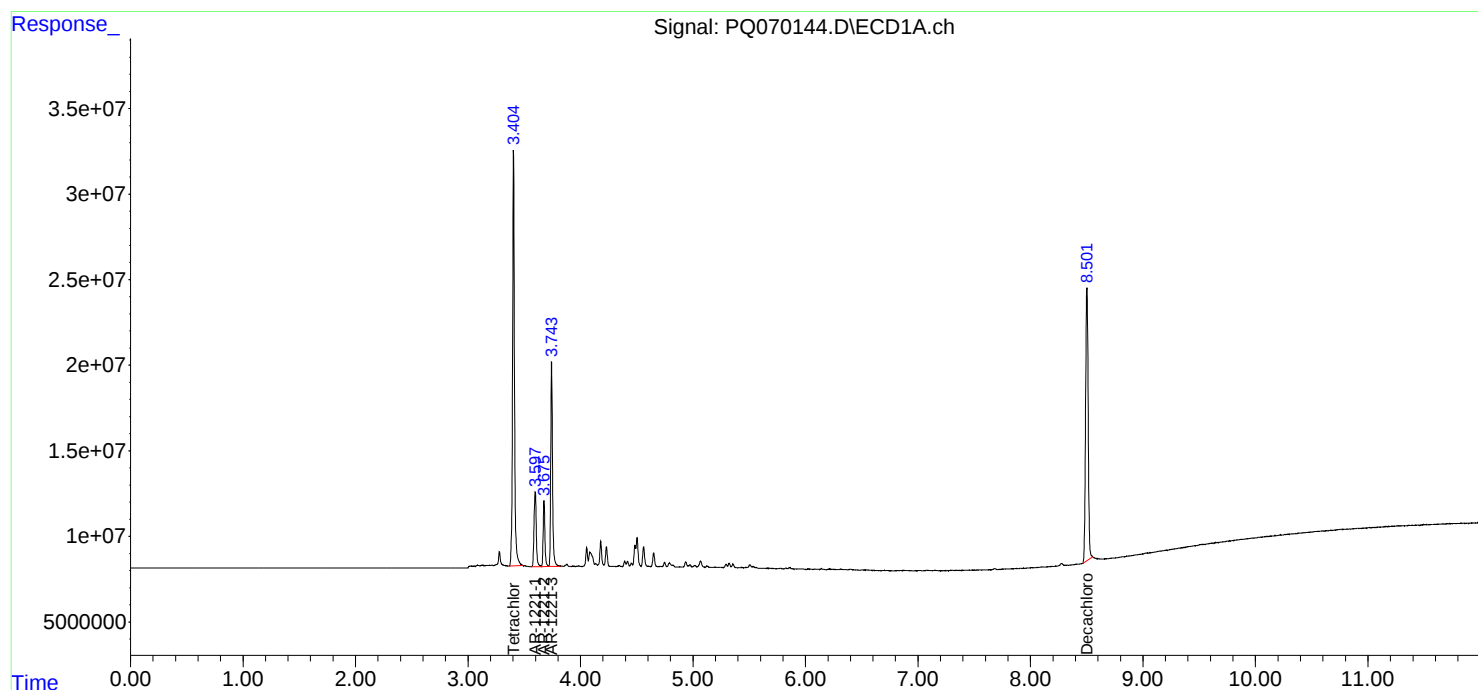

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070145.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 11:52
 Operator : YP\AJ
 Sample : AR1221ICC1600
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12215047

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 12:04:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 12:04:29 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.405	2.783	538.1E6	495.4E6	70.955	71.182
2) SA Decachlor...	8.502	7.546	485.3E6	782.3E6	143.429	141.086
Target Compounds						
8) L2 AR-1221-1	3.598	2.983	114.3E6	116.7E6	1356.305	1350.946
9) L2 AR-1221-2	3.675	3.059	78384109	82853455	1357.267	1351.993
10) L2 AR-1221-3	3.743	3.128	248.0E6	254.9E6	1323.988	1322.521



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070145.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 11:52
Operator : YP\AJ
Sample : AR1221ICC1600
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12215047

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 12:04:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 12:04:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

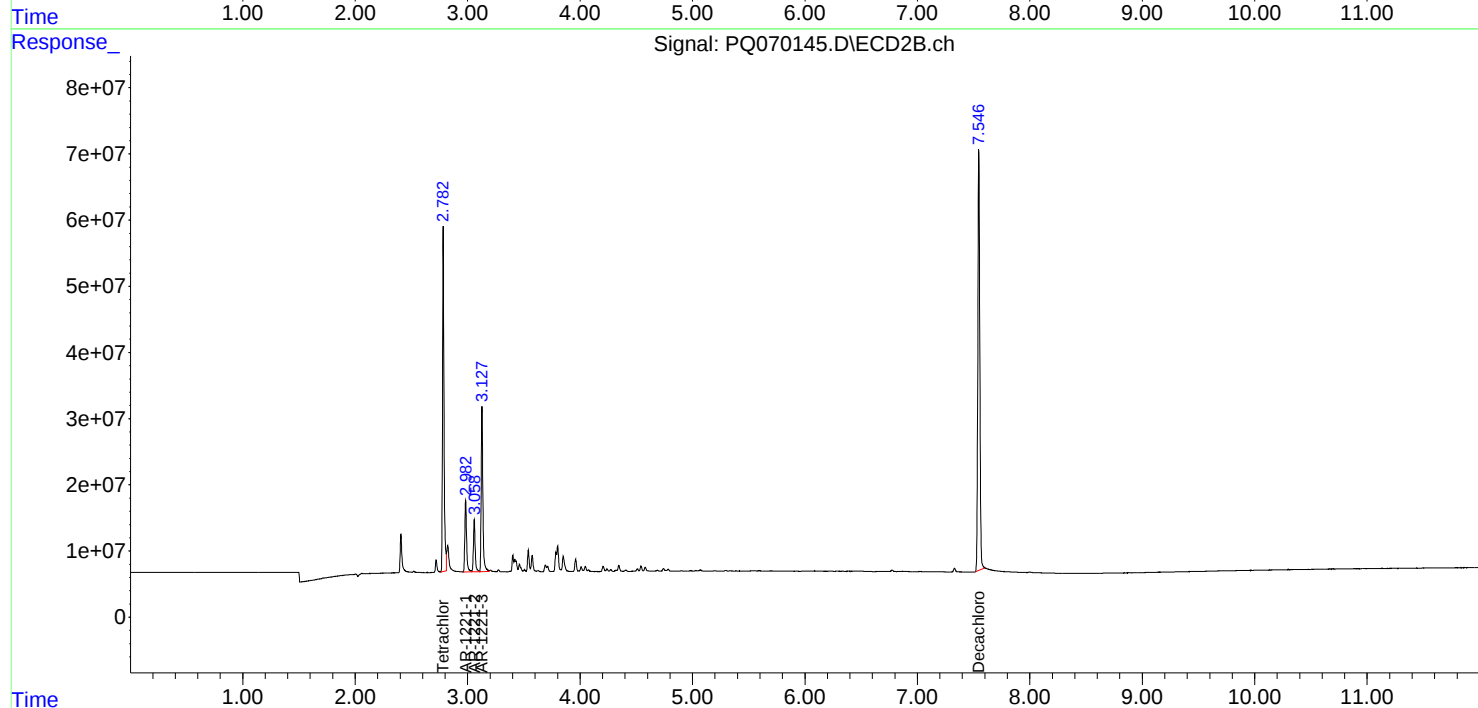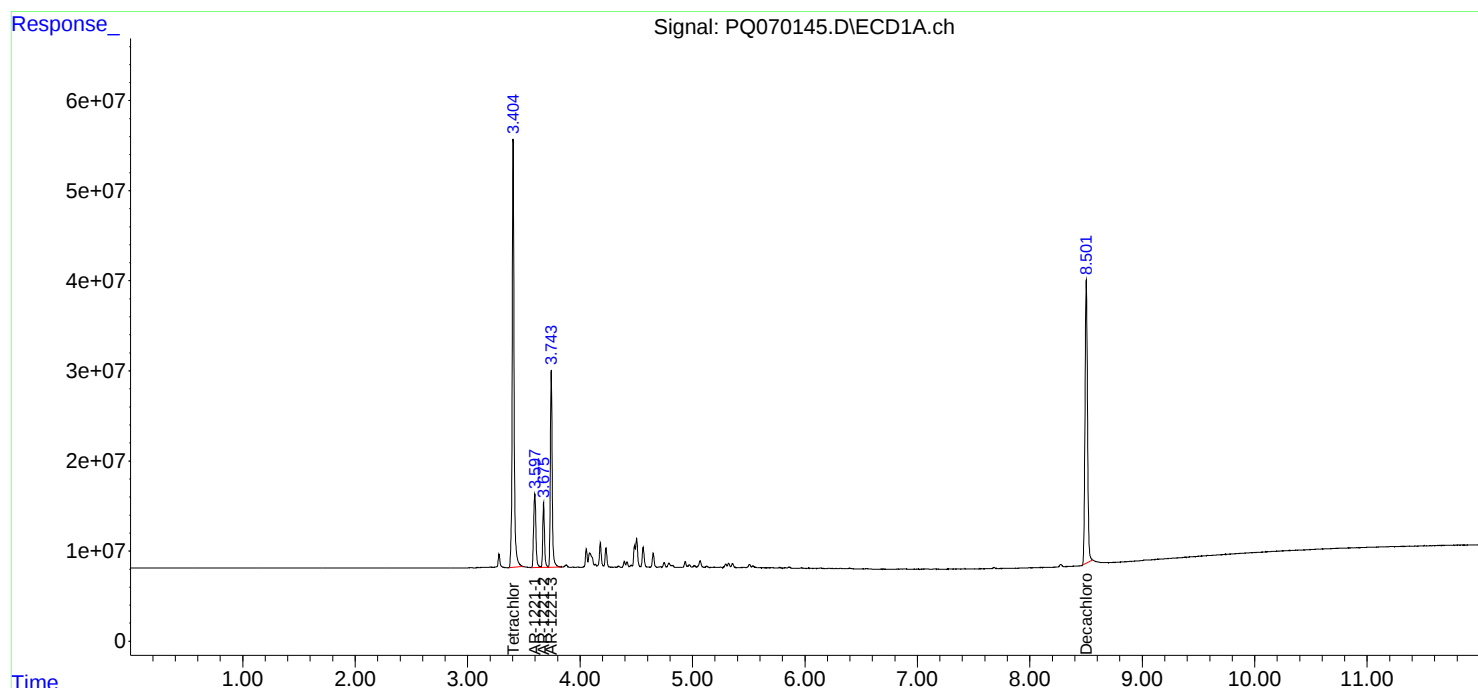

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070146.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 12:07
 Operator : YP\AJ
 Sample : AR1232ICC100
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12321048

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 13:02:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 13:01:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.783	44856927	40436329	5.510	5.419
2) SA Decachlor...	8.502	7.546	39341396	67043512	10.815	11.071
Target Compounds						
11) L3 AR-1232-1	3.743	3.128	17806642	18850703	110.269	109.867
12) L3 AR-1232-2	4.231	3.801	10358451	18630253	113.455	110.102
13) L3 AR-1232-3	4.503	3.961	18202428	10235473	109.525	111.860
14) L3 AR-1232-4	4.651	4.047	9464571	9000015	111.157	113.050
15) L3 AR-1232-5	4.748	4.204	6310138	10227841	111.771	114.650



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070146.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 12:07
Operator : YP\AJ
Sample : AR1232ICC100
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12321048

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 13:02:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 13:01:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

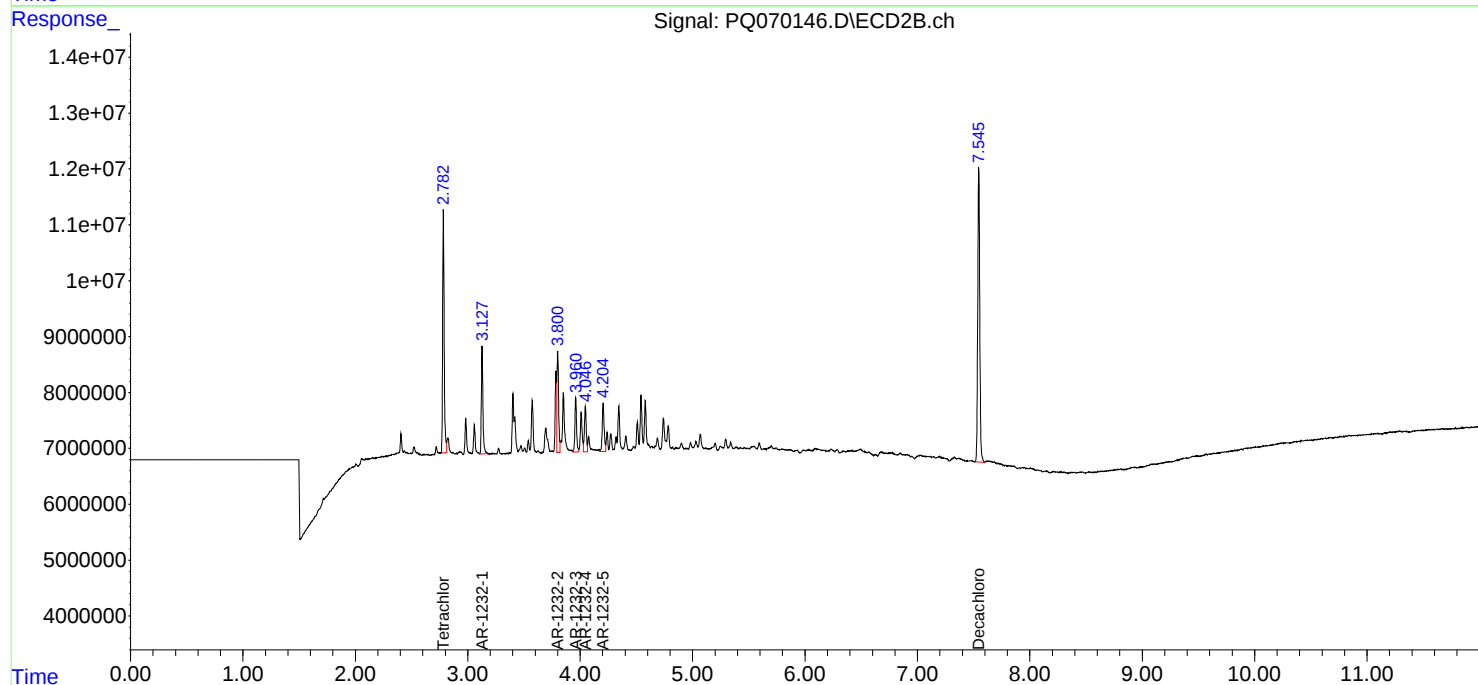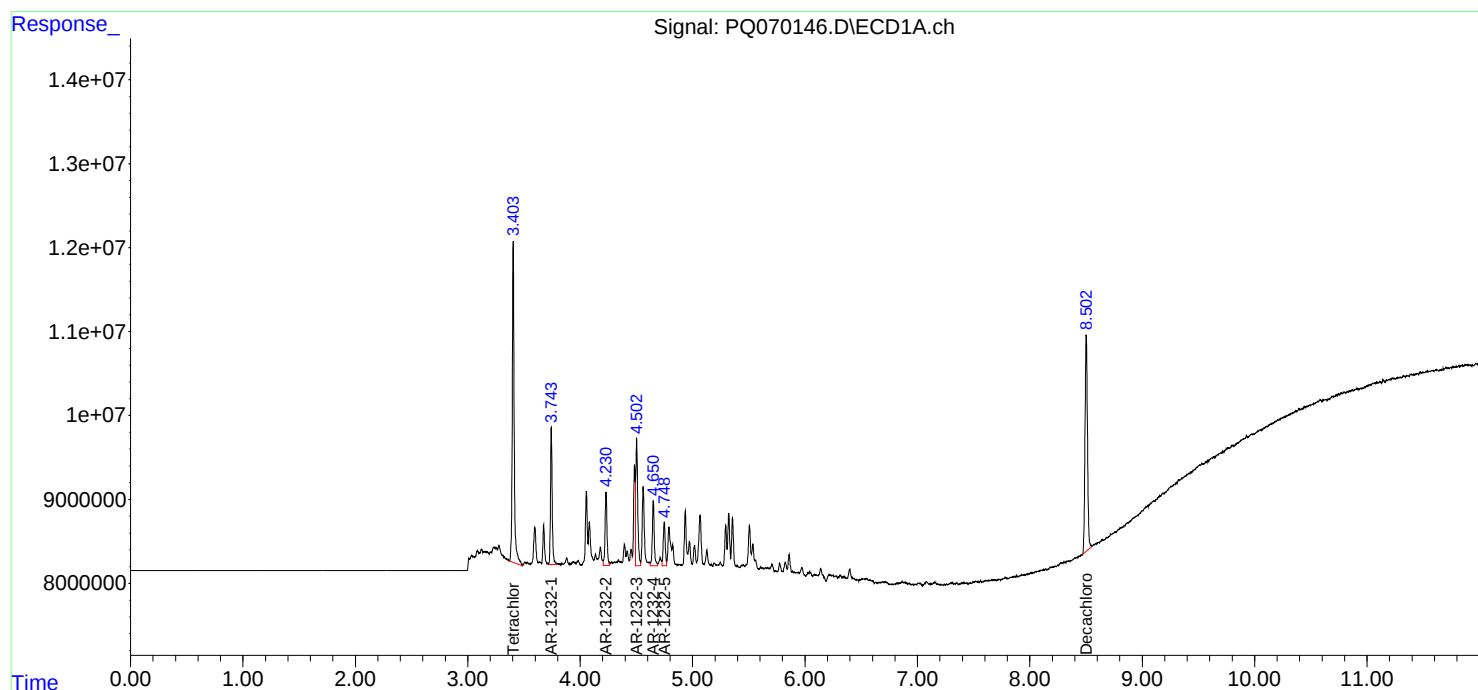

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070147.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 12:21
 Operator : YP\AJ
 Sample : AR1232ICC200
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12322049

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 12:59:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 12:58:56 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.405	2.783	80523674	74614219	10.422	10.436
2) SA Decachlor...	8.502	7.546	71755286	118.5E6	20.564	20.678
Target Compounds						
11) L3 AR-1232-1	3.744	3.127	31802291	34652211	207.598	212.444
12) L3 AR-1232-2	4.231	3.801	17801800	33692083	209.044	209.708
13) L3 AR-1232-3	4.503	3.961	32928986	17951215	208.044	208.550
14) L3 AR-1232-4	4.651	4.047	16526388	15491026	205.562	208.167
15) L3 AR-1232-5	4.748	4.205	10869745	17214870	204.577	208.225



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070147.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 12:21
Operator : YP\AJ
Sample : AR1232ICC200
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12322049

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 12:59:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 12:58:56 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

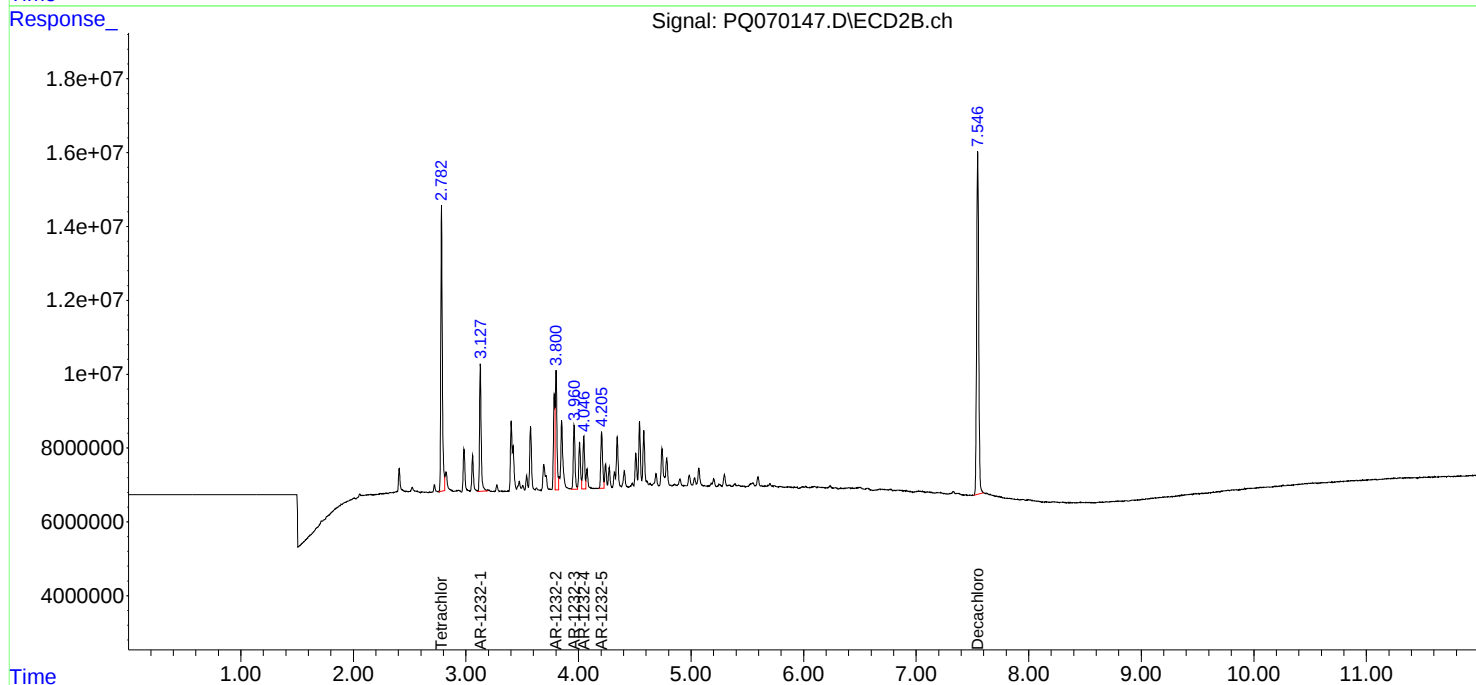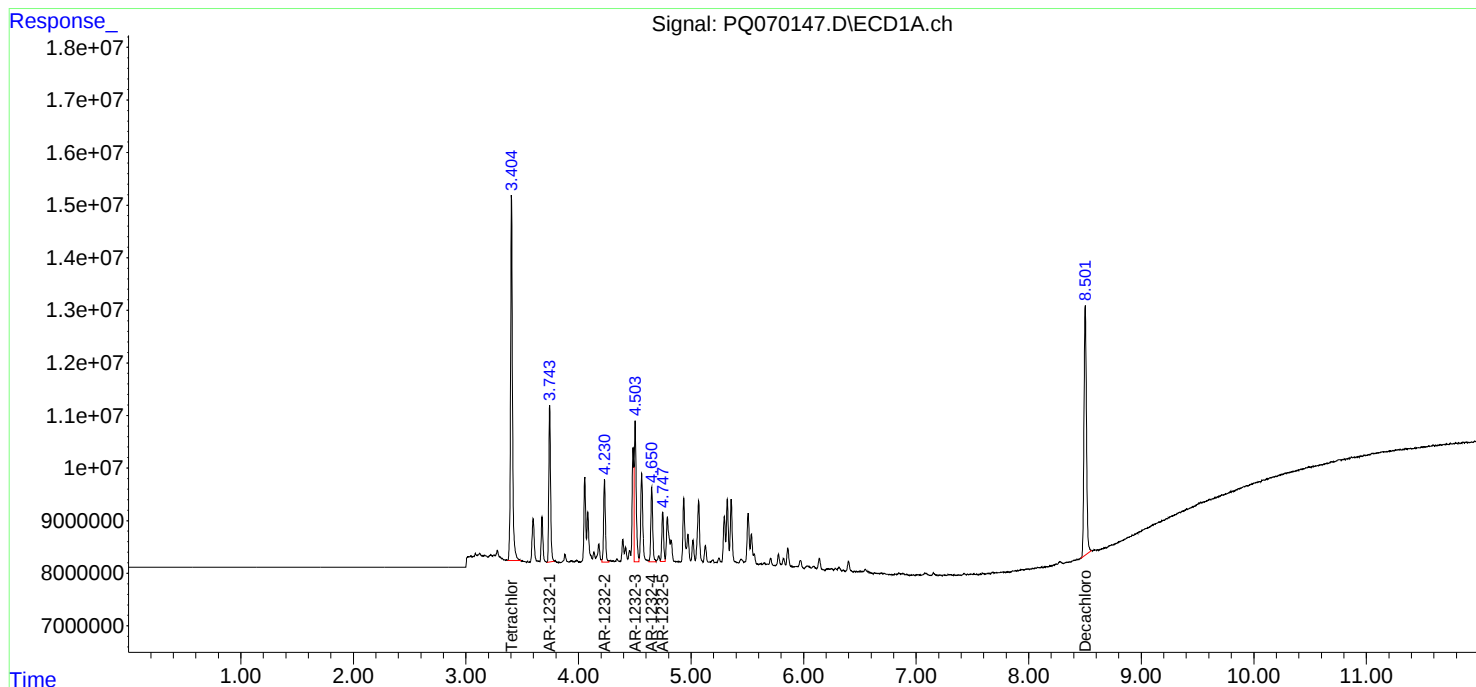

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070148.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 12:36
 Operator : YP\AJ
 Sample : AR1232ICC400
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12323050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 12:56:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 12:55:52 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.783	148.0E6	136.8E6	20.000	20.000
2) SA Decachlor...	8.502	7.547	135.6E6	221.5E6	40.000	40.000
Target Compounds						
11) L3 AR-1232-1	3.743	3.127	58948831	61185600	400.000	400.000
12) L3 AR-1232-2	4.231	3.801	32522994	61145442	400.000	400.000
13) L3 AR-1232-3	4.504	3.961	60765005	32958552	400.000	400.000
14) L3 AR-1232-4	4.651	4.047	31264113	28551120	400.000	400.000
15) L3 AR-1232-5	4.748	4.205	20766808	31709891	400.000	400.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070148.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 12:36
Operator : YP\AJ
Sample : AR1232ICC400
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12323050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 12:56:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 12:55:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

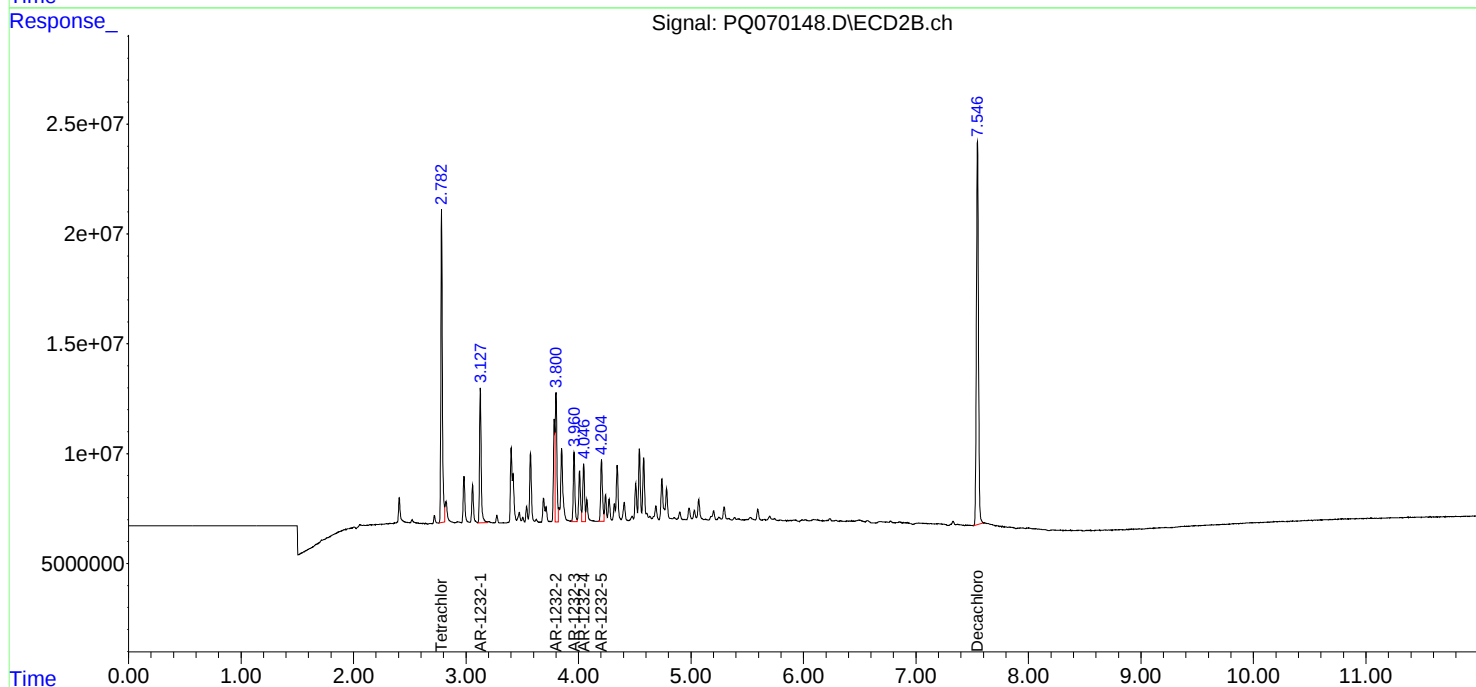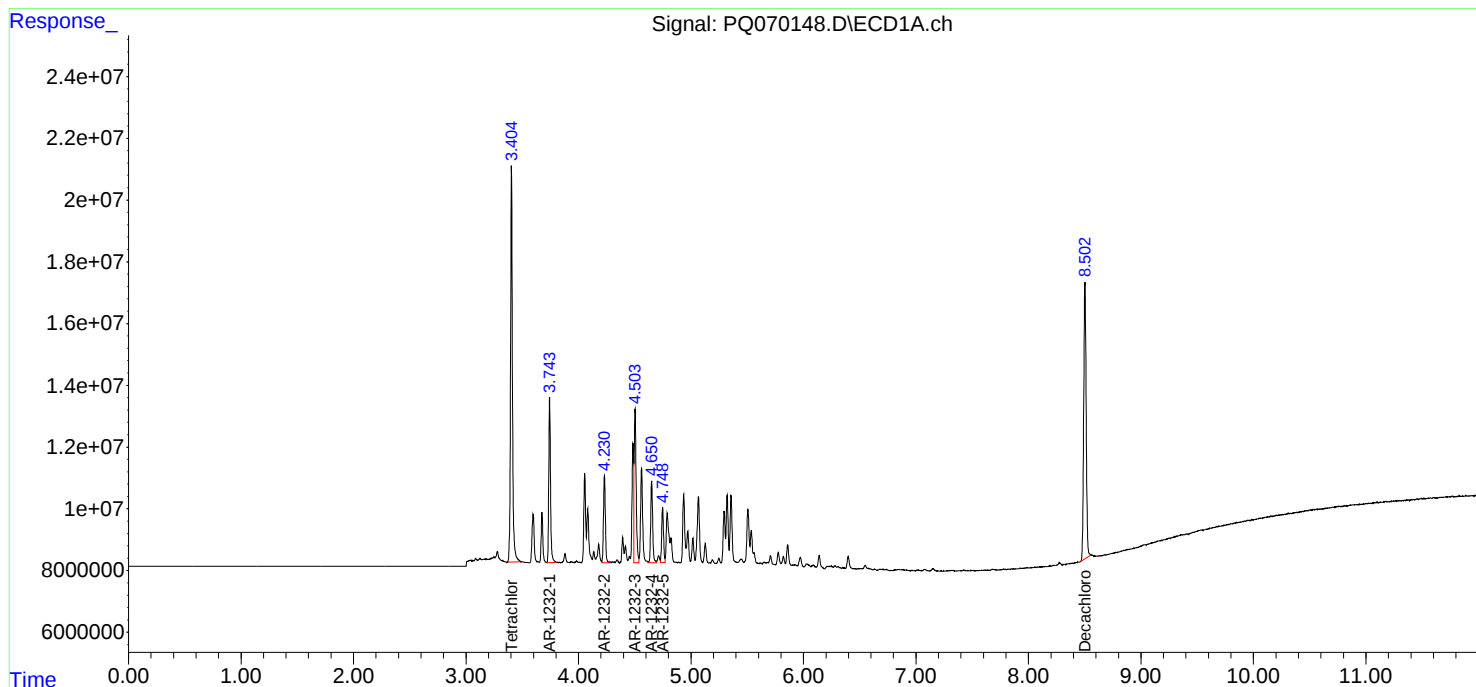

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070149.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 12:50
 Operator : YP\AJ
 Sample : AR1232ICC800
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12324001

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 13:28:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 13:28:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.405	2.783	279.2E6	258.2E6	35.559	35.812
2) SA Decachlor...	8.502	7.546	254.5E6	412.2E6	72.236	70.702
Target Compounds						
11) L3 AR-1232-1	3.744	3.127	109.1E6	111.1E6	702.903	679.688
12) L3 AR-1232-2	4.231	3.800	59801624	111.8E6	686.088	690.842
13) L3 AR-1232-3	4.503	3.961	112.9E6	60905500	705.844	694.794
14) L3 AR-1232-4	4.651	4.046	57231912	51897283	700.132	683.523
15) L3 AR-1232-5	4.749	4.204	38296619	57734456	705.155	679.638



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070149.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 12:50
Operator : YP\AJ
Sample : AR1232ICC800
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12324001

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 13:28:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 13:28:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

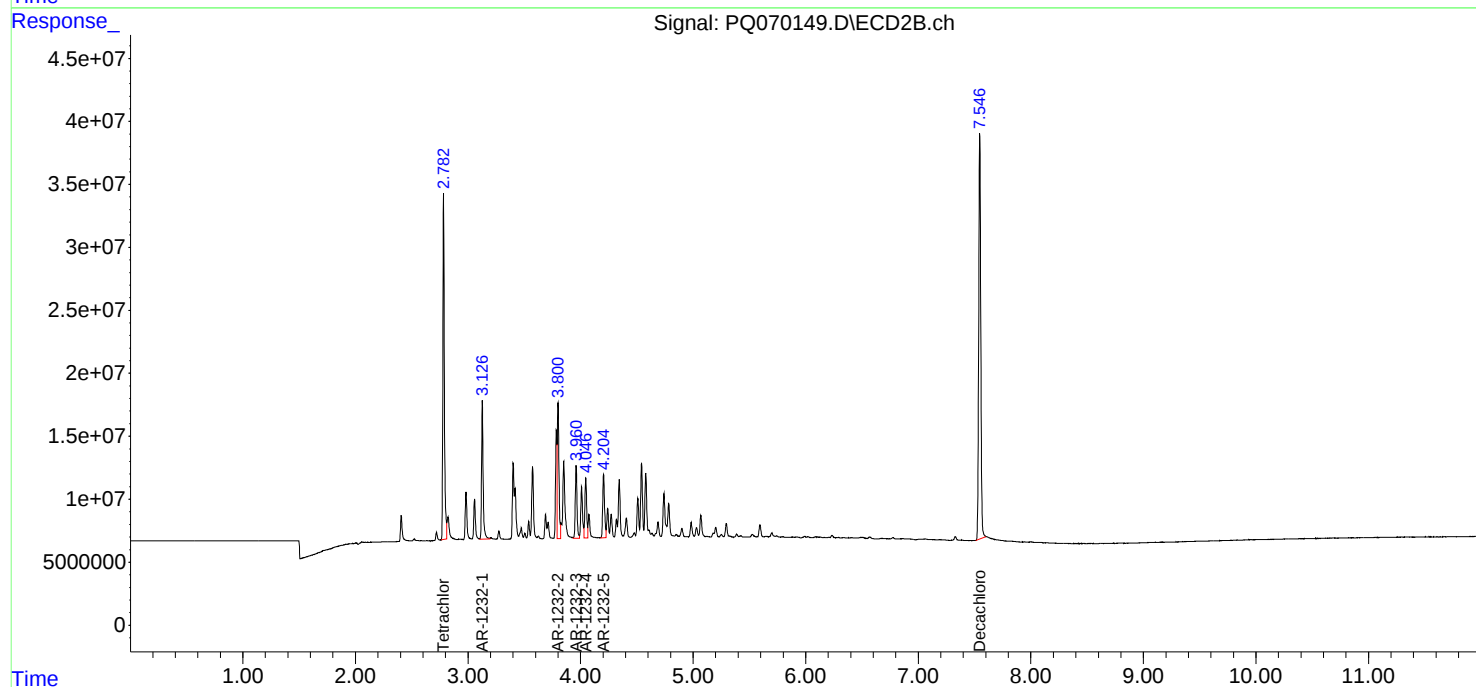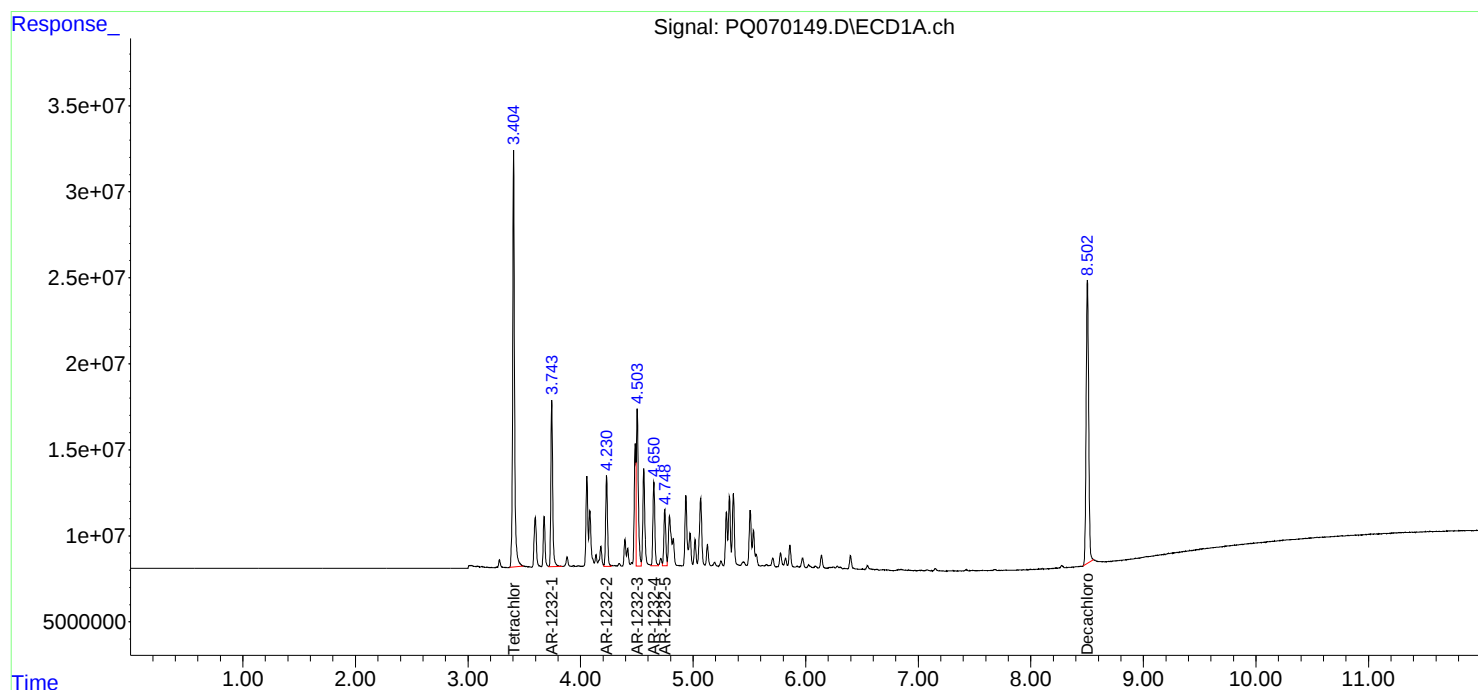

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070150.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 13:05
 Operator : YP\AJ
 Sample : AR1232ICC1600
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12325002

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 13:30:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 13:30:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.783	536.5E6	495.0E6	70.390	70.652
2) SA Decachlor...	8.502	7.547	488.9E6	786.4E6	142.545	139.270
Target Compounds						
11) L3 AR-1232-1	3.743	3.127	200.1E6	201.1E6	1341.638	1290.275
12) L3 AR-1232-2	4.230	3.801	111.9E6	209.6E6	1336.250	1346.633
13) L3 AR-1232-3	4.503	3.961	212.4E6	112.5E6	1374.946	1336.226
14) L3 AR-1232-4	4.650	4.047	107.8E6	94856296	1366.577	1306.597
15) L3 AR-1232-5	4.748	4.205	71516687	106.6E6	1365.157	1311.521



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070150.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 13:05
Operator : YP\AJ
Sample : AR1232ICC1600
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12325002

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 13:30:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 13:30:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

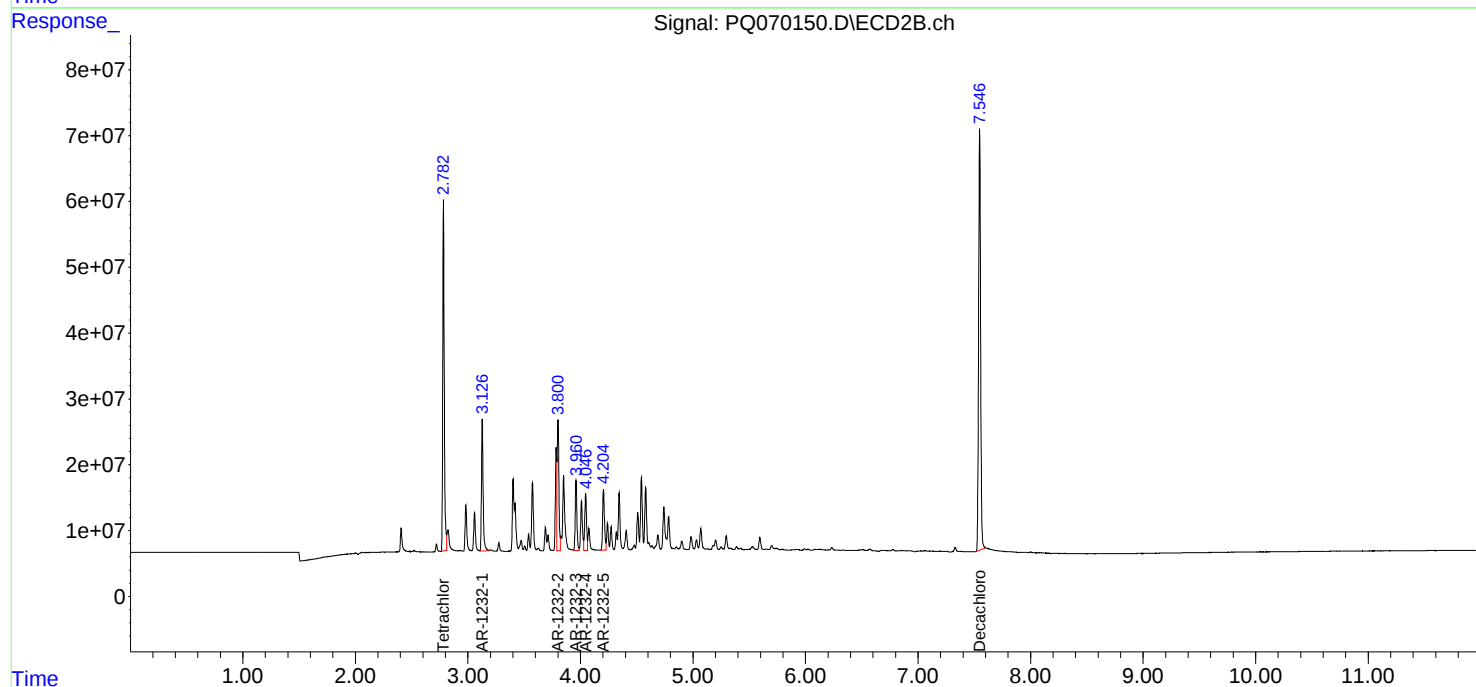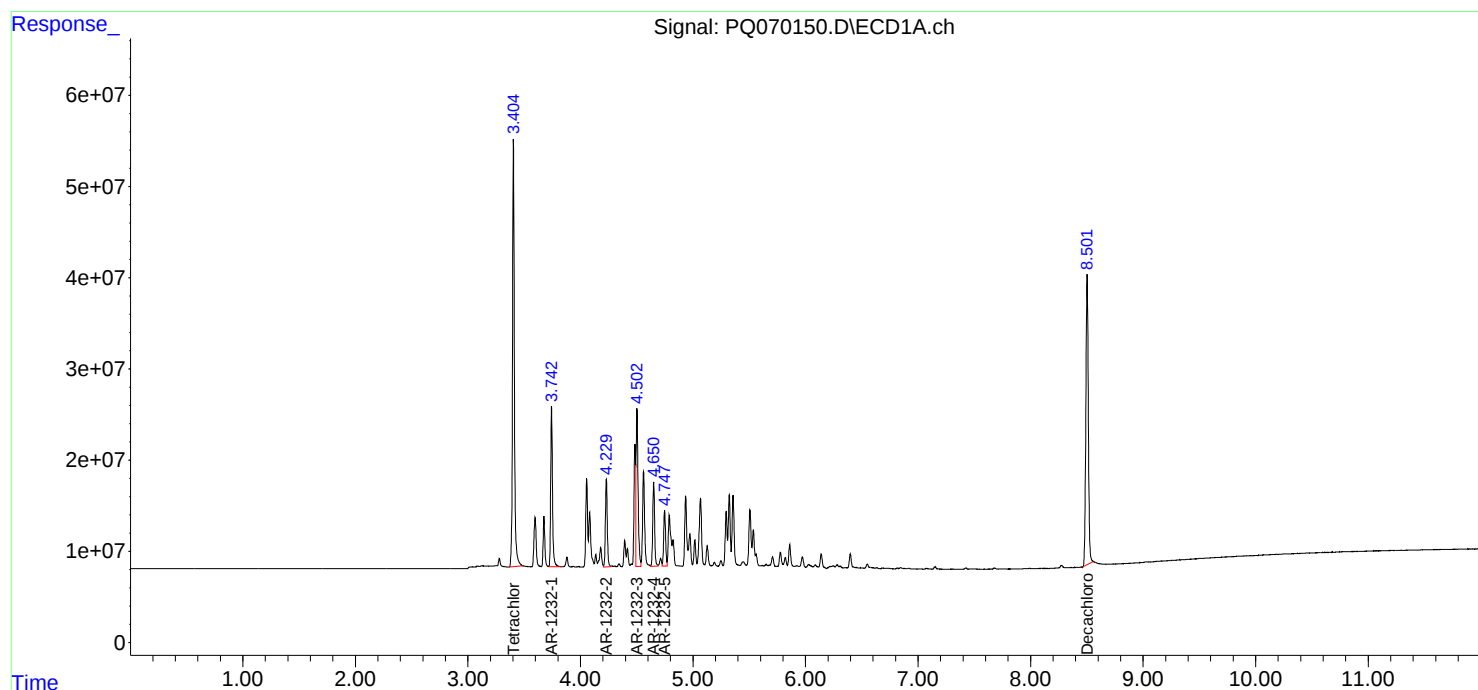

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070151.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 13:19
 Operator : YP\AJ
 Sample : AR1242ICC100
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12421003

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 14:13:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 14:07:03 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.783	42253357	40882224	5.279	5.356
2) SA Decachlor...	8.502	7.546	38831026	66566278	10.606	10.870
Target Compounds						
16) L4 AR-1242-1	4.484	3.785	21360308	22639999	108.736	111.401
17) L4 AR-1242-2	4.503	3.801	32830768	33501436	108.233	110.270
18) L4 AR-1242-3	4.561	3.961	21005591	18512869	108.840	110.014
19) L4 AR-1242-4	4.651	4.047	16979463	17676769	108.795	110.189
20) L4 AR-1242-5	5.356	4.542	15556172	22121669	104.527	109.641



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070151.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 13:19
Operator : YP\AJ
Sample : AR1242ICC100
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12421003

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 14:13:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 14:07:03 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

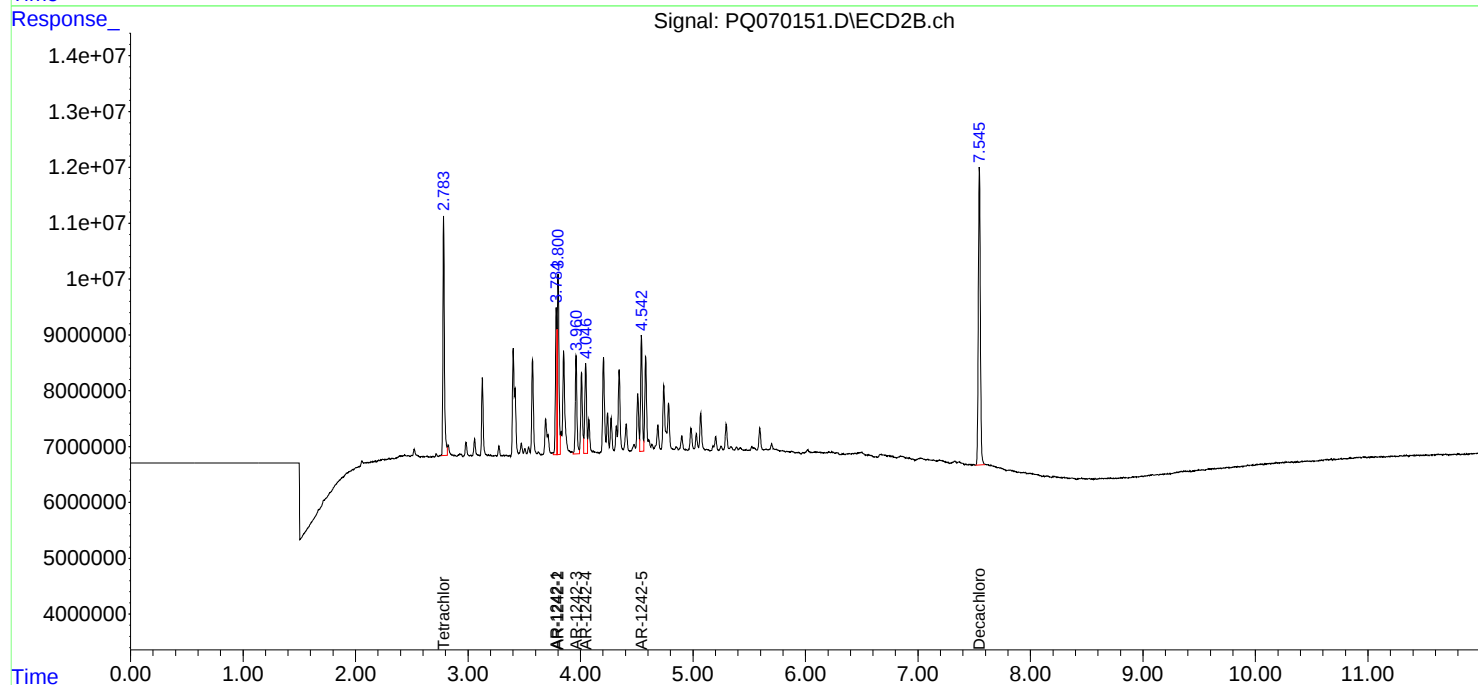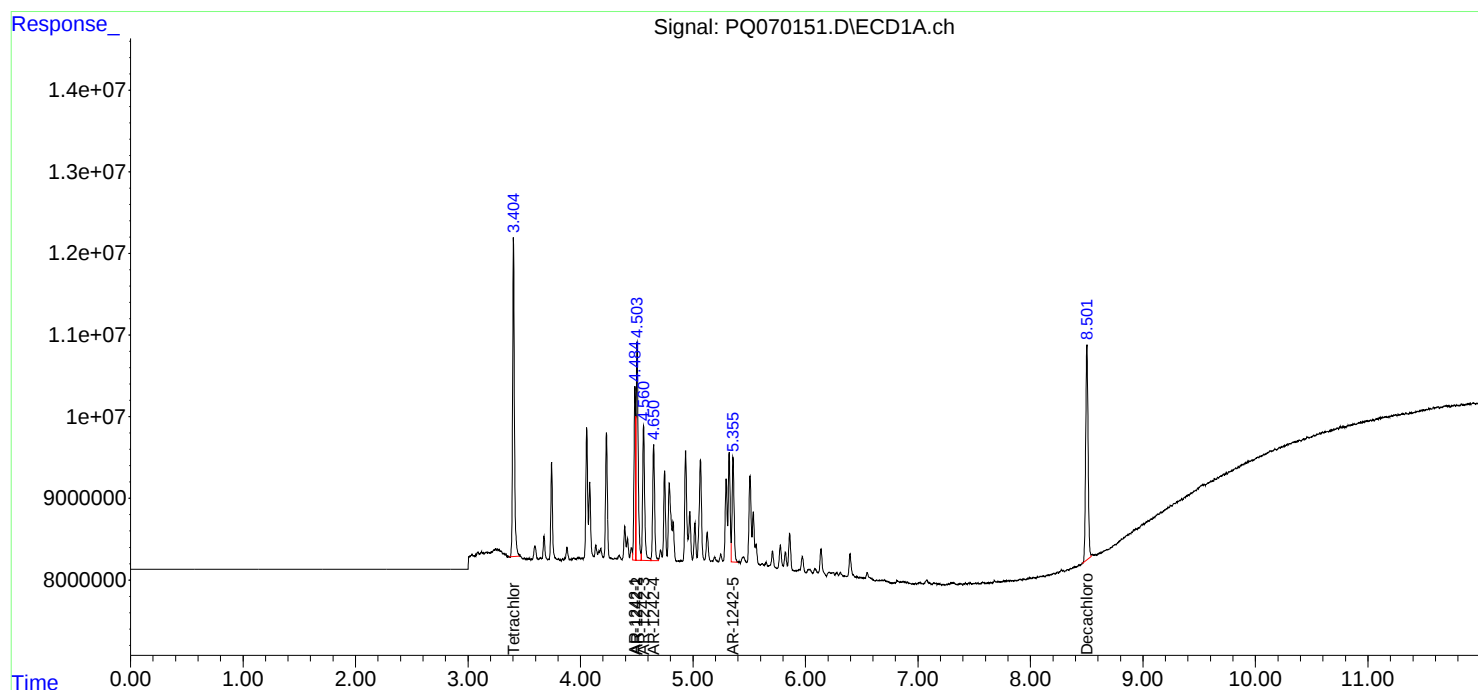

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070152.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 13:34
 Operator : YP\AJ
 Sample : AR1242ICC200
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12422004

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 14:09:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 14:07:03 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.405	2.783	80709608	77340700	10.372	10.506
2) SA Decachlor...	8.502	7.547	73730194	124.5E6	20.769	21.252
Target Compounds						
16) L4 AR-1242-1	4.485	3.785	39740795	41167524	211.543	214.813
17) L4 AR-1242-2	4.503	3.801	60561655	60832284	208.226	211.068
18) L4 AR-1242-3	4.562	3.961	38612496	34040773	209.322	212.951
19) L4 AR-1242-4	4.651	4.047	30989938	32586823	207.701	214.034
20) L4 AR-1242-5	5.357	4.542	30082009	40999638	206.812	213.498



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070152.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 13:34
Operator : YP\AJ
Sample : AR1242ICC200
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12422004

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 14:09:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 14:07:03 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

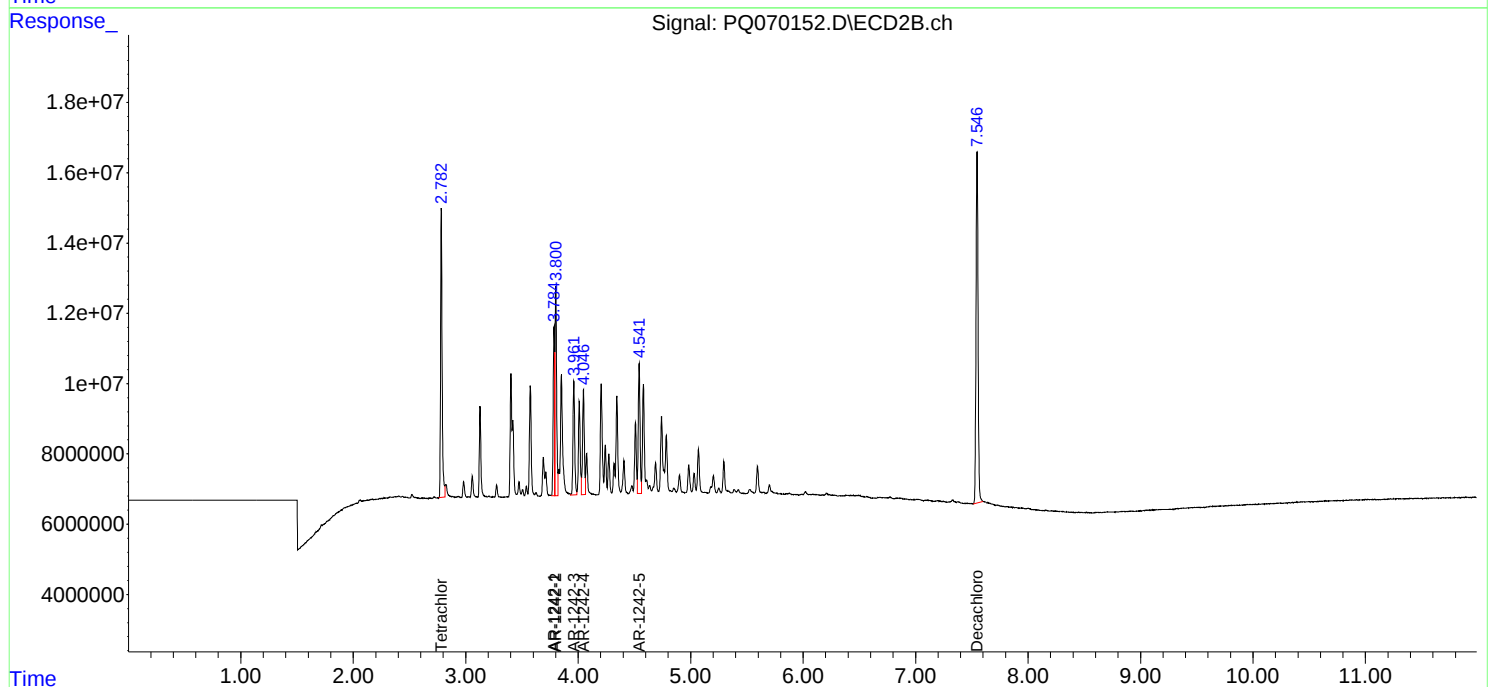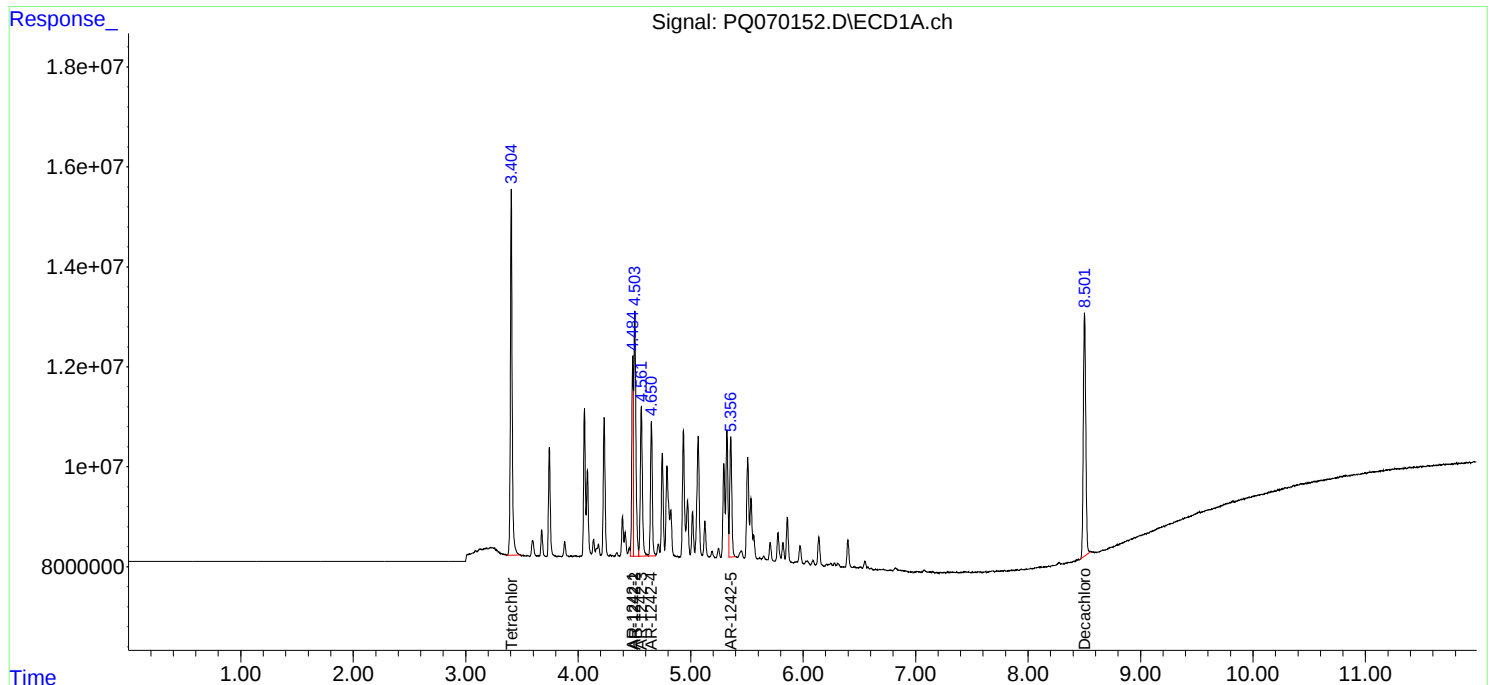

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070153.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 13:49
 Operator : YP\AJ
 Sample : AR1242ICC400
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12423005

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 14:07:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 14:07:03 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.783	149.8E6	139.8E6	20.000	20.000
2) SA Decachlor...	8.502	7.546	136.5E6	219.6E6	40.000	40.000
Target Compounds						
16) L4 AR-1242-1	4.485	3.785	70807416	70979677	400.000	400.000
17) L4 AR-1242-2	4.503	3.801	111.6E6	108.9E6	400.000	400.000
18) L4 AR-1242-3	4.561	3.961	70346365	59800661	400.000	400.000
19) L4 AR-1242-4	4.650	4.047	57383670	56626845	400.000	400.000
20) L4 AR-1242-5	5.356	4.542	56200494	71631018	400.000	400.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070153.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 13:49
Operator : YP\AJ
Sample : AR1242ICC400
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12423005

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 14:07:16 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 14:07:03 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

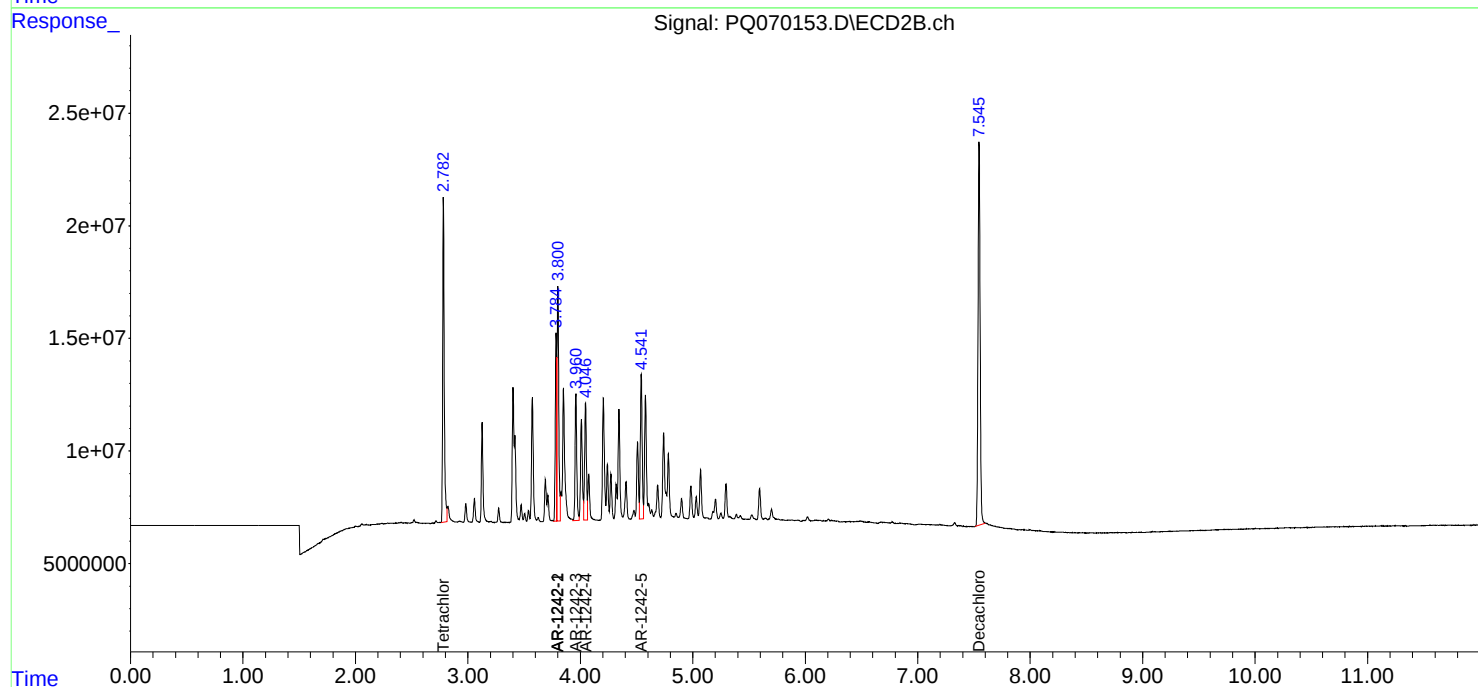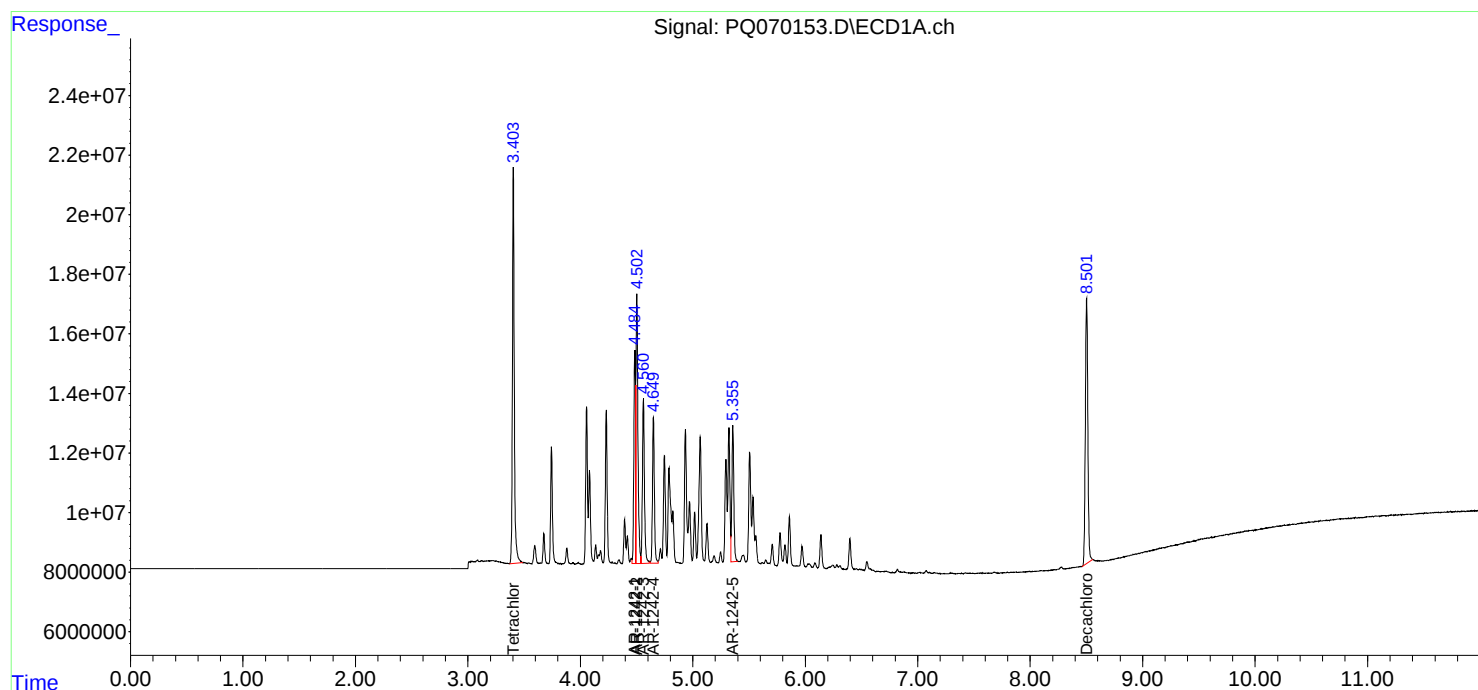

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070154.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 14:03
 Operator : YP\AJ
 Sample : AR1242ICC800
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12424006

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 14:20:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 14:07:03 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.783	281.4E6	261.6E6	36.251	35.544
2) SA Decachlor...	8.502	7.547	258.3E6	411.6E6	72.690	70.018
Target Compounds						
16) L4 AR-1242-1	4.484	3.785	131.2E6	129.0E6	696.541	669.182
17) L4 AR-1242-2	4.503	3.800	206.1E6	197.9E6	706.109	683.246
18) L4 AR-1242-3	4.561	3.961	130.7E6	110.0E6	704.227	684.914
19) L4 AR-1242-4	4.650	4.047	106.4E6	102.8E6	708.065	674.326
20) L4 AR-1242-5	5.357	4.542	104.5E6	130.8E6	724.525	680.350



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070154.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 14:03
Operator : YP\AJ
Sample : AR1242ICC800
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12424006

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 14:20:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 14:07:03 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

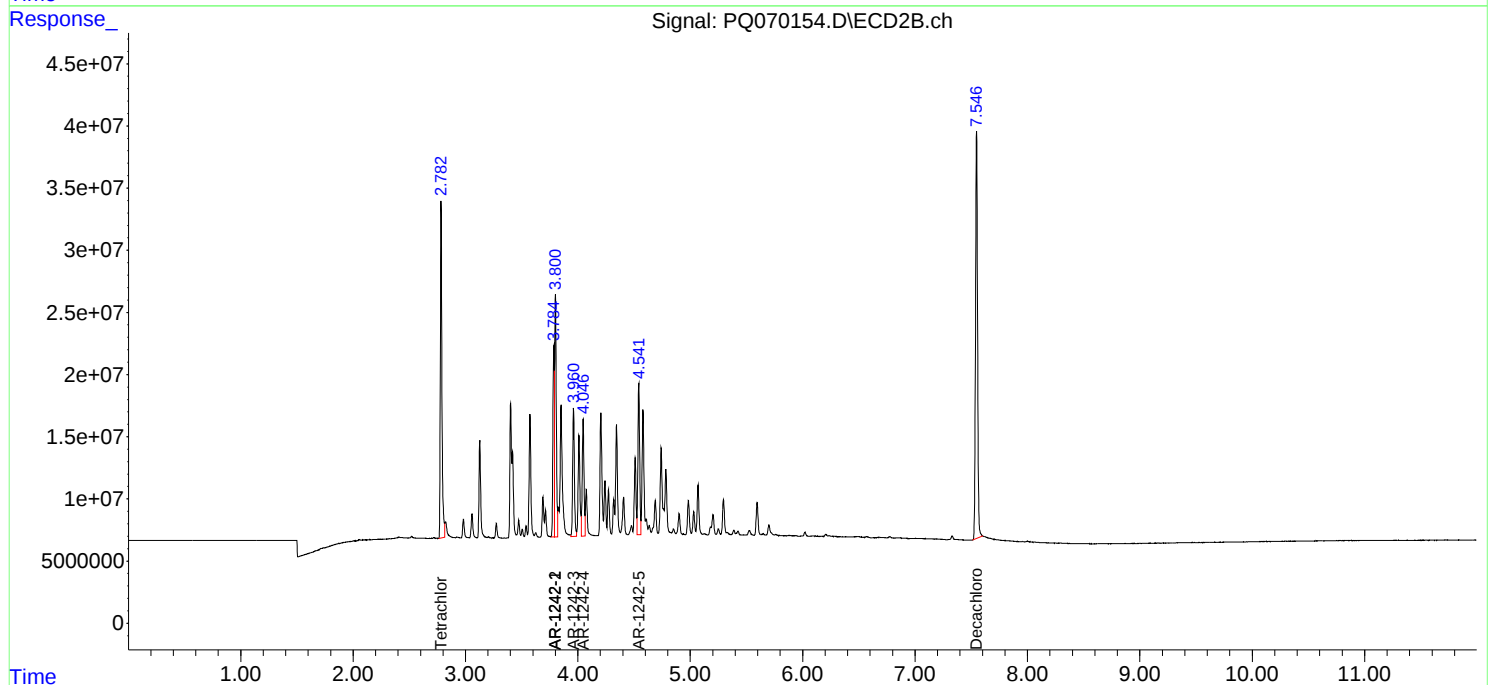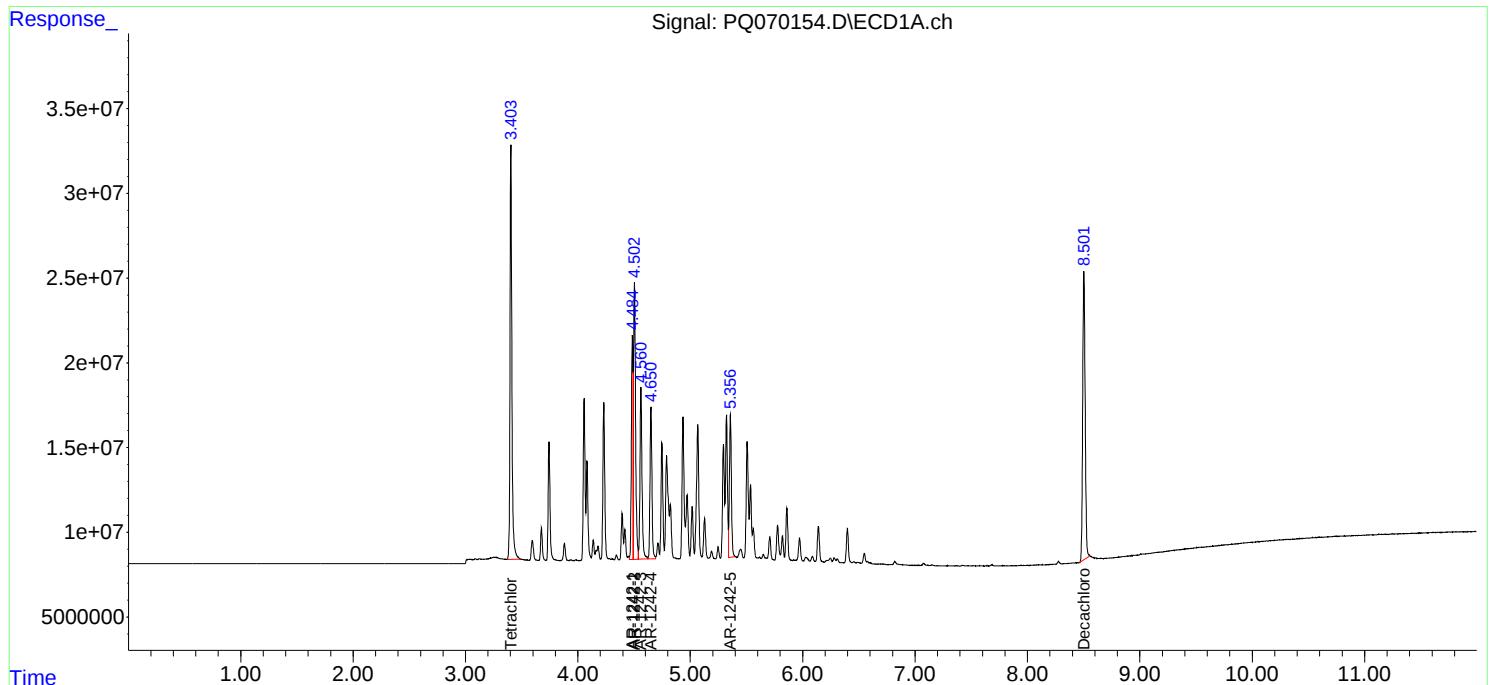

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070155.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 14:18
 Operator : YP\AJ
 Sample : AR1242ICC1600
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12425007

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 14:31:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 14:31:18 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.783	545.4E6	515.8E6	72.023	71.870
2) SA Decachlor...	8.502	7.546	501.5E6	809.0E6	144.555	141.566
Target Compounds						
16) L4 AR-1242-1	4.485	3.785	246.9E6	251.7E6	1360.109	1355.943
17) L4 AR-1242-2	4.503	3.800	398.9E6	388.1E6	1407.566	1384.769
18) L4 AR-1242-3	4.561	3.961	247.1E6	213.1E6	1377.795	1373.956
19) L4 AR-1242-4	4.651	4.047	203.2E6	195.3E6	1395.065	1334.393
20) L4 AR-1242-5	5.356	4.542	201.3E6	252.8E6	1431.791	1363.811



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070155.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 14:18
Operator : YP\AJ
Sample : AR1242ICC1600
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12425007

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 14:31:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 14:31:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

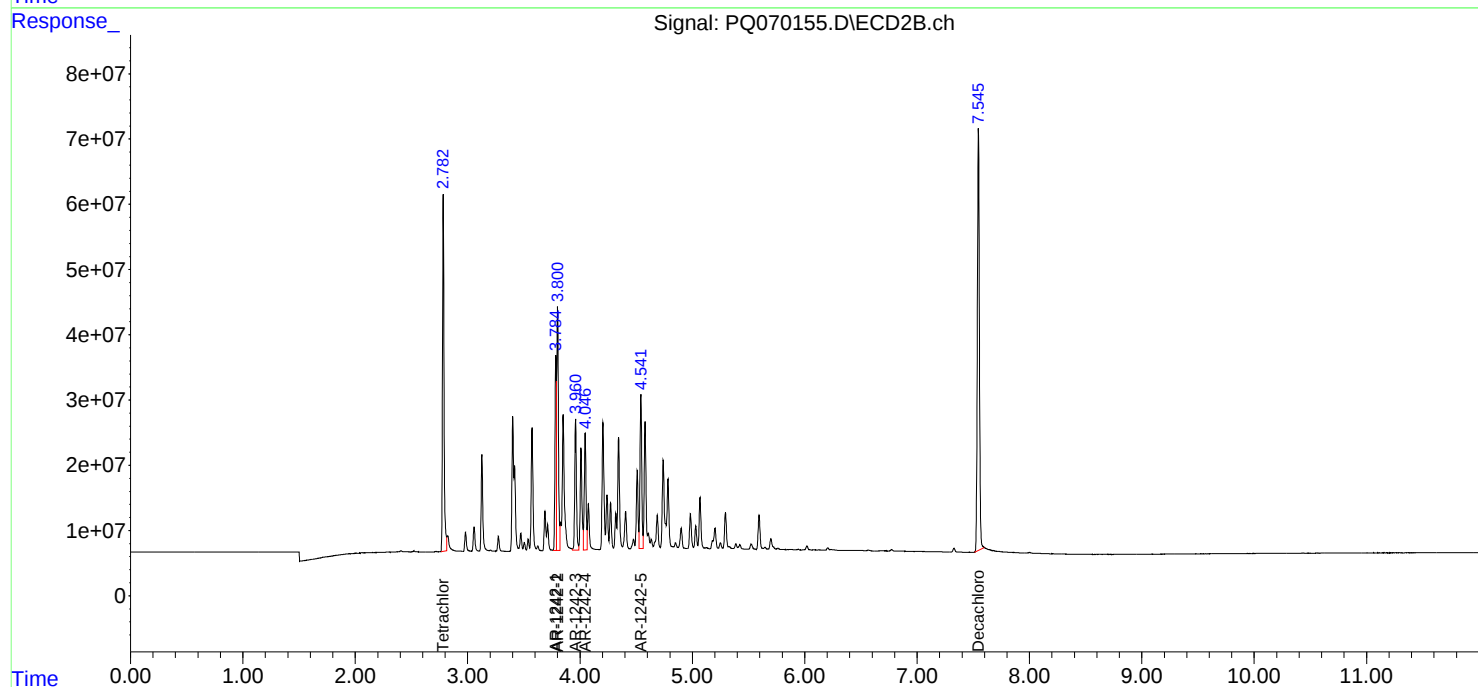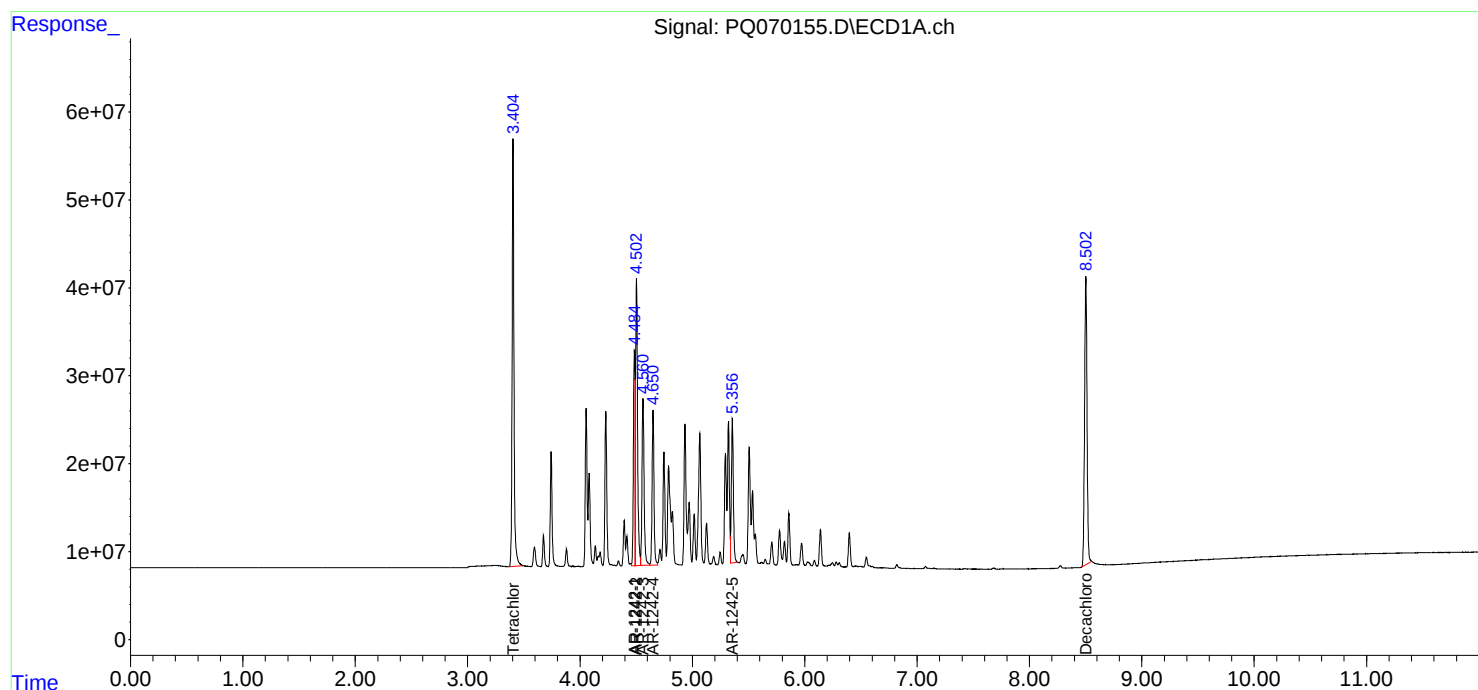

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070156.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 14:32
 Operator : YP\AJ
 Sample : AR1248ICC100
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12481008

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 15:18:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 15:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.783	44398041	42936616	5.510	5.497
2) SA Decachlor...	8.502	7.546	40579446	68218763	10.767	10.920
Target Compounds						
21) L5 AR-1248-1	4.484	3.785	16460589	17255135	110.659	112.335
22) L5 AR-1248-2	4.748	4.010	23380972	26559608	112.652	113.117
23) L5 AR-1248-3	4.935	4.047	27713860	25948779	111.721	113.446
24) L5 AR-1248-4	5.323	4.205	29004939	31620326	111.102	114.004
25) L5 AR-1248-5	5.357	4.580	27288953	30776163	110.409	113.322



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070156.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 14:32
Operator : YP\AJ
Sample : AR1248ICC100
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12481008

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 15:18:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 15:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

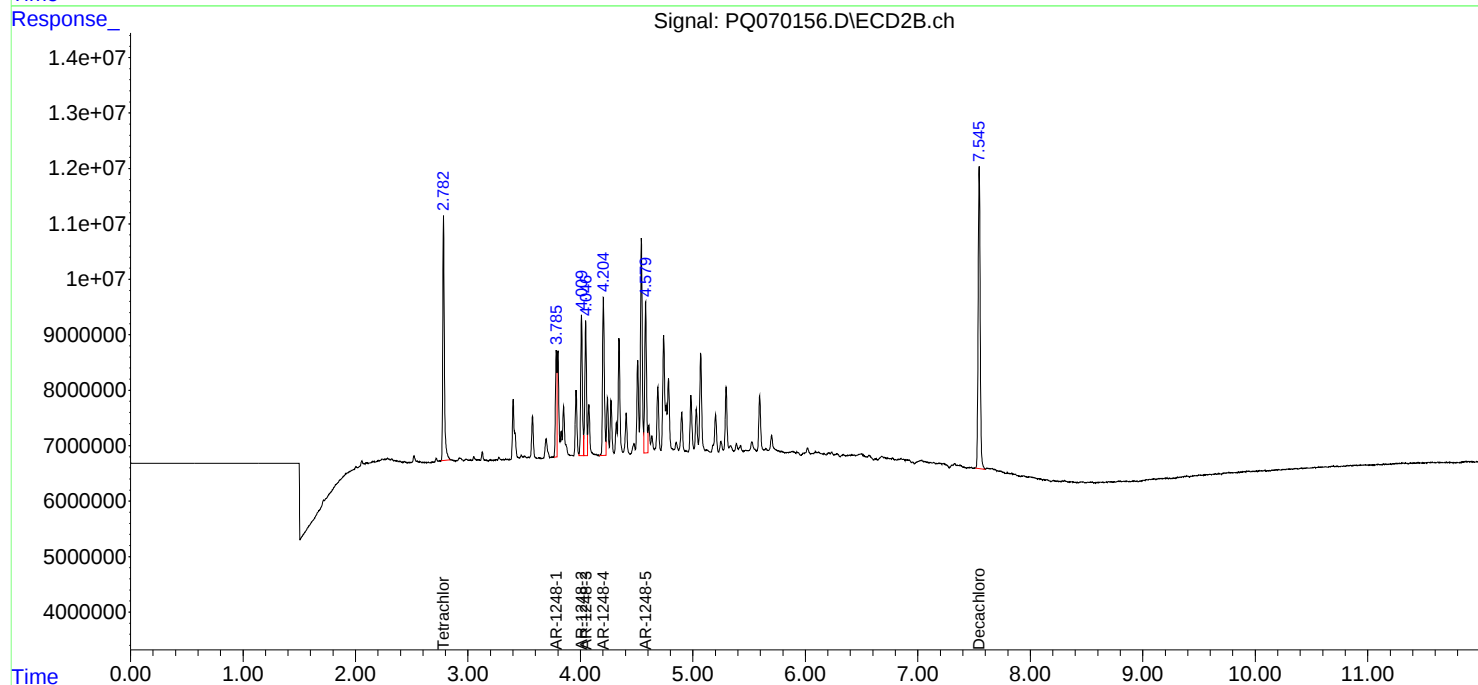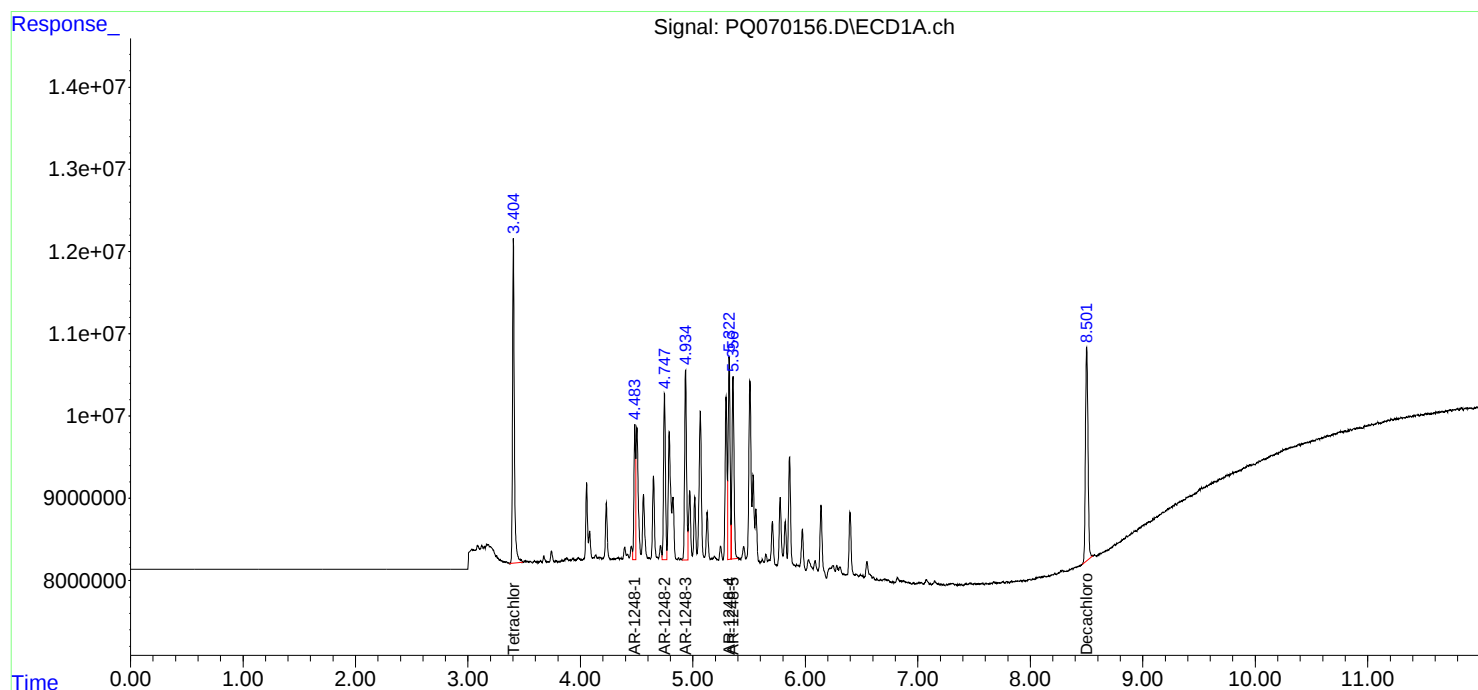

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070157.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 14:47
 Operator : YP\AJ
 Sample : AR1248ICC200
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12482009

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 15:16:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 15:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.405	2.783	79420578	76255093	10.385	10.273
2) SA Decachlor...	8.502	7.547	75694418	126.6E6	20.884	21.242
Target Compounds						
21) L5 AR-1248-1	4.485	3.785	29053308	30005306	206.311	208.182
22) L5 AR-1248-2	4.748	4.009	39900419	45382132	205.226	206.848
23) L5 AR-1248-3	4.936	4.047	48161322	44172985	206.236	207.041
24) L5 AR-1248-4	5.323	4.205	50668629	53178196	205.490	206.164
25) L5 AR-1248-5	5.356	4.579	46760853	52368916	199.579	206.591



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070157.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 14:47
Operator : YP\AJ
Sample : AR1248ICC200
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12482009

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 15:16:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 15:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

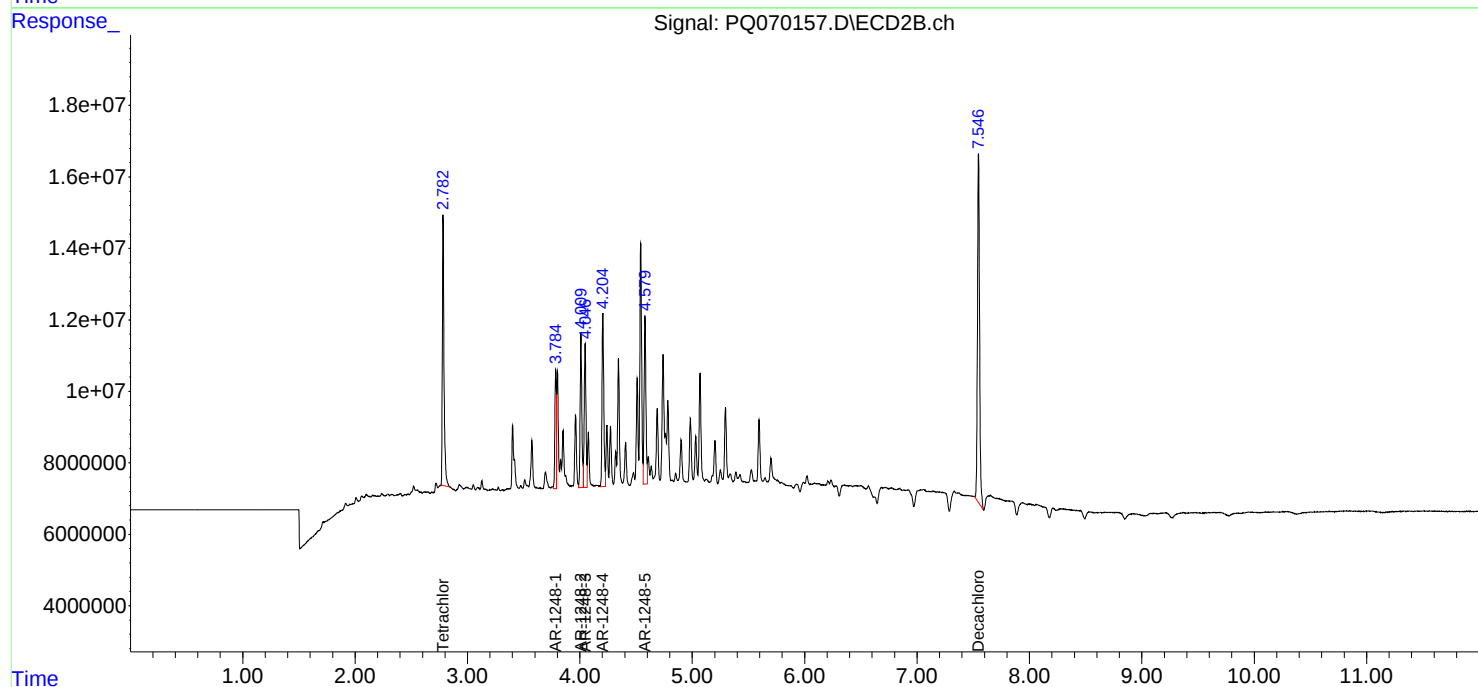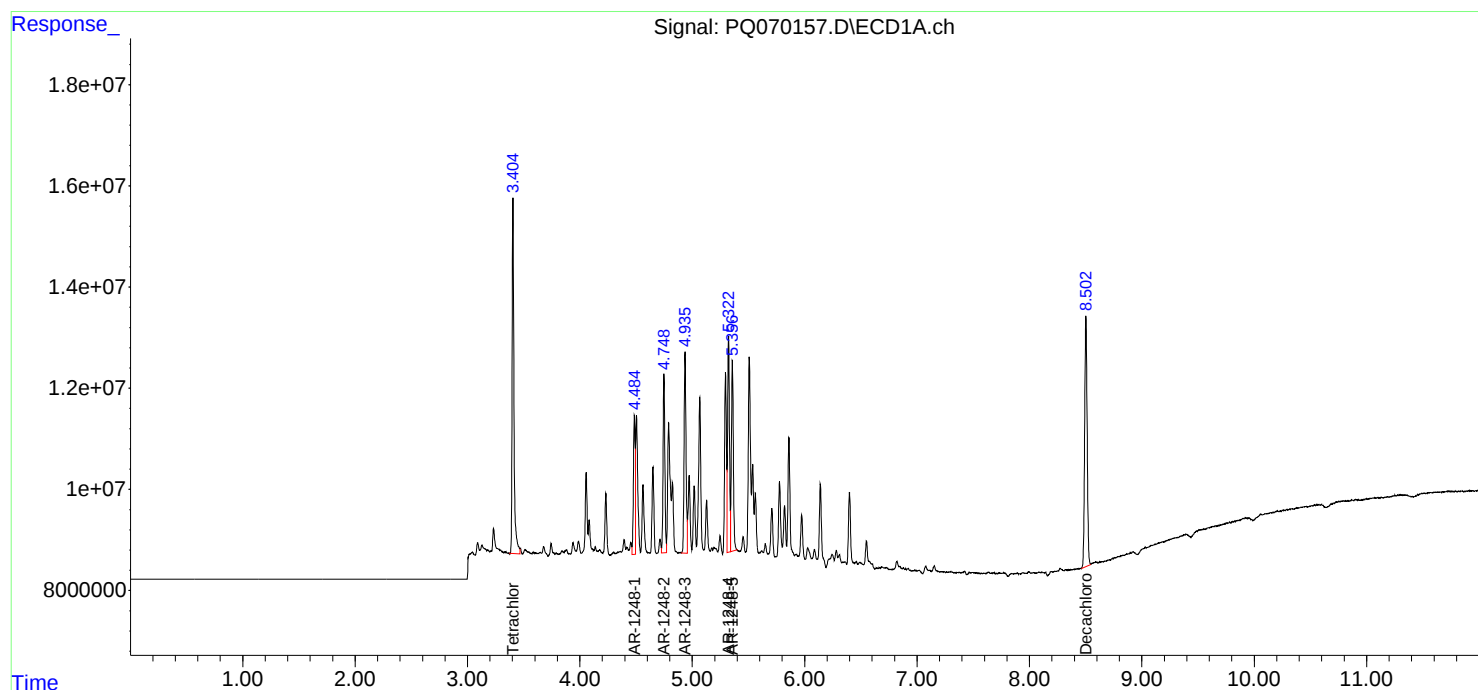

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070158.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 15:01
 Operator : YP\AJ
 Sample : AR1248ICC400
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12483010

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 15:13:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 15:13:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.782	147.1E6	144.4E6	20.000	20.000
2) SA Decachlor...	8.501	7.546	138.6E6	223.6E6	40.000	40.000
Target Compounds						
21) L5 AR-1248-1	4.484	3.784	54551467	55293579	400.000	400.000
22) L5 AR-1248-2	4.748	4.009	75736518	84754397	400.000	400.000
23) L5 AR-1248-3	4.935	4.046	90497943	82337298	400.000	400.000
24) L5 AR-1248-4	5.322	4.204	95922873	99996706	400.000	400.000
25) L5 AR-1248-5	5.357	4.579	93916291	98054967	400.000	400.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070158.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 15:01
Operator : YP\AJ
Sample : AR1248ICC400
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12483010

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 15:13:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 15:13:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

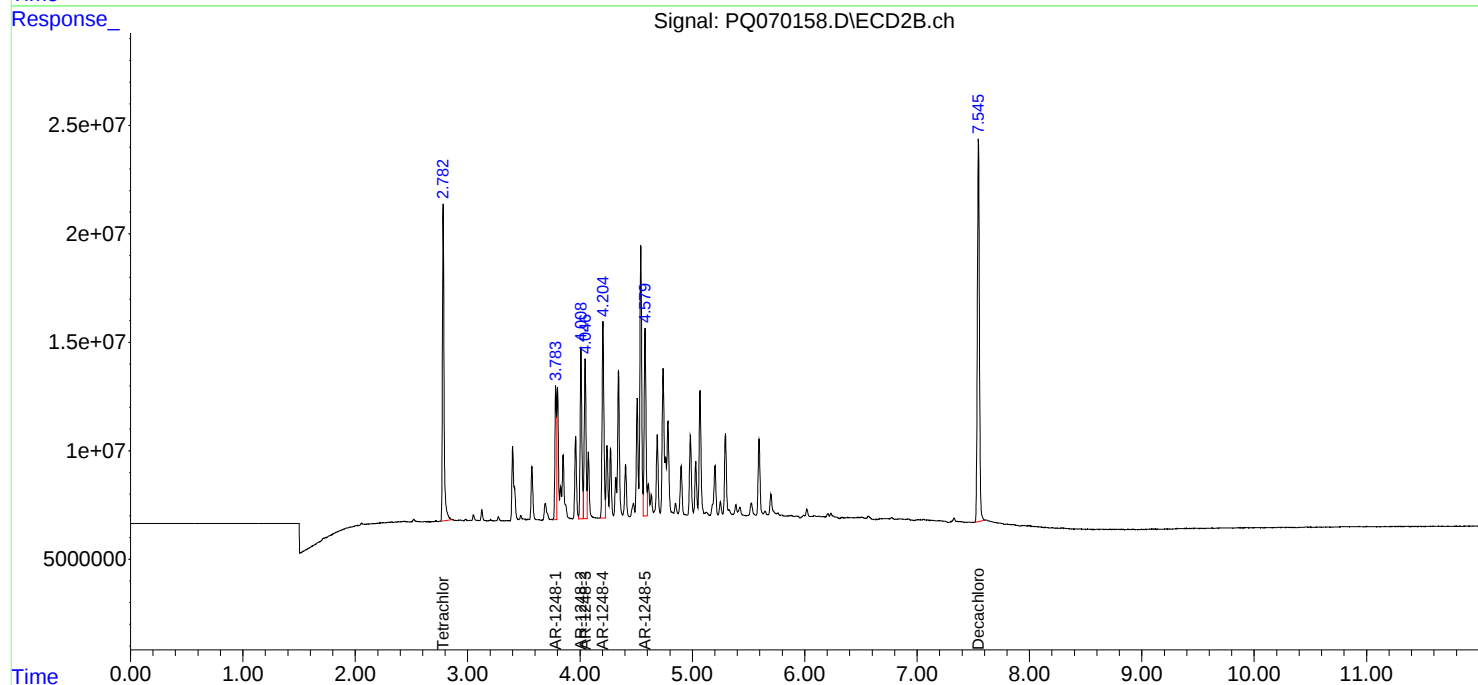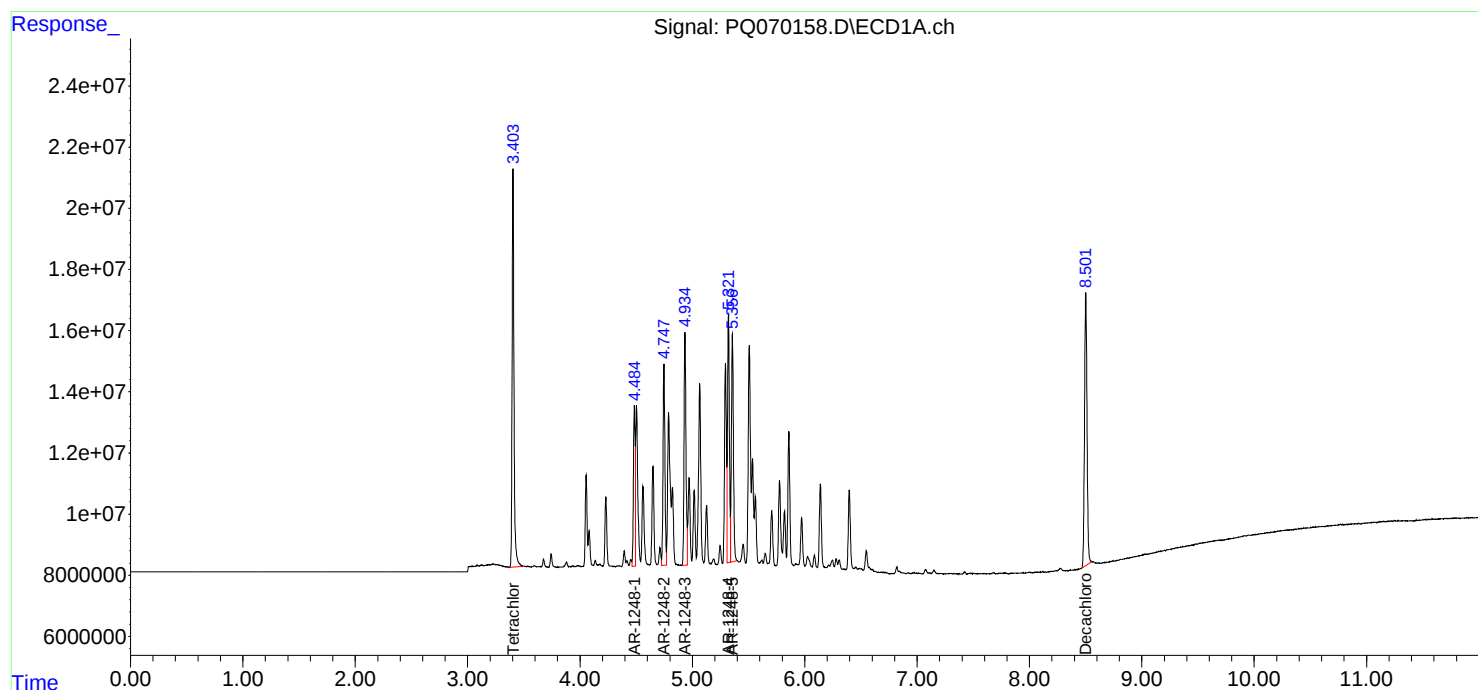

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070159.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 15:16
 Operator : YP\AJ
 Sample : AR1248ICC800
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12484011

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 15:27:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 15:27:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.783	274.0E6	267.6E6	35.332	35.533
2) SA Decachlor...	8.502	7.547	261.3E6	422.9E6	71.715	70.402
Target Compounds						
21) L5 AR-1248-1	4.484	3.785	100.6E6	100.1E6	703.350	683.379
22) L5 AR-1248-2	4.747	4.009	138.5E6	152.2E6	695.995	680.593
23) L5 AR-1248-3	4.935	4.047	166.5E6	148.1E6	699.219	679.904
24) L5 AR-1248-4	5.322	4.205	178.6E6	181.4E6	709.892	685.381
25) L5 AR-1248-5	5.356	4.579	173.3E6	178.8E6	723.610	688.724



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070159.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 15:16
Operator : YP\AJ
Sample : AR1248ICC800
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12484011

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 15:27:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 15:27:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

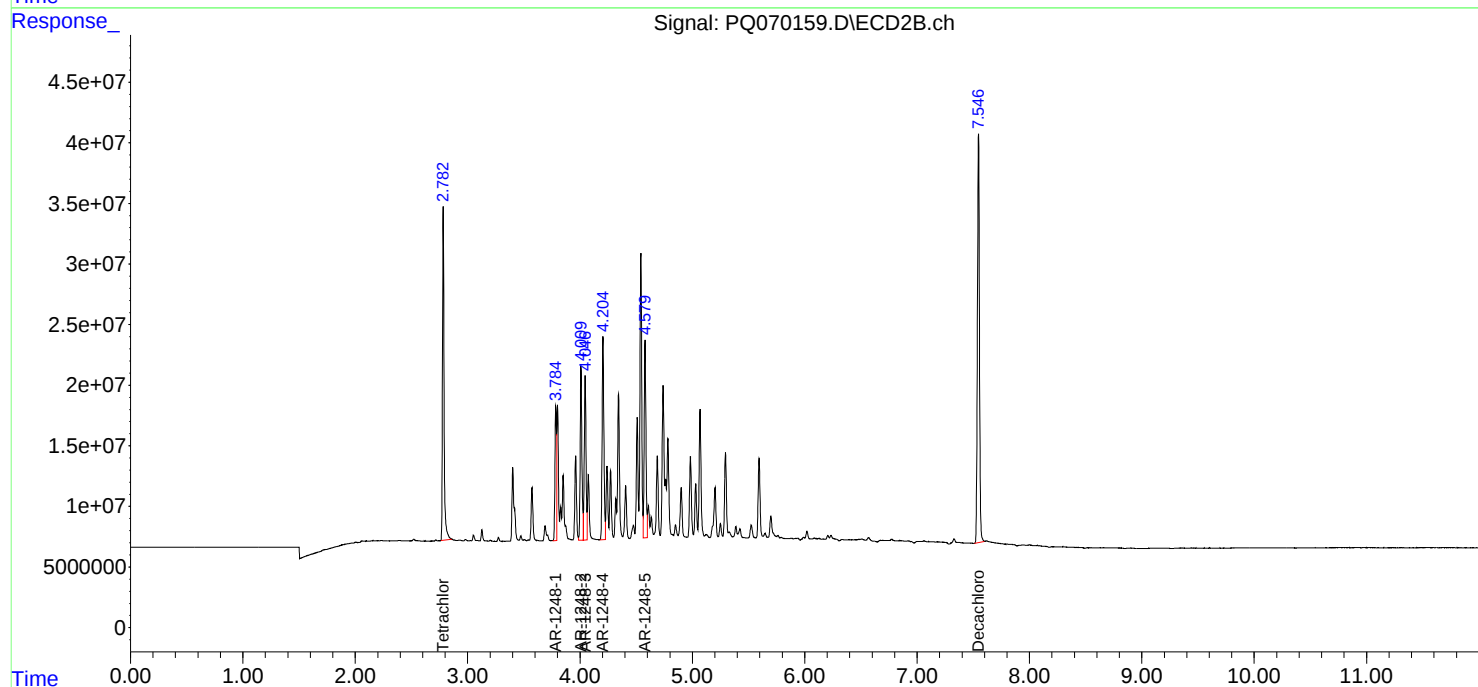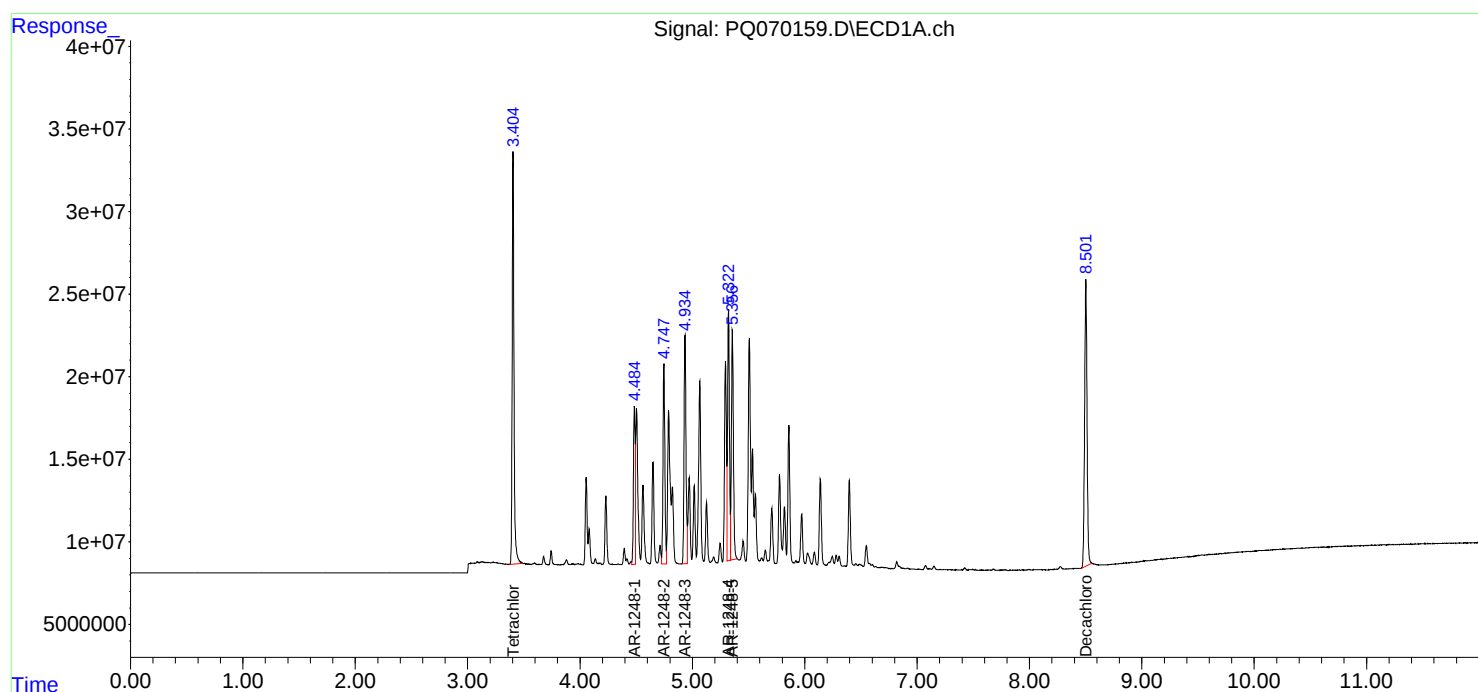

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070160.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 15:31
 Operator : YP\AJ
 Sample : AR1248ICC1600
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12485012

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 15:49:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 15:49:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.405	2.783	520.1E6	509.2E6	69.302	69.773
2) SA Decachlor...	8.502	7.546	498.2E6	783.2E6	140.838	135.391
Target Compounds						
21) L5 AR-1248-1	4.484	3.785	184.4E6	183.5E6	1341.427	1309.457
22) L5 AR-1248-2	4.748	4.010	253.6E6	278.9E6	1328.698	1304.623
23) L5 AR-1248-3	4.935	4.047	308.2E6	271.4E6	1346.123	1303.547
24) L5 AR-1248-4	5.322	4.205	334.9E6	335.0E6	1377.392	1320.682
25) L5 AR-1248-5	5.357	4.580	328.5E6	333.5E6	1411.855	1337.596



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070160.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 15:31
Operator : YP\AJ
Sample : AR1248ICC1600
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12485012

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 15:49:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 15:49:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

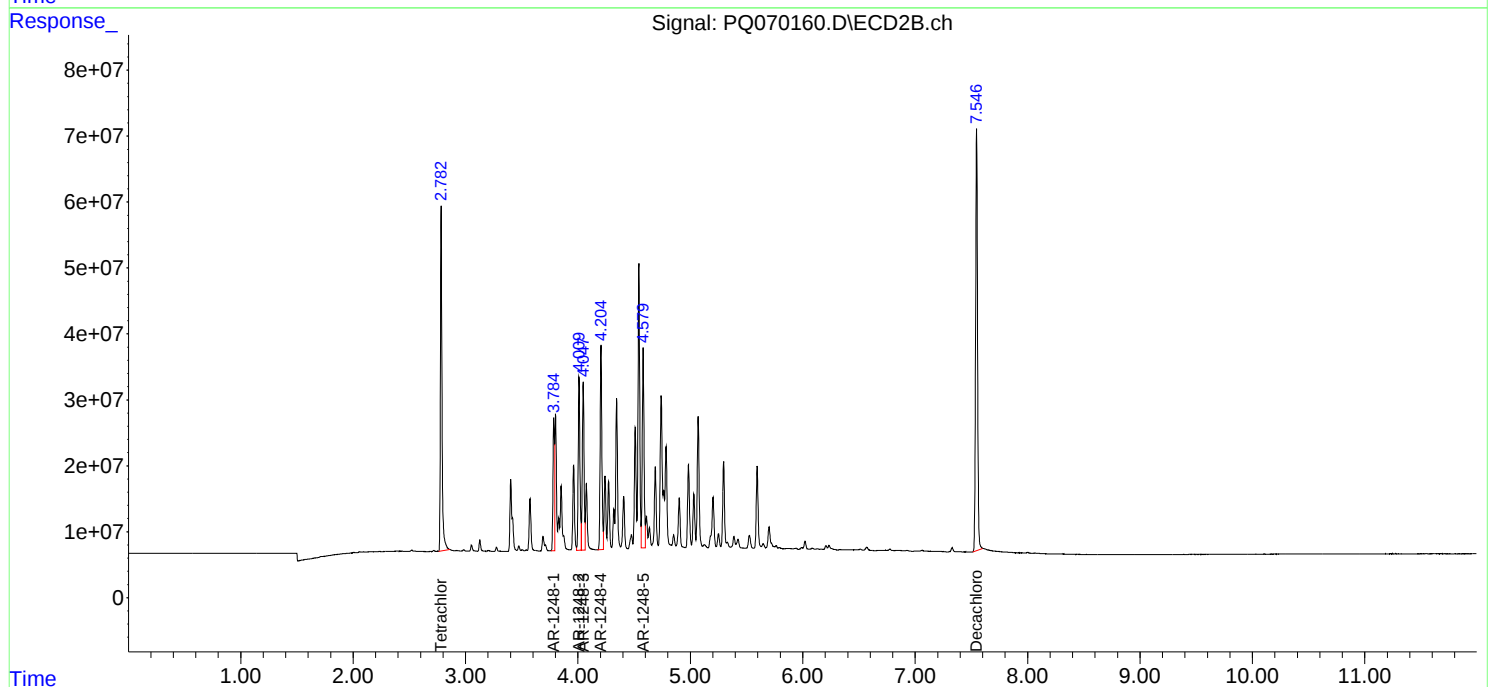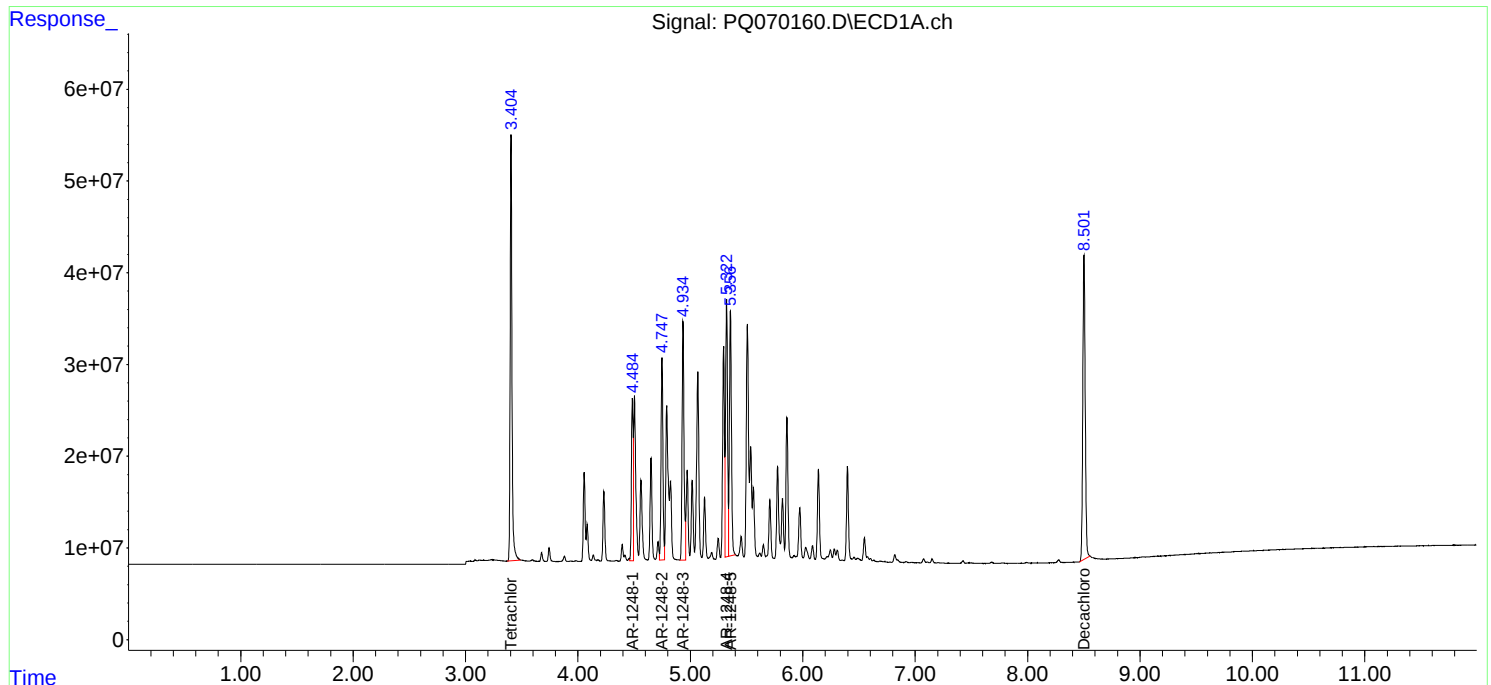

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070161.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 15:45
 Operator : YP\AJ
 Sample : AR1254ICC100
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12541013

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 16:35:18 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 16:29:29 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.783	41480456	41510216	5.285	5.370
2) SA Decachlor...	8.502	7.547	40646204	67181618	10.716	10.827
Target Compounds						
26) L6 AR-1254-1	5.297	4.541	30285461	45223252	108.587	109.173
27) L6 AR-1254-2	5.512	4.688	46414780	40196544	108.420	109.721
28) L6 AR-1254-3	5.859	5.069	47564820	63075126	107.380	108.782
29) L6 AR-1254-4	6.140	5.295	32840315	37736954	108.328	108.082
30) L6 AR-1254-5	6.548	5.699	36615774	56720987	106.846	107.718



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070161.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 15:45
Operator : YP\AJ
Sample : AR1254ICC100
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12541013

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 16:35:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 16:29:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

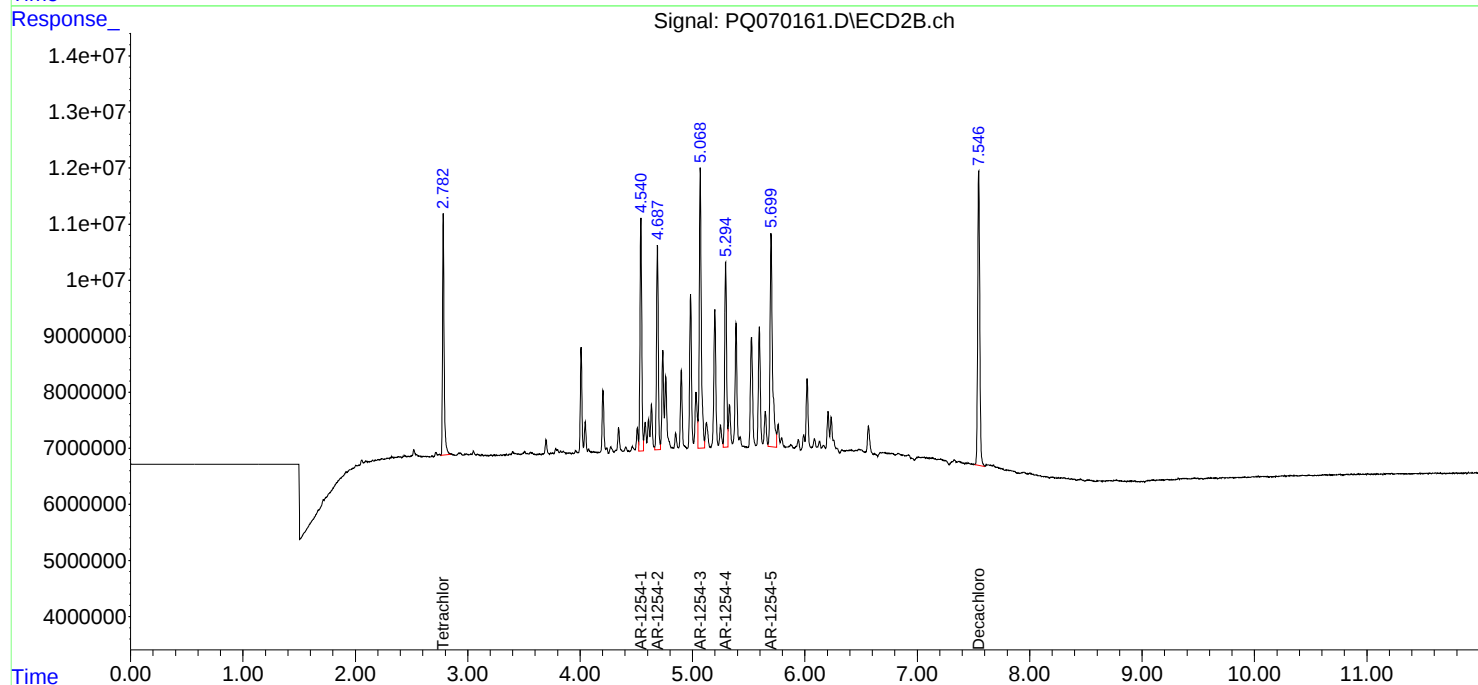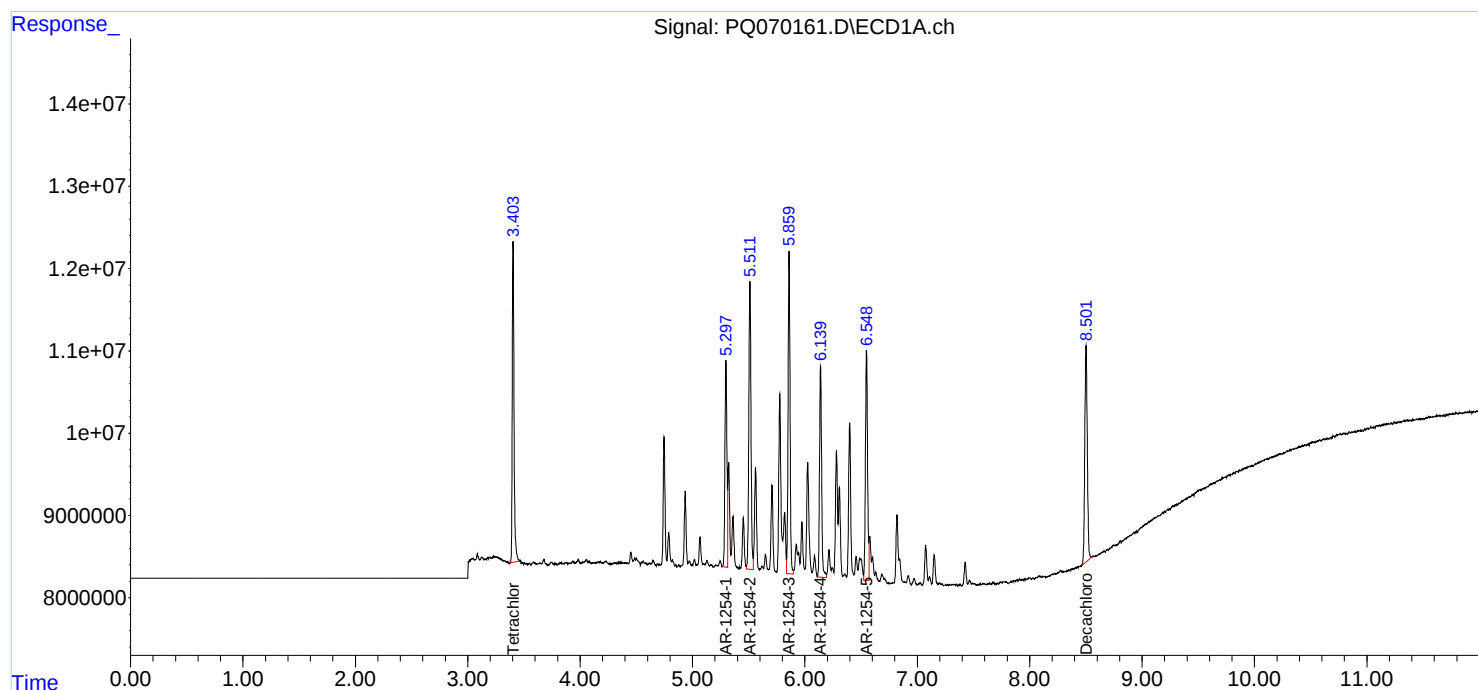

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070162.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 16:00
 Operator : YP\AJ
 Sample : AR1254ICC200
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12542014

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 16:32:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 16:29:29 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.405	2.783	79176159	77425354	10.385	10.401
2) SA Decachlor...	8.502	7.546	75543927	125.5E6	20.656	21.095
Target Compounds						
26) L6 AR-1254-1	5.297	4.541	55882361	83162036	209.353	210.412
27) L6 AR-1254-2	5.511	4.688	86190445	73610530	210.181	211.192
28) L6 AR-1254-3	5.859	5.069	88833046	116.8E6	208.230	210.611
29) L6 AR-1254-4	6.140	5.294	60009437	70154292	206.548	209.390
30) L6 AR-1254-5	6.549	5.699	68419692	106.3E6	206.726	209.990



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070162.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 16:00
Operator : YP\AJ
Sample : AR1254ICC200
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12542014

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 16:32:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 16:29:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

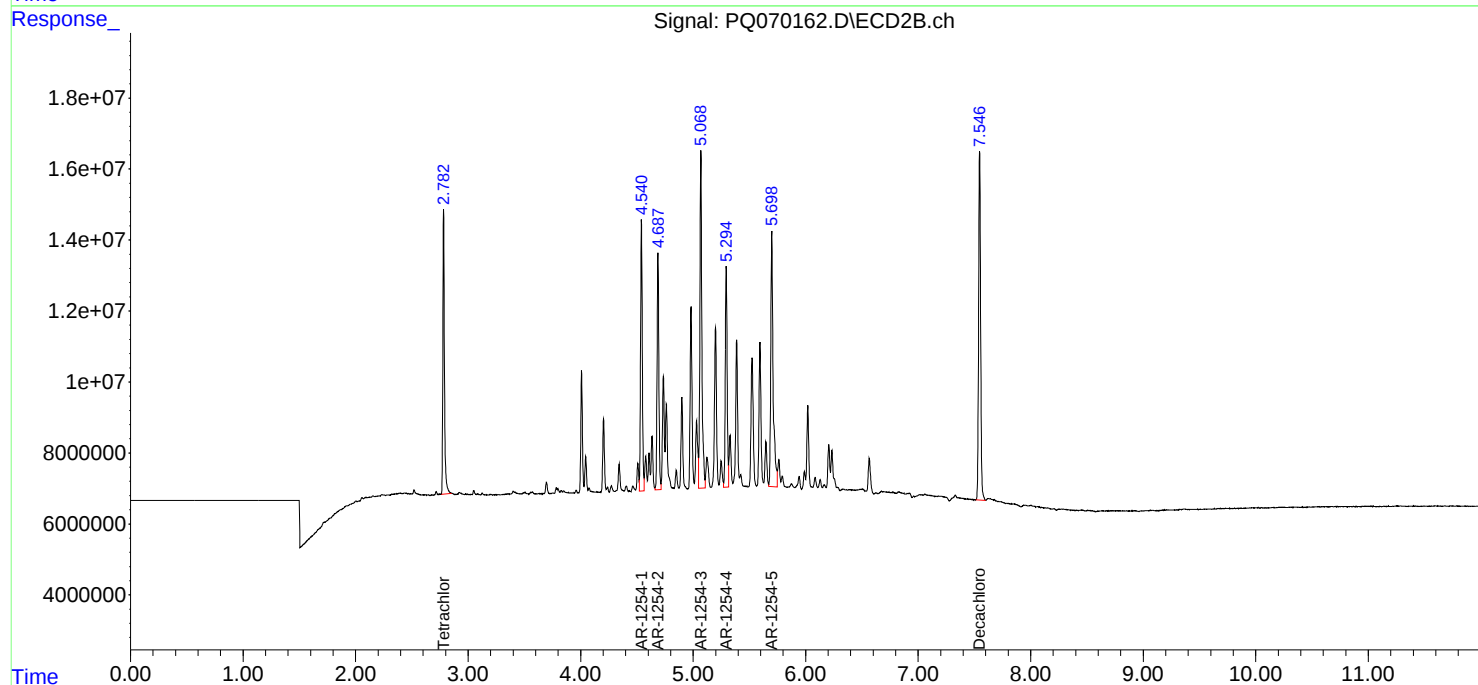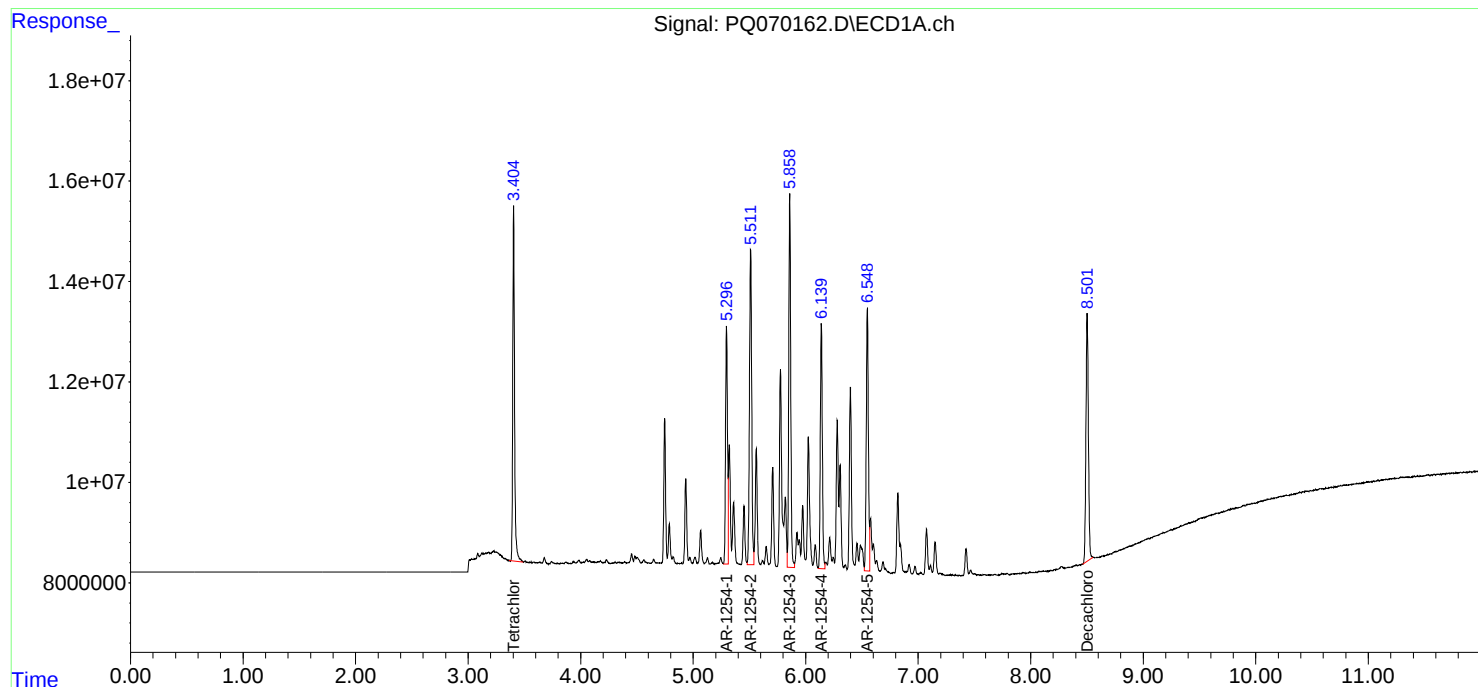

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070163.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 16:14
 Operator : YP\AJ
 Sample : AR1254ICC400
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12543015

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 16:29:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 16:29:29 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.783	146.6E6	142.9E6	20.000	20.000
2) SA Decachlor...	8.502	7.546	141.5E6	224.9E6	40.000	40.000
Target Compounds						
26) L6 AR-1254-1	5.297	4.542	101.8E6	149.9E6	400.000	400.000
27) L6 AR-1254-2	5.511	4.688	155.7E6	131.6E6	400.000	400.000
28) L6 AR-1254-3	5.859	5.069	163.6E6	210.0E6	400.000	400.000
29) L6 AR-1254-4	6.140	5.295	112.4E6	127.7E6	400.000	400.000
30) L6 AR-1254-5	6.549	5.700	127.9E6	192.4E6	400.000	400.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070163.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 16:14
Operator : YP\AJ
Sample : AR1254ICC400
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12543015

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 16:29:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 16:29:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

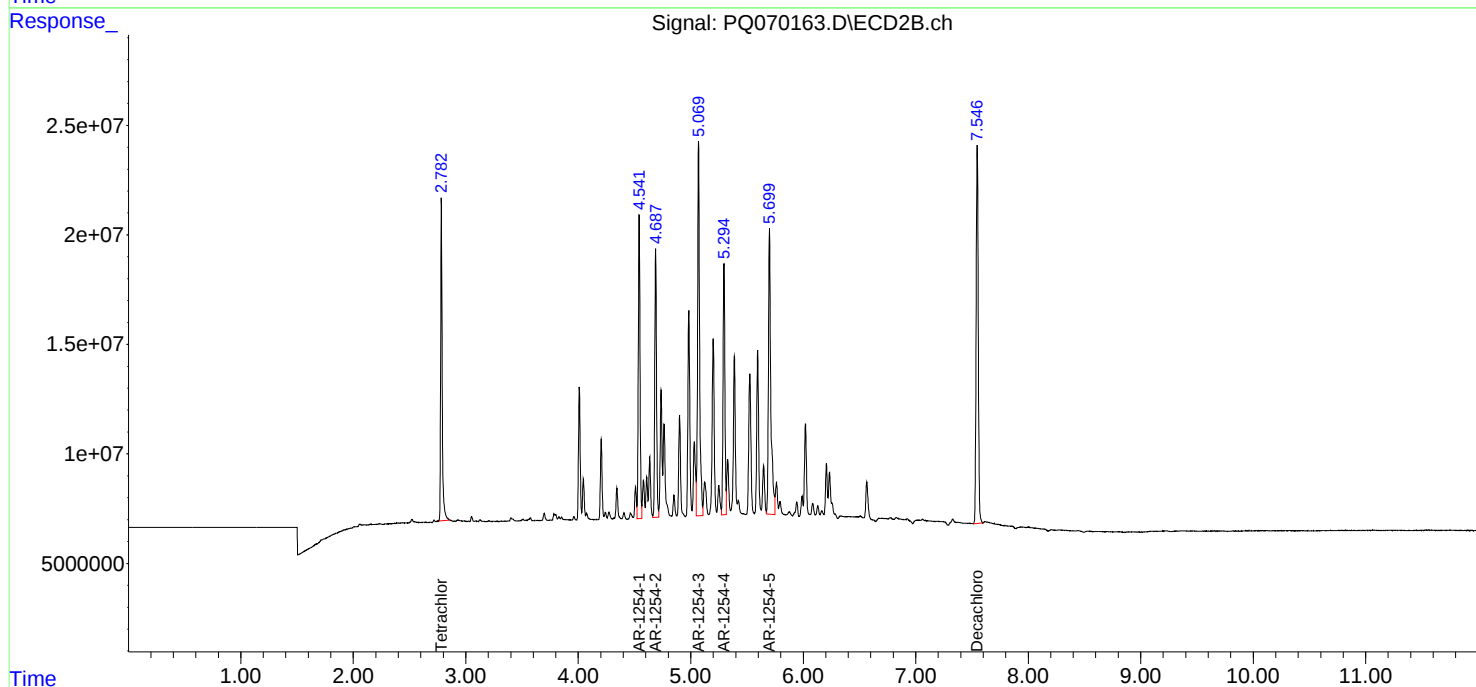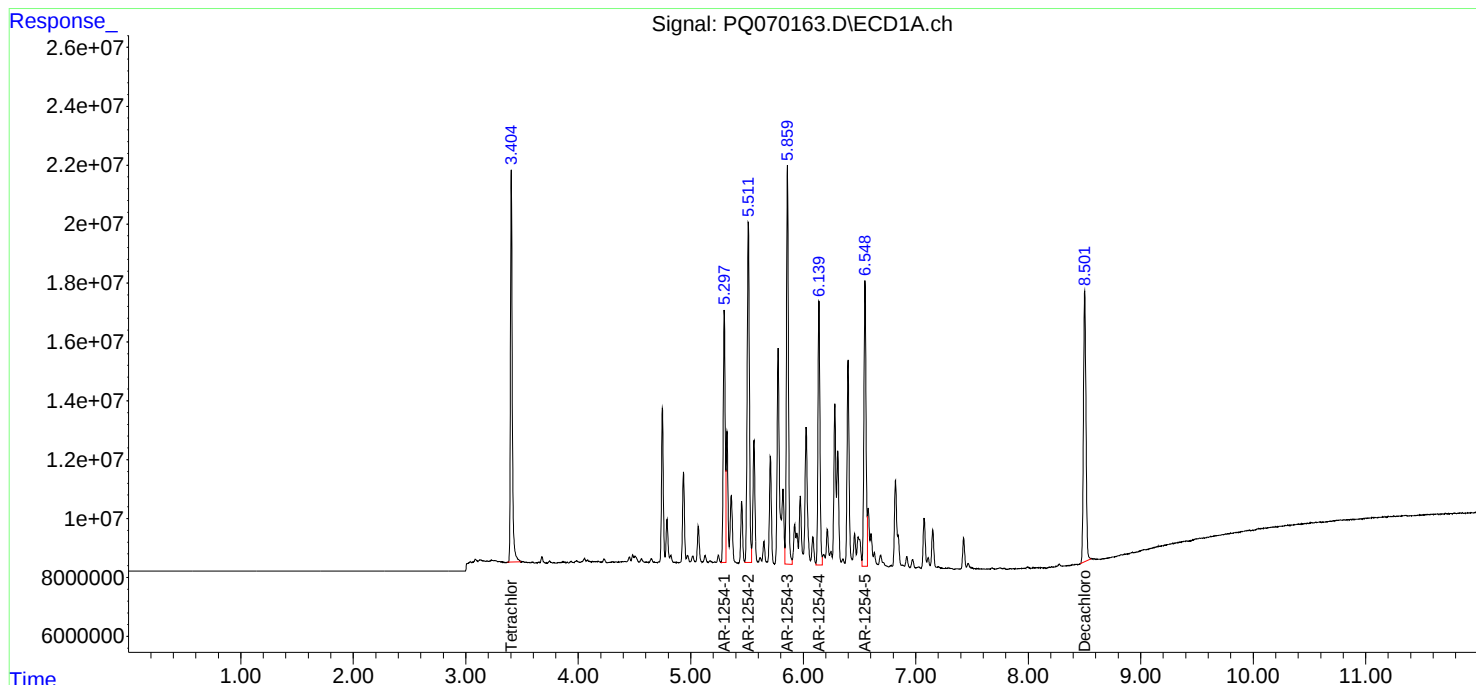

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070164.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 16:29
 Operator : YP\AJ
 Sample : AR1254ICC800
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12544016

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 17:21:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 17:21:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.404	2.783	264.8E6	254.6E6	35.116	34.455
2)	SA Decachlor...	8.502	7.547	258.6E6	406.5E6	70.799	68.614
Target Compounds							
26)	L6 AR-1254-1	5.297	4.541	180.9E6	262.3E6	680.779	668.046
27)	L6 AR-1254-2	5.511	4.688	278.4E6	229.4E6	682.182	662.037
28)	L6 AR-1254-3	5.859	5.069	296.4E6	368.9E6	697.662	670.492
29)	L6 AR-1254-4	6.140	5.295	204.0E6	225.3E6	700.834	678.143
30)	L6 AR-1254-5	6.548	5.700	230.8E6	342.9E6	701.120	683.025



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070164.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 16:29
Operator : YP\AJ
Sample : AR1254ICC800
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12544016

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 17:21:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 17:21:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

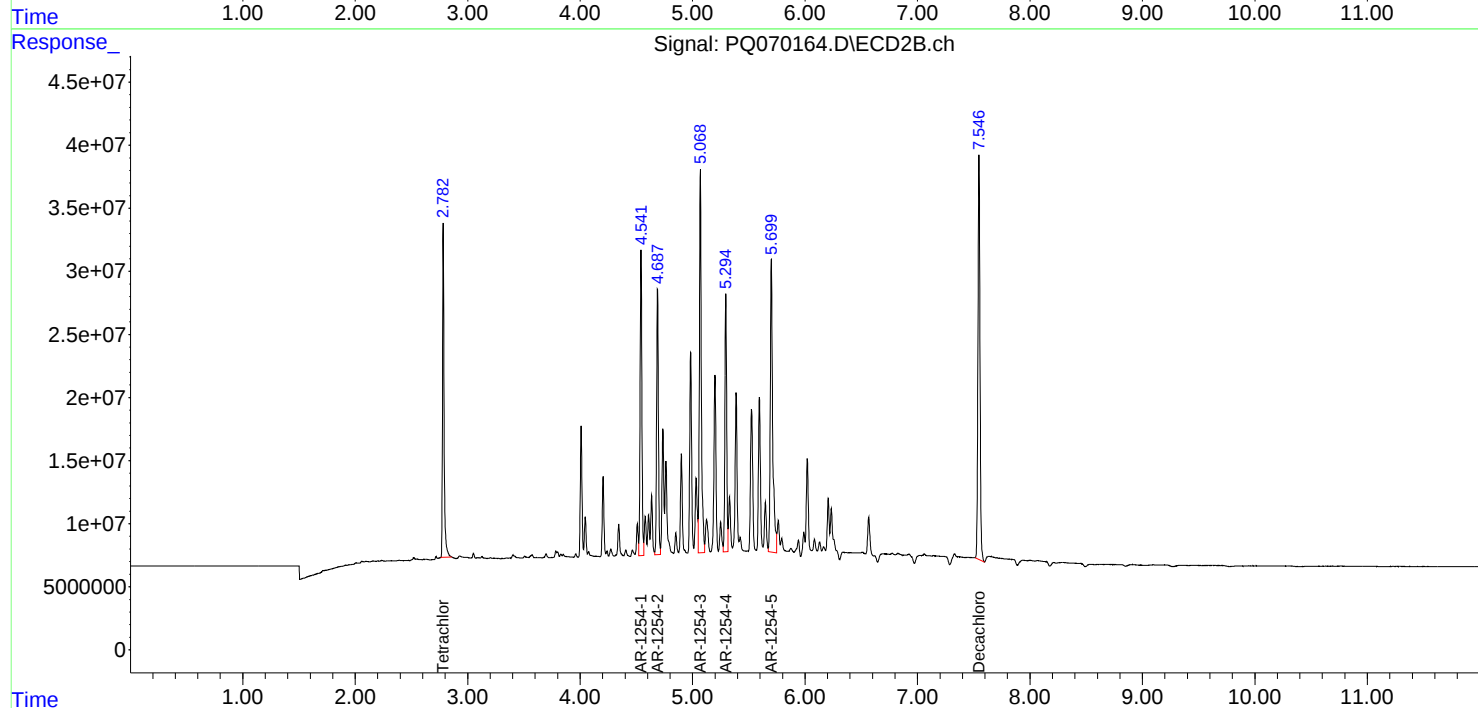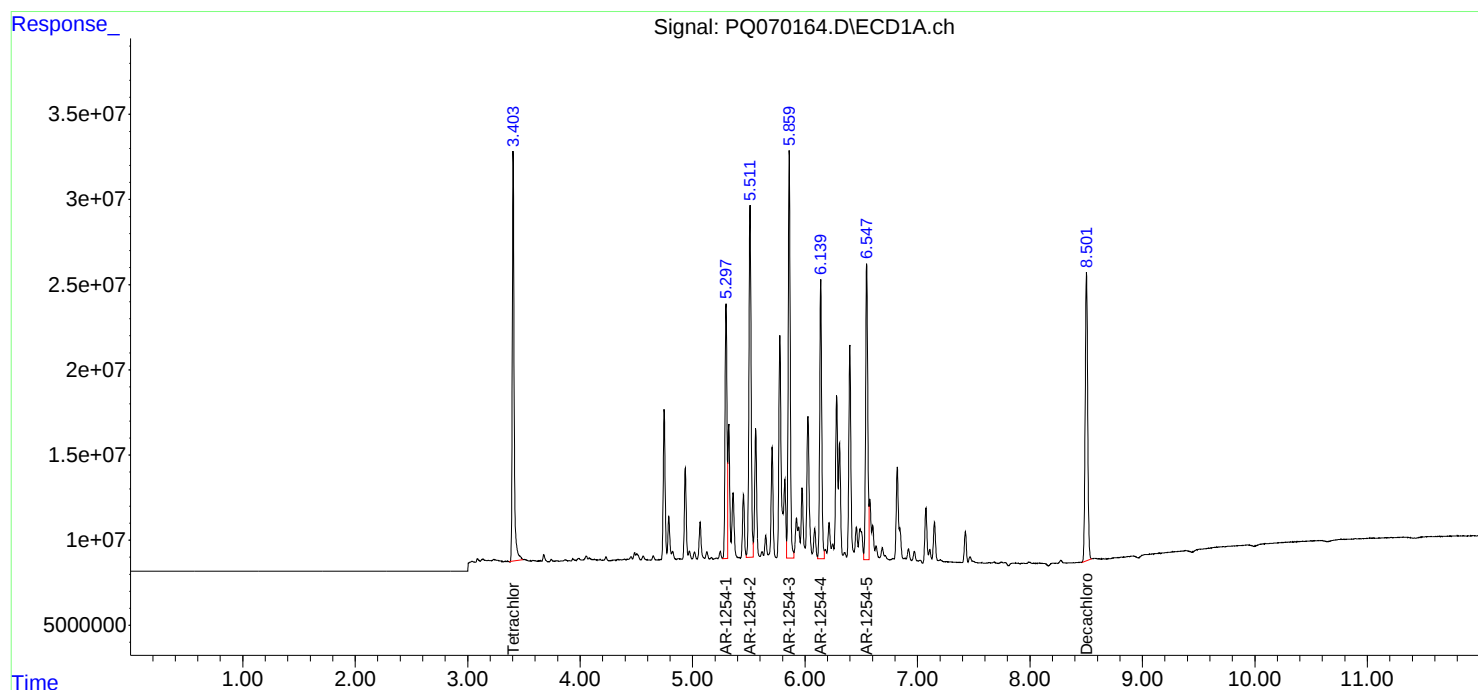

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070165.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 16:43
 Operator : YP\AJ
 Sample : AR1254ICC1600
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12545017

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 17:24:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 09 17:24:11 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.783	506.6E6	495.5E6	69.399	69.300
2) SA Decachlor...	8.502	7.546	497.4E6	778.2E6	140.339	136.234
Target Compounds						
26) L6 AR-1254-1	5.297	4.541	341.0E6	499.4E6	1336.241	1326.238
27) L6 AR-1254-2	5.511	4.688	529.7E6	435.2E6	1348.887	1312.584
28) L6 AR-1254-3	5.859	5.069	568.0E6	716.7E6	1382.363	1352.968
29) L6 AR-1254-4	6.139	5.295	395.9E6	439.1E6	1401.847	1369.092
30) L6 AR-1254-5	6.548	5.699	446.7E6	654.0E6	1399.730	1352.915



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070165.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 16:43
Operator : YP\AJ
Sample : AR1254ICC1600
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12545017

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 17:24:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 09 17:24:11 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

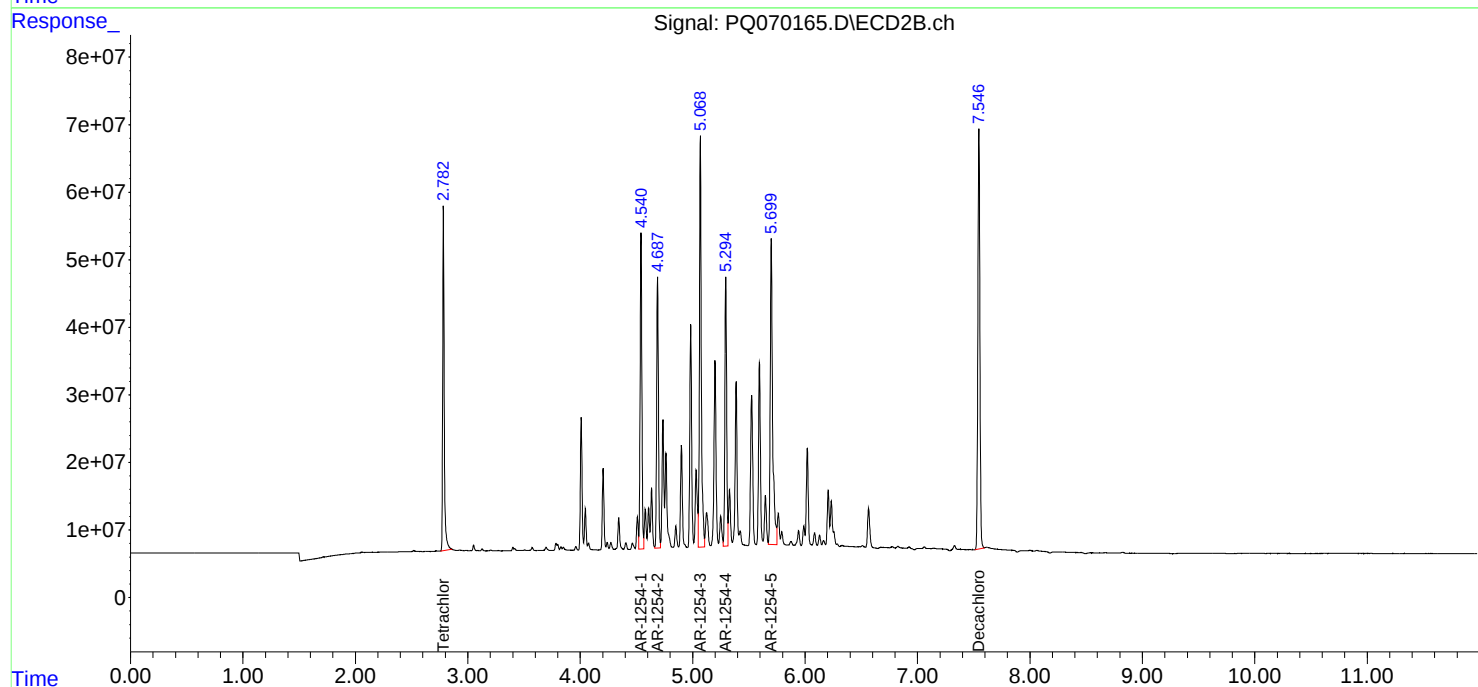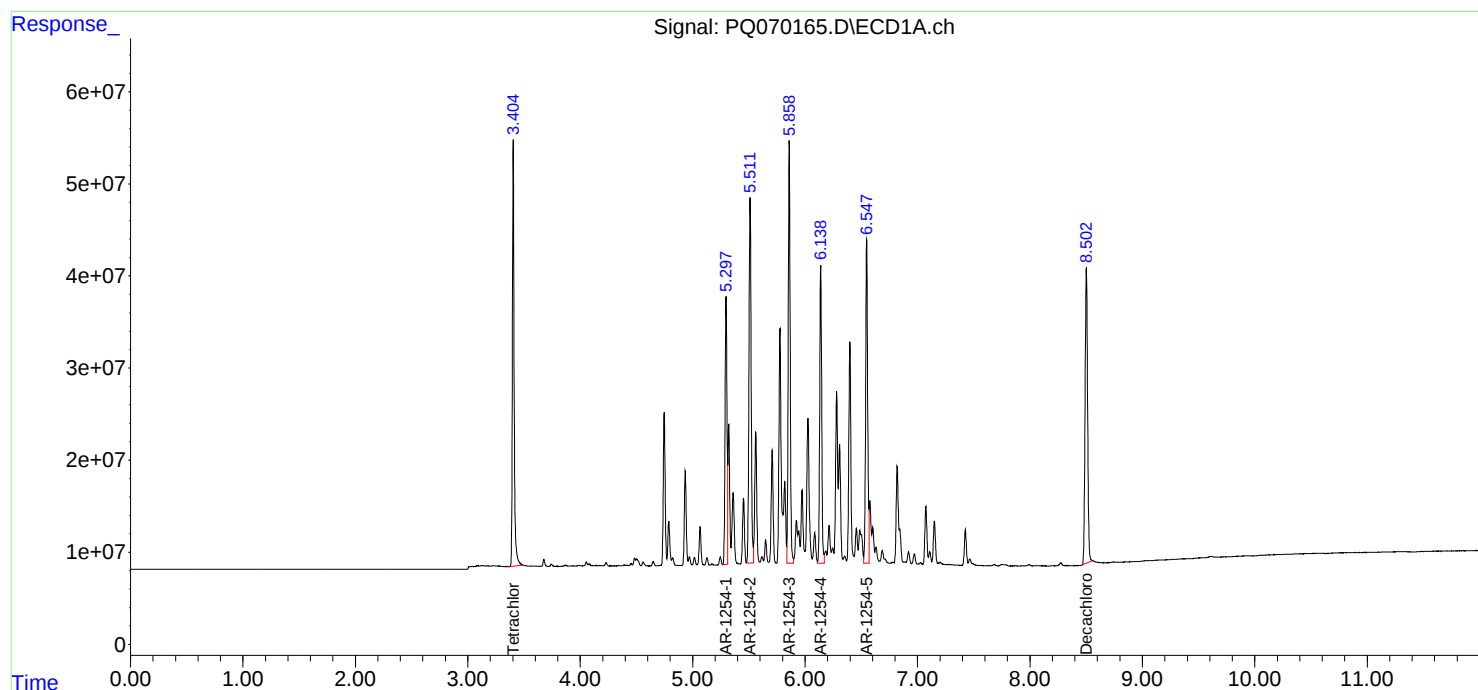

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070166.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 16:58
 Operator : YP\AJ
 Sample : AR1262ICC100
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12621018

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/10/2025
 Supervised By :mohammad ahmed 04/14/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 09:30:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 10 09:05:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.782	42699375	38250757	5.942	5.495
2) SA Decachlor...	8.502	7.544	43172201	62707119	12.135	11.427m
Target Compounds						
36) L8 AR-1262-1	6.846	5.740	41513718	54917557	116.818	113.238m
37) L8 AR-1262-2	7.151	5.987	74517704	50348453	119.126	113.059m
38) L8 AR-1262-3	7.424	6.509	43389123	43307256	104.006	124.159
39) L8 AR-1262-4	7.498	6.570	37360598	72425569	110.409	114.299
40) L8 AR-1262-5	7.993	7.060	23127368	32140928	116.162	106.673

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070166.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 16:58
Operator : YP\AJ
Sample : AR1262ICC100
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
AR12621018

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2025
Supervised By :mohammad ahmed 04/14/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 09:30:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 10 09:05:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

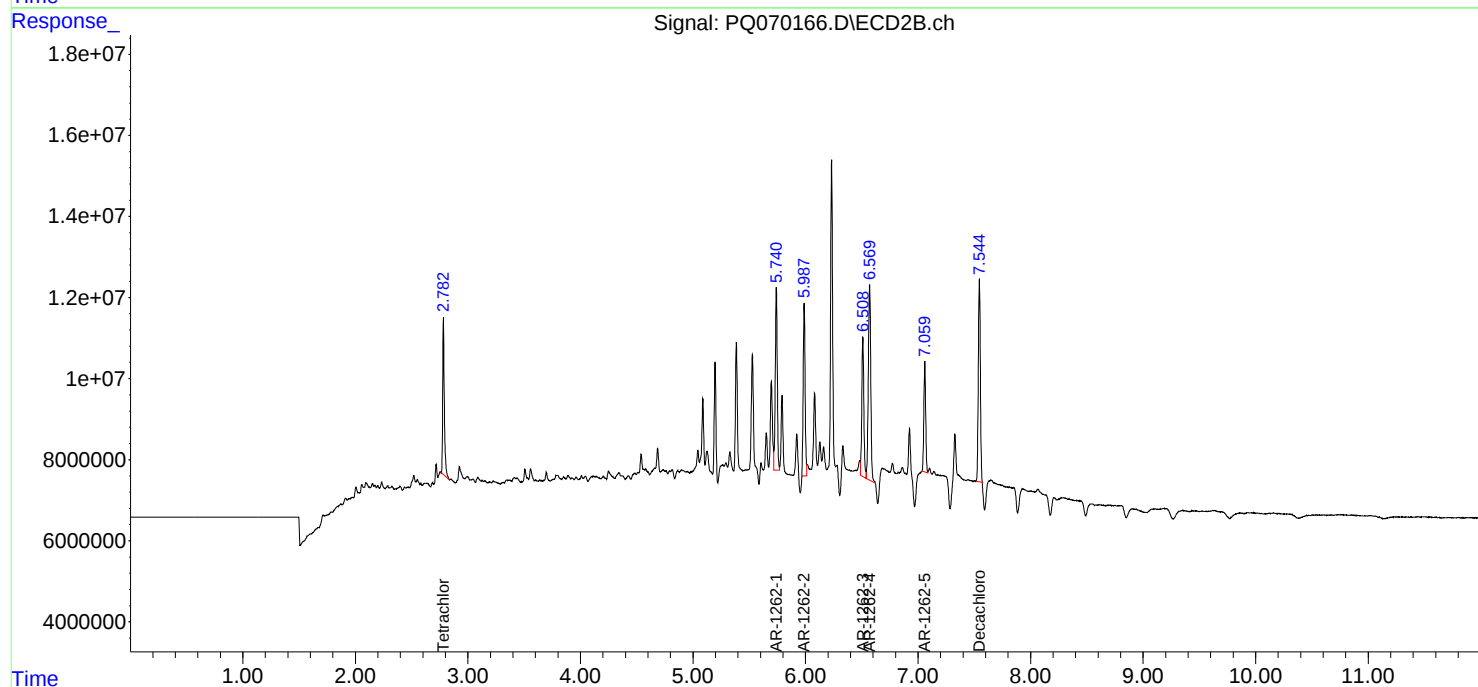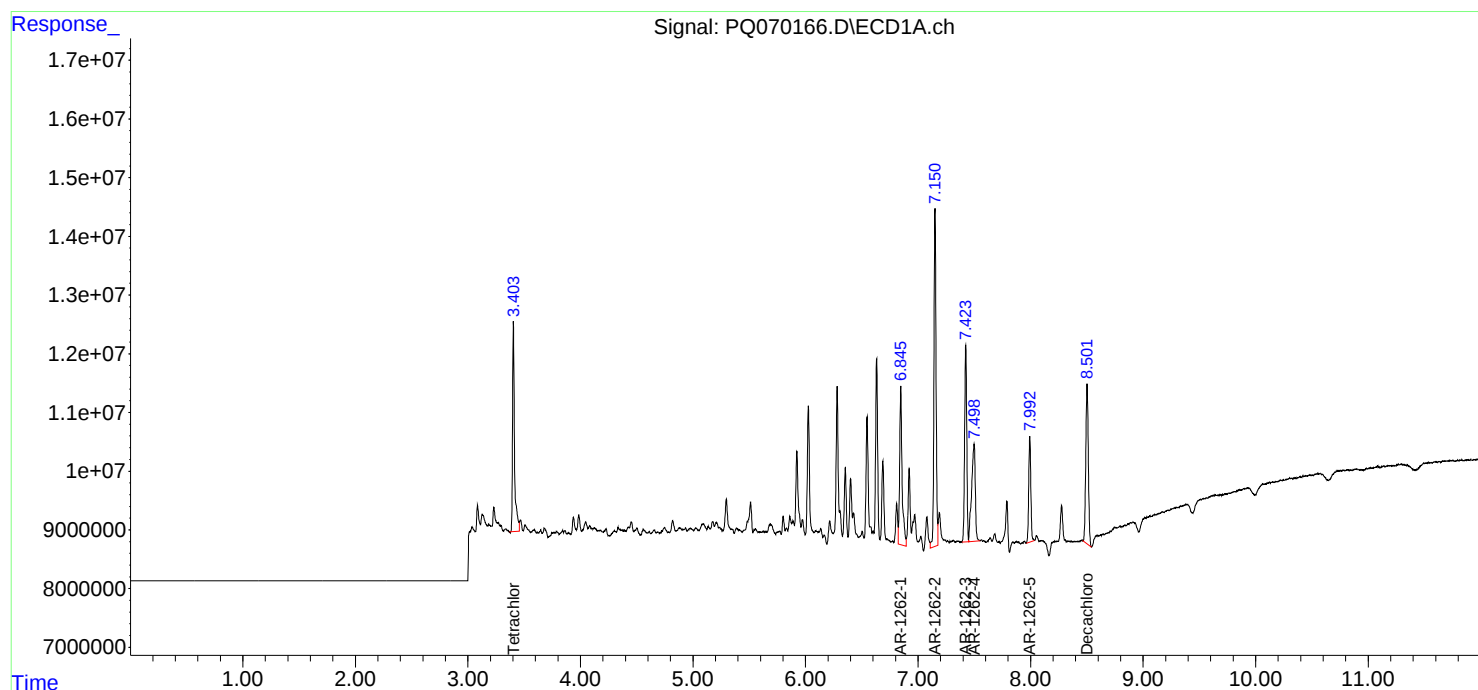

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070167.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 17:13
 Operator : YP\AJ
 Sample : AR1262ICC200
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12622019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 09:30:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 10 09:05:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.405	2.782	79217453	71638126	11.023	10.291
2) SA Decachlor...	8.503	7.545	76525200	121.6E6	21.510	22.164
Target Compounds						
36) L8 AR-1262-1	6.846	5.741	74933099	105.3E6	210.858	217.088
37) L8 AR-1262-2	7.151	5.988	134.6E6	101.8E6	215.162	228.617
38) L8 AR-1262-3	7.424	6.510	87352422	77050144	209.388	220.897
39) L8 AR-1262-4	7.497	6.569	69625144	129.9E6	205.757	205.056
40) L8 AR-1262-5	7.992	7.061	42828765	63147358	215.116	209.581



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070167.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 17:13
Operator : YP\AJ
Sample : AR1262ICC200
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12622019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 09:30:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 10 09:05:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

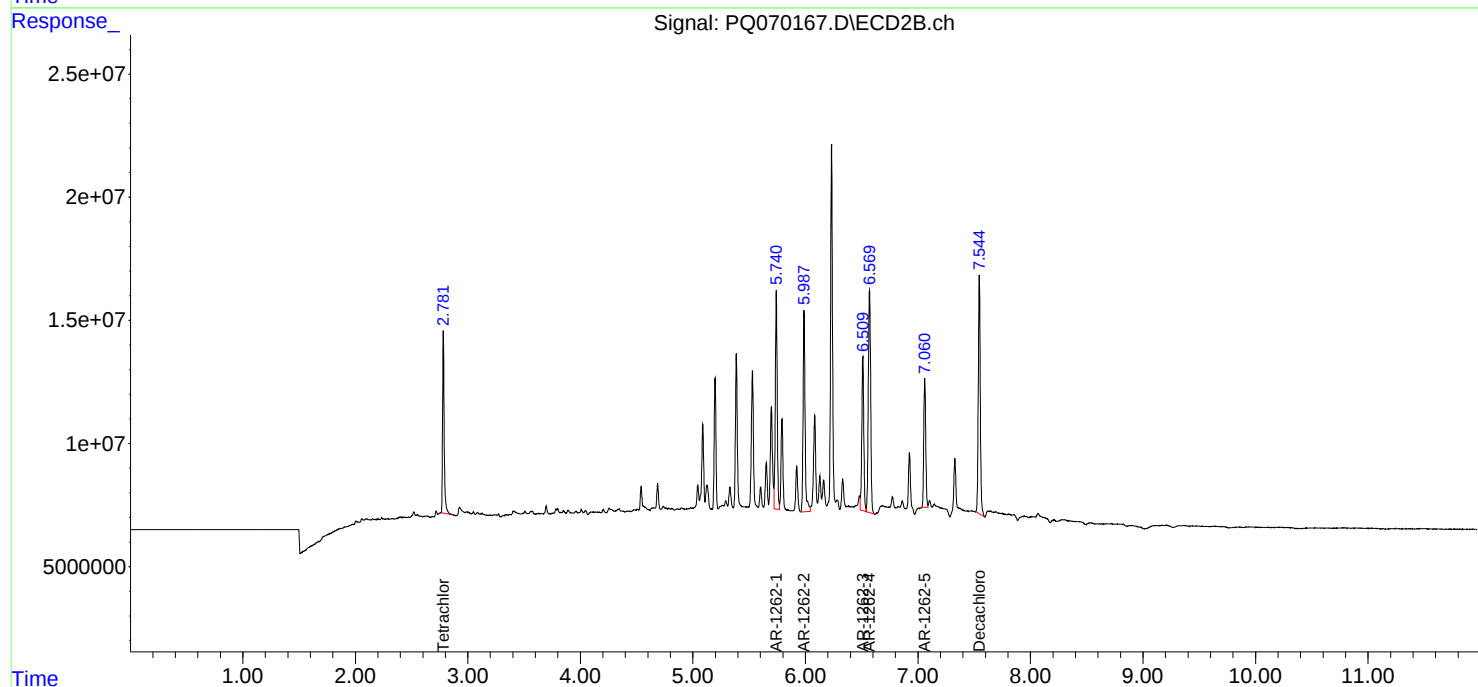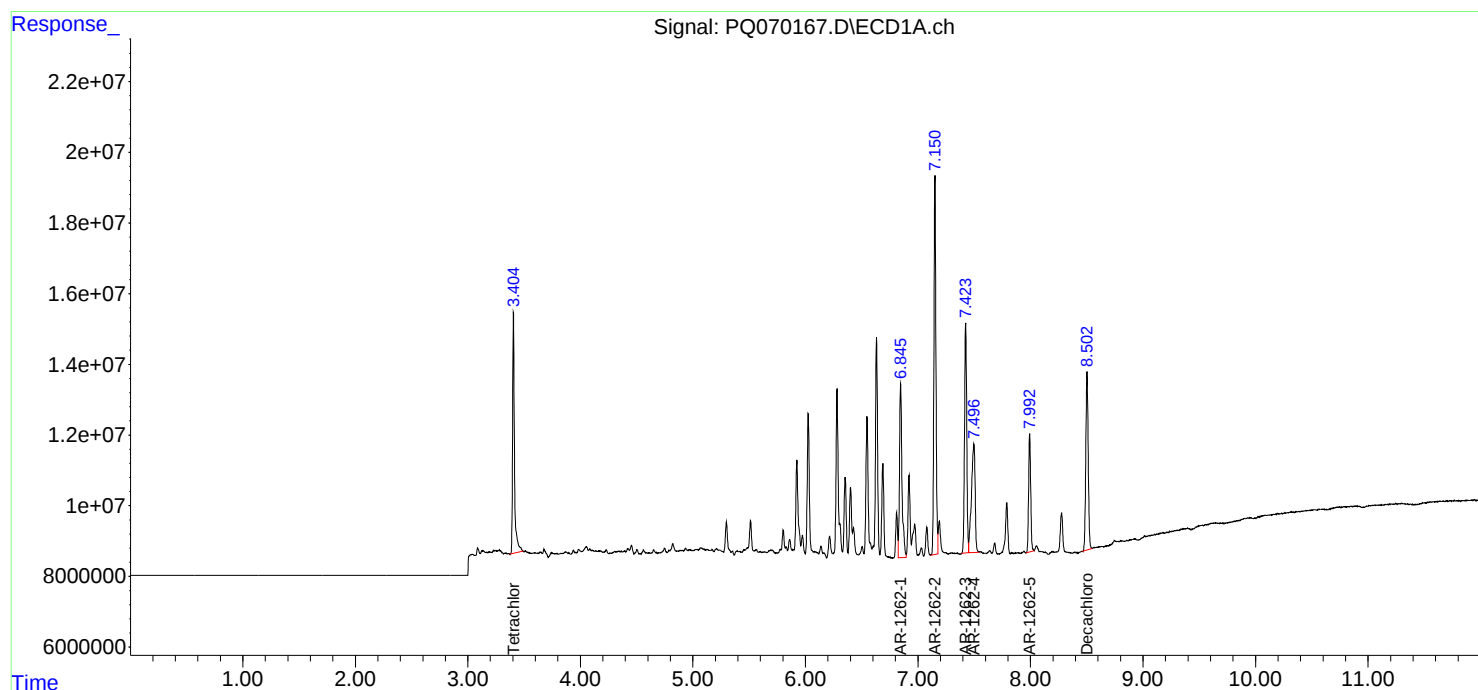

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070168.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 17:27
 Operator : YP\AJ
 Sample : AR1262ICC400
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12623020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 09:30:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 10 09:05:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.404	2.782	143.7E6	139.2E6	20.000	20.000
2)	SA Decachlor...	8.502	7.545	142.3E6	219.5E6	40.000	40.000
Target Compounds							
36)	L8 AR-1262-1	6.845	5.741	142.1E6	194.0E6	400.000	400.000
37)	L8 AR-1262-2	7.151	5.989	250.2E6	178.1E6	400.000	400.000
38)	L8 AR-1262-3	7.424	6.510	166.9E6	139.5E6	400.000	400.000
39)	L8 AR-1262-4	7.497	6.571	135.4E6	253.5E6	400.000	400.000
40)	L8 AR-1262-5	7.992	7.061	79638600	120.5E6	400.000	400.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070168.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 17:27
Operator : YP\AJ
Sample : AR1262ICC400
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12623020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 09:30:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 10 09:05:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

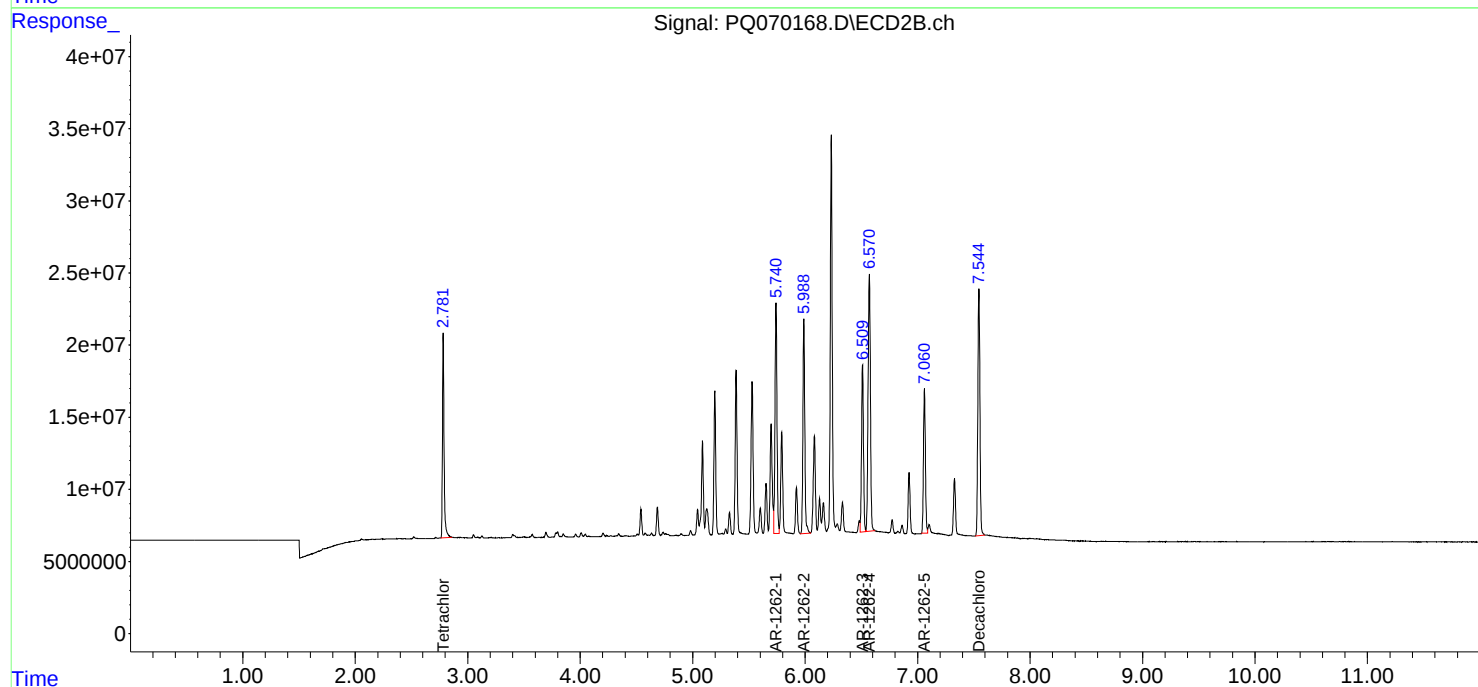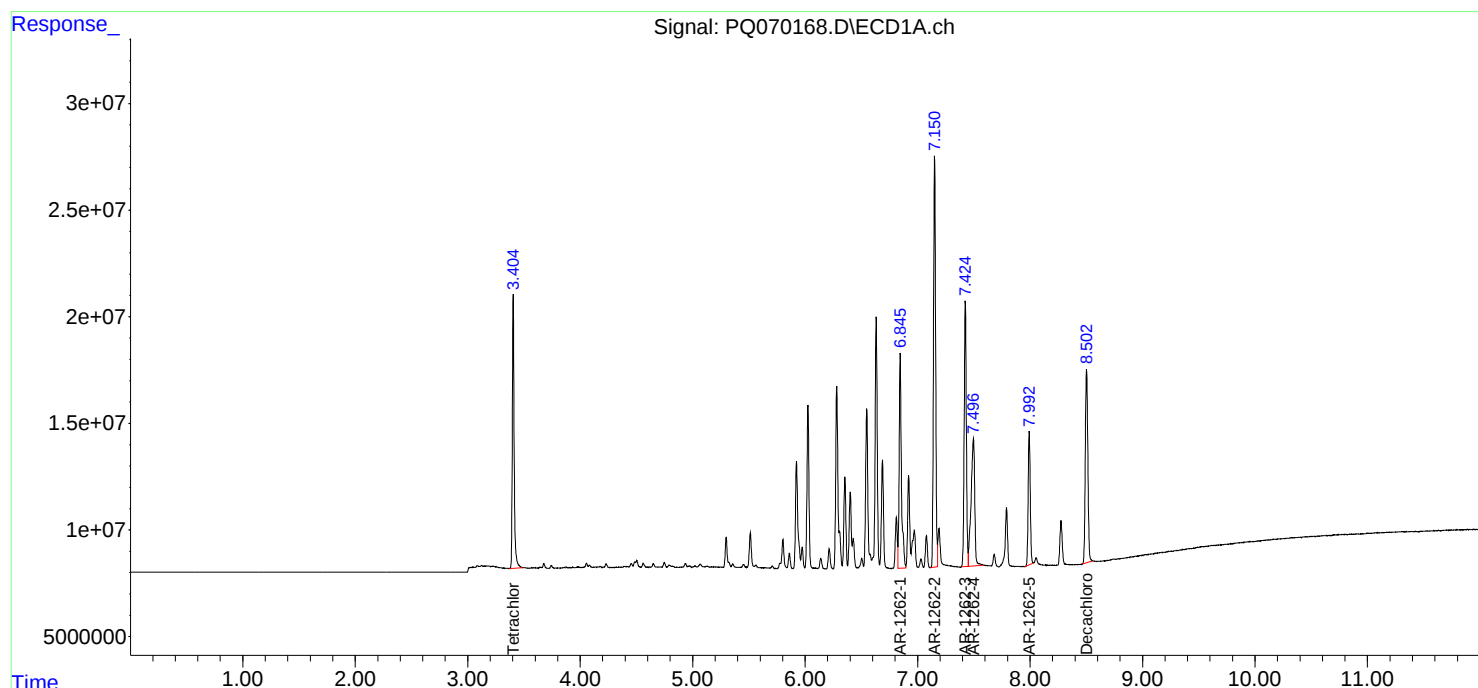

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070169.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 17:42
 Operator : YP\AJ
 Sample : AR1262ICC800
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12624021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 09:31:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 10 09:05:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.782	260.9E6	244.2E6	36.303	35.082
2) SA Decachlor...	8.503	7.545	264.0E6	404.1E6	74.214	73.636
Target Compounds						
36) L8 AR-1262-1	6.846	5.741	260.2E6	346.1E6	732.140	713.710
37) L8 AR-1262-2	7.151	5.988	473.7E6	333.8E6	757.346	749.652
38) L8 AR-1262-3	7.425	6.510	303.4E6	252.3E6	727.310	723.248
39) L8 AR-1262-4	7.496	6.570	248.6E6	456.9E6	734.802	721.057
40) L8 AR-1262-5	7.993	7.061	150.4E6	220.4E6	755.483	731.377



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070169.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 17:42
Operator : YP\AJ
Sample : AR1262ICC800
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12624021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 09:31:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 10 09:05:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

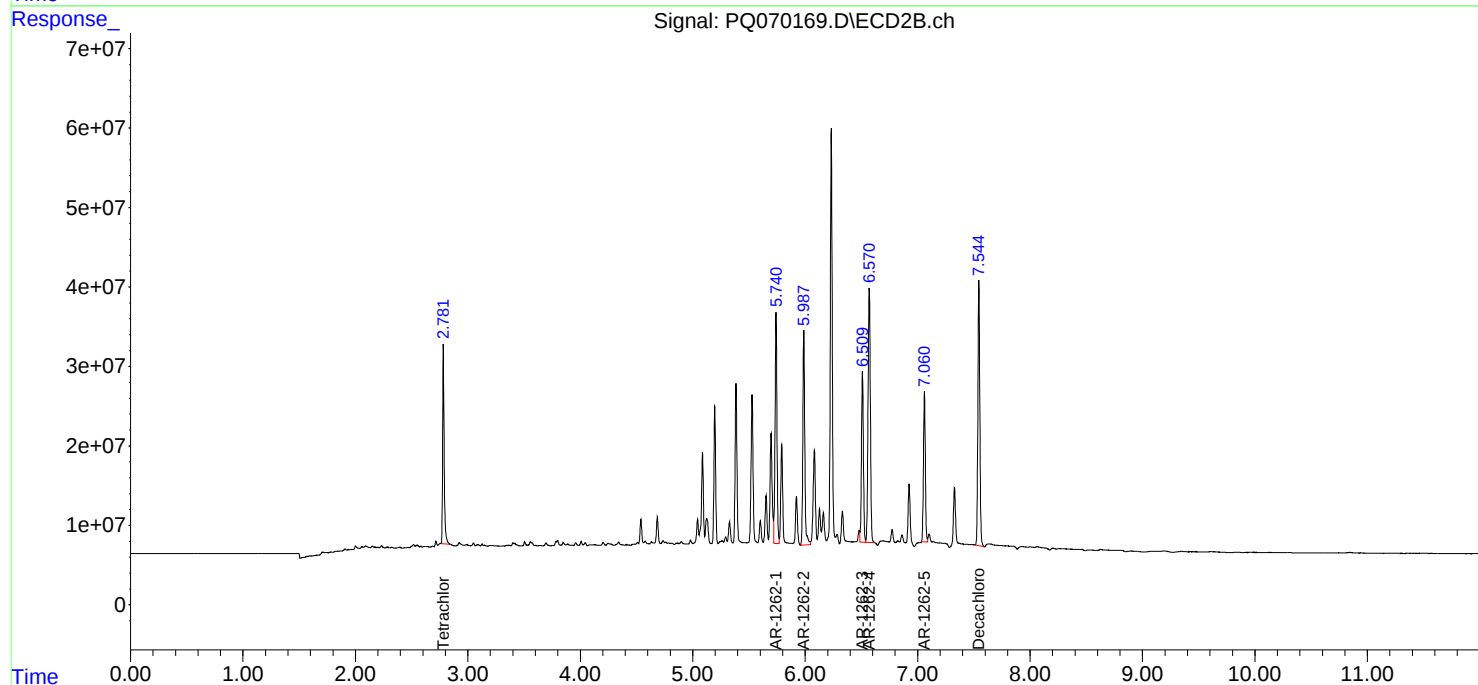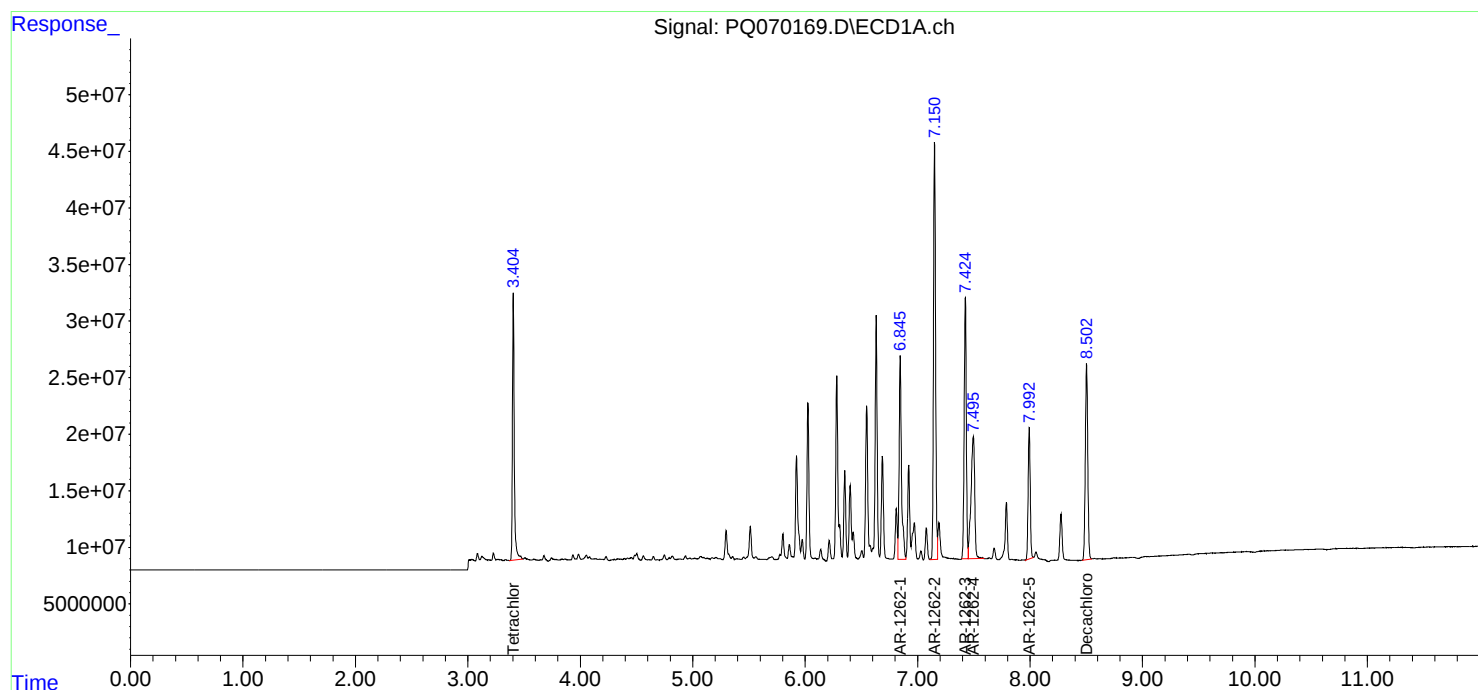

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070170.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 17:56
 Operator : YP\AJ
 Sample : AR1262ICC1600
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12625022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 09:31:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 10 09:05:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.782	514.4E6	497.4E6	71.577	71.451
2) SA Decachlor...	8.502	7.545	511.6E6	783.0E6	143.788	142.679
Target Compounds						
36) L8 AR-1262-1	6.846	5.741	510.4E6	677.6E6	1436.326	1397.267
37) L8 AR-1262-2	7.151	5.988	938.5E6	632.5E6	1500.271	1420.405
38) L8 AR-1262-3	7.424	6.510	611.7E6	498.7E6	1466.317	1429.752
39) L8 AR-1262-4	7.498	6.570	488.7E6	929.5E6	1444.359	1466.933
40) L8 AR-1262-5	7.992	7.060	290.4E6	437.9E6	1458.810	1453.514



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070170.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 17:56
Operator : YP\AJ
Sample : AR1262ICC1600
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12625022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 09:31:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 10 09:05:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

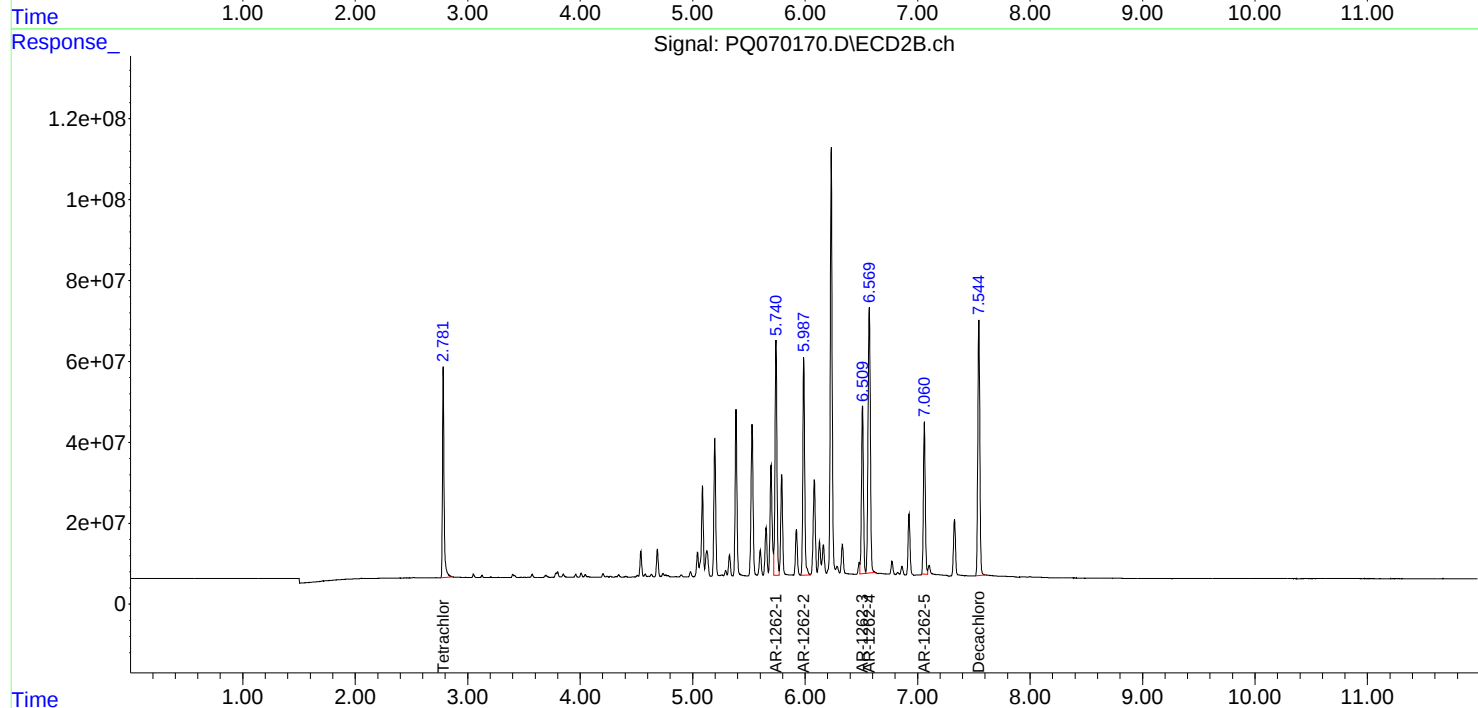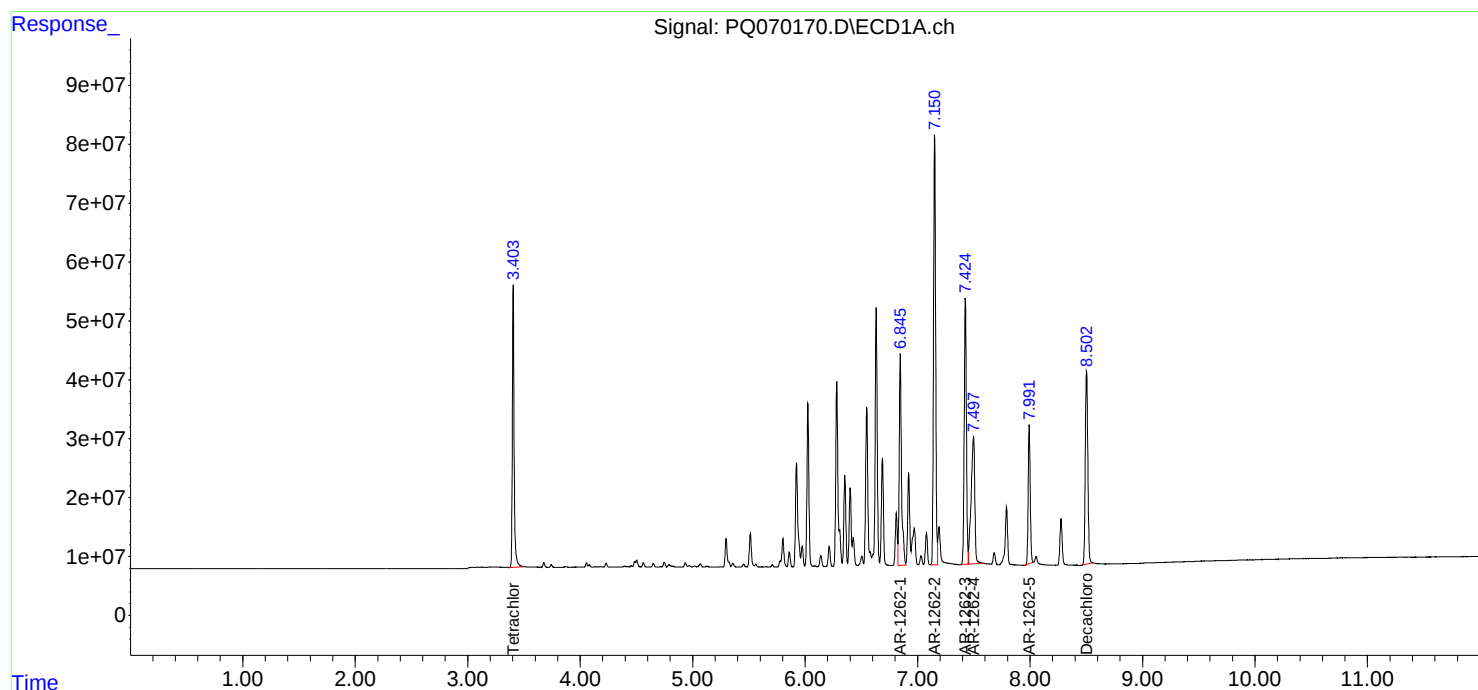

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070171.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 18:11
 Operator : YP\AJ
 Sample : AR1268ICC100
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12681023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 09:42:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 10 09:41:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.405	2.782	42945972	39726003	5.955	5.794
2) SA Decachlor...	8.503	7.545	80609661	124.8E6	11.907	11.894
Target Compounds						
41) L9 AR-1268-1	7.423	6.510	85186784	117.3E6	117.160	117.587
42) L9 AR-1268-2	7.500	6.572	79291940	106.0E6	115.451	117.409
43) L9 AR-1268-3	7.681	6.773	67390689	97060099	118.383	117.152
44) L9 AR-1268-4	7.992	7.060	26277255	39245243	114.118	113.682
45) L9 AR-1268-5	8.276	7.327	188.4E6	293.2E6	115.000	119.260



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070171.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 18:11
Operator : YP\AJ
Sample : AR1268ICC100
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12681023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 09:42:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 10 09:41:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

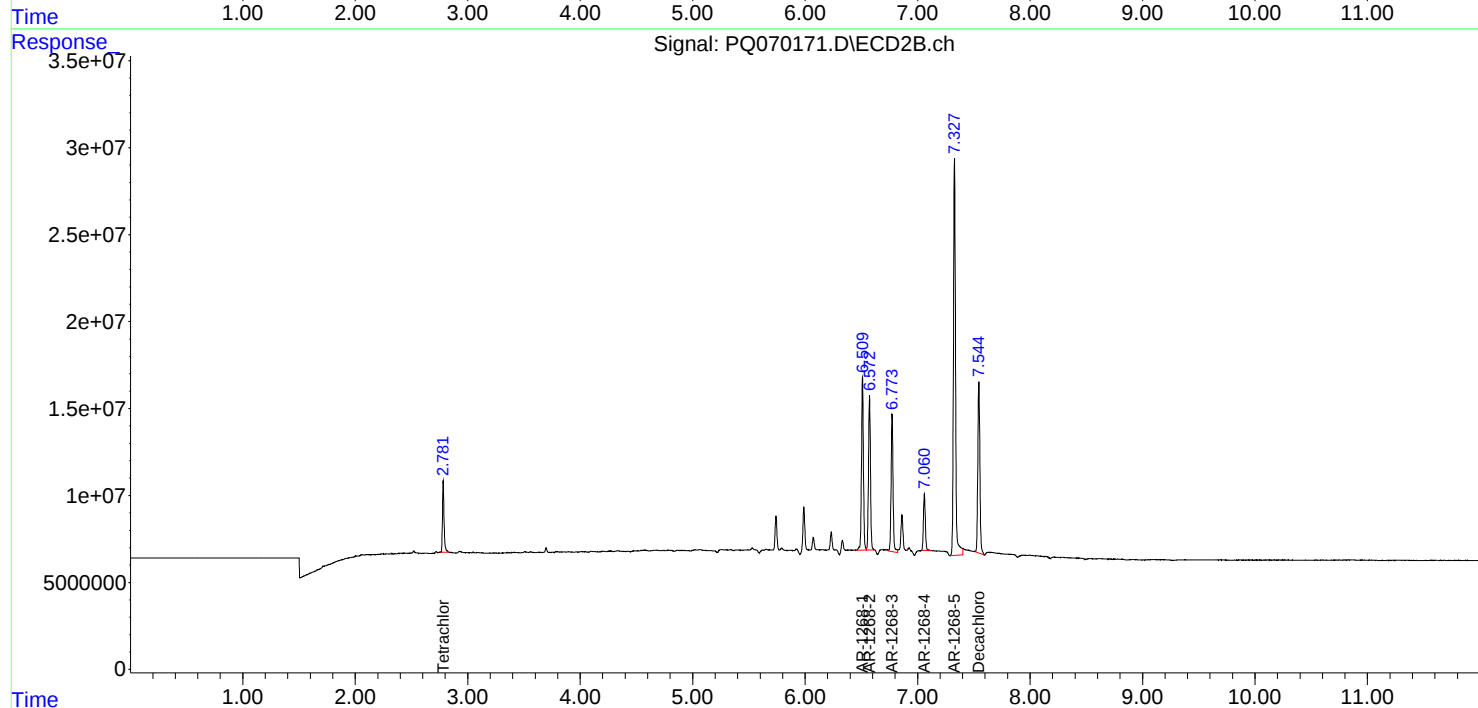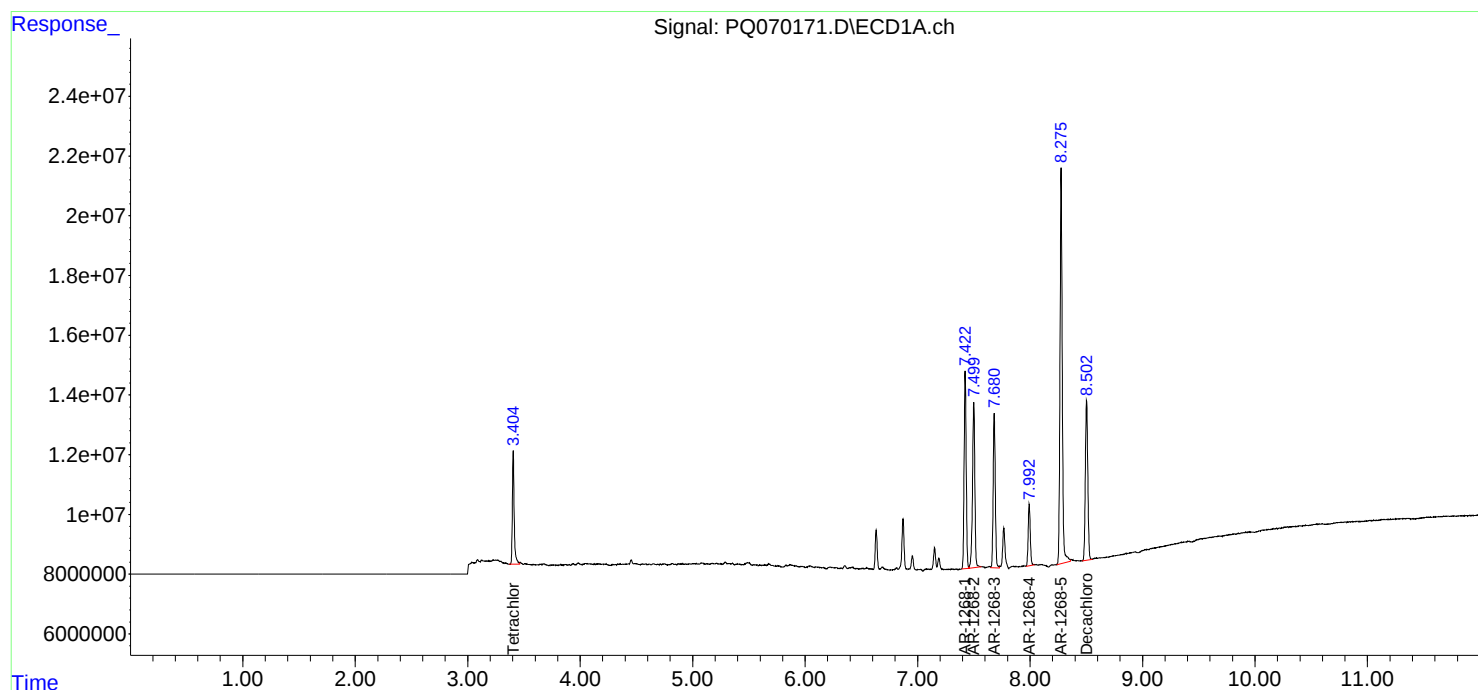

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070172.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 18:25
 Operator : YP\AJ
 Sample : AR1268ICC200
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12682024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 09:42:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 10 09:41:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.405	2.782	80407532	77332774	11.149	11.279
2) SA Decachlor...	8.502	7.543	150.3E6	231.0E6	22.202	22.018
Target Compounds						
41) L9 AR-1268-1	7.424	6.508	163.2E6	222.1E6	224.507	222.671
42) L9 AR-1268-2	7.500	6.571	152.1E6	202.9E6	221.485	224.854
43) L9 AR-1268-3	7.682	6.772	125.6E6	178.3E6	220.604	215.191
44) L9 AR-1268-4	7.993	7.059	51248131	75662928	222.562	219.174
45) L9 AR-1268-5	8.275	7.326	357.0E6	540.4E6	217.877	219.848



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070172.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 18:25
Operator : YP\AJ
Sample : AR1268ICC200
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12682024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 09:42:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 10 09:41:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

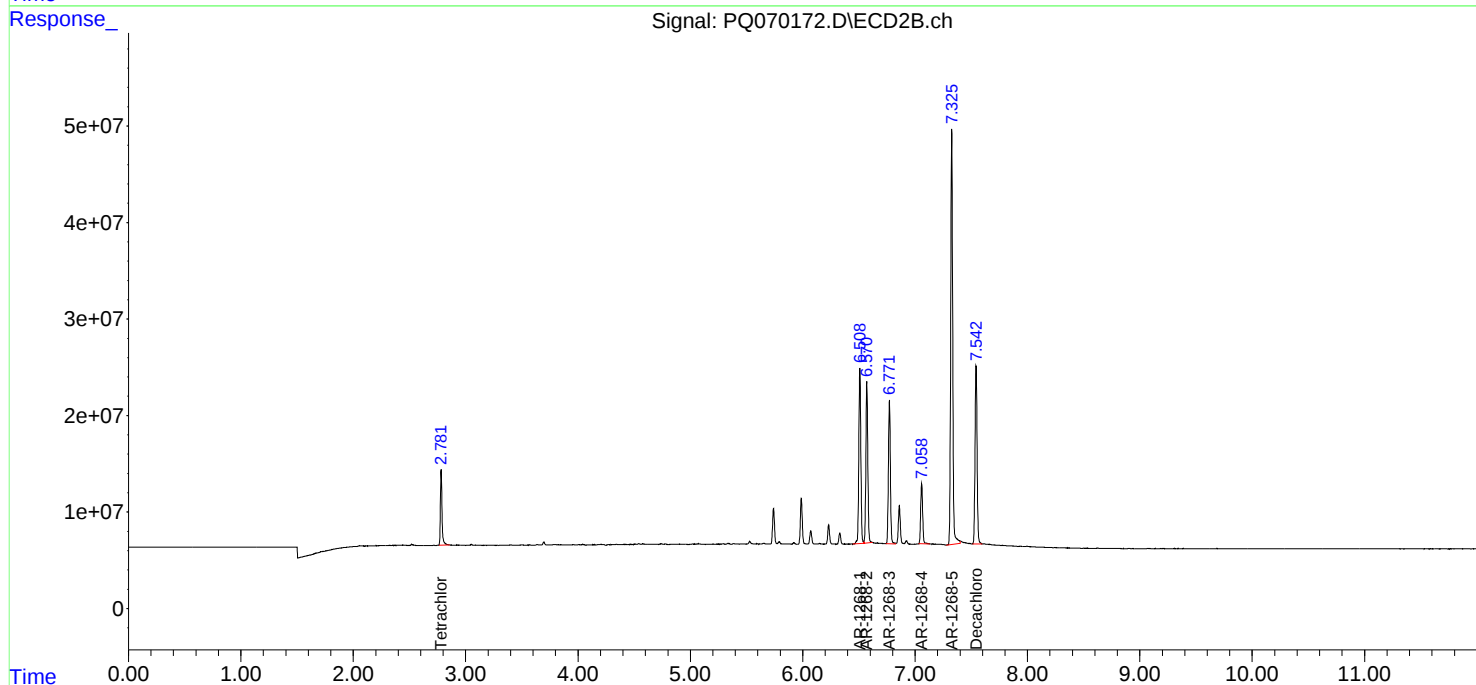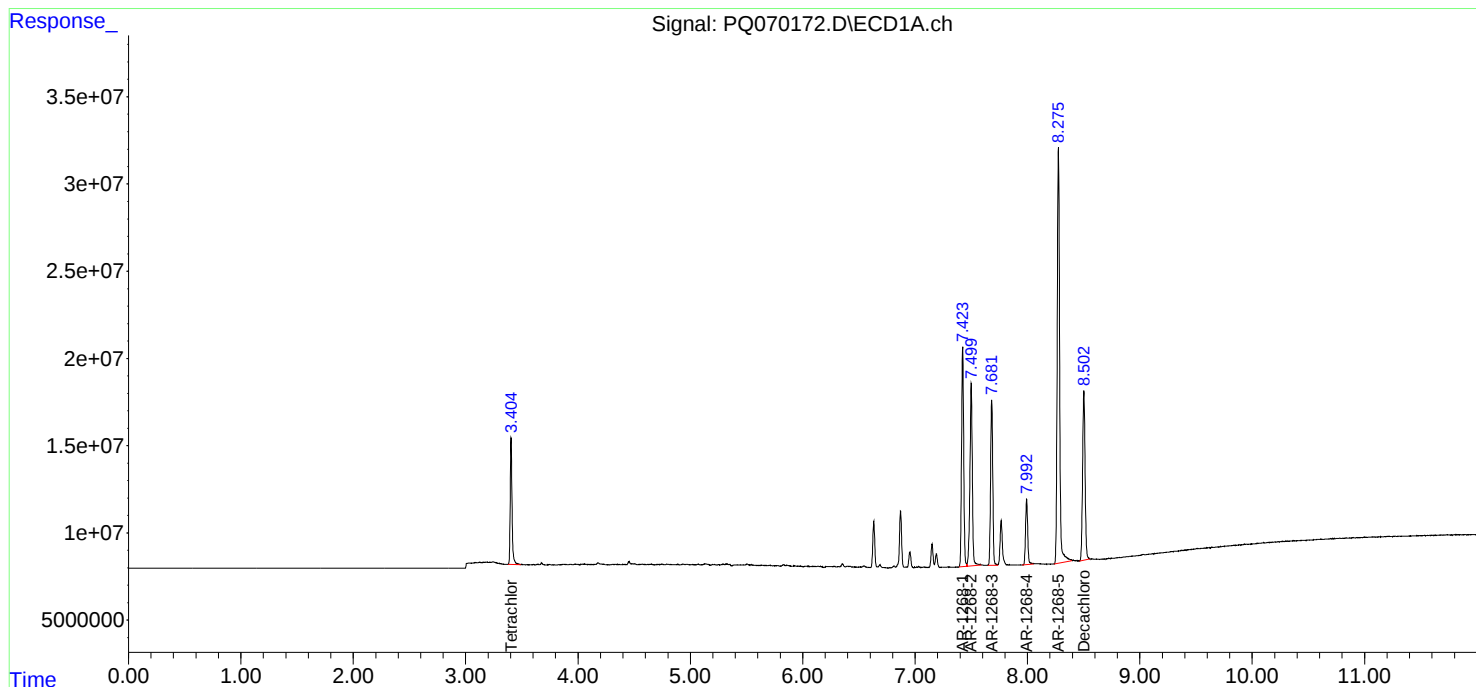

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070173.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 18:40
 Operator : YP\AJ
 Sample : AR1268ICC400
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12683025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 09:42:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 10 09:41:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.783	144.2E6	137.1E6	20.000	20.000
2) SA Decachlor...	8.502	7.546	270.8E6	419.6E6	40.000	40.000
Target Compounds						
41) L9 AR-1268-1	7.423	6.511	290.8E6	398.9E6	400.000	400.000
42) L9 AR-1268-2	7.499	6.574	274.7E6	361.0E6	400.000	400.000
43) L9 AR-1268-3	7.682	6.775	227.7E6	331.4E6	400.000	400.000
44) L9 AR-1268-4	7.992	7.062	92105904	138.1E6	400.000	400.000
45) L9 AR-1268-5	8.275	7.329	655.3E6	983.3E6	400.000	400.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070173.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 18:40
Operator : YP\AJ
Sample : AR1268ICC400
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12683025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 09:42:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 10 09:41:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

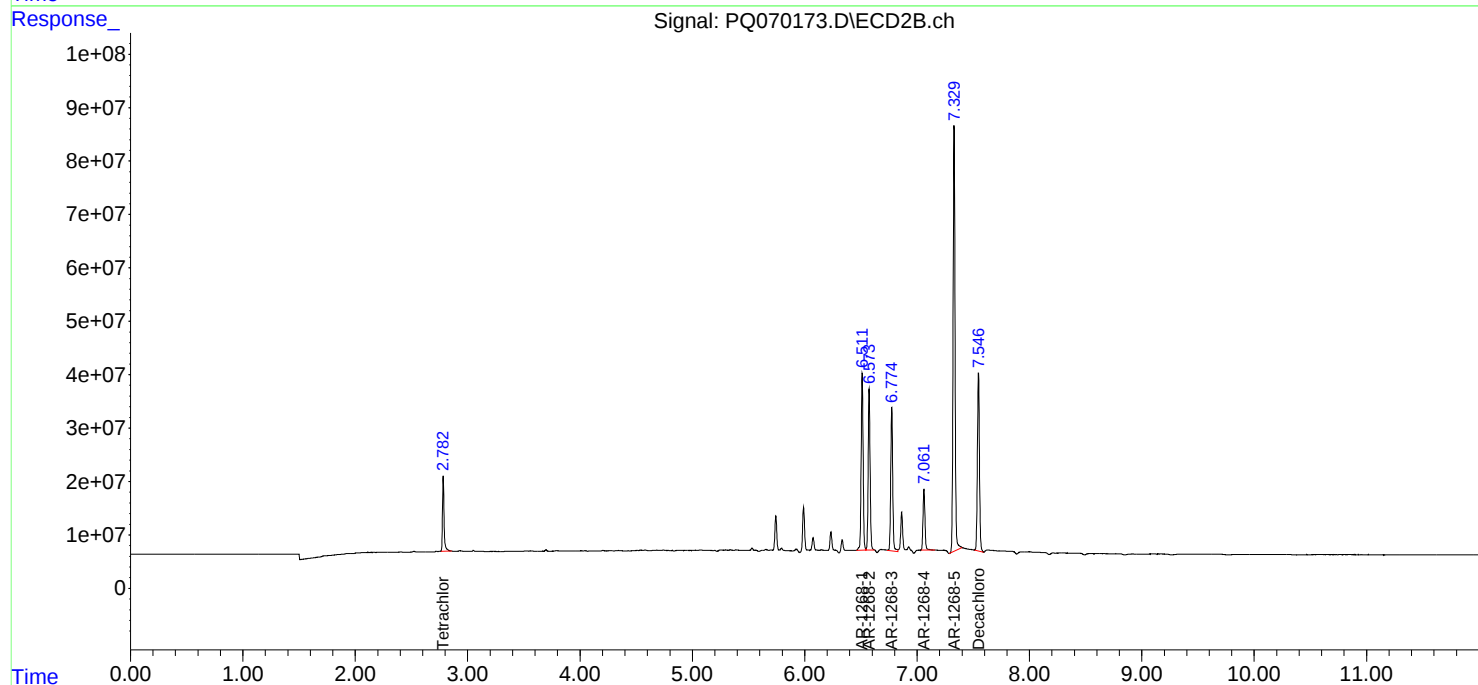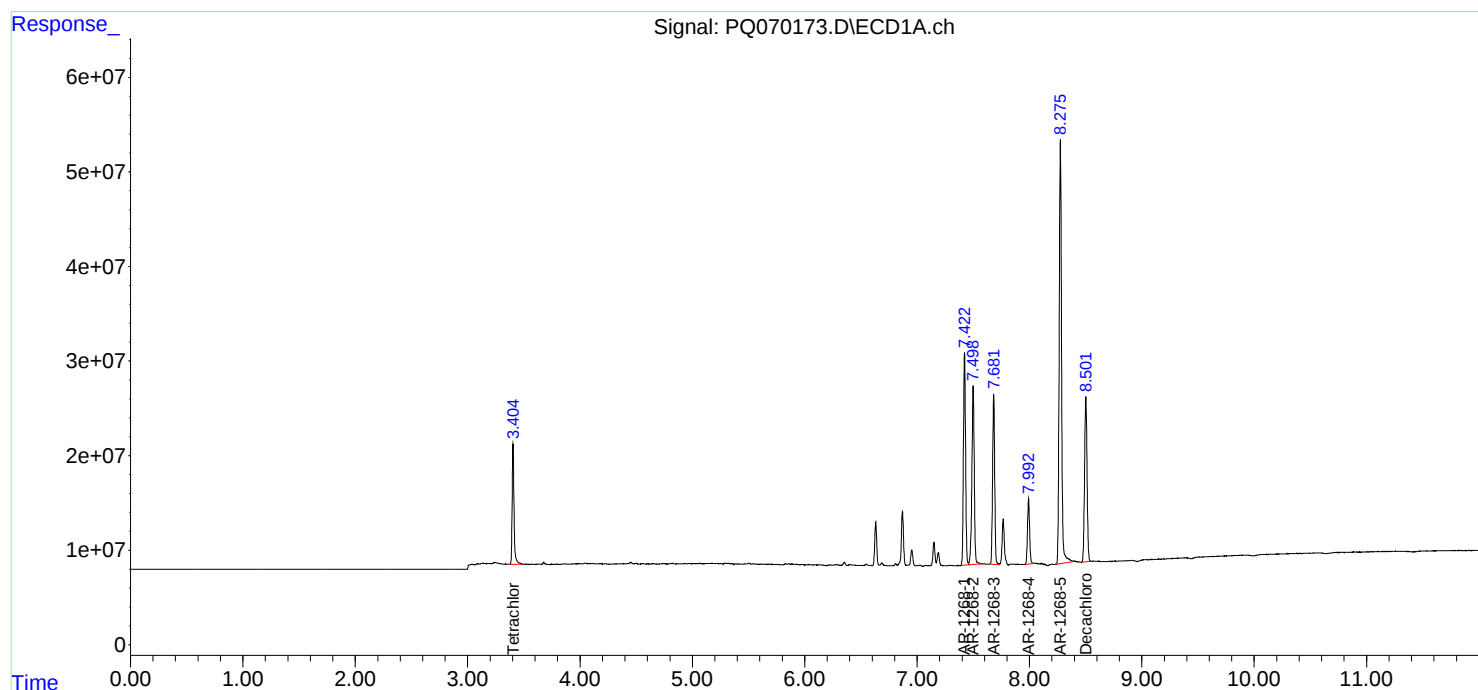

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070174.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 18:54
 Operator : YP\AJ
 Sample : AR1268ICC800
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12684026

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 09:43:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 10 09:41:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.783	266.1E6	255.5E6	36.902	37.259
2) SA Decachlor...	8.503	7.546	496.2E6	757.8E6	73.301	72.235
Target Compounds						
41) L9 AR-1268-1	7.423	6.512	544.5E6	737.9E6	748.917	739.944
42) L9 AR-1268-2	7.500	6.574	509.3E6	679.1E6	741.556	752.446
43) L9 AR-1268-3	7.681	6.775	419.0E6	595.7E6	735.962	719.065
44) L9 AR-1268-4	7.992	7.061	168.7E6	255.7E6	732.485	740.802
45) L9 AR-1268-5	8.275	7.329	1216.5E6	1832.0E6	742.534	745.241



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070174.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 18:54
Operator : YP\AJ
Sample : AR1268ICC800
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12684026

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 09:43:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 10 09:41:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

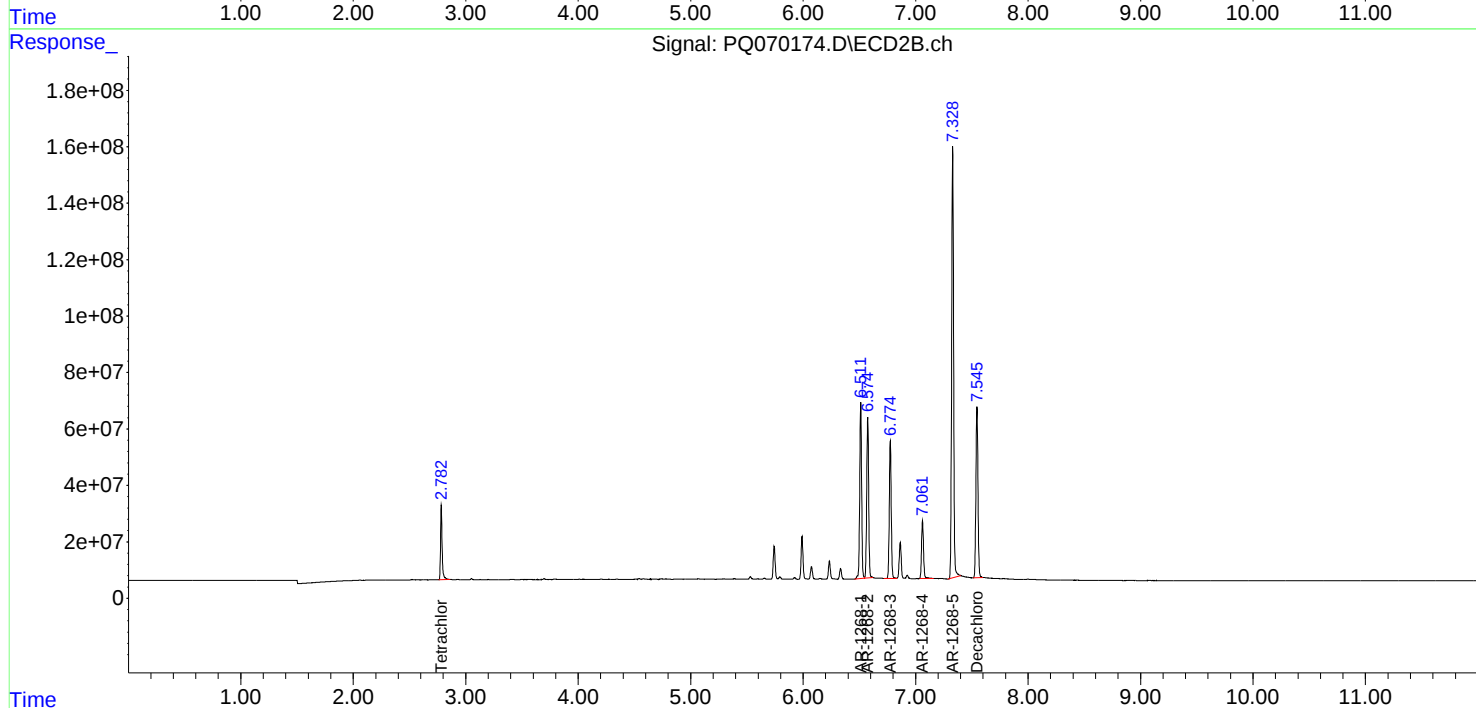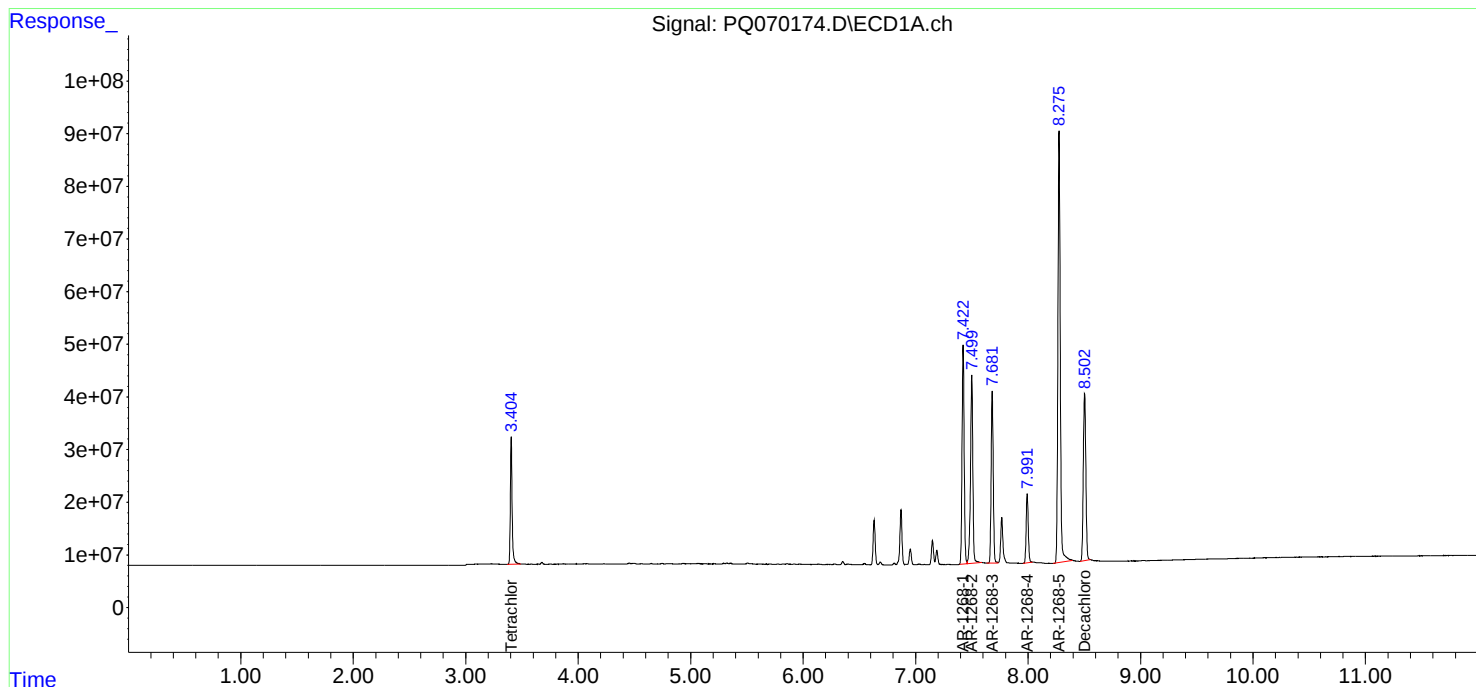

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
 Data File : PQ070175.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 19:09
 Operator : YP\AJ
 Sample : AR1268ICC1600
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AR12685027

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 09:43:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 10 09:41:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.405	2.783	503.2E6	485.1E6	69.769	70.756
2) SA Decachlor...	8.502	7.546	942.2E6	1442.0E6	139.177	137.456
Target Compounds						
41) L9 AR-1268-1	7.423	6.511	1049.0E6	1427.8E6	1442.753	1431.631
42) L9 AR-1268-2	7.500	6.574	980.3E6	1324.4E6	1427.279	1467.384
43) L9 AR-1268-3	7.681	6.774	808.3E6	1152.0E6	1419.918	1390.434
44) L9 AR-1268-4	7.993	7.061	322.9E6	488.5E6	1402.210	1415.181
45) L9 AR-1268-5	8.276	7.329	2373.1E6	3577.5E6	1448.512	1455.295



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040925\
Data File : PQ070175.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 19:09
Operator : YP\AJ
Sample : AR1268ICC1600
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
AR12685027

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 09:43:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040925CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 10 09:41:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

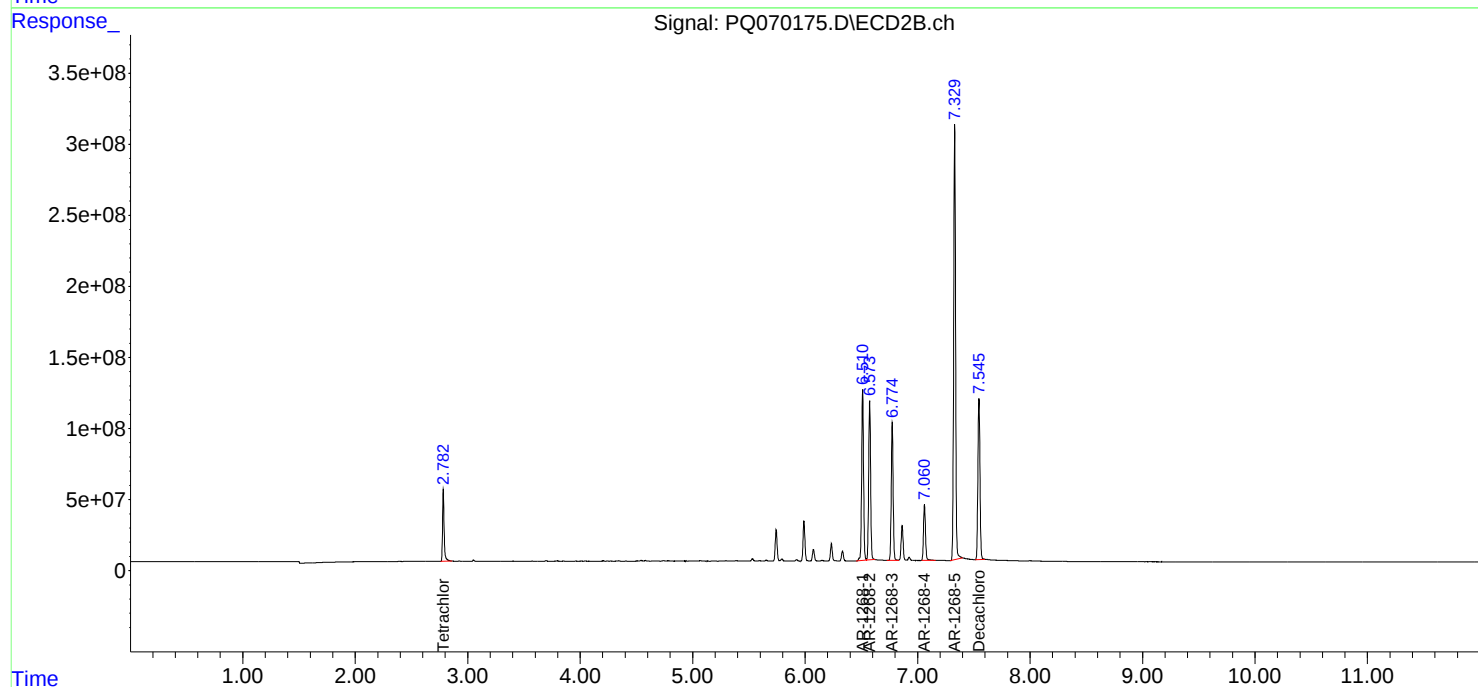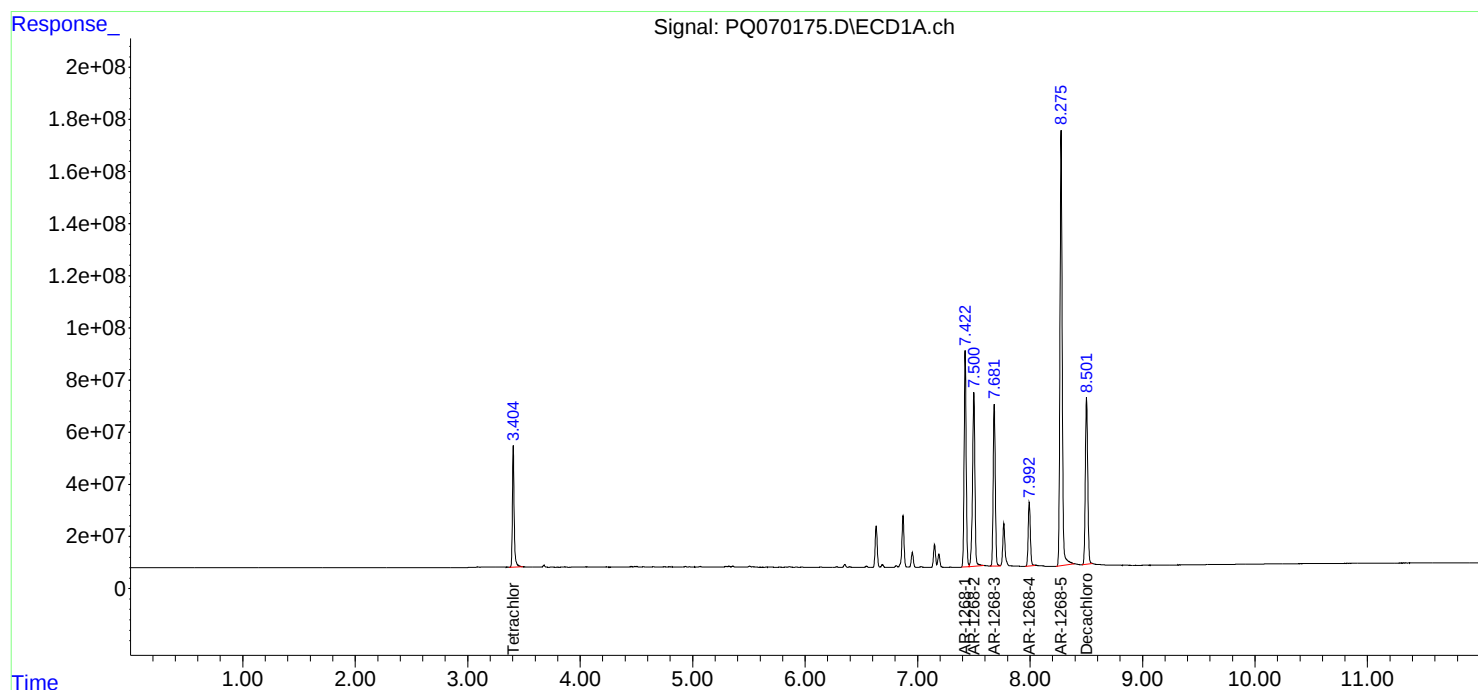

Analytical Sequence

Client: Chemtech Consulting Group

SDG No.: Q1942

Project: Weekly Storage Blanks

Instrument ID: ECD_Q

GC Column: ZB-MR1

ID: 0.32 (mm)

Inst. Calib. Date(s): 04/09/2025

04/09/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
AR16601038	AR1660ICC100	04/09/2025	09:41	PQ070136.D	8.50	3.40
AR16602039	AR1660ICC200	04/09/2025	09:55	PQ070137.D	8.50	3.41
AR16603040	AR1660ICC400	04/09/2025	10:10	PQ070138.D	8.50	3.40
AR16604041	AR1660ICC800	04/09/2025	10:25	PQ070139.D	8.50	3.41
AR16605042	AR1660ICC1600	04/09/2025	10:39	PQ070140.D	8.50	3.41
AR12211043	AR1221ICC100	04/09/2025	10:54	PQ070141.D	8.50	3.41
AR12212044	AR1221ICC200	04/09/2025	11:08	PQ070142.D	8.50	3.41
AR12213045	AR1221ICC400	04/09/2025	11:23	PQ070143.D	8.50	3.40
AR12214046	AR1221ICC800	04/09/2025	11:37	PQ070144.D	8.50	3.41
AR12215047	AR1221ICC1600	04/09/2025	11:52	PQ070145.D	8.50	3.41
AR12321048	AR1232ICC100	04/09/2025	12:07	PQ070146.D	8.50	3.40
AR12322049	AR1232ICC200	04/09/2025	12:21	PQ070147.D	8.50	3.41
AR12323050	AR1232ICC400	04/09/2025	12:36	PQ070148.D	8.50	3.40
AR12324001	AR1232ICC800	04/09/2025	12:50	PQ070149.D	8.50	3.41
AR12325002	AR1232ICC1600	04/09/2025	13:05	PQ070150.D	8.50	3.40
AR12421003	AR1242ICC100	04/09/2025	13:19	PQ070151.D	8.50	3.40
AR12422004	AR1242ICC200	04/09/2025	13:34	PQ070152.D	8.50	3.41
AR12423005	AR1242ICC400	04/09/2025	13:49	PQ070153.D	8.50	3.40
AR12424006	AR1242ICC800	04/09/2025	14:03	PQ070154.D	8.50	3.40
AR12425007	AR1242ICC1600	04/09/2025	14:18	PQ070155.D	8.50	3.40
AR12481008	AR1248ICC100	04/09/2025	14:32	PQ070156.D	8.50	3.40
AR12482009	AR1248ICC200	04/09/2025	14:47	PQ070157.D	8.50	3.41
AR12483010	AR1248ICC400	04/09/2025	15:01	PQ070158.D	8.50	3.40
AR12484011	AR1248ICC800	04/09/2025	15:16	PQ070159.D	8.50	3.40
AR12485012	AR1248ICC1600	04/09/2025	15:31	PQ070160.D	8.50	3.41
AR12541013	AR1254ICC100	04/09/2025	15:45	PQ070161.D	8.50	3.40
AR12542014	AR1254ICC200	04/09/2025	16:00	PQ070162.D	8.50	3.41
AR12543015	AR1254ICC400	04/09/2025	16:14	PQ070163.D	8.50	3.40
AR12544016	AR1254ICC800	04/09/2025	16:29	PQ070164.D	8.50	3.40
AR12545017	AR1254ICC1600	04/09/2025	16:43	PQ070165.D	8.50	3.40
AR12621018	AR1262ICC100	04/09/2025	16:58	PQ070166.D	8.50	3.40
AR12622019	AR1262ICC200	04/09/2025	17:13	PQ070167.D	8.50	3.41
AR12623020	AR1262ICC400	04/09/2025	17:27	PQ070168.D	8.50	3.40
AR12624021	AR1262ICC800	04/09/2025	17:42	PQ070169.D	8.50	3.40
AR12625022	AR1262ICC1600	04/09/2025	17:56	PQ070170.D	8.50	3.40
AR12681023	AR1268ICC100	04/09/2025	18:11	PQ070171.D	8.50	3.41
AR12682024	AR1268ICC200	04/09/2025	18:25	PQ070172.D	8.50	3.41
AR12683025	AR1268ICC400	04/09/2025	18:40	PQ070173.D	8.50	3.40
AR12684026	AR1268ICC800	04/09/2025	18:54	PQ070174.D	8.50	3.40
AR12685027	AR1268ICC1600	04/09/2025	19:09	PQ070175.D	8.50	3.41
PCB-GPC2-BLANK	Q1942-13	05/06/2025	10:42	PQ070236.D	0.00	0.00
PCB-GPC2-BLANK-SPIKE	Q1942-14	05/06/2025	10:56	PQ070237.D	0.00	0.00

Analytical Sequence

Analytical Sequence

Client: Chemtech Consulting Group	SDG No.: Q1942
Project: Weekly Storage Blanks	Instrument ID: ECD_Q
GC Column: ZB-MR2	ID: 0.32 (mm) Inst. Calib. Date(s): 04/09/2025 04/09/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
AR16601038	AR1660ICC100	04/09/2025	09:41	PQ070136.D	7.55	2.78
AR16602039	AR1660ICC200	04/09/2025	09:55	PQ070137.D	7.55	2.78
AR16603040	AR1660ICC400	04/09/2025	10:10	PQ070138.D	7.55	2.78
AR16604041	AR1660ICC800	04/09/2025	10:25	PQ070139.D	7.55	2.78
AR16605042	AR1660ICC1600	04/09/2025	10:39	PQ070140.D	7.55	2.78
AR12211043	AR1221ICC100	04/09/2025	10:54	PQ070141.D	7.55	2.78
AR12212044	AR1221ICC200	04/09/2025	11:08	PQ070142.D	7.55	2.78
AR12213045	AR1221ICC400	04/09/2025	11:23	PQ070143.D	7.55	2.78
AR12214046	AR1221ICC800	04/09/2025	11:37	PQ070144.D	7.55	2.78
AR12215047	AR1221ICC1600	04/09/2025	11:52	PQ070145.D	7.55	2.78
AR12321048	AR1232ICC100	04/09/2025	12:07	PQ070146.D	7.55	2.78
AR12322049	AR1232ICC200	04/09/2025	12:21	PQ070147.D	7.55	2.78
AR12323050	AR1232ICC400	04/09/2025	12:36	PQ070148.D	7.55	2.78
AR12324001	AR1232ICC800	04/09/2025	12:50	PQ070149.D	7.55	2.78
AR12325002	AR1232ICC1600	04/09/2025	13:05	PQ070150.D	7.55	2.78
AR12421003	AR1242ICC100	04/09/2025	13:19	PQ070151.D	7.55	2.78
AR12422004	AR1242ICC200	04/09/2025	13:34	PQ070152.D	7.55	2.78
AR12423005	AR1242ICC400	04/09/2025	13:49	PQ070153.D	7.55	2.78
AR12424006	AR1242ICC800	04/09/2025	14:03	PQ070154.D	7.55	2.78
AR12425007	AR1242ICC1600	04/09/2025	14:18	PQ070155.D	7.55	2.78
AR12481008	AR1248ICC100	04/09/2025	14:32	PQ070156.D	7.55	2.78
AR12482009	AR1248ICC200	04/09/2025	14:47	PQ070157.D	7.55	2.78
AR12483010	AR1248ICC400	04/09/2025	15:01	PQ070158.D	7.55	2.78
AR12484011	AR1248ICC800	04/09/2025	15:16	PQ070159.D	7.55	2.78
AR12485012	AR1248ICC1600	04/09/2025	15:31	PQ070160.D	7.55	2.78
AR12541013	AR1254ICC100	04/09/2025	15:45	PQ070161.D	7.55	2.78
AR12542014	AR1254ICC200	04/09/2025	16:00	PQ070162.D	7.55	2.78
AR12543015	AR1254ICC400	04/09/2025	16:14	PQ070163.D	7.55	2.78
AR12544016	AR1254ICC800	04/09/2025	16:29	PQ070164.D	7.55	2.78
AR12545017	AR1254ICC1600	04/09/2025	16:43	PQ070165.D	7.55	2.78
AR12621018	AR1262ICC100	04/09/2025	16:58	PQ070166.D	7.54	2.78
AR12622019	AR1262ICC200	04/09/2025	17:13	PQ070167.D	7.55	2.78
AR12623020	AR1262ICC400	04/09/2025	17:27	PQ070168.D	7.55	2.78
AR12624021	AR1262ICC800	04/09/2025	17:42	PQ070169.D	7.55	2.78
AR12625022	AR1262ICC1600	04/09/2025	17:56	PQ070170.D	7.55	2.78
AR12681023	AR1268ICC100	04/09/2025	18:11	PQ070171.D	7.55	2.78
AR12682024	AR1268ICC200	04/09/2025	18:25	PQ070172.D	7.54	2.78
AR12683025	AR1268ICC400	04/09/2025	18:40	PQ070173.D	7.55	2.78
AR12684026	AR1268ICC800	04/09/2025	18:54	PQ070174.D	7.55	2.78
AR12685027	AR1268ICC1600	04/09/2025	19:09	PQ070175.D	7.55	2.78
PCB-GPC2-BLANK	Q1942-13	05/06/2025	10:42	PQ070236.D	0.00	0.00
PCB-GPC2-BLANK-SPIKE	Q1942-14	05/06/2025	10:56	PQ070237.D	0.00	0.00

Analytical Sequence

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

PCB-GPC2-BLANK-SPIK

Contract: CHEM02

Lab Code: CHEM Case No.: Q1942 SAS No.: Q1942 SDG NO.: Q1942

Lab Sample ID: Q1942-14 Date(s) Analyzed: 05/06/2025 05/06/2025

Instrument ID (1): ECD_Q Instrument ID (2): ECD_Q

GC Column: (1): ZB-MR1 ID: 0.32 (mm) GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PQ070237.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	4.486	4.436	4.536	178	182	5.9
COLUMN 1	2	4.505	4.455	4.555	190		
	3	4.563	4.513	4.613	187		
	4	4.652	4.602	4.702	182		
	5	4.936	4.886	4.986	172		
	1	3.785	3.735	3.835	189		
COLUMN 2	2	3.801	3.751	3.851	219	193	
	3	3.961	3.911	4.011	188		
	4	4.009	3.959	4.059	182		
	5	4.204	4.154	4.254	185		
Aroclor-1260	1	6.026	5.976	6.076	204	190	10.3
COLUMN 1	2	6.282	6.232	6.332	201		
	3	6.632	6.582	6.682	168		
	4	6.847	6.797	6.897	188		
	5	7.152	7.102	7.202	187		
	1	5.197	5.147	5.247	220	209	
COLUMN 2	2	5.387	5.337	5.437	218		
	3	5.528	5.478	5.578	217		
	4	5.988	5.938	6.038	186		
	5	6.233	6.183	6.283	204		



QC SAMPLE DATA

Manual Integration Report

Sequence:

PQ040925

Instrument

ECD_q

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1262ICC100	PQ070166.D	AR-1262-1 #2	yogesh	4/10/2025 10:27:07 AM	mohammad	4/14/2025 12:39:35	Peak Integrated by Software
AR1262ICC100	PQ070166.D	AR-1262-2 #2	yogesh	4/10/2025 10:27:07 AM	mohammad	4/14/2025 12:39:35	Peak Integrated by Software
AR1262ICC100	PQ070166.D	Decachlorobiphenyl #2	yogesh	4/10/2025 10:27:07 AM	mohammad	4/14/2025 12:39:35	Peak Integrated by Software



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

Manual Integration Report

Sequence:

Pq050625

Instrument

ECD_q

Sample ID

File ID

Parameter

Review By

Review On

Supervised
By

Supervised On

Reason

Instrument ID: ECD_Q

Daily Analysis Runlog For Sequence/QC Batch ID # PQ040925

Review By	yogesh	Review On	4/10/2025 8:36:14 AM
Supervise By	mohammad	Supervise On	4/14/2025 12:39:35 AM
SubDirectory	PQ040925	HP Acquire Method	HP Processing Method PQ040925
STD. NAME	STD REF.#		
Tune/Reschk	PP24020,PP24019,PP24018,PP24017,PP24016,PP24025,PP24024,PP24023,PP24022,PP24021,PP24030,PP24029,PP24028,PP24027,PP24026,PP24035,PP24034,PP24033,PP24032,PP24031,PP24040,PP24039,PP24038,PP24037,PP24036,PP24045,PP24044,PP24043,PP24042,PP24041,PP24050,PP24049,PP24048,PP24047,PP24046,PP24055,PP24054,PP24053,PP24052,PP24051		
Initial Calibration Stds			
CCC			
Internal Standard/PEM			
ICV/I.BLK			
Surrogate Standard			
MS/MSD Standard			
LCS Standard	PP24018,PP24023,PP24028,PP24033,PP24038,PP24043,PP24048,PP24053		

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PQ070134.D	09 Apr 2025 09:12	YP\AJ	Ok
2	AIBLK13	PQ070135.D	09 Apr 2025 09:26	YP\AJ	Ok
3	AR1660ICC100	PQ070136.D	09 Apr 2025 09:41	YP\AJ	Ok
4	AR1660ICC200	PQ070137.D	09 Apr 2025 09:55	YP\AJ	Ok
5	AR1660ICC400	PQ070138.D	09 Apr 2025 10:10	YP\AJ	Ok
6	AR1660ICC800	PQ070139.D	09 Apr 2025 10:25	YP\AJ	Ok
7	AR1660ICC1600	PQ070140.D	09 Apr 2025 10:39	YP\AJ	Ok
8	AR1221ICC100	PQ070141.D	09 Apr 2025 10:54	YP\AJ	Ok
9	AR1221ICC200	PQ070142.D	09 Apr 2025 11:08	YP\AJ	Ok
10	AR1221ICC400	PQ070143.D	09 Apr 2025 11:23	YP\AJ	Ok
11	AR1221ICC800	PQ070144.D	09 Apr 2025 11:37	YP\AJ	Ok
12	AR1221ICC1600	PQ070145.D	09 Apr 2025 11:52	YP\AJ	Ok
13	AR1232ICC100	PQ070146.D	09 Apr 2025 12:07	YP\AJ	Ok
14	AR1232ICC200	PQ070147.D	09 Apr 2025 12:21	YP\AJ	Ok
15	AR1232ICC400	PQ070148.D	09 Apr 2025 12:36	YP\AJ	Ok
16	AR1232ICC800	PQ070149.D	09 Apr 2025 12:50	YP\AJ	Ok
17	AR1232ICC1600	PQ070150.D	09 Apr 2025 13:05	YP\AJ	Ok
18	AR1242ICC100	PQ070151.D	09 Apr 2025 13:19	YP\AJ	Ok
19	AR1242ICC200	PQ070152.D	09 Apr 2025 13:34	YP\AJ	Ok
20	AR1242ICC400	PQ070153.D	09 Apr 2025 13:49	YP\AJ	Ok
21	AR1242ICC800	PQ070154.D	09 Apr 2025 14:03	YP\AJ	Ok

Instrument ID: ECD_Q

Daily Analysis Runlog For Sequence/QC Batch ID # PQ040925

Review By	yogesh	Review On	4/10/2025 8:36:14 AM
Supervise By	mohammad	Supervise On	4/14/2025 12:39:35 AM
SubDirectory	PQ040925	HP Acquire Method	HP Processing Method PQ040925
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24020,PP24019,PP24018,PP24017,PP24016,PP24025,PP24024,PP24023,PP24022,PP24021,PP24030,PP24029,PP24028,PP24027,PP24026,PP24035,PP24034,PP24033,PP24032,PP24031,PP24040,PP24039,PP24038,PP24037,PP24036,PP24045,PP24044,PP24043,PP24042,PP24041,PP24050,PP24049,PP24048,PP24047,PP24046,PP24055,PP24054,PP24053,PP24052,PP24051		
CCC	PP24018,PP24023,PP24028,PP24033,PP24038,PP24043,PP24048,PP24053		
Internal Standard/PEM			
ICV/I.BLK			
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	AR1242ICC1600	PQ070155.D	09 Apr 2025 14:18	YP\AJ	Ok
23	AR1248ICC100	PQ070156.D	09 Apr 2025 14:32	YP\AJ	Ok
24	AR1248ICC200	PQ070157.D	09 Apr 2025 14:47	YP\AJ	Ok
25	AR1248ICC400	PQ070158.D	09 Apr 2025 15:01	YP\AJ	Ok
26	AR1248ICC800	PQ070159.D	09 Apr 2025 15:16	YP\AJ	Ok
27	AR1248ICC1600	PQ070160.D	09 Apr 2025 15:31	YP\AJ	Ok
28	AR1254ICC100	PQ070161.D	09 Apr 2025 15:45	YP\AJ	Ok
29	AR1254ICC200	PQ070162.D	09 Apr 2025 16:00	YP\AJ	Ok
30	AR1254ICC400	PQ070163.D	09 Apr 2025 16:14	YP\AJ	Ok
31	AR1254ICC800	PQ070164.D	09 Apr 2025 16:29	YP\AJ	Ok
32	AR1254ICC1600	PQ070165.D	09 Apr 2025 16:43	YP\AJ	Ok
33	AR1262ICC100	PQ070166.D	09 Apr 2025 16:58	YP\AJ	Ok,M
34	AR1262ICC200	PQ070167.D	09 Apr 2025 17:13	YP\AJ	Ok
35	AR1262ICC400	PQ070168.D	09 Apr 2025 17:27	YP\AJ	Ok
36	AR1262ICC800	PQ070169.D	09 Apr 2025 17:42	YP\AJ	Ok
37	AR1262ICC1600	PQ070170.D	09 Apr 2025 17:56	YP\AJ	Ok
38	AR1268ICC100	PQ070171.D	09 Apr 2025 18:11	YP\AJ	Ok
39	AR1268ICC200	PQ070172.D	09 Apr 2025 18:25	YP\AJ	Ok
40	AR1268ICC400	PQ070173.D	09 Apr 2025 18:40	YP\AJ	Ok
41	AR1268ICC800	PQ070174.D	09 Apr 2025 18:54	YP\AJ	Ok
42	AR1268ICC1600	PQ070175.D	09 Apr 2025 19:09	YP\AJ	Ok
43	AIBLK14	PQ070176.D	09 Apr 2025 19:24	YP\AJ	Ok

M : Manual Integration

Instrument ID: ECD_Q

Daily Analysis Runlog For Sequence/QC Batch ID # PQ050625

Review By	yogesh	Review On	5/6/2025 11:34:46 AM
Supervise By		Supervise On	
SubDirectory	PQ050625	HP Acquire Method	HP Processing Method PQ040925
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24020,PP24019,PP24018,PP24017,PP24016,PP24025,PP24024,PP24023,PP24022,PP24021,PP24030,PP24029,PP24028,PP24027,PP24026,PP24035,PP24034,PP24033,PP24032,PP24031,PP24040,PP24039,PP24038,PP24037,PP24036,PP24045,PP24044,PP24043,PP24042,PP24041,PP24050,PP24049,PP24048,PP24047,PP24046,PP24055,PP24054,PP24053,PP24052,PP24051		
CCC	PP24018,PP24023,PP24028,PP24033,PP24038,PP24043,PP24048,PP24053		
Internal Standard/PEM			
ICV/I.BLK			
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PQ070233.D	06 May 2025 09:51	YP\AJ	Ok
2	AIBLK22	PQ070234.D	06 May 2025 10:06	YP\AJ	Ok
3	AR1660CCC400	PQ070235.D	06 May 2025 10:20	YP\AJ	Ok
4	Q1942-13	PQ070236.D	06 May 2025 10:42	YP\AJ	Ok
5	Q1942-14	PQ070237.D	06 May 2025 10:56	YP\AJ	Ok
6	AIBLK23	PQ070238.D	06 May 2025 11:11	YP\AJ	Ok
7	AR1660CCC400	PQ070239.D	06 May 2025 11:25	YP\AJ	Ok

M : Manual Integration

Instrument ID: ECD_Q

Daily Analysis Runlog For Sequence/QC Batch ID # PQ040925

Review By	yogesh	Review On	4/10/2025 8:36:14 AM
Supervise By	mohammad	Supervise On	4/14/2025 12:39:35 AM
SubDirectory	PQ040925	HP Acquire Method	HP Processing Method PQ040925
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24020,PP24019,PP24018,PP24017,PP24016,PP24025,PP24024,PP24023,PP24022,PP24021,PP24030,PP24029,PP24028,PP24027,PP24026,P P24035,PP24034,PP24033,PP24032,PP24031,PP24040,PP24039,PP24038,PP24037,PP24036,PP24045,PP24044,PP24043,PP24042,PP24041,PP 24050,PP24049,PP24048,PP24047,PP24046,PP24055,PP24054,PP24053,PP24052,PP24051 PP24018,PP24023,PP24028,PP24033,PP24038,PP24043,PP24048,PP24053		

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PQ070134.D	09 Apr 2025 09:12		YP\AJ	Ok
2	AIBLK13	AIBLK340	PQ070135.D	09 Apr 2025 09:26		YP\AJ	Ok
3	AR1660ICC100	AR16601038	PQ070136.D	09 Apr 2025 09:41		YP\AJ	Ok
4	AR1660ICC200	AR16602039	PQ070137.D	09 Apr 2025 09:55		YP\AJ	Ok
5	AR1660ICC400	AR16603040	PQ070138.D	09 Apr 2025 10:10		YP\AJ	Ok
6	AR1660ICC800	AR16604041	PQ070139.D	09 Apr 2025 10:25		YP\AJ	Ok
7	AR1660ICC1600	AR16605042	PQ070140.D	09 Apr 2025 10:39		YP\AJ	Ok
8	AR1221ICC100	AR12211043	PQ070141.D	09 Apr 2025 10:54		YP\AJ	Ok
9	AR1221ICC200	AR12212044	PQ070142.D	09 Apr 2025 11:08		YP\AJ	Ok
10	AR1221ICC400	AR12213045	PQ070143.D	09 Apr 2025 11:23		YP\AJ	Ok
11	AR1221ICC800	AR12214046	PQ070144.D	09 Apr 2025 11:37		YP\AJ	Ok
12	AR1221ICC1600	AR12215047	PQ070145.D	09 Apr 2025 11:52		YP\AJ	Ok
13	AR1232ICC100	AR12321048	PQ070146.D	09 Apr 2025 12:07		YP\AJ	Ok
14	AR1232ICC200	AR12322049	PQ070147.D	09 Apr 2025 12:21		YP\AJ	Ok
15	AR1232ICC400	AR12323050	PQ070148.D	09 Apr 2025 12:36		YP\AJ	Ok
16	AR1232ICC800	AR12324001	PQ070149.D	09 Apr 2025 12:50		YP\AJ	Ok
17	AR1232ICC1600	AR12325002	PQ070150.D	09 Apr 2025 13:05		YP\AJ	Ok
18	AR1242ICC100	AR12421003	PQ070151.D	09 Apr 2025 13:19		YP\AJ	Ok

Instrument ID: ECD_Q

Daily Analysis Runlog For Sequence/QC Batch ID # PQ040925

Review By	yogesh	Review On	4/10/2025 8:36:14 AM
Supervise By	mohammad	Supervise On	4/14/2025 12:39:35 AM
SubDirectory	PQ040925	HP Acquire Method	HP Processing Method PQ040925
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24020,PP24019,PP24018,PP24017,PP24016,PP24025,PP24024,PP24023,PP24022,PP24021,PP24030,PP24029,PP24028,PP24027,PP24026,P P24035,PP24034,PP24033,PP24032,PP24031,PP24040,PP24039,PP24038,PP24037,PP24036,PP24045,PP24044,PP24043,PP24042,PP24041,PP 24050,PP24049,PP24048,PP24047,PP24046,PP24055,PP24054,PP24053,PP24052,PP24051 PP24018,PP24023,PP24028,PP24033,PP24038,PP24043,PP24048,PP24053		

19	AR1242ICC200	AR12422004	PQ070152.D	09 Apr 2025 13:34		YPIAJ	Ok
20	AR1242ICC400	AR12423005	PQ070153.D	09 Apr 2025 13:49		YPIAJ	Ok
21	AR1242ICC800	AR12424006	PQ070154.D	09 Apr 2025 14:03		YPIAJ	Ok
22	AR1242ICC1600	AR12425007	PQ070155.D	09 Apr 2025 14:18		YPIAJ	Ok
23	AR1248ICC100	AR12481008	PQ070156.D	09 Apr 2025 14:32		YPIAJ	Ok
24	AR1248ICC200	AR12482009	PQ070157.D	09 Apr 2025 14:47		YPIAJ	Ok
25	AR1248ICC400	AR12483010	PQ070158.D	09 Apr 2025 15:01		YPIAJ	Ok
26	AR1248ICC800	AR12484011	PQ070159.D	09 Apr 2025 15:16		YPIAJ	Ok
27	AR1248ICC1600	AR12485012	PQ070160.D	09 Apr 2025 15:31		YPIAJ	Ok
28	AR1254ICC100	AR12541013	PQ070161.D	09 Apr 2025 15:45		YPIAJ	Ok
29	AR1254ICC200	AR12542014	PQ070162.D	09 Apr 2025 16:00		YPIAJ	Ok
30	AR1254ICC400	AR12543015	PQ070163.D	09 Apr 2025 16:14		YPIAJ	Ok
31	AR1254ICC800	AR12544016	PQ070164.D	09 Apr 2025 16:29		YPIAJ	Ok
32	AR1254ICC1600	AR12545017	PQ070165.D	09 Apr 2025 16:43		YPIAJ	Ok
33	AR1262ICC100	AR12621018	PQ070166.D	09 Apr 2025 16:58		YPIAJ	Ok,M
34	AR1262ICC200	AR12622019	PQ070167.D	09 Apr 2025 17:13		YPIAJ	Ok
35	AR1262ICC400	AR12623020	PQ070168.D	09 Apr 2025 17:27		YPIAJ	Ok
36	AR1262ICC800	AR12624021	PQ070169.D	09 Apr 2025 17:42		YPIAJ	Ok
37	AR1262ICC1600	AR12625022	PQ070170.D	09 Apr 2025 17:56		YPIAJ	Ok

Instrument ID: ECD_Q

Daily Analysis Runlog For Sequence/QC Batch ID # PQ040925

Review By	yogesh	Review On	4/10/2025 8:36:14 AM
Supervise By	mohammad	Supervise On	4/14/2025 12:39:35 AM
SubDirectory	PQ040925	HP Acquire Method	HP Processing Method PQ040925
STD. NAME	STD REF.#		
Tune/Reschk	PP24020,PP24019,PP24018,PP24017,PP24016,PP24025,PP24024,PP24023,PP24022,PP24021,PP24030,PP24029,PP24028,PP24027,PP24026,P P24035,PP24034,PP24033,PP24032,PP24031,PP24040,PP24039,PP24038,PP24037,PP24036,PP24045,PP24044,PP24043,PP24042,PP24041,PP 24050,PP24049,PP24048,PP24047,PP24046,PP24055,PP24054,PP24053,PP24052,PP24051		
Initial Calibration Stds			
CCC			
Internal Standard/PEM			
ICV/I.BLK			
Surrogate Standard			
MS/MSD Standard			
LCS Standard	PP24018,PP24023,PP24028,PP24033,PP24038,PP24043,PP24048,PP24053		

38	AR1268ICC100	AR12681023	PQ070171.D	09 Apr 2025 18:11		YP\AJ	Ok
39	AR1268ICC200	AR12682024	PQ070172.D	09 Apr 2025 18:25		YP\AJ	Ok
40	AR1268ICC400	AR12683025	PQ070173.D	09 Apr 2025 18:40		YP\AJ	Ok
41	AR1268ICC800	AR12684026	PQ070174.D	09 Apr 2025 18:54		YP\AJ	Ok
42	AR1268ICC1600	AR12685027	PQ070175.D	09 Apr 2025 19:09		YP\AJ	Ok
43	AIBLK14	AIBLK341	PQ070176.D	09 Apr 2025 19:24		YP\AJ	Ok

M : Manual Integration

Instrument ID: ECD_Q

Daily Analysis Runlog For Sequence/QC Batch ID # PQ050625

Review By	yogesh	Review On	5/6/2025 11:34:46 AM
Supervise By		Supervise On	
SubDirectory	PQ050625	HP Acquire Method	HP Processing Method PQ040925
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24020,PP24019,PP24018,PP24017,PP24016,PP24025,PP24024,PP24023,PP24022,PP24021,PP24030,PP24029,PP24028,PP24027,PP24026,PP24035,PP24034,PP24033,PP24032,PP24031,PP24040,PP24039,PP24038,PP24037,PP24036,PP24045,PP24044,PP24043,PP24042,PP24041,PP24050,PP24049,PP24048,PP24047,PP24046,PP24055,PP24054,PP24053,PP24052,PP24051		
CCC	PP24018,PP24023,PP24028,PP24033,PP24038,PP24043,PP24048,PP24053		
Internal Standard/PEM			
ICV/I.BLK			
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	Sampleld	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PQ070233.D	06 May 2025 09:51		YP\AJ	Ok
2	AIBLK22	AIBLK348	PQ070234.D	06 May 2025 10:06		YP\AJ	Ok
3	AR1660CCC400	AR16603158	PQ070235.D	06 May 2025 10:20		YP\AJ	Ok
4	Q1942-13	PCB-GPC2-BLANK	PQ070236.D	06 May 2025 10:42		YP\AJ	Ok
5	Q1942-14	PCB-GPC2-BLANK-SP	PQ070237.D	06 May 2025 10:56		YP\AJ	Ok
6	AIBLK23	AIBLK349	PQ070238.D	06 May 2025 11:11		YP\AJ	Ok
7	AR1660CCC400	AR16603159	PQ070239.D	06 May 2025 11:25		YP\AJ	Ok

M : Manual Integration



PERCENT SOLID

Supervisor: Iwona
Analyst: jignesh
Date: 5/5/2025

OVENTEMP IN Celsius(°C): 107
Time IN: 17:00
In Date: 05/02/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 104
Time OUT: 08:25
Out Date: 05/03/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLID- OVEN

QC:LB135646

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
Q1913-01	WC-12-S-202504	1	1.18	10.32	11.5	9.49	80.5	
Q1913-03	WC-13-S-202504	2	1.19	10.37	11.56	9.83	83.3	
Q1936-01	SMALL-PILE-A	33	1.15	9.94	11.09	10.18	90.8	
Q1936-02	SMALL-PILE-A	34	1.17	9.94	11.11	10.22	91.0	
Q1936-03	SMALL-PILE-B	35	1.18	10.39	11.57	10.93	93.8	
Q1936-04	SMALL-PILE-B	36	1.18	9.88	11.06	10.44	93.7	
Q1936-05	SMALL-PILE-C	37	1.15	10.03	11.18	10.9	97.2	
Q1936-06	SMALL-PILE-C	38	1.15	10.25	11.4	11.01	96.2	
Q1936-07	SMALL-PILE-D	39	1.16	10.41	11.57	10.97	94.2	
Q1936-08	SMALL-PILE-D	40	1.18	9.96	11.14	10.55	94.1	
Q1937-01	LARGE-PILE-A	41	1.15	10.13	11.28	10.7	94.3	
Q1937-02	LARGE-PILE-A	42	1.18	9.58	10.76	10.2	94.2	
Q1937-03	LARGE-PILE-B	43	1.15	10.03	11.18	10.82	96.4	
Q1937-04	LARGE-PILE-B	44	1.17	10.04	11.21	10.72	95.1	
Q1937-05	LARGE-PILE-C	45	1.16	10.19	11.35	10.83	94.9	
Q1937-06	LARGE-PILE-C	46	1.19	10.06	11.25	10.63	93.8	
Q1937-07	LARGE-PILE-D	47	1.18	10.33	11.51	10.95	94.6	
Q1937-08	LARGE-PILE-D	48	1.17	9.75	10.92	10.33	93.9	
Q1937-09	LARGE-PILE-E	49	1.16	10.14	11.3	10.52	92.3	
Q1937-10	LARGE-PILE-E	50	1.18	10.30	11.48	10.76	93.0	
Q1937-11	LARGE-PILE-F	51	1.18	10.48	11.66	10.58	89.7	
Q1937-12	LARGE-PILE-F	52	1.18	10.25	11.43	10.44	90.3	
Q1938-01	LOWER-WALL-PILE-A	53	1.15	10.33	11.48	10.77	93.1	
Q1938-02	LOWER-WALL-PILE-A	54	1.17	10.50	11.67	10.71	90.9	
Q1938-03	LOWER-WALL-PILE-B	55	1.14	10.15	11.29	10.94	96.6	
Q1938-04	LOWER-WALL-PILE-B	56	1.18	9.90	11.08	10.68	96.0	
Q1938-05	LOWER-WALL-PILE-C	57	1.17	10.23	11.4	11.07	96.8	
Q1938-06	LOWER-WALL-PILE-C	58	1.12	9.82	10.94	10.7	97.6	



PERCENT SOLID

Supervisor: Iwona
Analyst: jignesh
Date: 5/5/2025

OVENTEMP IN Celsius(°C): 107
Time IN: 17:00
In Date: 05/02/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 104
Time OUT: 08:25
Out Date: 05/03/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLID- OVEN

QC:LB135646

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
Q1938-07	LOWER-WALL-PILE-D	59	1.19	10.01	11.2	10.7	95.0	
Q1938-08	LOWER-WALL-PILE-D	60	1.17	10.23	11.4	10.86	94.7	
Q1942-05	SVOC-GPC-BLANK	3	1.00	1.00	2.00	2.00	100.0	
Q1942-06	PEST-GPC-BLANK	4	1.00	1.00	2.00	2.00	100.0	
Q1942-07	PEST-GPC-BLANK-SPIKE	5	1.00	1.00	2.00	2.00	100.0	
Q1942-08	PCB-GPC-BLANK	6	1.00	1.00	2.00	2.00	100.0	
Q1942-09	PCB-GPC-BLANK-SPIKE	7	1.00	1.00	2.00	2.00	100.0	
Q1942-10	SVOC-GPC2-BLANK	8	1.00	1.00	2.00	2.00	100.0	
Q1942-11	PEST-GPC2-BLANK	9	1.00	1.00	2.00	2.00	100.0	
Q1942-12	PEST-GPC2-BLANK-SPIKE	10	1.00	1.00	2.00	2.00	100.0	
Q1942-13	PCB-GPC2-BLANK	11	1.00	1.00	2.00	2.00	100.0	
Q1942-14	PCB-GCP2-BLANK-SPIKE	12	1.00	1.00	2.00	2.00	100.0	
Q1944-01	MELTED-RUBBER-SAMPLE	13	1.00	1.00	2.00	2.00	100.0	MELTED-RUBBER-SAMPLE
Q1946-01	BB-CONCRETE	14	1.00	1.00	2.00	2.00	100.0	CONCRETE sample
Q1946-02	BB-CONCRETE	15	1.00	1.00	2.00	2.00	100.0	CONCRETE sample
Q1947-01	MH-P	16	1.18	10.19	11.37	9.28	79.5	
Q1947-02	MH-P-EPH	17	1.15	10.84	11.99	10.64	87.5	
Q1947-03	MH-P-VOC	18	1.16	10.71	11.87	10.5	87.2	
Q1947-05	MH-O	19	1.14	10.59	11.73	10.52	88.6	
Q1947-06	MH-O-EPH	20	1.12	10.00	11.12	9.91	87.9	
Q1947-07	MH-O-VOC	21	1.17	10.00	11.17	9.95	87.8	
Q1951-01	MH-KK	22	1.18	10.40	11.58	10.01	84.9	
Q1951-02	MH-KK-EPH	23	1.16	10.29	11.45	9.91	85.0	
Q1951-03	MH-KK-VOC	24	1.17	10.25	11.42	9.86	84.8	
Q1952-01	CLEAN-FILL	25	1.18	10.49	11.67	8.98	74.4	
Q1952-02	CLEAN-FILL-E2	26	1.13	10.10	11.23	8.47	72.7	
Q1953-01	AUD-25-0075	27	1.00	1.00	2.00	2.00	100.0	pile
Q1953-02	AUD-25-0076	28	1.00	1.00	2.00	2.00	100.0	pile



PERCENT SOLID

Supervisor: Iwona
Analyst: jignesh
Date: 5/5/2025

OVENTEMP IN Celsius(°C): 107
Time IN: 17:00
In Date: 05/02/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 104
Time OUT: 08:25
Out Date: 05/03/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLID- OVEN

QC:LB135646

Lab ID	Client SampleID	Dish #	Dish Wt (g) (A)	Sample Wt (g)	Dish + Sample Wt (g) (B)	Dish+Dry Sample Wt (g) (C)	% Solid	Comments
Q1953-03	AUD-25-0077	29	1.00	1.00	2.00	2.00	100.0	oilc
Q1954-01	BC260874-1-1	30	1.00	1.00	2.00	2.00	100.0	oilc
Q1954-02	BC260874-1-2	31	1.00	1.00	2.00	2.00	100.0	oilc
Q1955-01	LAW-25-0066	32	1.00	1.00	2.00	2.00	100.0	stone sample, 100 % solids

$$\% \text{ Solid} = \frac{(C-A) * 100}{(B-A)}$$

WORKLIST(Hardcopy Internal Chain)

173546

WorkList Name : %1-050225

WorkList ID : 189289

Department : Wet-Chemistry

Date : 05-02-2025 14:36:21

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1913-01	WC-12-S-202504	Solid	Percent Solids	Cool 4 deg C	AECO02	L21	04/29/2025	Chemtech -SO
Q1913-03	WC-13-S-202504	Solid	Percent Solids	Cool 4 deg C	AECO02	L21	04/29/2025	Chemtech -SO
Q1936-01	SMALL-PILE-A	Solid	Percent Solids	Cool 4 deg C	SAXT01	L51	05/01/2025	Chemtech -SO
Q1936-02	SMALL-PILE-A	Solid	Percent Solids	Cool 4 deg C	SAXT01	L51	05/01/2025	Chemtech -SO
Q1936-03	SMALL-PILE-B	Solid	Percent Solids	Cool 4 deg C	SAXT01	L51	05/01/2025	Chemtech -SO
Q1936-04	SMALL-PILE-B	Solid	Percent Solids	Cool 4 deg C	SAXT01	L51	05/01/2025	Chemtech -SO
Q1936-05	SMALL-PILE-C	Solid	Percent Solids	Cool 4 deg C	SAXT01	L51	05/01/2025	Chemtech -SO
Q1936-06	SMALL-PILE-C	Solid	Percent Solids	Cool 4 deg C	SAXT01	L51	05/01/2025	Chemtech -SO
Q1936-07	SMALL-PILE-D	Solid	Percent Solids	Cool 4 deg C	SAXT01	L51	05/01/2025	Chemtech -SO
Q1936-08	SMALL-PILE-D	Solid	Percent Solids	Cool 4 deg C	SAXT01	L51	05/01/2025	Chemtech -SO
Q1937-01	LARGE-PILE-A	Solid	Percent Solids	Cool 4 deg C	SAXT01	L41	05/01/2025	Chemtech -SO
Q1937-02	LARGE-PILE-A	Solid	Percent Solids	Cool 4 deg C	SAXT01	L41	05/01/2025	Chemtech -SO
Q1937-03	LARGE-PILE-B	Solid	Percent Solids	Cool 4 deg C	SAXT01	L41	05/01/2025	Chemtech -SO
Q1937-04	LARGE-PILE-B	Solid	Percent Solids	Cool 4 deg C	SAXT01	L41	05/01/2025	Chemtech -SO
Q1937-05	LARGE-PILE-C	Solid	Percent Solids	Cool 4 deg C	SAXT01	L41	05/01/2025	Chemtech -SO
Q1937-06	LARGE-PILE-C	Solid	Percent Solids	Cool 4 deg C	SAXT01	L41	05/01/2025	Chemtech -SO
Q1937-07	LARGE-PILE-D	Solid	Percent Solids	Cool 4 deg C	SAXT01	L41	05/01/2025	Chemtech -SO
Q1937-08	LARGE-PILE-D	Solid	Percent Solids	Cool 4 deg C	SAXT01	L41	05/01/2025	Chemtech -SO
Q1937-09	LARGE-PILE-E	Solid	Percent Solids	Cool 4 deg C	SAXT01	L41	05/01/2025	Chemtech -SO
Q1937-10	LARGE-PILE-E	Solid	Percent Solids	Cool 4 deg C	SAXT01	L41	05/01/2025	Chemtech -SO
Q1937-11	LARGE-PILE-F	Solid	Percent Solids	Cool 4 deg C	SAXT01	L41	05/01/2025	Chemtech -SO

Date/Time 05/02/25 15:10

Raw Sample Received by: [Signature]

Raw Sample Relinquished by: [Signature]

Date/Time 05/02/25 17:10

Raw Sample Received by: [Signature]

Raw Sample Relinquished by: [Signature]

WORKLIST(Hardcopy Internal Chain)

172546

WorkList Name : %1-050225

WorkList ID : 189289

Department : Wet-Chemistry

Date : 05-02-2025 14:36:21

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1937-12	LARGE-PILE-F	Solid	Percent Solids	Cool 4 deg C	SAXT01	L41	05/01/2025	Chemtech -SO
Q1938-01	LOWER-WALL-PILE-A	Solid	Percent Solids	Cool 4 deg C	SAXT01	L41	05/01/2025	Chemtech -SO
Q1938-02	LOWER-WALL-PILE-A	Solid	Percent Solids	Cool 4 deg C	SAXT01	L41	05/01/2025	Chemtech -SO
Q1938-03	LOWER-WALL-PILE-B	Solid	Percent Solids	Cool 4 deg C	SAXT01	L41	05/01/2025	Chemtech -SO
Q1938-04	LOWER-WALL-PILE-B	Solid	Percent Solids	Cool 4 deg C	SAXT01	L41	05/01/2025	Chemtech -SO
Q1938-05	LOWER-WALL-PILE-C	Solid	Percent Solids	Cool 4 deg C	SAXT01	L41	05/01/2025	Chemtech -SO
Q1938-06	LOWER-WALL-PILE-C	Solid	Percent Solids	Cool 4 deg C	SAXT01	L41	05/01/2025	Chemtech -SO
Q1938-07	LOWER-WALL-PILE-D	Solid	Percent Solids	Cool 4 deg C	SAXT01	L41	05/01/2025	Chemtech -SO
Q1938-08	LOWER-WALL-PILE-D	Solid	Percent Solids	Cool 4 deg C	SAXT01	L41	05/01/2025	Chemtech -SO
Q1942-05	SVOC-GPC-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	L41	05/01/2025	Chemtech -SO
Q1942-06	PEST-GPC-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	L41	04/25/2025	Chemtech -SO
Q1942-07	PEST-GPC-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	L41	04/25/2025	Chemtech -SO
Q1942-08	PCB-GPC-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	L41	04/25/2025	Chemtech -SO
Q1942-09	PCB-GPC-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	L41	04/25/2025	Chemtech -SO
Q1942-10	SVOC-GPC2-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	L41	04/25/2025	Chemtech -SO
Q1942-11	PEST-GPC2-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	L41	04/25/2025	Chemtech -SO
Q1942-12	PEST-GPC2-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	L41	04/25/2025	Chemtech -SO
Q1942-13	PCB-GPC2-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	L41	04/25/2025	Chemtech -SO
Q1942-14	PCB-GPC2-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	L41	04/25/2025	Chemtech -SO
Q1944-01	MELTED-RUBBER-SAMPLE	Solid	Percent Solids	Cool 4 deg C	METE01	L41	05/02/2025	Chemtech -SO
Q1946-01	BB-CONCRETE	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	05/02/2025	Chemtech -SO

Date/Time 05/02/25 15:10

Raw Sample Received by: *Se Lee*

Raw Sample Relinquished by: *Se Lee*

Date/Time 05/02/25

Raw Sample Received by: *Se Lee*

Raw Sample Relinquished by: *Se Lee*

WORKLIST(Hardcopy Internal Chain)

8/23/25

WorkList Name : %1-050225

WorkList ID : 189289

Department : Wet-Chemistry

Date : 05-02-2025 14:36:21

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1946-02	BB-CONCRETE	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	05/02/2025	Chemtech -SO
Q1947-01	MH-P	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	05/02/2025	Chemtech -SO
Q1947-02	MH-P-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	05/02/2025	Chemtech -SO
Q1947-03	MH-P-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	05/02/2025	Chemtech -SO
Q1947-05	MH-O	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	05/02/2025	Chemtech -SO
Q1947-06	MH-O-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	05/02/2025	Chemtech -SO
Q1947-07	MH-O-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	05/02/2025	Chemtech -SO
Q1951-01	MH-KK	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	05/02/2025	Chemtech -SO
Q1951-02	MH-KK-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	05/02/2025	Chemtech -SO
Q1951-03	MH-KK-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	05/02/2025	Chemtech -SO
Q1952-01	CLEAN-FILL	Solid	Percent Solids	Cool 4 deg C	PSEG03	L31	05/02/2025	Chemtech -SO
Q1952-02	CLEAN-FILL-E2	Solid	Percent Solids	Cool 4 deg C	PSEG03	L21	05/02/2025	Chemtech -SO
Q1953-01	AUD-25-0075	Solid	Percent Solids	Cool 4 deg C	PSEG03	L21	05/02/2025	Chemtech -SO
Q1953-02	AUD-25-0076	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	05/02/2025	Chemtech -SO
Q1953-03	AUD-25-0077	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	05/02/2025	Chemtech -SO
Q1954-01	BC260874-1-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	05/02/2025	Chemtech -SO
Q1954-02	BC260874-1-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	05/02/2025	Chemtech -SO
Q1955-01	LAW-25-0066	Solid	Percent Solids	Cool 4 deg C	PSEG03	L41	05/02/2025	Chemtech -SO

Date/Time 05/02/25 15:10

Raw Sample Received by: 88 WOC,

Raw Sample Relinquished by: 88 WOC,

Date/Time 05/02/25

Raw Sample Received by: 88 WOC,

Raw Sample Relinquished by: 88 WOC,

SOP ID: M3640A-GPC cleanup-6, M3665A-Sulfuric Acid Cleanup-7

Clean Up SOP #: GPC Cleanup, Acid Cleanup

Extraction Start Date : 05/05/2025

Matrix : Solid

Extraction Start Time : 10:42

Welgh By: N/A

Extraction By: N/A

Extraction End Date : 05/06/2025

Balance check: N/A

Filter By: N/A

Extraction End Time : 10:00

Balance ID: N/A

pH Meter ID: N/A

Concentration By: EH

pH Strip Lot#: N/A

Hood ID: 6,7

Supervisor By : RUPESH

Extraction Method: ☐ Separatory Funnel ☐ Continous Liquid/Liquid ☐ Sonication ☐ Waste Dilution ☒ Soxhlet

Standard Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
GPC Pcb Spike	10.0ML	400 PPB	PP24452
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
MeCl2/Acetone/1:1	N/A	EP2600
Baked Na2SO4	N/A	EP2607
Hexane	N/A	E3933
H2SO4 1:1	N/A	EP2565
Methylene Chloride	N/A	E3930
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

No Extraction only GPC Check prepared.

KD Bath ID: Water bath -01

Envap ID: NEVAP-02

KD Bath Temperature: 60 °C


Envap Temperature: 40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
5/6/25	RS(Ext Lab)	SR Post/PCB Lab
10:05	Preparation Group	Analysis Group

Analytical Method: M3640A-GPC cleanup-6, M3665A-Sulfuric Acid Cleanup-7

Concentration Date: 05/06/2025

Sample ID	Client Sample ID	Test	g / (mL)	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
Q1942-13	PCB-GPC2-BLANK	PCB	10.0	N/A	Evelyn	RUPESH	5			
Q1942-14	PCB-GCP2-BLANK-SPIKE	PCB	10.0	N/A	Evelyn	RUPESH	5			

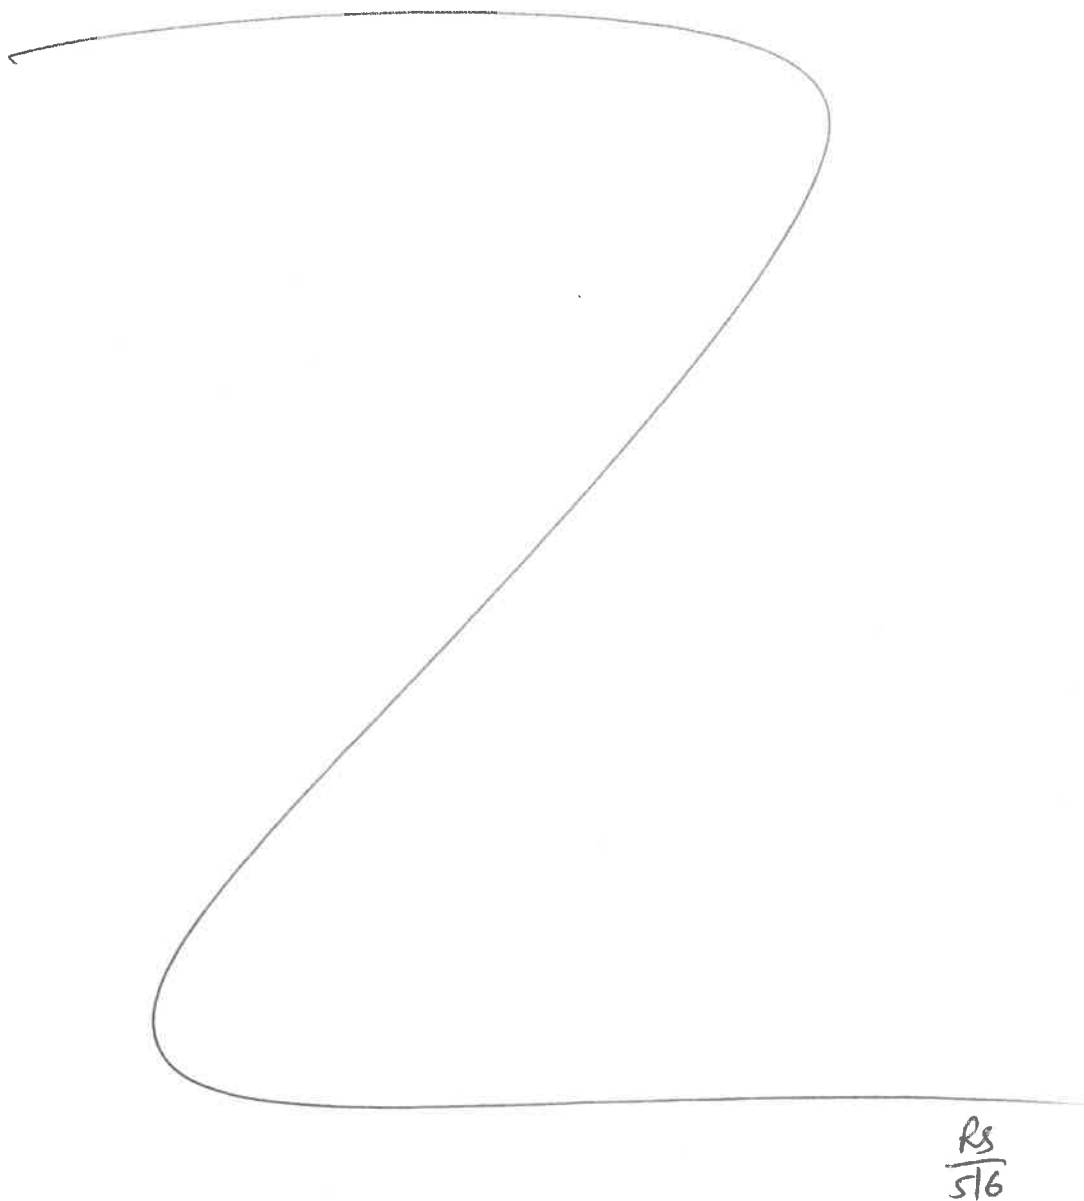

Rs
516

WORKLIST(Hardcopy Internal Chain)

WorkList Name : Q1942

WorkList ID : 189316

Department : Extraction

Date : 05-05-2025 10:36:47

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1942-10	SVOC-GPC2-BLANK	Solid	SVOC-Chemtech Full -25	Cool 4 deg C	CHEM02	L41	04/25/2025	SFAM_SVOC
Q1942-11	PEST-GPC2-BLANK	Solid	Pesticide-TCL	Cool 4 deg C	CHEM02	L41	04/25/2025	SFAM_PEST
Q1942-12	PEST-GPC2-BLANK-SPIKE	Solid	Pesticide-TCL	Cool 4 deg C	CHEM02	L41	04/25/2025	SFAM_PEST
Q1942-13	PCB-GPC2-BLANK	Solid	PCB	Cool 4 deg C	CHEM02	L41	04/25/2025	SFAM_PCB
Q1942-14	PCB-GPC2-BLANK-SPIKE	Solid	PCB	Cool 4 deg C	CHEM02	L41	04/25/2025	SFAM_PCB

Date/Time 5/5/25 10:37
 Raw Sample Received by: RJ (Ext-044)
 Raw Sample Relinquished by: [Signature]

Date/Time 5/5/25 11:00
 Raw Sample Received by: [Signature]
 Raw Sample Relinquished by: RJ (Ext-044)



SHIPPING DOCUMENTS



284 Sheffield Street, Mountainside, NJ 07092

(908) 789-8900 Fax: (908) 78-8922

www.chemtech.net

CHAIN OF CUSTODY RECORD

Alliance Project Number:

Q1942

COC Number:

CLIENT INFORMATION

COMPANY: Alliance Technical Group

ADDRESS: 284 Sheffield Street

CITY Mountainside STATE: NJ ZIP: 07092

ATTENTION: QA Officer

PHONE: 908-789-8900

FAX: 908-788-9222

PROJECT INFORMATION

PROJECT NAME: Weekly Storage Blanks

PROJECT #: LOCATION:

PROJECT MANAGER:

E-MAIL:

PHONE:

FAX:

BILLING INFORMATION

BILL TO: Same

PO#

ADDRESS:

CITY:

STATE:

ZIP:

ATTENTION:

PHONE:

ANALYSIS

VOC-Drinking H2O

SVOC-Full+25-

8270

PESTICIDE-TCL

PCB

1

2

3

4

5

6

7

8

9

PRESERVATIVES

COMMENTS

<-- Specify Preservatives

A-HCl B-HNO3

C-H2SO4 D-NaOH

E-ICE F-Other

DATA TURNAROUND INFORMATION

FAX: 10 DAYS*

HARD COPY: 10 DAYS*

EDD DAYS*

* TO BE APPROVED BY ALLIANCE

STANDARD TURNAROUND TIME IS 10 BUSINESS DAYS

DATA DELIVERABLE INFORMATION

☐ RESULTS ONLY (L1)☐ US EPA CLP (L4)☐ RESULTS + QC (L2)☐ NYS ASP "A" (L2)☐ NJ REDUCED (L3)☐ NYS ASP "B" (L4)☐ NJ FULL (L4)☐ Other☐ EDD Format

ALLIANCE SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# of Bottles	A/E	1	2	3	4	5	6	7	8	9	
			COMP	GRAB	DATE	TIME												
1.	Storage-Blank-SOIL-REF-6	AQ		X			2	X										
2.	Storage-Blank-WATER-REF-5	AQ		X			2	X										
3.	Storage-Blank-WATER-REF-4	AQ		X			2	X										
4.	Storage-Blank-SAMPLE-MANAGEMENT	AQ		X			2	X										
5.	SVOC-GPC-BLANK	SO		X			1		X									
6.	PEST-GPC-BLANK	SO		X			1			X								
7.	PEST-GPC-BLANK-SPIKE	SO		X			1			X								
8.	PCB-GPC-BLANK	SO		X			1				X							
9.	PCB-GPC-BLANK-SPIKE	SO		X			1				X							
10.	SVOC-GPC2-BLANK	SO		X			1		X									

SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE POSSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER	DATE/TIME	RECEIVED BY	Conditions of bottles or coolers at receipt: ☐ Compliant ☐ Non Compliant ☐ Cooler Temp _____ MeOH extraction requires an additional 4oz. Jar for percent solid ☐ Ice in Cooler?: _____
1.		1.	
RELINQUISHED BY	DATE/TIME	RECEIVED BY	Comments:
2.		2.	
RELINQUISHED BY	DATE/TIME	RECEIVED FOR LAB BY	
3.		3.	

Page 1 of 2

SHIPPED VIA: CLIENT: ☐ Hand Delivered ☐ Overnight
ALLIANCE: ☐ Picked Up ☐ Overnight

Shipment Complete
☐ YES ☐ NO

WHITE - ALLIANCE COPY FOR RETURN TO CLIENT

YELLOW - ALLIANCE COPY

PINK - SAMPLER COPY



284 Sheffield Street, Mountainside, NJ 07092
(908) 789-8900 Fax: (908) 78-8922
www.chemtech.net

Alliance Project Number:

Q1942

CHAIN OF CUSTODY RECORD

CLIENT INFORMATION

COMPANY: Alliance Technical Group
ADDRESS: 284 Sheffield Street
CITY Mountainside STATE: NJ ZIP: 07092
ATTENTION: QA Officer
PHONE: 908-789-8900 FAX: 908-788-9222

PROJECT INFORMATION

PROJECT NAME: Weekly Storage Blanks
PROJECT #: _____ LOCATION: _____
PROJECT MANAGER: _____
E-MAIL: _____
PHONE: _____ FAX: _____

COC Number:

BILLING INFORMATION

BILL TO: Same PO# _____
ADDRESS: _____
CITY: _____ STATE: _____ ZIP: _____
ATTENTION: _____ PHONE: _____

DATA TURNAROUND INFORMATION

FAX: _____ 10 _____ DAYS*
HARD COPY: _____ 10 _____ DAYS*
EDD _____ DAYS*
* TO BE APPROVED BY ALLIANCE
STANDARD TURNAROUND TIME IS 10 BUSINESS DAYS

DATA DELIVERABLE INFORMATION

- ☐ RESULTS ONLY (L1) ☐ US EPA CLP (L4)
☐ RESULTS + QC (L2) ☐ NYS ASP "A" (L2)
☐ NJ REDUCED (L3) ☐ NYS ASP "B" (L4)
☐ NJ FULL (L4) ☐ Other _____
☐ EDD Format

ANALYSIS

VOC-Drinking H2O	SVOC-Full+25-8270	PESTICIDE-TCL	PCB						
1	2	3	4	5	6	7	8	9	

PRESERVATIVES

COMMENTS

<-- Specify Preservatives
A-HCl B-HNO3
C-H2SO4 D-NaOH
E-ICE F-Other

ALLIANCE SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# of Bottles	PRESERVATIVES										
			COMP	GRAB	DATE	TIME		A/E										
								1	2	3	4	5	6	7	8	9		
1.	PEST-GPC2-BLANK	SO		X			1			X								
2.	PEST-GPC2-BLANK-SPIKE	SO		X			1			X								
3.	PCB-GPC2-BLANK	SO		X			1			X								
4.	PCB-GPC2-BLANK-SPIKE	SO		X			1				X							
5.							1				X							
6.																		
7.																		
8.																		
9.																		
10.																		

SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE POSSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER	DATE/TIME	RECEIVED BY
1.		1.
RELINQUISHED BY	DATE/TIME	RECEIVED BY
2.		2.
RELINQUISHED BY	DATE/TIME	RECEIVED FOR LAB BY
3.		3.

Conditions of bottles or coolers at receipt: ☐ Compliant ☐ Non Compliant ☐ Cooler Temp _____
MeOH extraction requires an additional 4oz. Jar for percent solid ☐ Ice in Cooler?: _____
Comments:

Page 2 of 2

SHIPPED VIA: CLIENT: ☐ Hand Delivered ☐ Overnight
ALLIANCE: ☐ Picked Up ☐ Overnight

Shipment Complete
☐ YES ☐ NO

WHITE - ALLIANCE COPY FOR RETURN TO CLIENT

YELLOW - ALLIANCE COPY

PINK - SAMPLER COPY

Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488