
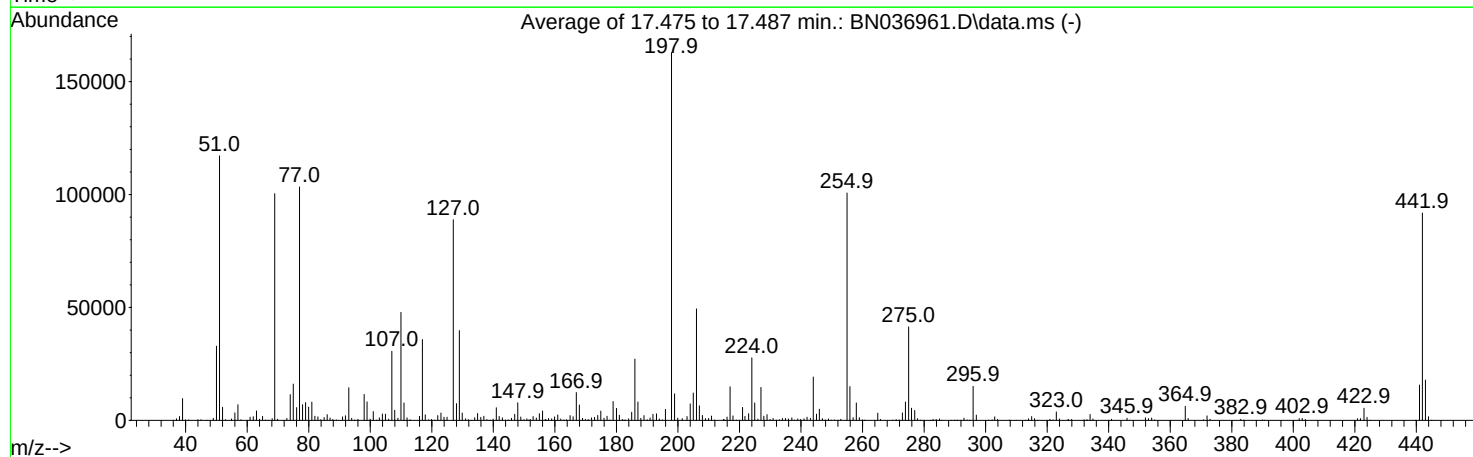


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050725\
Data File : BN036961.D
Acq On : 07 May 2025 13:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN042825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 28 15:35:03 2025

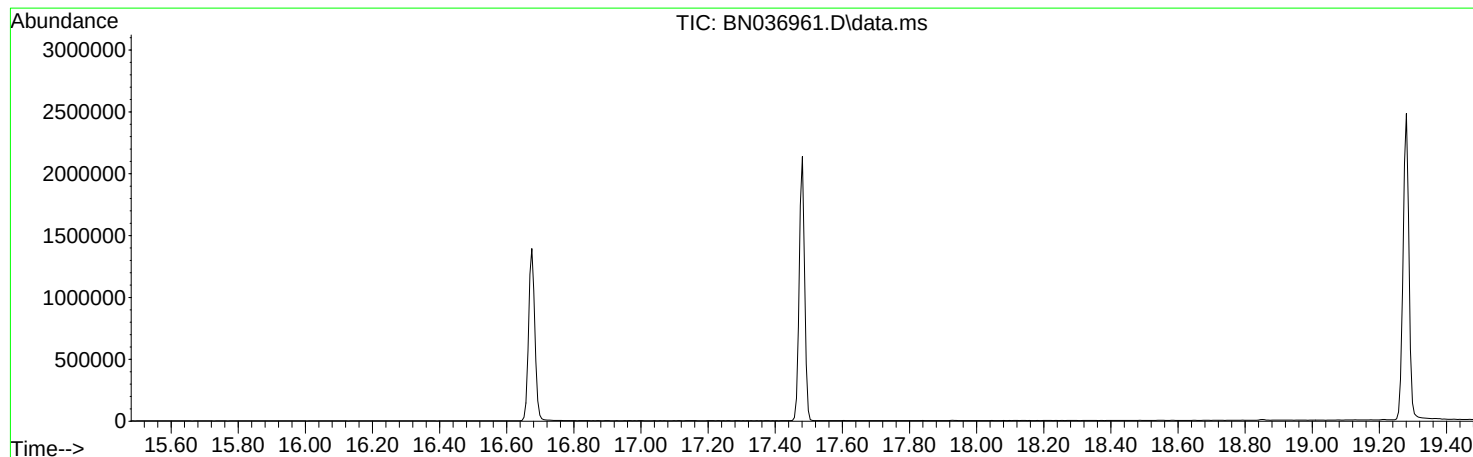

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	71.9	117144	PASS
68	69	0.00	2	0.8	753	PASS
69	198	0.00	100	61.6	100395	PASS
70	69	0.00	2	0.5	493	PASS
127	198	10	80	54.5	88848	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	162917	PASS
199	198	5	9	7.2	11786	PASS
275	198	10	60	25.4	41355	PASS
365	198	1	100	3.8	6226	PASS
441	198	0.01	100	9.6	15699	PASS
442	442	50	100	100.0	91848	PASS
443	442	15	24	19.4	17862	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/7/2025	BNA_N	<u>BN036961.D</u>
Compound Name	Response	Retention Time
DDT	521728	20.522
DDD	4347	20.128
DDE	0	19.58
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4347	526075	0.83

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050725\
Data File : BN036961.D
Acq On : 07 May 2025 13:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 07 16:12:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

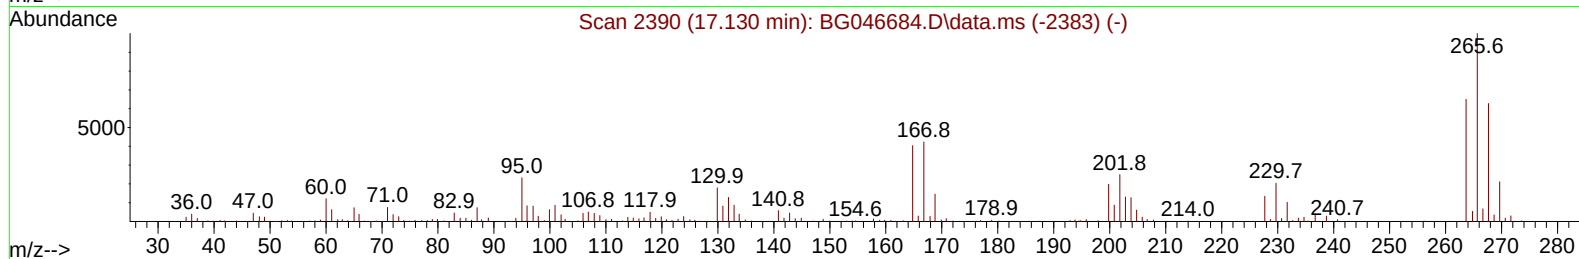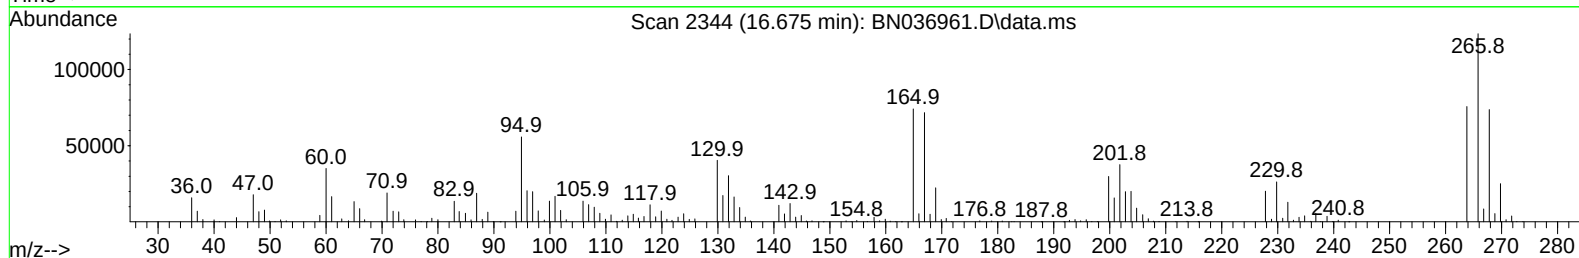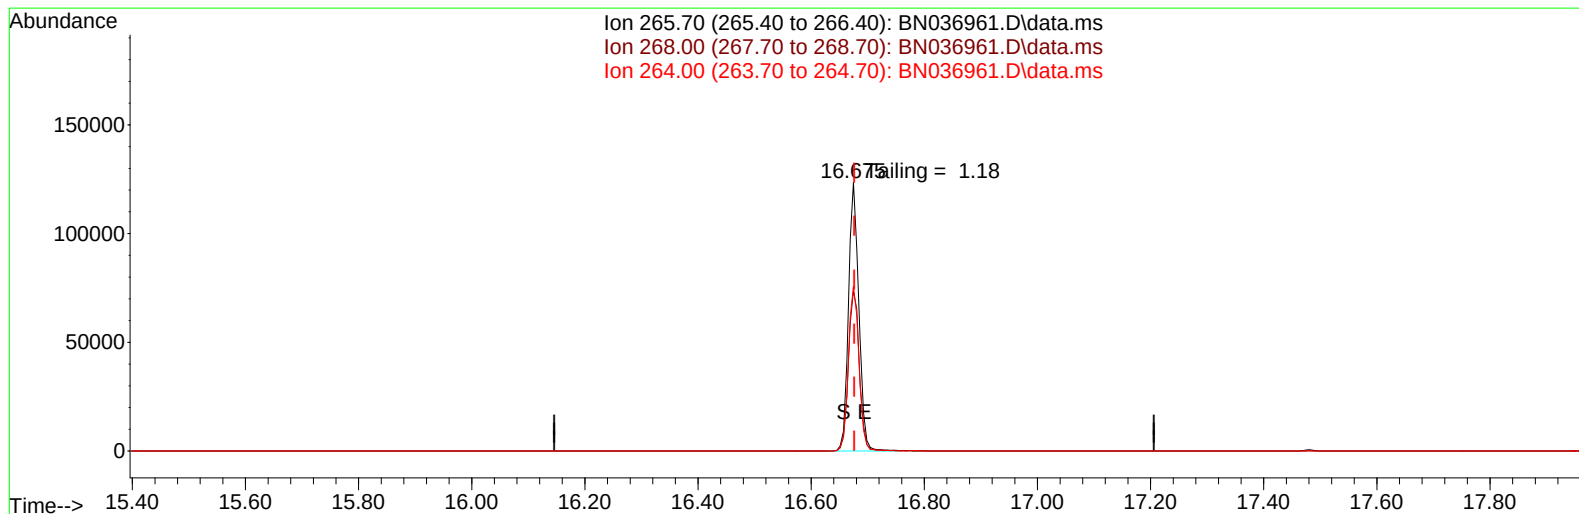

TIC: BN036961.D\data.ms

(70) Pentachlorophenol (C)

16.675min (-0.001) 16880.98 ng




response 157251

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.69
264.00	61.60	61.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050725\
Data File : BN036961.D
Acq On : 07 May 2025 13:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 07 16:10:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

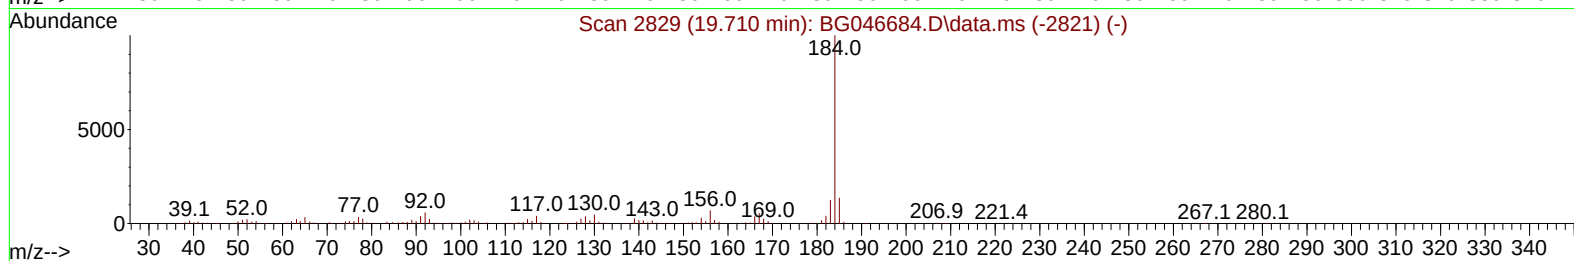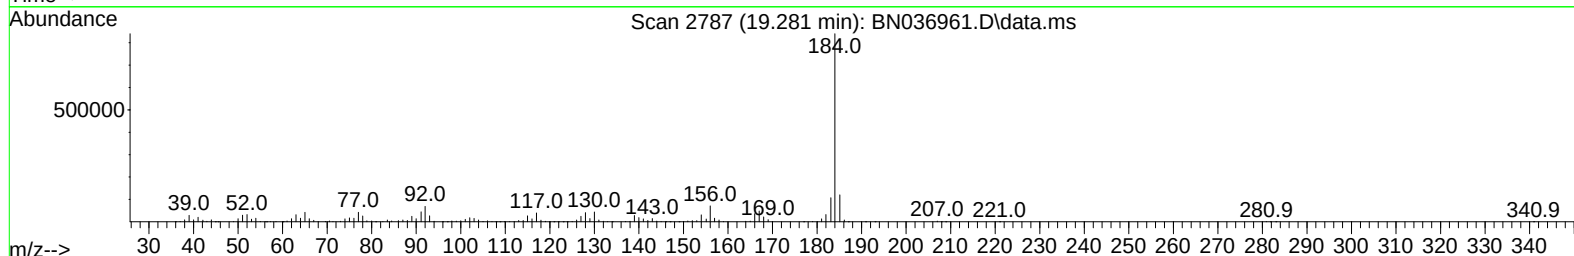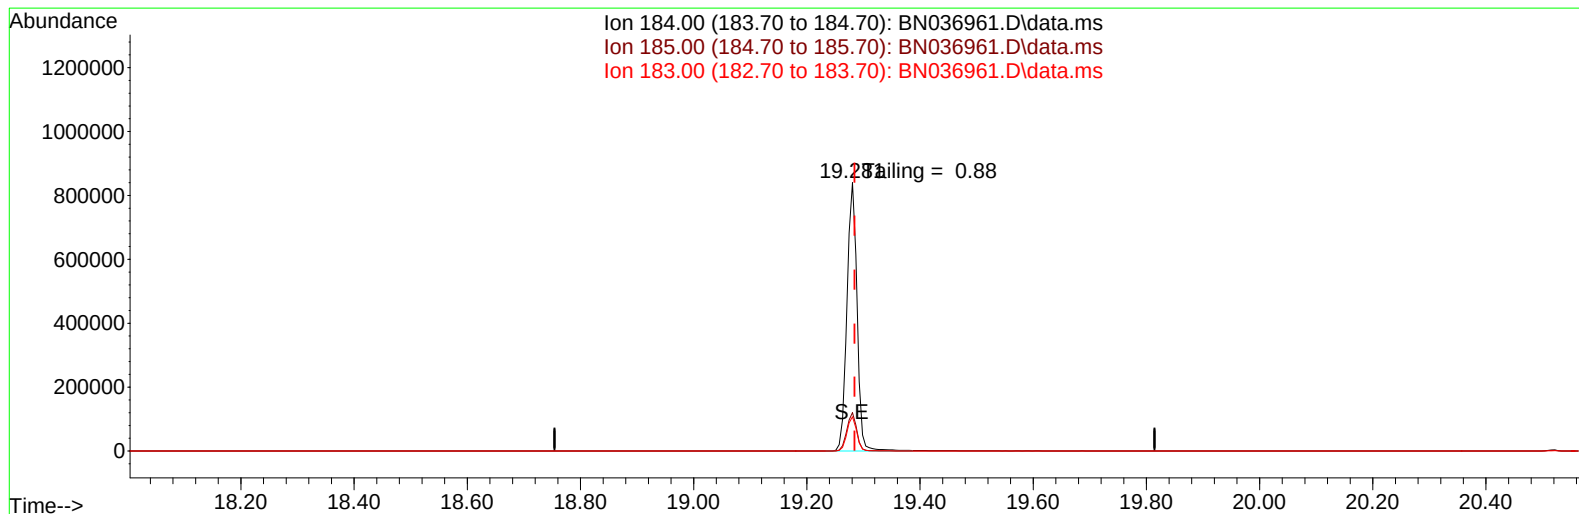

TIC: BN036961.D\data.ms

(77) Benzidine

19.281min (-0.003) 0.00 ng

response 1045231

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.34
183.00	13.20	12.75
0.00	0.00	0.00