

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050725\
 Data File : PL095560.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2025 10:13
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 01:40:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 23 16:23:18 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.596	2.913	56471702	66378571	17.298	20.875
28)	SA Decachlor...	9.121	8.091	54780398	61072212	19.771	20.638
Target Compounds							
6)	B beta-BHC	0.000	4.020f	0	5677948	N.D.	2.735 #
8)	B Heptachlo...	5.729	0.000	91198682	0	22.770	N.D. #
10)	B gamma-Chl...	5.975f	0.000	26517071	0	6.500	N.D. #
14)	MA Endrin	0.000	5.816	0	4635470	N.D.	1.273 #
25)	Chlordane-3	5.975f	0.000	26517071	0	34.043	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050725\
Data File : PL095560.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2025 10:13
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 01:40:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
Quant Title : GC Extractables
QLast Update : Wed Apr 23 16:23:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

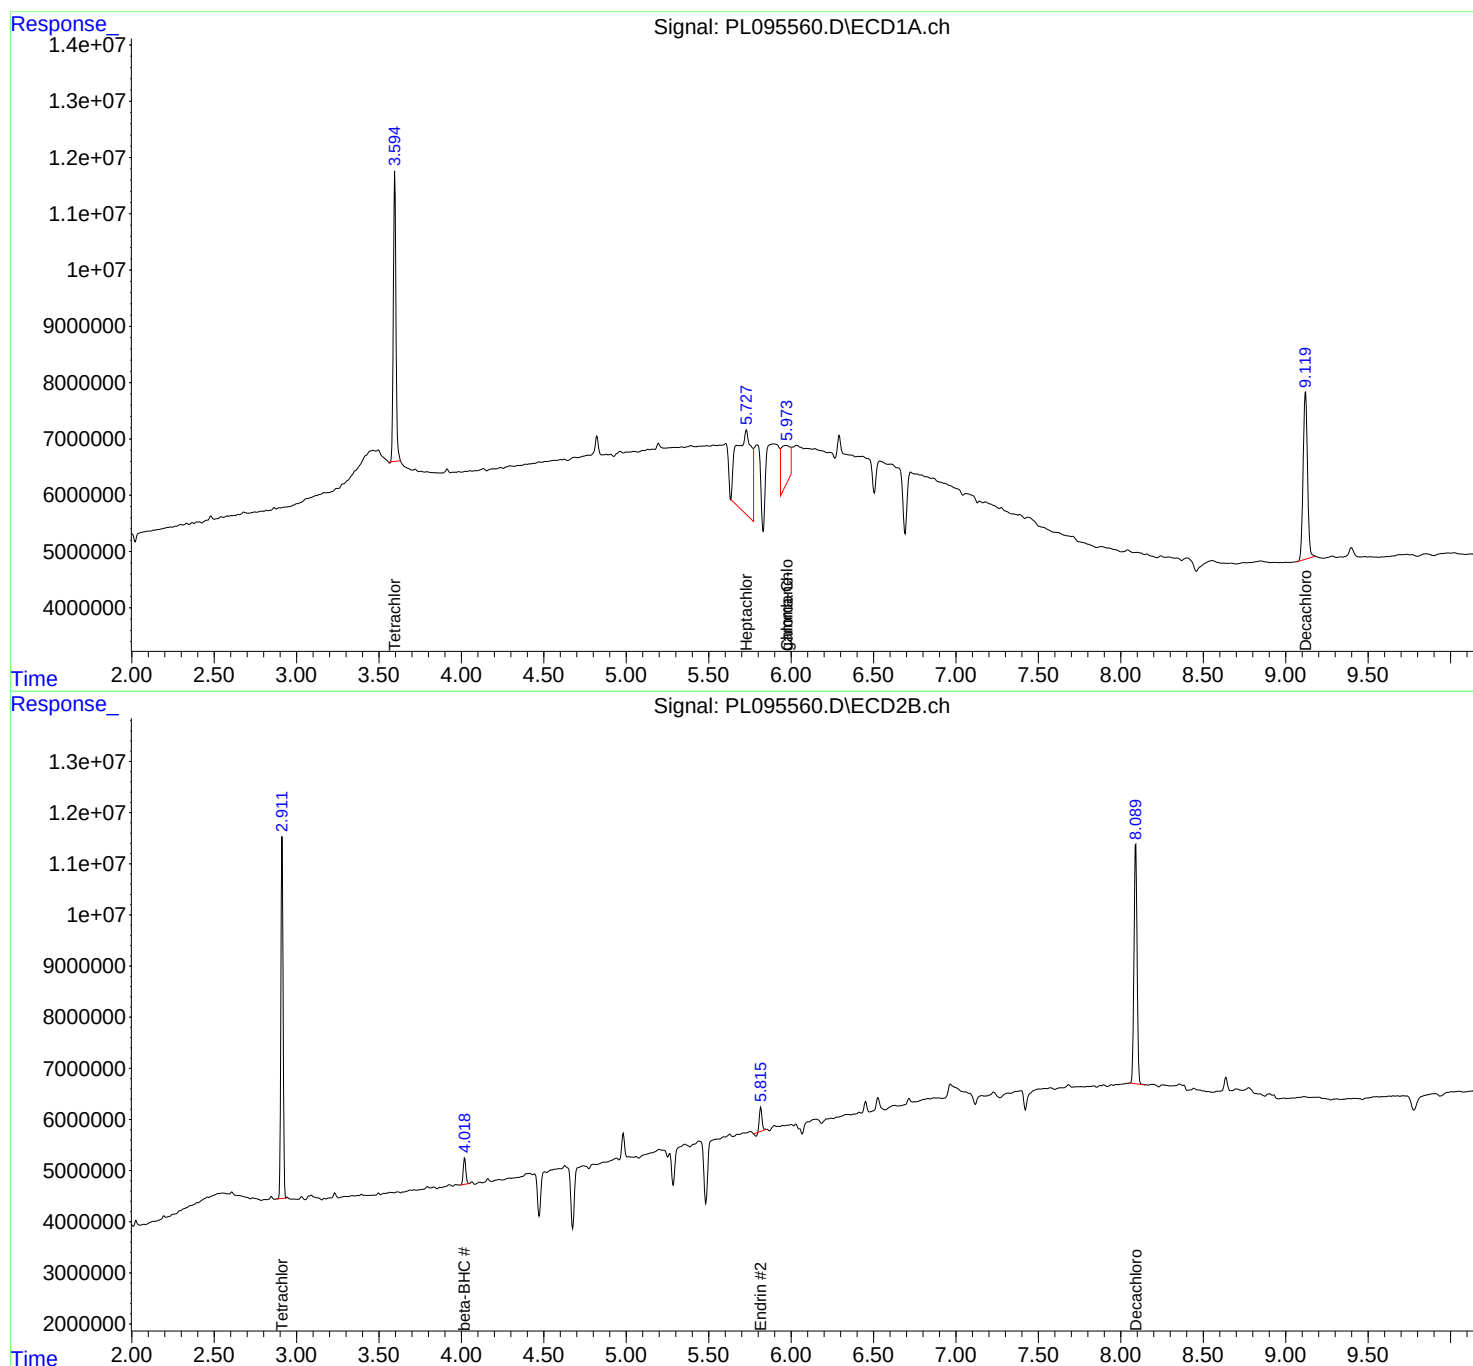


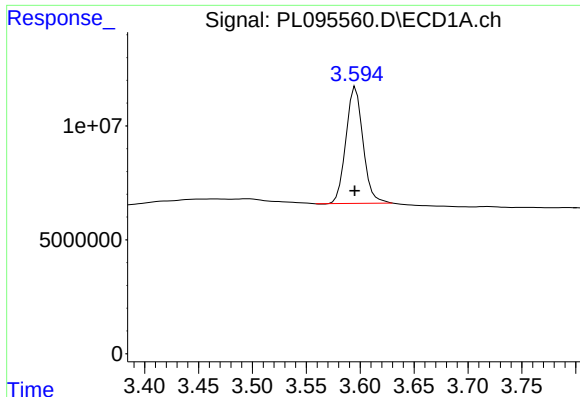

#1 Tetrachloro-m-xylene


R.T.: 3.596 min
Delta R.T.: 0.000 min
Response: 56471702
Conc: 17.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

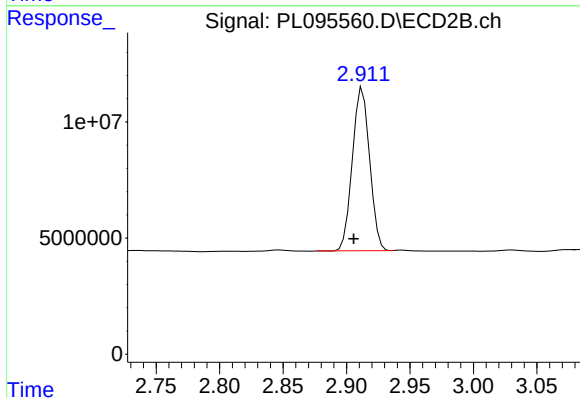


#1 Tetrachloro-m-xylene

R.T.: 2.913 min
Delta R.T.: 0.007 min
Response: 66378571
Conc: 20.88 ng/ml

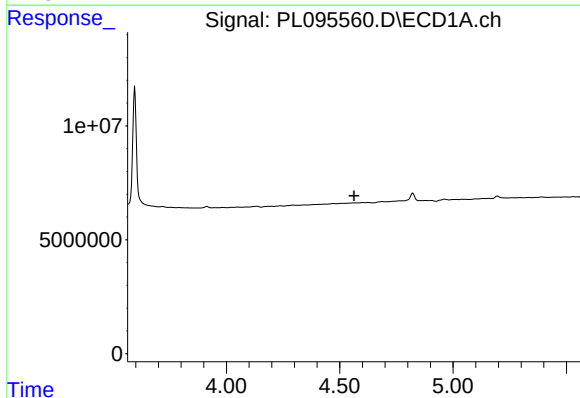


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.564 min
Response: 0
Conc: N.D.

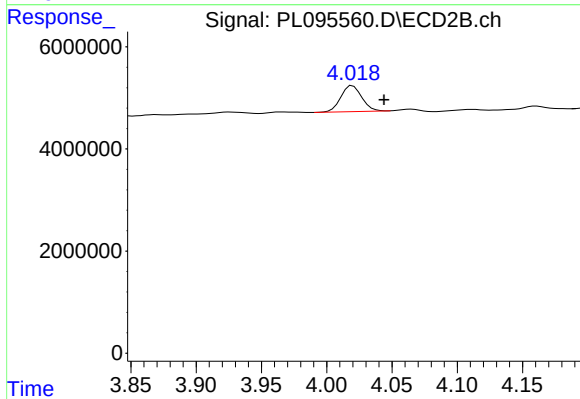

#6 beta-BHC


R.T.: 4.020 min
Delta R.T.: -0.024 min
Response: 5677948
Conc: 2.74 ng/ml

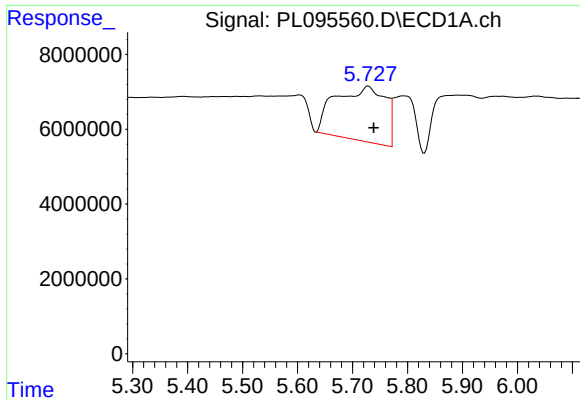

#8 Heptachlor epoxide


R.T.: 5.729 min
Delta R.T.: -0.010 min
Response: 91198682
Conc: 22.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

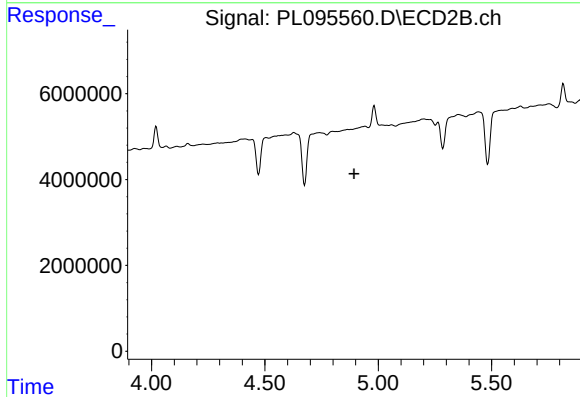


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.893 min
Response: 0
Conc: N.D.

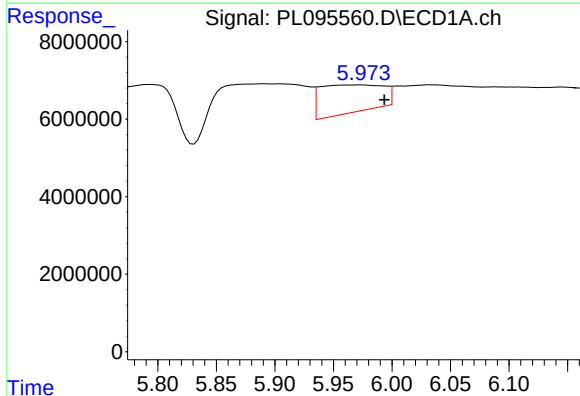


#10 gamma-Chlordane

R.T.: 5.975 min
Delta R.T.: -0.019 min
Response: 26517071
Conc: 6.50 ng/ml

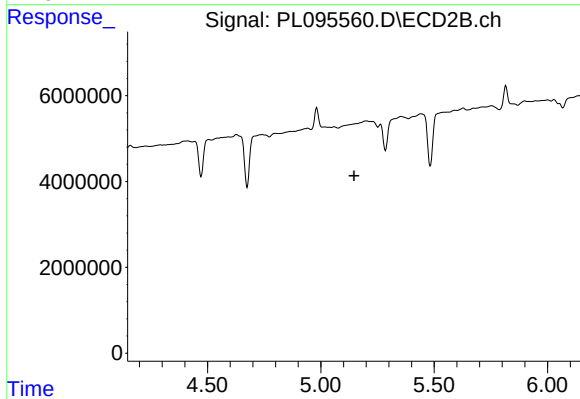

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.147 min
Response: 0
Conc: N.D.

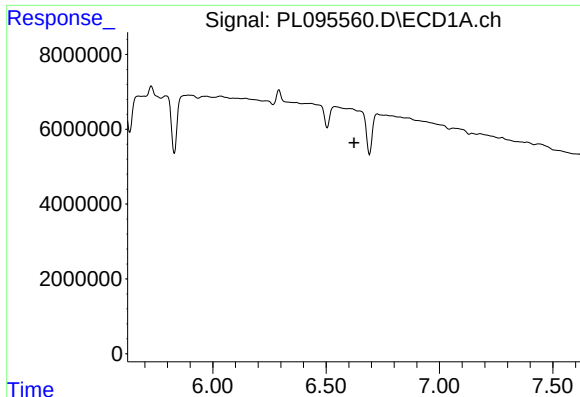

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.623 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

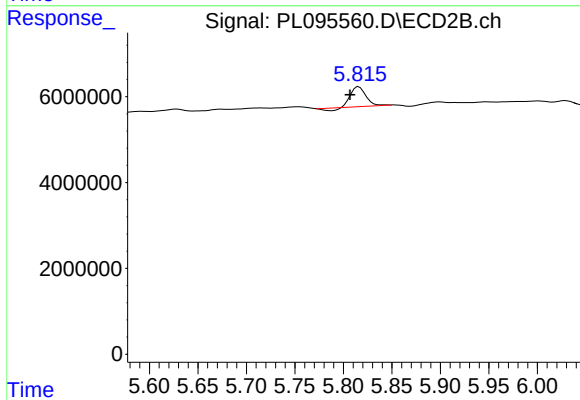


#14 Endrin

R.T.: 5.816 min
Delta R.T.: 0.009 min
Response: 4635470
Conc: 1.27 ng/ml

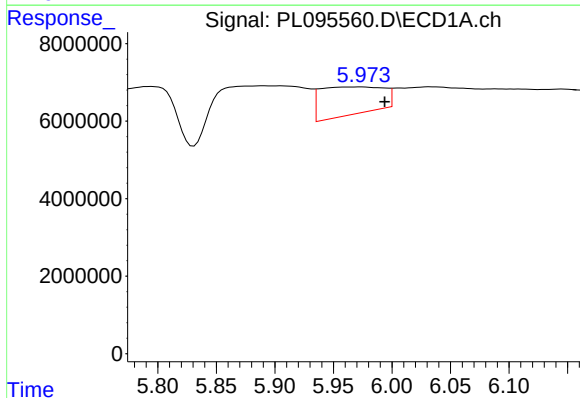


#25 Chlordane-3

R.T.: 5.975 min
Delta R.T.: -0.019 min
Response: 26517071
Conc: 34.04 ng/ml

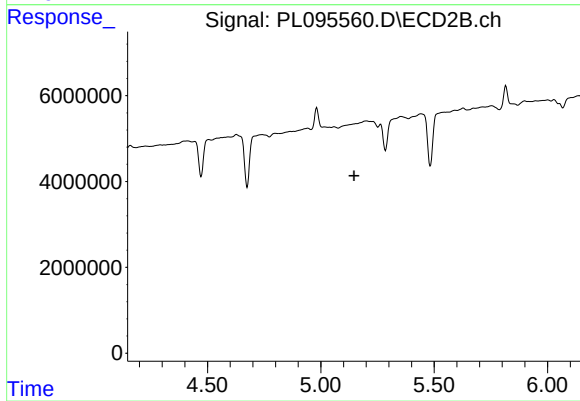

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.147 min
Response: 0
Conc: N.D.

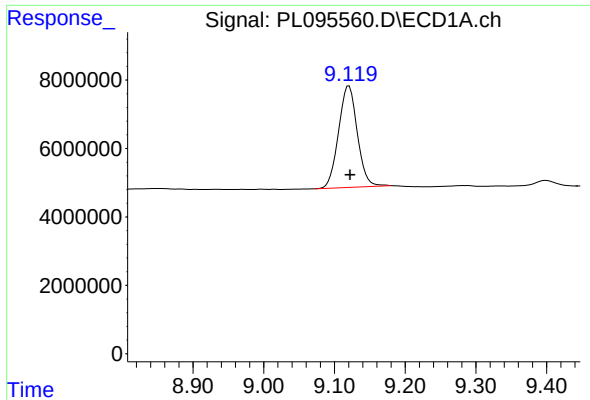

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: -0.002 min
Response: 54780398
Conc: 19.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

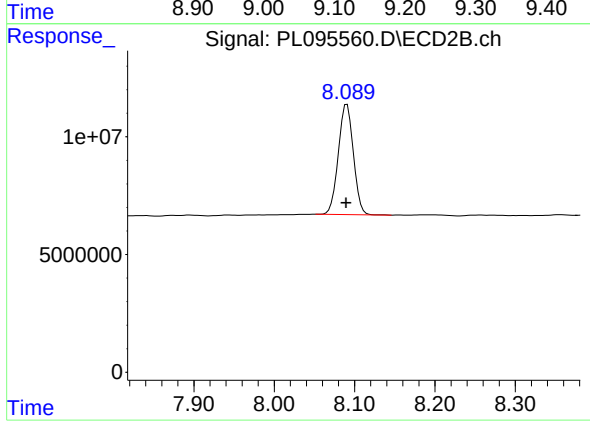

#28 Decachlorobiphenyl

R.T.: 8.091 min
Delta R.T.: 0.001 min
Response: 61072212
Conc: 20.64 ng/ml