
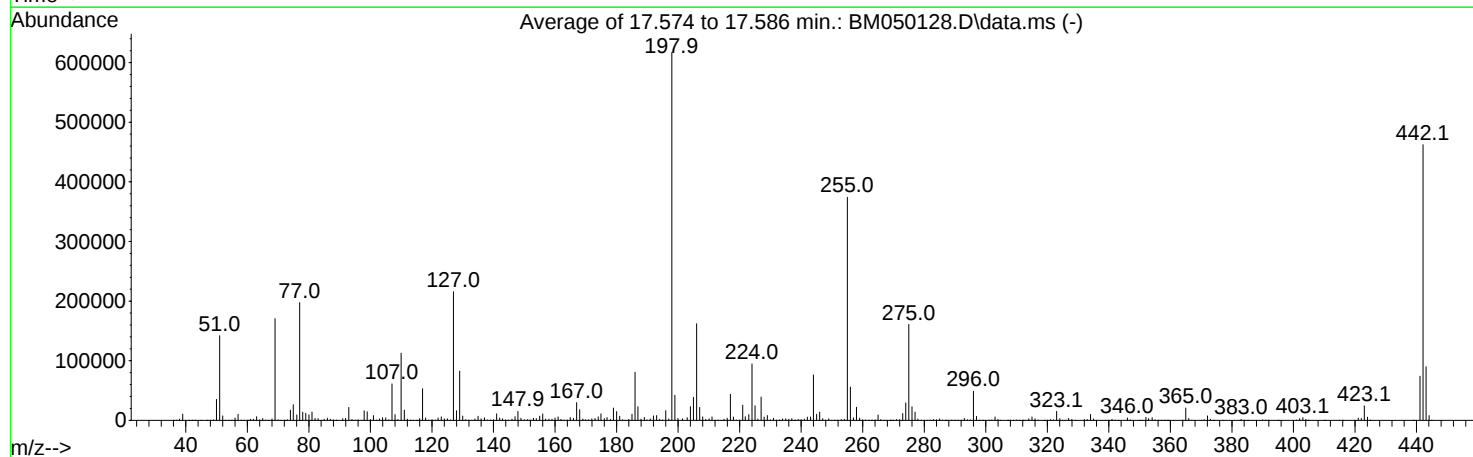


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050725\
Data File : BM050128.D
Acq On : 07 May 2025 09:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 28 18:09:16 2025

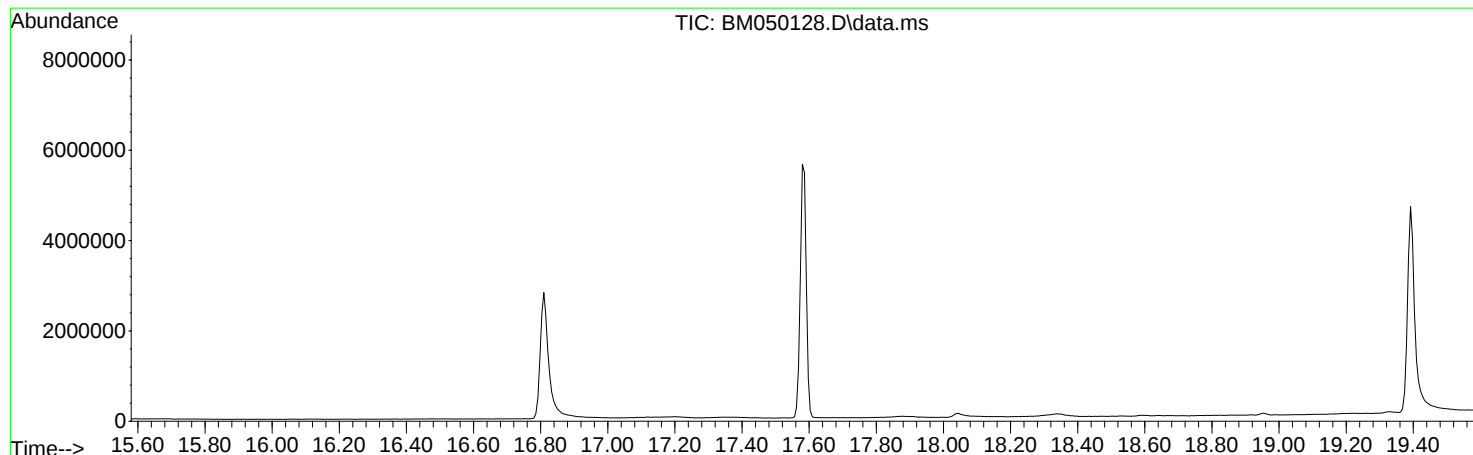

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.0	142053	PASS
68	69	0.00	2	1.4	2411	PASS
69	198	0.00	100	27.7	170733	PASS
70	69	0.00	2	0.5	908	PASS
127	198	10	80	35.0	215732	PASS
197	198	0.00	2	0.4	2403	PASS
198	198	100	100	100.0	616960	PASS
199	198	5	9	6.9	42292	PASS
275	198	10	60	26.1	161005	PASS
365	198	1	100	3.4	20678	PASS
441	198	0.01	100	12.0	74035	PASS
442	442	50	100	100.0	462379	PASS
443	442	15	24	19.4	89800	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/7/2025	BNA_M	<u>BM050128.D</u>
Compound Name	Response	Retention Time
DDT	1909705	20.621
DDD	35773	20.186
DDE	4017	19.674
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
39790	1949495	2.04

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050725\
Data File : BM050128.D
Acq On : 07 May 2025 09:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 07 11:57:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

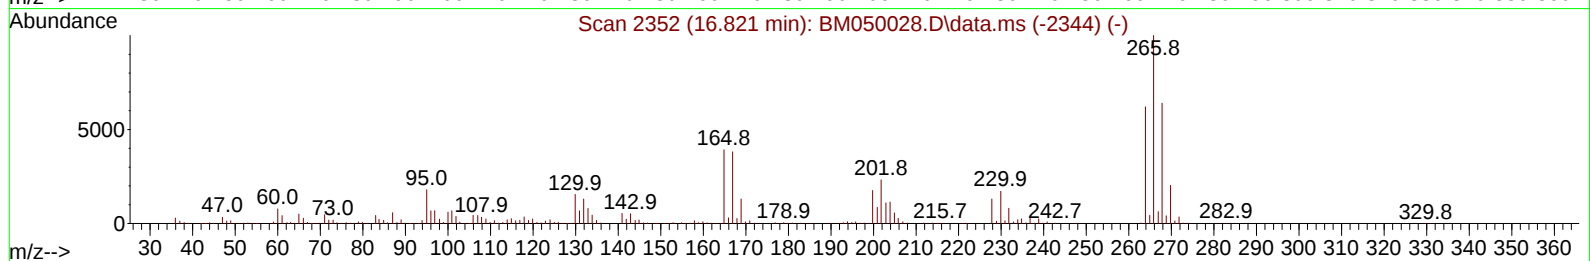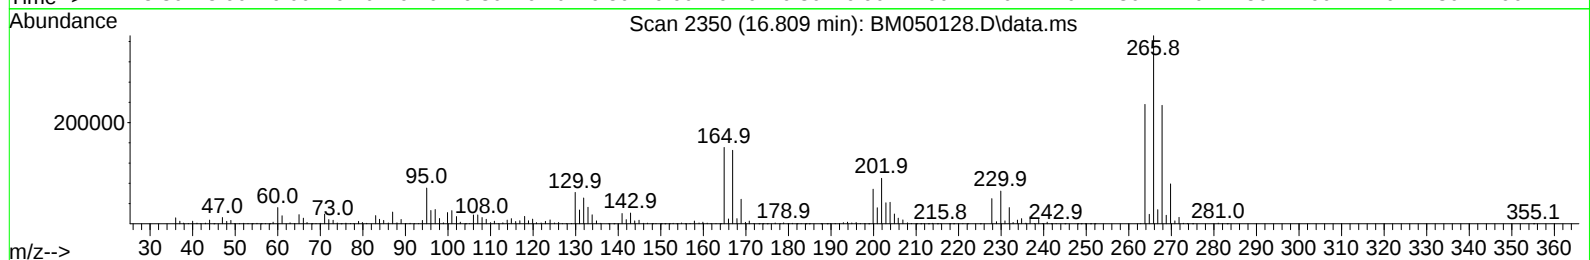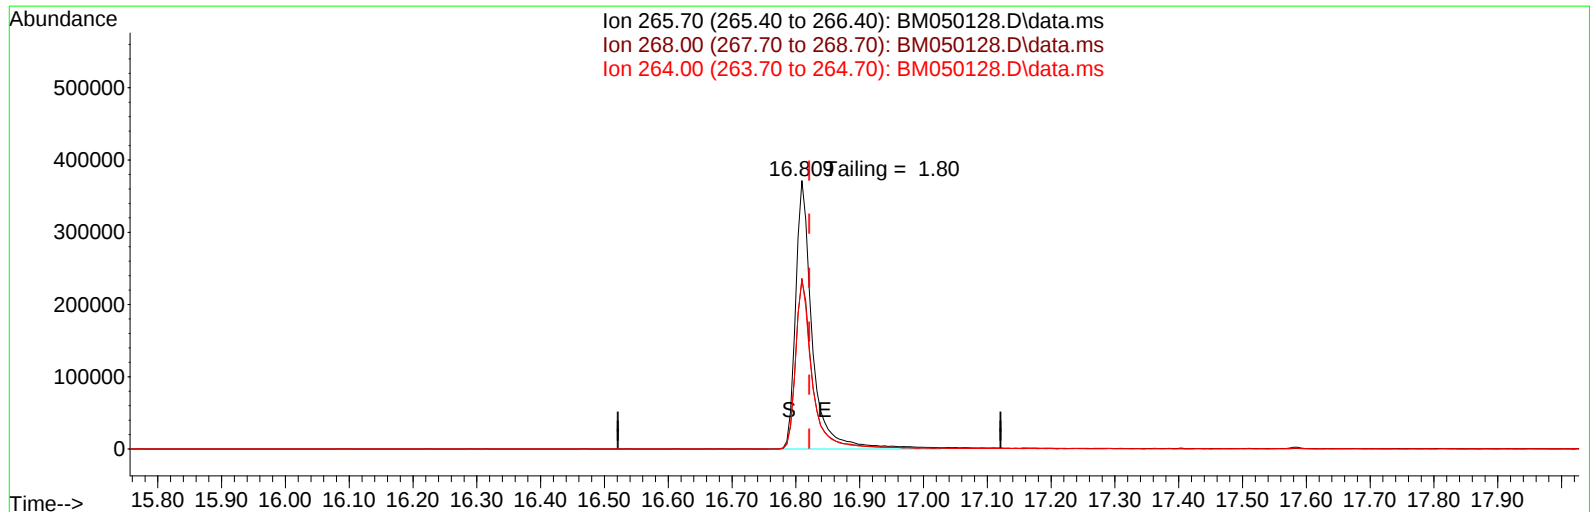

TIC: BM050128.D\data.ms

(70) Pentachlorophenol (C)

16.809min (-0.012) 191312.72 ng




response 680000

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	62.98
264.00	62.00	63.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050725\
Data File : BM050128.D
Acq On : 07 May 2025 09:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 07 11:57:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

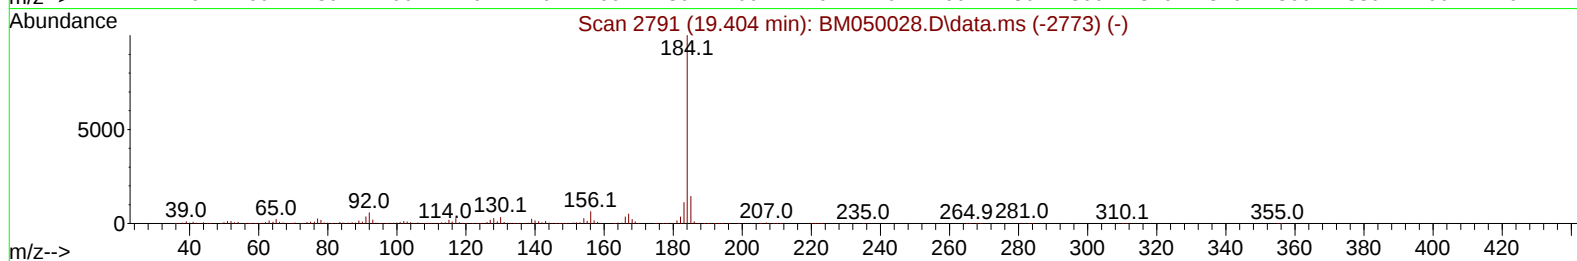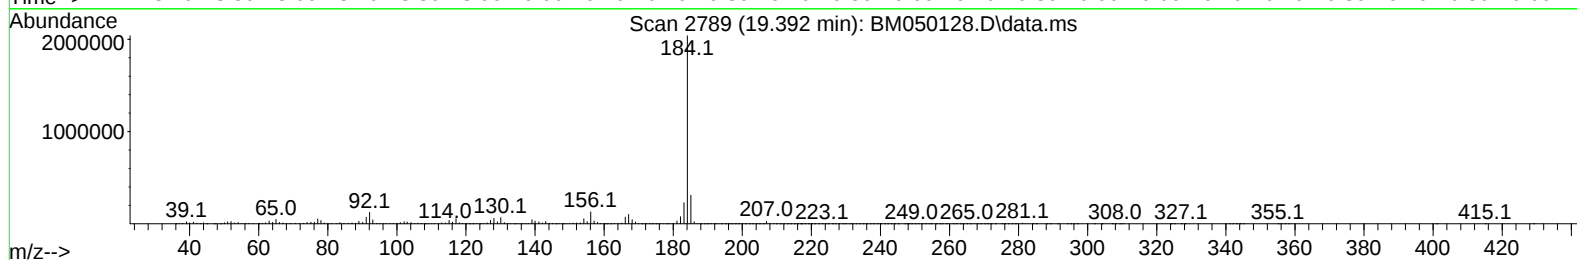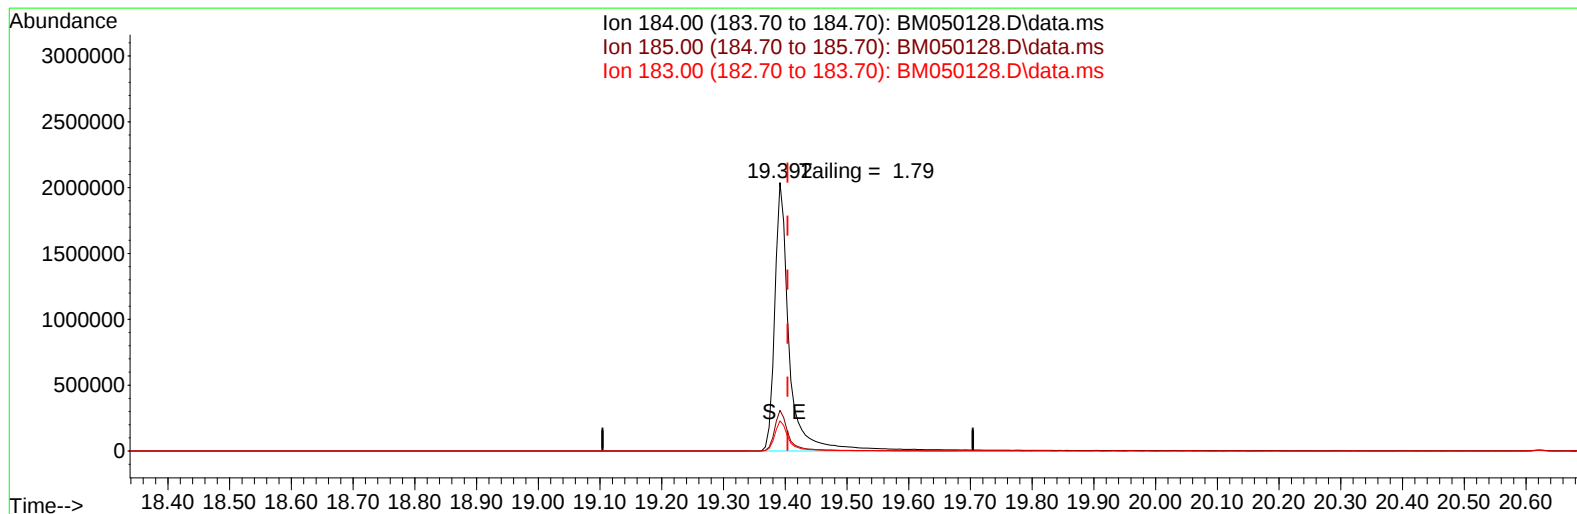

TIC: BM050128.D\data.ms

(77) Benzidine

19.392min (-0.012) 51539.94 ng

response 3372211

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.17
183.00	11.10	11.22
0.00	0.00	0.00