


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050625\
Data File : BP024539.D
Acq On : 06 May 2025 09:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 18 12:04:48 2025

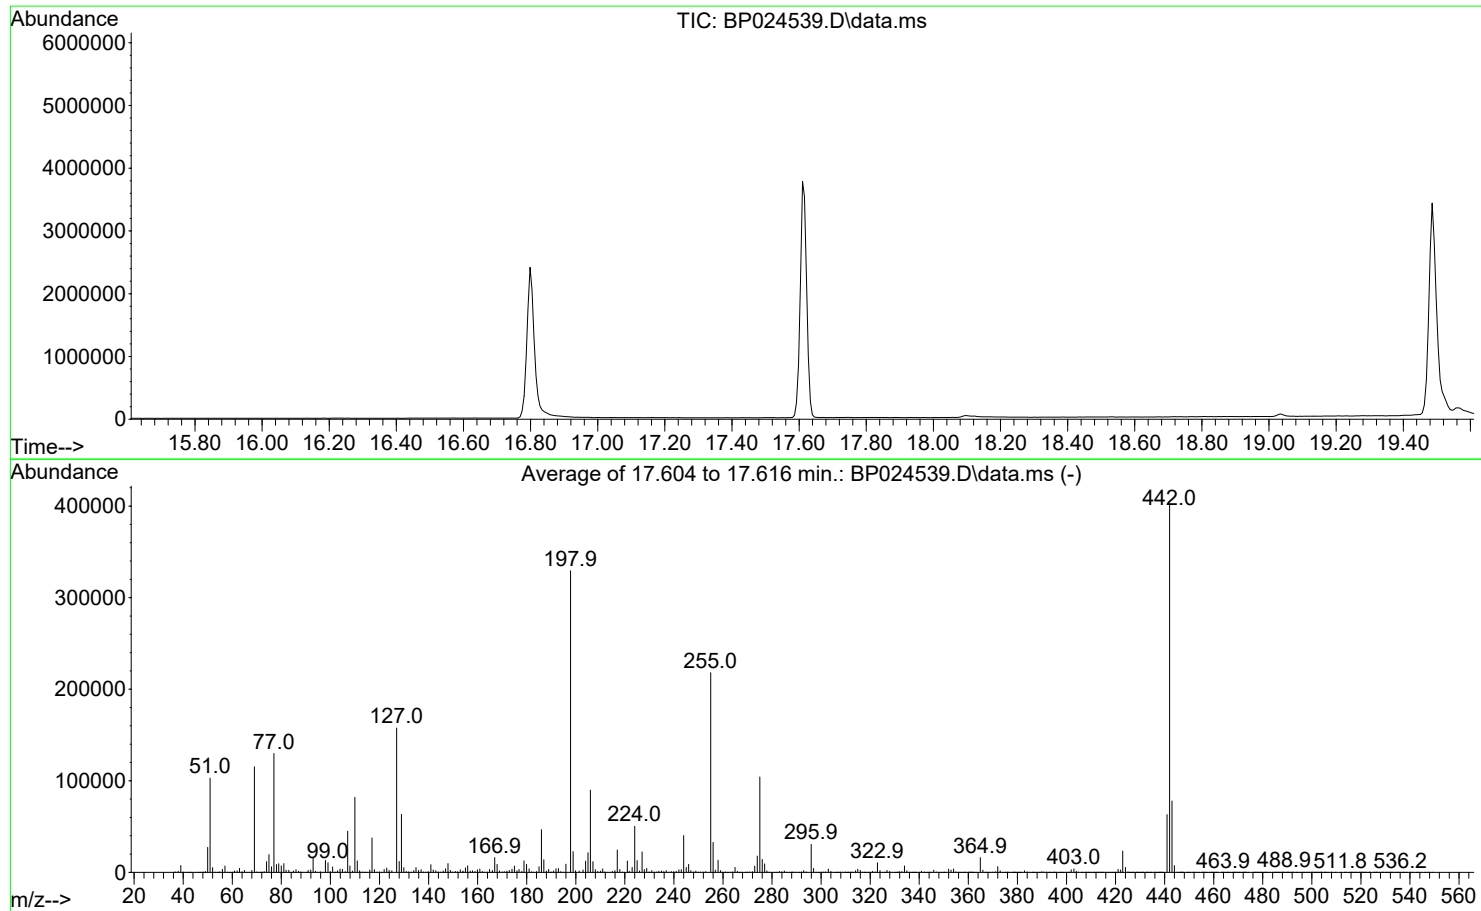

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.3	102943	PASS
68	69	0.00	2	1.8	2073	PASS
69	198	0.00	100	35.0	115286	PASS
70	69	0.00	2	0.5	578	PASS
127	198	10	80	47.9	157656	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	329357	PASS
199	198	5	9	6.9	22794	PASS
275	198	10	60	31.6	104219	PASS
365	198	1	100	4.9	16170	PASS
441	198	0.01	100	19.1	63029	PASS
442	442	100	100	100.0	401749	PASS
443	442	15	24	19.4	77992	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/6/2025	BNA_P	<u>BP024539.D</u>
Compound Name	Response	Retention Time
DDT	1350082	20.769
DDD	38430	20.316
DDE	0	19.775
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
38430	1388512	2.77

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050625\
Data File : BP024539.D
Acq On : 06 May 2025 09:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 06 13:41:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

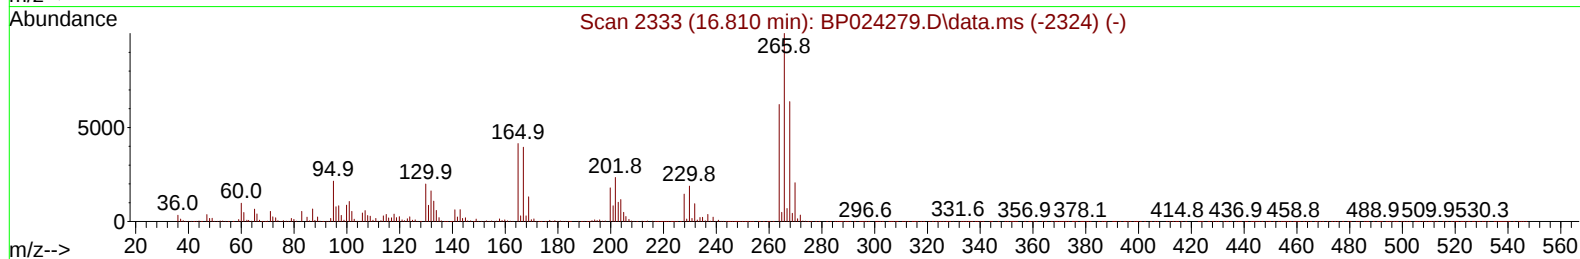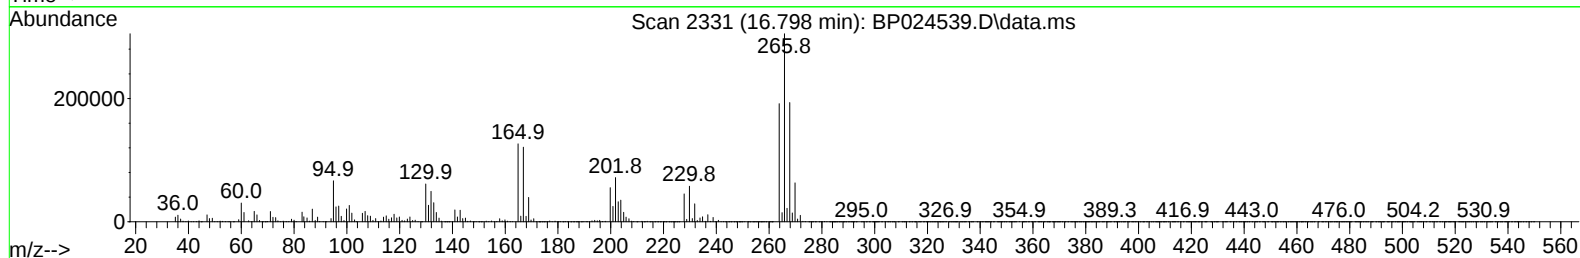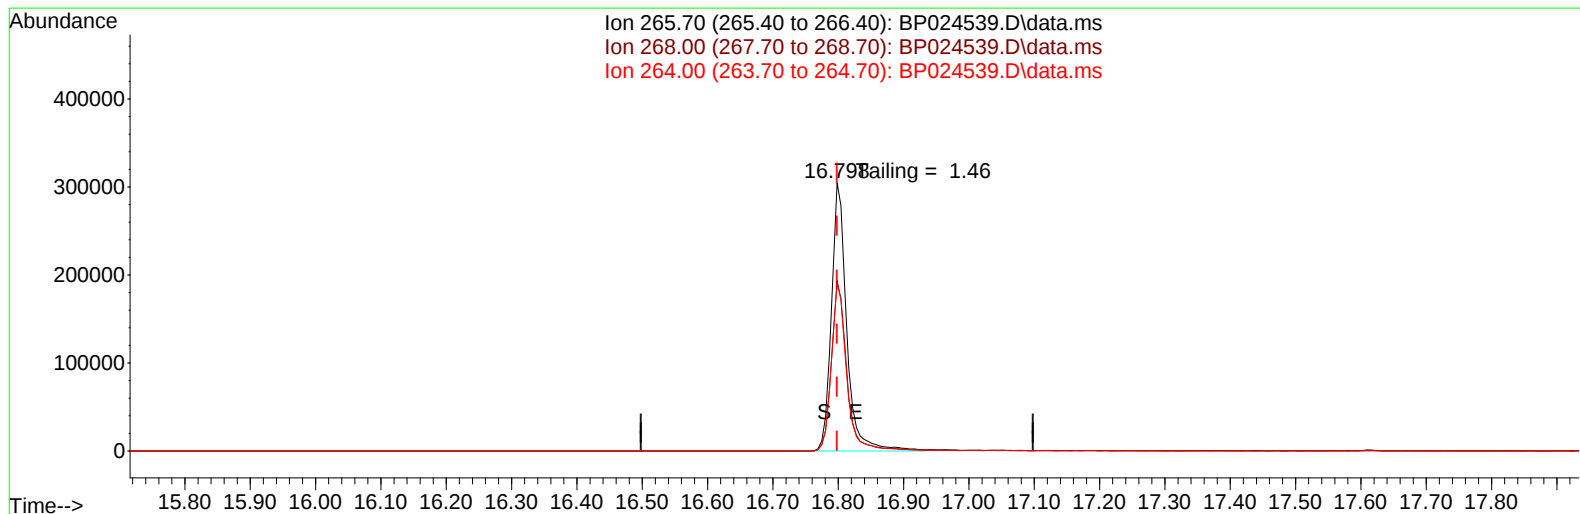

TIC: BP024539.D\data.ms

(70) Pentachlorophenol (C)

16.798min (+ 0.000) 36682.01 ng




response 497194

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.43
264.00	62.20	62.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050625\
Data File : BP024539.D
Acq On : 06 May 2025 09:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 06 13:41:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

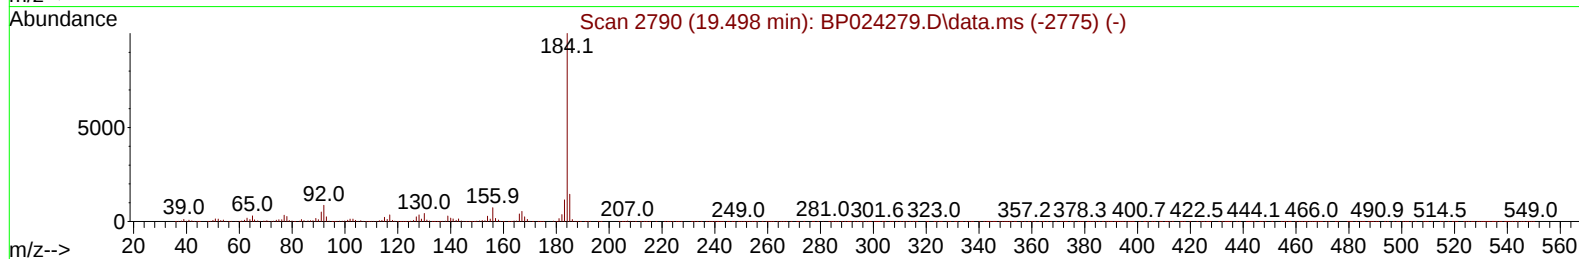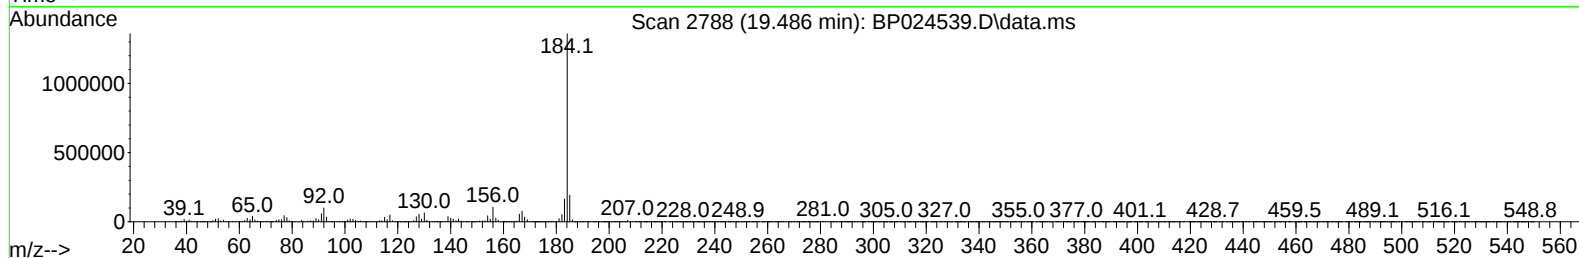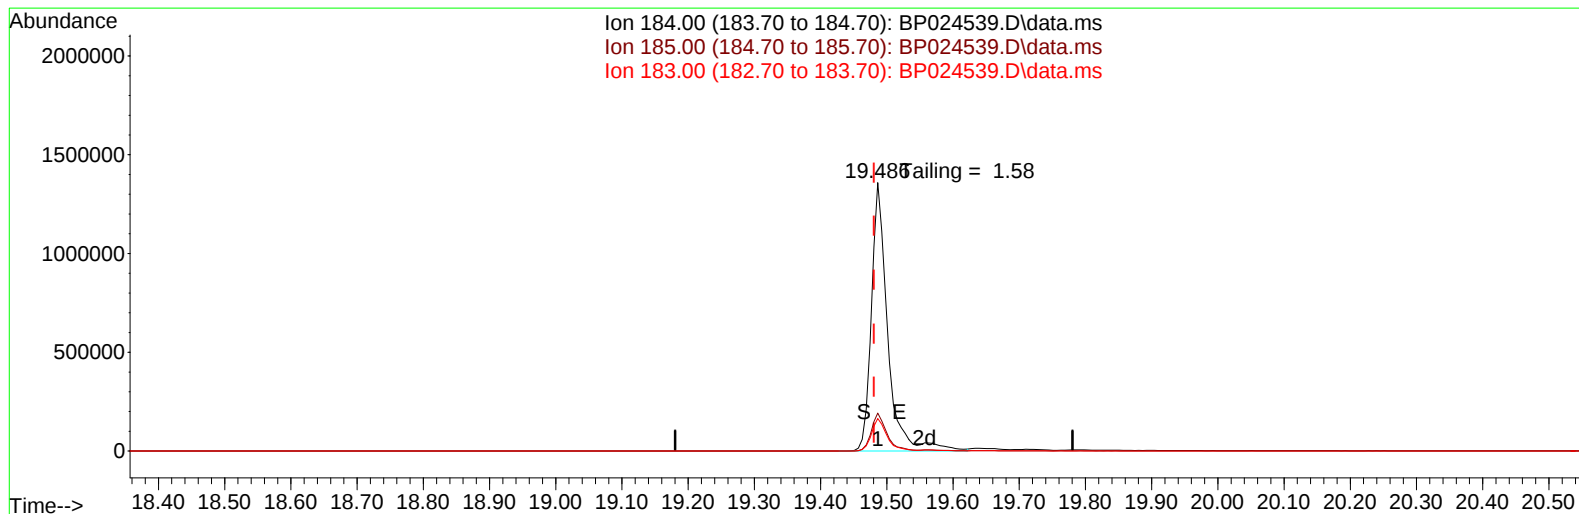

TIC: BP024539.D\data.ms

(77) Benzidine

19.486min (+ 0.006) 48697.69 ng

response 2219755

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.17
183.00	11.50	12.11
0.00	0.00	0.00