
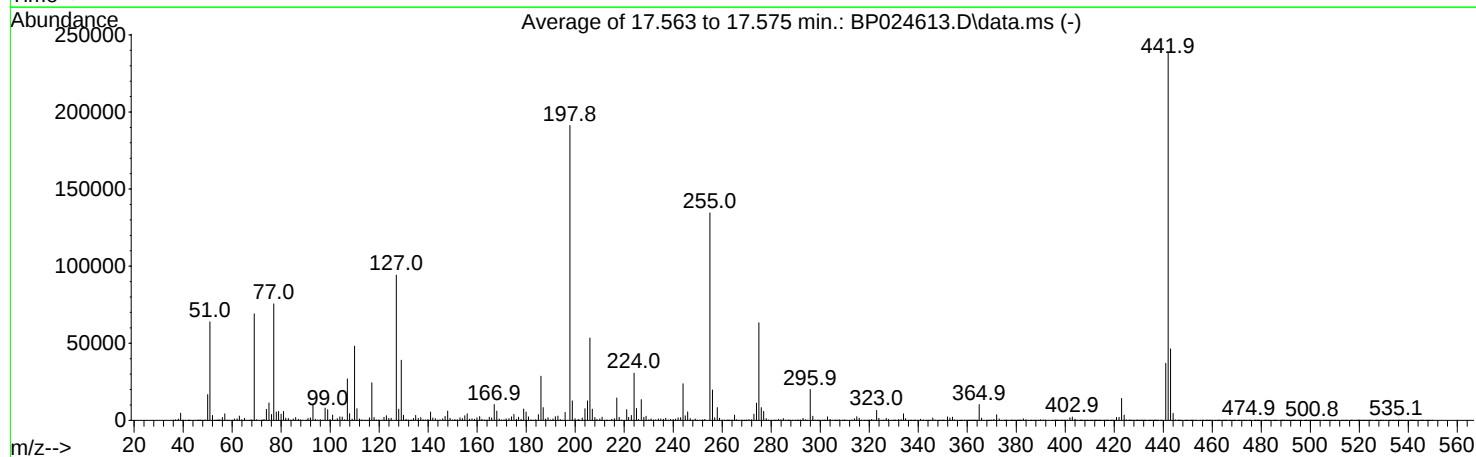


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051325\
Data File : BP024613.D
Acq On : 13 May 2025 10:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 13 16:21:39 2025

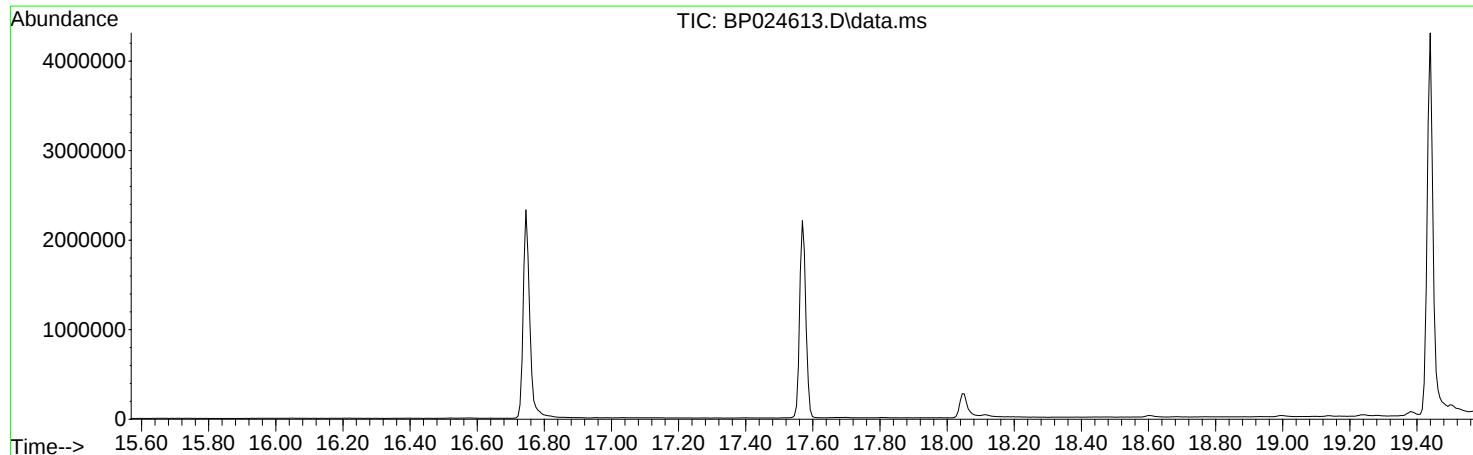

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	63968	PASS
68	69	0.00	2	0.6	438	PASS
69	198	0.00	100	36.2	69152	PASS
70	69	0.00	2	0.6	419	PASS
127	198	10	80	49.3	94192	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	191223	PASS
199	198	5	9	6.6	12661	PASS
275	198	10	60	33.1	63293	PASS
365	198	1	100	5.4	10286	PASS
441	198	0.01	100	19.4	37080	PASS
442	442	100	100	100.0	238569	PASS
443	442	15	24	19.4	46397	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/13/2025	BNA_P	<u>BP024613.D</u>
Compound Name	Response	Retention Time
DDT	750509	20.716
DDD	13774	20.269
DDE	1248	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15022	765531	1.96

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051325\
Data File : BP024613.D
Acq On : 13 May 2025 10:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 13 12:28:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 12:28:24 2025
Response via : Initial Calibration

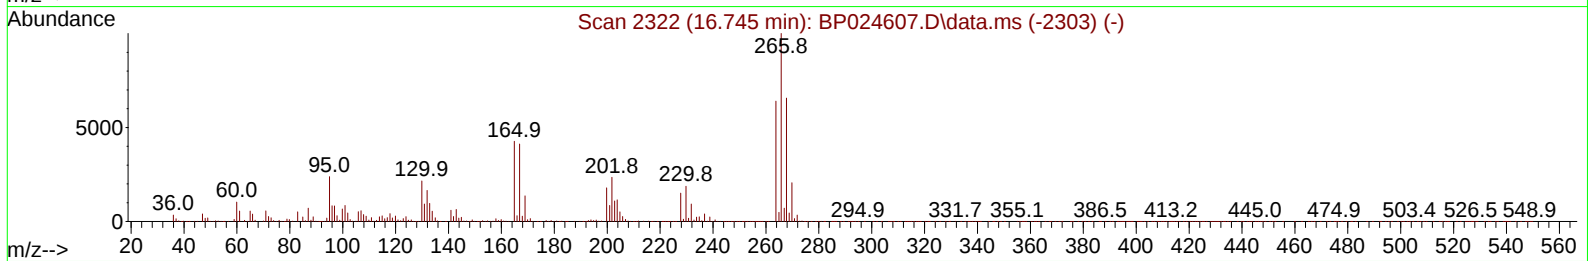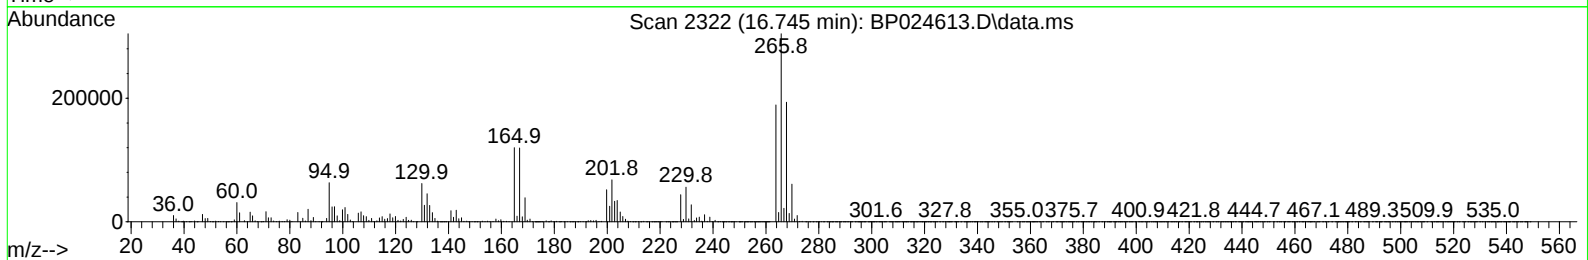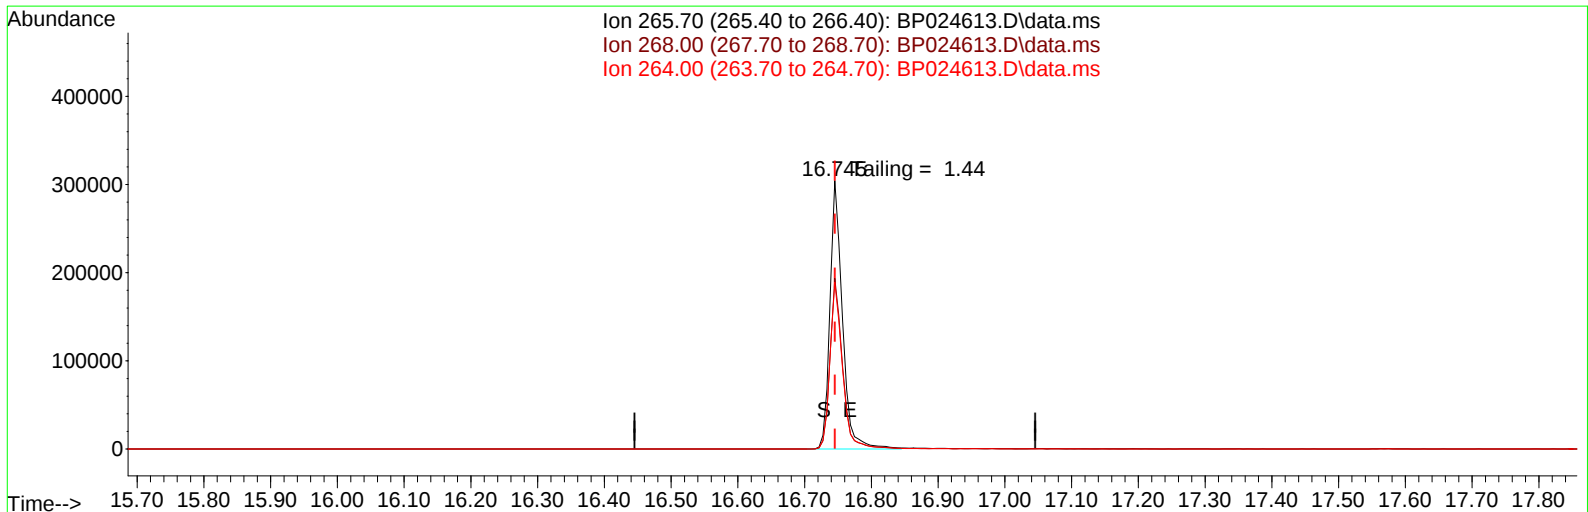

TIC: BP024613.D\data.ms

(70) Pentachlorophenol (C)

16.745min (-0.000) 42670.46 ng




response 398426

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.60	63.59
264.00	64.00	62.12
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051325\  
Data File : BP024613.D  
Acq On    : 13 May 2025  10:00  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 13 12:28:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Tue May 13 12:28:24 2025
Response via : Initial Calibration

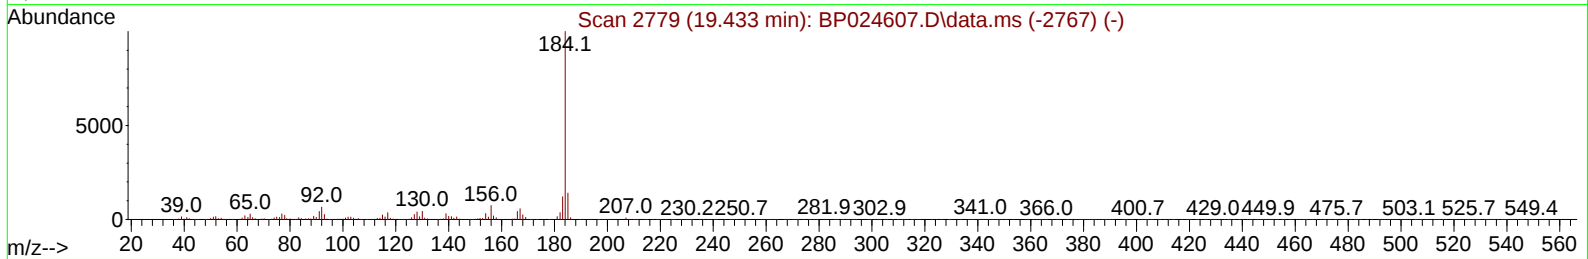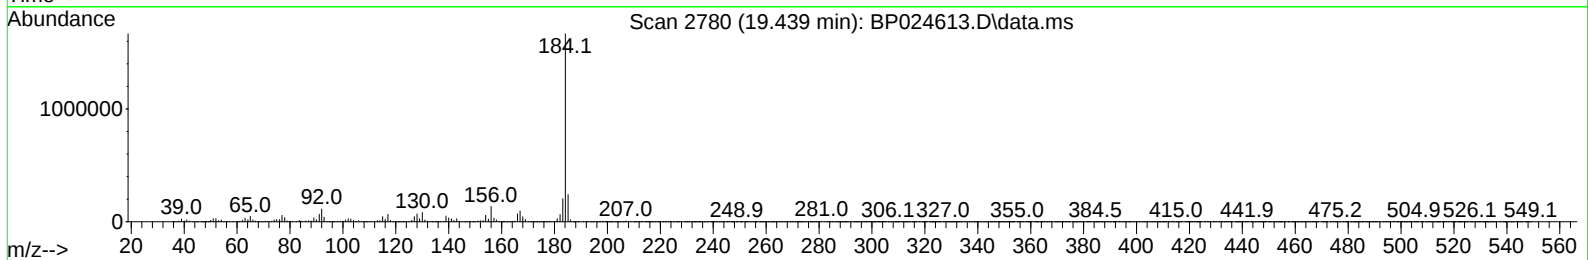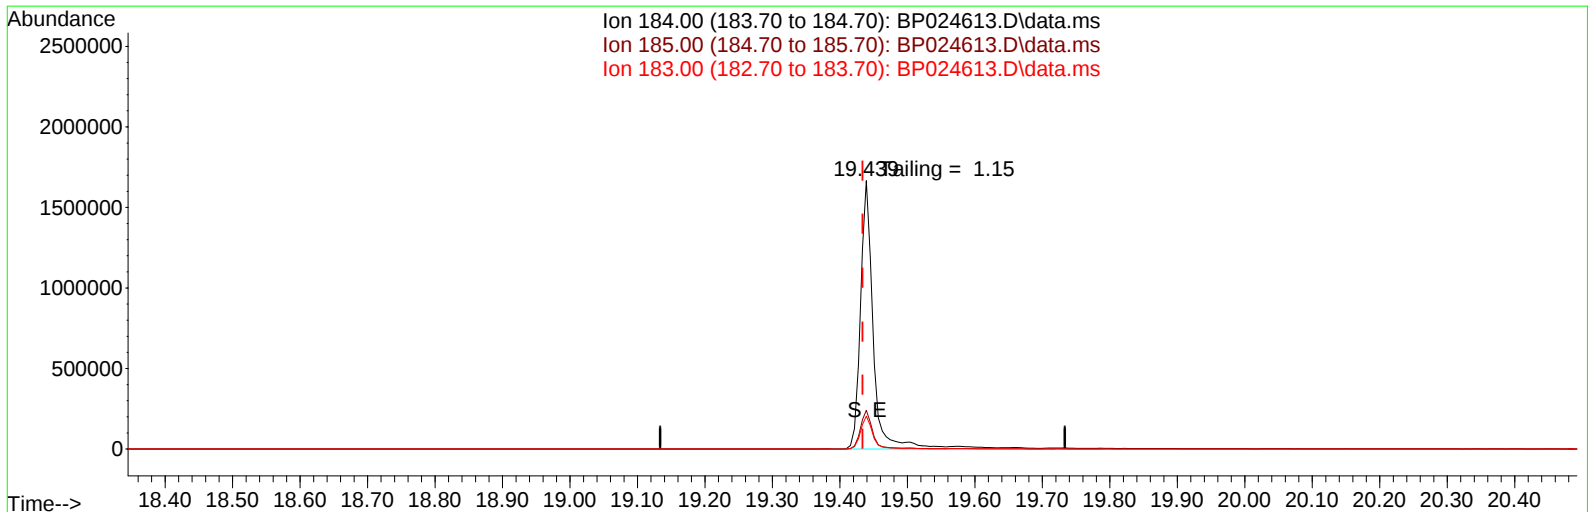

TIC: BP024613.D\data.ms

(77) Benzidine

19.439min (+ 0.006) 5637.89 ng

response **2074486**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.46
183.00	12.10	12.23
0.00	0.00	0.00