
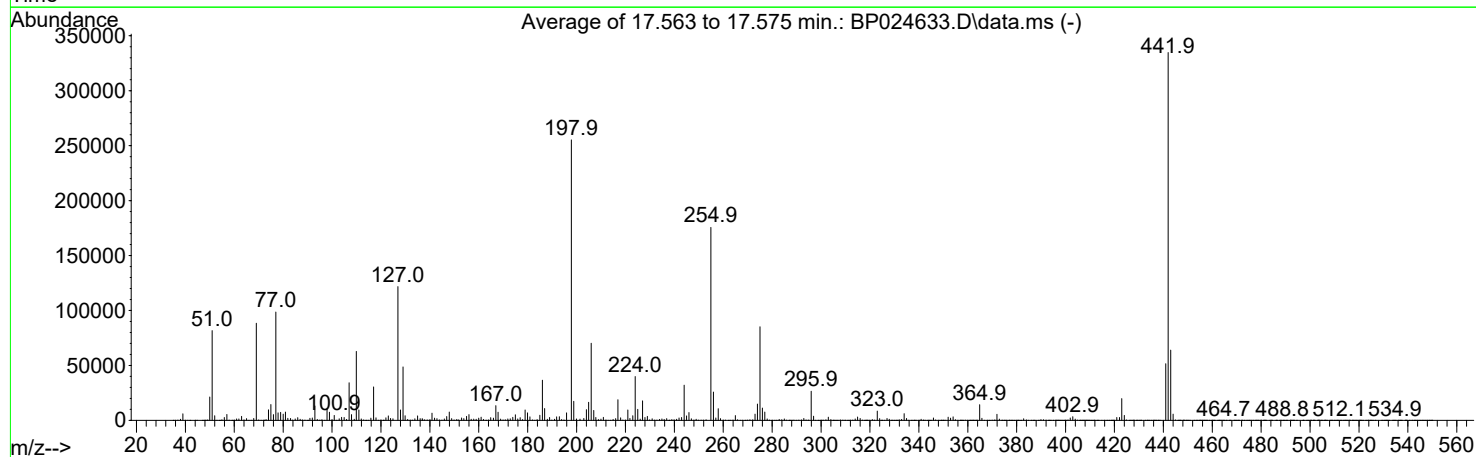


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
Data File : BP024633.D
Acq On : 15 May 2025 11:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 13 16:21:39 2025

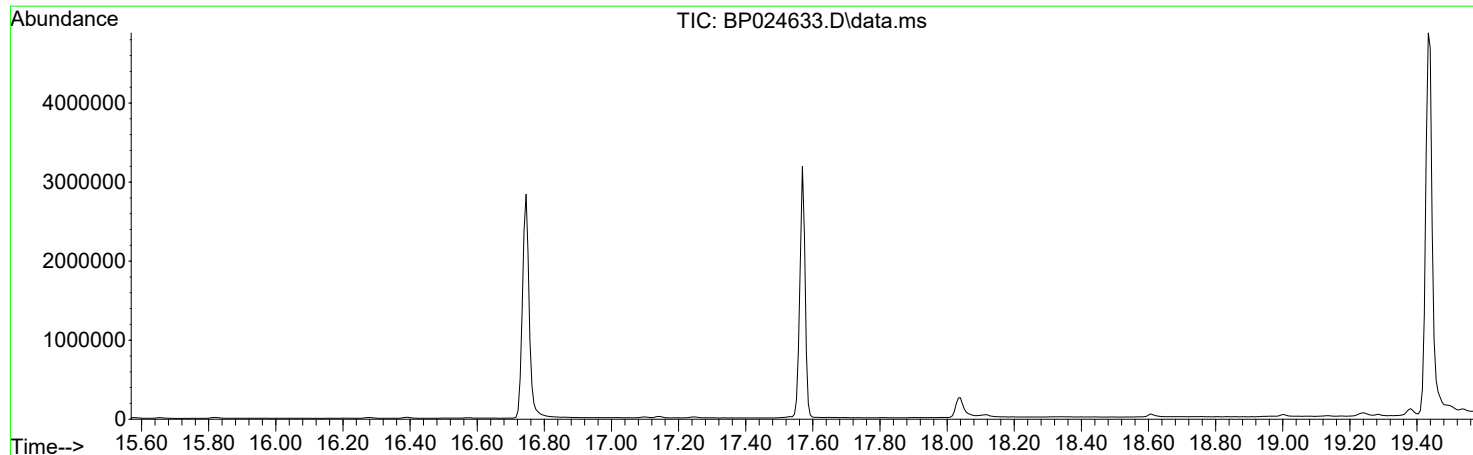

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	81645	PASS
68	69	0.00	2	1.9	1680	PASS
69	198	0.00	100	34.7	88475	PASS
70	69	0.00	2	0.5	470	PASS
127	198	10	80	47.7	121754	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	255334	PASS
199	198	5	9	6.8	17403	PASS
275	198	10	60	33.3	85133	PASS
365	198	1	100	5.6	14303	PASS
441	198	0.01	100	20.2	51620	PASS
442	442	100	100	100.0	334783	PASS
443	442	15	24	19.1	63921	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/15/2025	BNA_P	<u>BP024633.D</u>
Compound Name	Response	Retention Time
DDT	908054	20.728
DDD	22084	20.275
DDE	1154	19.822
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23238	931292	2.50

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
Data File : BP024633.D
Acq On : 15 May 2025 11:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 15 13:40:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

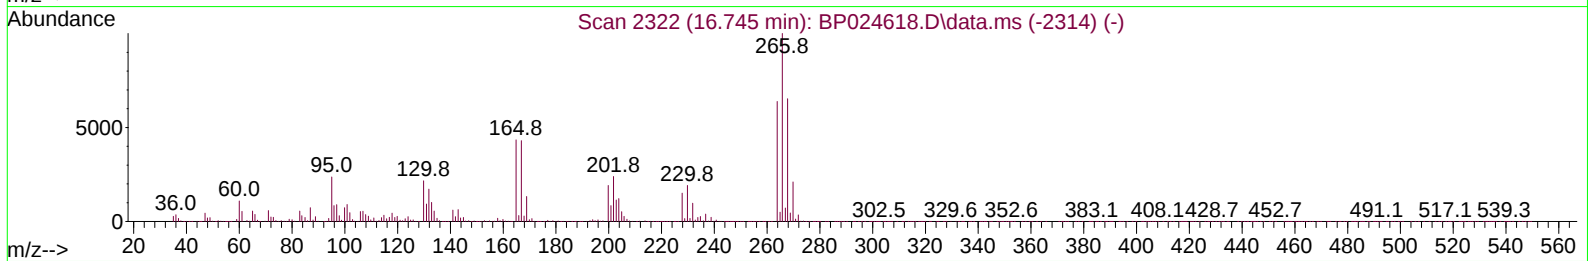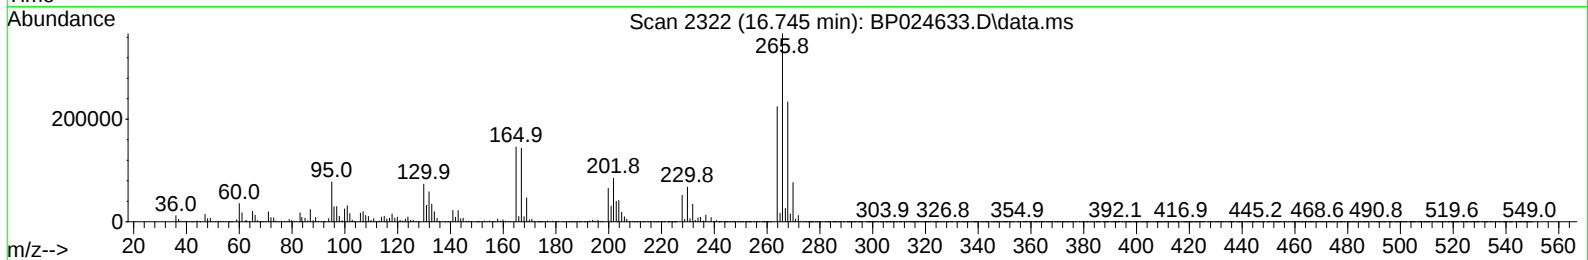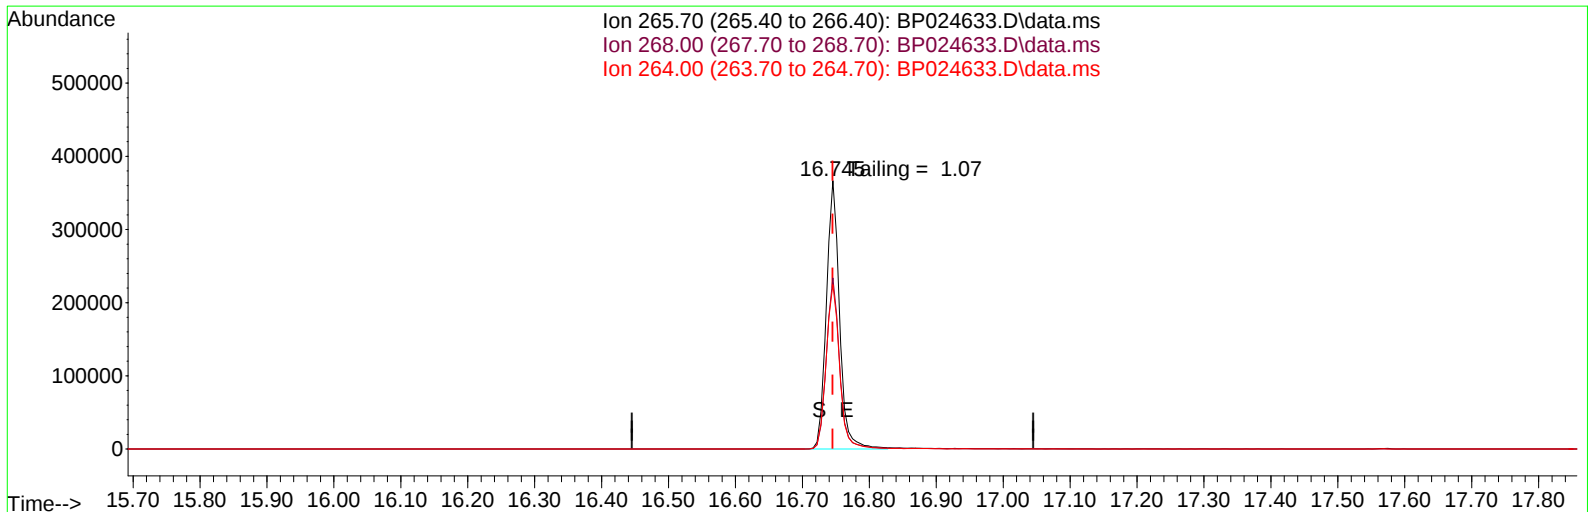

TIC: BP024633.D\data.ms

(70) Pentachlorophenol (C)

16.745min (+ 0.000) 9498.09 ng




response 503182

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	63.72
264.00	63.90	61.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
Data File : BP024633.D
Acq On : 15 May 2025 11:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 15 13:40:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

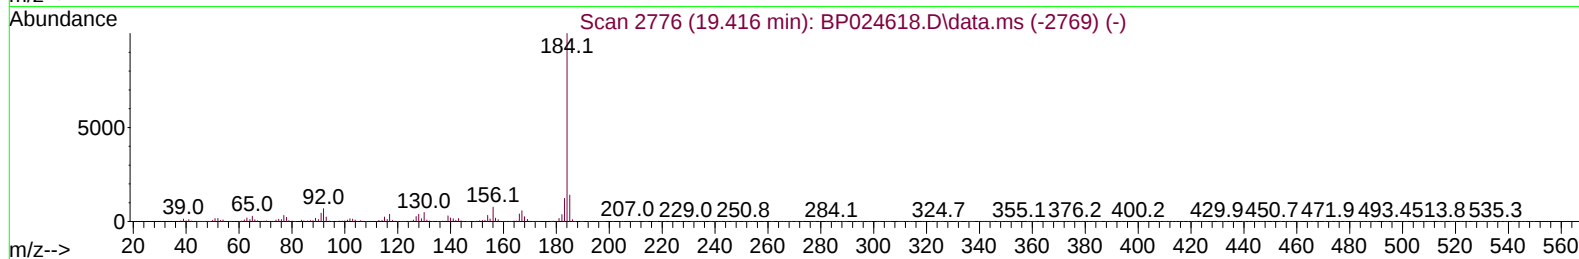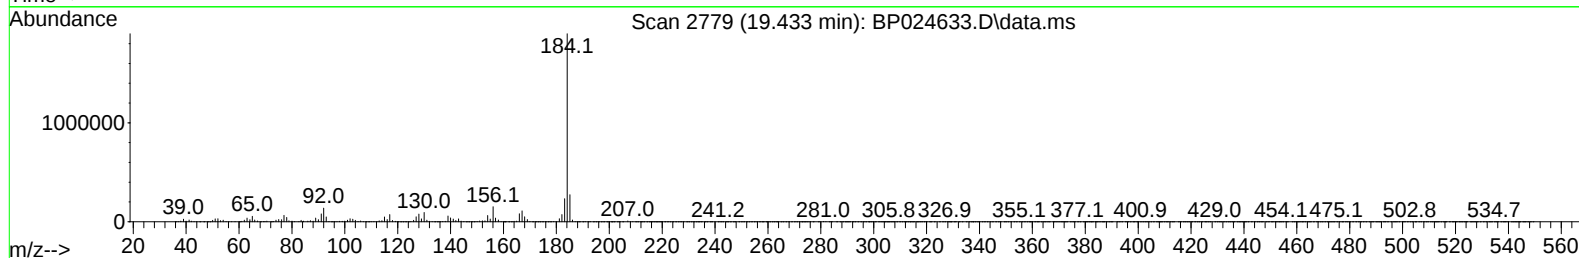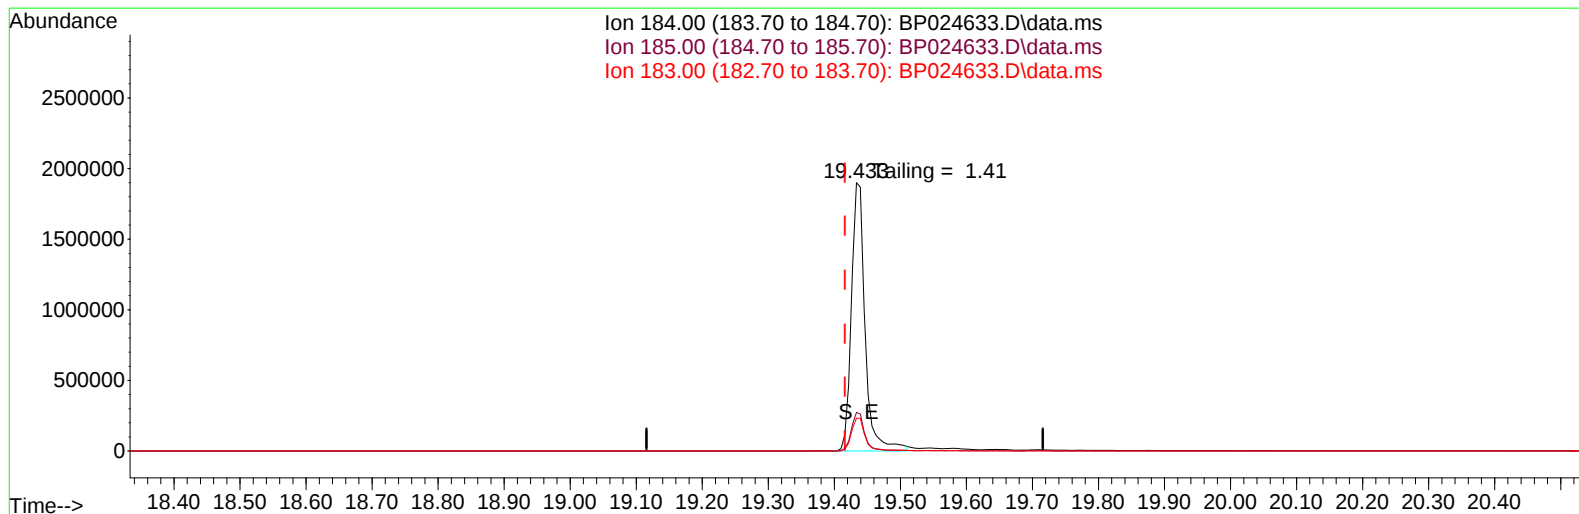

TIC: BP024633.D\data.ms

(77) Benzidine

19.433min (+ 0.017) 2596.29 ng

response 2759335

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.40
183.00	12.30	12.29
0.00	0.00	0.00