

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051625\
 Data File : VY022278.D
 Acq On : 16 May 2025 09:37
 Operator : SY/MD
 Sample : VY0516SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0516SBL01

Quant Time: May 17 01:27:50 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051525S.M
 Quant Title : SW846 8260
 QLast Update : Fri May 16 01:42:09 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	314347	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	555500	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.420	117	426459	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	151389	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	150831	43.903	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	87.800%
35) Dibromofluoromethane	7.634	113	158963	47.945	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	95.880%
50) Toluene-d8	10.109	98	662270	48.771	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	97.540%
62) 4-Bromofluorobenzene	12.408	95	208685	48.485	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	96.980%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051625\
Data File : VY022278.D
Acq On : 16 May 2025 09:37
Operator : SY/MD
Sample : VY0516SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0516SBL01

Quant Time: May 17 01:27:50 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051525S.M
Quant Title : SW846 8260
QLast Update : Fri May 16 01:42:09 2025
Response via : Initial Calibration




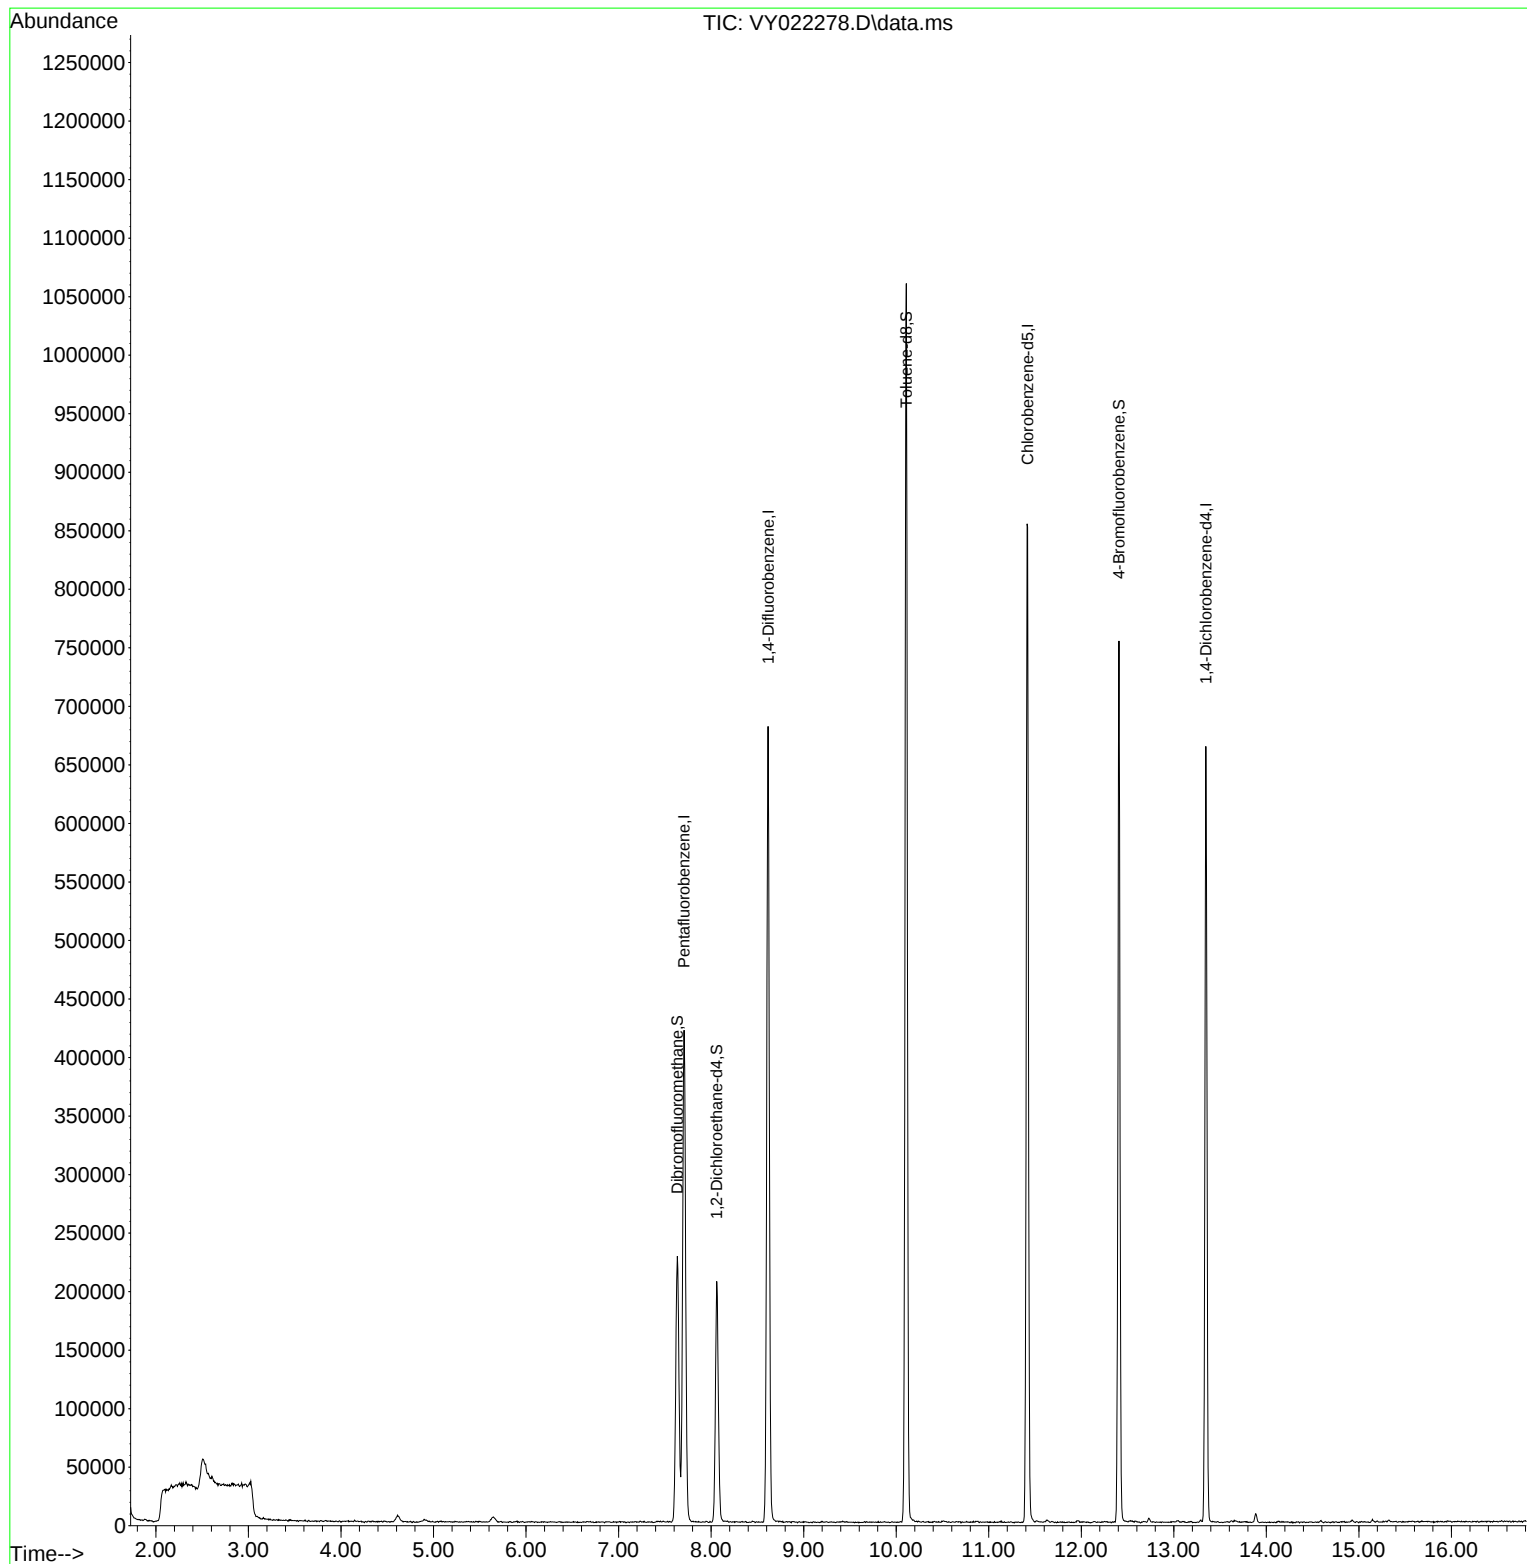


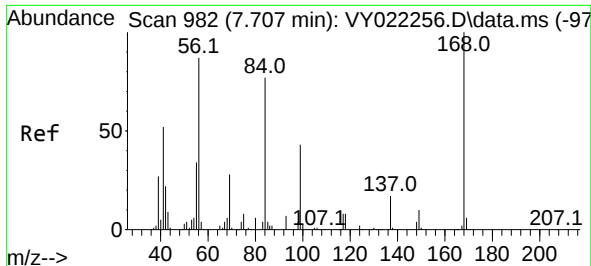

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 982
Delta R.T. 0.000 min
Lab File: VY022278.D
Acq: 16 May 2025 09:37




Instrument :
MSVOA_Y
ClientSampleId :
VY0516SBL01


Tgt Ion:168 Resp: 314347
Ion Ratio Lower Upper
168 100
99 55.4 44.2 66.4

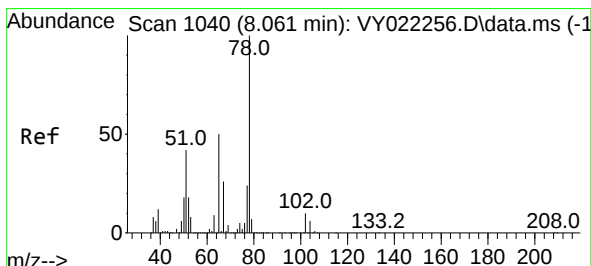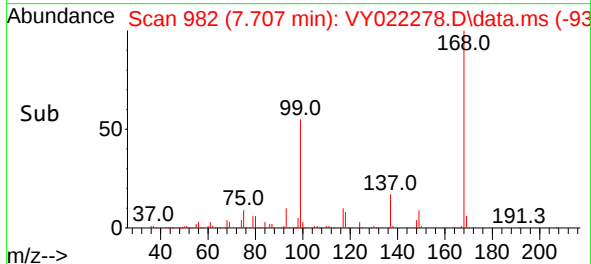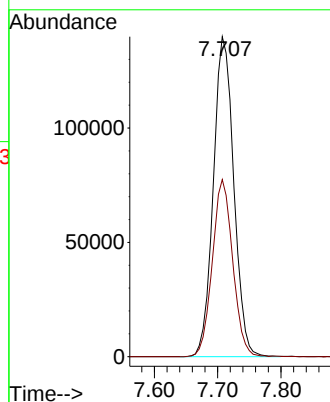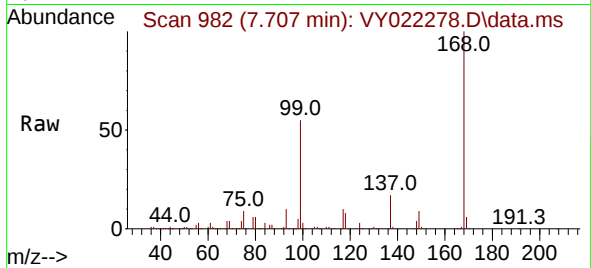

#33
1,2-Dichloroethane-d4
Concen: 43.903 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY022278.D
Acq: 16 May 2025 09:37

Tgt Ion: 65 Resp: 150831
Ion Ratio Lower Upper
65 100
67 52.5 0.0 104.6


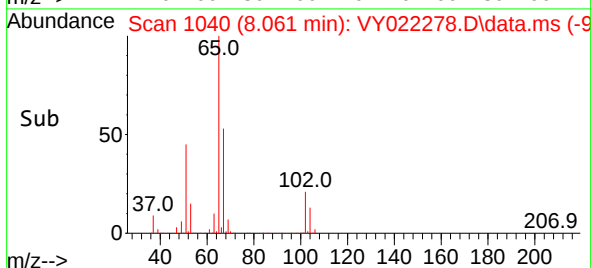
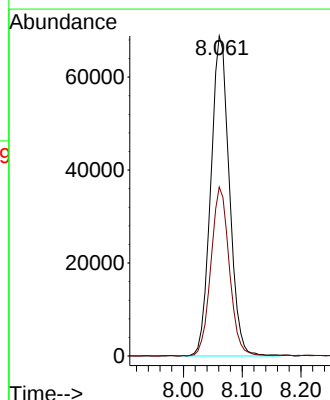
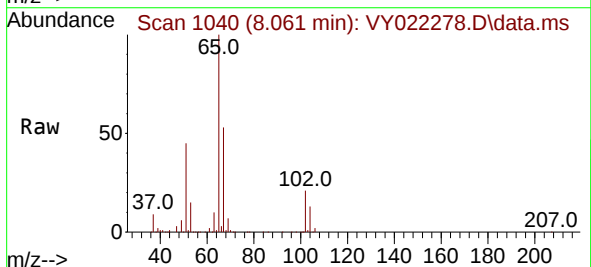


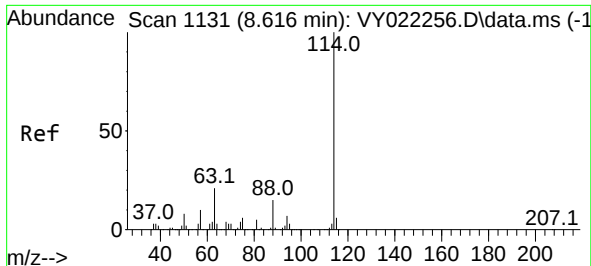

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. 0.000 min
Lab File: VY022278.D
Acq: 16 May 2025 09:37




Instrument :
MSVOA_Y
ClientSampleId :
VY0516SBL01


Tgt Ion:114 Resp: 555500
Ion Ratio Lower Upper
114 100
63 20.8 0.0 41.0
88 14.6 0.0 29.4

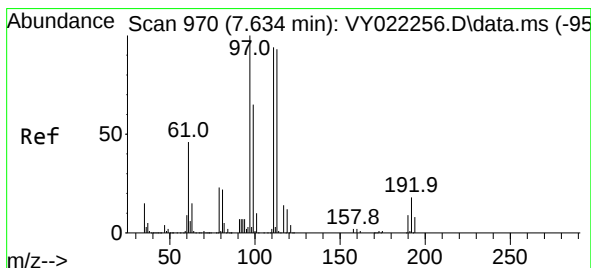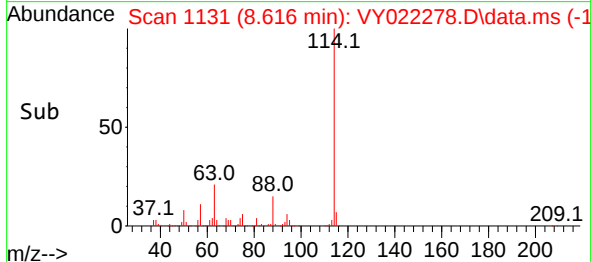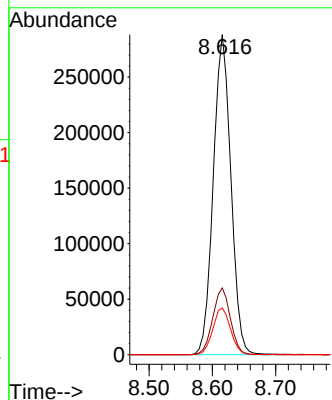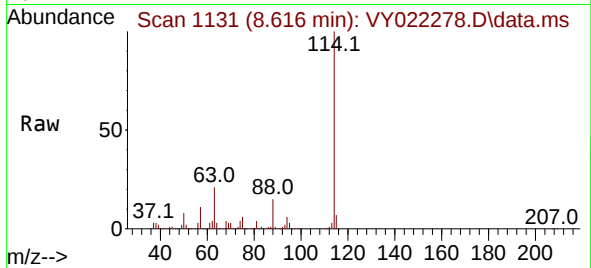

#35
Dibromofluoromethane
Concen: 47.945 ug/l
RT: 7.634 min Scan# 970
Delta R.T. 0.000 min
Lab File: VY022278.D
Acq: 16 May 2025 09:37

Tgt Ion:113 Resp: 158963
Ion Ratio Lower Upper
113 100
111 102.9 82.6 123.8
192 18.4 15.2 22.8

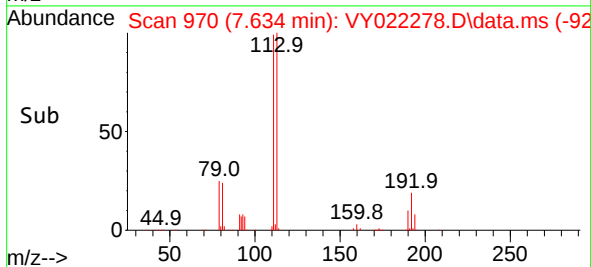
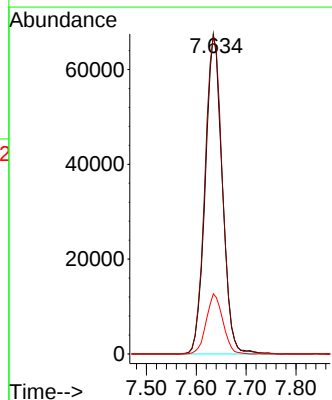
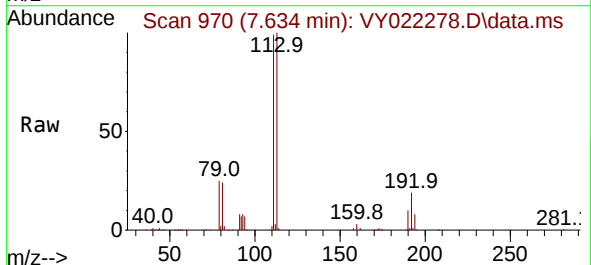


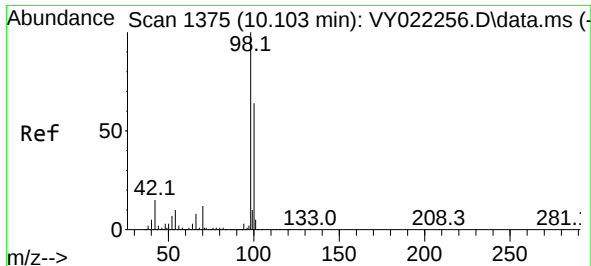

#50
Toluene-d8
Concen: 48.771 ug/l
RT: 10.109 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY022278.D
Acq: 16 May 2025 09:37




Instrument :
MSVOA_Y
ClientSampleId :
VY0516SBL01


Tgt Ion: 98 Resp: 662270
Ion Ratio Lower Upper
98 100
100 64.9 51.8 77.8

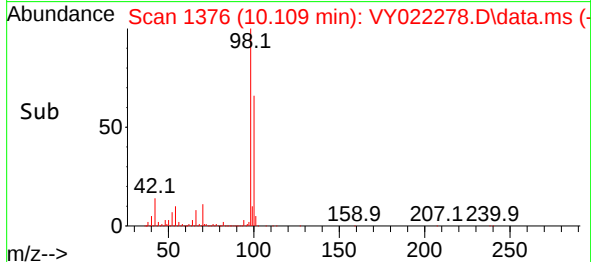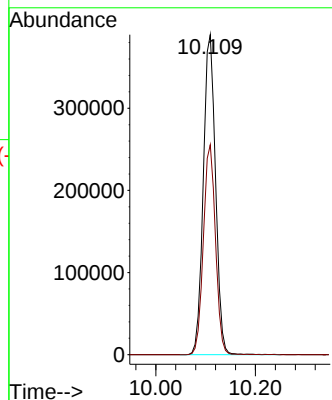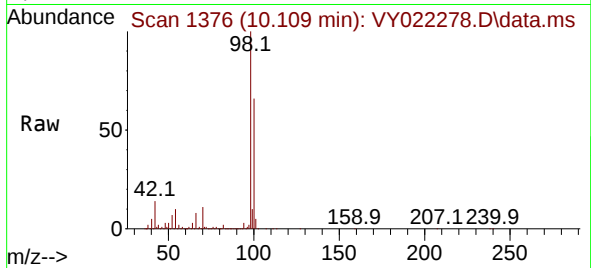

#62
4-Bromofluorobenzene
Concen: 48.485 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.000 min
Lab File: VY022278.D
Acq: 16 May 2025 09:37

Tgt Ion: 95 Resp: 208685
Ion Ratio Lower Upper
95 100
174 83.9 0.0 166.8
176 81.7 0.0 160.8

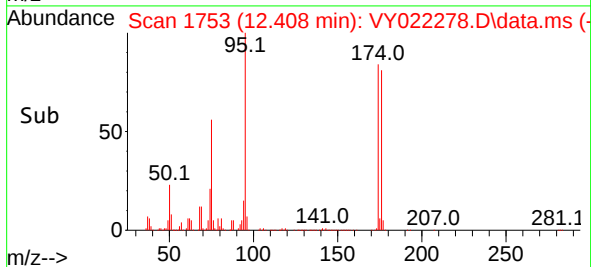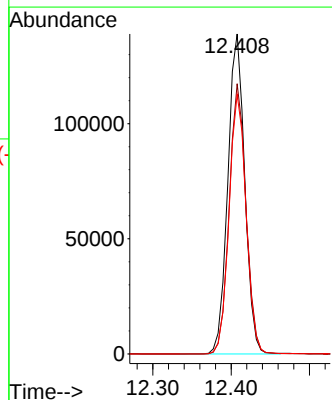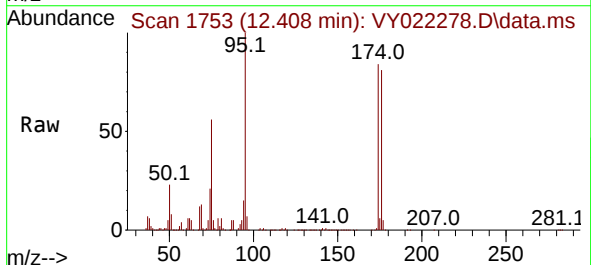

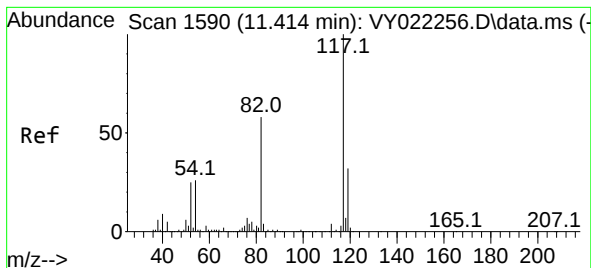

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.420 min Scan# 11

Delta R.T. 0.006 min

Lab File: VY022278.D

Acq: 16 May 2025 09:37

Instrument :

MSVOA_Y

ClientSampleId :

VY0516SBL01





Tgt Ion:117 Resp: 426459

Ion Ratio Lower Upper

117 100

82 55.8 46.6 70.0

119 32.7 25.8 38.6

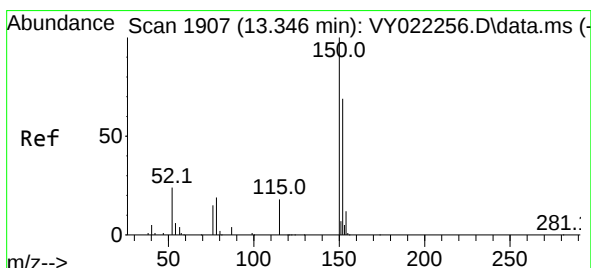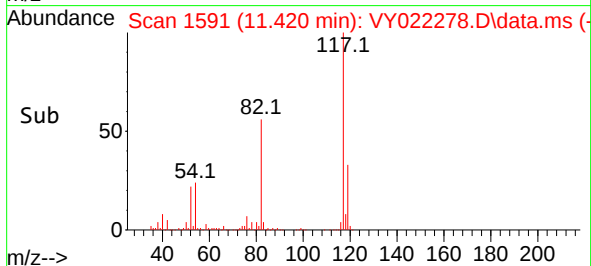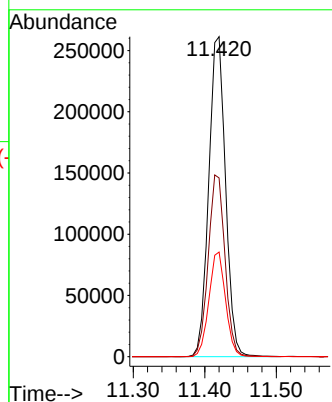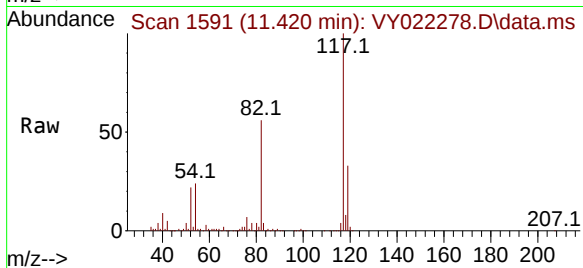

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.347 min Scan# 1907

Delta R.T. 0.000 min

Lab File: VY022278.D

Acq: 16 May 2025 09:37

Tgt Ion:152 Resp: 151389

Ion Ratio Lower Upper

152 100

115 58.4 29.4 88.2

150 156.5 0.0 353.8

