

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041825\
 Data File : PD088123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2025 13:43
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 06:03:25 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041825.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 19 06:32:27 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.552	2.883	37870717	290.8E6	18.960	19.885
28)	SA Decachlor...	9.075	8.076	66771462	372.0E6	20.184	20.130
Target Compounds							
9)	A Endosulfan I	6.077	5.251	29410187	177.2E6	8.709	9.836
10)	B gamma-Chl...	5.948	5.130	32853106	209.1E6	9.070	10.304
12)	B 4,4'-DDE	6.198	5.379	60393989	395.9E6	18.311	20.100
13)	MA Dieldrin	6.349	5.517	64800077	392.3E6	18.159	19.682
19)	B Endosulfa...	7.151	6.486	54061534	339.7E6	18.799	19.830
20)	A Methoxychlor	7.495	6.758	137.4E6	780.0E6	91.608	85.519
21)	B Endrin ke...	7.631	6.995	57978754	371.5E6	18.784	19.864



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041825\
Data File : PD088123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2025 13:43
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 06:03:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041825.M
Quant Title : GC Extractables
QLast Update : Sat Apr 19 06:32:27 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

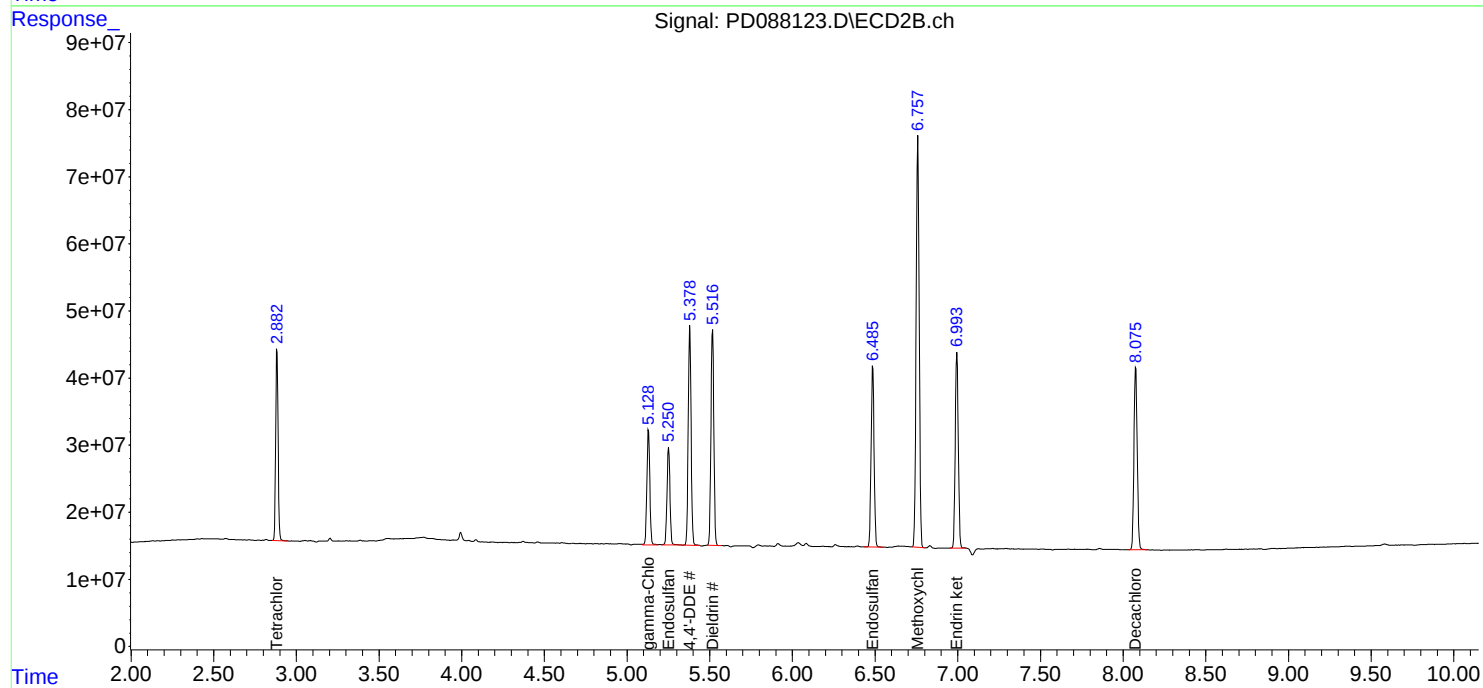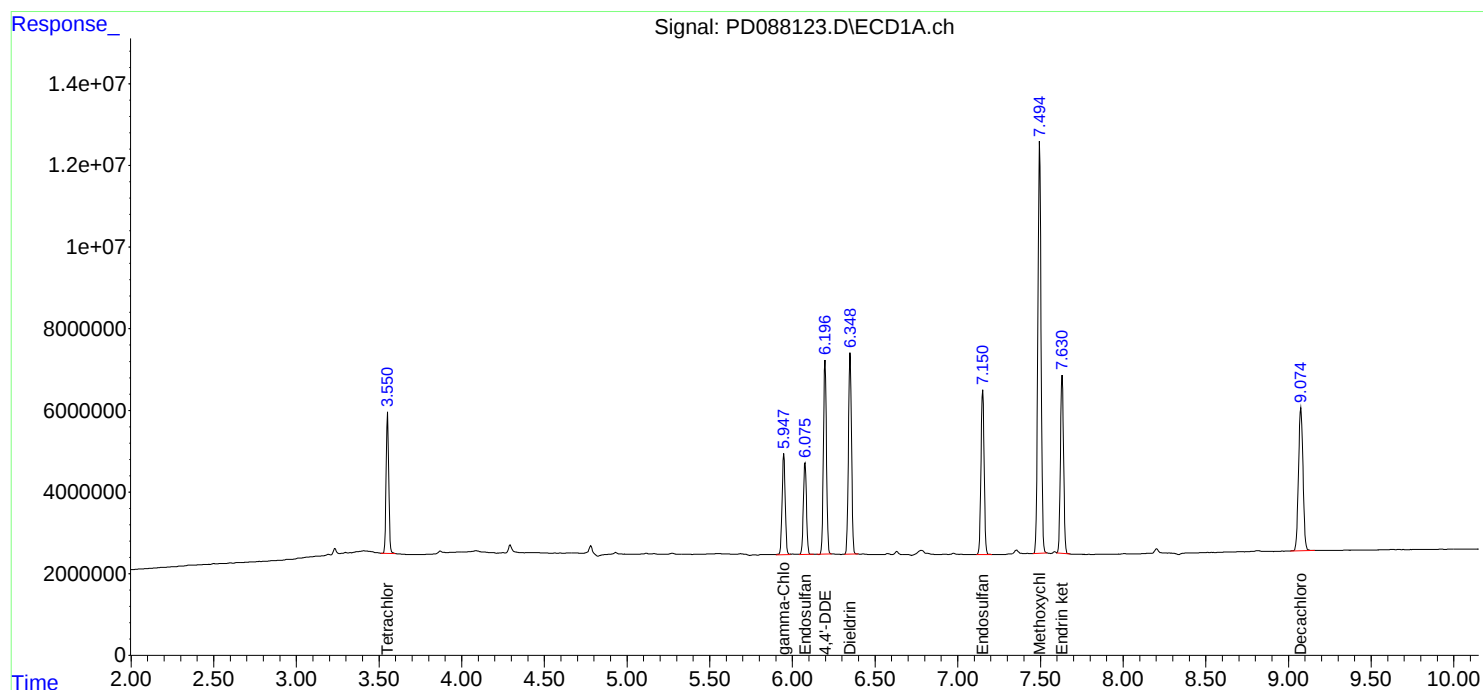


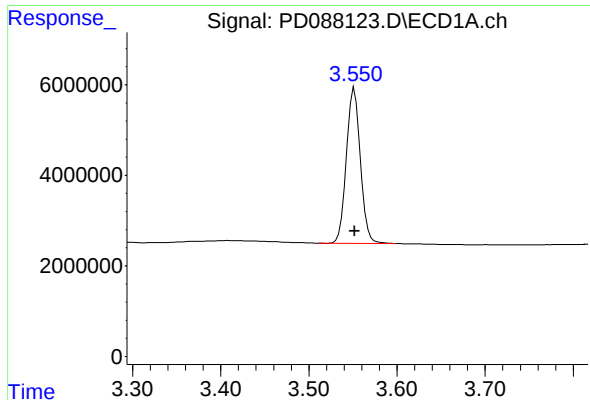

#1 Tetrachloro-m-xylene


R.T.: 3.552 min
Delta R.T.: 0.000 min
Response: 37870717
Conc: 18.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

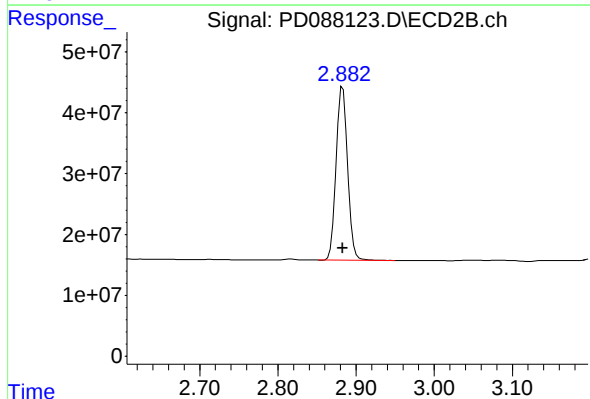


#1 Tetrachloro-m-xylene

R.T.: 2.883 min
Delta R.T.: 0.000 min
Response: 290753510
Conc: 19.89 ng/ml

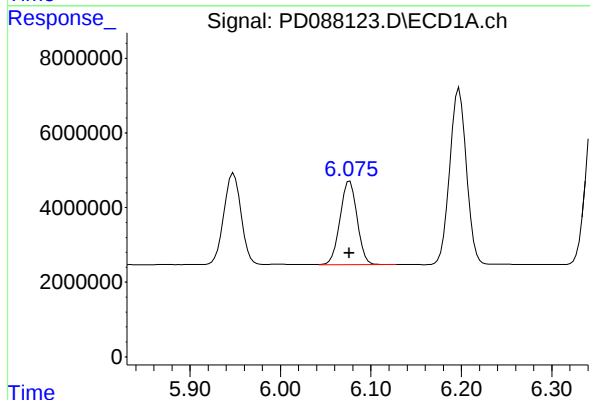


#9 Endosulfan I

R.T.: 6.077 min
Delta R.T.: 0.000 min
Response: 29410187
Conc: 8.71 ng/ml

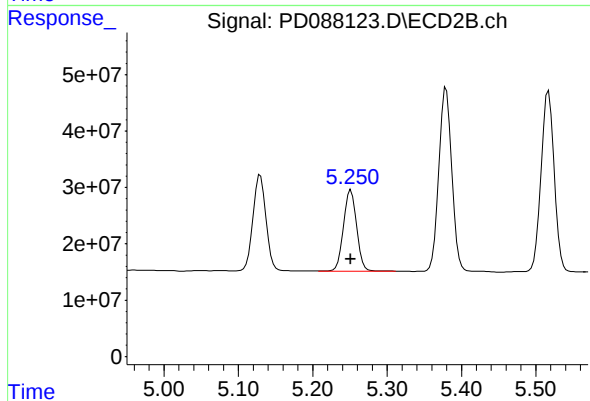

#9 Endosulfan I


R.T.: 5.251 min
Delta R.T.: 0.000 min
Response: 177177453
Conc: 9.84 ng/ml

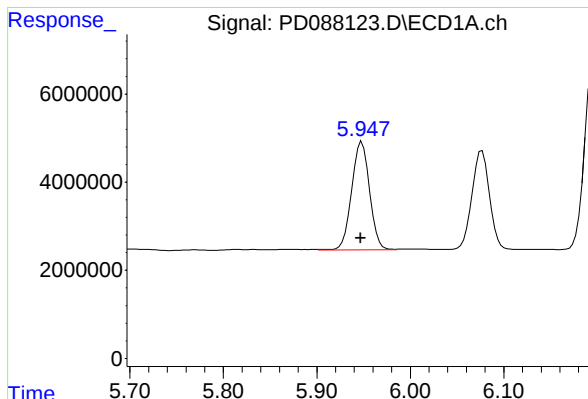

#10 gamma-Chlordane


R.T.: 5.948 min
Delta R.T.: 0.001 min
Response: 32853106
Conc: 9.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

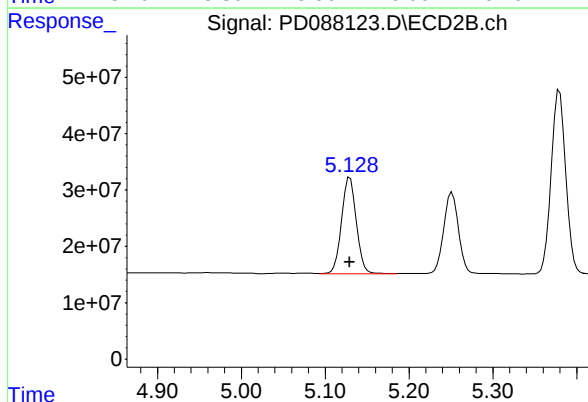


#10 gamma-Chlordane

R.T.: 5.130 min
Delta R.T.: 0.000 min
Response: 209139105
Conc: 10.30 ng/ml

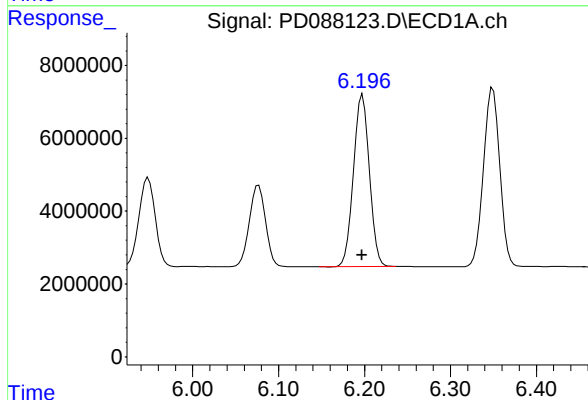


#12 4,4'-DDE

R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 60393989
Conc: 18.31 ng/ml

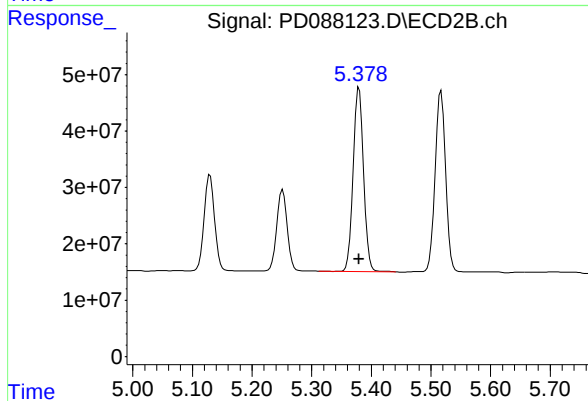

#12 4,4'-DDE


R.T.: 5.379 min
Delta R.T.: 0.000 min
Response: 395851321
Conc: 20.10 ng/ml

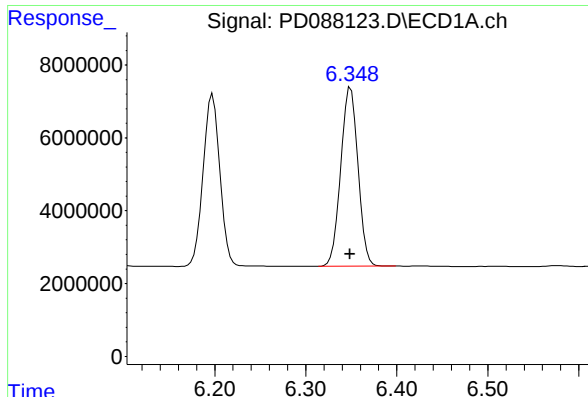

#13 Dieldrin


R.T.: 6.349 min
Delta R.T.: 0.000 min
Response: 64800077
Conc: 18.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

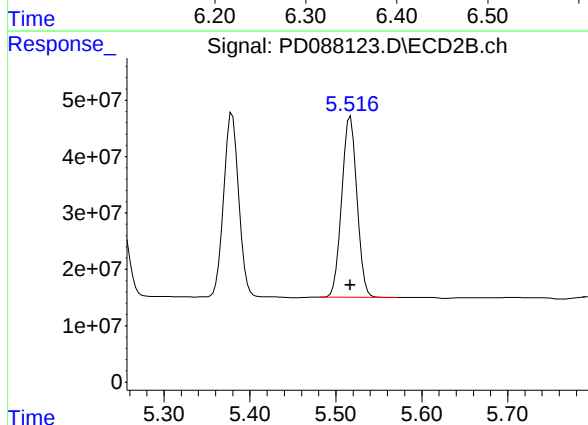


#13 Dieldrin

R.T.: 5.517 min
Delta R.T.: 0.000 min
Response: 392323553
Conc: 19.68 ng/ml

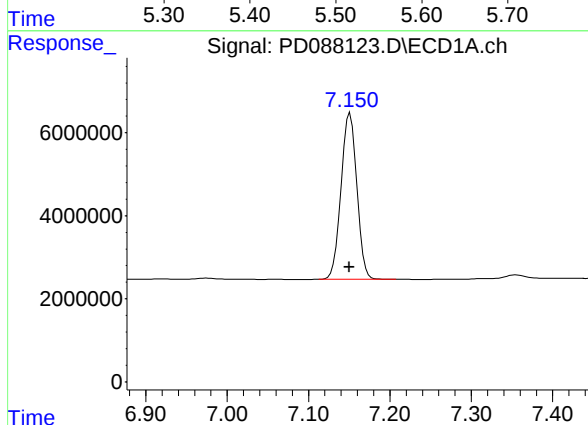


#19 Endosulfan Sulfate

R.T.: 7.151 min
Delta R.T.: 0.000 min
Response: 54061534
Conc: 18.80 ng/ml

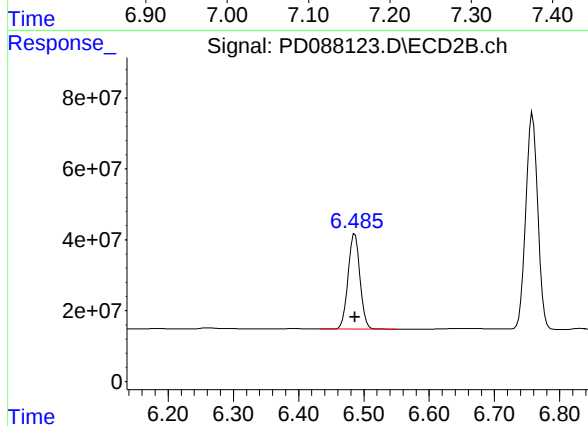

#19 Endosulfan Sulfate


R.T.: 6.486 min
Delta R.T.: 0.000 min
Response: 339744835
Conc: 19.83 ng/ml

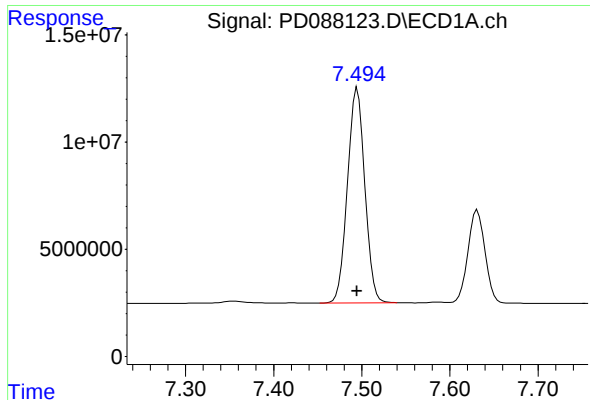

#20 Methoxychlor


R.T.: 7.495 min
Delta R.T.: 0.000 min
Response: 137370950
Conc: 91.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

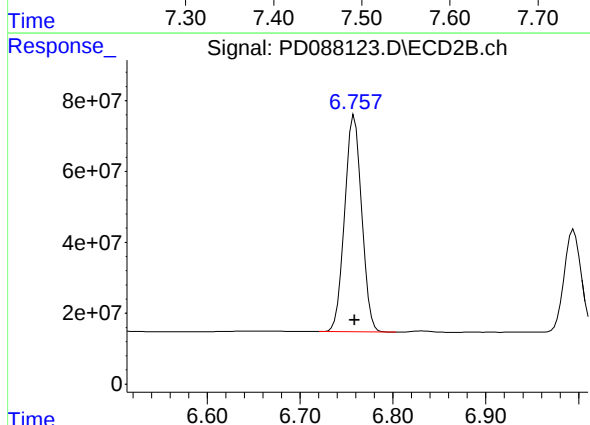


#20 Methoxychlor

R.T.: 6.758 min
Delta R.T.: 0.000 min
Response: 780024876
Conc: 85.52 ng/ml

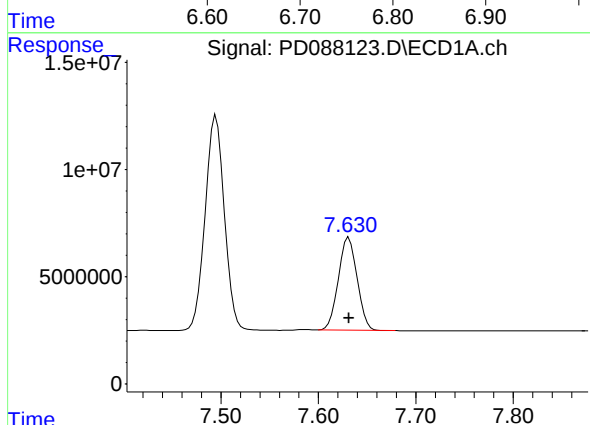


#21 Endrin ketone

R.T.: 7.631 min
Delta R.T.: 0.000 min
Response: 57978754
Conc: 18.78 ng/ml

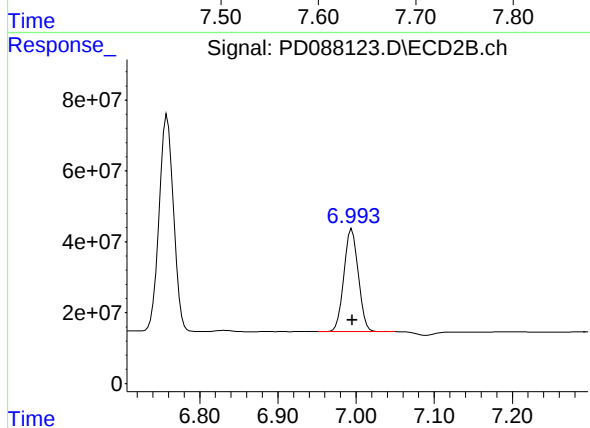

#21 Endrin ketone


R.T.: 6.995 min
Delta R.T.: 0.000 min
Response: 371541118
Conc: 19.86 ng/ml

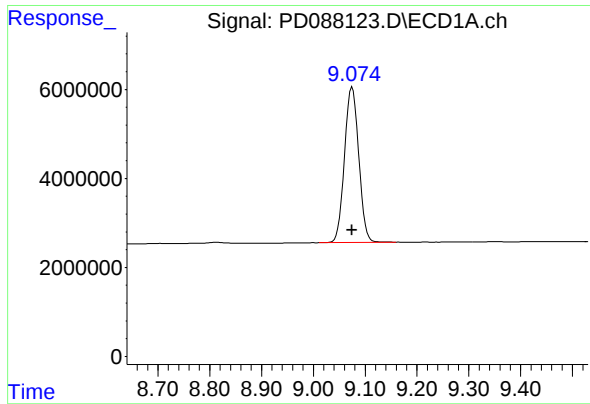

#28 Decachlorobiphenyl

R.T.: 9.075 min
Delta R.T.: 0.000 min
Response: 66771462
Conc: 20.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

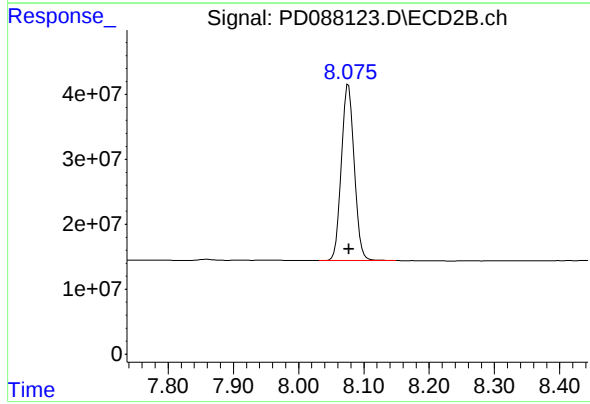

#28 Decachlorobiphenyl

R.T.: 8.076 min
Delta R.T.: 0.000 min
Response: 371985891
Conc: 20.13 ng/ml