


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052025\
Data File : BP024719.D
Acq On : 21 May 2025 00:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 13 16:21:39 2025

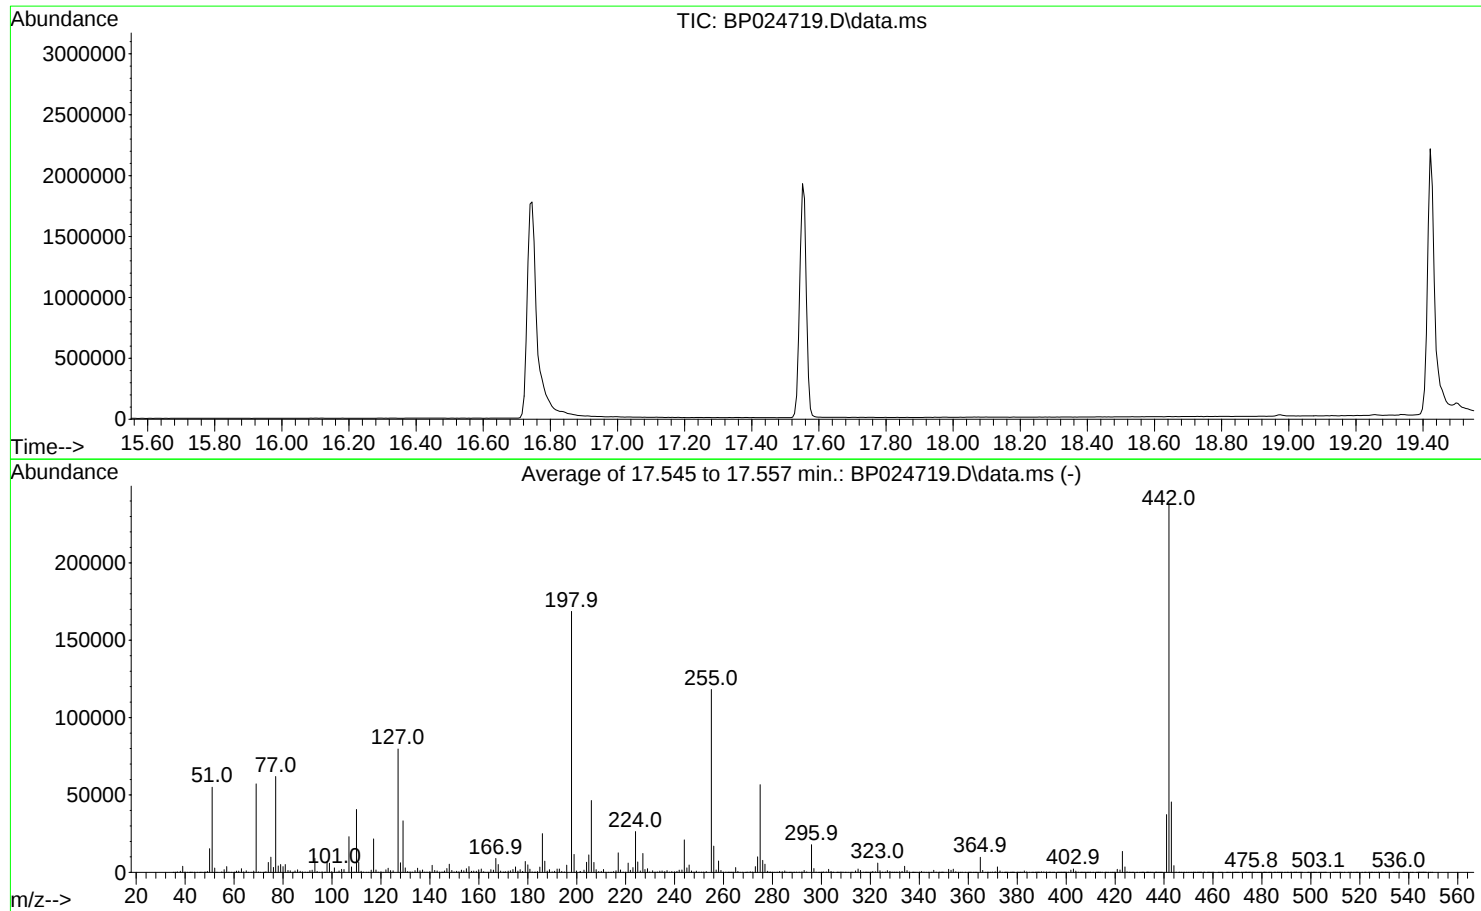




AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	55010	PASS
68	69	0.00	2	1.5	860	PASS
69	198	0.00	100	33.9	57147	PASS
70	69	0.00	2	0.5	296	PASS
127	198	10	80	47.3	79720	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	168604	PASS
199	198	5	9	6.9	11589	PASS
275	198	10	60	33.6	56664	PASS
365	198	1	100	5.8	9757	PASS
441	198	0.01	100	22.1	37312	PASS
442	442	100	100	100.0	237717	PASS
443	442	15	24	19.1	45464	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052025\
Data File : BP024719.D
Acq On : 21 May 2025 00:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 21 02:08:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

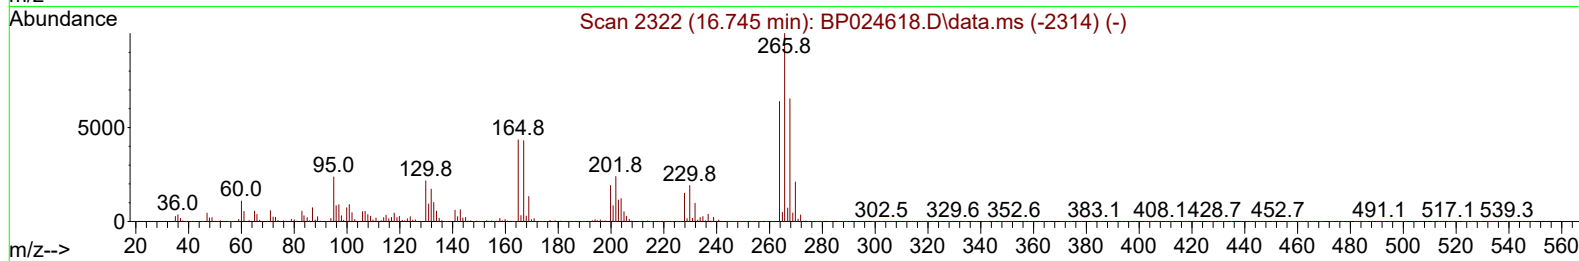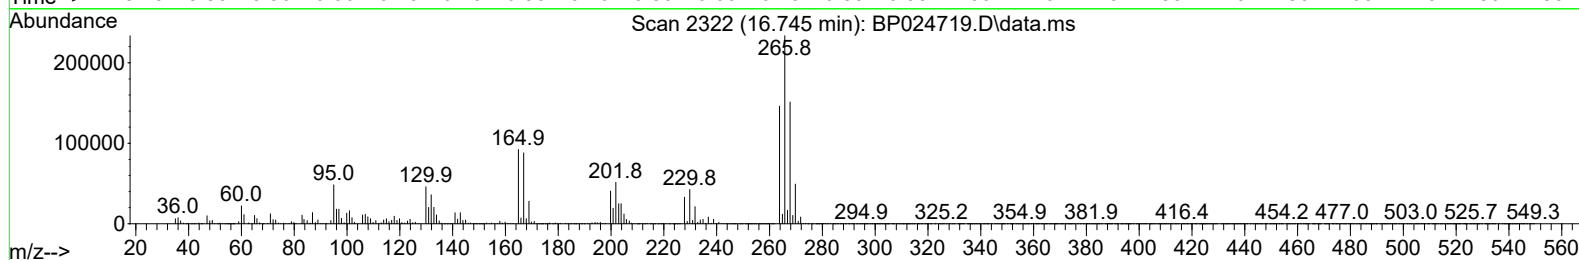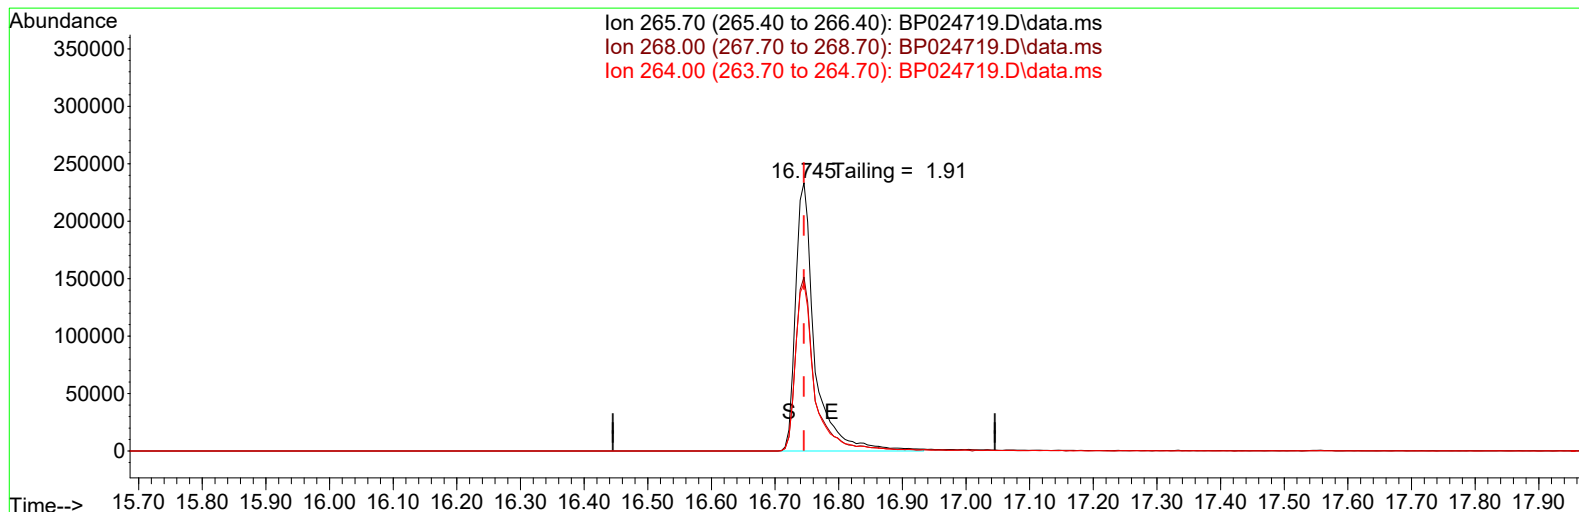

TIC: BP024719.D\data.ms

(70) Pentachlorophenol (C)

16.745min (+ 0.000) 574282.04 ng




response 492342

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.77
264.00	63.90	62.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052025\
Data File : BP024719.D
Acq On : 21 May 2025 00:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 21 02:08:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

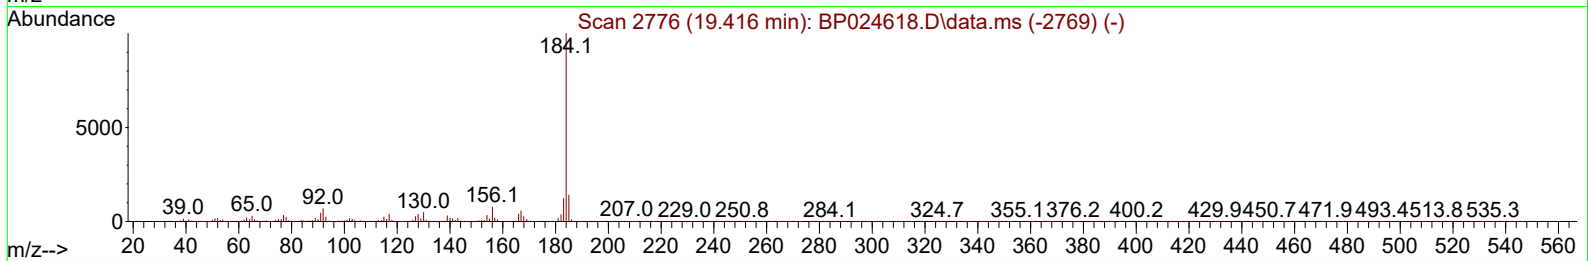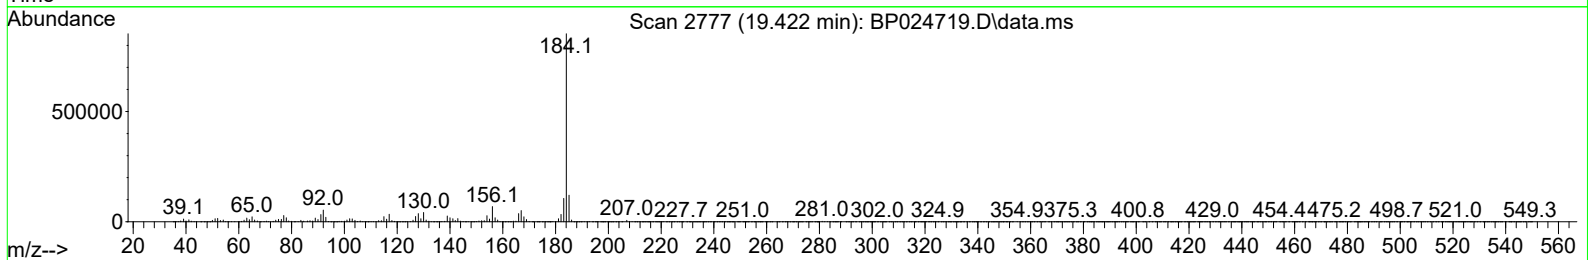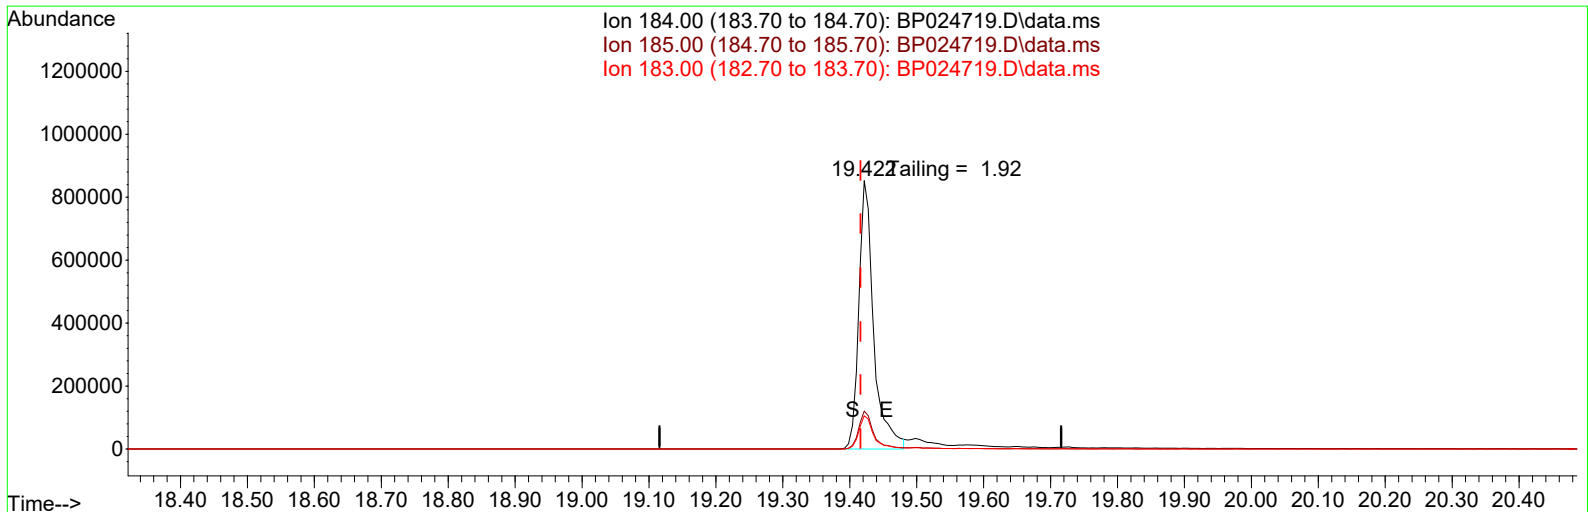

TIC: BP024719.D\data.ms

(77) Benzidine

19.422min (+ 0.006) 97951.15 ng

response 1323225

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.13
183.00	12.30	12.40
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/20/2025	BNA_P	<u>BP024719.D</u>
Compound Name	Response	Retention Time
DDT	647981	20.698
DDD	21430	20.239
DDE	4529	19.722
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25959	673940	3.85

Instrument :
BNA_P
ClientSampleId :
DFTPP