

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052025\
 Data File : BP024723.D
 Acq On : 21 May 2025 02:49
 Operator : RC/JU
 Sample : Q1984-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OU4-PCS-TC-34-050725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024723.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.470	62	65	75	rBV	37338	60119	1.01%	0.224%
2	4.822	289	295	305	rBV	106584	159180	2.67%	0.594%
3	5.287	368	374	391	rBV	1210832	1844416	30.91%	6.880%
4	6.858	634	641	671	rBV	969447	1854114	31.07%	6.916%
5	7.652	768	776	786	rBV	417435	663881	11.13%	2.476%
6	8.805	964	972	993	rBV	745929	1304941	21.87%	4.868%
7	10.422	1239	1247	1263	rBV	483403	930566	15.59%	3.471%
8	11.193	1371	1378	1394	rBV2	23164	79656	1.33%	0.297%
9	12.893	1658	1667	1682	rBV	2085805	3393039	56.86%	12.657%
10	14.281	1895	1903	1923	rBV	799022	1241624	20.81%	4.632%
11	14.516	1934	1943	1952	rBV2	51344	113262	1.90%	0.423%
12	15.804	2155	2162	2182	rBV	1887361	3202754	53.67%	11.947%
13	17.086	2373	2380	2394	rBV	1043268	1573735	26.37%	5.871%
14	18.022	2533	2539	2548	rBV	137190	245178	4.11%	0.915%
15	18.457	2609	2613	2620	rBV	73223	90902	1.52%	0.339%
16	19.351	2761	2765	2778	rBV3	52123	117219	1.96%	0.437%
17	19.804	2836	2842	2854	rBV	3818596	5967371	100.00%	22.260%
18	21.180	3072	3076	3087	rVB2	123172	213880	3.58%	0.798%
19	21.510	3127	3132	3149	rBV	1178074	1853038	31.05%	6.912%
20	24.780	3681	3688	3703	rVB	700030	1898402	31.81%	7.082%




Sum of corrected areas: 26807277

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052025\
Data File : BP024723.D
Acq On : 21 May 2025 02:49
Operator : RC/JU
Sample : Q1984-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-PCS-TC-34-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

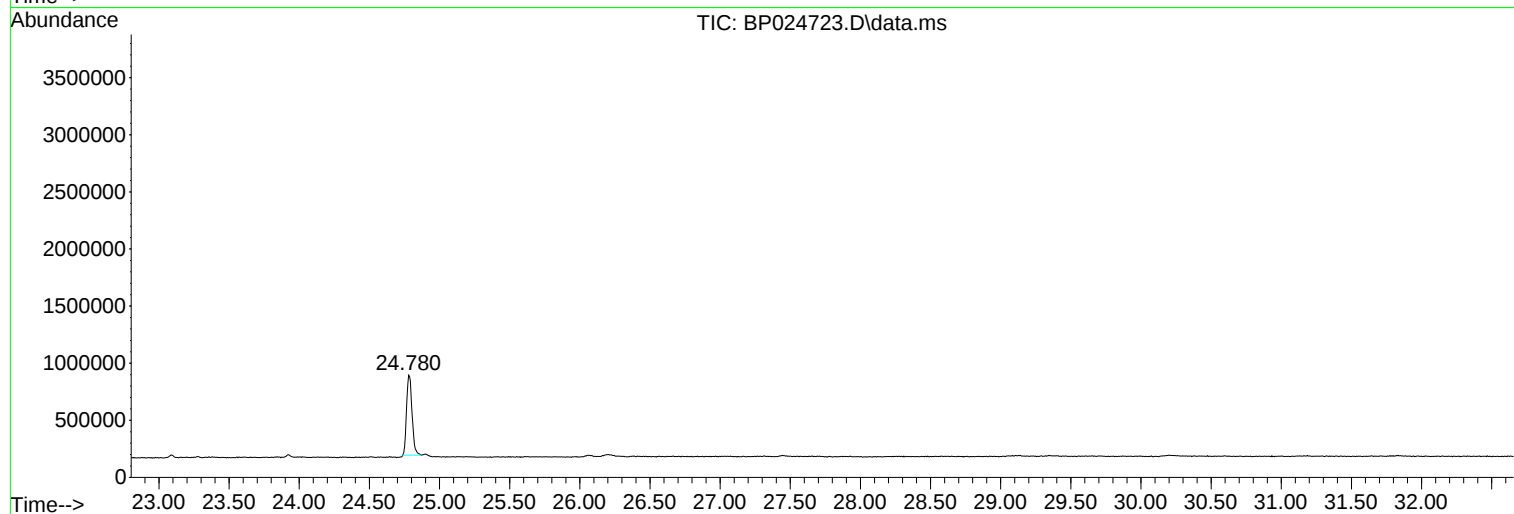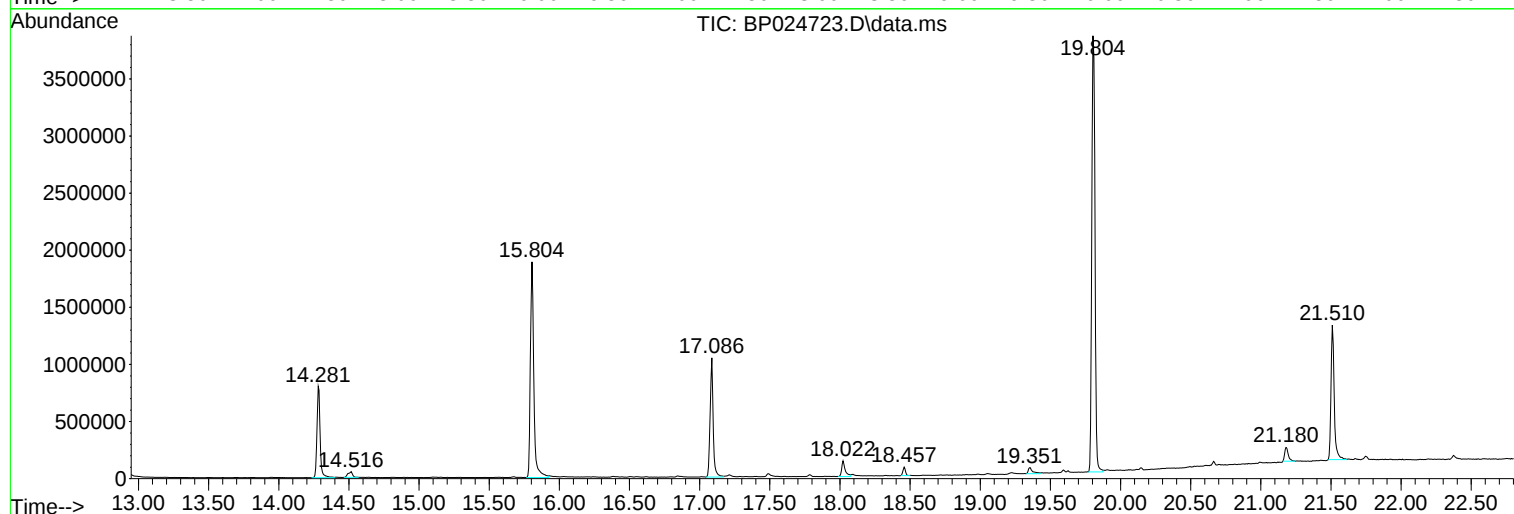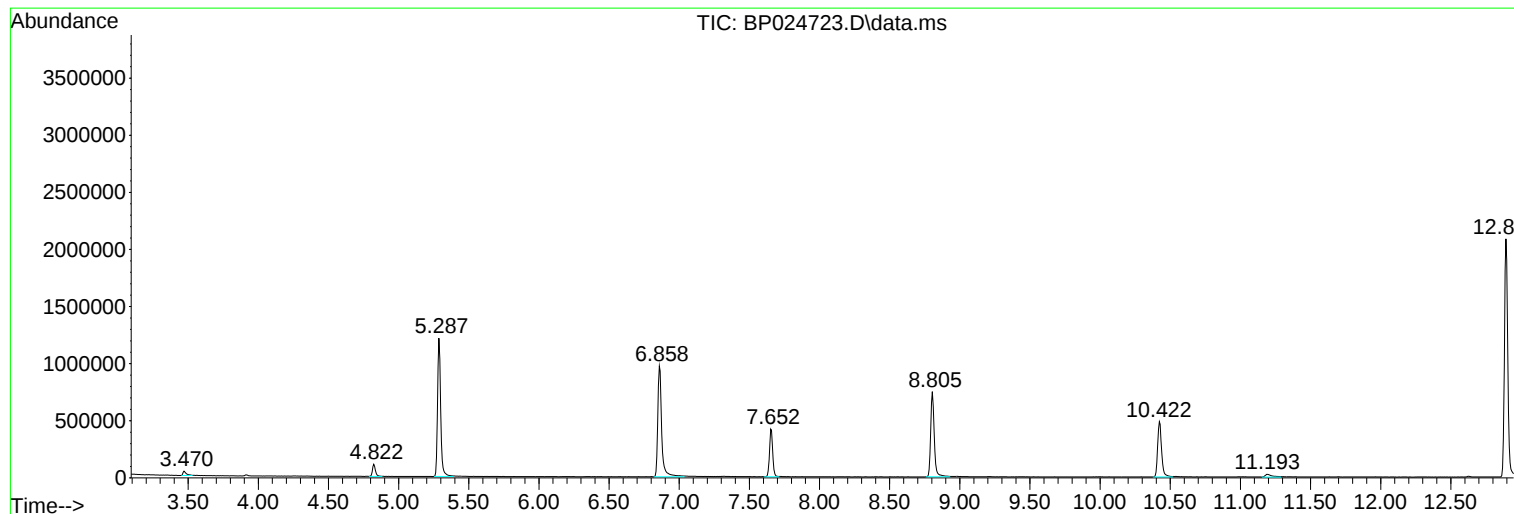

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052025\
Data File : BP024723.D
Acq On : 21 May 2025 02:49
Operator : RC/JU
Sample : Q1984-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-PCS-TC-34-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052025\
Data File : BP024723.D
Acq On : 21 May 2025 02:49
Operator : RC/JU
Sample : Q1984-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-PCS-TC-34-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------