
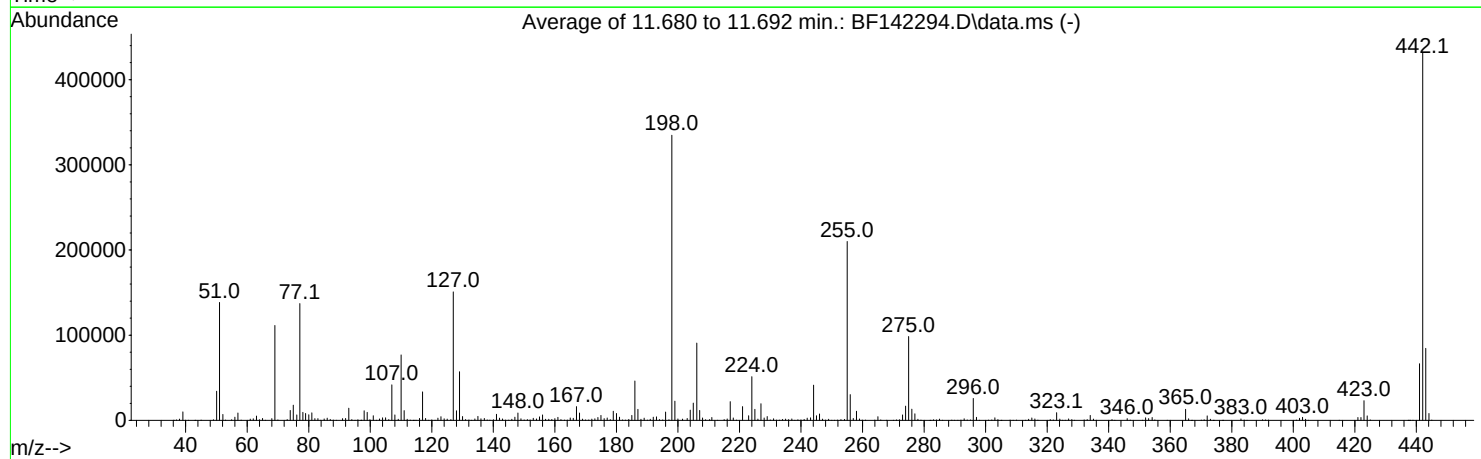


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050525\
Data File : BF142294.D
Acq On : 05 May 2025 13:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 05 18:41:44 2025

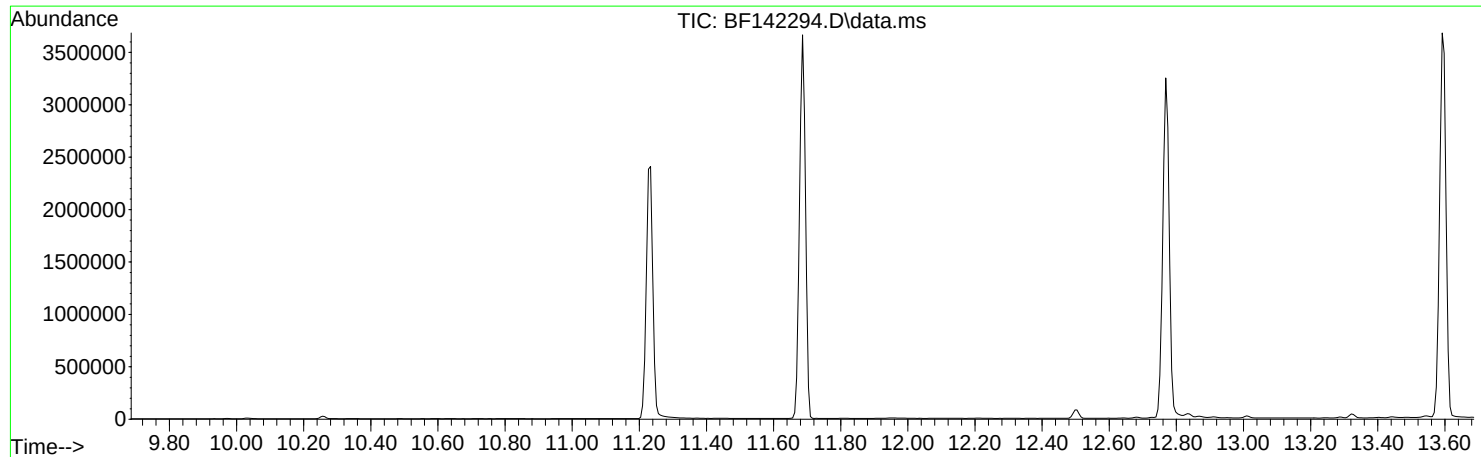

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.3	138422	PASS
68	69	0.00	2	1.8	2002	PASS
69	198	0.00	100	33.3	111451	PASS
70	69	0.00	2	0.5	606	PASS
127	198	10	80	45.1	150915	PASS
197	198	0.00	2	0.2	791	PASS
198	198	100	100	100.0	334827	PASS
199	198	5	9	6.7	22493	PASS
275	198	10	60	29.4	98472	PASS
365	198	1	100	3.9	13004	PASS
441	198	0.01	100	19.9	66483	PASS
442	442	50	100	100.0	431915	PASS
443	442	15	24	19.6	84477	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/5/2025	BNA_F	<u>BF142294.D</u>
Compound Name	Response	Retention Time
DDT	875067	13.592
DDD	9793	13.321
DDE	601	12.957
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10394	885461	1.17

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050525\
Data File : BF142294.D
Acq On : 05 May 2025 13:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 05 15:26:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 15:26:28 2025
Response via : Initial Calibration

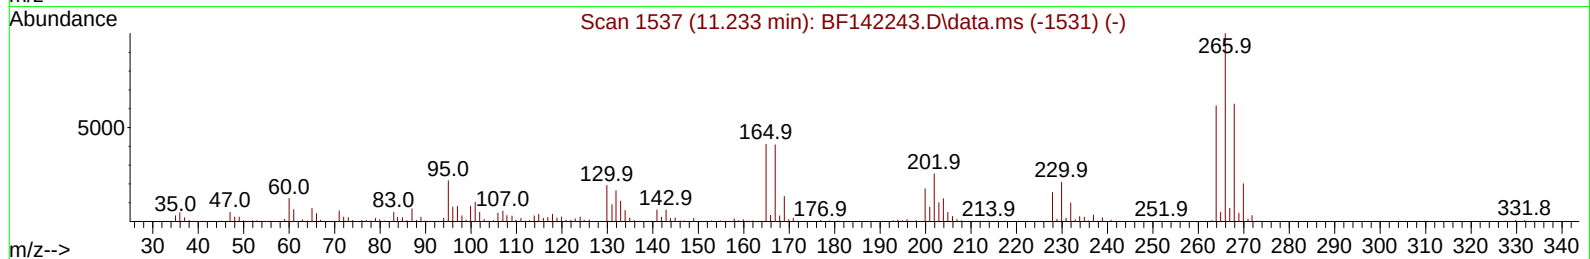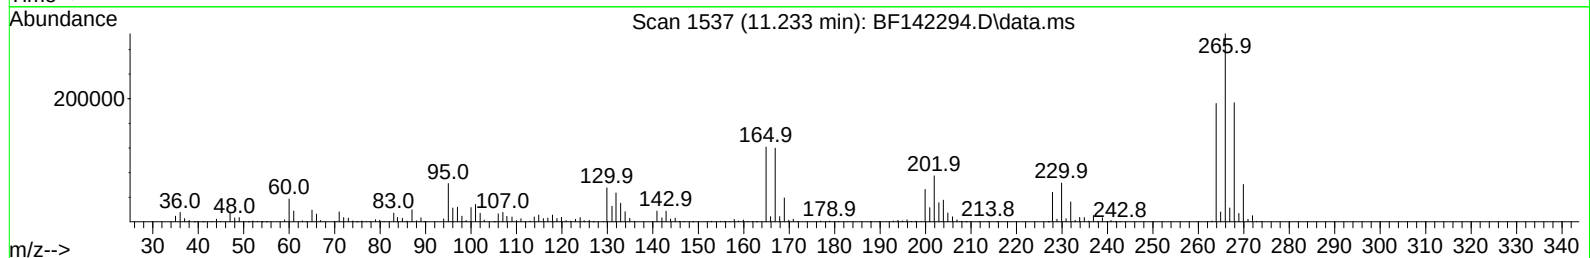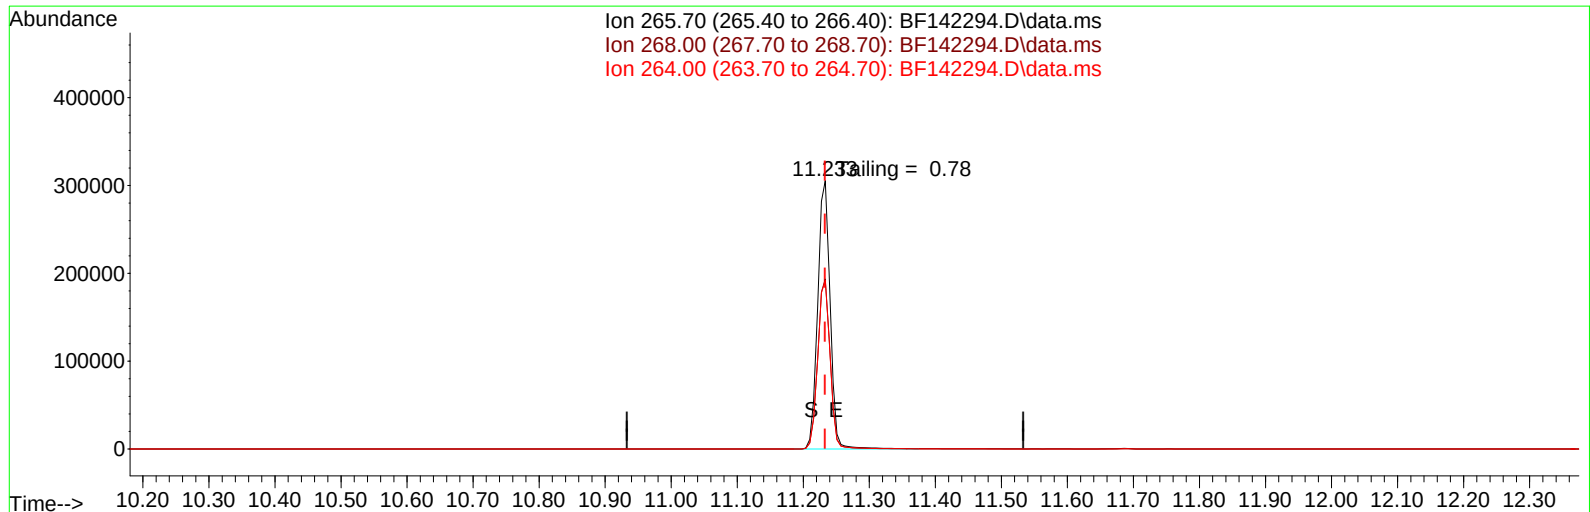

TIC: BF142294.D\data.ms

(70) Pentachlorophenol (C)

11.233min (+ 0.000) 69841.70 ng




response 401301

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	63.35
264.00	61.60	62.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF050525\
Data File : BF142294.D
Acq On : 05 May 2025 13:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 05 15:26:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 15:26:28 2025
Response via : Initial Calibration

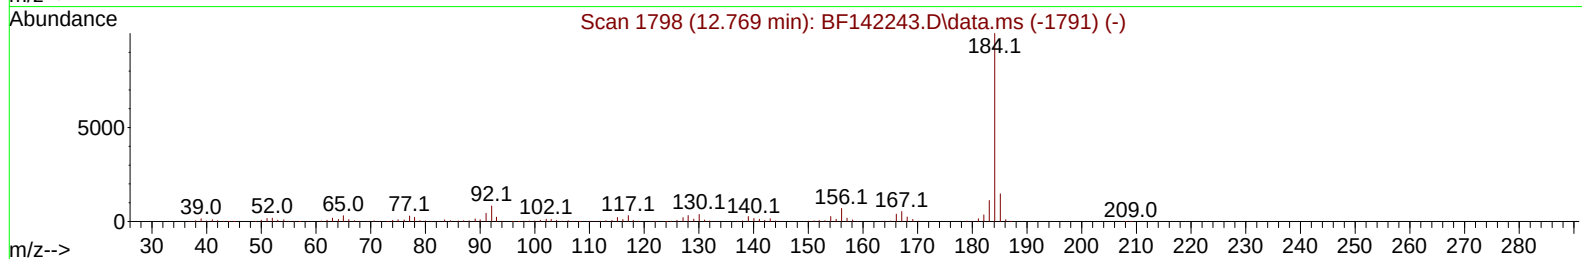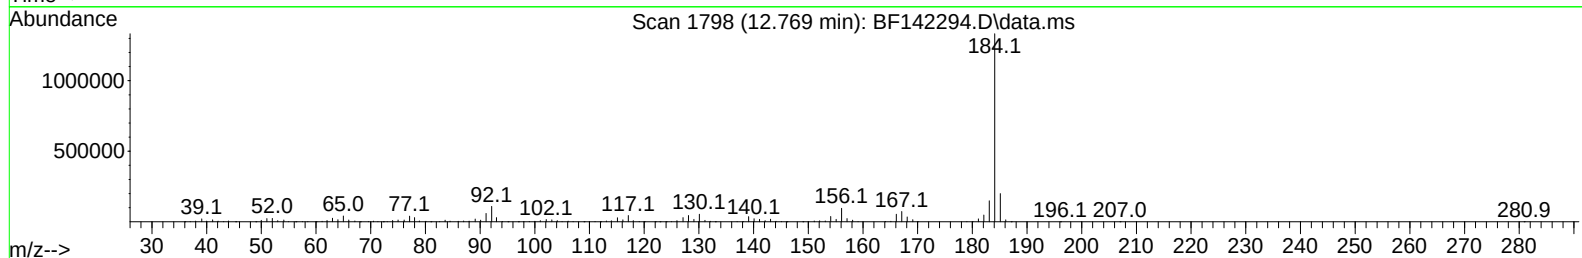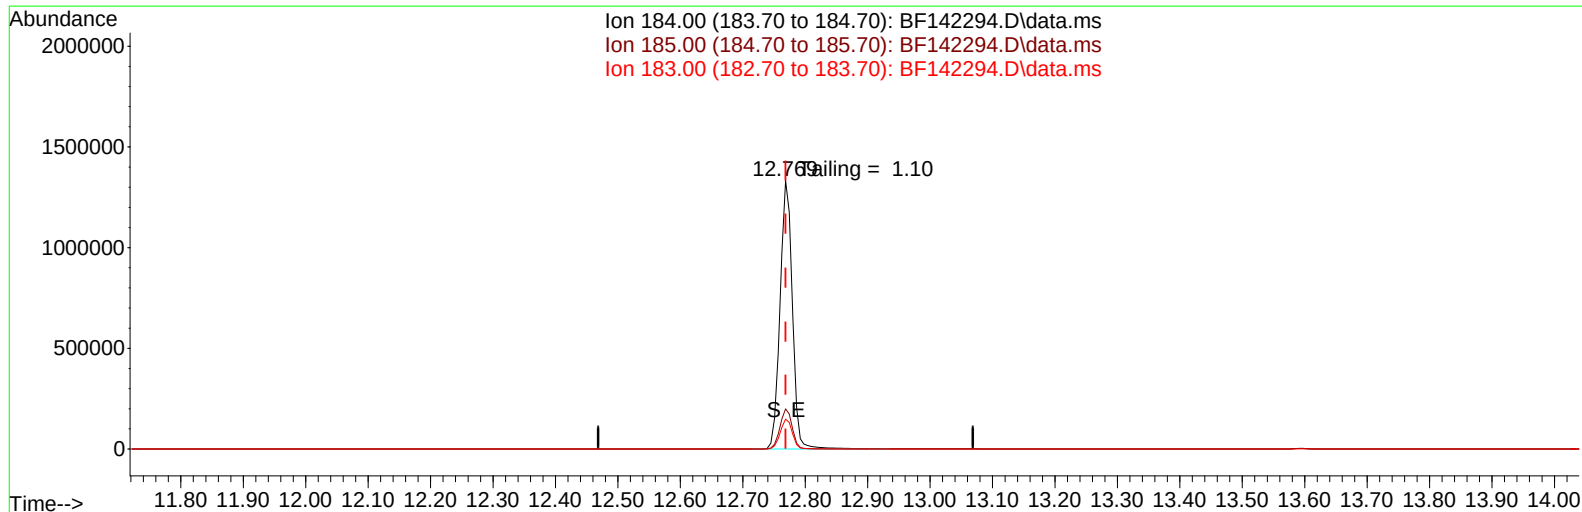

TIC: BF142294.D\data.ms

(77) Benzidine

12.769min (-0.000) 69201.02 ng

response 1834842

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.01
183.00	11.10	11.15
0.00	0.00	0.00