
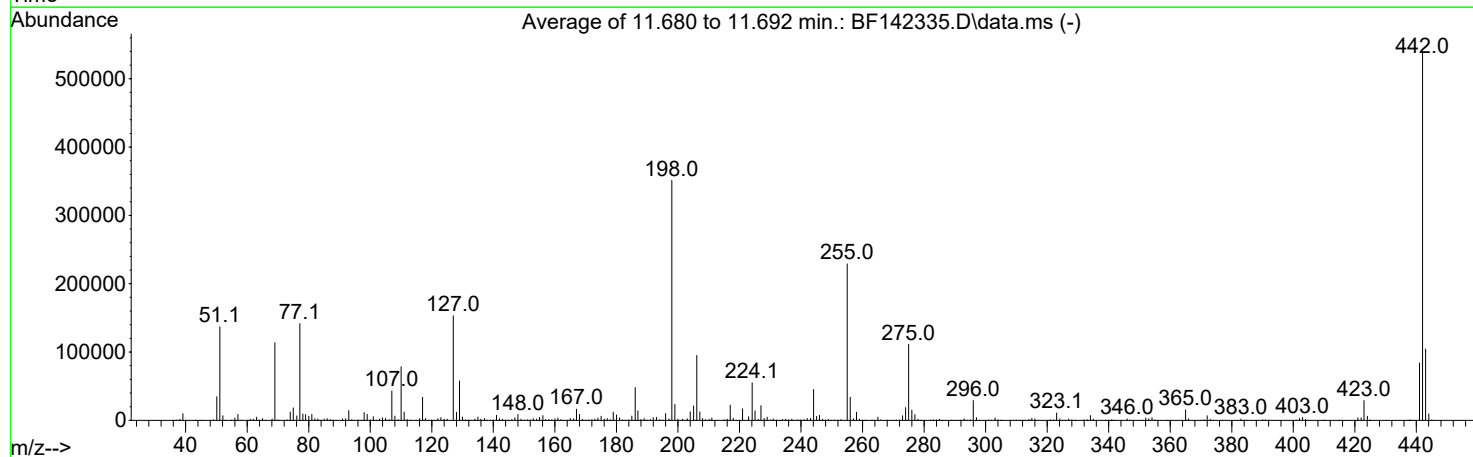


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051325\
Data File : BF142335.D
Acq On : 13 May 2025 10:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 05 18:41:44 2025

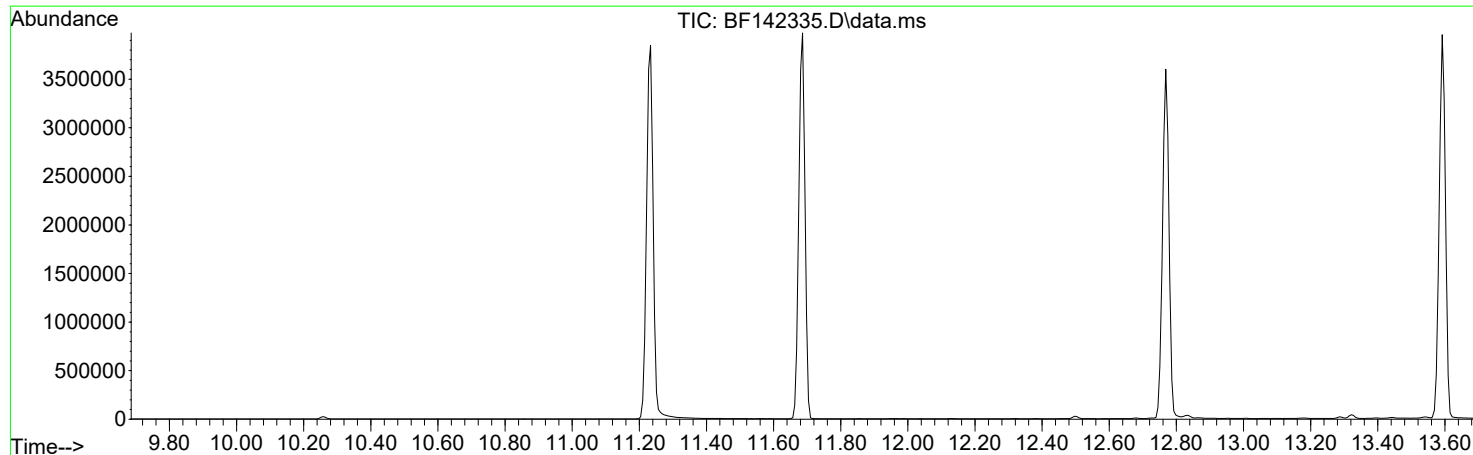

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	137011	PASS
68	69	0.00	2	1.9	2133	PASS
69	198	0.00	100	32.4	113659	PASS
70	69	0.00	2	0.6	668	PASS
127	198	10	80	43.6	153267	PASS
197	198	0.00	2	0.6	2125	PASS
198	198	100	100	100.0	351232	PASS
199	198	5	9	6.7	23472	PASS
275	198	10	60	31.7	111221	PASS
365	198	1	100	4.4	15525	PASS
441	198	0.01	100	23.9	83896	PASS
442	442	50	100	100.0	538432	PASS
443	442	15	24	19.4	104517	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/13/2025	BNA_F	<u>BF142335.D</u>
Compound Name	Response	Retention Time
DDT	977951	13.592
DDD	13135	13.322
DDE	606	12.957
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13741	991692	1.39

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051325\
Data File : BF142335.D
Acq On : 13 May 2025 10:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 13 11:35:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 18:41:44 2025
Response via : Initial Calibration

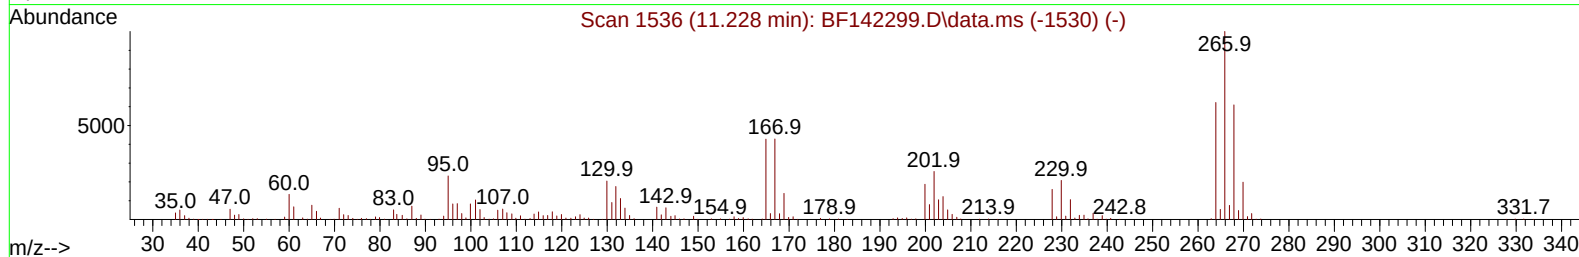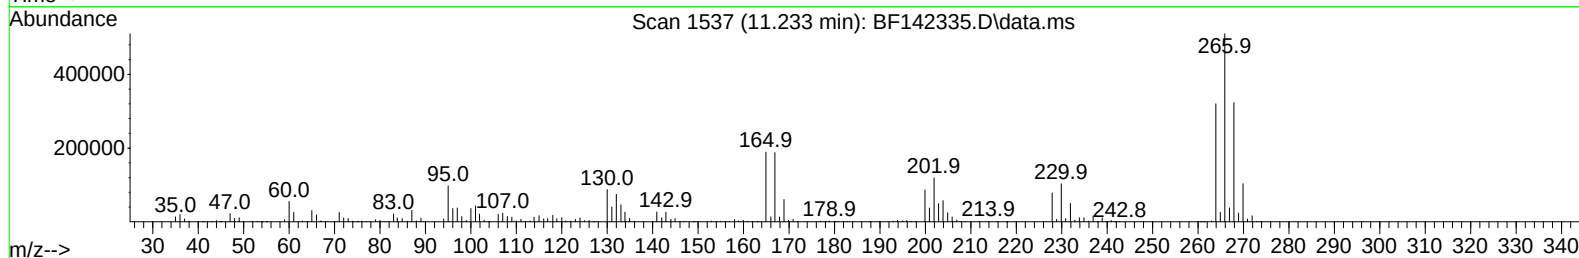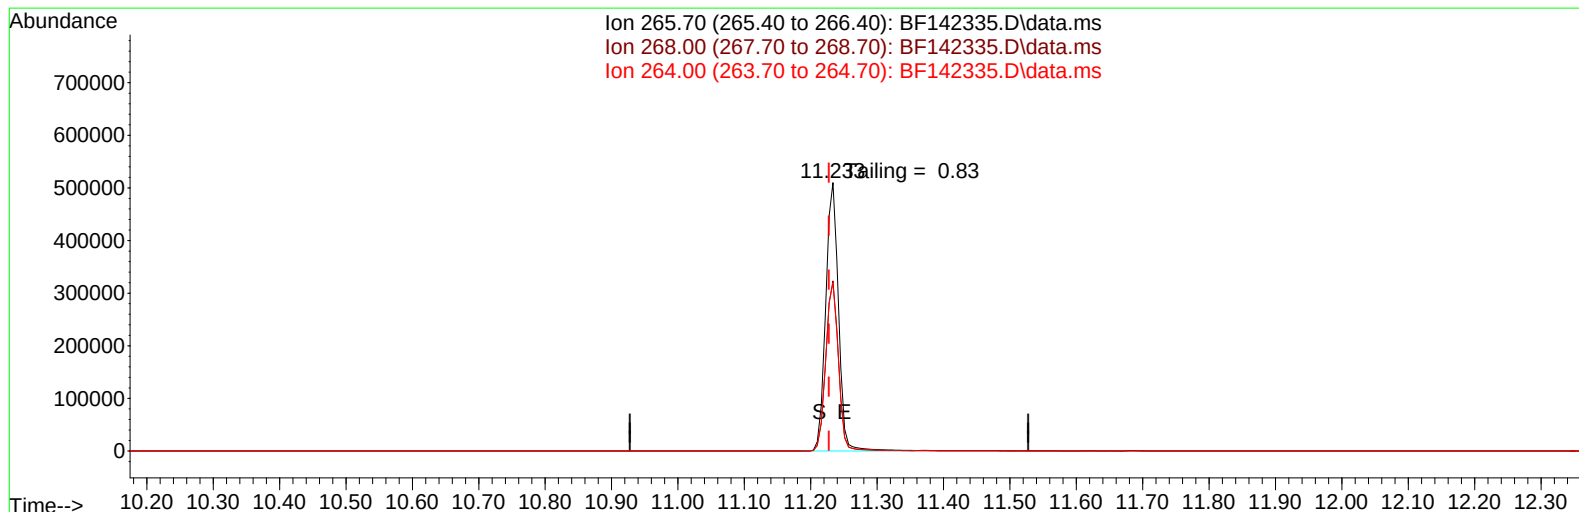

TIC: BF142335.D\data.ms

(70) Pentachlorophenol (C)

11.233min (+ 0.006) 828247.03 ng




response 684411

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.90	63.40
264.00	62.20	62.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051325\
Data File : BF142335.D
Acq On : 13 May 2025 10:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 13 11:35:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 18:41:44 2025
Response via : Initial Calibration

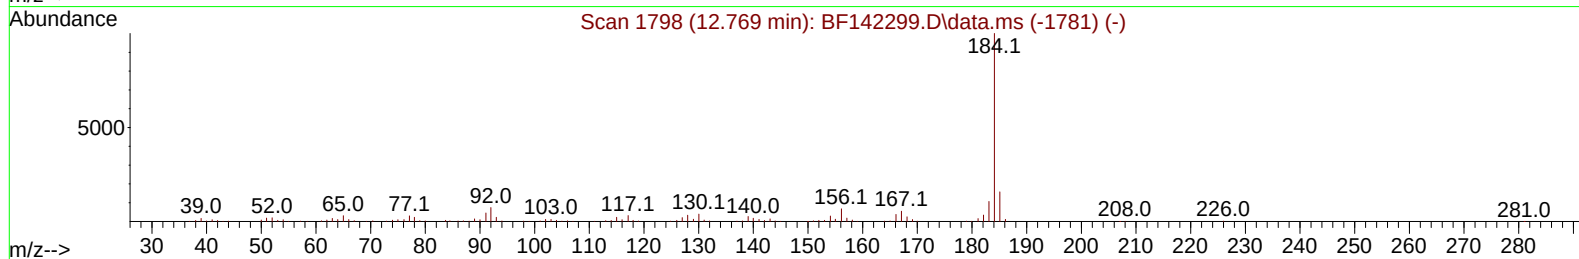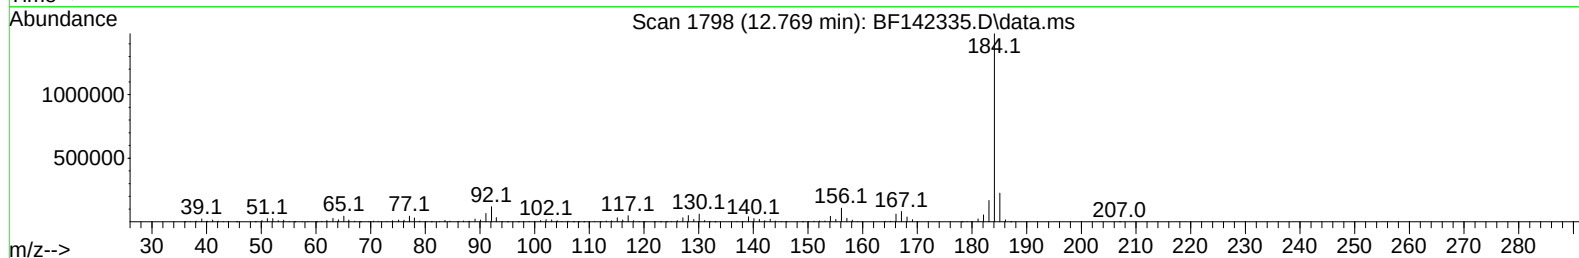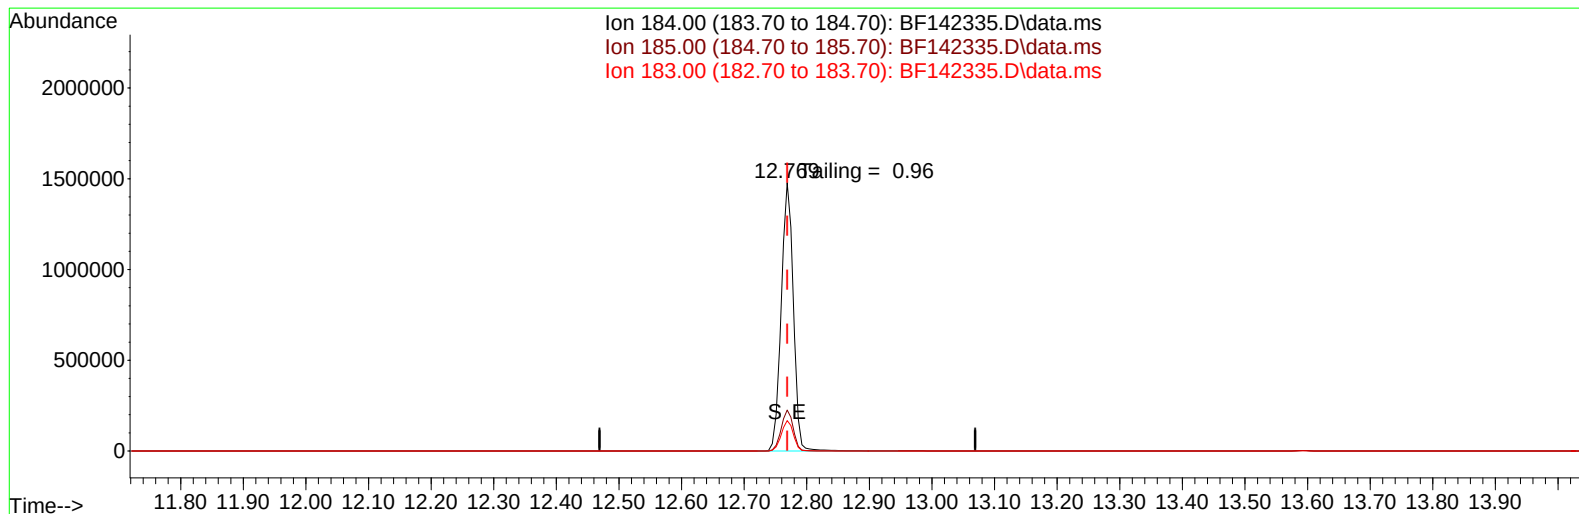

TIC: BF142335.D\data.ms

(77) Benzidine

12.769min (-0.000) 1007757.80 ng

response 1996205

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	15.25
183.00	10.70	11.33
0.00	0.00	0.00