
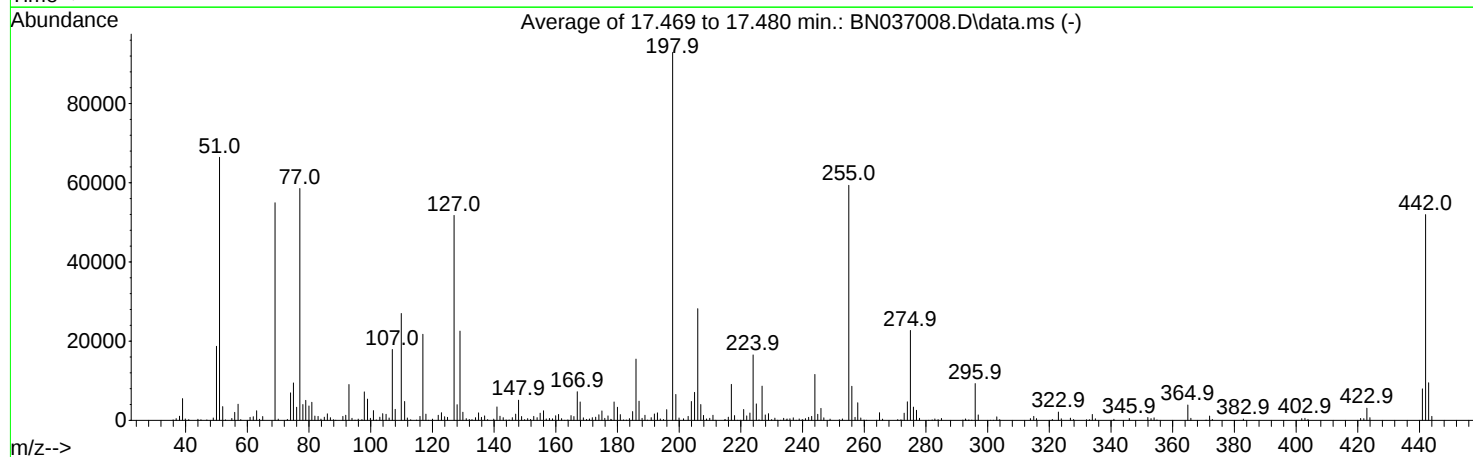


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051425\
Data File : BN037008.D
Acq On : 14 May 2025 09:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 14 11:26:32 2025

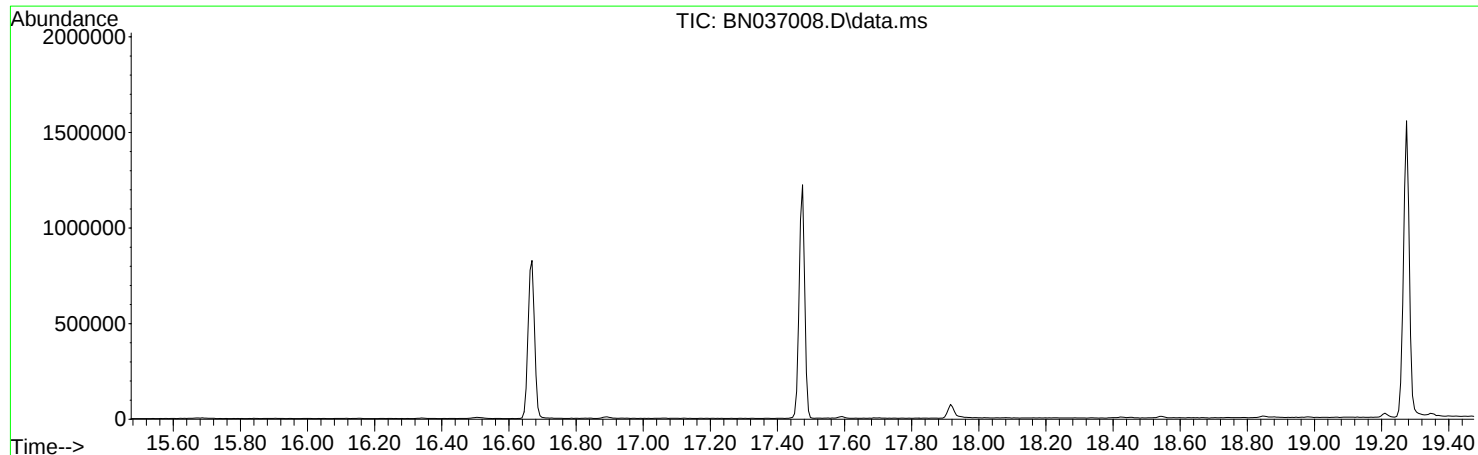

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	71.5	66416	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	59.2	54957	PASS
70	69	0.00	2	0.6	338	PASS
127	198	10	80	55.7	51752	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	92899	PASS
199	198	5	9	7.0	6530	PASS
275	198	10	60	24.4	22707	PASS
365	198	1	100	4.2	3903	PASS
441	198	0.01	100	8.6	7967	PASS
442	442	50	100	100.0	51981	PASS
443	442	15	24	18.3	9515	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/14/2025	BNA_N	<u>BN037008.D</u>
Compound Name	Response	Retention Time
DDT	330267	20.516
DDD	11810	20.074
DDE	264	19.569
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12074	342341	3.53

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051425\
Data File : BN037008.D
Acq On : 14 May 2025 09:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 14 13:52:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 14 01:22:17 2025
Response via : Initial Calibration

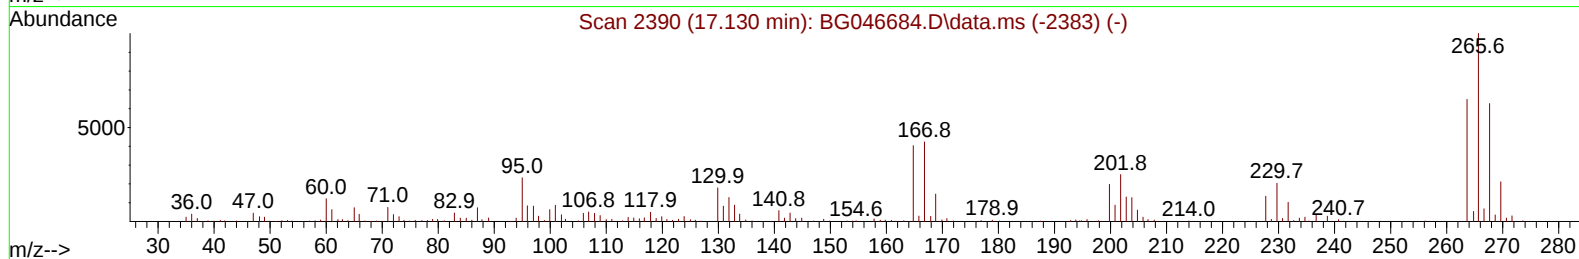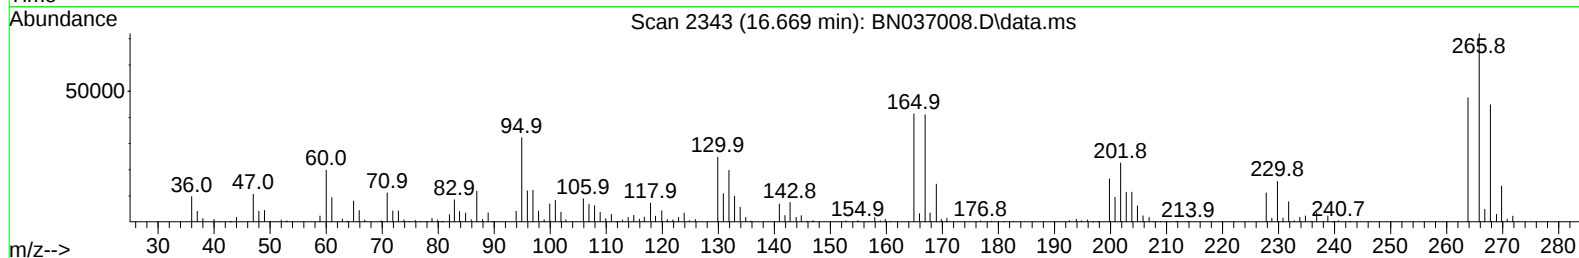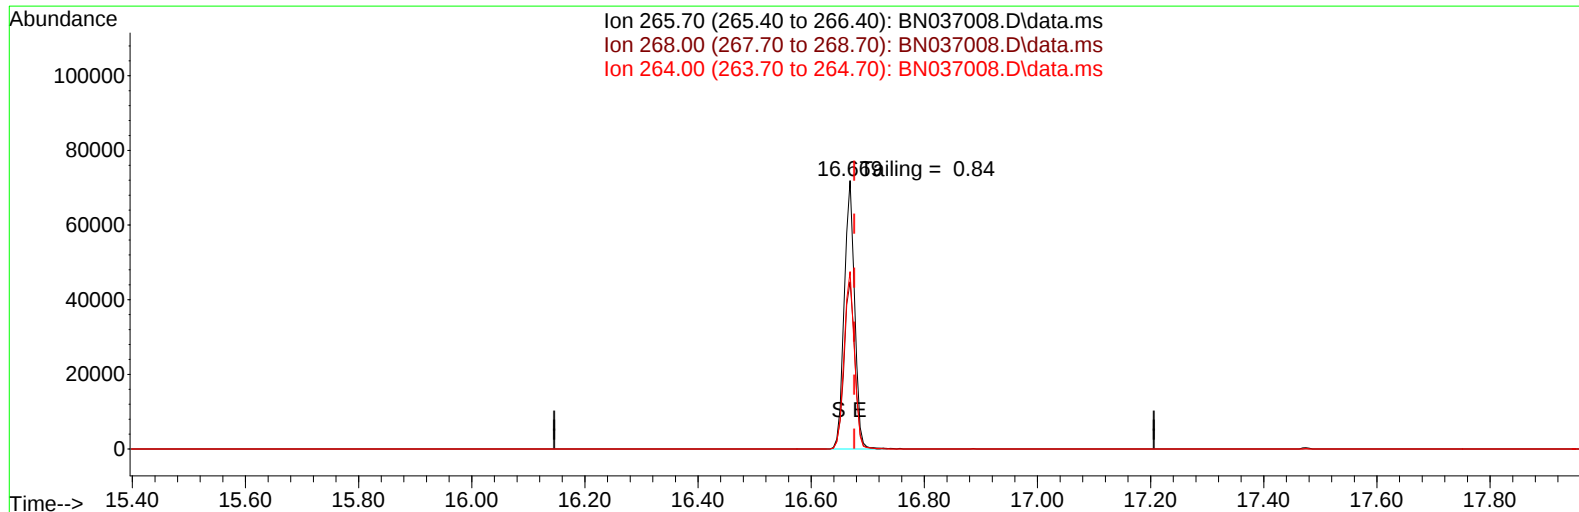

TIC: BN037008.D\data.ms

(70) Pentachlorophenol (C)

16.669min (-0.007) 17871.17 ng




response 91442

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.31
264.00	61.60	66.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051425\
Data File : BN037008.D
Acq On : 14 May 2025 09:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 14 13:52:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 14 01:22:17 2025
Response via : Initial Calibration

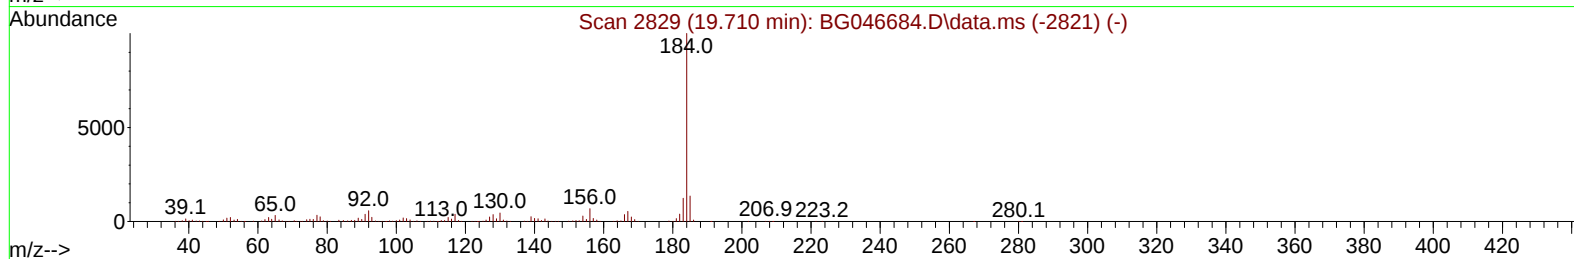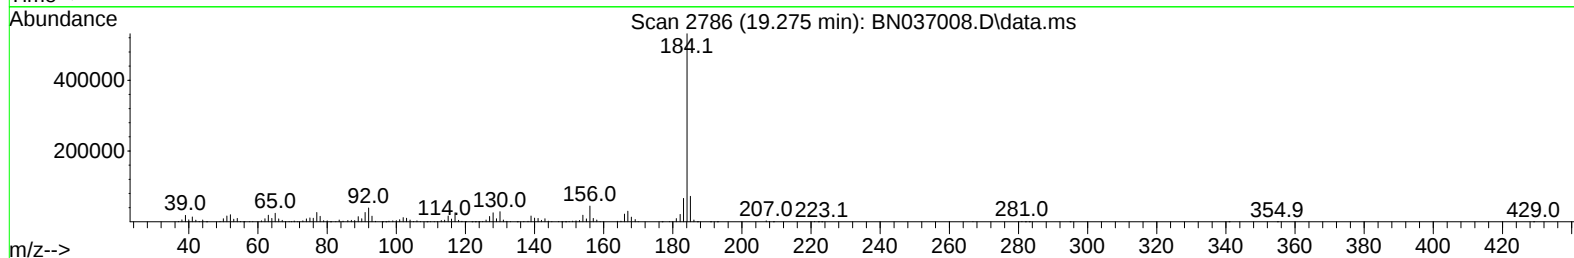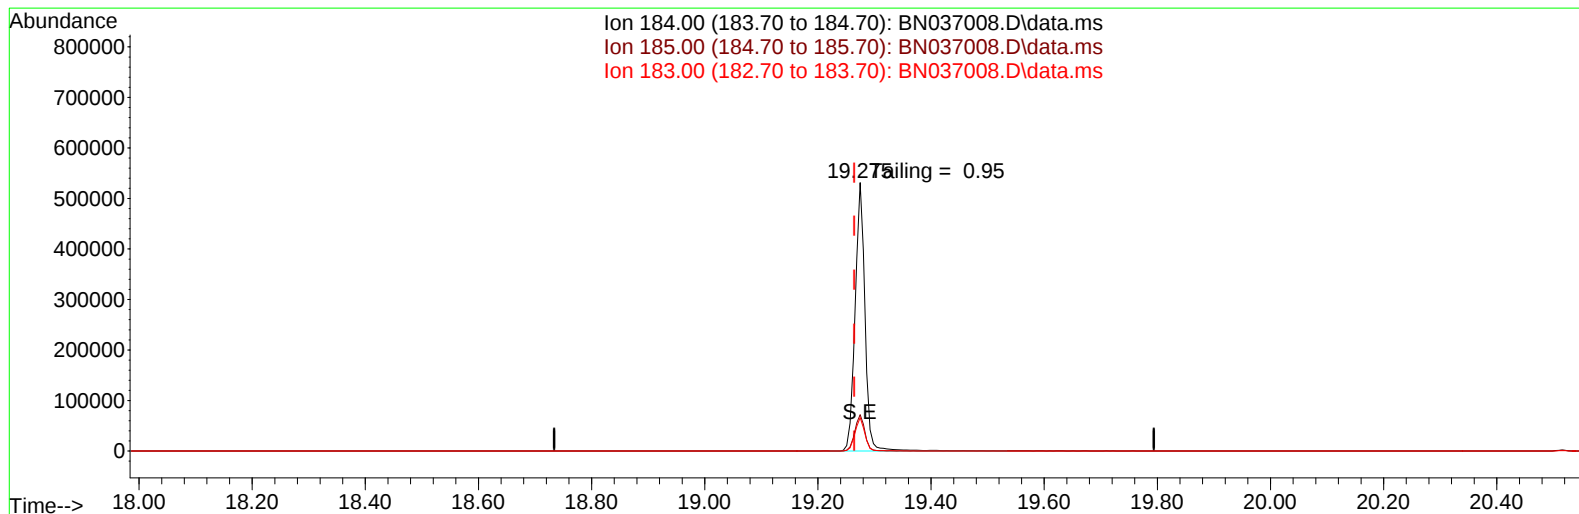

TIC: BN037008.D\data.ms

(77) Benzidine

19.275min (+ 0.010) 0.00 ng

response 642035

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.53
183.00	13.20	12.49
0.00	0.00	0.00