
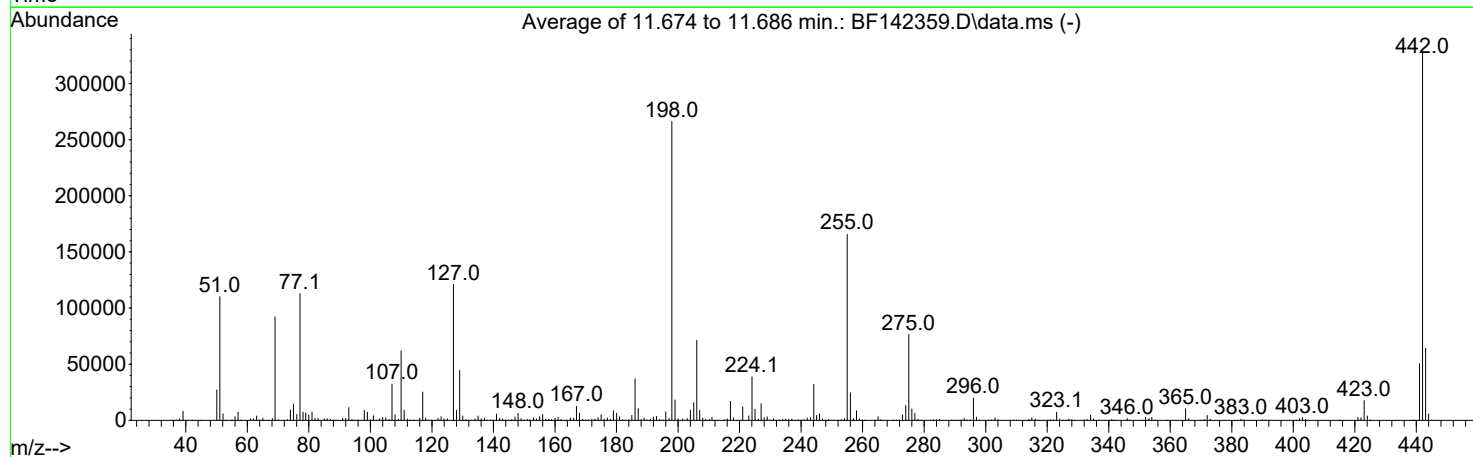


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051425\
Data File : BF142359.D
Acq On : 14 May 2025 11:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 05 18:41:44 2025

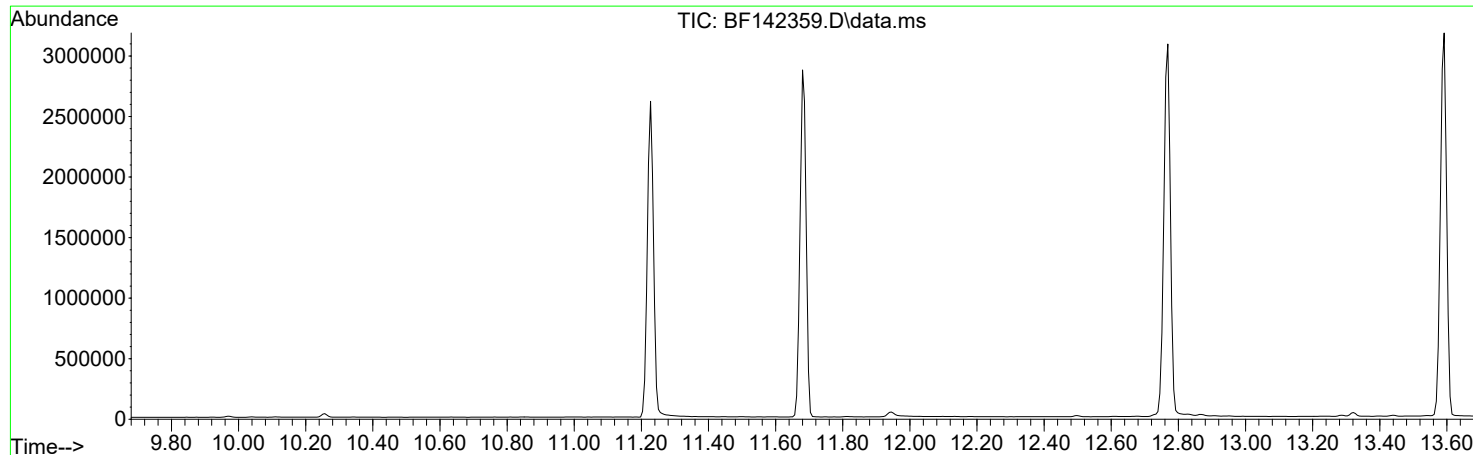

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	110185	PASS
68	69	0.00	2	1.8	1667	PASS
69	198	0.00	100	34.6	92128	PASS
70	69	0.00	2	0.5	480	PASS
127	198	10	80	45.5	121075	PASS
197	198	0.00	2	0.7	1788	PASS
198	198	100	100	100.0	266176	PASS
199	198	5	9	6.8	18073	PASS
275	198	10	60	28.7	76357	PASS
365	198	1	100	3.9	10304	PASS
441	198	0.01	100	19.0	50461	PASS
442	442	50	100	100.0	327595	PASS
443	442	15	24	19.6	64315	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/14/2025	BNA_F	<u>BF142359.D</u>
Compound Name	Response	Retention Time
DDT	815887	13.592
DDD	10078	13.321
DDE	683	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10761	826648	1.30

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051425\
Data File : BF142359.D
Acq On : 14 May 2025 11:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 14 12:47:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 18:41:44 2025
Response via : Initial Calibration

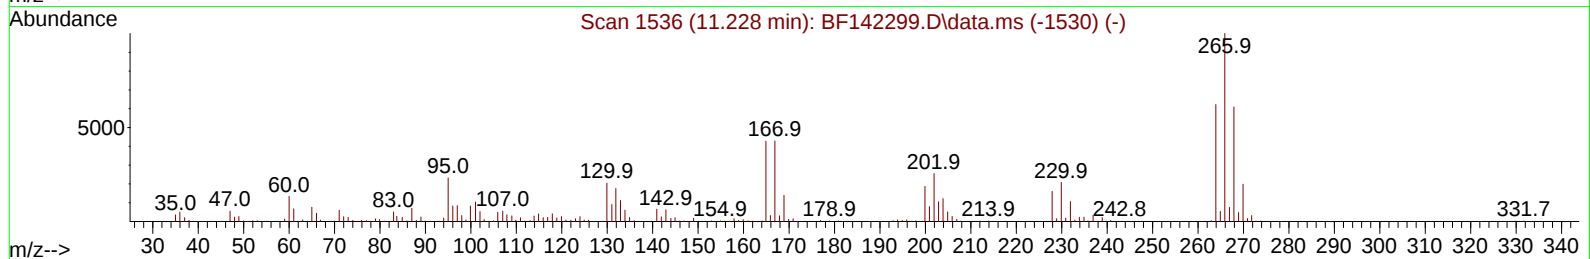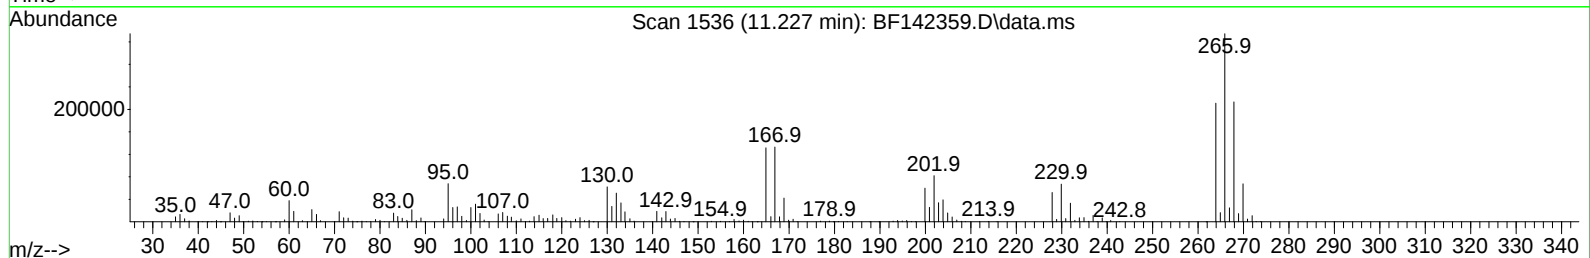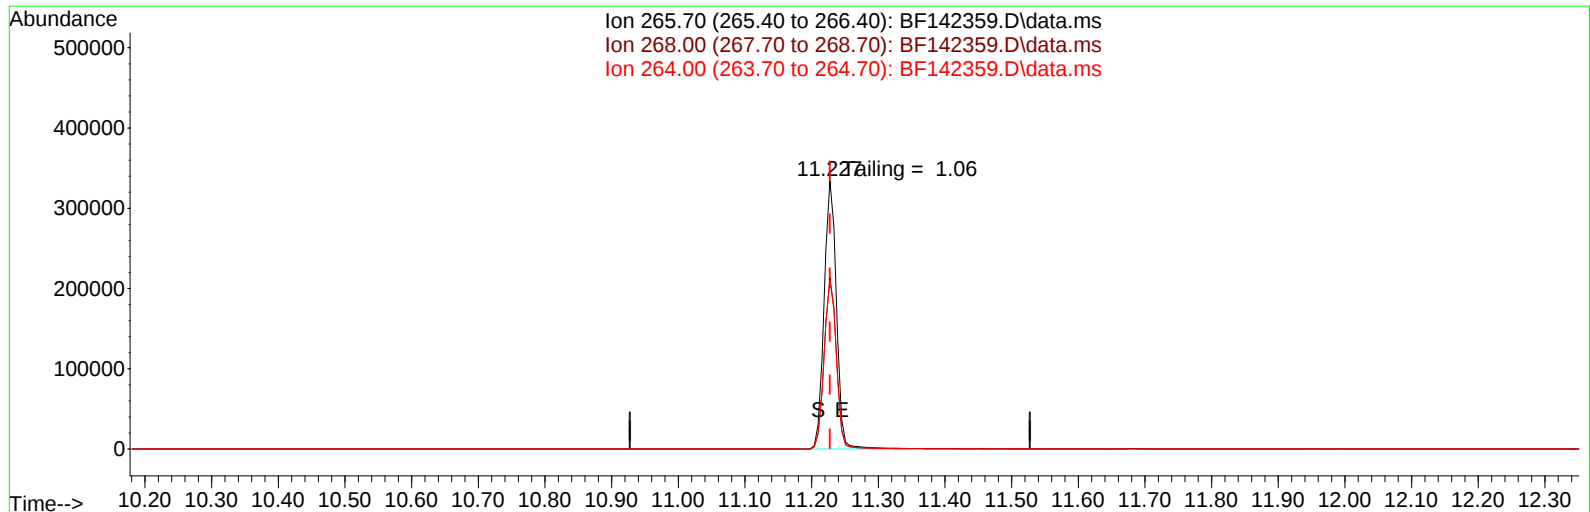

TIC: BF142359.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.000) 177289.14 ng




response 430200

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.90	63.74
264.00	62.20	63.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051425\
Data File : BF142359.D
Acq On : 14 May 2025 11:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 14 12:47:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 18:41:44 2025
Response via : Initial Calibration

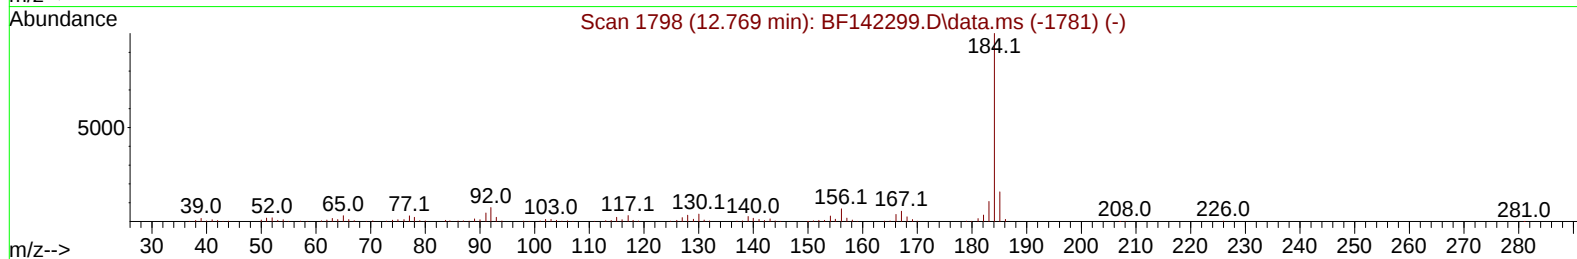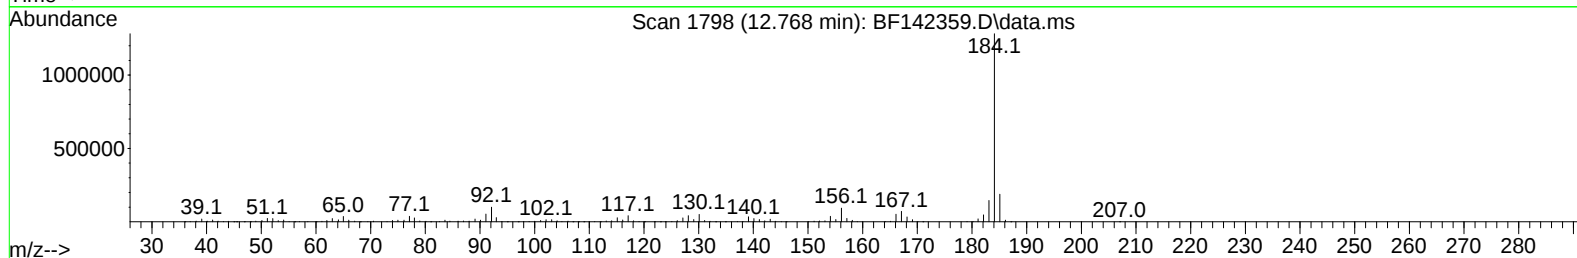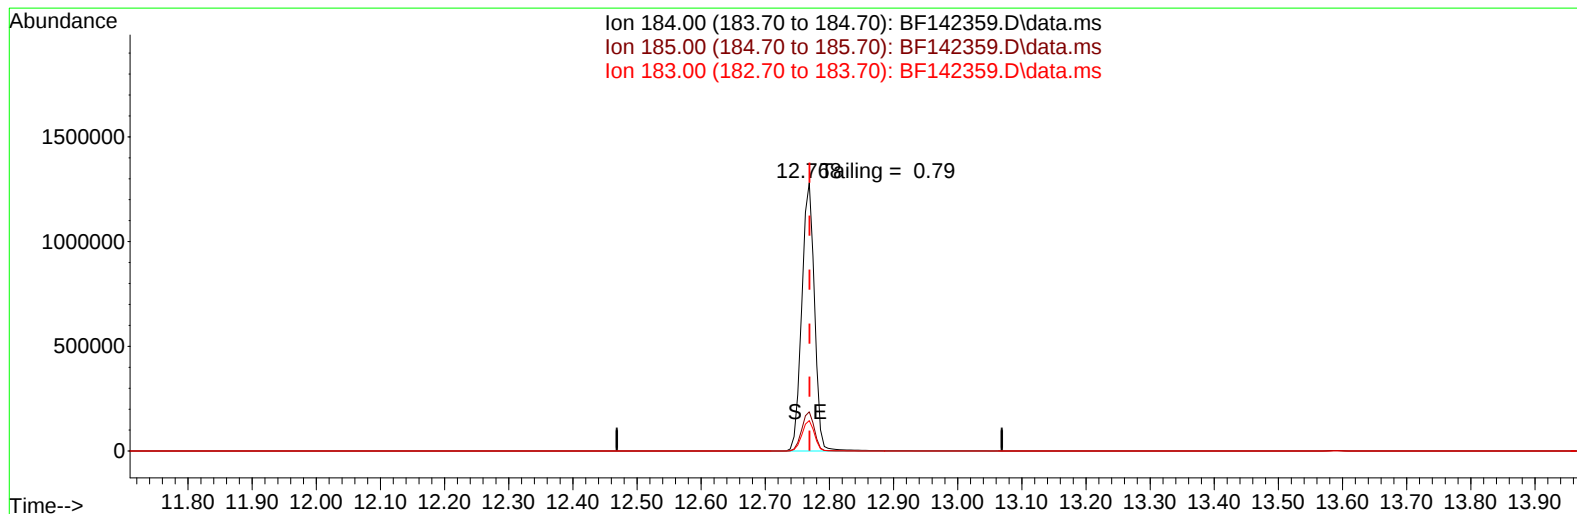

TIC: BF142359.D\data.ms

(77) Benzidine

12.768min (-0.001) 344992.34 ng

response 1767995

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.65
183.00	10.70	11.35
0.00	0.00	0.00