
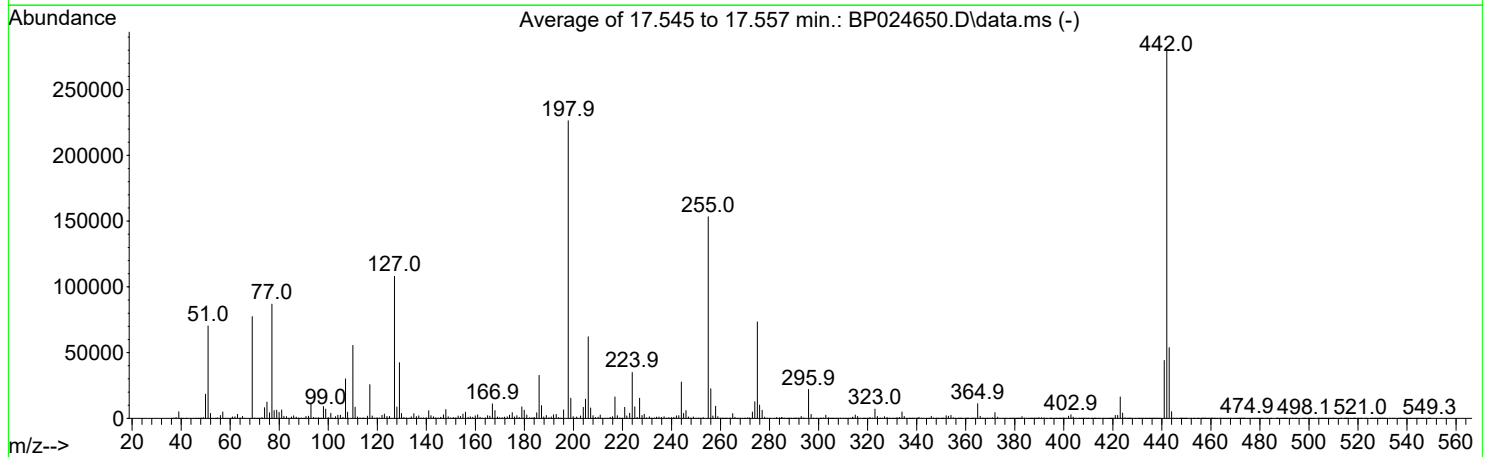


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051625\
Data File : BP024650.D
Acq On : 16 May 2025 10:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 13 16:21:39 2025

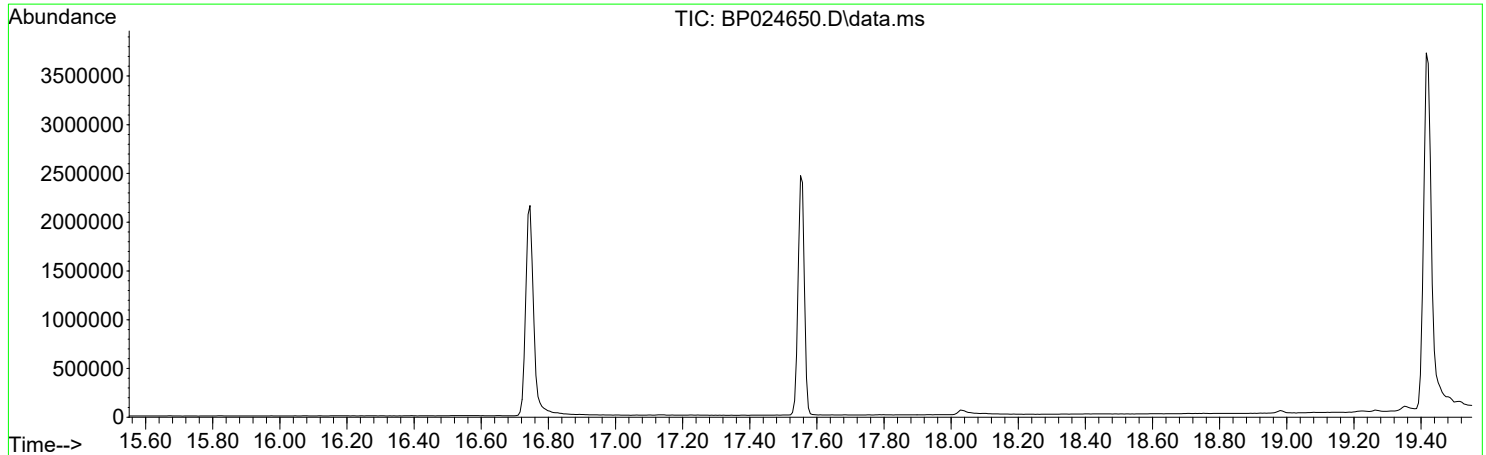

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.1	70396	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.2	77409	PASS
70	69	0.00	2	0.5	369	PASS
127	198	10	80	47.7	108031	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	226304	PASS
199	198	5	9	6.8	15346	PASS
275	198	10	60	32.4	73333	PASS
365	198	1	100	5.0	11247	PASS
441	198	0.01	100	19.5	44040	PASS
442	442	100	100	100.0	279744	PASS
443	442	15	24	19.2	53844	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/16/2025	BNA_P	<u>BP024650.D</u>
Compound Name	Response	Retention Time
DDT	891212	20.704
DDD	17896	20.251
DDE	477	19.804
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18373	909585	2.02

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051625\
Data File : BP024650.D
Acq On : 16 May 2025 10:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 16 11:41:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

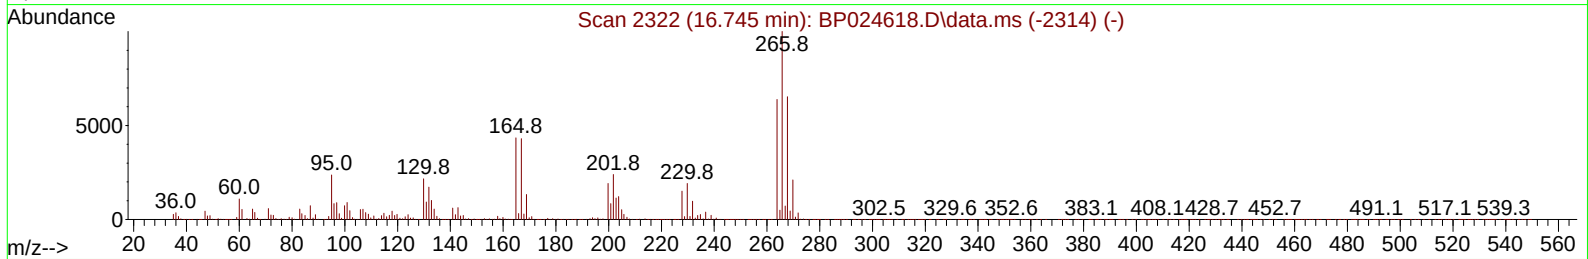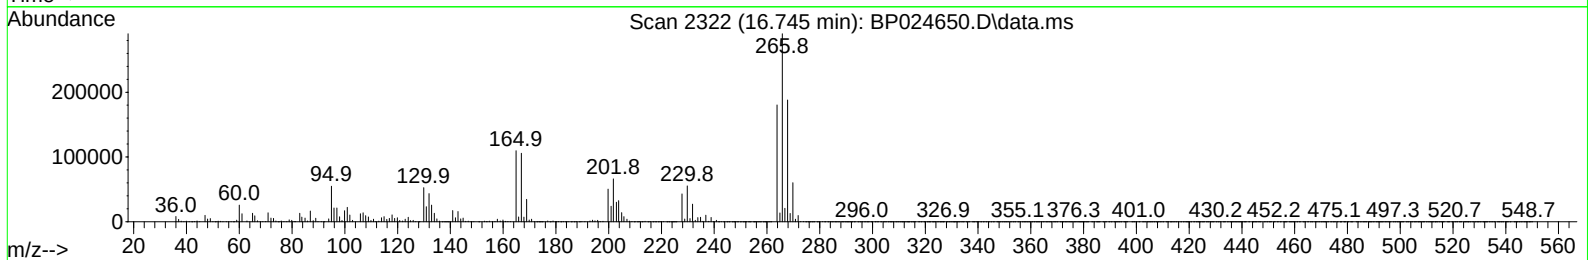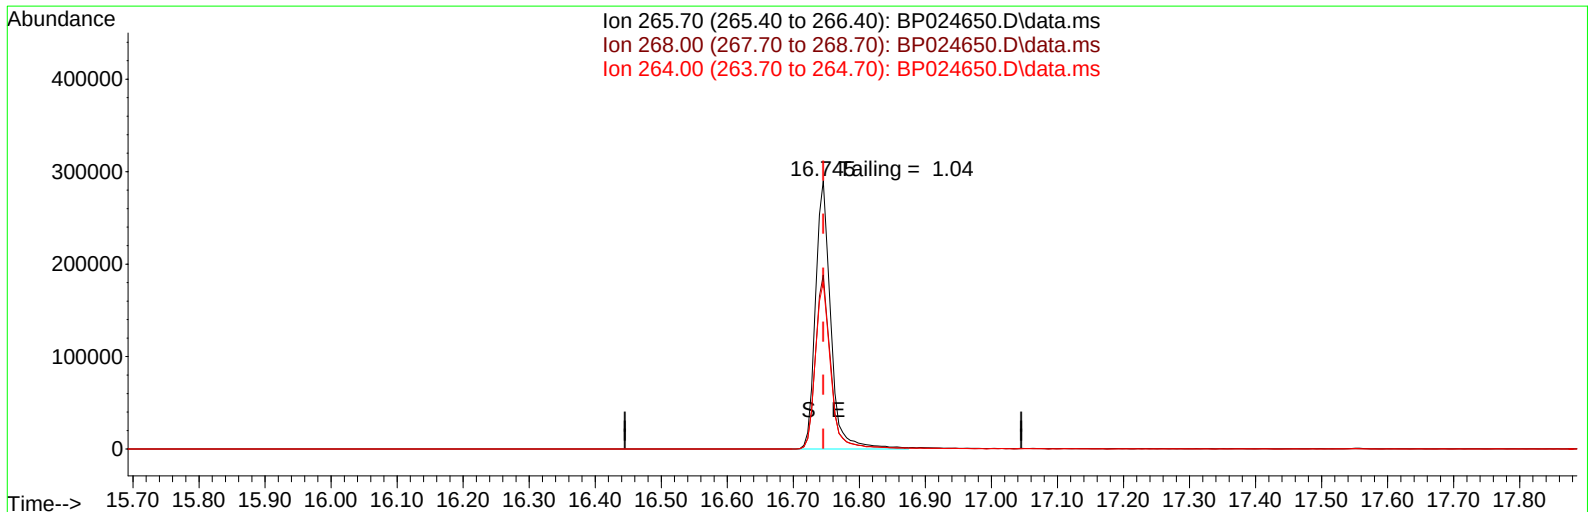

TIC: BP024650.D\data.ms

(70) Pentachlorophenol (C)

16.745min (+ 0.000) 55883.60 ng




response 469236

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.79
264.00	63.90	62.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051625\
Data File : BP024650.D
Acq On : 16 May 2025 10:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 16 11:41:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

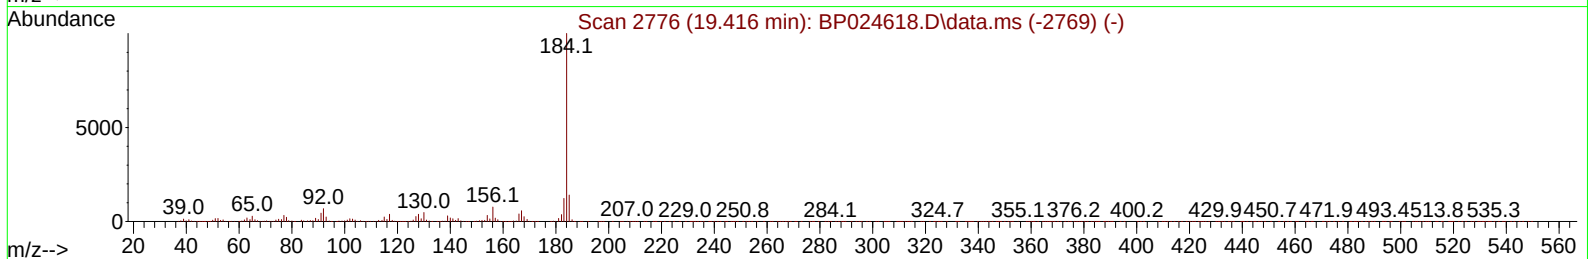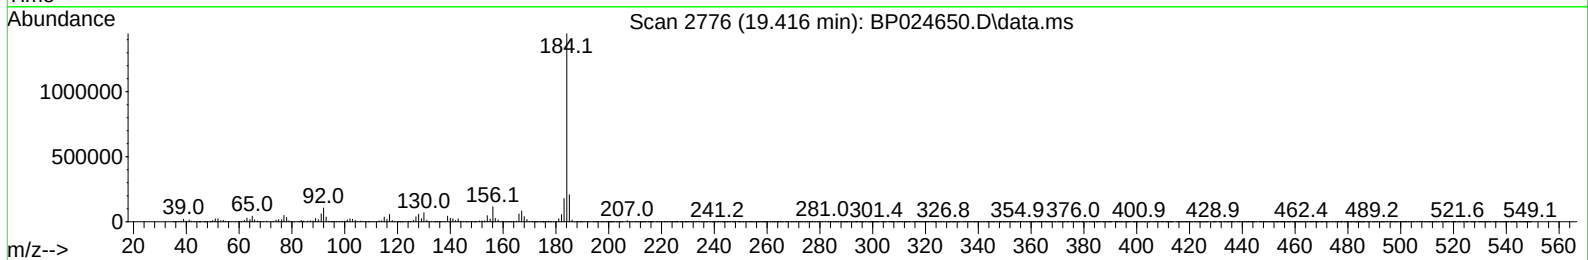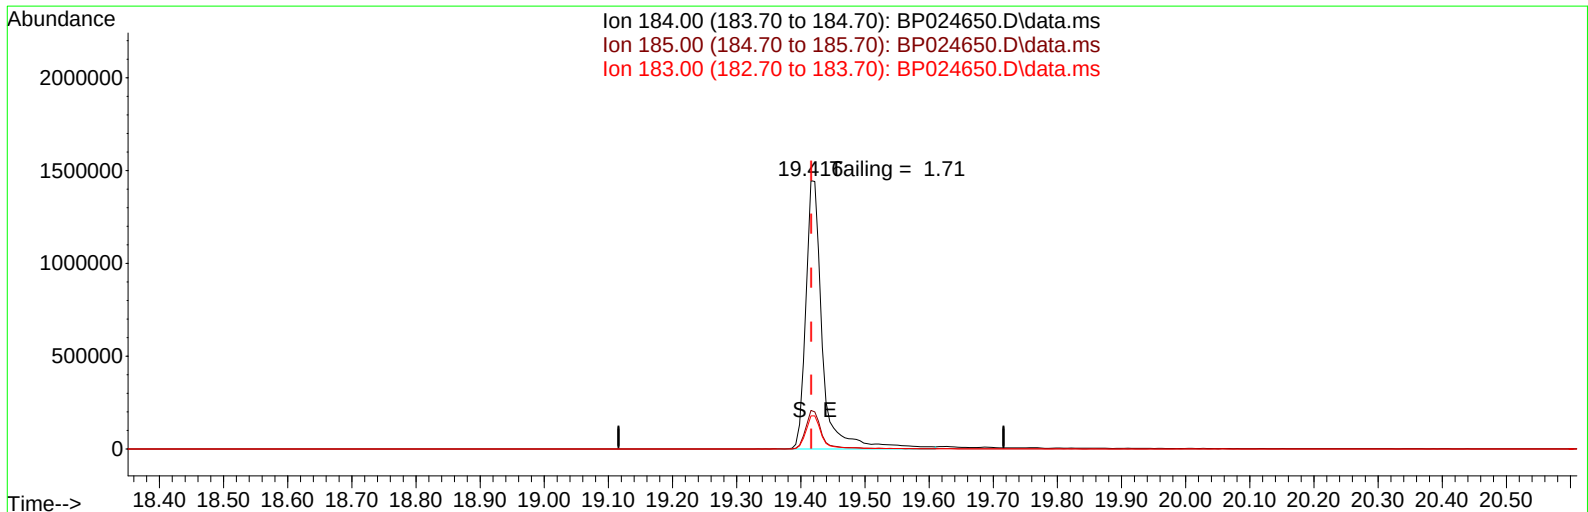

TIC: BP024650.D\data.ms

(77) Benzidine

19.416min (-0.000) 43939.06 ng

response 2620821

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.40
183.00	12.30	12.37
0.00	0.00	0.00