
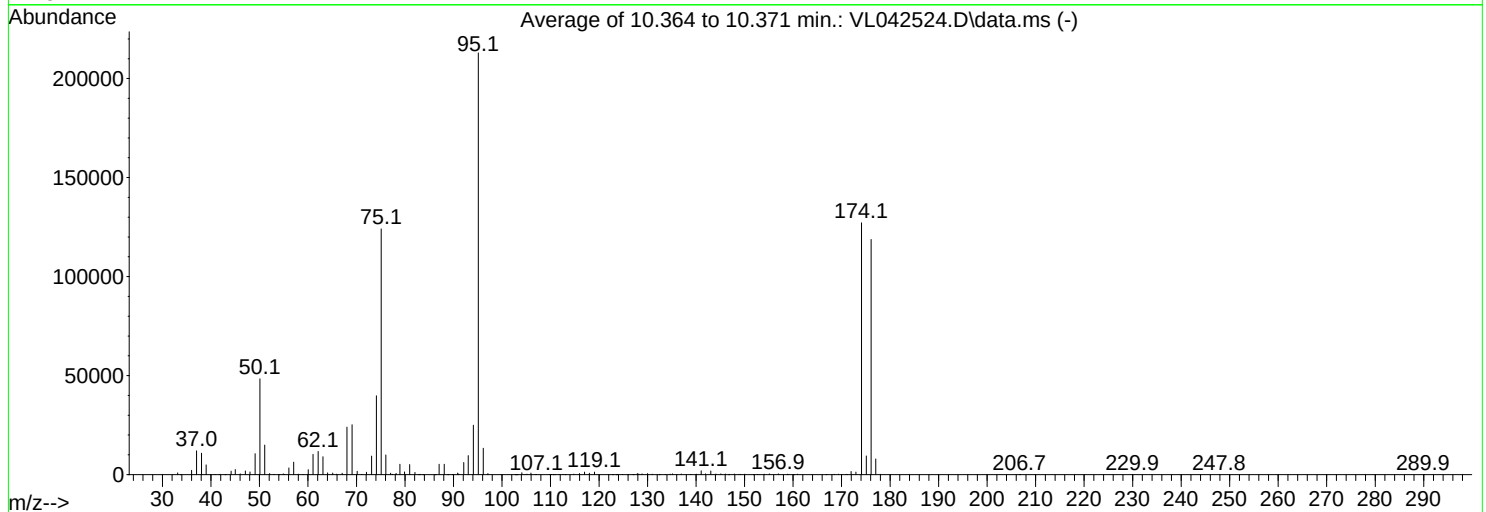


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL051225\
Data File : VL042524.D
Acq On : 12 May 2025 07:58
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL051225AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue May 13 02:07:03 2025

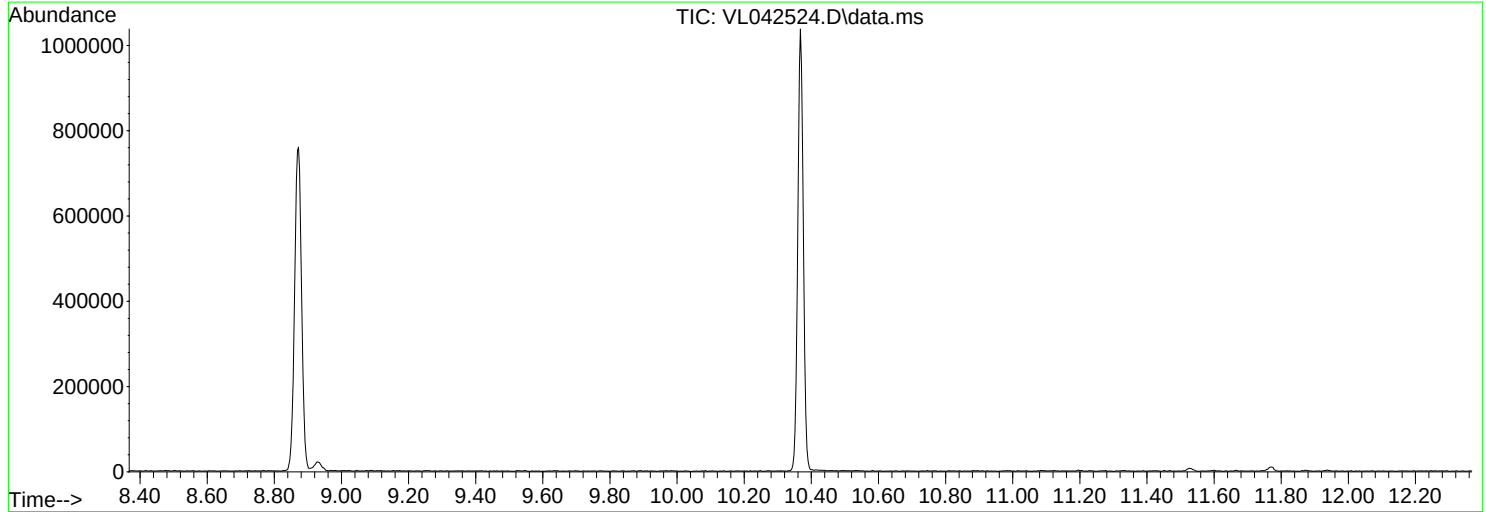

AutoFind: Scans 3175, 3176, 3177; Background Corrected with Scan 3159

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.7	48371	PASS
75	95	30	66	58.3	124085	PASS
95	95	100	100	100.0	212971	PASS
96	95	5	9	6.3	13350	PASS
173	174	0.00	2	1.0	1276	PASS
174	95	50	120	59.7	127141	PASS
175	174	4	9	7.4	9432	PASS
176	174	93	101	93.4	118768	PASS
177	176	5	9	6.7	7924	PASS

Average of 10.364 to 10.371 min.: VL042524.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.15	868	45.00	2557	55.20	95	65.85	23
33.70	39	46.05	386	56.05	3385	67.05	76
36.00	2167	47.10	1839	57.05	6316	68.05	2397
37.05	12047	48.05	1342	58.05	287	69.10	2519
38.05	10800	49.10	10630	59.00	57	70.15	1666
39.00	4939	50.10	48371	60.05	2504	71.10	140
39.95	104	51.10	14914	61.05	10298	72.05	1243
40.85	57	52.10	608	62.10	11719	73.10	9363
41.85	135	53.00	182	63.10	9057	74.10	39824
42.90	31	54.00	32	64.05	890	75.10	124085
44.15	1778	54.90	412	65.10	838	76.05	9975

Average of 10.364 to 10.371 min.: VL042524.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.05	752	87.05	5236	97.10	611	109.85	70
77.40	137	88.10	5237	99.80	50	110.20	83
78.15	629	88.80	28	102.70	40	110.60	38
78.95	5264	89.80	40	102.90	39	111.05	95
79.90	1363	90.85	809	103.10	21	111.75	118
80.95	5062	91.10	297	104.10	977	112.55	148
82.05	1164	92.10	6139	104.75	111	113.00	37
82.80	30	93.05	9614	105.15	252	114.80	282
83.20	164	94.10	24992	105.95	832	115.95	562
83.70	37	95.10	212971	106.85	107	117.00	1265
86.20	44	96.15	13350	107.10	110	118.00	762

Average of 10.364 to 10.371 min.: VL042524.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
119.05	1319	130.00	547	141.95	384	151.80	24
121.90	49	130.95	252	143.05	1855	152.05	63
122.80	31	132.40	24	144.10	364	152.65	109
123.50	40	133.65	63	145.10	399	153.00	112
123.80	139	134.65	258	146.05	353	154.05	247
124.90	89	135.15	380	146.70	29	155.10	393
125.90	17	135.95	104	146.90	130	156.95	440
127.00	18	136.95	359	147.90	332	158.85	237
127.90	569	138.90	182	148.85	144	159.10	85
128.20	348	140.05	255	149.20	149	160.10	19
128.85	429	141.05	1965	150.05	234	160.90	266

Average of 10.364 to 10.371 min.: VL042524.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
166.80	42	177.05	7924				
168.50	151	178.00	150				
169.35	220	206.70	26				
170.00	83	229.95	84				
170.95	194	247.85	96				
171.20	124	289.90	39				
171.95	1635						
172.95	1276						
174.10	127141						
175.10	9432						
176.10	118768						