
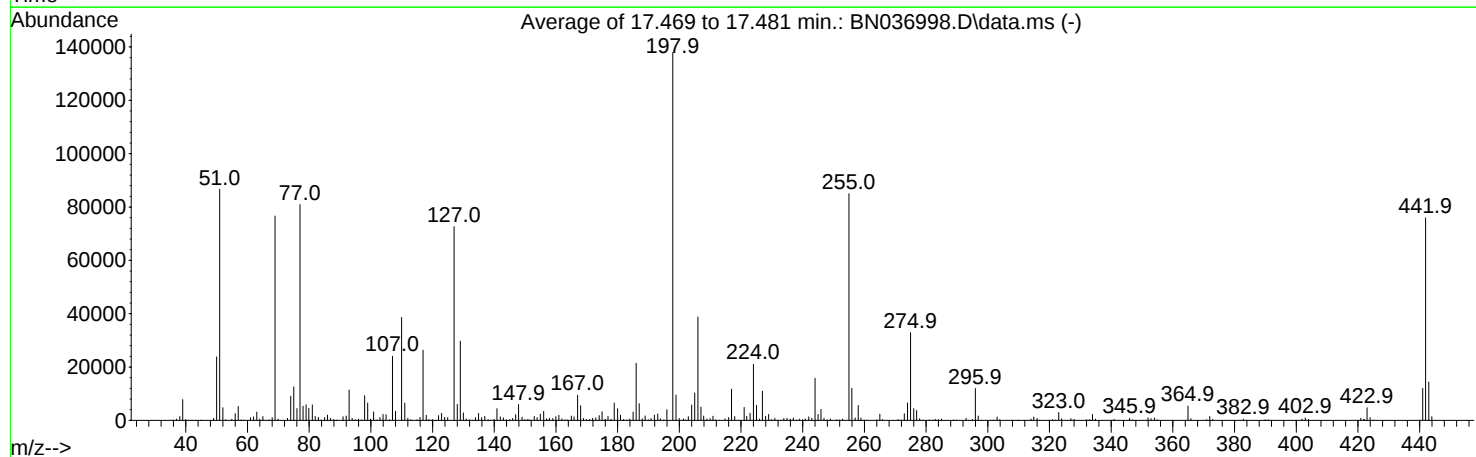


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051425\
Data File : BN036998.D
Acq On : 13 May 2025 17:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 14 00:45:40 2025

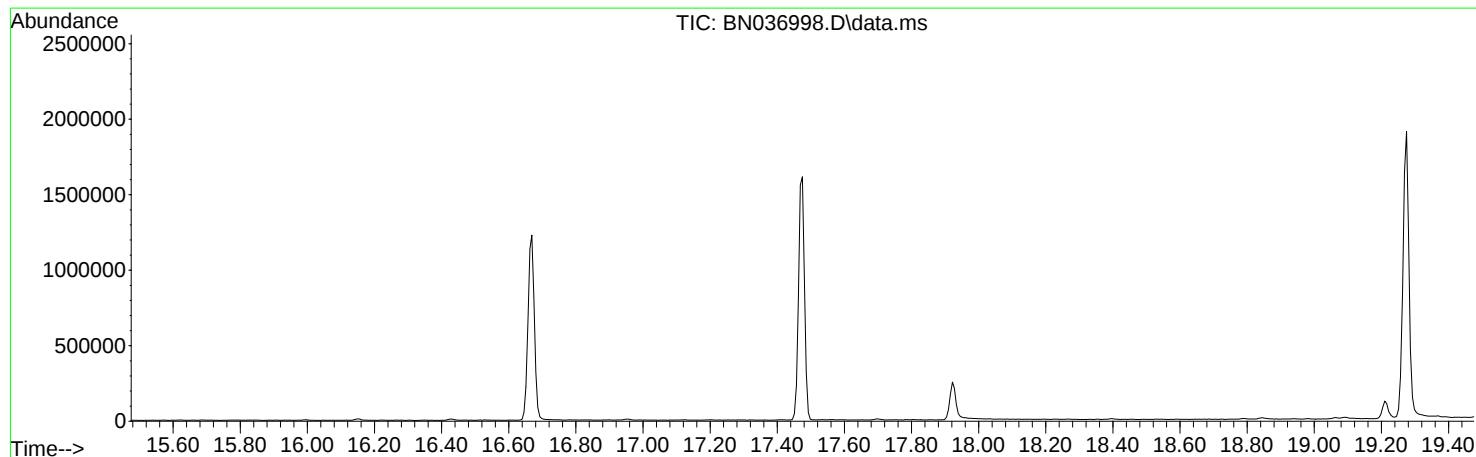

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.8	86619	PASS
68	69	0.00	2	1.4	1066	PASS
69	198	0.00	100	55.6	76627	PASS
70	69	0.00	2	0.6	478	PASS
127	198	10	80	52.7	72651	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	137931	PASS
199	198	5	9	6.9	9502	PASS
275	198	10	60	23.8	32893	PASS
365	198	1	100	3.9	5315	PASS
441	198	0.01	100	8.7	12010	PASS
442	442	50	100	100.0	75872	PASS
443	442	15	24	19.0	14396	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/14/2025	BNA_N	<u>BN036998.D</u>
Compound Name	Response	Retention Time
DDT	424954	20.516
DDD	27353	20.075
DDE	333	19.563
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27686	452640	6.12

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051425\
Data File : BN036998.D
Acq On : 13 May 2025 17:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 14 01:22:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 14 01:22:17 2025
Response via : Initial Calibration

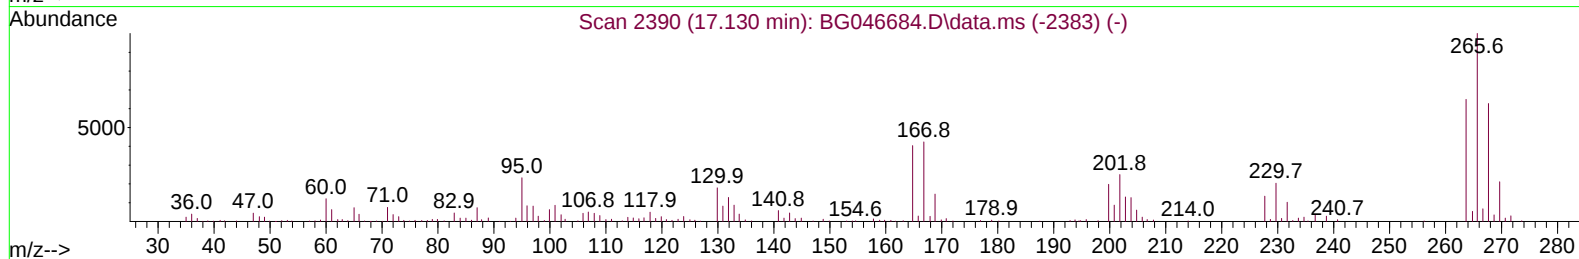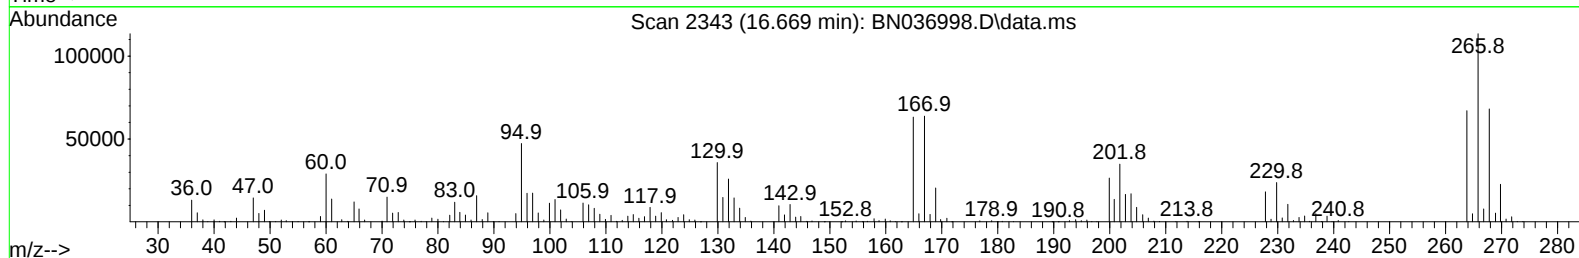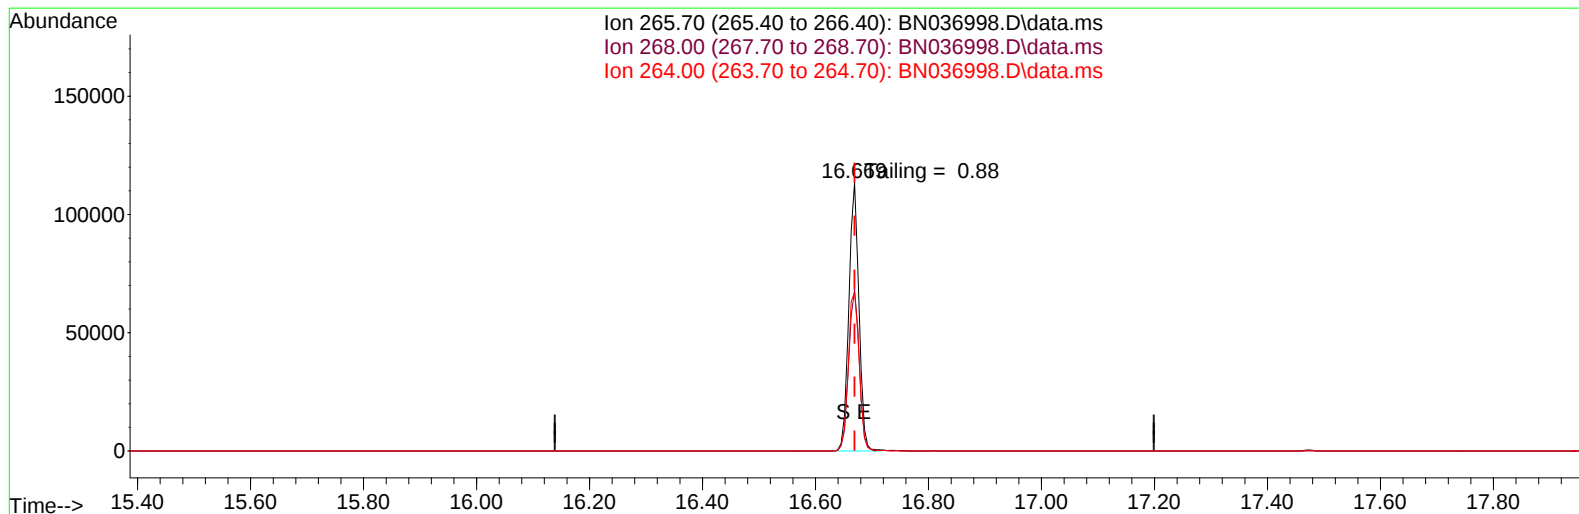

TIC: BN036998.D\data.ms

(70) Pentachlorophenol (C)

16.669min (0.000) 18563.73 ng




response 141750

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.06
264.00	61.60	59.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051425\
Data File : BN036998.D
Acq On : 13 May 2025 17:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 14 01:22:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 14 01:22:17 2025
Response via : Initial Calibration

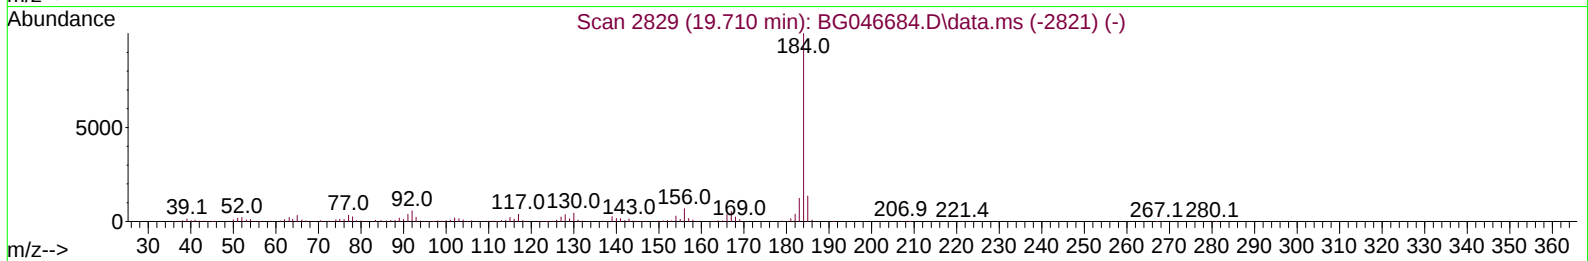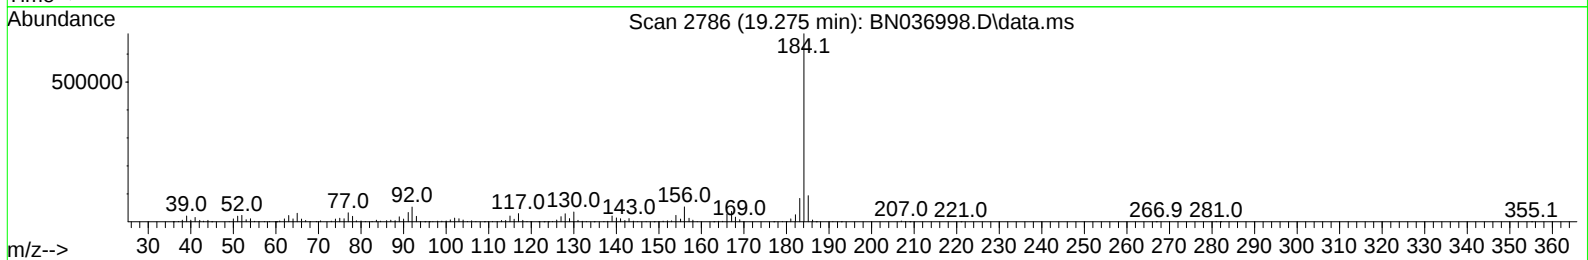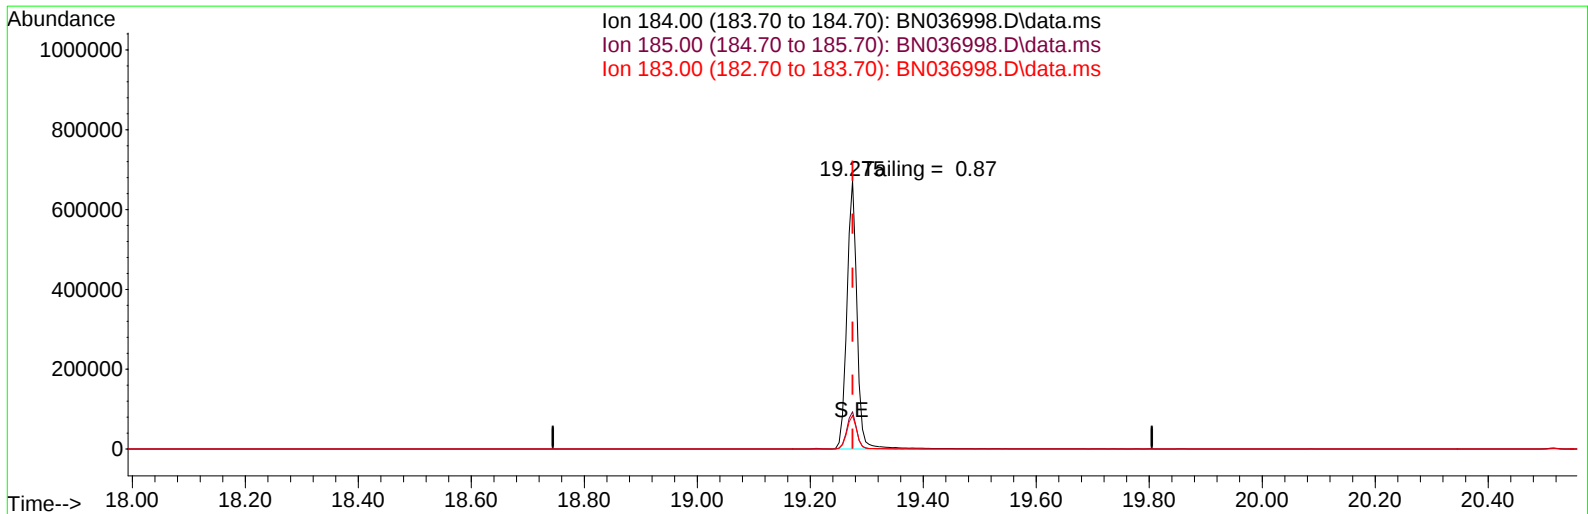

TIC: BN036998.D\data.ms

(77) Benzidine

19.275min (0.000) 0.00 ng

response 833154

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.89
183.00	13.20	12.48
0.00	0.00	0.00